



US00D745661S

(12) **United States Design Patent**
Collins et al.

(10) **Patent No.:** **US D745,661 S**
(45) **Date of Patent:** **** Dec. 15, 2015**

(54) **APPARATUS TO CONTROL FLUID FLOW THROUGH A TUBE**

4,105,028 A 8/1978 Sadlier et al.
4,155,362 A 5/1979 Jess
4,303,376 A 12/1981 Siekmann

(71) Applicant: **DEKA Products Limited Partnership**,
Manchester, NH (US)

(Continued)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **David E. Collins**, Groveland, MA (US);
Alexander R. Therrien, Manchester,
NH (US)

AU 2247783 A 6/1985
CA 1213749 A1 11/1986

(Continued)

(73) Assignee: **DEKA Products Limited Partnership**,
Manchester, NH (US)

OTHER PUBLICATIONS

(**) Term: **14 Years**

AAMI and FDA, Infusing Patients Safely: Priority Issues from the
AAMI/FDA Infusion Device Summit, Symposium, Oct. 5-6, 2010,
pp. 1-48, AAMI, Arlington, VA, USA.

(Continued)

(21) Appl. No.: **29/471,859**

(22) Filed: **Nov. 6, 2013**

Primary Examiner — Anhdao Doan

(51) **LOC (10) Cl.** **24-02**

(74) *Attorney, Agent, or Firm* — James D. Wyninegar, Jr.

(52) **U.S. Cl.**
USPC **D24/111**; D24/108; D24/169

(57) **CLAIM**

The ornamental design for an apparatus to control fluid flow
through a tube, as shown and described.

(58) **Field of Classification Search**
USPC D24/107, 108, 111, 167, 169, 186, 129;
601/150–152, 148, 149; 606/201, 202;
128/DIG. 20; 600/7–9, 67, 123, 131,
600/151, 246, 251, 253
CPC A61H 2209/00; A61H 2201/5002;
A61H 2201/5015
See application file for complete search history.

DESCRIPTION


FIG. 1 is a front, bottom, and right side perspective view of the
apparatus to control fluid flow through a tube, showing my
new design;
FIG. 2 is a back, bottom, and left side perspective view
thereof;
FIG. 3 is a front elevational view thereof;
FIG. 4 is a back elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a right side elevational view thereof;
FIG. 7 is a top plan view thereof;
FIG. 8 is a bottom plan view thereof; and,
FIG. 9 is a front, bottom, and right side perspective view
showing the door open thereof.
The broken lines in the drawings represent an environmental
subject matter and form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,888,877 A 6/1959 Shellman et al.
3,173,372 A 3/1965 Baldwin
3,384,336 A 5/1968 Pulman
3,609,379 A 9/1971 Hildebrandt
3,685,787 A 8/1972 Adelberg
3,733,149 A 5/1973 Jacobson
3,790,042 A 2/1974 McCormick et al.
3,831,600 A 8/1974 Yum et al.
4,038,982 A 8/1977 Burke et al.

1 Claim, 6 Drawing Sheets

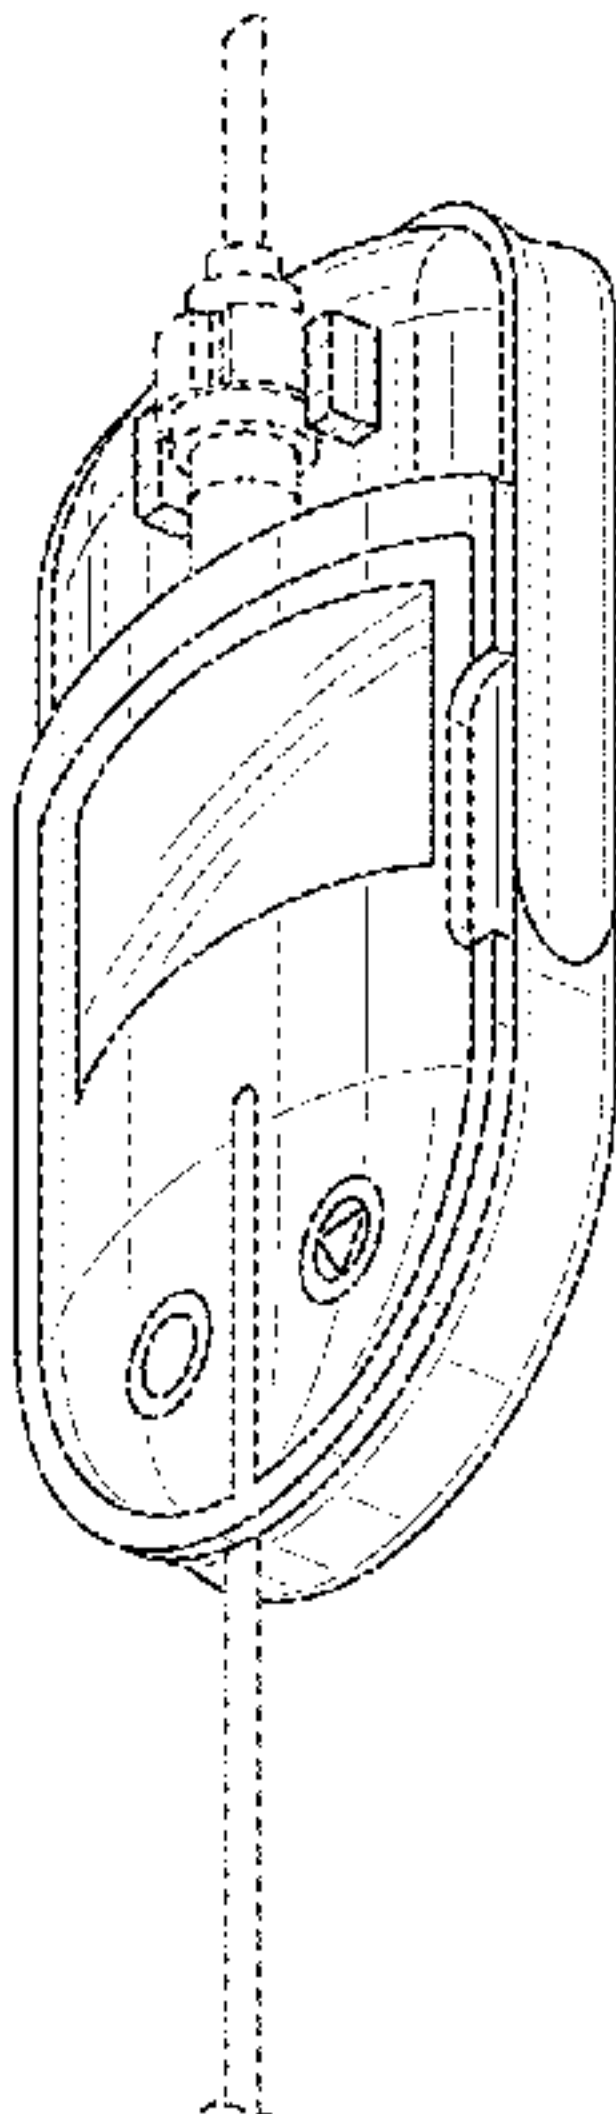

(56)

References Cited

U.S. PATENT DOCUMENTS

4,321,461 A	3/1982	Walter, Jr. et al.	6,984,052 B1	1/2006	Del Castillo
4,328,800 A	5/1982	Marx et al.	7,001,365 B2	2/2006	Makkink
4,328,801 A	5/1982	Marx et al.	7,190,275 B2	3/2007	Goldberg et al.
4,397,642 A	8/1983	Lamadrid	D564,087 S *	3/2008	Yodfat et al. D24/108
4,421,506 A	12/1983	Danby et al.	7,338,475 B2	3/2008	Brown
4,449,534 A	5/1984	Leibinsohn Saul	7,498,563 B2	3/2009	Mandro et al.
4,469,480 A	9/1984	Figler et al.	7,499,581 B2	3/2009	Tribble et al.
4,504,263 A	3/1985	Steuer et al.	7,540,859 B2	6/2009	Claude et al.
4,525,163 A	6/1985	Slavik et al.	7,695,448 B2	4/2010	Cassidy et al.
4,583,975 A	4/1986	Pekkarinen et al.	7,767,991 B2	8/2010	Sacchetti
RE32,294 E	11/1986	Knute	D629,503 S *	12/2010	Caffey et al. D24/108
4,634,426 A	1/1987	Kamen	7,892,204 B2	2/2011	Kraus
4,648,869 A	3/1987	Bobo, Jr.	7,905,859 B2	3/2011	Bynum et al.
4,662,829 A	5/1987	Nehring	7,918,834 B2	4/2011	Mernoe et al.
4,668,216 A	5/1987	Martin et al.	7,933,780 B2	4/2011	De La Huerga
4,673,820 A	6/1987	Kamen	8,025,634 B1	9/2011	Moubayed et al.
4,680,977 A	7/1987	Conero et al.	8,038,657 B2	10/2011	Davis et al.
4,703,314 A	10/1987	Spani	8,147,448 B2	4/2012	Sundar et al.
4,718,896 A	1/1988	Arndt et al.	8,147,464 B2	4/2012	Spohn et al.
4,720,636 A	1/1988	Benner, Jr.	8,256,984 B2	9/2012	Fathallah et al.
4,820,281 A	4/1989	Lawler, Jr.	D676,551 S *	2/2013	Desai et al. D24/129
4,834,744 A	5/1989	Ritson	8,529,511 B2	9/2013	Boulanger et al.
4,837,708 A	6/1989	Wright	8,531,517 B2	9/2013	Kai Tao
4,846,792 A	7/1989	Bobo, Jr. et al.	8,552,361 B2	10/2013	Mandro et al.
4,909,786 A	3/1990	Gijssels et al.	8,622,979 B2	1/2014	Hungerford et al.
4,920,336 A	4/1990	Meijer	D712,043 S *	8/2014	Sliger D24/186
4,936,828 A	6/1990	Chiang	8,834,429 B2	9/2014	Grant et al.
4,959,050 A	9/1990	Bobo, Jr.	D720,449 S *	12/2014	Galbraith et al. D24/111
4,979,940 A	12/1990	Bobo, Jr. et al.	2002/0194933 A1	12/2002	Roelofs
4,981,467 A	1/1991	Bobo, Jr. et al.	2003/0045840 A1	3/2003	Burko
5,002,539 A	3/1991	Coble et al.	2003/0055406 A1	3/2003	Lebel et al.
5,045,069 A	9/1991	Imparato	2003/0217962 A1	11/2003	Childers et al.
5,057,090 A	10/1991	Bessman	2004/0044306 A1 *	3/2004	Lynch et al. 604/93.01
5,154,693 A *	10/1992	East et al. 604/9	2004/0171994 A1	9/2004	Goldberg et al.
5,154,704 A	10/1992	Archibald	2005/0096581 A1 *	5/2005	Chan 604/9
5,181,910 A	1/1993	Scanlon	2005/0171791 A1	8/2005	Chimenti et al.
5,186,057 A	2/1993	Everhart	2006/0140466 A1	6/2006	Seshimo et al.
RE34,413 E	10/1993	McCullough	2006/0291211 A1	12/2006	Rodriguez et al.
5,267,980 A	12/1993	Dirr, Jr. et al.	2008/0004574 A1	1/2008	Dyar et al.
5,279,558 A *	1/1994	Kriesel 128/DIG. 12	2008/0051732 A1	2/2008	Chen
5,314,316 A	5/1994	Shibamoto et al.	2008/0147008 A1	6/2008	Lewis et al.
5,328,341 A	7/1994	Forni	2008/0147016 A1	6/2008	Faries et al.
5,331,309 A	7/1994	Sakai	2008/0154214 A1	6/2008	Spohn et al.
5,415,641 A	5/1995	Yerlikaya et al.	2008/0235765 A1	9/2008	Shimizu
D362,721 S *	9/1995	Peeler et al. D24/169	2009/0112115 A1	4/2009	Huang et al.
5,482,446 A	1/1996	Williamson et al.	2009/0224638 A1	9/2009	Weber
5,562,615 A	10/1996	Nassif	2009/0254025 A1	10/2009	Simmons
5,588,963 A	12/1996	Roelofs	2009/0276167 A1	11/2009	Glaser et al.
5,718,562 A	2/1998	Lawless et al.	2009/0281460 A1	11/2009	Lowery et al.
5,753,820 A	5/1998	Reed et al.	2010/0097451 A1	4/2010	Bruce et al.
5,782,805 A	7/1998	Meinzer et al.	2010/0114027 A1	5/2010	Jacobson et al.
5,800,140 A	9/1998	Forni	2010/0168671 A1	7/2010	Faries, Jr. et al.
5,899,665 A	5/1999	Makino et al.	2010/0211003 A1	8/2010	Sundar et al.
D416,999 S *	11/1999	Miyamoto D24/111	2010/0292635 A1	11/2010	Sundar
6,049,381 A	4/2000	Reintjes et al.	2010/0309005 A1	12/2010	Warner et al.
6,050,713 A	4/2000	O'Donnell et al.	2011/0004186 A1	1/2011	Butterfield
6,083,206 A	7/2000	Molko	2011/0125103 A1	5/2011	Rondeau
6,110,153 A	8/2000	Davis et al.	2011/0166511 A1	7/2011	Sharvit et al.
6,149,631 A	11/2000	Haydel, Jr.	2011/0196306 A1	8/2011	De La Huerga
6,159,186 A	12/2000	Wickhem et al.	2011/0208123 A1	8/2011	Gray et al.
6,213,354 B1	4/2001	Kay	2011/0231204 A1	9/2011	De La Huerga
6,228,047 B1	5/2001	Dadson	2011/0251557 A1	10/2011	Powers
D446,860 S	8/2001	Mezière et al.	2011/0313351 A1 *	12/2011	Kamen et al. 604/67
6,305,908 B1	10/2001	Hermann et al.	2011/0313789 A1	12/2011	Kamen et al.
6,328,712 B1	12/2001	Cartledge	2012/0013735 A1	1/2012	Tao
6,362,887 B1	3/2002	Meisberger	2012/0059318 A1	3/2012	Dewey
6,500,151 B1	12/2002	Cobb et al.	2012/0059350 A1	3/2012	Siefert
6,503,221 B1	1/2003	Briggs et al.	2012/0095415 A1	4/2012	Sharvit et al.
6,523,414 B1	2/2003	Malmstrom et al.	2012/0095433 A1	4/2012	Hungerford et al.
D471,274 S *	3/2003	Diaz et al. D24/111	2012/0185267 A1	7/2012	Kamen et al.
6,562,012 B1	5/2003	Brown et al.	2012/0197185 A1	8/2012	Tao
6,599,282 B2	7/2003	Burko	2012/0238997 A1	9/2012	Dewey
6,641,556 B1	11/2003	Shigezawa	2012/0265166 A1	10/2012	Yodfat
6,657,545 B1	12/2003	Lin et al.	2012/0310153 A1	12/2012	Moberg et al.
6,736,801 B1	5/2004	Gallagher	2013/0035659 A1	2/2013	Hungerford et al.
			2013/0177455 A1	7/2013	Kamen et al.
			2013/0182381 A1	7/2013	Gray et al.
			2013/0184676 A1	7/2013	Kamen et al.
			2013/0188040 A1	7/2013	Kamen et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0191513 A1 7/2013 Kamen et al.
 2013/0197693 A1 8/2013 Kamen et al.
 2013/0201482 A1 8/2013 Munro
 2013/0204188 A1 8/2013 Kamen et al.
 2013/0253442 A1 9/2013 Travis et al.
 2013/0272773 A1 10/2013 Kamen et al.
 2013/0281965 A1 10/2013 Kamen et al.
 2013/0297330 A1 11/2013 Kamen et al.
 2013/0310990 A1 11/2013 Peret et al.
 2013/0317753 A1 11/2013 Kamen et al.
 2013/0317837 A1 11/2013 Ballantyne et al.
 2013/0336814 A1 12/2013 Kamen et al.
 2013/0339049 A1 12/2013 Blumberg, Jr. et al.
 2013/0346108 A1 12/2013 Kamen et al.
 2014/0081233 A1 3/2014 Hungerford et al.
 2014/0135695 A1 5/2014 Grant et al.
 2014/0148757 A1 5/2014 Ambrosina et al.
 2014/0165703 A1 6/2014 Wilt et al.
 2014/0180711 A1 6/2014 Kamen et al.
 2014/0194818 A1 7/2014 Yodfat et al.
 2014/0227021 A1 8/2014 Kamen et al.
 2014/0309612 A1 10/2014 Smisson, III et al.
 2014/0318639 A1 10/2014 Peret et al.
 2015/0002667 A1 1/2015 Peret et al.
 2015/0002668 A1 1/2015 Peret et al.
 2015/0002677 A1 1/2015 Peret et al.

FOREIGN PATENT DOCUMENTS

DE 2023027 11/1970
 DE 3617723 A1 12/1987
 DE 3822057 C2 1/1989
 DE 69229832 T2 2/2000
 EP 0112699 A2 7/1984
 EP 1722310 A1 4/2005
 EP 2319551 A2 10/2008
 FR 2042606 A1 2/1971
 FR 2458804 1/1981
 FR 2617593 1/1989
 GB 1301033 A 12/1972
 GB 2020735 A 11/1979
 GB 2207239 B 1/1989
 GB 2328982 B 3/1999
 JP S58163843 9/1983
 JP 3110458 B2 11/2000
 JP 2011 062371 A 3/2011
 NL 7006908 11/1970
 NL 8801680 2/1989
 NL 9101825 A 5/1993
 SE 376843 6/1975
 WO WO 81/02770 A1 10/1981
 WO WO 93/09407 A1 5/1993
 WO WO 00/72181 A2 11/2000
 WO WO 02/40084 A2 5/2002
 WO WO 02/100262 A1 12/2002
 WO WO 2004/035116 A1 4/2004
 WO WO 2005/094919 A1 10/2005
 WO WO 2006/086723 A2 8/2006
 WO WO 2008/022880 A1 2/2008
 WO WO 2008/079023 A1 7/2008
 WO WO 2009/039203 A2 3/2009
 WO WO 2009/039214 A2 3/2009
 WO WO 2009/055639 A2 4/2009
 WO WO 2010/129720 A2 11/2010
 WO WO 2011/021098 A1 2/2011
 WO WO 2011/136667 A1 11/2011
 WO WO 2013/095459 A9 6/2013
 WO WO 2013/096713 A2 6/2013
 WO WO 2013/096718 A2 6/2013

WO WO 2013/096722 A2 6/2013
 WO WO 2013/096909 A2 6/2013

OTHER PUBLICATIONS

Conway, "Analytical Analysis of Tip Travel in a Bourdon Tube", Master's Thesis, Naval Postgraduate School Monterey, Dec. 1995, pp. i-89.
 "Principles of Flow Cytometry: An Overview." Methods in Cell Biology: Cytometry. Ed. Zbigniew Darzynkiewicz. 3rd ed. vol. 63. Academic, 2000. 44-48.
 "Feature Detection", *OpenCV Wiki*, 2010, 7 pgs, http://opencv.willowgarage.com/documentation/cpp/imgproc_feature_detection.html.
 Galambos et al., "Progressive Probabilistic Hough Transform for Line Detection", IEEE, 7 pgs, 1999.
 International Search Report & Written Opinion dated May 14, 2012, received in International patent application No. PCT/US2011/066588 (I97WO), 9 pgs.
 International Search Report & Written Opinion dated Jun. 18, 2013, received in International patent application No. PCT/US2012/071142 (J79WO), 14 pgs.
 International Search Report & Written Opinion dated Oct. 1, 2013, received in International patent application No. PCT/US2012/071490 (J76WO), 19 pgs.
 International Search Report & Written Opinion dated Dec. 4, 2013, received in International patent application No. PCT/US2013/032445 (K14WO), 20 pgs.
 International Search Report & Written Opinion dated Nov. 7, 2013, received in International patent application No. PCT/US2013/042350 (K66WO), 18 pgs.
 Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 9, 2013, received in International patent application No. PCT/U52013/032445 (K14WO), 10 pgs.
 Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 26, 2013, received in International patent application No. PCT/U52013/042350 (K66WO), 7 pgs.
 Hofmann, "Modeling Medical Devices for Plug-and-Play Interoperability", MIT Department of Electrical Engineering and Computer Science, Jun. 2007, pp. 1-187.
 King et al. *Prototyping closed loop physiologic control with the medical device coordination framework*. In *SEHC 2010: Proceedings of the 2010 ICSE Workshop on Software Engineering in Health Care* (pp. 1-11). New York, NY: ACM. (2010).
 Jetley et al., "Safety Requirements Based Analysis of Infusion Pump Software", Proceedings of the IEEE Real Time Systems Symposium, Tuscon, Dec. 2007 pp. 1-4.
 FDA US Food and Drug Administration, "SEDASYS® Computer-Assisted Personalized Sedation System—P08000", Jul. 16, 2013, pp. 1-2, www.fda.gov/MedicalDevices/ProductsandMedicalProcedures/DeviceApprovalsandClearances/Recently-Approved-Devices/ucm353950.htm.
 Luerkens, David W. "Theory and Application of Morphological Analysis: Fine Particles and Surfaces". Boca Raton: CRC, 1991. 5-7.
 Matas et al., *Progressive Probabilistic Hough Transform*.
 "Miscellaneous Image Transformations", *OpenCV Wiki*, 2011, 9 pgs., http://opencv.willowgarage.com/documentation/cpp/miscellaneous_image_transformations.
 National Patient Safety Agency, *Design for Patient Safety: A Guide to the Design of Electronic Infusion Devices*, booklet, 2010, pp. 1-96, Edition 1, National Patient Safety Agency, London.
 "Object Detection", *OpenCV Wiki*, 2011, 2 pgs., http://opencv.willowgarage.com/documentation/cpp/object_detection.html.
 "The OpenCV Reference Manual Release 2.4.6.0", Jul. 1, 2013, pp. 1-813.
 Leor et al., "A System for the Measurement of Drop Volume of Intravenous Solutions", Proceedings Computers in Cardiology 1990, pp. 405-406, Los Alamitos, California.
 Butterfield, "Alaris SE Pump, Monitoring and Detection of IV Line Occlusions.", CareFusion Corporation, 2010, 4 pgs.
 "Vista Basic: Instructions for Use: Software IFVB", manual, 2002, pp. 3, B. Braun Medical Inc.
 Hugli et al., "Drop volume measurement by vision." Proceedings of SPIE Electronic Imaging Conference, San Diego, Jan. 2000. SPIE vol. 3866-11, pp. 60-66.

* cited by examiner

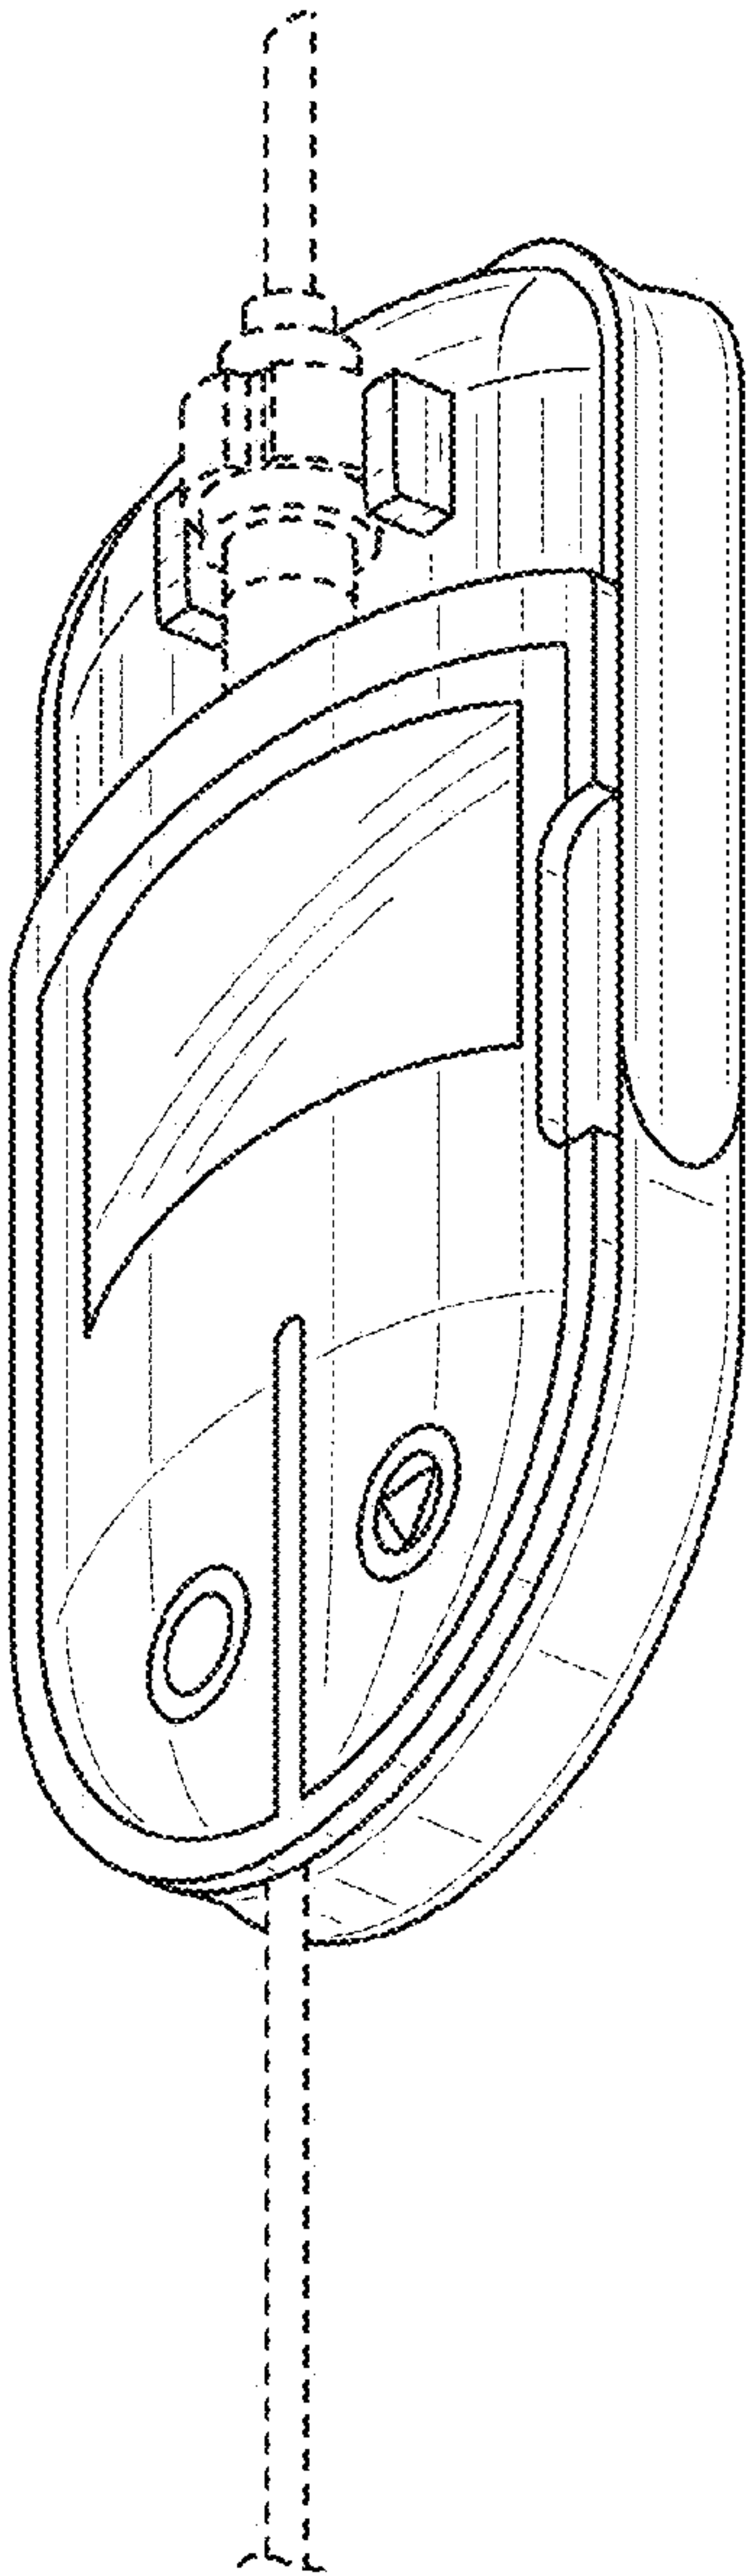


FIG. 1

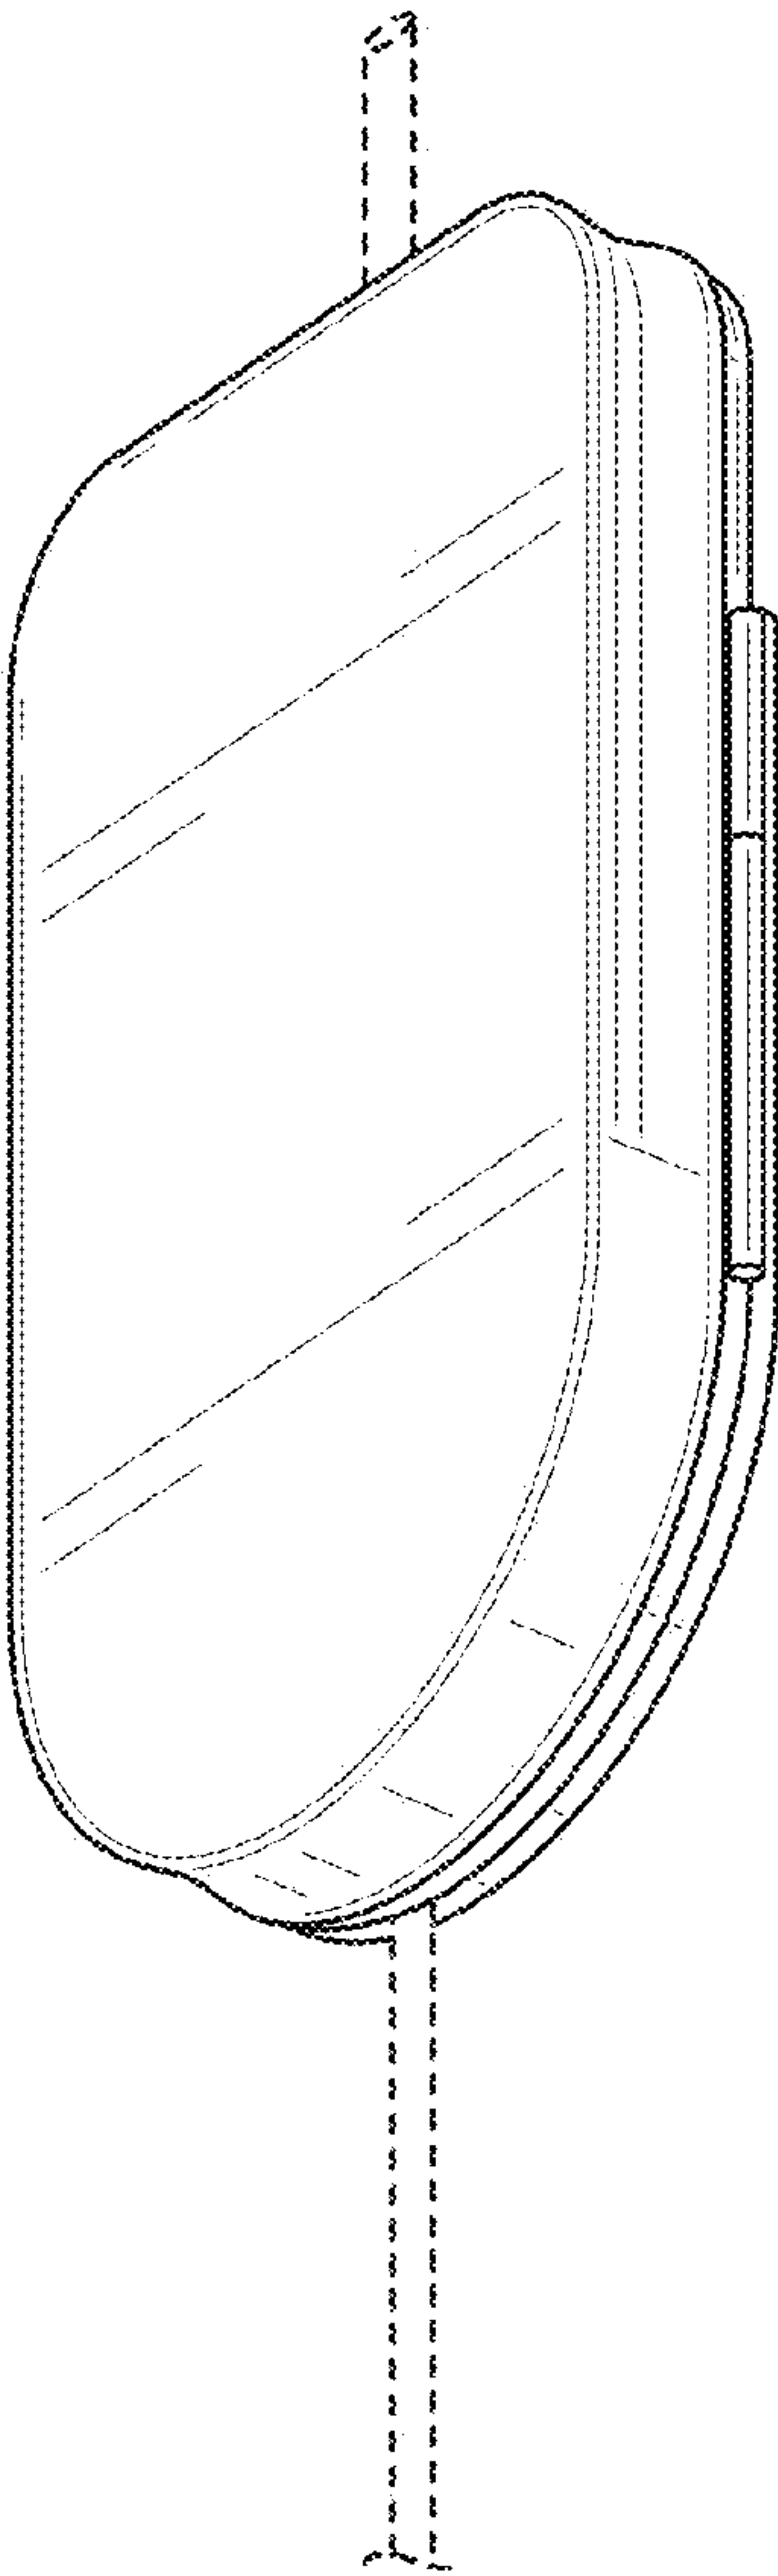


FIG. 2

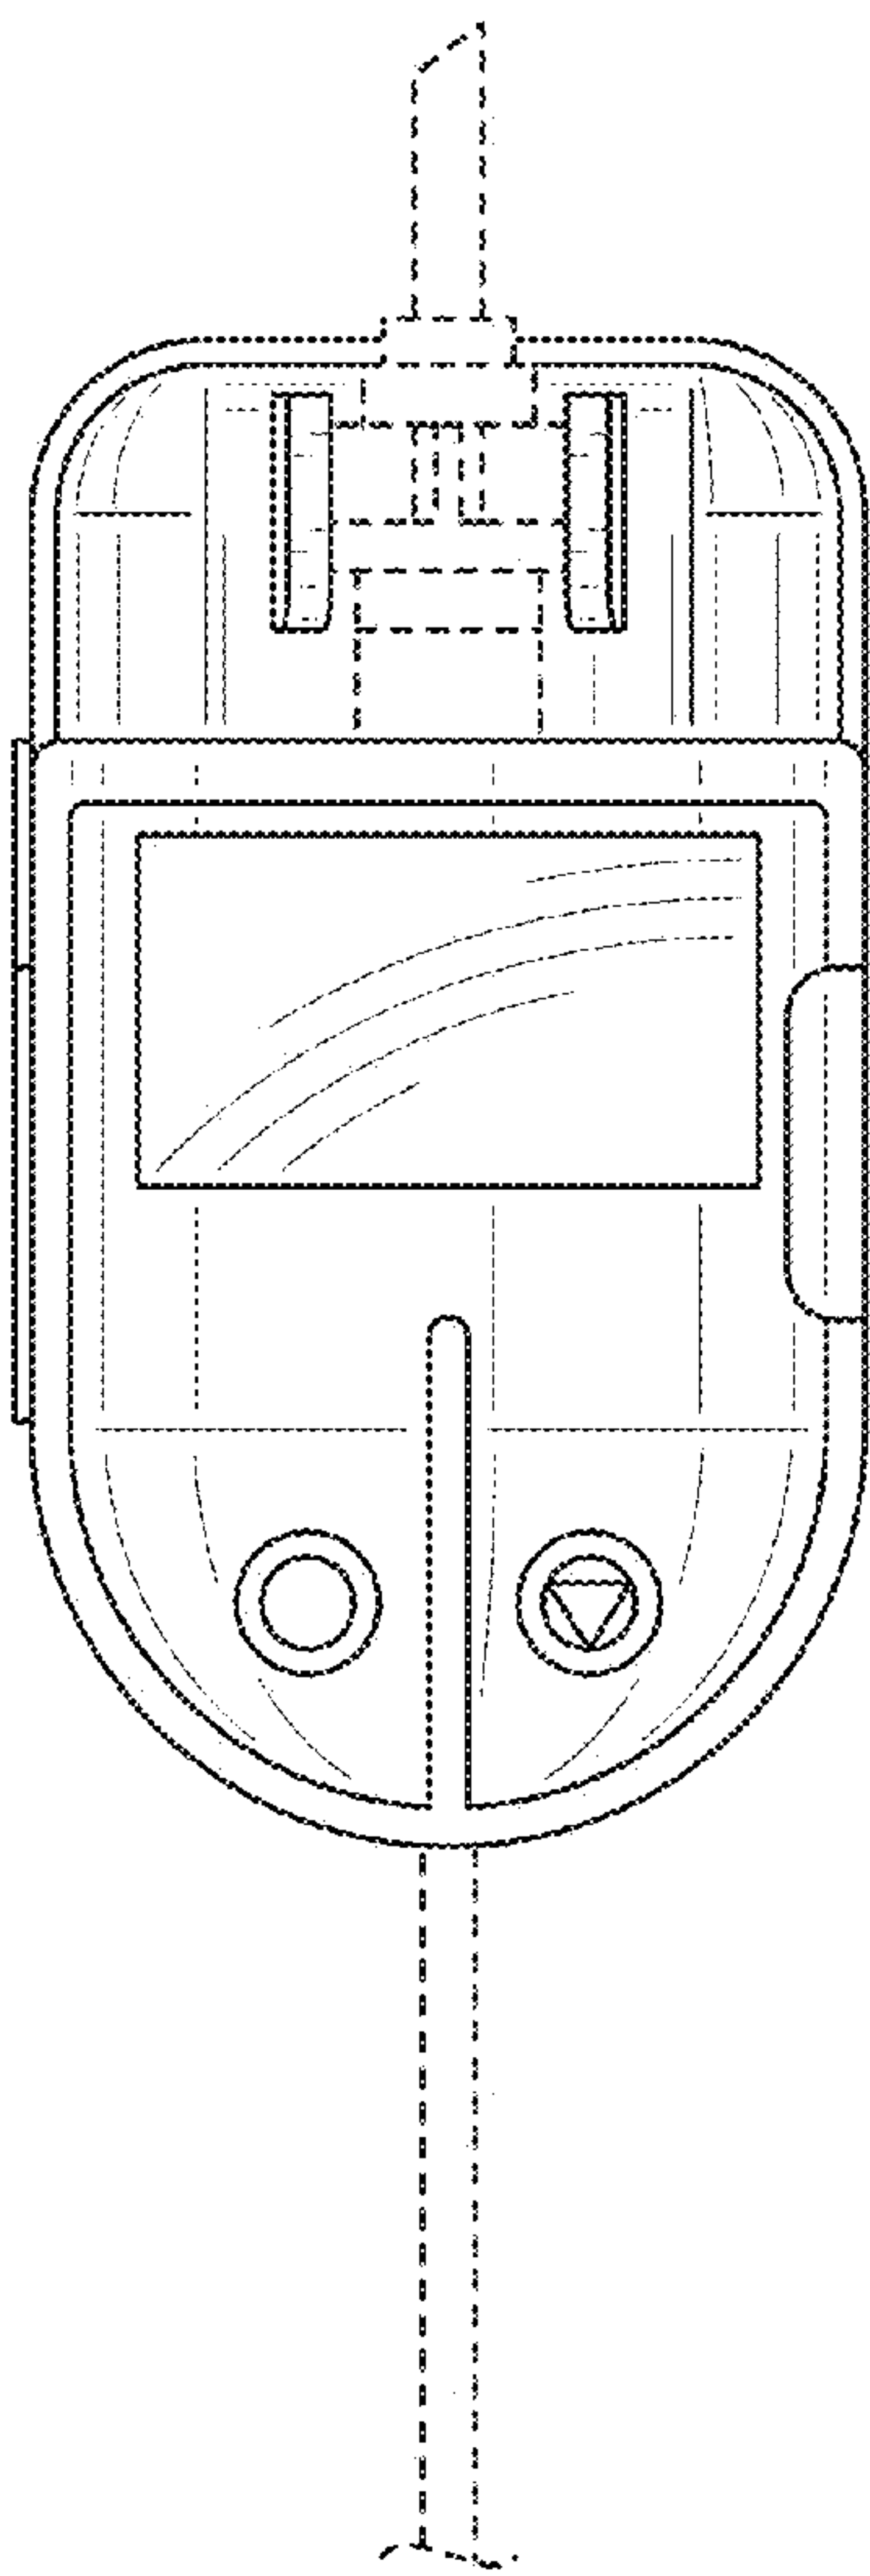


FIG. 3

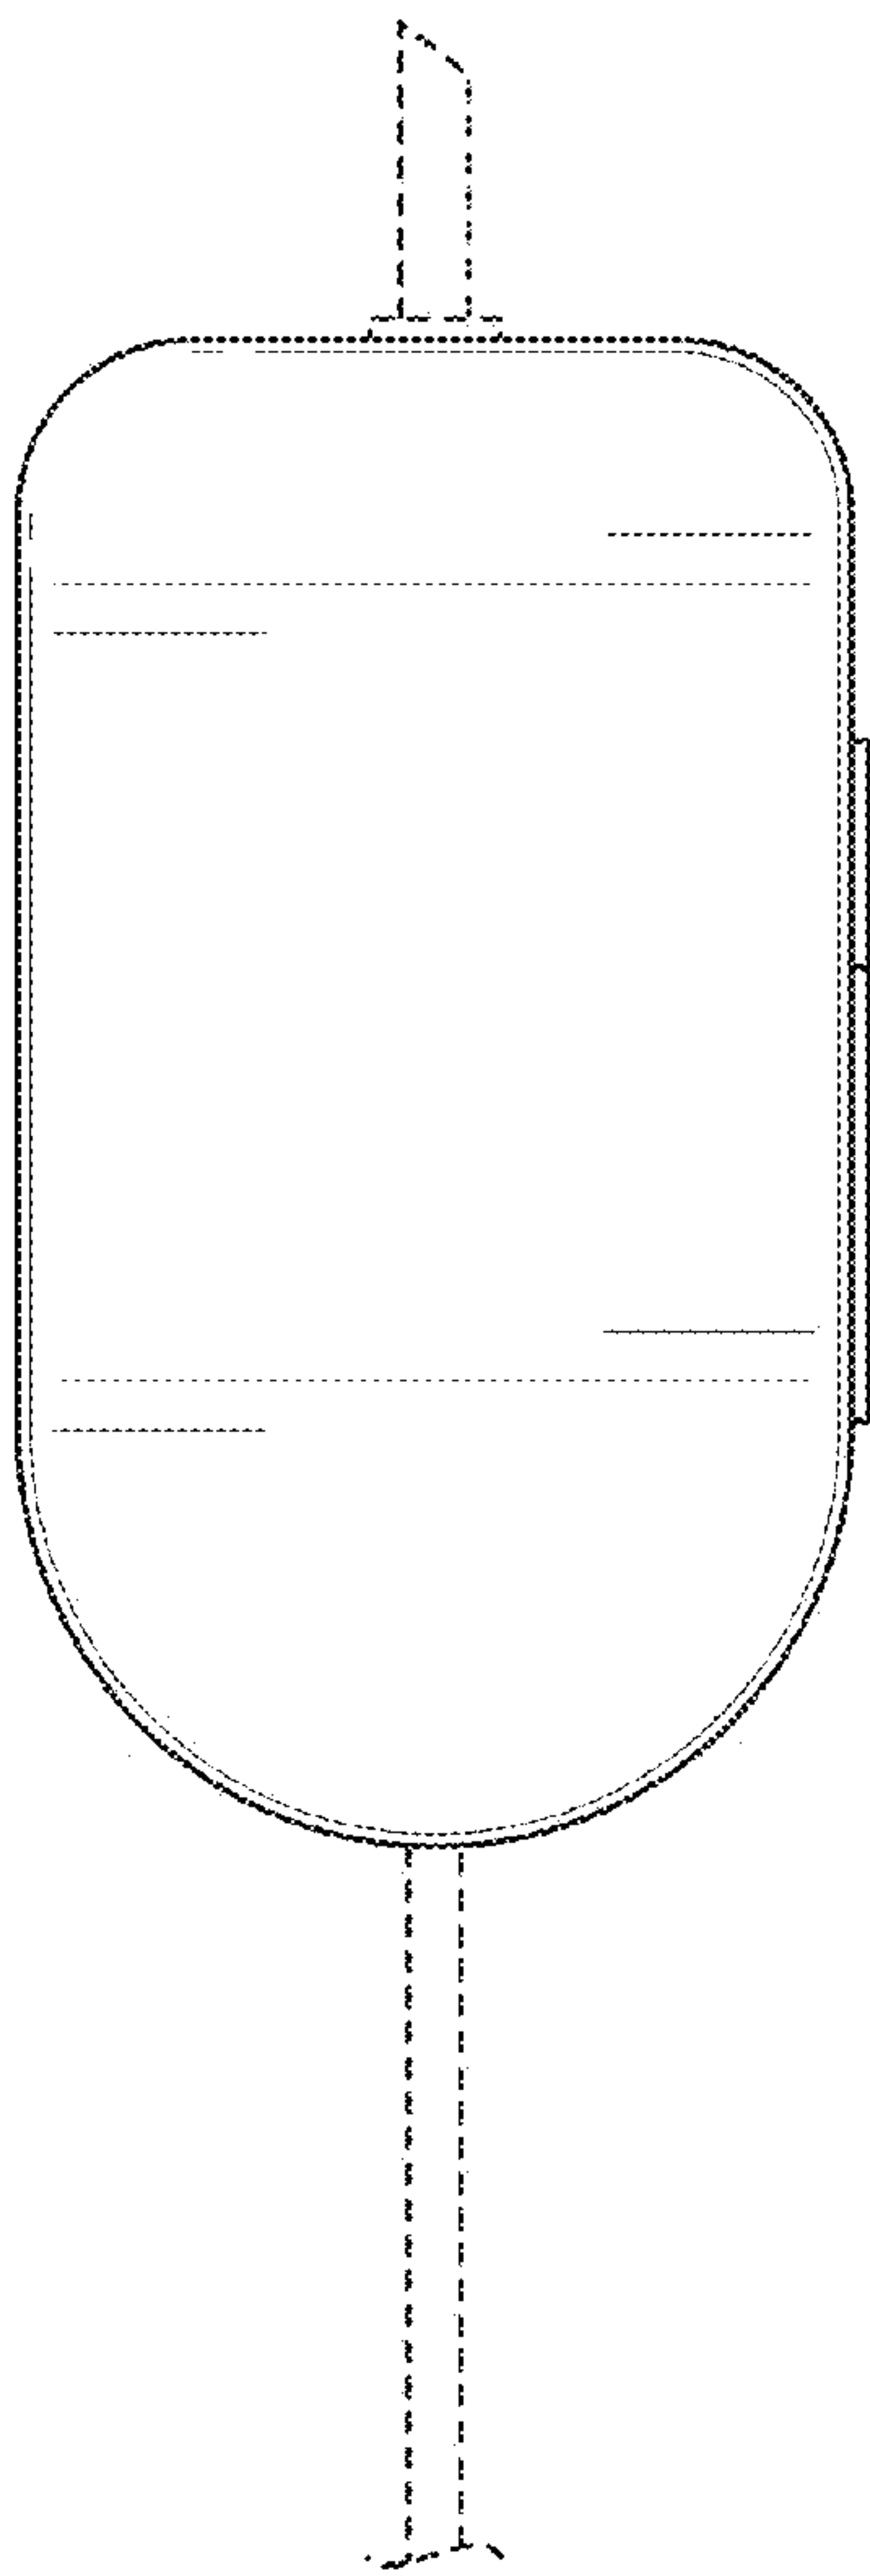


FIG. 4

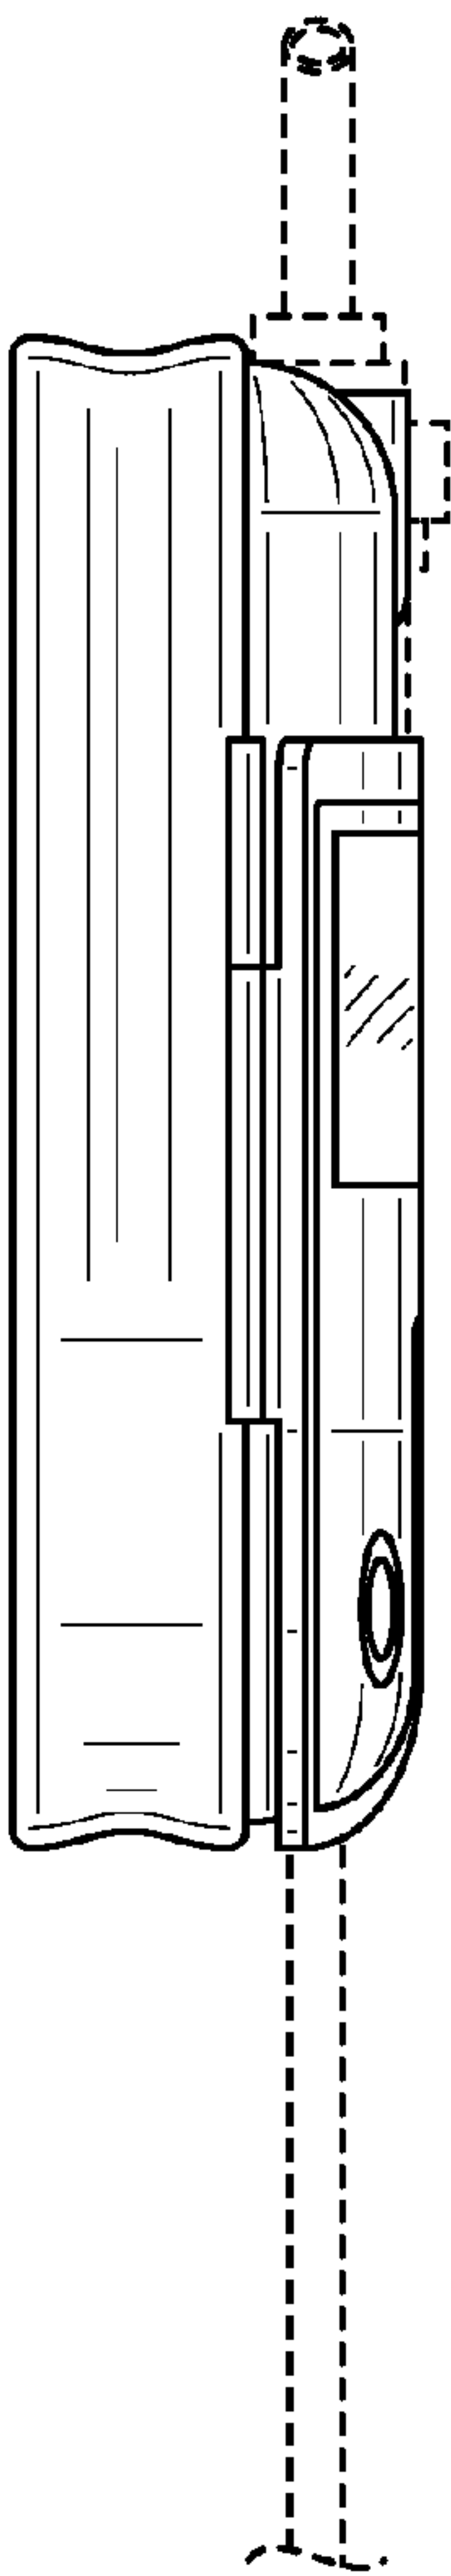


FIG. 5

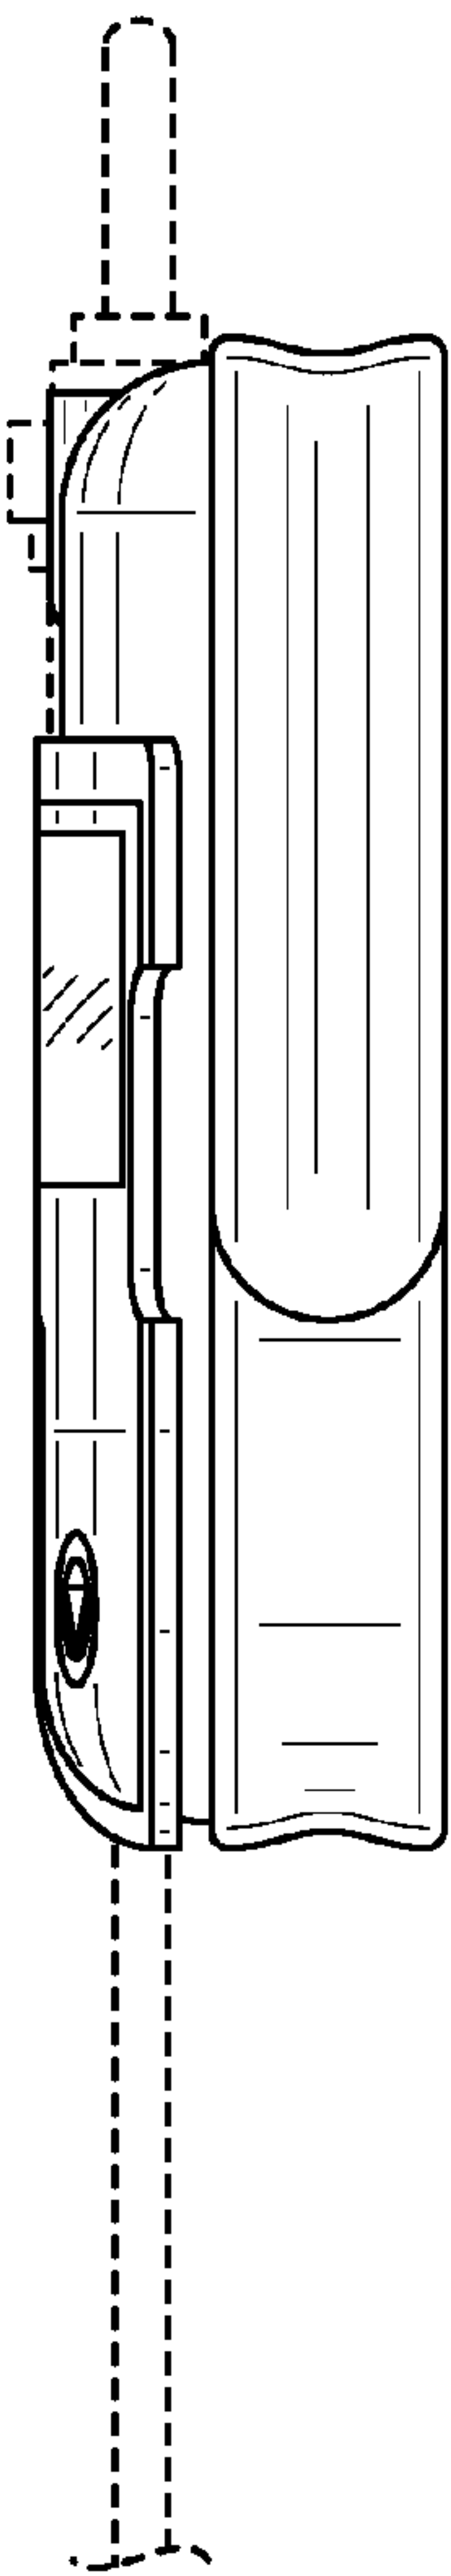


FIG. 6

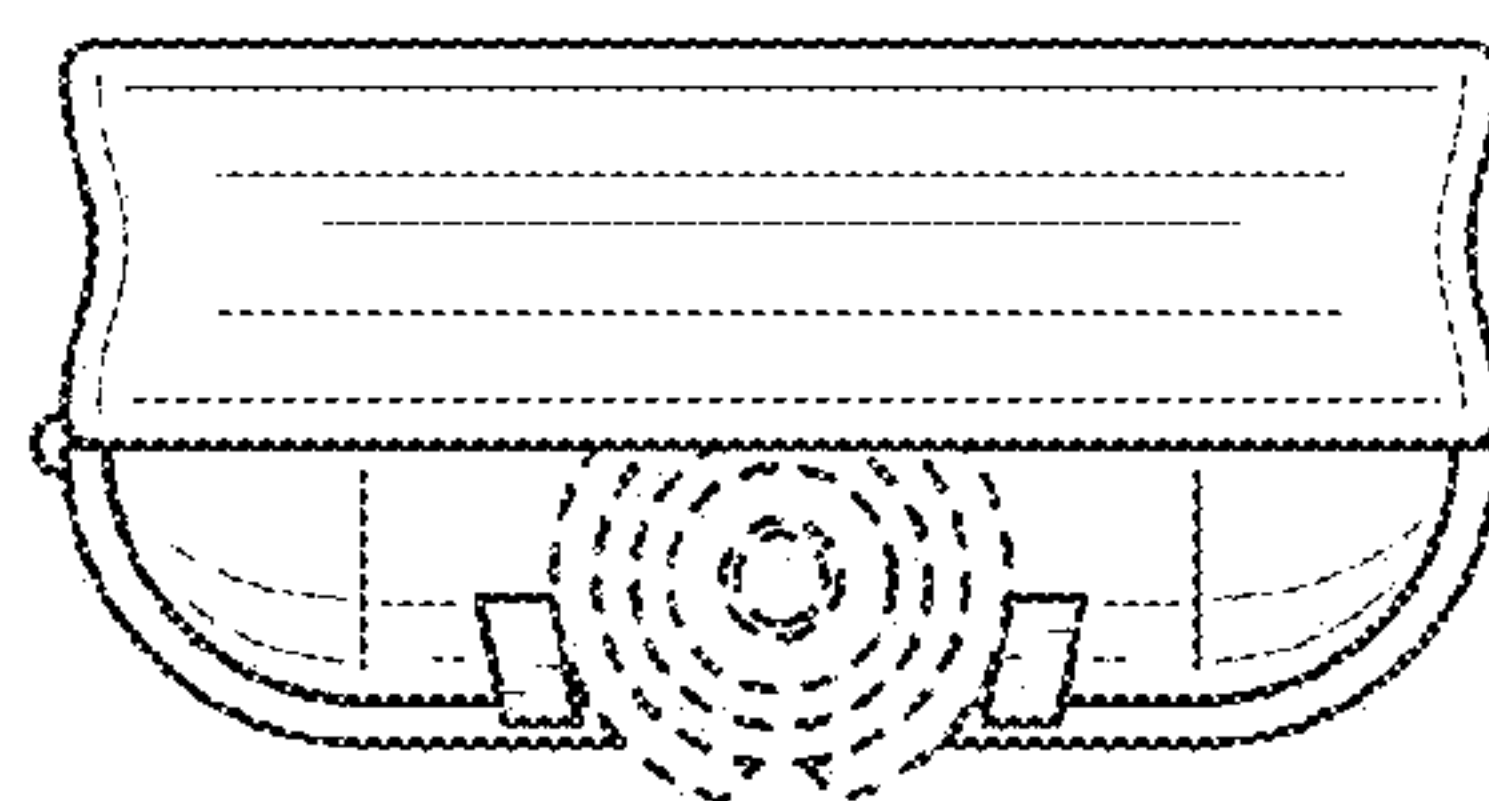


FIG. 7

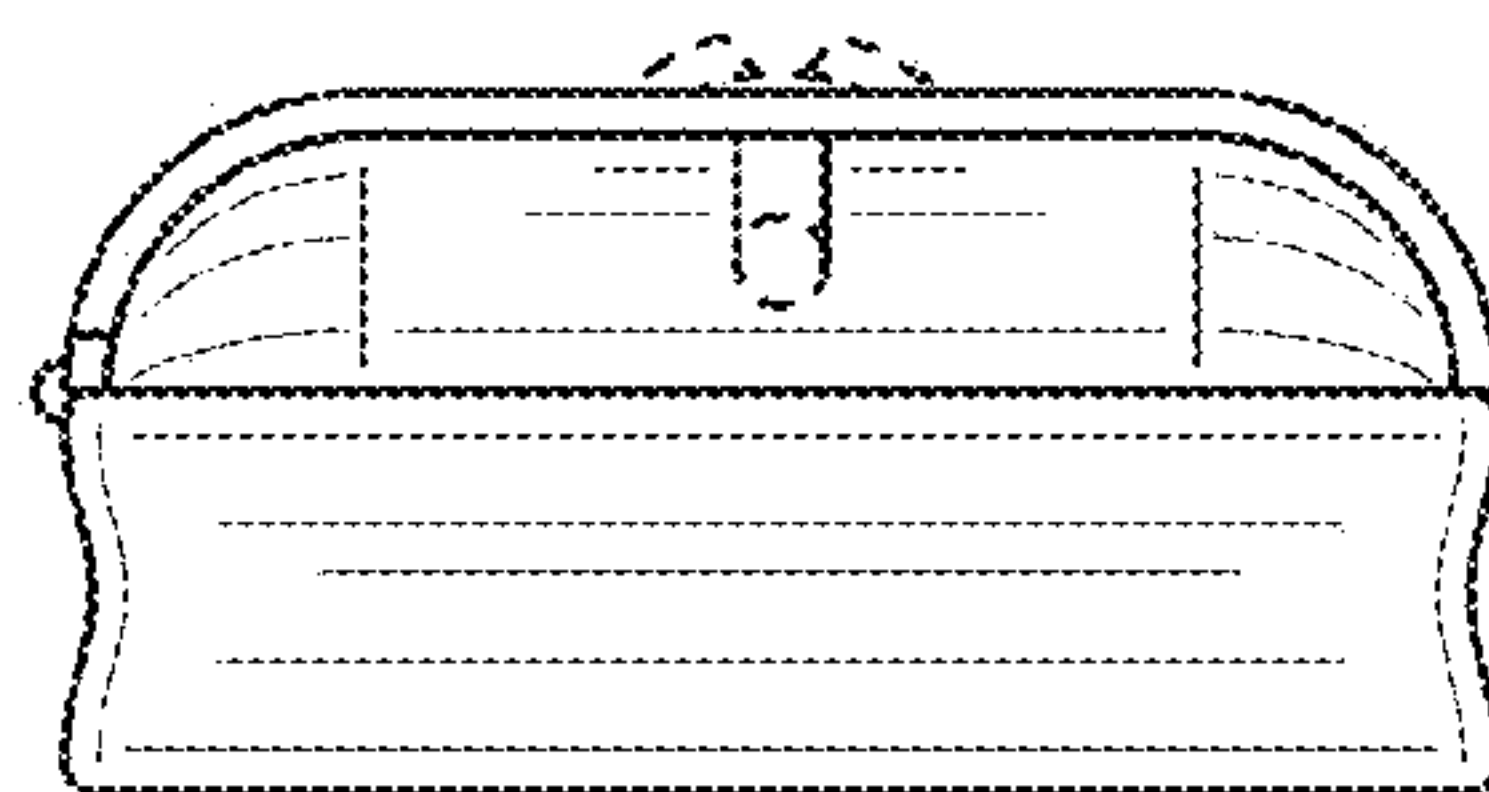


FIG. 8

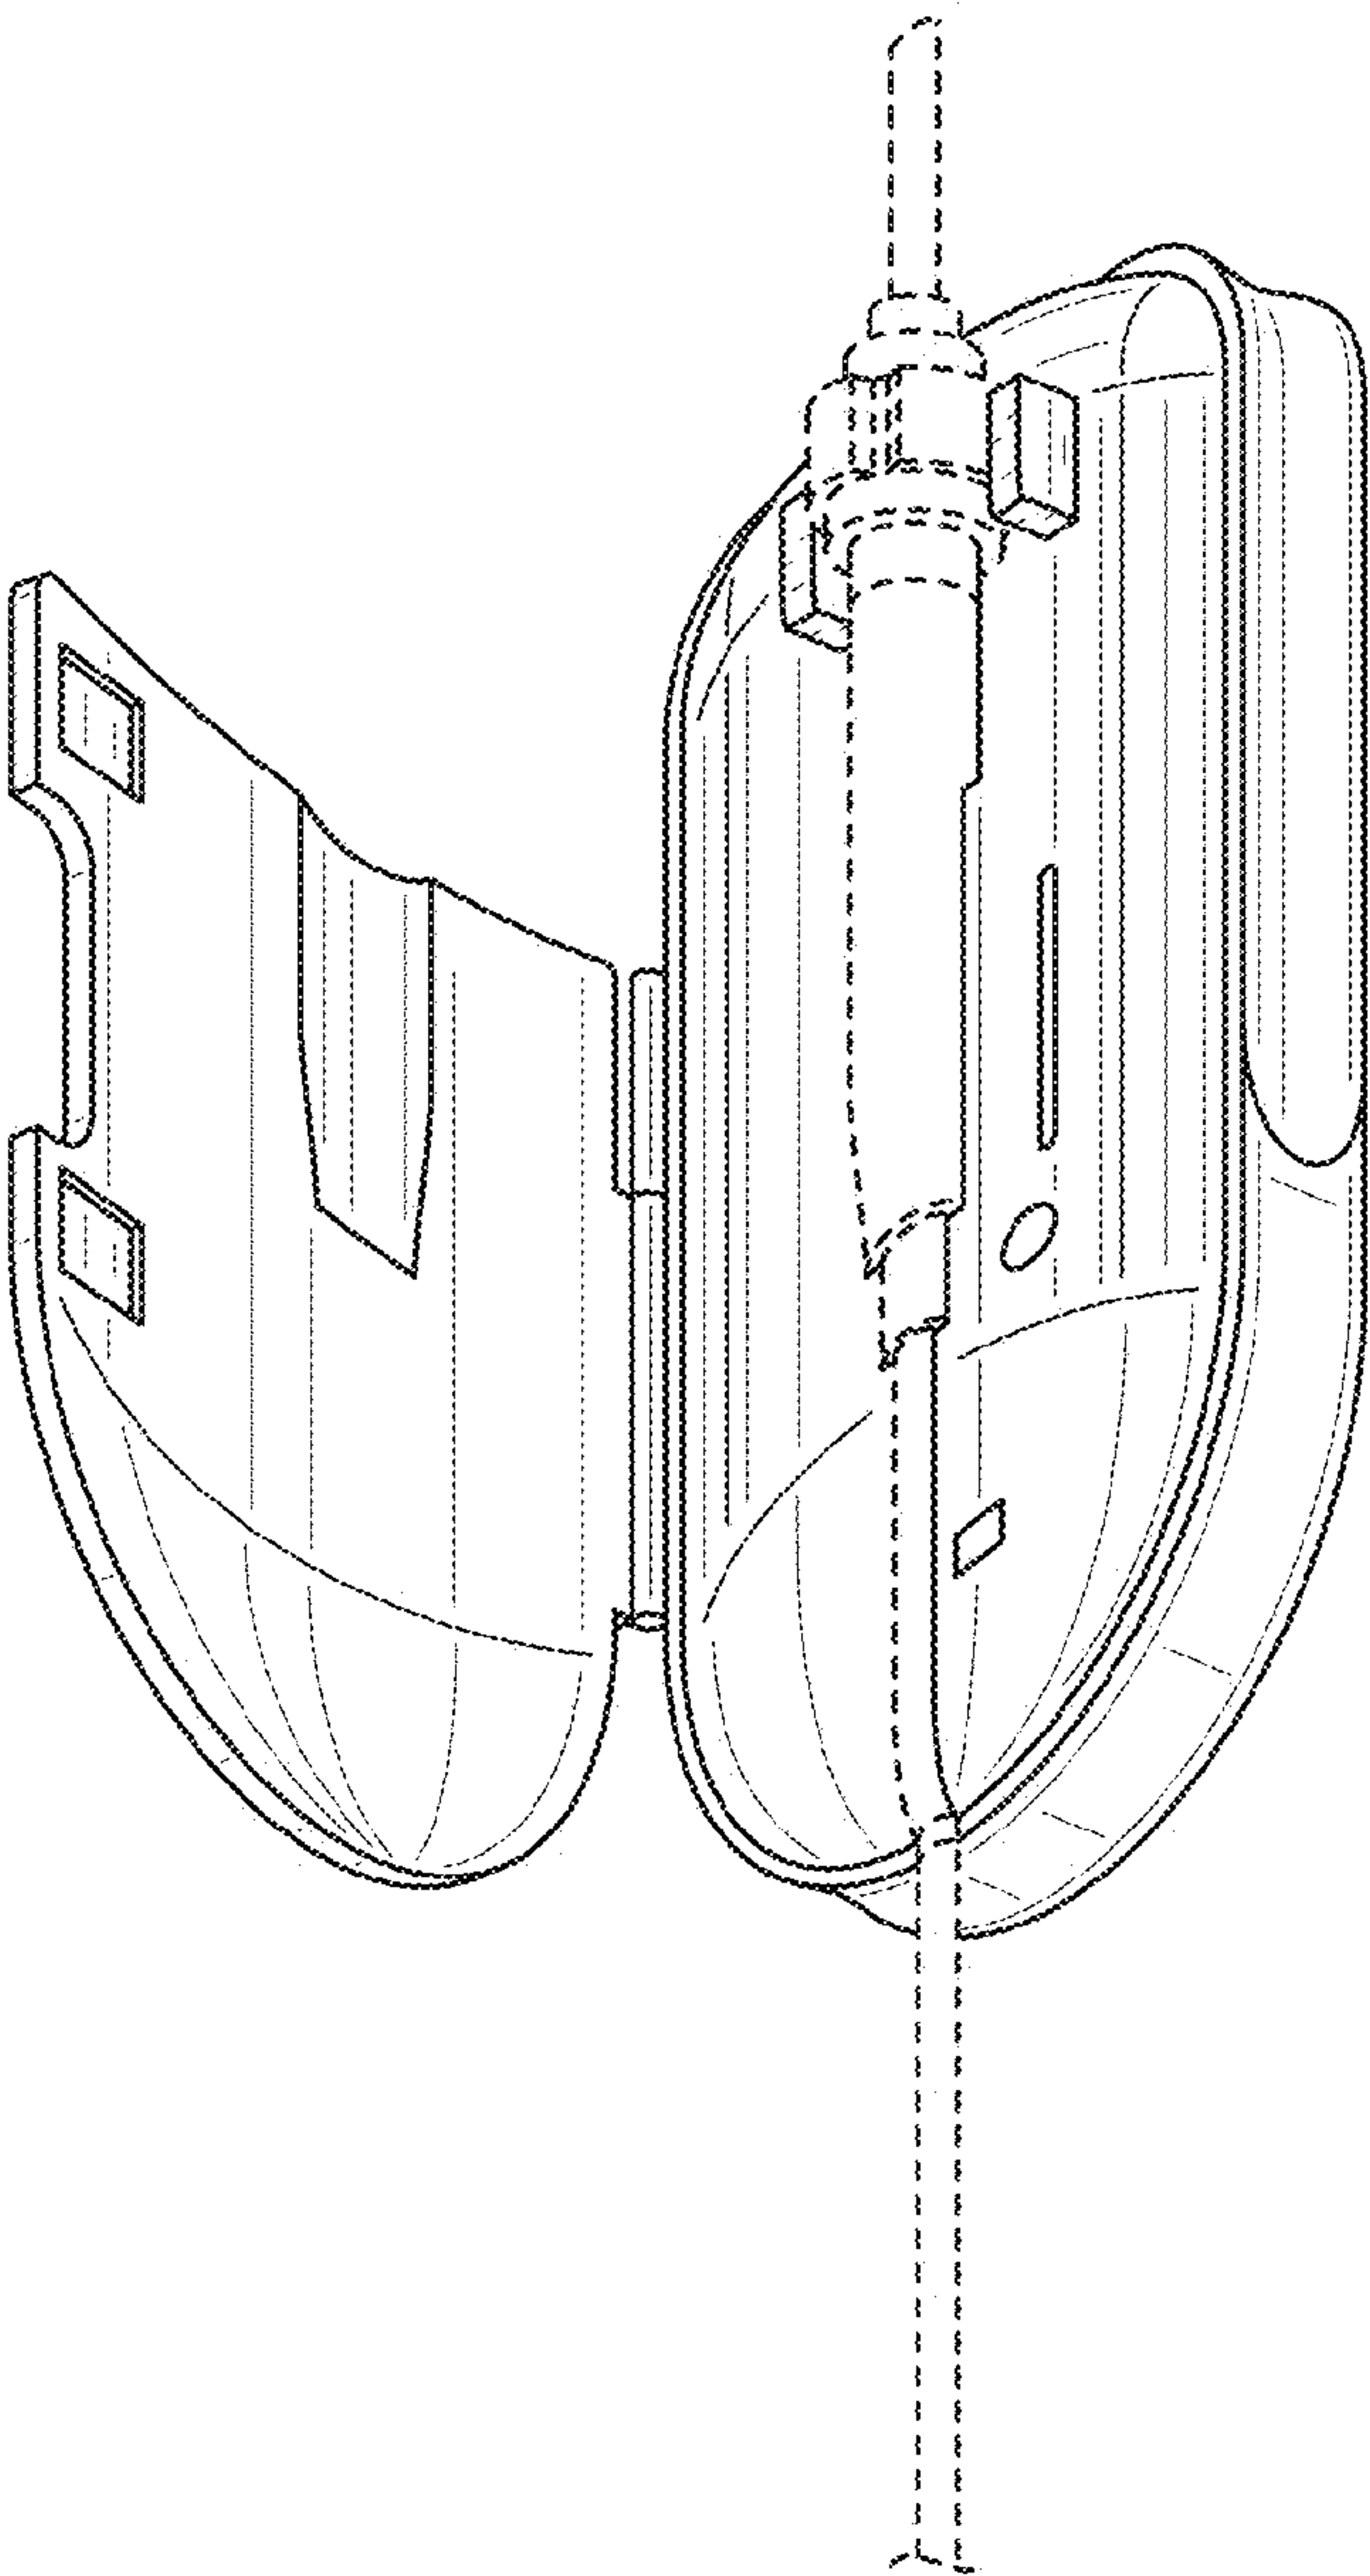


FIG. 9