



US00D746995S

(12) **United States Design Patent**
Matsumura et al.

(10) **Patent No.:** **US D746,995 S**
(45) **Date of Patent:** **** Jan. 5, 2016**

(54) **ULTRASONIC PROBE**

(71) Applicant: **GE MEDICAL SYSTEMS GLOBAL TECHNOLOGY COMPANY, LLC**,
Waukesha, WI (US)

(72) Inventors: **Kiyoshi Matsumura**, Tokyo (JP); **Koji Yanagihara**, Tokyo (JP)

(73) Assignee: **General Electric Company**,
Schenectady, NY (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/500,932**

(22) Filed: **Aug. 29, 2014**

(30) **Foreign Application Priority Data**

Mar. 3, 2014 (JP) 2014-004462

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/138, 186-187, 133; D10/78;
600/407, 446, 459, 461; 378/98.7,
378/98.8, 189
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D389,918	S	*	1/1998	Ninomiya et al.	D24/186
D389,919	S	*	1/1998	Ninomiya et al.	D24/186
6,709,392	B1	*	3/2004	Salgo et al.	600/439
D616,991	S	*	6/2010	Kitayama	D24/186
D622,401	S	*	8/2010	Suzuki	D24/187
D667,557	S	*	9/2012	Boudier	D24/186
D679,021	S	*	3/2013	Tani et al.	D24/187
D681,820	S	*	5/2013	Shinohara et al.	D24/186
D681,823	S	*	5/2013	Shinohara et al.	D24/186
D681,825	S	*	5/2013	Shinohara et al.	D24/186

D681,827	S	*	5/2013	Shinohara et al.	D24/186
D681,828	S	*	5/2013	Shinohara et al.	D24/186
D685,100	S	*	6/2013	Shinohara et al.	D24/186
D701,606	S		3/2014	Ohmukai		
D701,608	S		3/2014	Baba		
D701,965	S		4/2014	Matsumura et al.		
D703,330	S		4/2014	Saeki		
D703,331	S		4/2014	Kitayama		
D703,332	S		4/2014	Saeki		
D703,333	S		4/2014	Saeki		
D704,341	S		5/2014	Ryu et al.		
D704,844	S		5/2014	Saeki		

* cited by examiner

Primary Examiner — T. Chase Nelson
Assistant Examiner — Mark Cavanna

(57) **CLAIM**

The ornamental design for an ultrasonic probe, as shown and described.

DESCRIPTION

FIG. 1 is a front view of an ultrasonic probe showing our new design.

FIG. 2 is a left view of the ultrasonic probe design shown in FIG. 1;

FIG. 3 is a front perspective view of the ultrasonic probe design shown in FIG. 1.

FIG. 4 is a rear perspective view of the ultrasonic probe design shown in FIG. 1;

FIG. 5 is a bottom perspective view of the ultrasonic probe design shown in FIG. 1;


FIG. 6 is a top view of the ultrasonic probe design shown in FIG. 1;

FIG. 7 is a rear view of the ultrasonic probe design shown in FIG. 1;

FIG. 8 is a right view of the ultrasonic probe design shown in FIG. 1; and,

FIG. 9 is a bottom view of the ultrasonic probe design shown in FIG. 1.

1 Claim, 9 Drawing Sheets

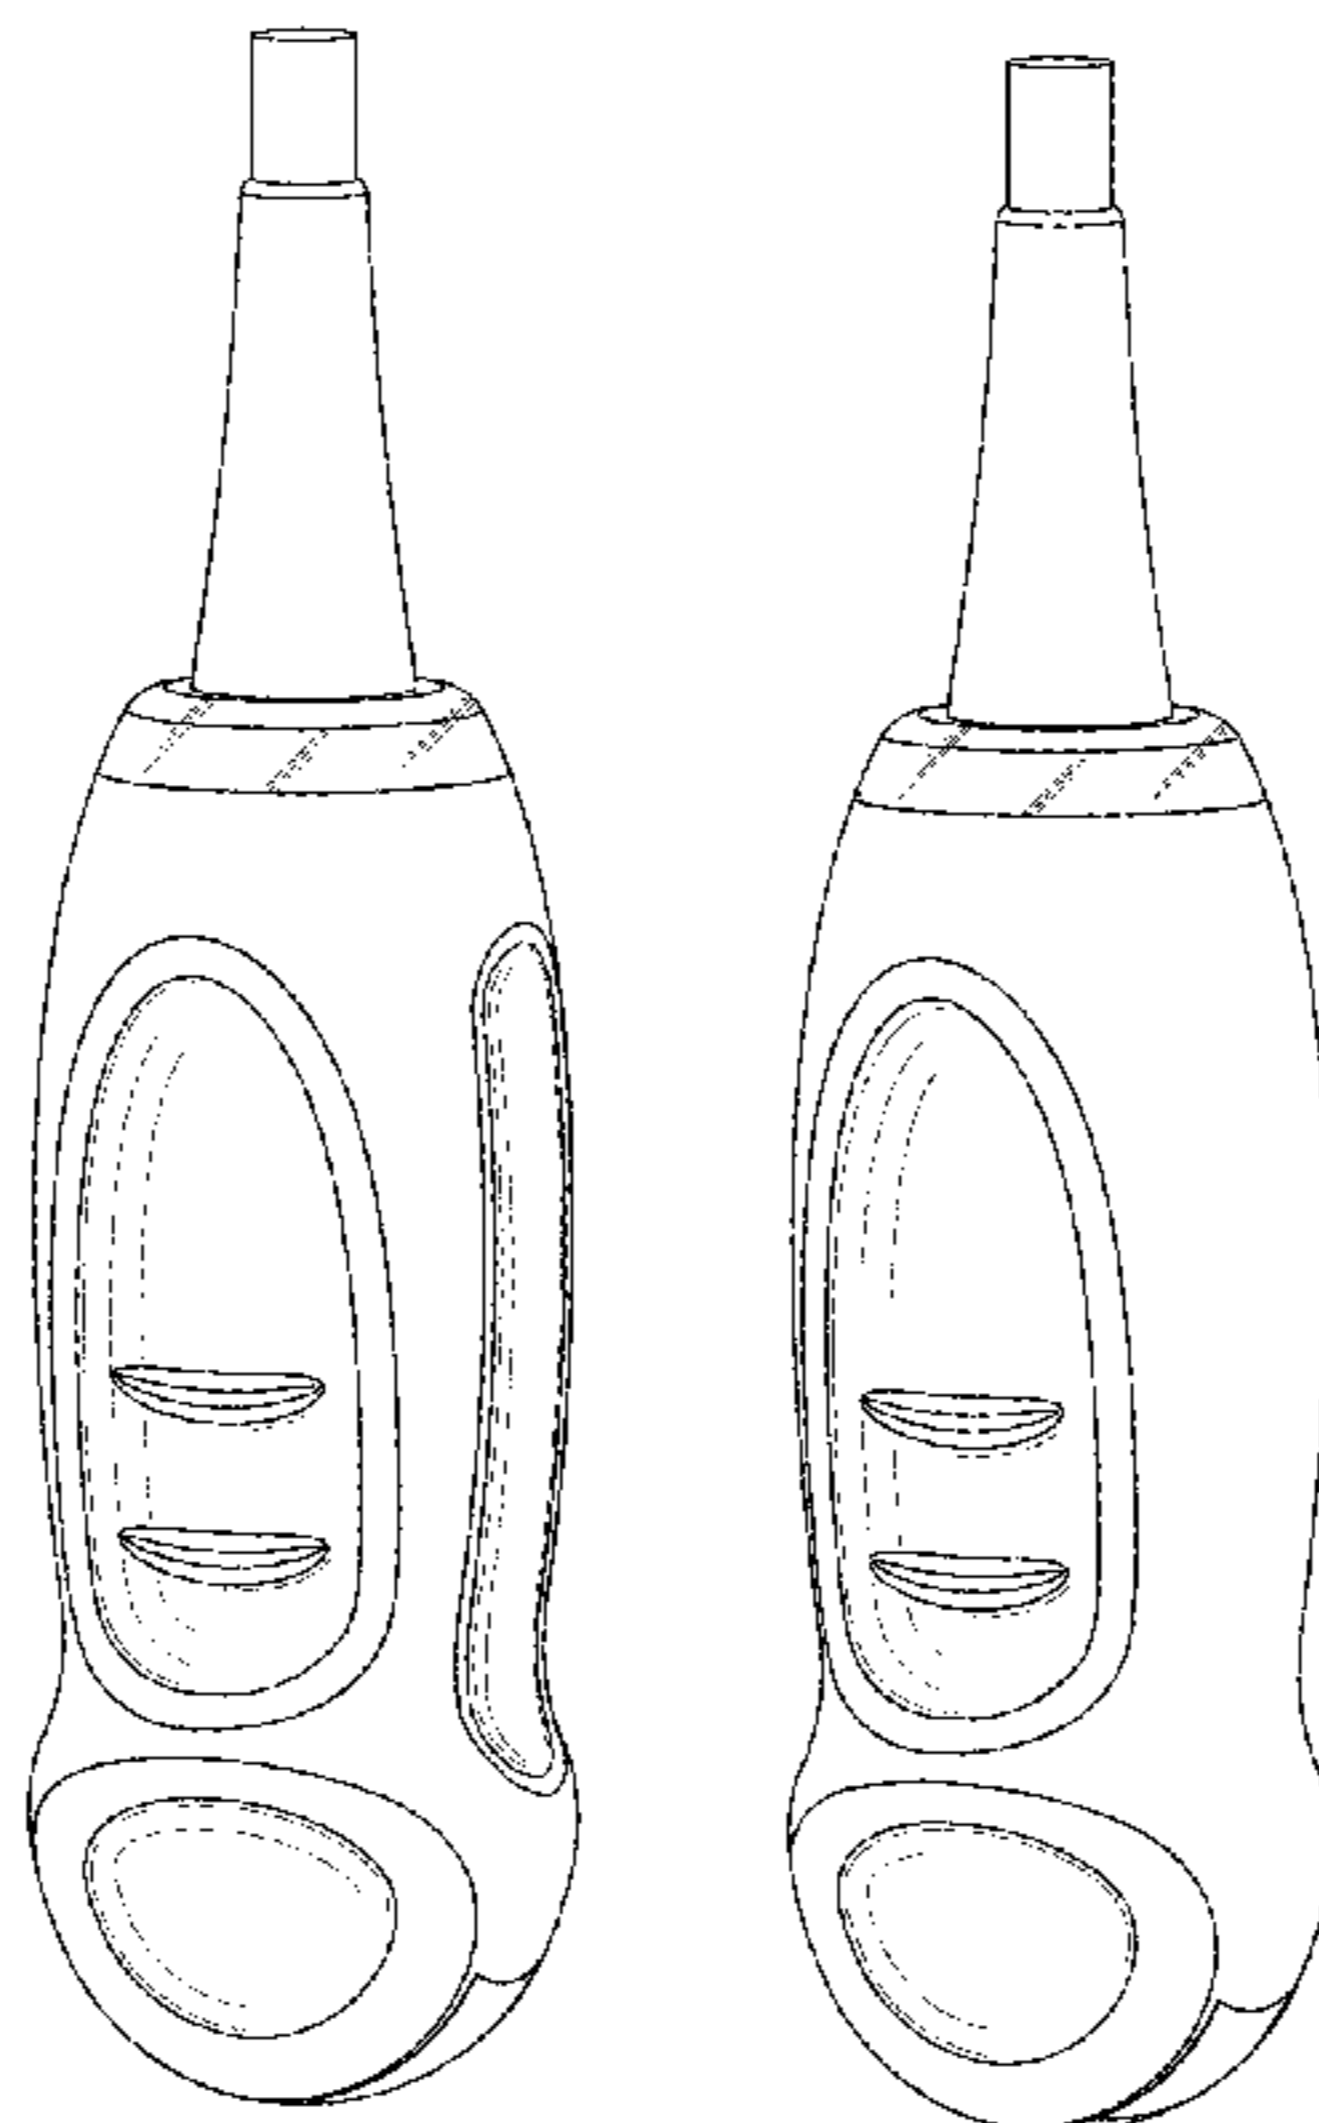

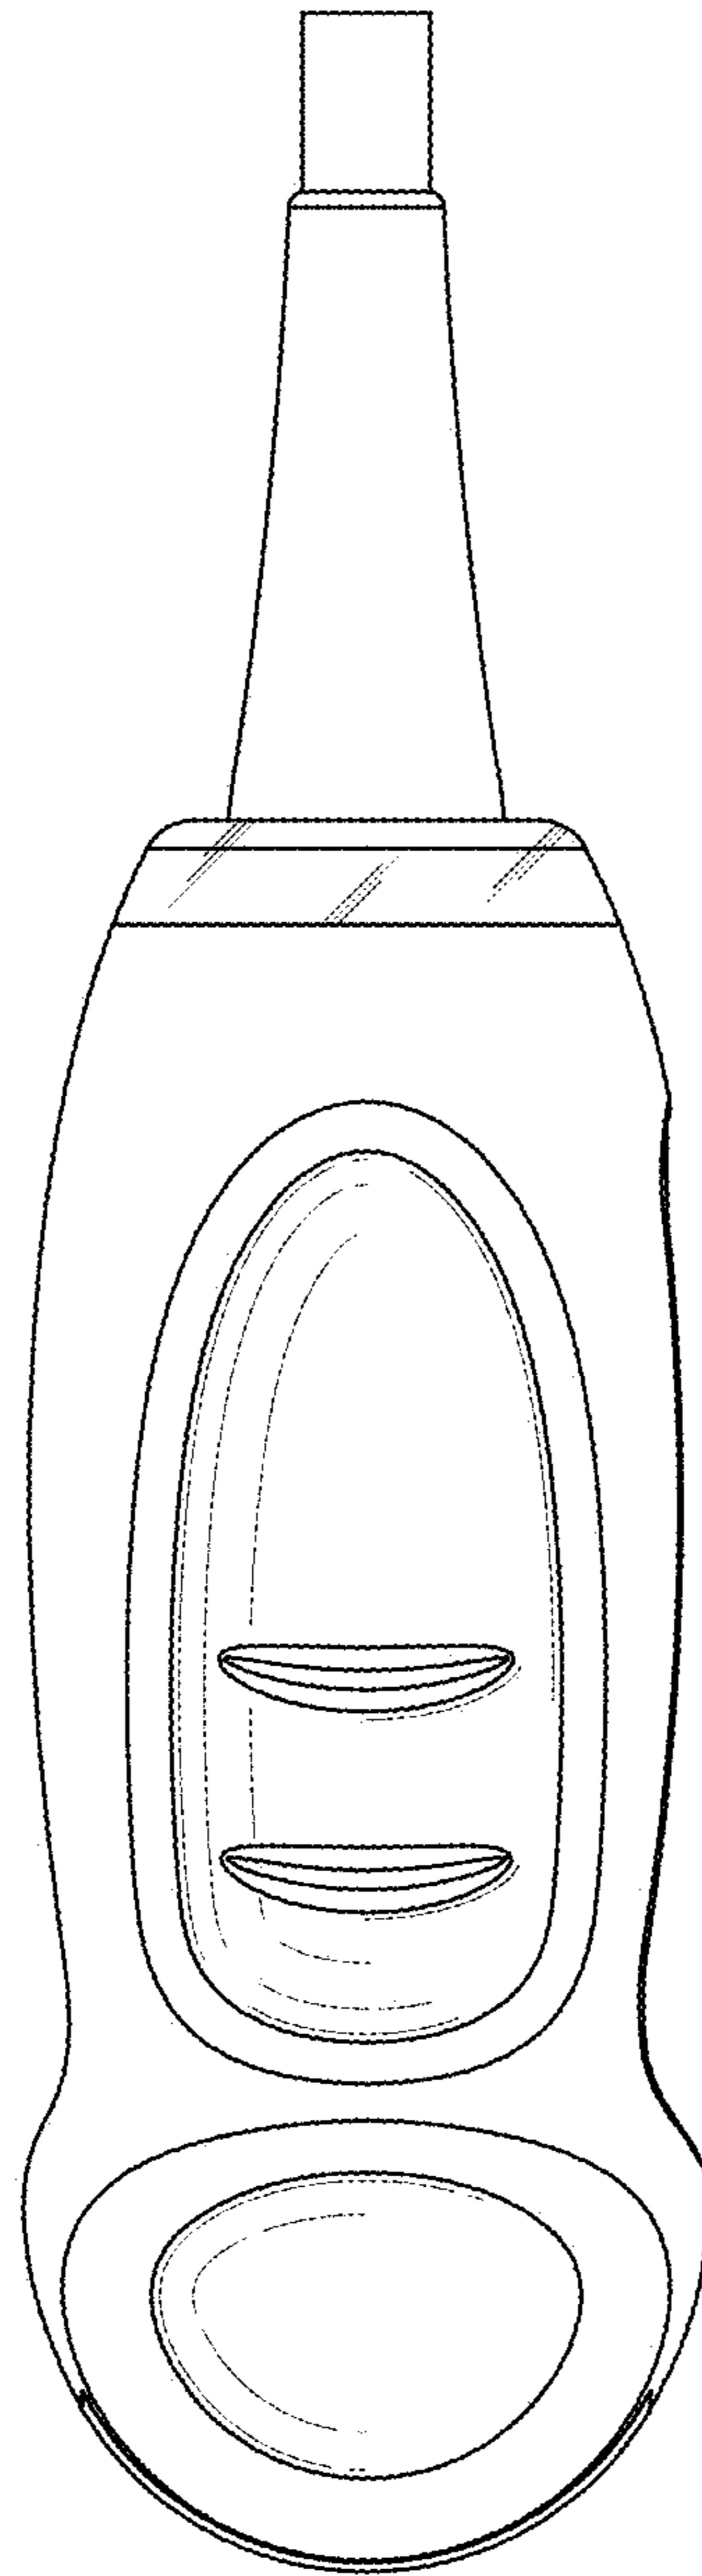


FIG. 1

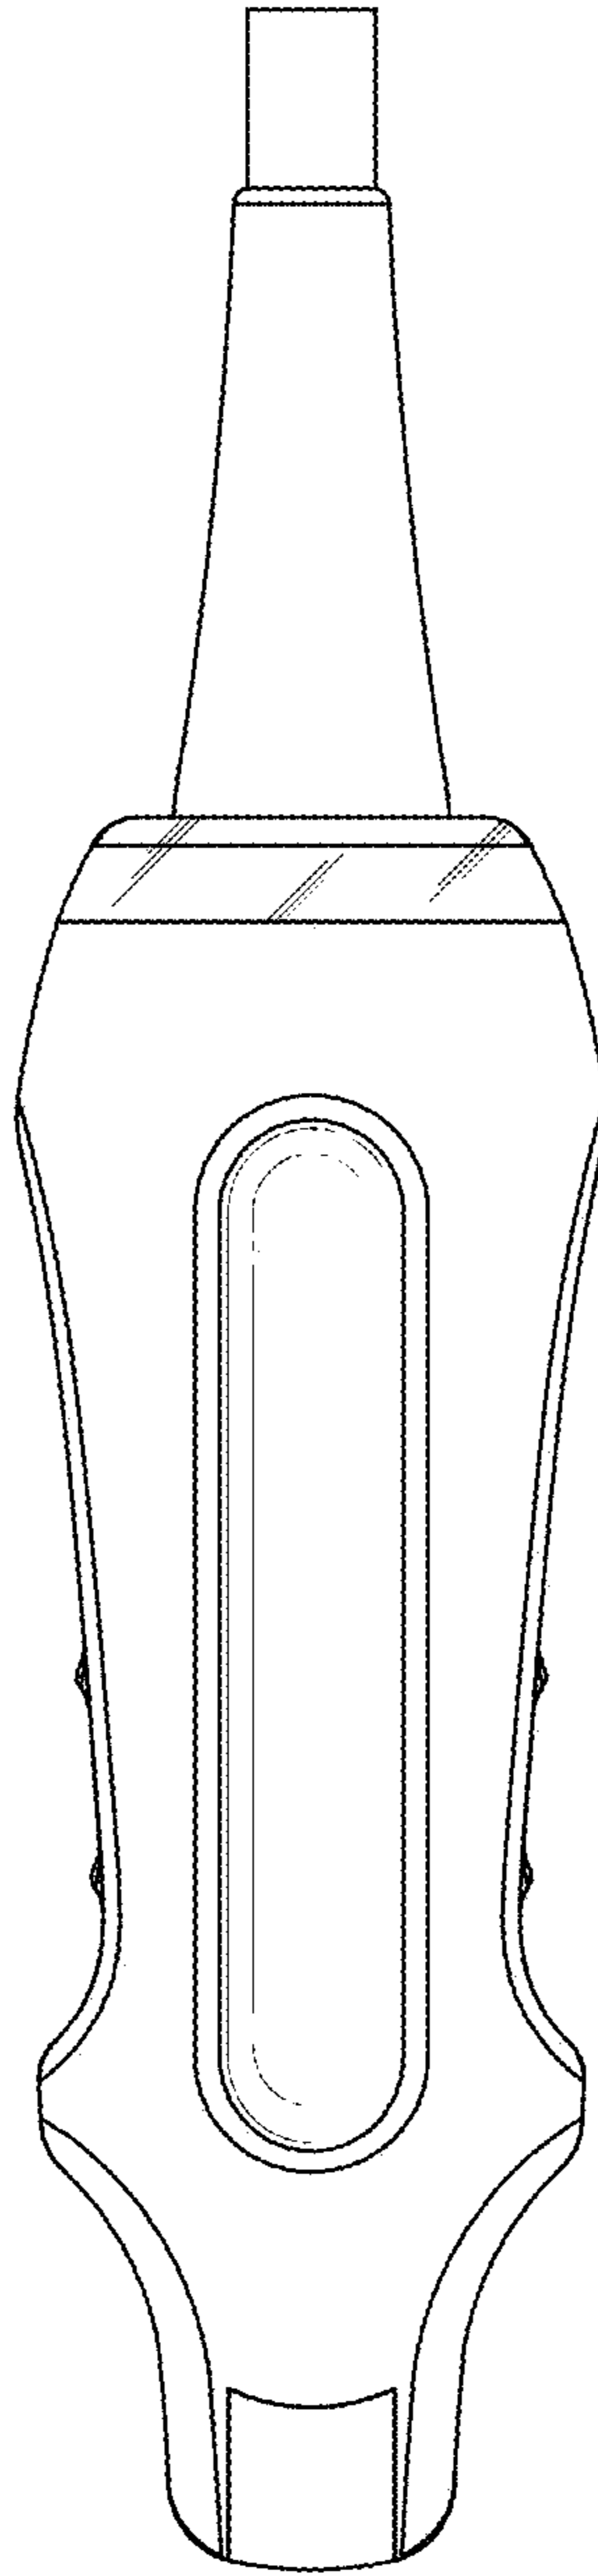


FIG. 2

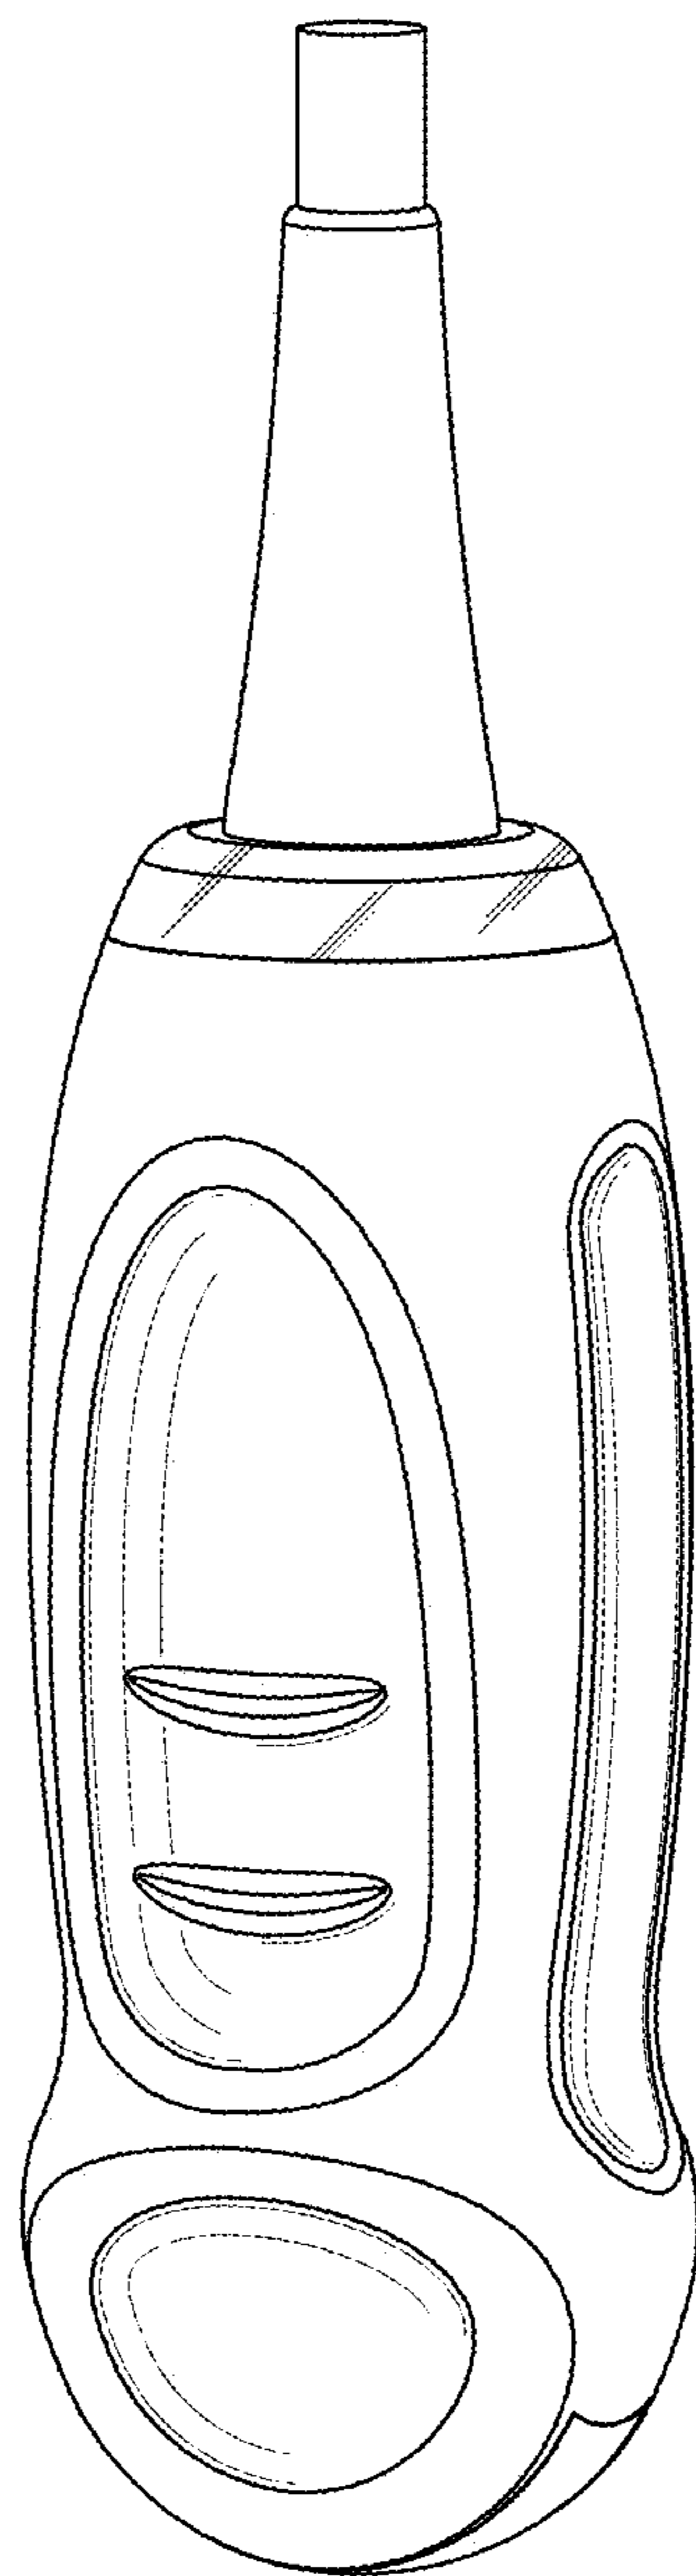


FIG. 3

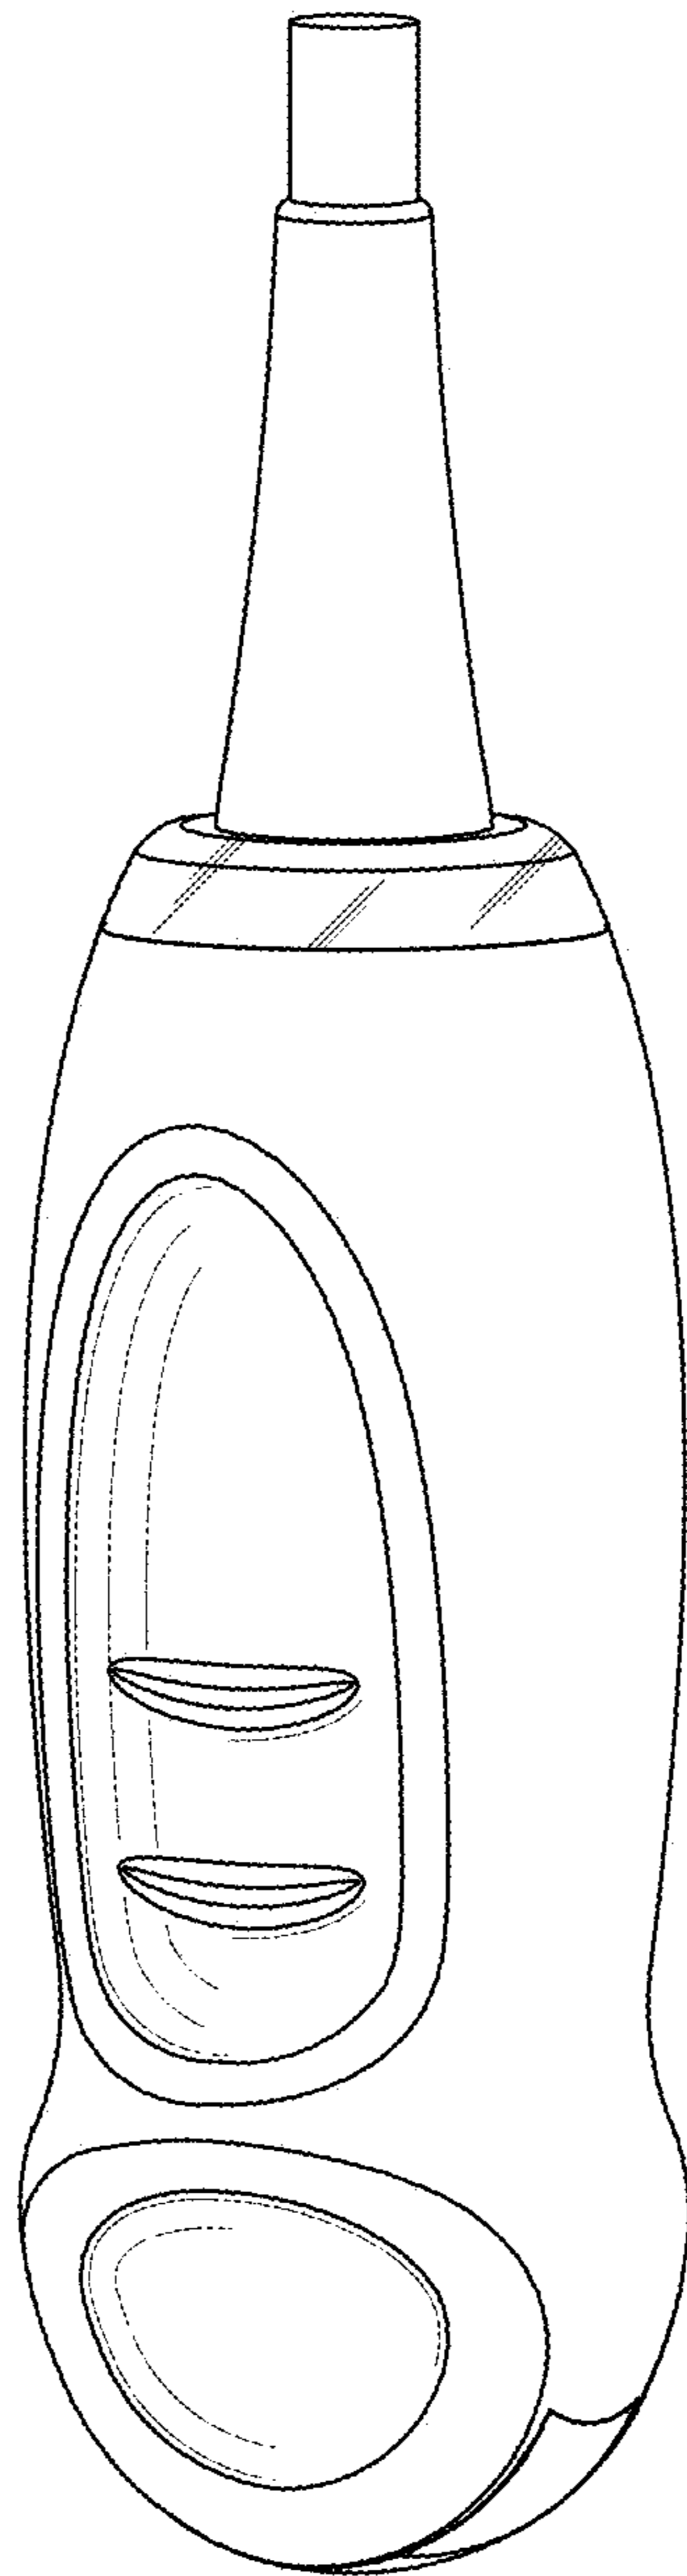


FIG. 4

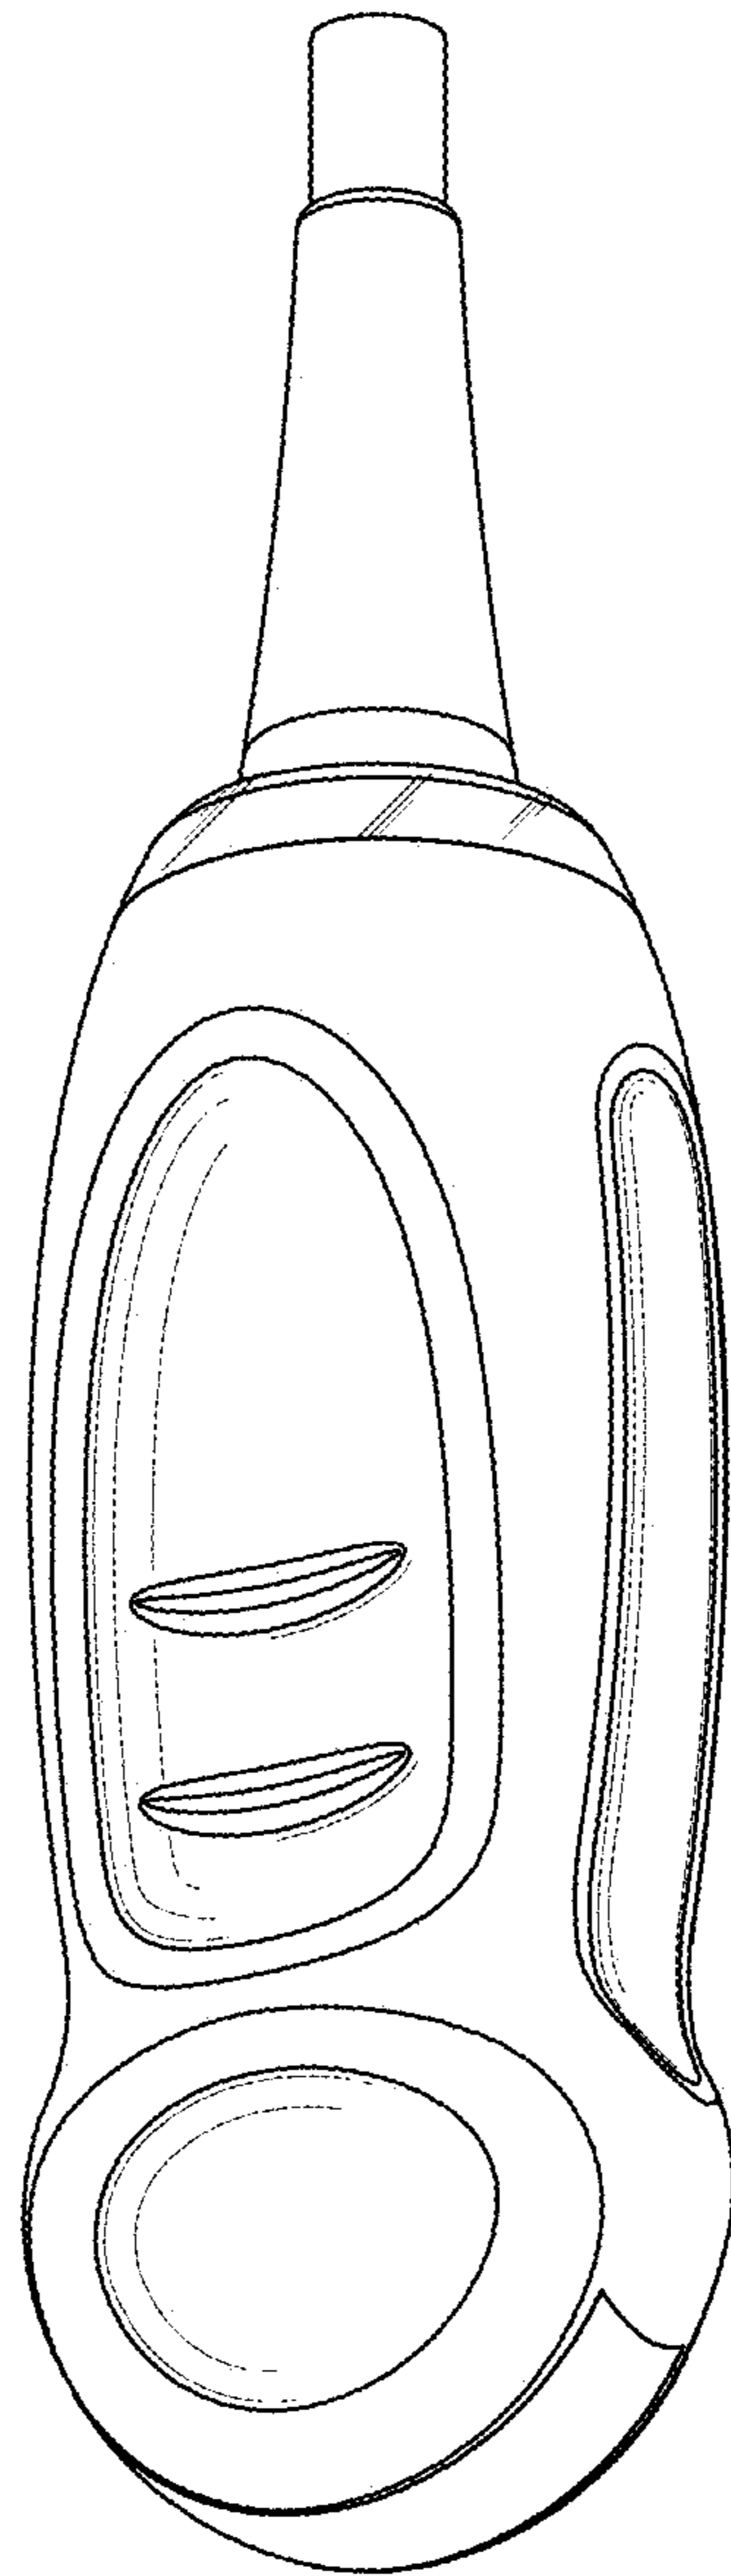


FIG. 5

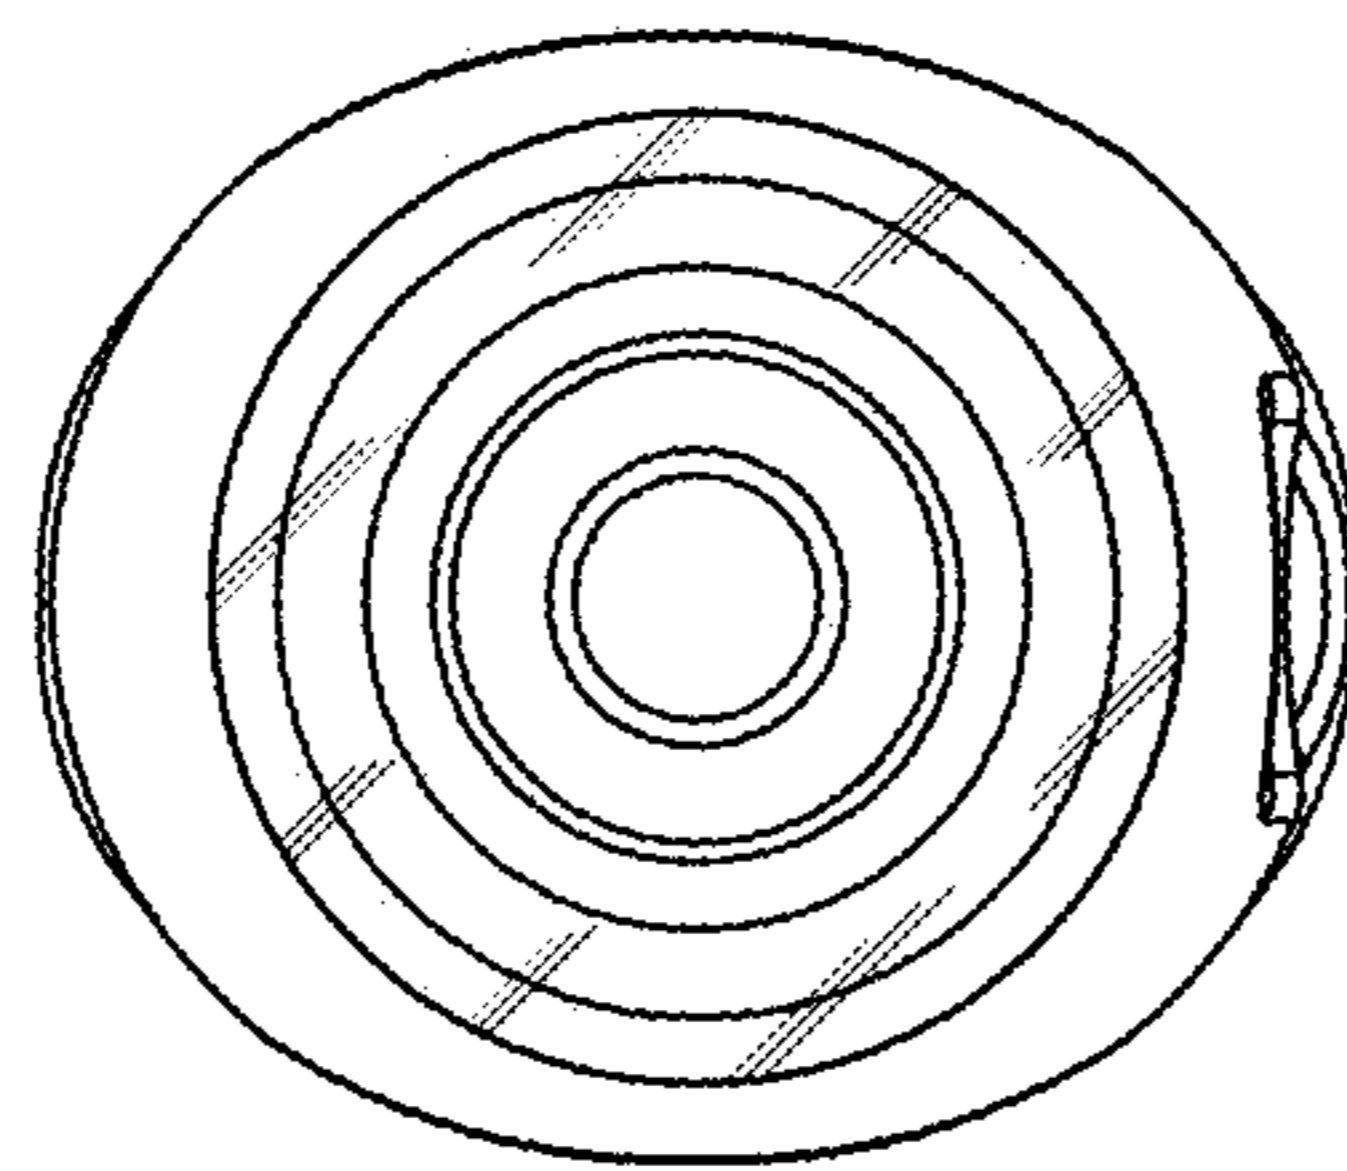


FIG. 6

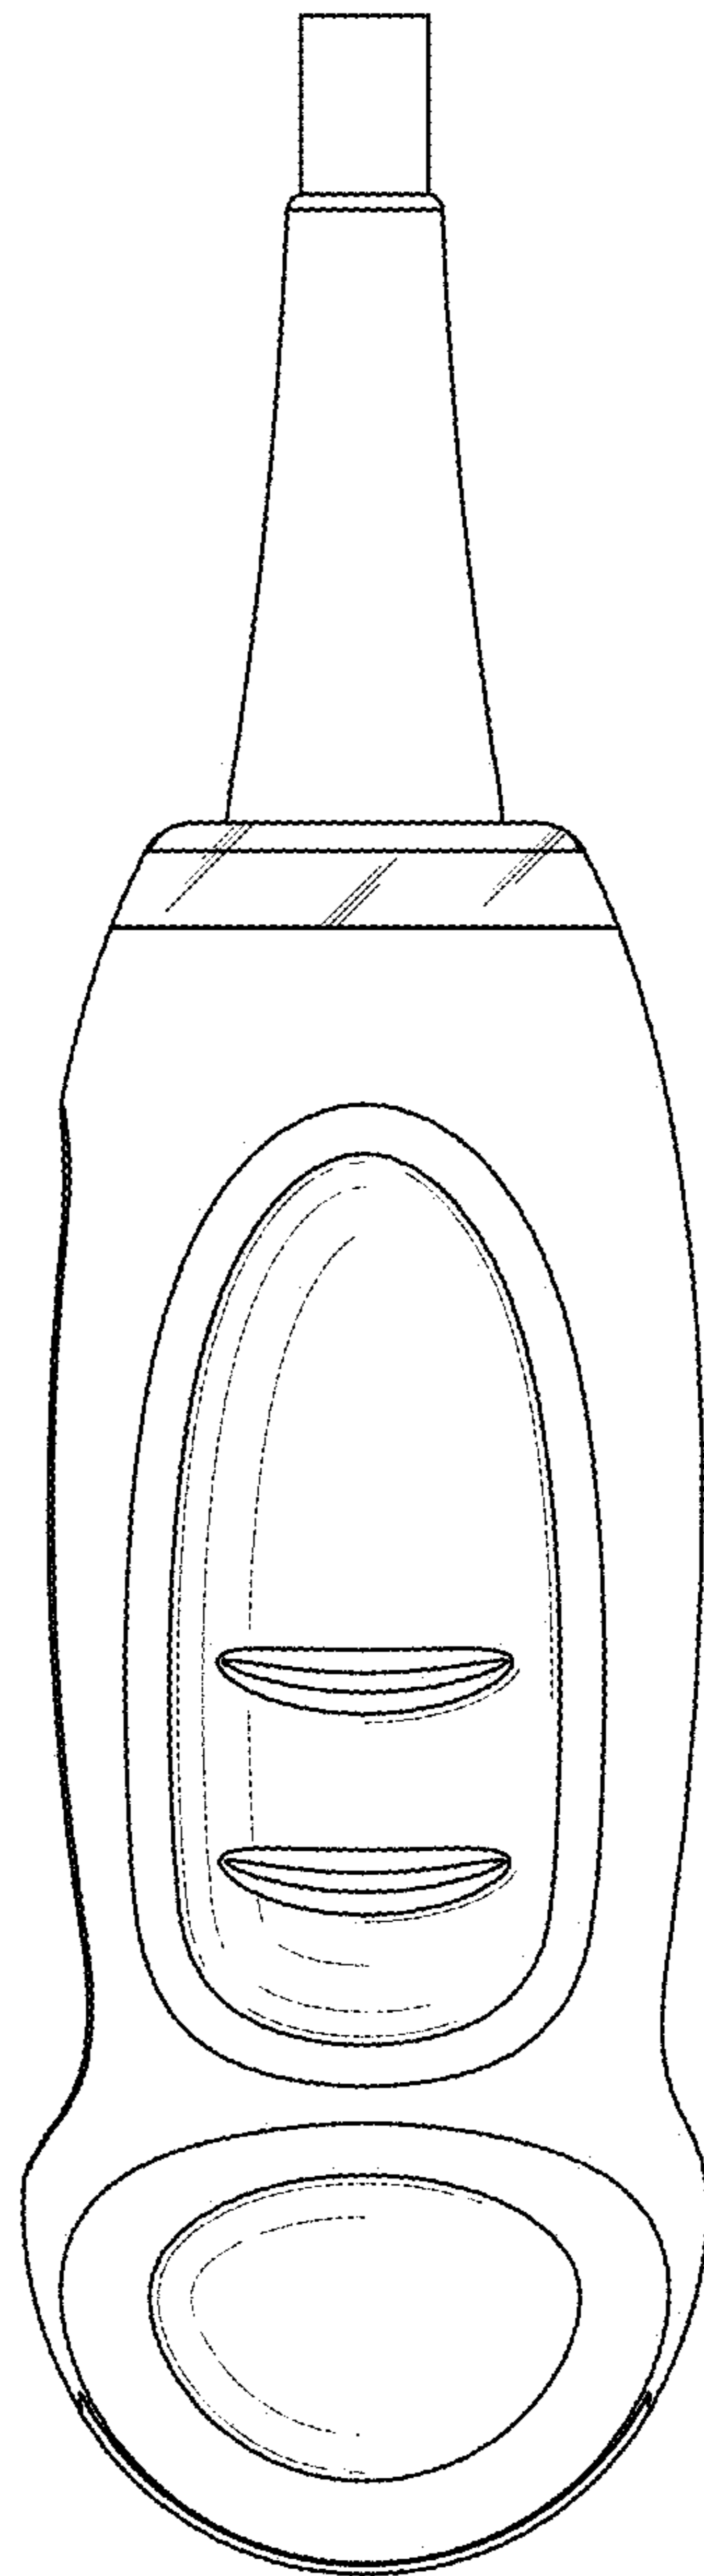


FIG. 7

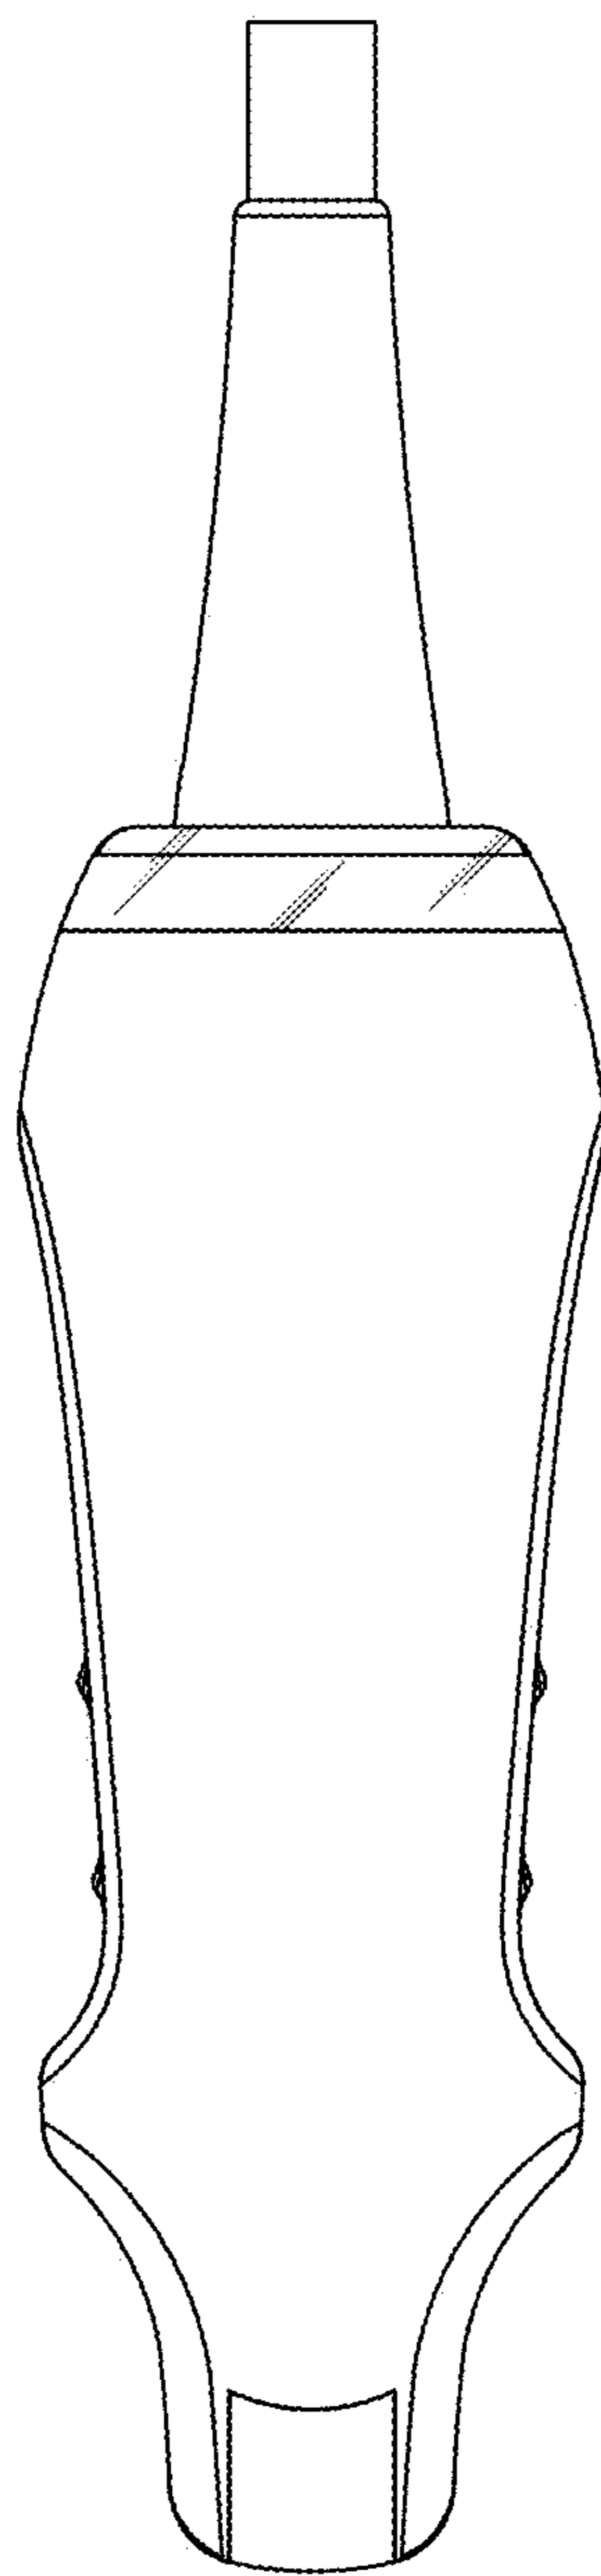


FIG. 8

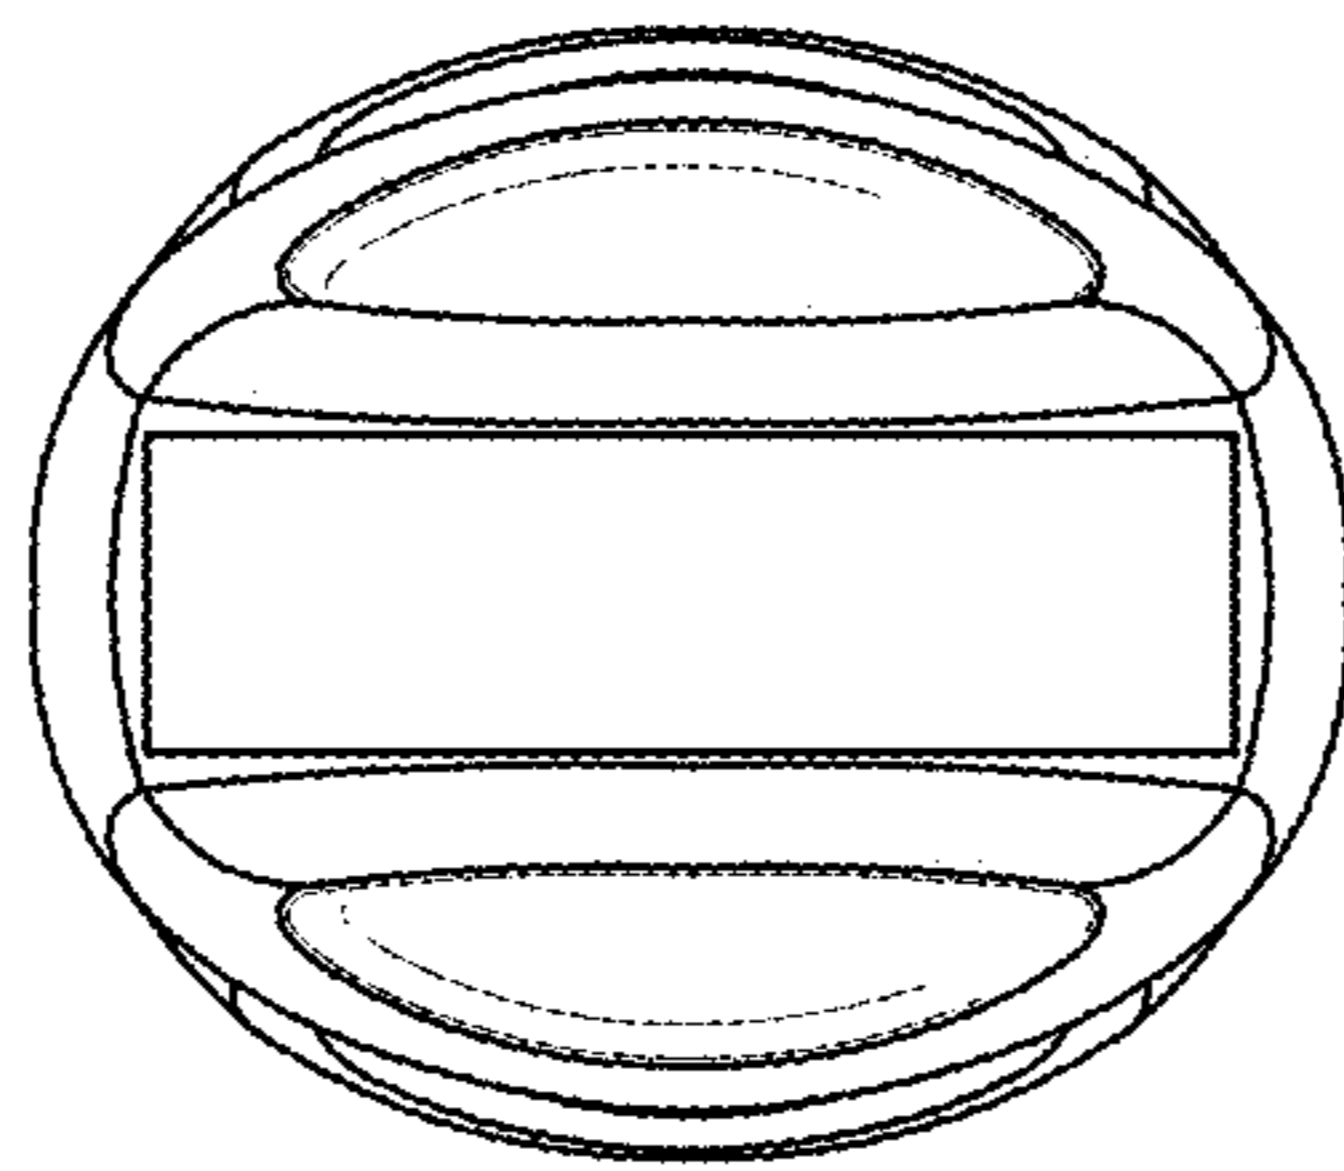


FIG. 9