



US00D747490S

(12) **United States Design Patent**
Harkin et al.

(10) **Patent No.:** **US D747,490 S**
(45) **Date of Patent:** **** Jan. 12, 2016**

(54) **BLOOD GLUCOSE METER**

(71) Applicant: **Roche Diabetes Care, Inc.**,
Indianapolis, IN (US)
(72) Inventors: **Thomas Z. Harkin**, Bristol (GB);
Sebastian Liedtke, Heidelberg (DE);
Anthony J. Uberta, III, Indianapolis, IN
(US); **Scott A. Wooldridge**, Carmel, IN
(US)

(73) Assignee: **Roche Diabetes Care, Inc.**,
Indianapolis, IN (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/510,579**

(22) Filed: **Dec. 1, 2014**

Related U.S. Application Data

(62) Division of application No. 29/490,202, filed on May 7, 2014, now Pat. No. Des. 721,178.

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/169**

(58) **Field of Classification Search**
USPC D24/216, 223, 231, 232, 107, 169, 186;
D10/81; 422/68.1, 420, 500;
435/287.1, 287.3; 436/43, 45, 47;
600/309, 365, 368, 583, 584
CPC . G01N 33/48707; G01N 33/52; G01N 33/49;
G01N 33/492

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D406,895 S	3/1999	Byrd et al.	
D545,436 S	6/2007	Padain	
D546,457 S	7/2007	Hannant et al.	
D546,458 S	7/2007	Hannant	
D611,853 S	3/2010	Salter et al.	
D648,029 S *	11/2011	Presta et al. D24/169
8,114,028 B2	2/2012	List et al.	

(Continued)

OTHER PUBLICATIONS

ACCU-CHEK® Active Meter System, www.accu-chek.com/glucose-meters/active.html (printed therefrom on Apr. 15, 2014).
ACCU-CHEK® Advantage Meter System, www.accu-chek.com/us/glucose-meters/advantage.html (printed therefrom on Apr. 15, 2014).

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Roche Diabetes Care, Inc.


(57) **CLAIM**

The ornamental design for a blood glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a blood glucose meter; FIG. 2 is a bottom perspective view of the blood glucose meter; FIG. 3 is a top view of the blood glucose meter; FIG. 4 is a bottom view of the blood glucose meter; FIG. 5 is an upper end view of the blood glucose meter; FIG. 6 is a lower end view of the blood glucose meter; FIG. 7 is a right side view of the blood glucose meter; and, FIG. 8 is a left side view of the blood glucose meter. The broken lines in the drawing views are included for the purpose of illustrating a portion of the blood glucose meter that forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

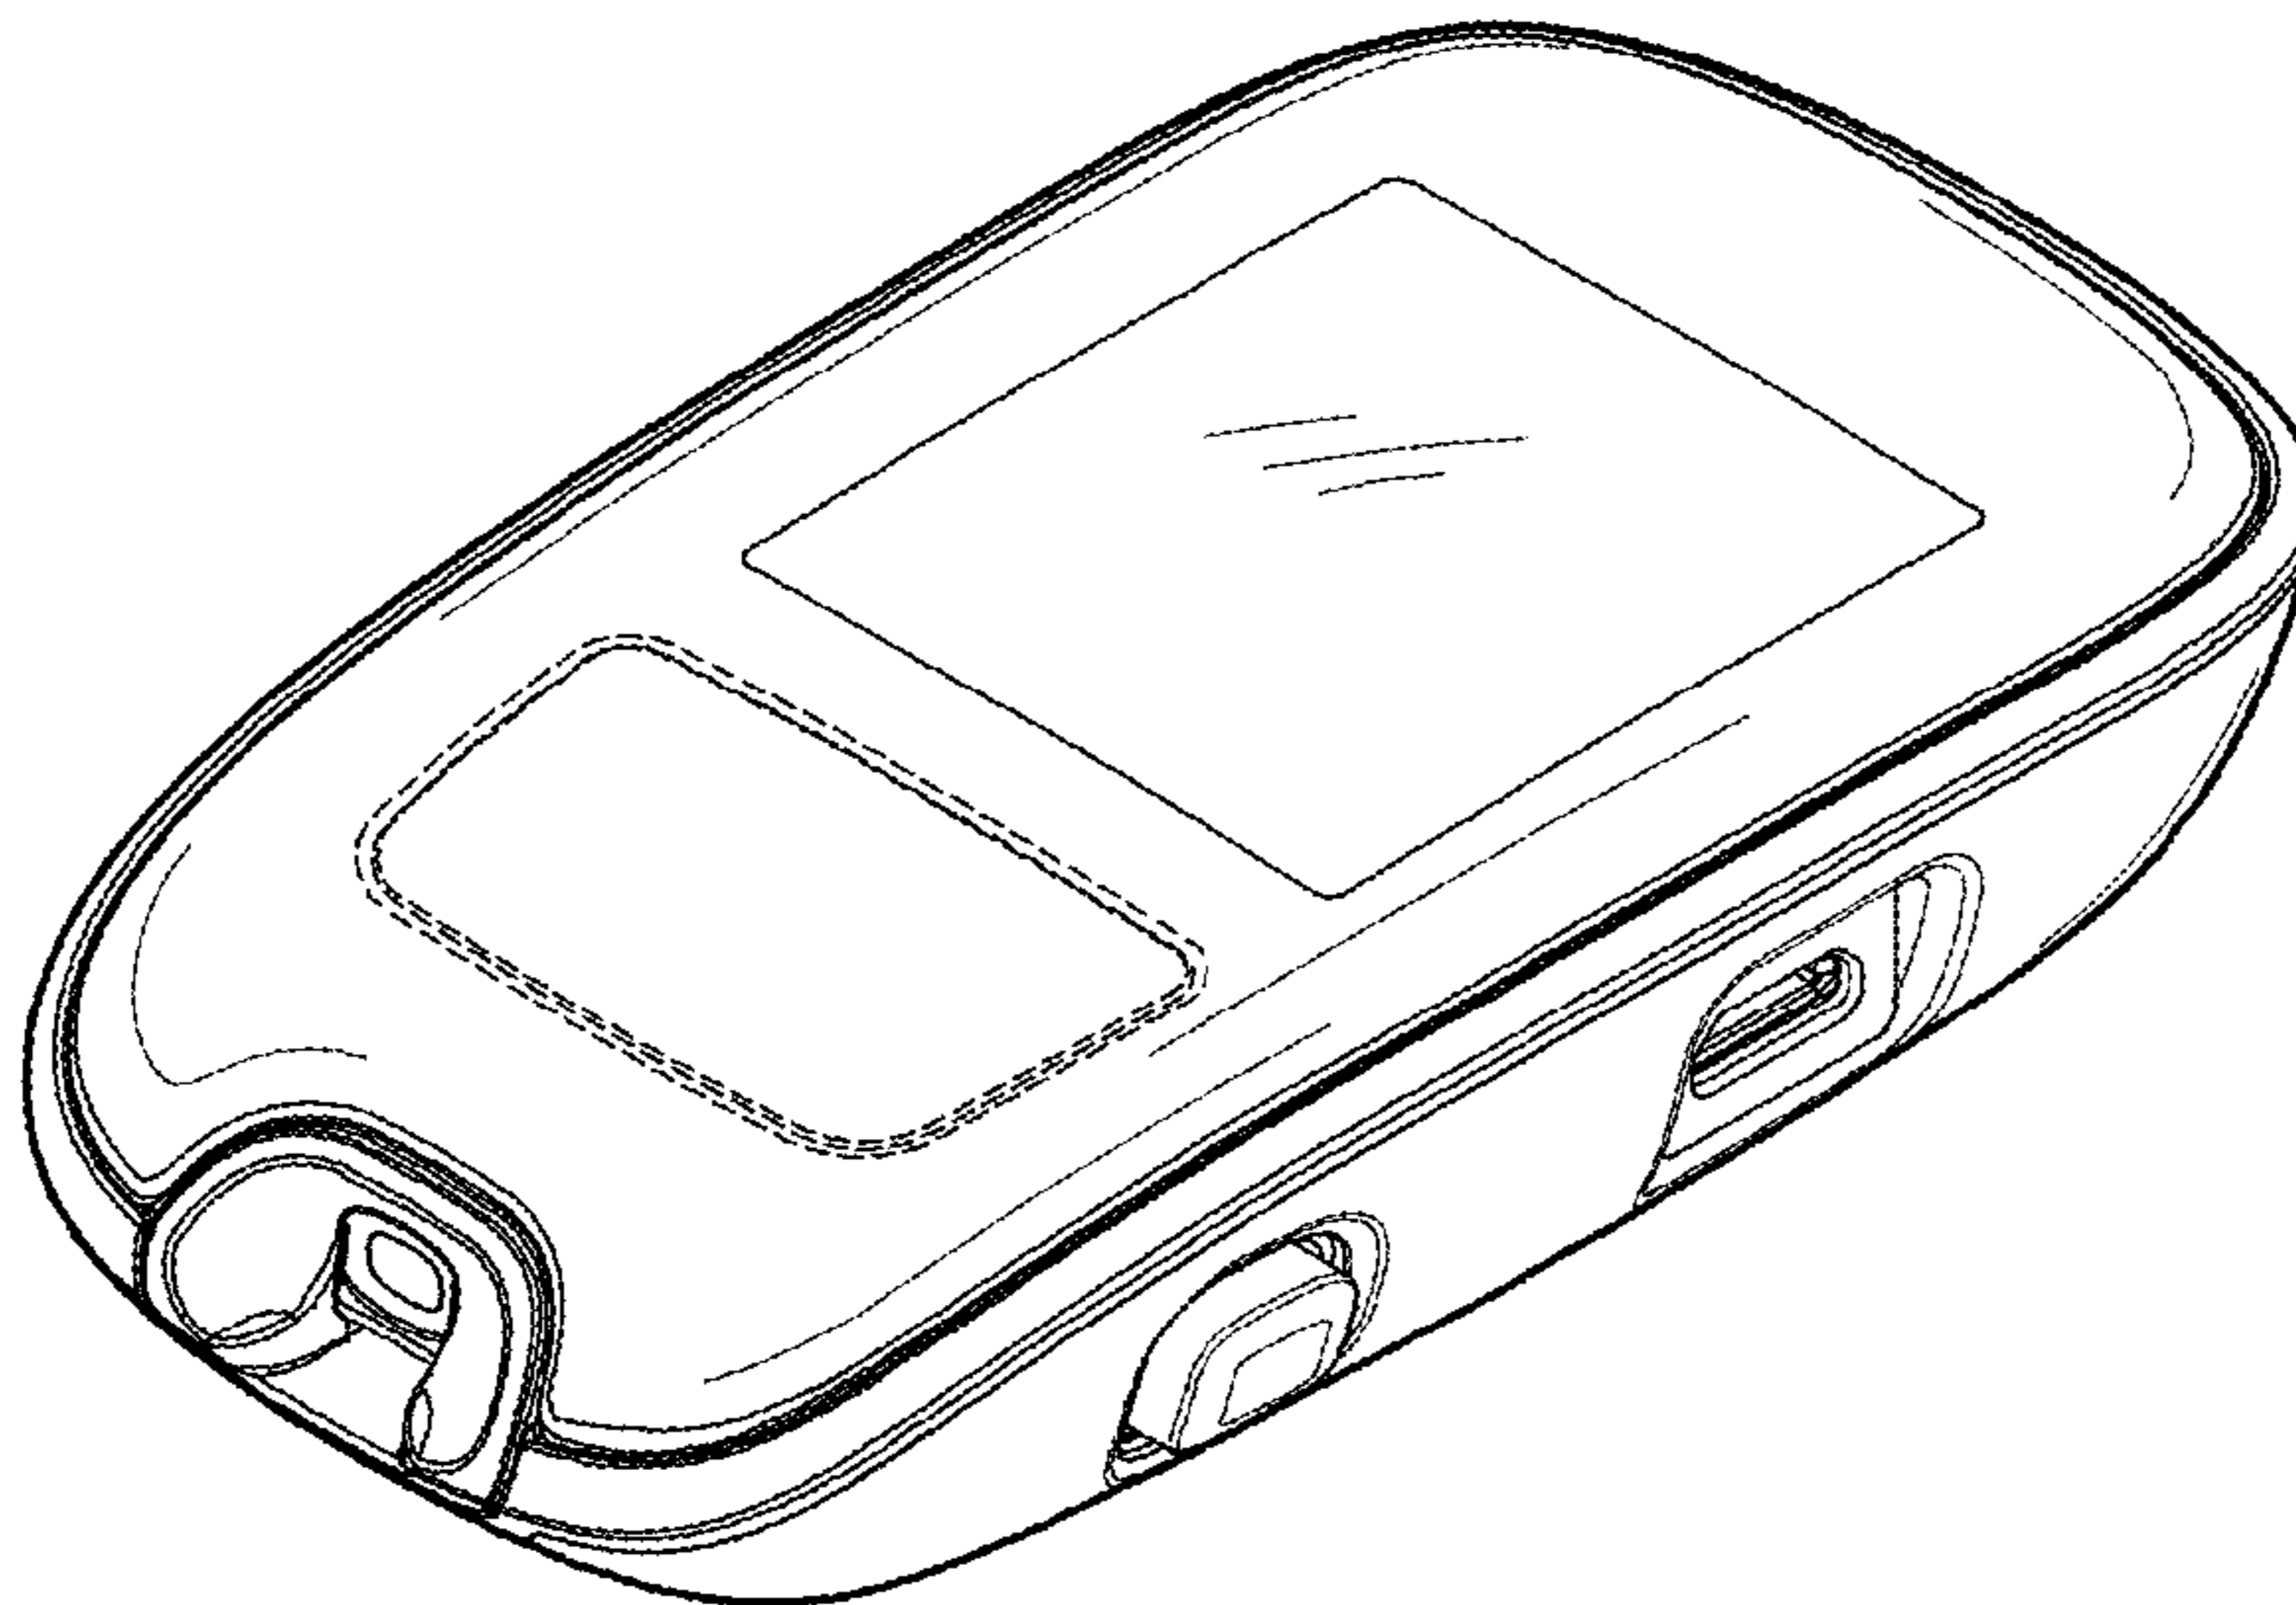

(56)

References Cited

U.S. PATENT DOCUMENTS

D696,404 S 12/2013 Golnik et al.
D713,963 S 9/2014 Liedtke et al.
2010/0113896 A1 5/2010 Cadio et al.
2010/0331650 A1 12/2010 Batman et al.
2011/0034786 A1 2/2011 Cadio et al.
2012/0221064 A1 8/2012 Wooldridge
2014/0051958 A1* 2/2014 Fern et al. 600/365

OTHER PUBLICATIONS

ACCU-CHEK® Aviva Plus System, www.accu-chek.com/us/glucose-meters/aviva.html (printed therefrom on Apr. 15, 2014).
ACCU-CHEK® Compact Plus Meter System, www.accu-chek.com/us/glucose-meters/compact-plus.html (printed therefrom on Apr. 15, 2014).
ACCU-CHEK® Nano Meter, www.accu-chek.com/us/glucose-meters/nano.html (printed therefrom on Apr. 15, 2014).

* cited by examiner

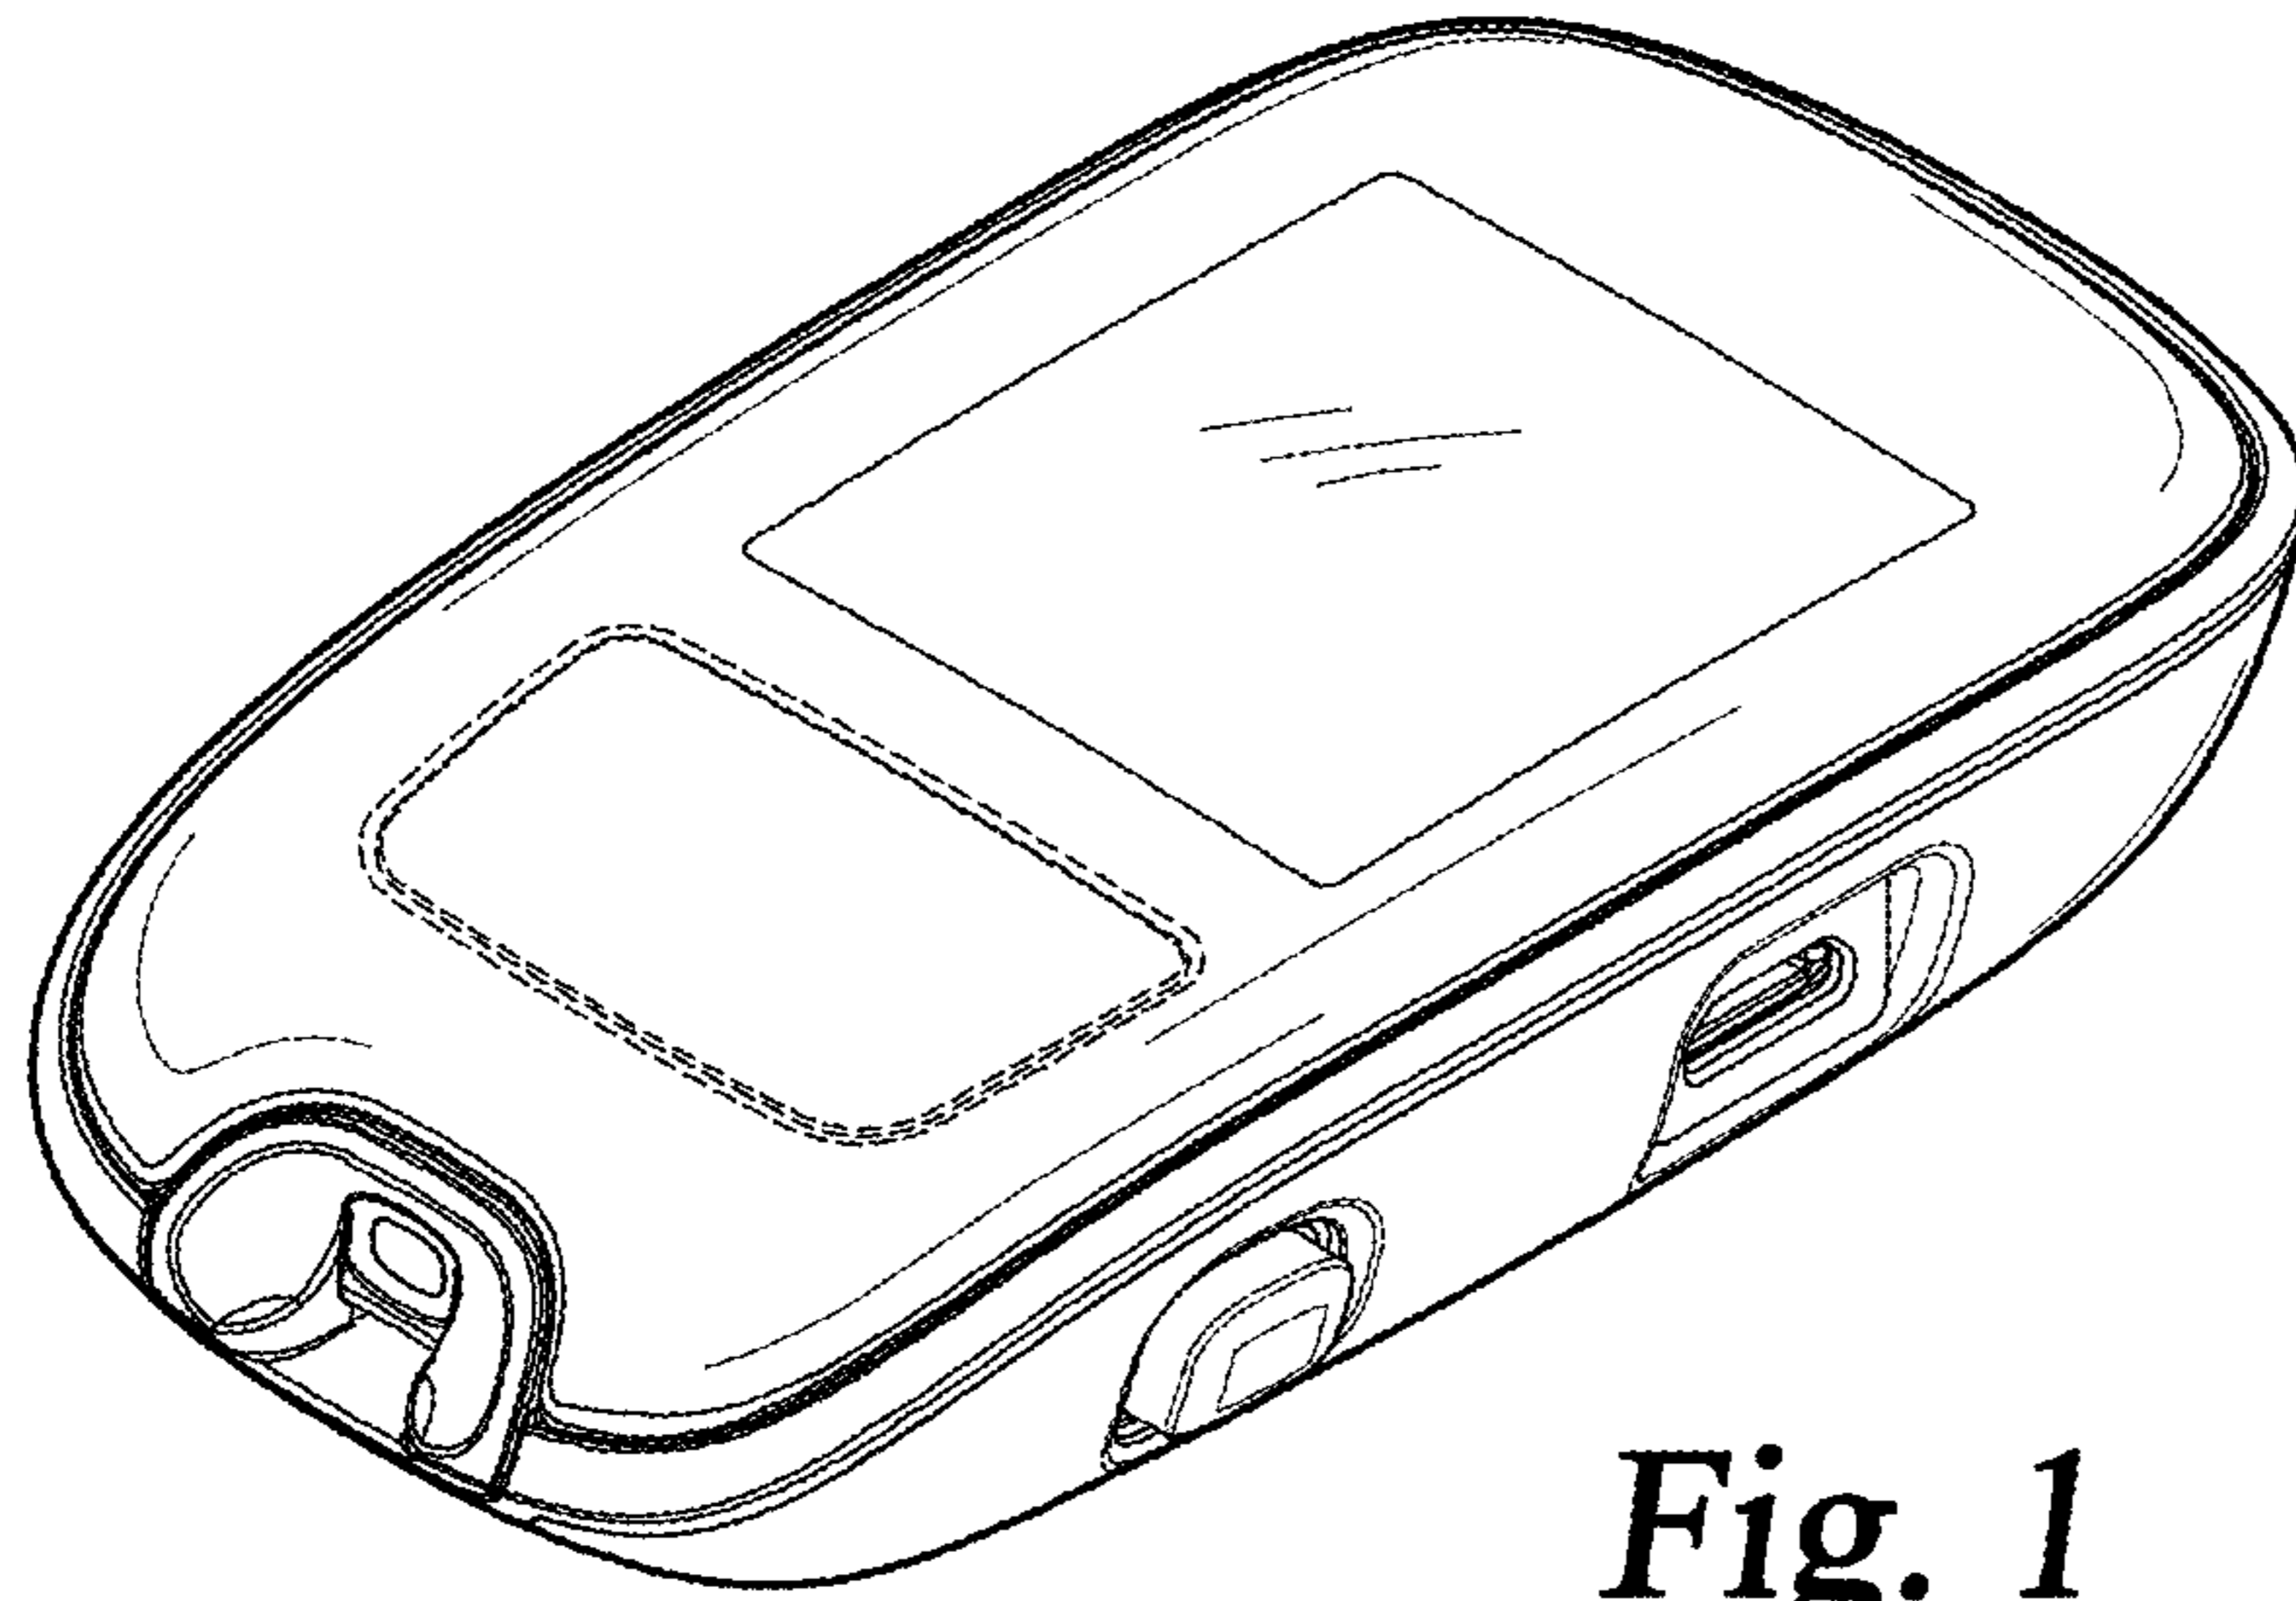


Fig. 1

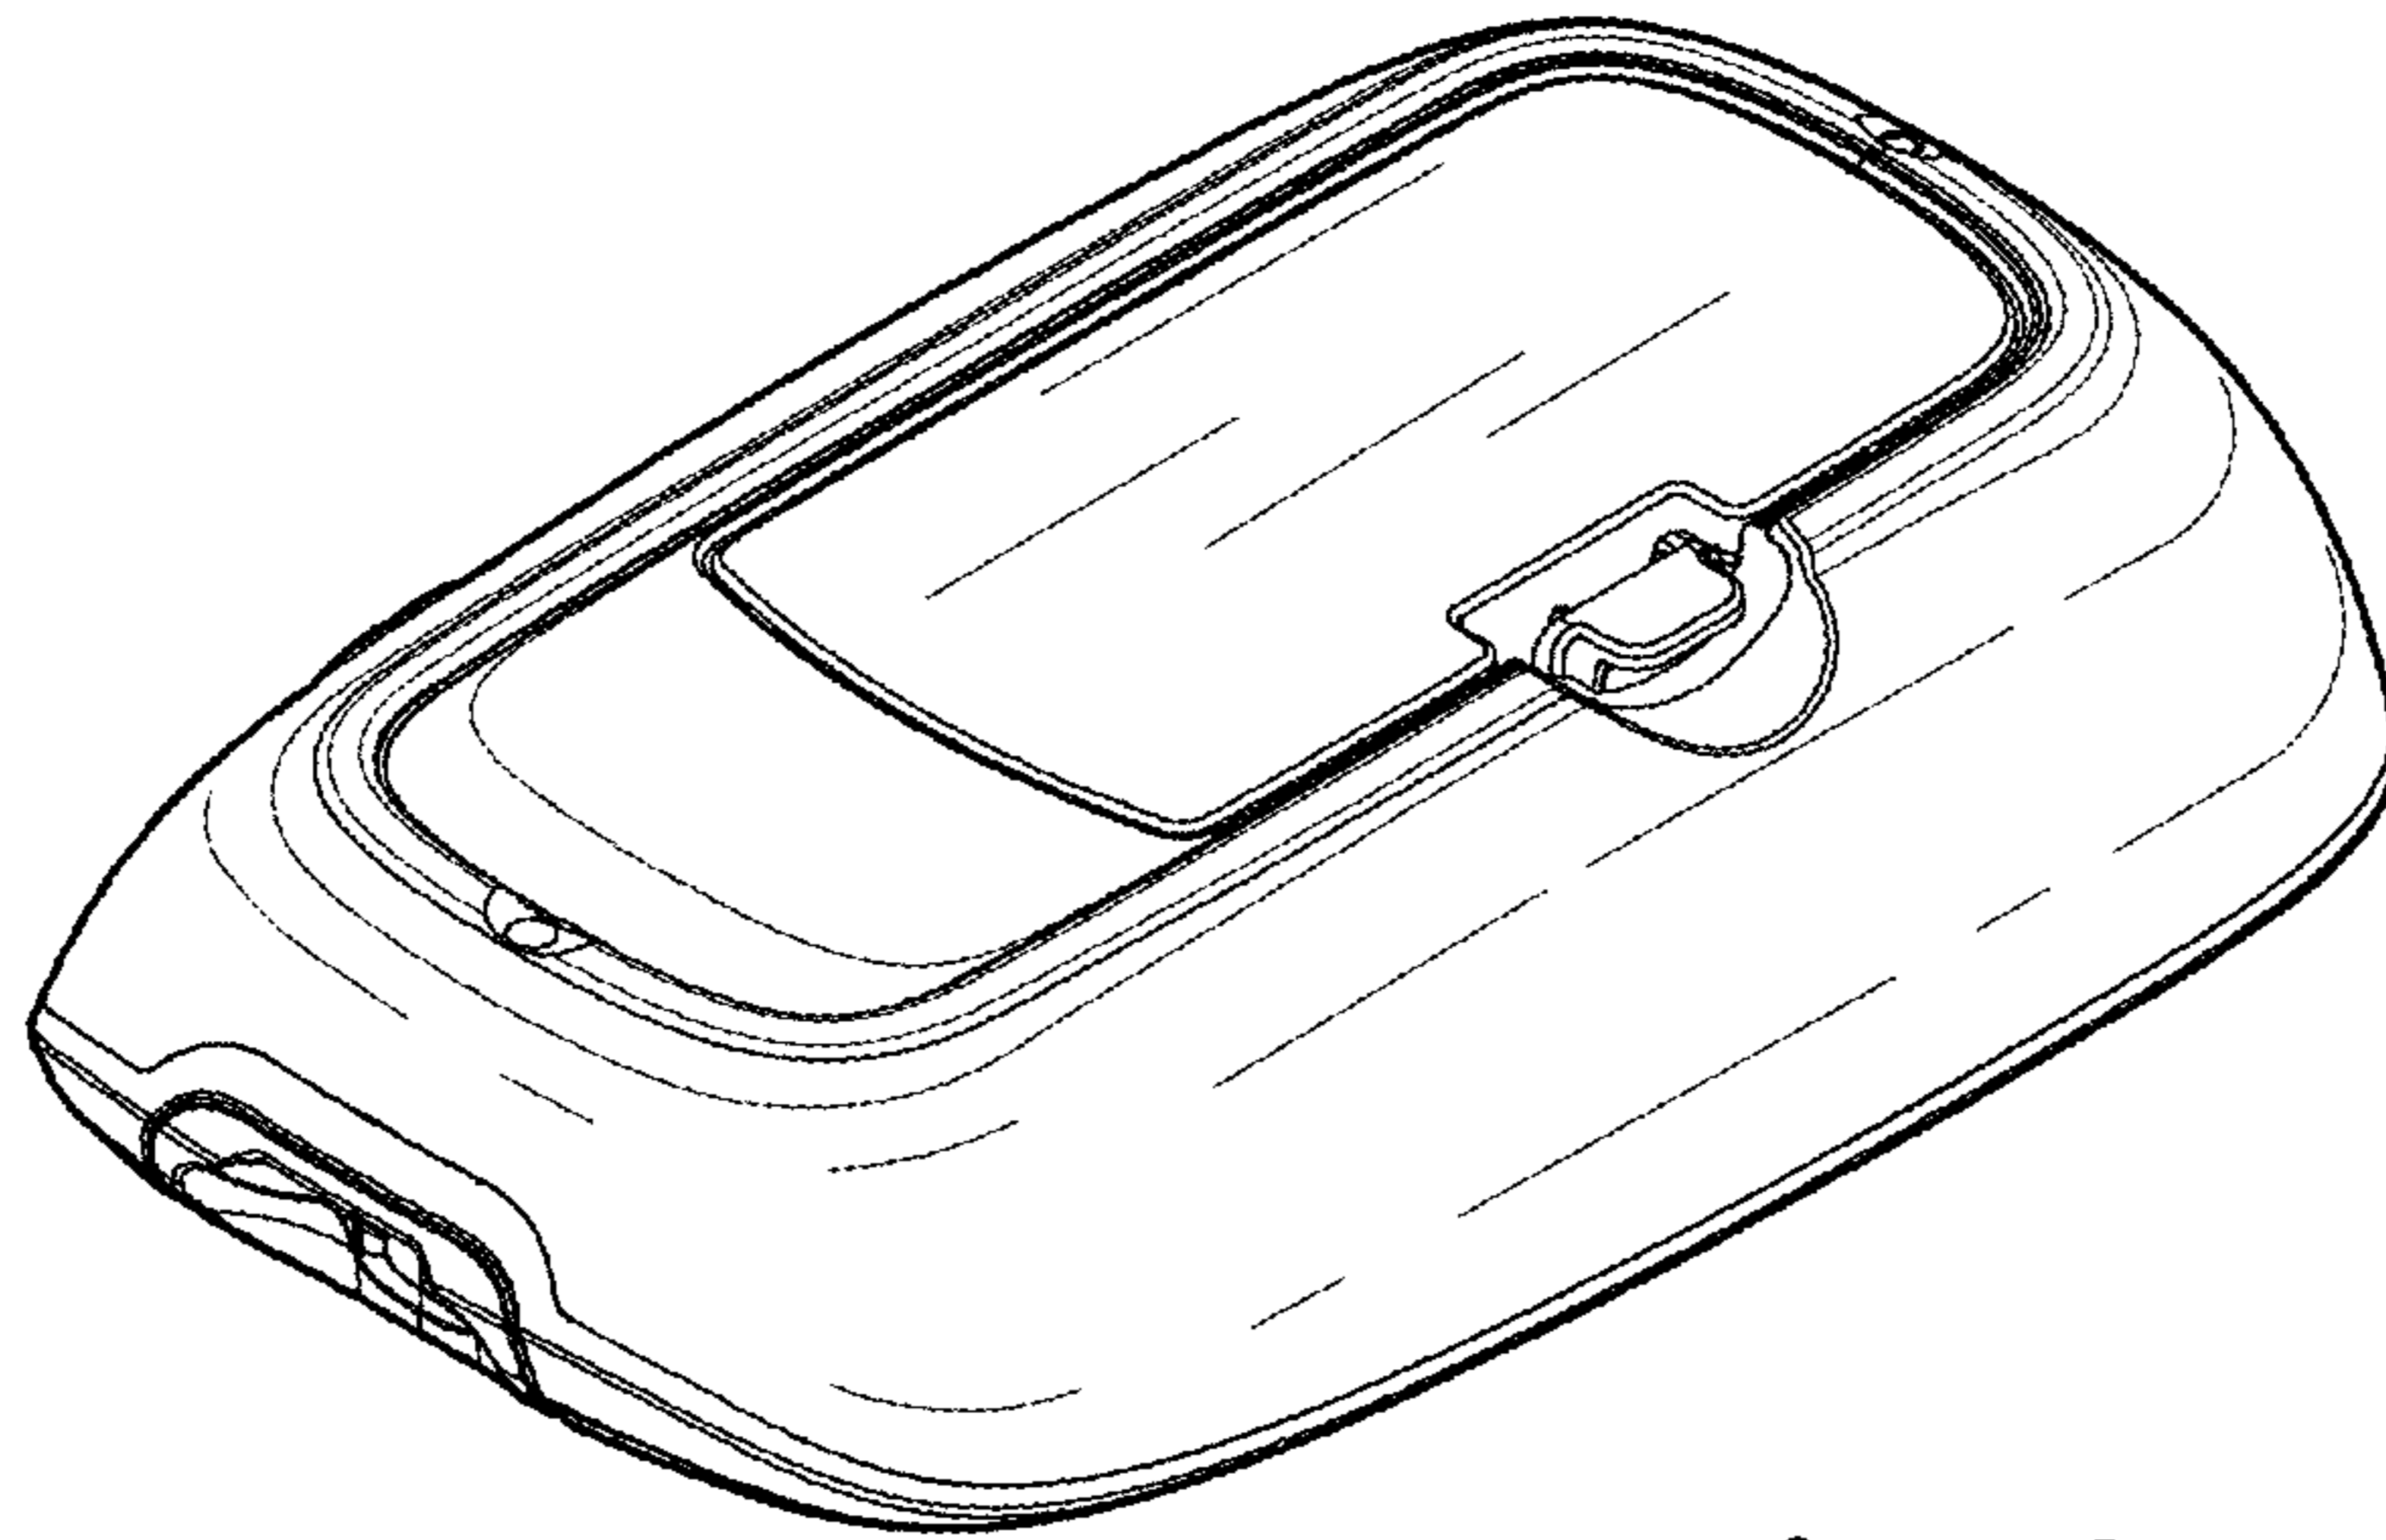


Fig. 2

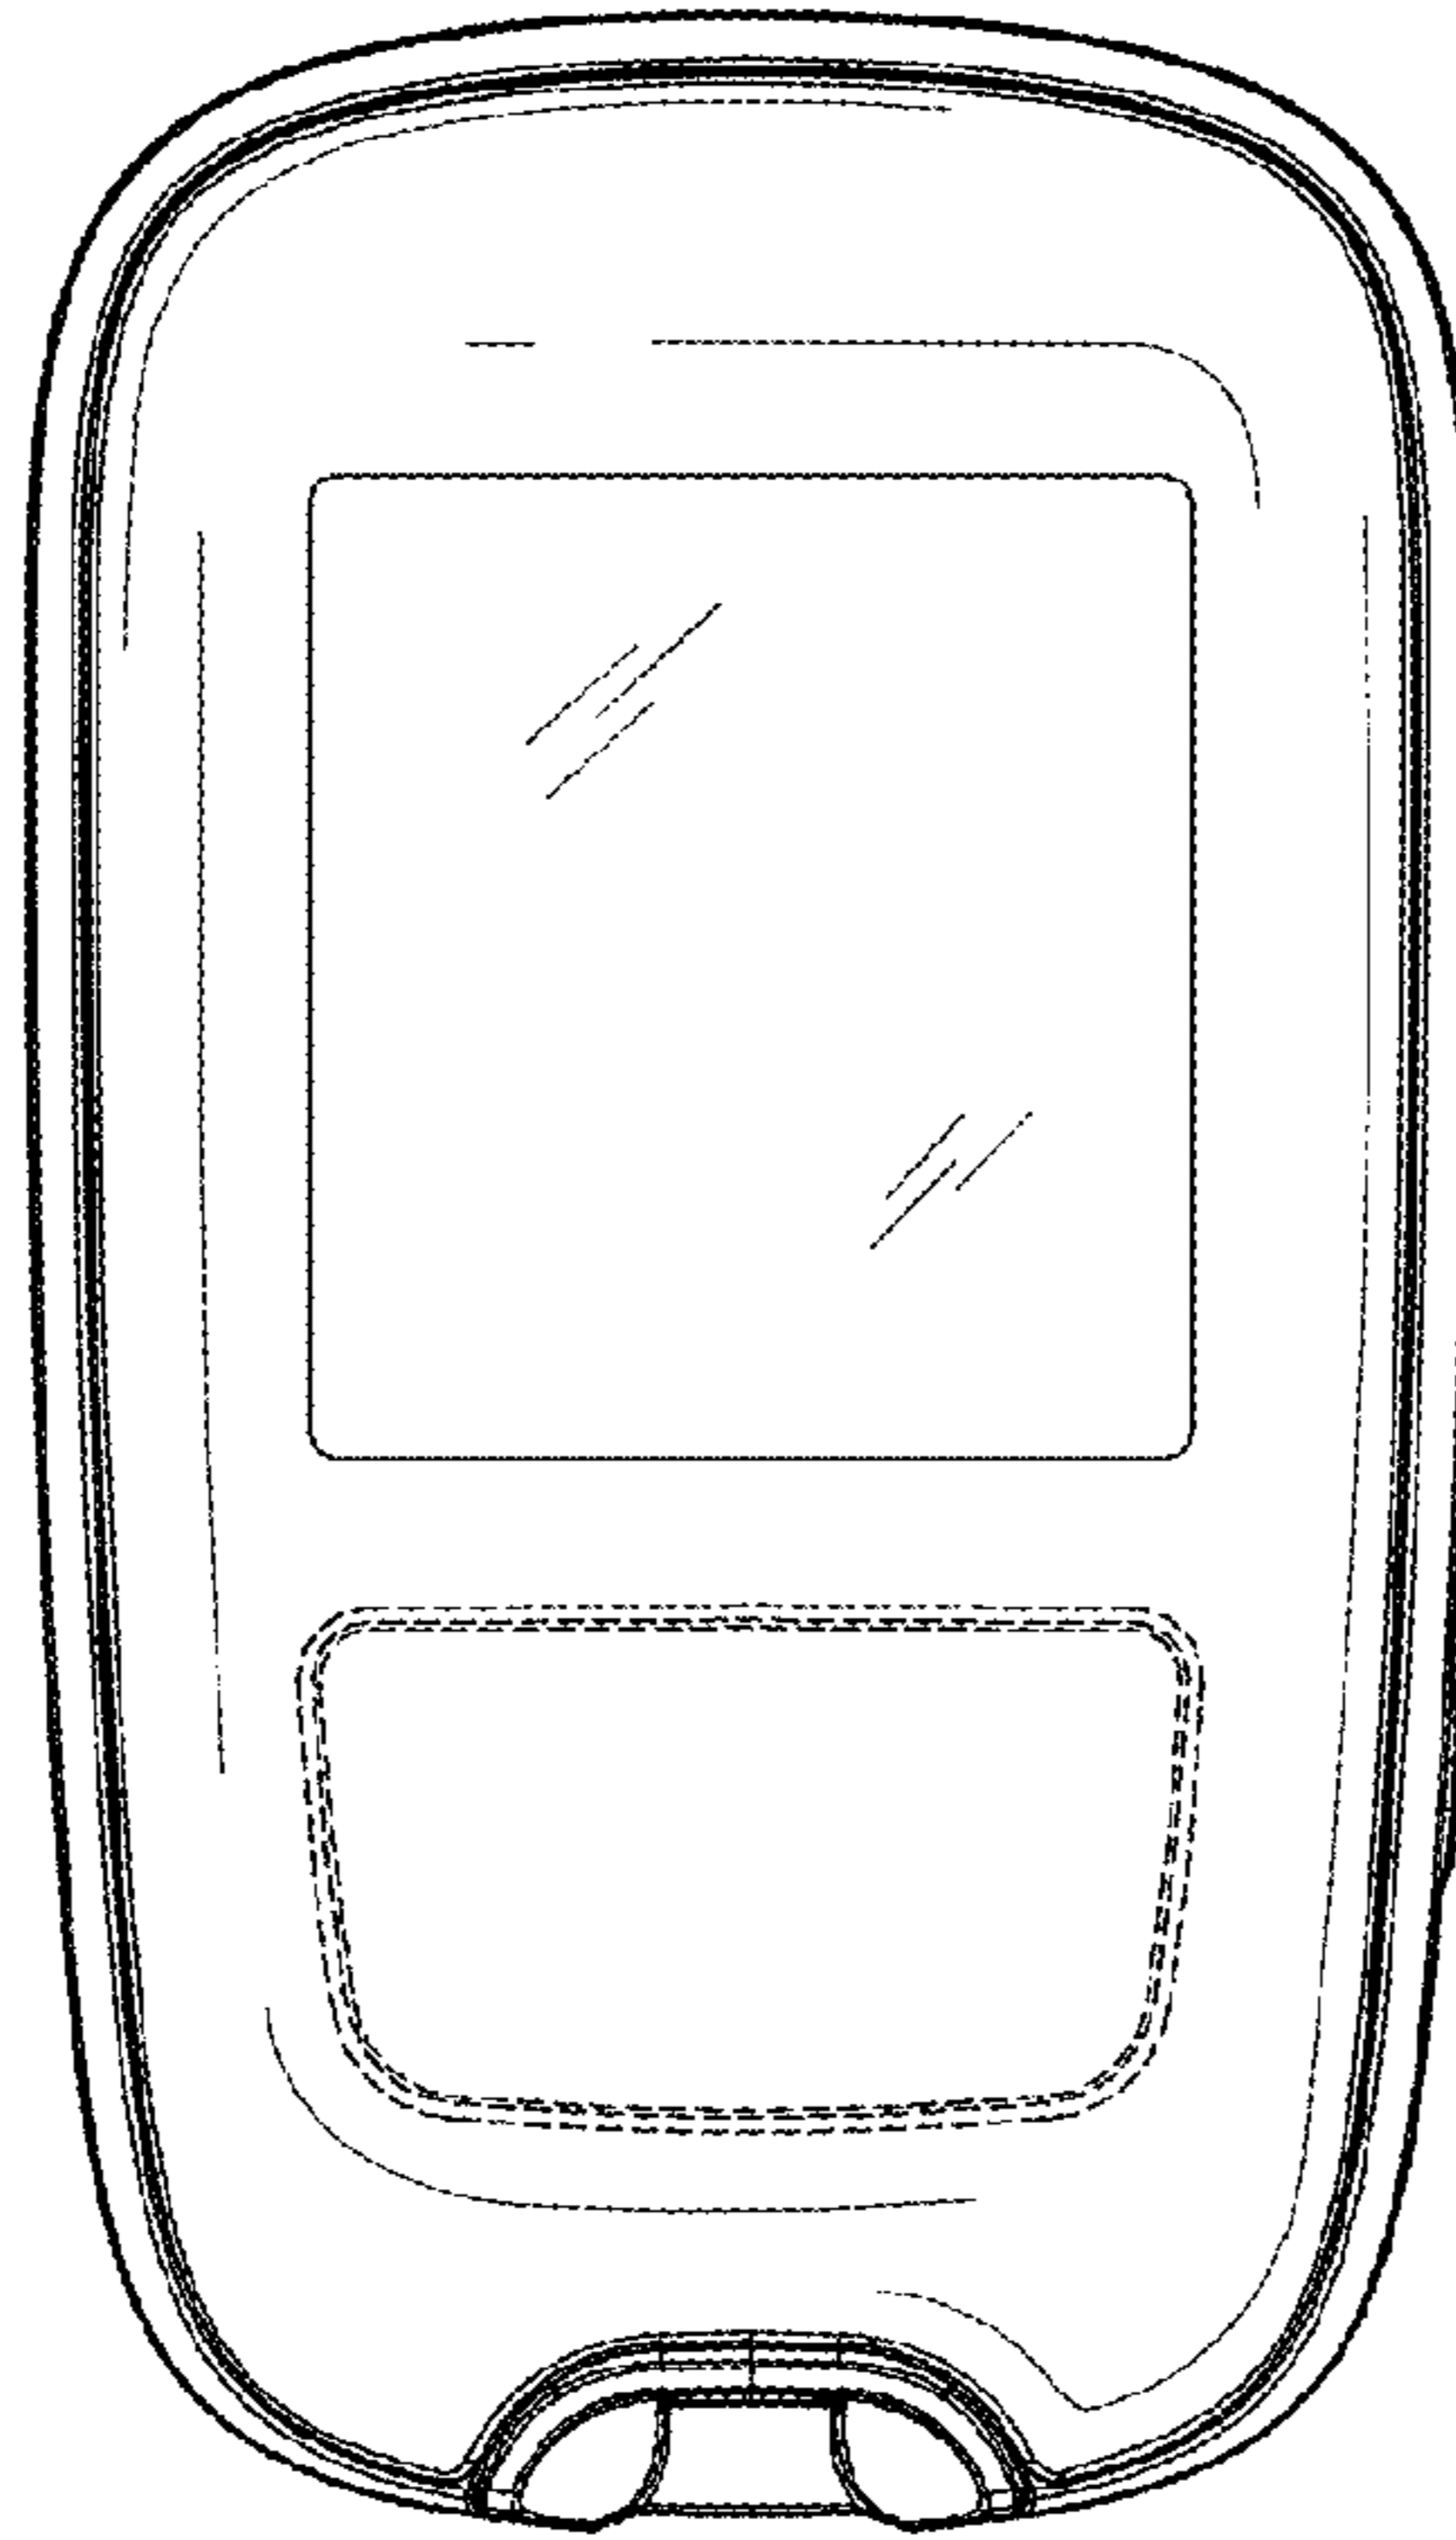


Fig. 3

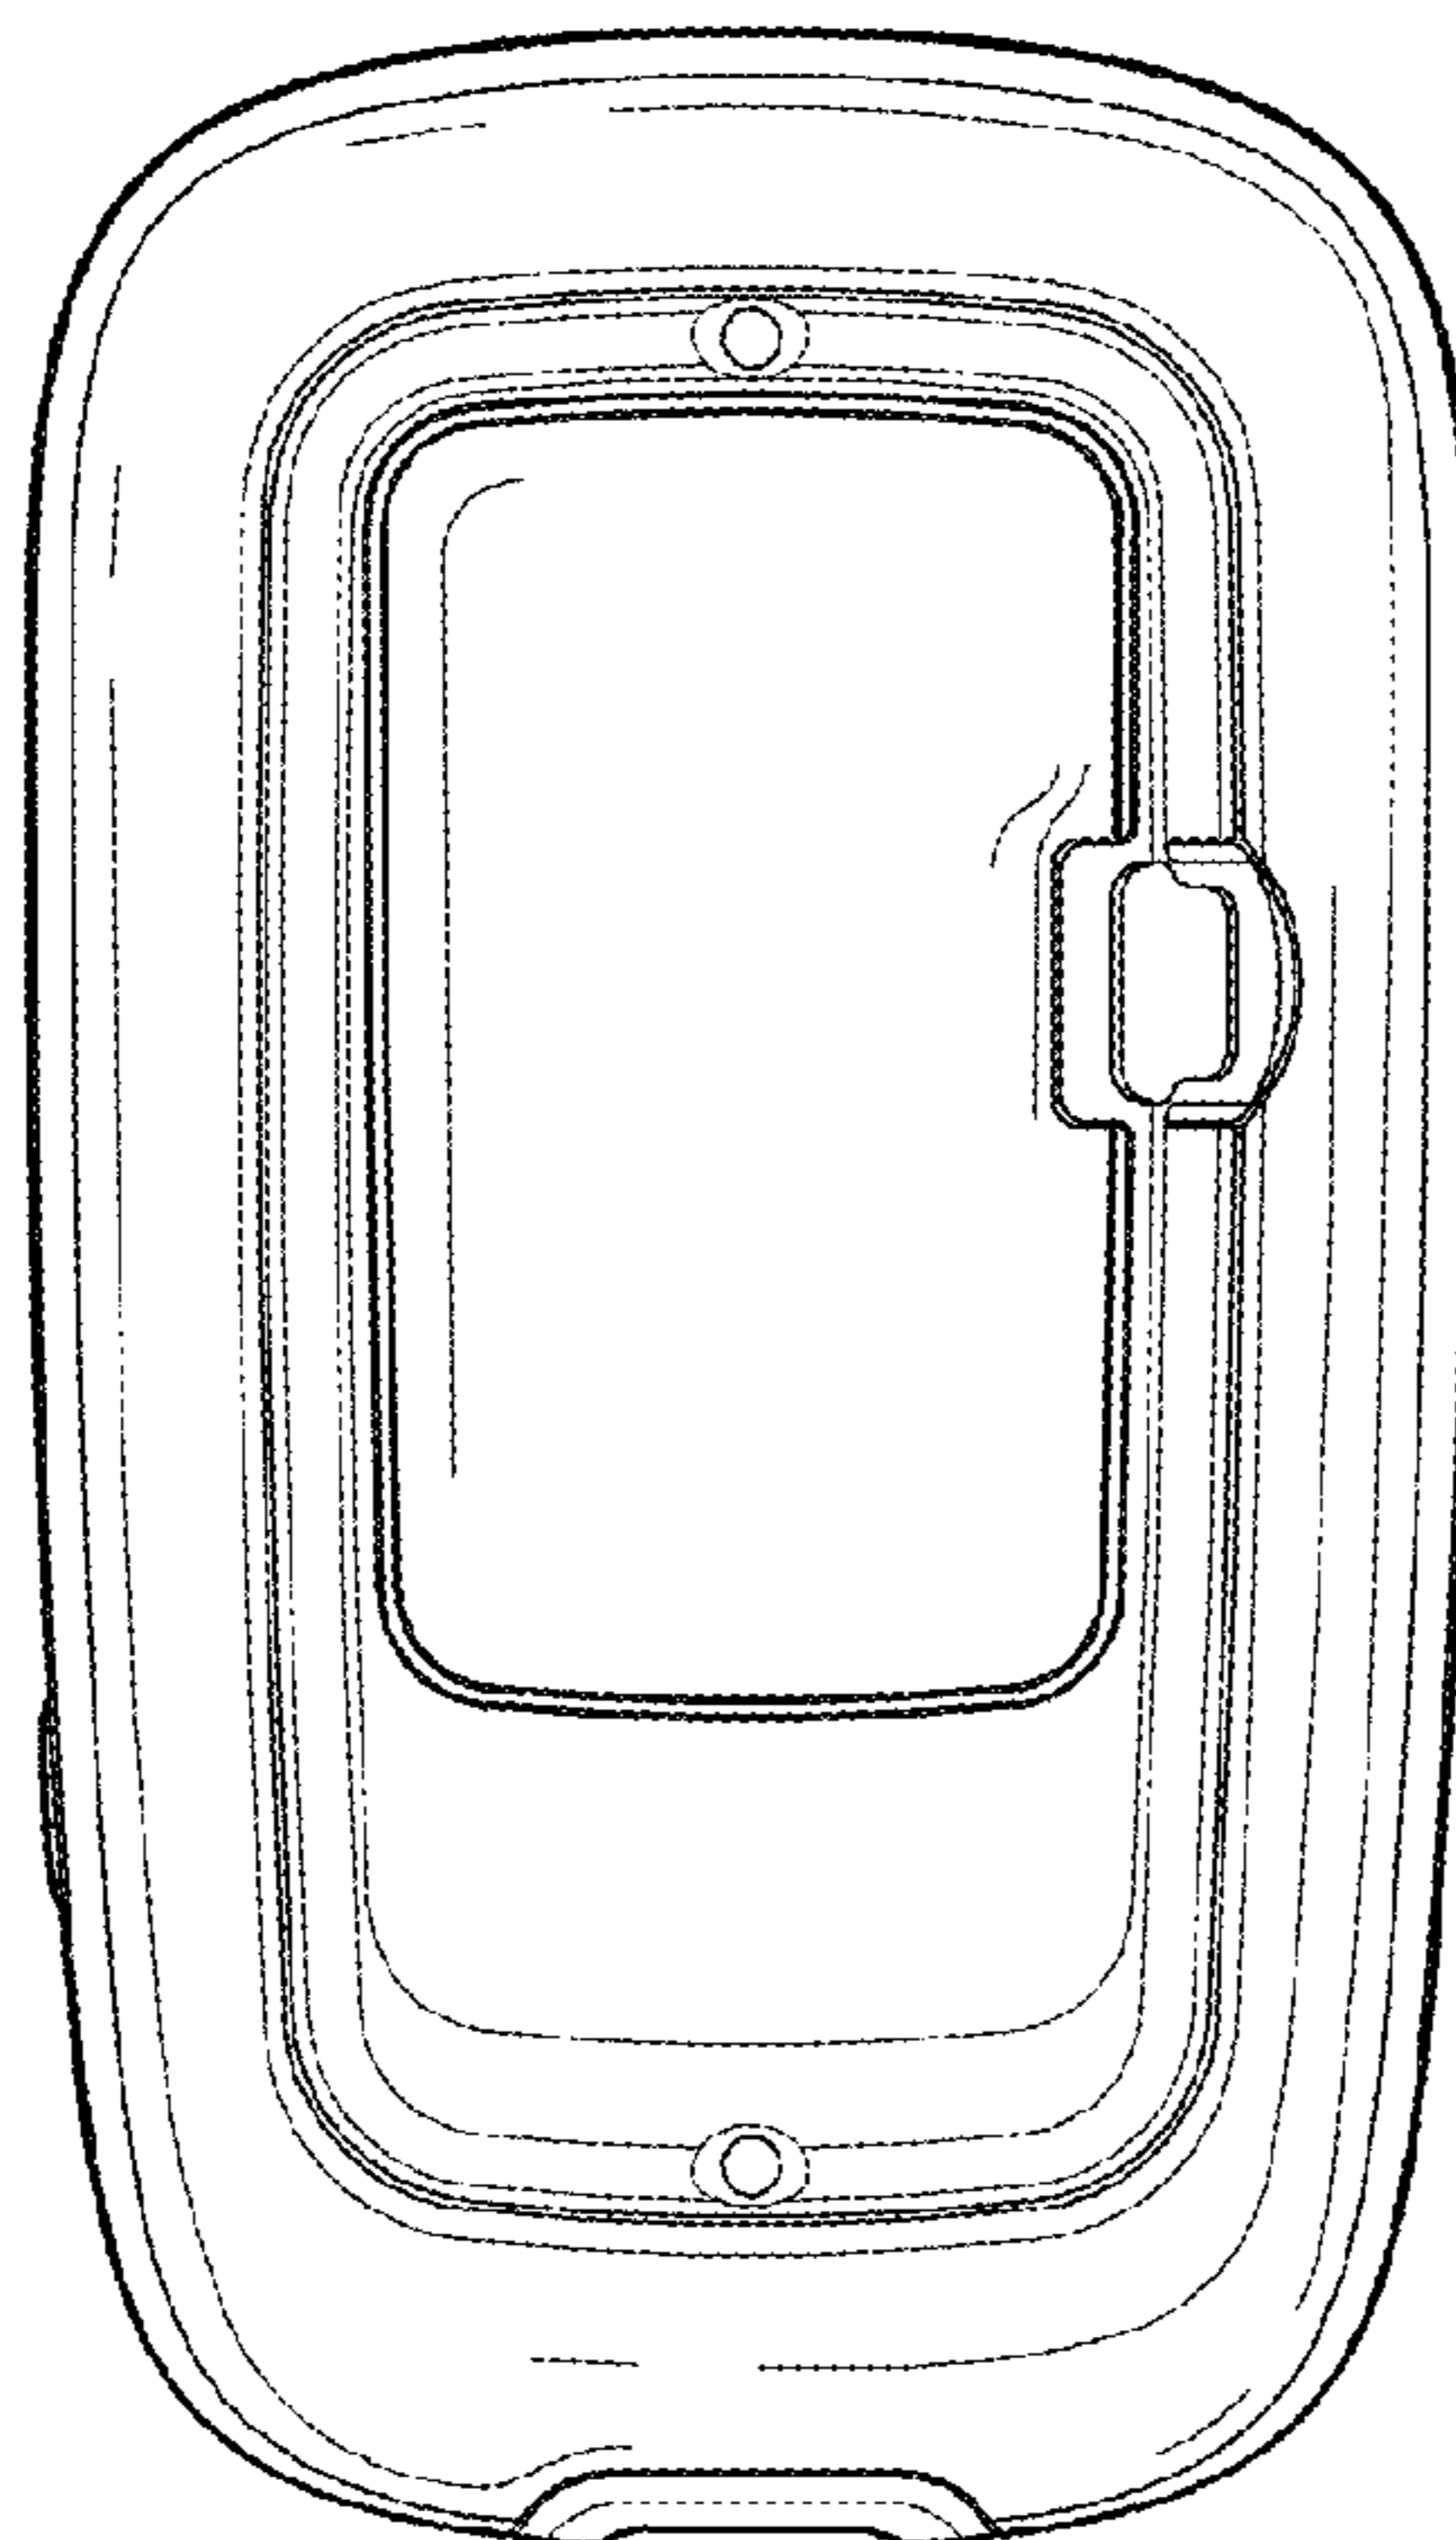


Fig. 4

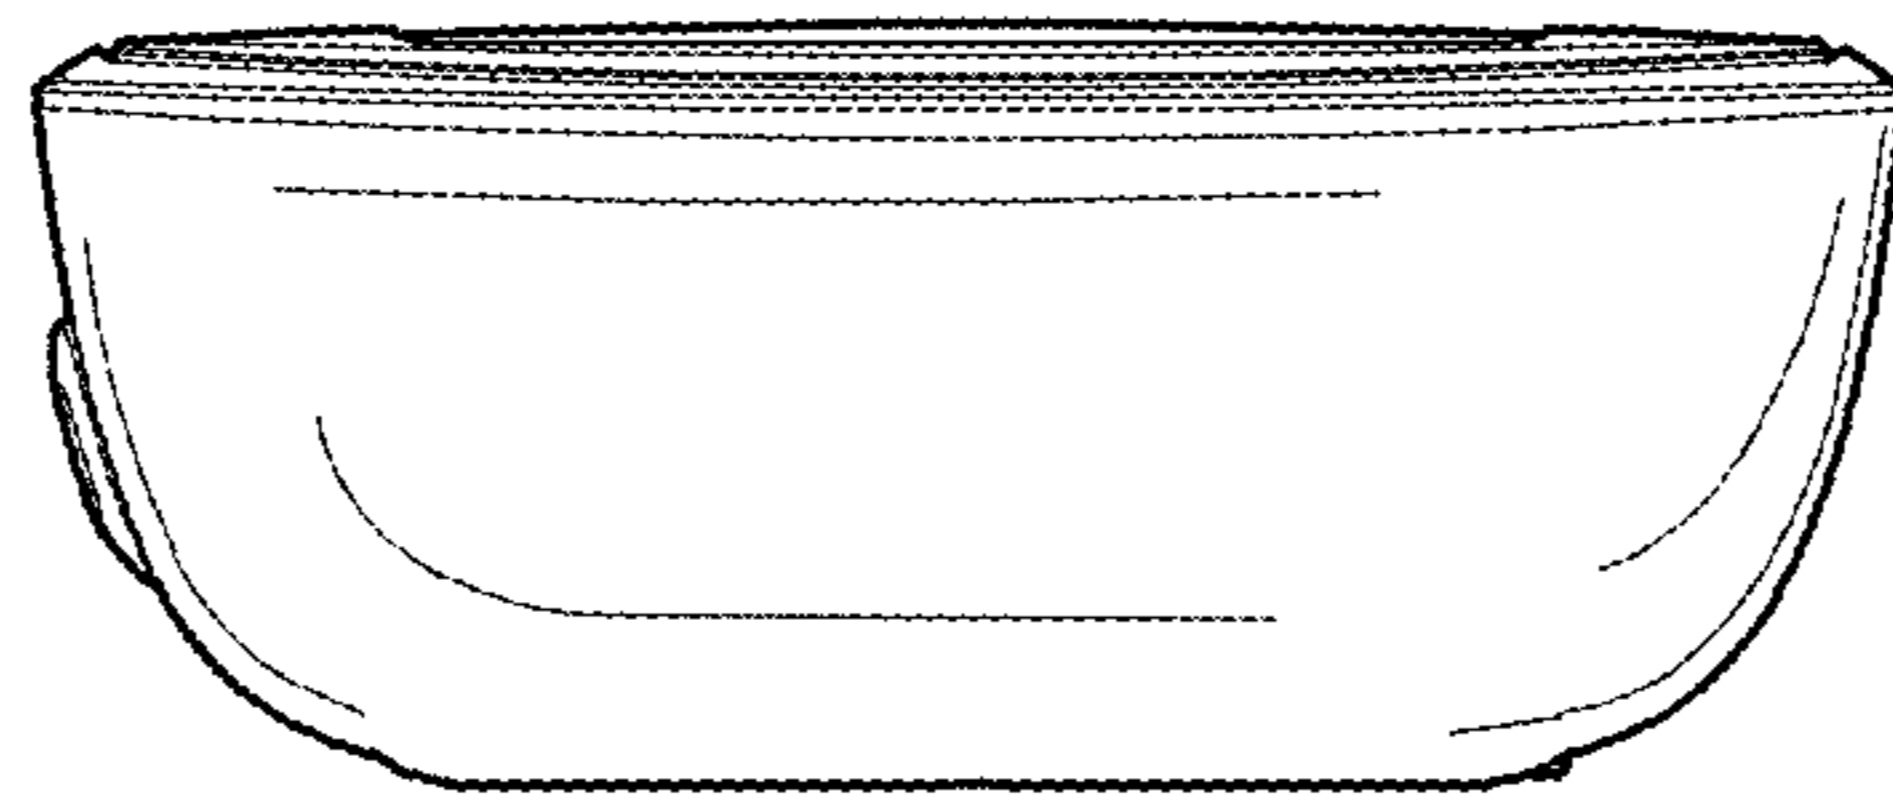


Fig. 5

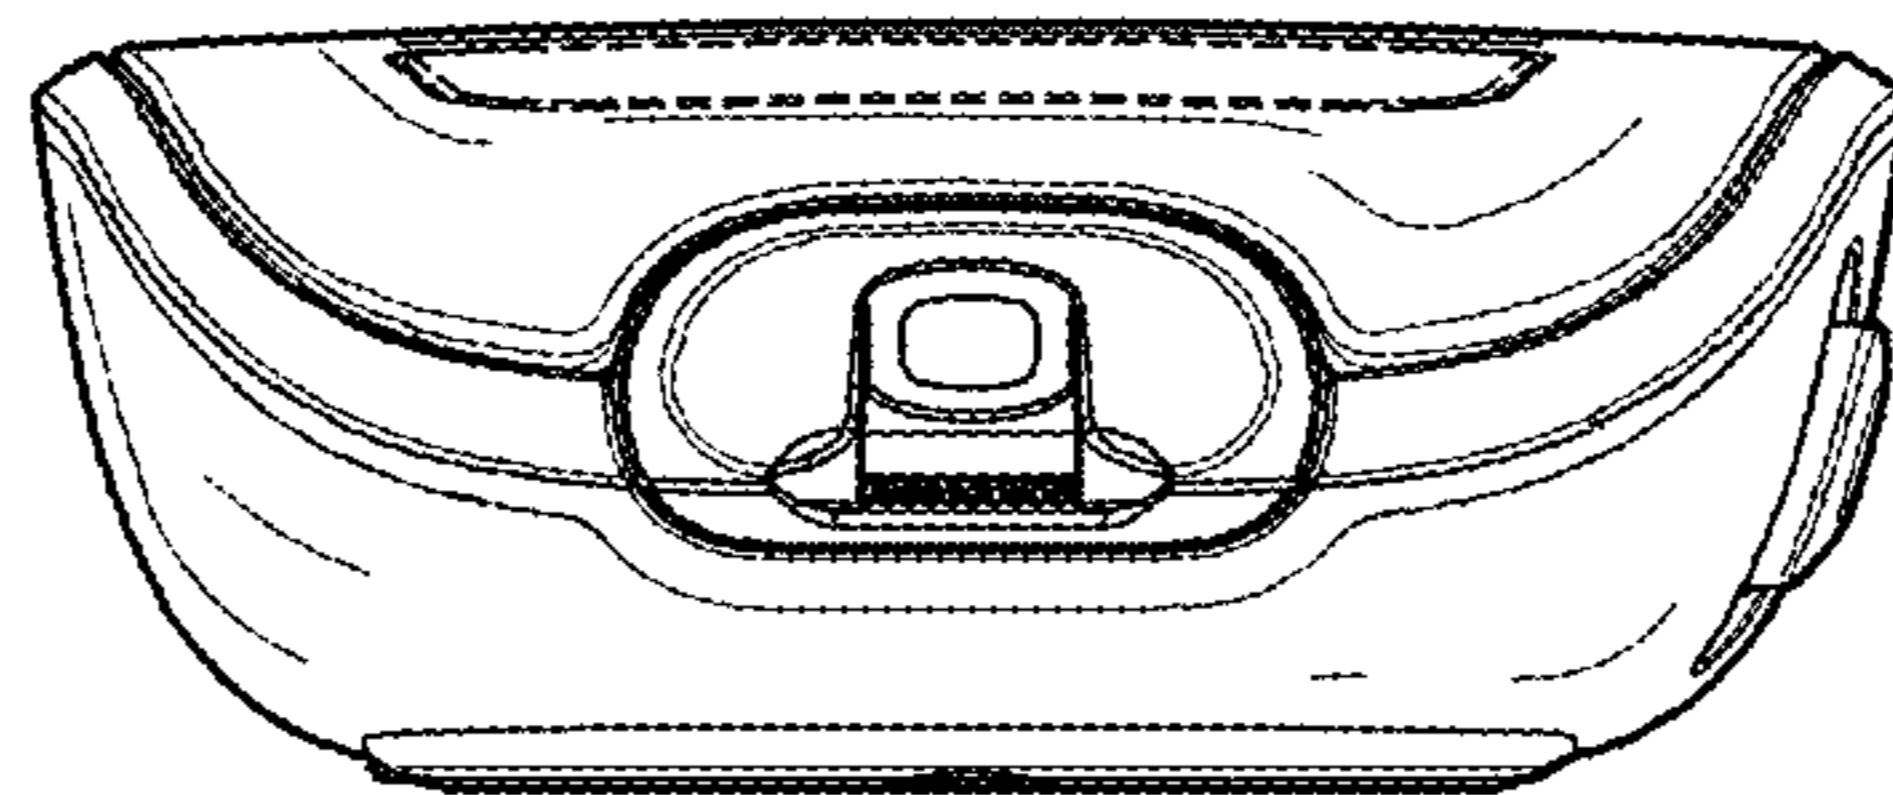


Fig. 6

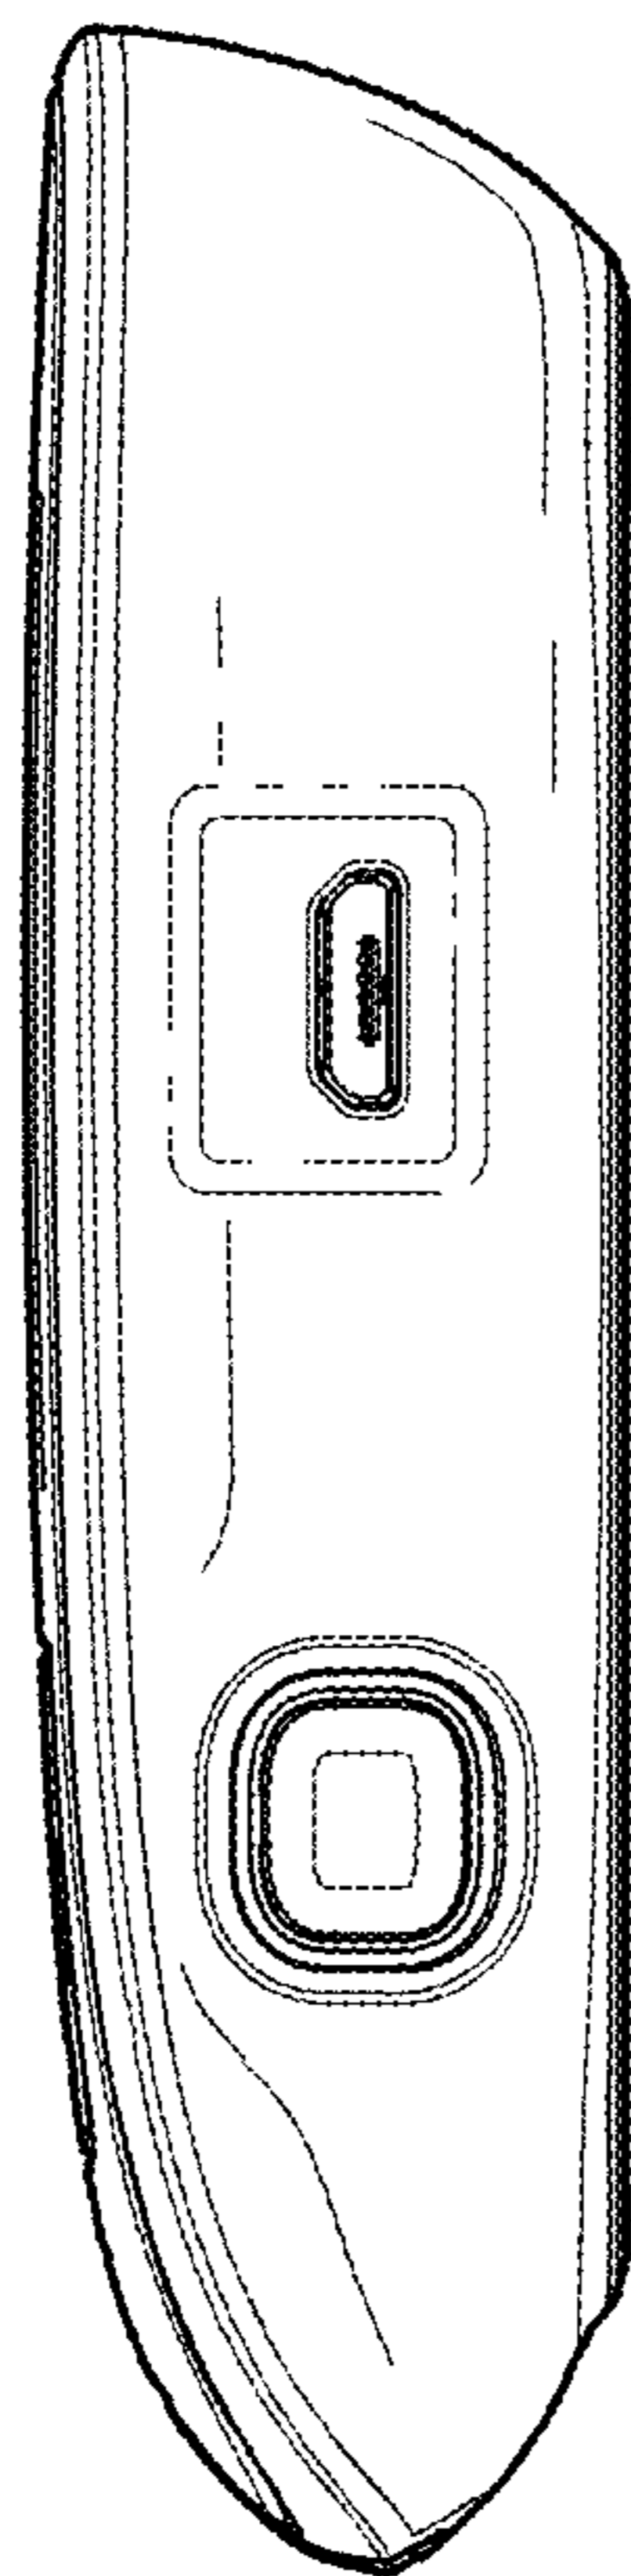


Fig. 7

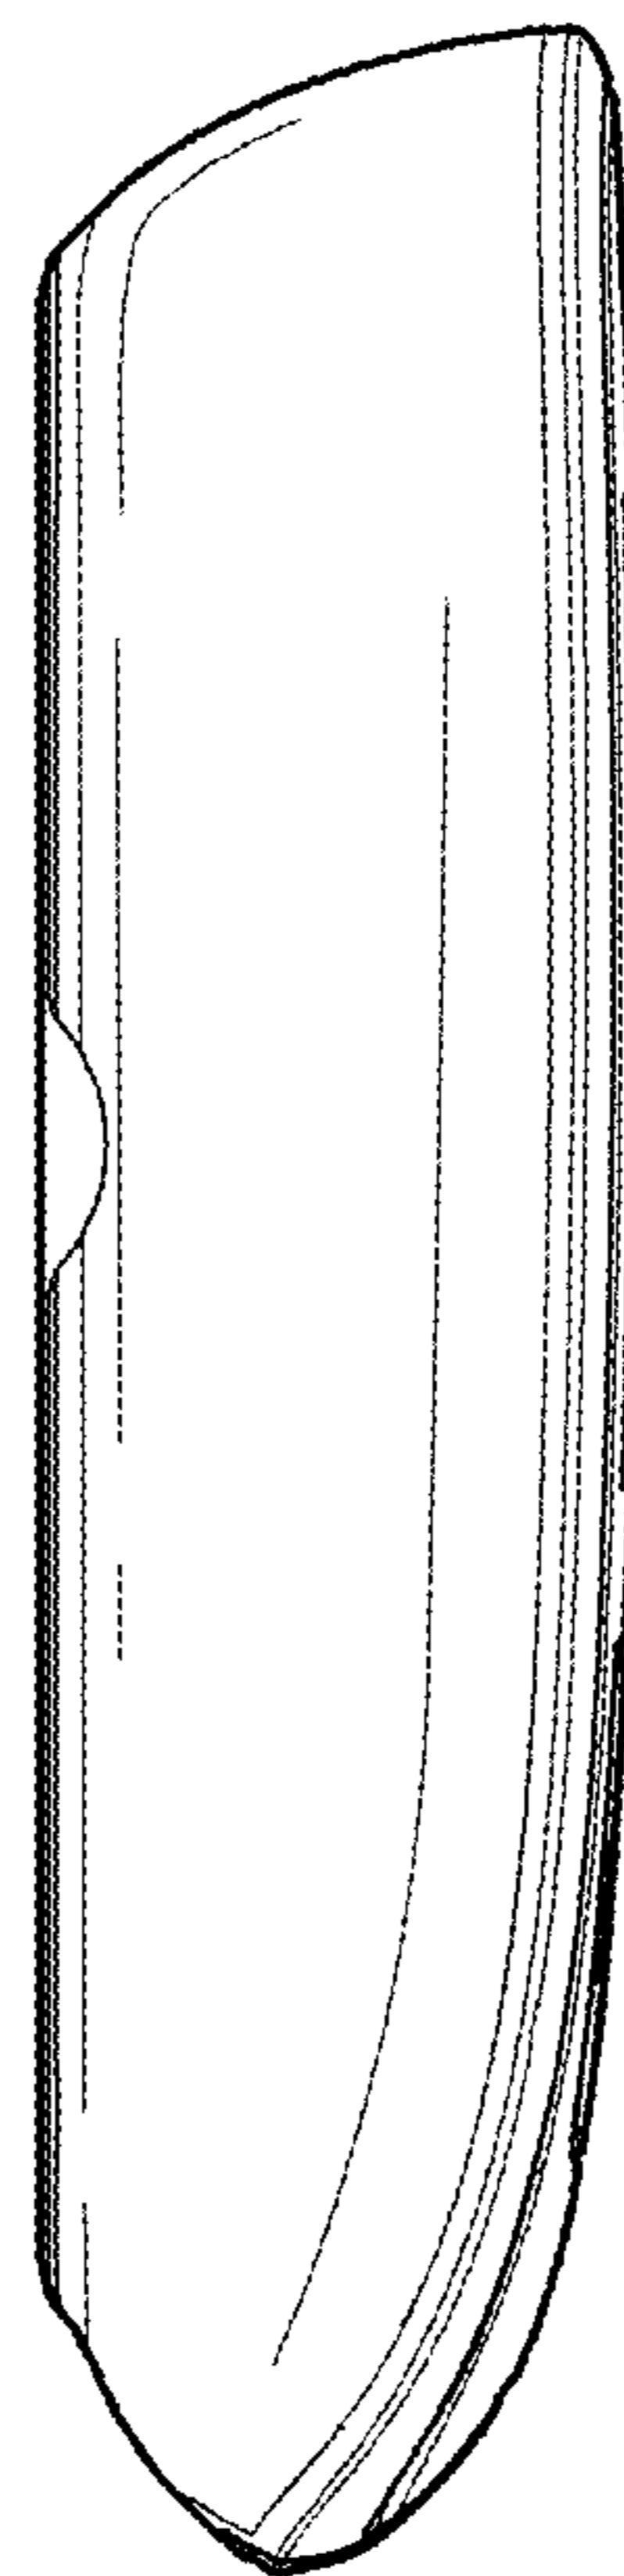


Fig. 8