



US00D748798S

(12) **United States Design Patent**
Ohmukai et al.

(10) **Patent No.:** **US D748,798 S**
(45) **Date of Patent:** **** Feb. 2, 2016**

(54) **X-RAY APPARATUS FOR MEDICAL TREATMENT**

(71) Applicants: **Kabushiki Kaisha Toshiba**, Minato-ku, Tokyo (JP); **Toshiba Medical Systems Corporation**, Otawara-shi, Tochigi-ken (JP)

(72) Inventors: **Shinya Ohmukai**, Tokyo (JP); **Kentaro Ichise**, Tokyo (JP)

(73) Assignees: **Kabushiki Kaisha Toshiba**, Minato-ku, Tokyo (JP); **Toshiba Medical Systems Corporation**, Otawara-shi, Tochigi-ken (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/525,377**

(22) Filed: **Apr. 29, 2015**

(30) **Foreign Application Priority Data**

Oct. 29, 2014 (JP) 2014-024207

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/158-161, 185, 186, 107
CPC A61B 6/06; A61B 6/4405; A61B 6/4411;
A61B 6/032; A61B 5/055; A61B 6/4441;
A61B 6/4435; G01N 2223/1016; G01N 2223/301;
G01N 23/046; G01N 2223/031;
G01N 2223/419; G01R 33/48
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D378,133 S * 2/1997 Murakami D24/158

6,222,906 B1 * 4/2001 Sakaguchi A61B 6/06
257/E27.132
D480,142 S * 9/2003 Chikuma D24/158
D553,748 S * 10/2007 Ogiwara D24/158
D554,257 S * 10/2007 Ogiwara D24/158

(Continued)

FOREIGN PATENT DOCUMENTS

JP D1003753 2/1998

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.


(57) **CLAIM**

The ornamental design for a X-ray apparatus for medical treatment, as shown and described.

DESCRIPTION

FIG. 1 is a front, top and right side perspective view of a X-ray apparatus for medical treatment, showing our new design; FIG. 2 is a rear, top and left side perspective view thereof; FIG. 3 is a front view thereof; FIG. 4 is a rear view thereof; FIG. 5 is a top view thereof; FIG. 6 is a bottom view thereof; FIG. 7 is a left side view thereof; FIG. 8 is a right side view thereof; FIG. 9 is a cross sectional view thereof, taken along the line 9-9 in FIG. 3 with its internal mechanisms omitted; FIG. 10 is a cross sectional view thereof, taken along the line 10-10 in FIG. 3 with its internal mechanisms omitted; FIG. 11 is an enlarged view thereof, taken along the line 11-11 in FIG. 9; and, FIG. 12 is a front view thereof, showing the state of the FPD detector, which is lifted up. The broken lines are for illustrative purpose only and form no part of the claimed design. The broken lines in FIG. 9 are included to indicate the point at which the magnified view is cut off. The uneven spaced broken lines define the bounds of the claimed designs and form no part thereof.

1 Claim, 12 Drawing Sheets

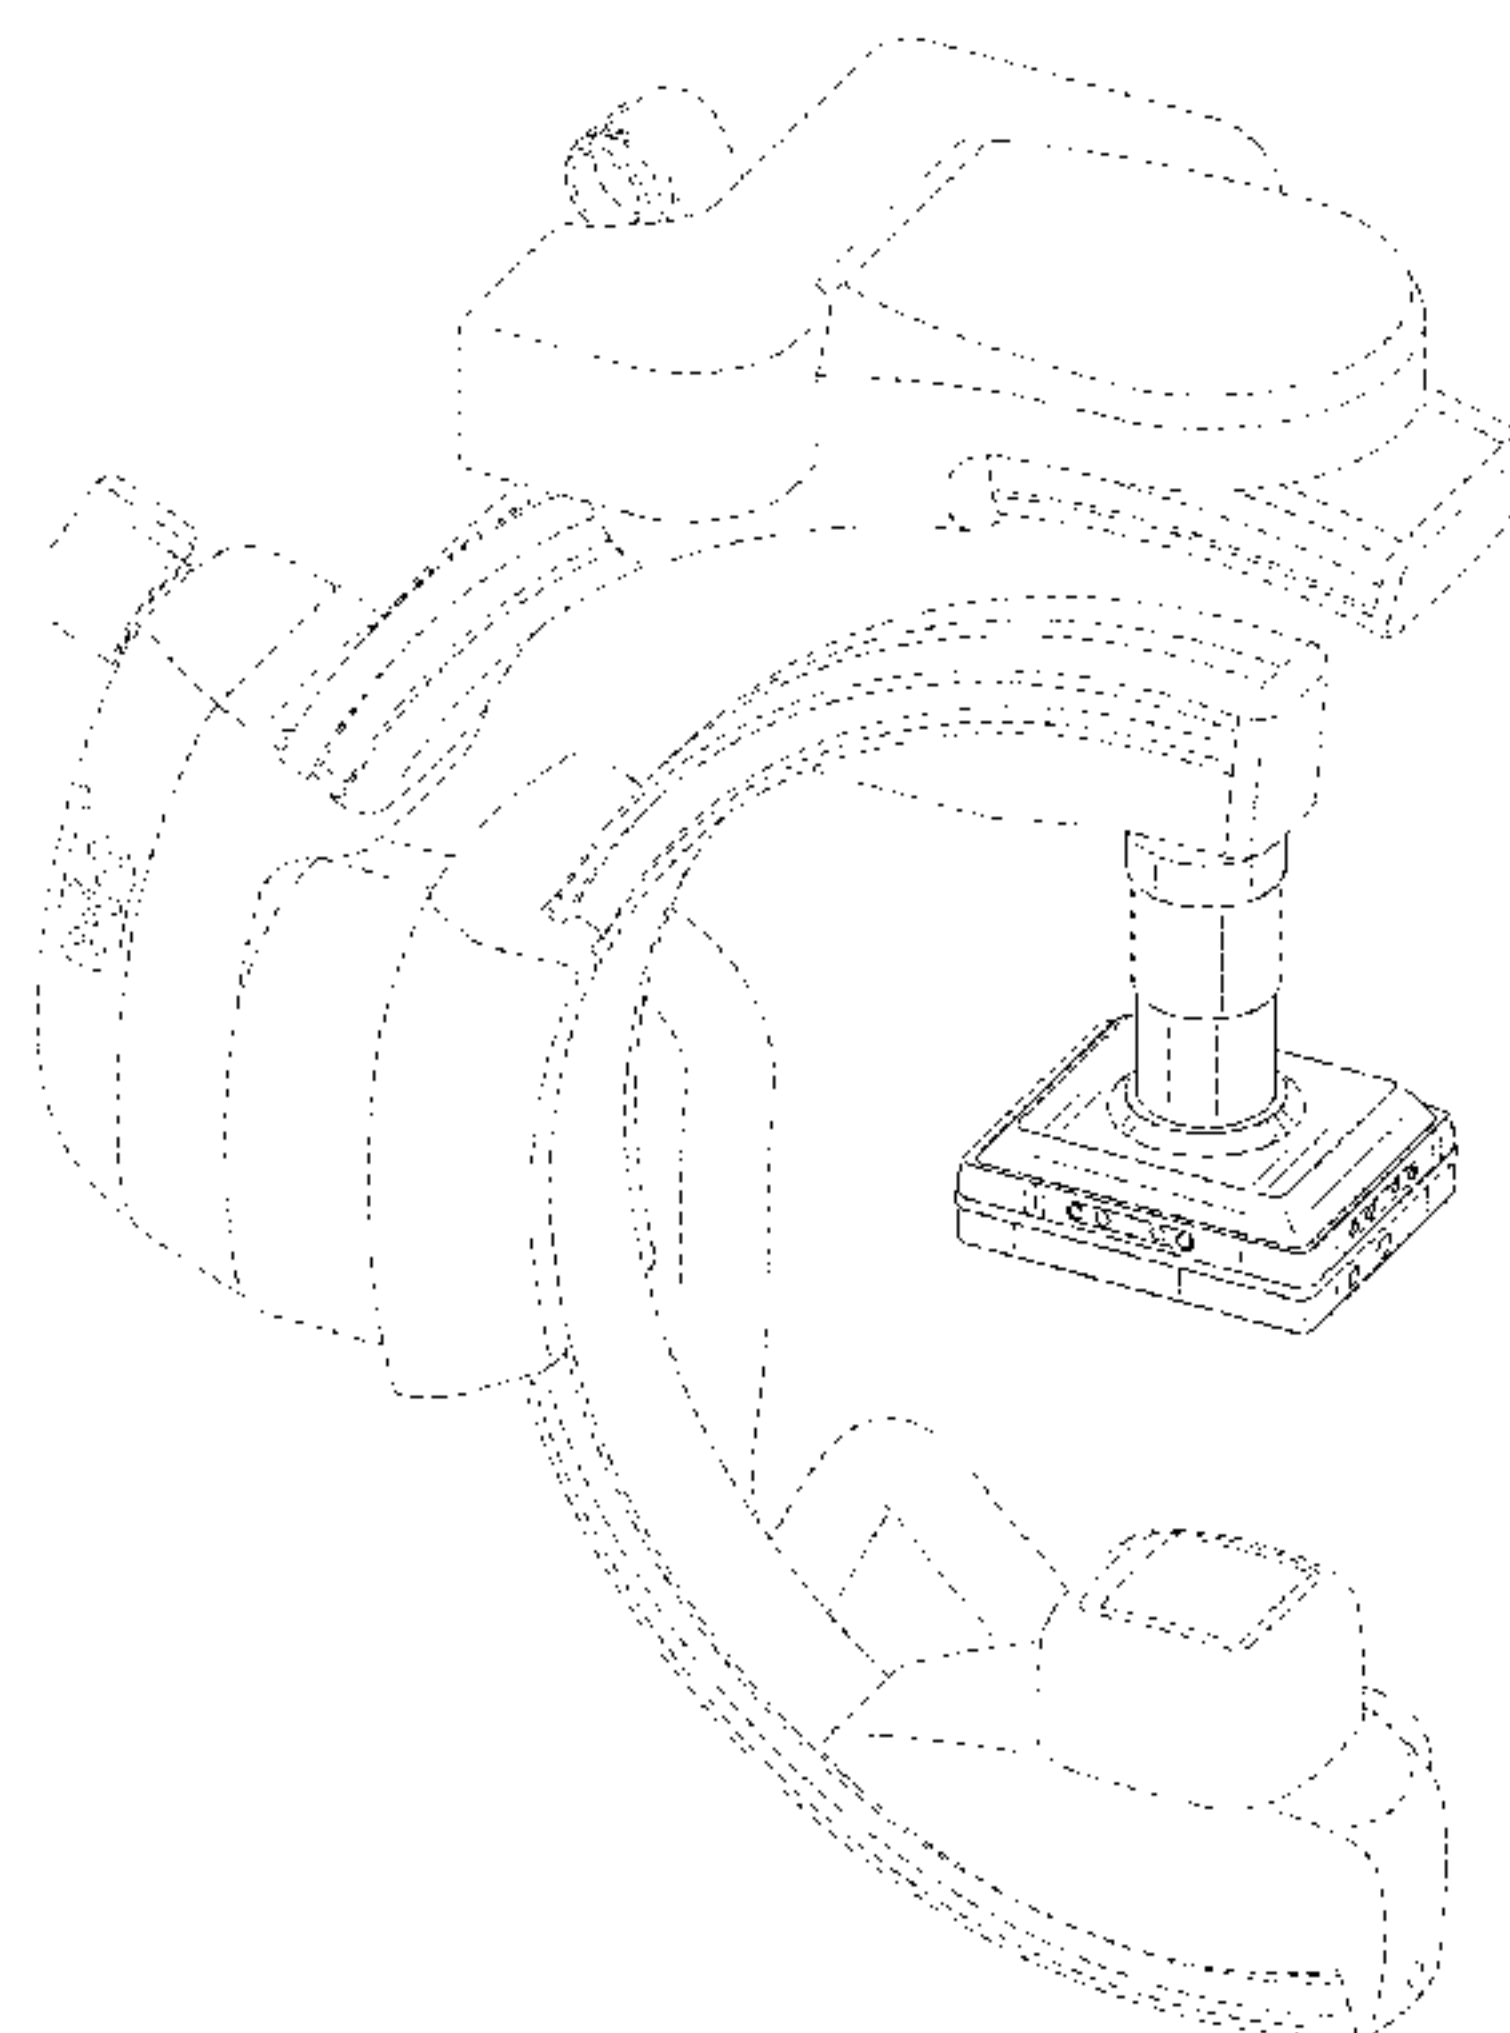

US D748,798 S

Page 2

(56)

References Cited

U.S. PATENT DOCUMENTS

D558,877 S *	1/2008	Ogiwara	D24/158	2011/0179895 A1*	7/2011	Mueller	A61B 6/4441 74/29
2007/0121790 A1*	5/2007	Grady	A61B 6/4405 378/198	2015/0023470 A1*	1/2015	Baumann	A61B 6/4441 378/62

* cited by examiner

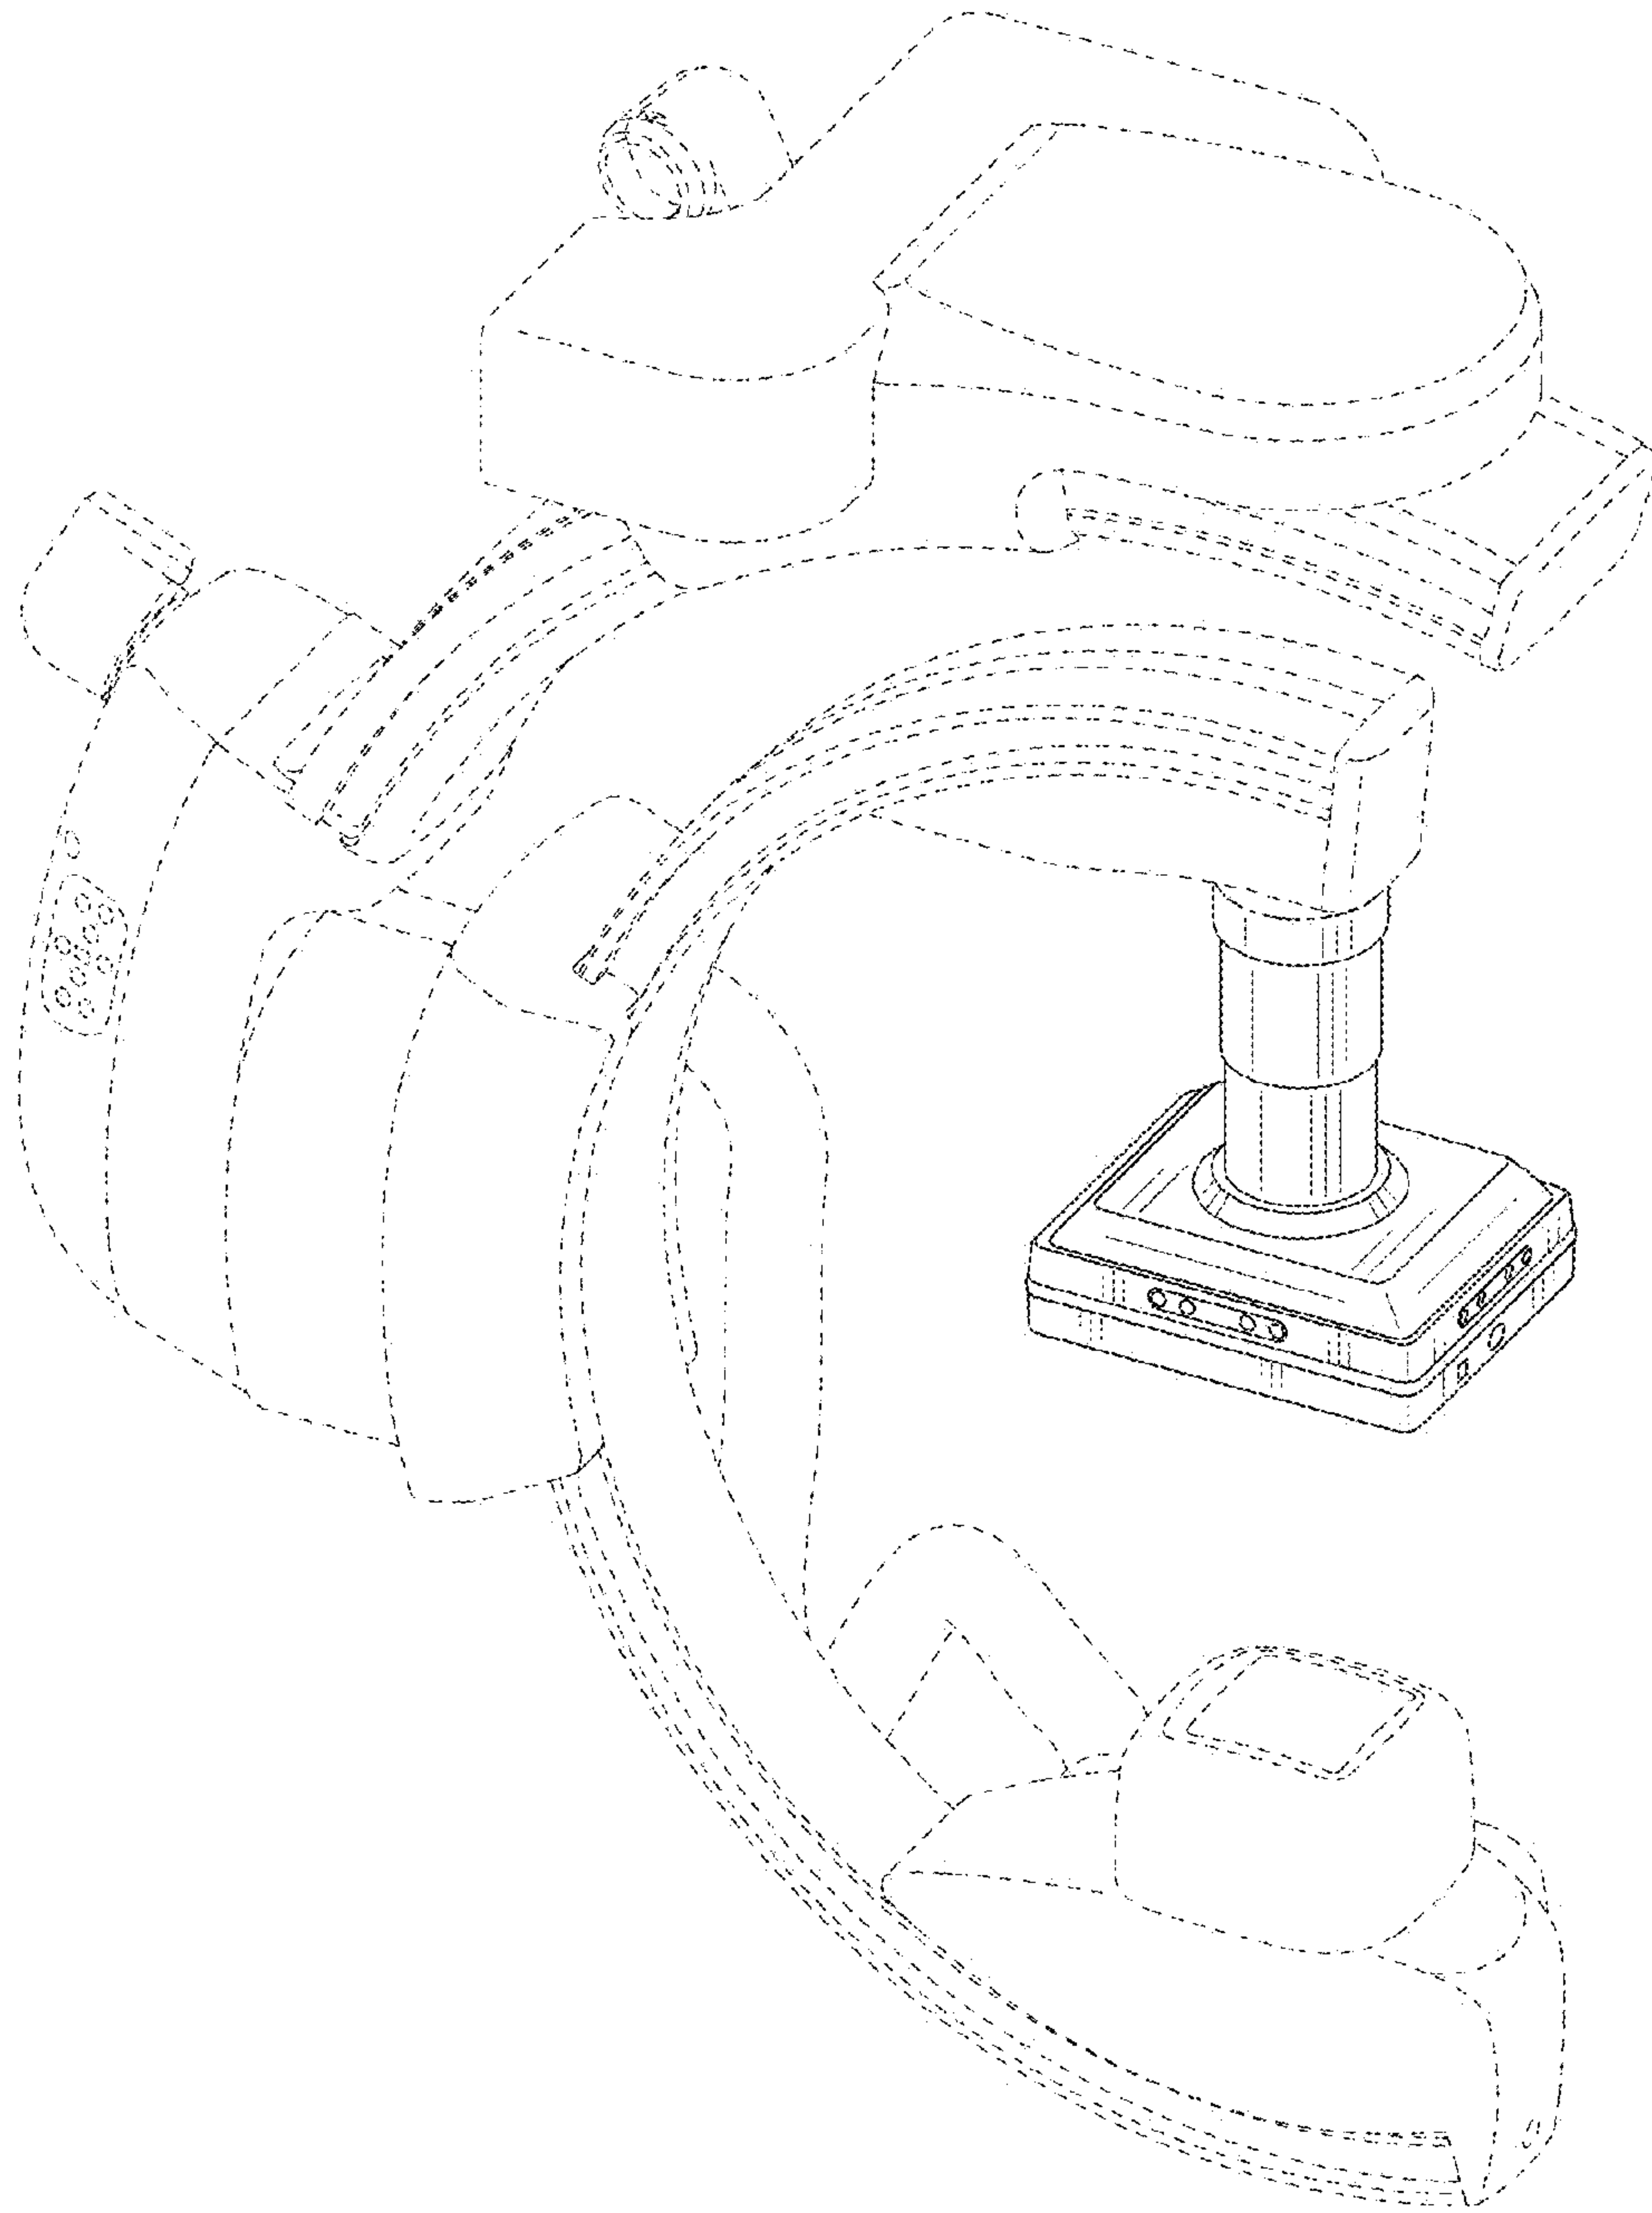


Fig. 1

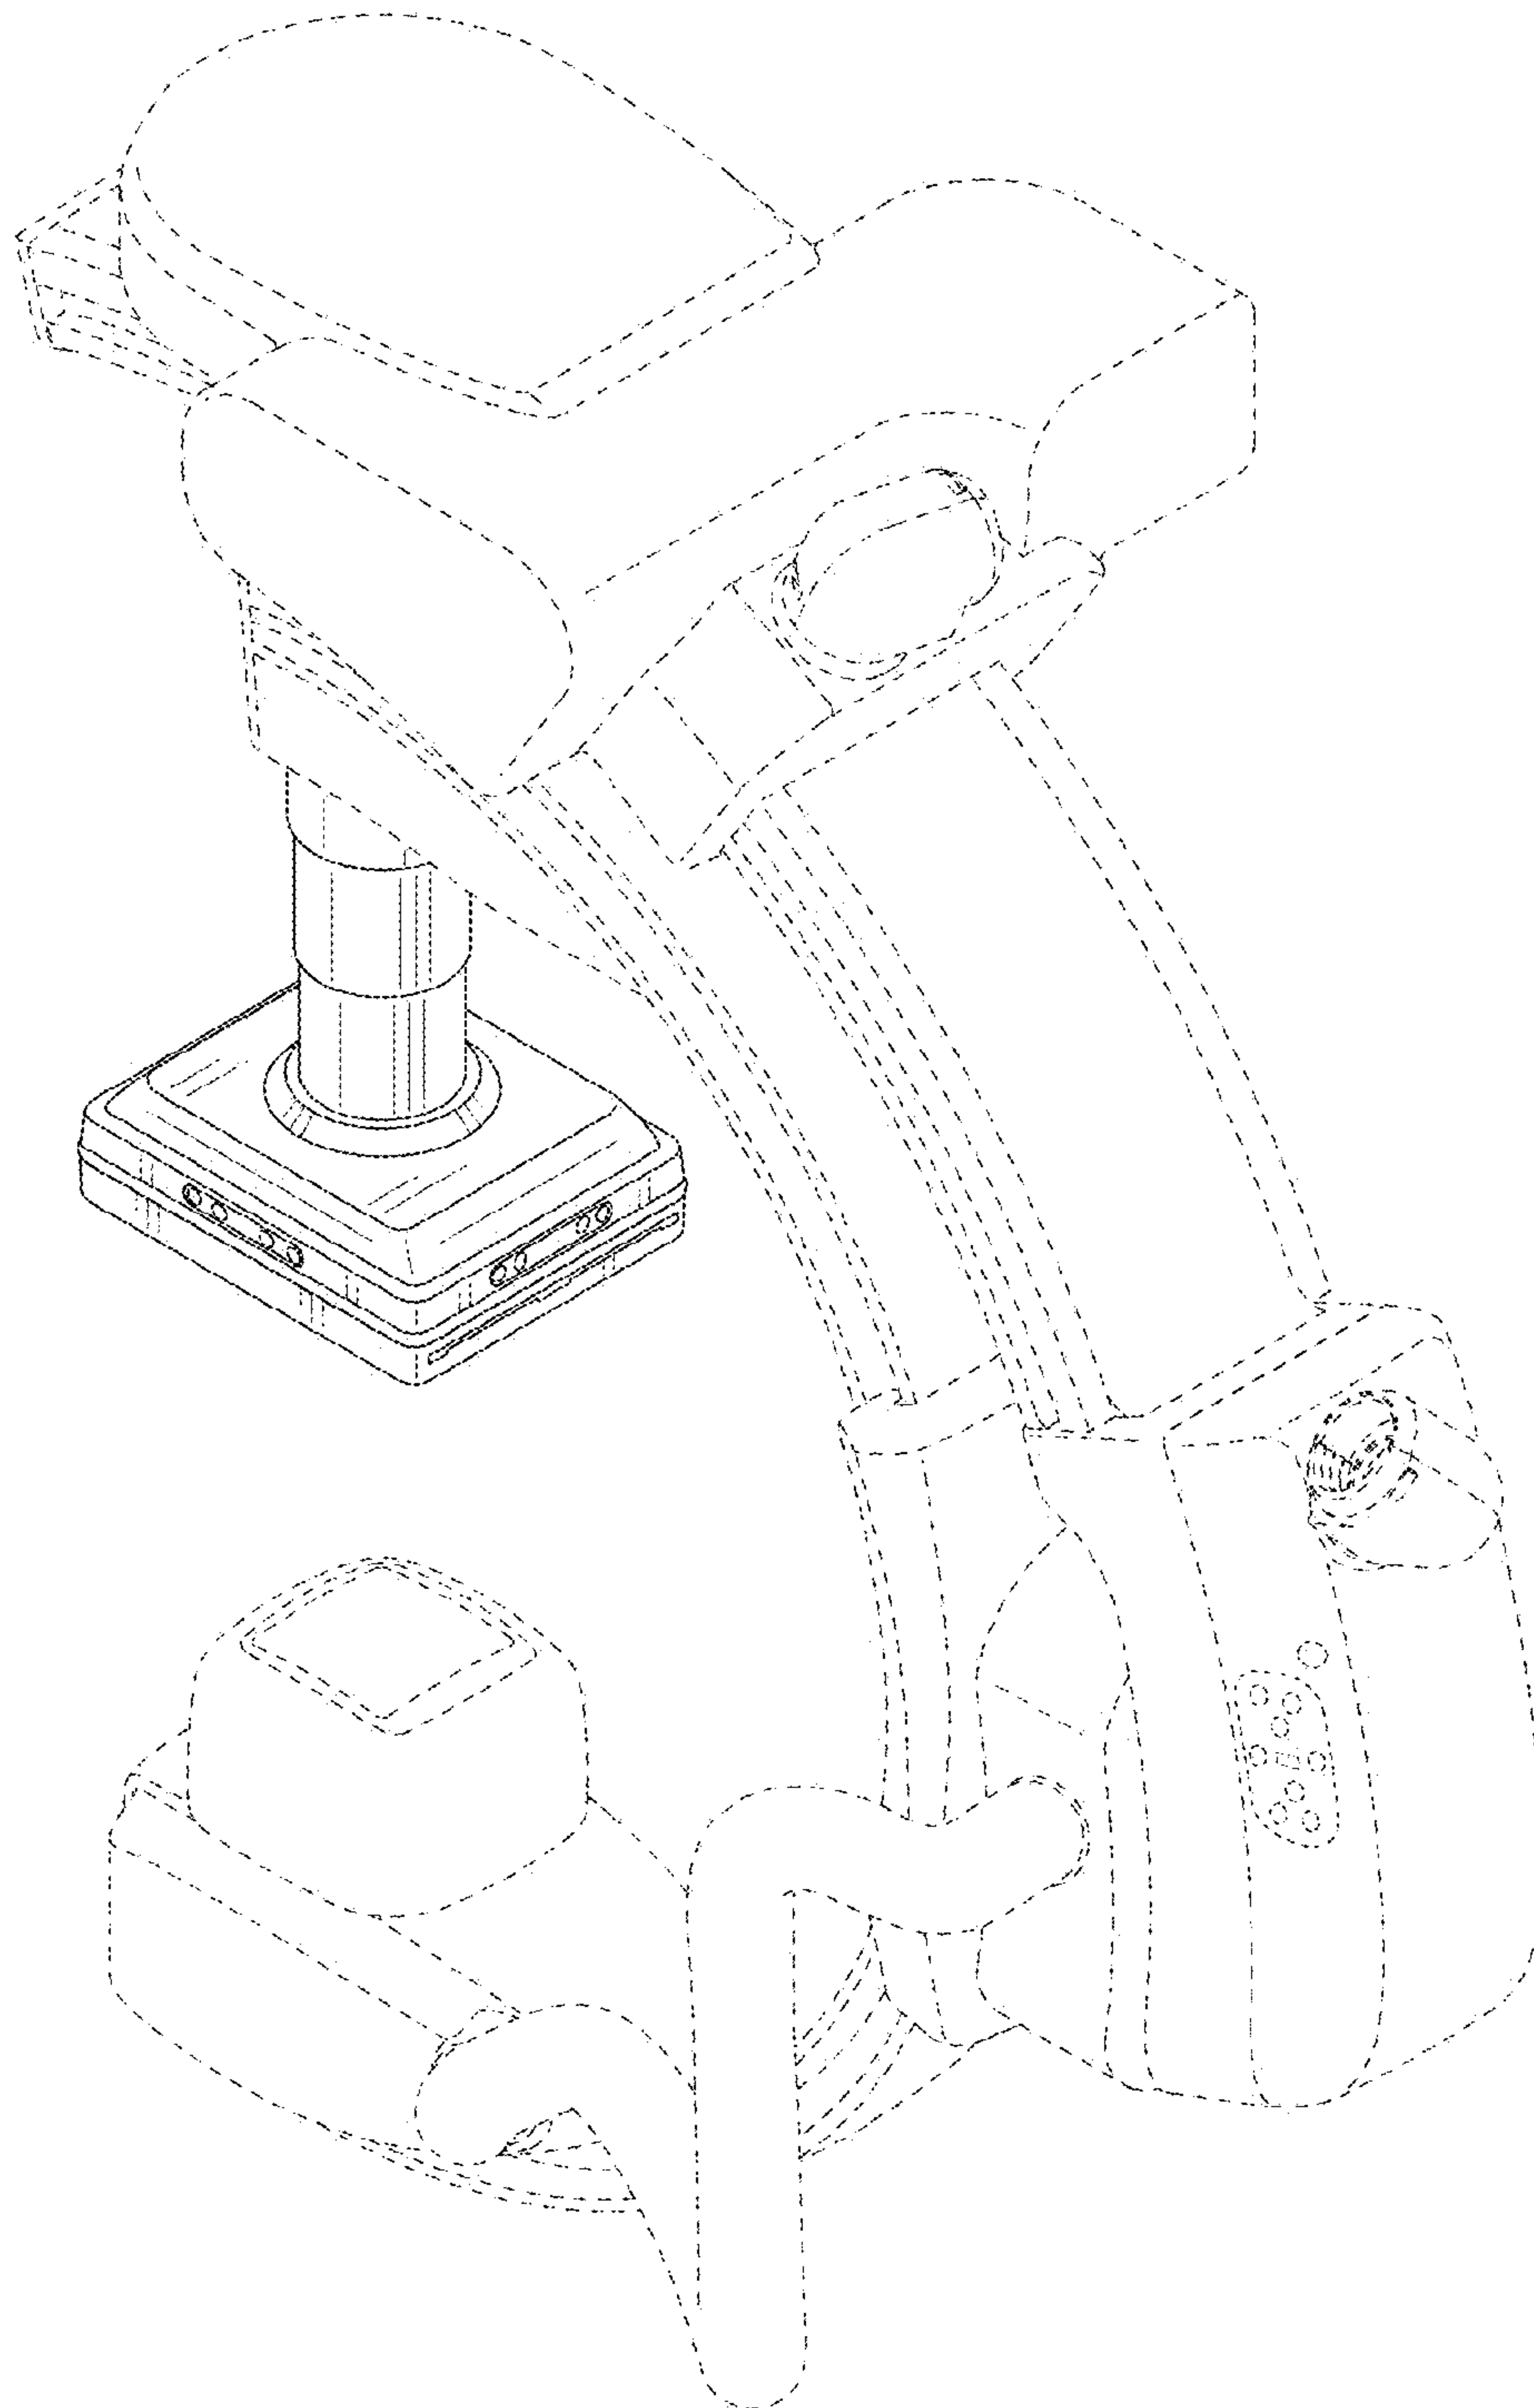


Fig. 2

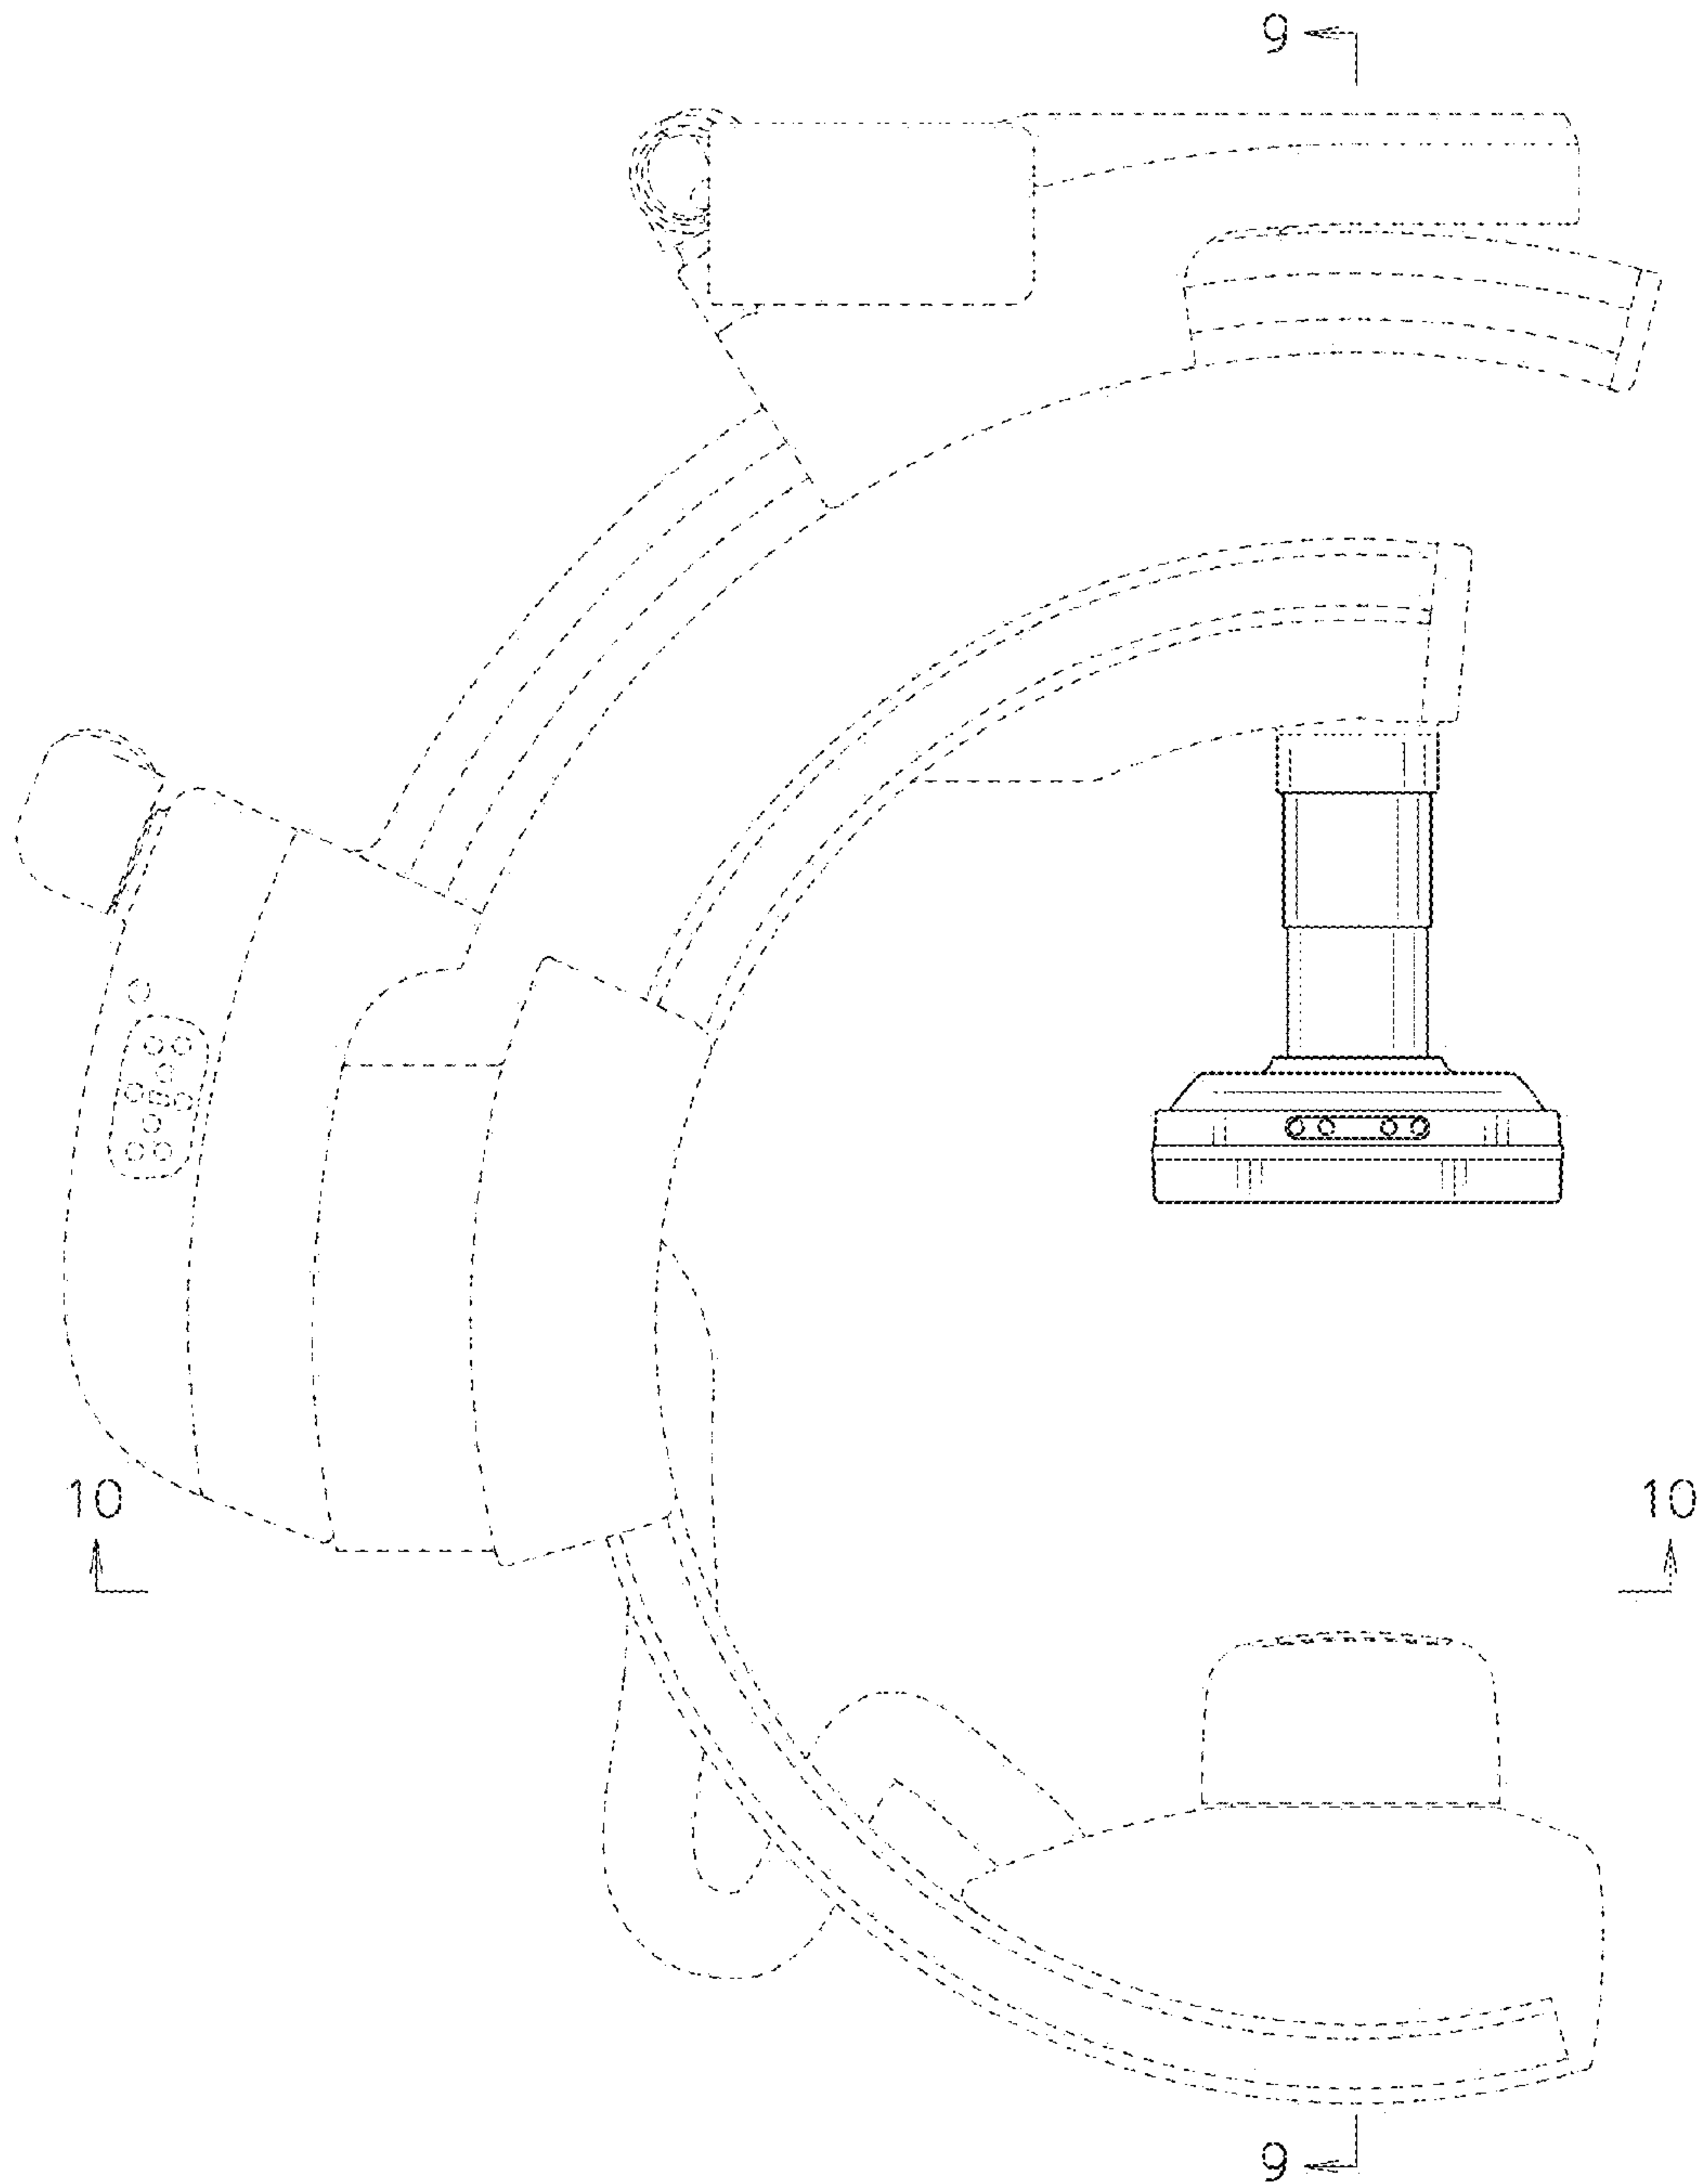


Fig. 3

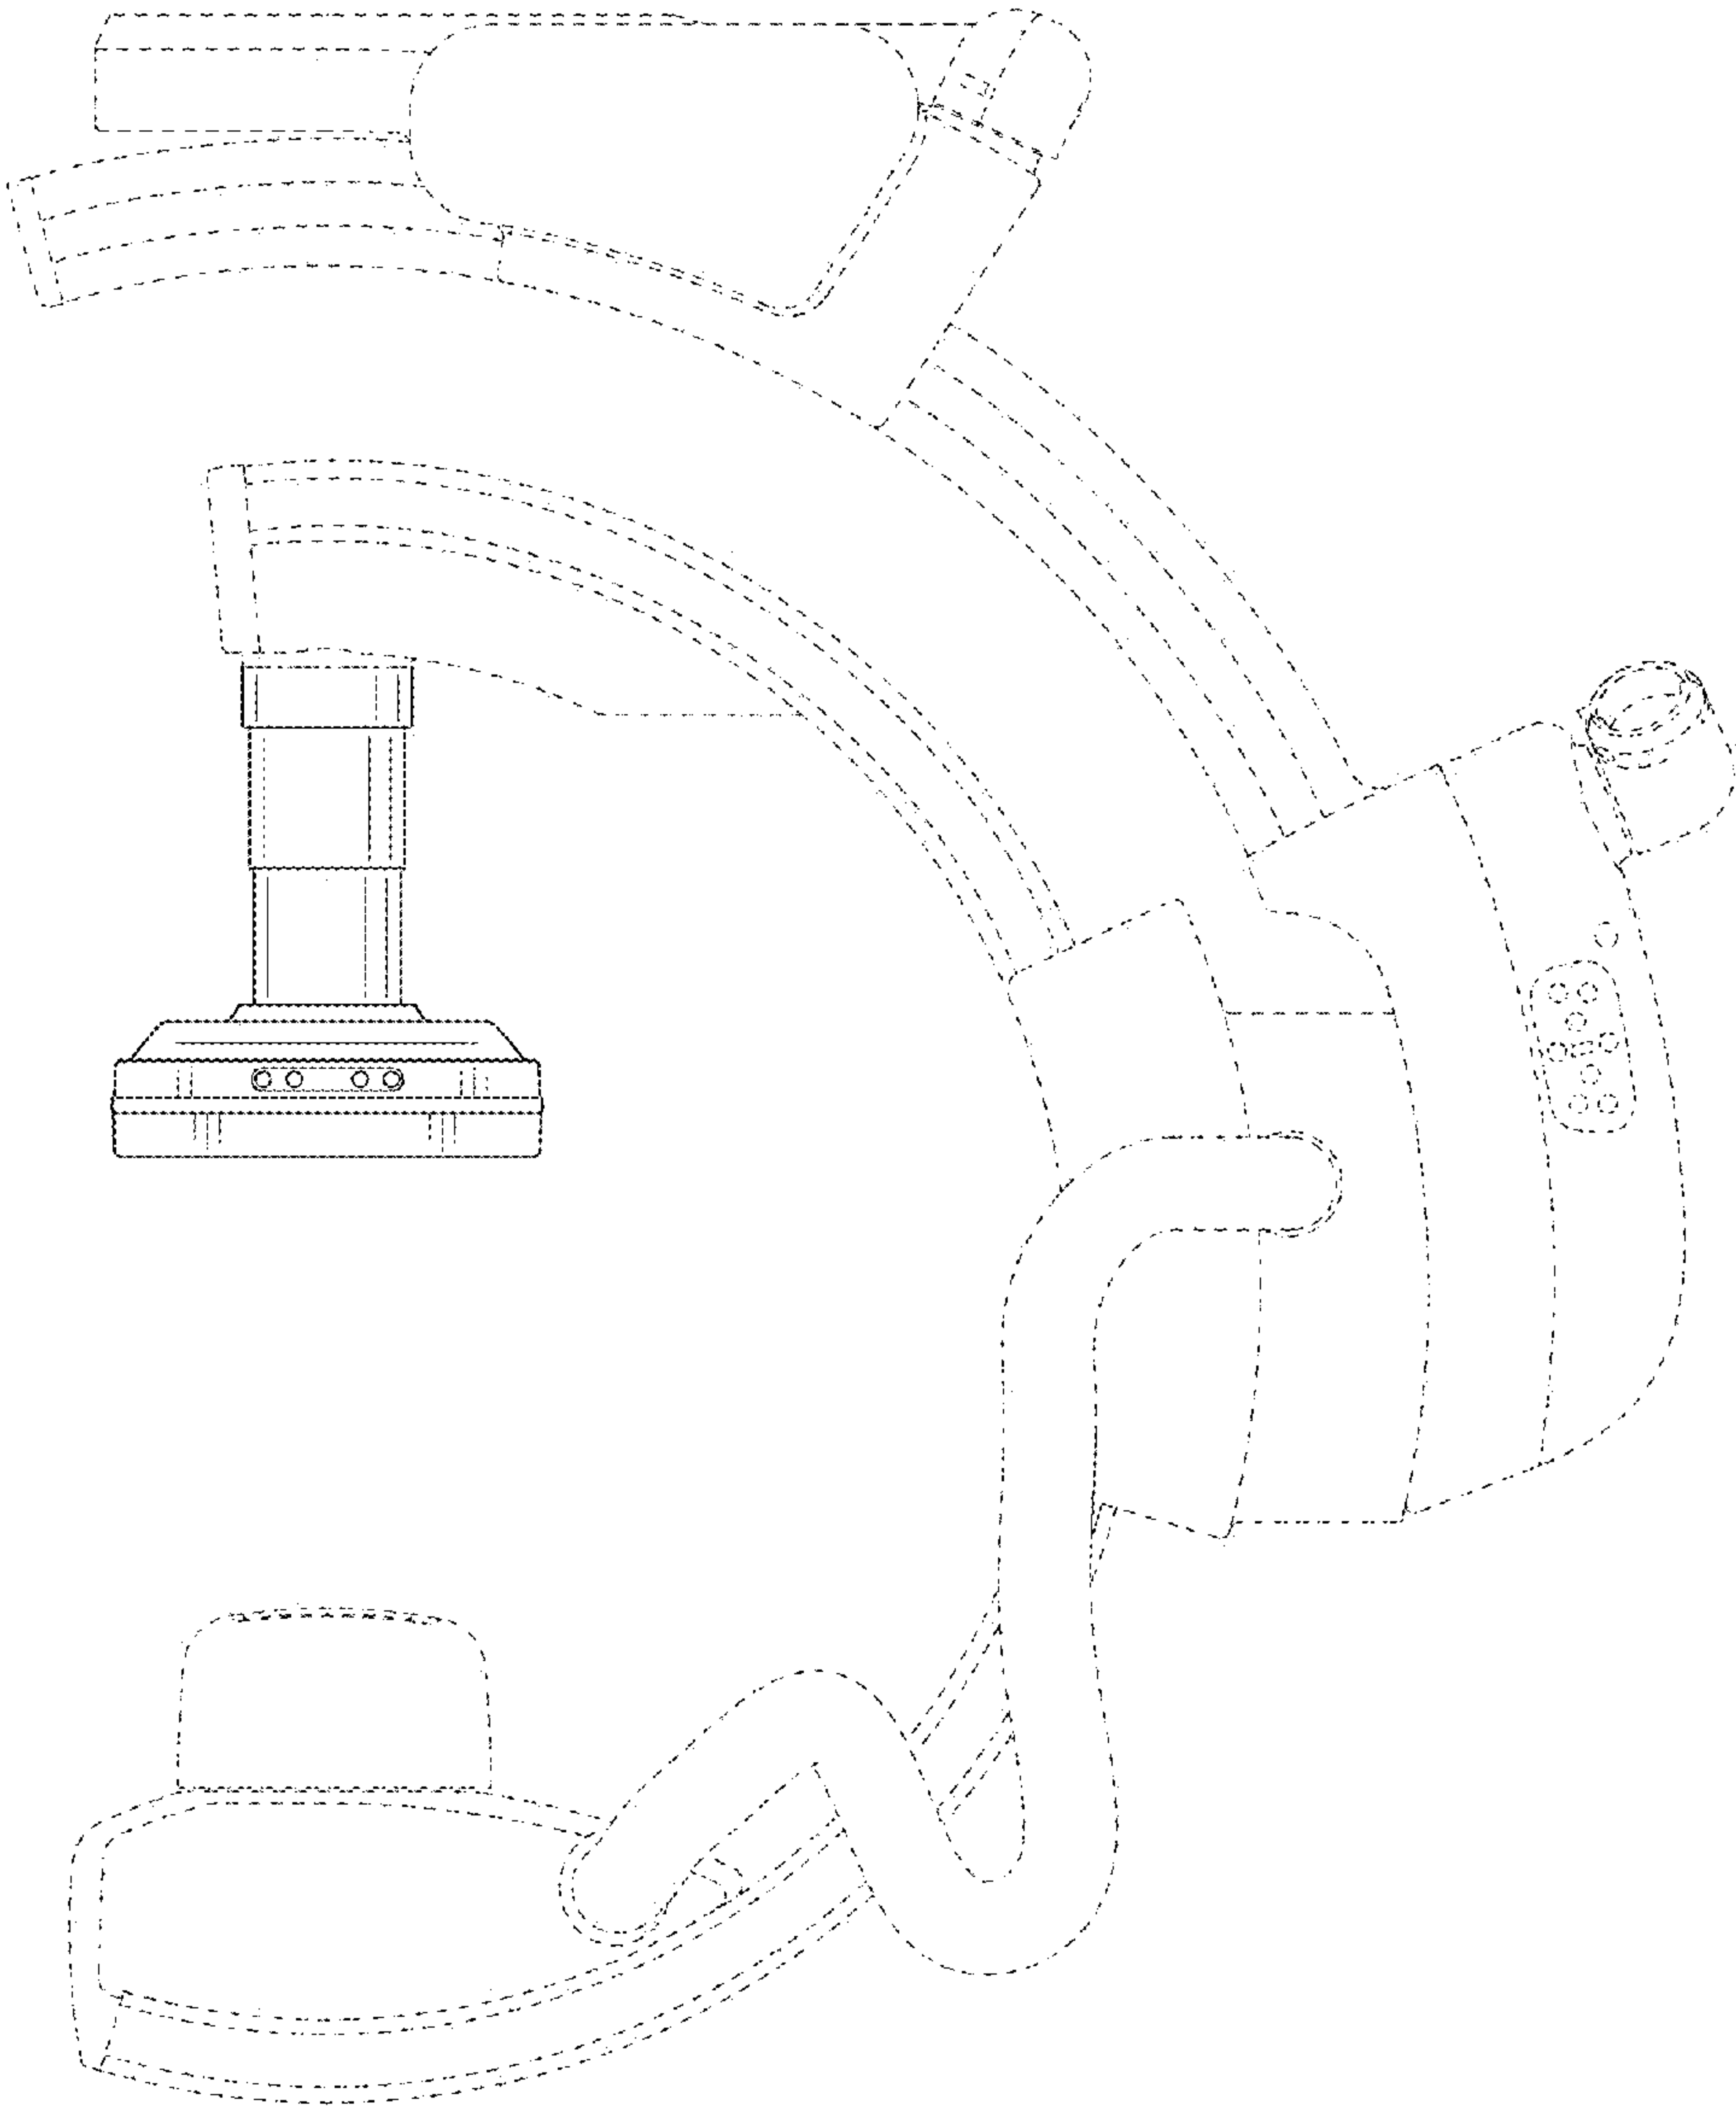


Fig. 4

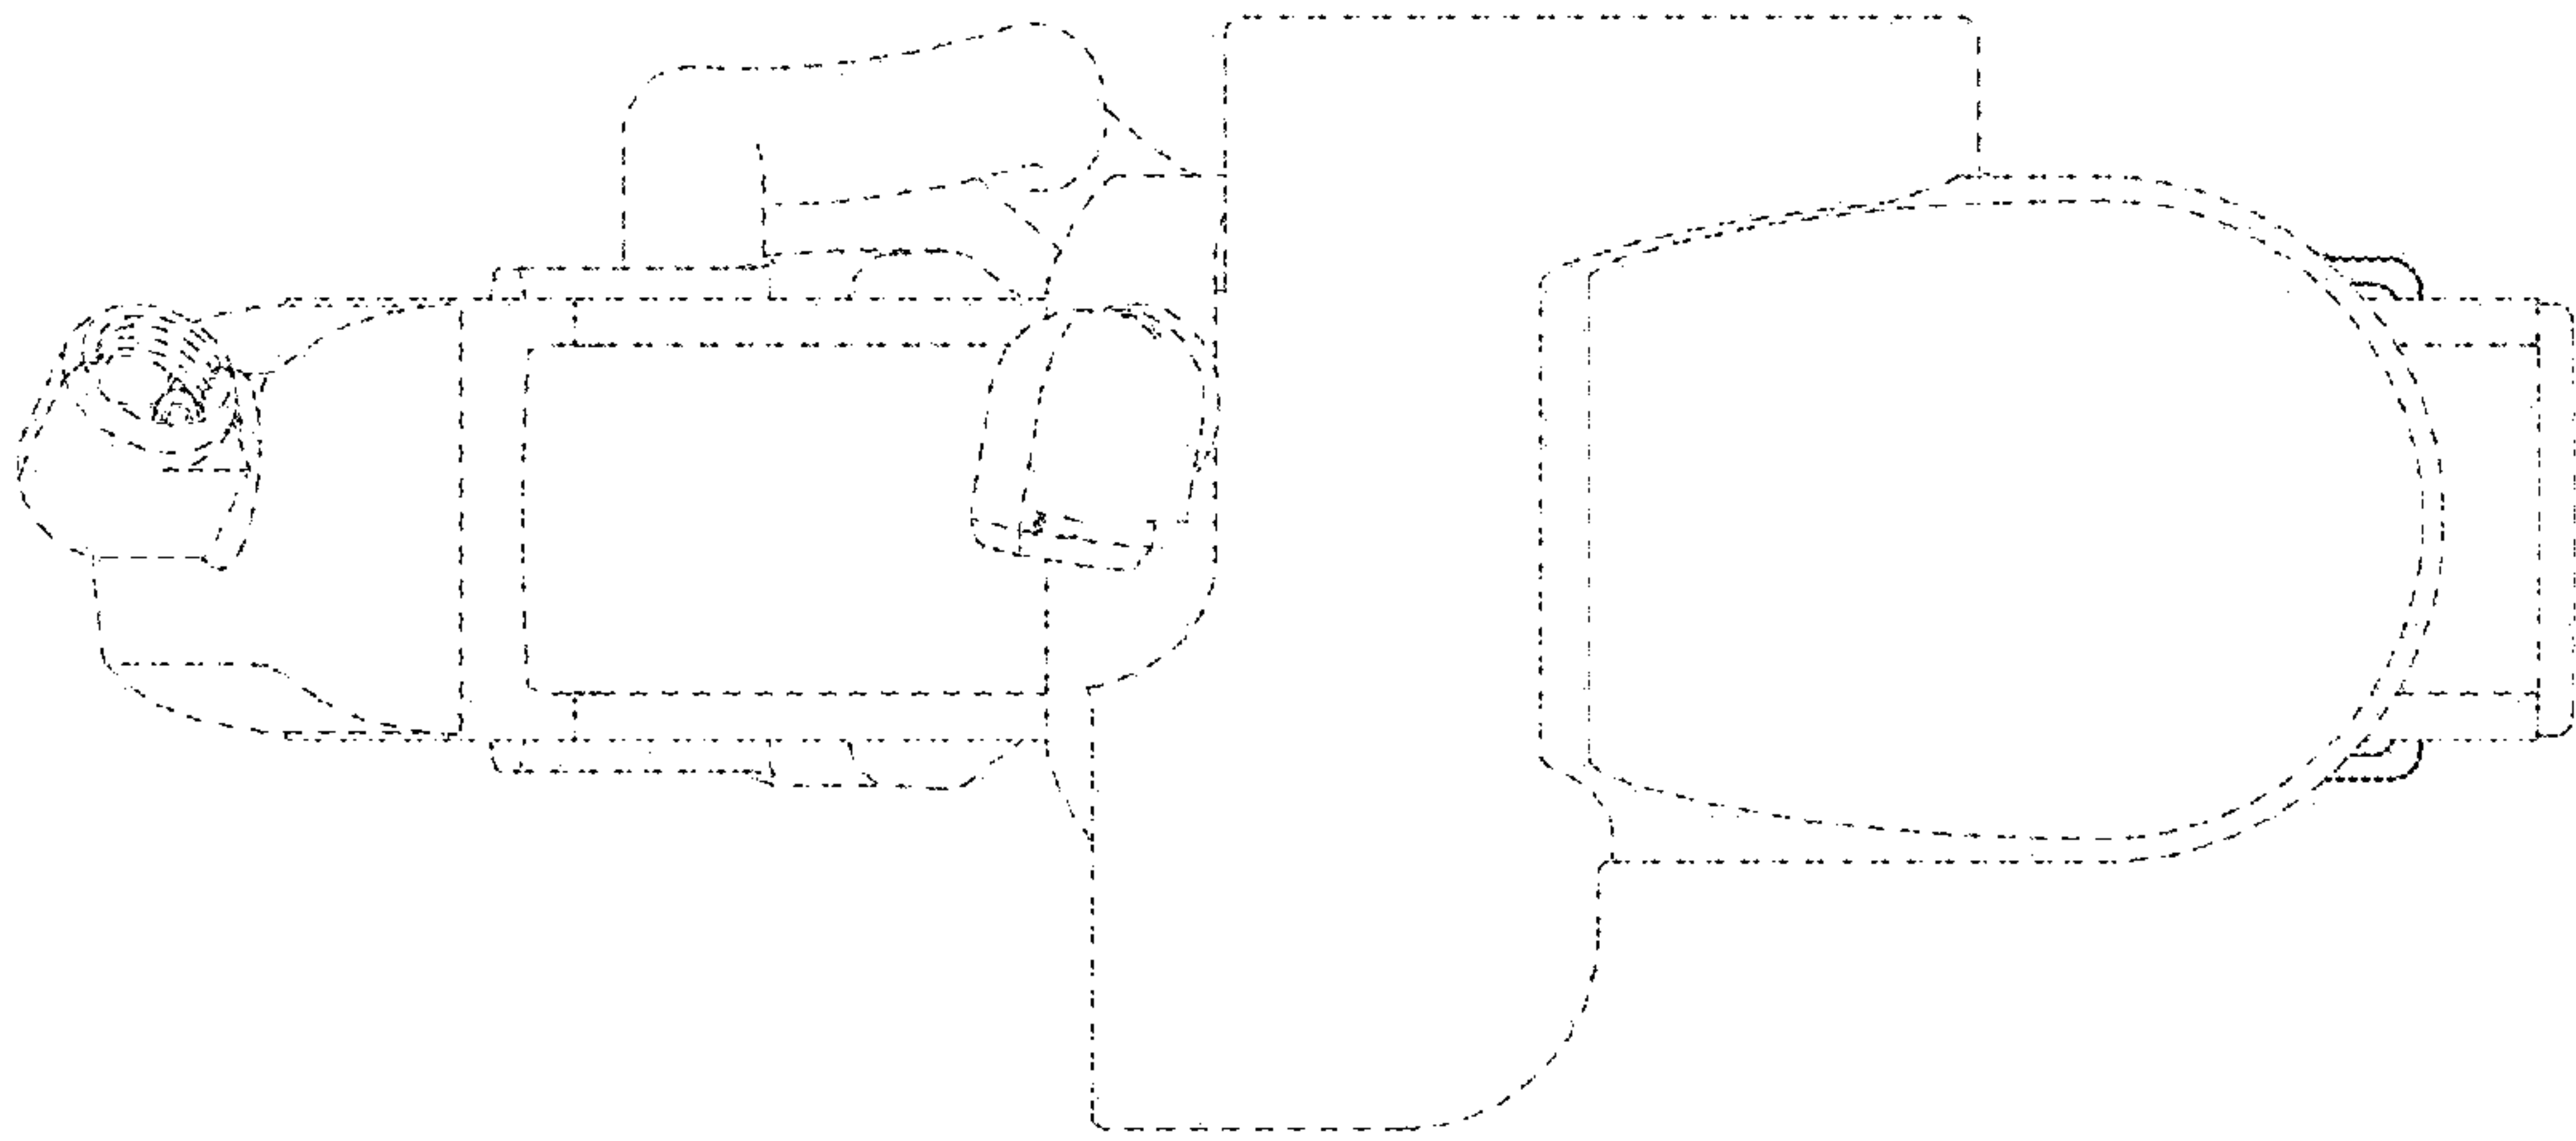


Fig. 5

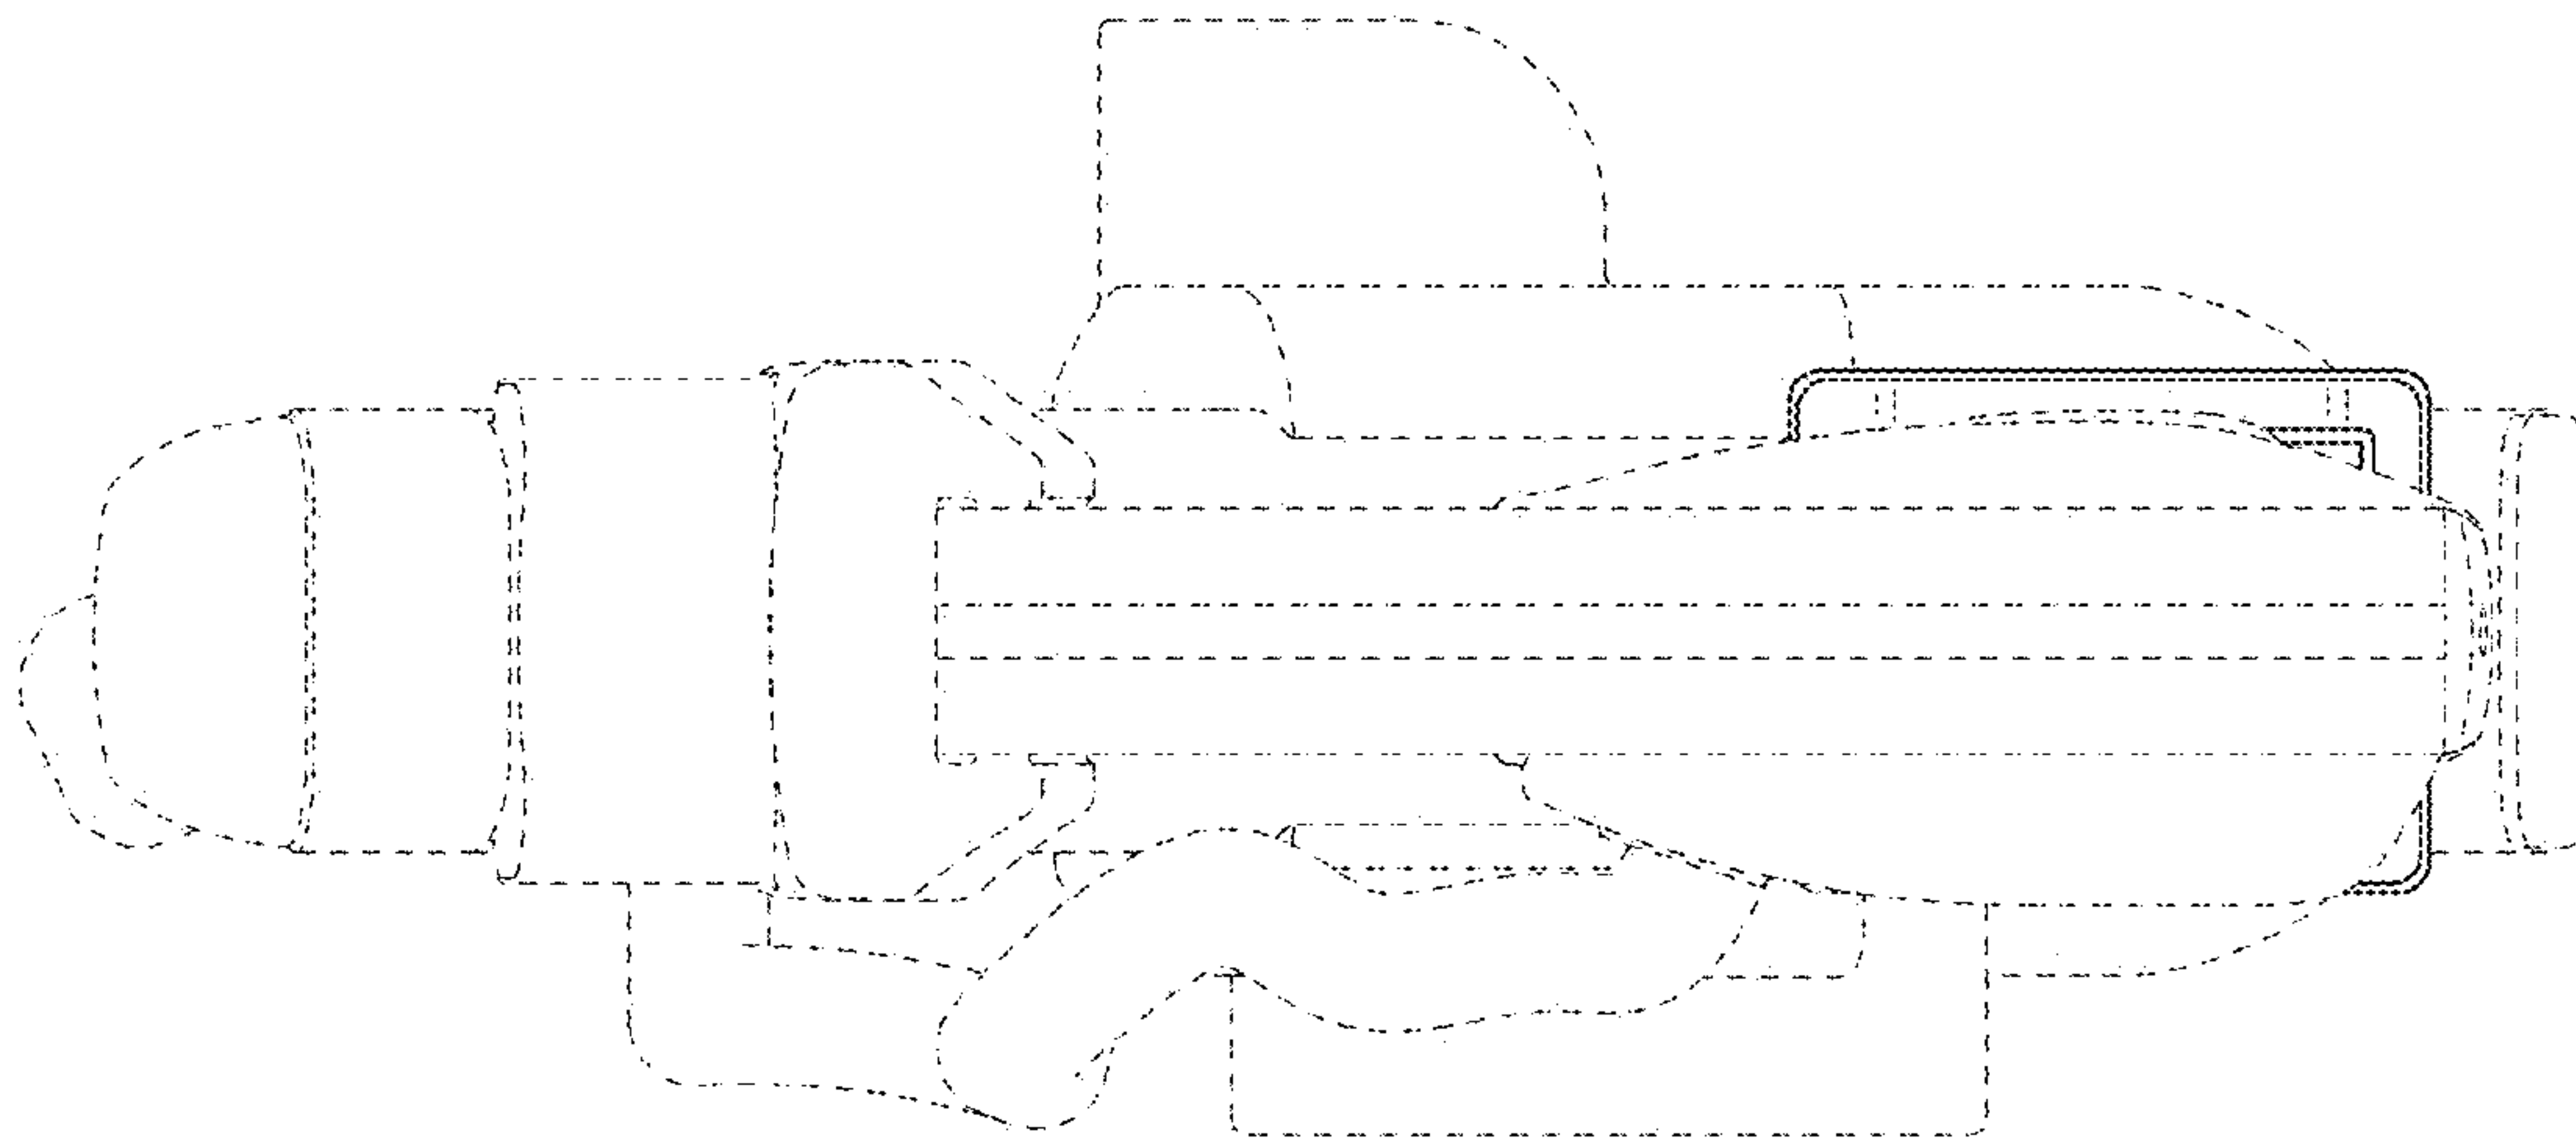


Fig. 6

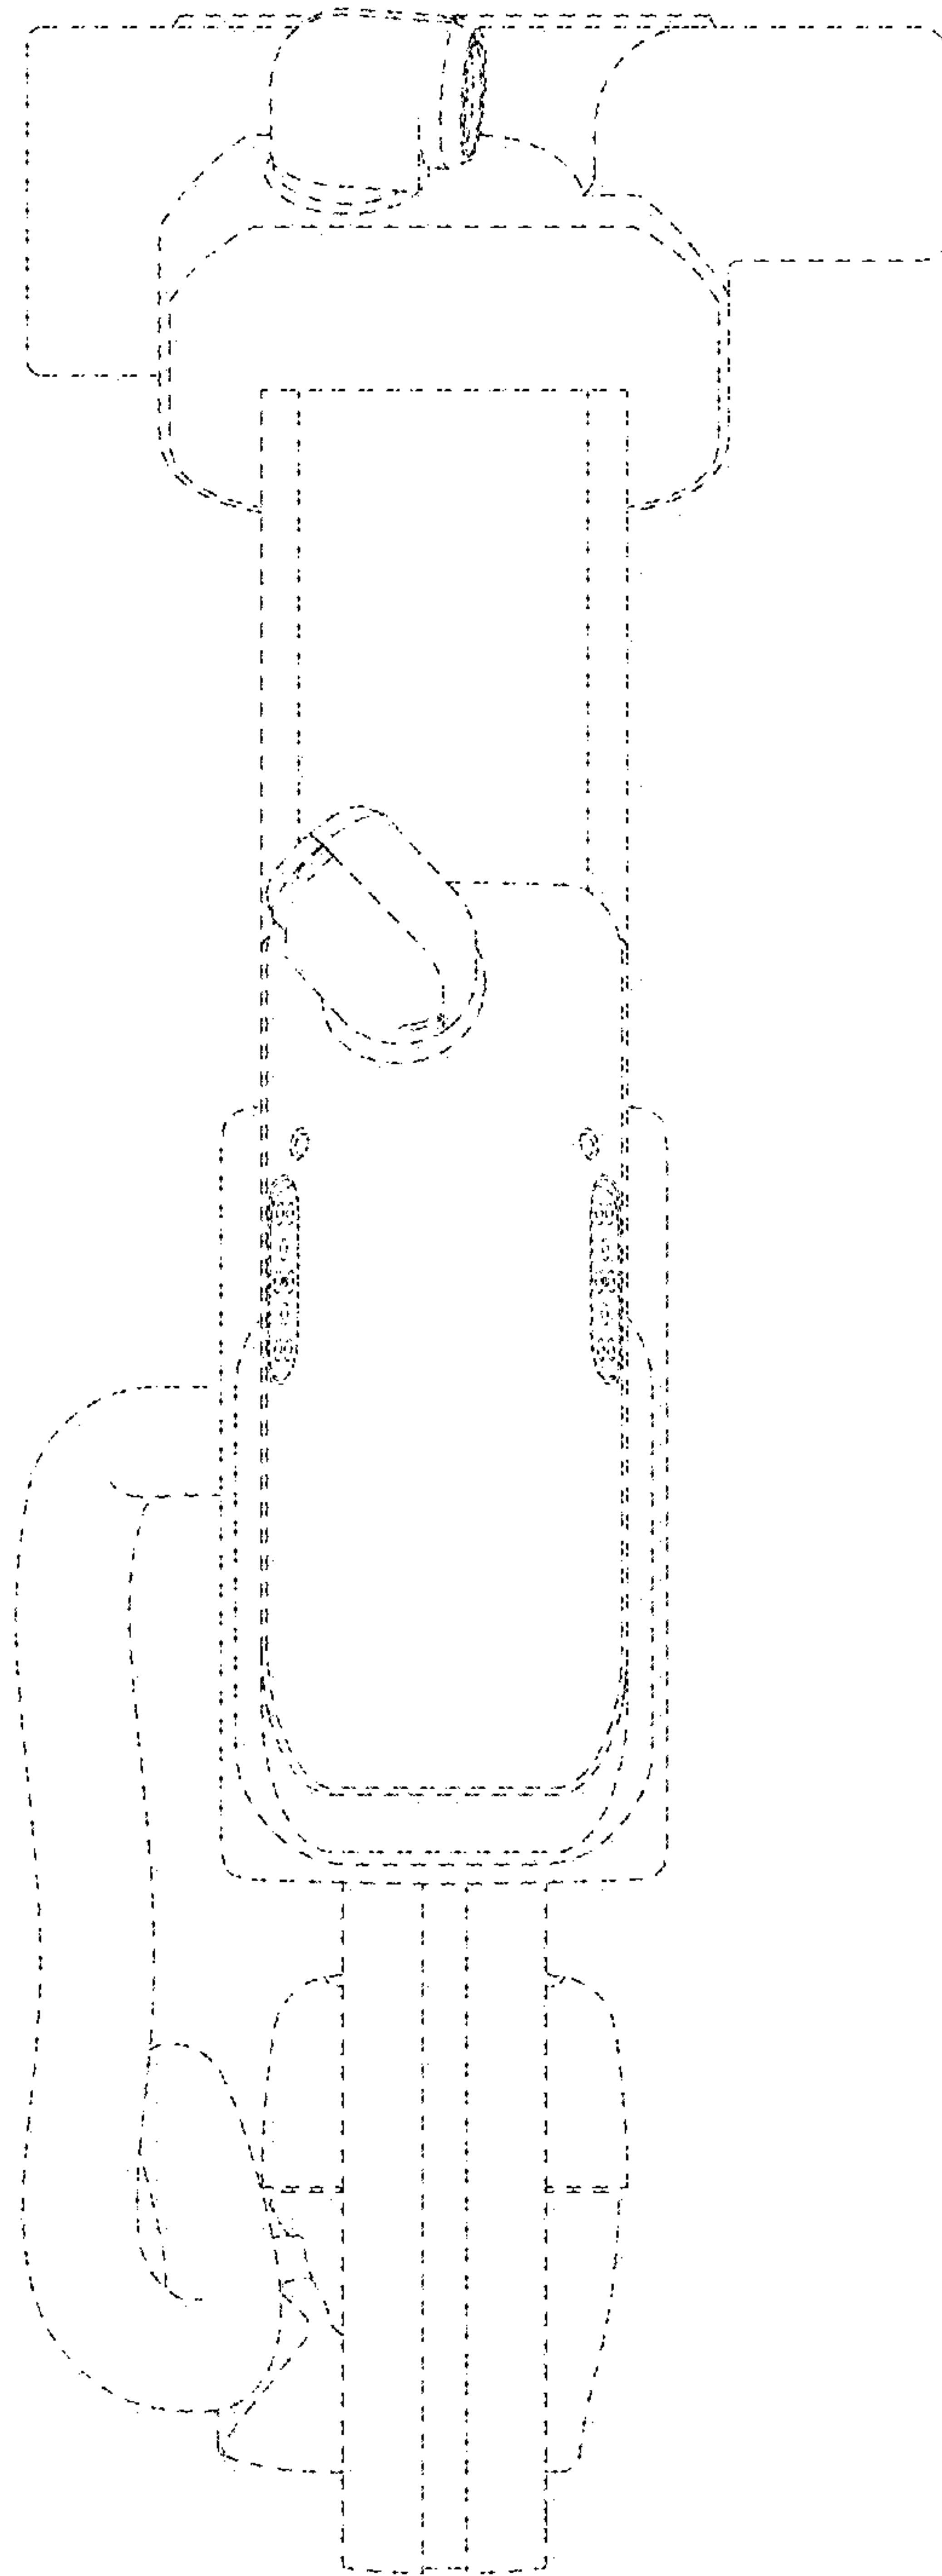


Fig. 7

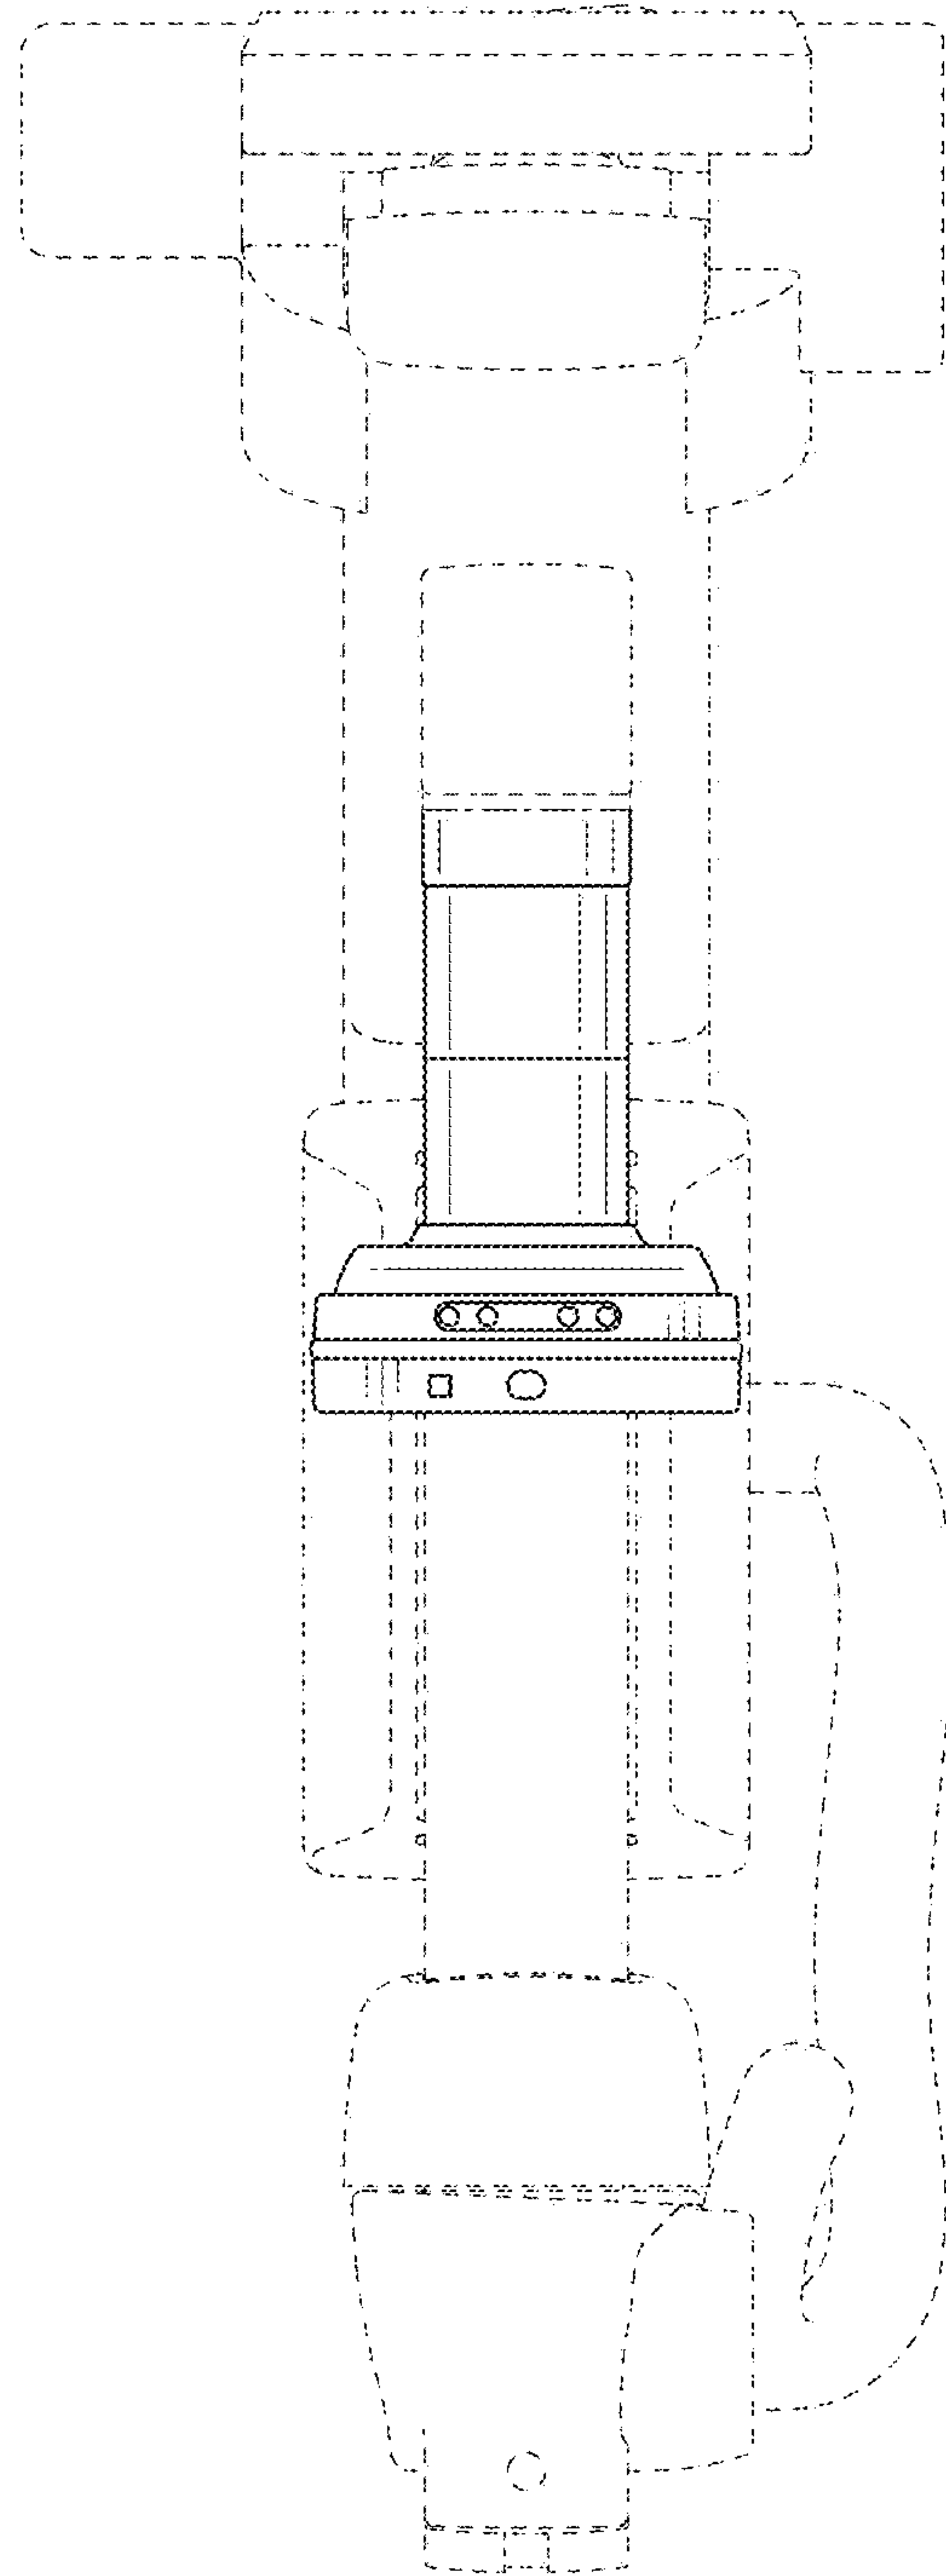


Fig. 8

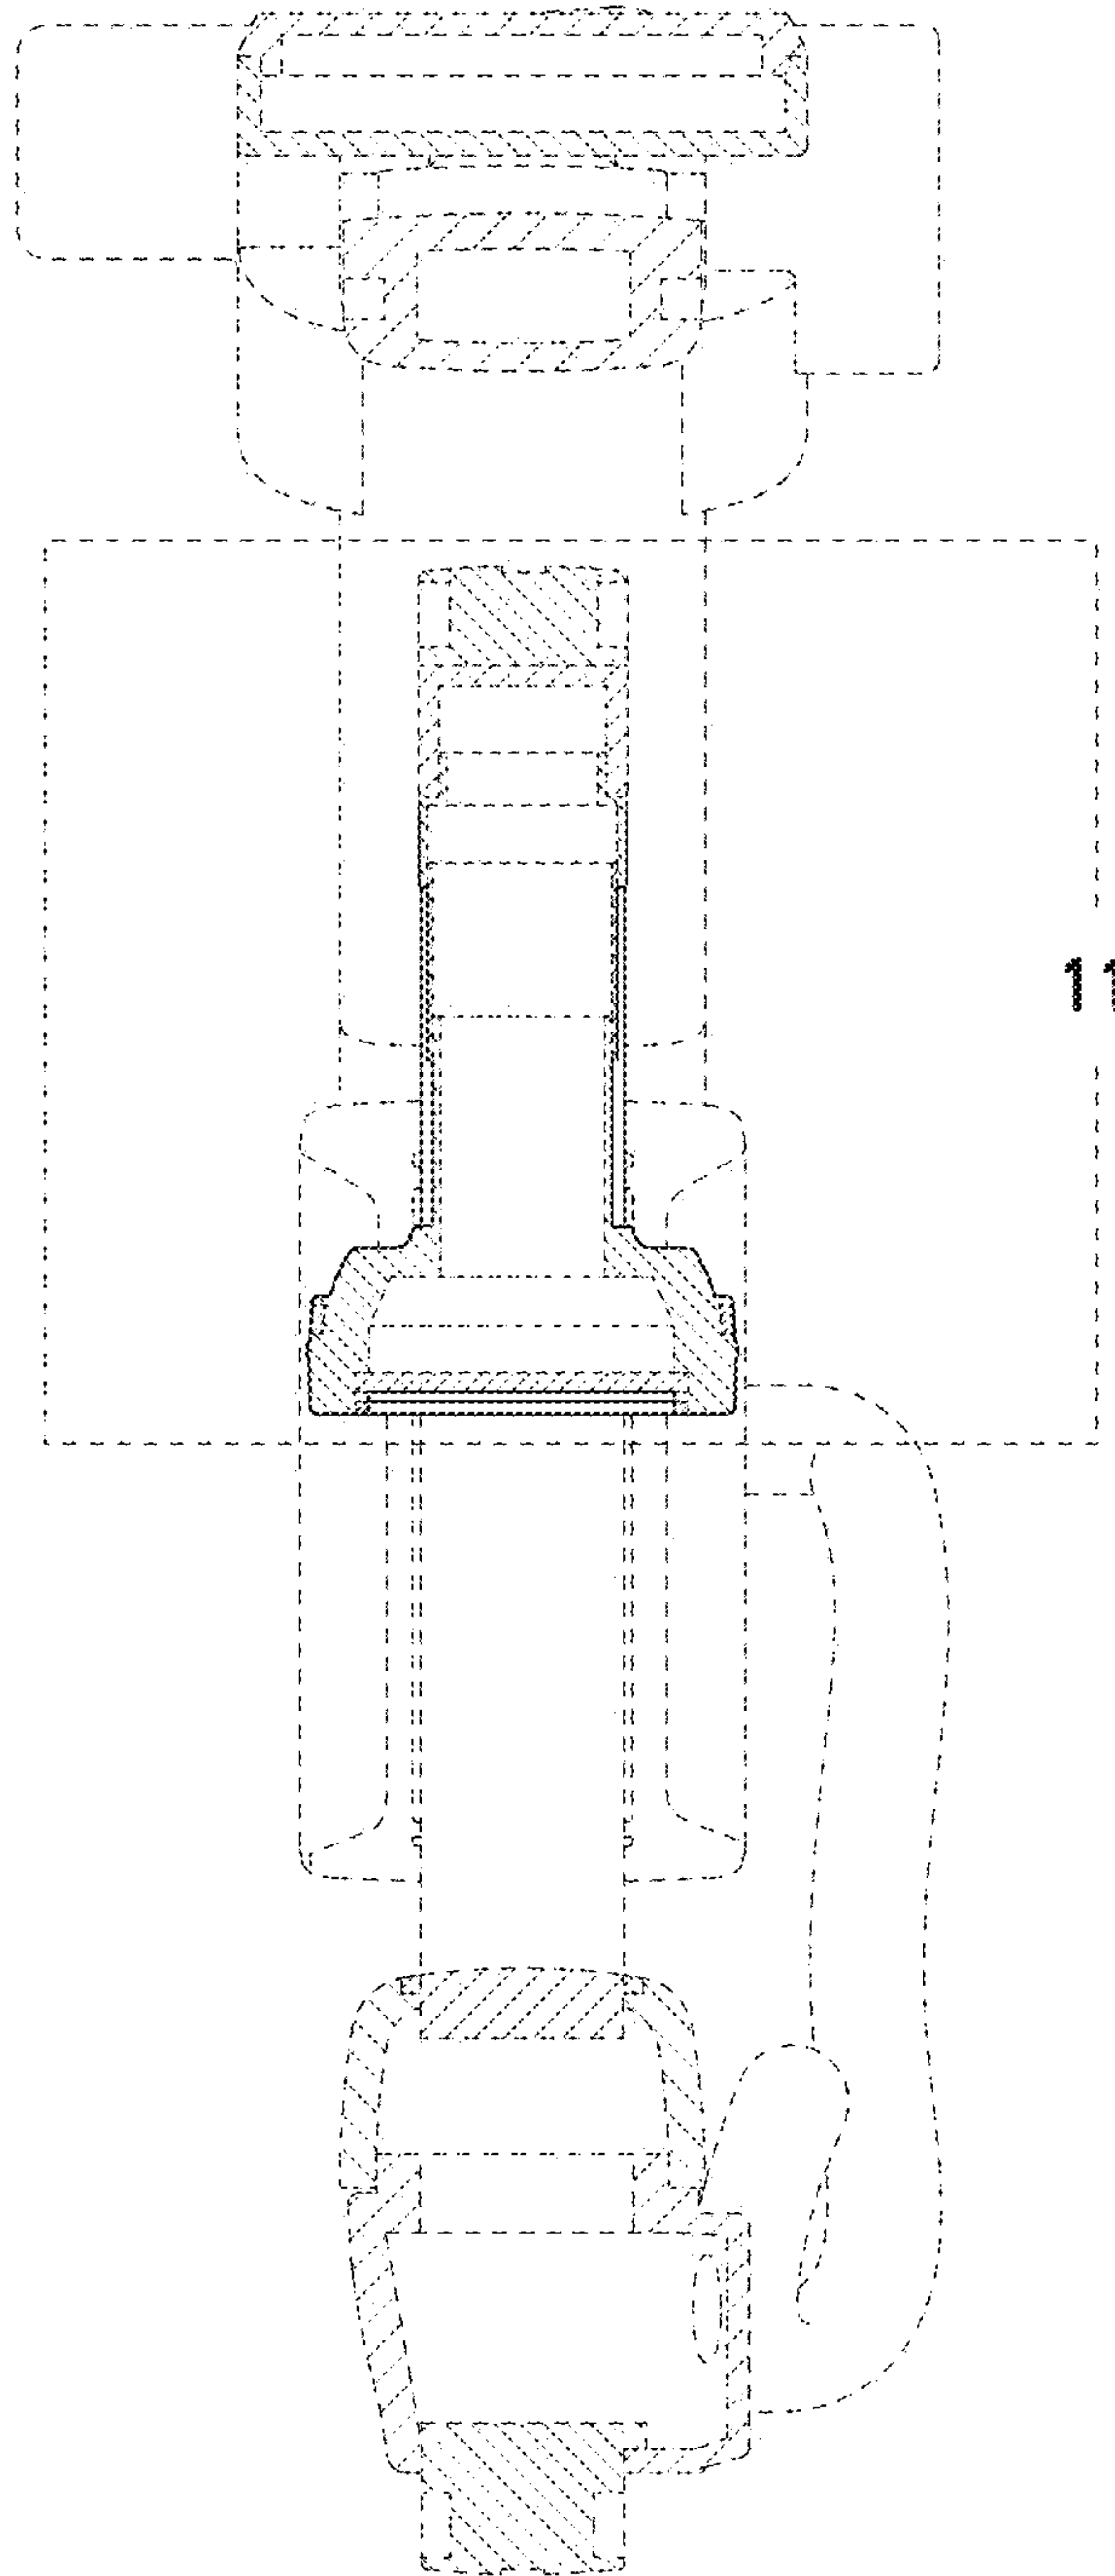


Fig. 9

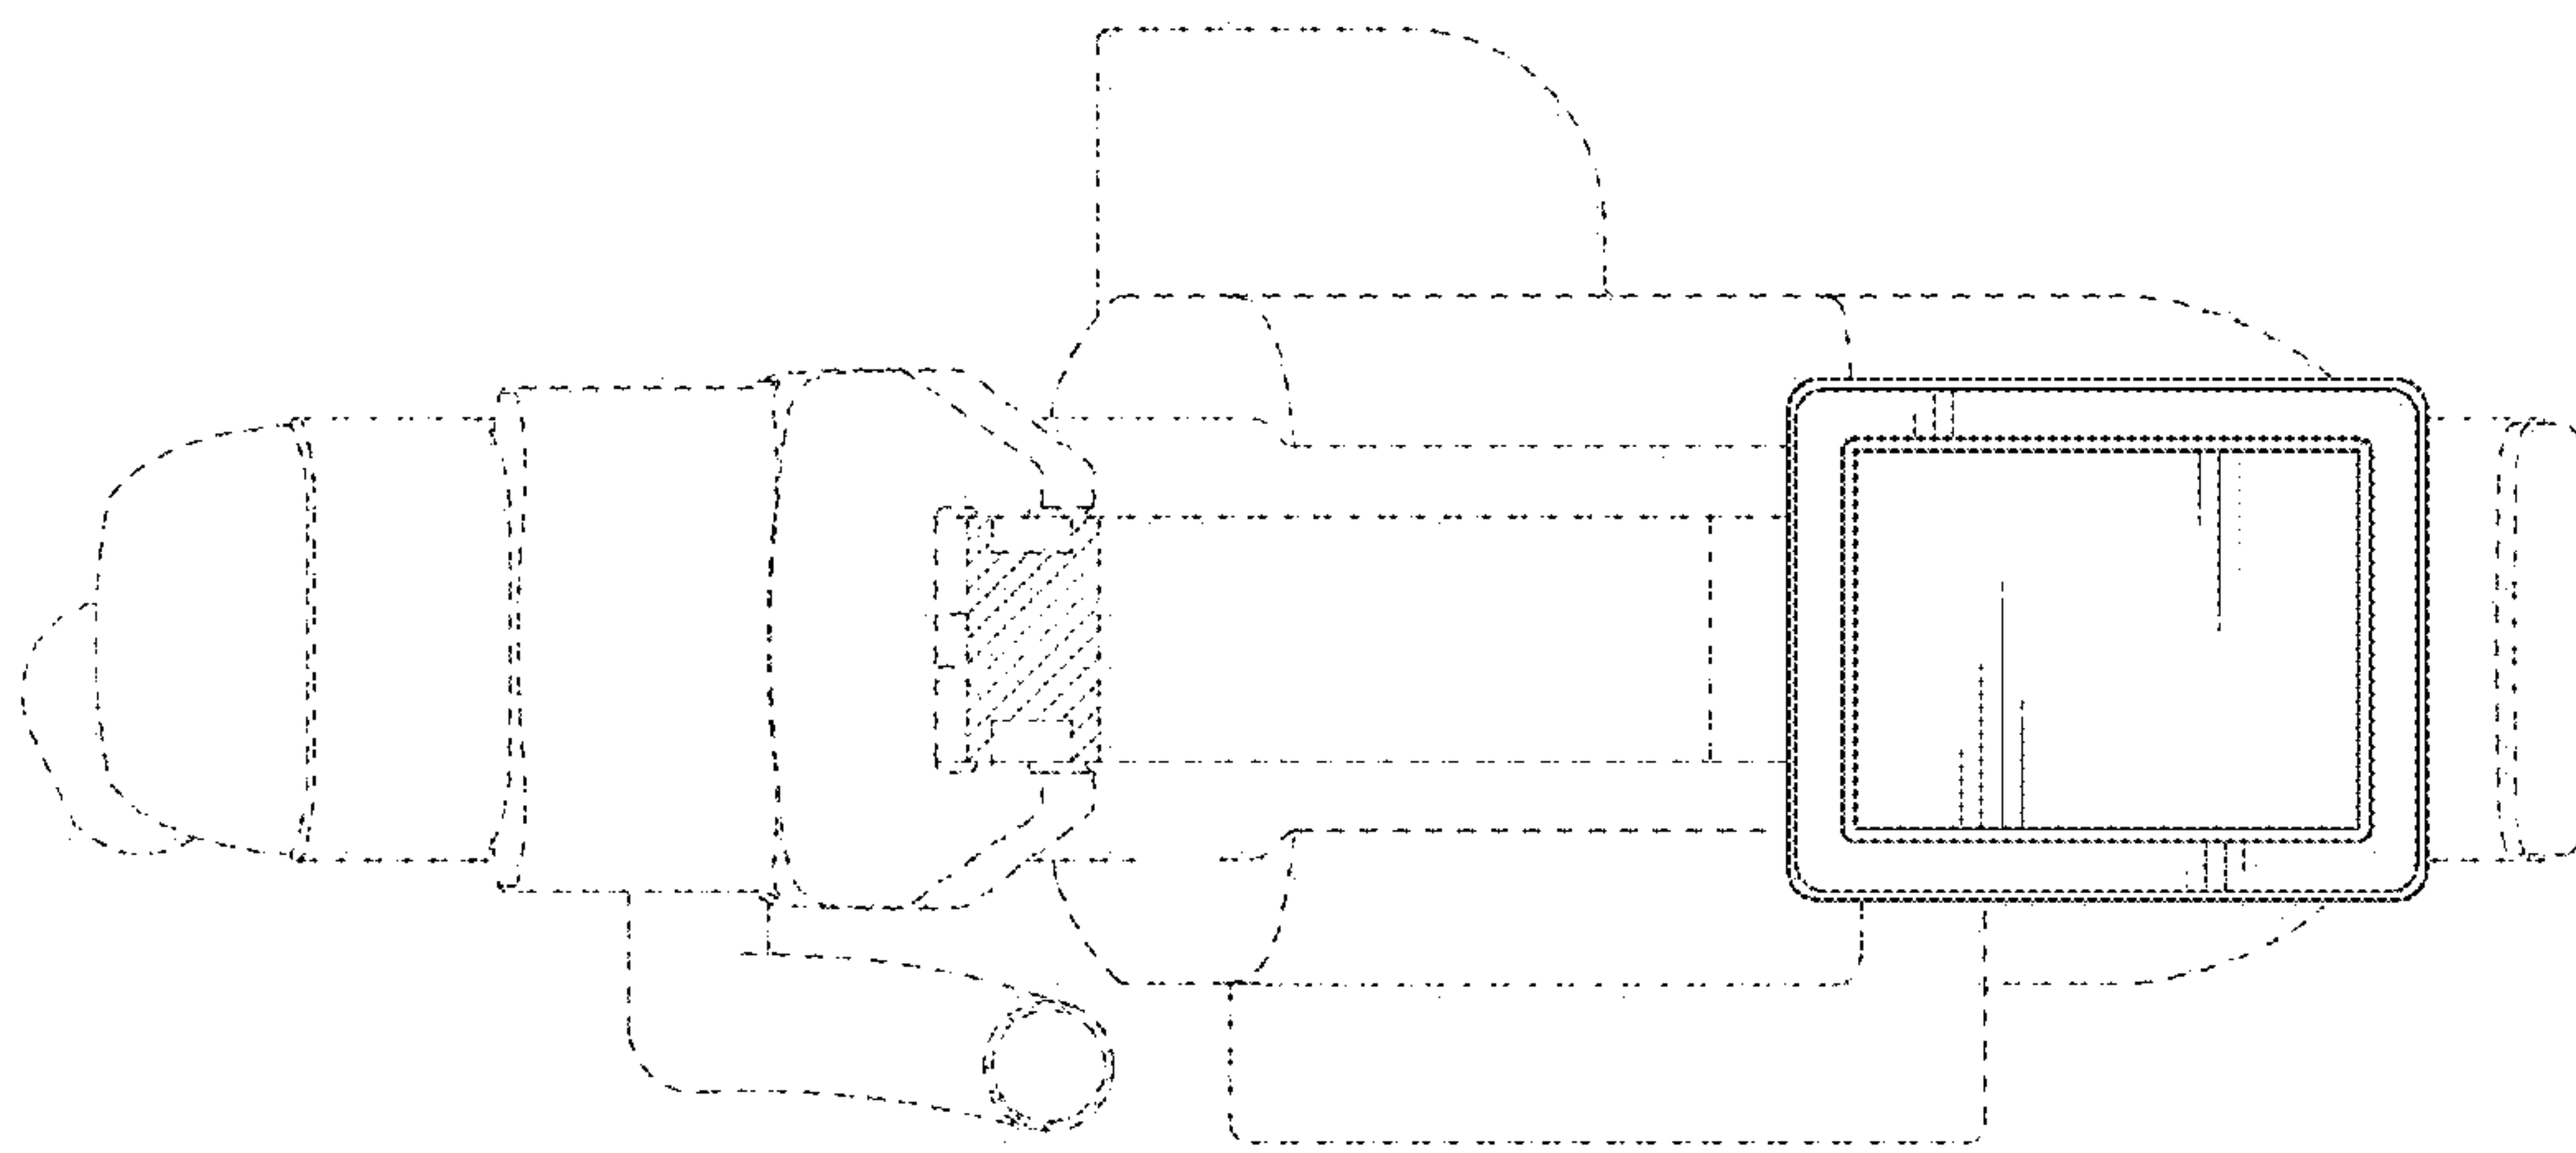


Fig. 10

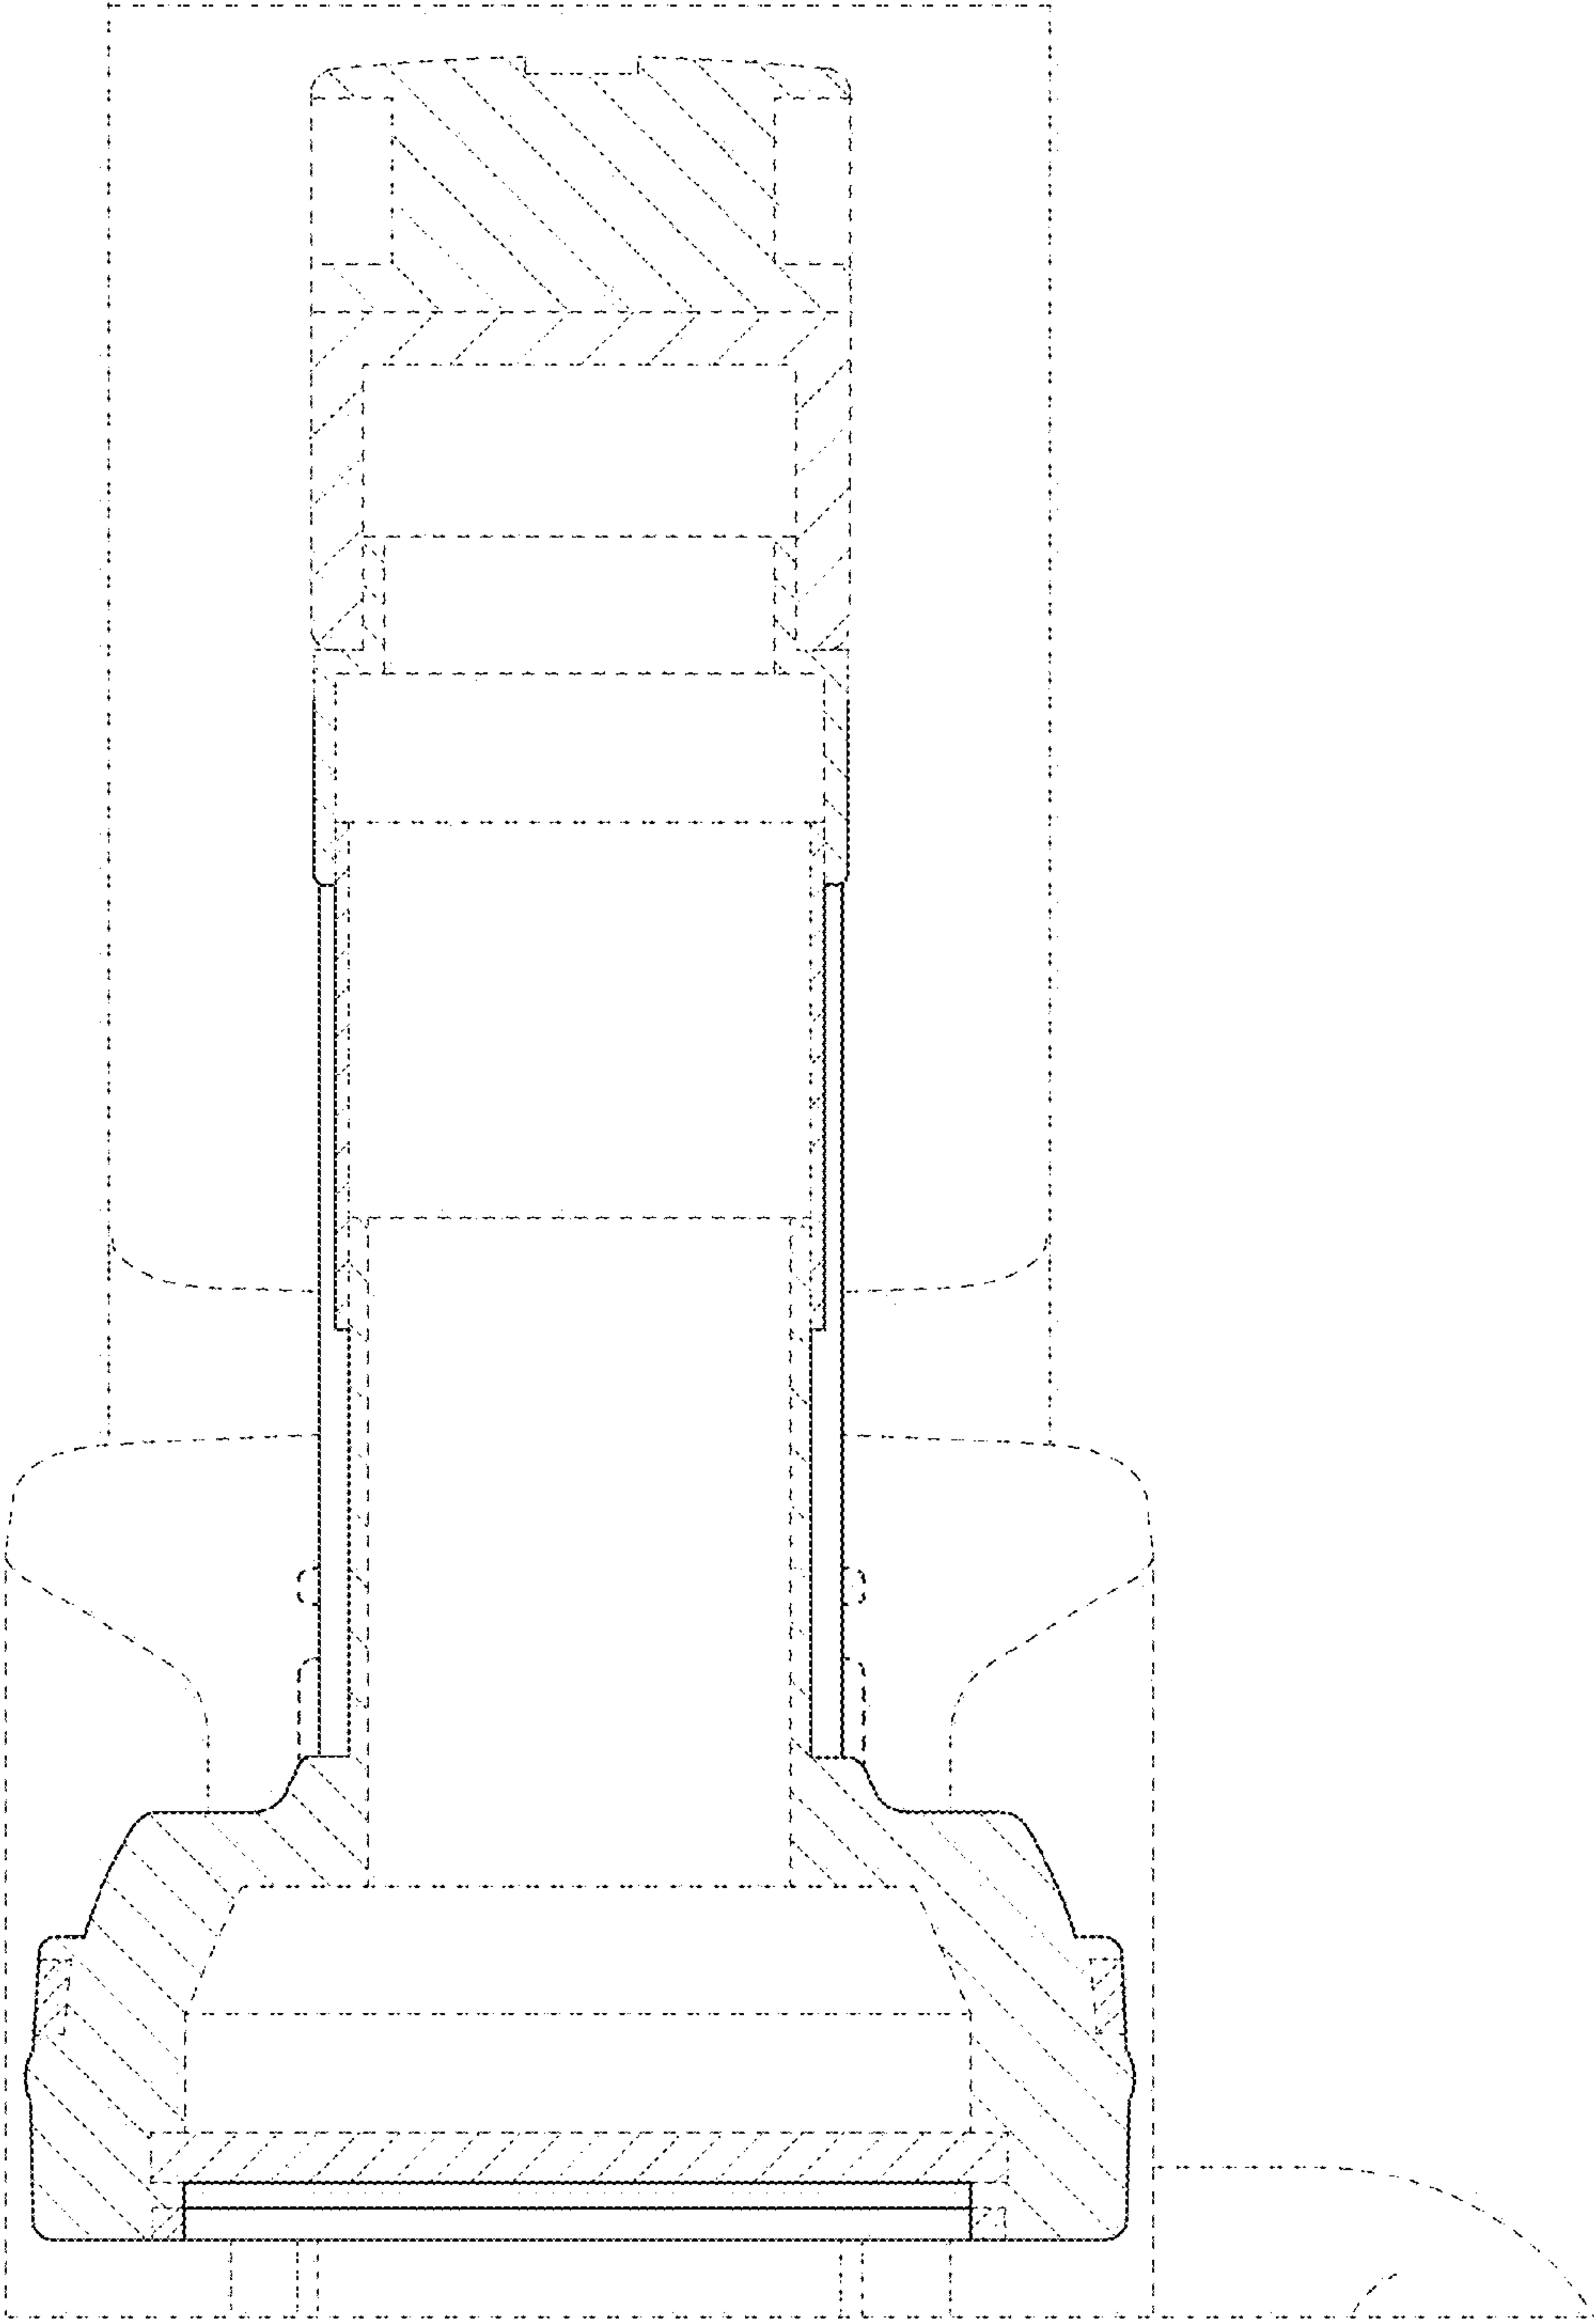


Fig. 11

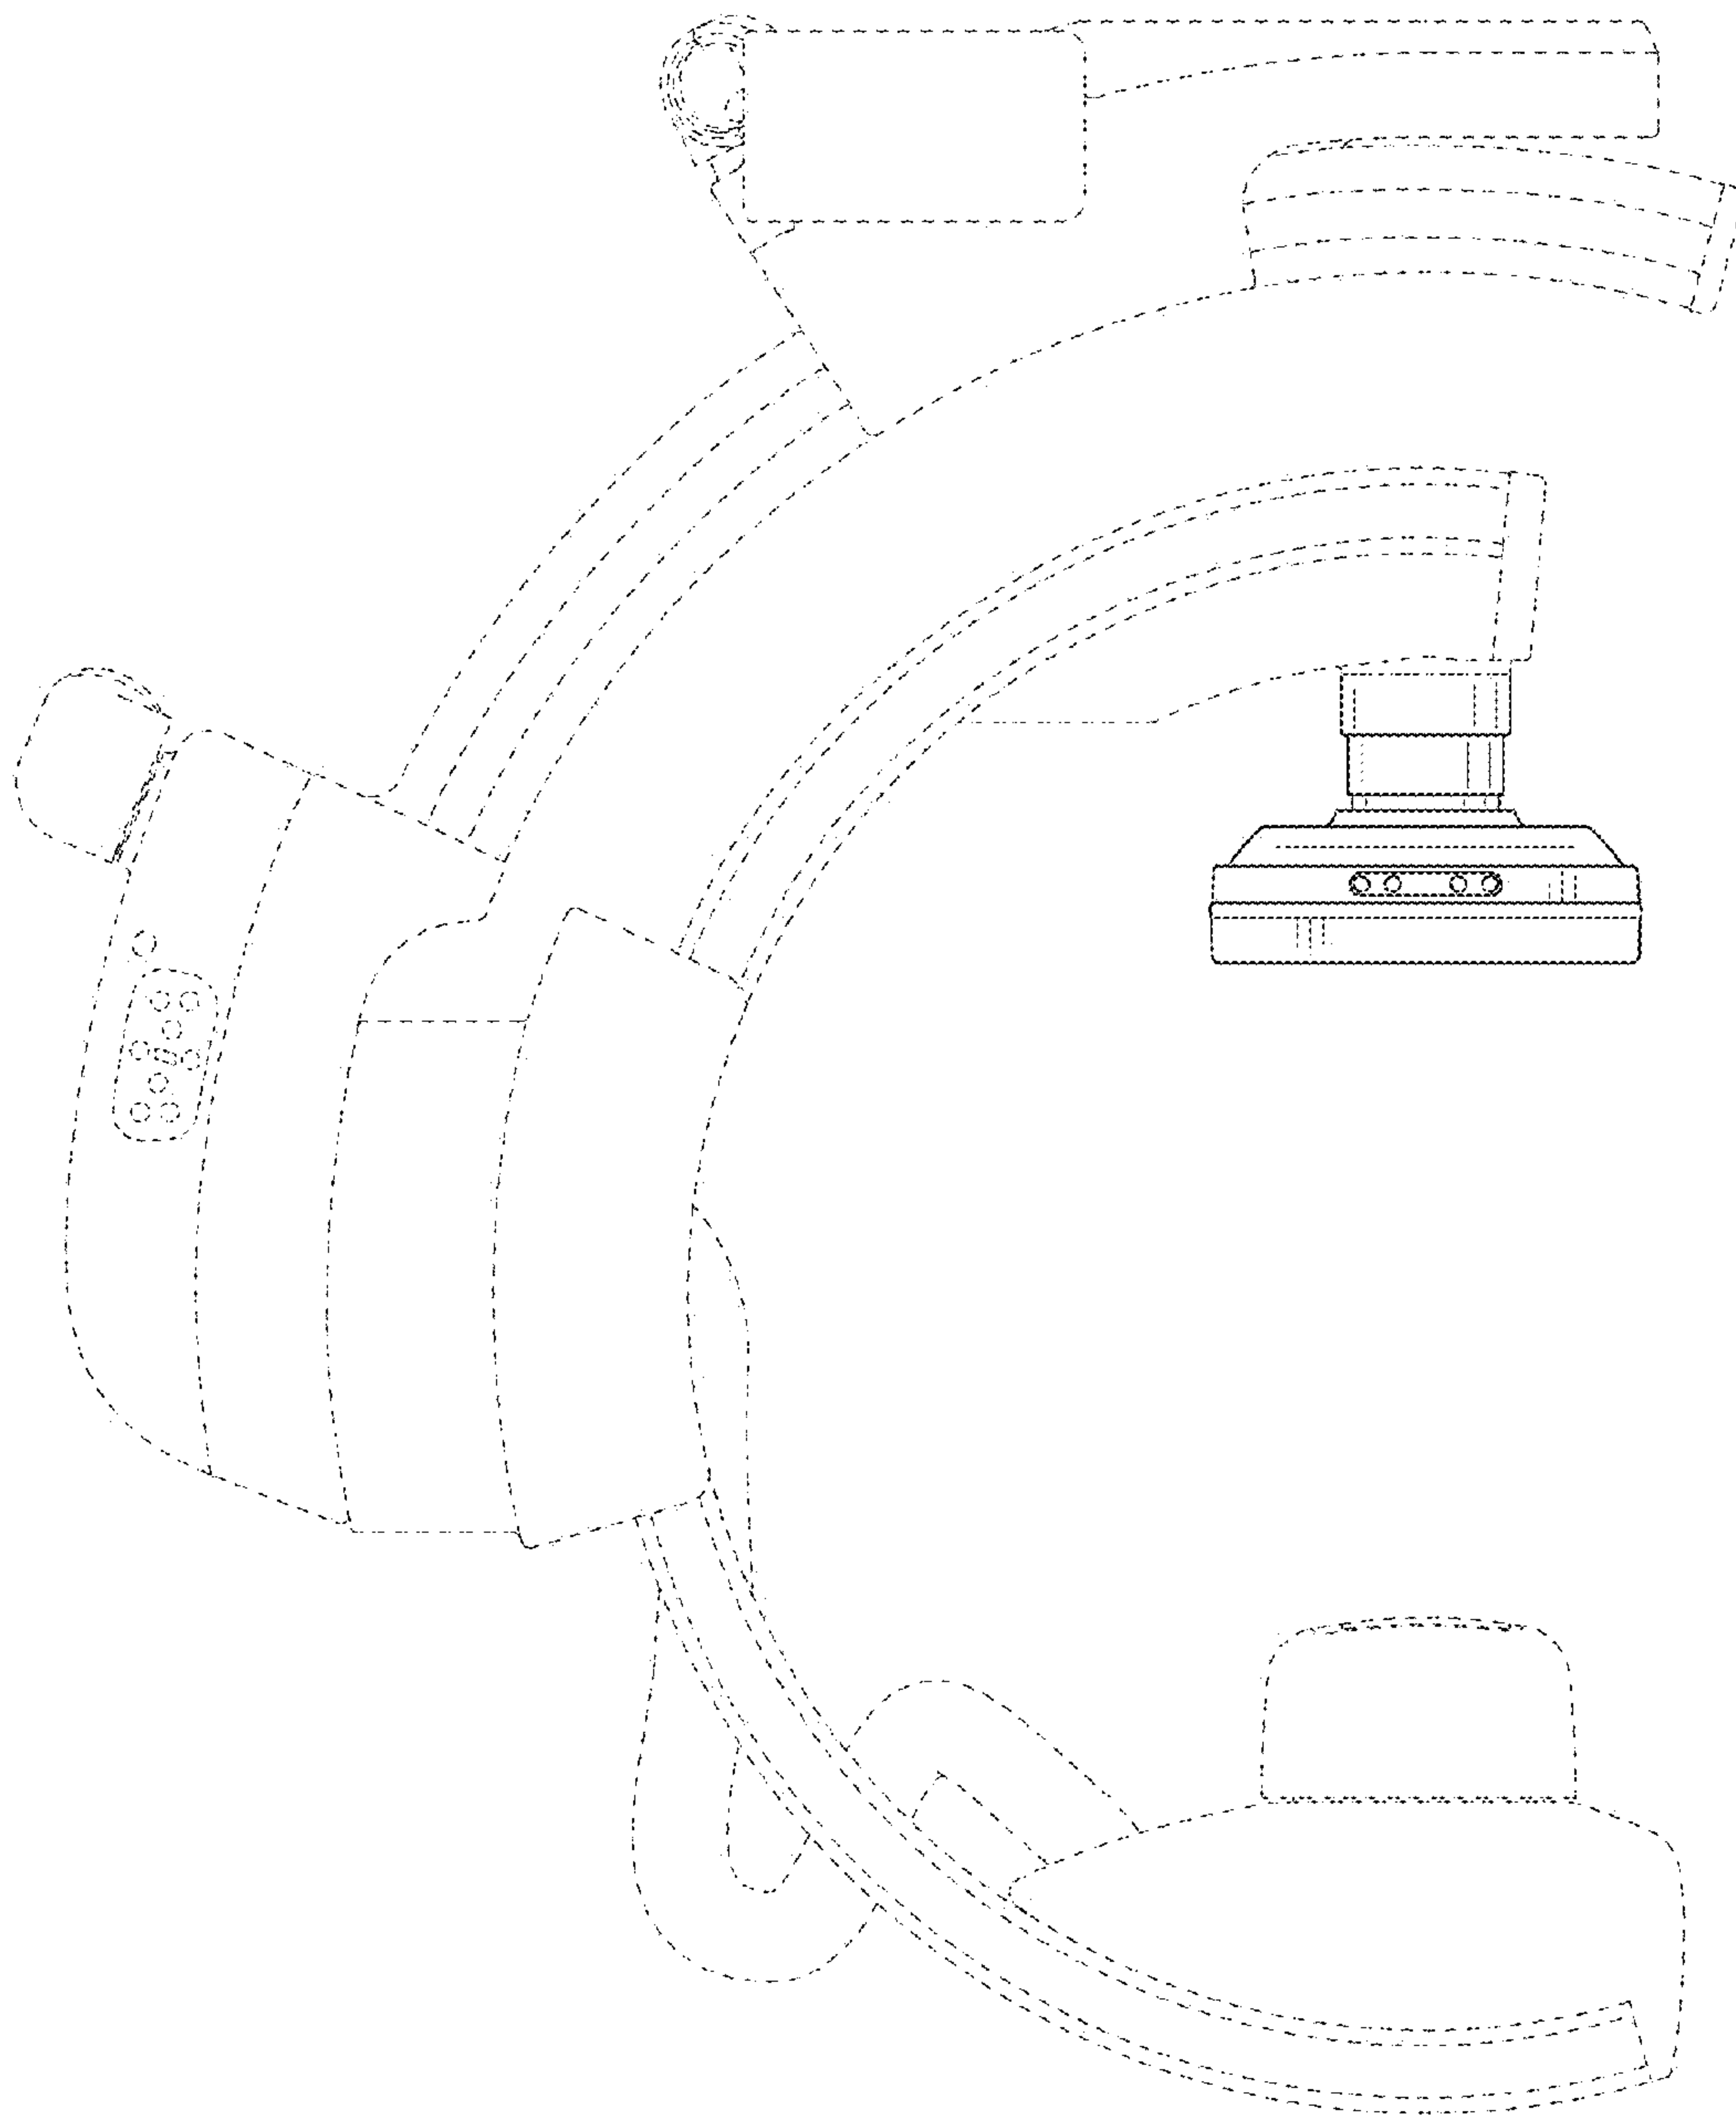


Fig. 12