

US00D751000S

(12) **United States Design Patent**
Dietz et al.

(10) **Patent No.:** **US D751,000 S**
(45) **Date of Patent:** **** Mar. 8, 2016**

(54) **CONTROL PANEL OF A PATIENT
TRANSPORT DEVICE HAVING SURFACE
ORNAMENTATION**

4,155,588 A 5/1979 Danziger
D289,992 S * 5/1987 Schrage D12/132
4,745,647 A * 5/1988 Goodwin 5/713

(Continued)

(71) Applicant: **Ferno-Washington, Inc.**, Wilmington,
OH (US)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Timothy J. Dietz**, Springboro, OH (US);
Michael Jeffries, Maineville, OH (US);
Brian M. Magill, Morrow, OH (US);
Timothy P. Schroeder, Mason, OH
(US); **Timothy R. Wells**, Hillsboro, OH
(US)

CN 102781392 A 11/2012
EP 2412355 A1 2/2012

(Continued)

(73) Assignee: **Ferno-Washington, Inc.**, Wilmington,
OH (US)

OTHER PUBLICATIONS

(**) Term: **14 Years**

Search Report and Written Opinion for International Application No.
PCT/US2013/051271 dated Jan. 15, 2014.

(Continued)

(21) Appl. No.: **29/458,151**

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Charles Hanson

(22) Filed: **Jun. 17, 2013**

(74) *Attorney, Agent, or Firm* — Dinsmore & Shohl LLP

(51) **LOC (10) Cl.** **12-12**

(52) **U.S. Cl.**
USPC **D12/132**; D12/133

(58) **Field of Classification Search**
USPC D12/128–133
CPC A61G 1/04; A61G 1/00; A61G 1/044;
A61G 1/048; A61G 1/0212; A61G 1/003;
A61G 1/0237; A61G 1/0231; A61G 1/0262;
A61G 1/052; A61G 1/0562; A61G 1/0567;
A61G 7/0504; A61G 7/103; A61G 7/1046;
A61G 13/105

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,203,204 A 6/1940 Nicolai
3,631,546 A 1/1972 Eliasson
4,037,871 A 7/1977 Bourgraf et al.

(57) **CLAIM**

The ornamental design for a control panel of a patient trans-
port device having surface ornamentation, as shown and
described.

DESCRIPTION

This application is related to U.S. patent application Ser. Nos.
29/458,150 entitled Legs of a Patient Transport Device Hav-
ing Surface Ornamentation; 29/458/153 entitled Legs and
Frame of a Patient Transport Device; and 29/442,947 entitled
Patient Transport Device, filed concurrently herewith.

FIG. 1 is a right side elevational view of a control panel of a
patient transport device having surface ornamentation show-
ing our new design;

FIG. 2 is a left side elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a front elevational view thereof;

FIG. 5 is a top plan view thereof;


FIG. 6 is a bottom plan view thereof;

FIG. 7 is a left side perspective view thereof;

FIG. 8 is a bottom isometric view thereof; and,

FIG. 9 is a partially enlarged top plan view of FIG. 5 thereof.

1 Claim, 8 Drawing Sheets

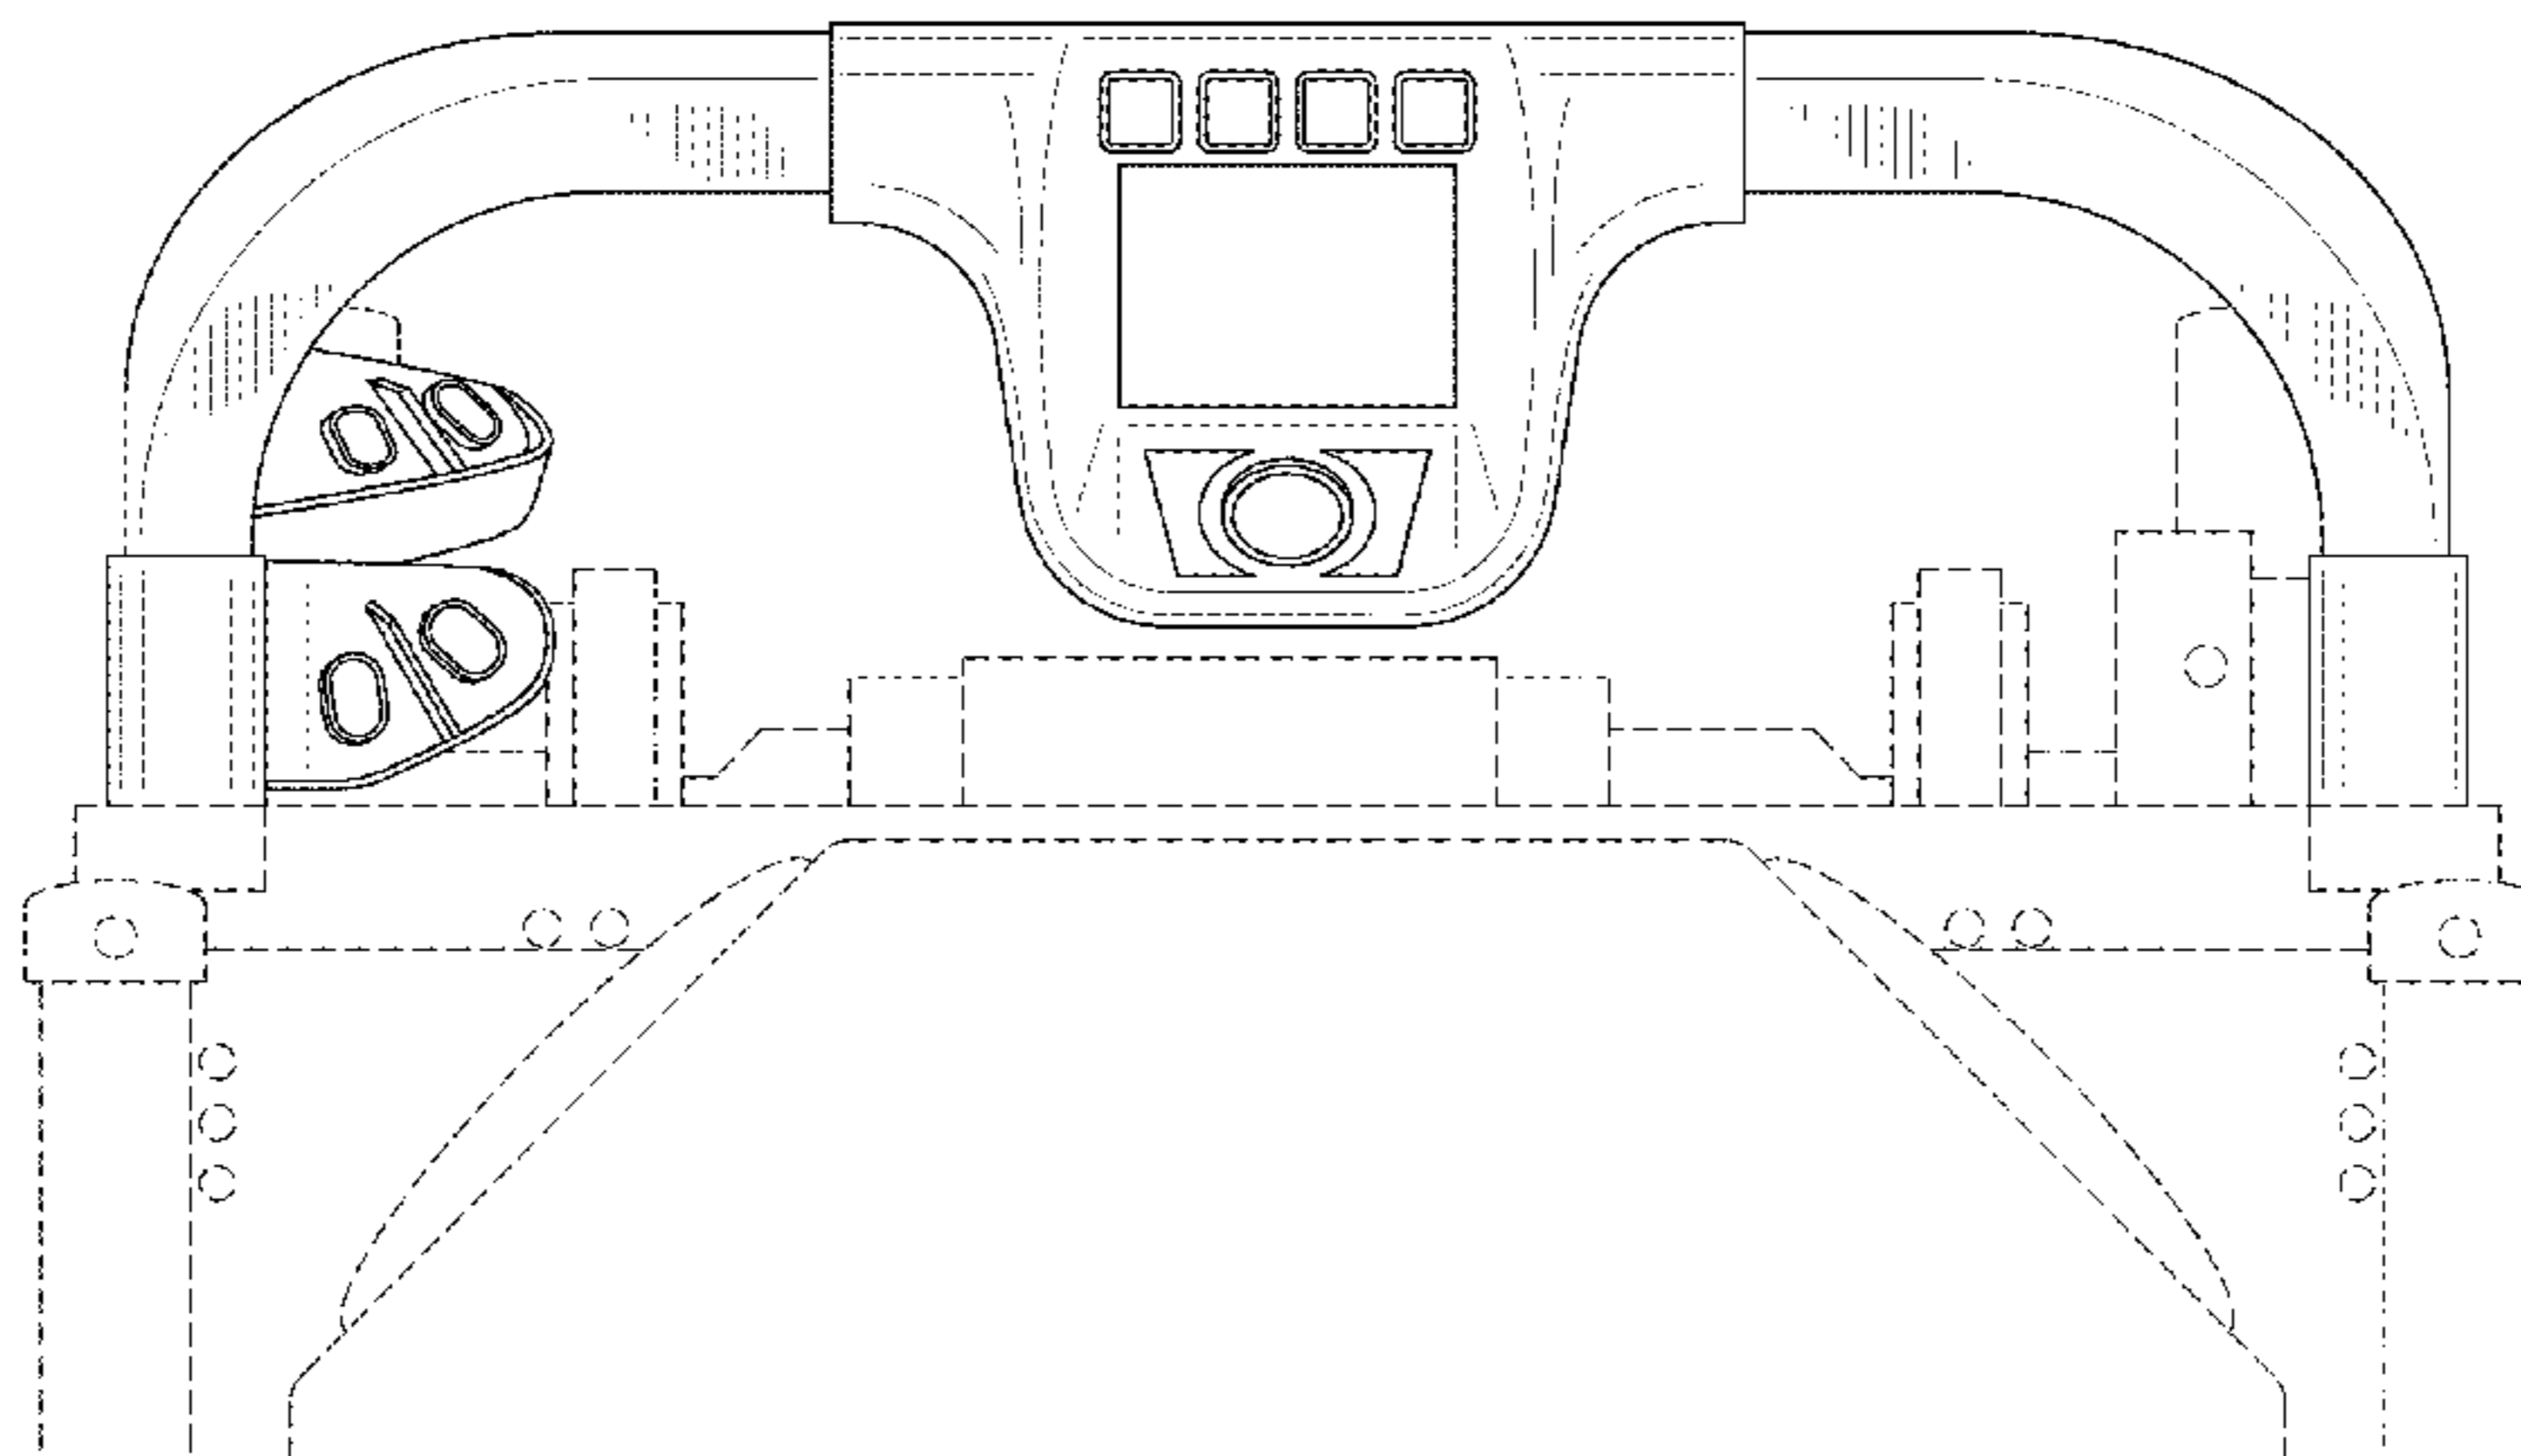

(56)

References Cited

U.S. PATENT DOCUMENTS

4,761,841 A * 8/1988 Larsen 5/81.1 C
 4,921,295 A 5/1990 Stollenwerk
 5,023,968 A * 6/1991 Diehl et al. 5/81.1 R
 5,088,136 A 2/1992 Stryker et al.
 5,431,087 A 7/1995 Kambara
 5,509,159 A 4/1996 Du Boise
 5,586,346 A * 12/1996 Stacy et al. 5/710
 5,720,057 A 2/1998 Duncan
 5,839,136 A 11/1998 Vance et al.
 6,311,952 B2 11/2001 Bainter
 D454,319 S * 3/2002 Ito D12/131
 6,654,973 B2 * 12/2003 Van Den Heuvel et al. 5/611
 6,976,696 B2 12/2005 O'Krangley et al.
 7,013,510 B1 3/2006 Johnson
 7,621,003 B2 * 11/2009 Myers et al. 5/86.1
 D606,910 S * 12/2009 Malassigne et al. D12/132
 7,631,373 B2 12/2009 Broadley et al.
 7,641,211 B2 1/2010 Ivanchenko
 7,841,611 B2 11/2010 Ivanchenko
 7,941,881 B2 5/2011 Hayes et al.
 7,996,939 B2 * 8/2011 Benedict et al. 5/611
 8,051,513 B2 * 11/2011 Reed et al. 5/627
 8,056,950 B2 * 11/2011 Souke et al. 296/20
 8,100,307 B2 * 1/2012 Chinn et al. 224/407
 8,240,410 B2 * 8/2012 Heimbrock et al. 180/65.1
 RE44,884 E * 5/2014 Lambarth 5/611
 8,714,612 B2 * 5/2014 Chinn 296/20
 2002/0056162 A1 5/2002 Flynn et al.
 2002/0174486 A1 * 11/2002 Heuvel et al. 5/611
 2004/0088792 A1 5/2004 O'Krangley et al.
 2006/0075558 A1 4/2006 Lambarth et al.
 2006/0082176 A1 4/2006 Broadley et al.
 2006/0096029 A1 5/2006 Osborne et al.
 2006/0265807 A1 11/2006 Choy et al.
 2007/0163044 A1 7/2007 Arnold et al.
 2008/0128571 A1 6/2008 Dostaler et al.
 2009/0165208 A1 7/2009 Reed et al.
 2009/0172883 A1 7/2009 Benedict et al.
 2009/0313758 A1 12/2009 Menkedick et al.
 2010/0306921 A1 * 12/2010 Kramer 5/618
 2011/0266821 A1 * 11/2011 Goto et al. 296/20

2012/0275896 A1 * 11/2012 Magill et al. 414/800
 2014/0059768 A1 * 3/2014 Lemire et al. 5/611
 2014/0276269 A1 * 9/2014 Illindala 601/41

FOREIGN PATENT DOCUMENTS

GB 2351439 A 1/2001
 JP 02-200262 8/1990
 WO 2011088169 A1 7/2011

OTHER PUBLICATIONS

Preliminary Rejection dated Sep. 2, 2014 pertaining to Korean Design Application No. 30-2013-0063154.
 Preliminary Rejection dated Sep. 2, 2014 pertaining to Korean Design Application No. 30-2013-0063155.
 Preliminary Rejection dated Sep. 2, 2014 pertaining to Korean Design Application No. 30-2013-0063157.
 Australian Examination Report for Registration No. 353436 dated Jul. 30, 2014.
 Office Action pertaining to U.S. Appl. No. 29/442,947 dated Oct. 1, 2014.
 Examination Report corresponding to Japanese Patent Application No. 2012-549057, dated Oct. 28, 2014.
 Chinese first Office Action pertaining to Chinese Patent Application No. 201180011448.8, dated Aug. 14, 2014.
 Search Report and Written Opinion for International Application No. PCT/US11/21069 dated May 25, 2011.
 Election/Restriction Requirement dated Nov. 3, 2014 pertaining to U.S. Appl. No. 13/520,627.
 Examiner's Report, dated May 13, 2014 pertaining to Canadian Design Patent application 154348.
 Examiner's Report, dated May 13, 2014 pertaining to Canadian Design Patent application 154349.
 Examiner's Report, dated May 13, 2014 pertaining to Canadian Design Patent application 154350.
 Examiner's Report, dated May 13, 2014 pertaining to Canadian Design Patent application 154351.
 International Search Report and Written Opinion, dated Apr. 28, 2014 pertaining to PCT/US2013/073005.

* cited by examiner

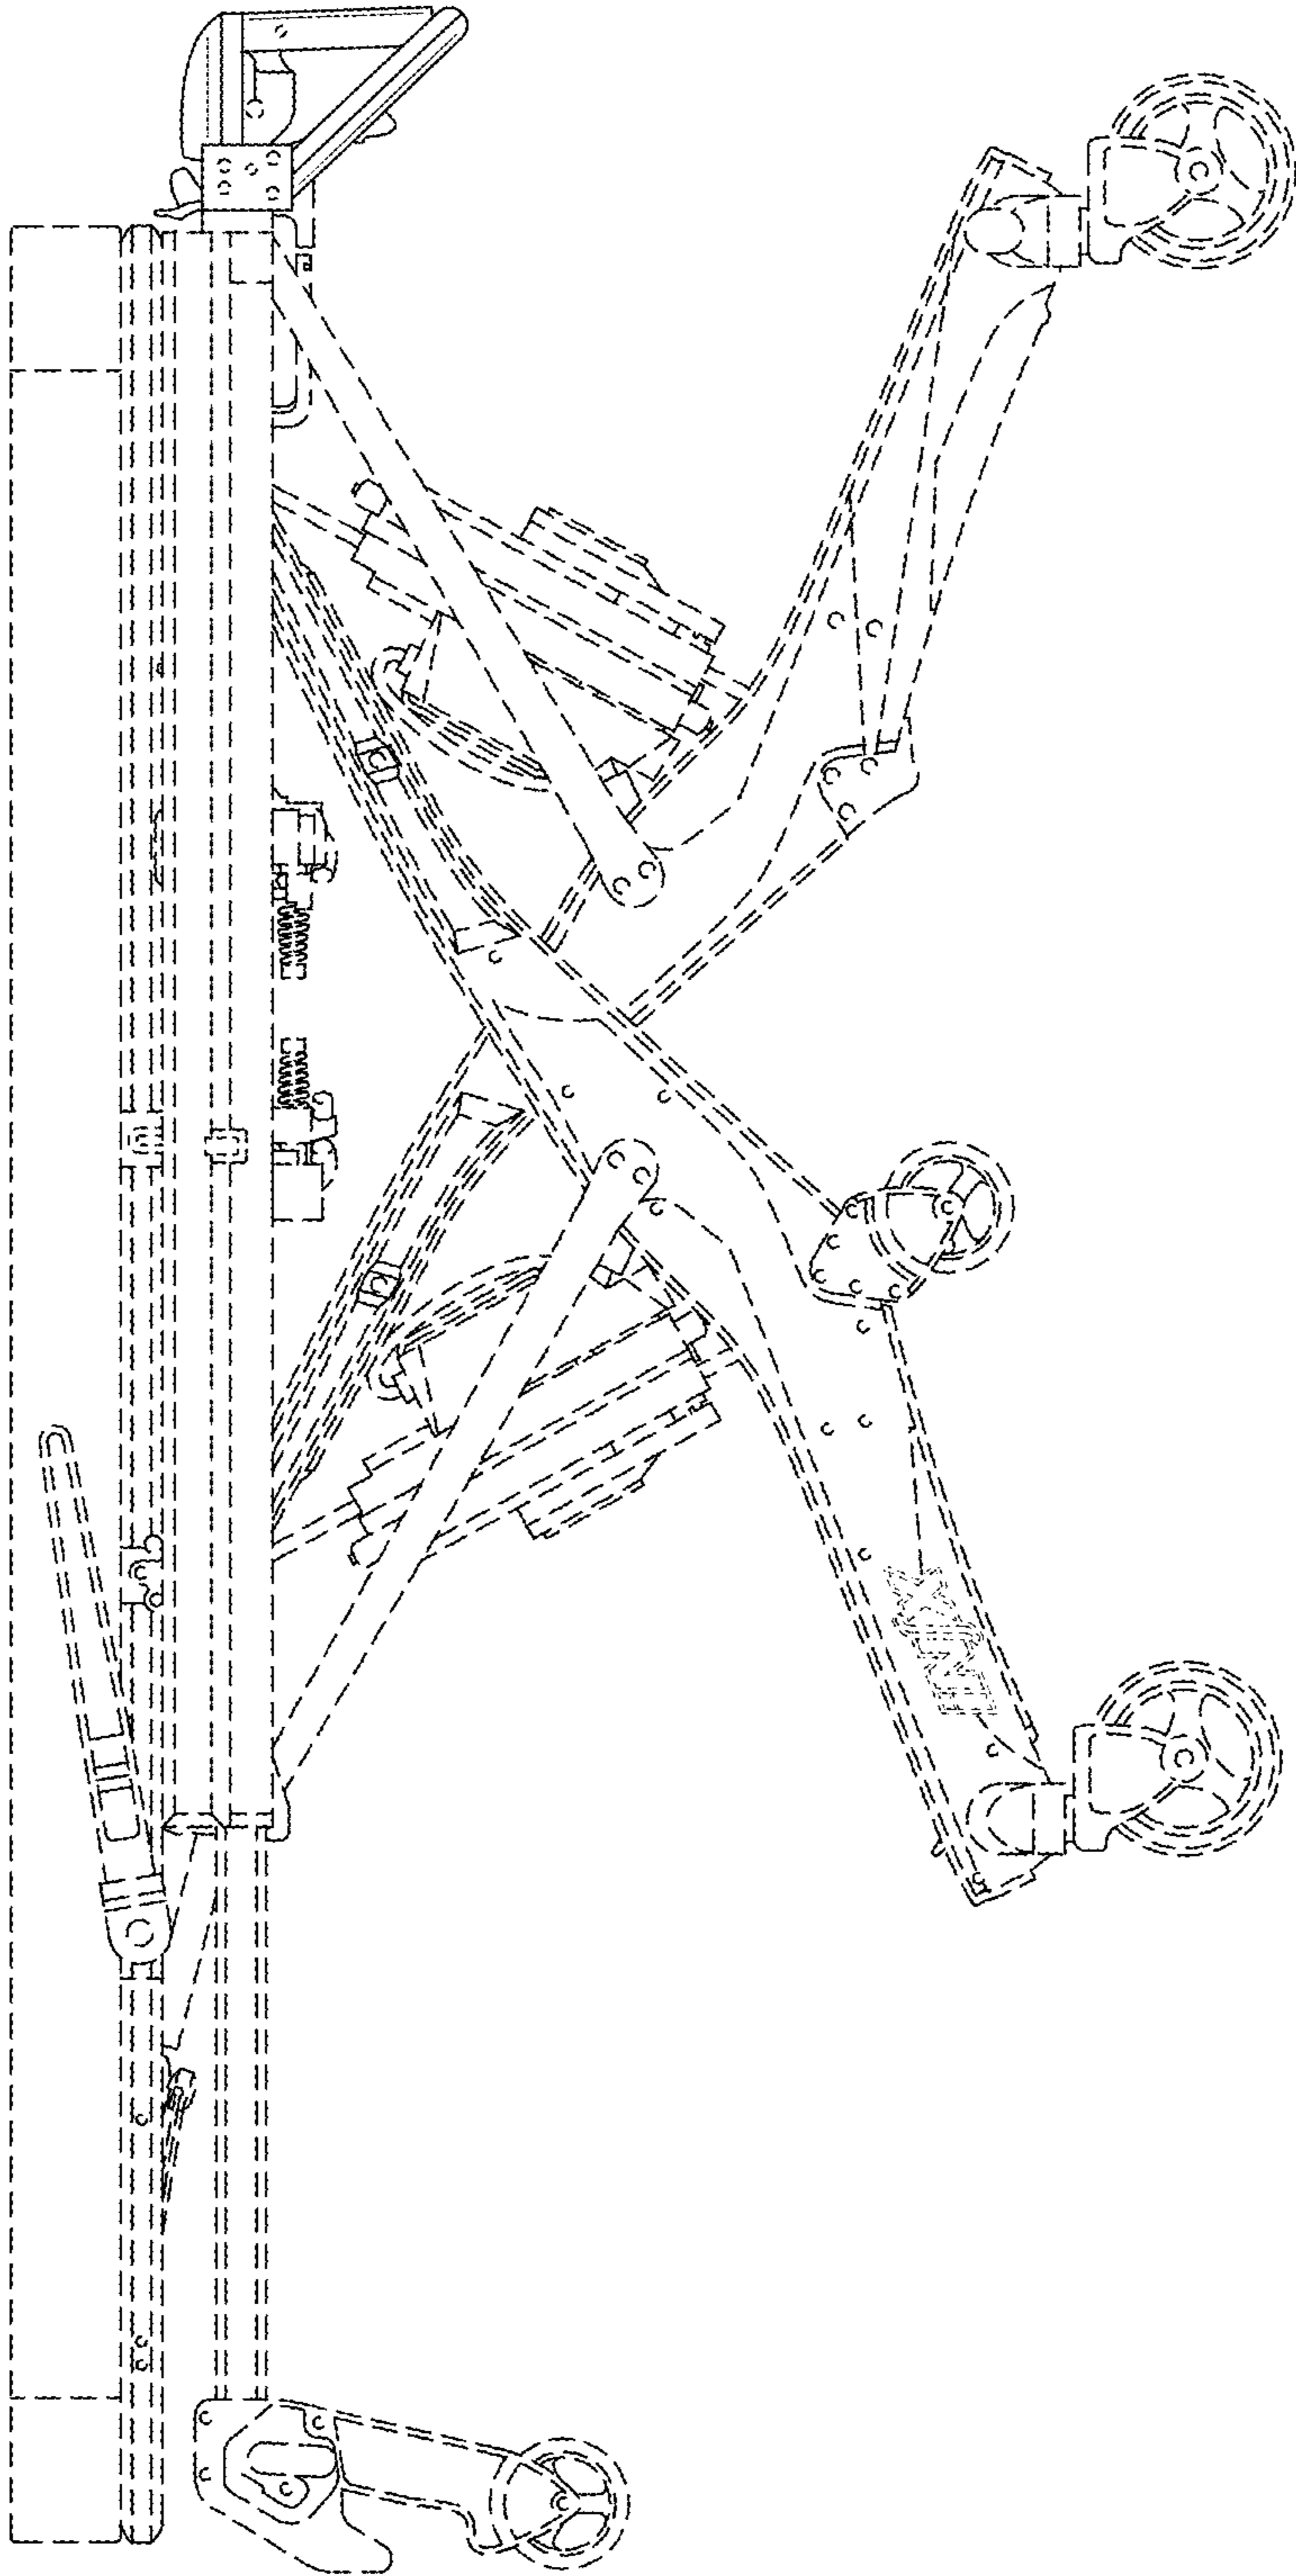


FIG. 1

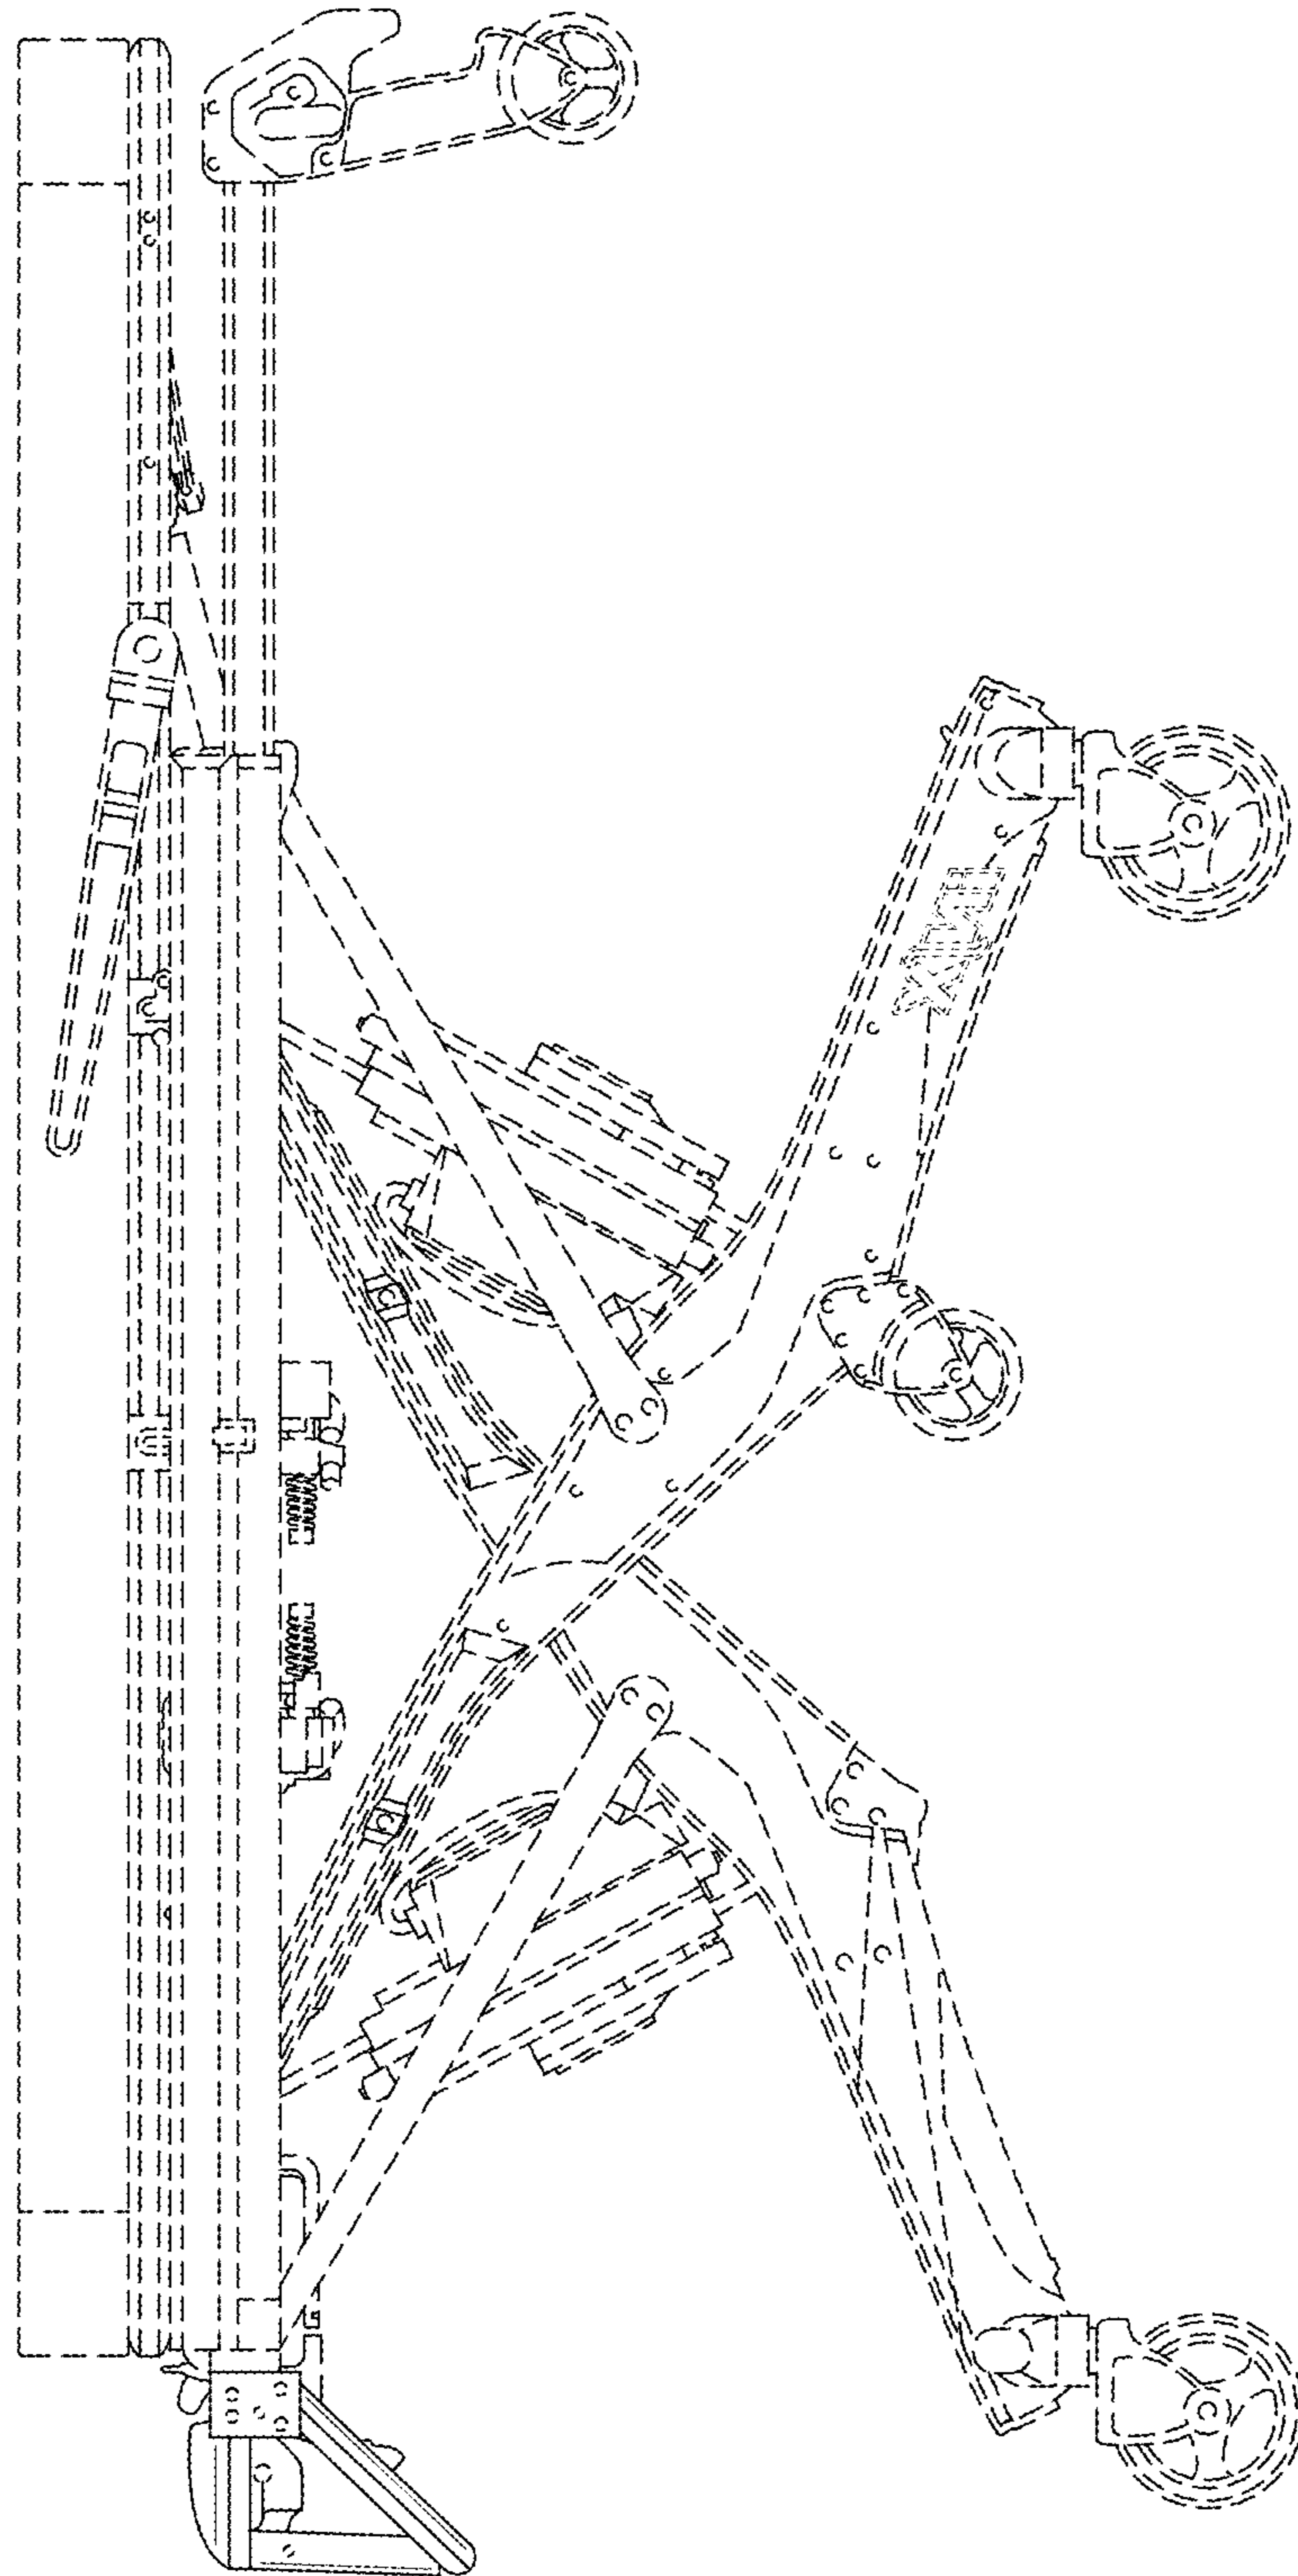


FIG. 2

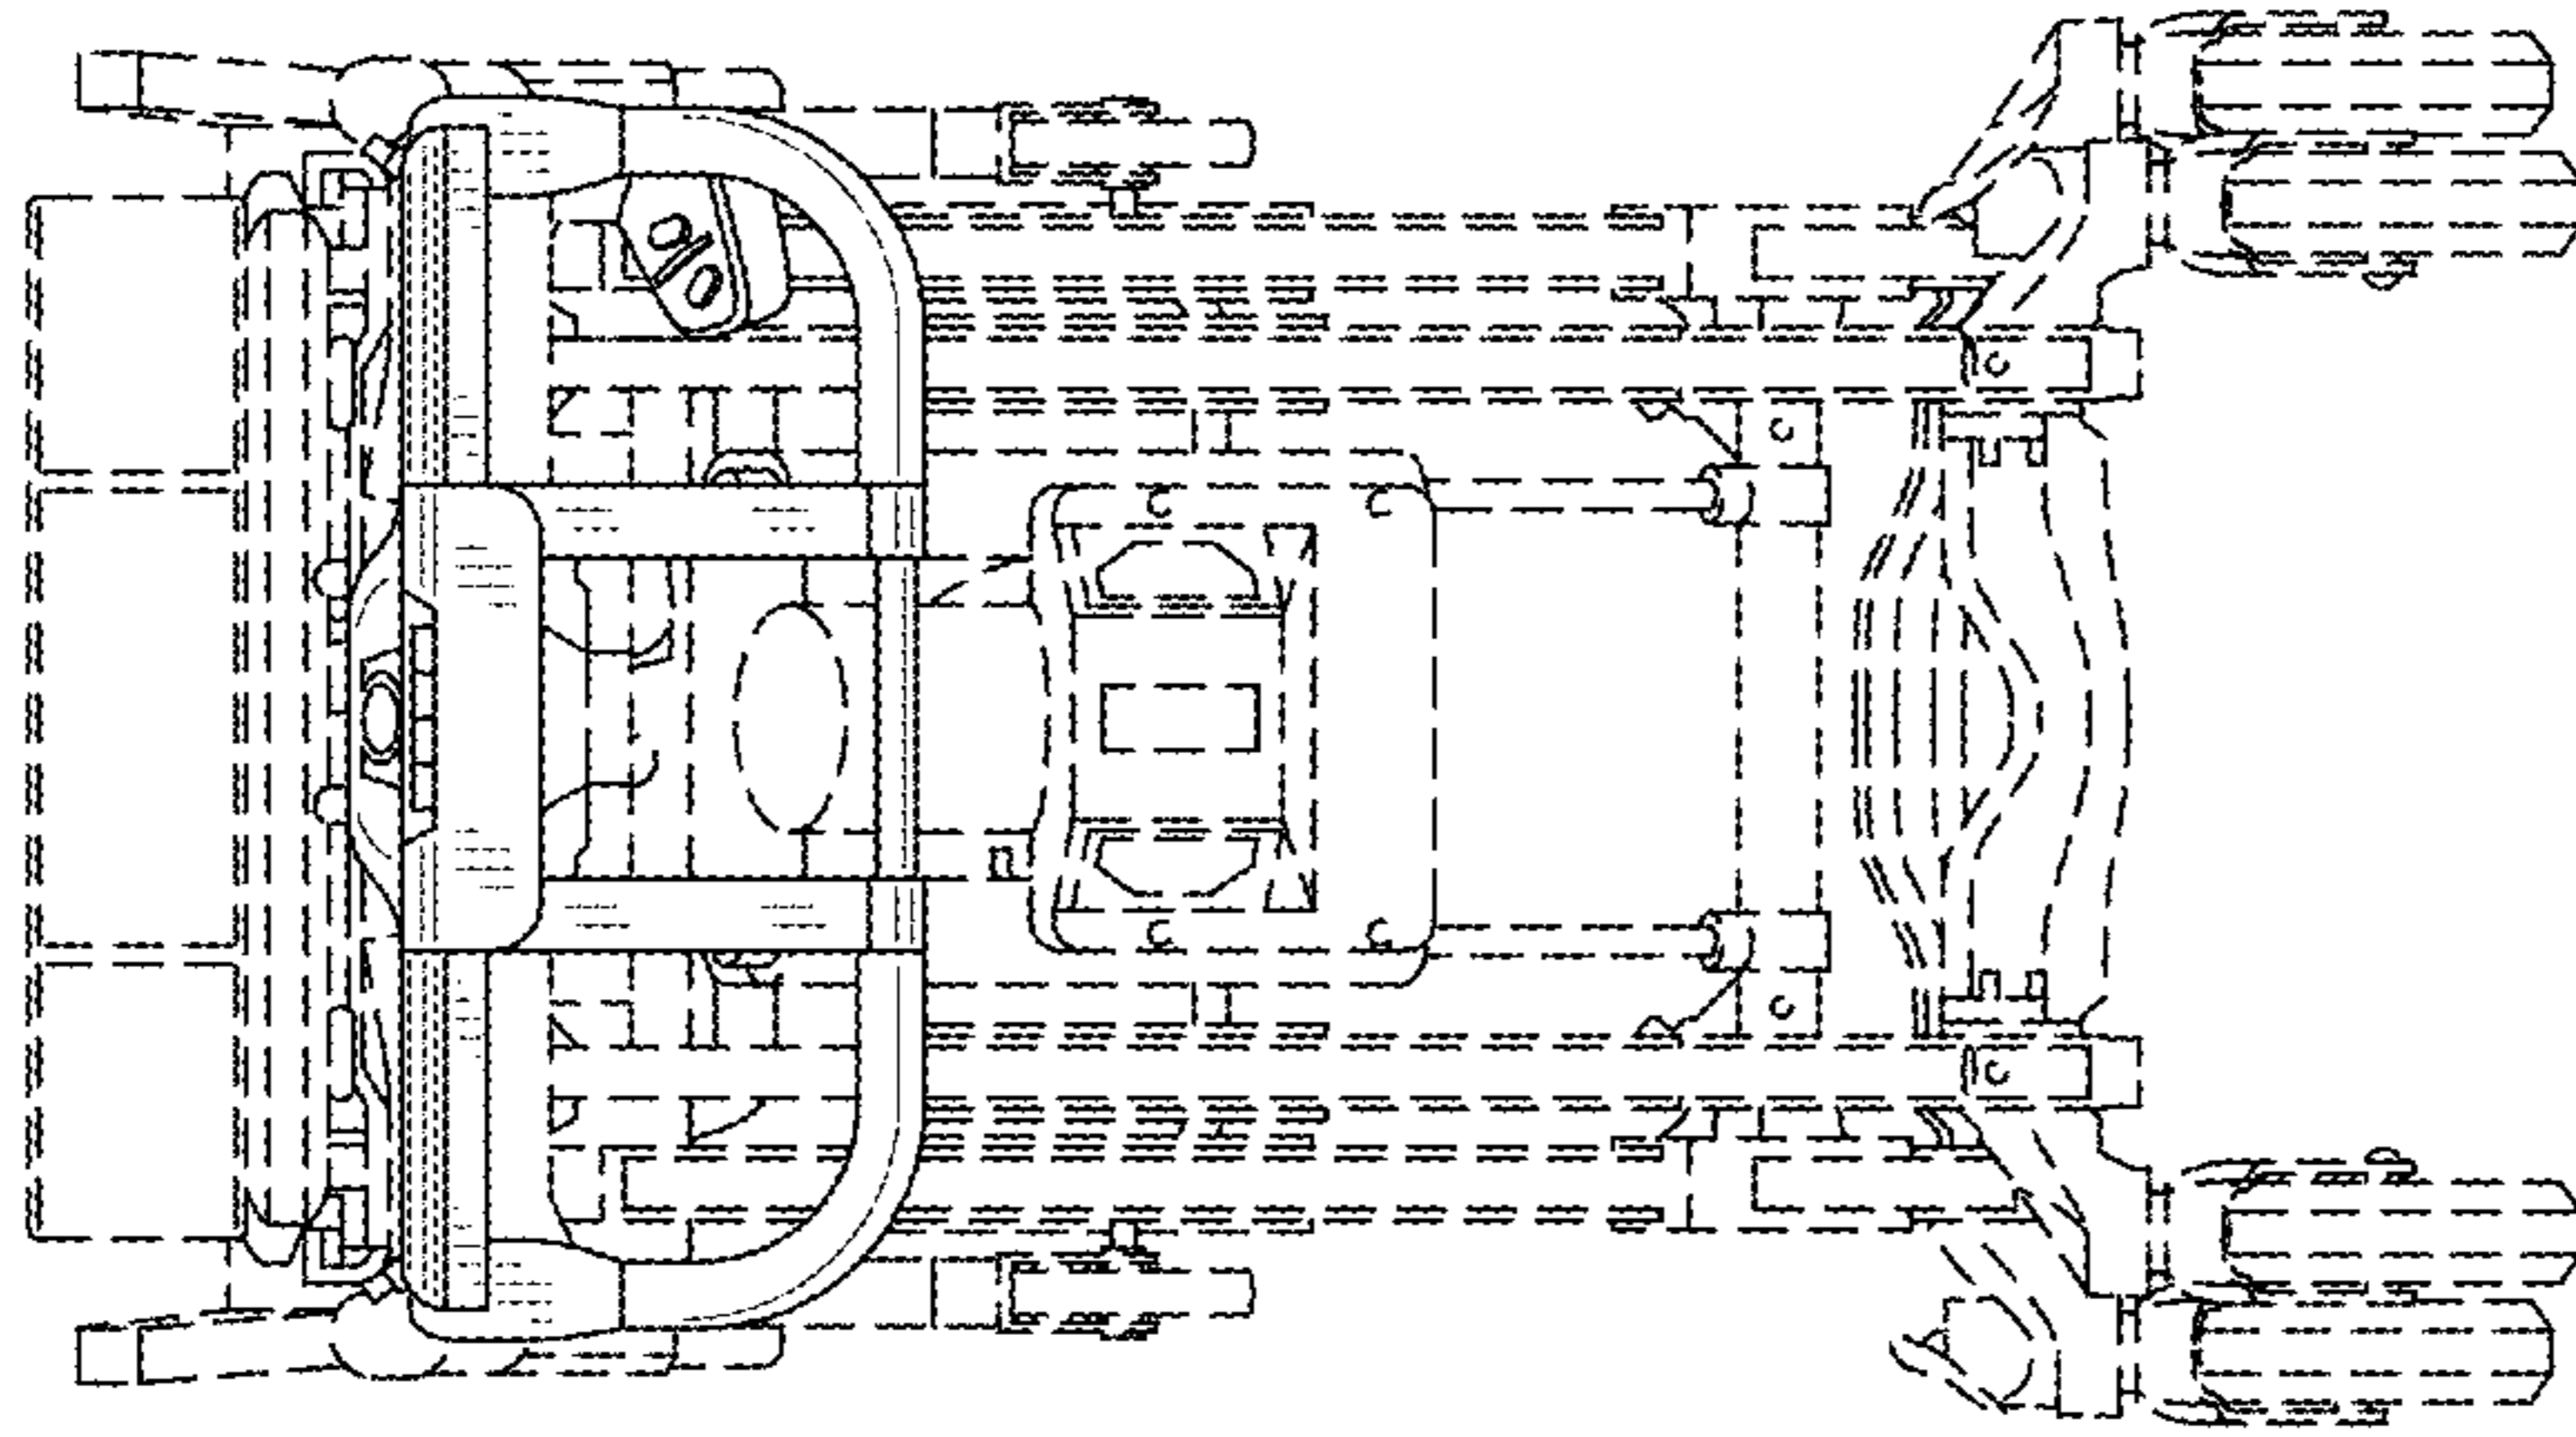


FIG. 4

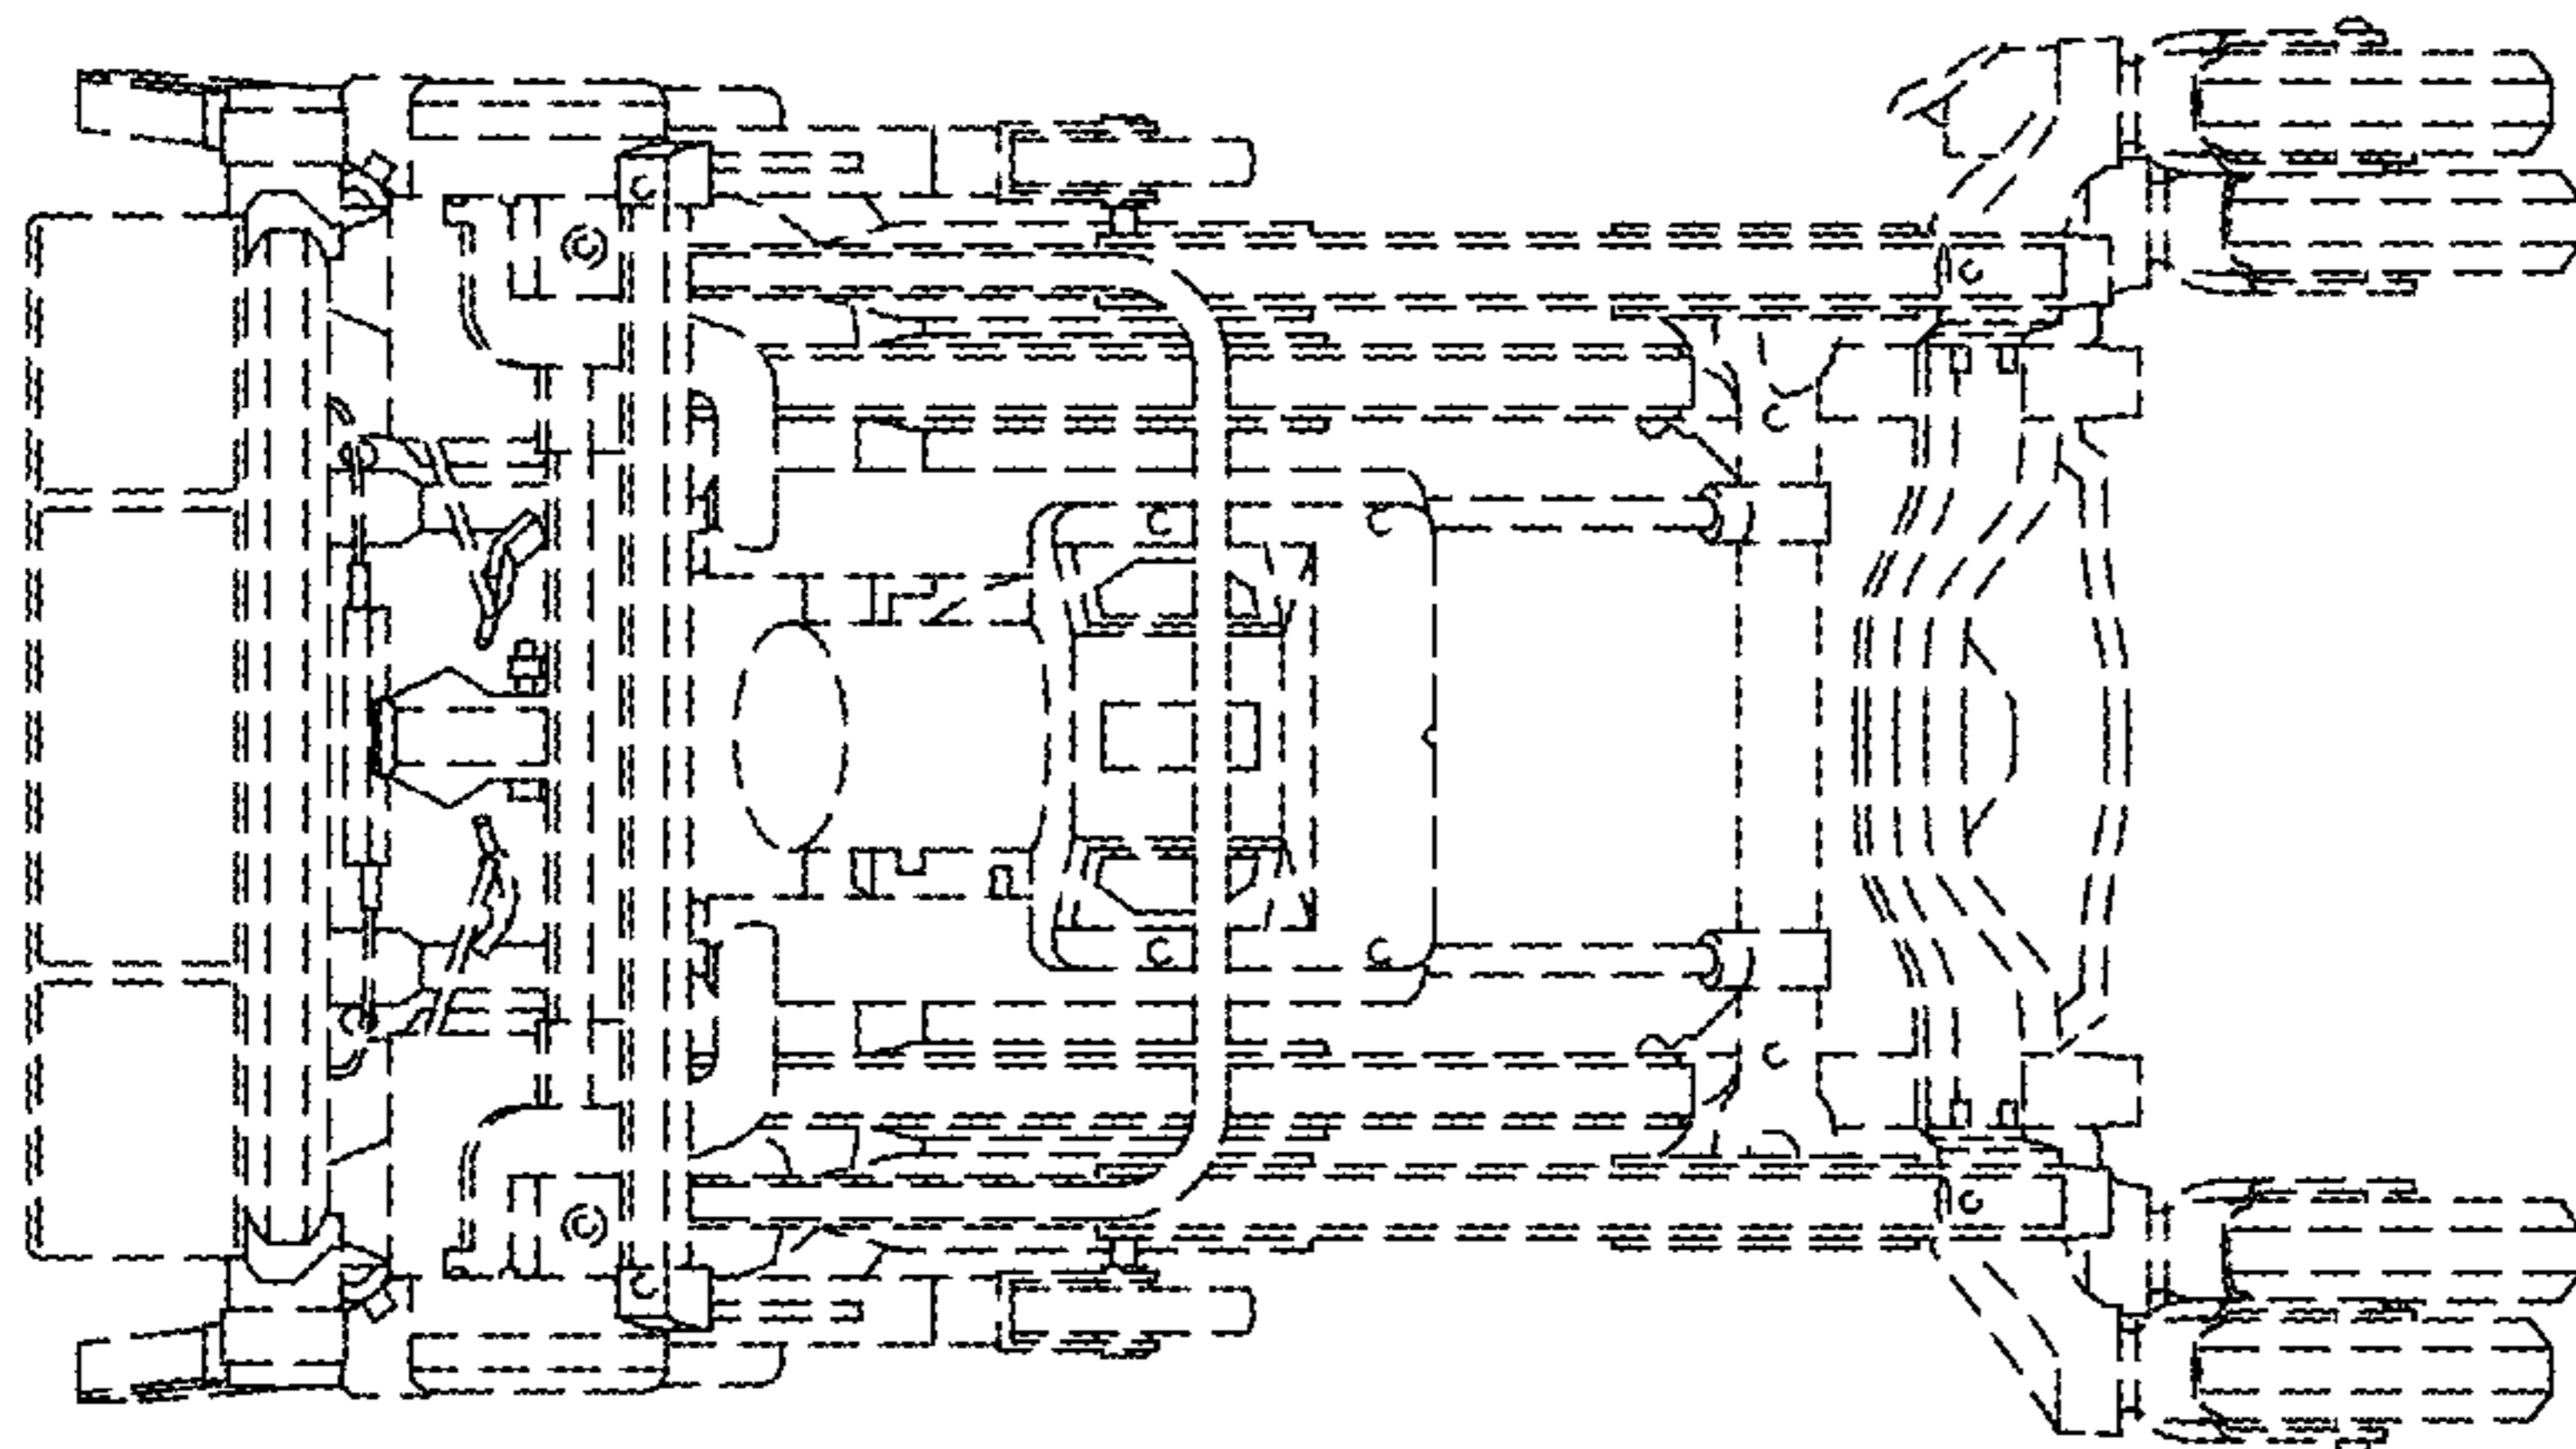


FIG. 3

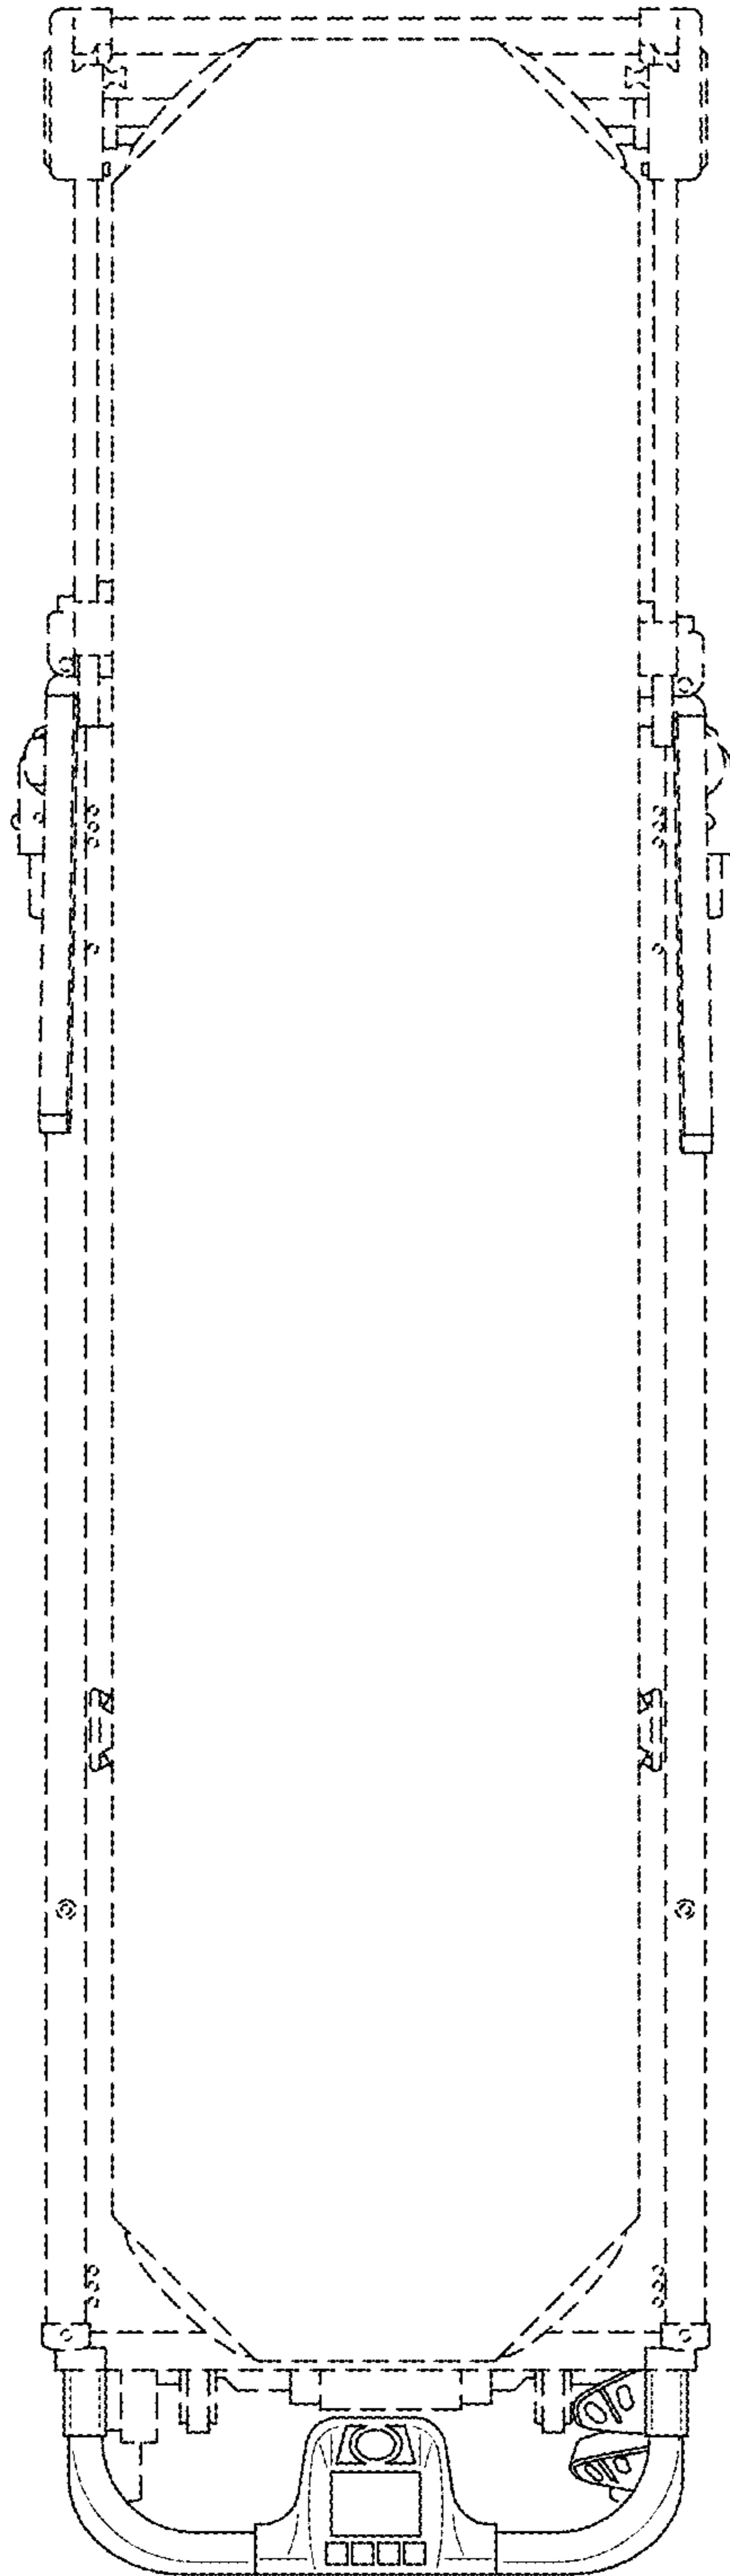


FIG. 5

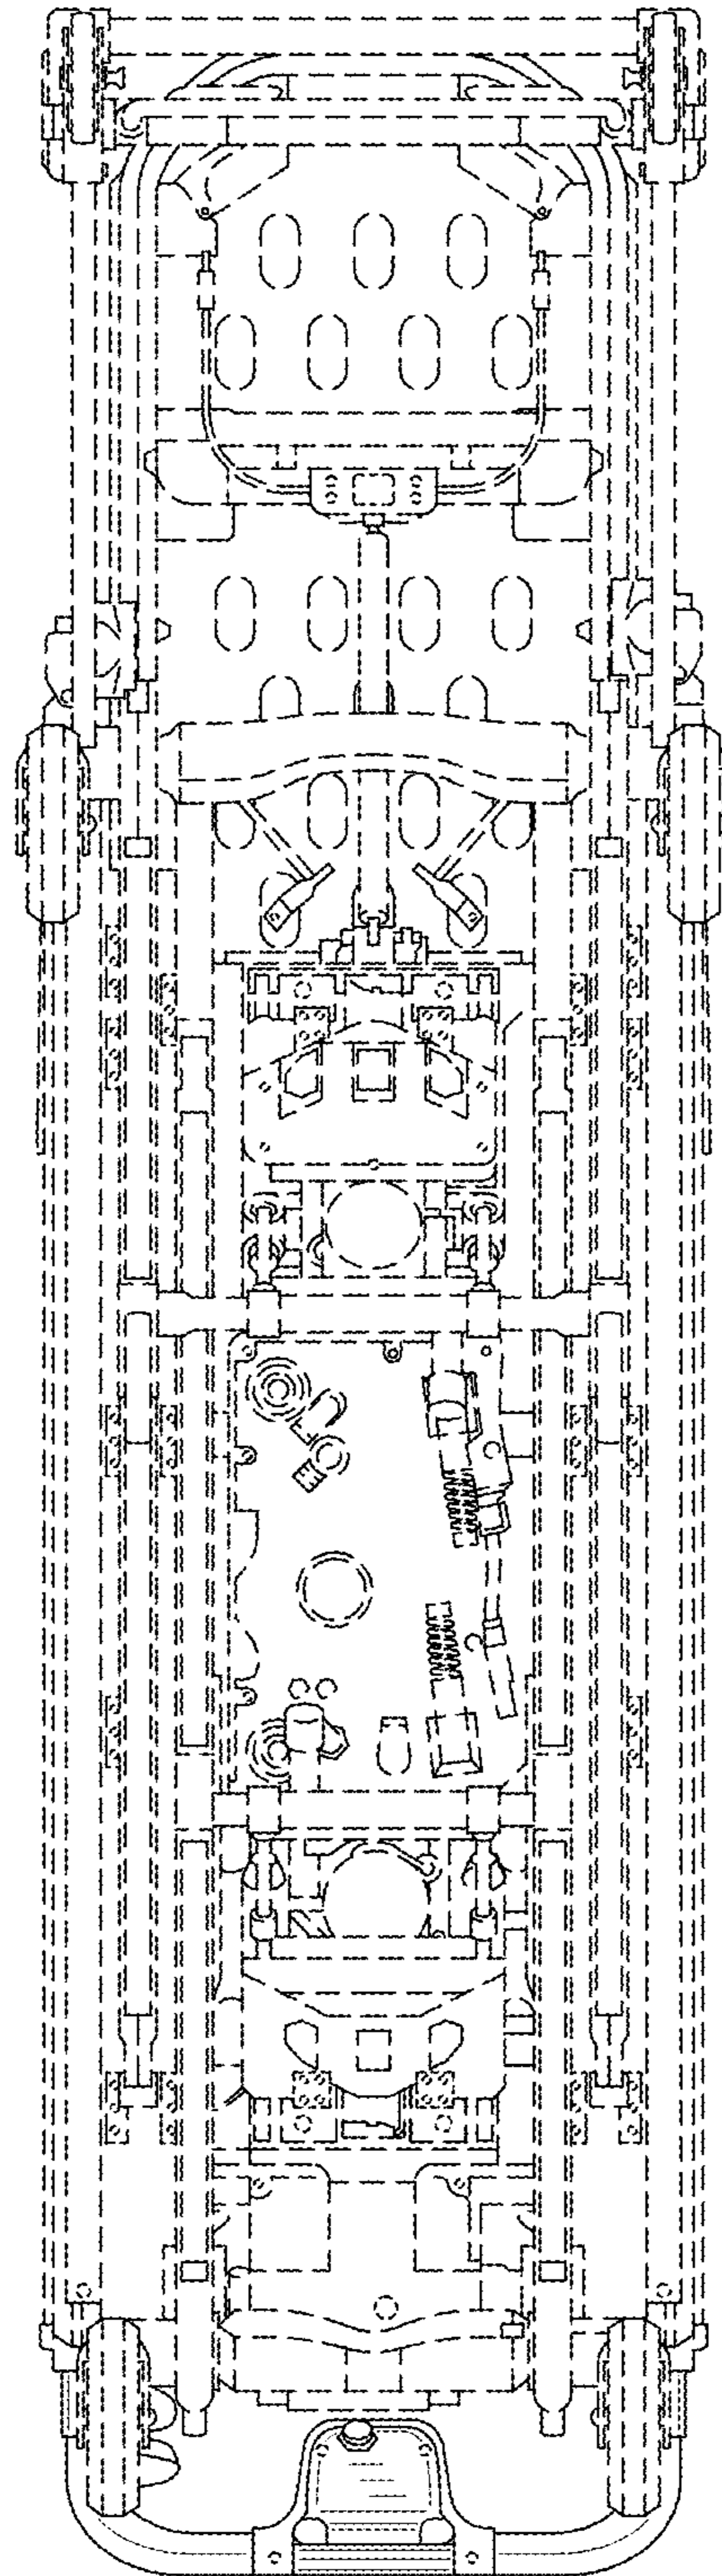


FIG. 6

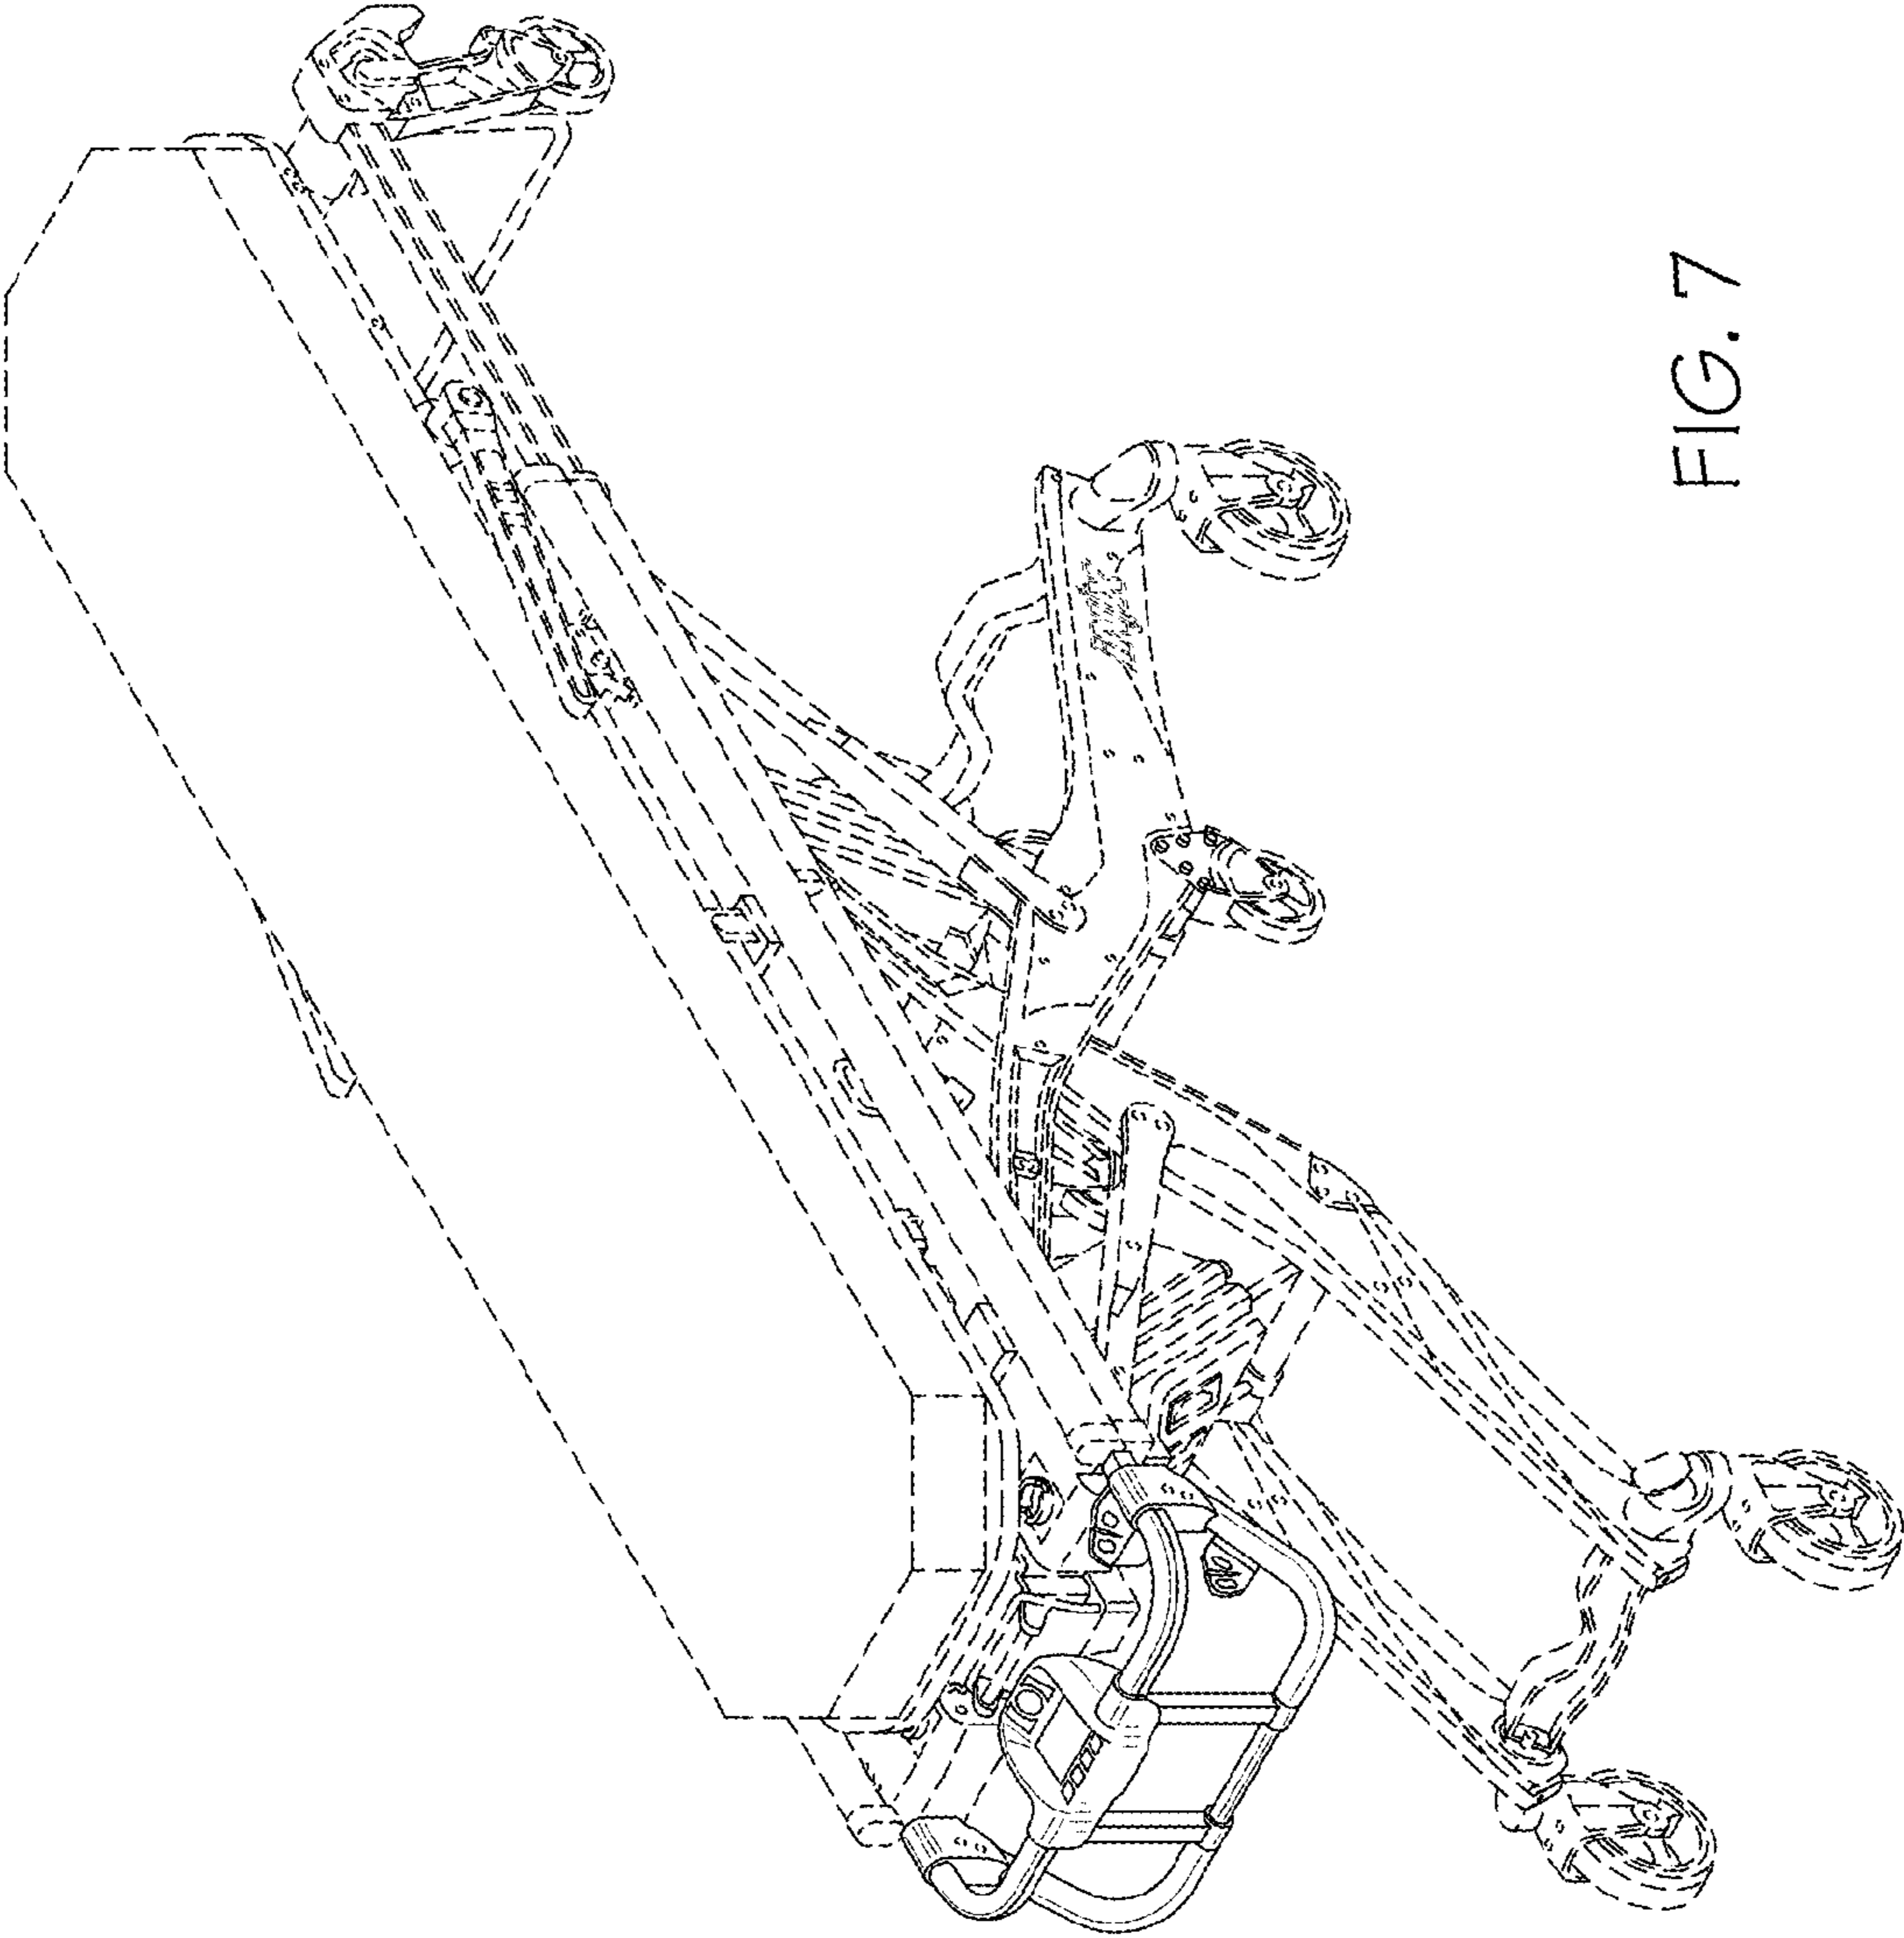


FIG. 7

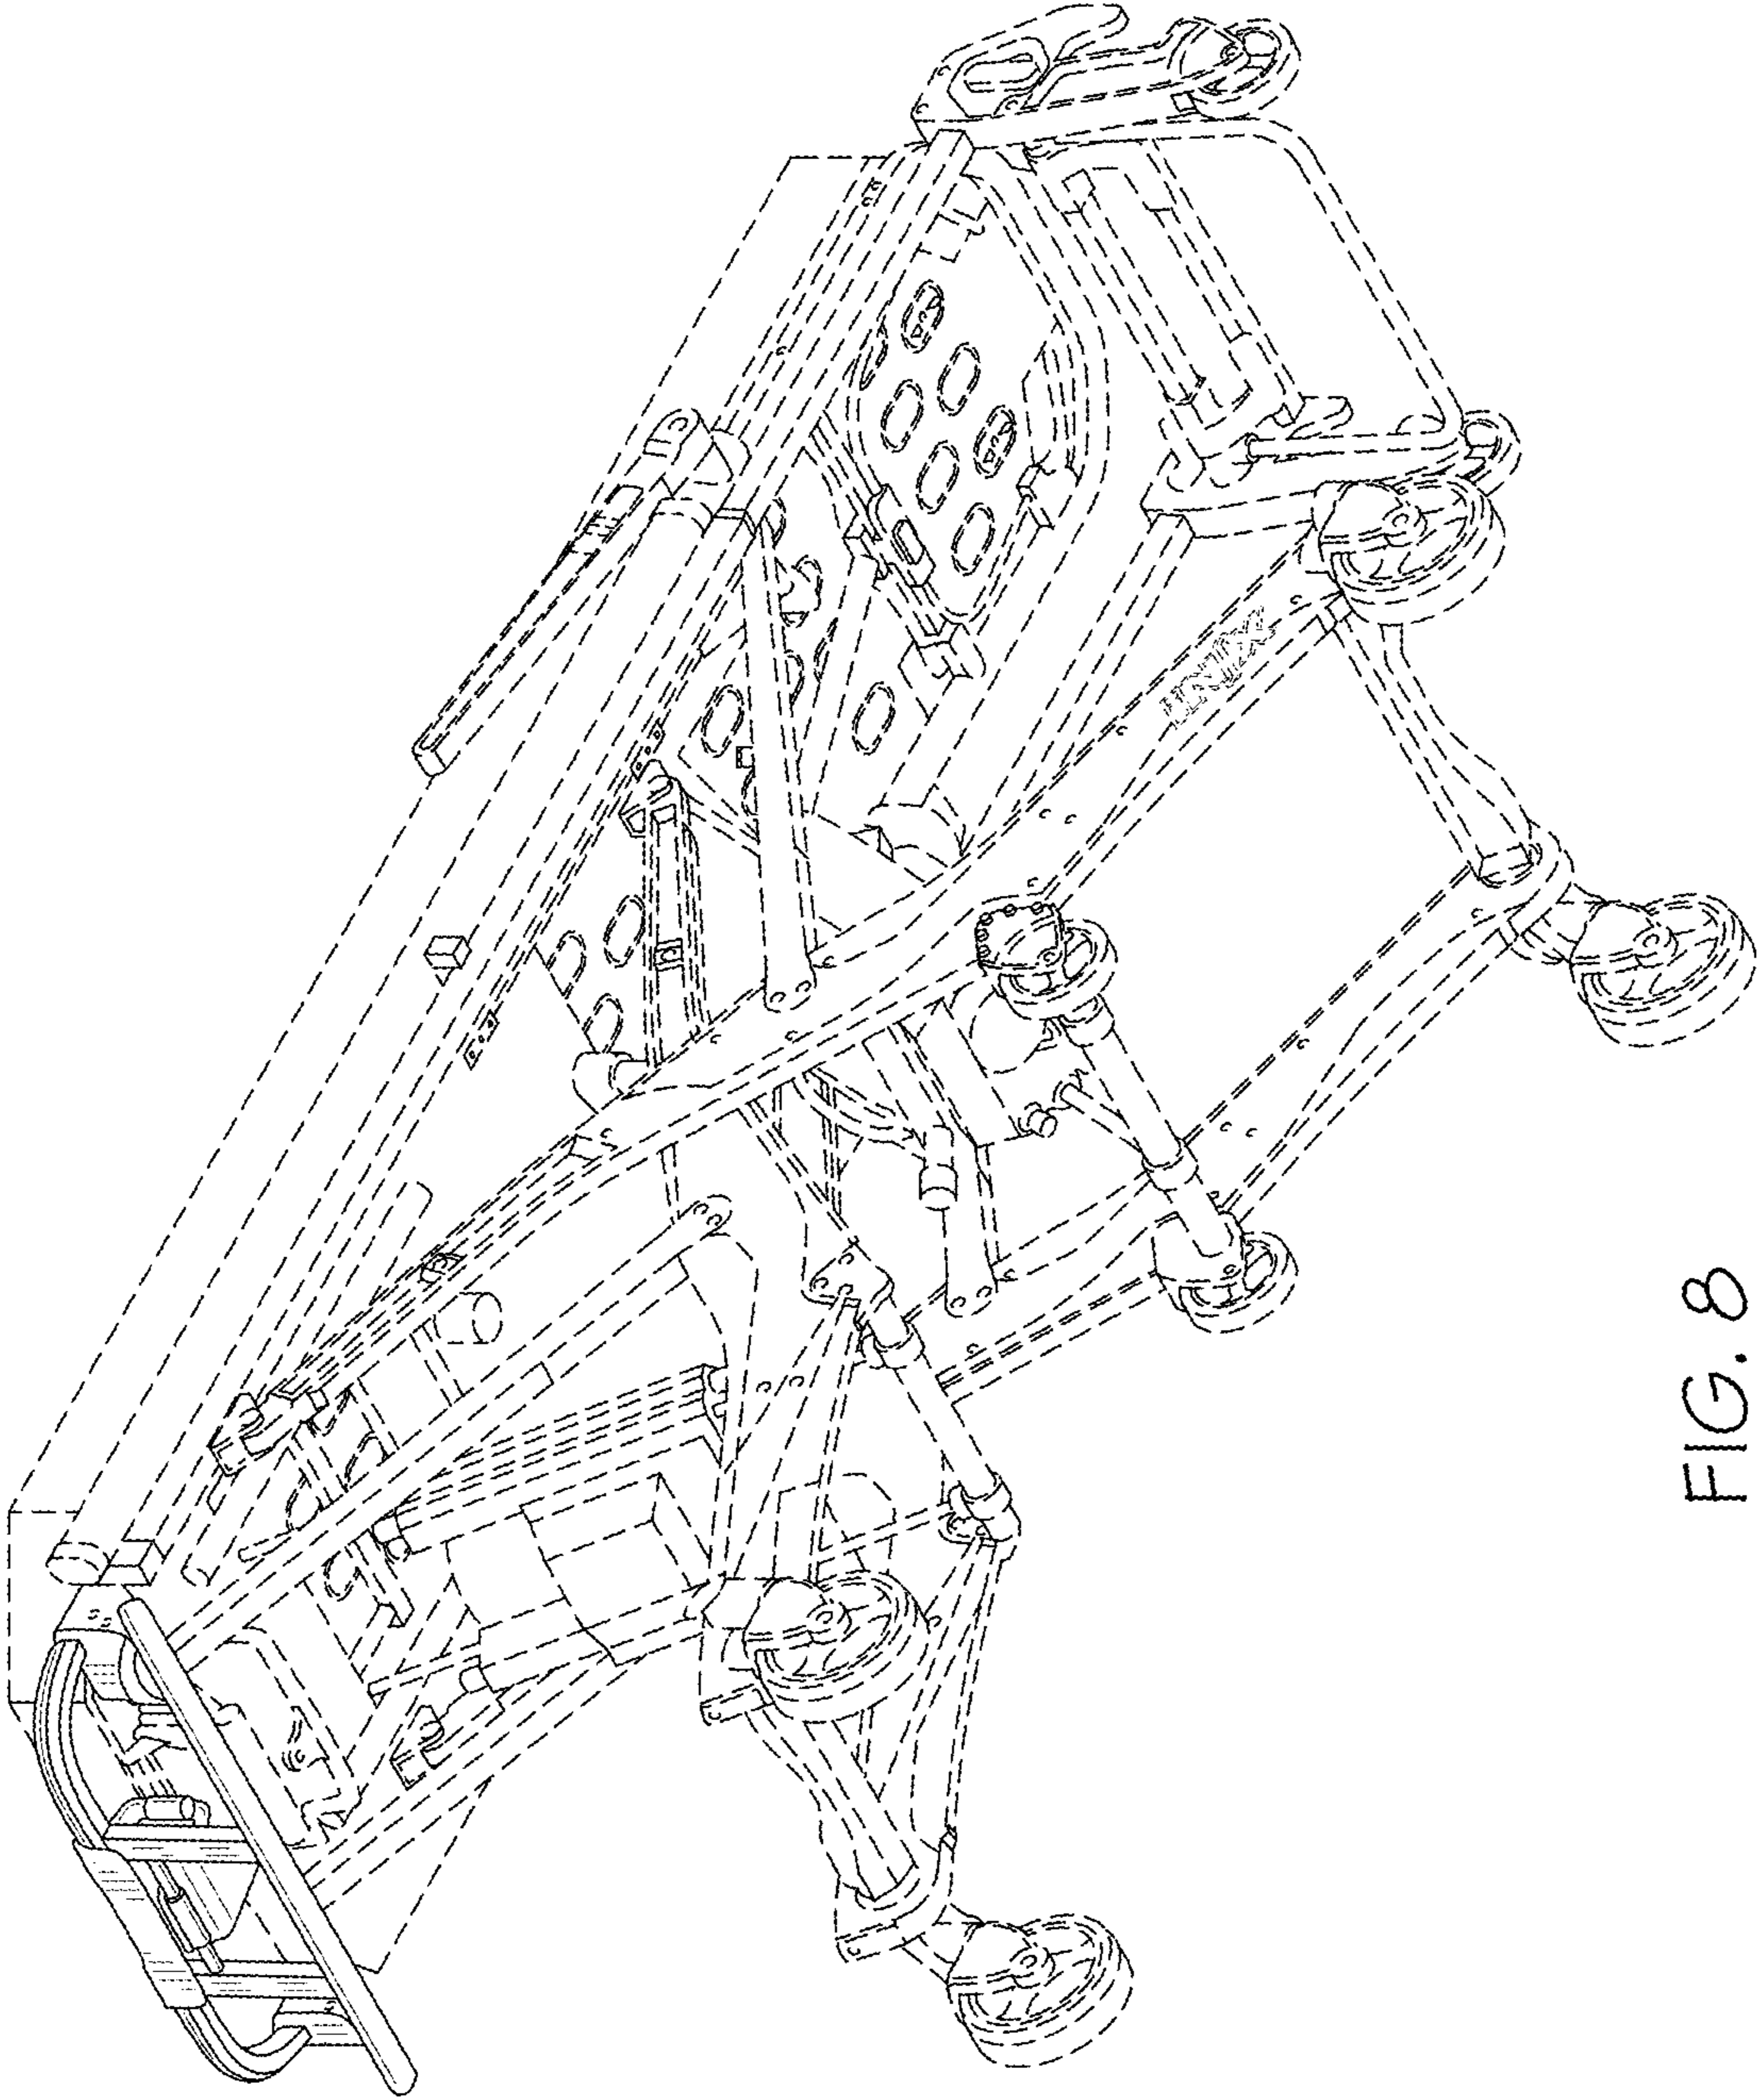


FIG. 8

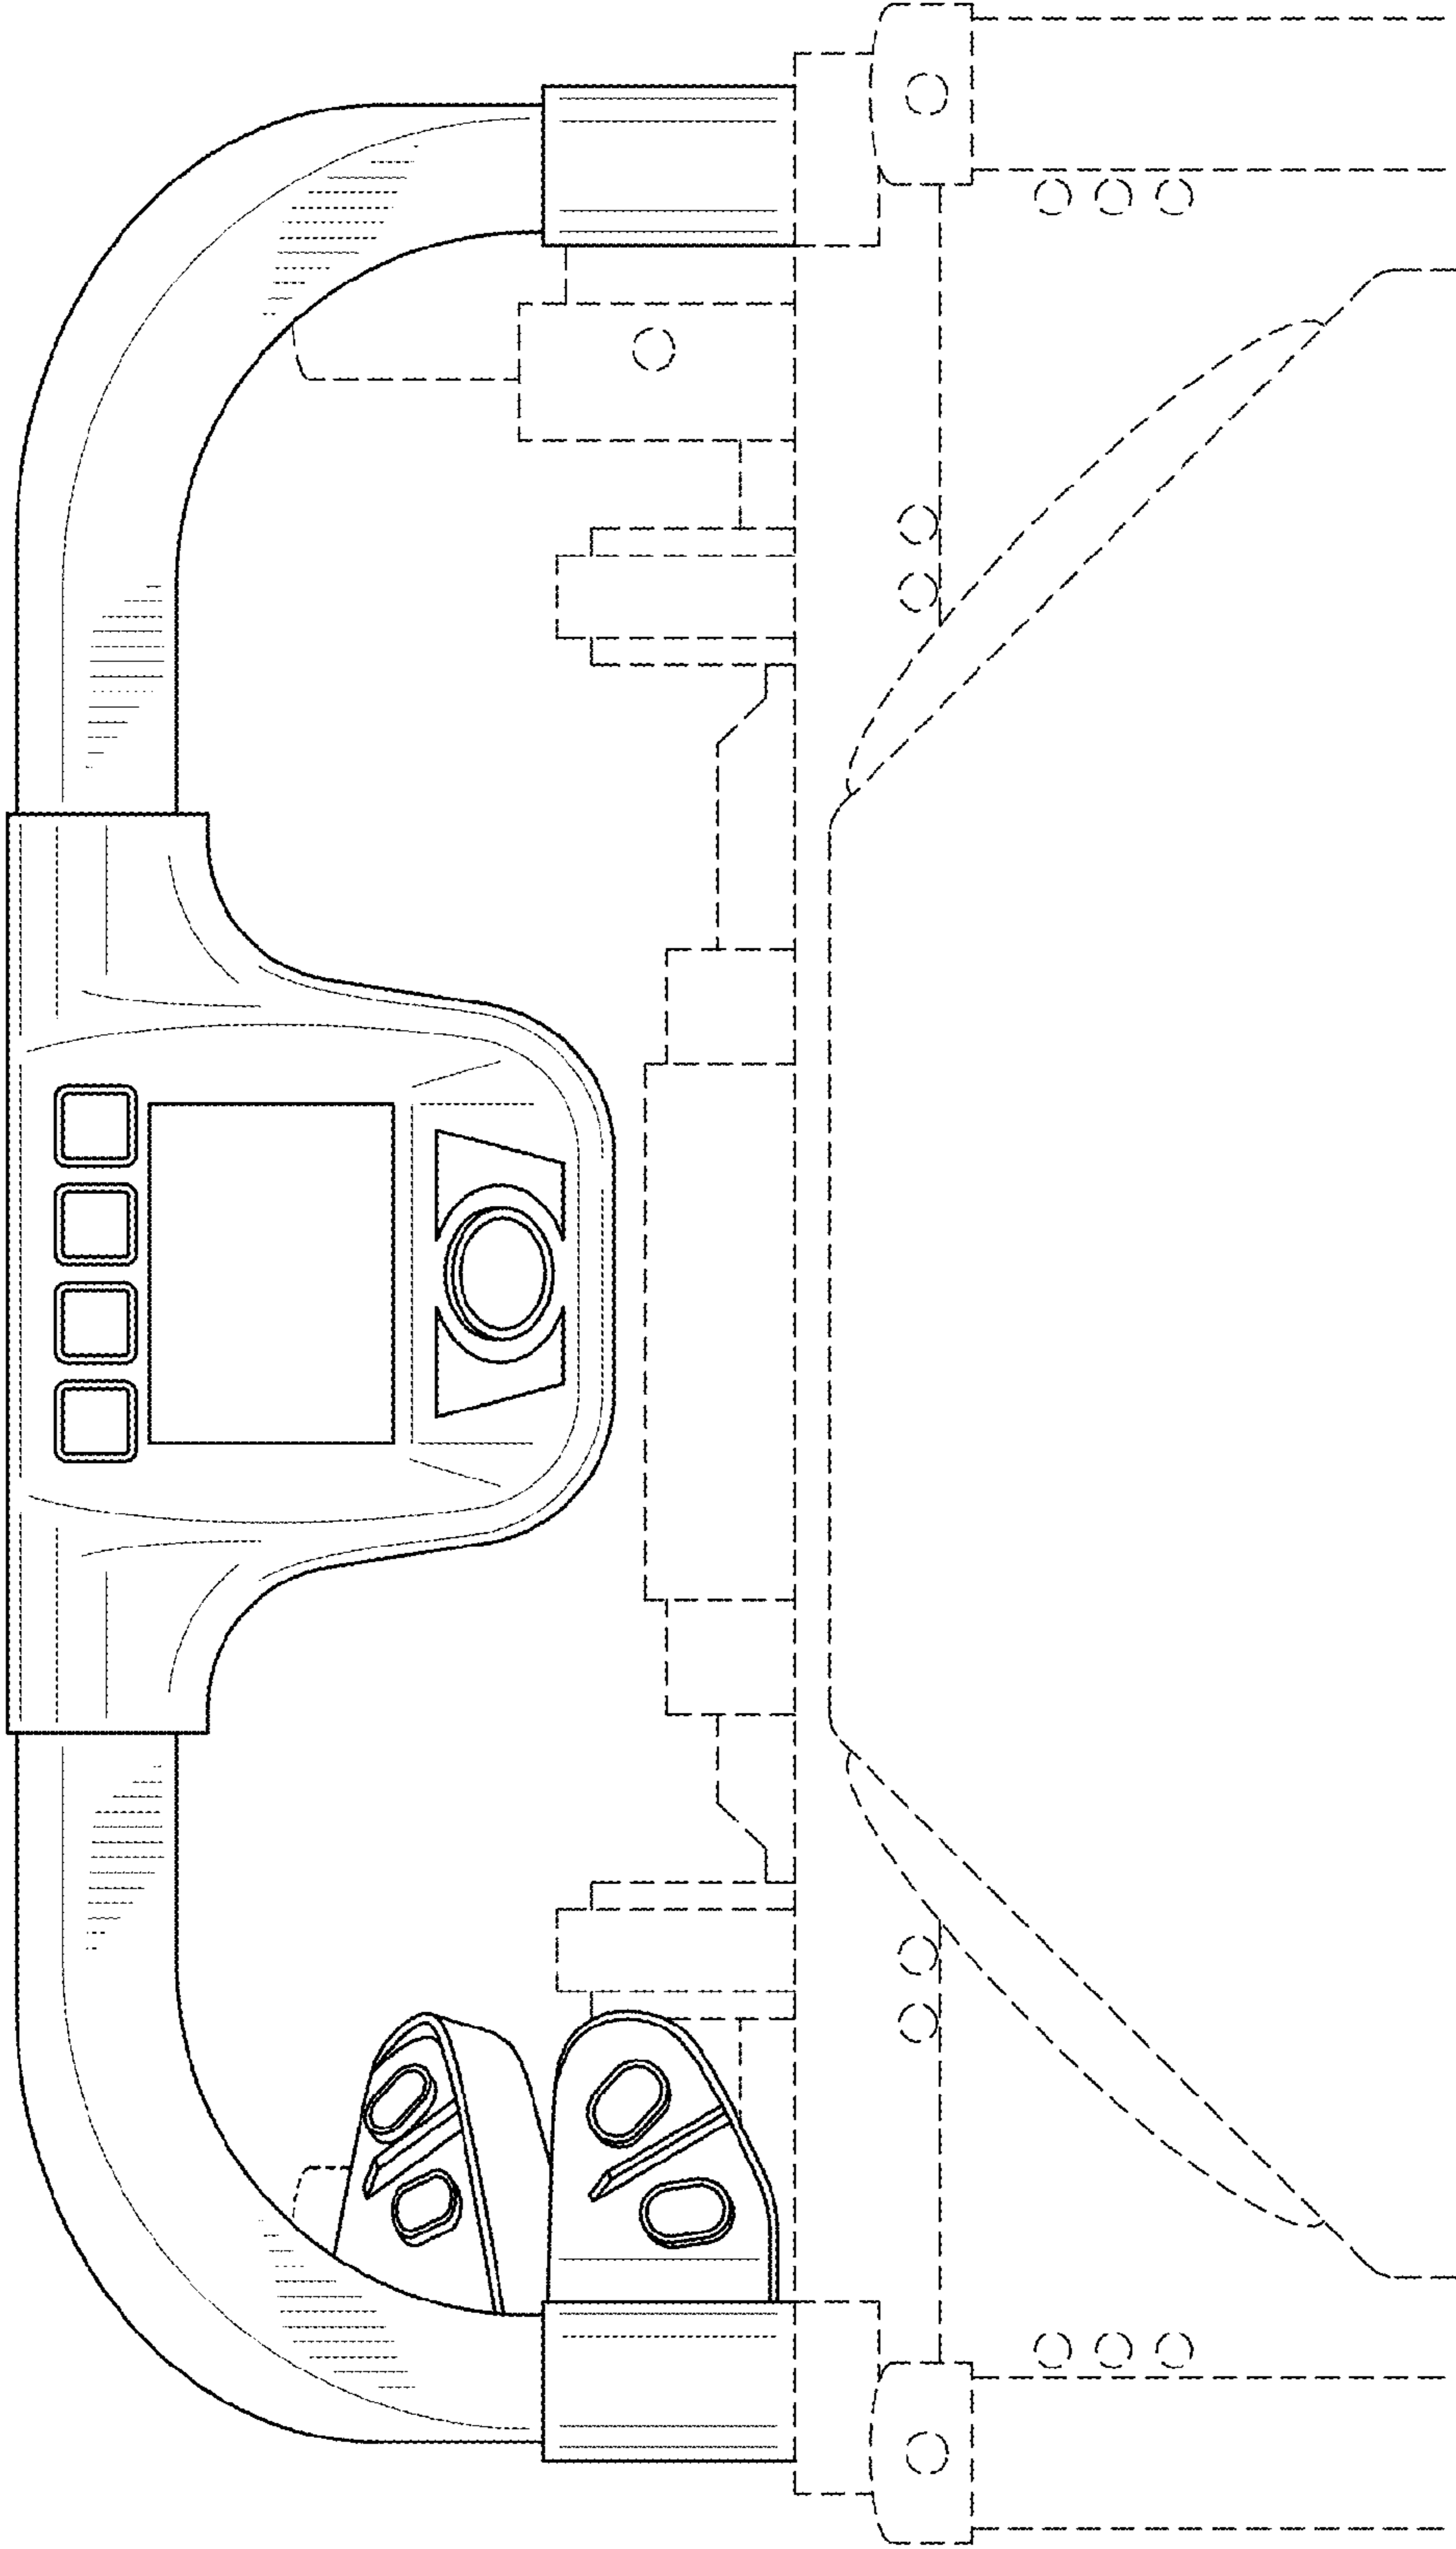


FIG. 9