



US00D751690S

(12) **United States Design Patent**  
**Peret et al.**

(10) **Patent No.:** **US D751,690 S**  
(45) **Date of Patent:** **\*\* Mar. 15, 2016**

(54) **APPARATUS TO CONTROL FLUID FLOW THROUGH A TUBE**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(71) Applicant: **DEKA Products Limited Partnership**,  
Manchester, NH (US)

2,888,877 A 6/1959 Shellman et al.  
3,173,372 A 3/1965 Baldwin  
3,384,336 A 5/1968 Pulman  
3,609,379 A 9/1971 Hildebrandt

(72) Inventors: **Bob D. Peret**, Bedford, NH (US); **Brian H. Yoo**, Cambridge, MA (US); **Kaitlyn S. Clarke**, Manchester, NH (US);  
**Thomas A. Friedrich**, Loudon, NH (US)

(Continued)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **DEKA Products Limited Partnership**,  
Manchester, NH (US)

AU 2247783 A 6/1985  
CA 1213749 A1 11/1986

(Continued)

OTHER PUBLICATIONS

(\*\*) Term: **14 Years**

AAMI and FDA, Infusing Patients Safely: Priority Issues from the AAMI/FDA Infusion Device Summit, Symposium, Oct. 5-6, 2010, pp. 1-48, AAMI, Arlington, VA, USA.

(Continued)

(21) Appl. No.: **29/471,858**

(22) Filed: **Nov. 6, 2013**

*Primary Examiner* — Wan Laymon  
*Assistant Examiner* — Mark Booker

(51) **LOC (10) Cl.** ..... **24-02**

(74) *Attorney, Agent, or Firm* — James D. Wyninegar, Jr.

(52) **U.S. Cl.**  
USPC ..... **D24/111**

(57) **CLAIM**

The ornamental design for an apparatus to control fluid flow through a tube, as shown and described.


(58) **Field of Classification Search**  
USPC ..... D24/111, 107, 112, 169; 604/7-9, 19, 604/67, 123-125, 143, 151-152, 154-156, 604/218, 246, 256, 253, 250-251, 108, 604/169; 417/234; 403/380, 381; 206/363-368; D9/526, 529, 668  
CPC ..... A61M 5/14232; A61M 5/16831; A61M 5/172; A61M 5/14228; A61M 2205/3365; A61M 2205/3313; A61M 5/145; A61M 5/1689; A61M 5/1413; A61M 5/1415; A61M 2205/3569; G01D 5/2451; G01D 5/3473; Y10S 128/13

**DESCRIPTION**

FIG. 1 is a front, bottom, and right side perspective view of the apparatus to control fluid flow through a tube, showing my new design;  
FIG. 2 is a front, top, and left side perspective view thereof;  
FIG. 3 is a bottom plan view thereof;  
FIG. 4 is a top plan view thereof;  
FIG. 5 is a left side elevational view thereof;  
FIG. 6 is a right side elevational view thereof;  
FIG. 7 is a front side elevational view thereof; and,  
FIG. 8 is a back side elevational view thereof.  
The ornamental design which is claimed is shown in solid lines in the drawings. The broken lines shown in the figures represent portions of the article that form no part of the claimed design.

See application file for complete search history.

**1 Claim, 8 Drawing Sheets**

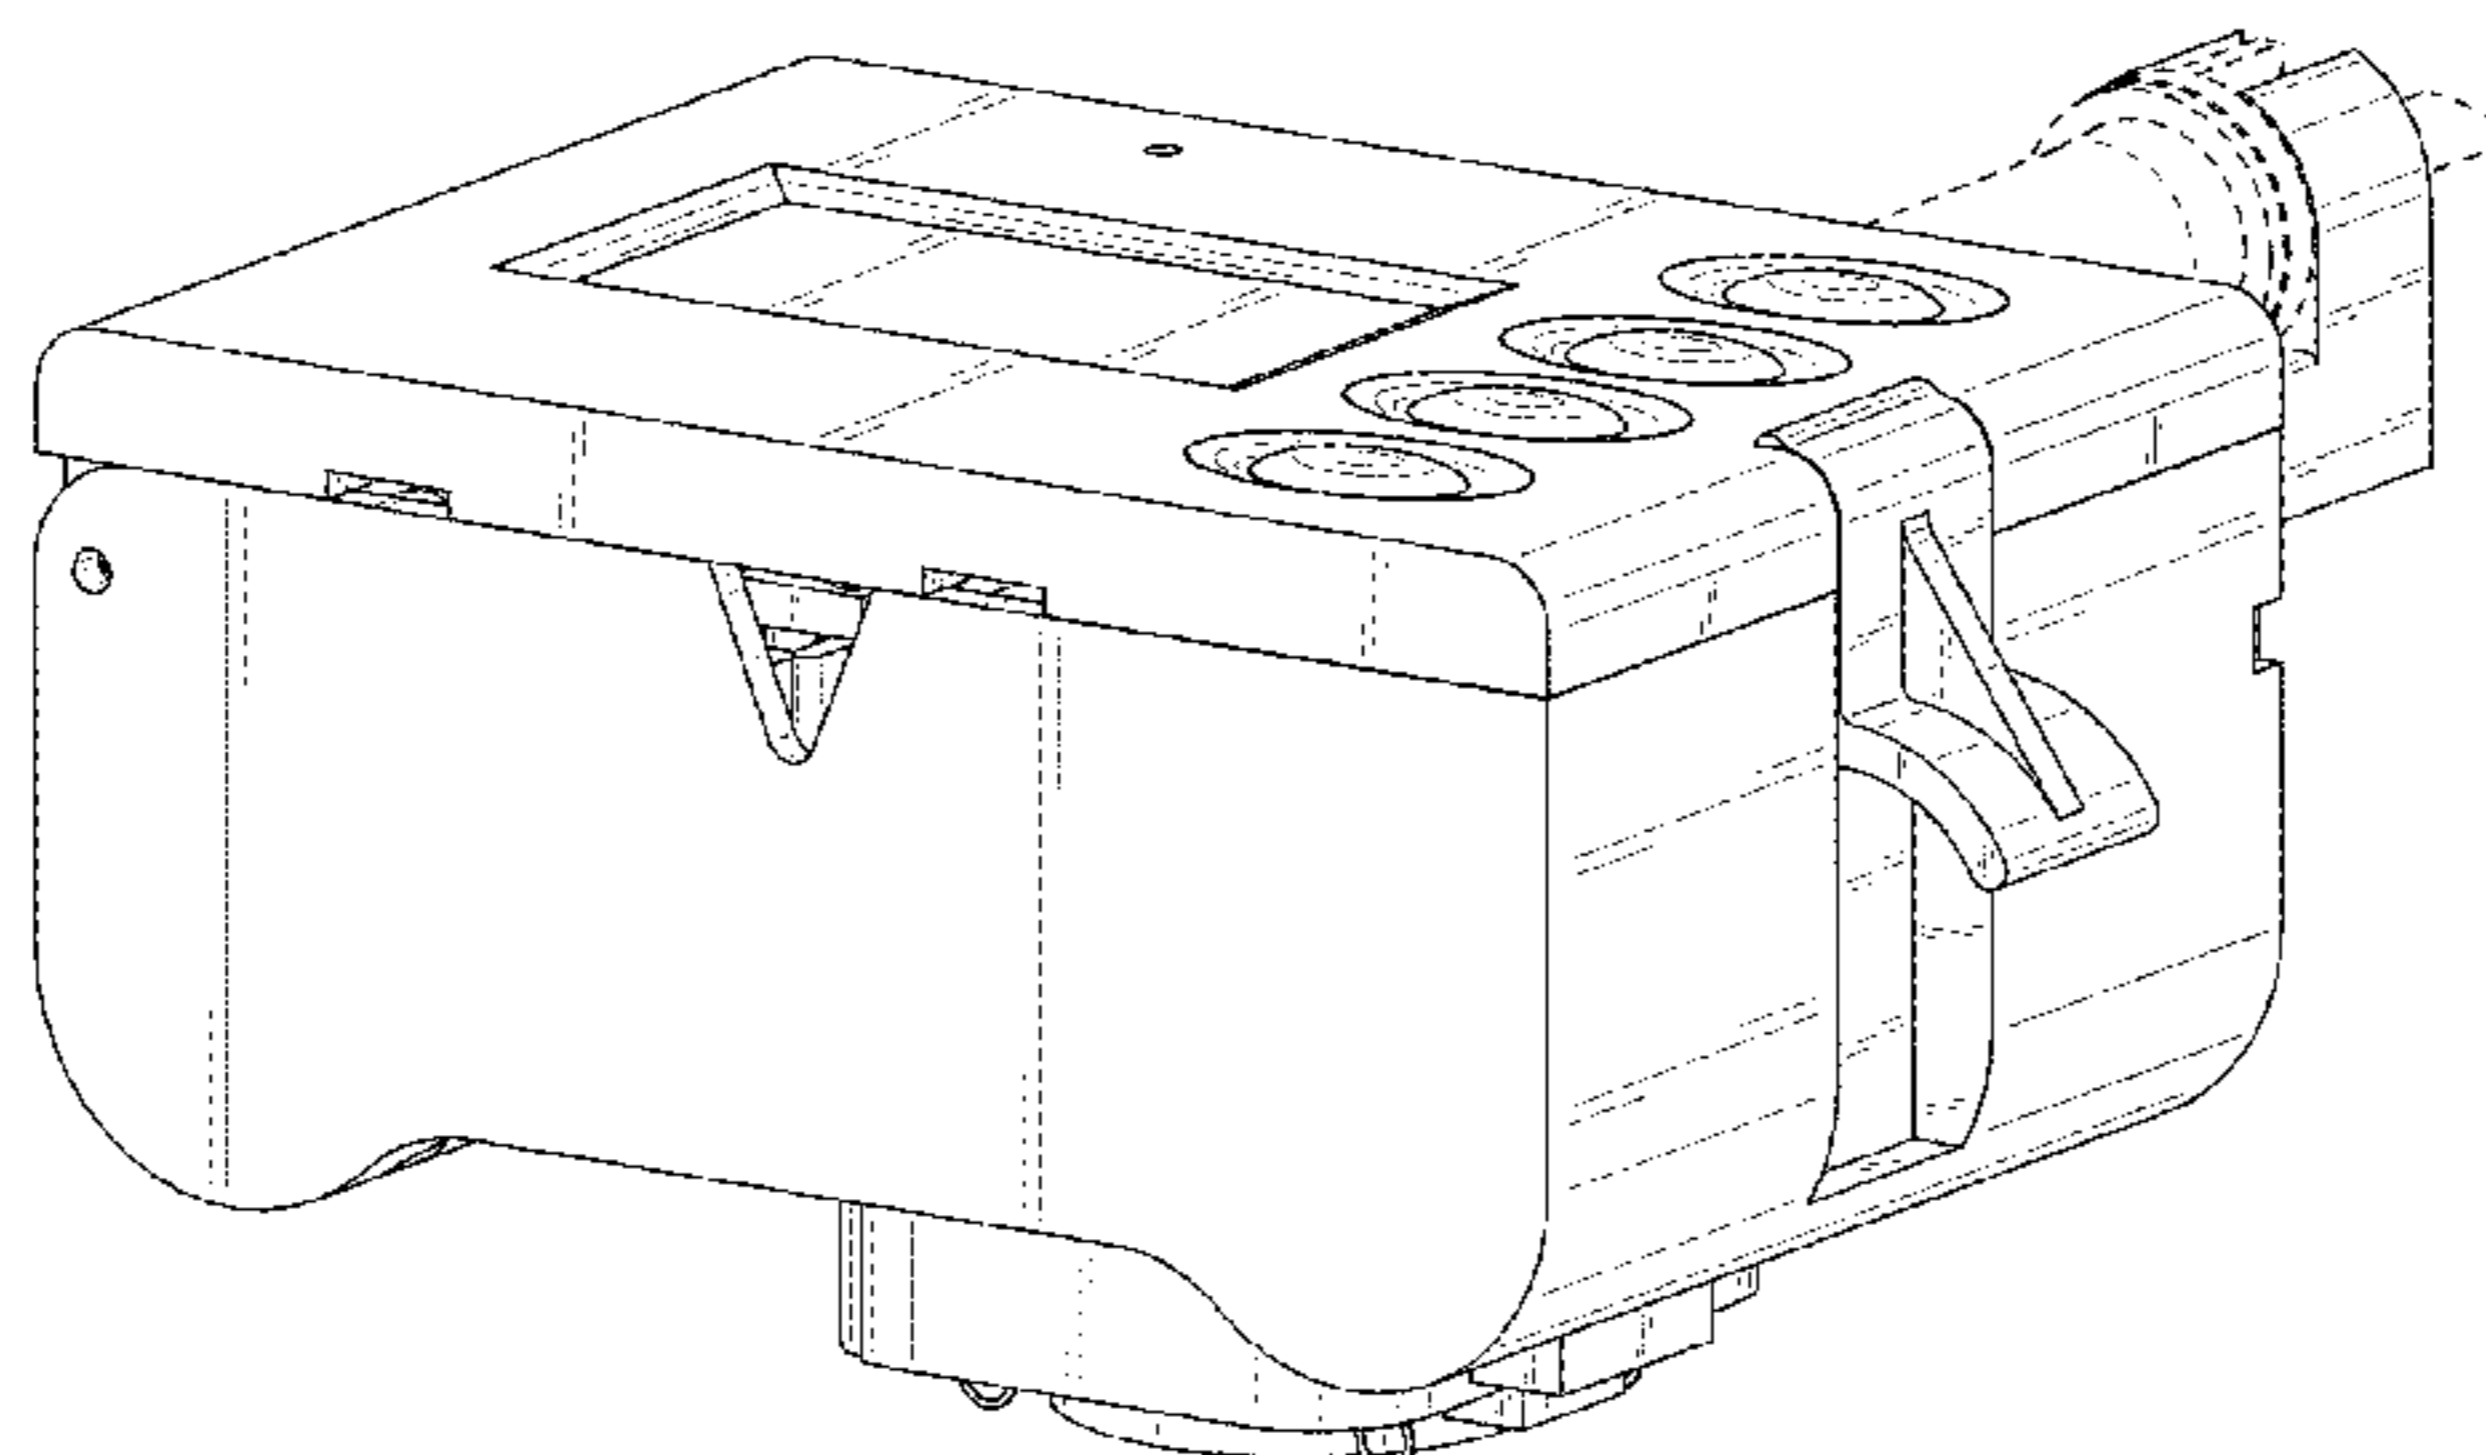



(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0185267 A1 7/2012 Kamen et al.  
 2012/0197185 A1 8/2012 Tao  
 2012/0238997 A1 9/2012 Dewey  
 2012/0265166 A1\* 10/2012 Yodfat ..... A61M 5/1413  
 604/506  
 2012/0310153 A1\* 12/2012 Moberg ..... A61M 5/14566  
 604/67  
 2013/0035659 A1 2/2013 Hungerford et al.  
 2013/0177455 A1 7/2013 Kamen et al.  
 2013/0182381 A1 7/2013 Gray et al.  
 2013/0184676 A1 7/2013 Kamen et al.  
 2013/0188040 A1 7/2013 Kamen et al.  
 2013/0191513 A1 7/2013 Kamen et al.  
 2013/0197693 A1 8/2013 Kamen et al.  
 2013/0201482 A1 8/2013 Munro  
 2013/0204188 A1 8/2013 Kamen et al.  
 2013/0253442 A1\* 9/2013 Travis ..... A61M 39/28  
 604/250  
 2013/0272773 A1 10/2013 Kamen et al.  
 2013/0281965 A1 10/2013 Kamen et al.  
 2013/0297330 A1 11/2013 Kamen et al.  
 2013/0310990 A1 11/2013 Peret et al.  
 2013/0317753 A1 11/2013 Kamen et al.  
 2013/0317837 A1 11/2013 Ballantyne et al.  
 2013/0336814 A1 12/2013 Kamen et al.  
 2013/0339049 A1 12/2013 Blumberg, Jr. et al.  
 2013/0346108 A1 12/2013 Kamen et al.  
 2014/0081233 A1 3/2014 Hungerford et al.  
 2014/0135695 A1\* 5/2014 Grant ..... A61M 5/14244  
 604/111  
 2014/0148757 A1\* 5/2014 Ambrosina ..... A61M 5/38  
 604/67  
 2014/0165703 A1 6/2014 Wilt et al.  
 2014/0180711 A1 6/2014 Kamen et al.  
 2014/0194818 A1\* 7/2014 Yodfat ..... A61M 5/1413  
 604/151  
 2014/0227021 A1 8/2014 Kamen et al.  
 2014/0309612 A1\* 10/2014 Smisson, III ..... A61M 1/0281  
 604/500  
 2014/0318639 A1 10/2014 Peret et al.  
 2015/0002667 A1 1/2015 Peret et al.  
 2015/0002668 A1 1/2015 Peret et al.  
 2015/0002677 A1 1/2015 Peret et al.

FOREIGN PATENT DOCUMENTS

DE 2023027 11/1970  
 DE 3617723 A1 12/1987  
 DE 3822057 C2 1/1989  
 DE 69229832 T2 2/2000  
 EP 0112699 A2 7/1984  
 EP 1722310 A1 4/2005  
 EP 2319551 A2 10/2008  
 FR 2042606 A1 2/1971  
 FR 2458804 1/1981  
 FR 2617593 1/1989  
 GB 1301033 A 12/1972  
 GB 2020735 A 11/1979  
 GB 2207239 B 1/1989  
 GB 2328982 B 3/1999  
 JP S58163843 9/1983  
 JP 3110458 B2 11/2000  
 JP 2011 062371 A 3/2011  
 NL 7006908 11/1970  
 NL 8801680 2/1989  
 NL 9101825 A 5/1993  
 SE 376843 6/1975  
 WO WO 81/02770 A1 10/1981  
 WO WO 93/09407 A1 5/1993  
 WO WO 00/72181 A2 11/2000  
 WO WO 02/40084 A2 5/2002  
 WO WO 02/0100262 A1 12/2002  
 WO WO 2004/035116 A1 4/2004  
 WO WO 2005/094919 A1 10/2005

WO WO 2006/086723 A2 8/2006  
 WO WO 2008/022880 A1 2/2008  
 WO WO 2008/079023 A1 7/2008  
 WO WO 2009/039203 A2 3/2009  
 WO WO 2009/039214 A2 3/2009  
 WO WO 2009/055639 A2 4/2009  
 WO WO 2010/129720 A2 11/2010  
 WO WO 2011/021098 A1 2/2011  
 WO WO 2011/136667 A1 11/2011  
 WO WO 2013/095459 A9 6/2013  
 WO WO 2013/096713 A2 6/2013  
 WO WO 2013/096718 A2 6/2013  
 WO WO 2013/096722 A2 6/2013  
 WO WO 2013/096909 A2 6/2013

OTHER PUBLICATIONS

Conway, "Analytical Analysis of Tip Travel in a Bourdon Tube", Master's Thesis, Naval Postgraduate School Monterey, Dec. 1995, pp. i-89.  
 "Principles of Flow Cytometry: An Overview." Methods in Cell Biology: Cytometry. Ed. Zbigniew Darzynkiewicz. 3rd ed. vol. 63. Academic, 2000. 44-48.  
 "Feature Detection", *OpenCV Wiki, 2010*, 7 pgs, [http://opencv.willowgarage.com/documentation/cpp/imgproc\\_feature\\_detection.html](http://opencv.willowgarage.com/documentation/cpp/imgproc_feature_detection.html).  
 Galambos et al., "Progressive Probabilistic Hough Transform for Line Detection", IEEE, 7 pgs, 1999.  
 International Search Report & Written Opinion dated May 14, 2012, received in International patent application No. PCT/US2011/066588 (197WO), 9 pgs.  
 International Search Report & Written Opinion dated Jun. 18, 2013, received in International patent application No. PCT/US2012/071142 (J79WO), 14 pgs.  
 International Search Report & Written Opinion dated Oct. 1, 2013, received in International patent application No. PCT/US2012/071490 (J76WO), 19 pgs.  
 International Search Report & Written Opinion dated Dec. 4, 2013, received in International patent application No. PCT/US2013/032445 (K14WO), 20 pgs.  
 International Search Report & Written Opinion dated Nov. 7, 2013, received in International patent application No. PCT/US2013/042350 (K66WO), 18 pgs.  
 Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 9, 2013, received in International patent application No. PCT/US2013/032445 (K14WO), 10 pgs.  
 Invitation to Pay Additional Fees and, Where Applicable, Protest Fee dated Sep. 26, 2013, received in International patent application No. PCT/US2013/042350 (K66WO), 7 pgs.  
 Hofmann, "Modeling Medical Devices for Plug-and-Play Interoperability", MIT Department of Electrical Engineering and Computer Science, Jun. 2007, pp. 1-187.  
 King et al. *Prototyping closed loop physiologic control with the medical device coordination framework*. In *SEHC 2010: Proceedings of the 2010 ICSE Workshop on Software Engineering in Health Care* (pp. 1-11). New York, NY: ACM. (2010).  
 Jetley et al., "Safety Requirements Based Analysis of Infusion Pump Software", Proceedings of the IEEE Real Time Systems Symposium, Tuscon, Dec. 2007 pp. 1-4.  
 FDA US Food and Drug Administration, "SEDASYS® Computer-Assisted Personalized Sedation System—P08000", Jul. 16, 2013, pp. 1-2, [www.fda.gov/MedicalDevices/ProductsandMedicalProcedures/DeviceApprovalsandClearances/Recently-ApprovedDevices/ucm353950.htm](http://www.fda.gov/MedicalDevices/ProductsandMedicalProcedures/DeviceApprovalsandClearances/Recently-ApprovedDevices/ucm353950.htm).  
 Luerkens, David W. "Theory and Application of Morphological Analysis: Fine Particles and Surfaces". Boca Raton: CRC, 1991. 5-7.  
 Matas et al., *Progressive Probabilistic Hough Transform*.  
 "Miscellaneous Image Transformations", *OpenCV Wiki, 2011*, 9 pgs., [http://opencv.willowgarage.com/documentation/cpp/miscellaneous\\_image\\_transformations](http://opencv.willowgarage.com/documentation/cpp/miscellaneous_image_transformations).  
 National Patient Safety Agency, *Design for Patient Safety: A Guide to the Design of Electronic Infusion Devices*, booklet, 2010, pp. 1-96, Edition 1, National Patient Safety Agency, London.

(56)

**References Cited**

OTHER PUBLICATIONS

“Object Detection”, OpenCV Wiki, 2011, 2 pgs., [http://opencv.wil-lowgarage.com/documentation/cpp/object\\_detection.html](http://opencv.wil-lowgarage.com/documentation/cpp/object_detection.html).

“The OpenCV Reference Manual Release 2.4.6.0”, Jul. 1, 2013, pp. 1-813.

Leor et al., “A System for the Measurement of Drop Volume of Intra-venous Solutions”, Proceedings Computers in Cardiology 1990, pp. 405-406, Los Alamitos, California.

Butterfield, “Alaris SE Pump, Monitoring and Detection of IV Line Occlusions.”, CareFusion Corporation, 2010, 4 pgs.

“Vista Basic: Instructions for Use: Software IFVB”, manual, 2002, pgs. 3, B. Braun Medical Inc.

Hugli et al., “Drop volume measurement by vision.” Proceedings of SPIE Electronic Imaging Conference, San Diego, Jan. 2000. SPIE vol. 3866-11, pp. 60-66.

\* cited by examiner

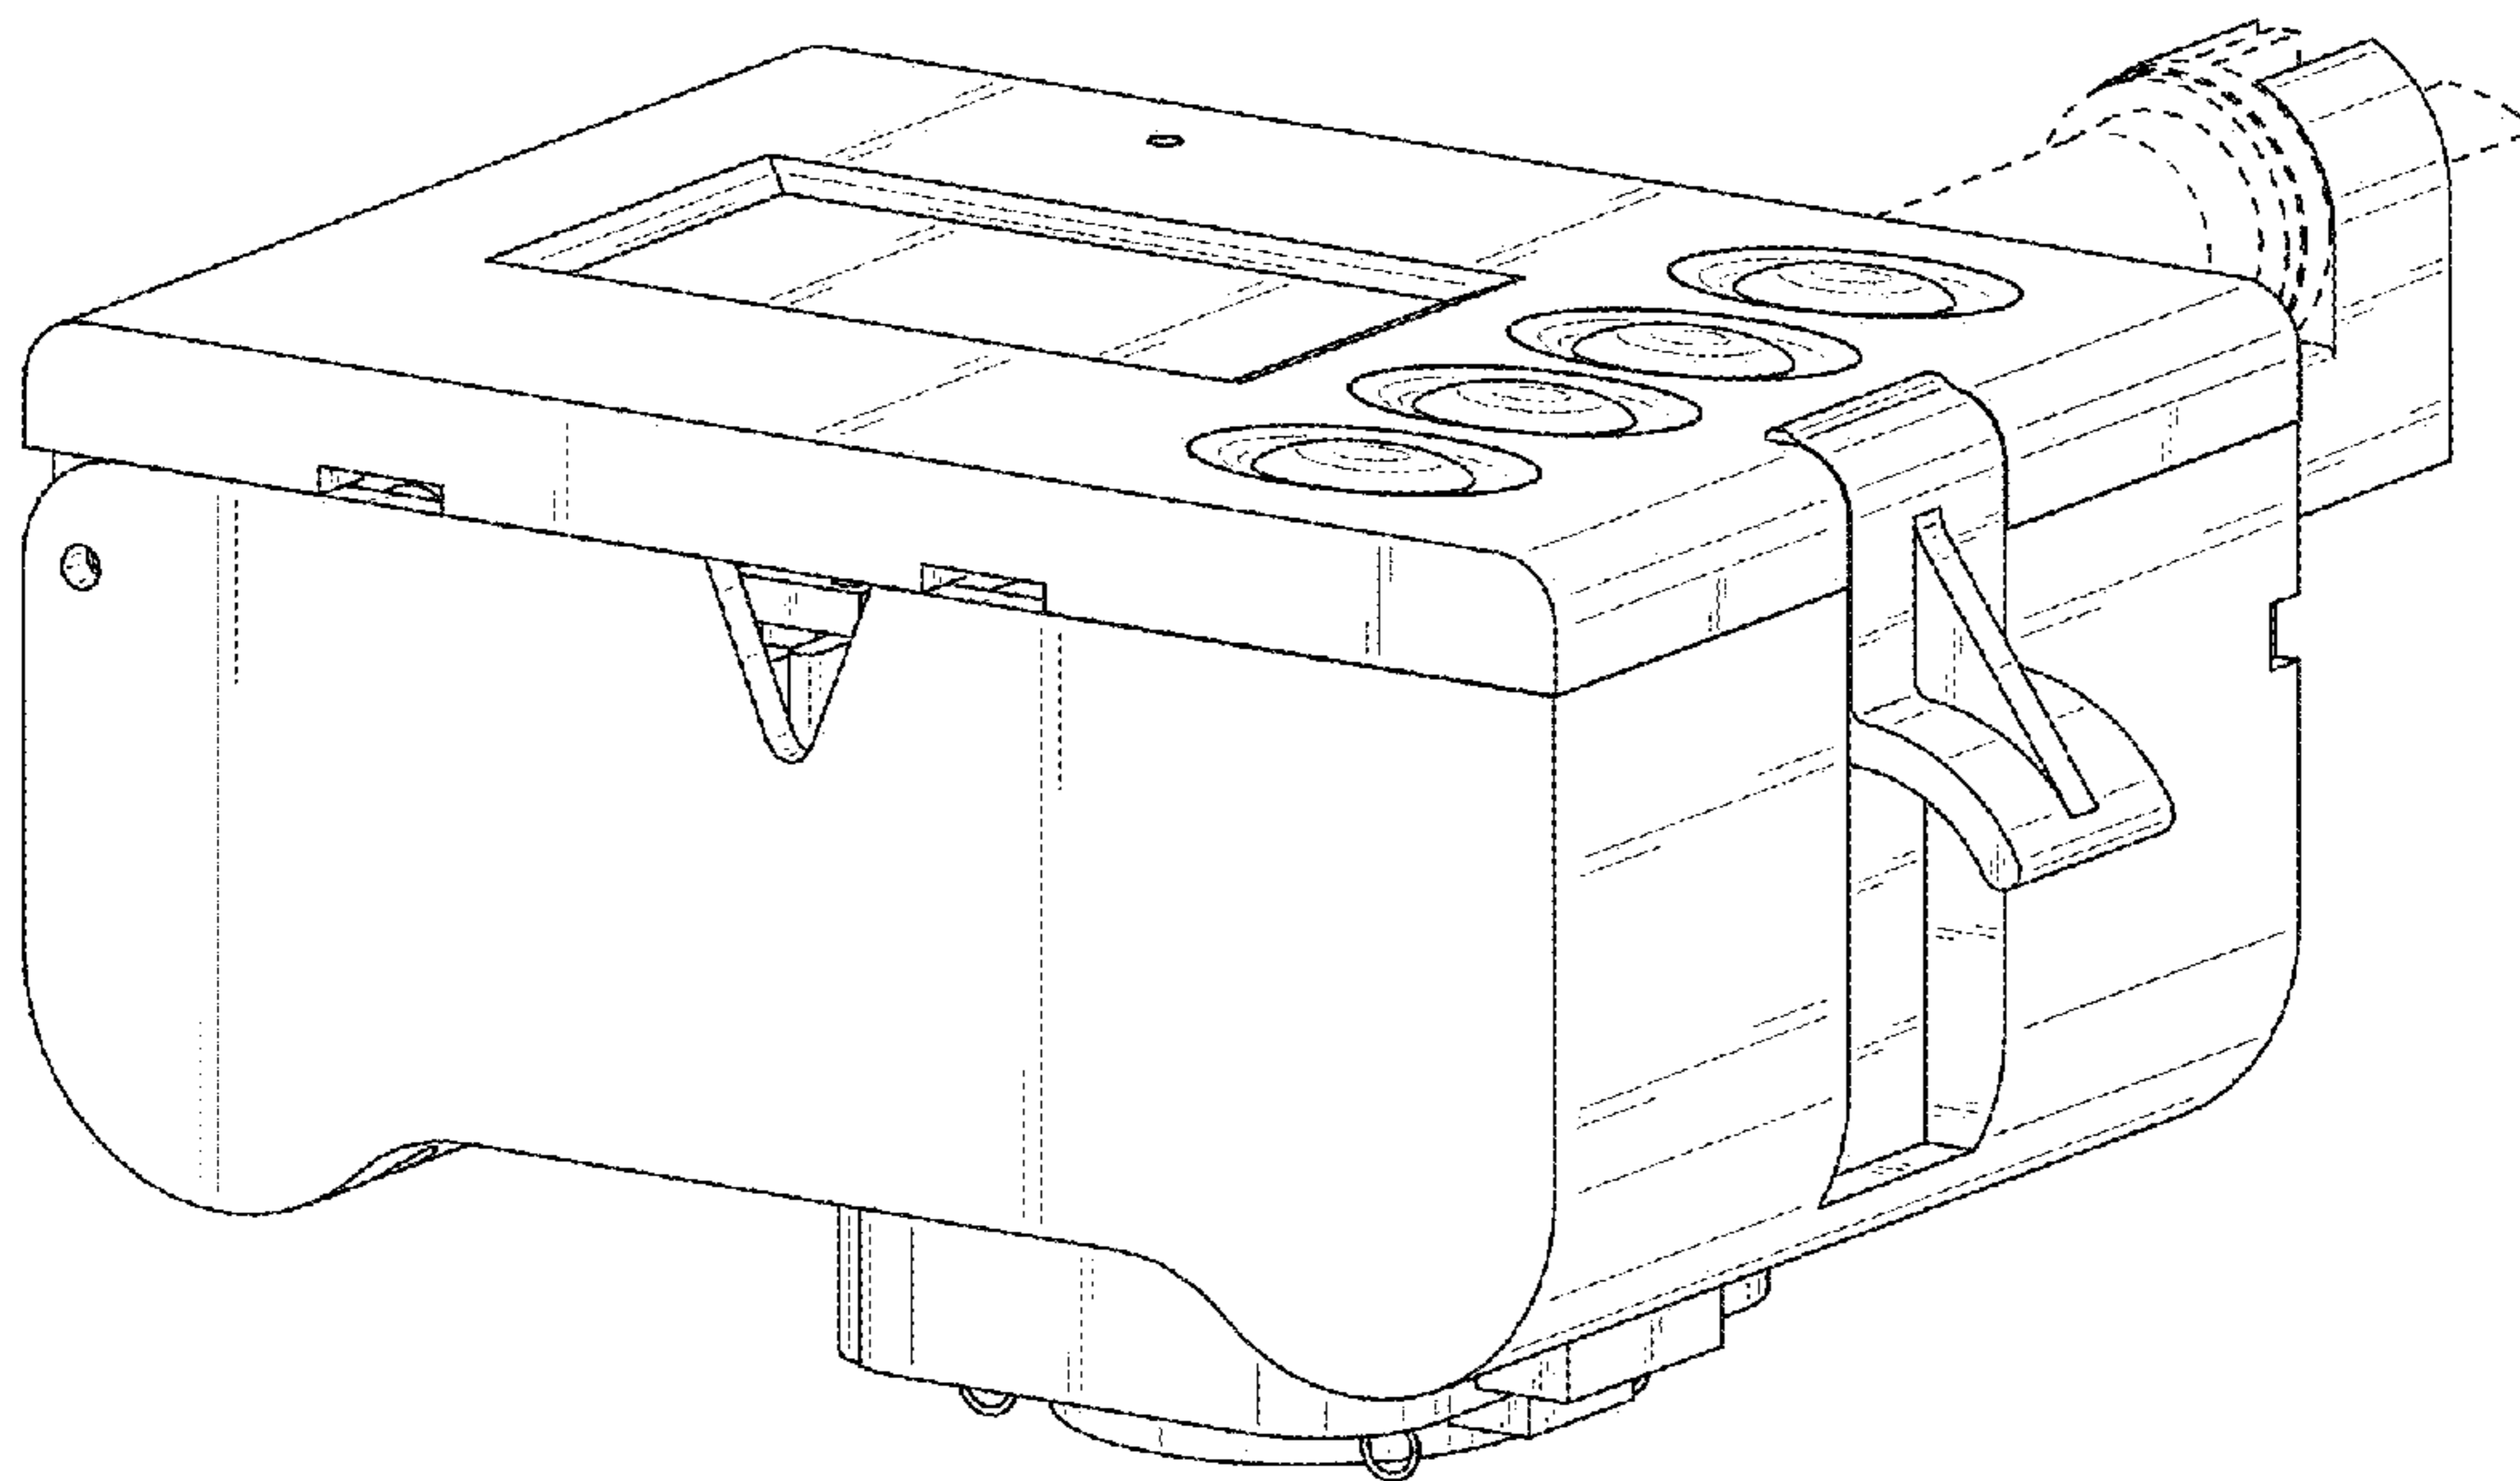


FIG. 1

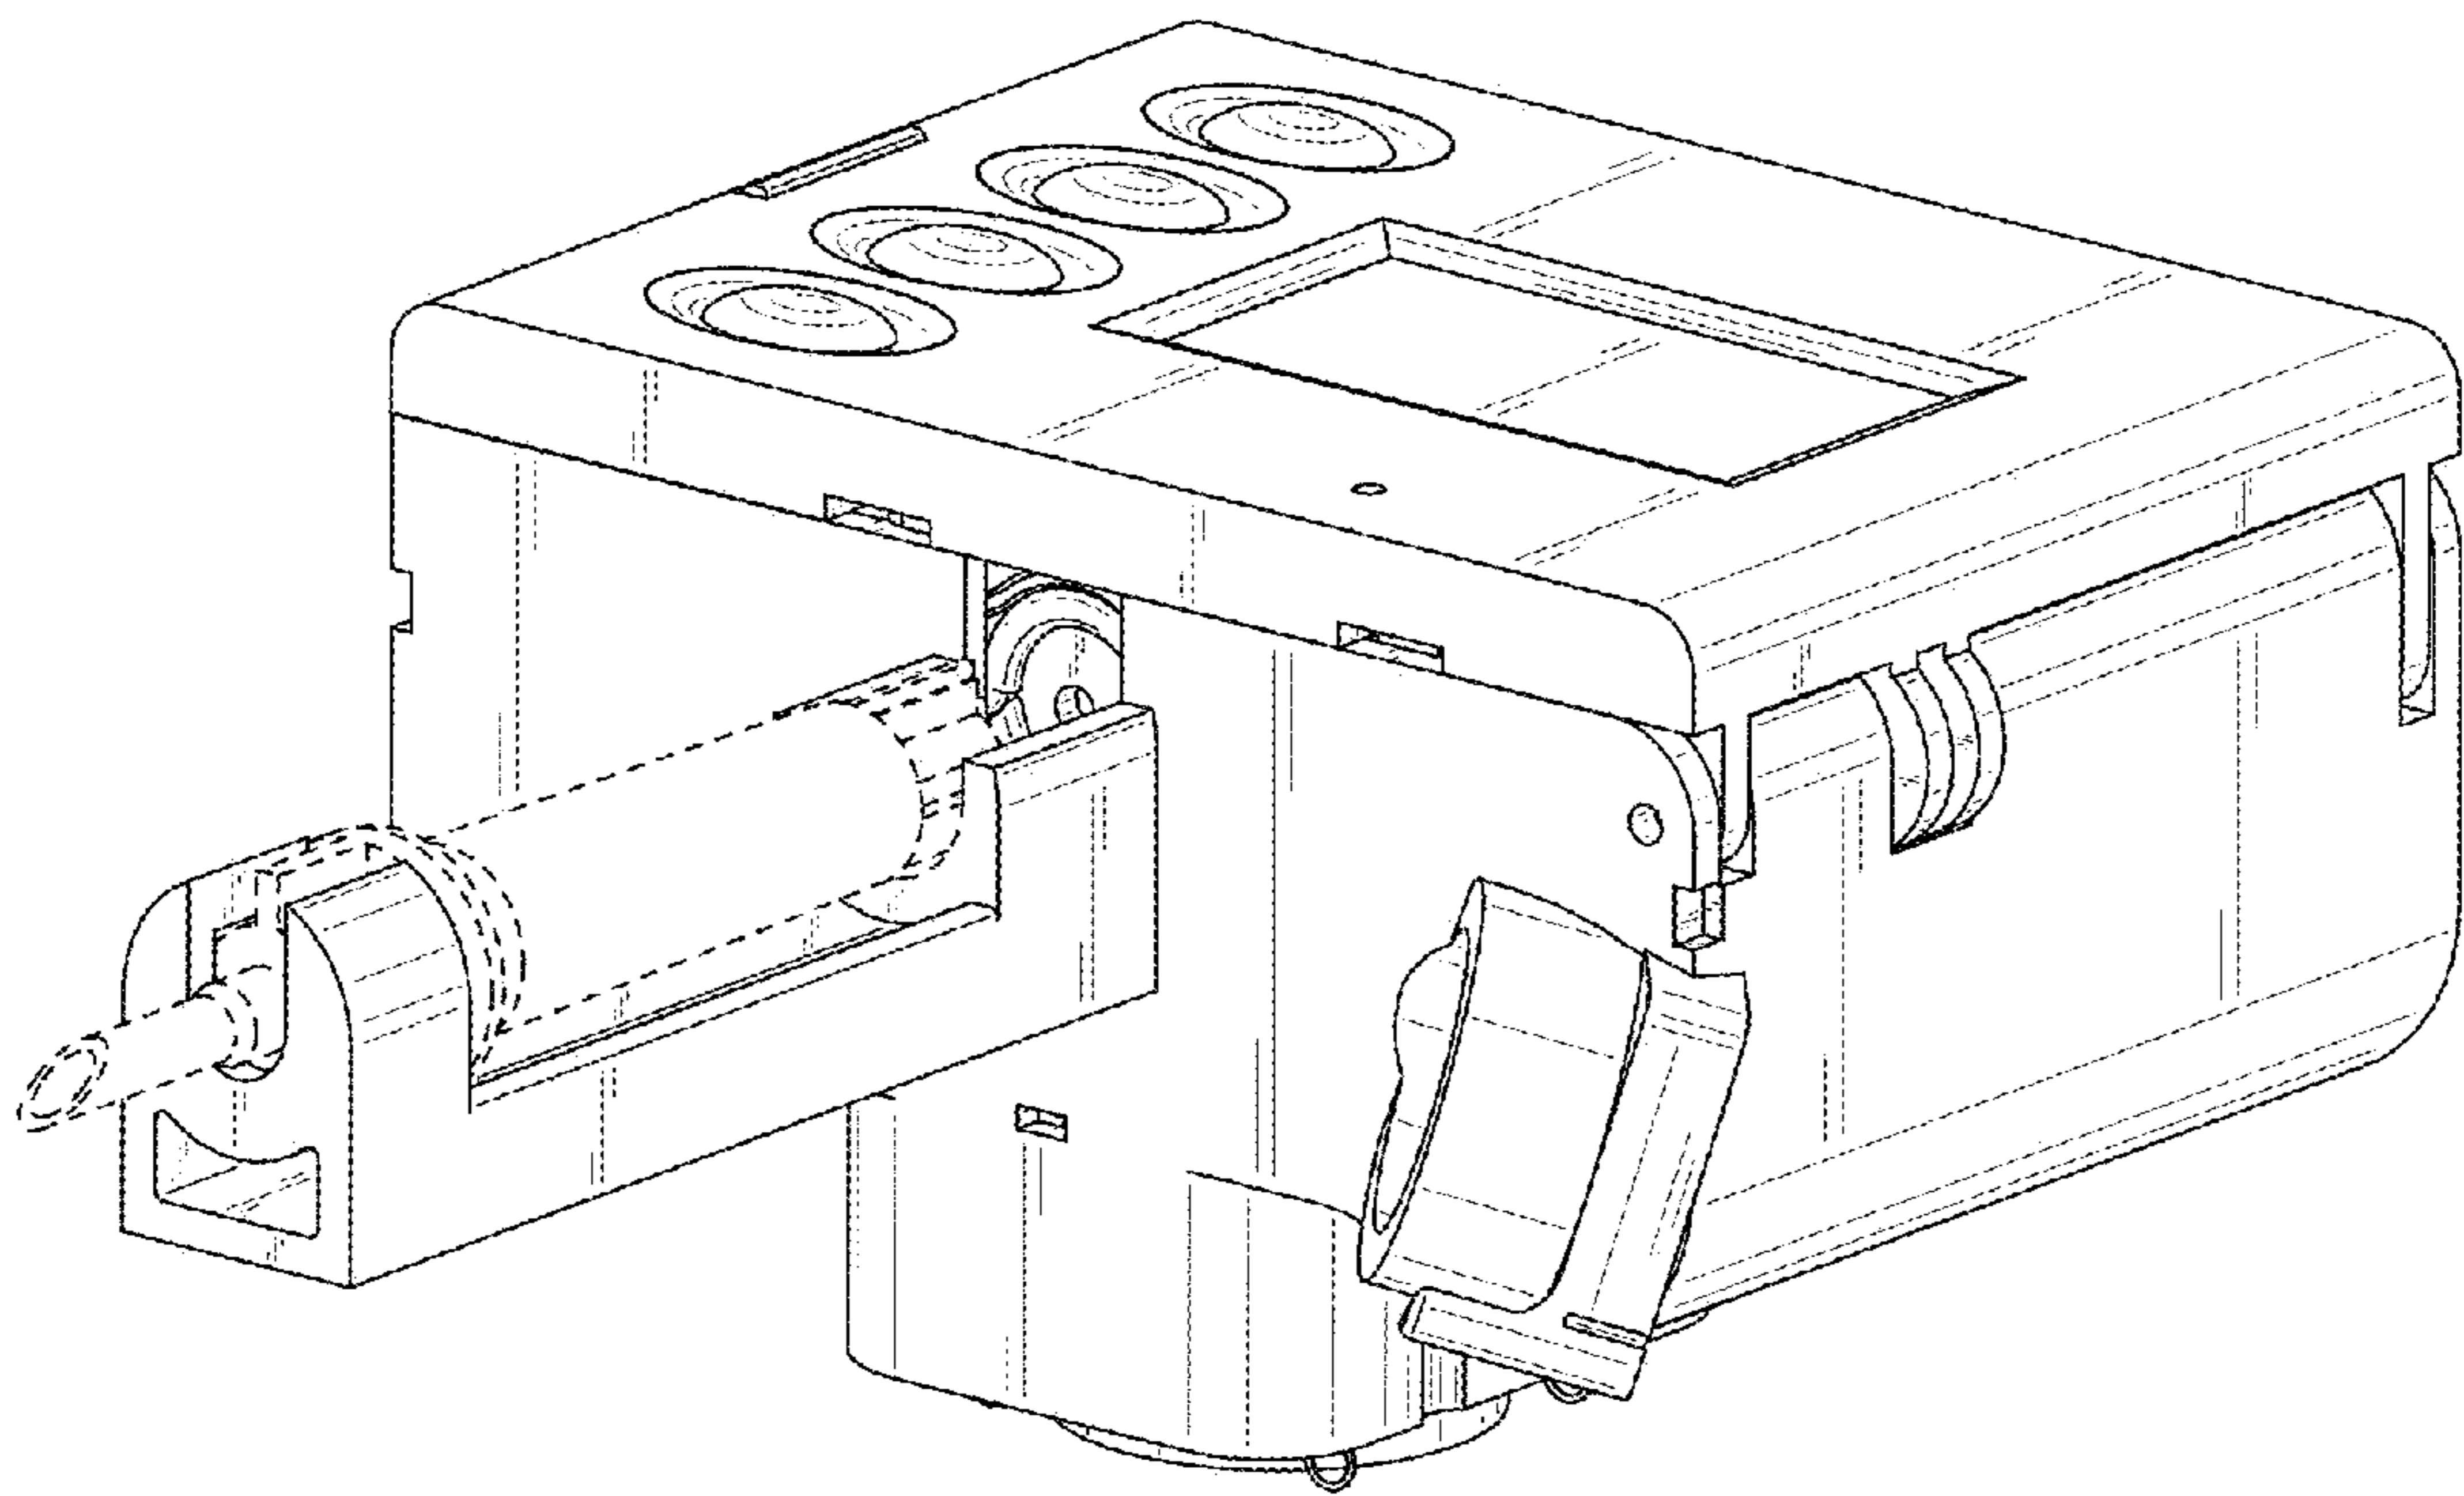


FIG. 2

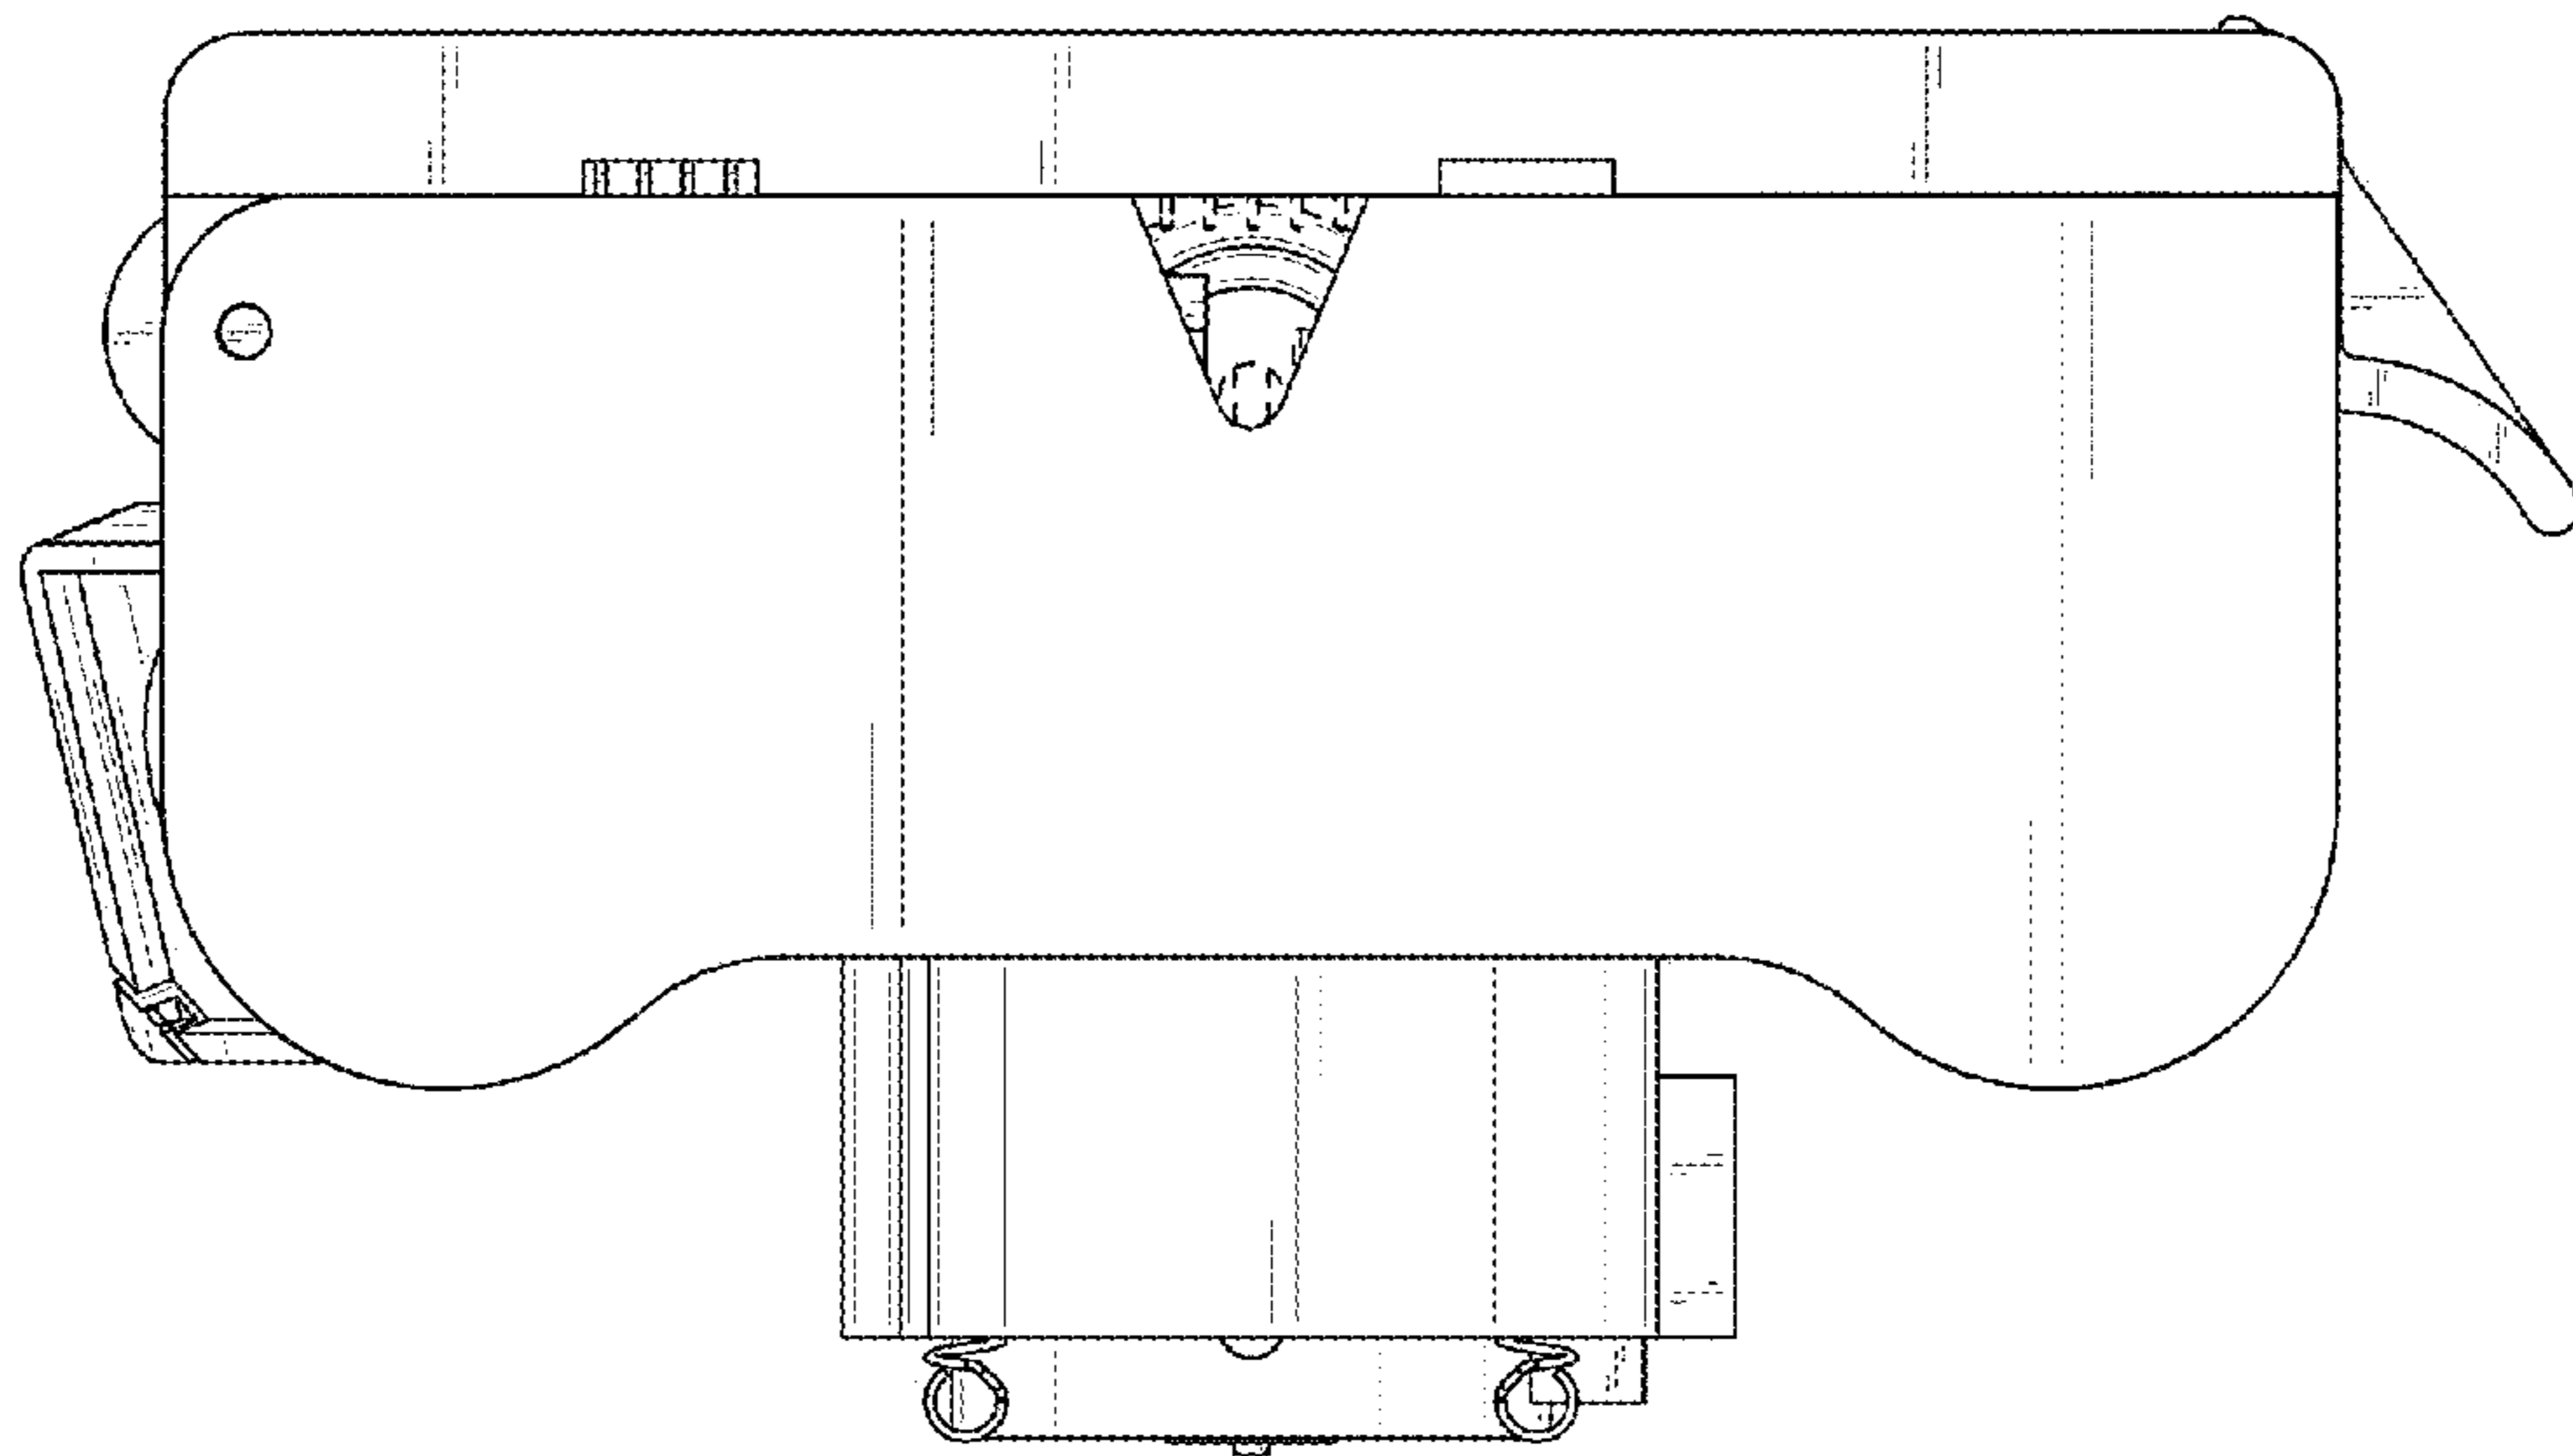


FIG. 3

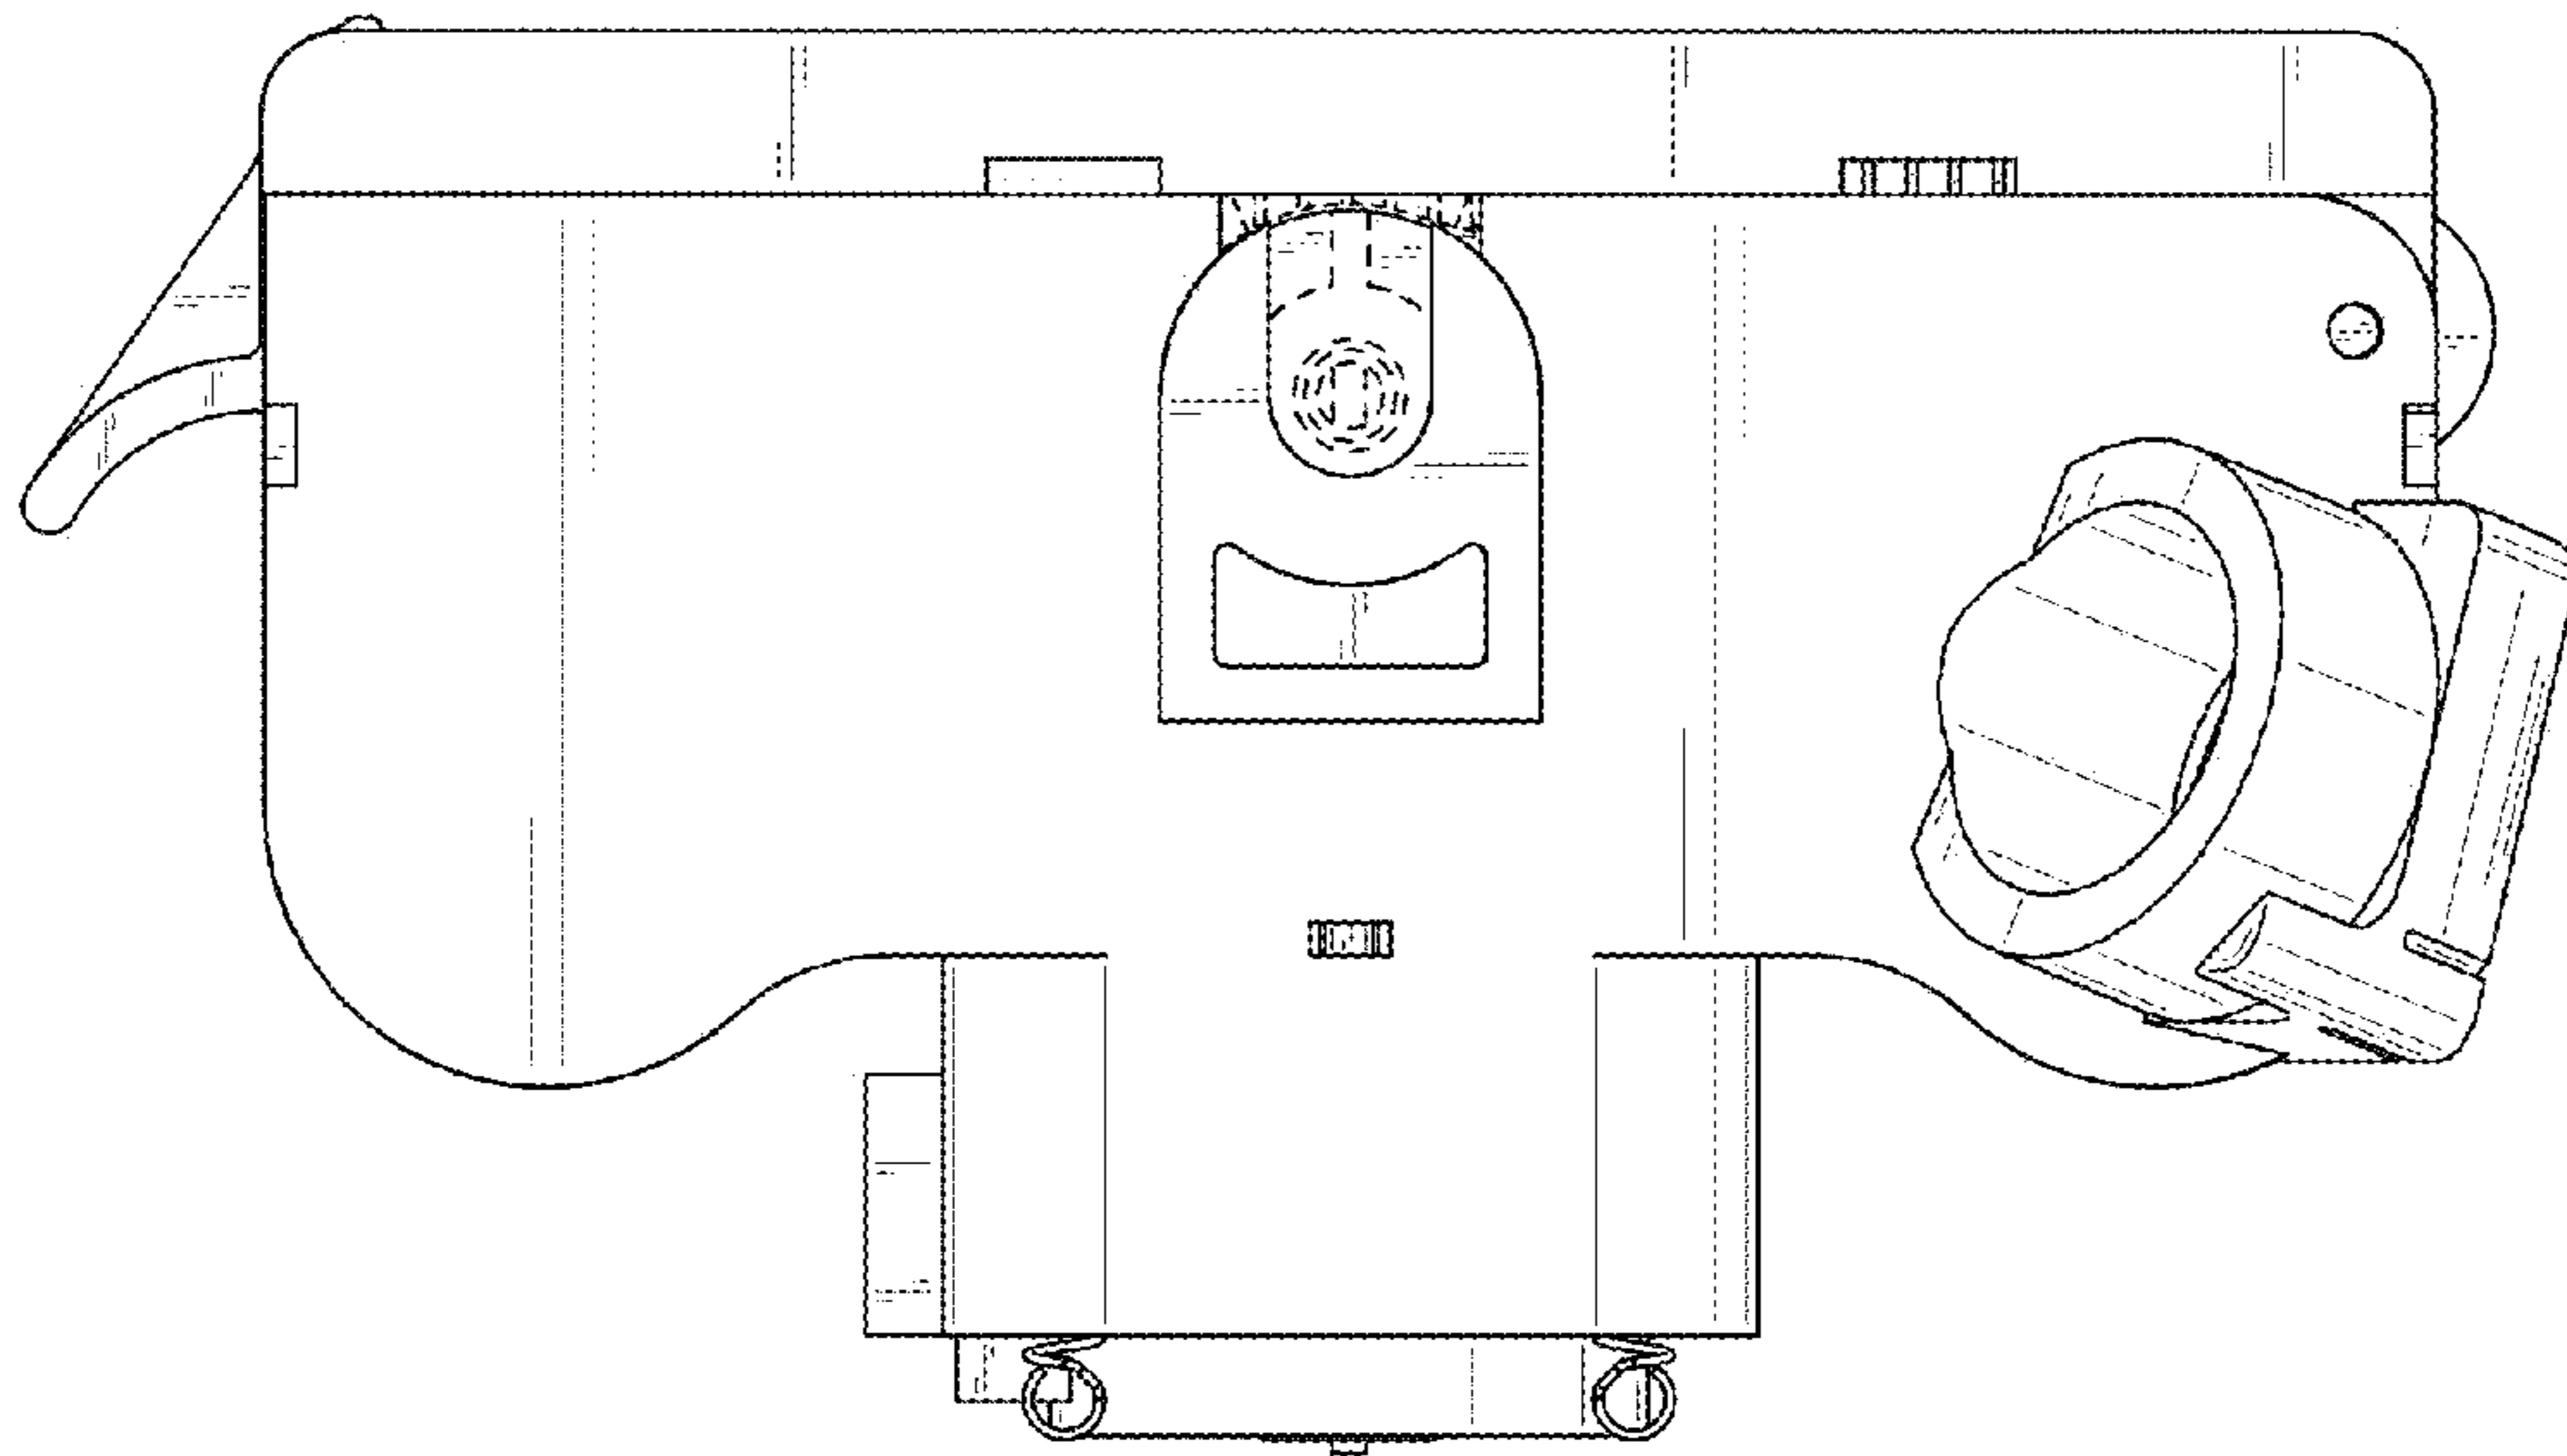


FIG. 4



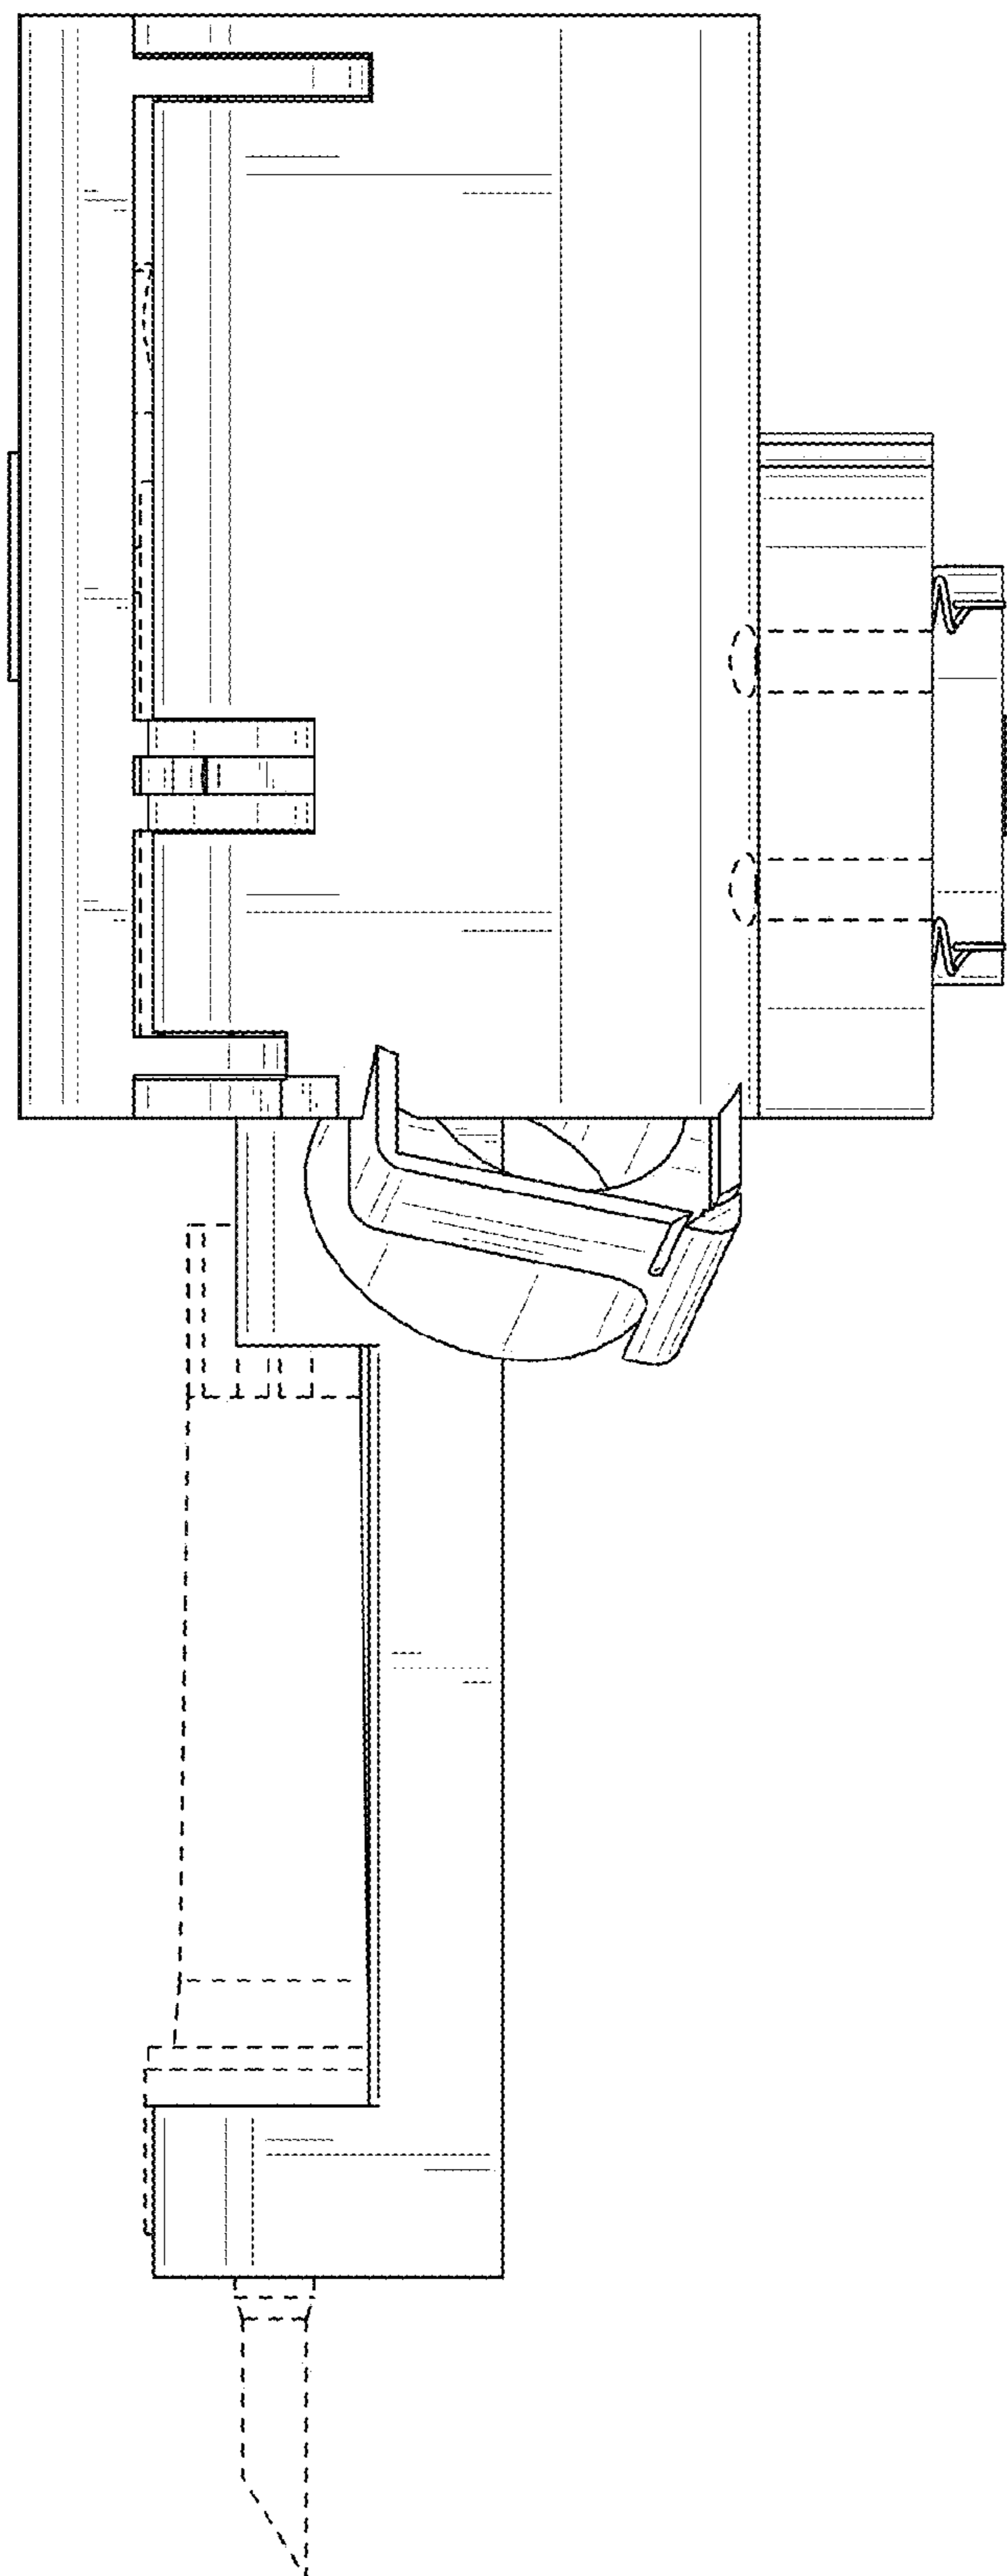


FIG. 5

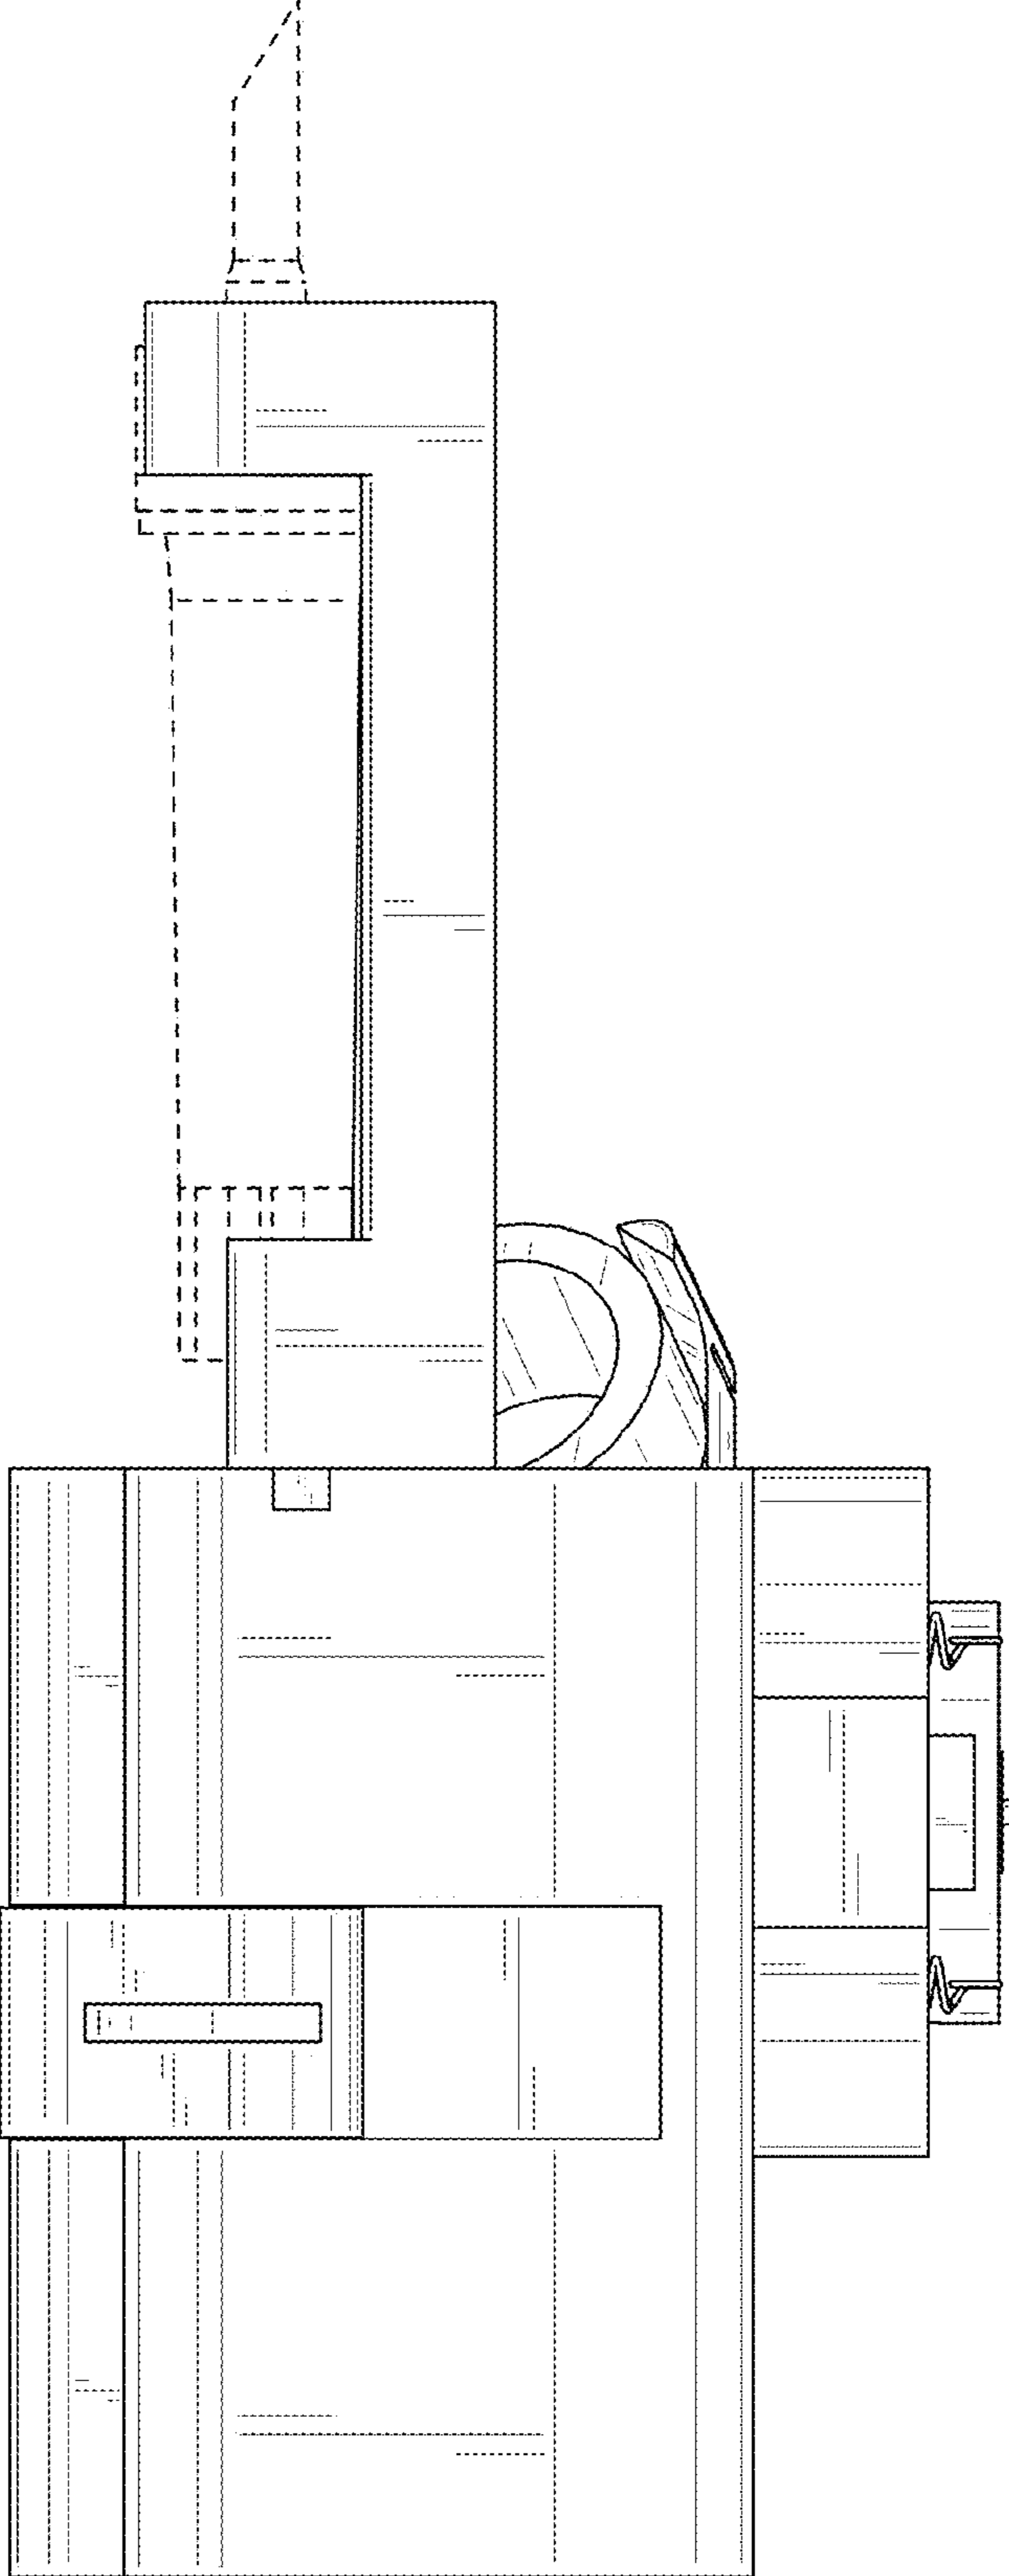


FIG. 6

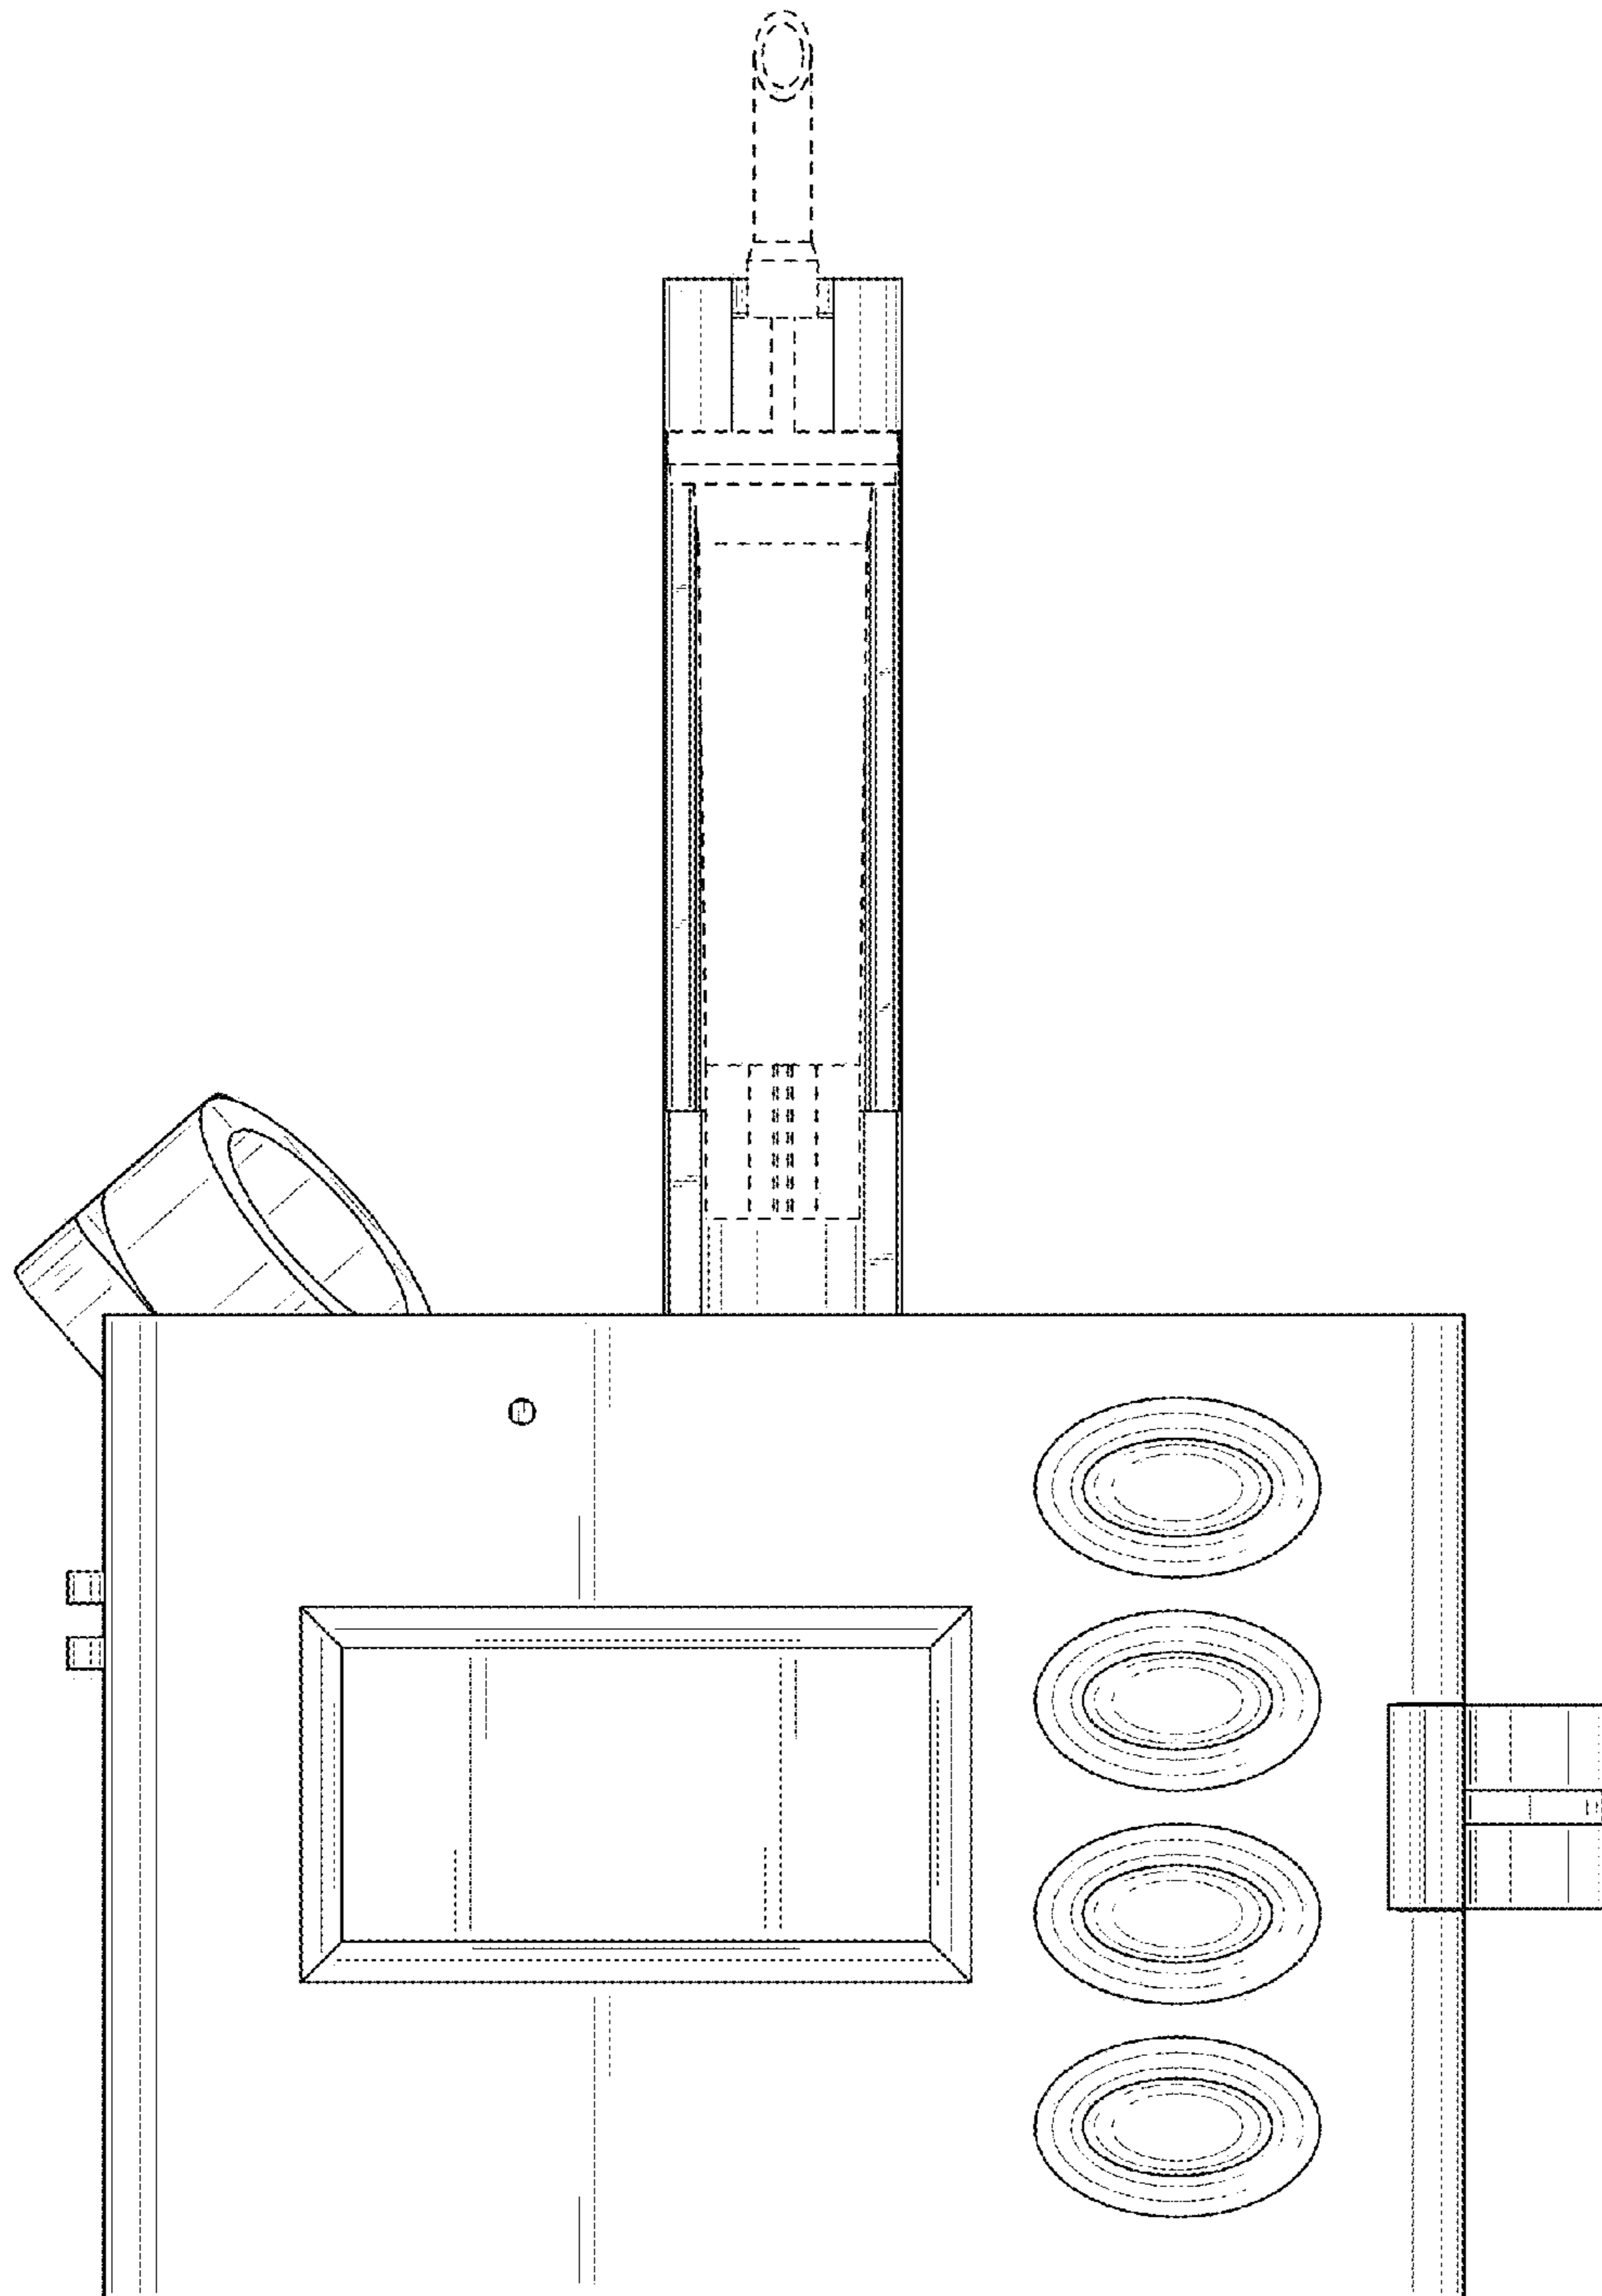


FIG. 7

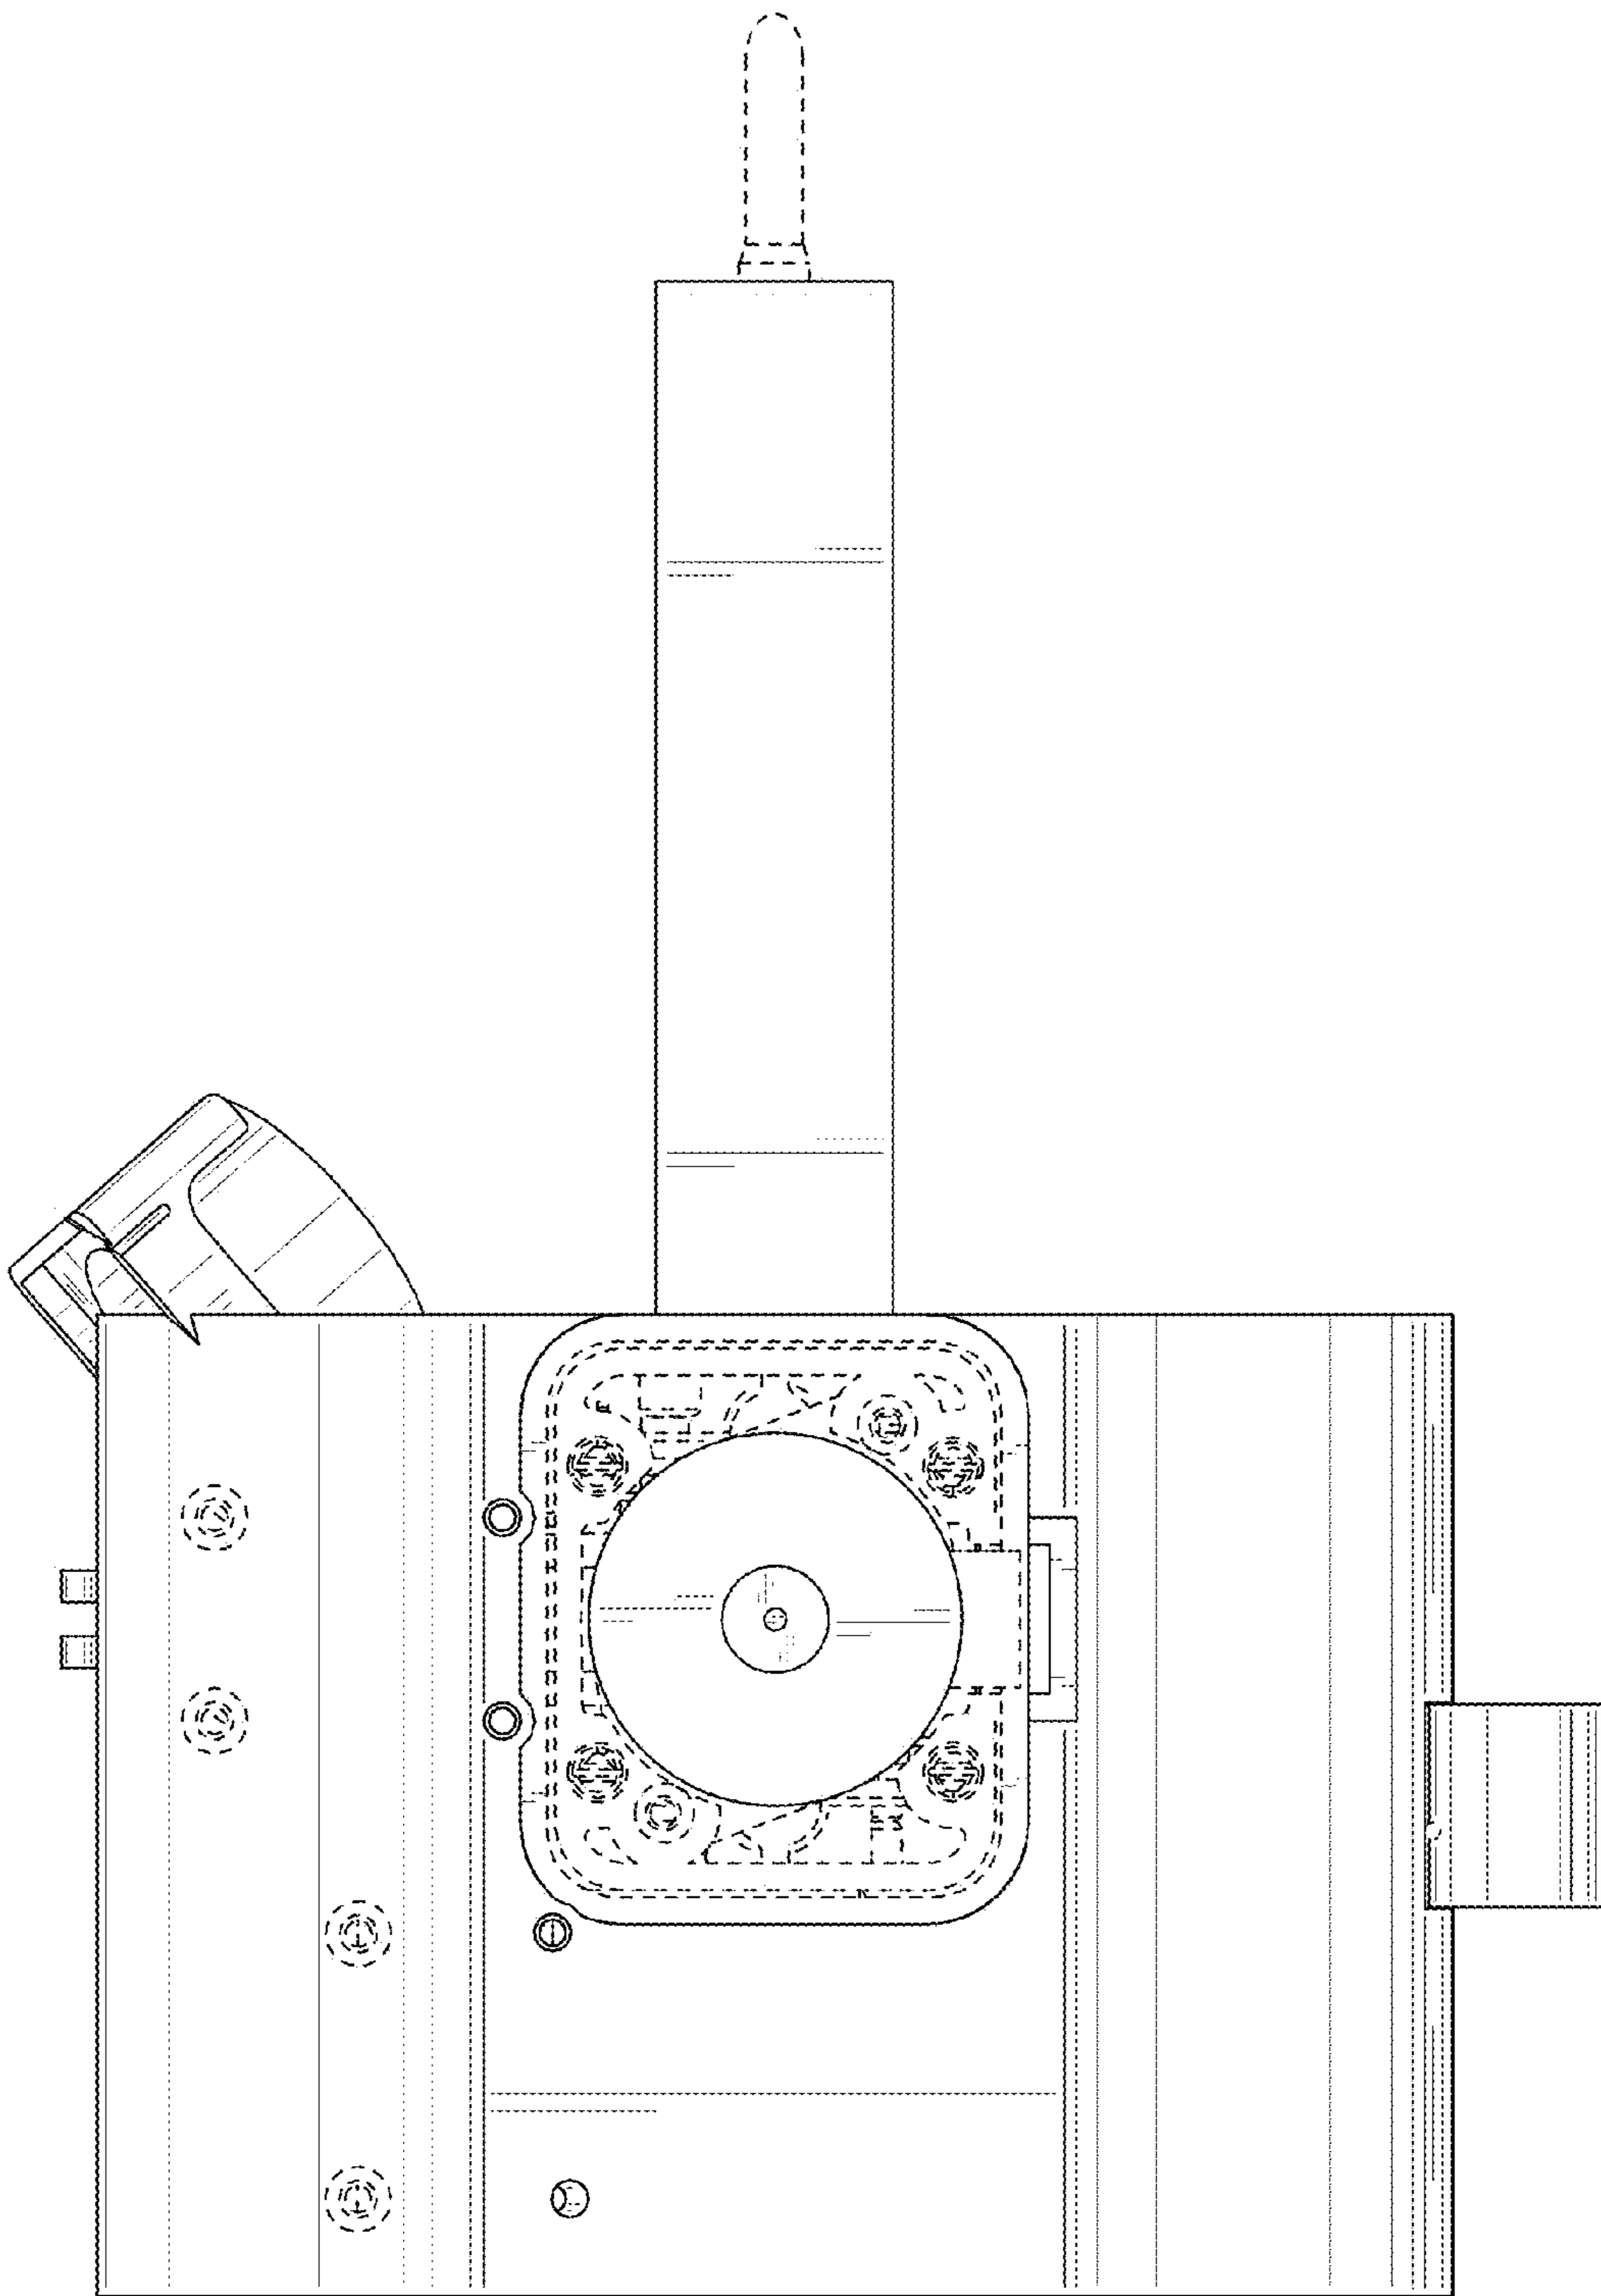


FIG. 8