



US00D756363S

(12) **United States Design Patent**  
**Mathis et al.**

(10) **Patent No.:** **US D756,363 S**

(45) **Date of Patent:** **\*\* May 17, 2016**

(54) **DISPLAY FOR USE WITH PEN-TYPE INJECTION DEVICE**

(71) Applicant: **Sanofi-Aventis Deutschland GmbH**,  
Frankfurt am Main (DE)

(72) Inventors: **Jan Mathis**, Vienna (AT); **Nik Pelzl**,  
Vienna (AT)

(73) Assignee: **SANOFI-AVENTIS DEUTSCHLAND GMBH**,  
Frankfurt am Main (DE)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/536,761**

(22) Filed: **Aug. 19, 2015**

**Related U.S. Application Data**

(62) Division of application No. 29/481,184, filed on Feb. 3, 2014.

(30) **Foreign Application Priority Data**

Aug. 2, 2013 (EM) ..... 002 286 054

(51) **LOC (10) Cl.** ..... **14-02**

(52) **U.S. Cl.**  
USPC ..... **D14/432; D14/402**

(58) **Field of Classification Search**  
USPC ..... D14/372, 496, 432, 371, 125, 126, 129,  
D14/299; D16/300-342; 351/158, 153, 144;  
345/7-9, 905; 455/344; 348/115, 53,  
348/121, 739

CPC ..... G02B 27/017; G02B 27/0158; G02B  
27/0161; G02B 27/0181; G02B 27/0185;  
G02B 27/0189

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D352,930	S	*	11/1994	Tsuji	.....	D13/168
D392,959	S	*	3/1998	Edwards	.....	D14/402
5,788,195	A	*	8/1998	Rice	.....	G06F 3/039 248/118.5
D410,638	S	*	6/1999	Sheehan	.....	D14/409
D630,213	S	*	1/2011	Fidali	.....	D14/402
D654,918	S	*	2/2012	Cheng	.....	D14/402
D696,668	S	*	12/2013	Chen	.....	D14/402
D697,914	S	*	1/2014	Bates	.....	D14/402
D718,309	S	*	11/2014	Roberts	.....	D14/402
D743,963	S	*	11/2015	Osterhout	.....	D14/402
2015/0343150	A1	*	12/2015	Draper	.....	A61M 5/31525 604/189
2015/0343152	A1	*	12/2015	Butler	.....	A61M 5/31568 604/207

\* cited by examiner

*Primary Examiner* — Austin Murphy

(74) *Attorney, Agent, or Firm* — Scully, Scott, Murphy & Presser, P.C.


(57) **CLAIM**

The ornamental design for a display for use with pen-type injection device, as shown.

**DESCRIPTION**

FIG. 1 is a perspective view of a display for use with pen-type injection device, showing our new design;  
FIG. 2 is a side view of FIG. 1;  
FIG. 3 is an opposite view of FIG. 1;  
FIG. 4 is a back view of FIG. 1; and,  
FIG. 5 is a top view of FIG. 1.

**1 Claim, 5 Drawing Sheets**

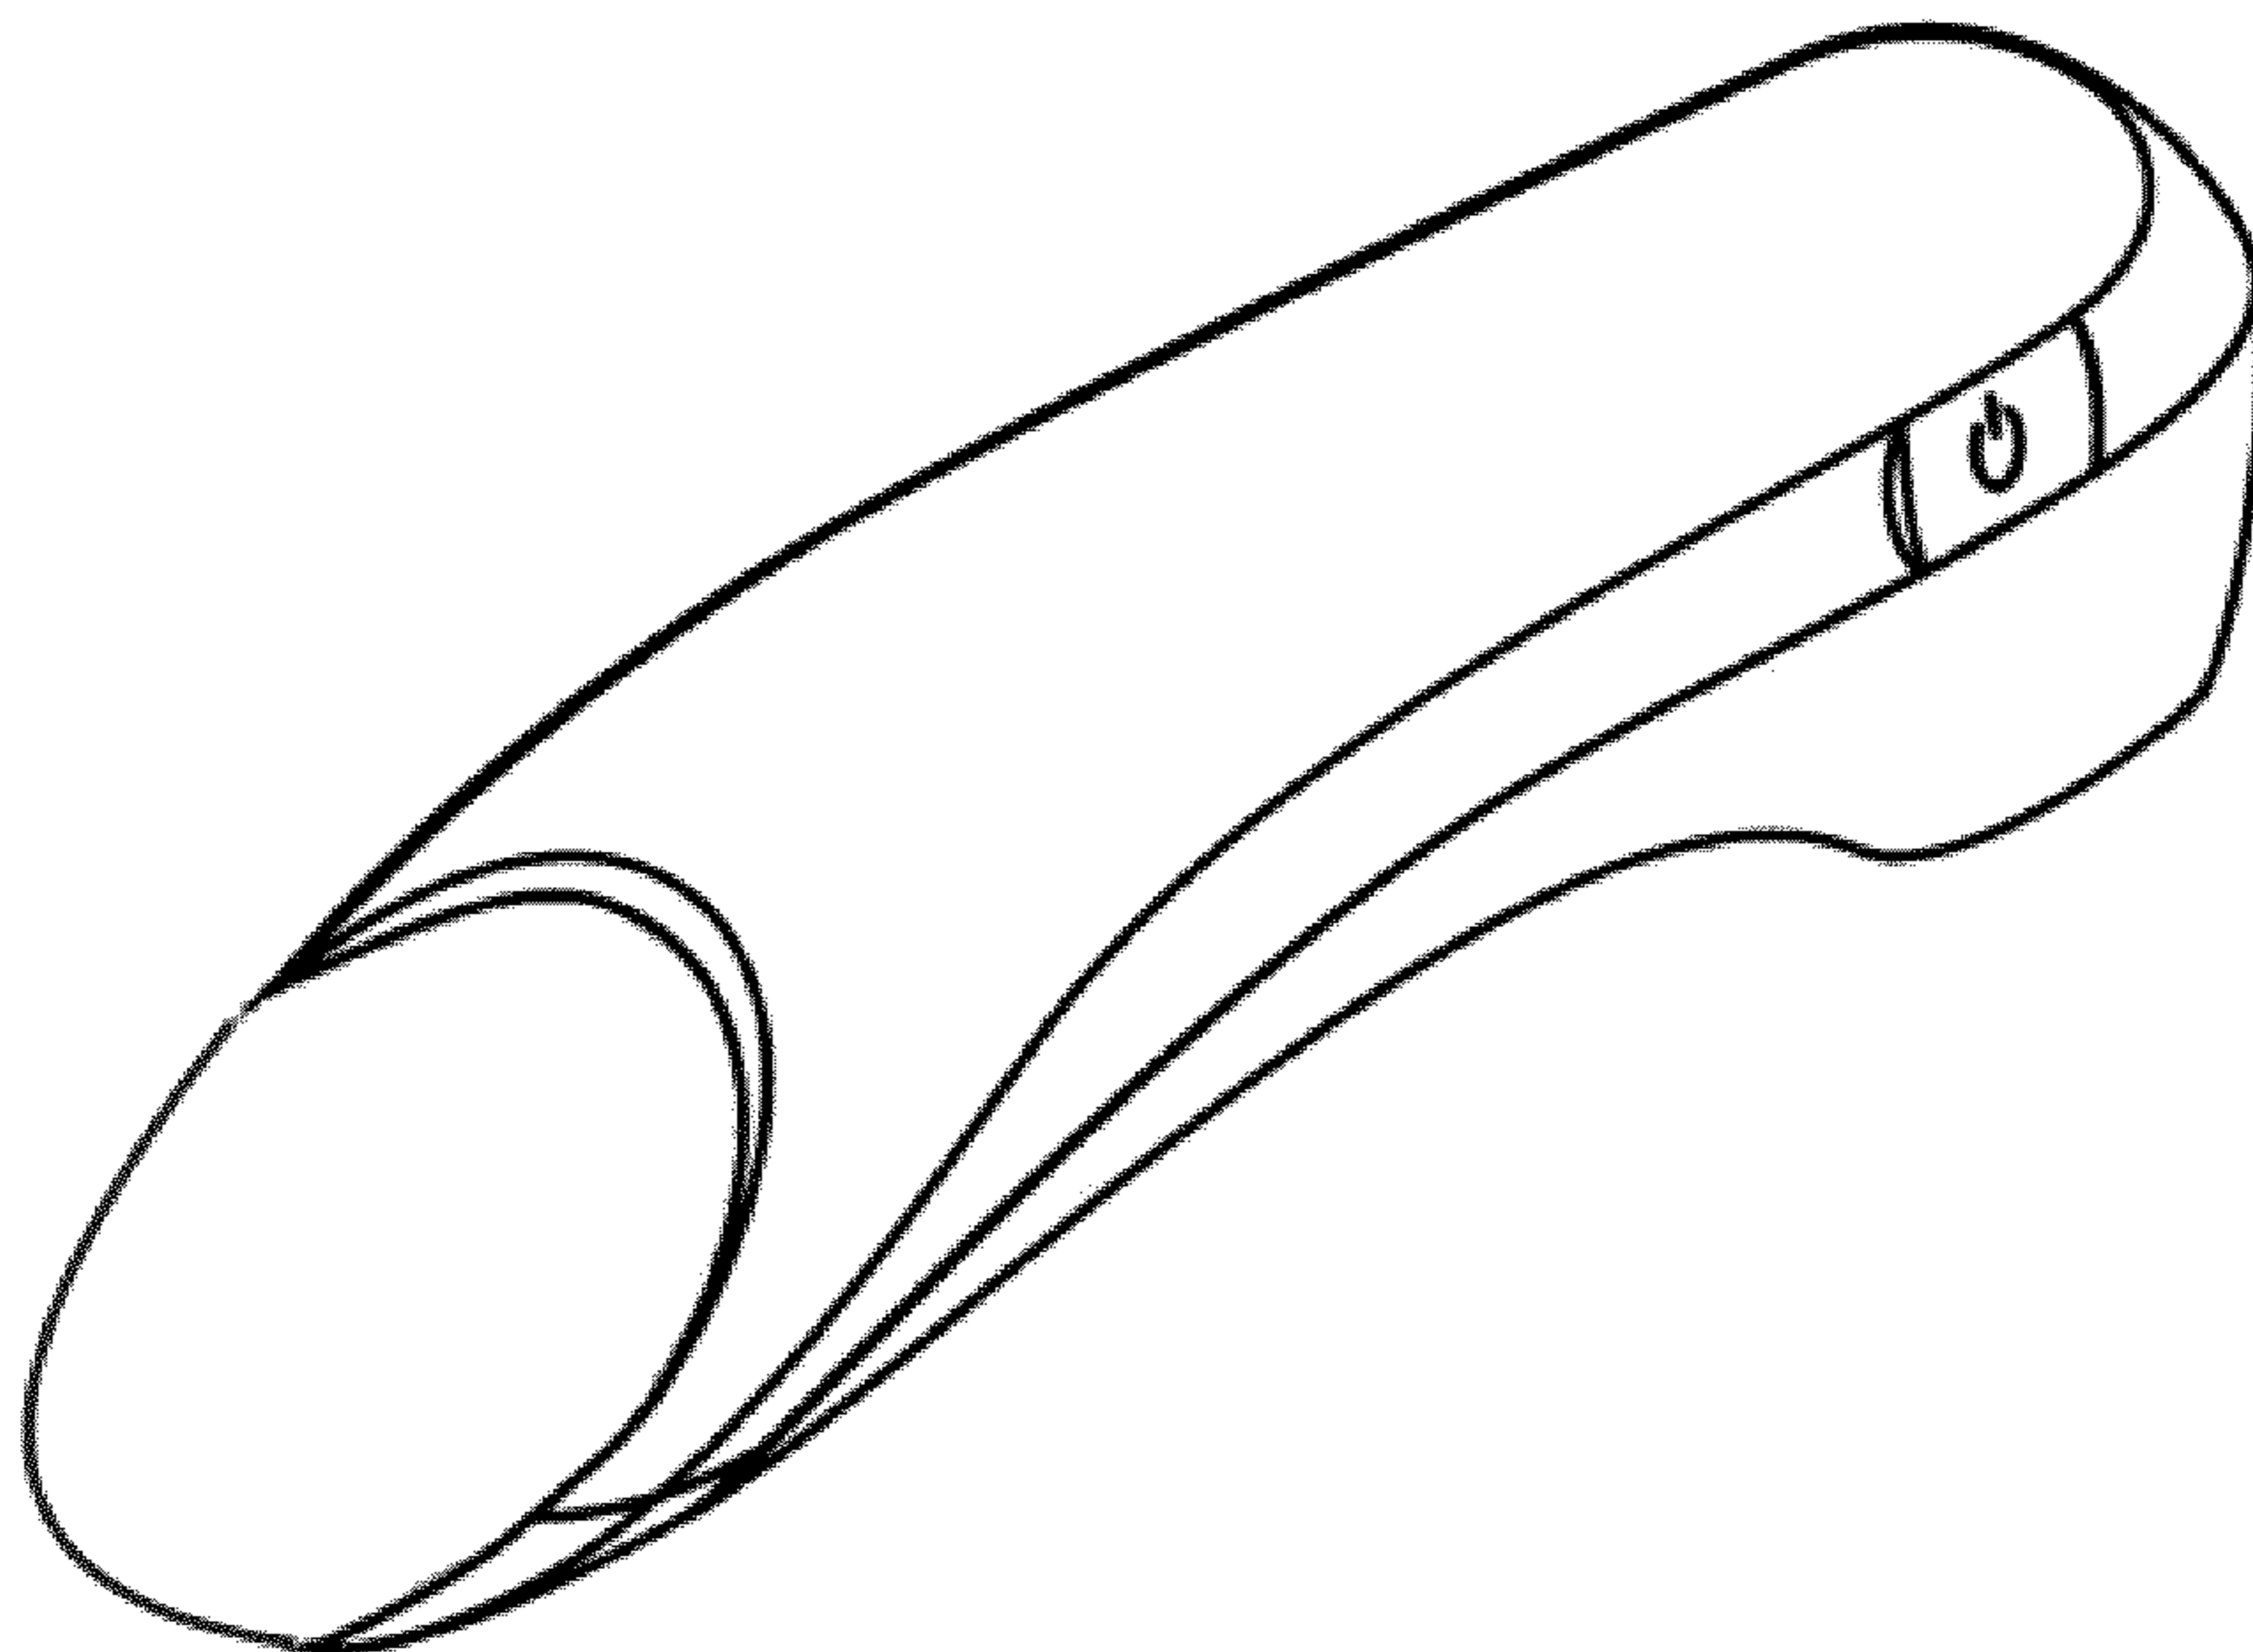

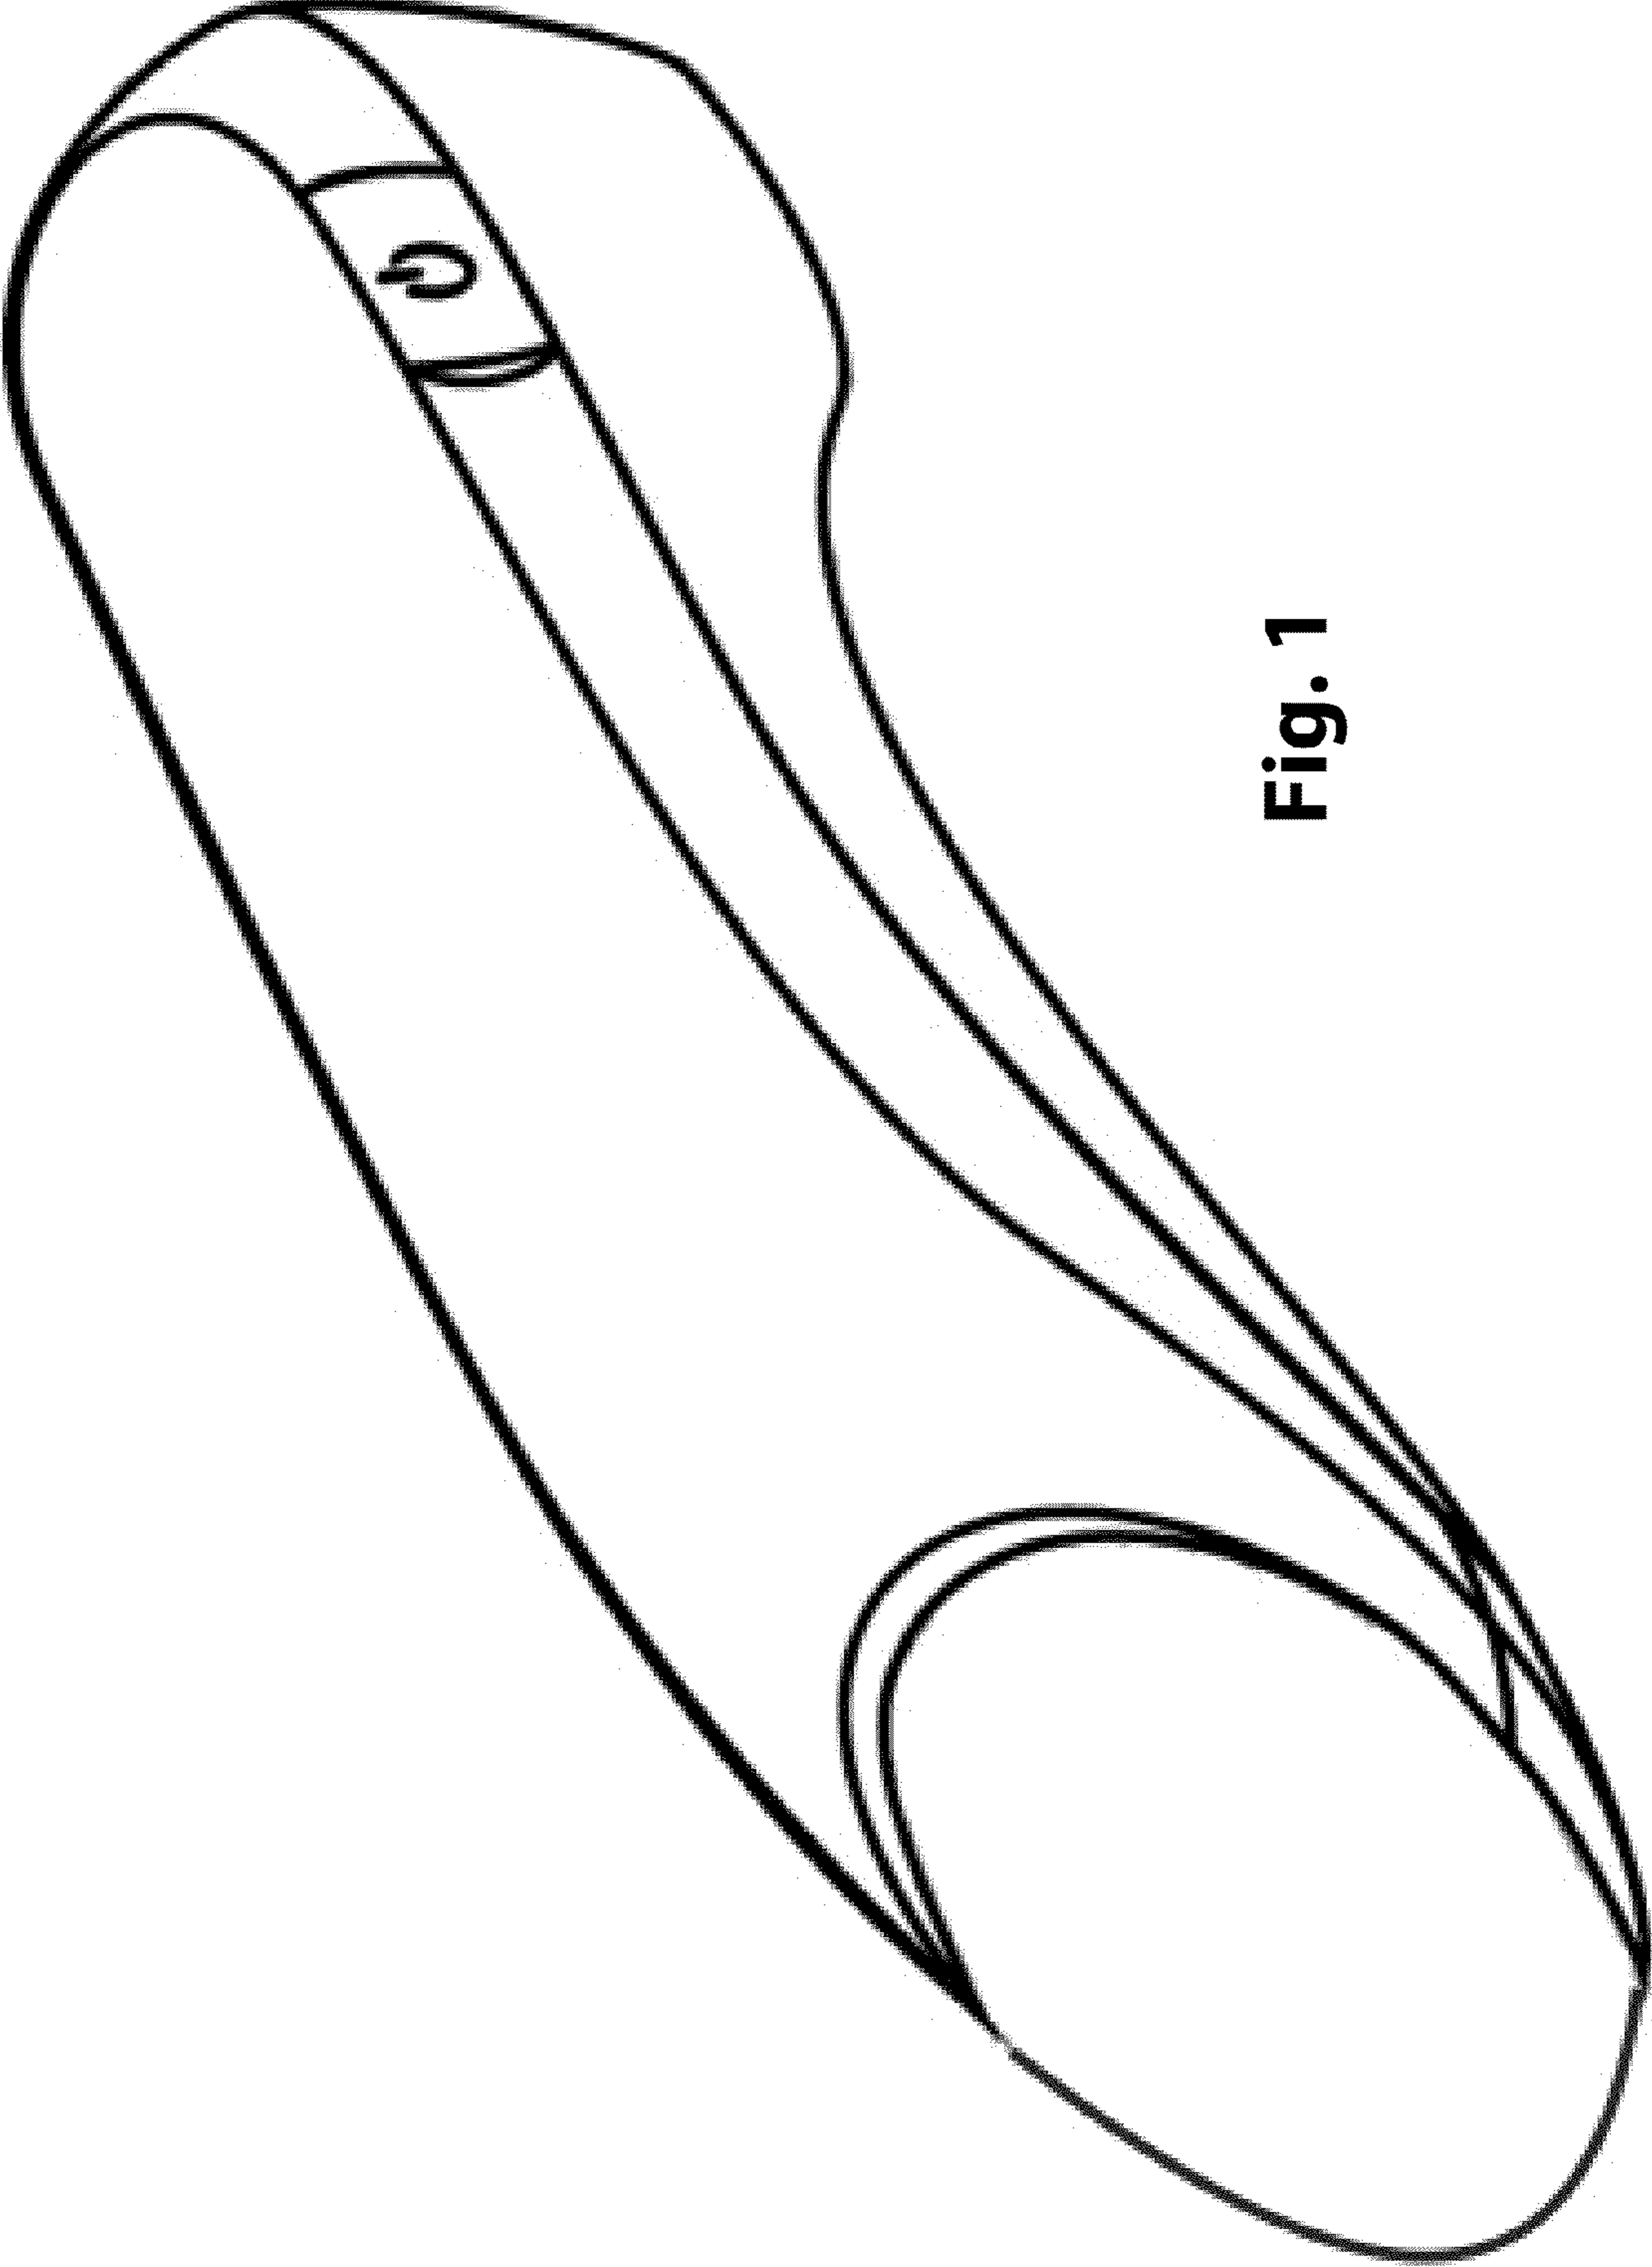


Fig. 1



Fig. 2



Fig. 3

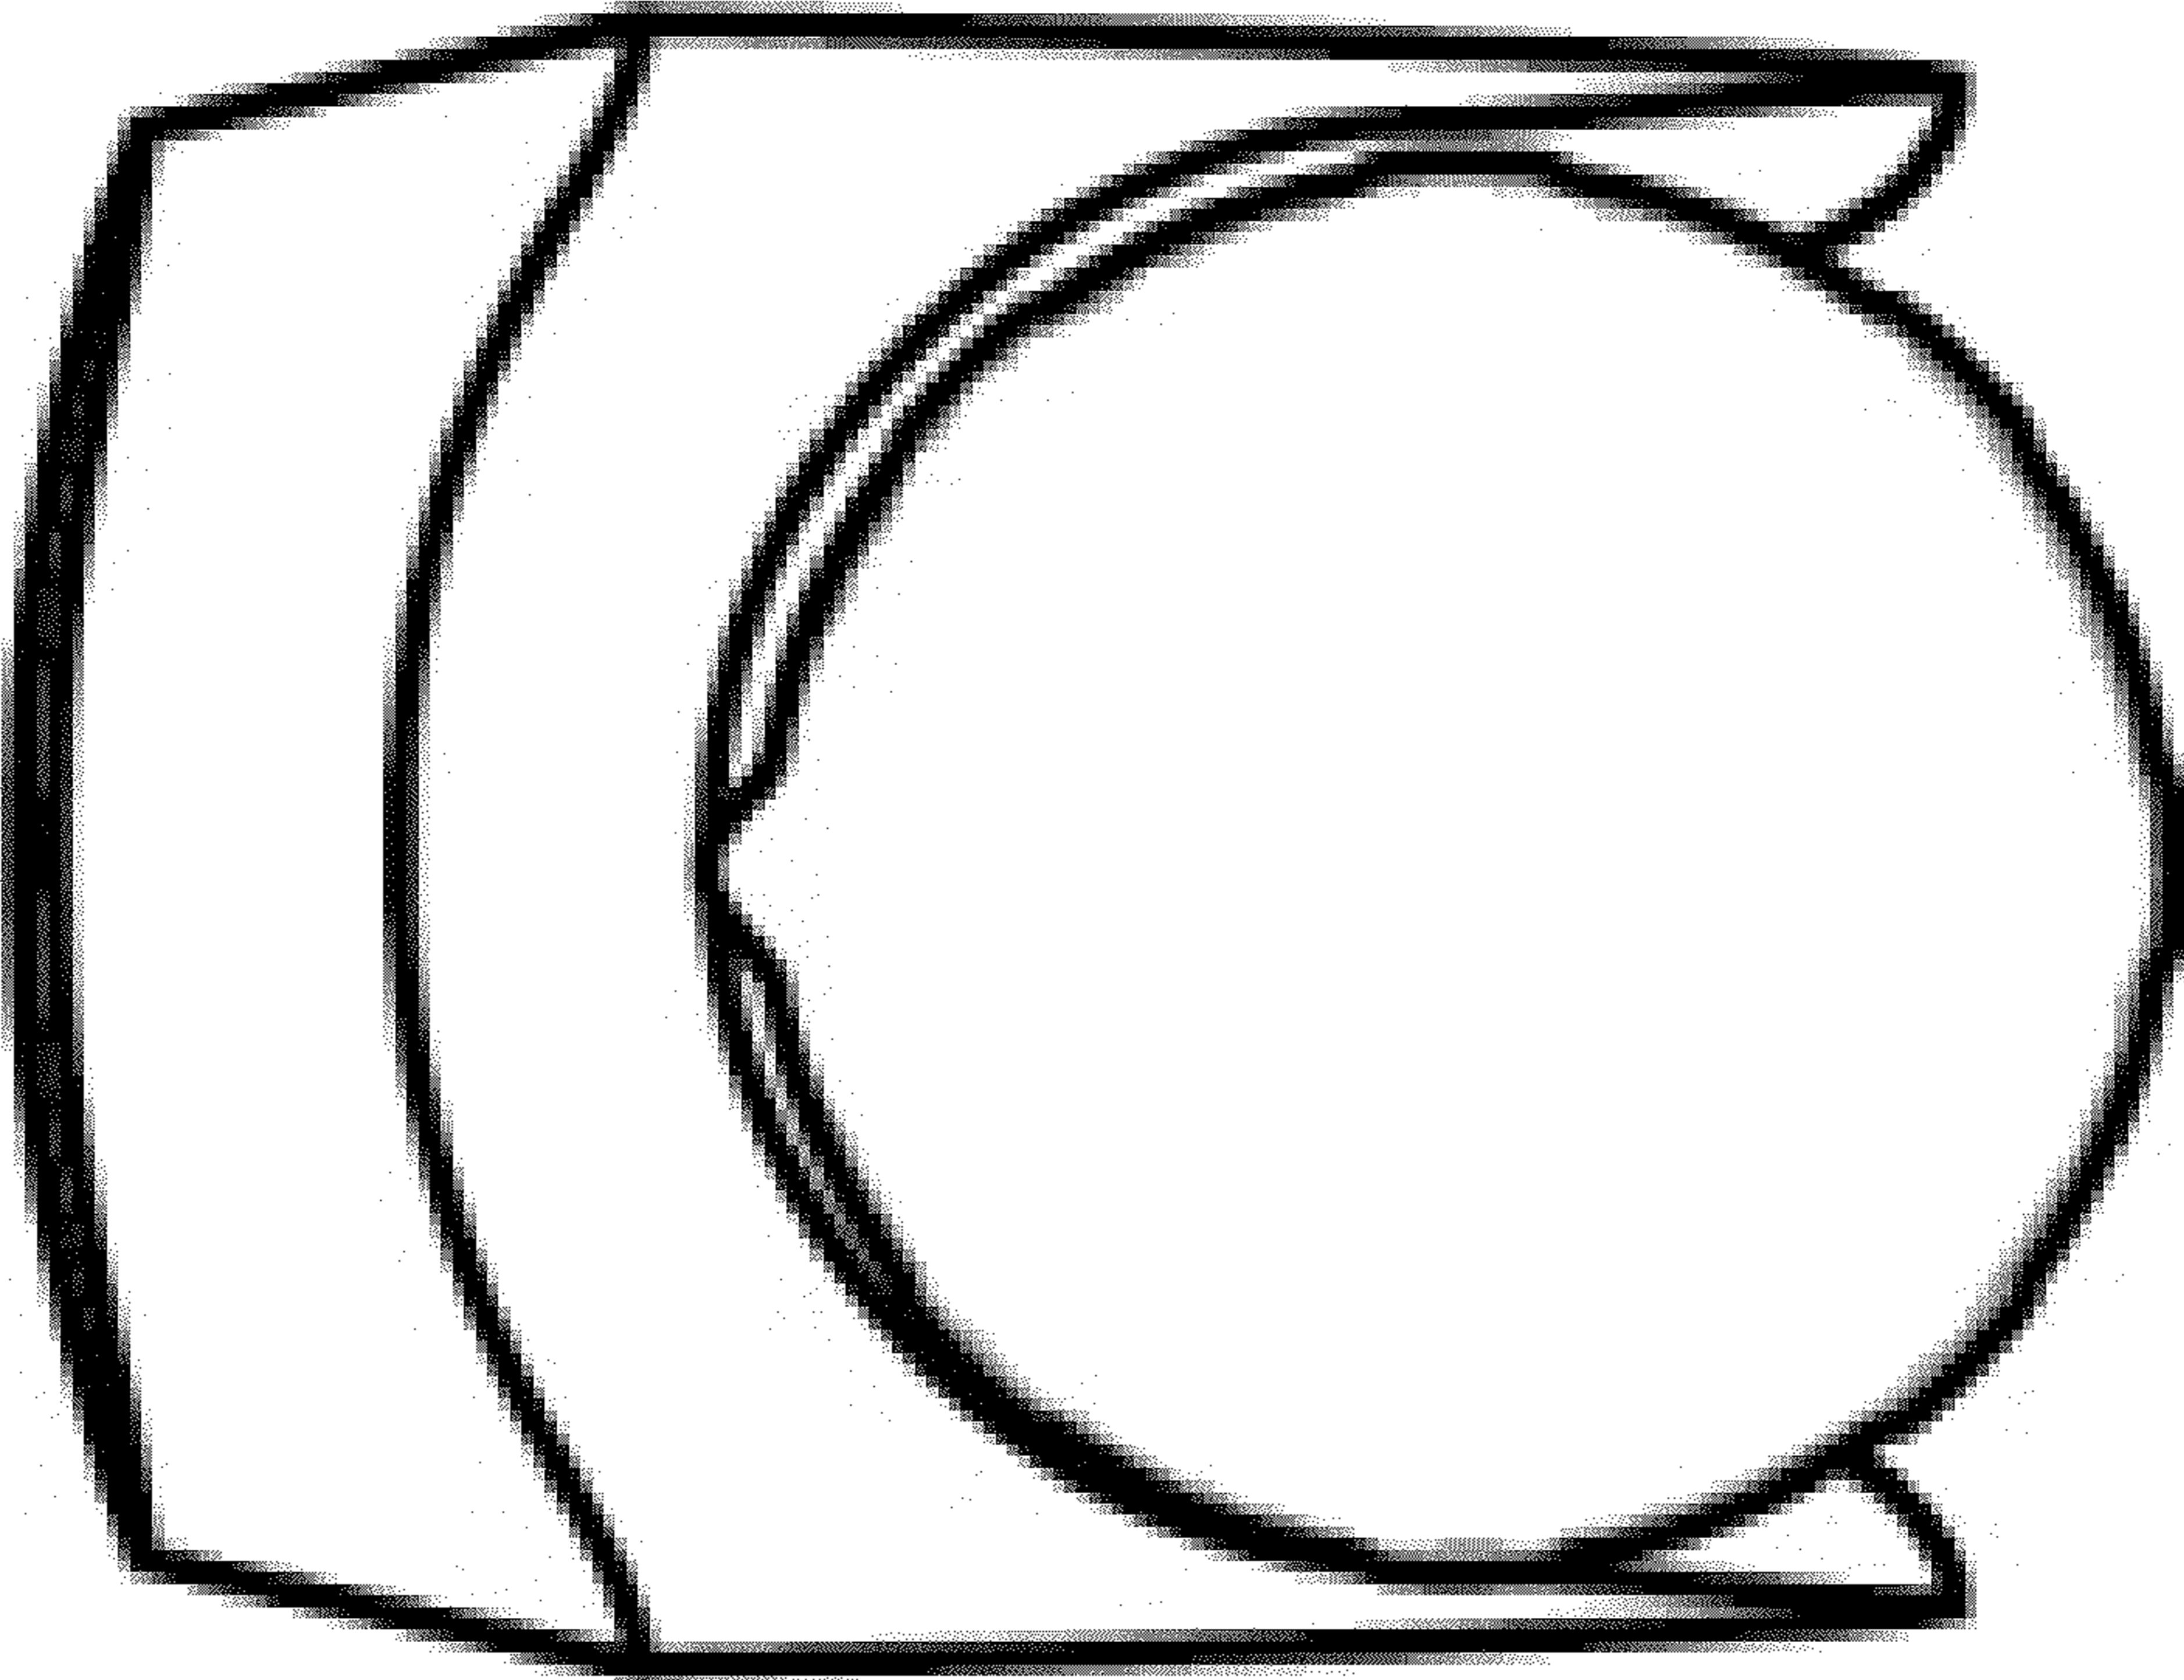


Fig. 4

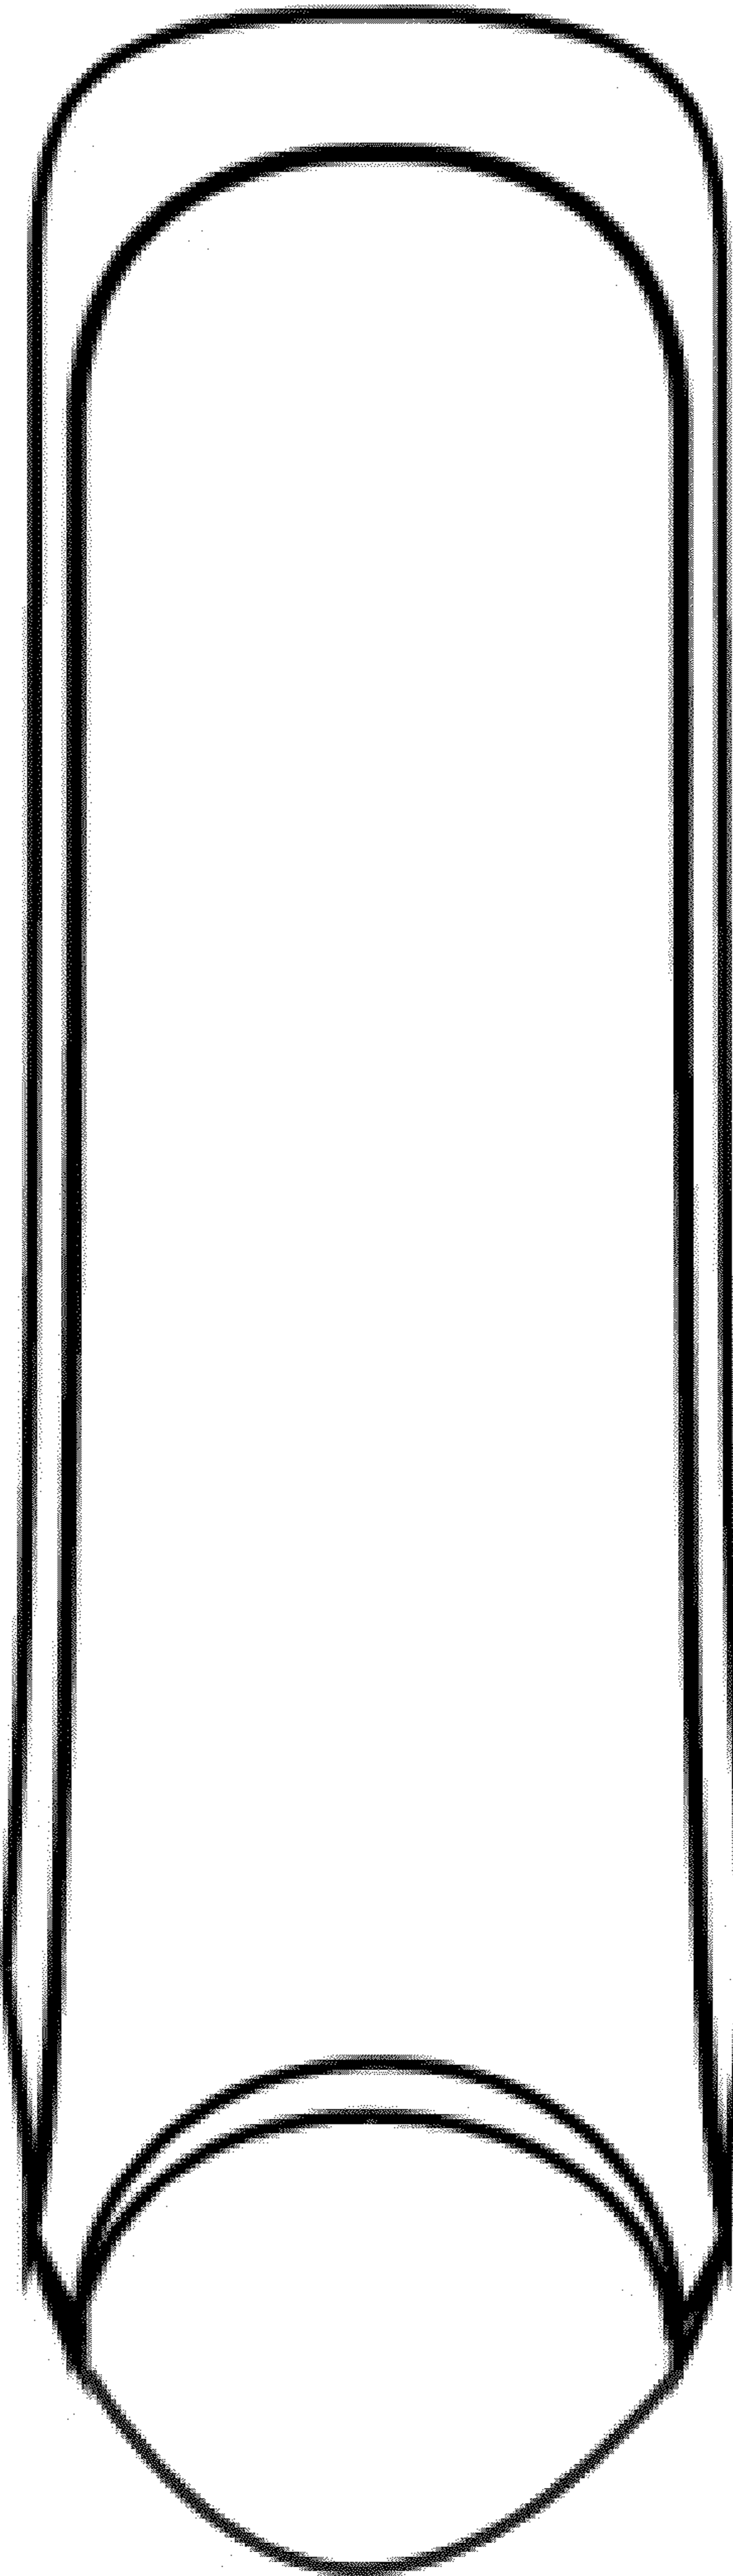


Fig. 5