

US00D758583S

(12) **United States Design Patent**
Matyas et al.

(10) **Patent No.:** **US D758,583 S**
(45) **Date of Patent:** **** Jun. 7, 2016**

- (54) **BROACH**
- (71) Applicant: **DEPUY SYNTHES PRODUCTS, INC.**, Raynham, MA (US)
- (72) Inventors: **Aaron J. Matyas**, Fort Wayne, IN (US);
Rebecca L. Chaney, Warsaw, IN (US);
Craig S. Tsukayama, Fort Wayne, IN (US)
- (73) Assignee: **DEPUY (IRELAND)**, Ringaskiddy (IE)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/457,174**
- (22) Filed: **Jun. 7, 2013**
- (51) **LOC (10) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/147**
- (58) **Field of Classification Search**
USPC D24/146, 147, 130, 133, 155, 156;
606/79, 80, 85, 86 R, 87, 88, 89, 96,
606/105, 916
CPC A61B 17/3421; A61B 2017/345;
A61B 2017/3452; A61B 2017/3437; A61B
17/34; A61B 2017/3407; A61B 2017/3409;
A61B 2017/1602; A61B 17/1764
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D446,859 S *	8/2001	Hurson	D24/156
D458,373 S *	6/2002	Jackson	D24/155
D470,939 S *	2/2003	Daftary	D24/156
6,626,911 B1 *	9/2003	Engman et al.	606/916
D507,650 S *	7/2005	Teich	D24/156
D524,942 S *	7/2006	Felix	D24/155
D577,121 S *	9/2008	Nishida et al.	D24/155
D588,699 S *	3/2009	Aldecoa	D24/156

D620,117 S *	7/2010	Dawson et al.	D24/156
D621,047 S *	8/2010	Strobel et al.	D24/155
D659,247 S *	5/2012	Lussi et al.	D24/156
D666,295 S *	8/2012	Hung	D24/156
D667,955 S *	9/2012	Spahn	D24/156
D717,436 S *	11/2014	Park	D24/156
D732,669 S *	6/2015	Fisler et al.	D24/156
2009/0125114 A1	5/2009	May et al.		

(Continued)

OTHER PUBLICATIONS

Zimmer NexGen LCCK, Surgical Technique for use with LCCK 4-in-1 Instrument, 2009, 52 pages.

(Continued)

Primary Examiner — Ian Simmons

Assistant Examiner — Carissa C Fitts

(74) *Attorney, Agent, or Firm* — Barnes & Thornburg LLP


(57) **CLAIM**

We claim the ornamental design for a broach, as shown and described.

DESCRIPTION

FIG. 1 is a top-front perspective view of a design of the broach;
 FIG. 2 is a front elevation view of the broach of FIG. 1;
 FIG. 3 is a rear elevation view of the broach of FIG. 1;
 FIG. 4 is a top plan view of the broach of FIG. 1;
 FIG. 5 is a bottom plan view of the broach of FIG. 1;
 FIG. 6 is a first side elevation view of the broach of FIG. 1;
 and,
 FIG. 7 is a second side elevation view the broach of FIG. 1.
 The broken lines represent unclaimed portions of the article and form no part of the claimed design. The dash-dot-dot-dash broken line in FIG. 1 indicates a boundary of claimed subject matter.

1 Claim, 4 Drawing Sheets

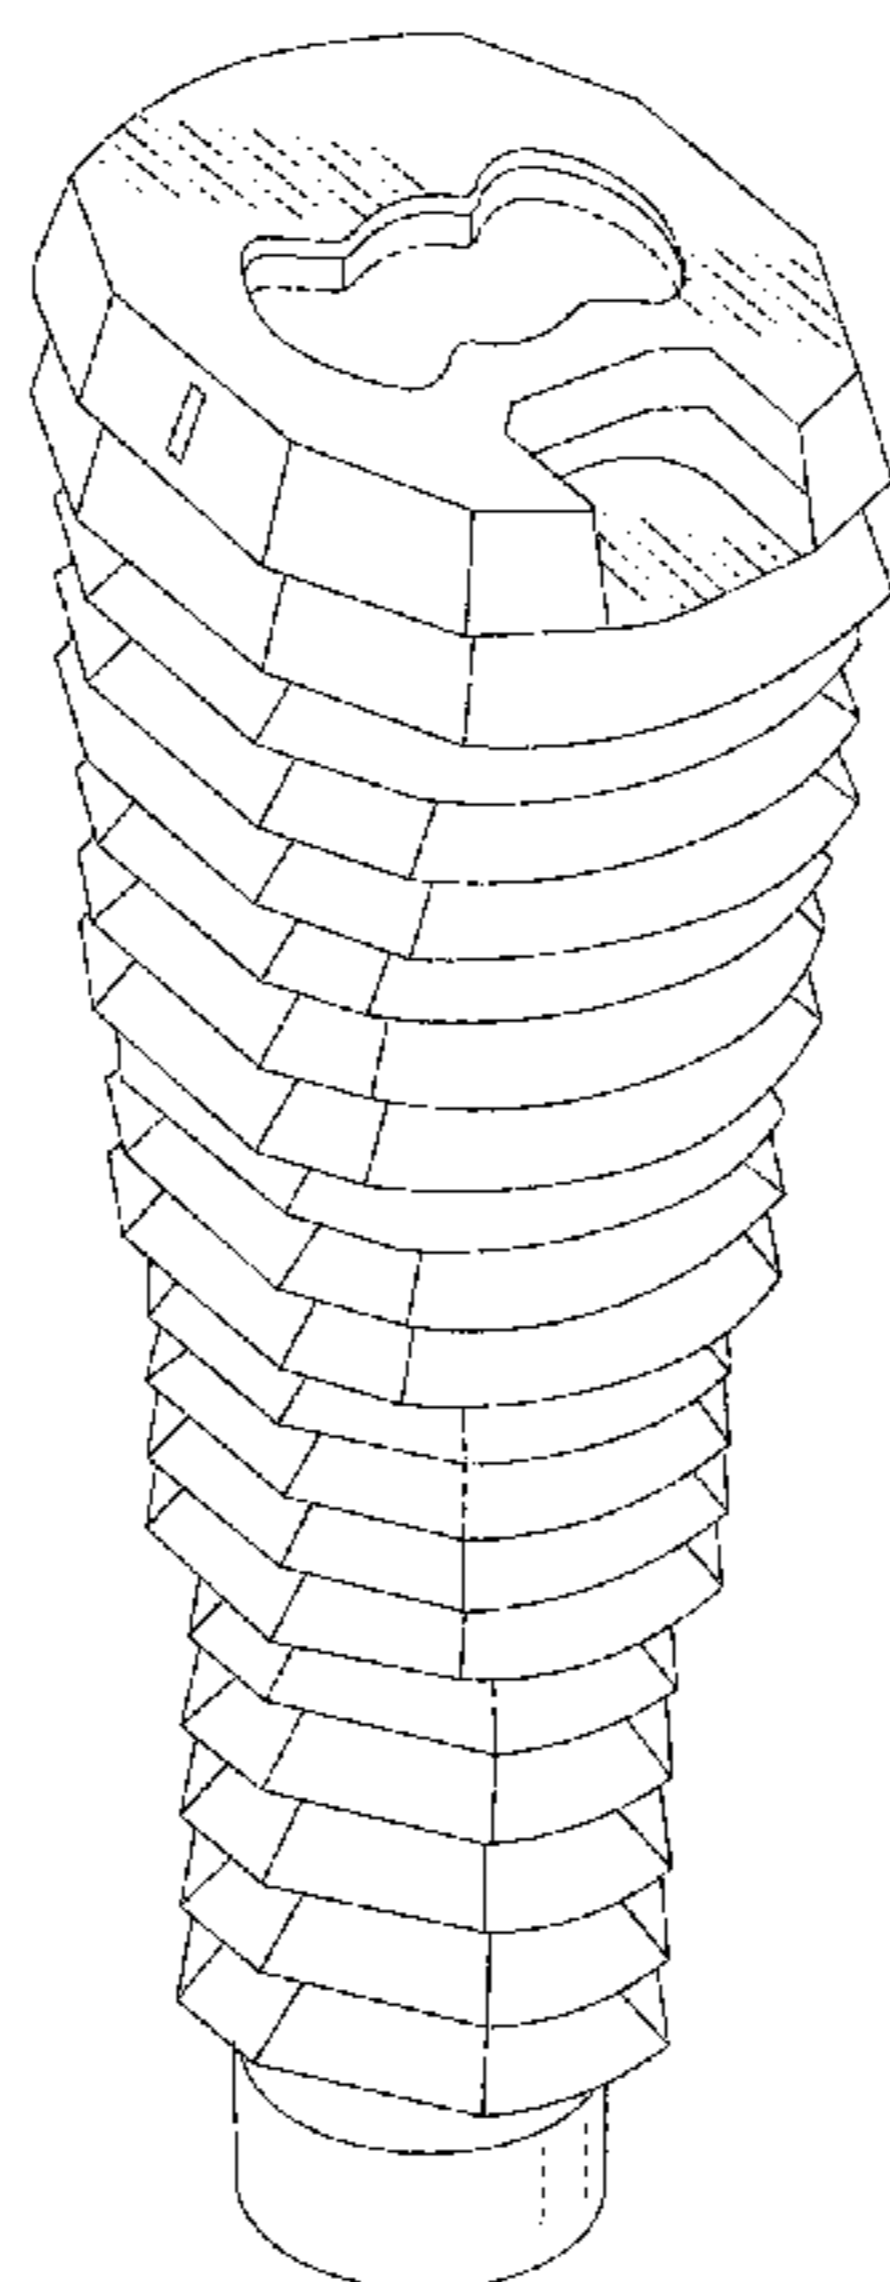

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0325014 A1 12/2013 Sordelet et al.
2013/0325016 A1 12/2013 Sordelet et al.
2013/0325018 A1 12/2013 Thomas et al.
2013/0325019 A1 12/2013 Thomas et al.
2013/0325021 A1 12/2013 Sordelet et al.
2013/0325136 A1 12/2013 Thomas et al.

OTHER PUBLICATIONS

DePuy Orthopaedics, Inc., Sigma Revision and M.B.T. Revision Tray, Surgical Technique, 2008, 82 pages.

Smith & Nephew, Legion, Revision Knee System, Surgical Technique, 2005, 40 pages.

Biomet, Vanguard SSK, Revision System, Surgical Technique, Feb. 2008, 64 pages.

GMK Revision, Surgical Technique, Ref. 99.27.12US rev. 1, 1999, 74 pages.

PFC Sigma RP-F, Specialist 2 Instruments, Surgical Technique, Performance in Flexion, 2007, 32 pages.

P.F.C. Sigma Rotating Platform Knee System with M.B.T Tray, Primary Procedure with a Curved or Posterior Stabilised Implant, 2003, 43 pages.

LCS High Performance Instruments, Surgical Technique, 2008, 44 pages.

Sigma High Performance Instruments, Design Rationale, 2007, 12 pages.

Sigma High Performance Instruments, Classic Surgical Technique, 2010, 52 pages.

Attune Knee System Surgical Technique, 2013, 73 pages.

* cited by examiner

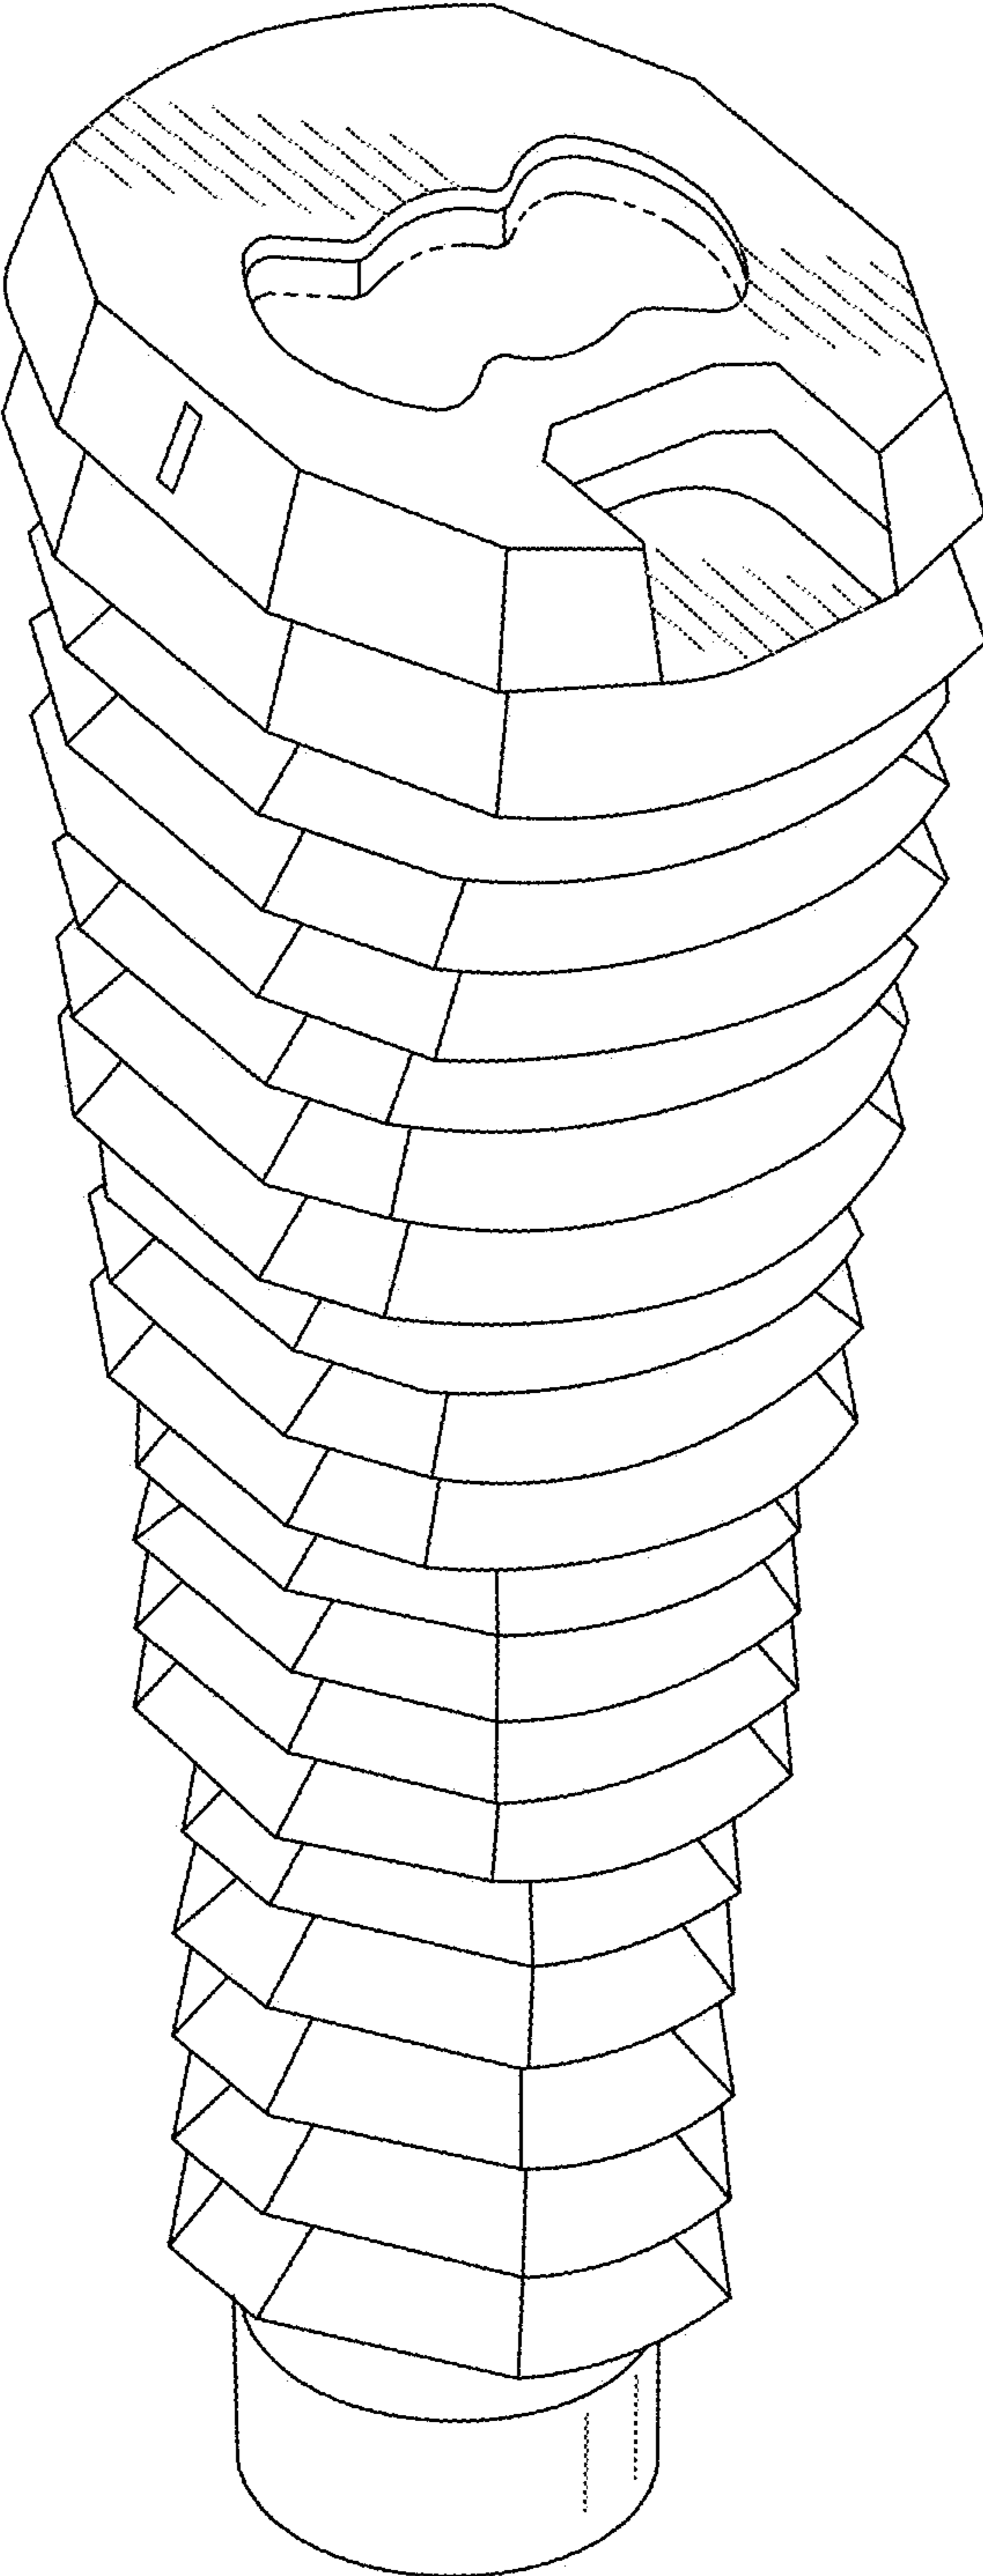


Fig. 1

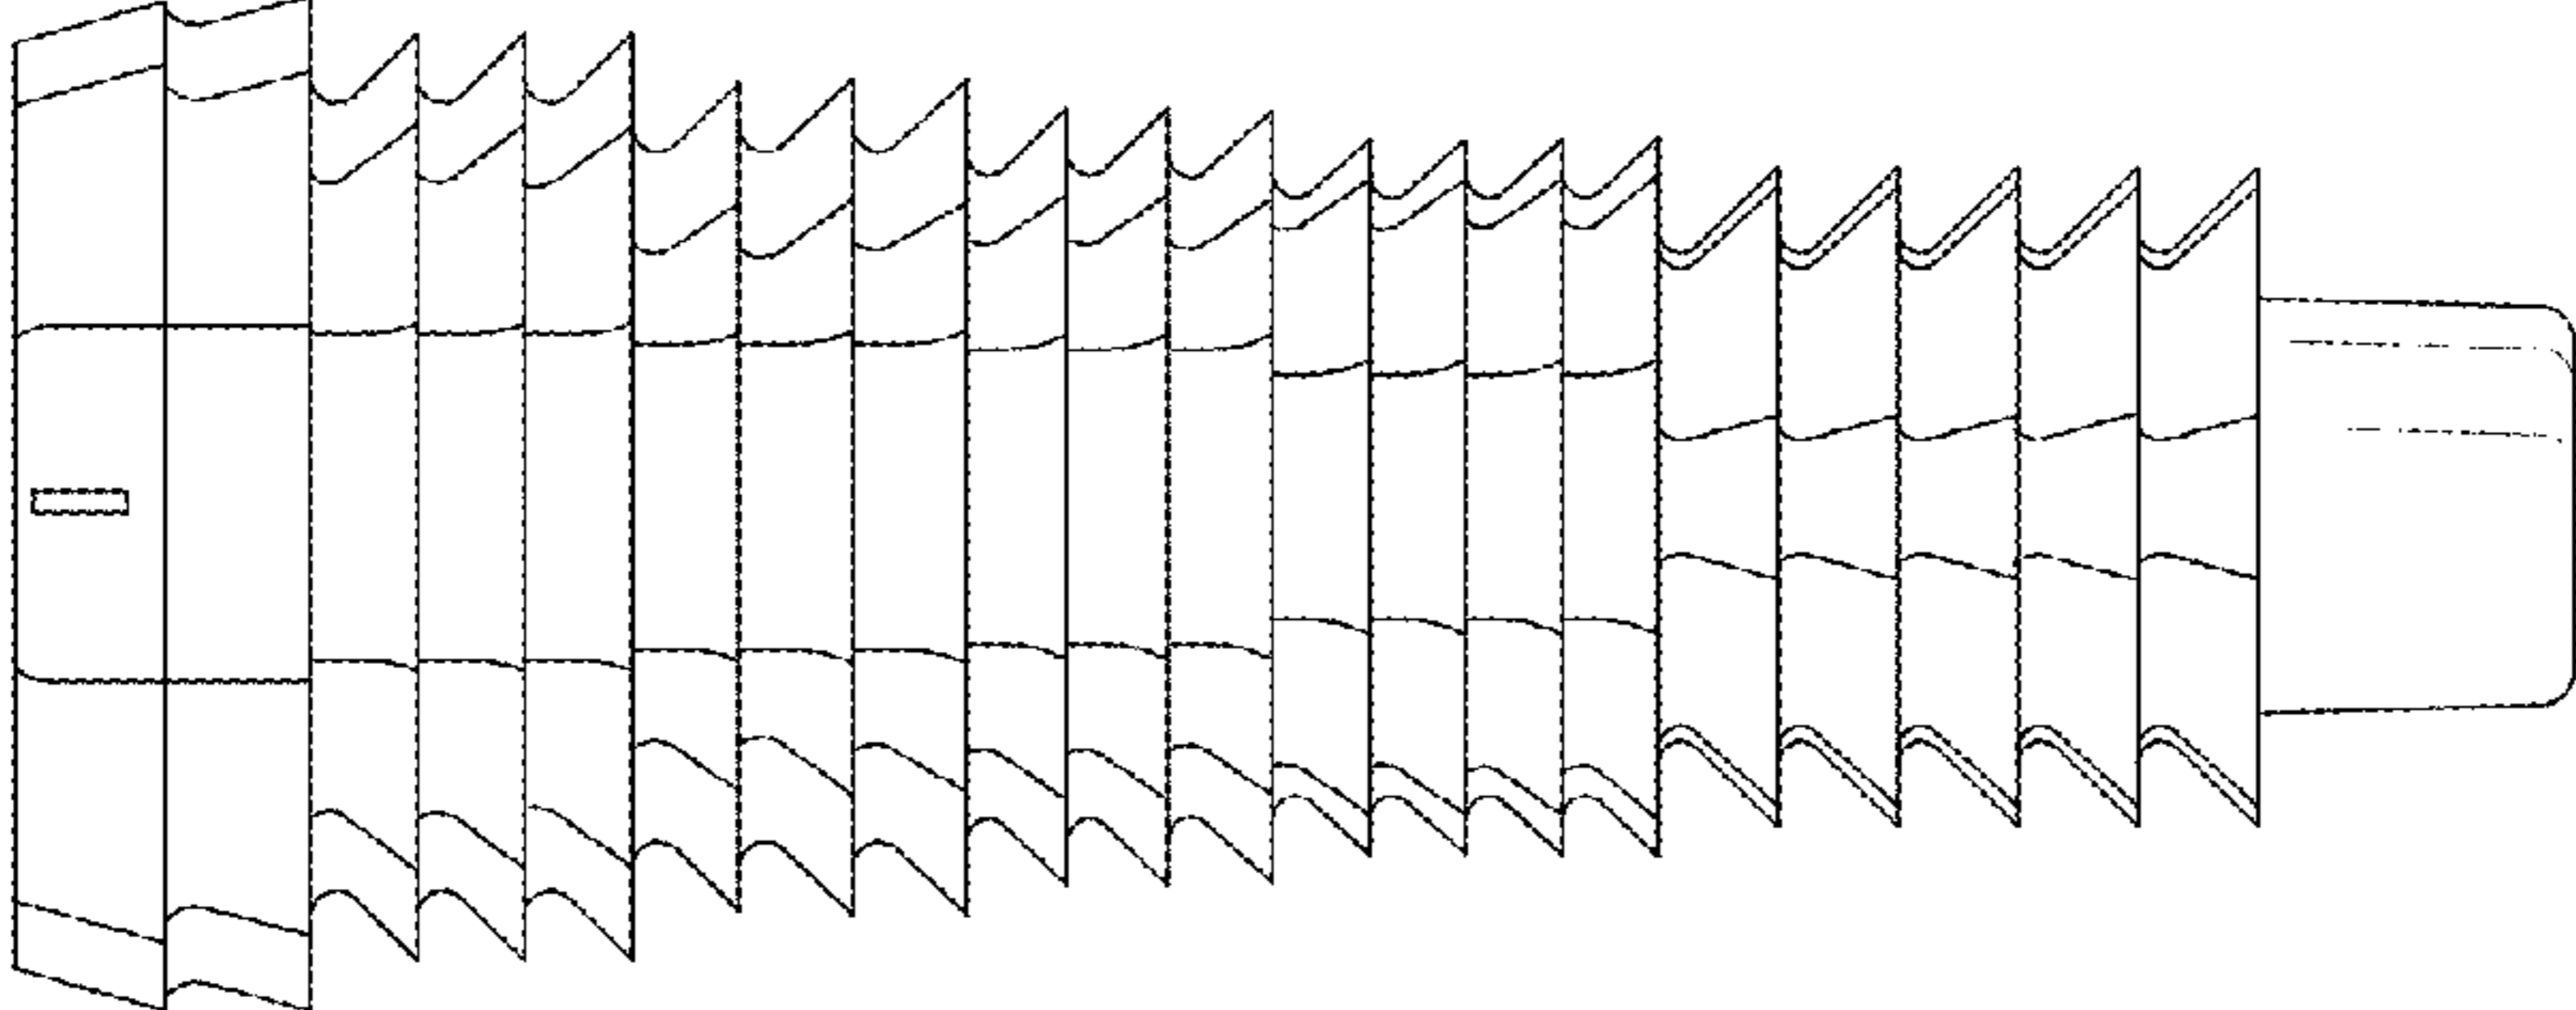


Fig. 3

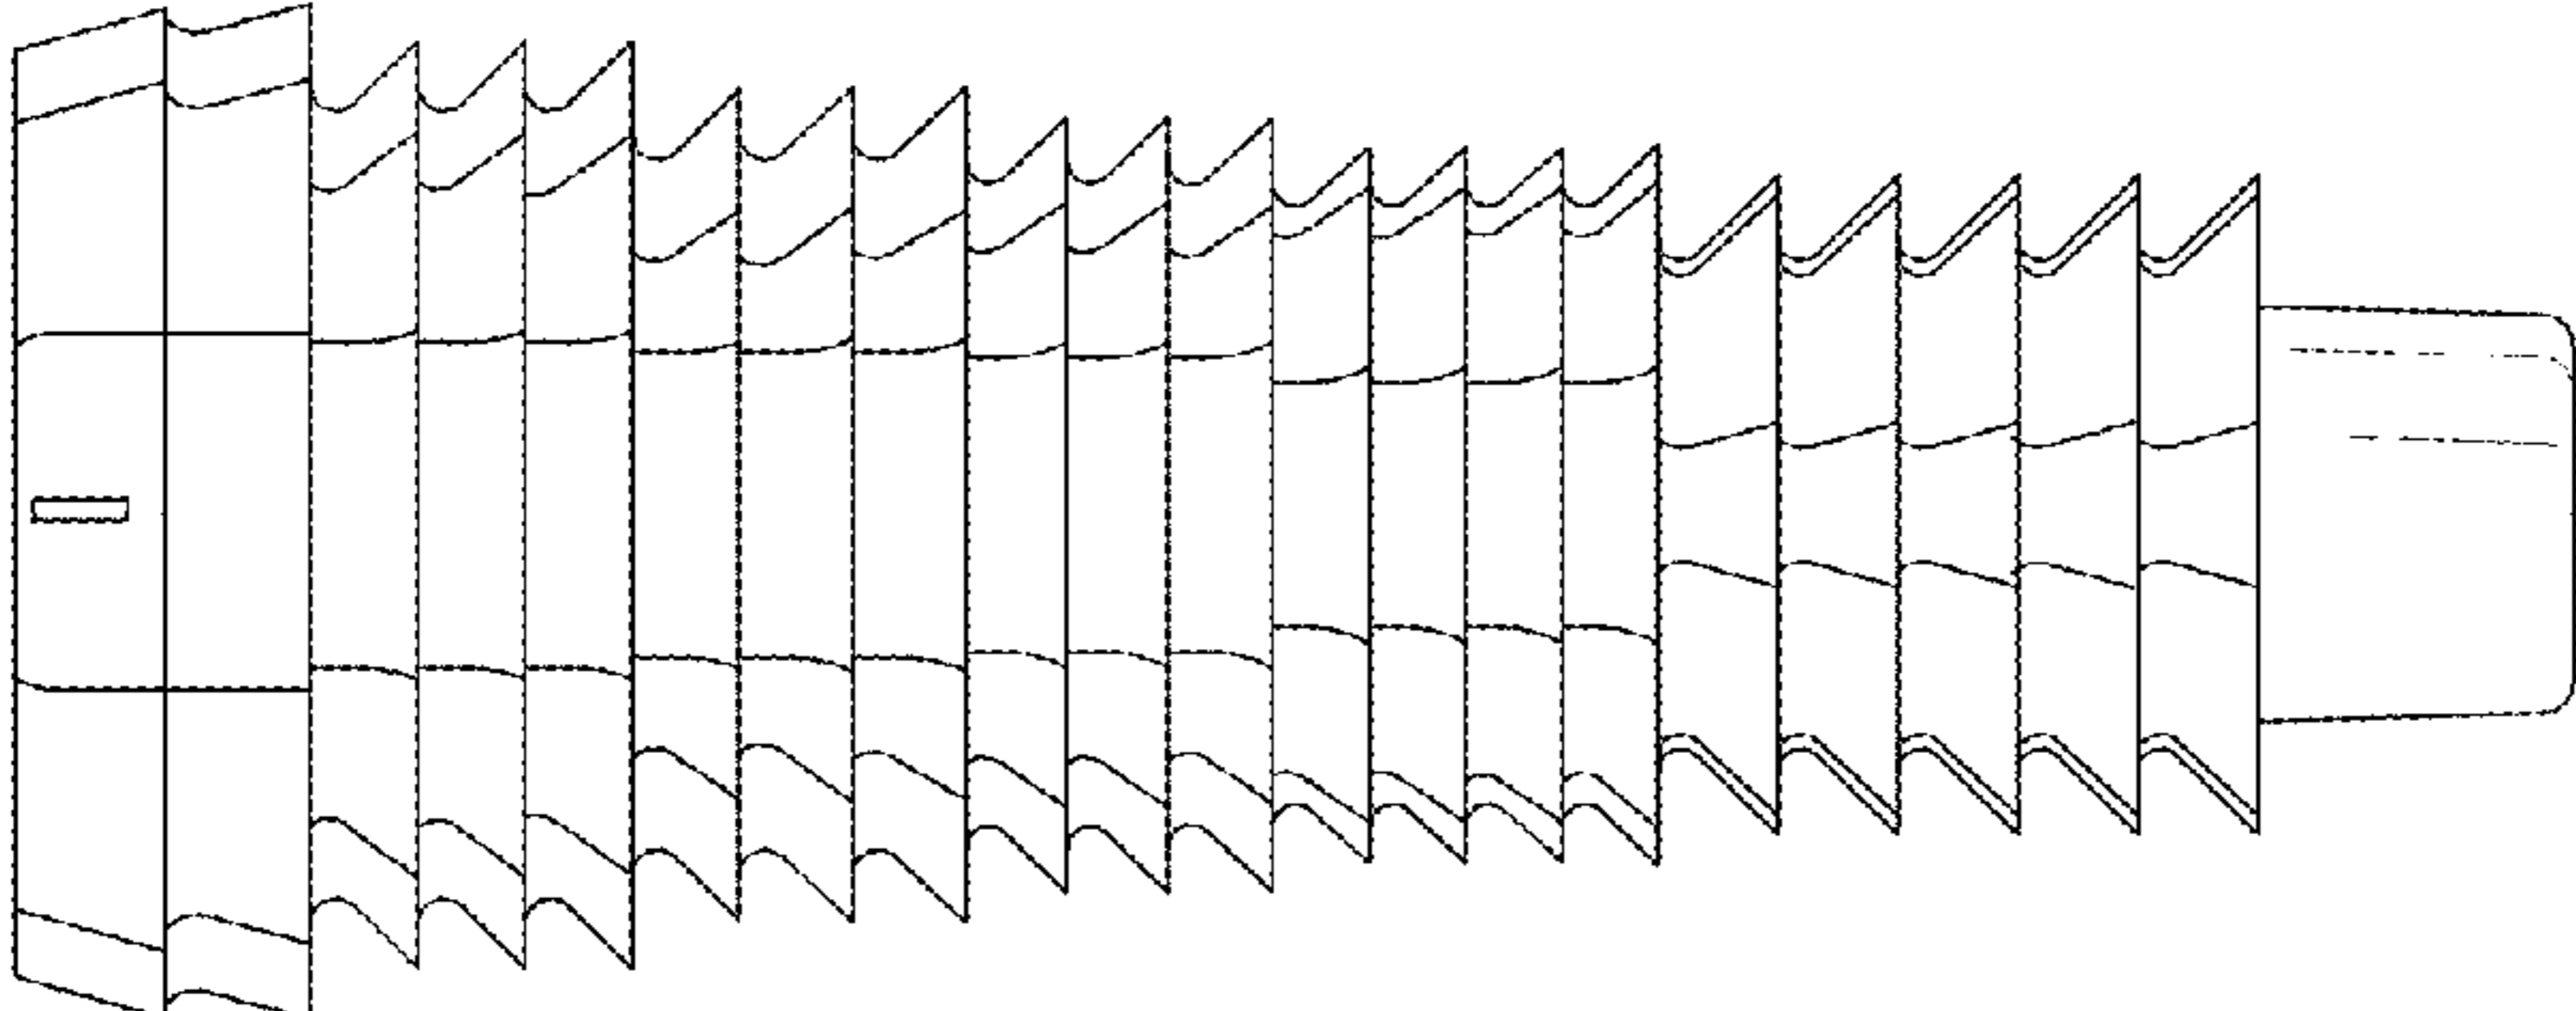


Fig. 2

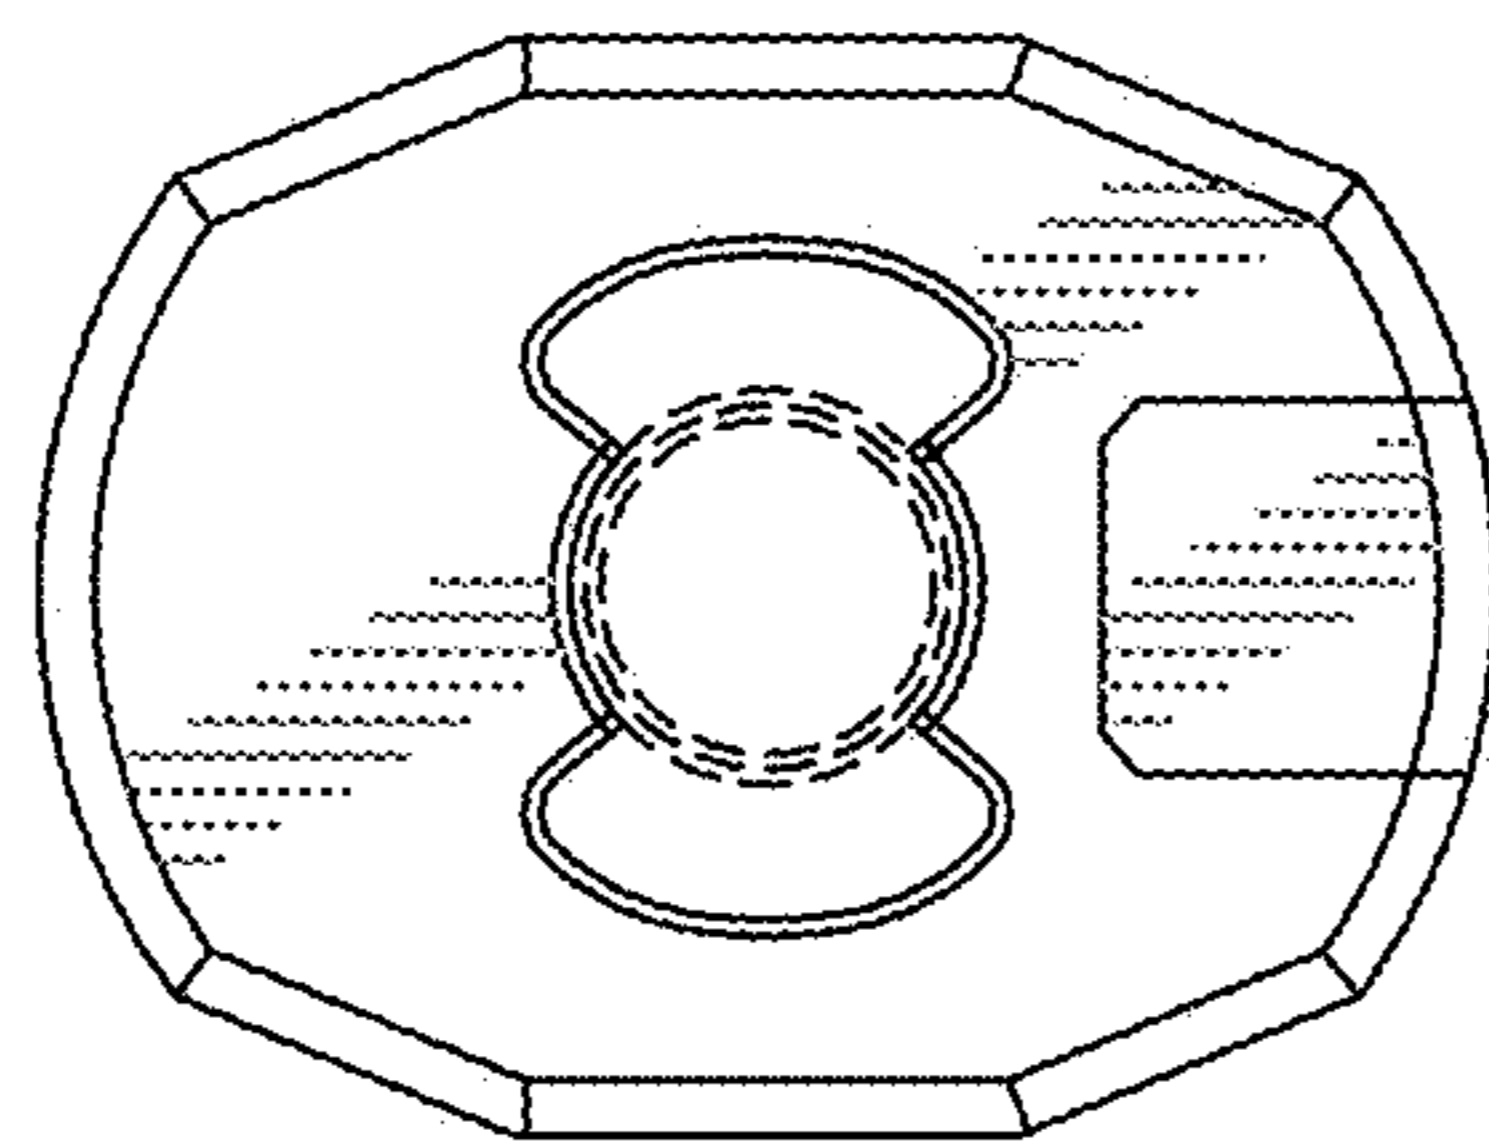


Fig. 4

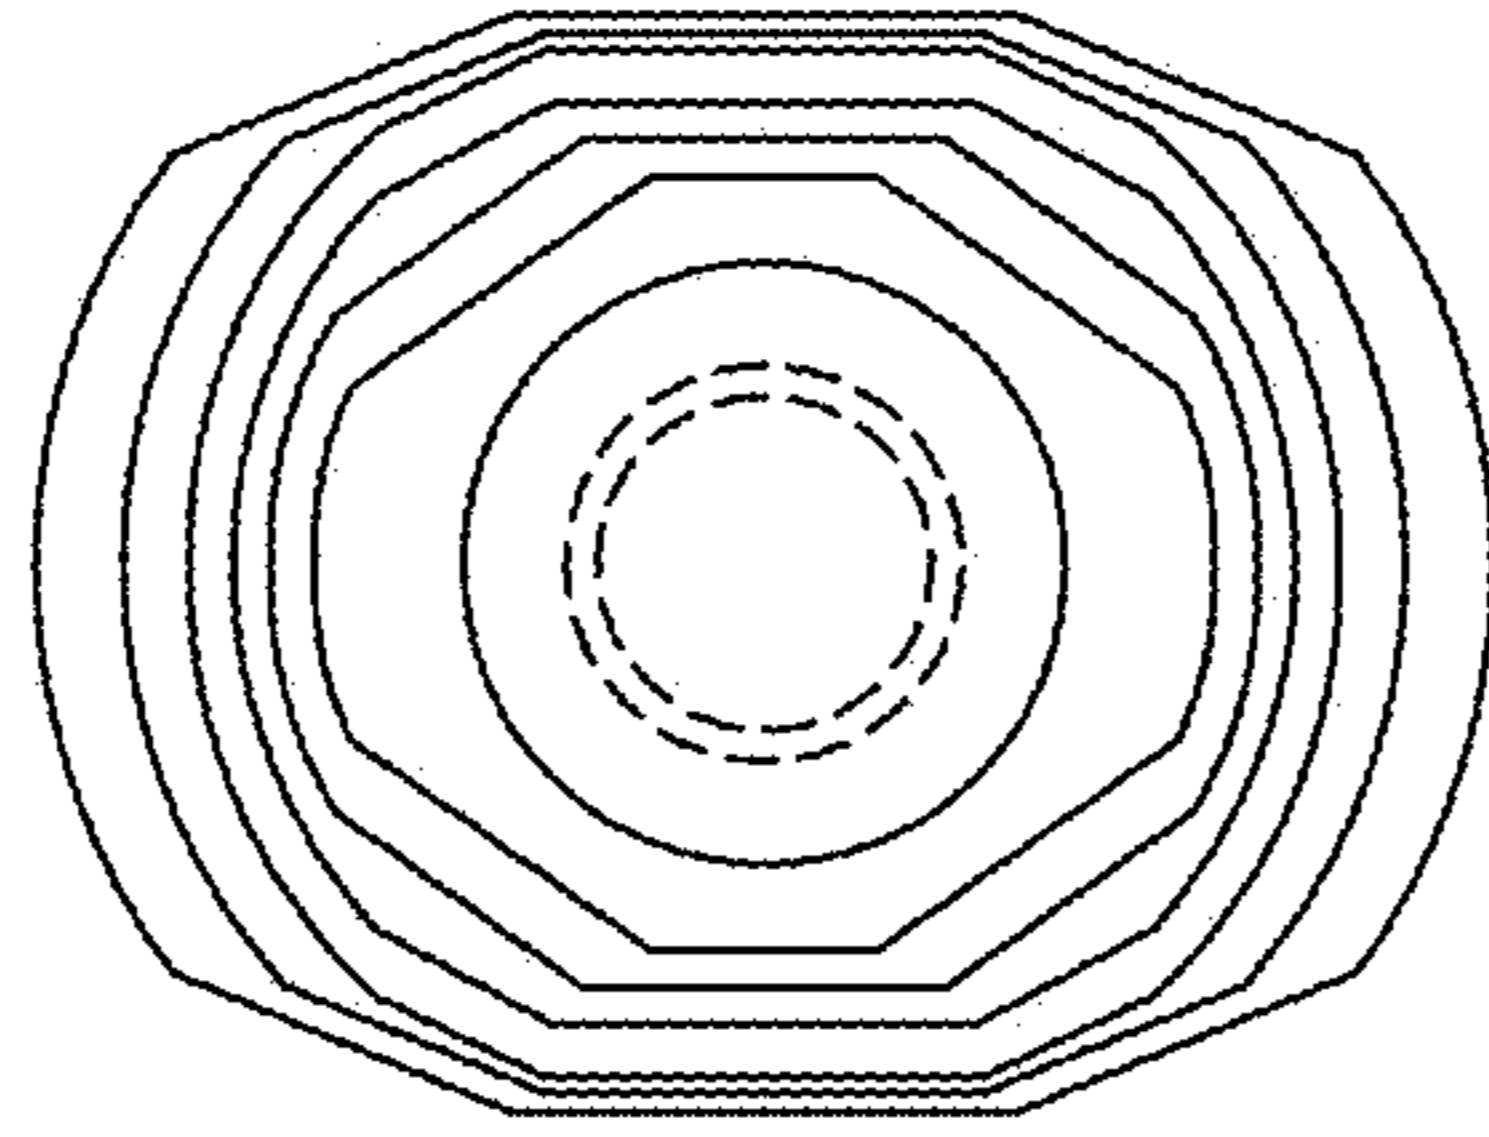


Fig. 5

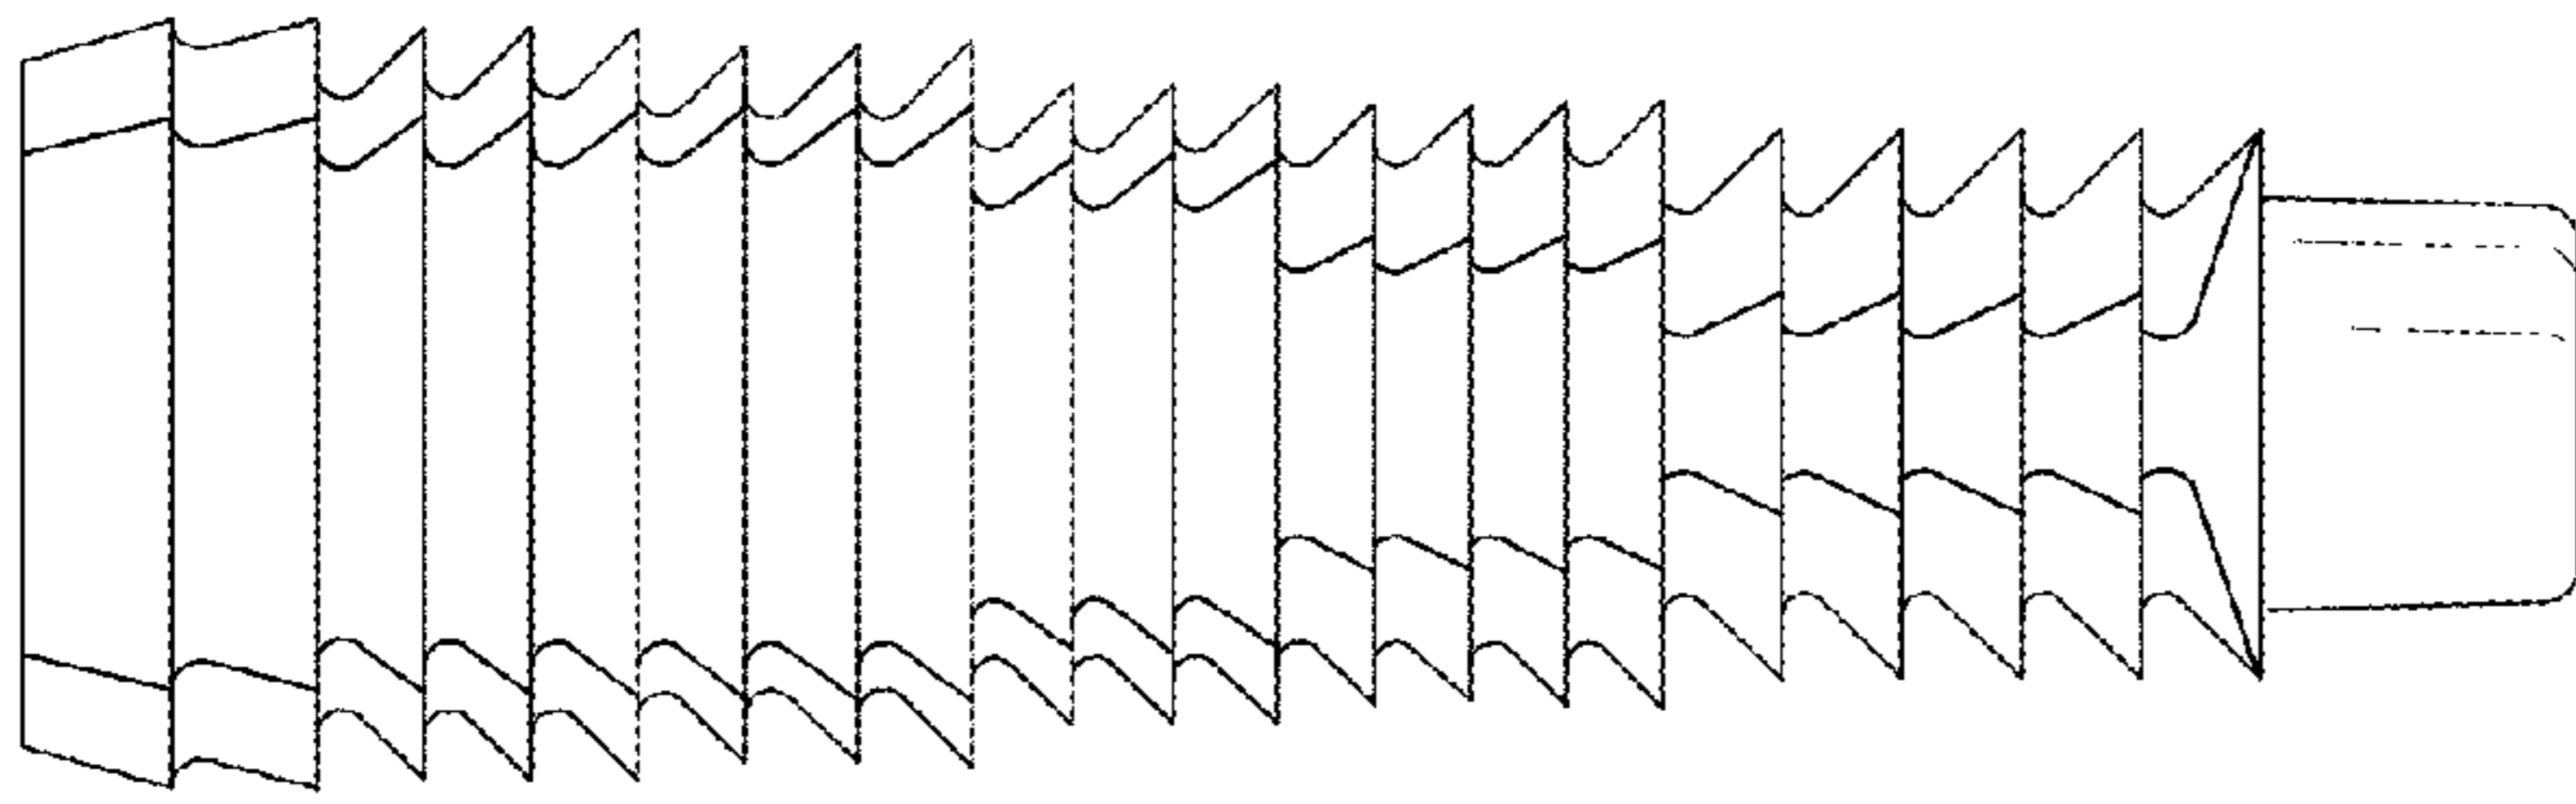


Fig. 7

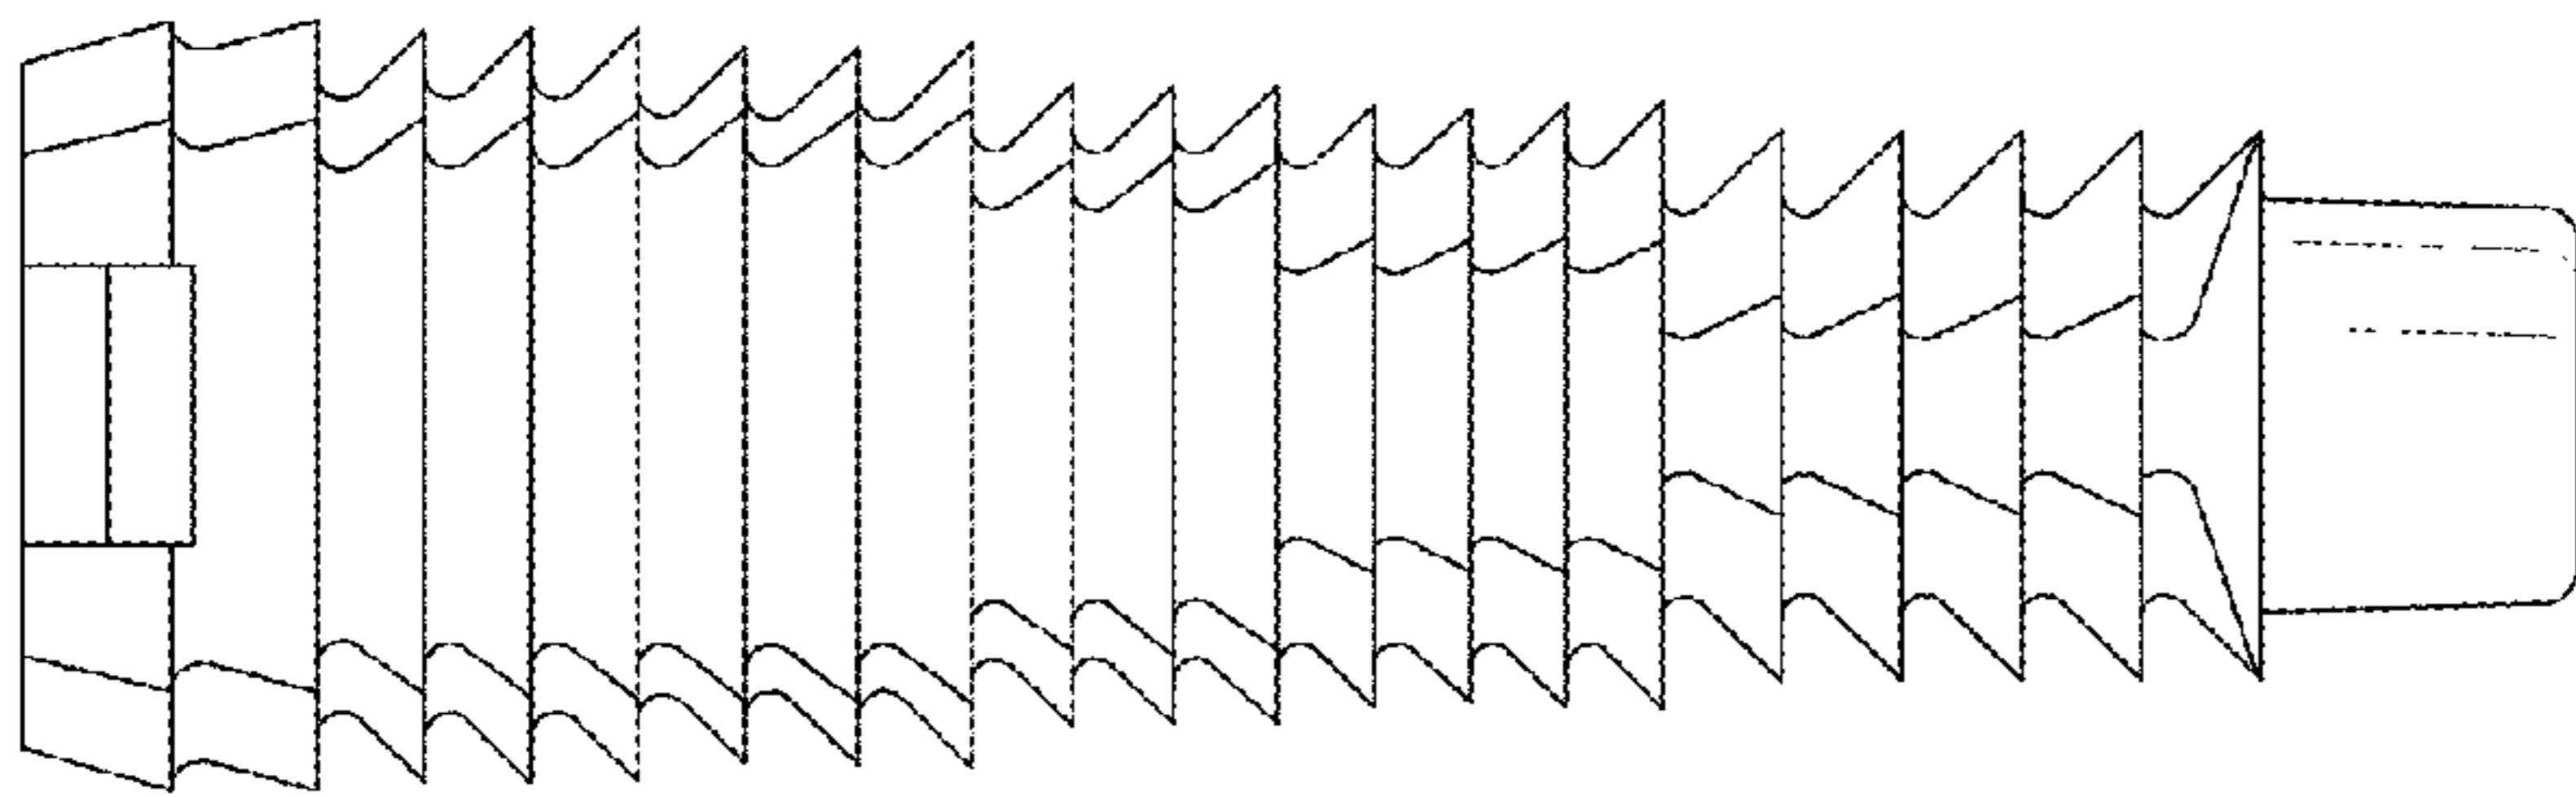


Fig. 6