



US00D759235S

(12) **United States Design Patent**
Rizvi

(10) **Patent No.:** **US D759,235 S**
(45) **Date of Patent:** **** Jun. 14, 2016**

(54) **ANESTHESIA DELIVERY DEVICE WITH HEMISPHERICAL TIP**

(71) Applicant: **Syed Rizvi**, Murrieta, CA (US)

(72) Inventor: **Syed Rizvi**, Murrieta, CA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/494,564**

(22) Filed: **Jun. 23, 2014**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/127**

(58) **Field of Classification Search**
USPC D24/127-131, 112-114, 133, 186;
606/181, 185; 604/264, 272, 115, 232,
604/187, 158, 164.08, 192, 263, 163, 181,
604/184, 198, 227; 600/101, 139, 143;
128/200.24, 207.14, 207.15
CPC A61B 2017/320048; A61B 2017/00557;
A61M 25/1002
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,474,188	A *	6/1949	Pohl	604/174
D263,873	S *	4/1982	Genese	D24/112
5,369,807	A *	12/1994	Cho et al.	2/159
D372,308	S *	7/1996	Stuart	D24/112
D375,358	S *	11/1996	Clark	D24/133

5,830,220	A *	11/1998	Wan et al.	606/139
6,820,740	B1 *	11/2004	Spector	206/219
D503,799	S *	4/2005	Beck	D24/129
D574,490	S *	8/2008	Patzer	D24/129
D625,809	S *	10/2010	Cuschieri et al.	D24/143
2002/0026936	A1 *	3/2002	Kirn	128/200.24
2012/0316594	A1 *	12/2012	Palese	606/185
2014/0107593	A1 *	4/2014	Gao et al.	604/272

* cited by examiner

Primary Examiner — David Muller

Assistant Examiner — Nathan Johnston


(57) **CLAIM**

I claim the ornamental design for an anesthesia delivery device with hemispherical tip, as shown and described.

DESCRIPTION

FIG. 1 is a top side perspective view of the anesthesia delivery device with hemispherical tip of the present invention; FIG. 2 is a top plan view thereof; FIG. 3 is a bottom plan view thereof; FIG. 4 is a left side elevation view thereof; FIG. 5 is a right side elevation view thereof; FIG. 6 is a rear elevation view thereof; FIG. 7 is a front elevation view thereof; and, FIG. 8 is a top side, perspective, magnified view of the hemispherical tip of the device of FIG. 1. The broken lines showing the anesthetic exit port in the hemispherical tip of the device are included for the purpose of illustrating structure that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

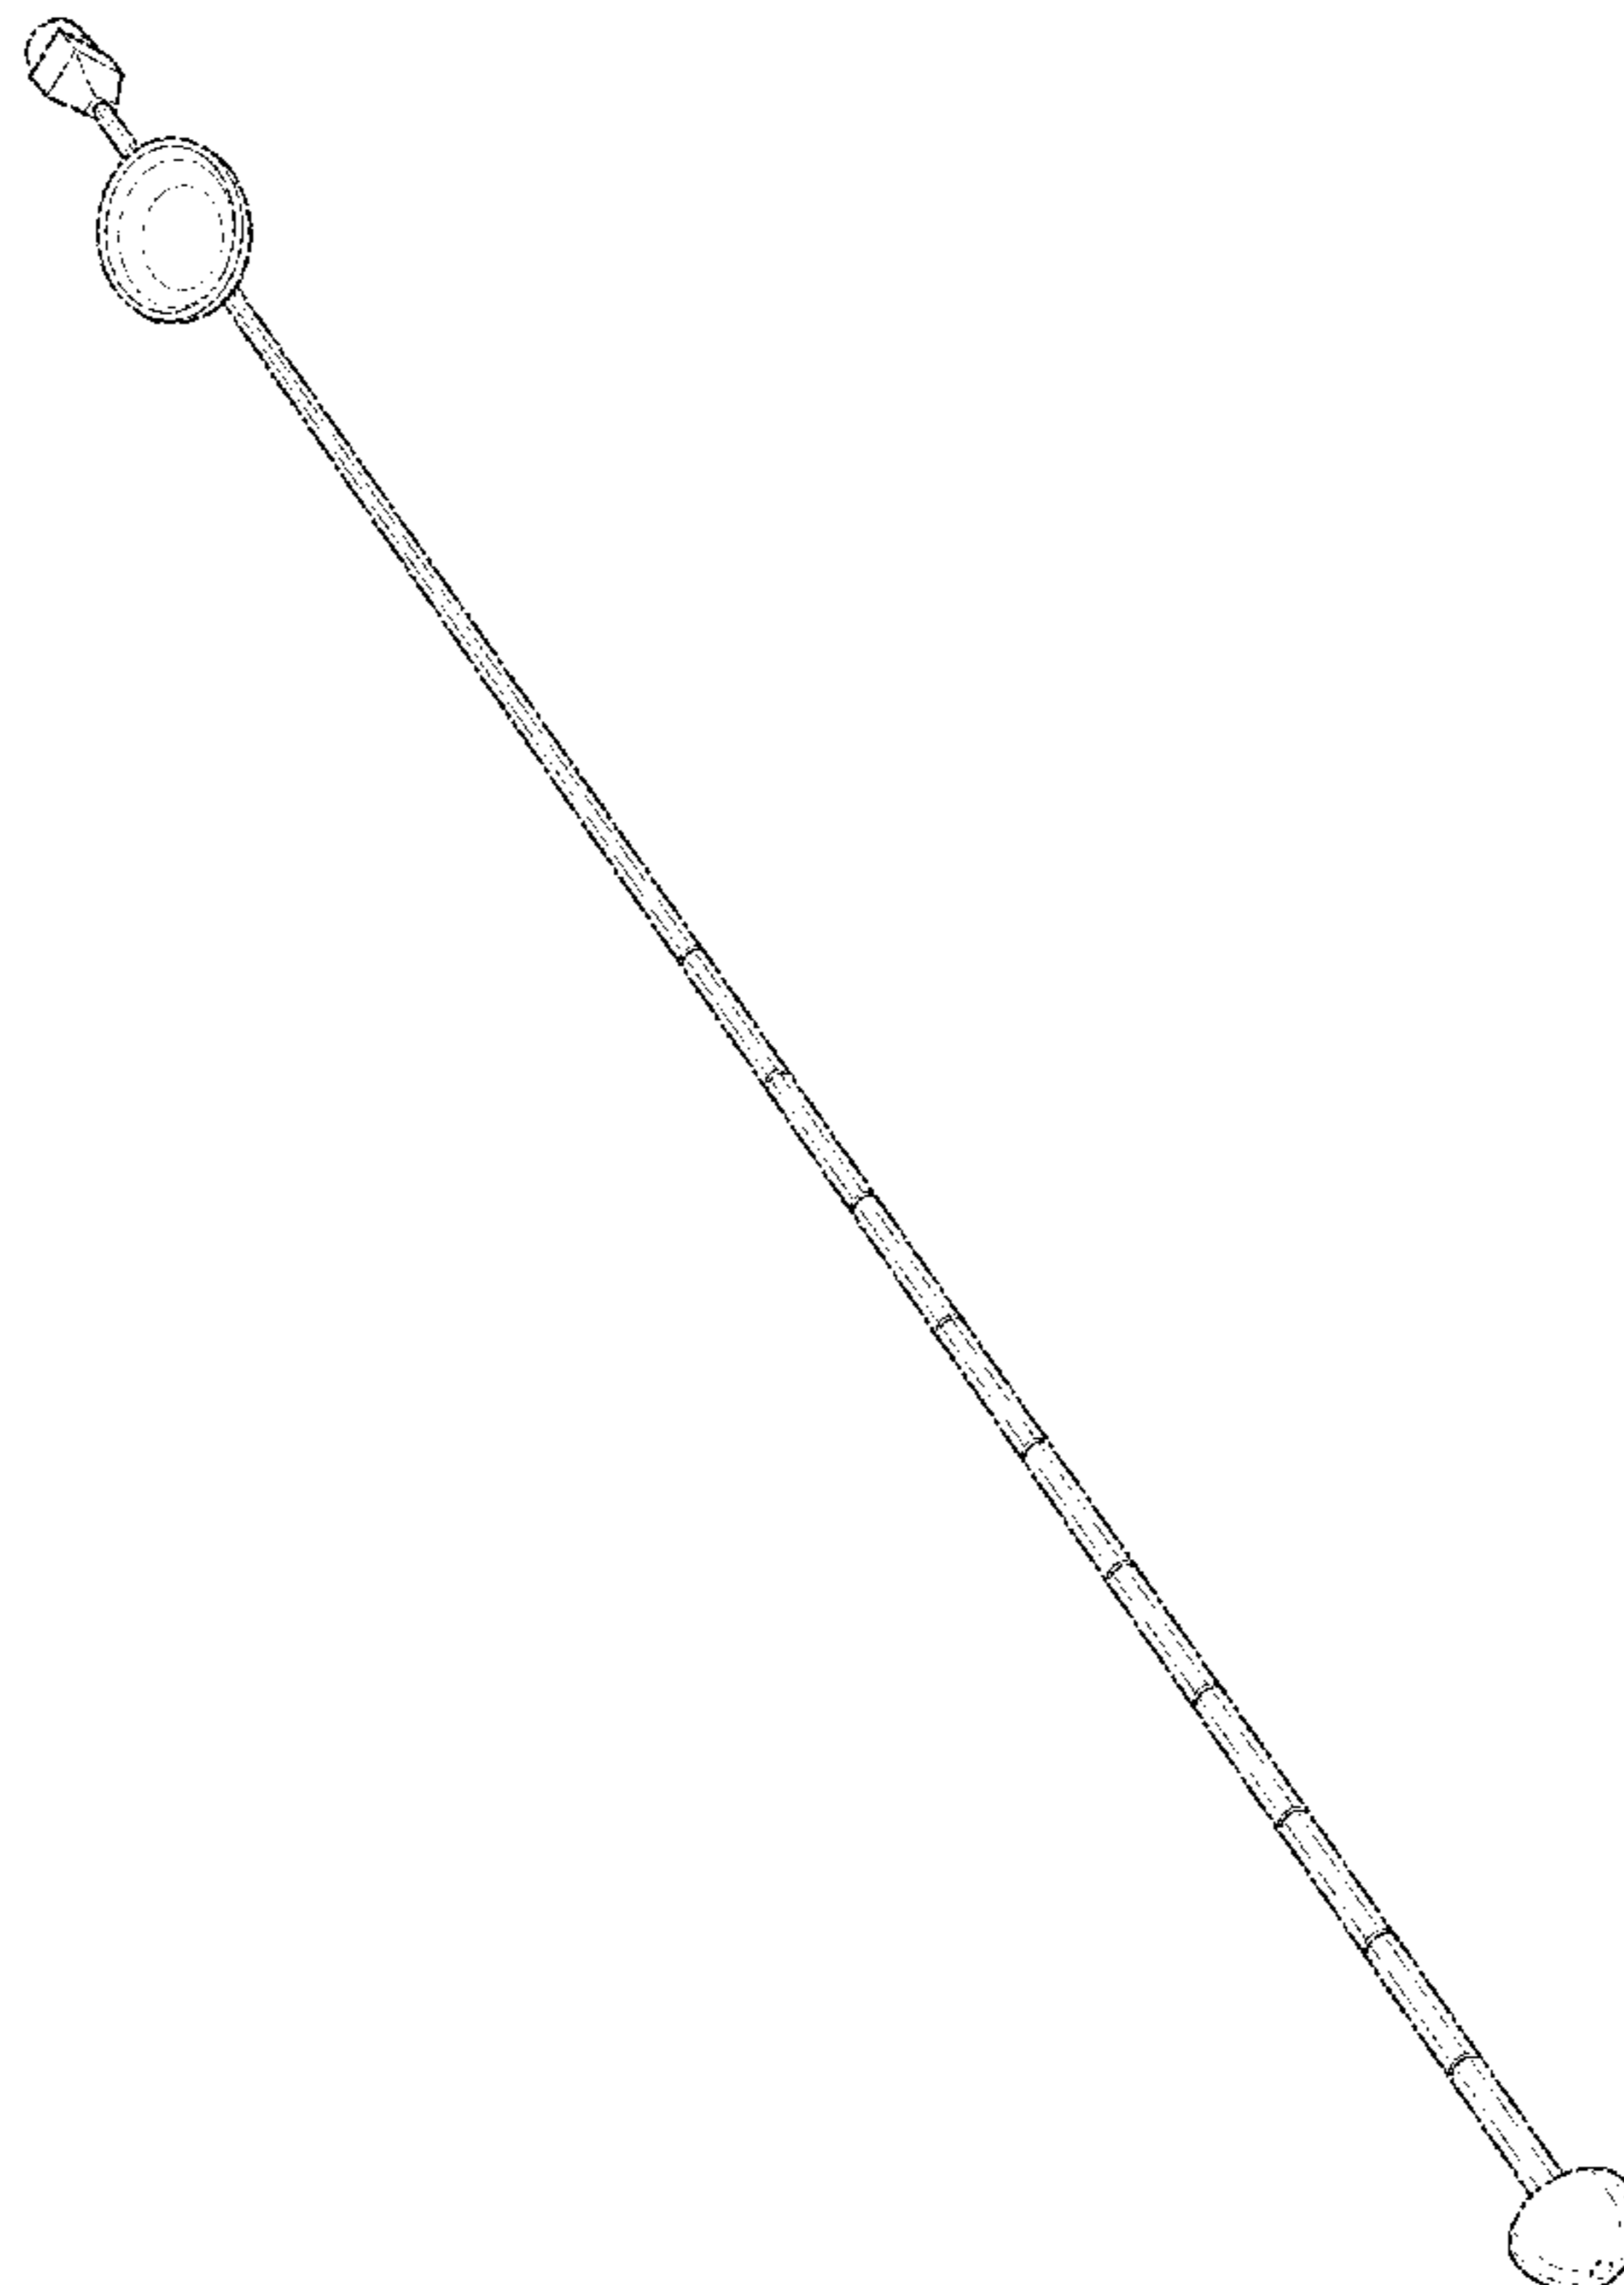

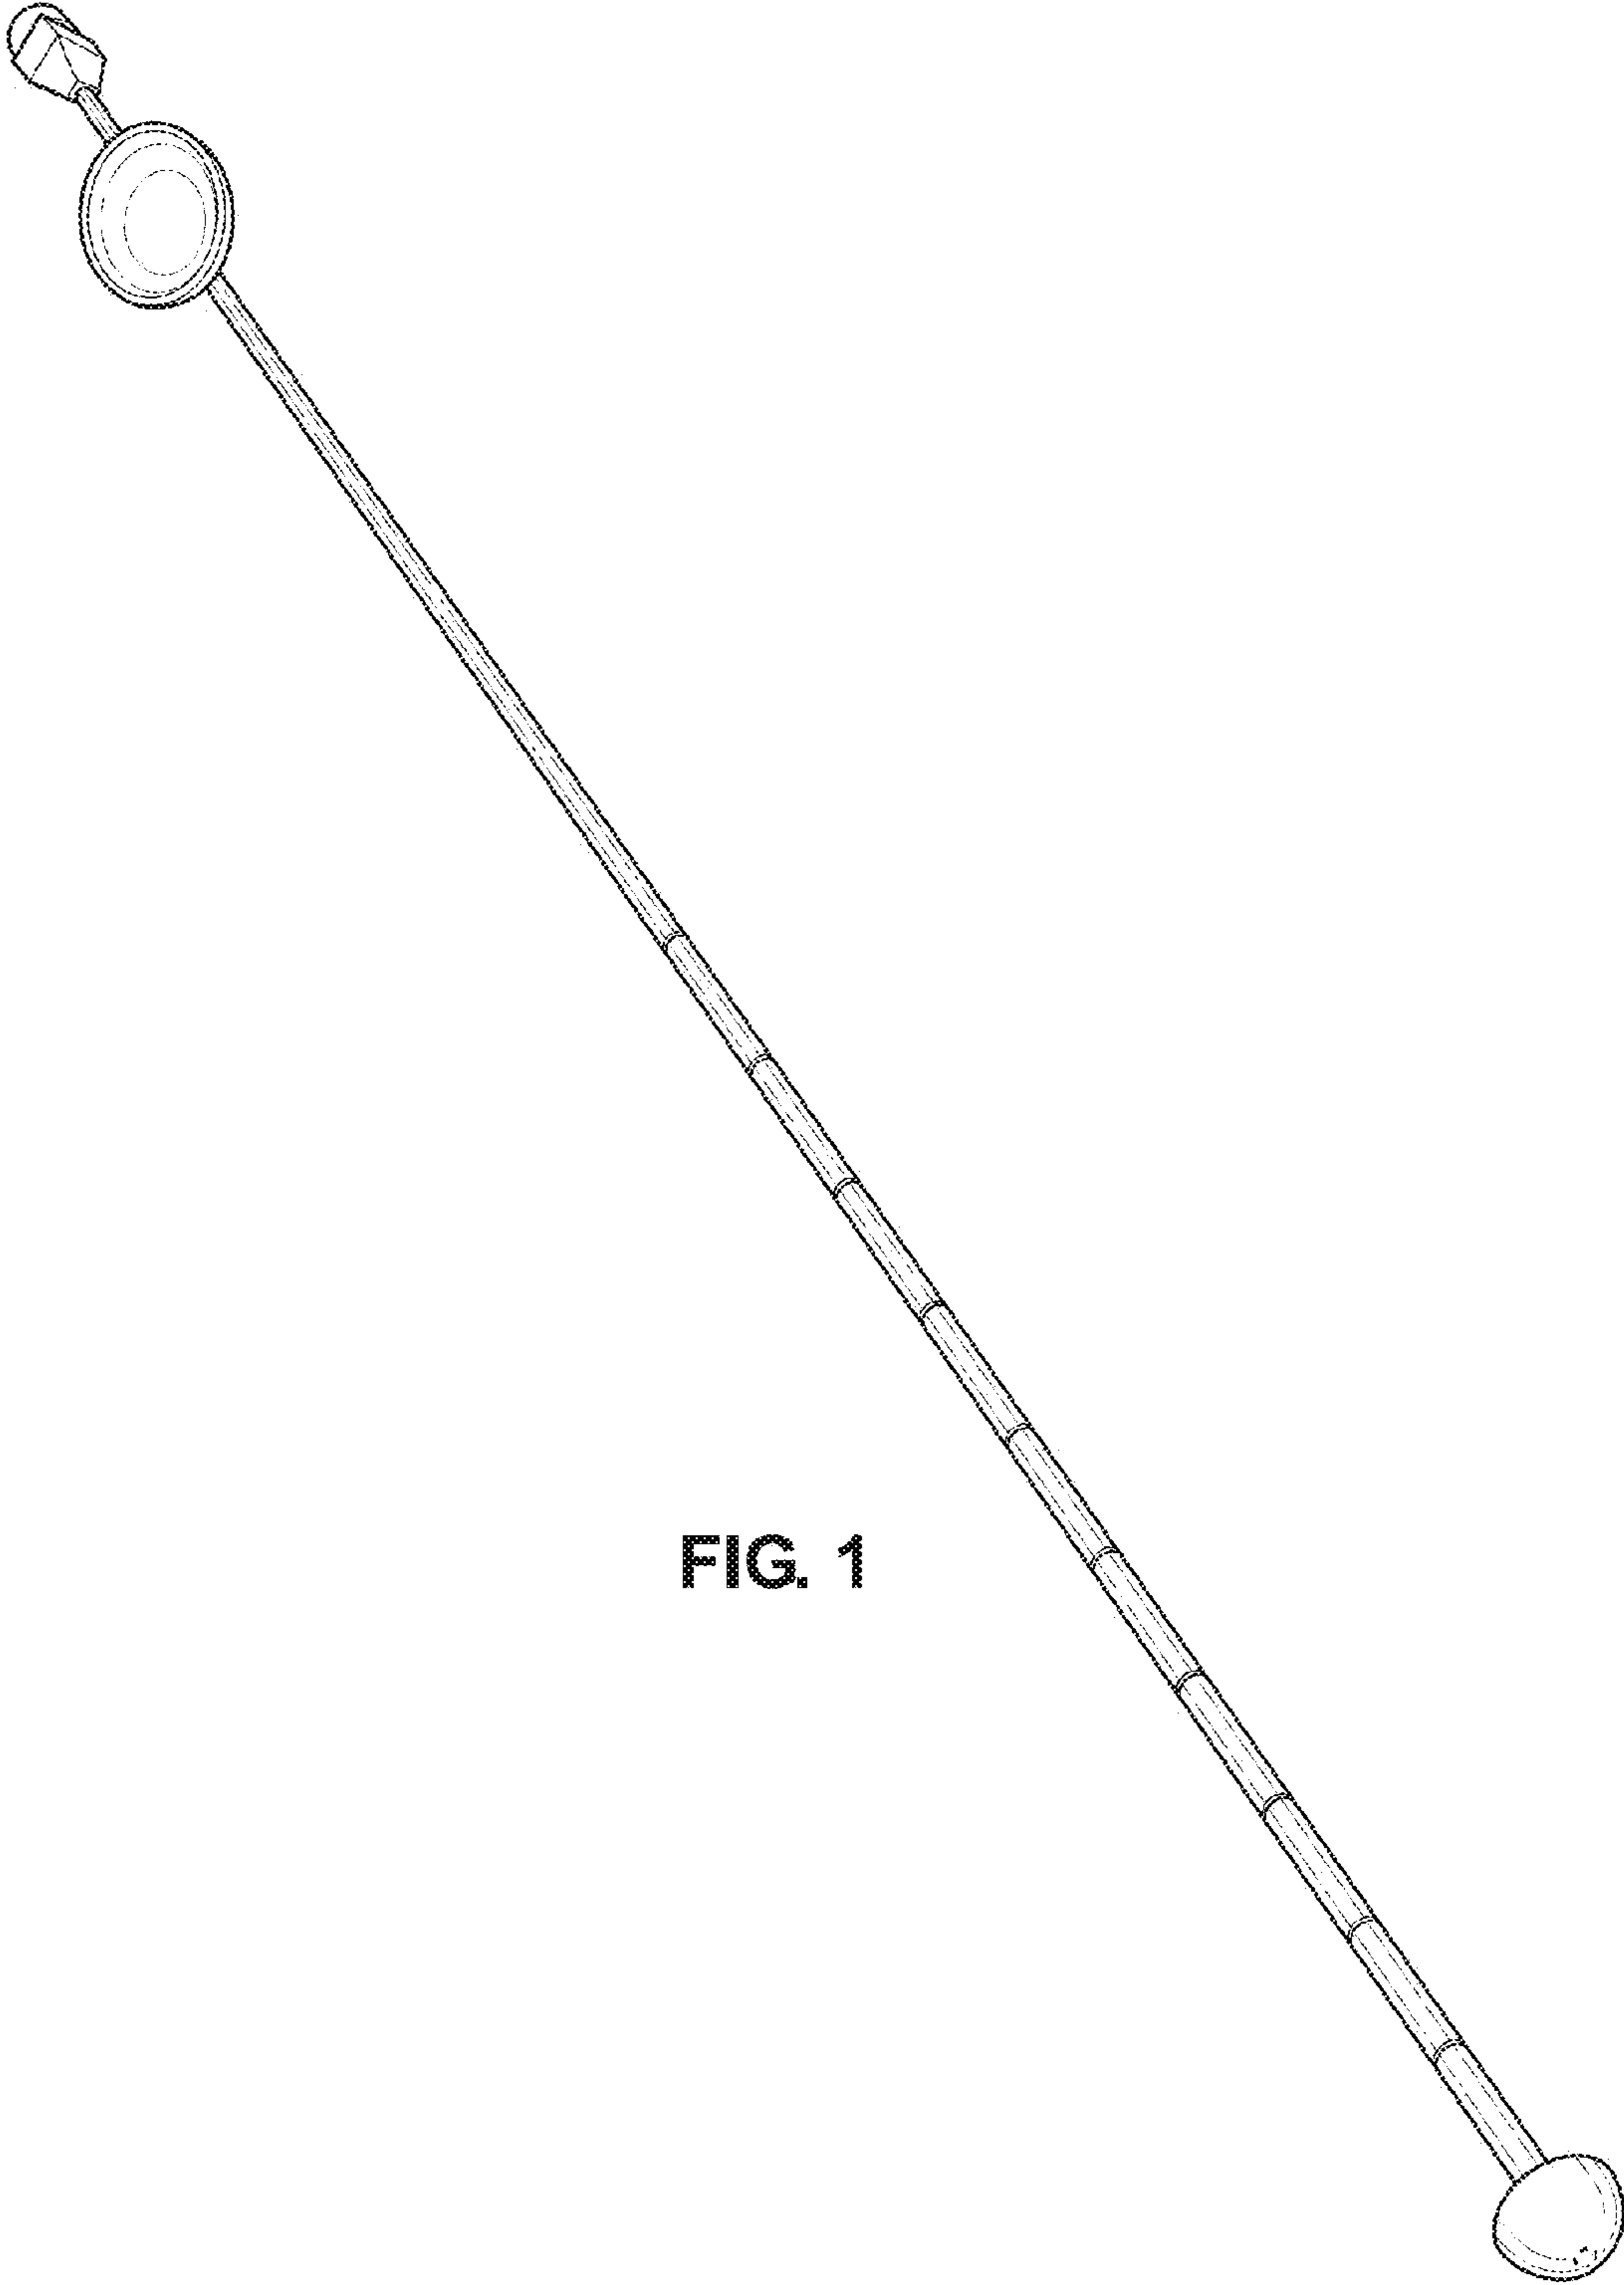


FIG. 1

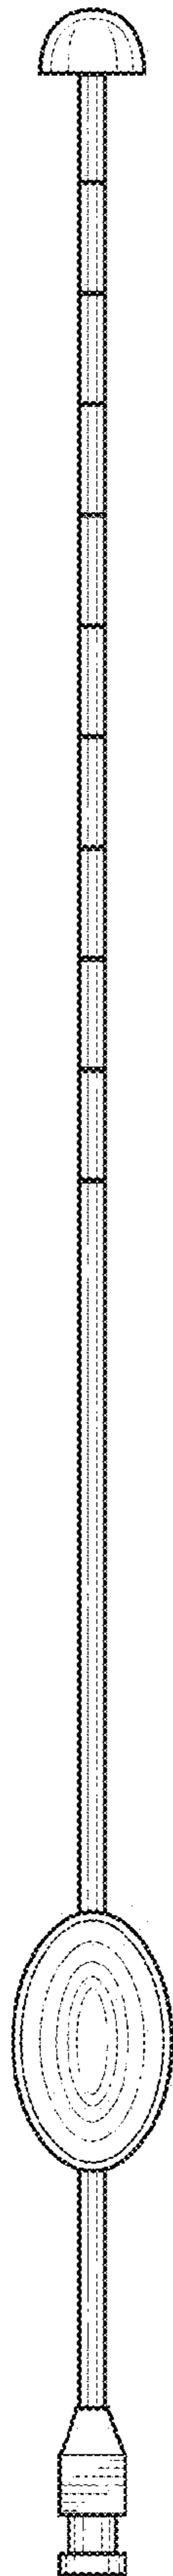


FIG. 2

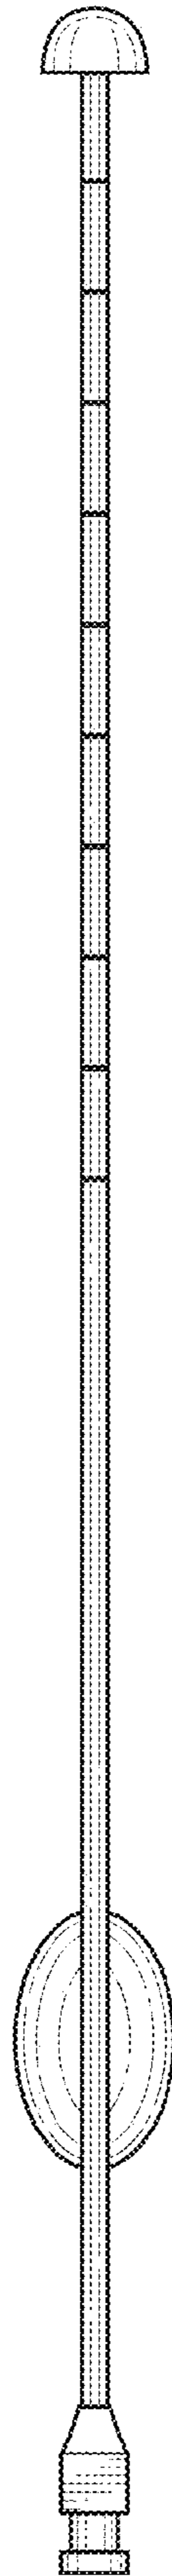


FIG. 3

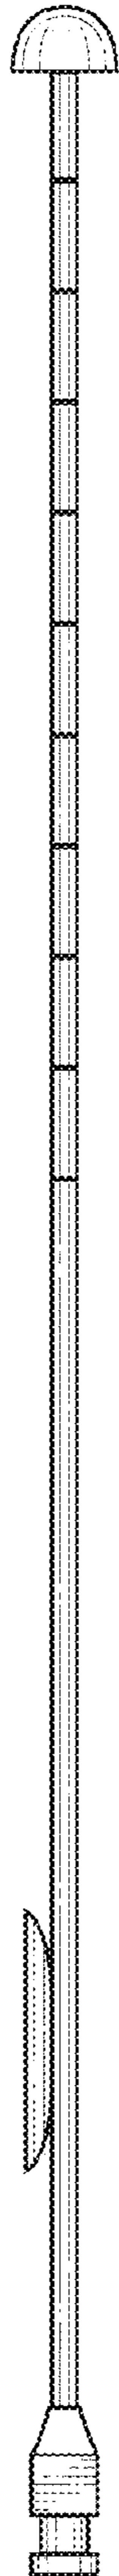


FIG. 4

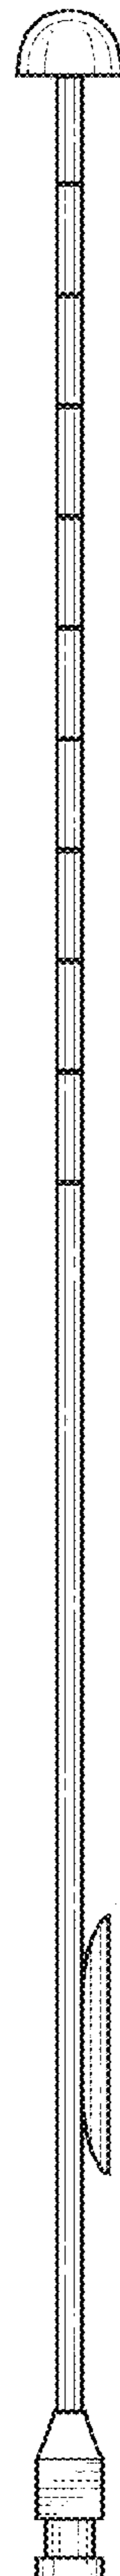


FIG. 5

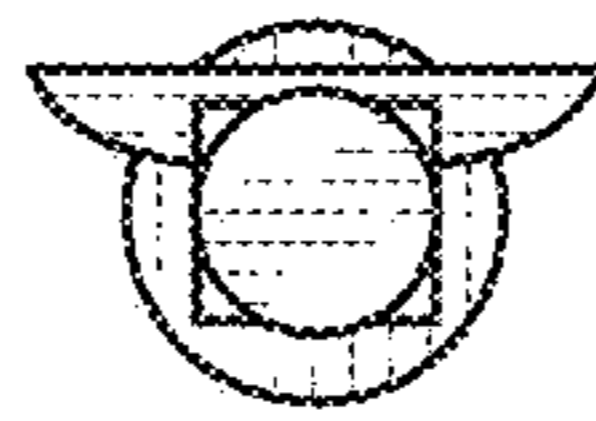


FIG. 6

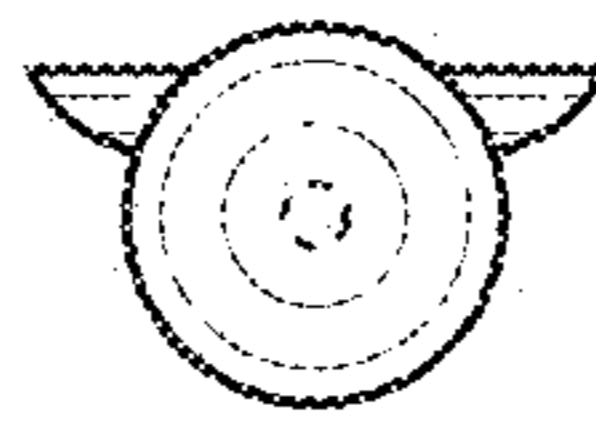


FIG. 7

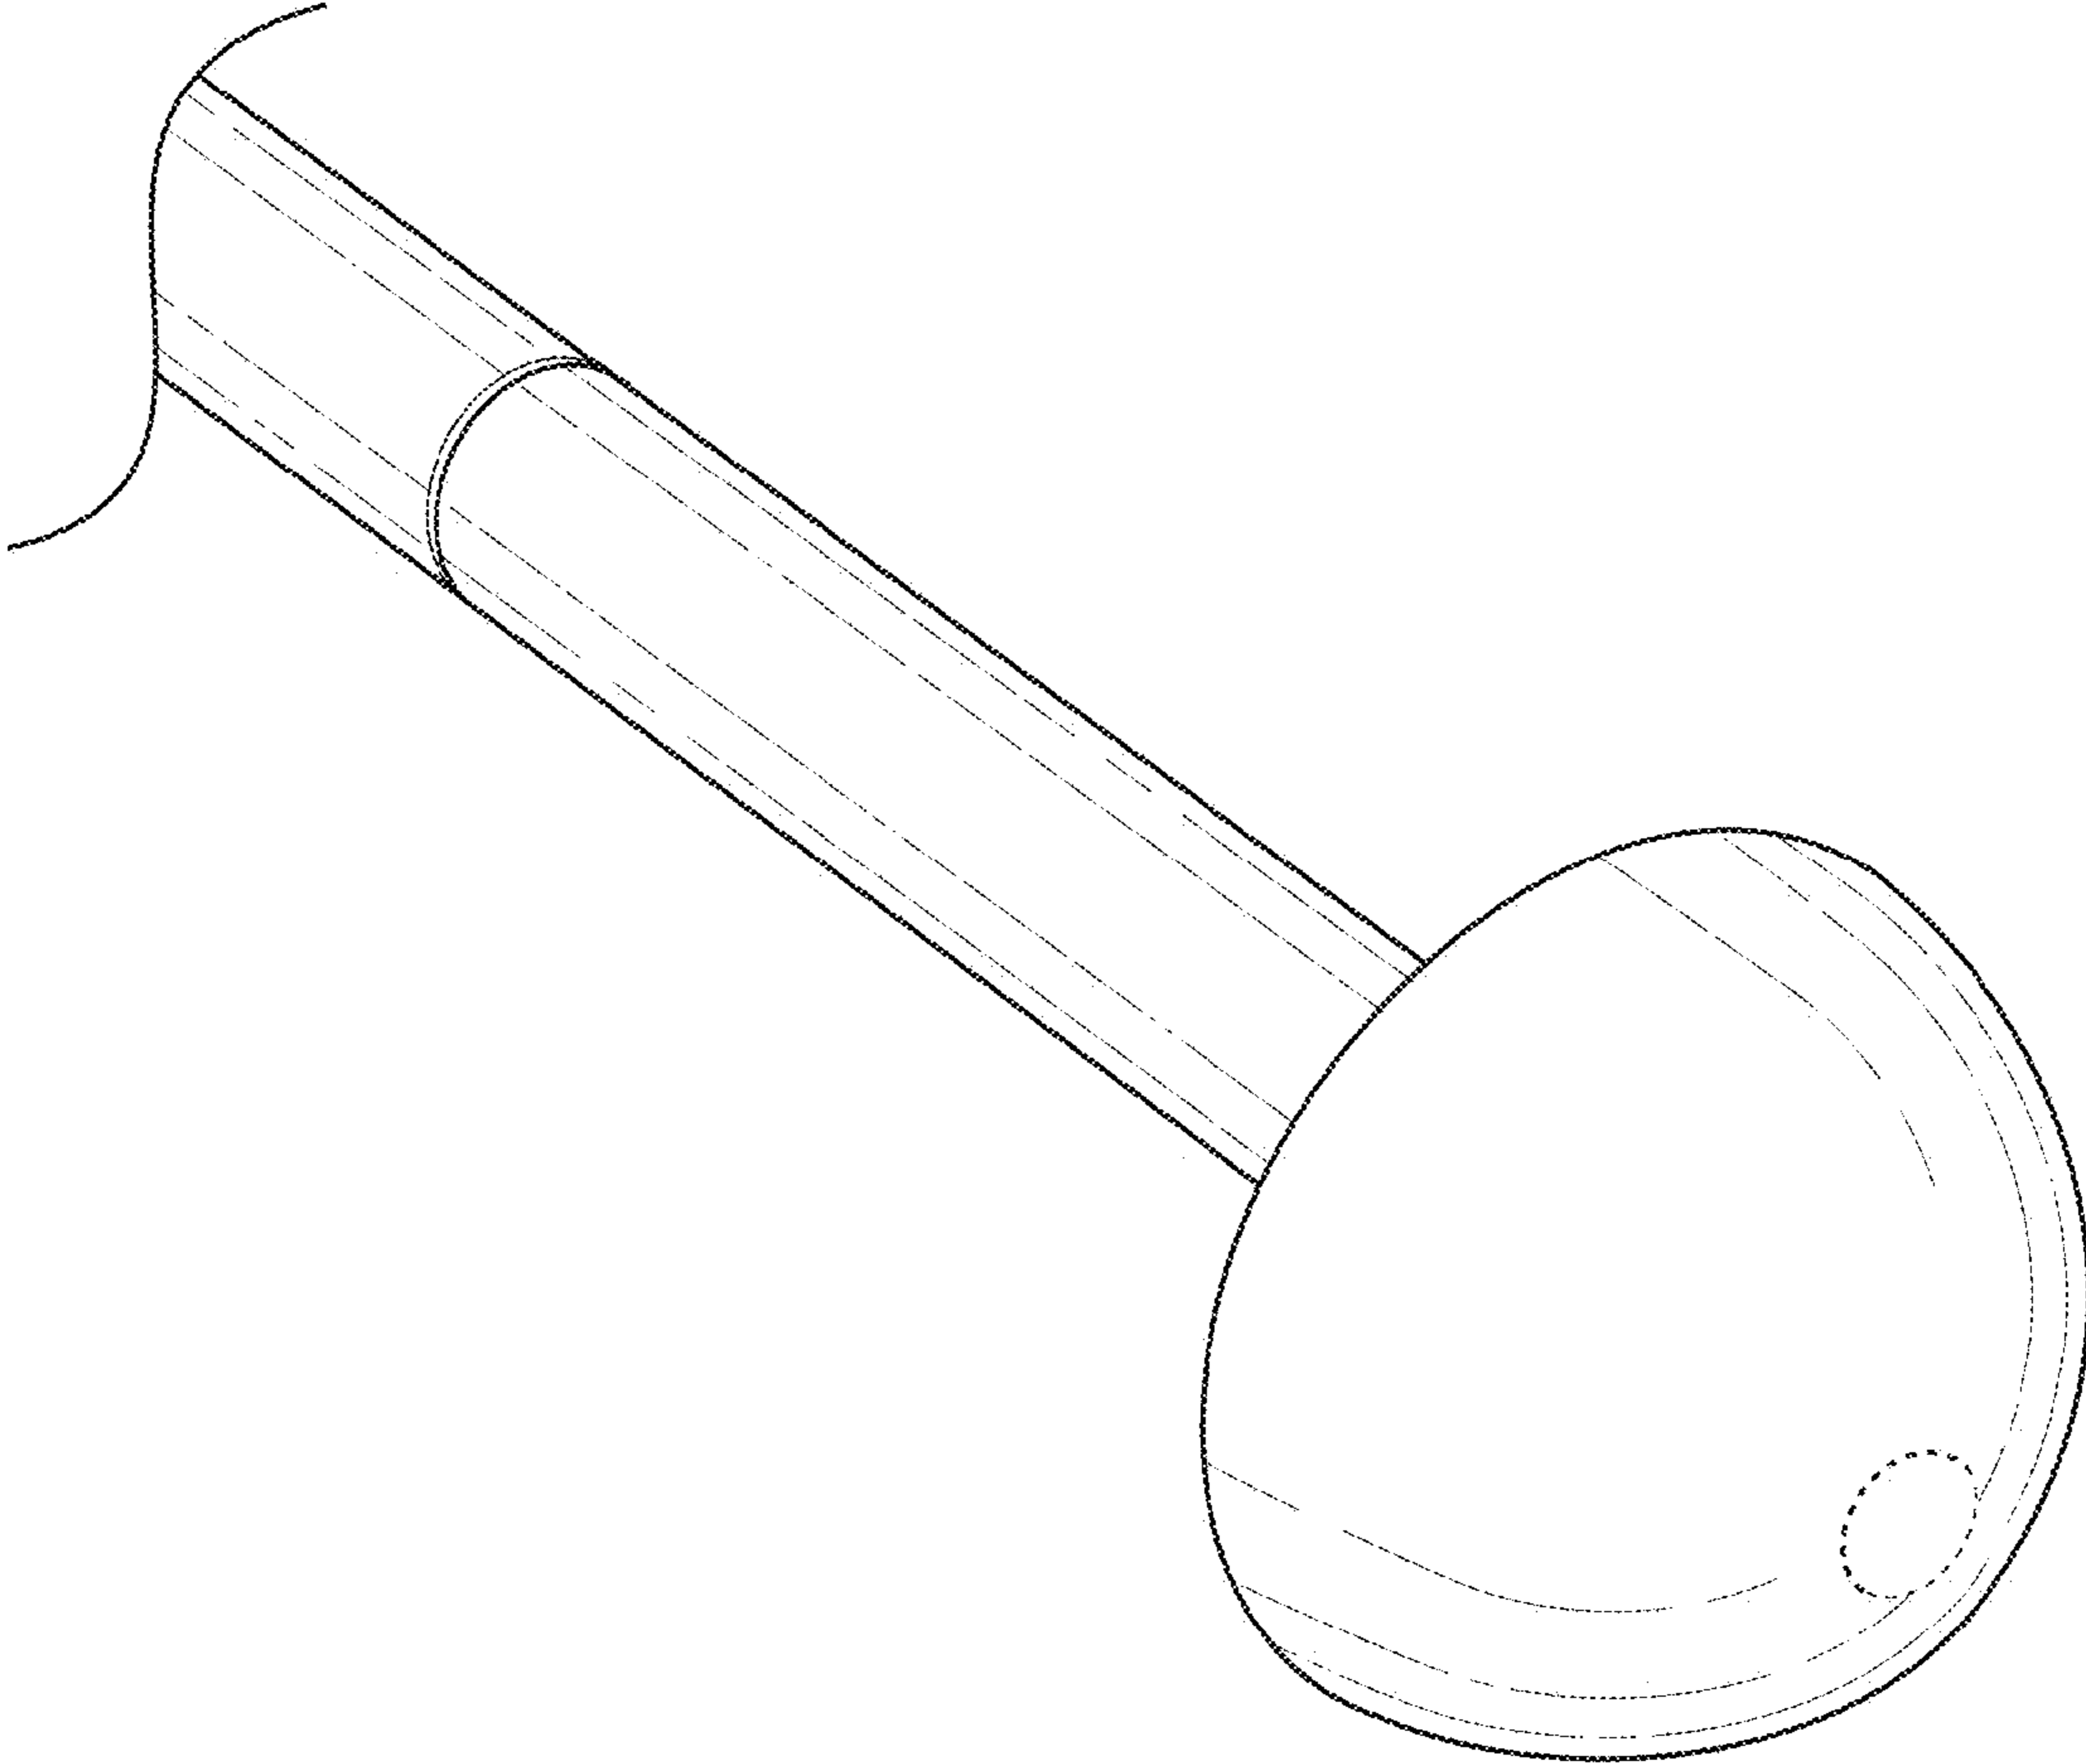


FIG. 8