



US00D760288S

(12) **United States Design Patent**
Kendler et al.

(10) **Patent No.:** **US D760,288 S**
(45) **Date of Patent:** **** Jun. 28, 2016**

(54) **MEDICAL PUMP DISPLAY SCREEN WITH
TRANSITIONAL GRAPHICAL USER
INTERFACE**

D696,686 S * 12/2013 Yuk D14/486
D698,362 S * 1/2014 Ramesh D14/487
D701,232 S * 3/2014 Na D14/486
D705,244 S * 5/2014 Arnold D14/486

(Continued)

(71) Applicant: **DEKA Products Limited Partnership,**
Manchester, NH (US)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Jonathan Kendler**, Utrecht (NL);
Jonathan I. Tilliss, Somerville, MA
(US)

WO WO2013095459 A9 6/2013
WO WO2013096713 A2 6/2013

(Continued)

(73) Assignee: **DEKA Products Limited Partnership,**
Manchester, NH (US)

Primary Examiner — Eric Goodman
Assistant Examiner — Daniel J Domino

(**) Term: **14 Years**

(74) *Attorney, Agent, or Firm* — James D. Wyninegar, Jr.

(21) Appl. No.: **29/477,236**

(57) **CLAIM**

The ornamental design for a medical pump display screen with transitional graphical user interface, as shown and described.

(22) Filed: **Dec. 20, 2013**

DESCRIPTION

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**

USPC **D14/492**; D14/493

(58) **Field of Classification Search**

USPC D14/485–495

CPC . G06F 3/048; G06F 3/04842; G06F 3/04847;

G06F 3/0481; G06F 17/211; G06F 17/212

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D622,730 S * 8/2010 Krum D14/486
D625,322 S * 10/2010 Guntaur D14/486
7,890,881 B1 * 2/2011 Skidgel G06F 17/212
715/243
D655,301 S * 3/2012 Ray D14/486
D664,988 S * 8/2012 Gleasman D14/488
D665,401 S * 8/2012 Rai D14/486
D666,208 S * 8/2012 Spears D14/486
D668,262 S * 10/2012 Gleasman D14/488
D671,551 S * 11/2012 Deng D14/486
D673,168 S * 12/2012 Frijlink D14/487
D675,224 S * 1/2013 Lee D14/488
D696,684 S * 12/2013 Yuk D14/486

FIG. 1 is a front view of the medical pump display screen with transitional graphical user interface, showing a first embodiment of the new design;

FIG. 2 is a second image thereof;

FIG. 3 is a third image thereof;

FIG. 4 is a fourth image thereof;

FIG. 5 is a front view of the medical pump display screen with transitional graphical user interface, showing second embodiment of the new design;

FIG. 6 is a second image thereof;



FIG. 7 is a third image thereof; and,

FIG. 8 is a fourth image thereof.

The broken lines of a medical pump and portions of the graphical user interface form portions of the article and form no part of the claimed design.

The images transition sequentially among the images shown in FIGS. 1-4 in embodiment 1 and FIGS. 5-8 in embodiment 2. The process or period in which one image transitions to another image forms no part of the claimed design.

1 Claim, 8 Drawing Sheets

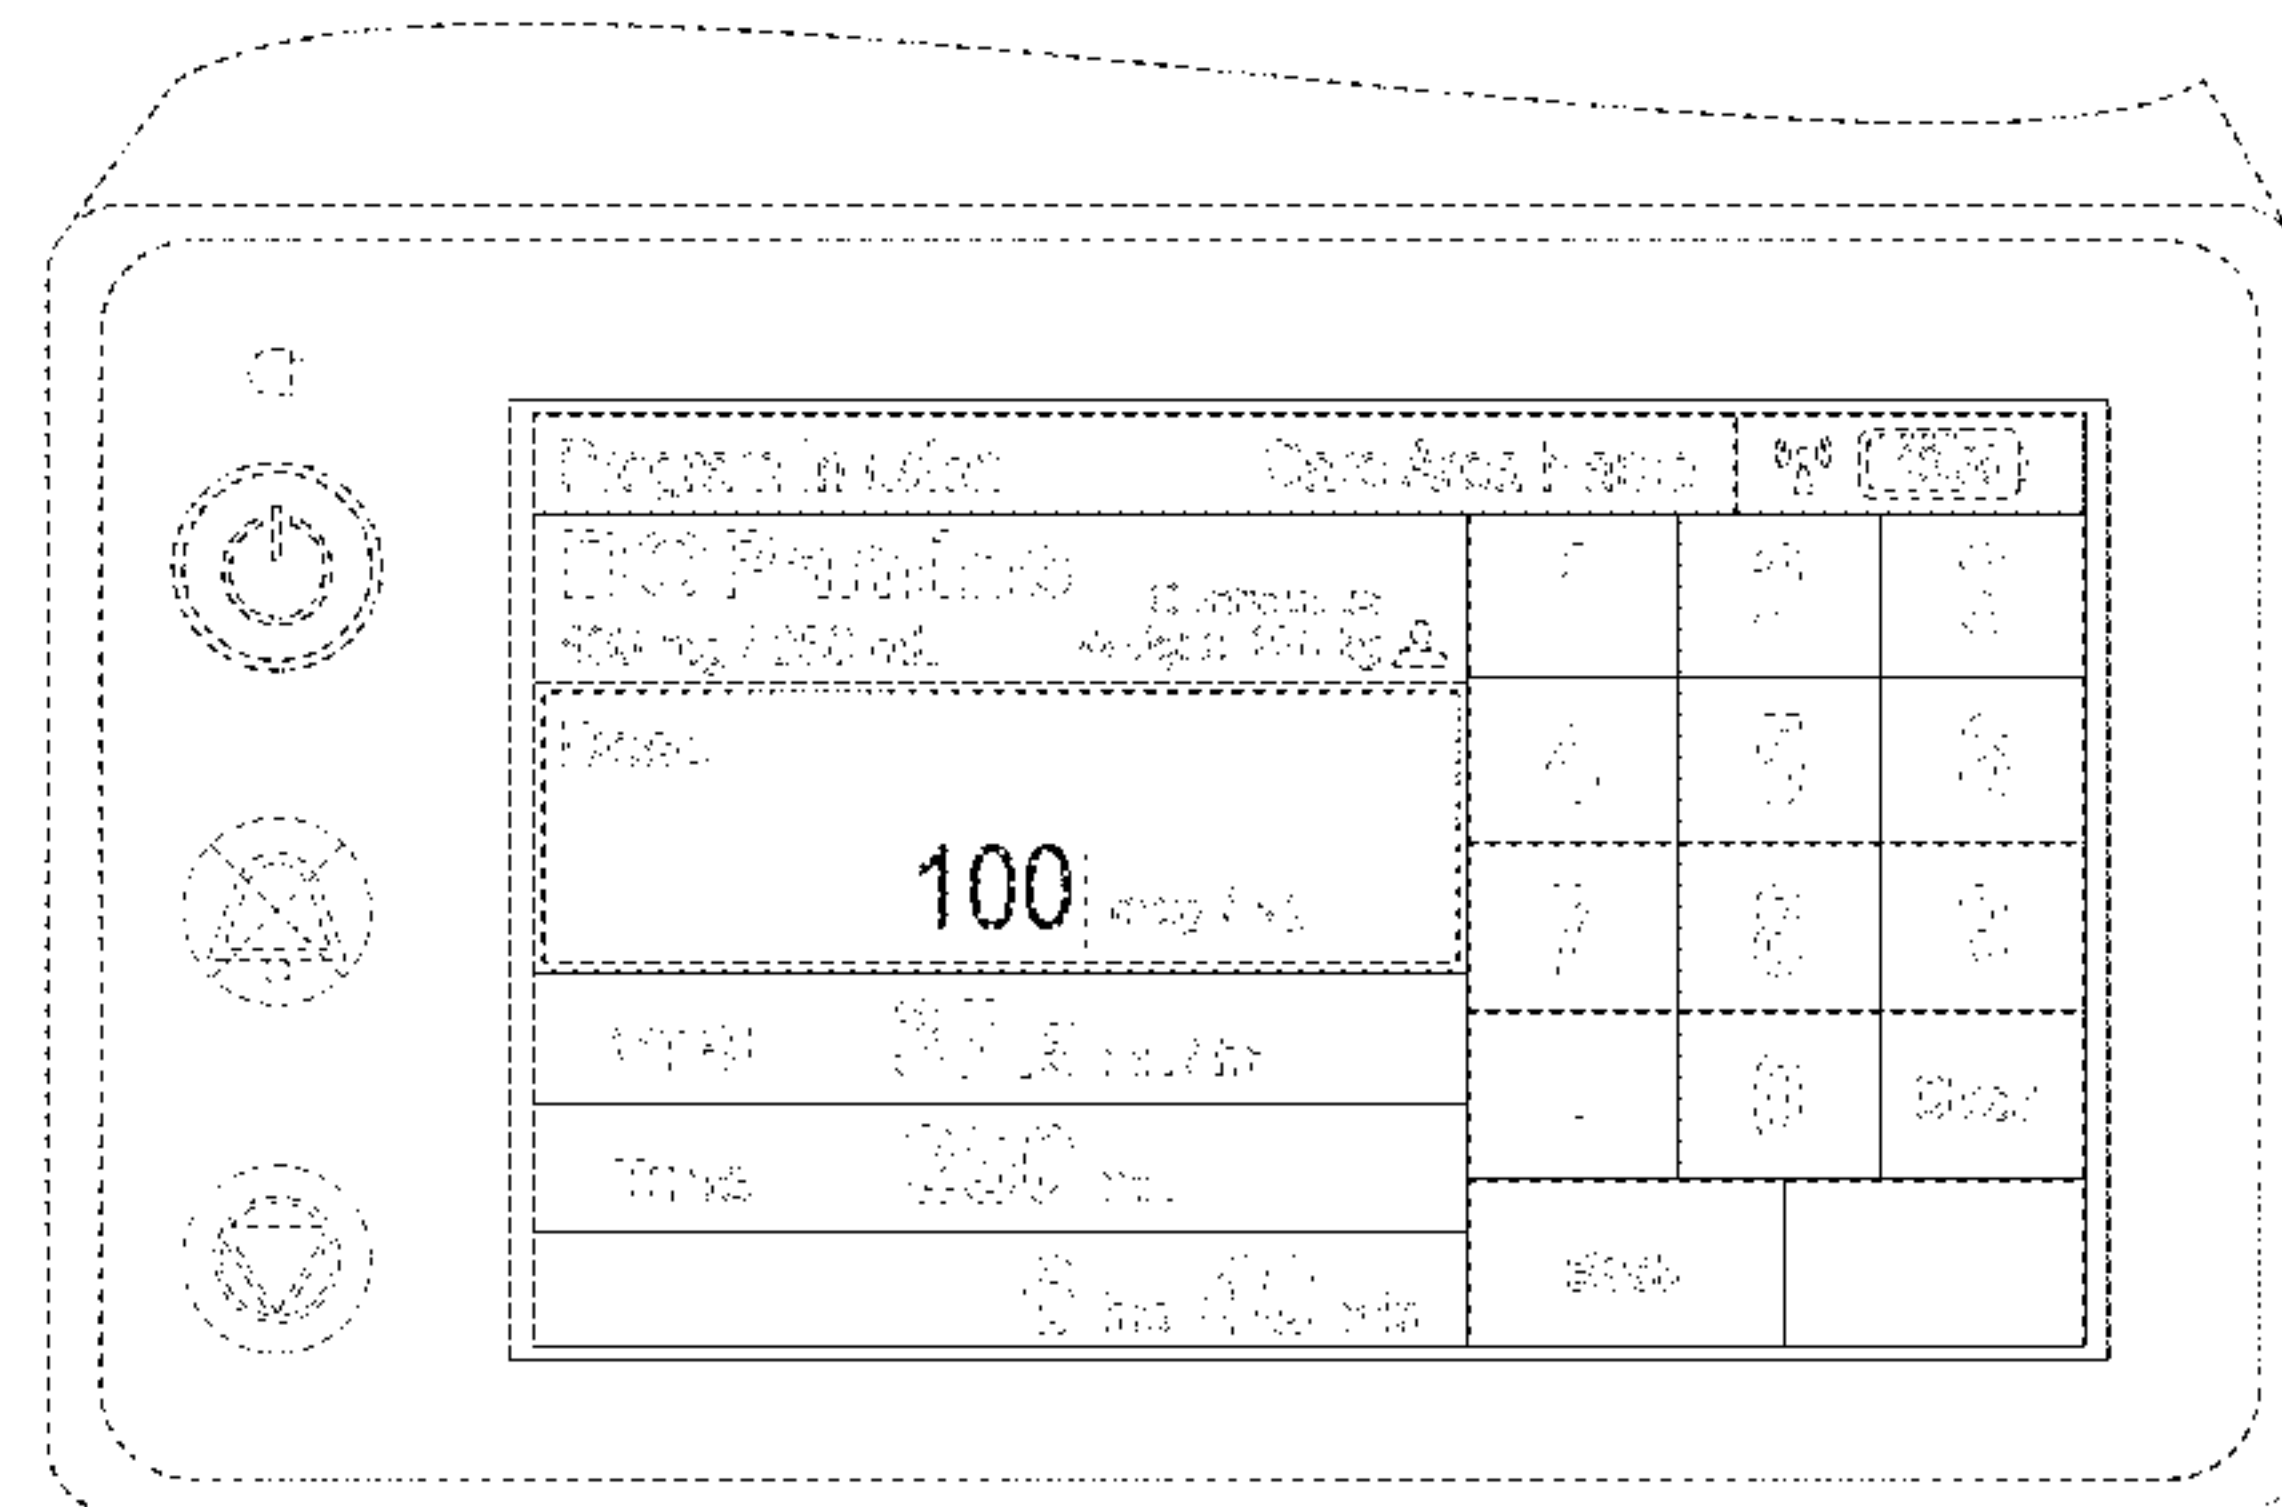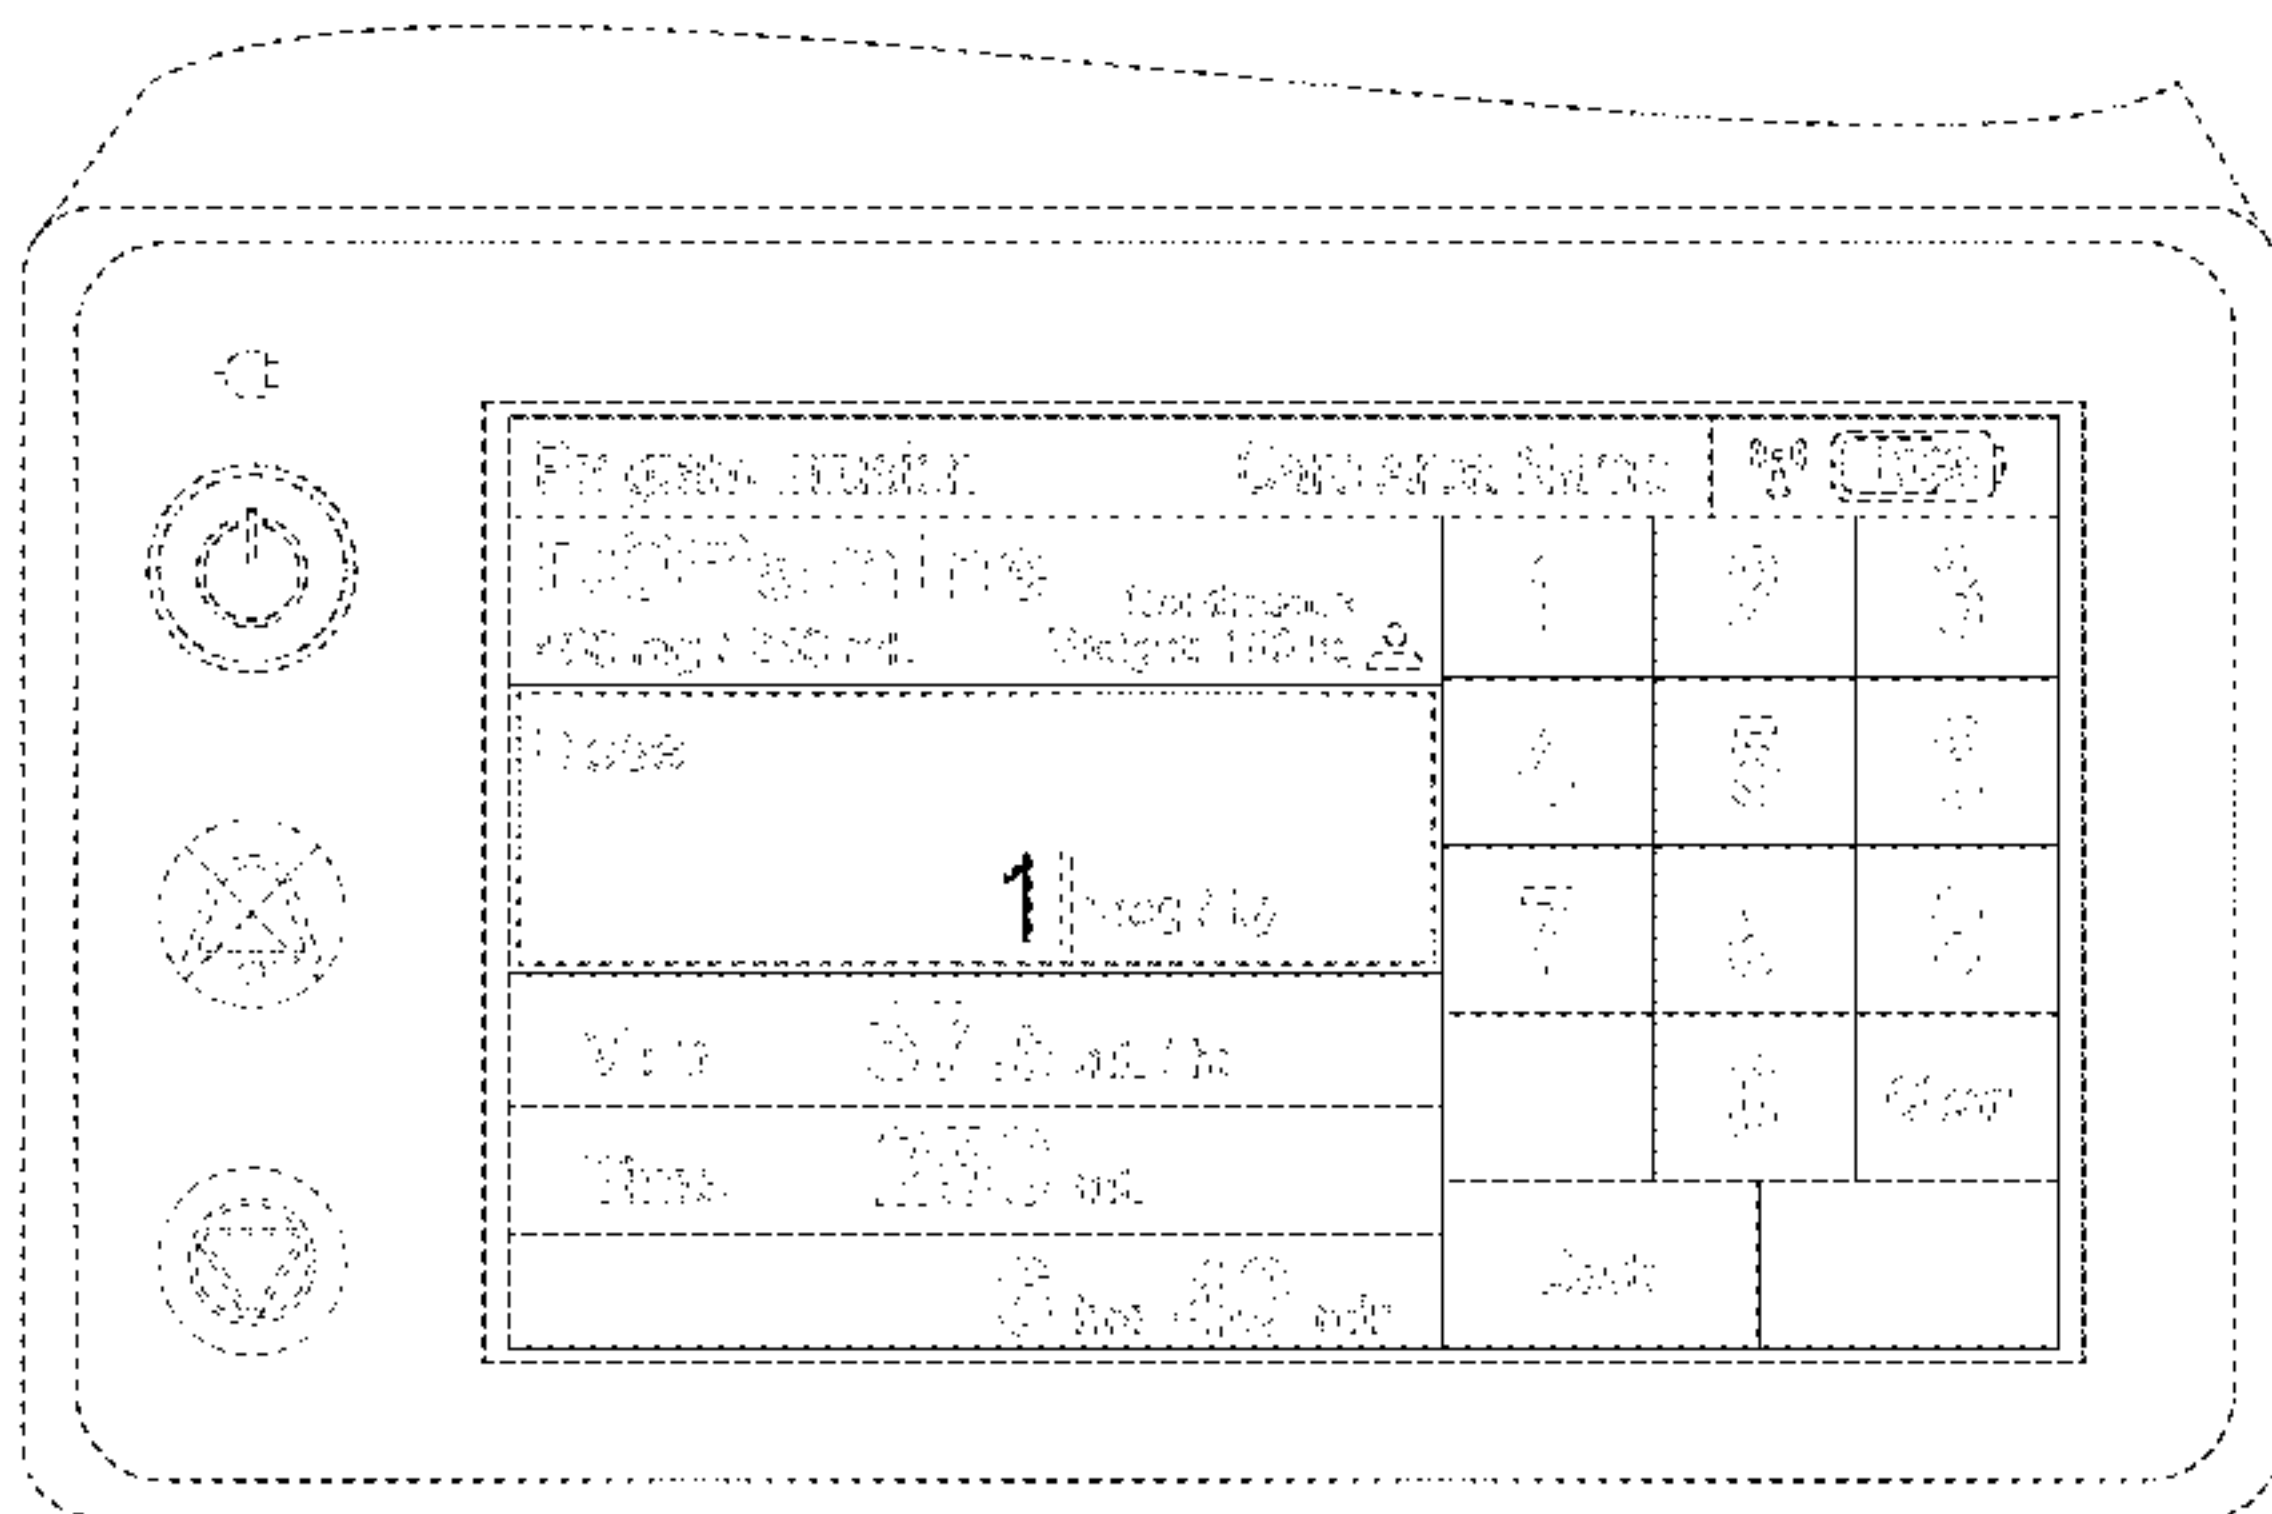

(56)

References Cited

U.S. PATENT DOCUMENTS

D705,248 S * 5/2014 McCormack D14/486
 D708,626 S * 7/2014 Klein D14/486
 D708,627 S * 7/2014 Klein D14/486
 D715,320 S * 10/2014 McCormack D14/486
 D716,332 S * 10/2014 Chotin D14/486
 D717,814 S * 11/2014 Zuckerberg D14/486
 D718,776 S * 12/2014 Hobbs D14/486
 D718,777 S * 12/2014 Hobbs D14/486
 D718,778 S * 12/2014 Hobbs D14/486
 D719,963 S * 12/2014 Hobbs D14/486
 D719,964 S * 12/2014 Hobbs D14/486
 D721,719 S * 1/2015 Lee D14/486
 D722,612 S * 2/2015 Lee D14/486
 D723,052 S * 2/2015 Lai D14/486
 D725,670 S * 3/2015 Zhang D14/488
 D728,779 S 5/2015 Sabin et al.
 D731,509 S * 6/2015 Sueishi D14/486
 D735,319 S 7/2015 Sabin et al.
 D735,746 S * 8/2015 Zuckerberg D14/486
 D736,370 S 8/2015 Sabin et al.
 9,151,646 B2 10/2015 Kamen et al.
 D745,661 S 12/2015 Collins et al.
 D749,206 S 2/2016 Johnson et al.
 9,295,778 B2 3/2016 Kamen et al.
 2005/0050301 A1 * 3/2005 Whittle G06F 9/4443
 712/32
 2005/0267827 A1 * 12/2005 Grant, Jr. G06Q 40/08
 705/35
 2009/0144620 A1 * 6/2009 Bauchot G06F 17/2288
 715/277
 2010/0153872 A1 * 6/2010 Ahn G06F 3/0481
 715/768
 2010/0169389 A1 * 7/2010 Weber G06F 17/30056
 707/804
 2010/0169783 A1 * 7/2010 Weber G11B 27/034
 715/731
 2011/0161806 A1 * 6/2011 Stern G06F 17/211
 715/247
 2011/0271221 A1 * 11/2011 Lategan G06F 8/70
 715/772
 2011/0313789 A1 12/2011 Kamen et al.
 2012/0079416 A1 * 3/2012 Fagans H04N 1/3875
 715/781
 2012/0185267 A1 7/2012 Kamen
 2012/0254044 A1 * 10/2012 Flanagan G06Q 10/06395
 705/301
 2013/0127870 A1 * 5/2013 Baudel G06F 9/4443
 345/441
 2013/0177455 A1 7/2013 Kamen
 2013/0182381 A1 7/2013 Gray
 2013/0184676 A1 7/2013 Kamen
 2013/0188040 A1 7/2013 Kamen

2013/0191513 A1 7/2013 Kamen
 2013/0197693 A1 8/2013 Kamen
 2013/0204188 A1 8/2013 Kamen
 2013/0272773 A1 10/2013 Kamen
 2013/0281965 A1 10/2013 Kamen
 2013/0297330 A1 11/2013 Kamen
 2013/0310990 A1 11/2013 Peret et al.
 2013/0317753 A1 11/2013 Kamen
 2013/0317837 A1 11/2013 Ballantyne
 2013/0318429 A1 * 11/2013 Dantas G06F 3/048
 715/234
 2013/0336814 A1 12/2013 Kamen
 2013/0339049 A1 12/2013 Blumberg, Jr.
 2013/0346108 A1 12/2013 Kamen
 2014/0165703 A1 6/2014 Wilt
 2014/0180711 A1 6/2014 Kamen
 2014/0188076 A1 7/2014 Kamen
 2014/0188516 A1 7/2014 Kamen
 2014/0195639 A1 7/2014 Kamen
 2014/0227021 A1 8/2014 Kamen
 2014/0318639 A1 10/2014 Peret
 2014/0343492 A1 11/2014 Kamen
 2015/0002667 A1 1/2015 Peret et al.
 2015/0002668 A1 1/2015 Peret et al.
 2015/0002677 A1 1/2015 Peret et al.
 2015/0033823 A1 2/2015 Blumberg, Jr.
 2015/0089364 A1 * 3/2015 Meller G06F 3/0488
 715/708
 2015/0154364 A1 6/2015 Biasi et al.
 2015/0157791 A1 6/2015 Desch et al.
 2015/0257974 A1 9/2015 Demers et al.
 2015/0314083 A1 11/2015 Blumberg, Jr. et al.
 2015/0332009 A1 11/2015 Kane et al.
 2016/0055397 A1 2/2016 Peret et al.
 2016/0055649 A1 2/2016 Peret et al.
 2016/0061641 A1 3/2016 Peret et al.
 2016/0063353 A1 3/2016 Peret et al.
 2016/0073063 A1 3/2016 Peret et al.

FOREIGN PATENT DOCUMENTS

WO WO2013096718 A2 6/2013
 WO WO2013096722 A2 6/2013
 WO WO2013096909 A2 6/2013
 WO WO2013176770 A2 11/2013
 WO WO2013177357 A1 11/2013
 WO WO2014100557 A2 6/2014
 WO WO2014100571 A2 6/2014
 WO WO2014100658 A1 6/2014
 WO WO2014100687 A2 6/2014
 WO WO2014100736 A2 6/2014
 WO WO2014100744 A2 6/2014
 WO WO2014144557 A2 9/2014
 WO WO2015017275 A1 2/2015

* cited by examiner

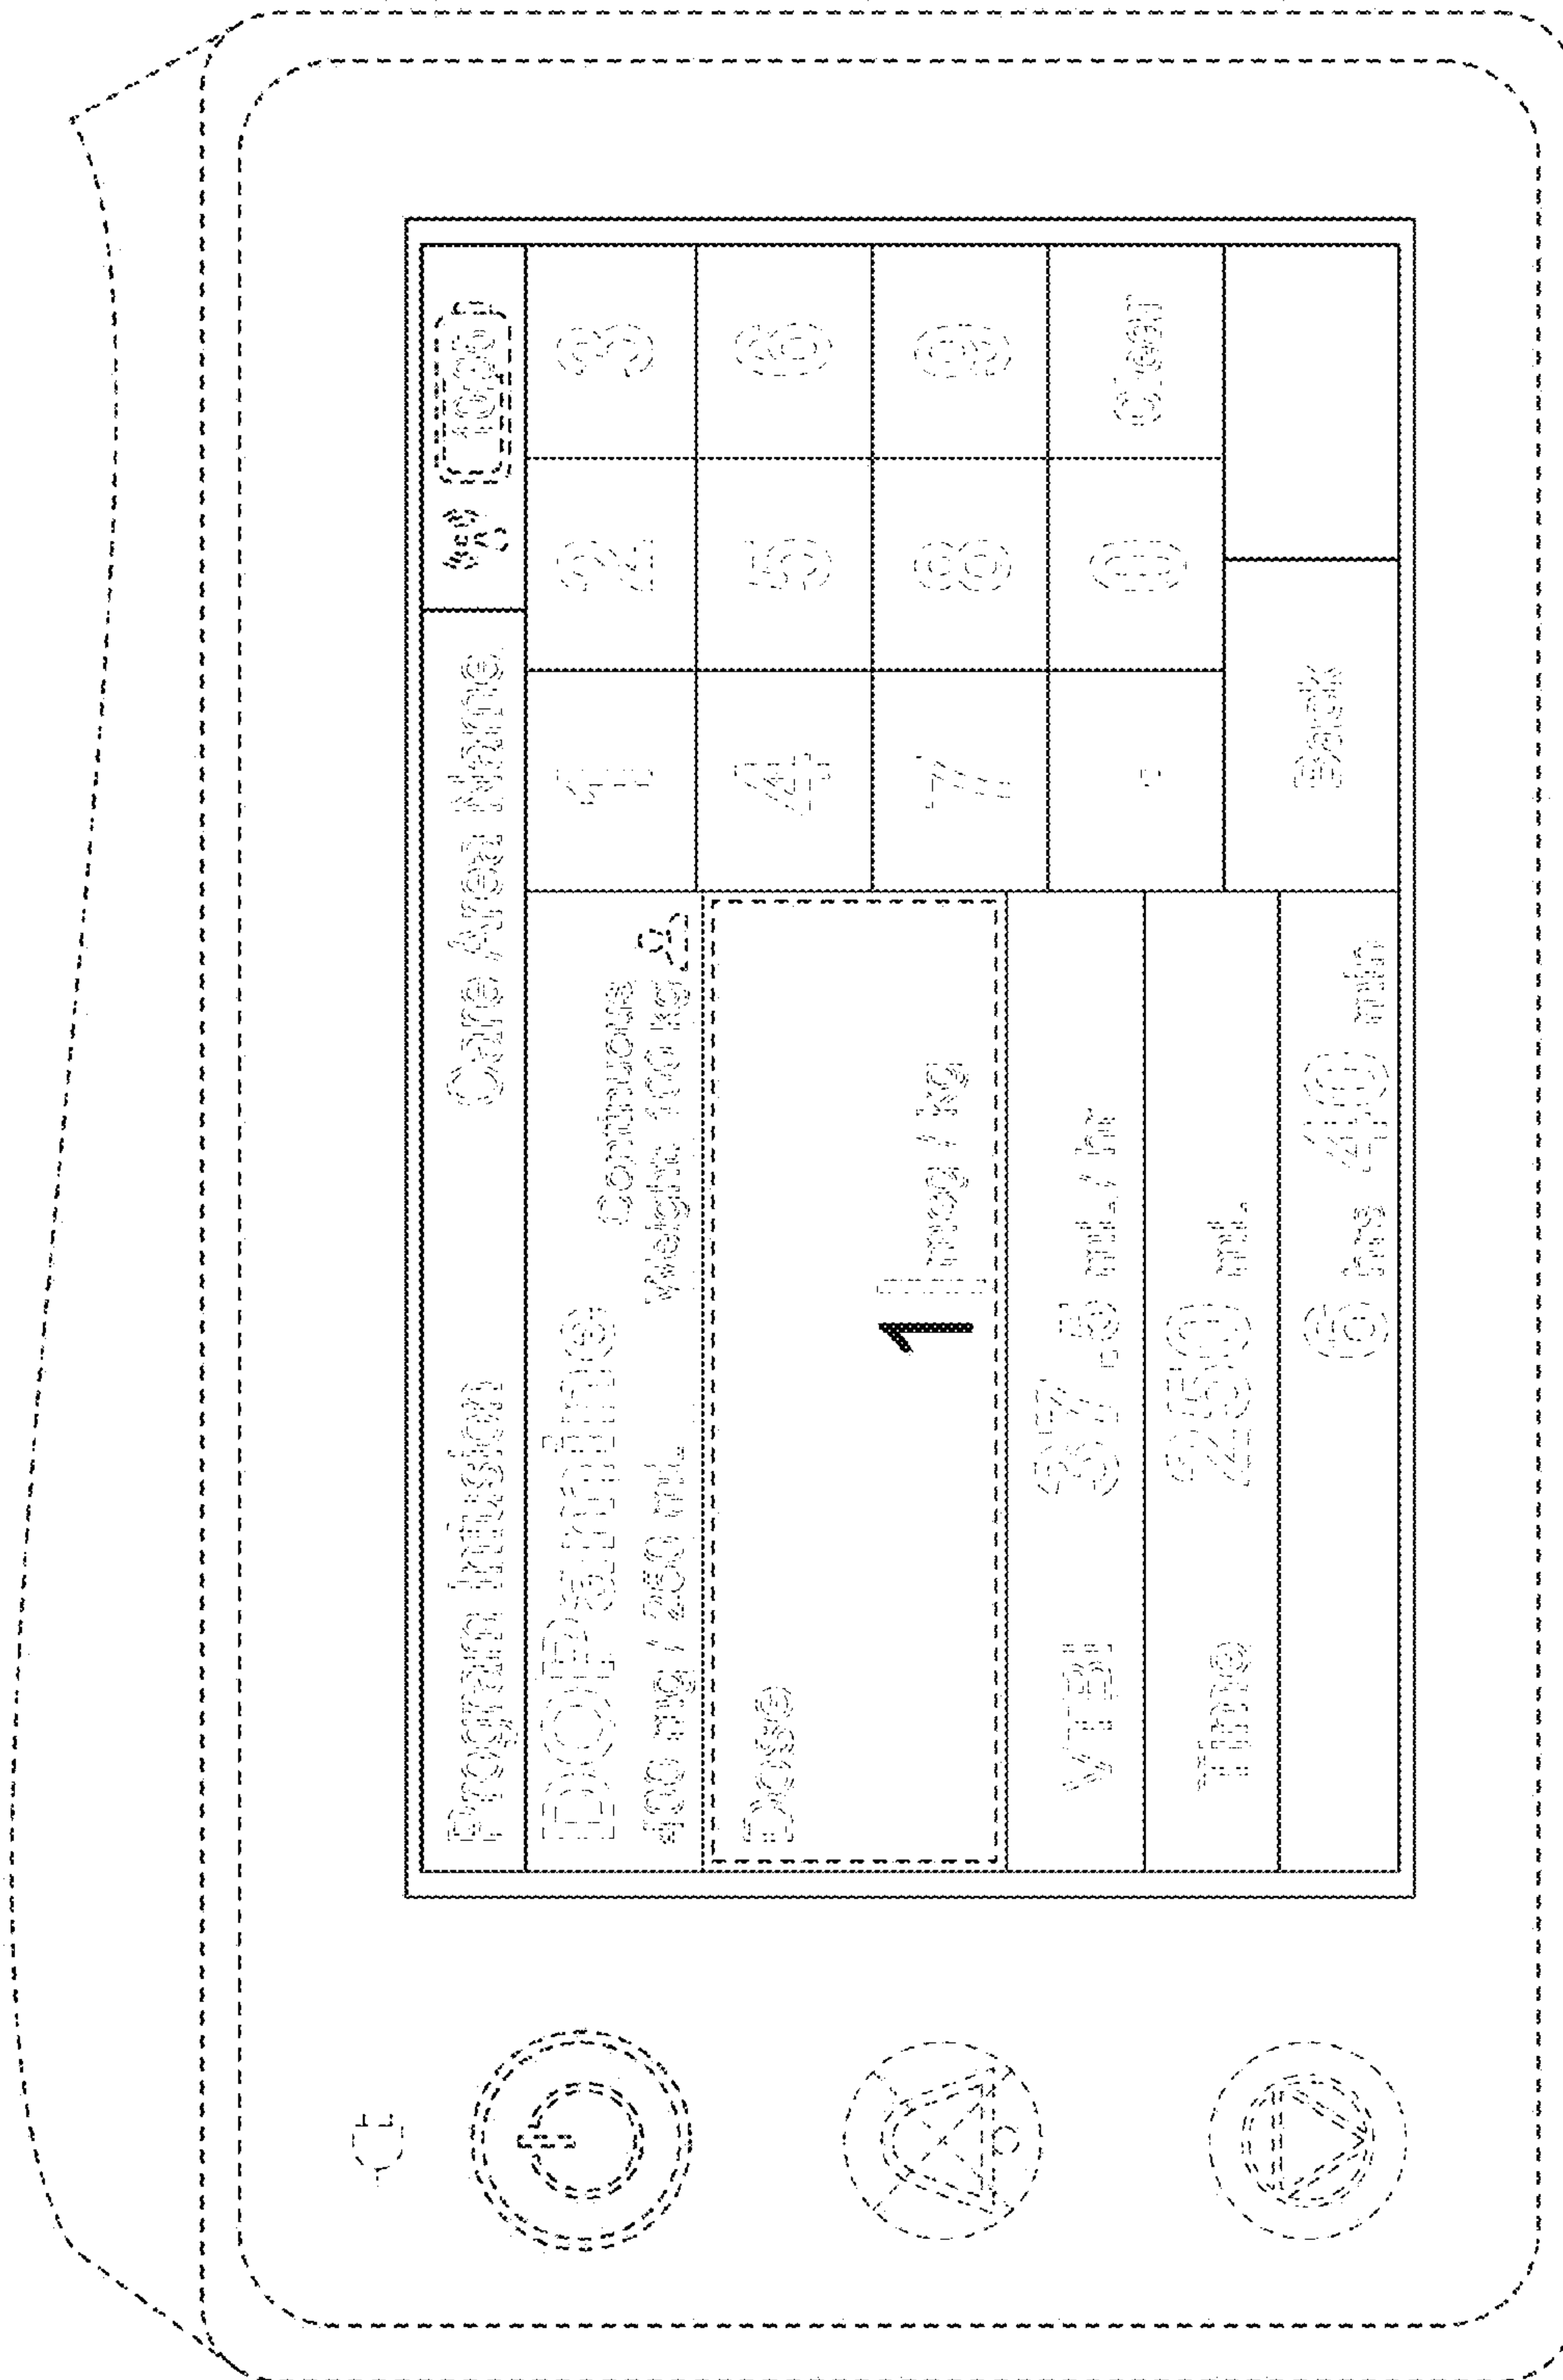


FIG. 1

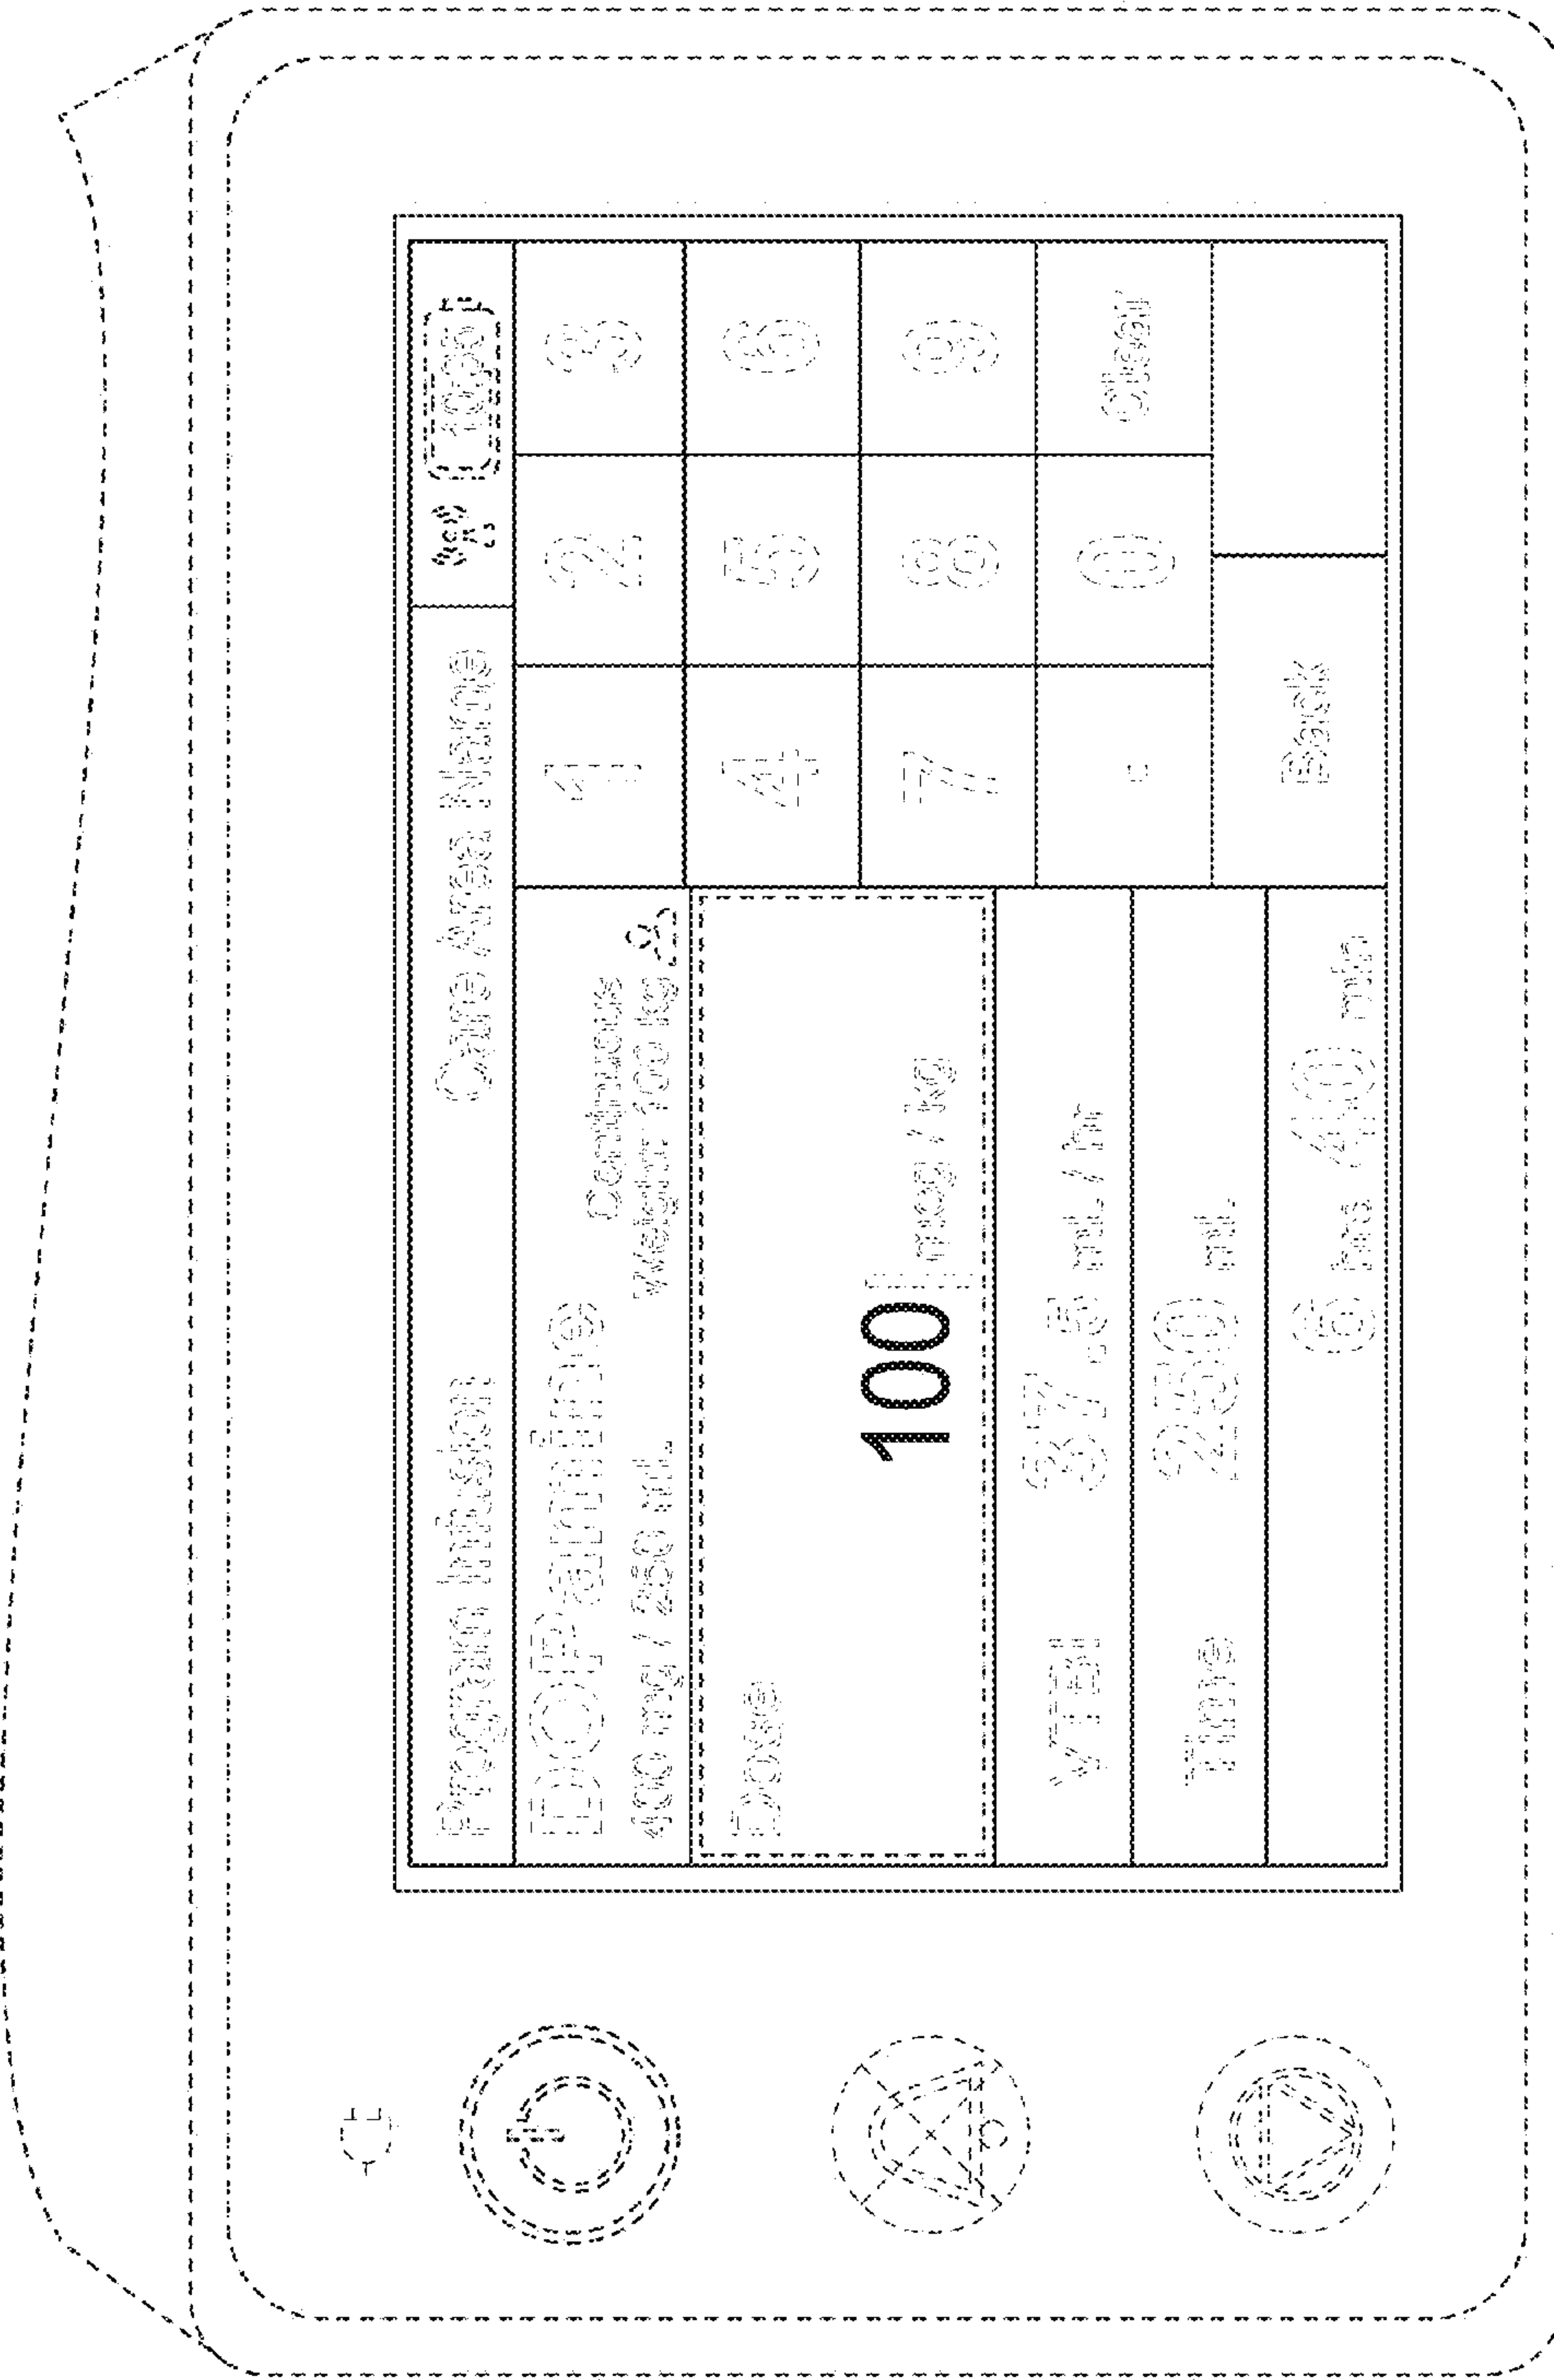


FIG. 2

Program	Infusion	Care Area Name	Unit	Rate
EDICOP	paumilime	Continuous	3	3
400 mg / 250 mL	Weight: 100 kg		2	6
Dose	10,000 mg / hr		5	9
VTEI	37.5 mL / hr		8	Clear
Time	250 mL		10	
	6 hrs	4:00 min	Back	

FIG. 3

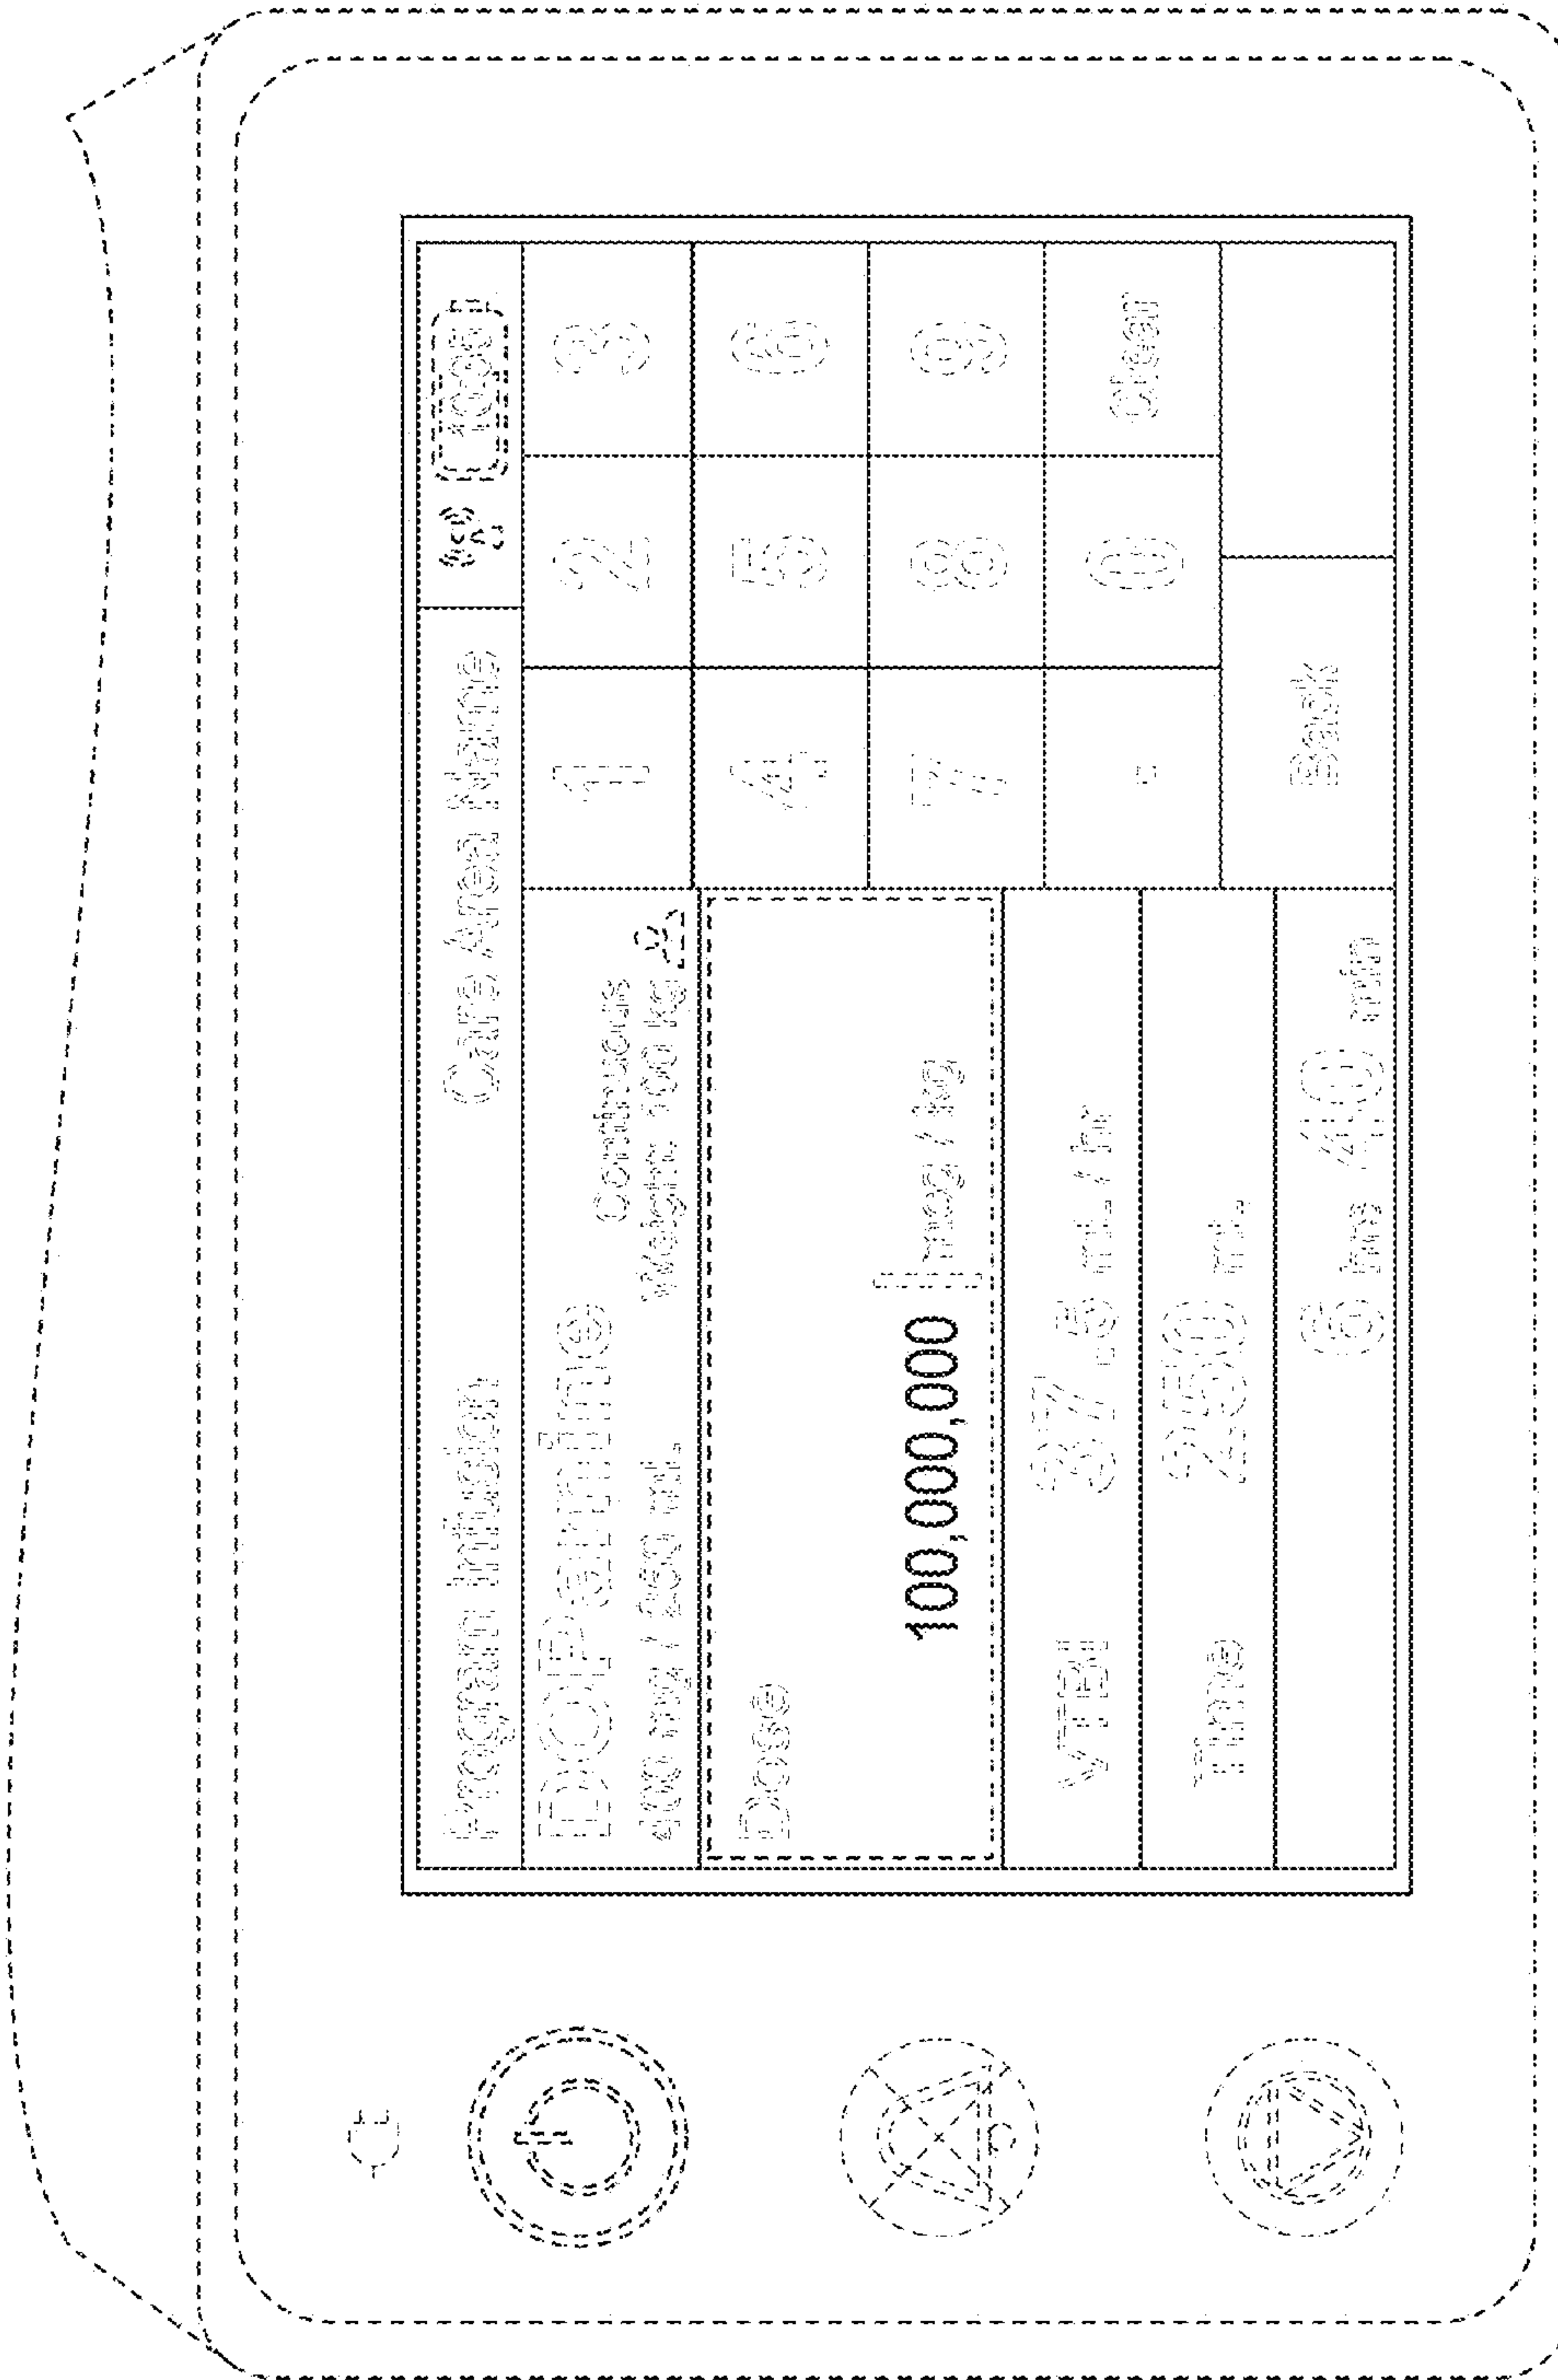


FIG. 4

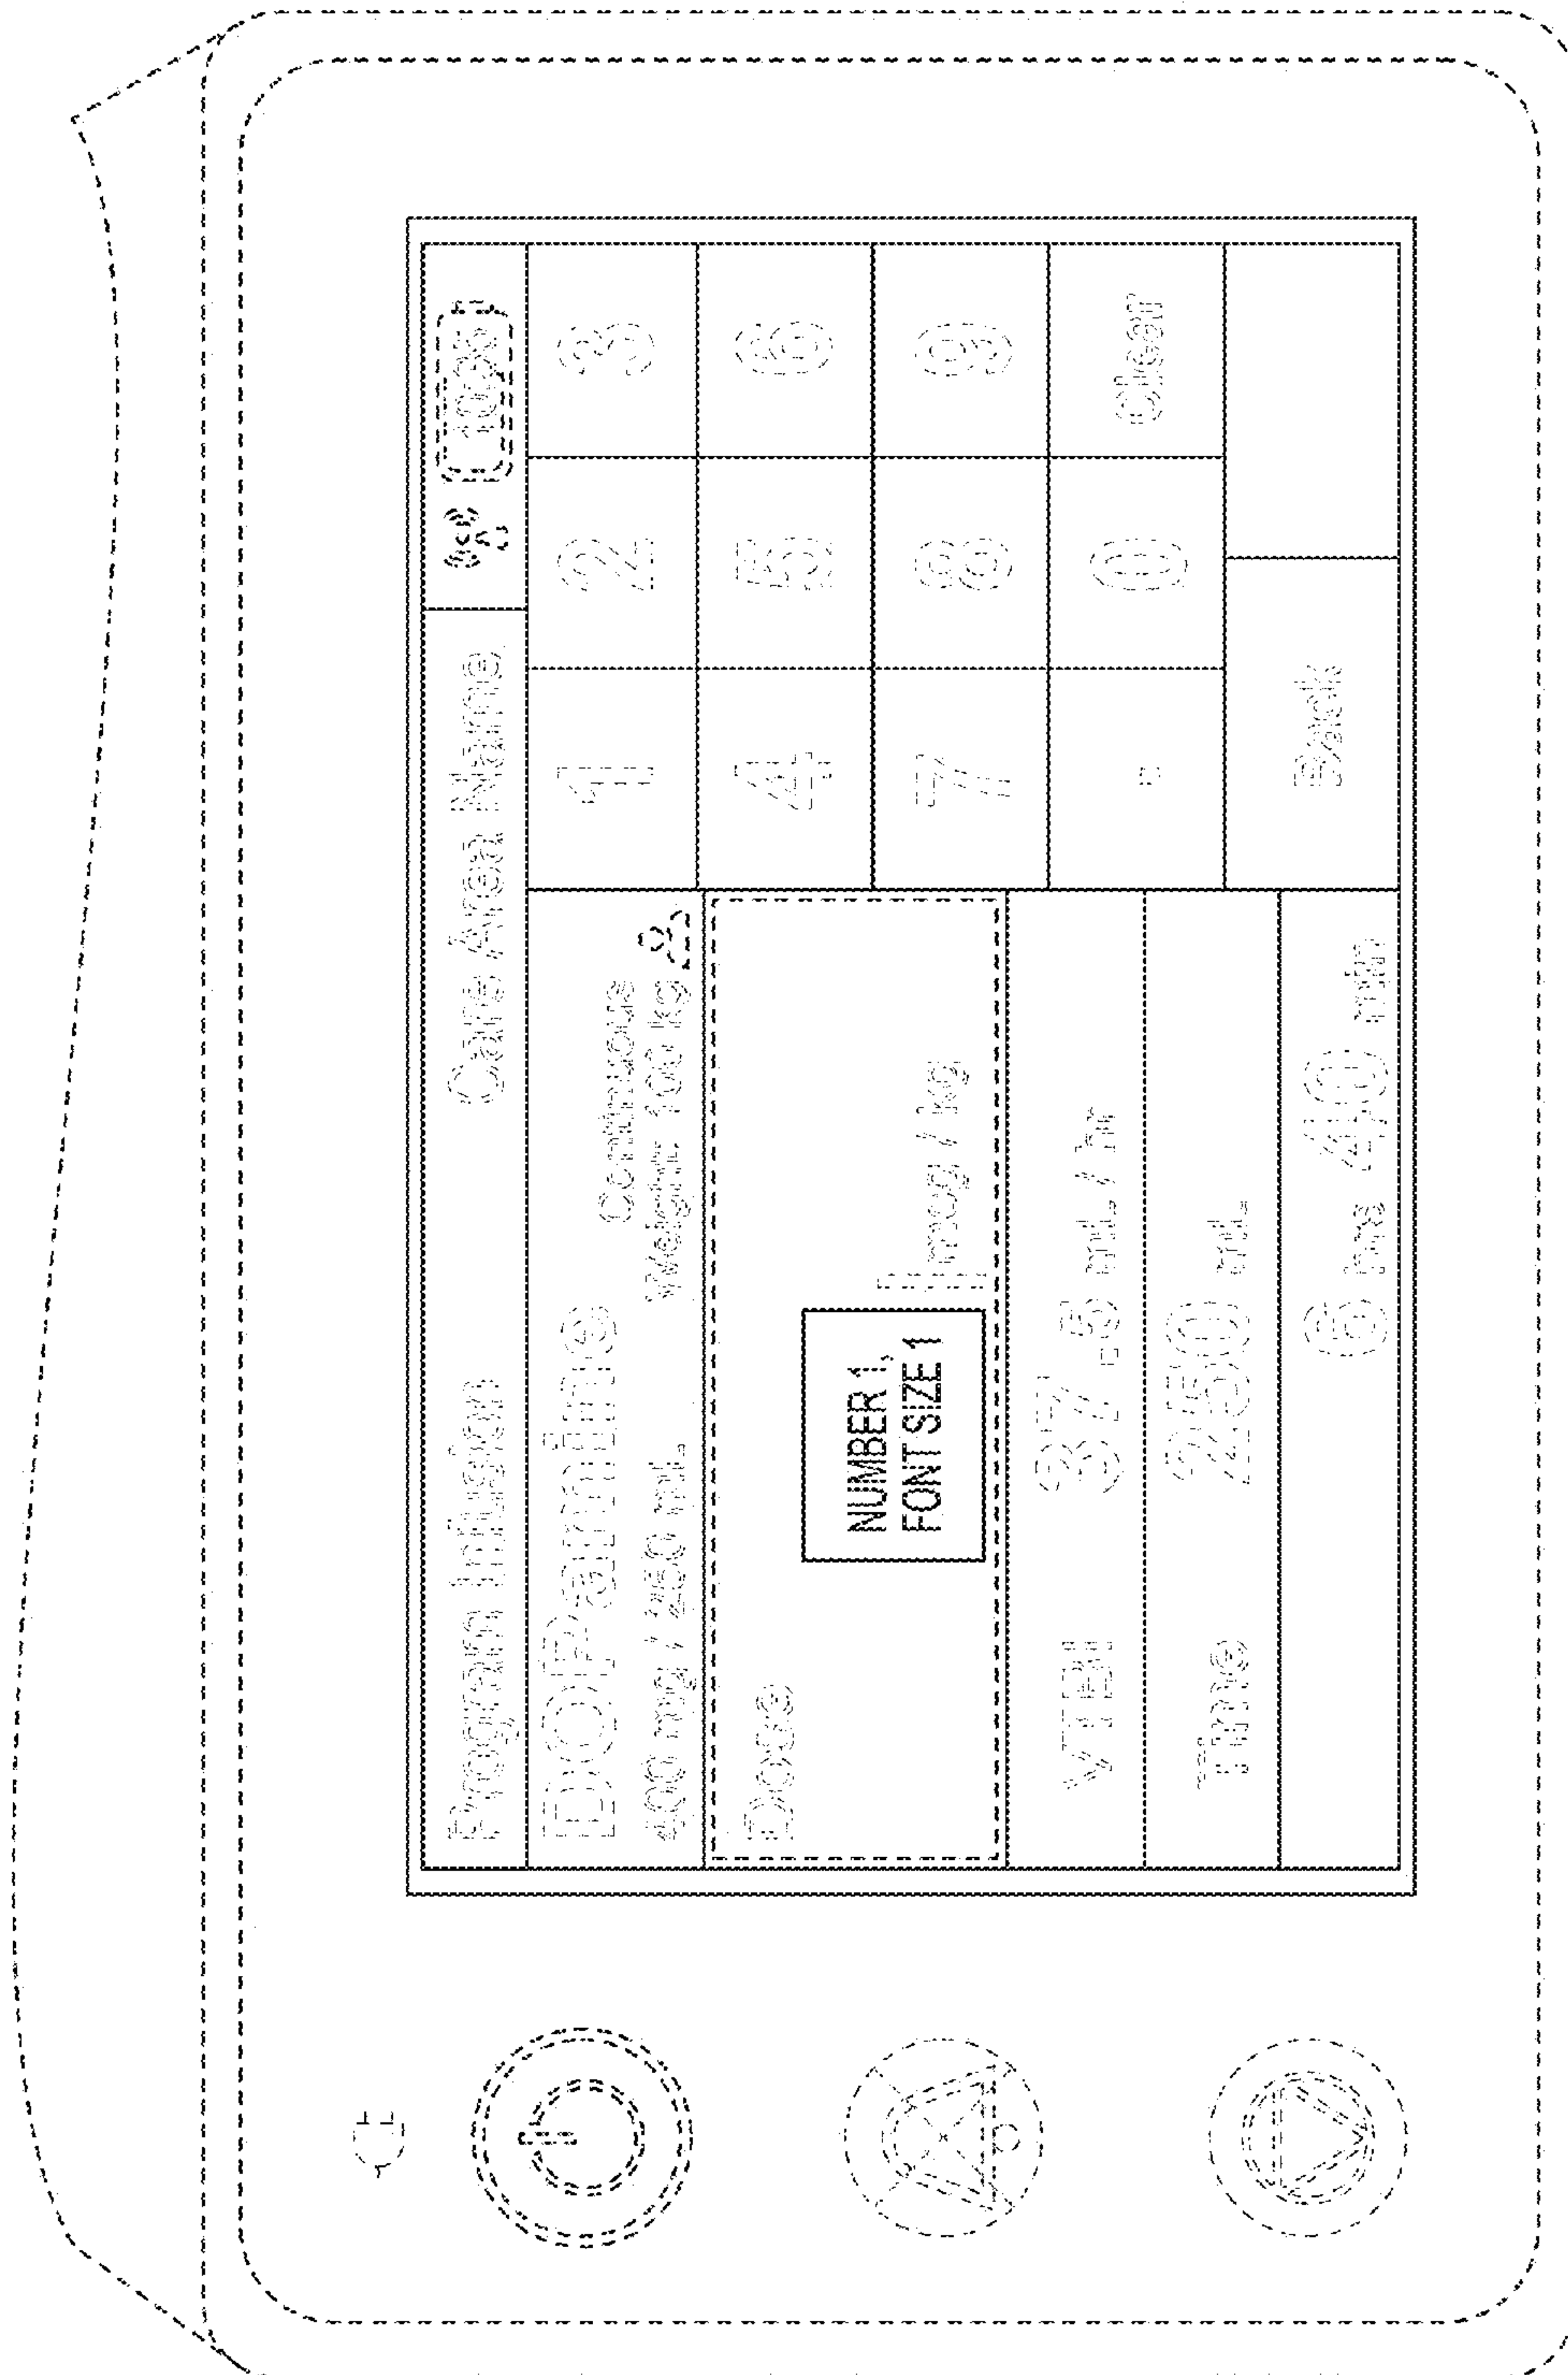


FIG. 5

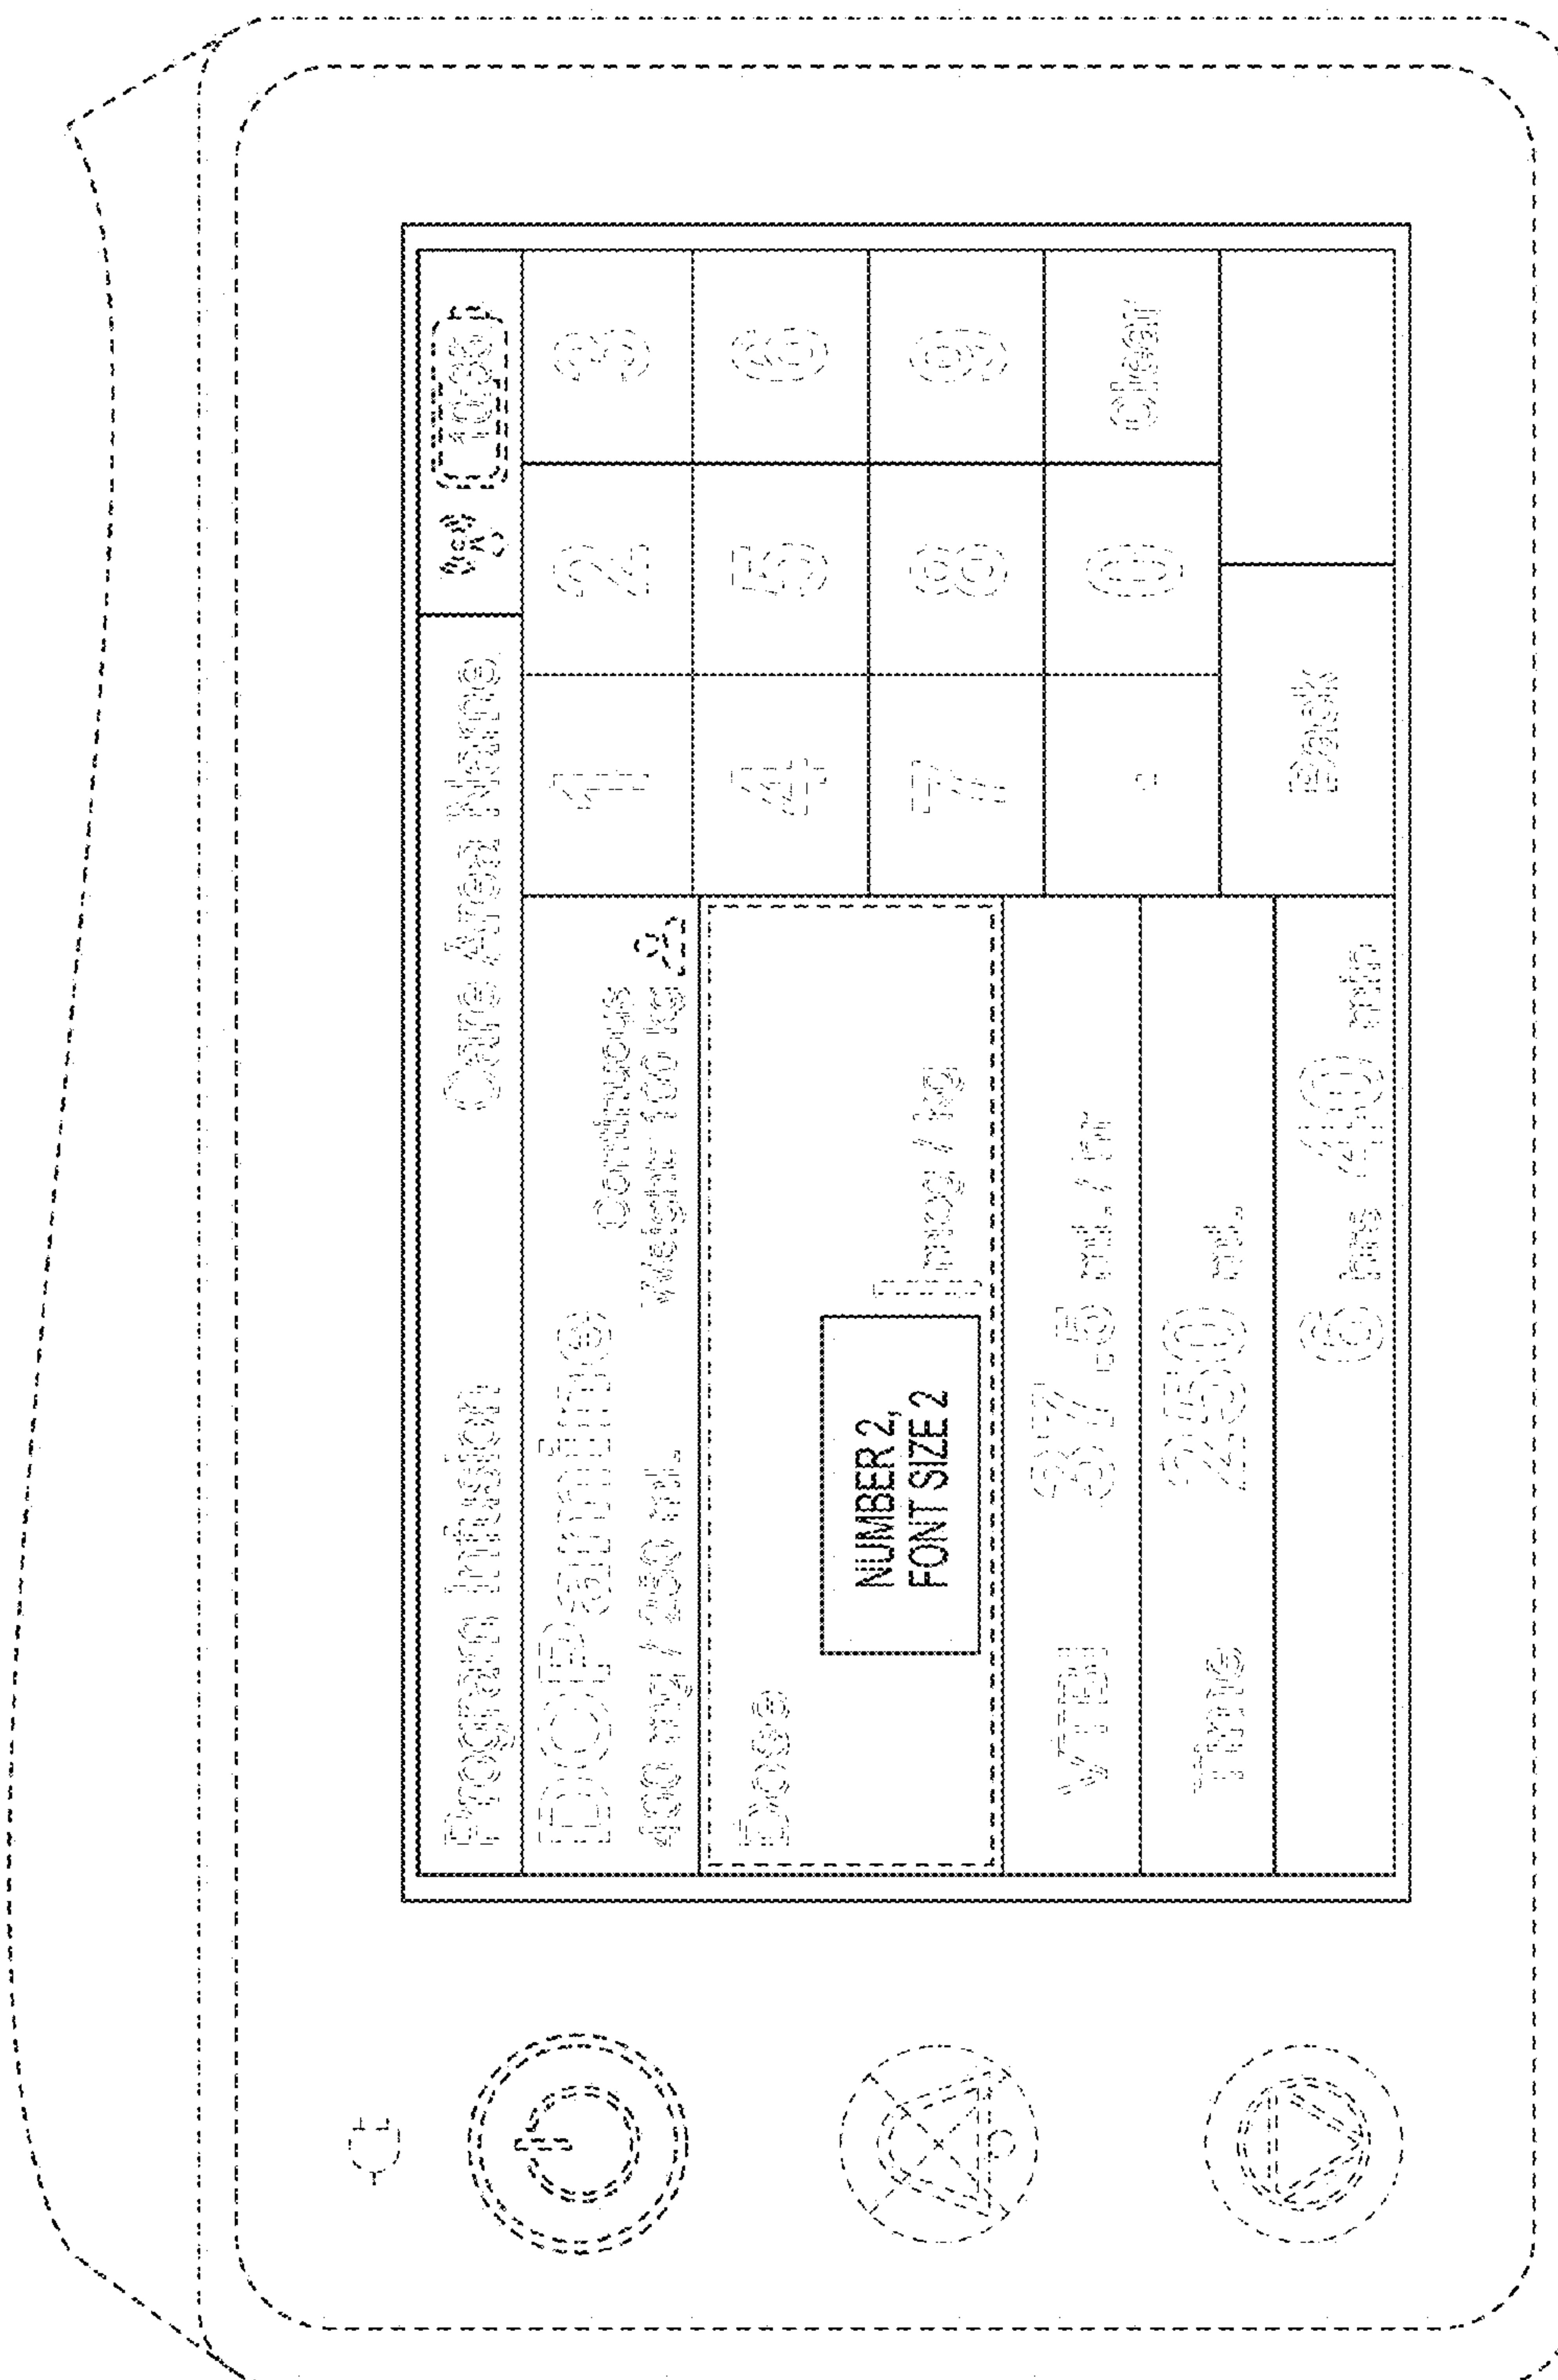


FIG. 6

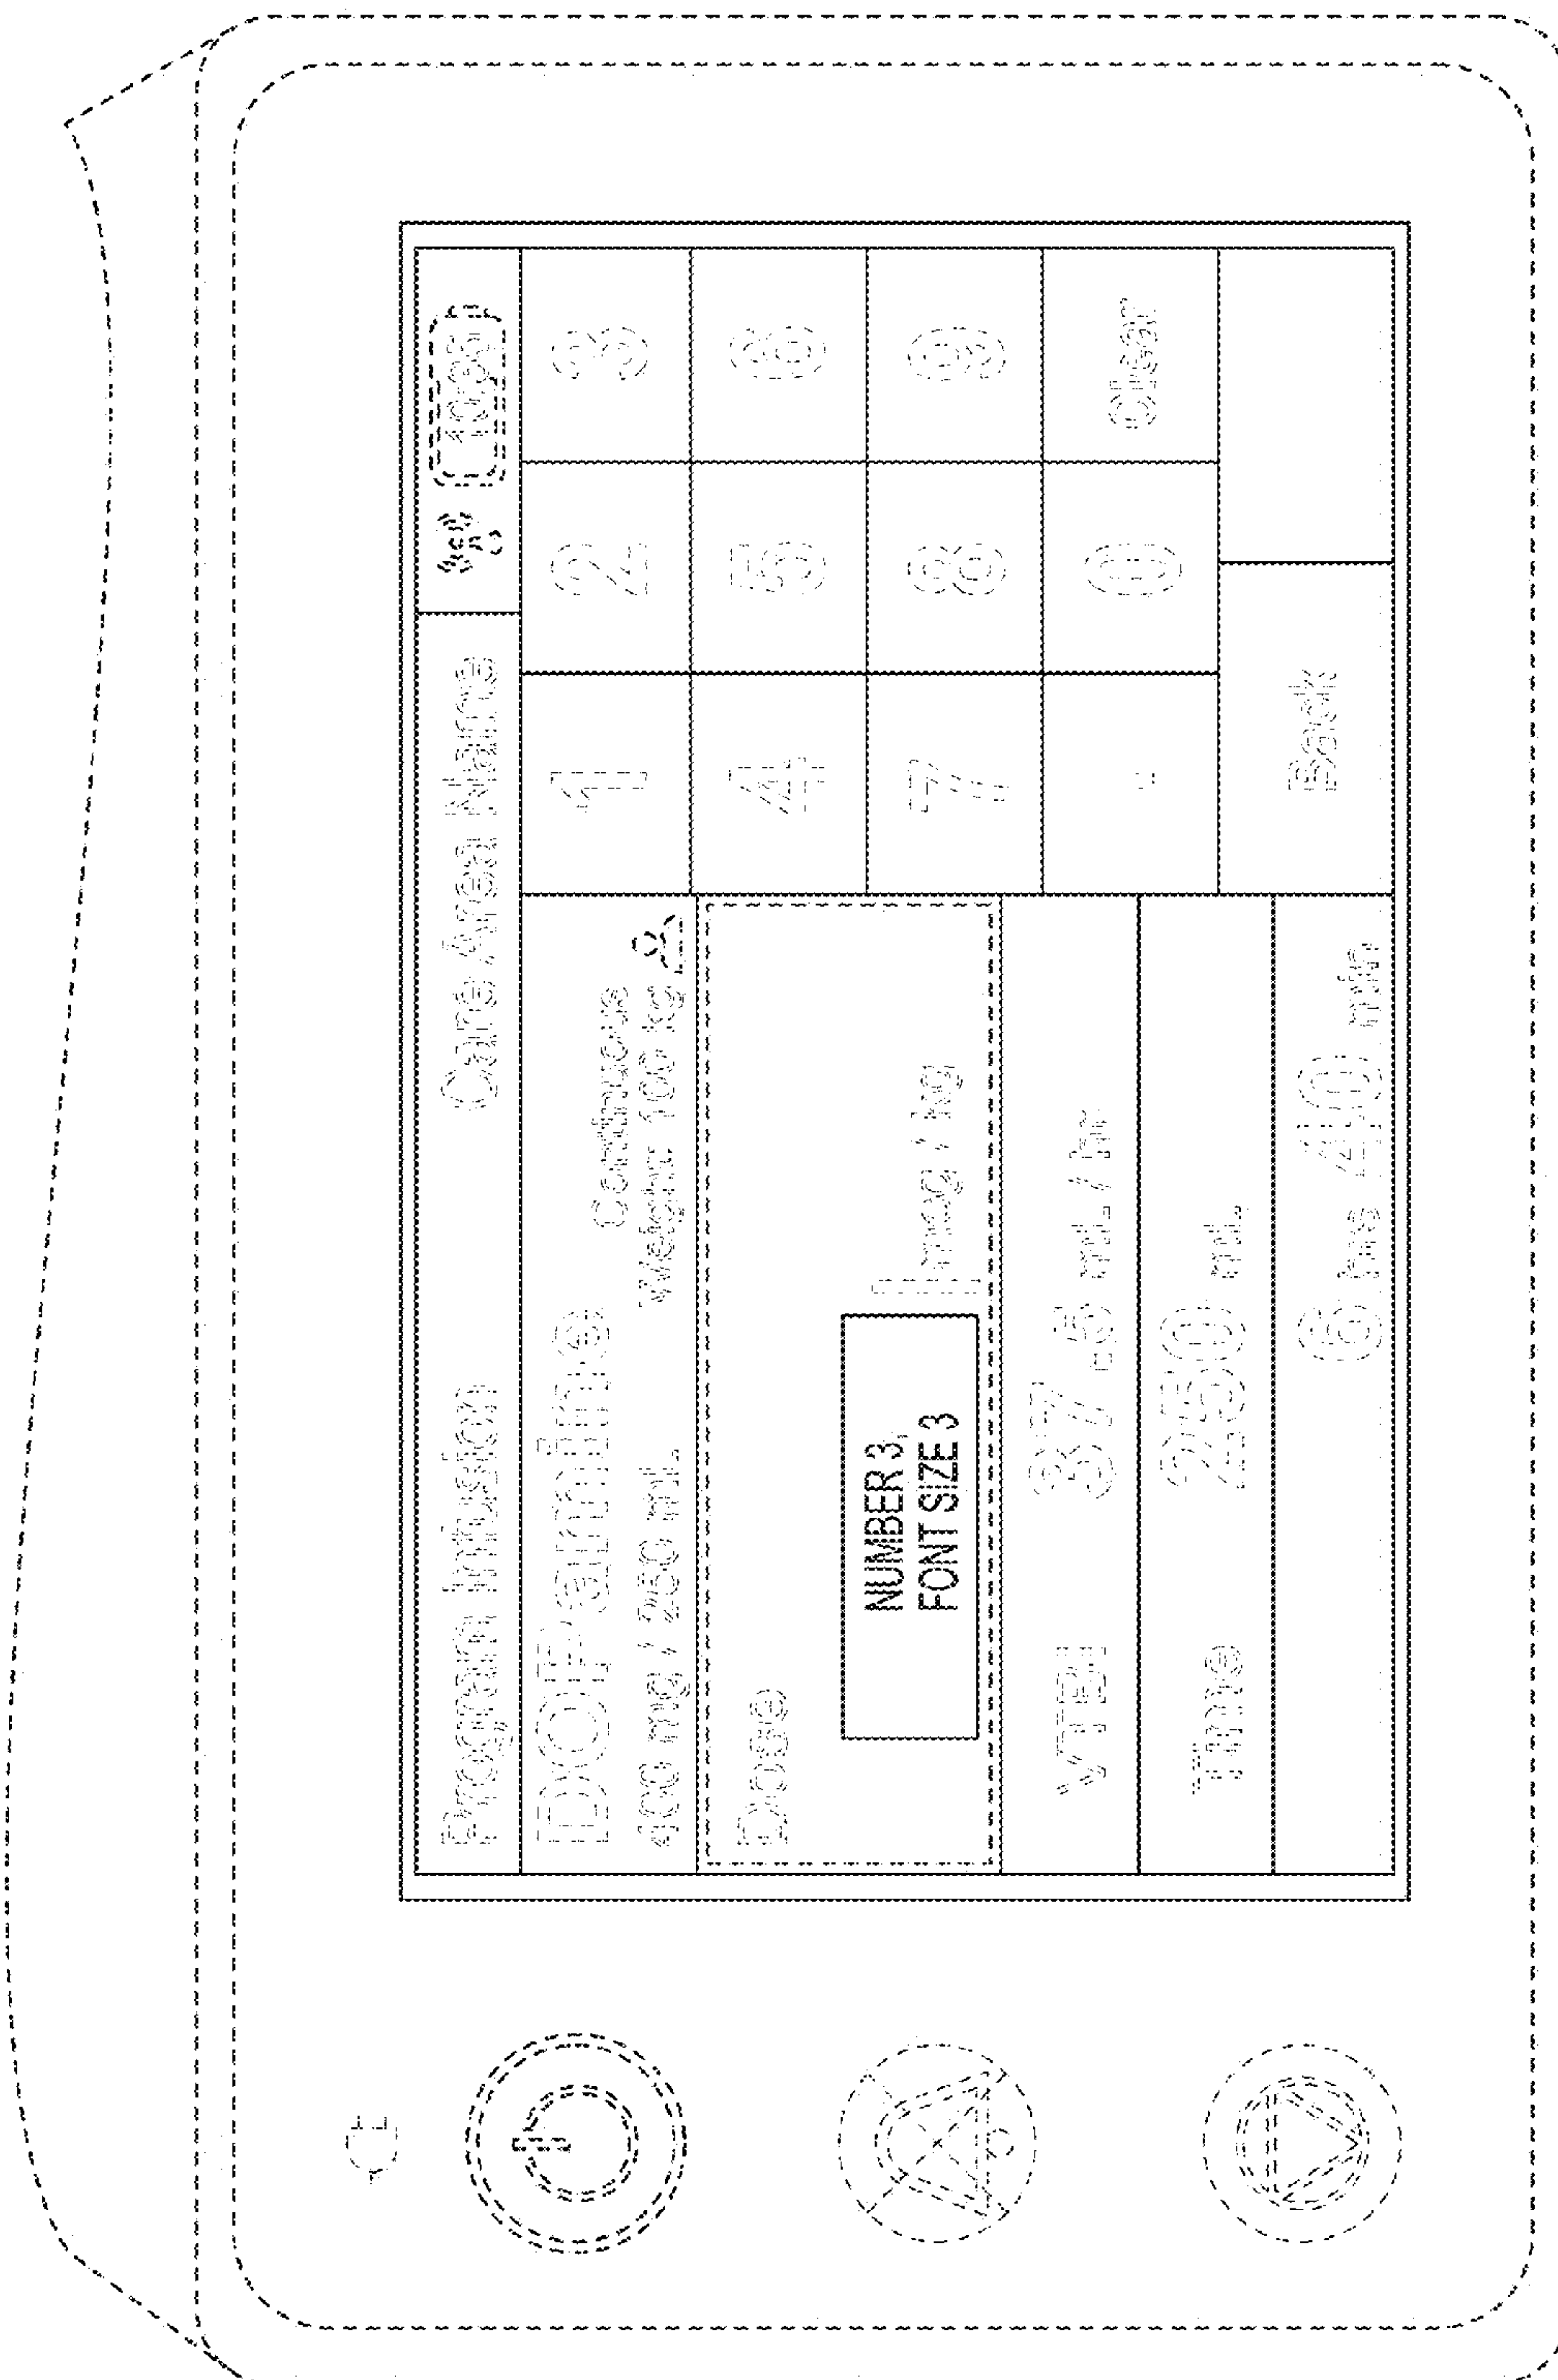


FIG. 7

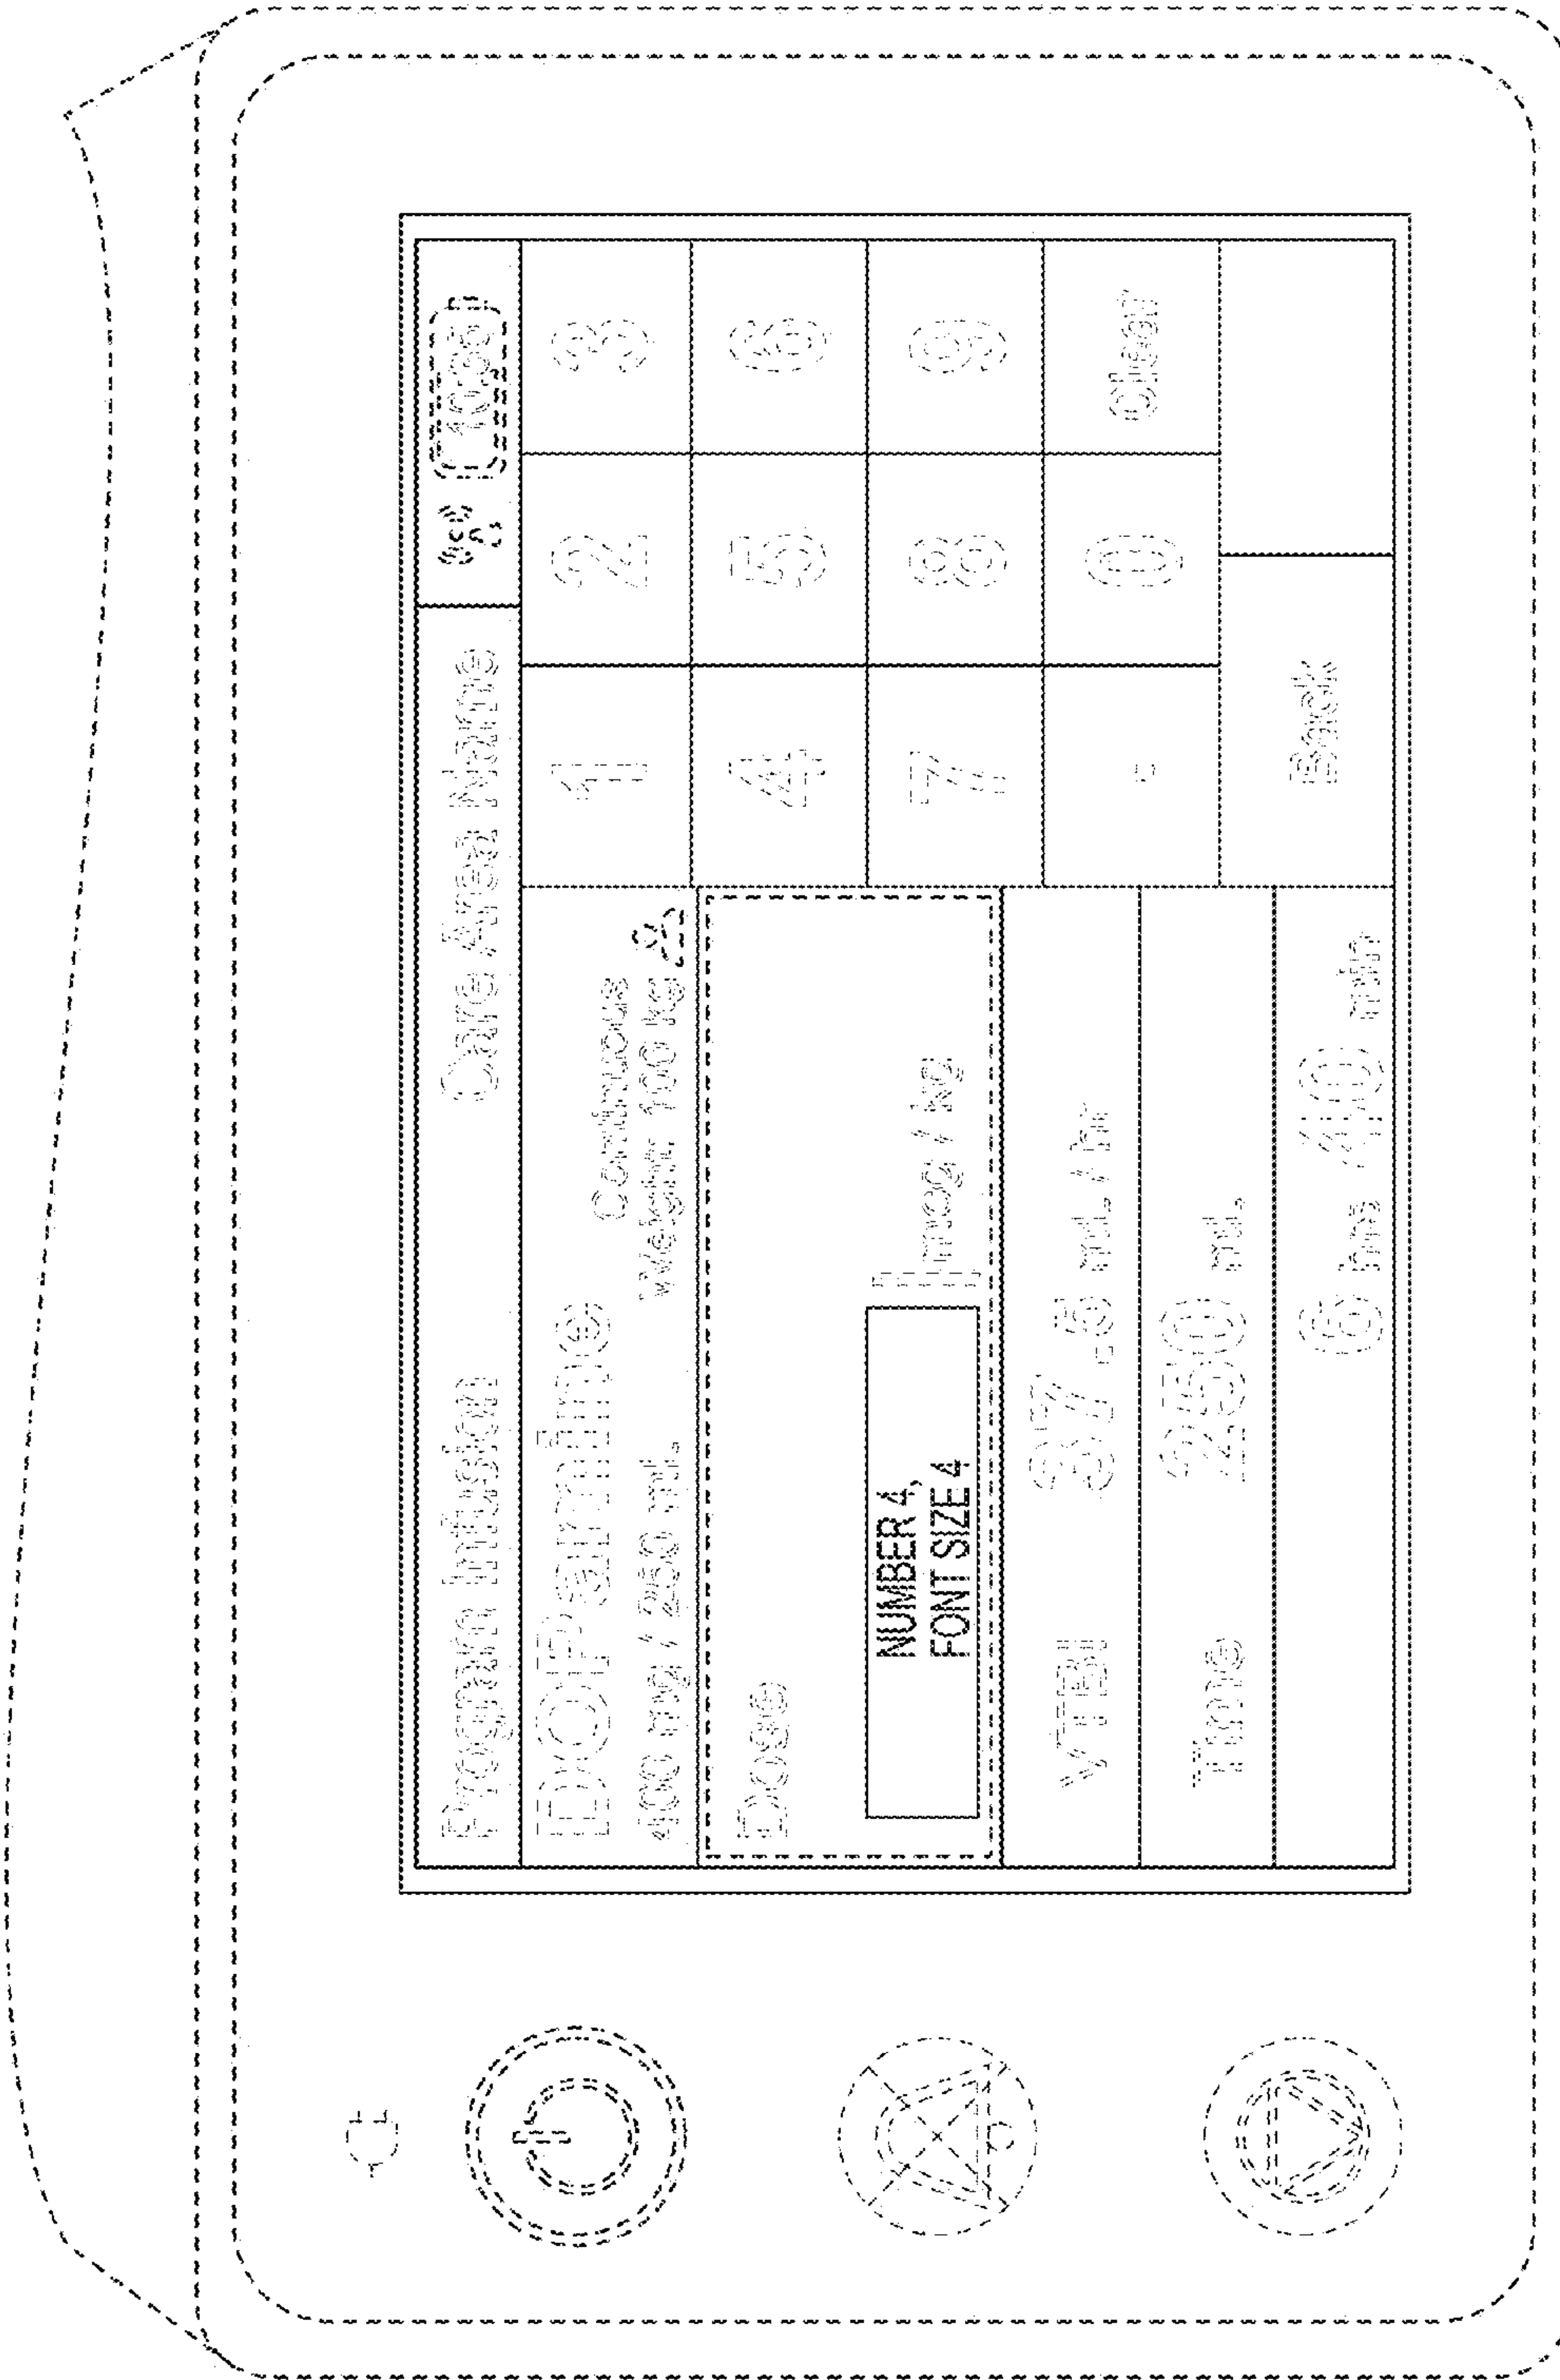


FIG. 8