



US00D763939S

(12) **United States Design Patent**
Khanicheh et al.

(10) **Patent No.:** **US D763,939 S**
(45) **Date of Patent:** **** Aug. 16, 2016**

(54) **OPTICAL SENSOR ARRAY LINER WITH
OPTICAL SENSOR ARRAY PAD**

(71) Applicant: **Cephalogics, LLC**, Boston, MA (US)

(72) Inventors: **Azadeh Khanicheh**, Wakefield, MA (US); **Judy Walish**, Brighton, MA (US); **Melissa Rosen Ceruolo**, Salem, MA (US); **Michel Bruehwiler**, Newton, MA (US); **Cole Constantineau**, Cambridge, MA (US); **Russell L. Herrig**, Lexington, MA (US); **Jeffery J. Caputo**, Winchester, MA (US)

(73) Assignee: **Cephalogics, LLC**, Boston, MA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/486,804**

(22) Filed: **Apr. 2, 2014**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D16/130; D24/187**

(58) **Field of Classification Search**
USPC D10/46, 64; D16/130, 134, 136;
D24/107, 167, 168, 185, 186, 187, 200,
D24/206, 207, 232, 233; 600/310, 324, 384,
600/391, 393, 425; 607/142, 148, 152
CPC . A61B 5/6801; A61B 5/1455; A61B 5/14553
See application file for complete search history.

(56) **References Cited**


U.S. PATENT DOCUMENTS

3,769,974 A 11/1973 Smart et al.
4,281,645 A 8/1981 Jöbbsis

(Continued)

FOREIGN PATENT DOCUMENTS

JP D1486111 * 12/2013

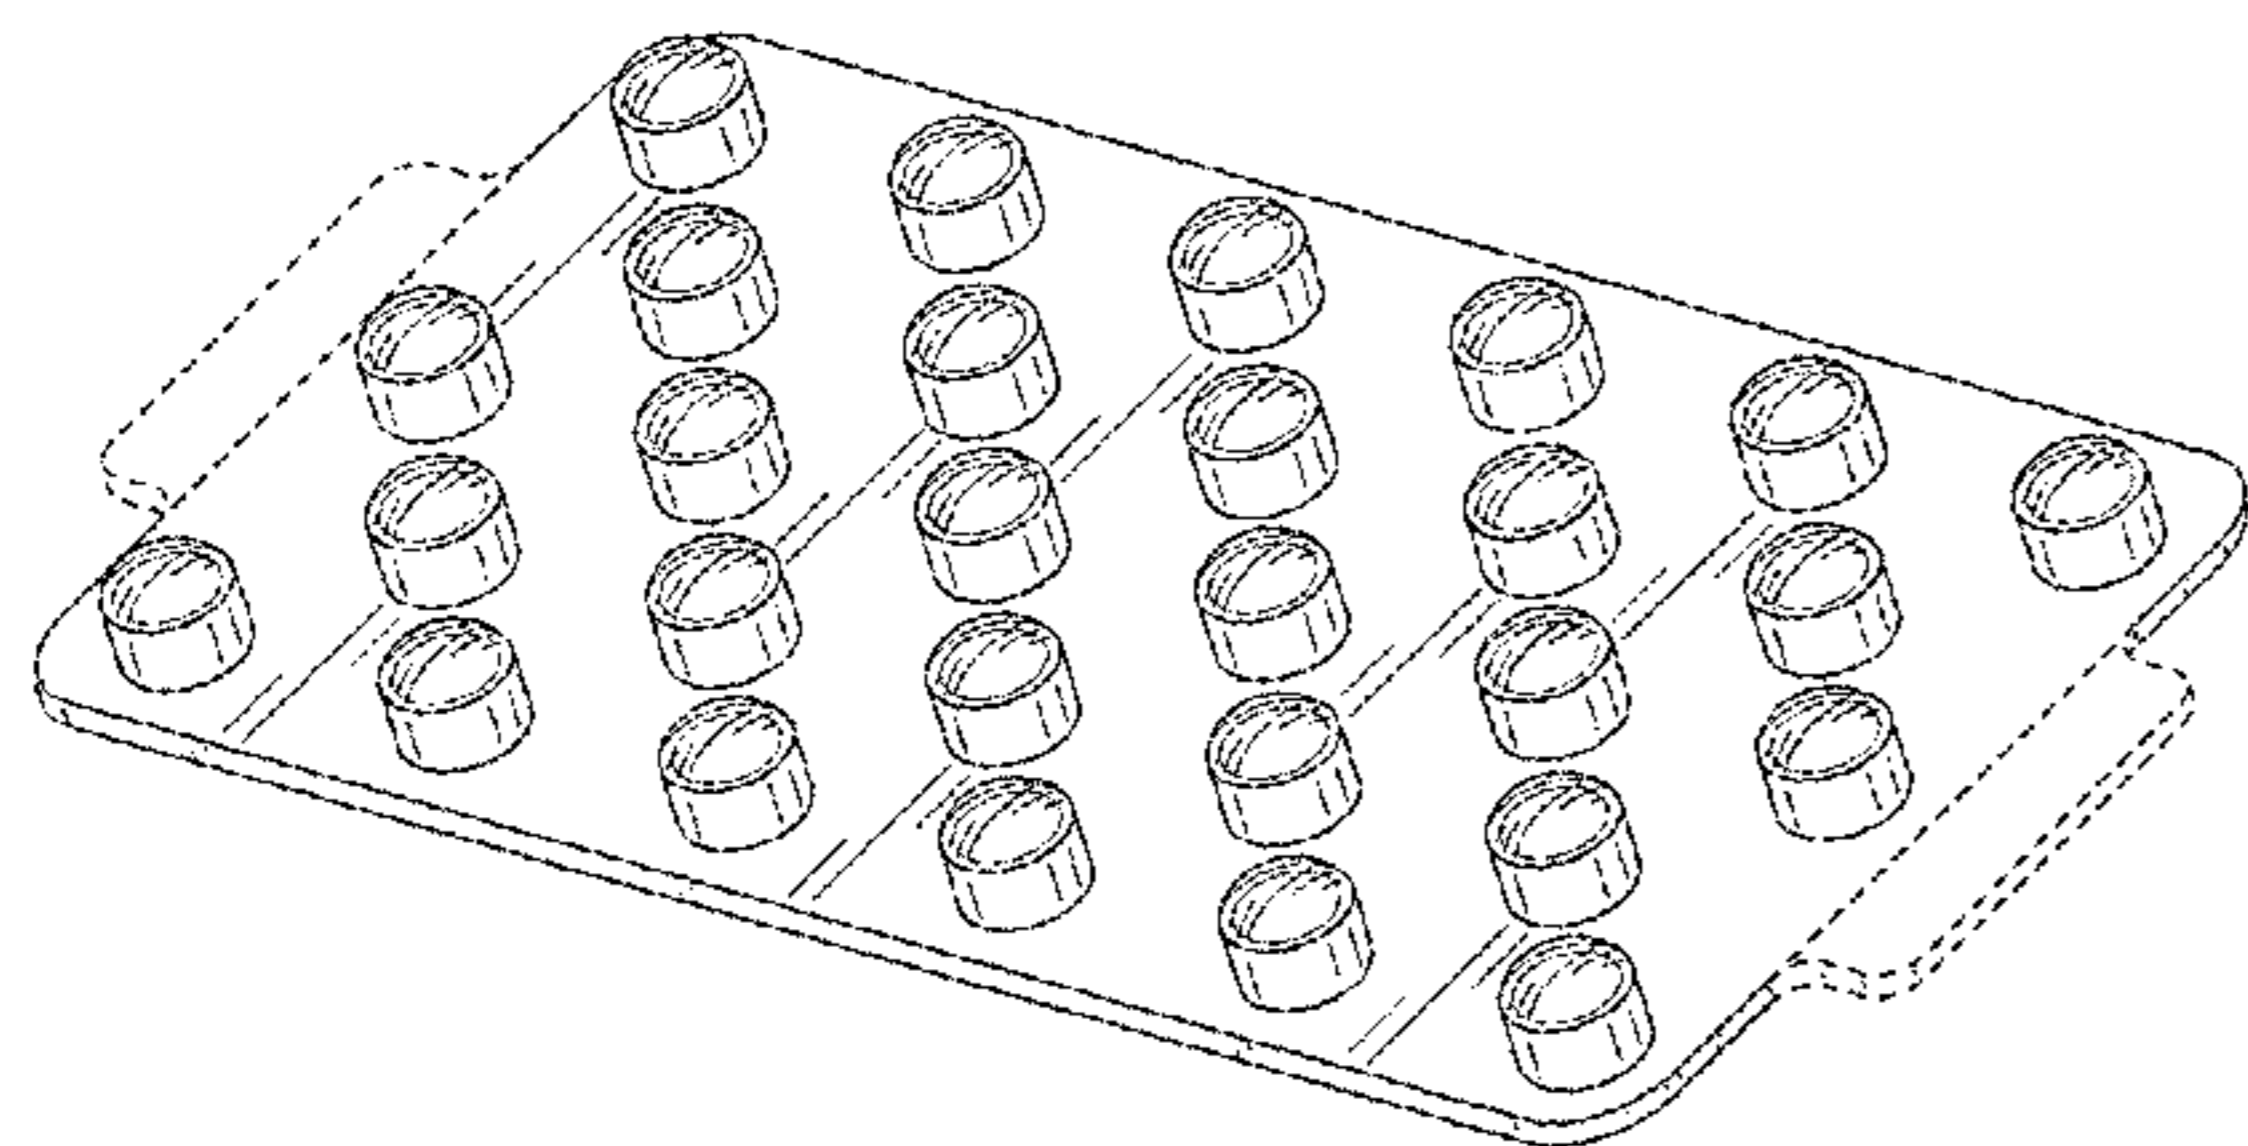

OTHER PUBLICATIONS

[No Author Listed] fNIR Optical Brain Imaging Systems. Product Sheet. Biopac Systems, Inc. 5 pages. https://www.biopac.com/Product_Spec_PDF/fNIR%20Systems.pdf [last updated Mar. 3, 2014].

(Continued)

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Leanne Was

(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

(57) **CLAIM**

The ornamental design for an optical sensor array liner with optical sensor array pad, as shown and described.

DESCRIPTION

FIG. 1 is a front, right perspective view of an optical sensor array liner;

FIG. 2 is a front view of the optical sensor array liner;

FIG. 3 is a back view of the optical sensor array liner;

FIG. 4 is a left side view of the optical sensor array liner;

FIG. 5 is a right side view of the optical sensor array liner;

FIG. 6 is a top view of the optical sensor array liner;

FIG. 7 is a bottom view of the optical sensor array liner;

FIG. 8 is a front, right perspective view of the optical sensor array liner of FIG. 1 positioned on an optical sensor array;

FIG. 9 is a front, right perspective view of an optical sensor array pad;

FIG. 10 is a front view of the optical sensor array pad;

FIG. 11 is a back view of the optical sensor array pad;

FIG. 12 is a left side view of the optical sensor array pad;

FIG. 13 is a right side view of the optical sensor array pad;

FIG. 14 is a top view of the optical sensor array pad;


FIG. 15 is a bottom view of the optical sensor array pad;

FIG. 16 is a front, right perspective view of the optical sensor array pad of FIG. 9 positioned on the optical sensor array liner of FIG. 1; and,

FIG. 17 is a front, right perspective view of the optical sensor array pad of FIG. 9 positioned on the optical sensor array liner of FIG. 1 positioned on an optical sensory array.

The evenly spaced dashed lines depict unclaimed environment.

1 Claim, 13 Drawing Sheets

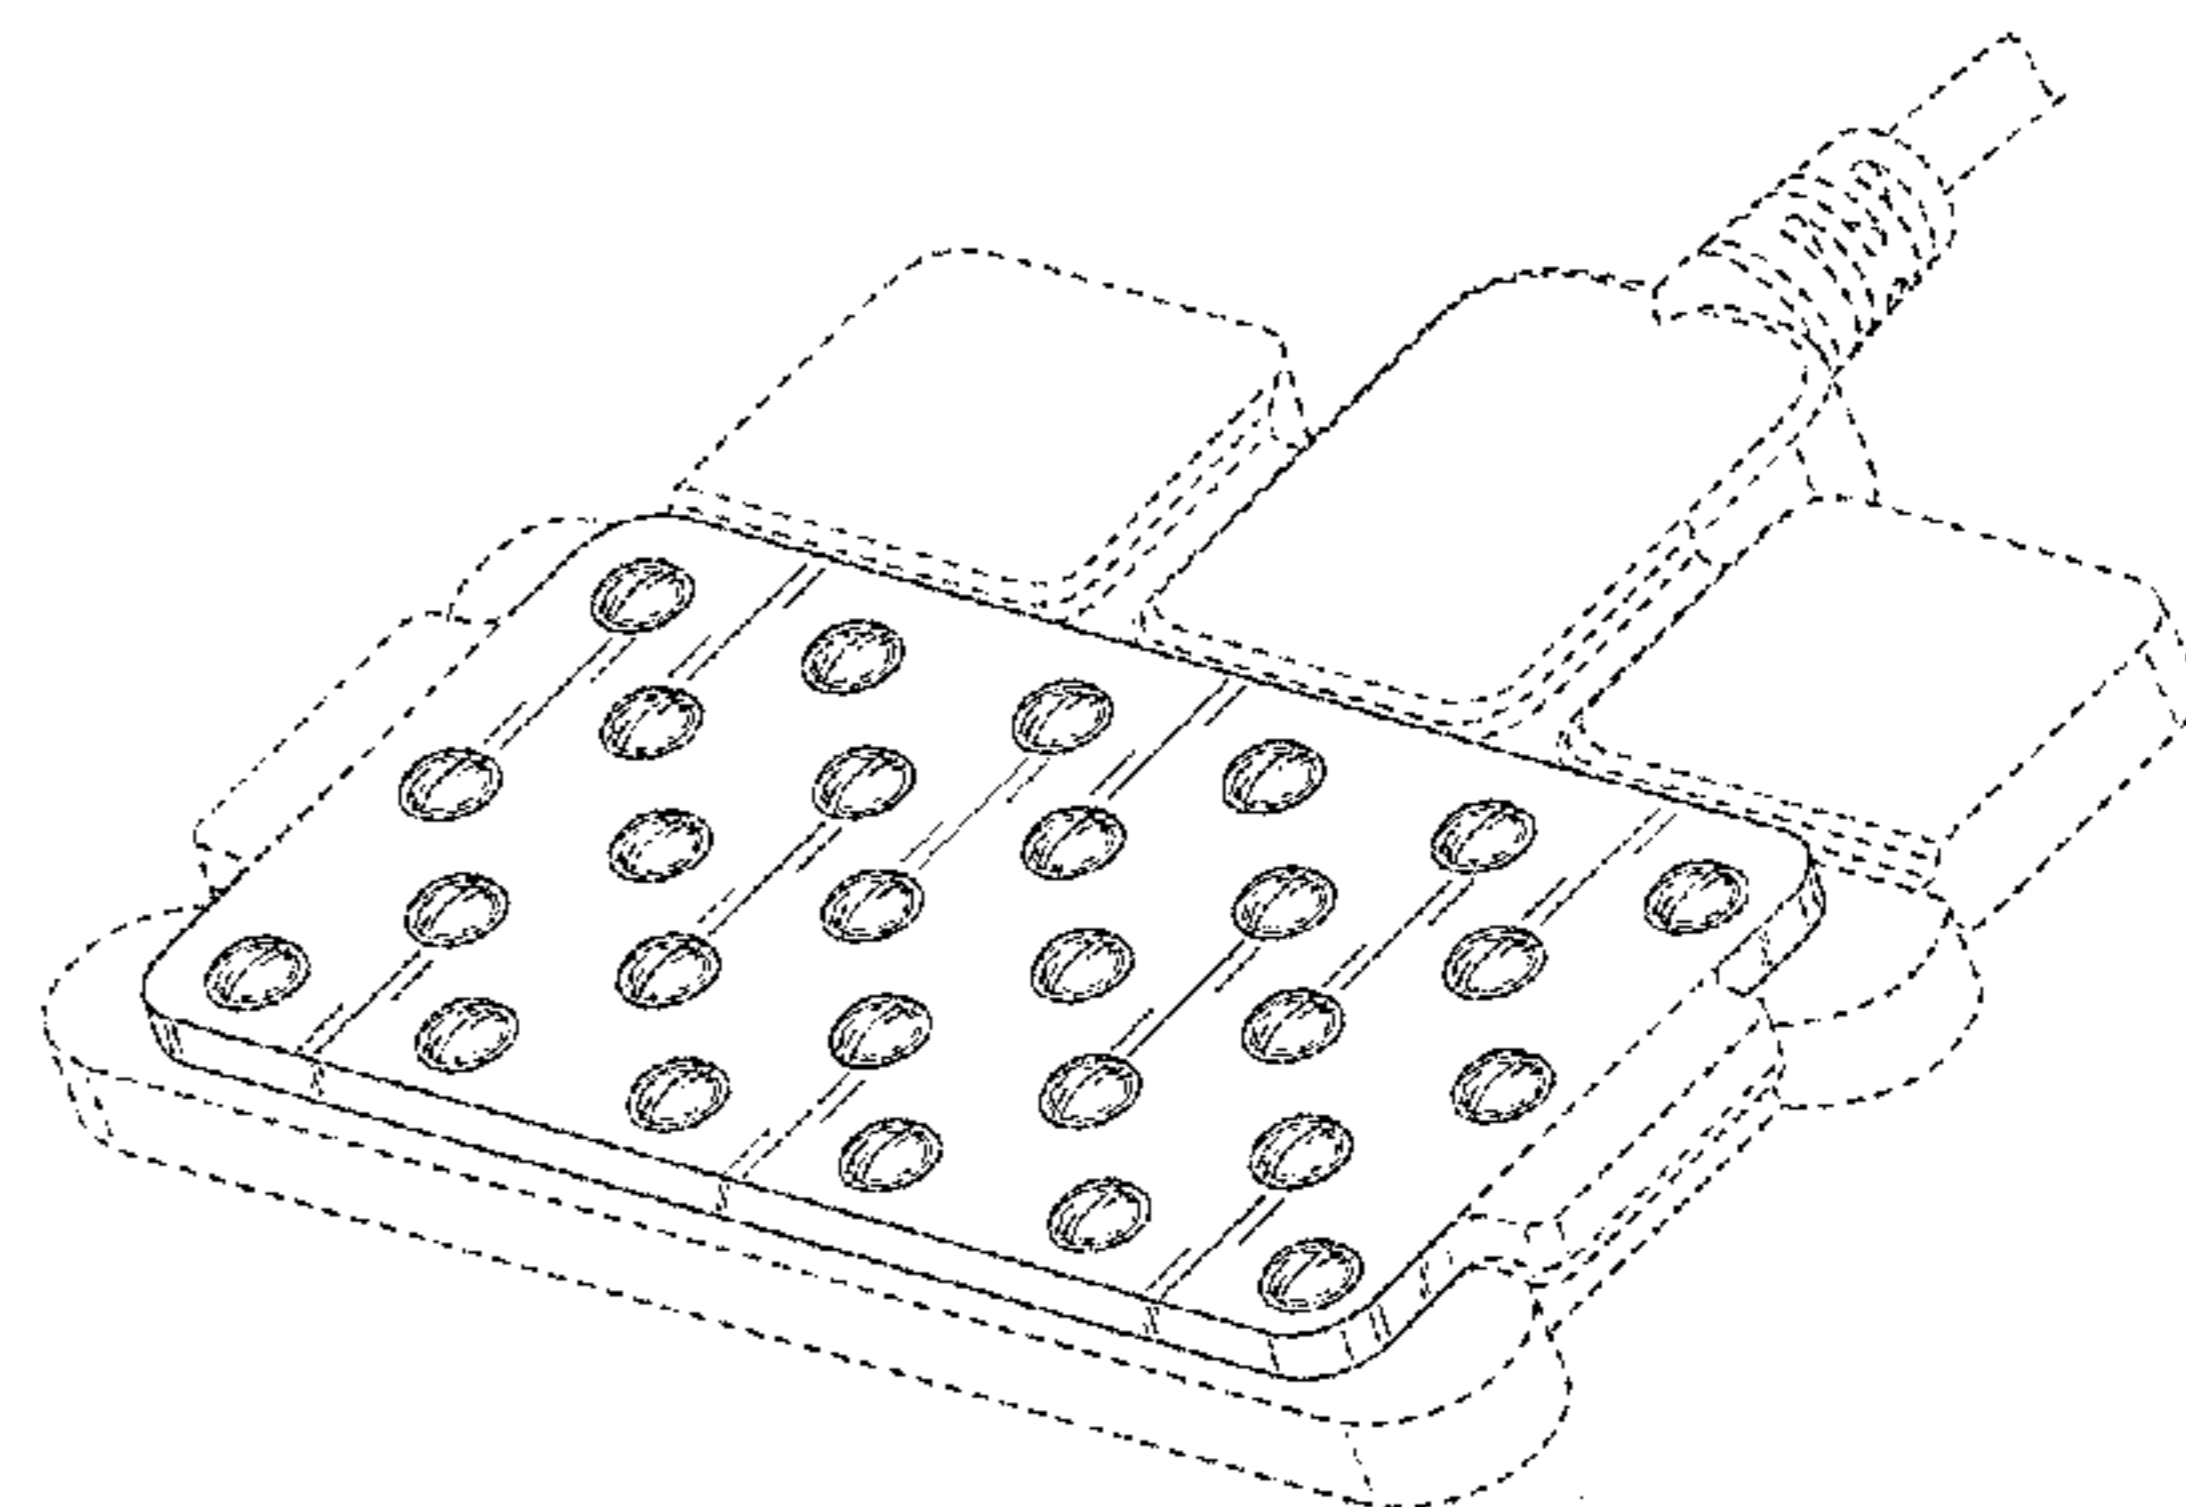

(56)

References Cited

U.S. PATENT DOCUMENTS

4,825,872	A	5/1989	Tan et al.	7,869,849	B2	1/2011	Ollerdessen et al.
4,967,038	A	10/1990	Gevins et al.	7,880,884	B2	2/2011	Medina
4,972,331	A	11/1990	Chance	7,979,102	B2	7/2011	Hannula et al.
5,137,355	A	8/1992	Barbour et al.	7,983,740	B2	7/2011	Culver et al.
5,139,025	A	8/1992	Lewis et al.	8,040,519	B2	10/2011	Kawasaki et al.
5,217,013	A	6/1993	Lewis et al.	8,050,744	B2	11/2011	Maki et al.
5,222,496	A	6/1993	Clarke et al.	8,060,189	B2	11/2011	Ben Dor et al.
5,465,714	A	11/1995	Scheuing	8,095,194	B2	1/2012	Ninomiya et al.
5,482,034	A	1/1996	Lewis et al.	8,131,347	B2	3/2012	Cho et al.
5,517,987	A	5/1996	Tsuchiya	8,175,671	B2	5/2012	Hoarau
5,584,296	A	12/1996	Cui et al.	8,190,225	B2	5/2012	Hoarau
5,596,987	A	1/1997	Chance	8,798,702	B2 *	8/2014	Trumble A61B 5/14551 600/310
5,664,574	A	9/1997	Chance	8,821,397	B2 *	9/2014	Al-Ali 600/301
5,792,051	A	8/1998	Chance	8,849,369	B2 *	9/2014	Cogan A61B 5/0006 600/378
5,800,349	A	9/1998	Isaacson et al.	D723,701	S *	3/2015	Maki D24/187
5,803,909	A	9/1998	Maki et al.	2004/0064052	A1	4/2004	Chance et al.
5,820,558	A	10/1998	Chance	2007/0260129	A1 *	11/2007	Chin A61B 5/02411 600/323
5,835,617	A	11/1998	Ohta et al.	2008/0154126	A1	6/2008	Culver et al.
5,853,370	A	12/1998	Chance et al.	2008/0177163	A1	7/2008	Wang et al.
5,873,821	A	2/1999	Chance et al.	2008/0228053	A1	9/2008	Wang et al.
5,902,235	A	5/1999	Lewis et al.	2008/0242958	A1 *	10/2008	Al-Ali A61B 5/02427 600/323
5,987,351	A	11/1999	Chance	2008/0316488	A1	12/2008	Mao et al.
6,075,610	A	6/2000	Ueda et al.	2009/0108205	A1	4/2009	Duffy et al.
6,078,833	A	6/2000	Hueber	2009/0234245	A1	9/2009	Jaffe et al.
6,192,261	B1	2/2001	Gratton et al.	2009/0259114	A1 *	10/2009	Johnson A61B 5/14552 600/310
6,240,309	B1	5/2001	Yamashita et al.	2009/0281403	A1	11/2009	Benni
6,272,367	B1	8/2001	Chance	2009/0292210	A1	11/2009	Culver et al.
6,282,438	B1	8/2001	Maki et al.	2009/0326345	A1	12/2009	Jaffe et al.
6,304,767	B1	10/2001	Soller et al.	2010/0049018	A1	2/2010	Duffy et al.
6,335,792	B1	1/2002	Tsuchiya	2010/0174160	A1	7/2010	Chance
6,397,099	B1 *	5/2002	Chance A61B 5/0059 600/323	2010/0198029	A1	8/2010	Wang
6,456,862	B2	9/2002	Benni	2010/0222654	A1 *	9/2010	Gonopolskiy A61B 5/6833 600/310
6,516,209	B2	2/2003	Cheng et al.	2010/0241006	A1	9/2010	Choi et al.
6,542,763	B1	4/2003	Yamashita et al.	2010/0249608	A1	9/2010	Chance
6,549,284	B1	4/2003	Boas et al.	2010/0317949	A1	12/2010	Chamness et al.
6,577,884	B1	6/2003	Boas	2010/0331640	A1 *	12/2010	Medina A61B 5/14535 600/324
6,587,703	B2	7/2003	Cheng et al.	2011/0046459	A1	2/2011	Zhang et al.
6,597,931	B1	7/2003	Cheng et al.	2011/0060197	A1	3/2011	Zhang et al.
6,611,698	B1	8/2003	Yamashita et al.	2011/0176217	A1 *	7/2011	Fujii G02B 3/0056 359/619
6,615,065	B1	9/2003	Barrett et al.	2011/0190613	A1	8/2011	Zhang et al.
6,618,614	B1	9/2003	Chance	2011/0205535	A1	8/2011	Soller et al.
6,795,195	B1	9/2004	Barbour et al.	2011/0264411	A1	10/2011	Yang et al.
6,901,284	B1	5/2005	Maki et al.	2012/0253153	A1 *	10/2012	Trumble A61B 5/14551 600/324
6,937,884	B1	8/2005	Barbour	2013/0079609	A1 *	3/2013	Besko A61B 5/14552 600/324
RE38,800	E	9/2005	Barbour	2013/0079611	A1 *	3/2013	Besko A61B 5/14552 600/344
6,947,779	B2	9/2005	Yamamoto et al.	2013/0144365	A1 *	6/2013	Kipke A61B 5/04001 607/93
7,034,303	B2	4/2006	Schotland et al.	2013/0158372	A1 *	6/2013	Haisley A61B 5/1455 600/310
7,047,054	B2	5/2006	Benni	2014/0012108	A1 *	1/2014	McPeak A61B 5/0295 600/324
7,142,304	B1	11/2006	Barbour et al.	2014/0031793	A1 *	1/2014	Constantineau .. A61M 5/14248 604/510
7,197,357	B2	3/2007	Istvan et al.	2014/0180046	A1 *	6/2014	Campbell A61B 5/0205 600/324
7,248,909	B2	7/2007	Lee et al.	2014/0276013	A1 *	9/2014	Muehlemann A61B 5/0013 600/425
7,286,870	B2	10/2007	Maki et al.	2014/0276014	A1 *	9/2014	Khanicheh A61B 5/0013 600/425
7,313,427	B2	12/2007	Benni	2015/0157225	A1 *	6/2015	Gillberg A61B 5/04085 600/393
7,355,688	B2	4/2008	Lash et al.				
D568,479	S *	5/2008	Mao D24/168				
7,440,794	B2	10/2008	Maki et al.				
7,463,362	B2	12/2008	Lasker et al.				
7,477,924	B2 *	1/2009	Chin A61B 5/02411 600/323				
7,503,927	B1 *	3/2009	Vetanze A61N 1/0408 607/115				
7,538,865	B2	5/2009	Lash et al.				
D594,127	S *	6/2009	Causevic D24/187				
7,551,950	B2	6/2009	Cheng				
7,576,853	B2	8/2009	Barbour				
7,610,082	B2	10/2009	Chance				
7,643,858	B2	1/2010	Agashe et al.				
7,676,253	B2	3/2010	Raridan, Jr.				
7,740,588	B1	6/2010	Sciarra				
7,741,592	B1	6/2010	Gonopolskiy et al.				
7,761,127	B2	7/2010	Al-Ali et al.				
7,774,047	B2	8/2010	Yamashita et al.				
7,778,694	B2	8/2010	Kaga et al.				
RE41,949	E	11/2010	Barbour et al.				

OTHER PUBLICATIONS

[No Author Listed] New Functional Near Infrared Systems to Study Brain Activity: Emerging fNIR technology monitors cortical hemodynamic changes to brain activation and provides objective real-time response data. Biopac Systems, Inc. 2 pages. <http://www>.

(56)

References Cited

OTHER PUBLICATIONS

biopac.com/Manuals/fnir%20product%20sheet.pdf.[last accessed Mar. 28, 2012].

Bozkurt et al., A portable near infrared spectroscopy system for bedside monitoring of newborn brain. *Biomed Eng Online*. 2005;4(29). 11 pages.

Cohn, Near-Infrared Spectroscopy: Potential Clinical Benefits in Surgery. *J Am Coll Surg*. Aug. 2007;205(2):322-32.

Culver et al., Diffuse Optical Tomography of Cerebral Blood Flow, Oxygenation, and Metabolism in Rat During Focal Ischemia. *J Cereb Blood Flow Metab*. 2003;23(8):911-24.

Curtin et al., Functional near-infrared spectroscopy for the measurement of propofol effects in conscious sedation during outpatient elective colonoscopy. *NeuroImage*. 2013. 11 pages. <http://dx.doi.org/10.1016/j.neuroimage.2013.07.009> [last accessed Mar. 28, 2012].

Dam et al., Fiber-optic probe for noninvasive real-time determination of tissue optical properties at multiple wavelengths. *Appl Optics*. Mar. 1, 2001;40(7):1155-64.

Fantini et al., Frequency-domain multichannel optical detector for noninvasive tissue spectroscopy and oximetry. *Opt Eng*. Jan. 1995;34(1):32-42.

Ferradal et al., Bedside Monitoring of Cerebral Oxygenation Using DOT. *Biomed Optics*. Biomed/DH Joint Poster Session. Apr. 11-14, 2010. 3 pages.

Franceschini et al., Optical Study of the Skeletal Muscle During Exercise with a Second Generation Frequency-Domain Tissue Oximeter. 1997;807-814.

Gratton et al., Measurement of brain activity by near-infrared light. *J Biomed Optics*. Jan./Feb. 2005;10(1):011008.1-13.

Liao et al., Neonatal hemodynamic response to visual cortex activity: high-density near-infrared spectroscopy study. *J Biomed Optics*. Mar./Apr. 2010;15(2):026010.1-9.

Mühlemann, A Novel wireless Near-Infrared Spectrophotometer Applied to Measure Cortical Haemodynamics in Humans and Sheep. ETH Dissertation No. 19051. ETH Zurich. 2010. 112 pages.

Nishimura et al., A New Approach to Functional Near-Infrared Technology. *IEEE Eng Med Biol Mag*. Jul./Aug. 2007;26(4):25-9.

Shah et al., Noninvasive functional optical spectroscopy of human breast tissue. *PNAS*. Apr. 10, 2001;98(8):4420-5.

Shiga et al., Development of a portable tissue oximeter using near infra-red spectroscopy. *Med & Biol Eng & Comput*. Jul. 1995;33:622-6.

Taber et al., Optical Imaging: A New Window to the Adult Brain. *J Neuropsychiatry Clin Neurosci*. 2010 Fall;22(4):356-60.

Vaithianathan et al., Design of a portable near infrared system for topographic imaging of the brain in babies. *Rev Sci Instrum*. Oct. 2004;75(10):3276-83.

White et al., Phase-encoded retinotopy as an evaluation of diffuse optical neuroimaging. *NeuroImage*. 2010;49:568-77.

White et al., Quantitative evaluation of high-density diffuse optical tomography: in vivo resolution and mapping performance *J Biomed Optics*. Mar./Apr. 2010;15(2):026006.1-14.

White et al., Resting-state functional connectivity in the human brain revealed with diffuse optical tomography. *NeuroImage*. 2009;47:148-56.

Zeff et al., Retinotopic mapping of adult human visual cortex with high-density diffuse optical tomography. *PNAS*. Jul. 17, 2007;104(29):12169-74.

U.S. Appl. No. 29/486,801, filed Apr. 2, 2014, Muehleemann et al.

* cited by examiner

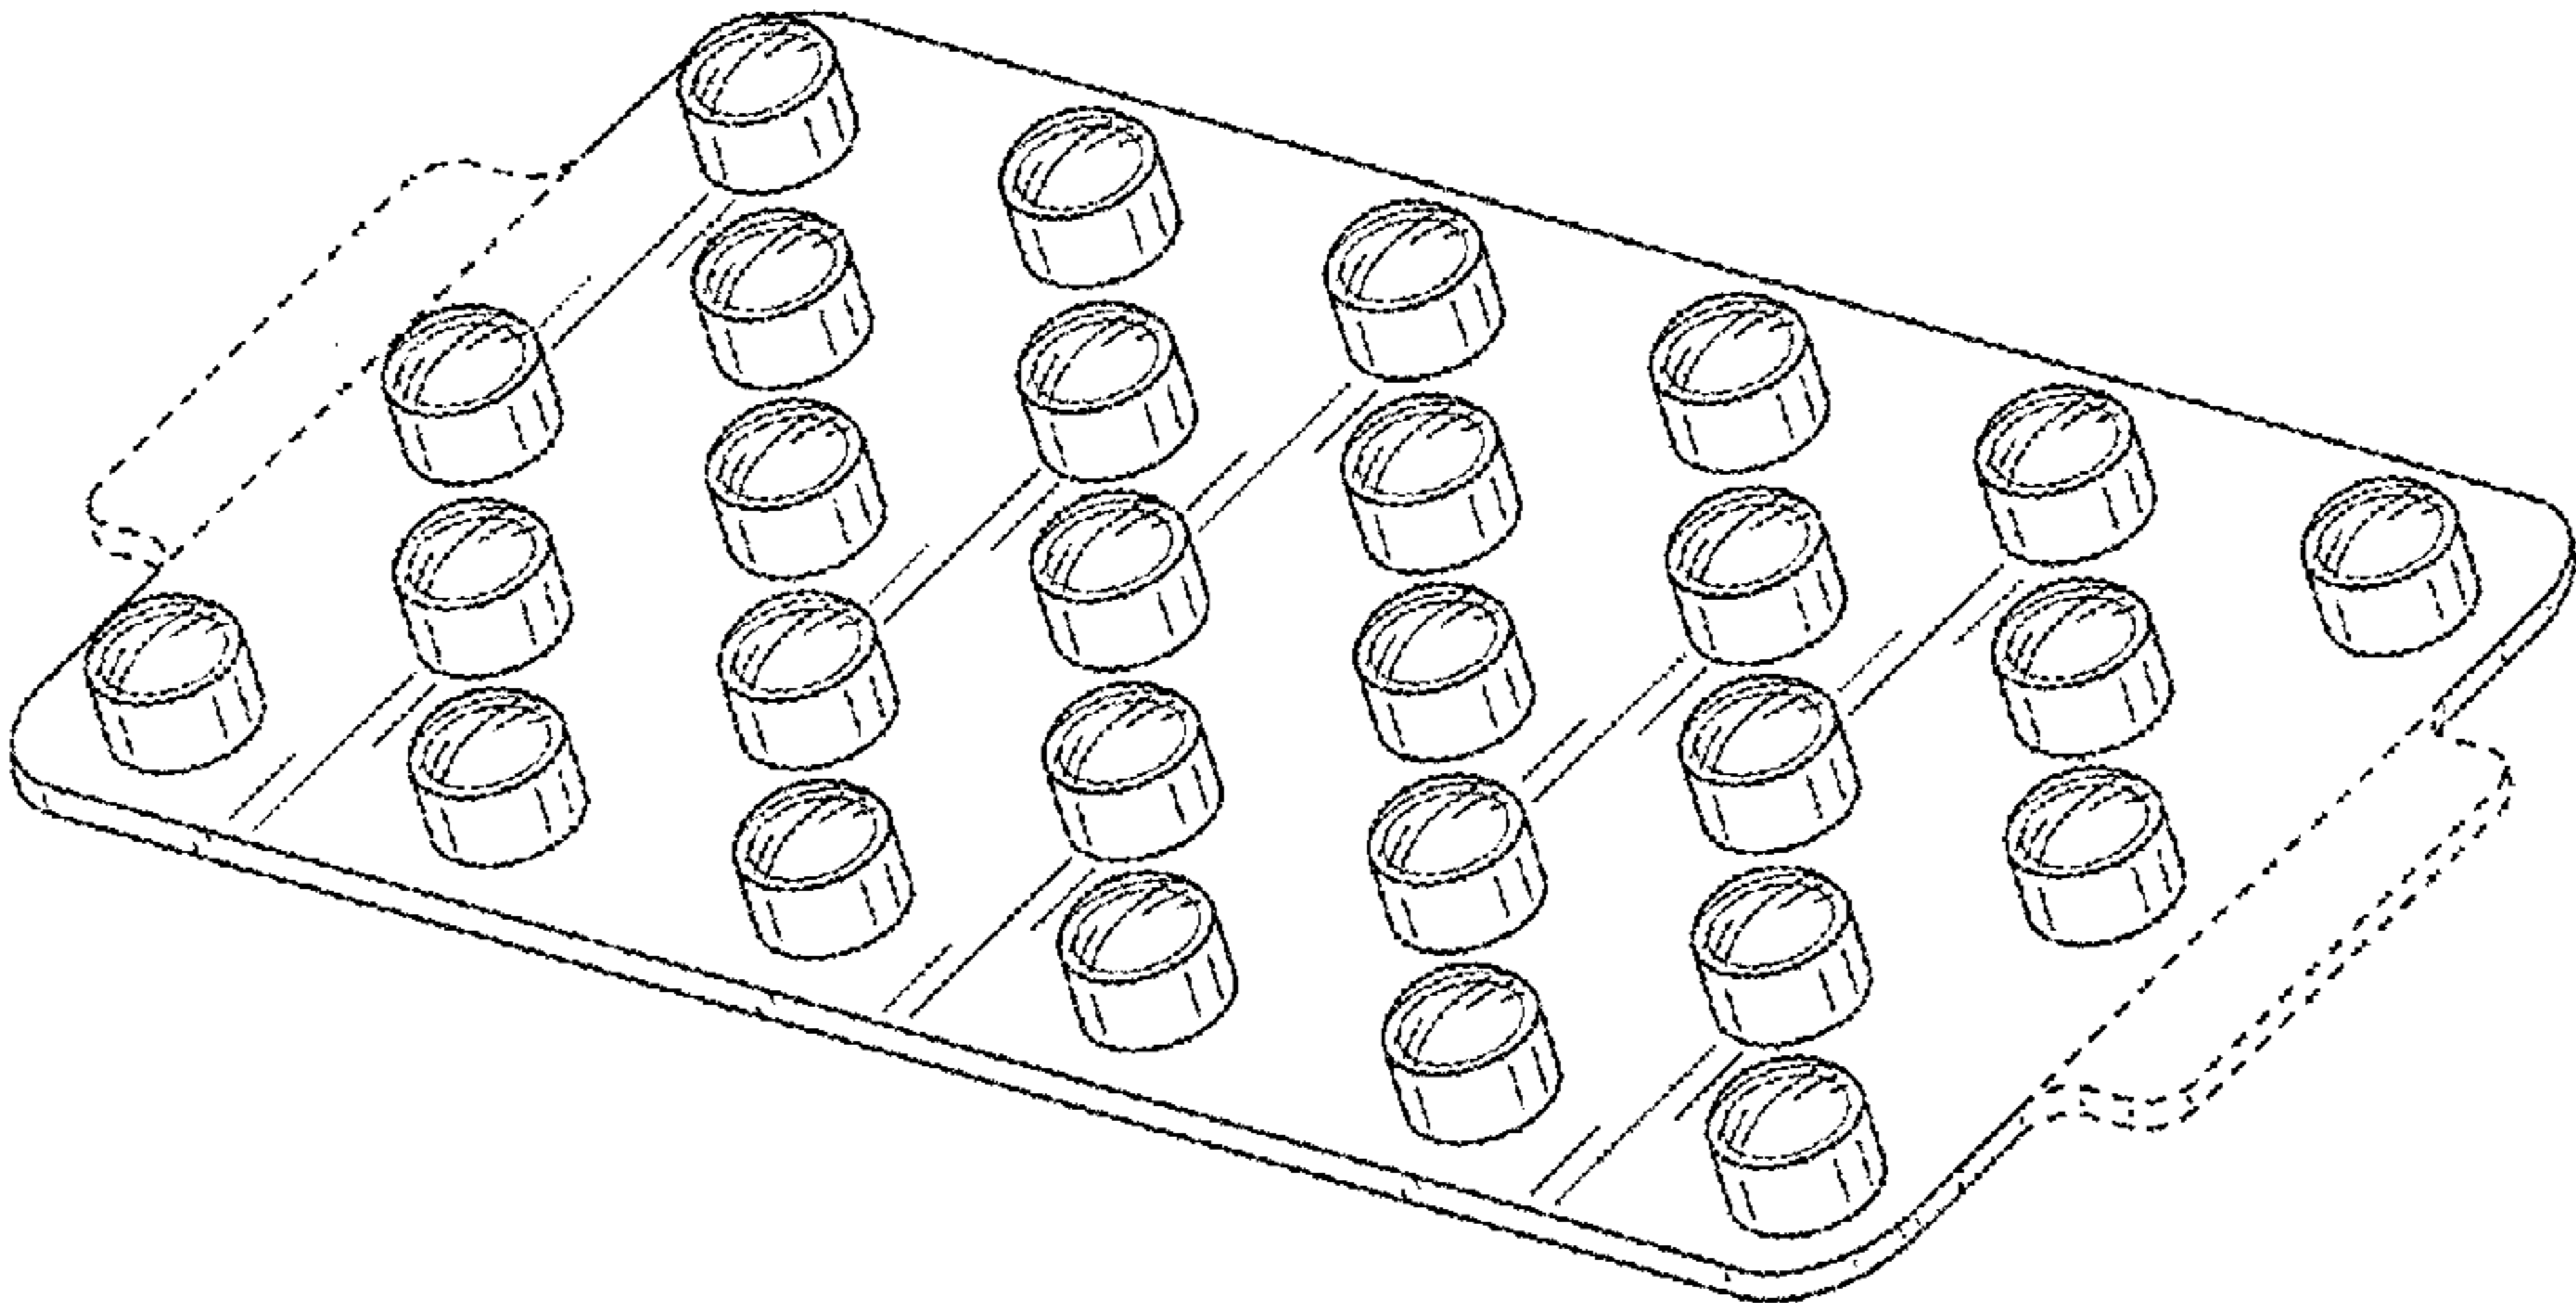


FIG. 1

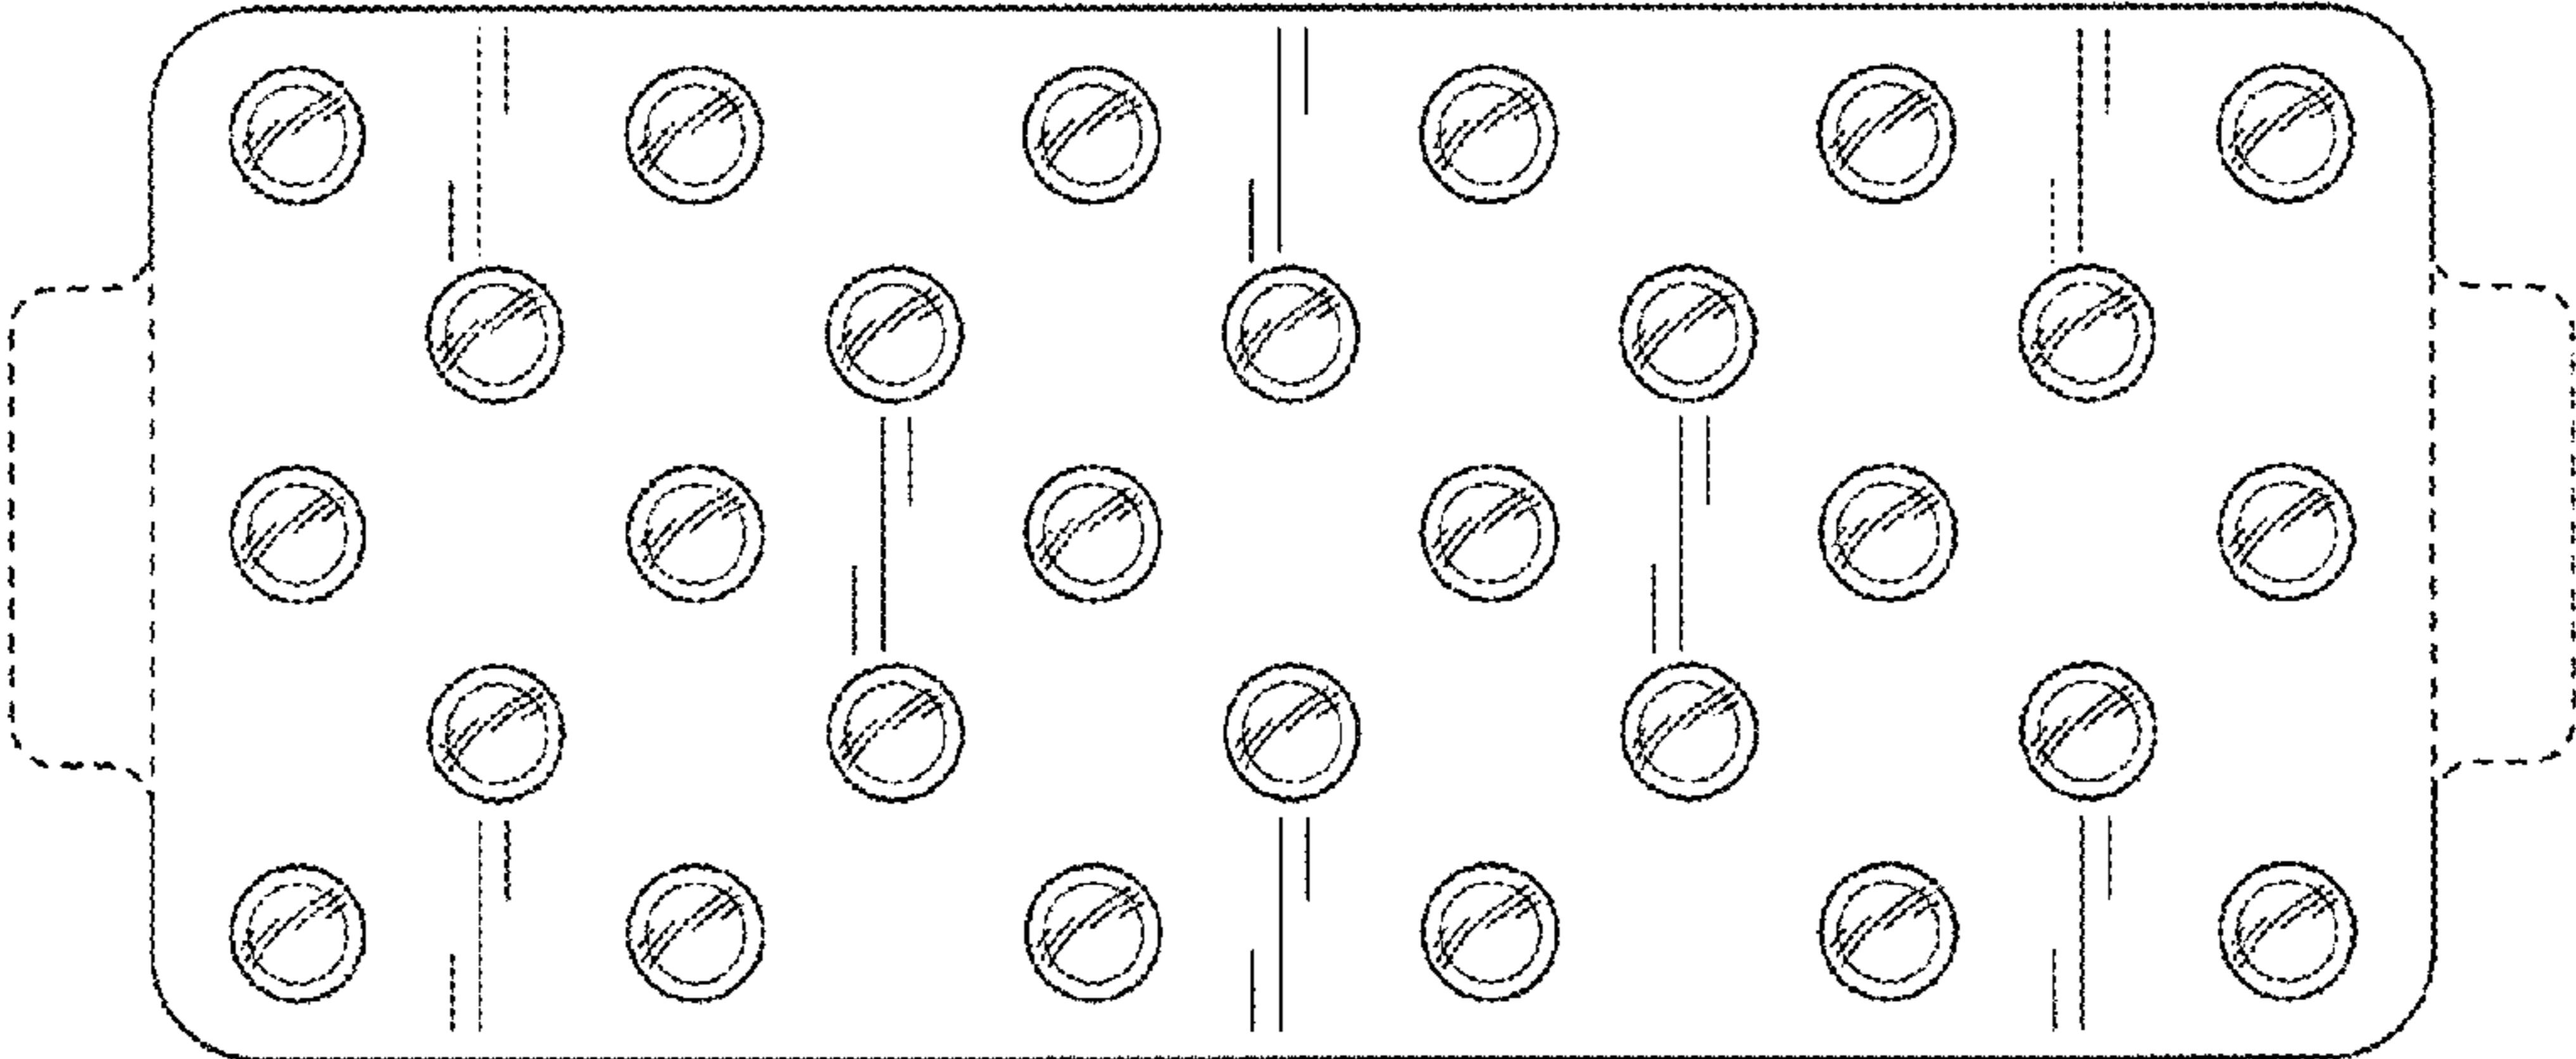


FIG. 2

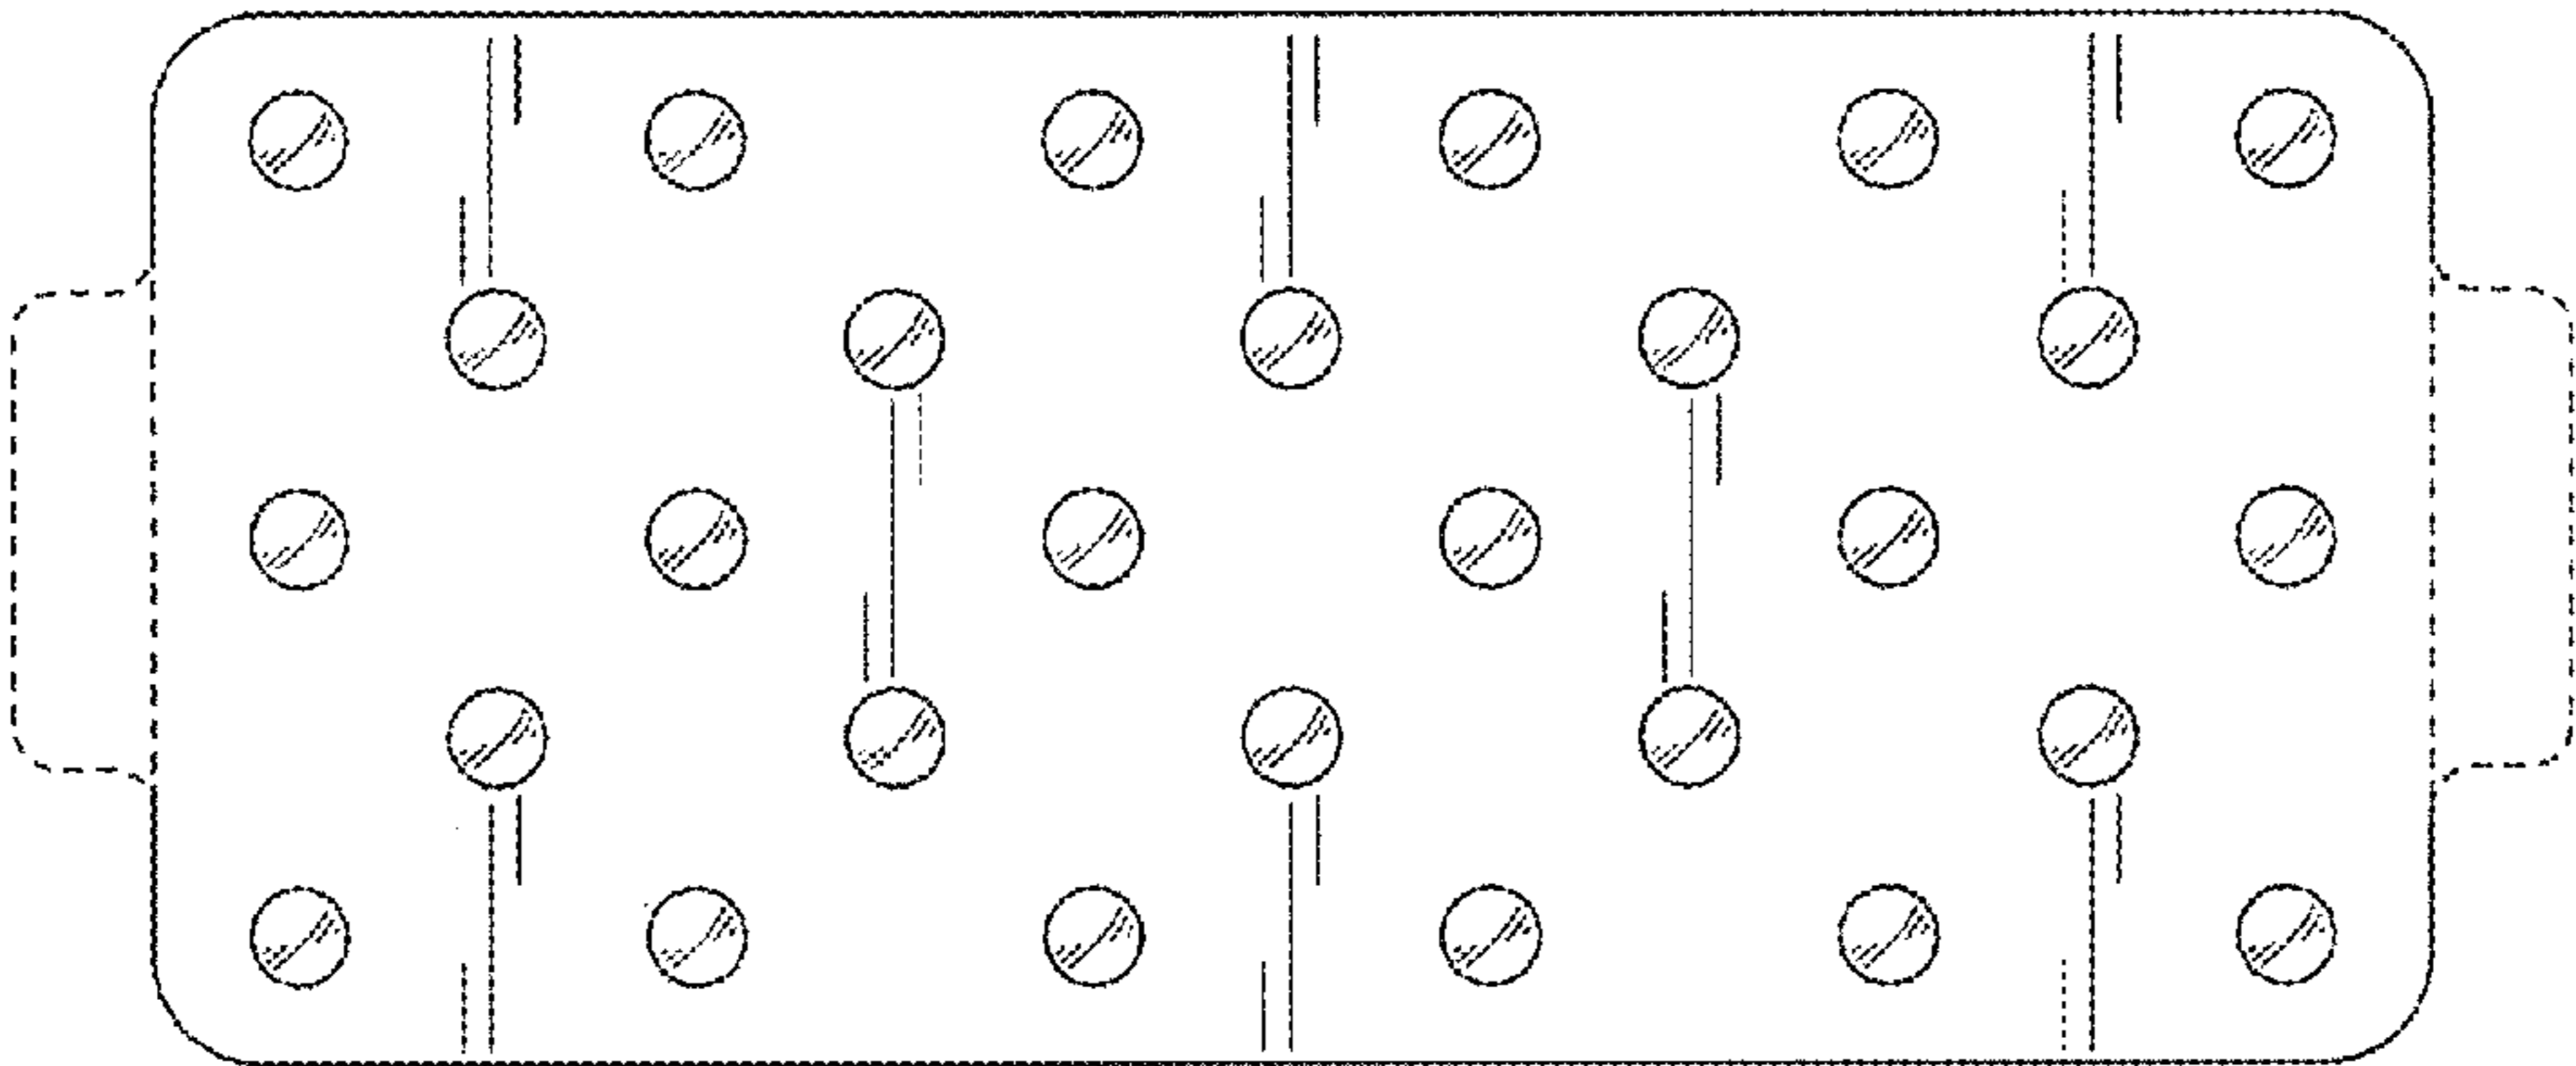


FIG. 3



FIG. 4



FIG. 5



FIG. 6

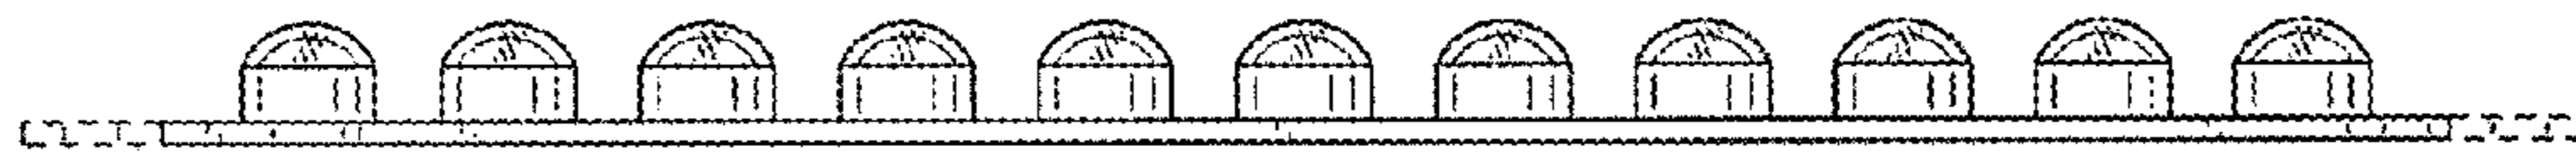


FIG. 7

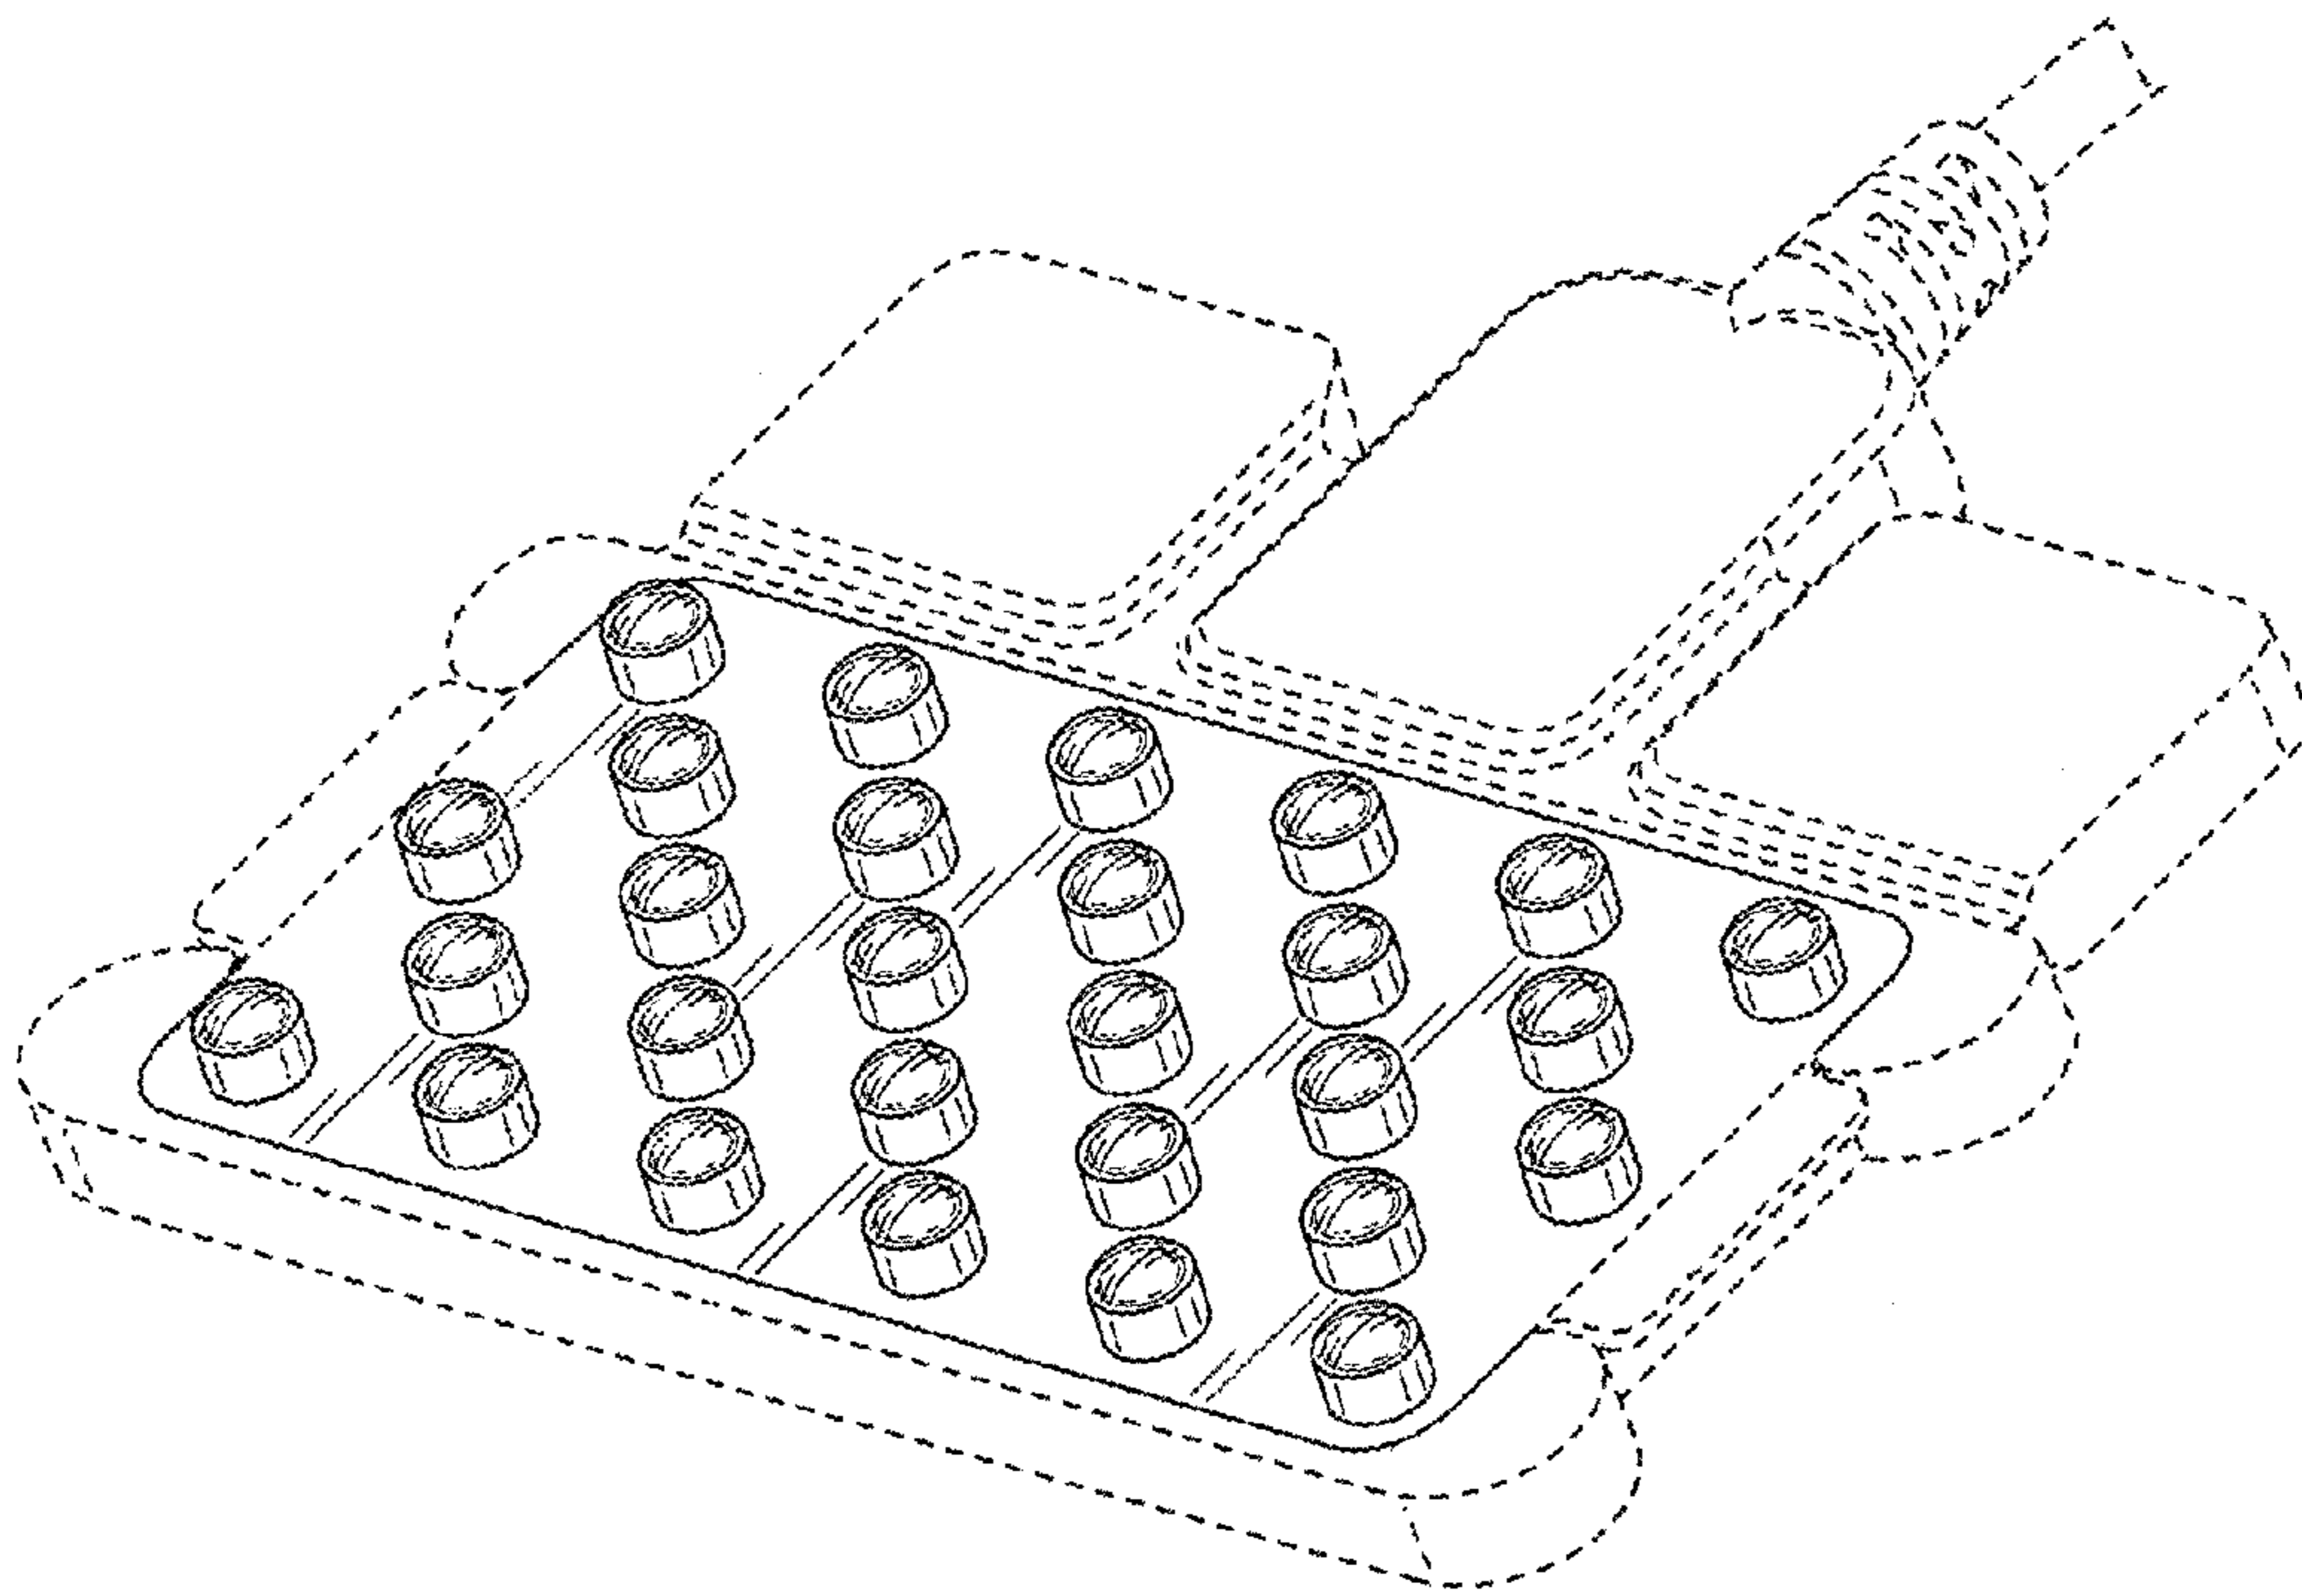


FIG. 8

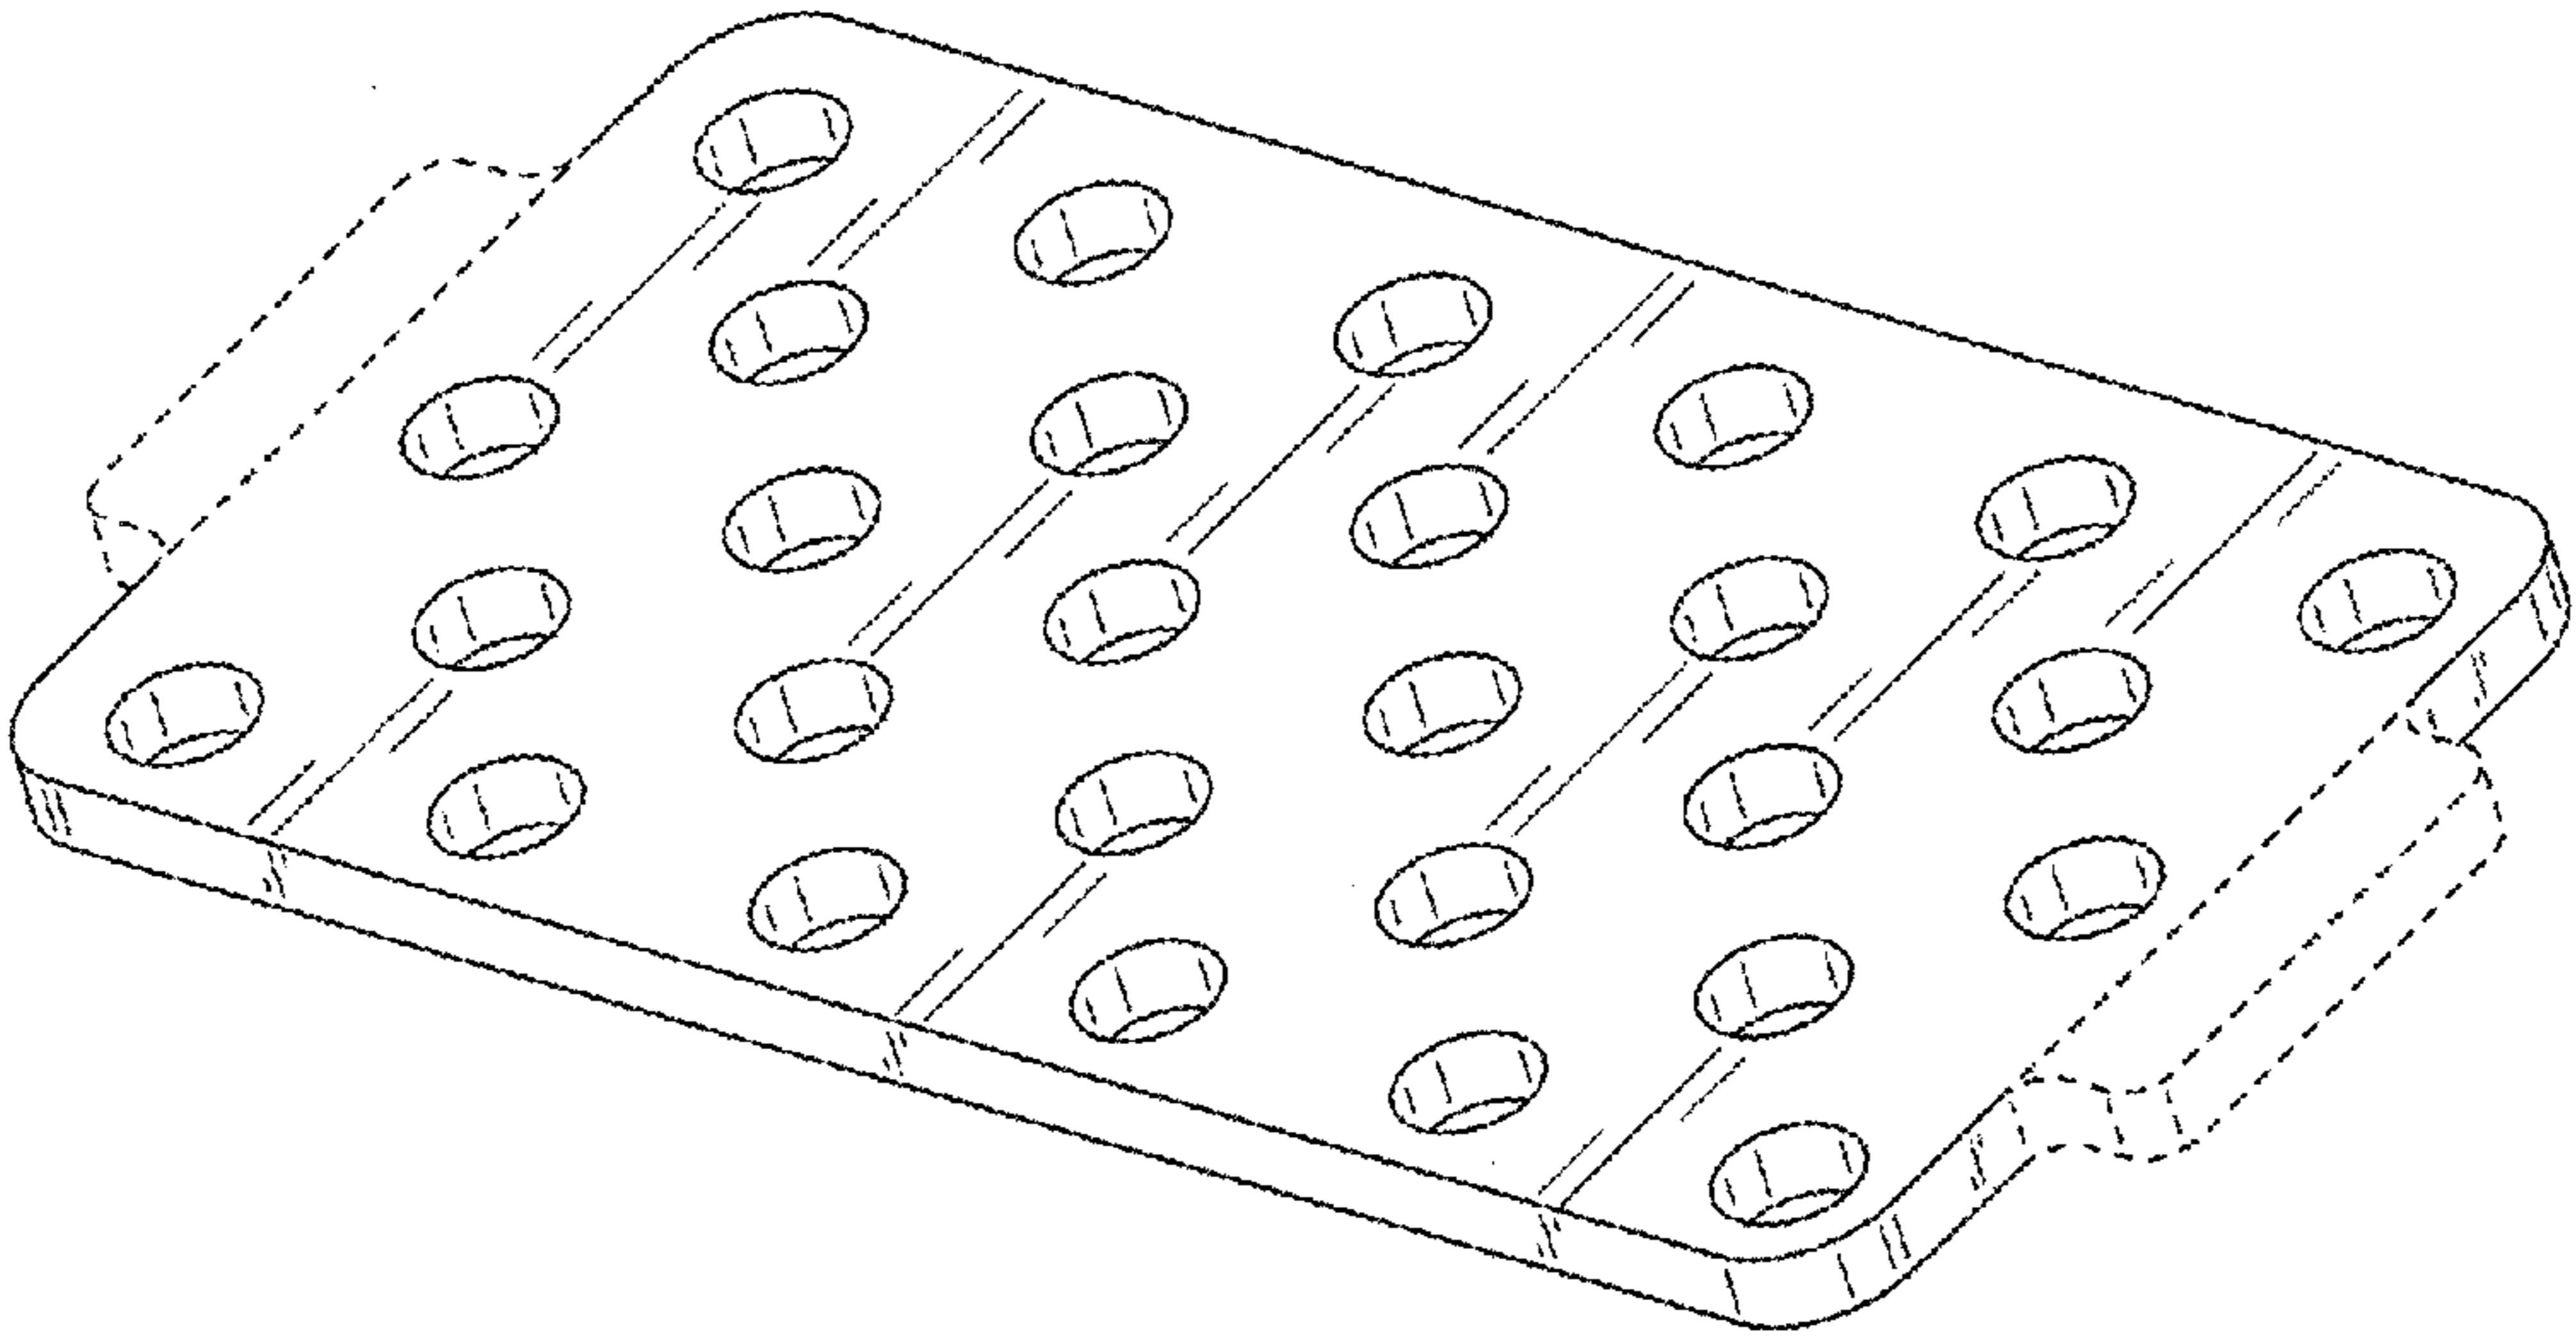


FIG. 9

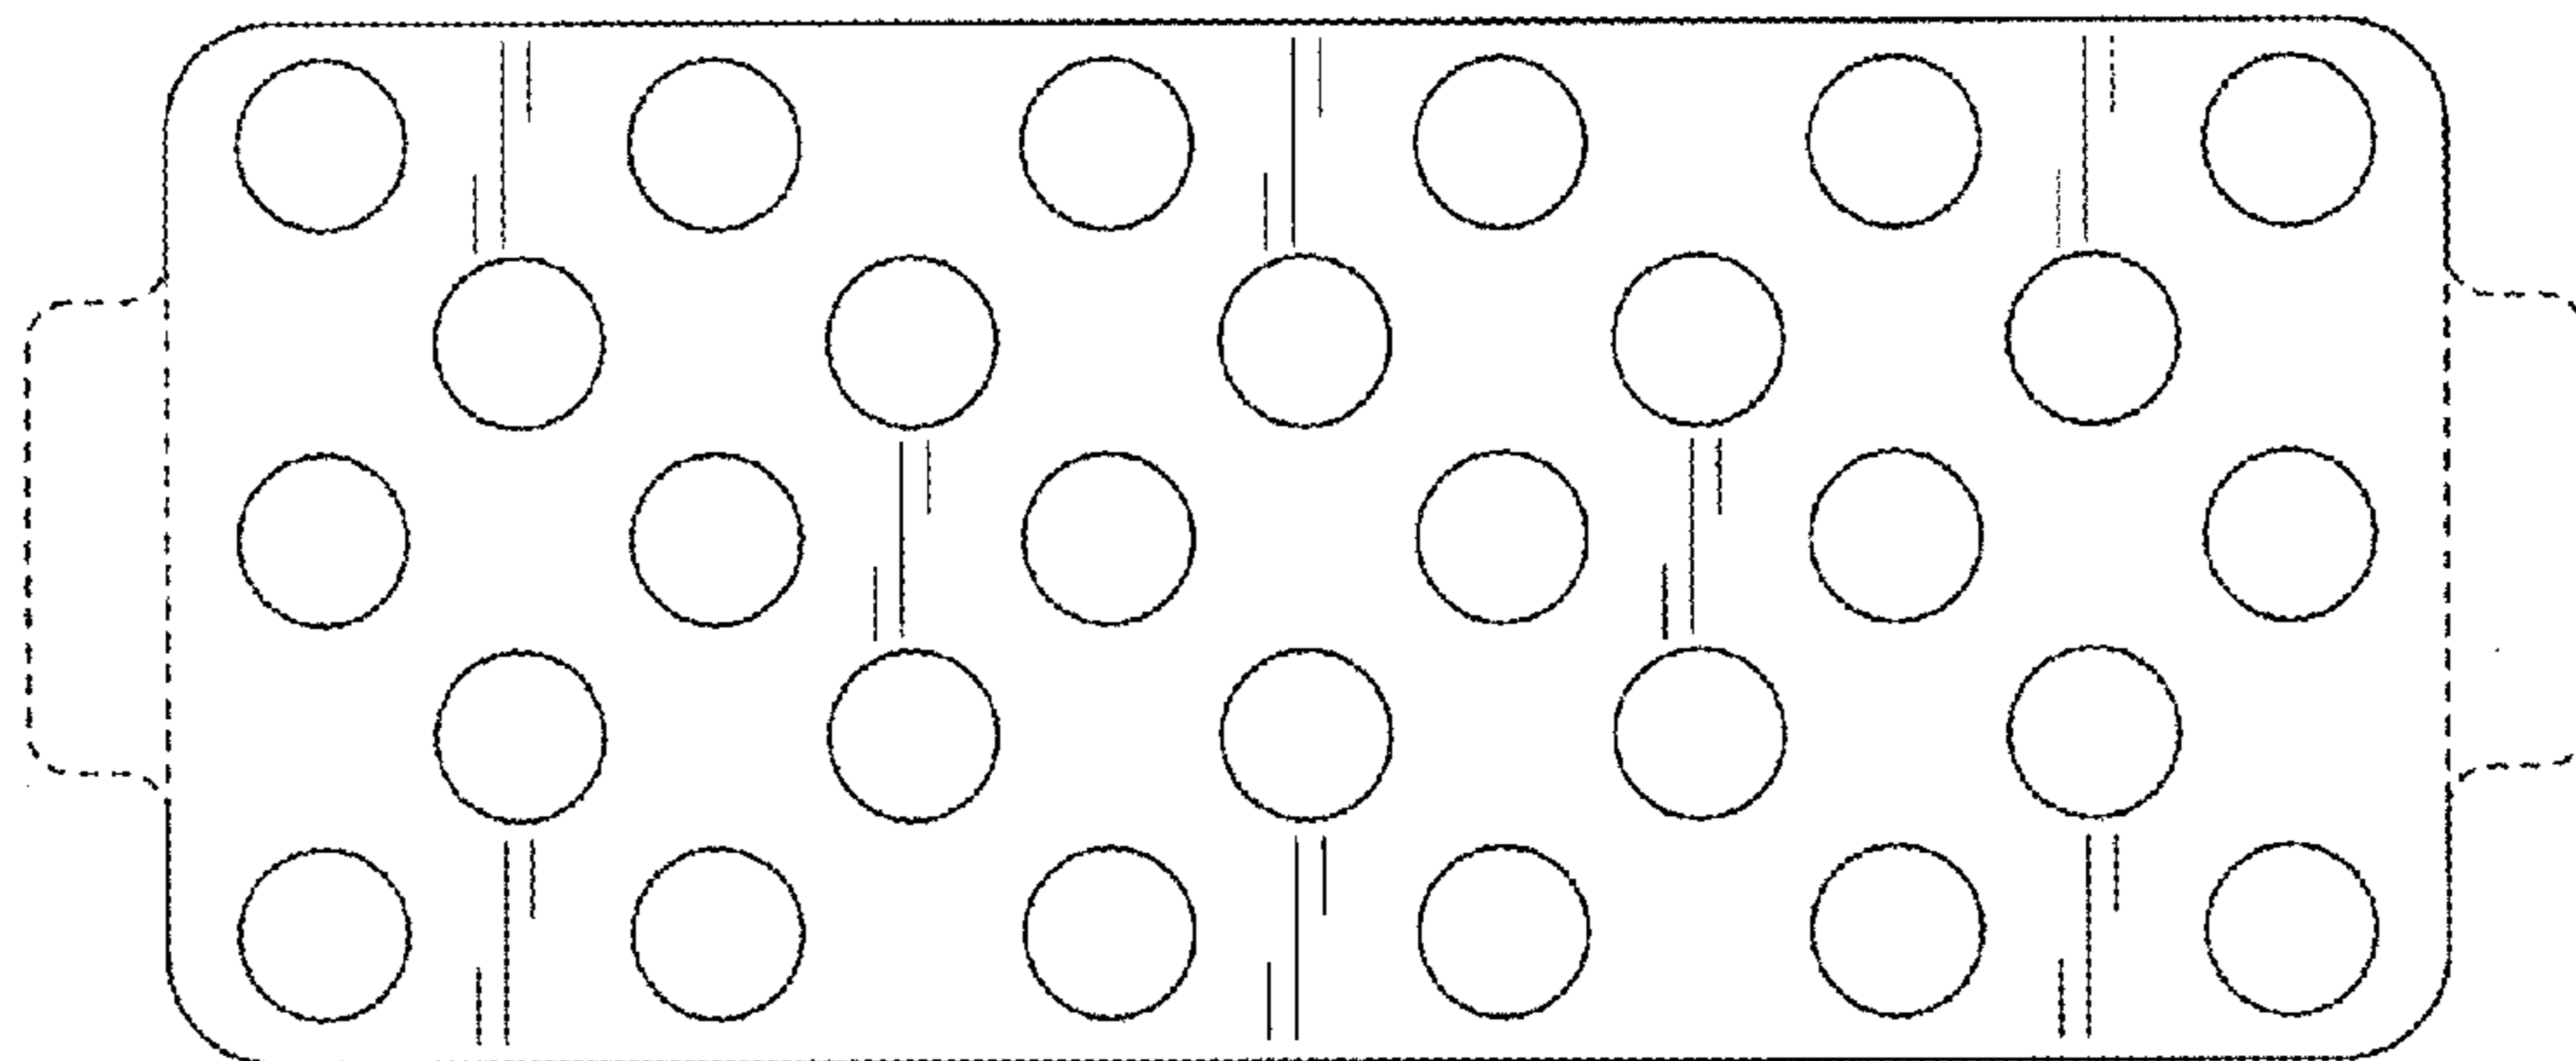


FIG. 10

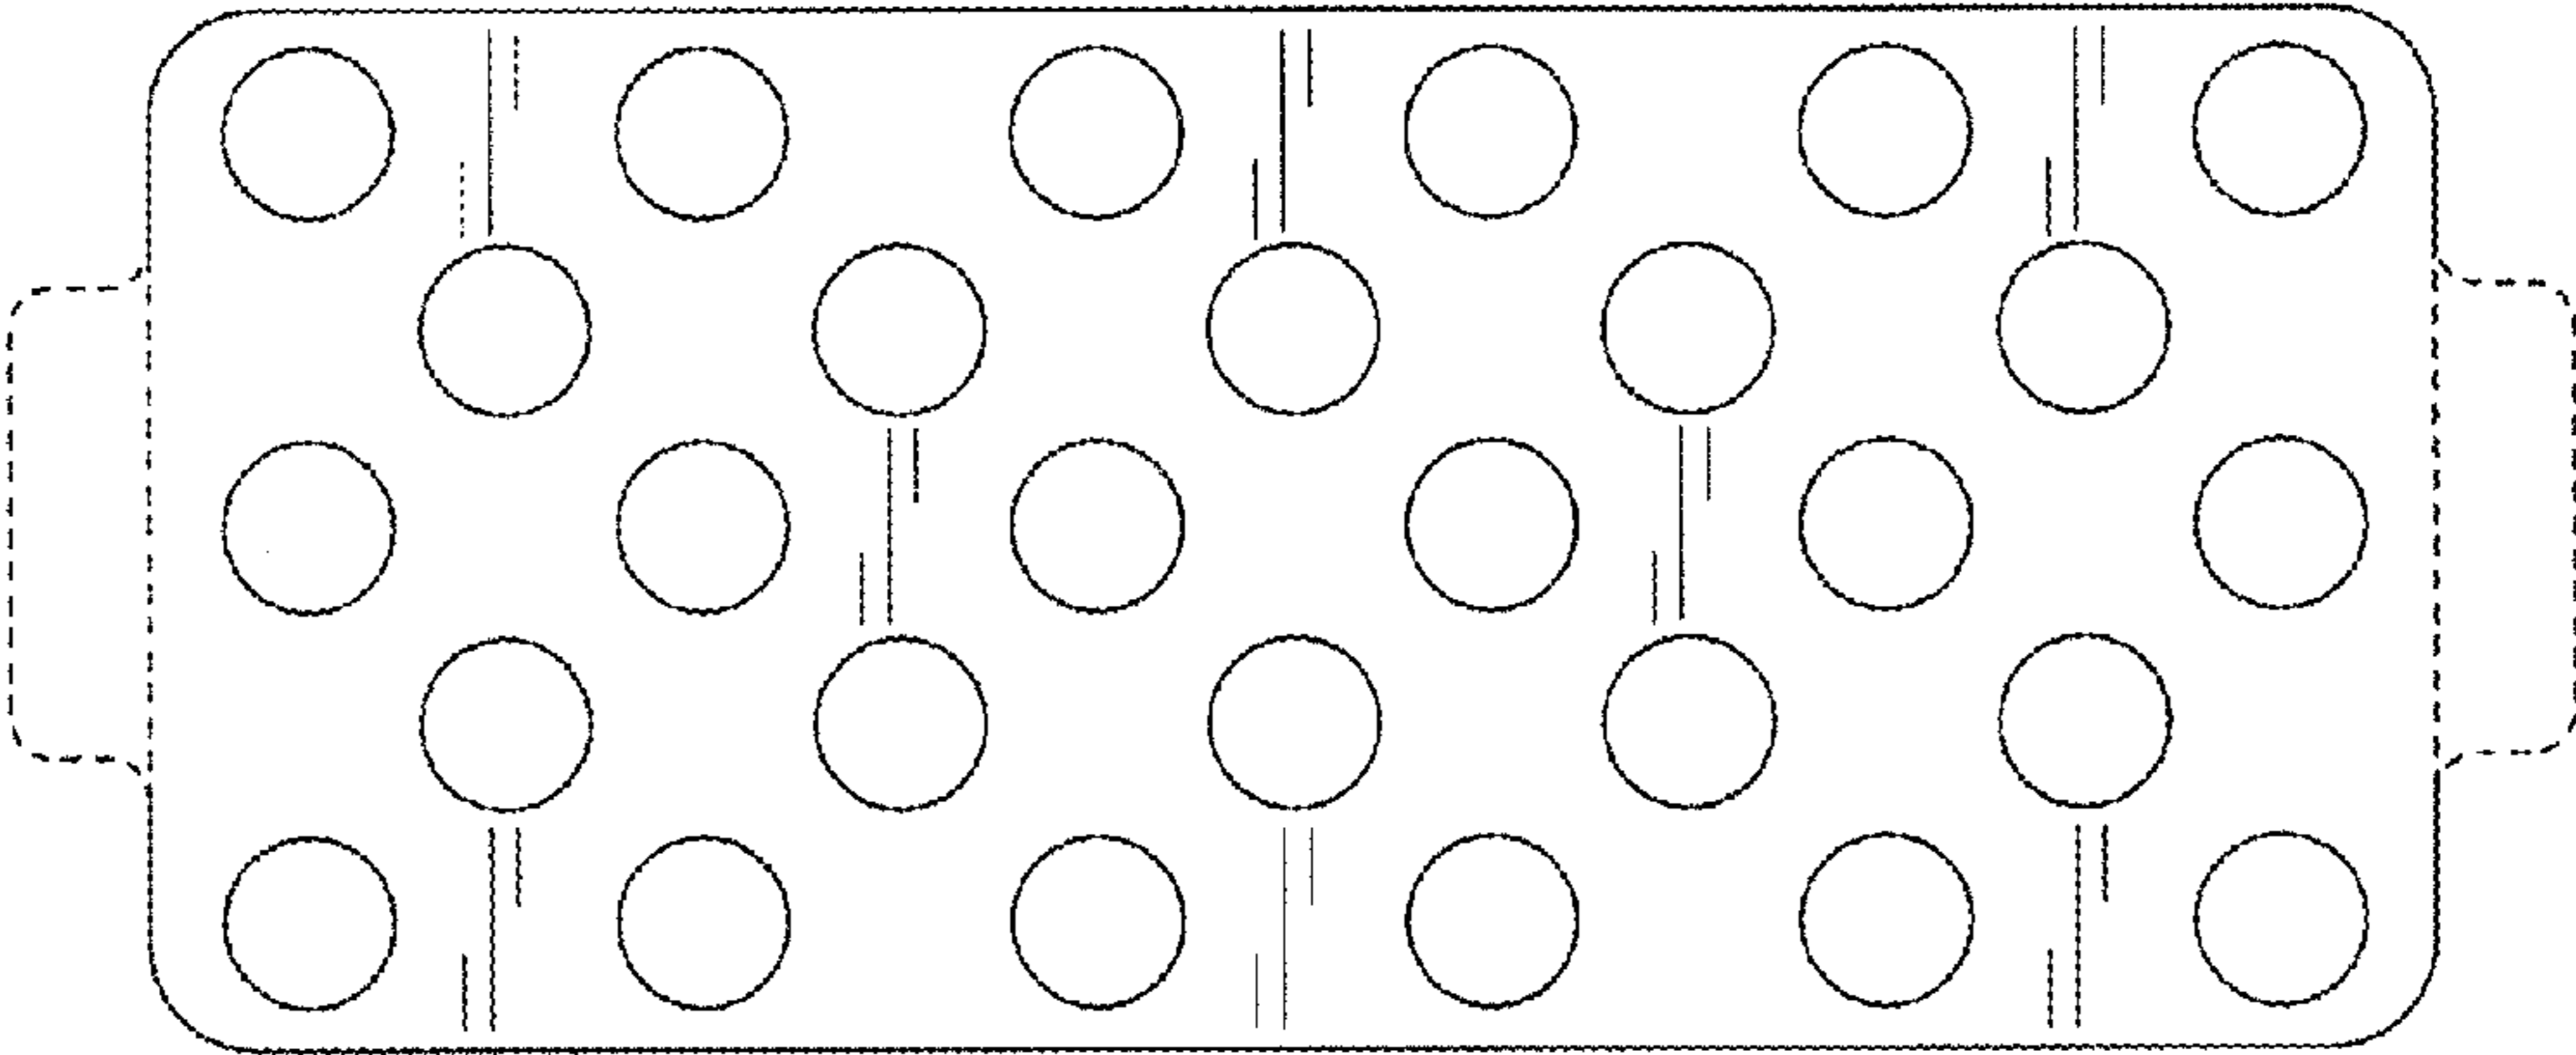


FIG. 11

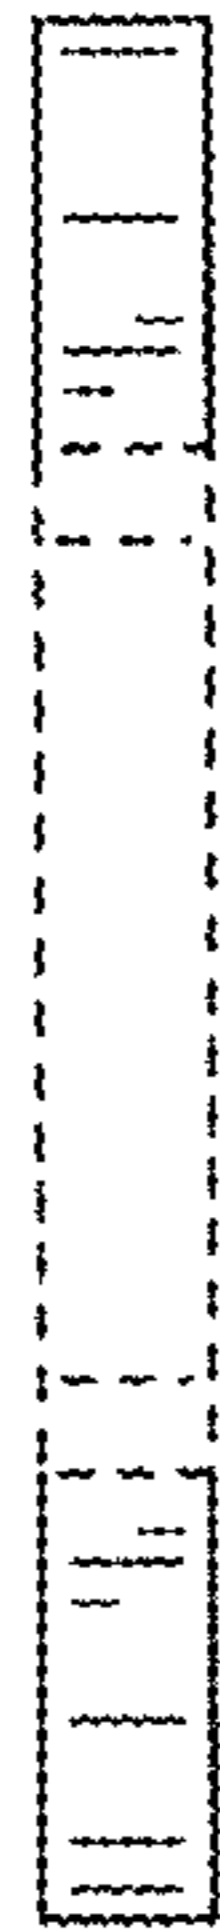


FIG. 12



FIG. 13

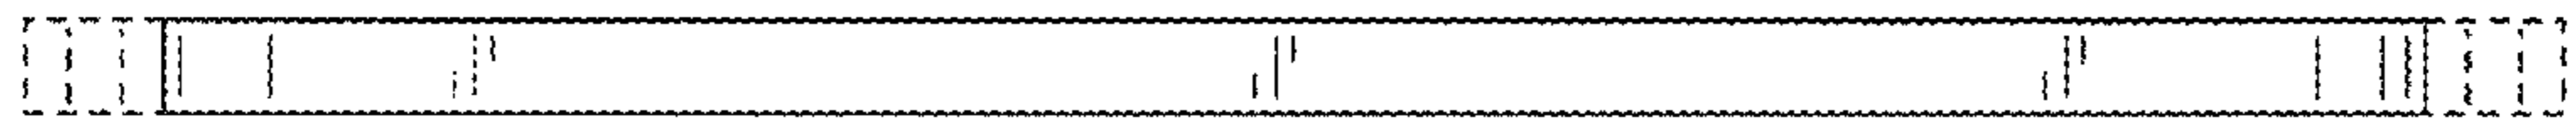


FIG. 14



FIG. 15

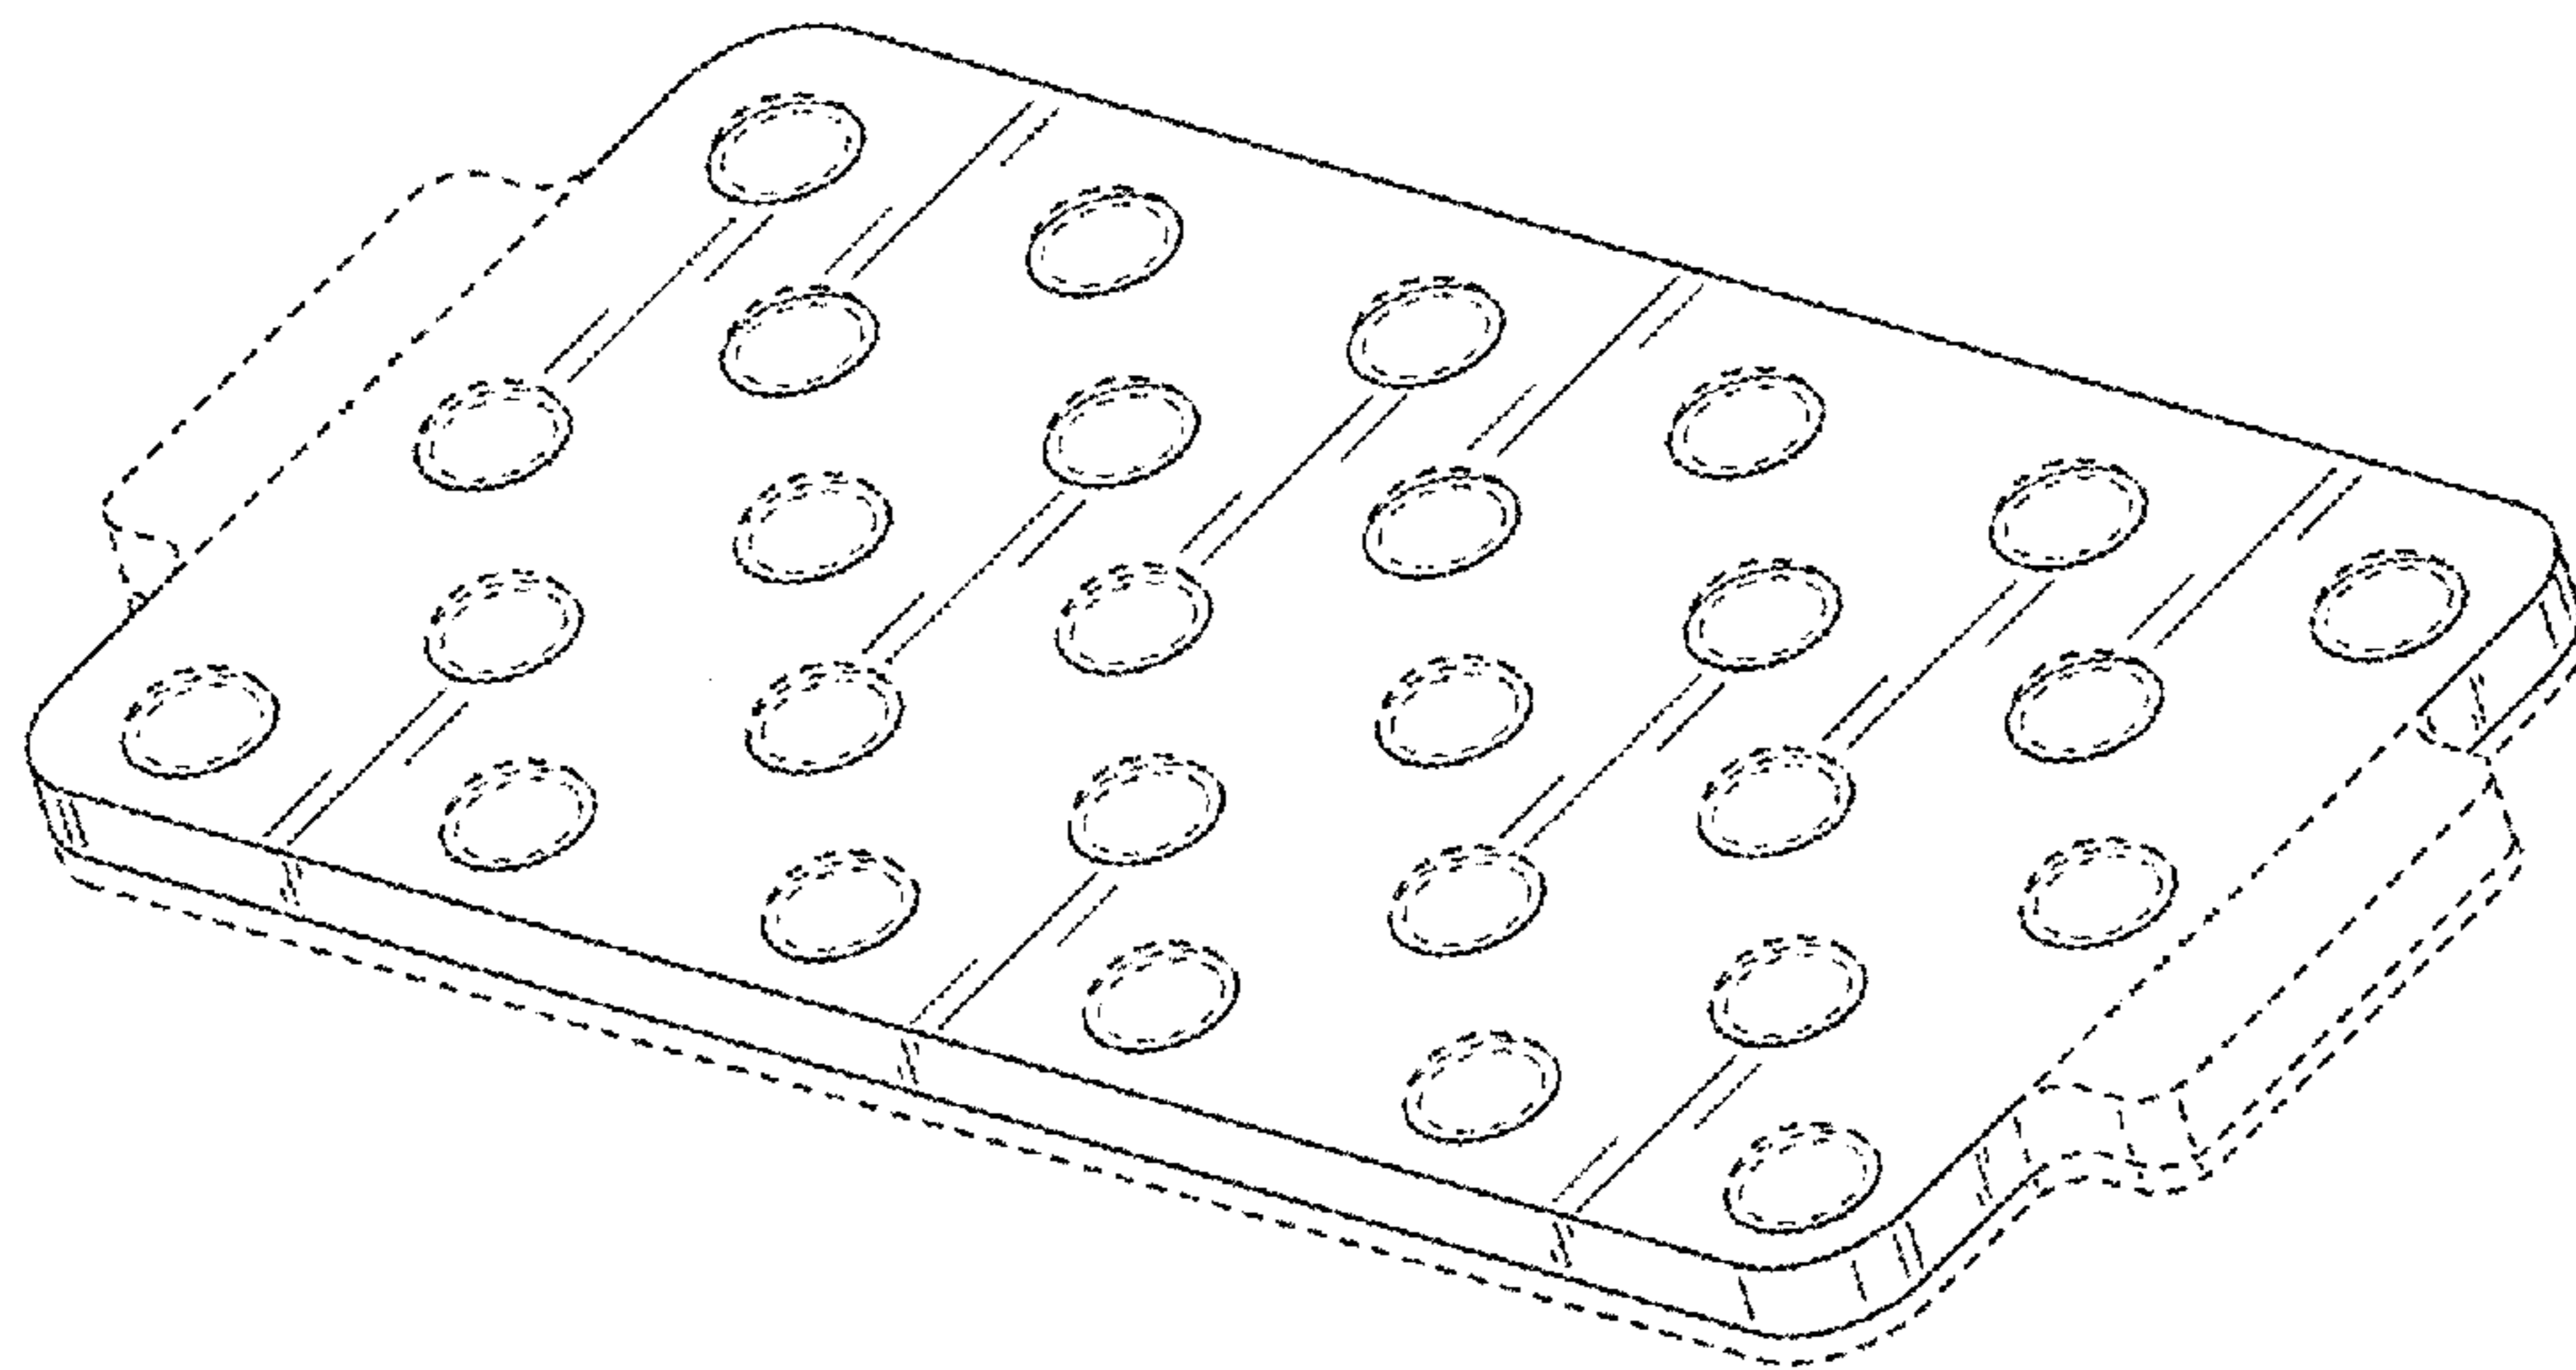


FIG. 16

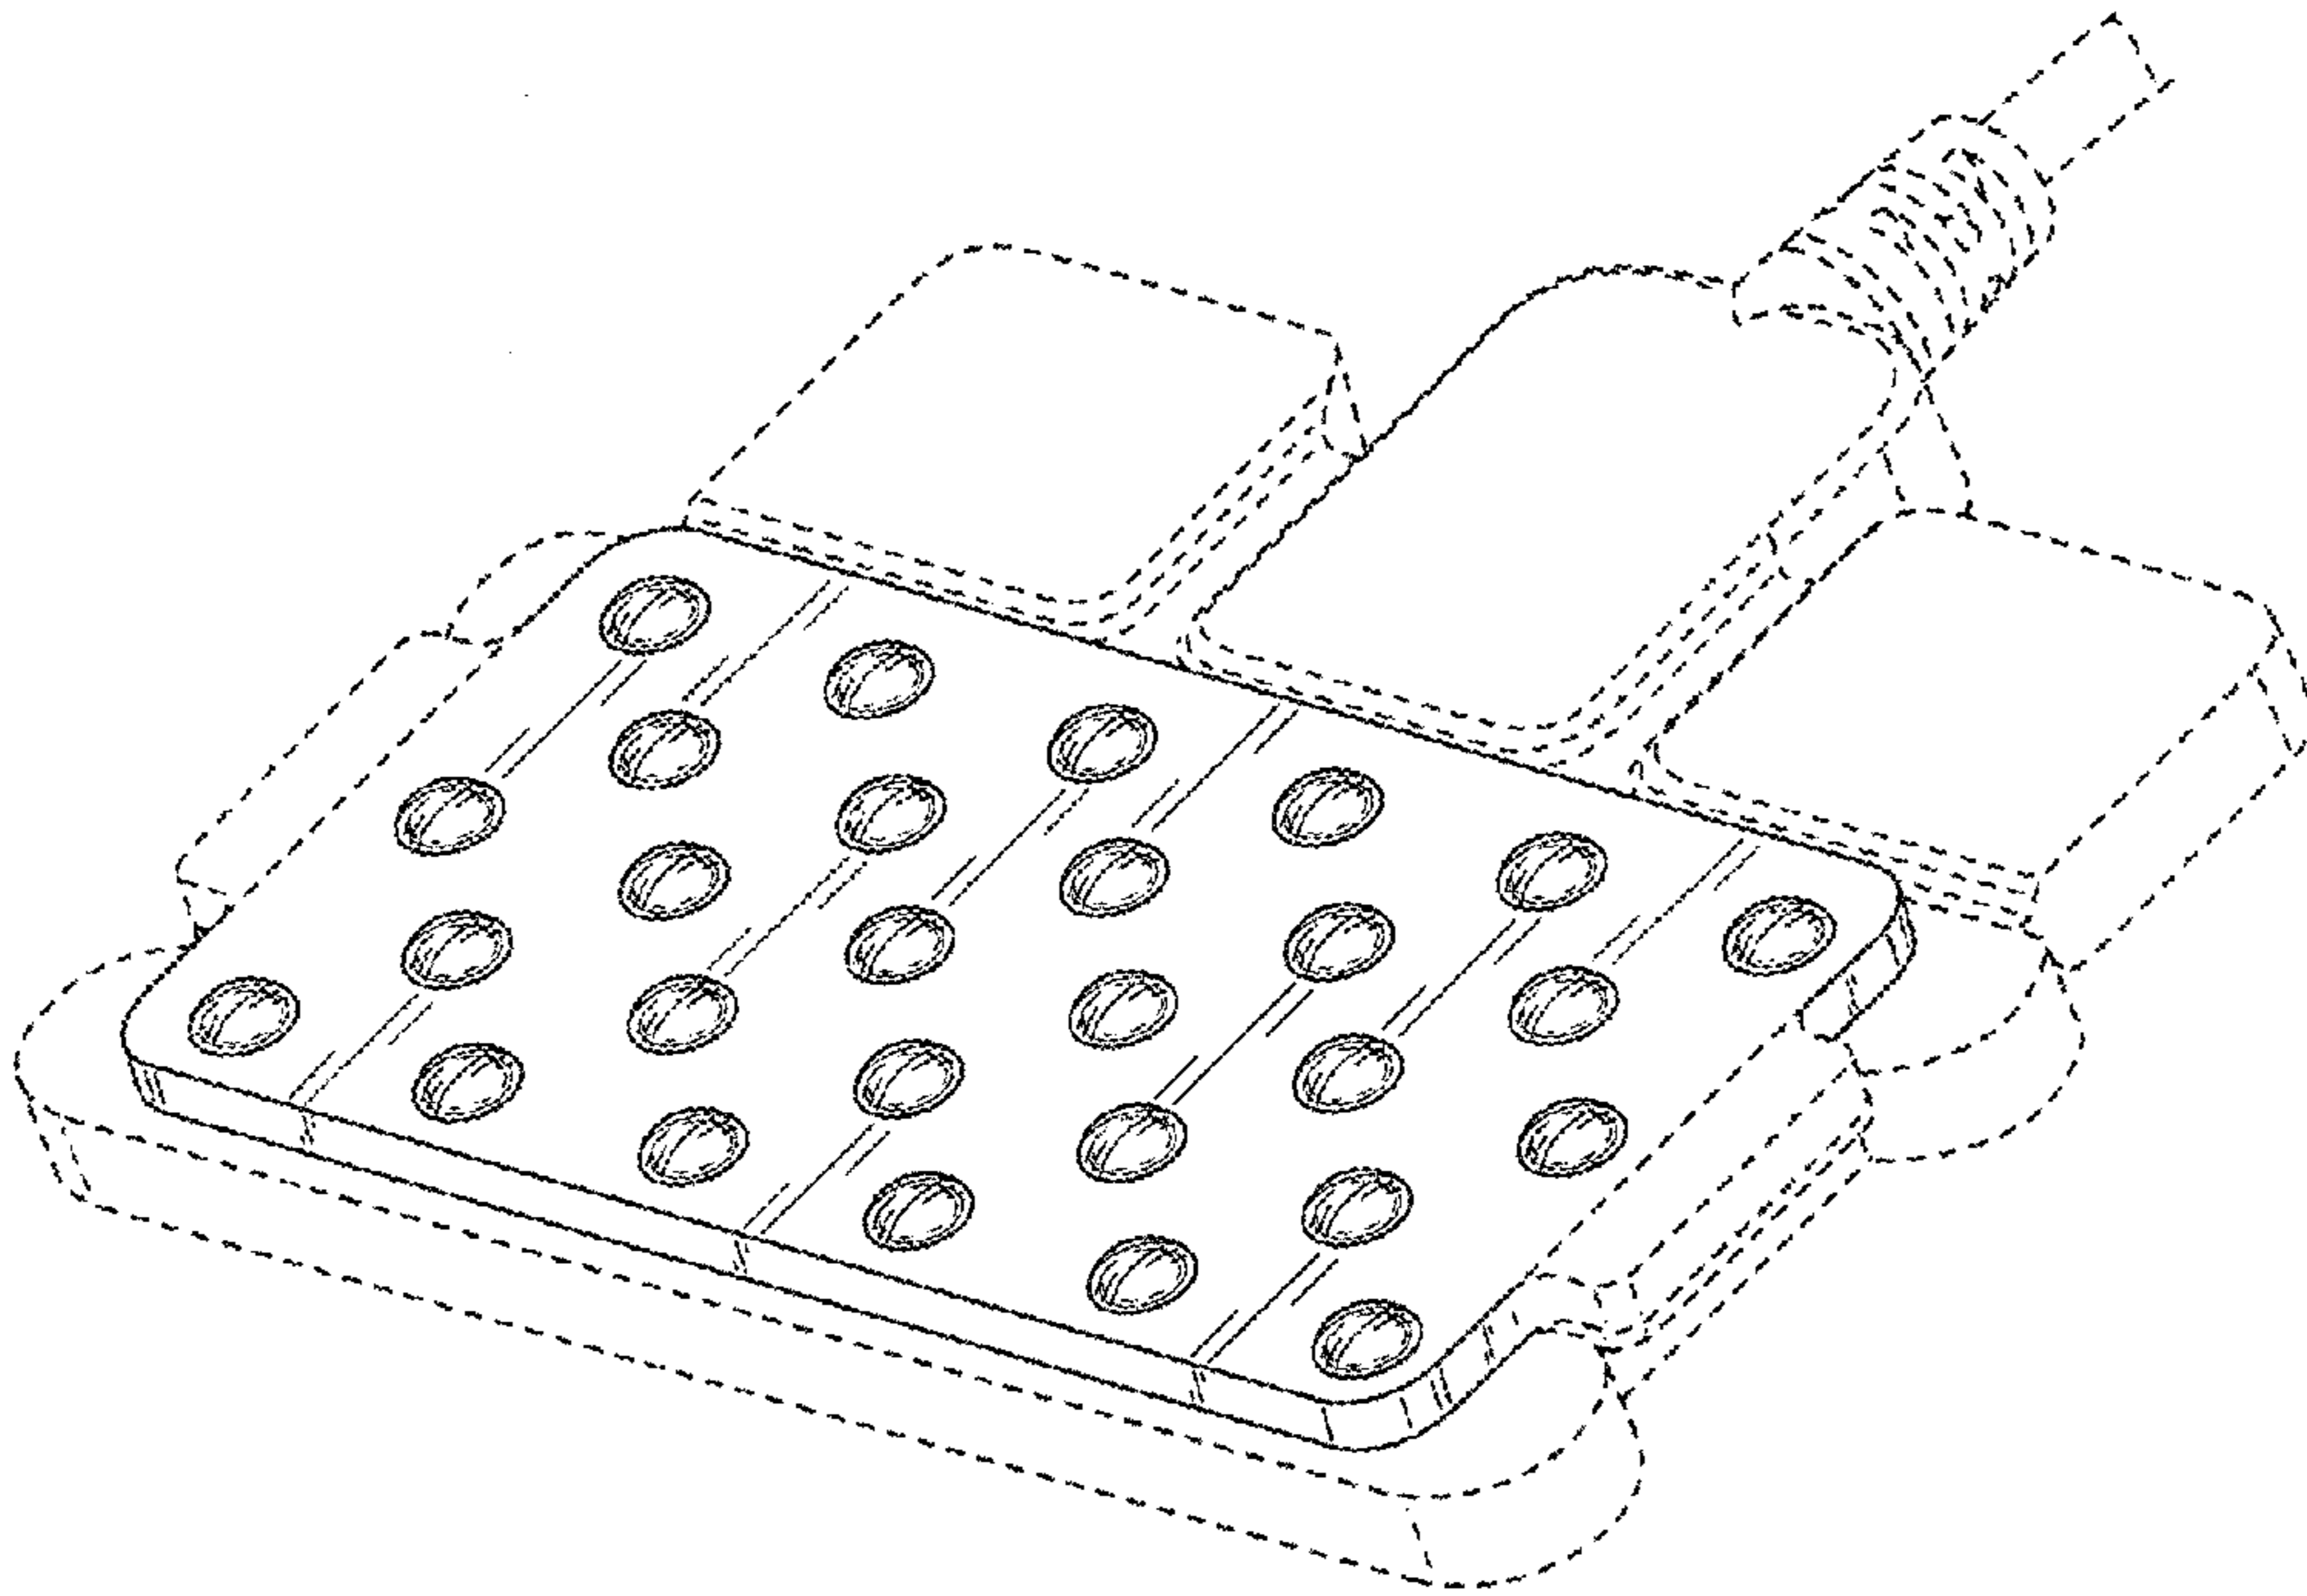


FIG. 17