

US00D764059S

(12) **United States Design Patent**
Browne et al.

(10) **Patent No.:** **US D764,059 S**
(45) **Date of Patent:** **** Aug. 16, 2016**

(54) **CHEST PAD FOR CPR FEEDBACK DEVICE**

(56) **References Cited**

(71) Applicant: **Physio-Control, Inc.**, Redmond, WA (US)

U.S. PATENT DOCUMENTS

(72) Inventors: **Gregory V. Browne**, Victoria (CA); **Adam Looker**, Victoria (CA); **Ryan D. Lee**, Victoria (CA); **Sarah A. Smith**, Victoria (CA); **Corey J. Centen**, Victoria (CA); **Maegan P. Wilkinson**, Seattle, WA (US); **Richard C. Nova**, Kirkland, WA (US); **Cathlene Durand Buchanan**, Shoreline, WA (US); **Chad Alan Follmar**, Louisville, CO (US); **David Mark VandeRiet**, Louisville, CO (US); **Seth Paul Lynch**, Raleigh, NC (US); **Mark Allen Catron**, Superior, CO (US); **Chad Clayton Walters**, Apex, NC (US)

D452,318 S	12/2001	Merry et al.	
D498,535 S	11/2004	Genau et al.	
D516,217 S	2/2006	Brown et al.	
D567,949 S	4/2008	Lash et al.	
7,429,250 B2	9/2008	Halperin et al.	
D604,855 S	11/2009	Shearlaw et al.	
D609,813 S	2/2010	Molden et al.	
D629,524 S	12/2010	Zeller et al.	
D639,437 S *	6/2011	Bishay et al.	D24/167
D643,929 S *	8/2011	DelloStritto et al.	D24/165
D654,179 S	2/2012	Bedingham et al.	
D659,251 S	5/2012	Kawamura et al.	
2009/0163838 A1	6/2009	Hecox et al.	
2010/0228165 A1	9/2010	Centen	
2012/0083720 A1 *	4/2012	Centen et al.	601/41

* cited by examiner

(73) Assignee: **PHYSIO-CONTROL, INC.**, Redmond, WA (US)

Primary Examiner — Anhdao Doan

(**) Term: **14 Years**

(74) *Attorney, Agent, or Firm* — Marger Johnson

(21) Appl. No.: **29/461,118**

(57) **CLAIM**

The ornamental design for a chest pad for CPR feedback device, as shown and described.

(22) Filed: **Jul. 18, 2013**

DESCRIPTION

Related U.S. Application Data

(62) Division of application No. 29/403,126, filed on Sep. 30, 2011, now Pat. No. Des. 689,614.

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/167**

(58) **Field of Classification Search**
USPC D24/165–168, 107, 186, 187; D10/46, D10/78, 98; 600/587, 509; 128/200.24; 601/41; 434/262, 265; 607/5–7, 142
See application file for complete search history.

FIG. 1 is a bottom and side perspective view of a chest pad for CPR feedback device showing our new design.

FIG. 2 is a bottom view of the chest pad for CPR feedback device shown in FIG. 1.


FIG. 3 is a side view of the chest pad for CPR feedback device shown in FIG. 1, the opposite side view being identical.

FIG. 4 is a first end view of the chest pad for CPR feedback device shown in FIG. 1; and,

FIG. 5 is a second end view of the chest pad for CPR feedback device shown in FIG. 1.

The broken lines in the drawing views are included for the purpose of illustrating portions of the chest pad for CPR feedback device that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

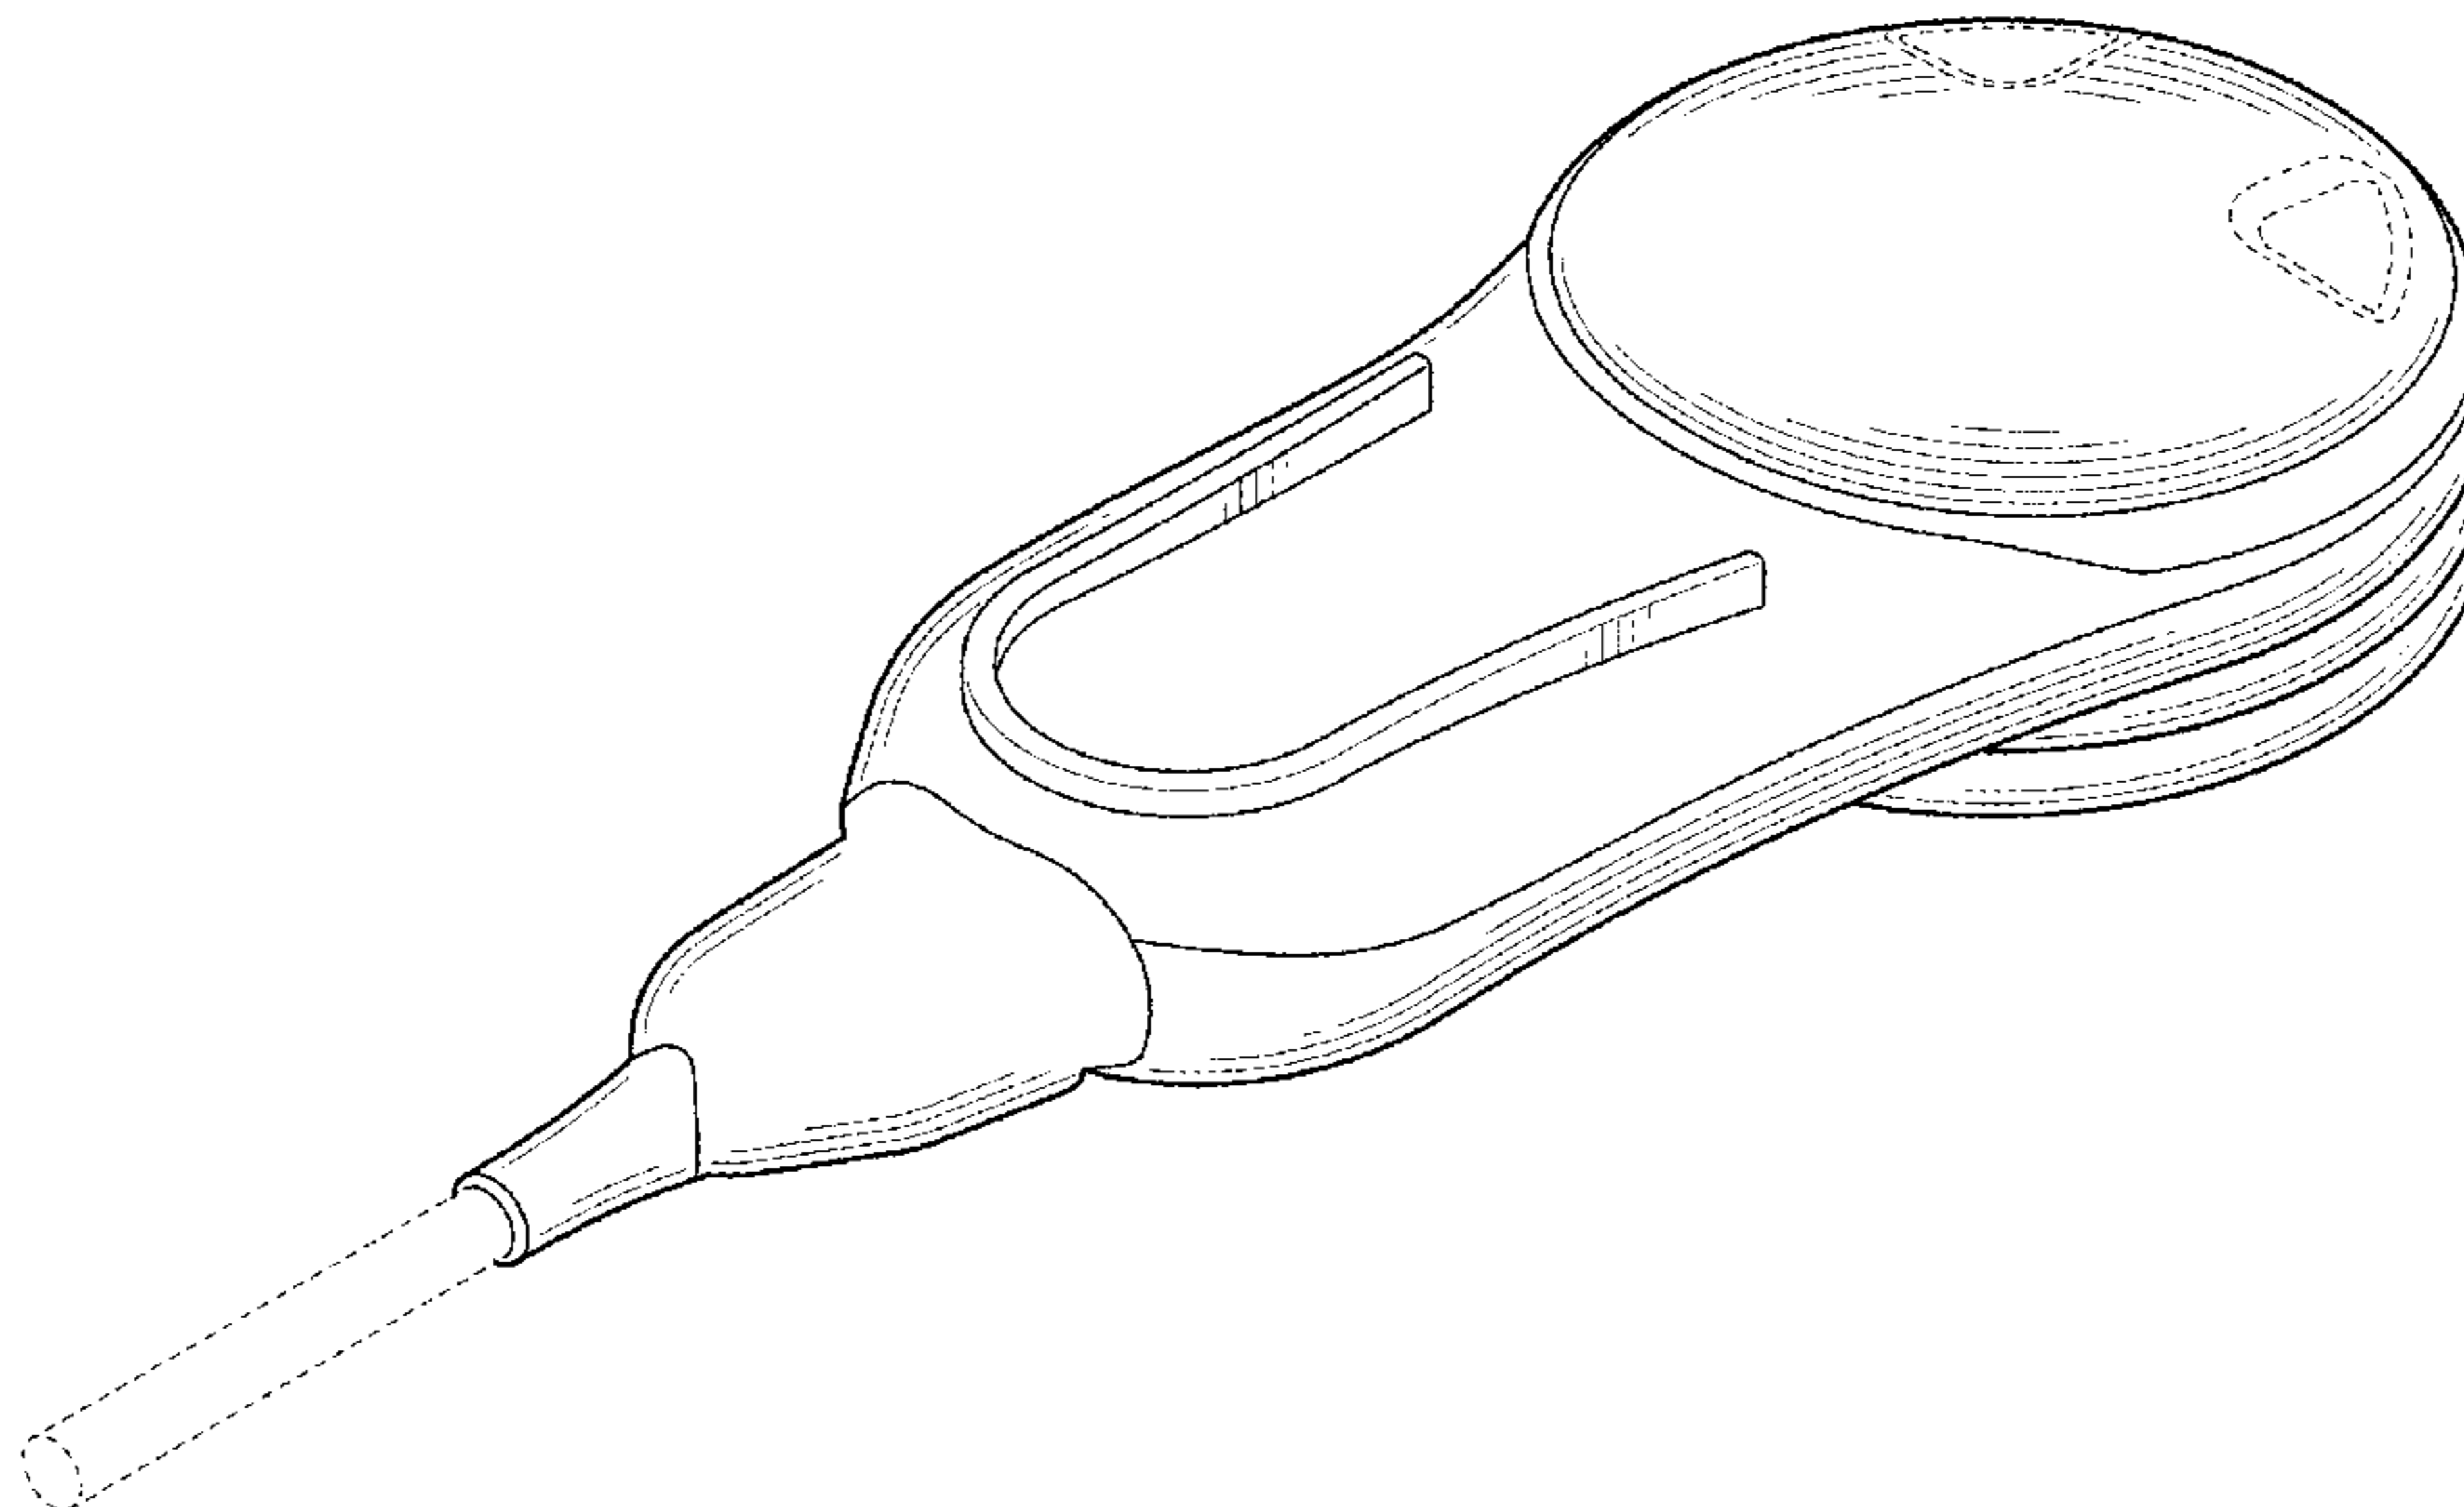

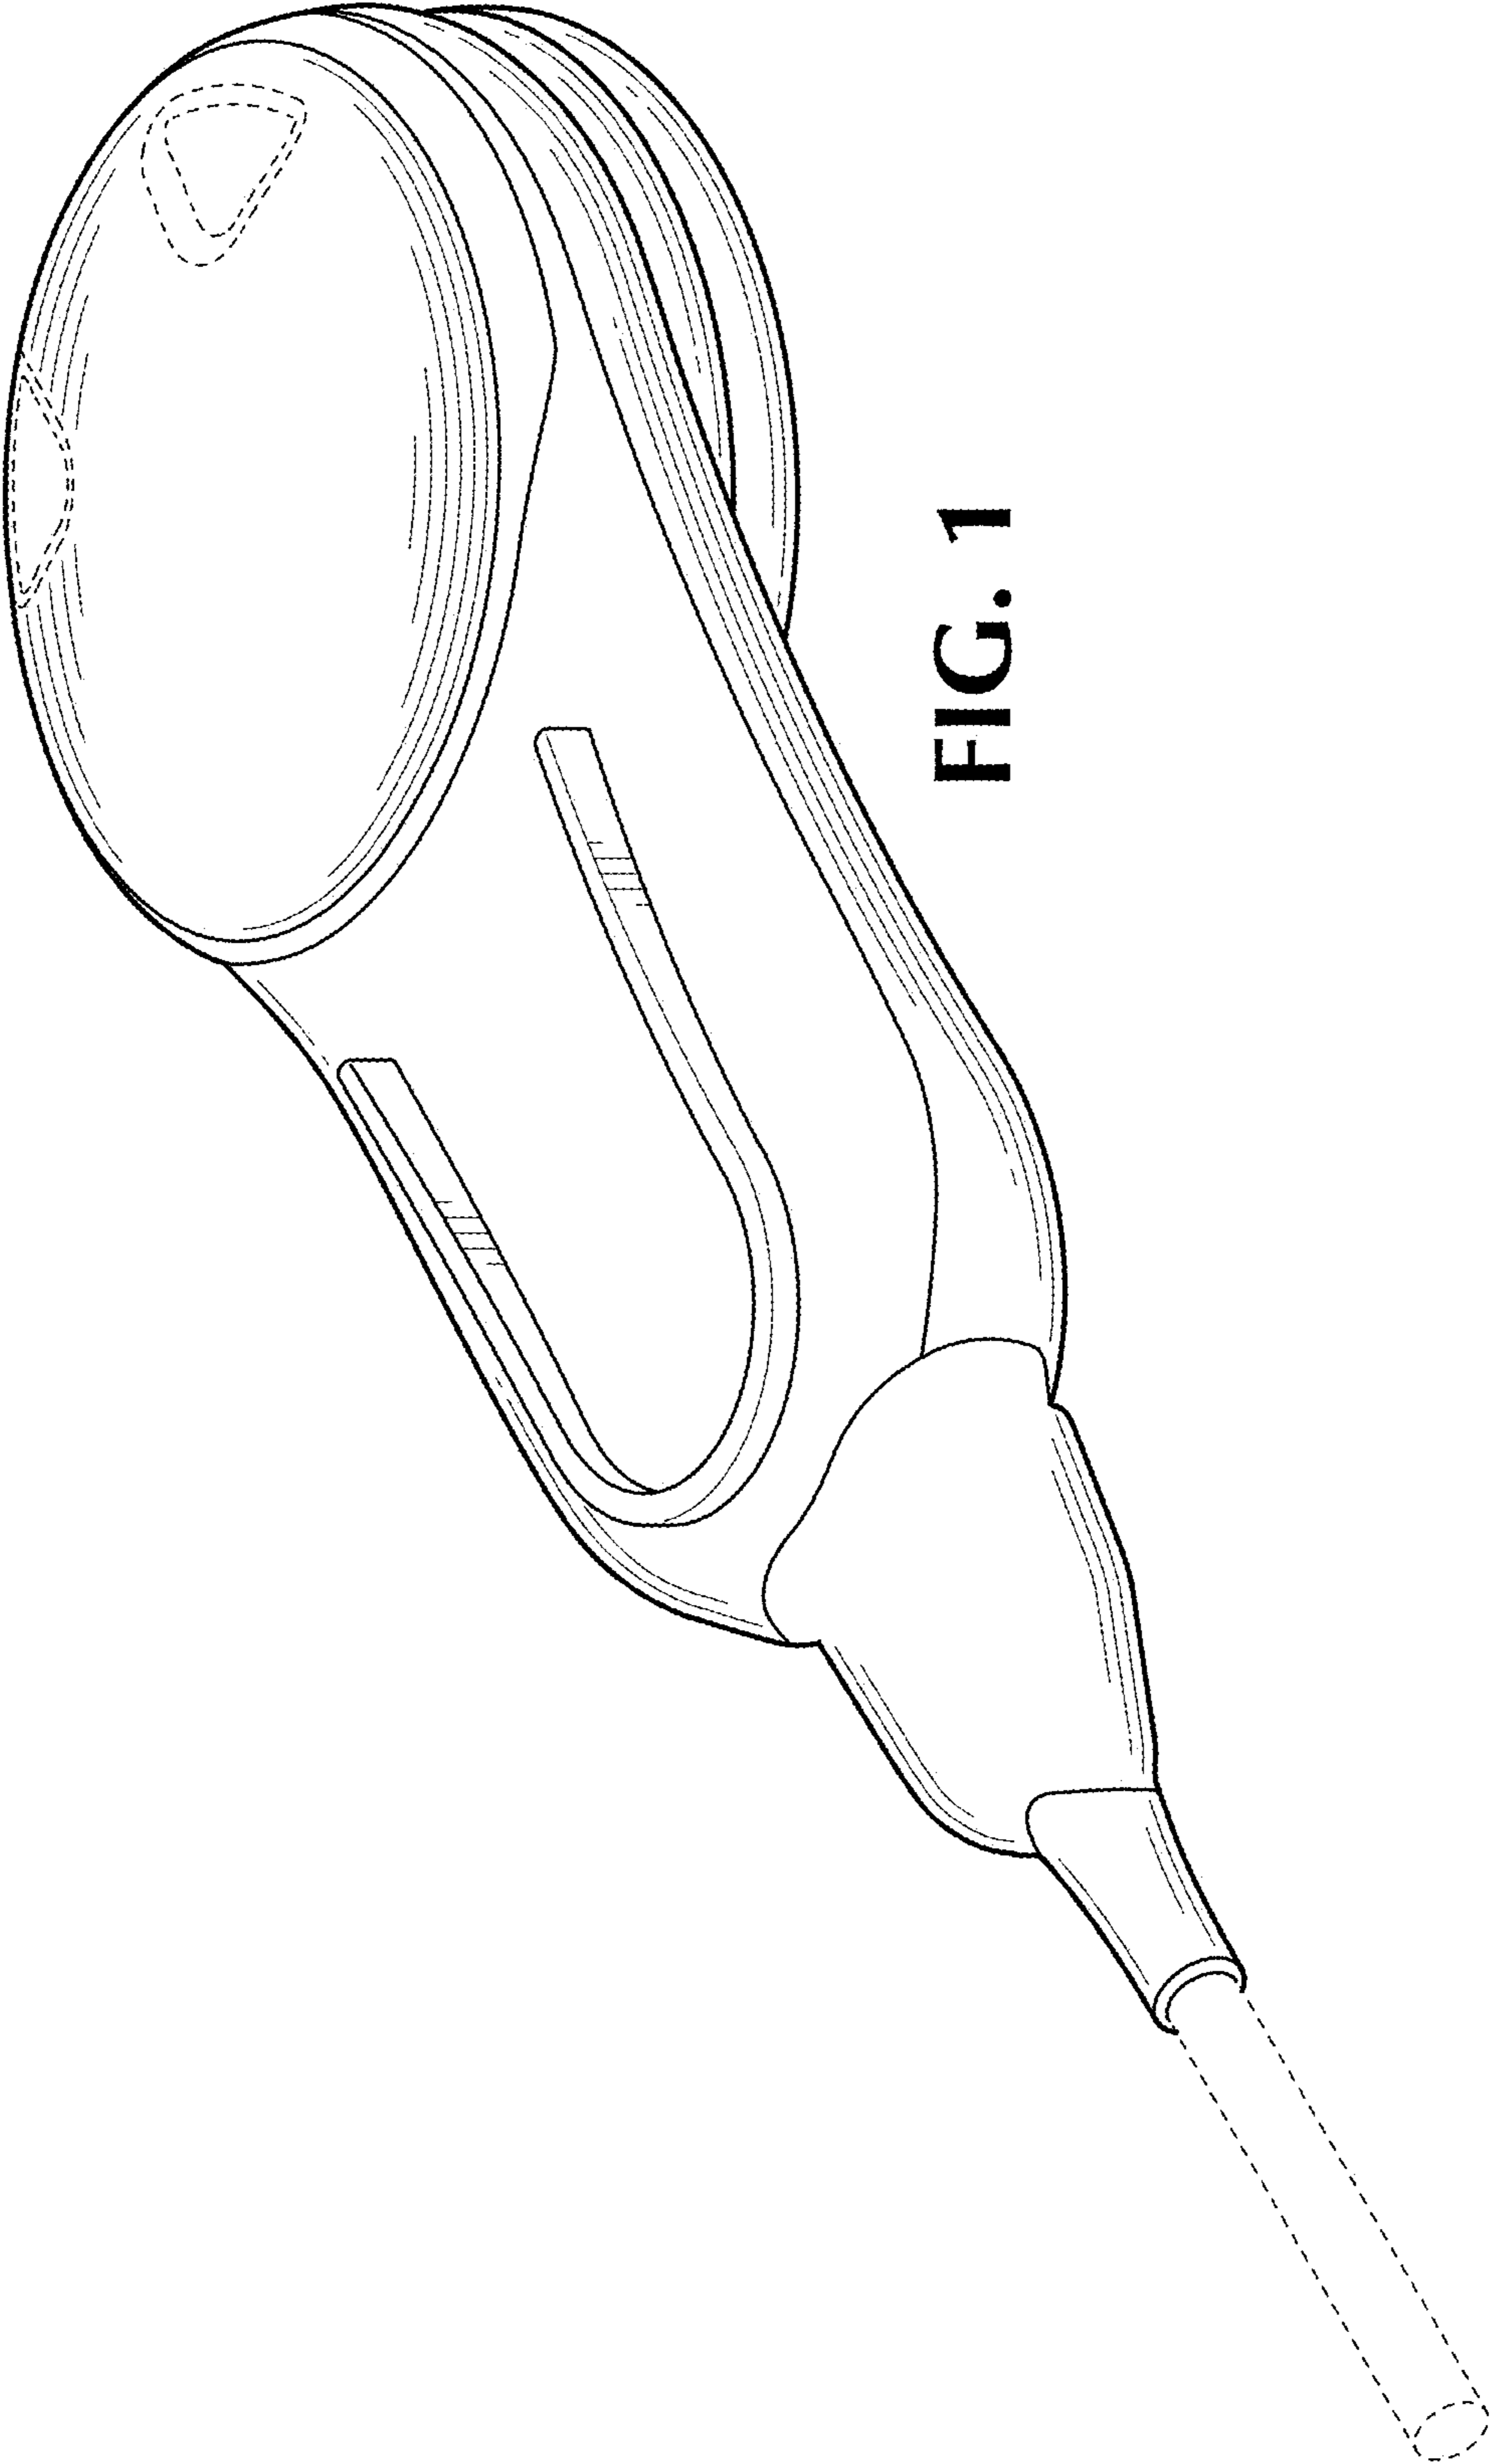


FIG. 1

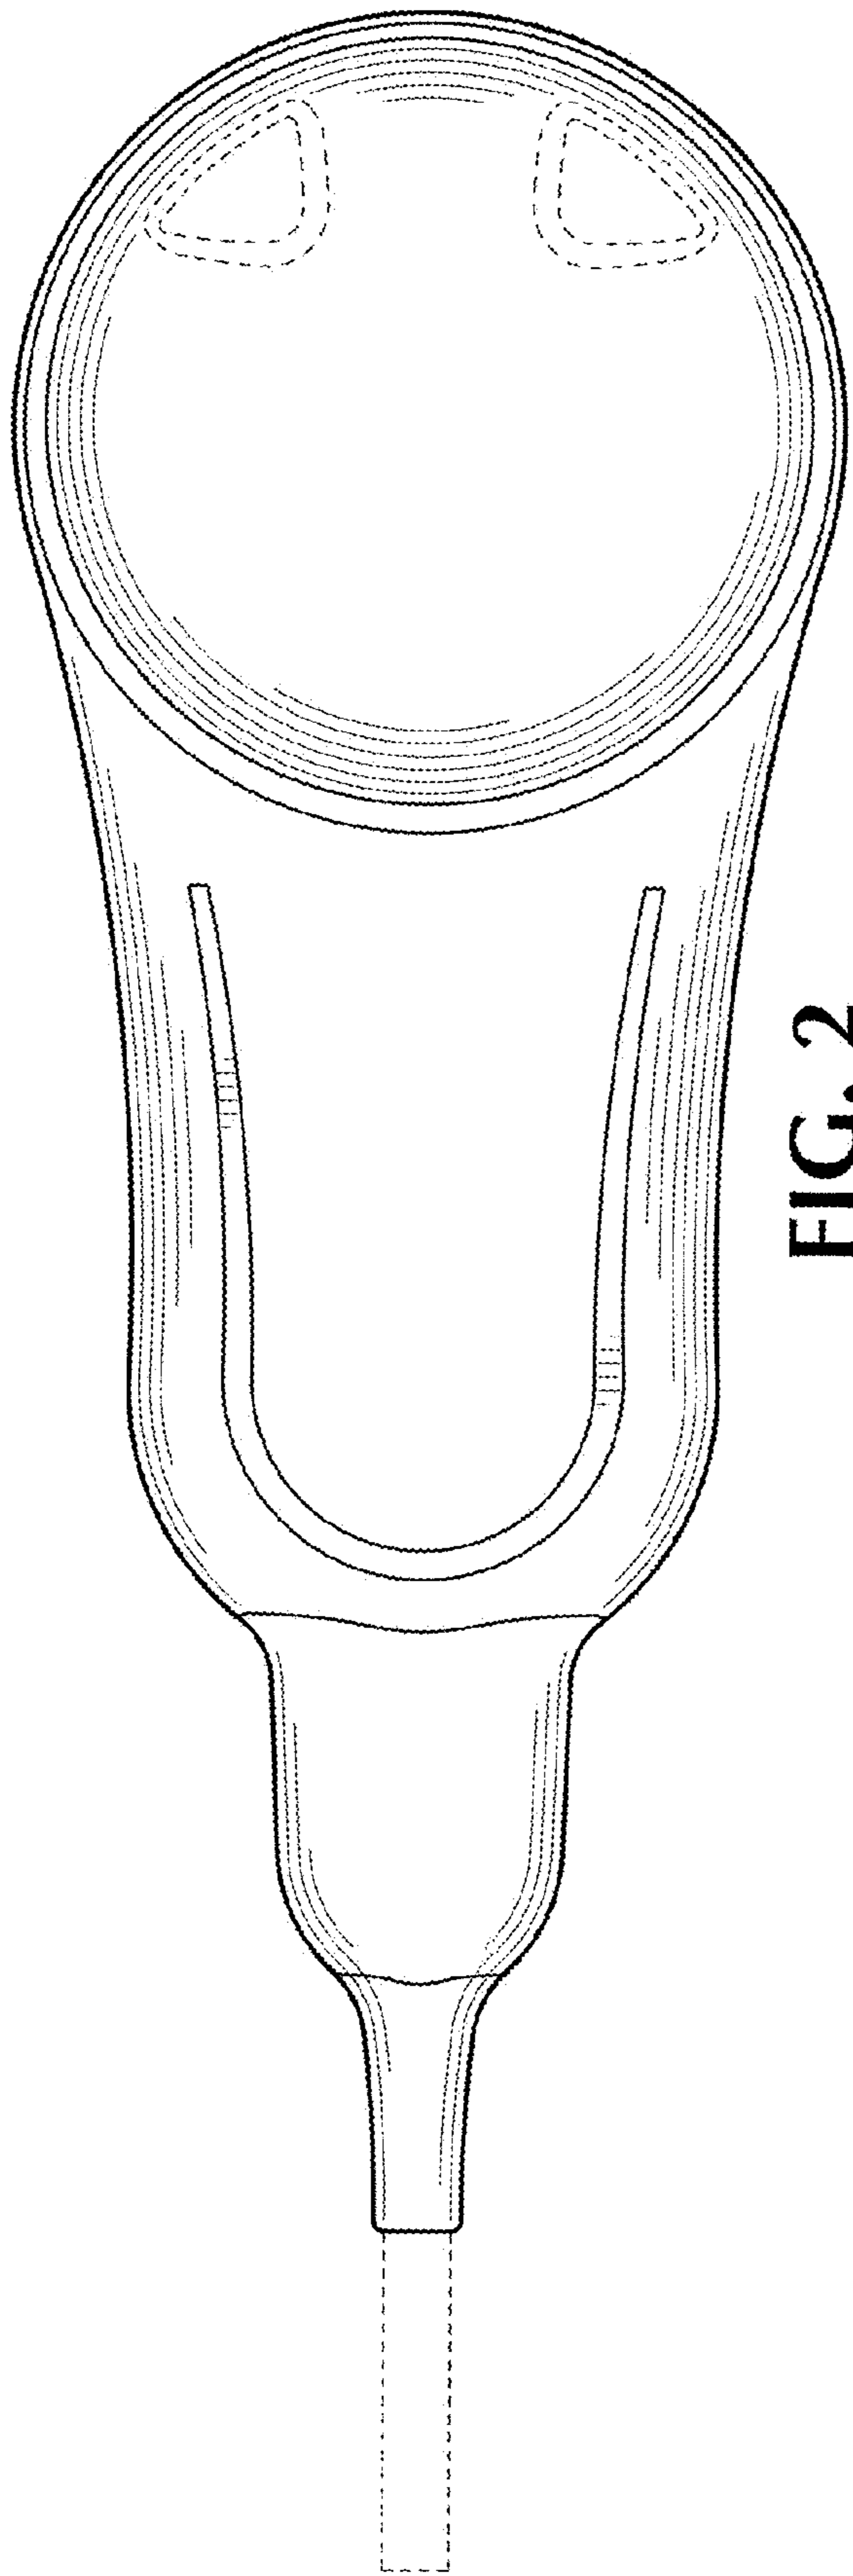


FIG. 2

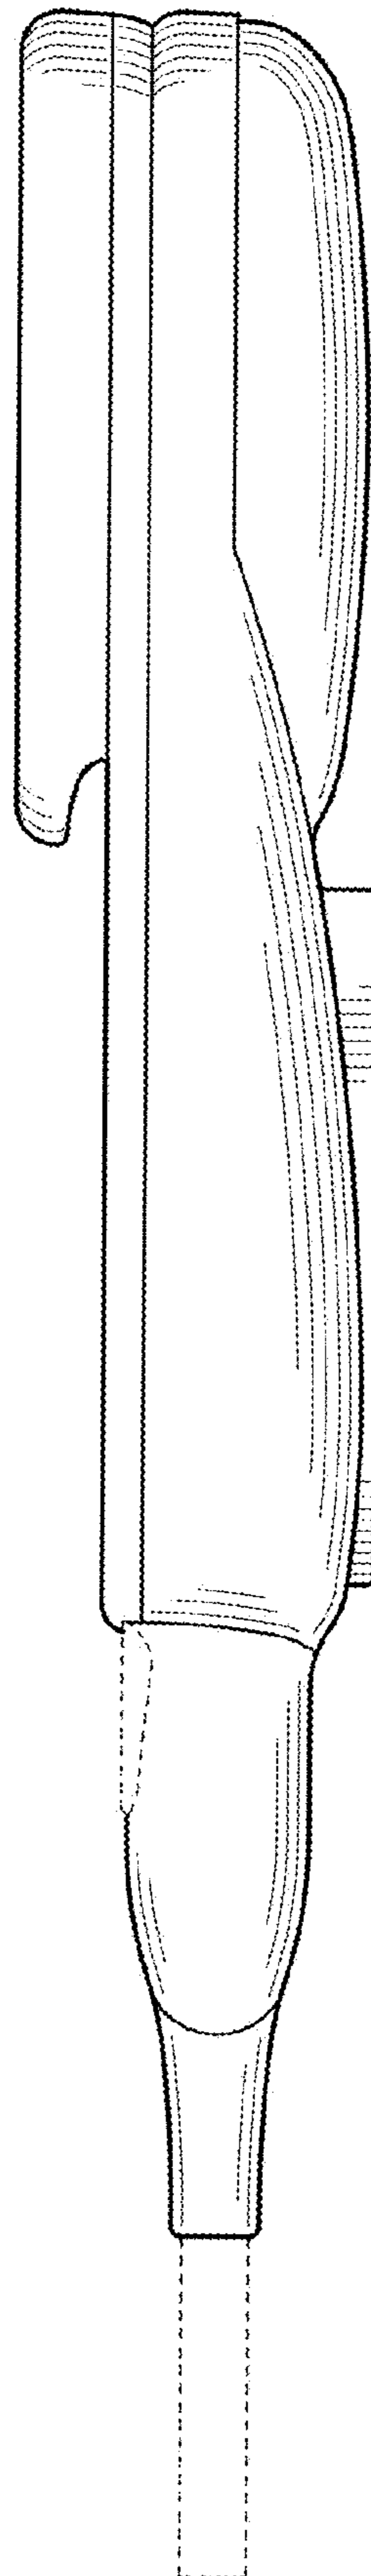


FIG. 3

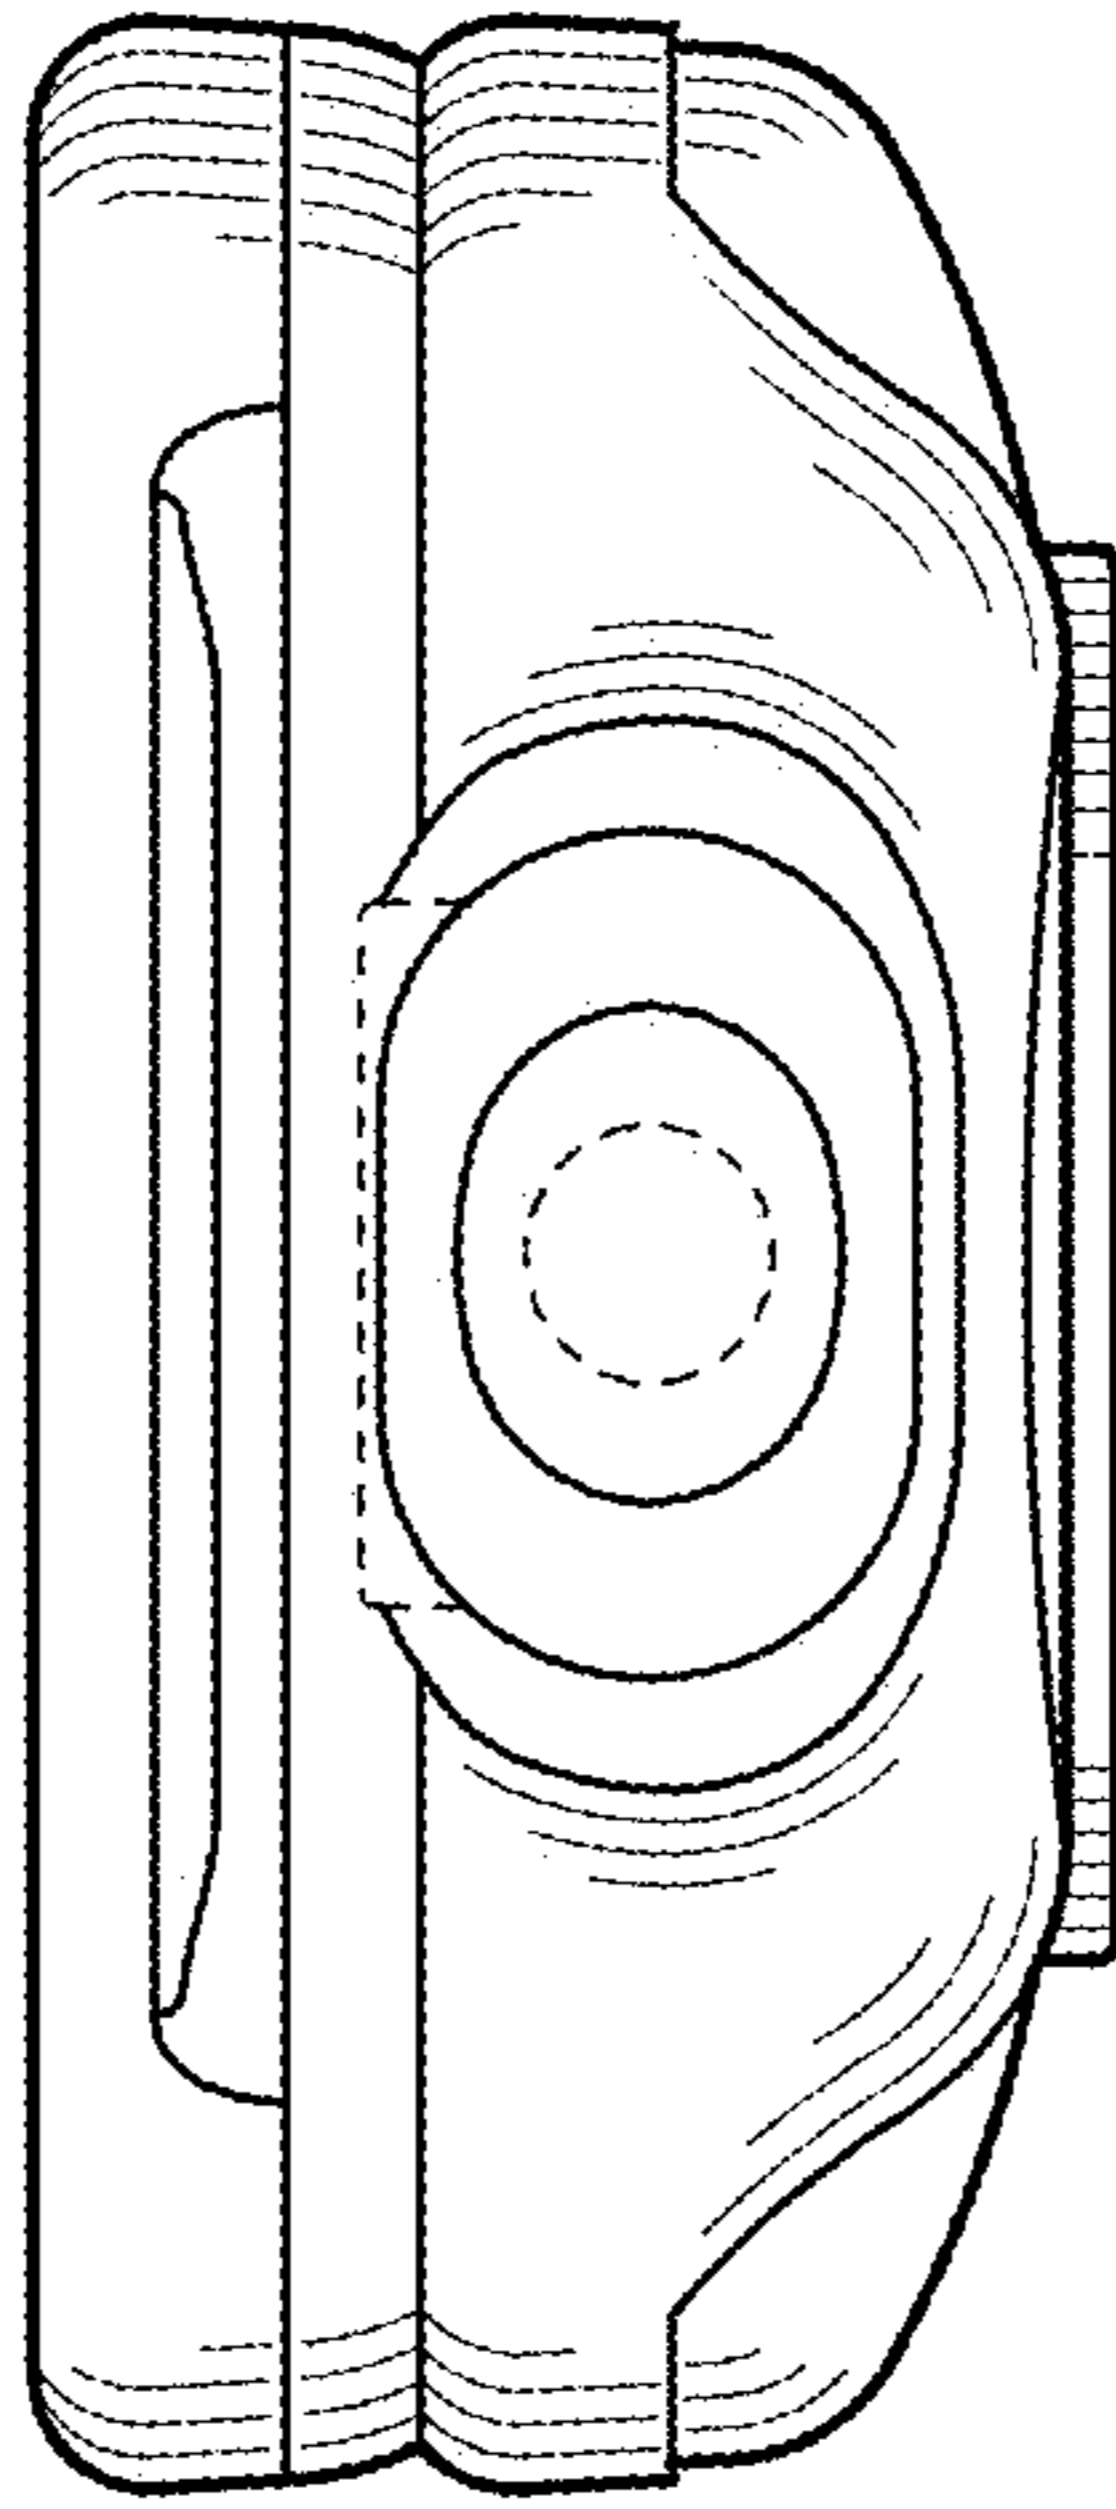


FIG. 5

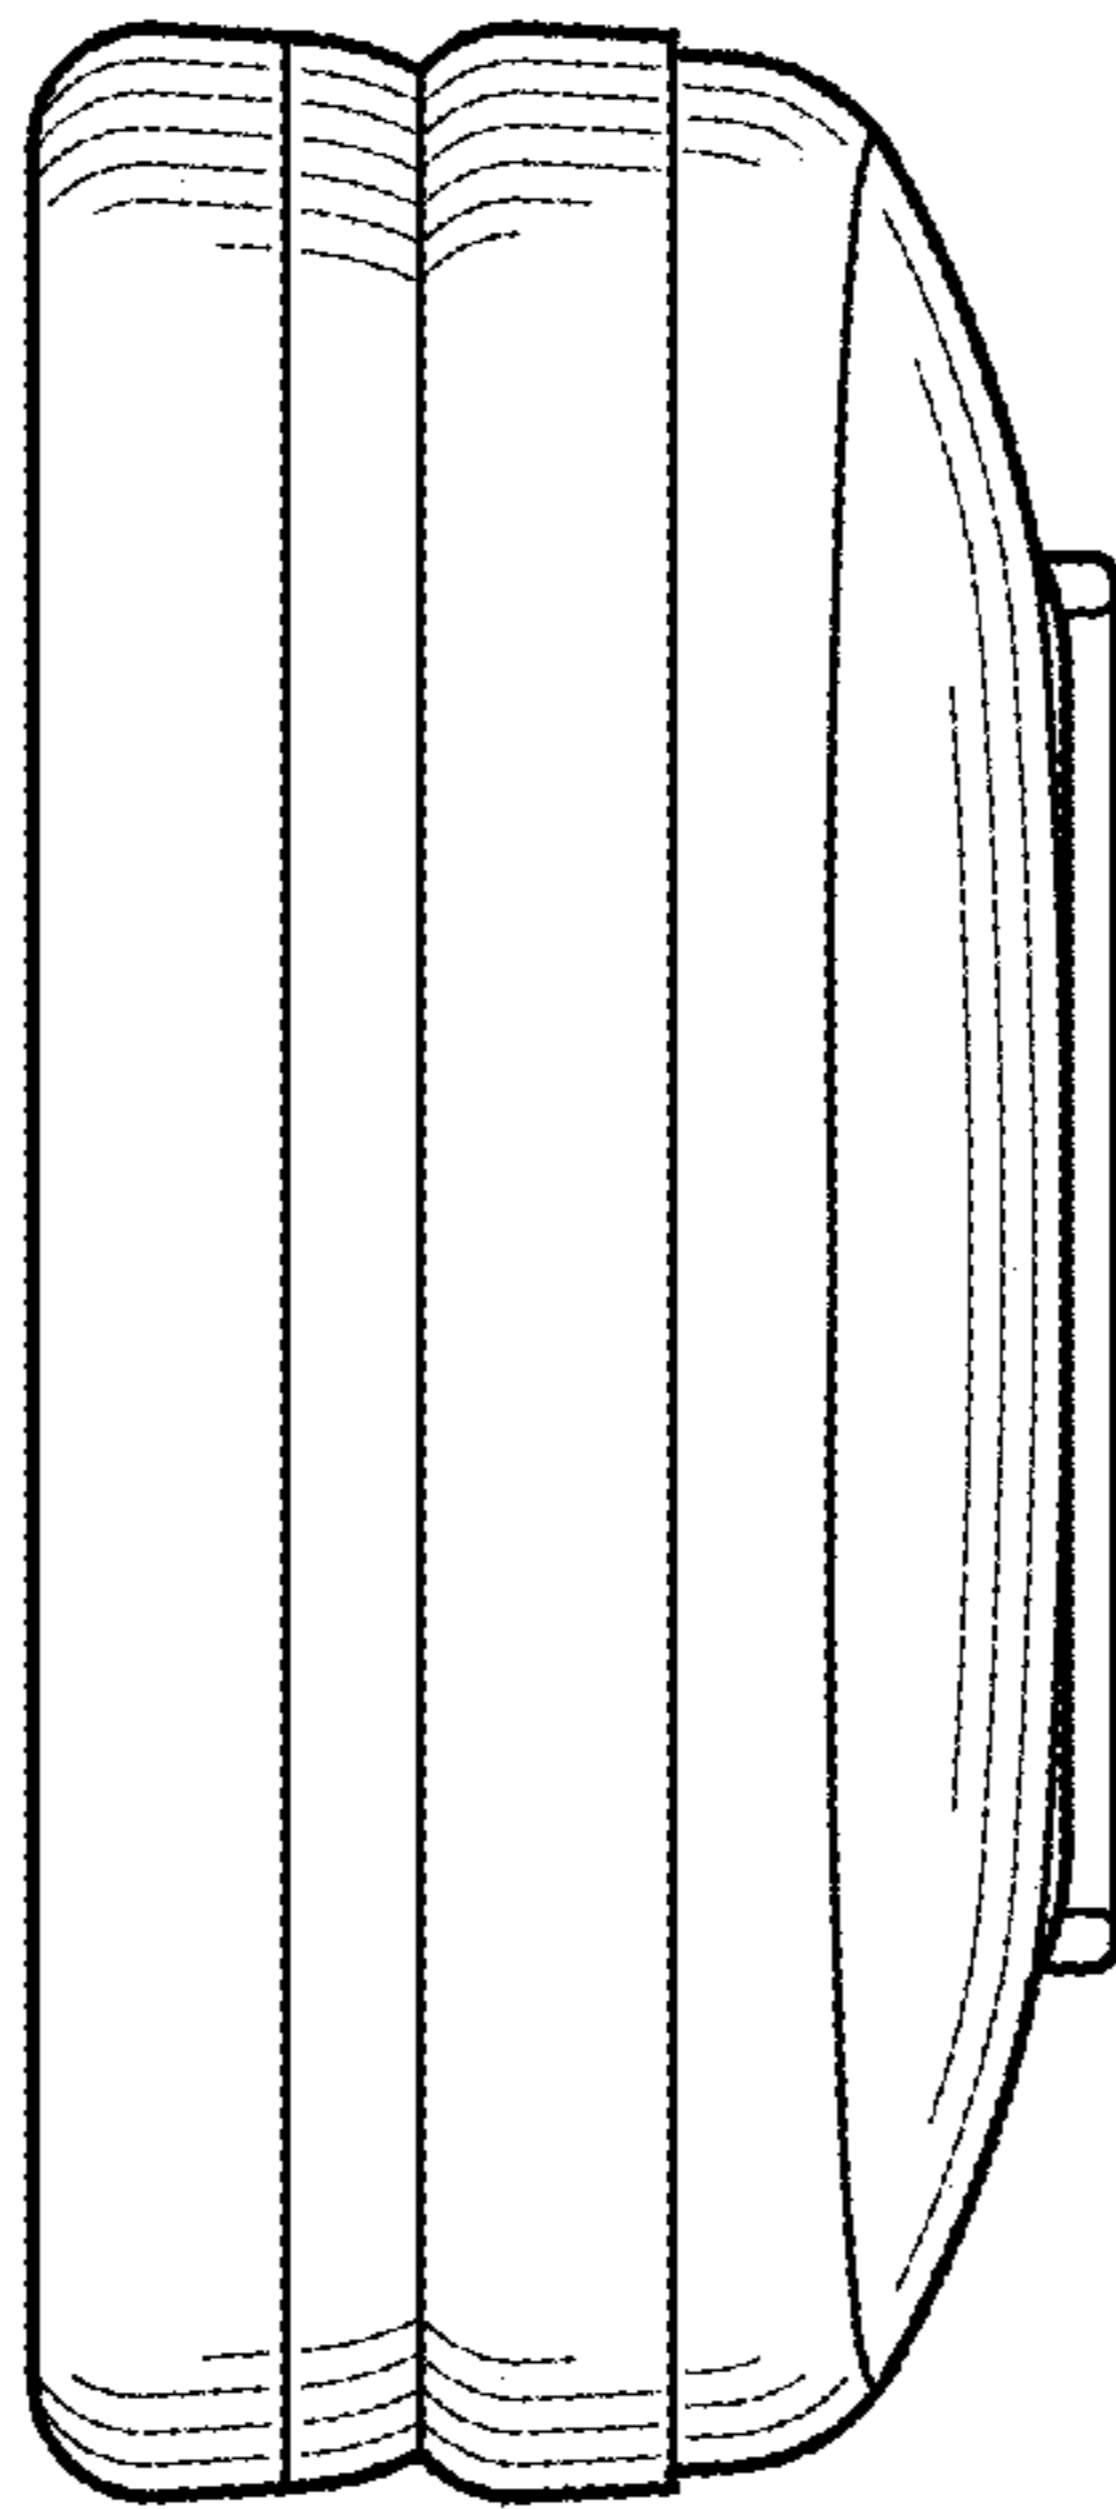


FIG. 4