

US00D764059S

(12) **United States Design Patent**
Browne et al.

(10) **Patent No.:** **US D764,059 S**
(45) **Date of Patent:** **** Aug. 16, 2016**

(54) **CHEST PAD FOR CPR FEEDBACK DEVICE**

(56) **References Cited**

(71) Applicant: **Physio-Control, Inc.**, Redmond, WA (US)

U.S. PATENT DOCUMENTS

(72) Inventors: **Gregory V. Browne**, Victoria (CA); **Adam Looker**, Victoria (CA); **Ryan D. Lee**, Victoria (CA); **Sarah A. Smith**, Victoria (CA); **Corey J. Centen**, Victoria (CA); **Maegan P. Wilkinson**, Seattle, WA (US); **Richard C. Nova**, Kirkland, WA (US); **Cathlene Durand Buchanan**, Shoreline, WA (US); **Chad Alan Follmar**, Louisville, CO (US); **David Mark VandeRiet**, Louisville, CO (US); **Seth Paul Lynch**, Raleigh, NC (US); **Mark Allen Catron**, Superior, CO (US); **Chad Clayton Walters**, Apex, NC (US)

| | | | |
|-------------------|---------|--------------------------|---------|
| D452,318 S | 12/2001 | Merry et al. | |
| D498,535 S | 11/2004 | Genau et al. | |
| D516,217 S | 2/2006 | Brown et al. | |
| D567,949 S | 4/2008 | Lash et al. | |
| 7,429,250 B2 | 9/2008 | Halperin et al. | |
| D604,855 S | 11/2009 | Shearlaw et al. | |
| D609,813 S | 2/2010 | Molden et al. | |
| D629,524 S | 12/2010 | Zeller et al. | |
| D639,437 S * | 6/2011 | Bishay et al. | D24/167 |
| D643,929 S * | 8/2011 | DelloStritto et al. | D24/165 |
| D654,179 S | 2/2012 | Bedingham et al. | |
| D659,251 S | 5/2012 | Kawamura et al. | |
| 2009/0163838 A1 | 6/2009 | Hecox et al. | |
| 2010/0228165 A1 | 9/2010 | Centen | |
| 2012/0083720 A1 * | 4/2012 | Centen et al. | 601/41 |

* cited by examiner

(73) Assignee: **PHYSIO-CONTROL, INC.**, Redmond, WA (US)

Primary Examiner — Anhdao Doan

(**) Term: **14 Years**

(74) *Attorney, Agent, or Firm* — Marger Johnson

(21) Appl. No.: **29/461,118**

(57) **CLAIM**

The ornamental design for a chest pad for CPR feedback device, as shown and described.

(22) Filed: **Jul. 18, 2013**

DESCRIPTION

Related U.S. Application Data

(62) Division of application No. 29/403,126, filed on Sep. 30, 2011, now Pat. No. Des. 689,614.

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/167**

(58) **Field of Classification Search**
USPC D24/165–168, 107, 186, 187; D10/46, D10/78, 98; 600/587, 509; 128/200.24; 601/41; 434/262, 265; 607/5–7, 142
See application file for complete search history.

FIG. 1 is a bottom and side perspective view of a chest pad for CPR feedback device showing our new design.

FIG. 2 is a bottom view of the chest pad for CPR feedback device shown in FIG. 1.


FIG. 3 is a side view of the chest pad for CPR feedback device shown in FIG. 1, the opposite side view being identical.

FIG. 4 is a first end view of the chest pad for CPR feedback device shown in FIG. 1; and,

FIG. 5 is a second end view of the chest pad for CPR feedback device shown in FIG. 1.

The broken lines in the drawing views are included for the purpose of illustrating portions of the chest pad for CPR feedback device that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

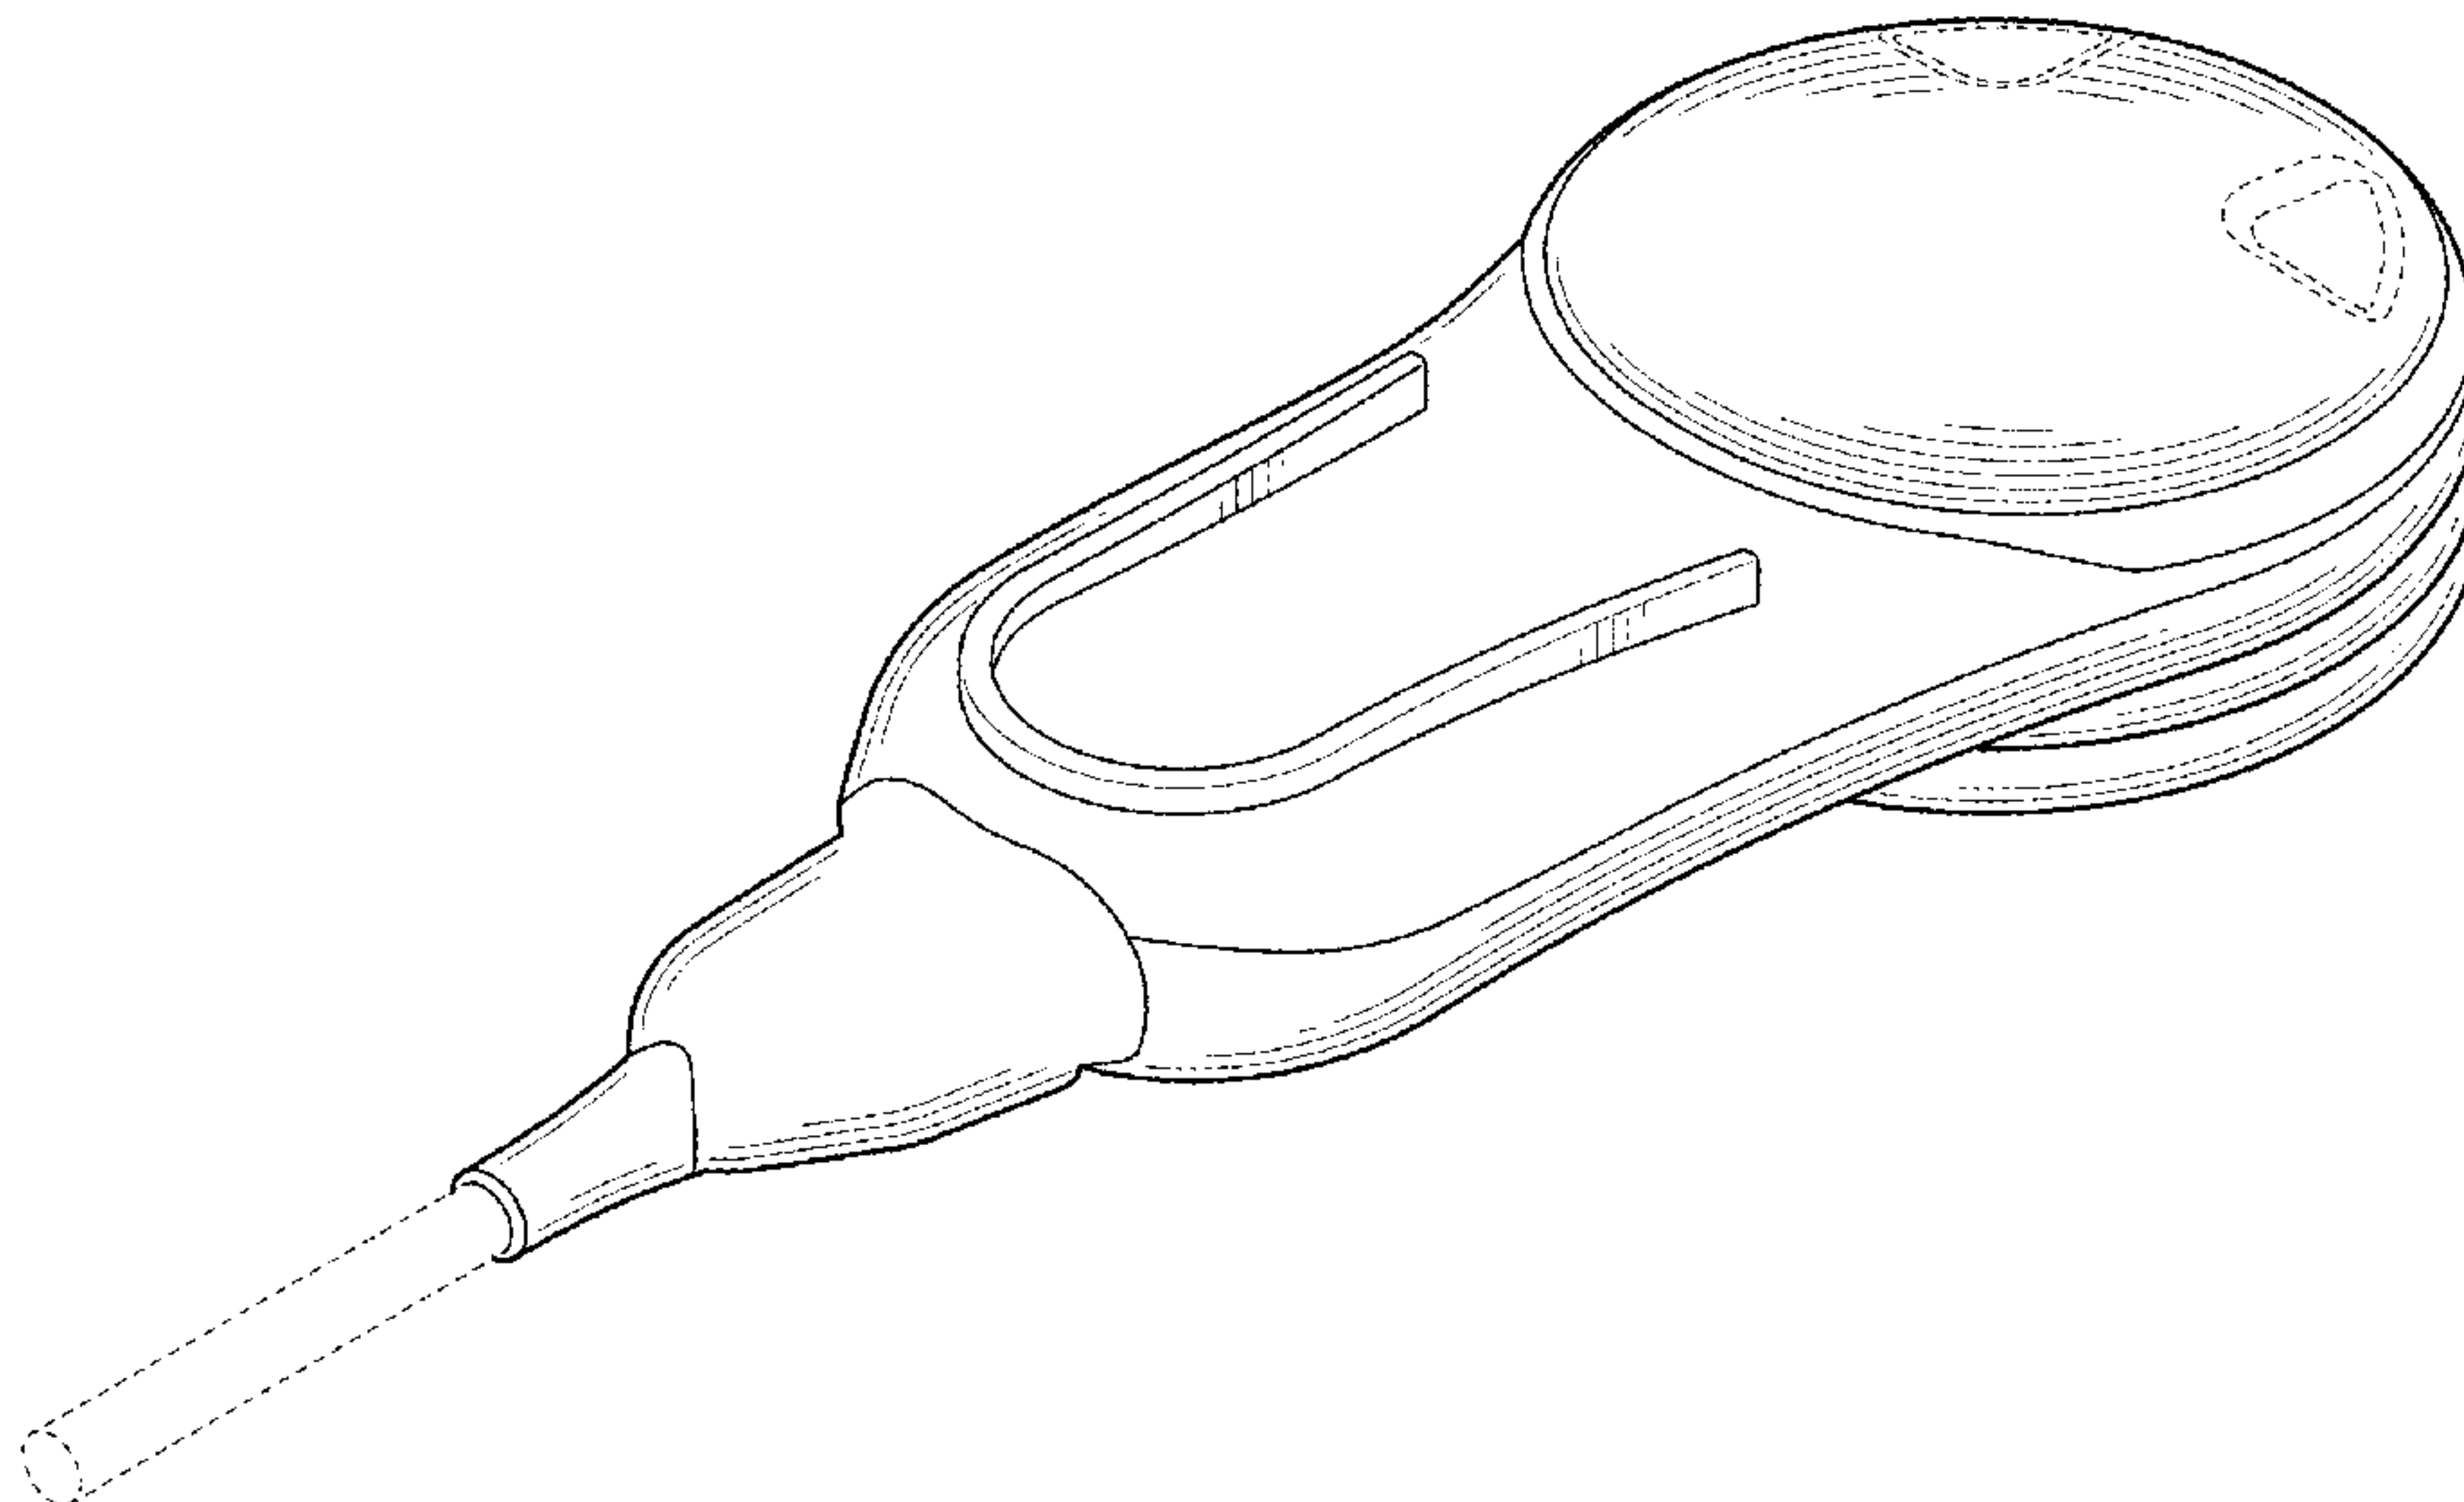

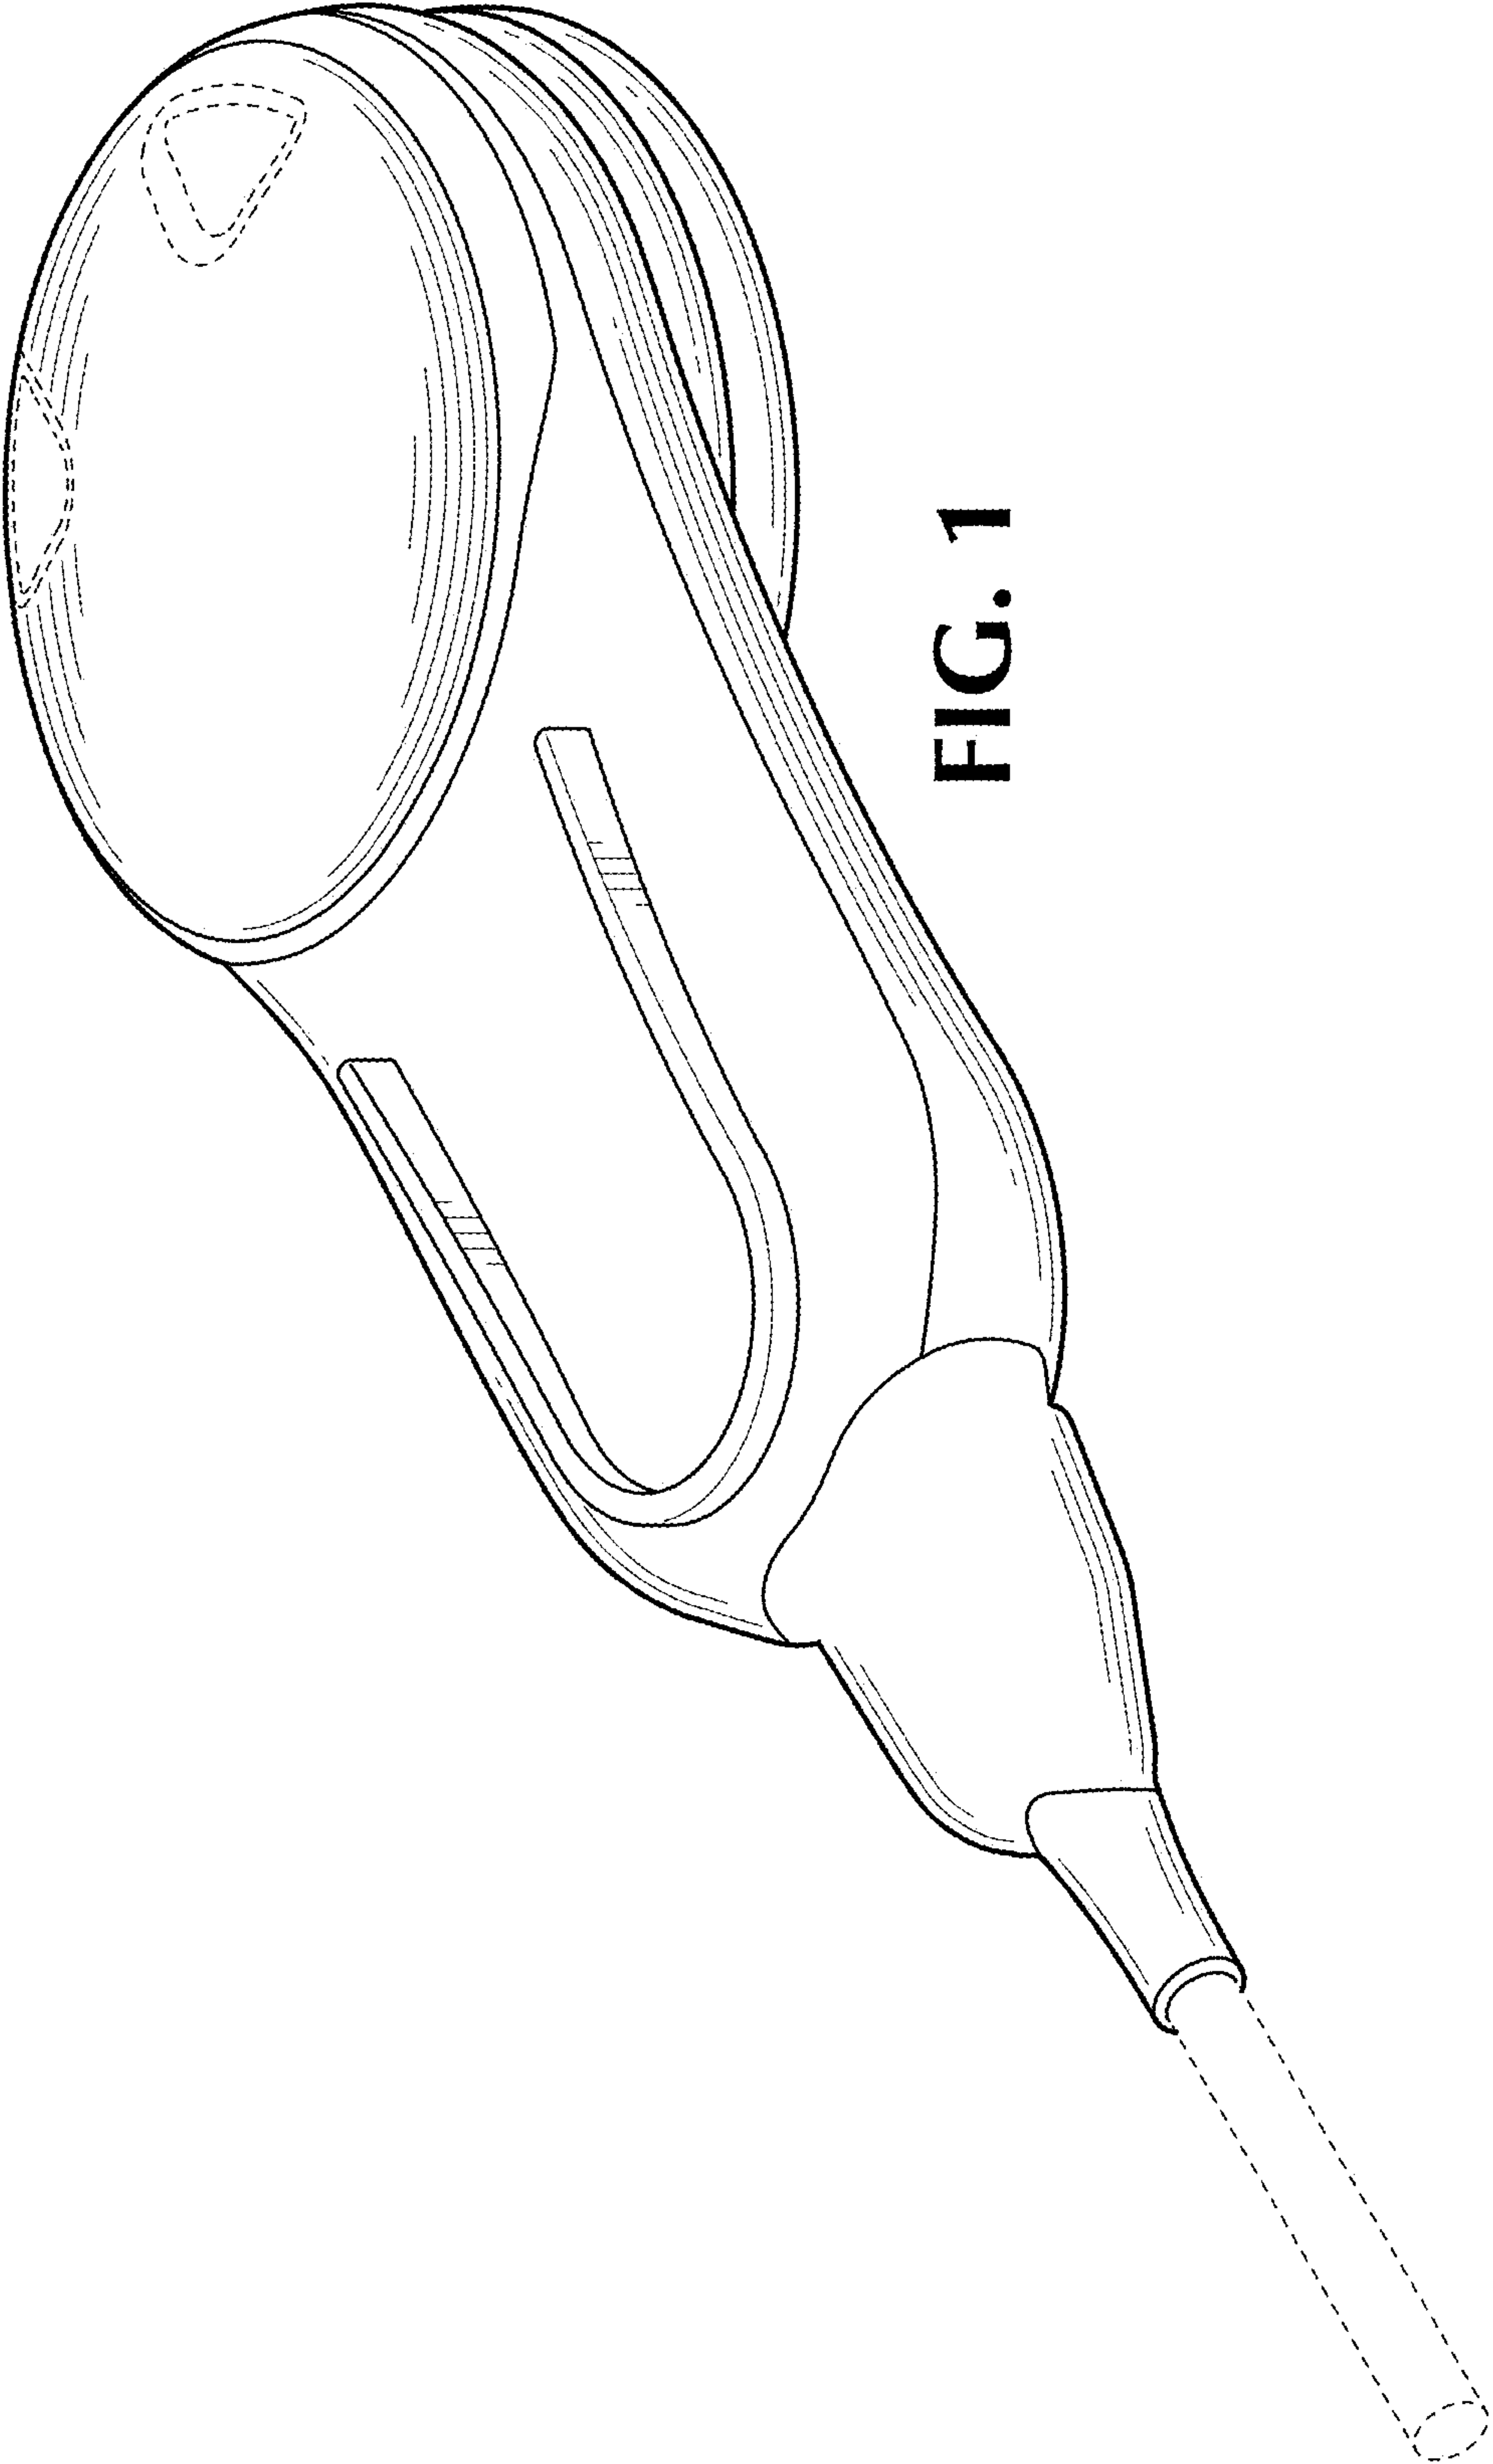


FIG. 1

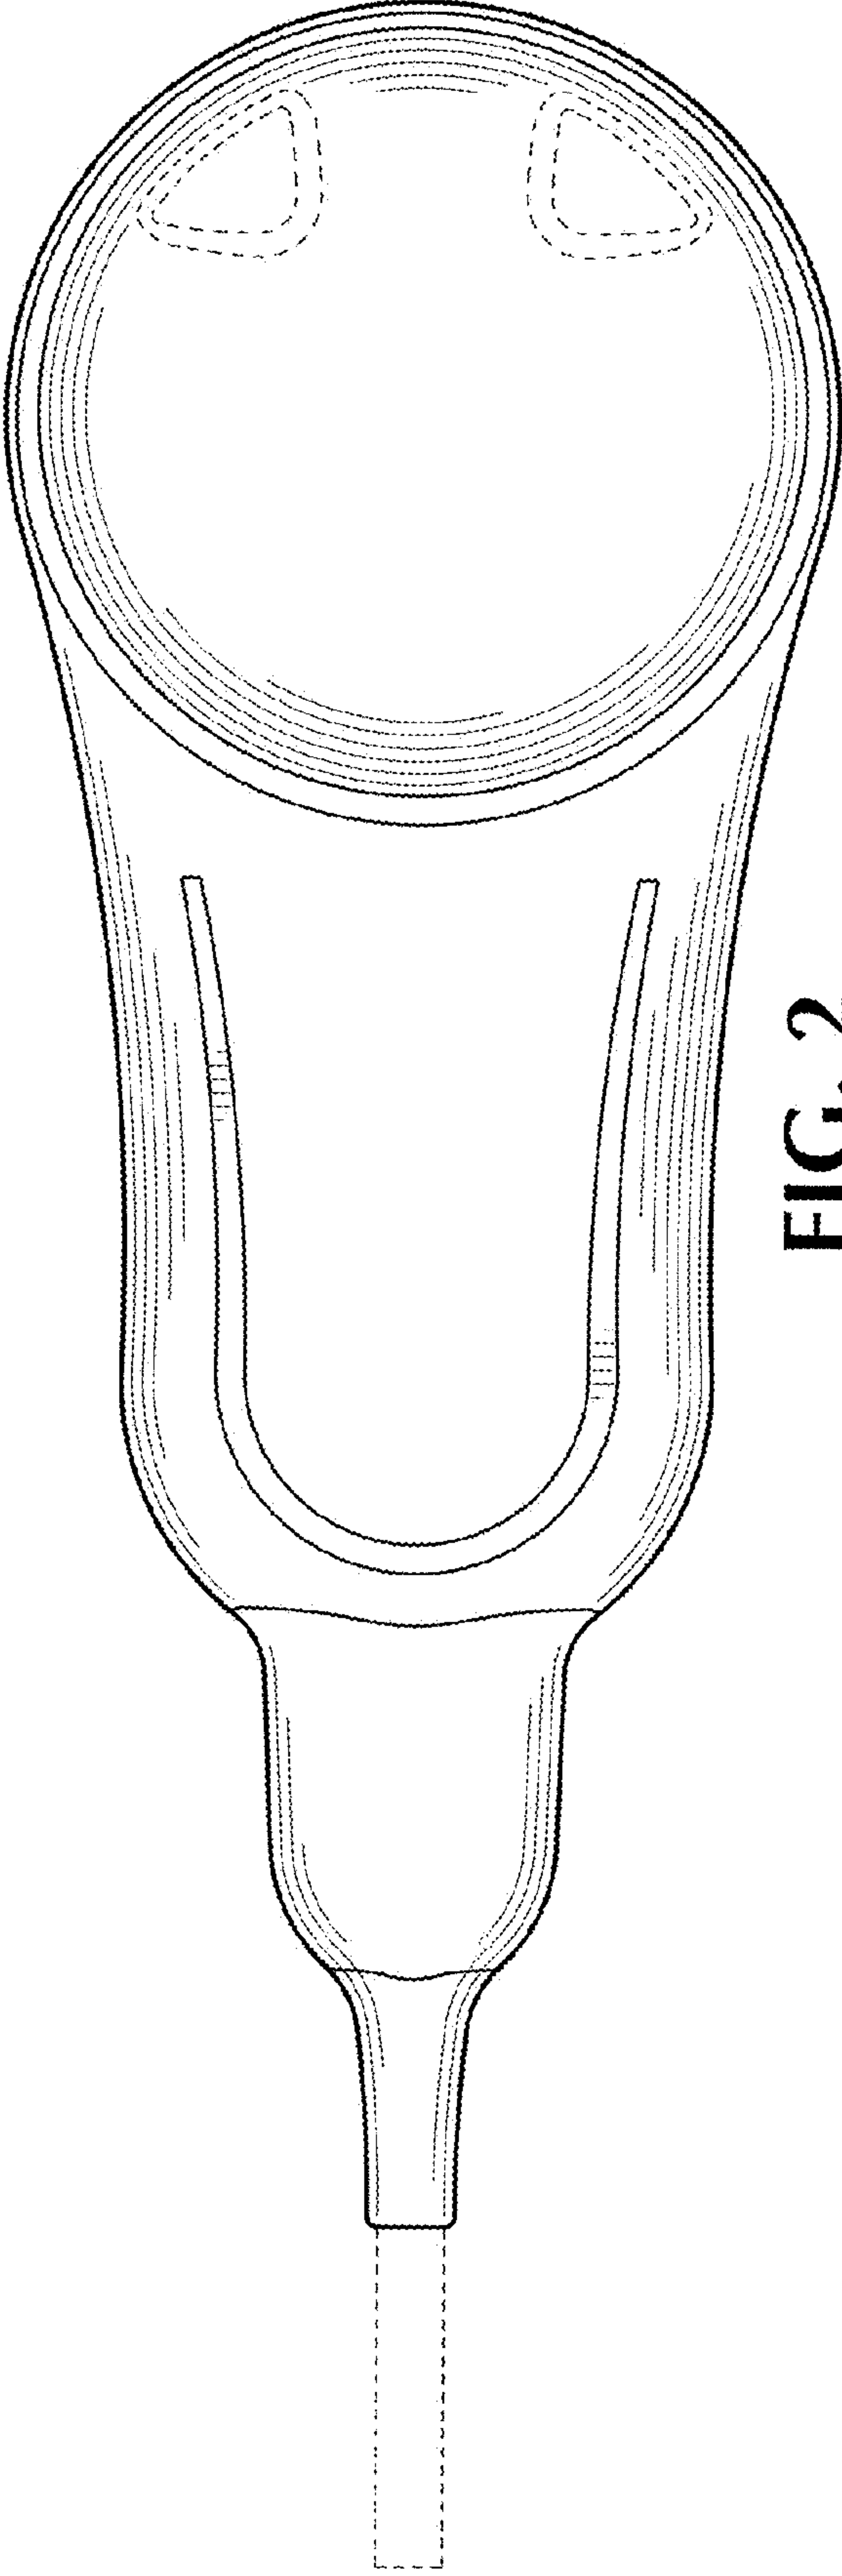


FIG. 2

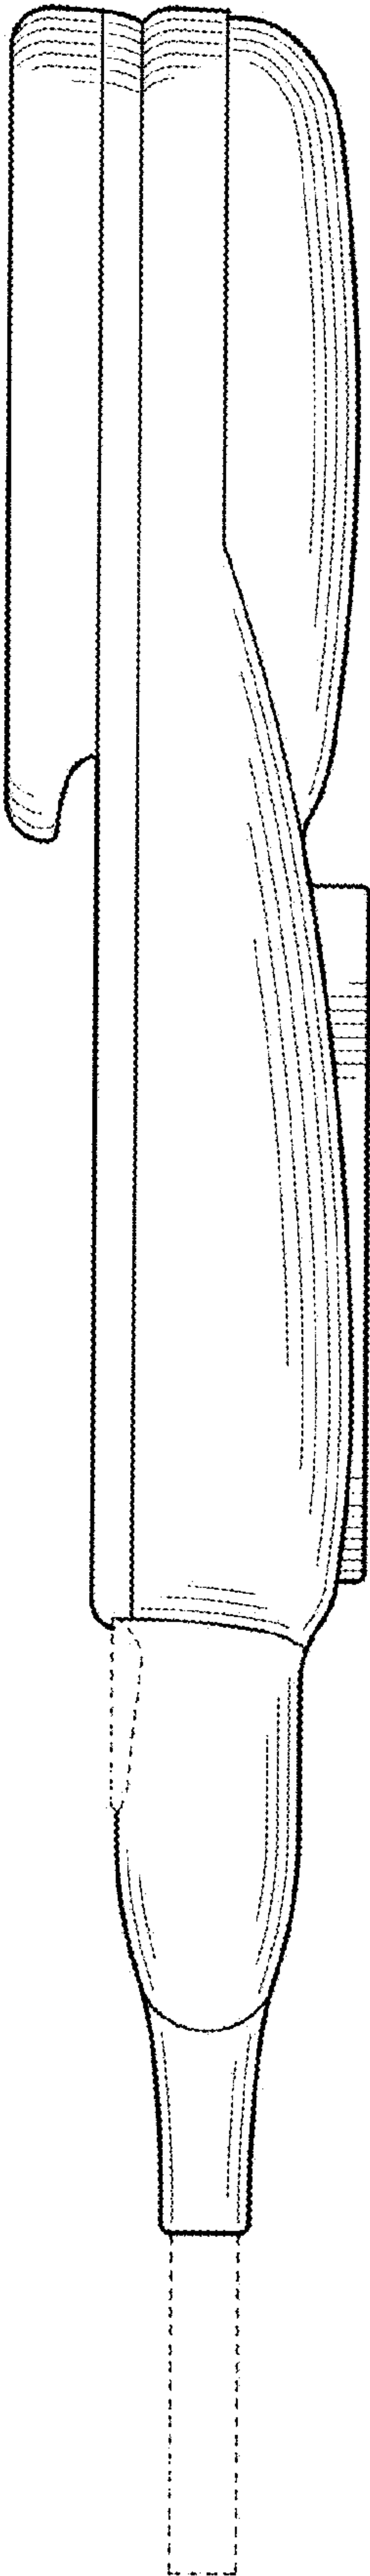


FIG. 3

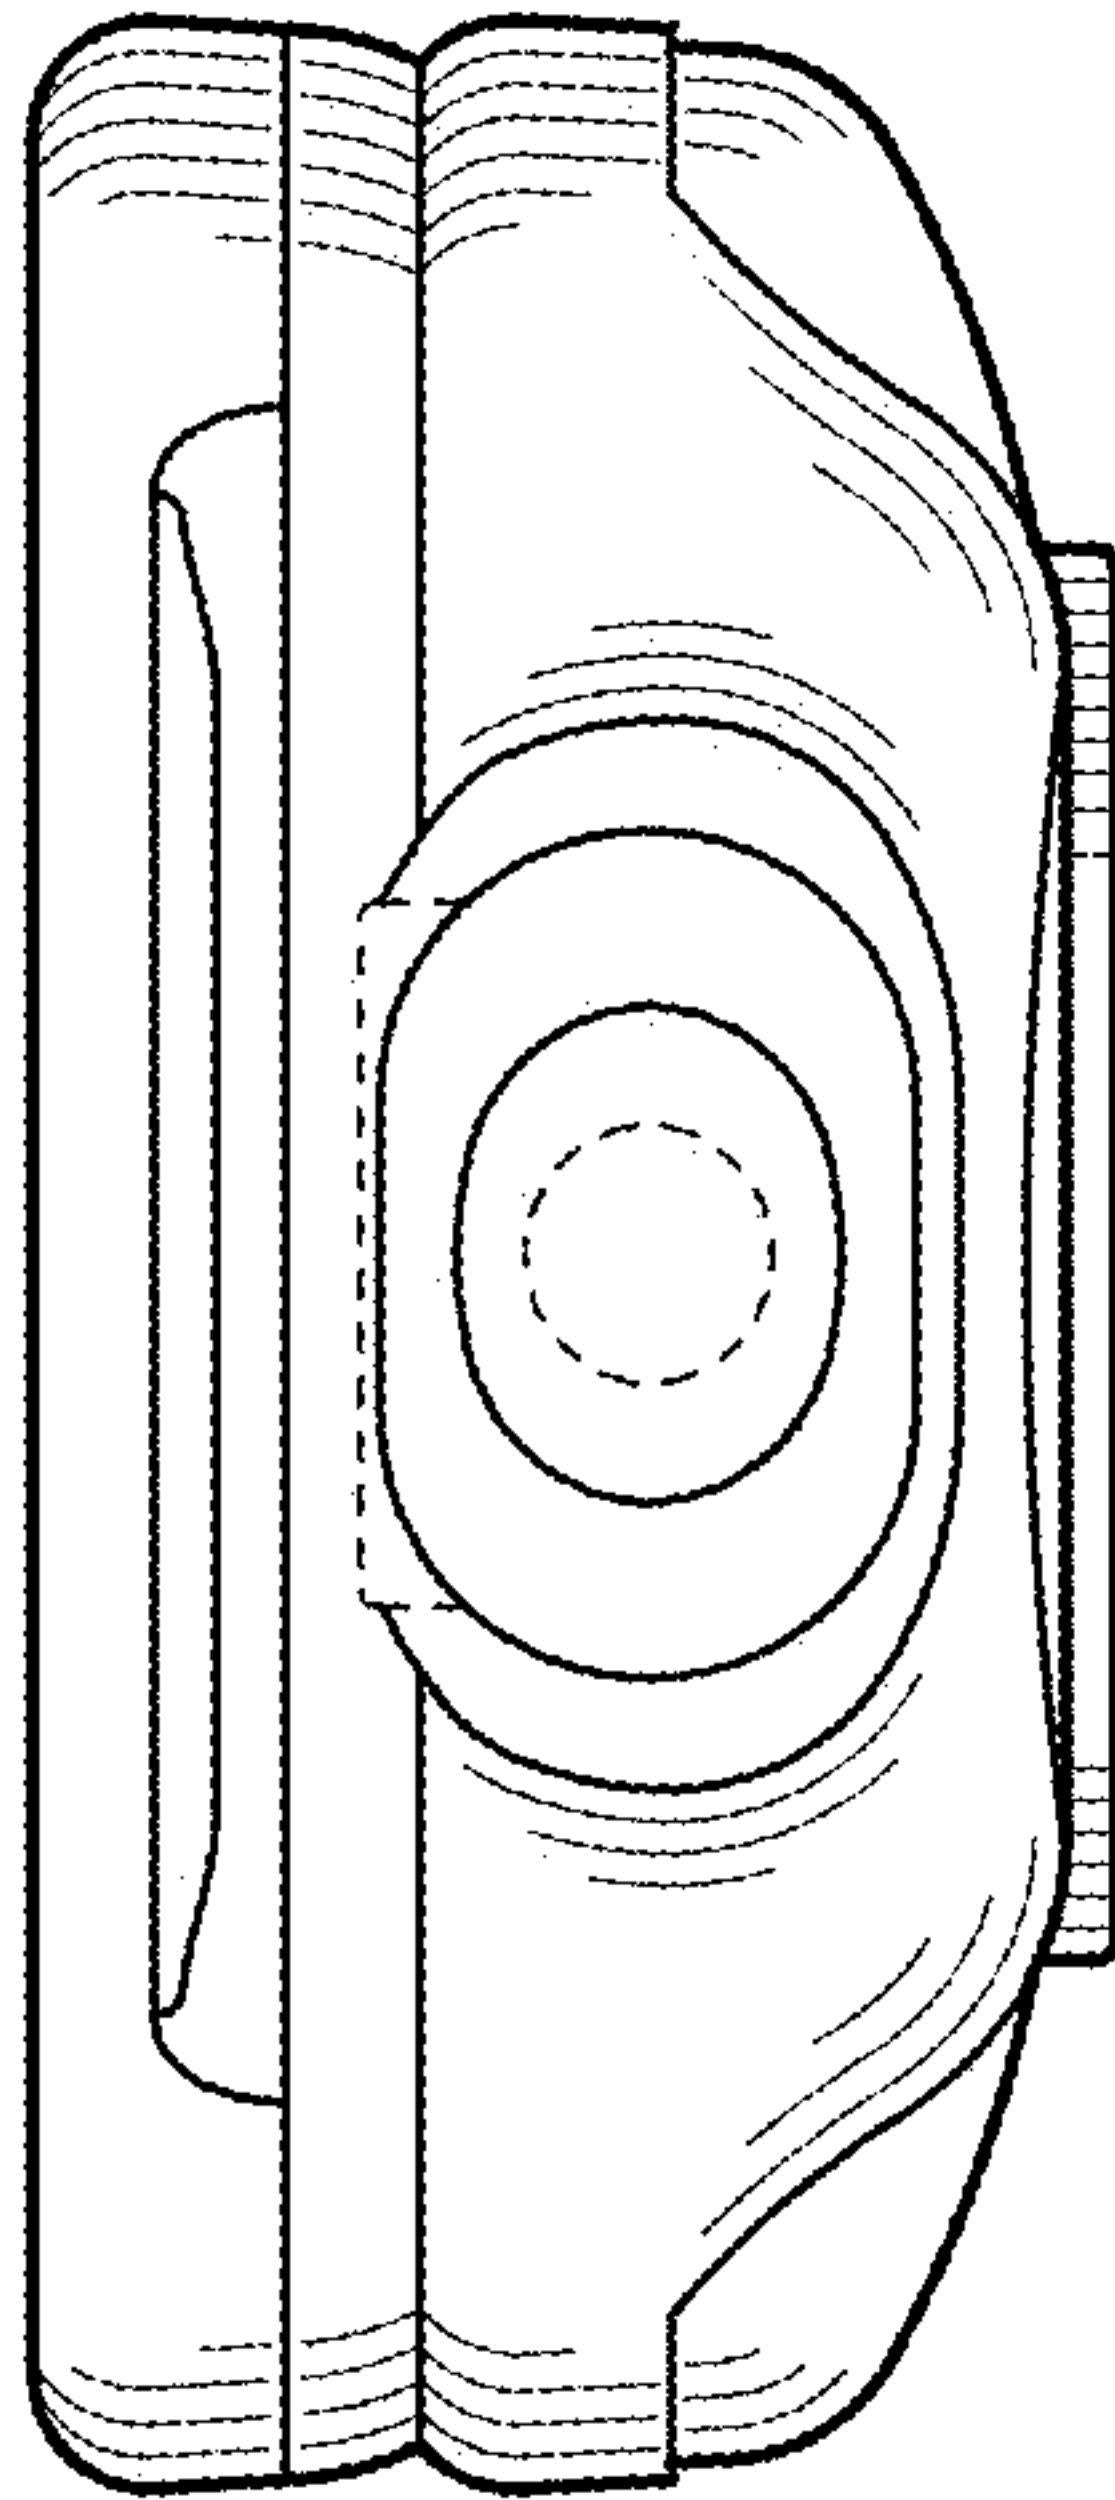


FIG. 5

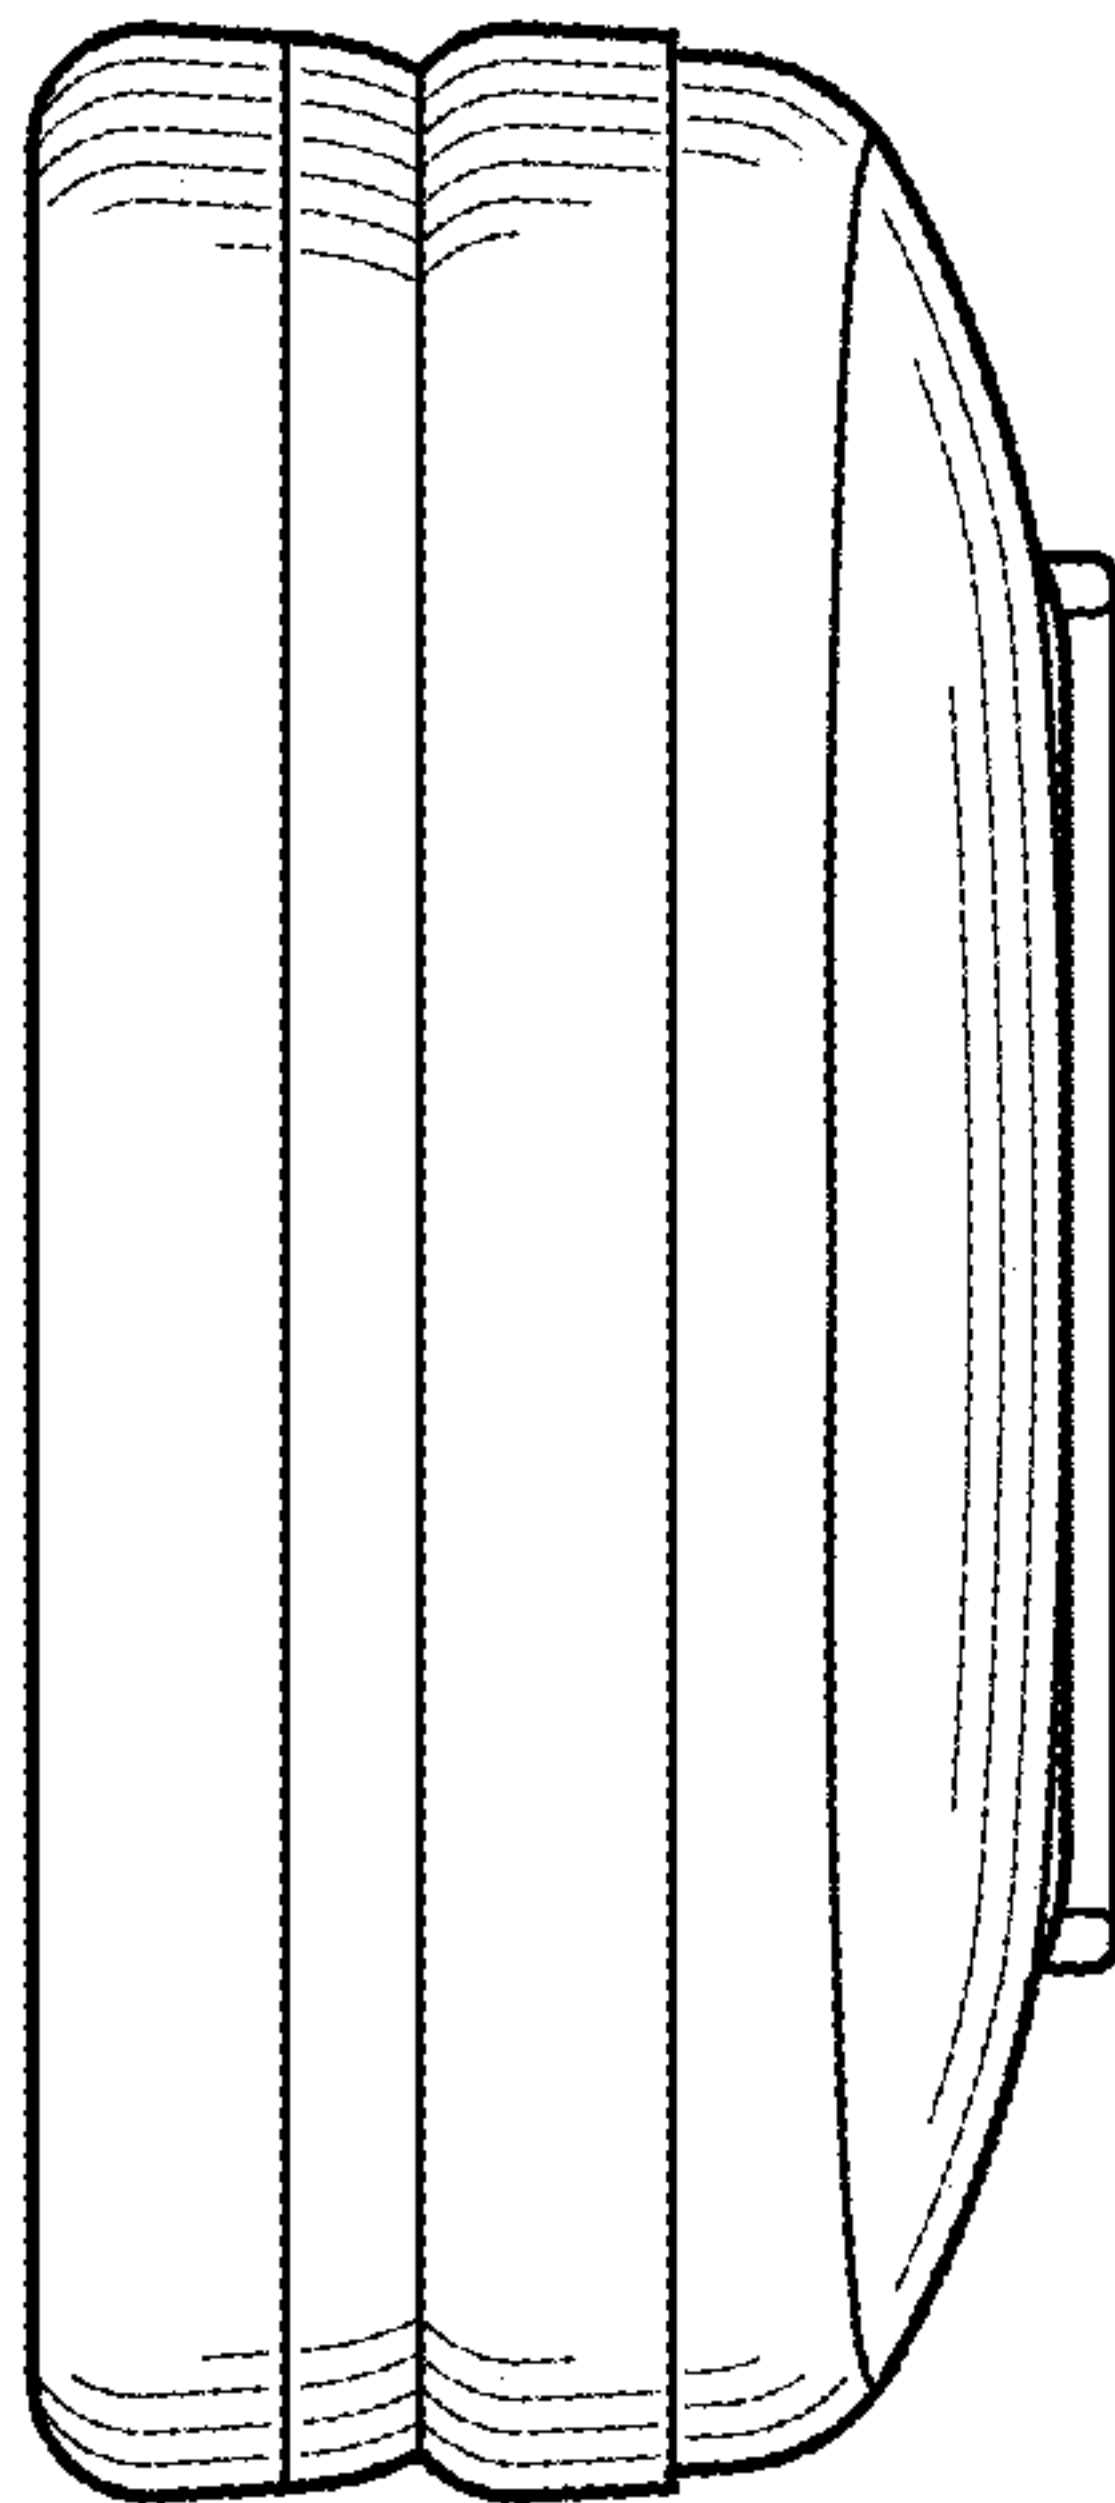


FIG. 4