



US00D764064S

(12) **United States Design Patent**
Vezina

(10) **Patent No.:** **US D764,064 S**
(45) **Date of Patent:** **** Aug. 16, 2016**

(54) **SECURING MECHANISM FOR A
PERIPHERAL ULTRASOUND DEVICE**

(71) Applicant: **Guardsman Scientific, Inc.**, Park City,
UT (US)

(72) Inventor: **Daniel P. Vezina**, Park City, UT (US)

(73) Assignee: **Guardsman Scientific, Inc.**, Park City,
UT (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/457,196**

(22) Filed: **Jun. 7, 2013**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**

USPC D24/127–128, 137–138, 184, 186–187,
D24/200, 215, 231; 600/437–461, 407;
601/2; D10/60, 80; D16/219, 250;
D8/354, 356; 396/530–532, 448, 828
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,017,878 A * 4/1977 Hagiwara 396/530
4,165,270 A 8/1979 Ost et al.
4,305,207 A 12/1981 Lantz
4,307,954 A * 12/1981 Ludwig 396/531
4,343,092 A 8/1982 Wahl et al.
4,659,203 A * 4/1987 Niwa et al. 396/531
4,766,453 A * 8/1988 Shiokama et al. 396/532
4,827,943 A 5/1989 Bornn et al.
4,857,836 A 8/1989 Söelkner
4,908,568 A 3/1990 Söelkner
4,920,966 A * 5/1990 Hon et al. 600/459
4,947,853 A 8/1990 Hon
5,022,410 A 6/1991 Hall et al.
5,070,880 A 12/1991 Gomez et al.
5,394,877 A 3/1995 Orr et al.

5,469,852 A 11/1995 Nakamura et al.
5,598,845 A 2/1997 Chandraratna et al.
5,634,468 A 6/1997 Platt et al.
5,704,352 A 1/1998 Tremblay et al.
5,740,804 A 4/1998 Cerofolini
5,771,896 A 6/1998 Sliwa, Jr. et al.
5,807,268 A 9/1998 Reeves et al.
5,947,961 A 9/1999 Netherly
6,031,383 A 2/2000 Streib et al.
6,124,723 A 9/2000 Costello
6,126,636 A 10/2000 Naka

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0607490 7/1994
JP 05337108 12/1993

OTHER PUBLICATIONS

U.S. Appl. No. 29/457,201, filed Jun. 7, 2013, Vezina.
(Continued)

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Polsinelli PC

(57)

CLAIM

The ornamental design for a securing mechanism for a
peripheral ultrasound device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a securing mechanism for
a peripheral ultrasound device showing my new design.


FIG. 2 is a bottom view thereof.

FIG. 3 is a top view thereof; and,

FIG. 4 is a side view thereof.

The broken lines in FIG. 4 are included for the purpose of
illustrating unclaimed portions of the securing mechanism for
a peripheral ultrasound device and form no part of the claimed
design.

1 Claim, 4 Drawing Sheets

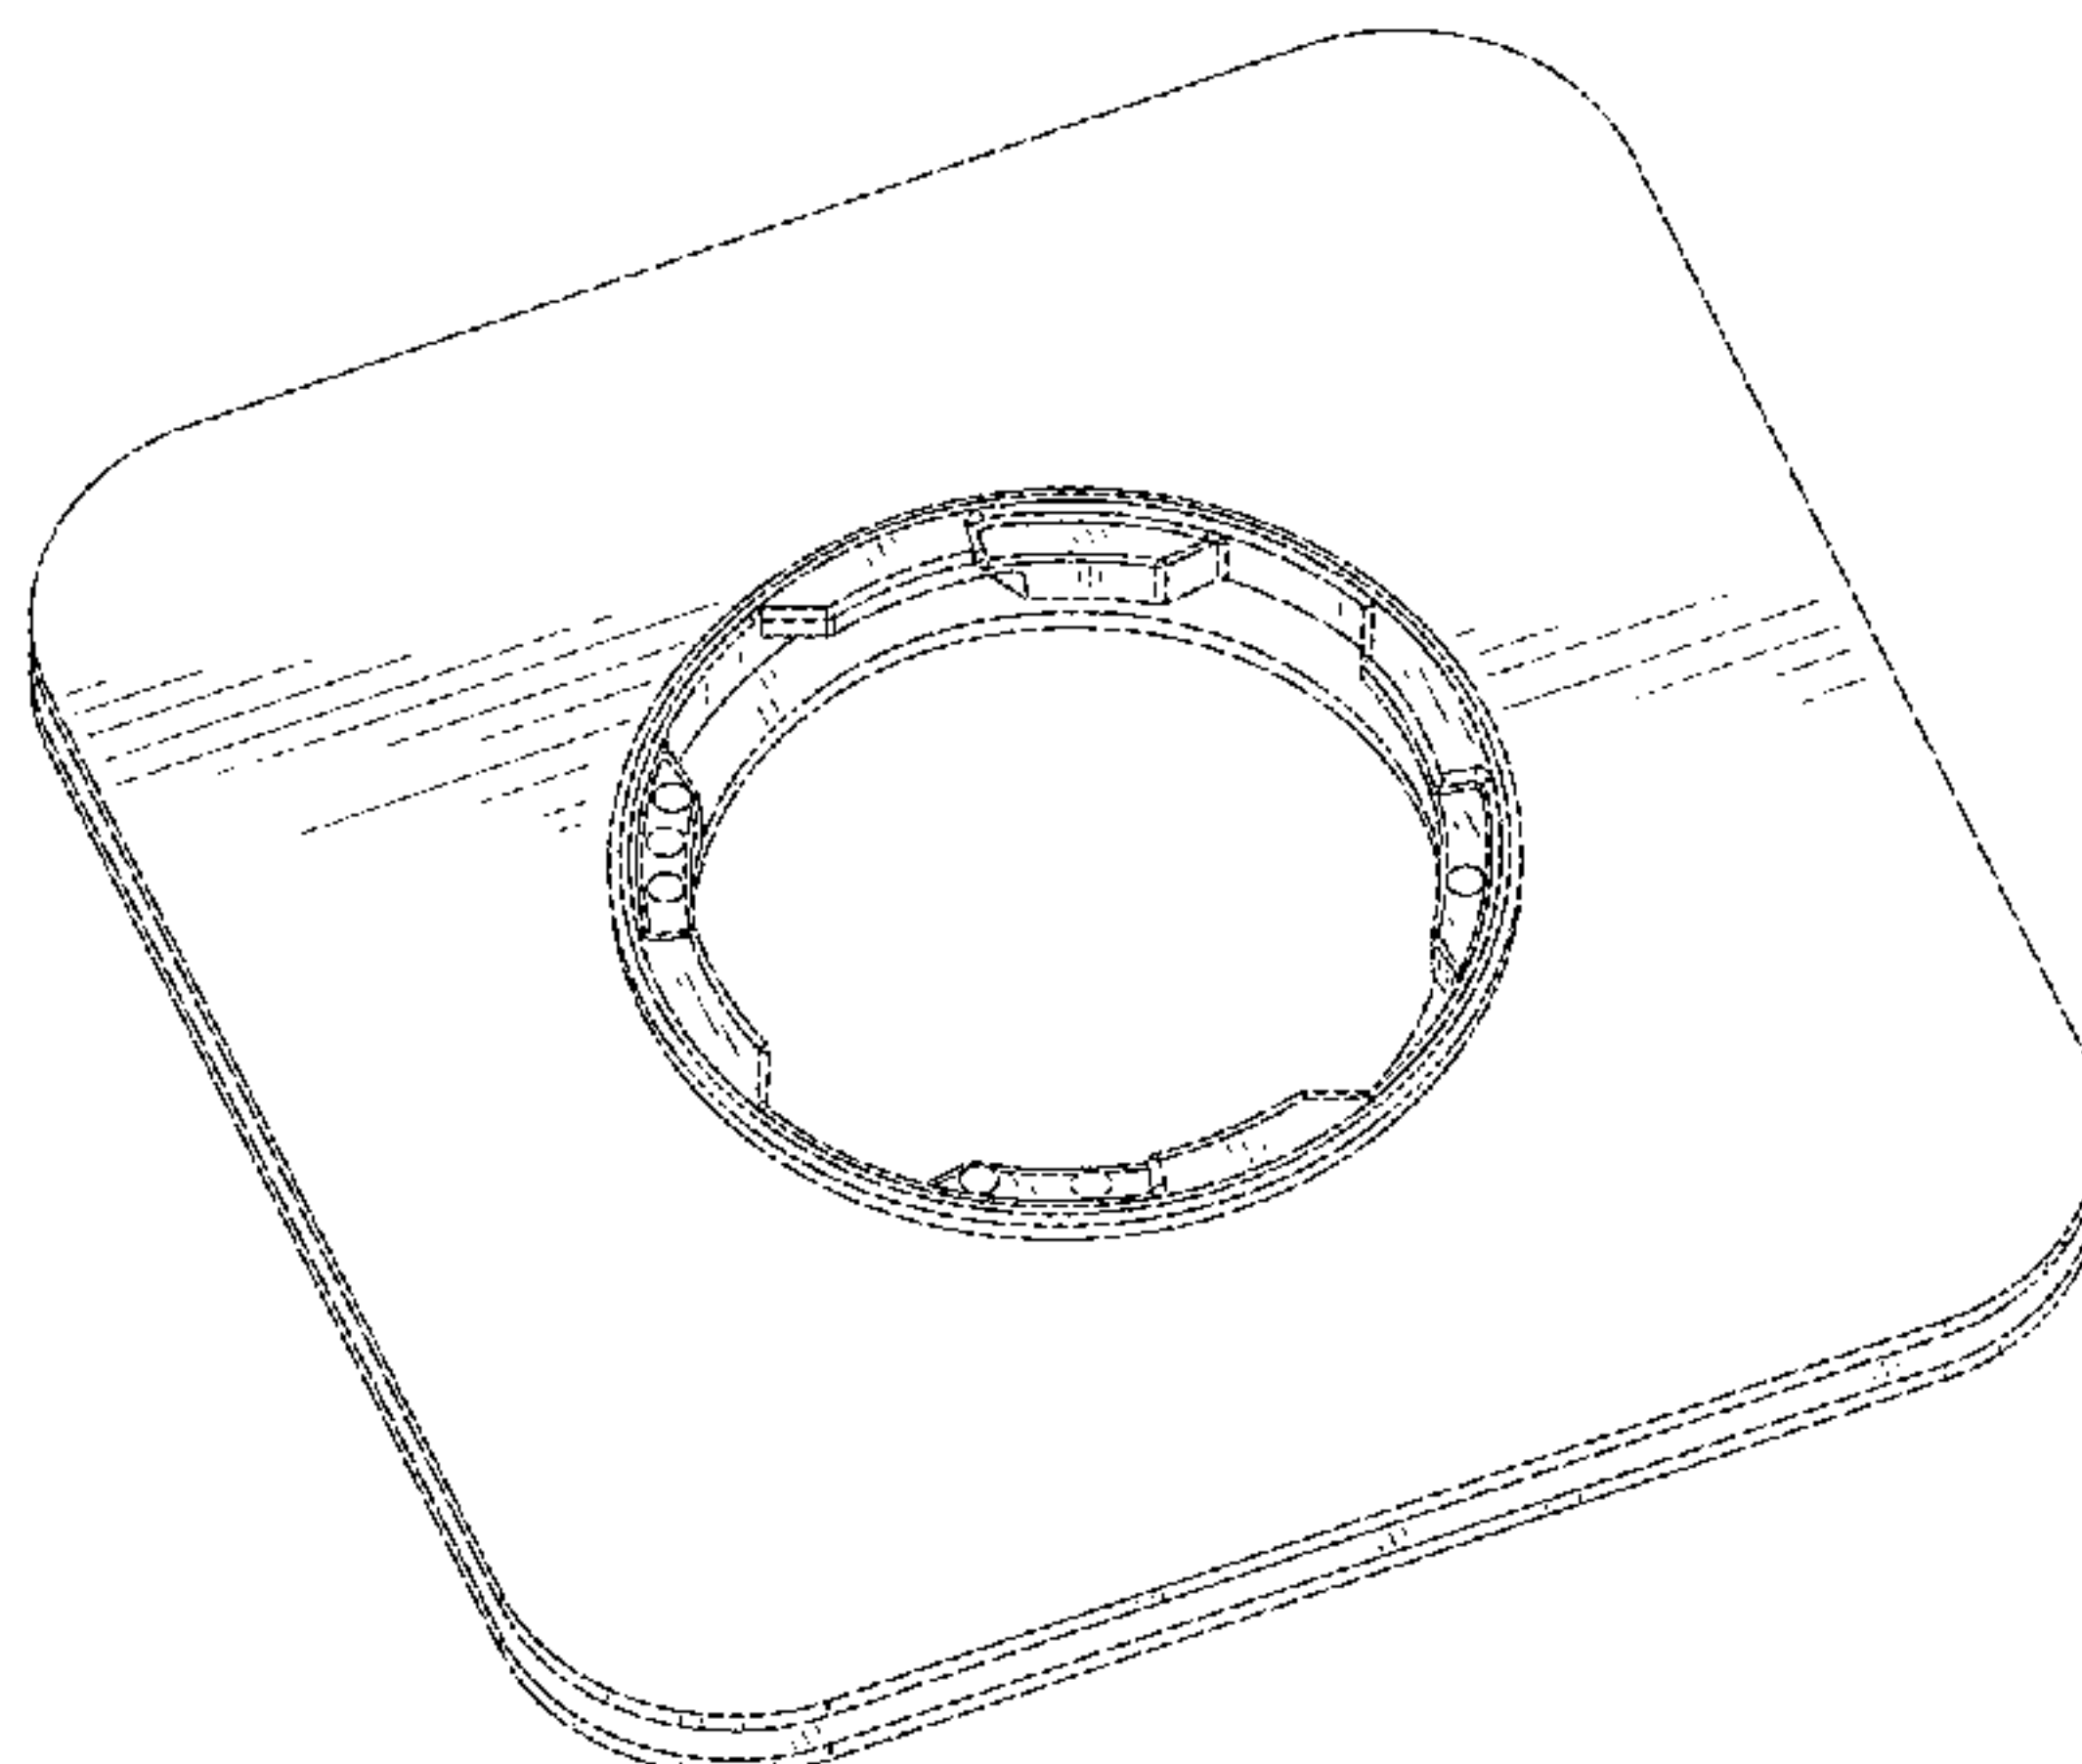

(56)

References Cited**U.S. PATENT DOCUMENTS**

6,132,371	A	10/2000	Dempsey et al.	
6,248,101	B1	6/2001	Whitmore, III et al.	
6,261,231	B1	7/2001	Damphousse et al.	
6,285,180	B1	9/2001	Pas	
6,577,893	B1	6/2003	Besson et al.	
6,653,825	B2	11/2003	Munniksma	
7,087,024	B1 *	8/2006	Pruter	600/461
7,215,991	B2	5/2007	Besson et al.	
7,244,230	B2	7/2007	Duggirala et al.	
D585,556	S *	1/2009	Kosaku	D24/186
7,600,930	B2 *	10/2009	Wang et al.	396/448
D603,520	S *	11/2009	Ninomiya et al.	D24/187
D629,527	S *	12/2010	Crunkilton	D24/187
8,348,847	B2	1/2013	Vezina	
D692,564	S *	10/2013	Ninomiya et al.	D24/187
8,573,868	B2 *	11/2013	Hasuda et al.	396/531
8,687,299	B1 *	4/2014	Sanford et al.	359/828
D712,043	S *	8/2014	Sliger	D24/186
2001/0053289	A1 *	12/2001	Imanari et al.	396/531
2002/0120310	A1	8/2002	Linden et al.	
2003/0187362	A1	10/2003	Murphy et al.	
2003/0220578	A1	11/2003	Ho et al.	
2004/0006278	A1	1/2004	Webb et al.	
2004/0015081	A1	1/2004	Kramer et al.	
2005/0157888	A1	7/2005	Yang	
2005/0232434	A1	10/2005	Andersen	
2005/0288584	A1	12/2005	McMorrow et al.	
2006/0030782	A1	2/2006	Shennib	
2006/0241464	A1	10/2006	Ohtake et al.	
2006/0264767	A1	11/2006	Shennib	
2007/0106751	A1	5/2007	Moore	
2007/0260285	A1	11/2007	Libbus et al.	
2007/0261493	A1	11/2007	Kim	
2007/0276251	A1	11/2007	Orenstein et al.	
2007/0276270	A1	11/2007	Tran	
2008/0004904	A1	1/2008	Tran	
2008/0013747	A1	1/2008	Tran	
2010/0168577	A1	7/2010	Vezina	
2011/0270089	A1	11/2011	Vezina	
2013/0102899	A1	4/2013	Vezina	
2013/0102900	A1	4/2013	Vezina	

OTHER PUBLICATIONS

U.S. Appl. No. 29/457,200, filed Jun. 7, 2013, Vezina.

U.S. Appl. No. 13/912,763, filed Jun. 7, 2013, Vezina.

Anderson G. Chronic Conditions: Making the Case for Ongoing Care. Johns Hopkins University, Baltimore, MD. Nov. 2007, 77 pages.

Devereux et al. A population-based assessment of left ventricular systolic dysfunction in middle-aged and older adults; the Strong Heart Study. Am Heart J. 2001 Mar. 2001 141(3): 439-46.

Devereux et al. Congestive heart failure despite normal ventricular systolic function in a population-based sample: the Strong Heart Study. Am. J. Cardiol. Nov. 15, 2000; 86 (10): 1090-6.

Eagle et al. ACC/AHA Guideline Update for Perioperative Cardiovascular Evaluation for Noncardiac Surgery-Executive Summary. A report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines (Committee to Update the 1996 Guidelines on Perioperative Cardiovascular Evaluation for Noncardiac Summary) Anesth. Analg. May 4-5, 2002) 1052-64.

Garrett et al. The boomers are coming; a total cost of care model of the impact of population aging on the cost of chronic conditions in the United States. Dis Manag. Apr. 2007; 10(2): 51-60.

Hammill et al. Impact of heart failure on patients undergoing major noncardiac surgery. Anesthesiology, 2008; 108:559-567.

International Search Report and Written Opinion, PCT/US2009/052850, Sep. 29, 2009, 11 pages.

International Search Report and Written Opinion, PCT/US2009/069474, 10 pages, Feb. 25, 2010.

Jencks et al. Rehospitalizations among patients in the Medicare fee-for-service program. N. Engl J Med 2009;360:1418-28.

Maurer et al. Ventricular structure and function in hypertensive participants with heart failure and a normal ejection fraction; the Cardiovascular Health Study. J. Am. Col. Cardiol. Mar. 6, 2007; 49(9): 982-85.

Non-Final Office Action, U.S. Appl. No. 12/536,247, mailed Feb. 16, 2012, 24 pages.

Notice of Allowance, U.S. Appl. No. 12/536,247, mailed Sep. 18, 2012, 8 pages.

Owings et al. Ambulatory and Inpatient procedures in the United States, 1996. National Center for Health Statistics. Vital Health Stat 13(139), 1998.

Pelletier et al. Increasing US Emergency Department Visit Rates and Subsequent Hospital Admissions for Atrial Fibrillation from 1993 to 2004. Ann. Emerg Med. Jan. 2008;51(1):58-65.

Polanczyk et al. Right heart catheterization and the cardiac complications in patients undergoing noncardiac surgery: An observational study. JAMA 2001; 286: 309-314.

Practice Guidelines for Transesophageal Echocardiography. A report by the American Society of Anesthesiologists and the Society of Cardiovascular Anesthesiologists Task Force on Transesophageal Echocardiography. Anesthesiology. 1996: 986-1006.

Redfield et al. Burden of systolic and diastolic ventricular dysfunction in the community: appreciating the scope of the heart failure epidemic, JAMA, 2003; 289: 194-202.

Response to Non-Final Office Action, U.S. Appl. No. 12/536,247, filed Jun. 15, 2012, 12 pages.

Sandham et al. A randomized, controlled trial of the use of pulmonary-artery catheters in high-risk surgical patients. N Engl J. Med, vol. 348, No. 1, Jan. 2, 2003.

Standards for Basic Anesthetic Monitoring (Approved by the ASA House of Delegates on Oct. 21, 1986, and last amended on Oct. 25, 2005). <http://www.asahg.org/publicationsAndServices/standards/02.pdf> last accessed Mar. 12, 2008.

U.S. Census Bureau. U.S. Interim Projections by Age, Sex, Race, and Hispanic Origin. <http://www.census.gov/proj/www/usinterimproj/> Mar. 18, 2004. Last accessed Mar. 12, 2008.

* cited by examiner

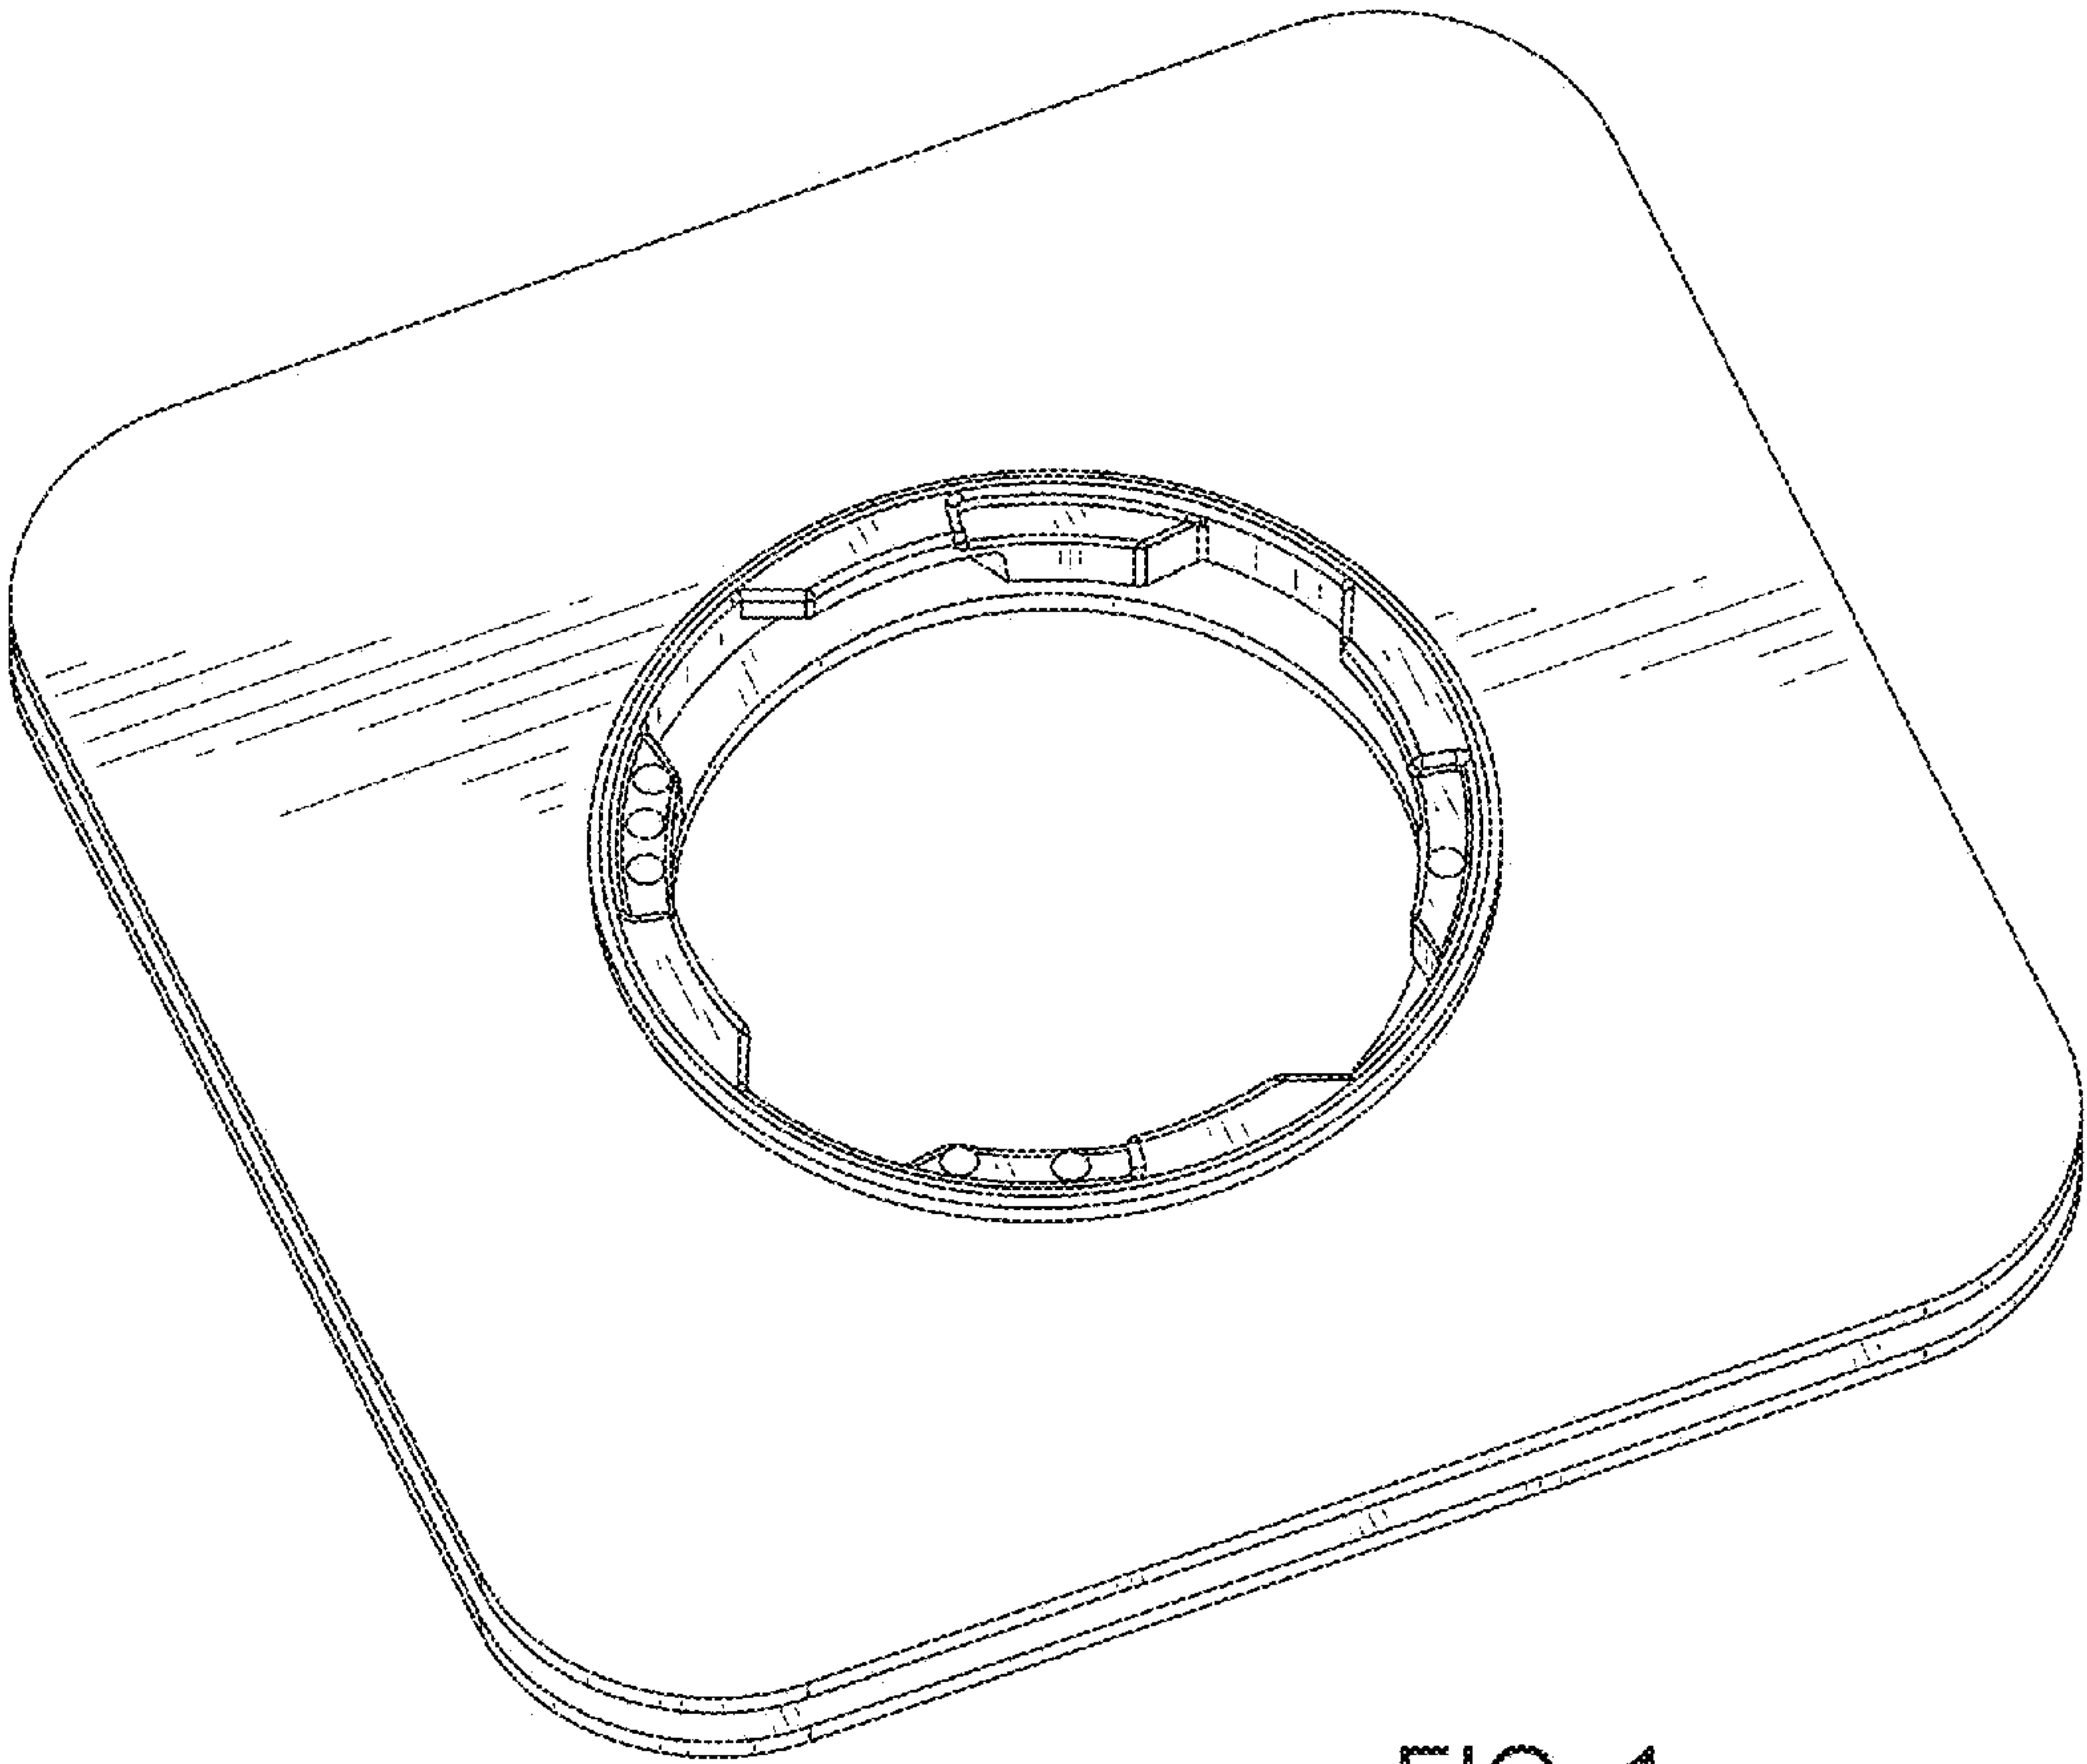


FIG. 1

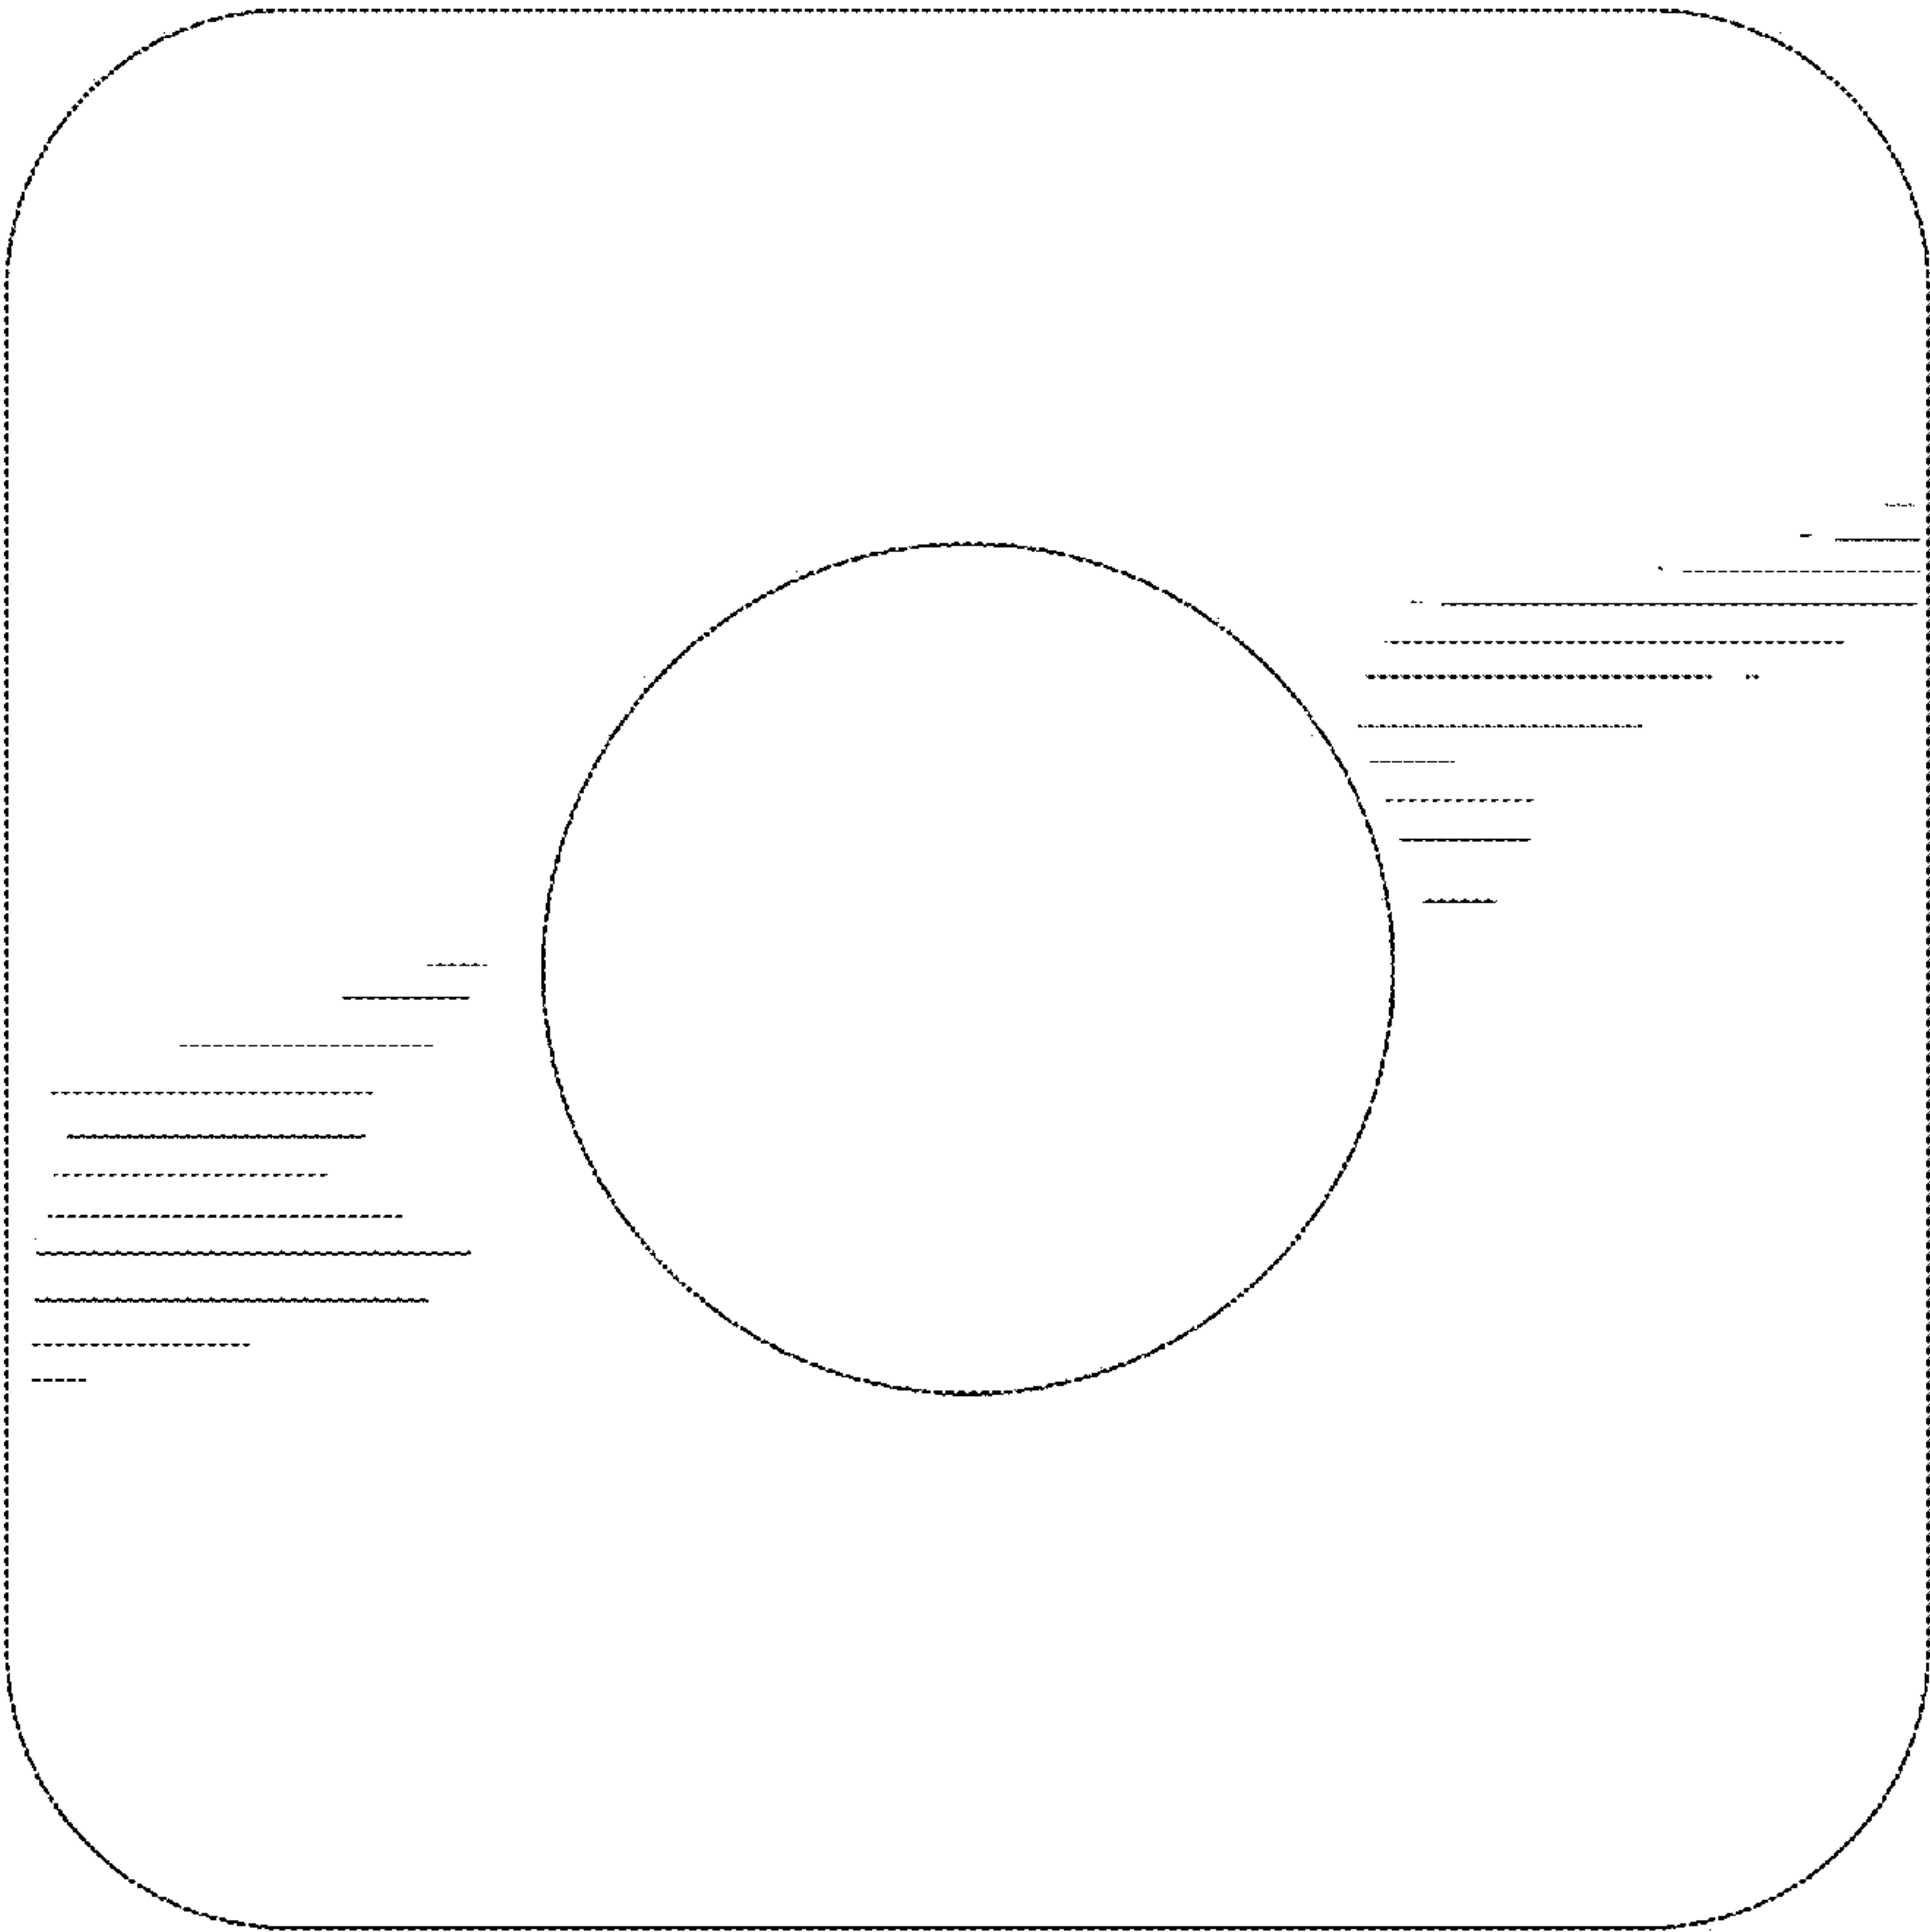


FIG. 2

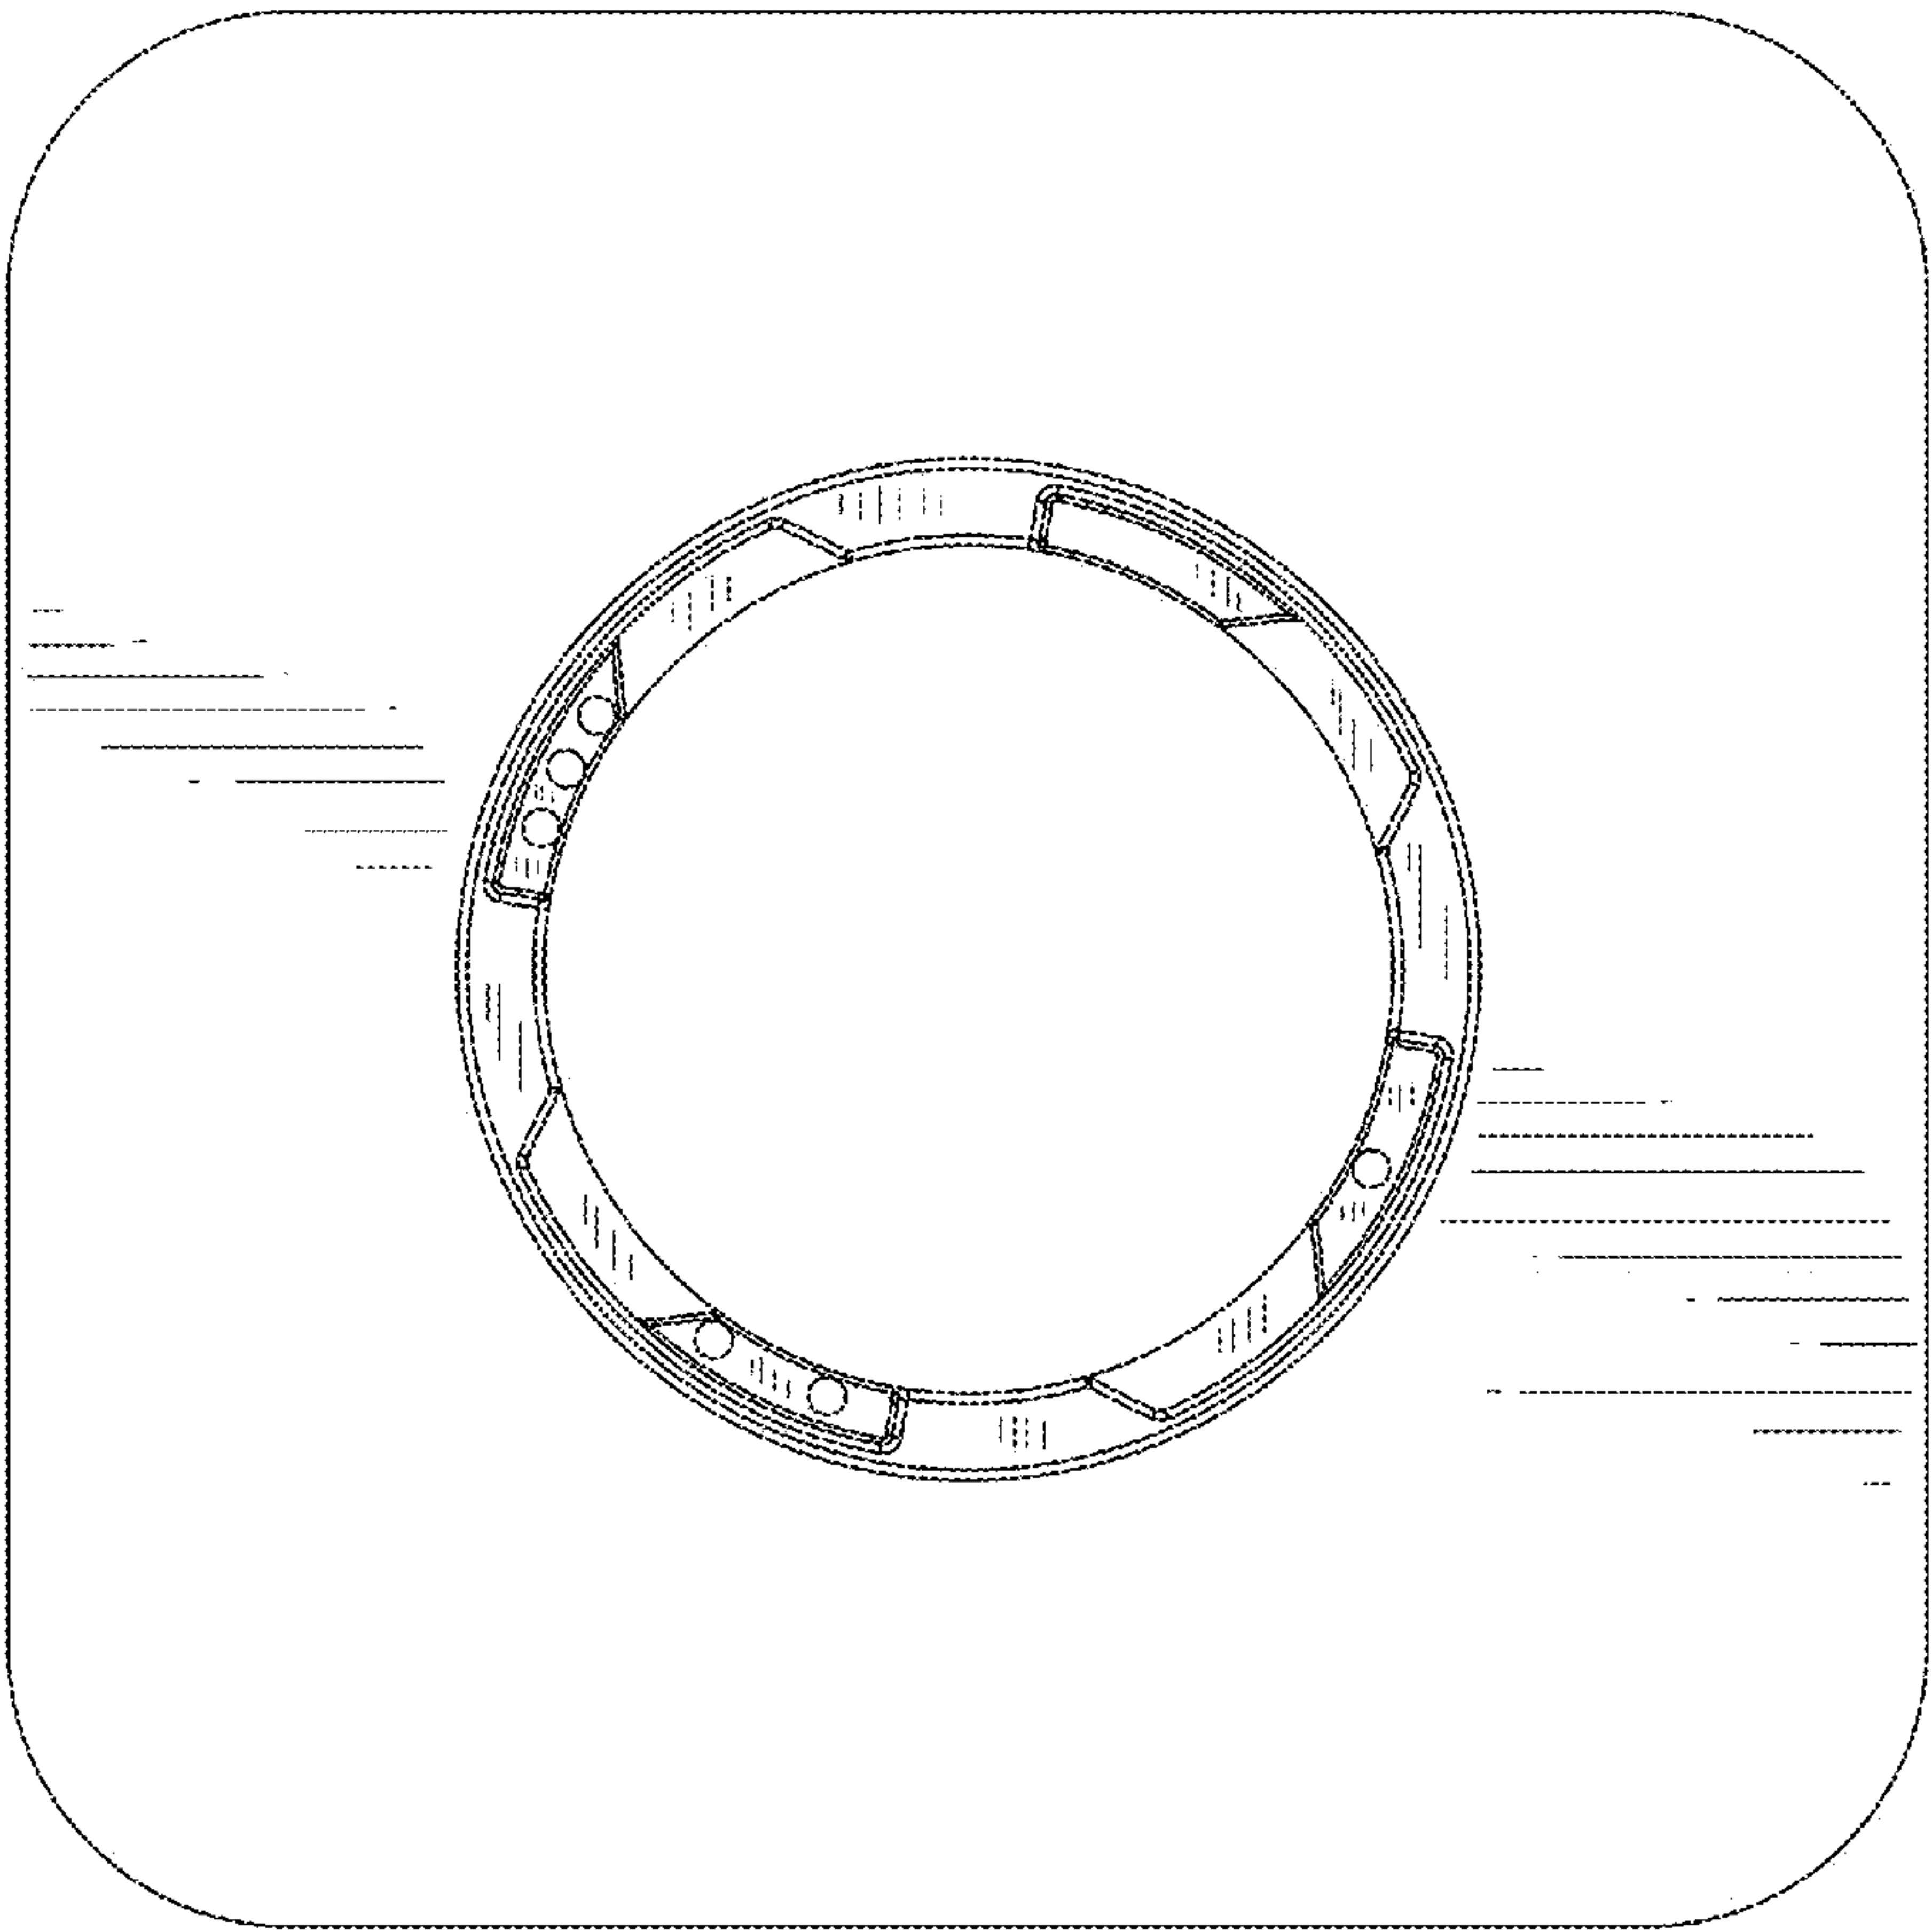


FIG. 3

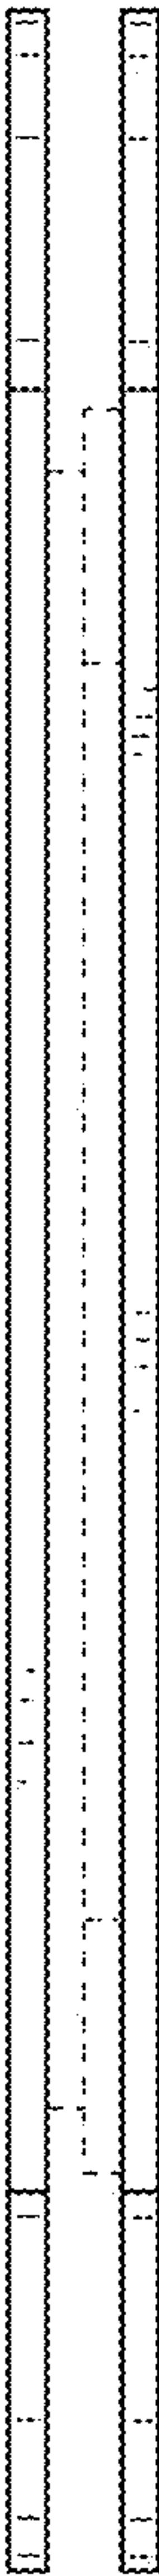


FIG. 4