

US00D765852S

(12) **United States Design Patent**
Early et al.

(10) **Patent No.:** **US D765,852 S**
(45) **Date of Patent:** **** Sep. 6, 2016**

(54) **ANTEROLATERAL TIBIA FRACTURE PLATE**

(71) Applicant: **OsteoMed LLC**, Addison, TX (US)

(72) Inventors: **John Early**, Dallas, TX (US); **Michael E. Brage**, Laguna Woods, CA (US); **Gregory Pomeroy**, Cape Elizabeth, ME (US); **Brian Carpenter**, Ft. Worth, TX (US); **Douglas W. Miller**, Dallas, TX (US); **Joel Bales**, Carrollton, TX (US)

(73) Assignee: **OsteoMed LLC**, Addison, TX (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/518,084**

(22) Filed: **Feb. 19, 2015**

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/155**

(58) **Field of Classification Search**
USPC D24/155-157
CPC A61B 17/8061; A61B 17/7059; A61B 17/8052; A61B 17/8605; A61B 17/8085; A61B 17/809; A61B 17/8014; A61B 17/8033; A61B 17/8004; A61B 17/888; A61B 17/842; A61B 17/8023; A61B 17/8009; A61B 17/86; A61B 17/1739; A61B 17/8066; A61B 17/1671; A61B 17/1757; A61B 17/8071; A61B 17/176; A61B 2017/1782; A61B 2017/1775
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D443,060 S * 5/2001 Benirschke D24/155
D458,684 S * 6/2002 Bryant D24/155

D463,559 S * 9/2002 Bryant D24/155
D469,533 S * 1/2003 Bryant D24/155
D469,874 S * 2/2003 Bryant D24/155
D469,875 S * 2/2003 Bryant D24/155
D480,141 S * 9/2003 Benirschke D24/155
7,655,029 B2 * 2/2010 Niederberger A61B 17/8057
606/280
D622,853 S * 8/2010 Raven, III D24/155
7,846,189 B2 * 12/2010 Winqvist A61B 17/8085
606/280
D630,750 S * 1/2011 Graham D24/155
8,460,344 B2 * 6/2013 Niederberger A61B 17/8057
606/280
8,740,905 B2 * 6/2014 Price A61B 17/1728
606/71

* cited by examiner

Primary Examiner — Charles Hanson

(74) *Attorney, Agent, or Firm* — Norton Rose Fulbright US LLP


(57) **CLAIM**

The ornamental design for an anterolateral tibia fracture plate, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the anterolateral tibia fracture plate;
FIG. 2 is a front view thereof;
FIG. 3 is a back view thereof;
FIG. 4 is a perspective view thereof;
FIG. 5 is a bottom view thereof;
FIG. 6 is a bottom view thereof;
FIG. 7 is a top view thereof;
FIG. 8 is a right side view thereof; and,
FIG. 9 is a left side view thereof.
The broken lines showing on the anterolateral tibia fracture plate are for the purpose of illustrating environmental structure and form no part of the claimed design.

1 Claim, 5 Drawing Sheets

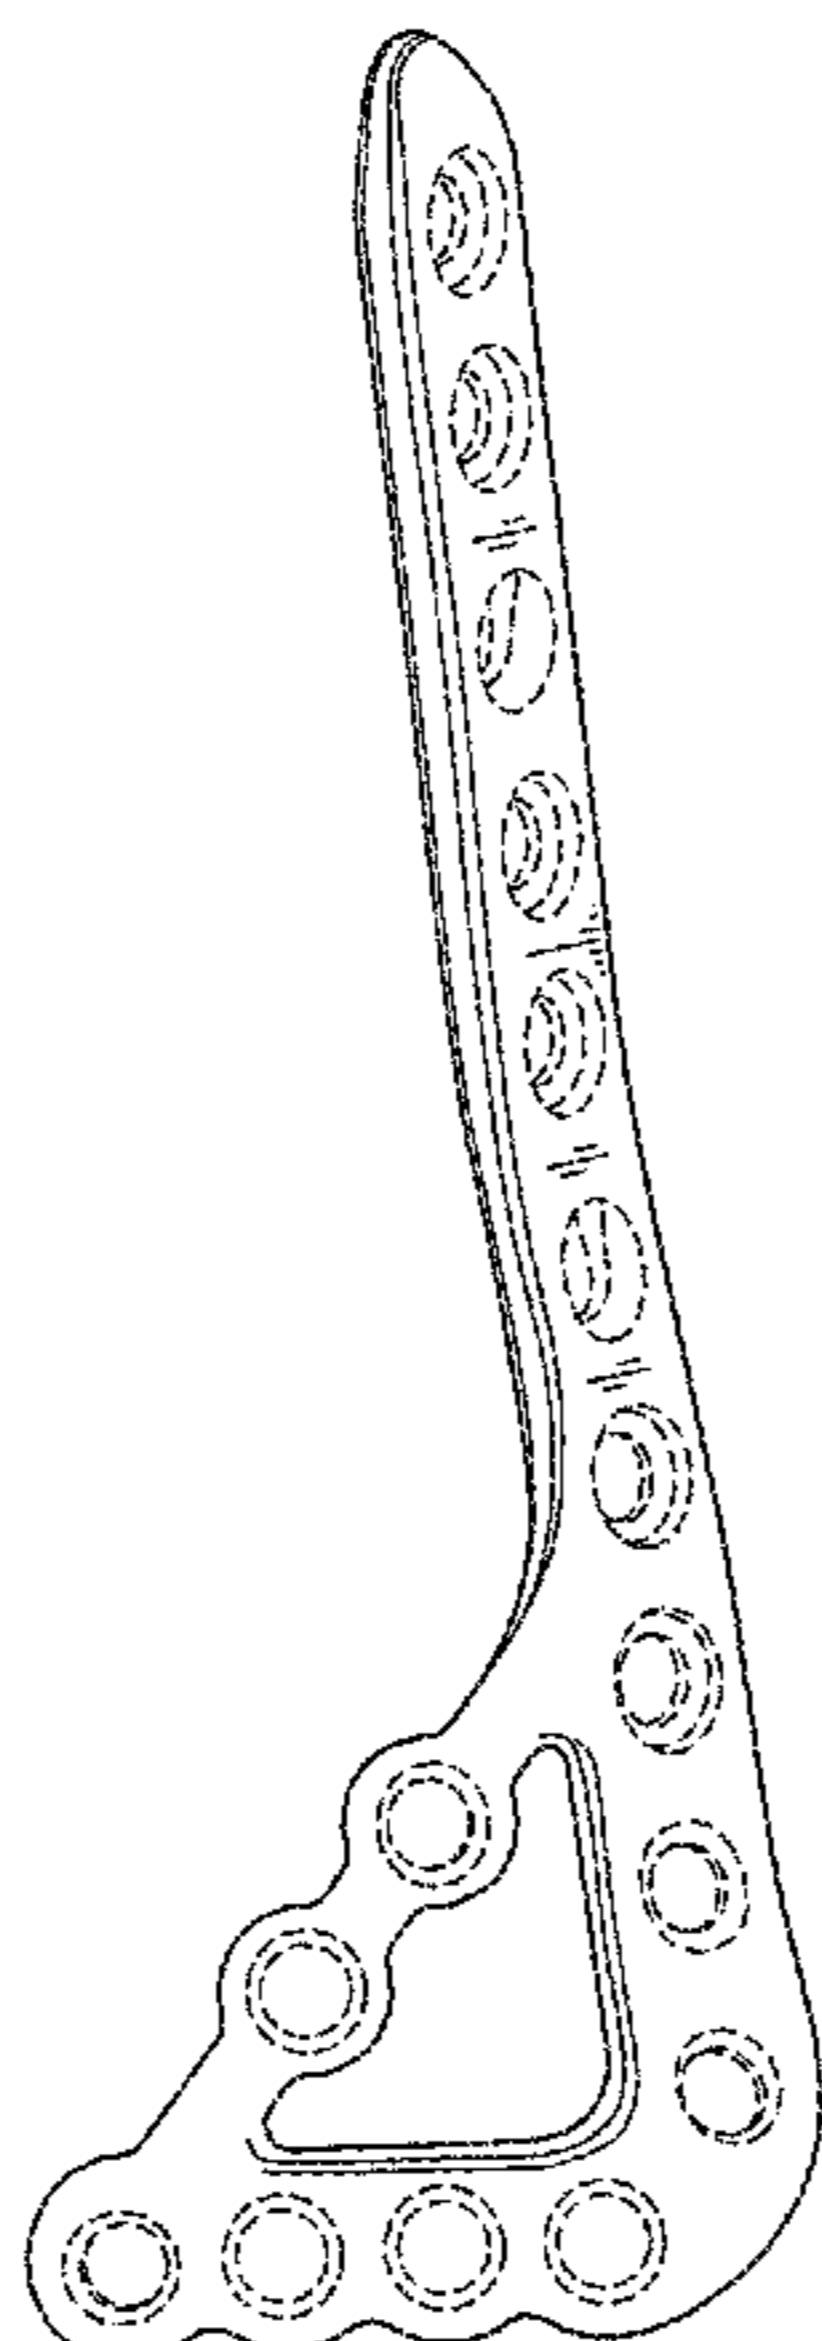

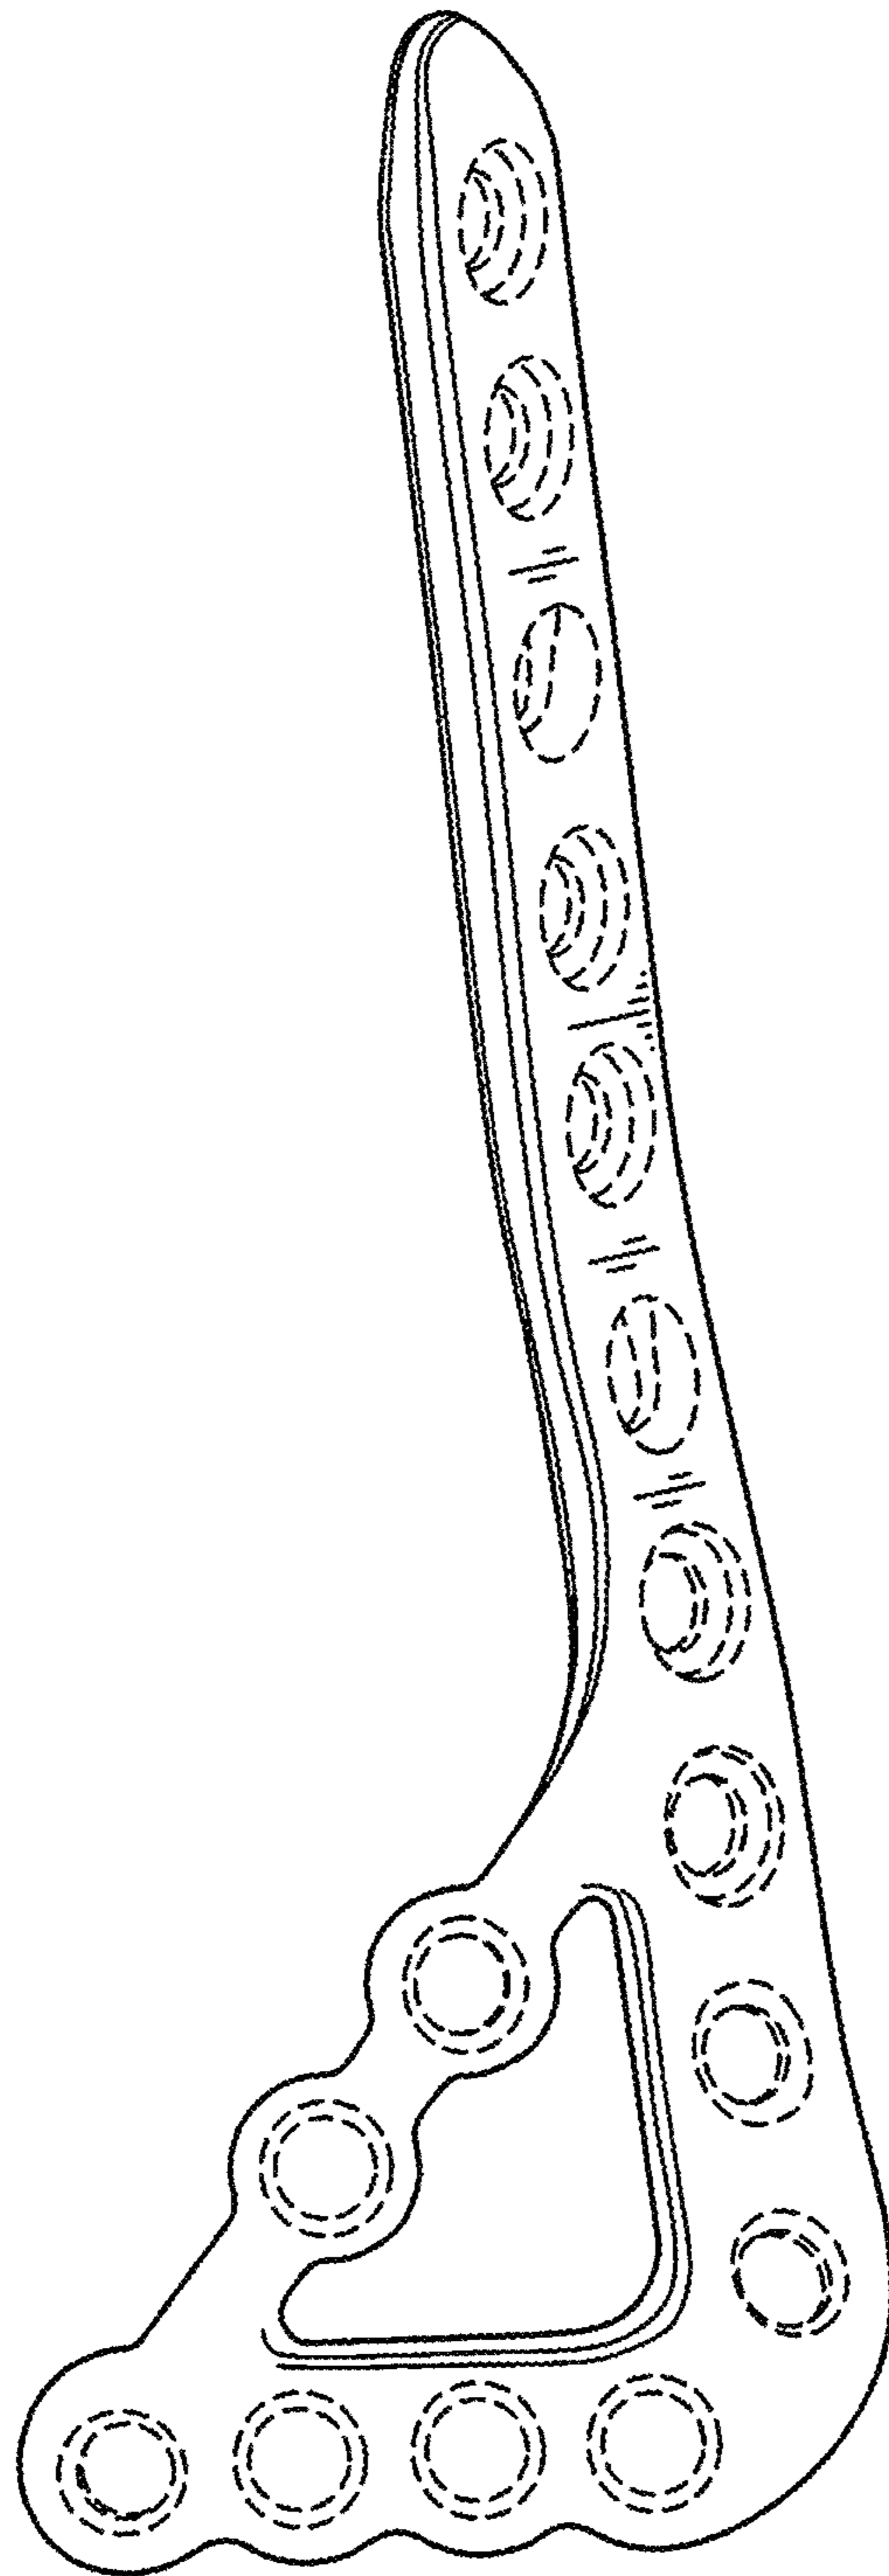


FIG. 1

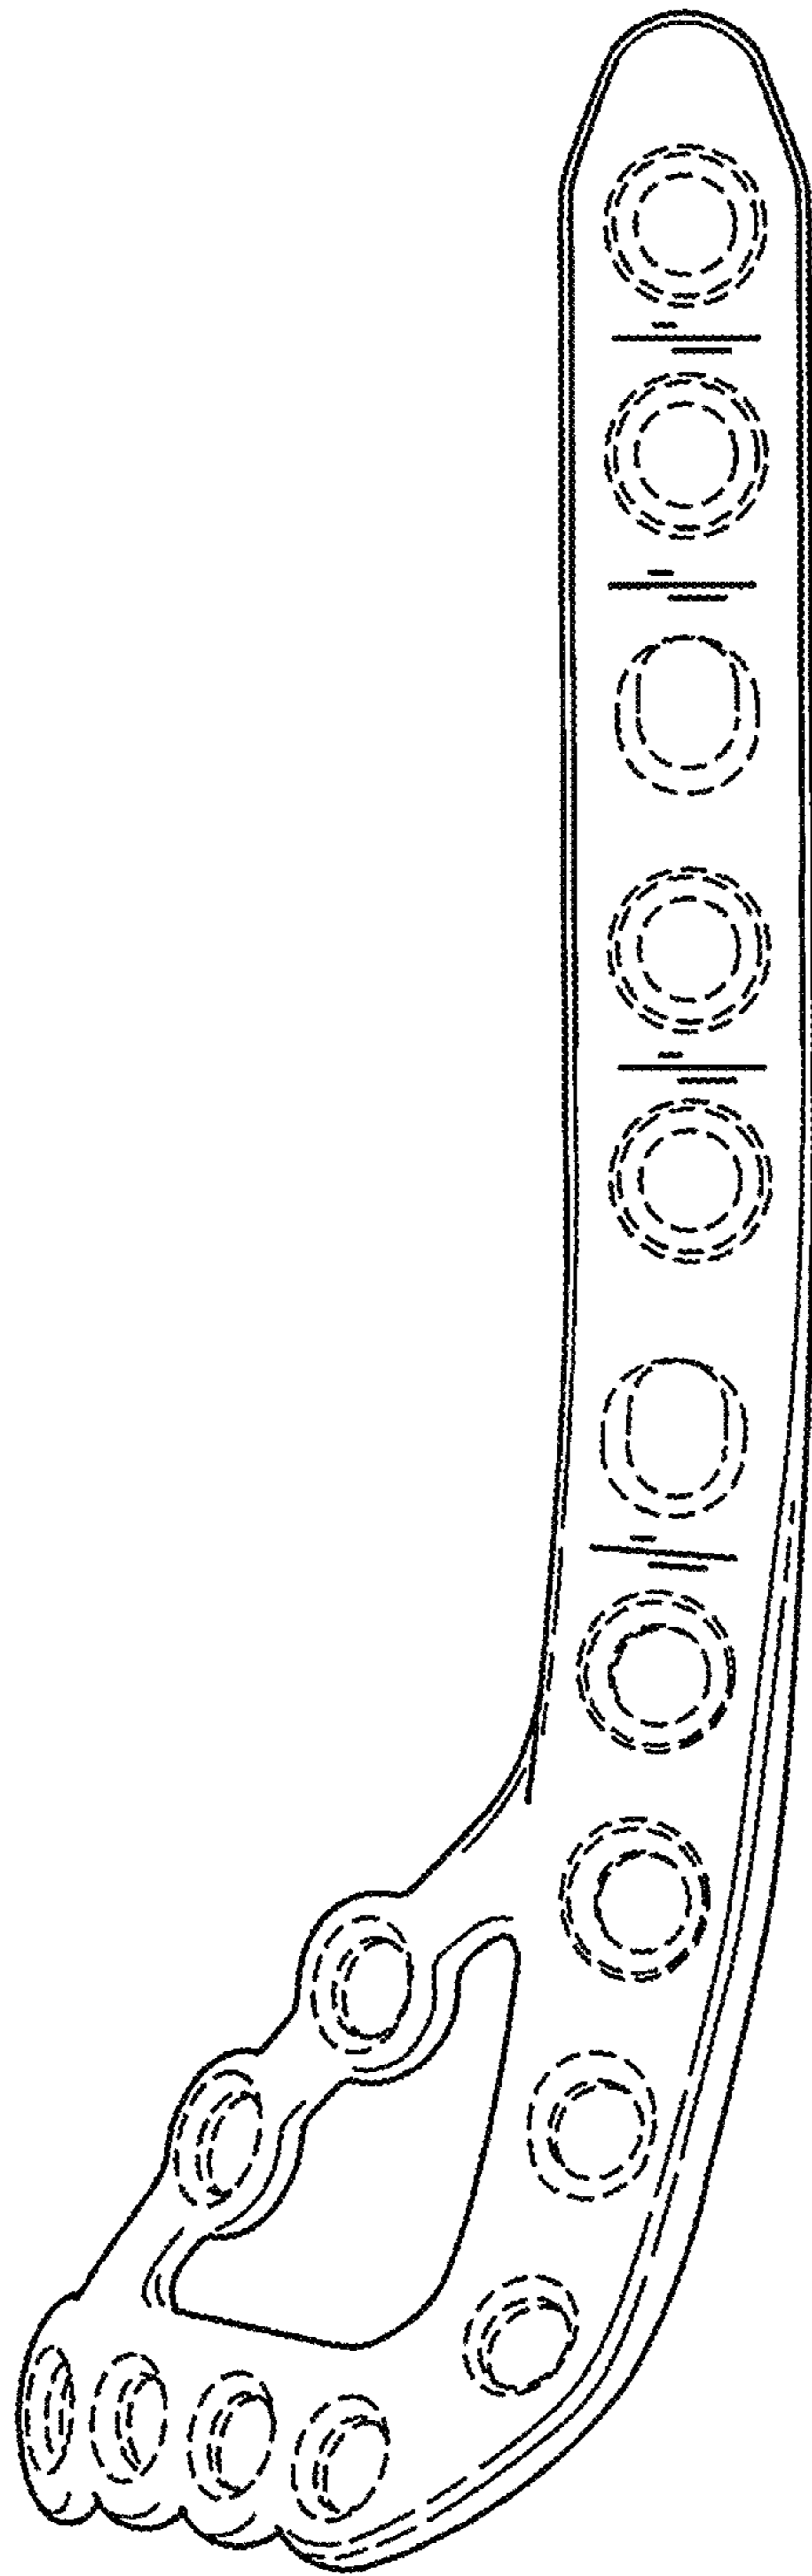


FIG. 2

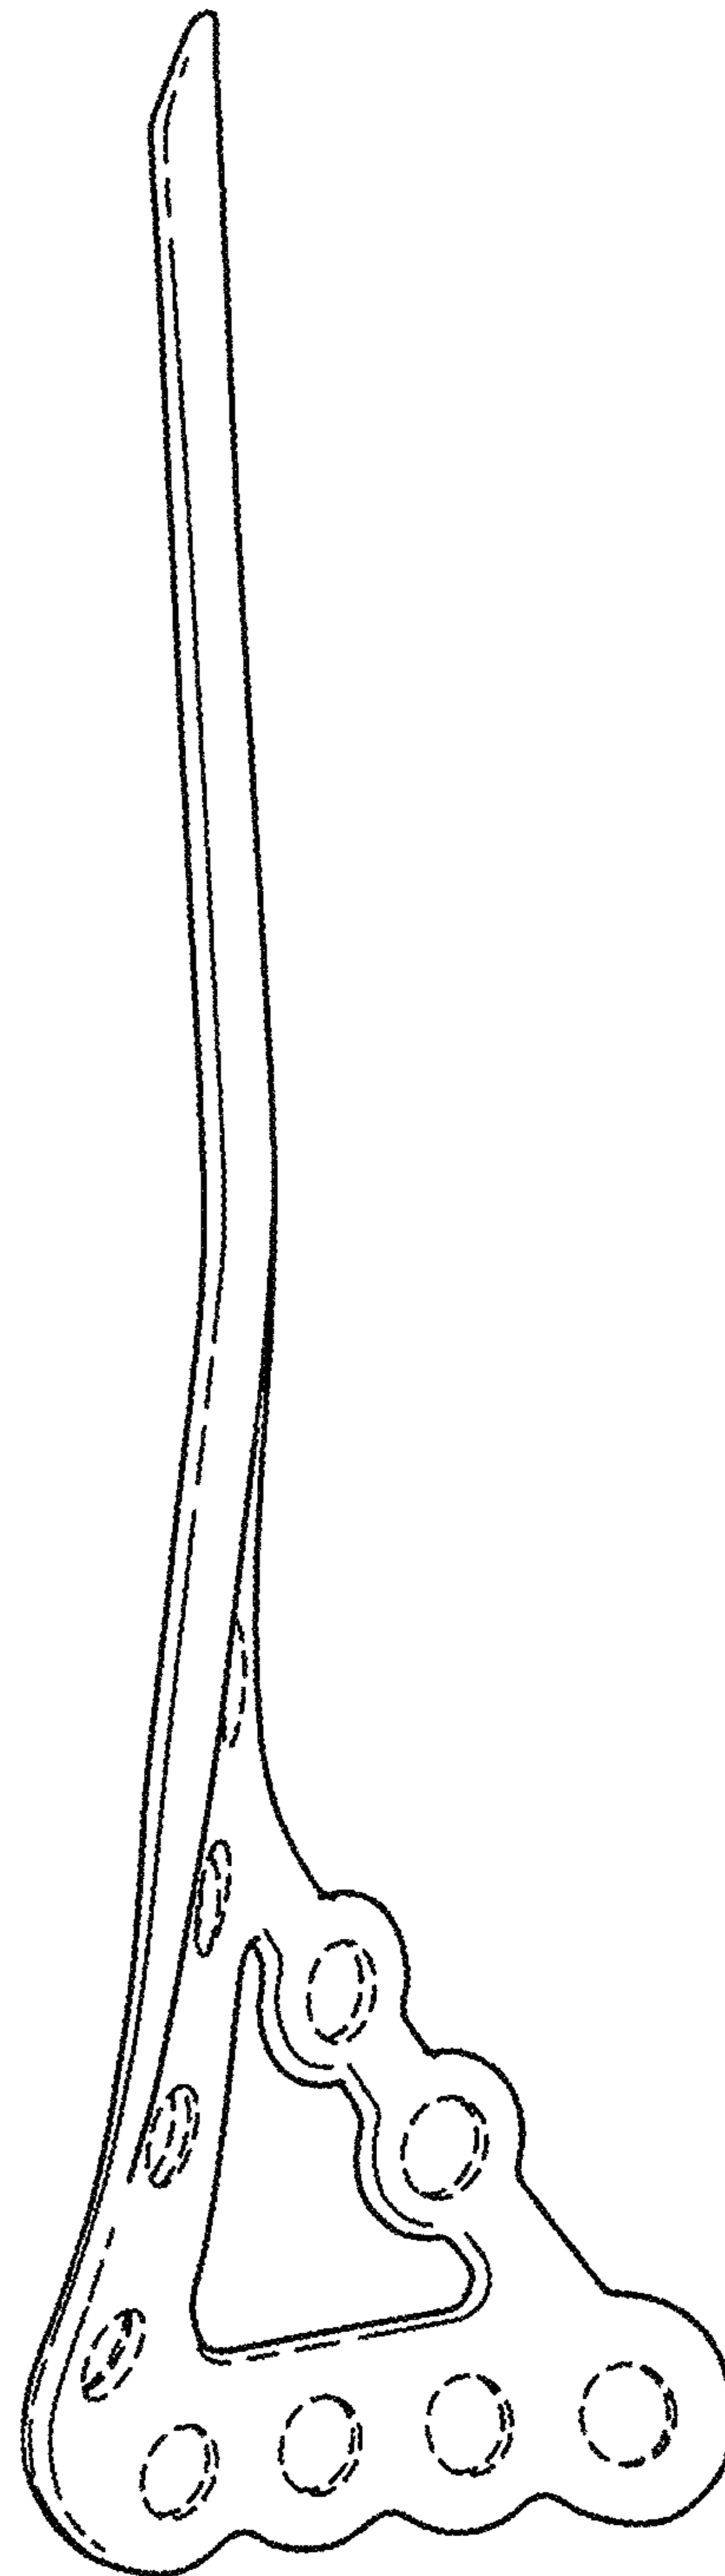


FIG. 3

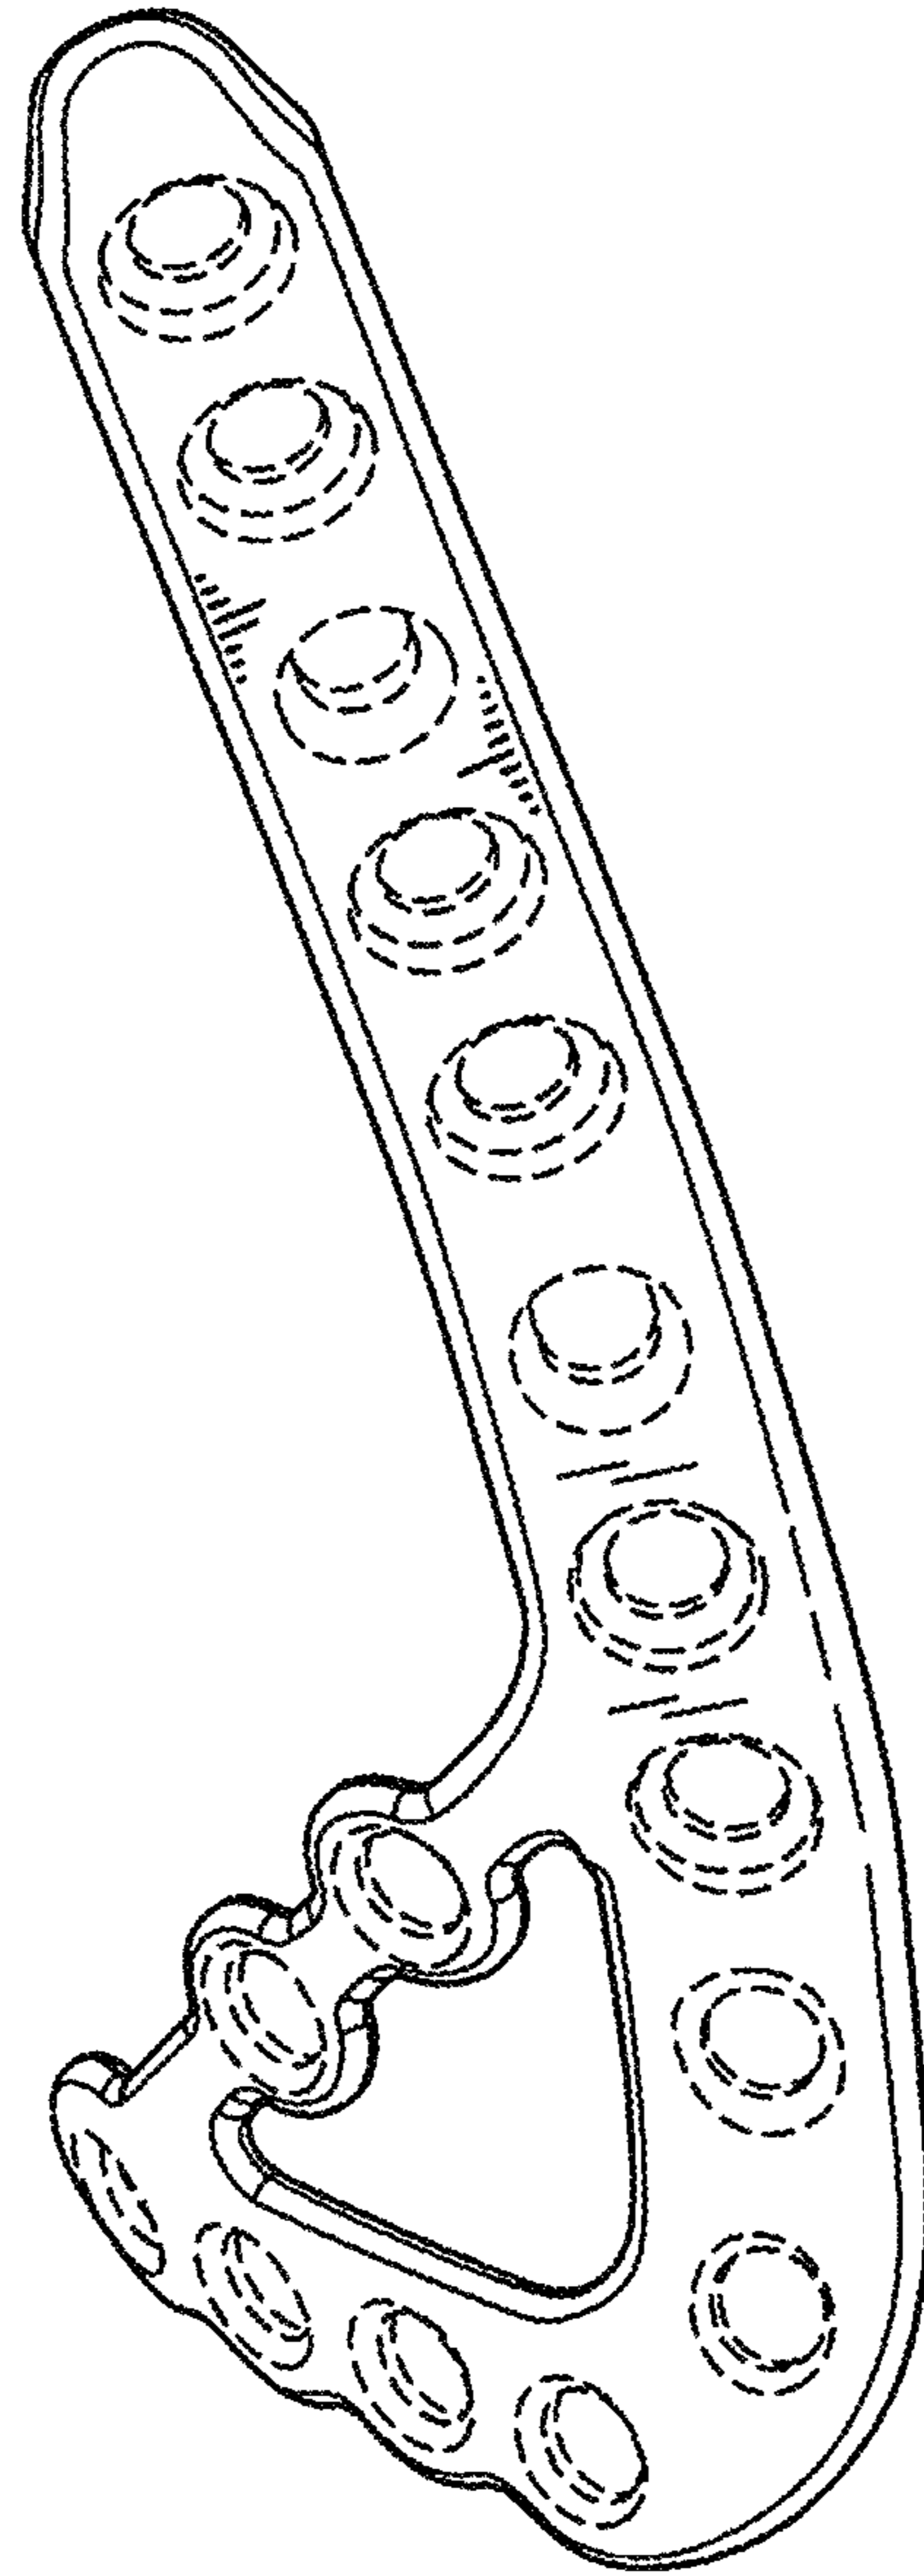


FIG. 4

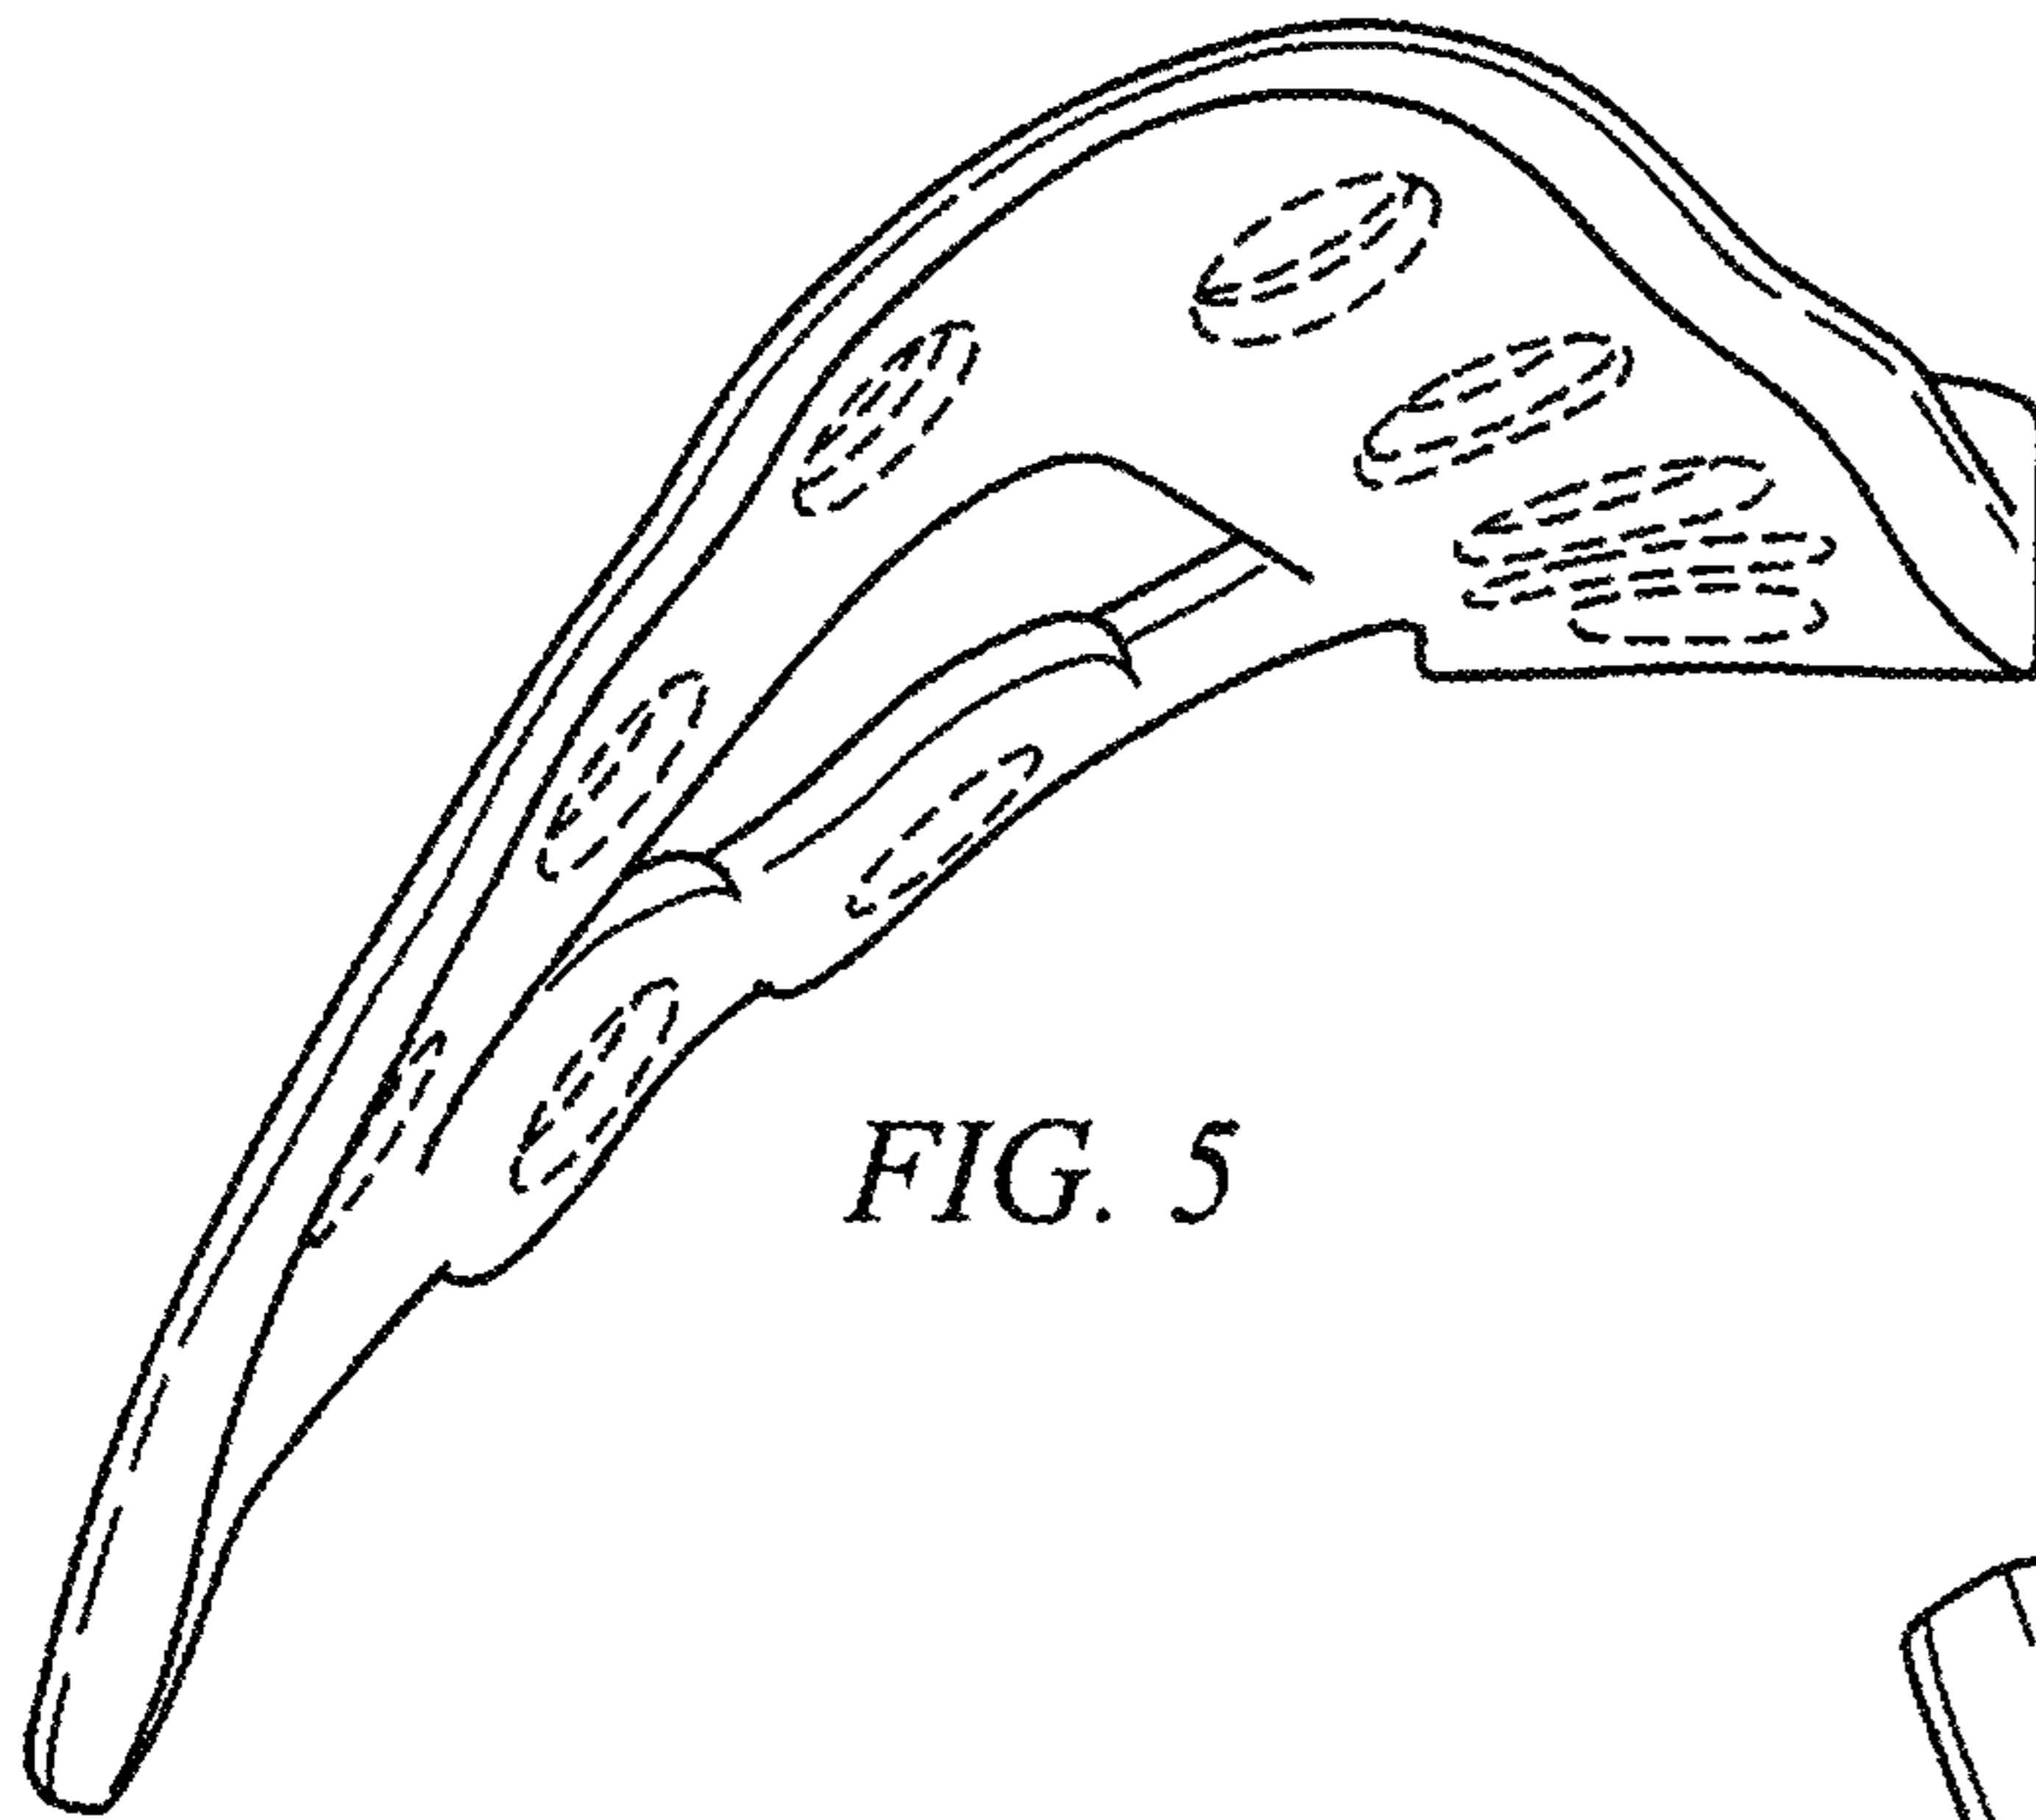


FIG. 5

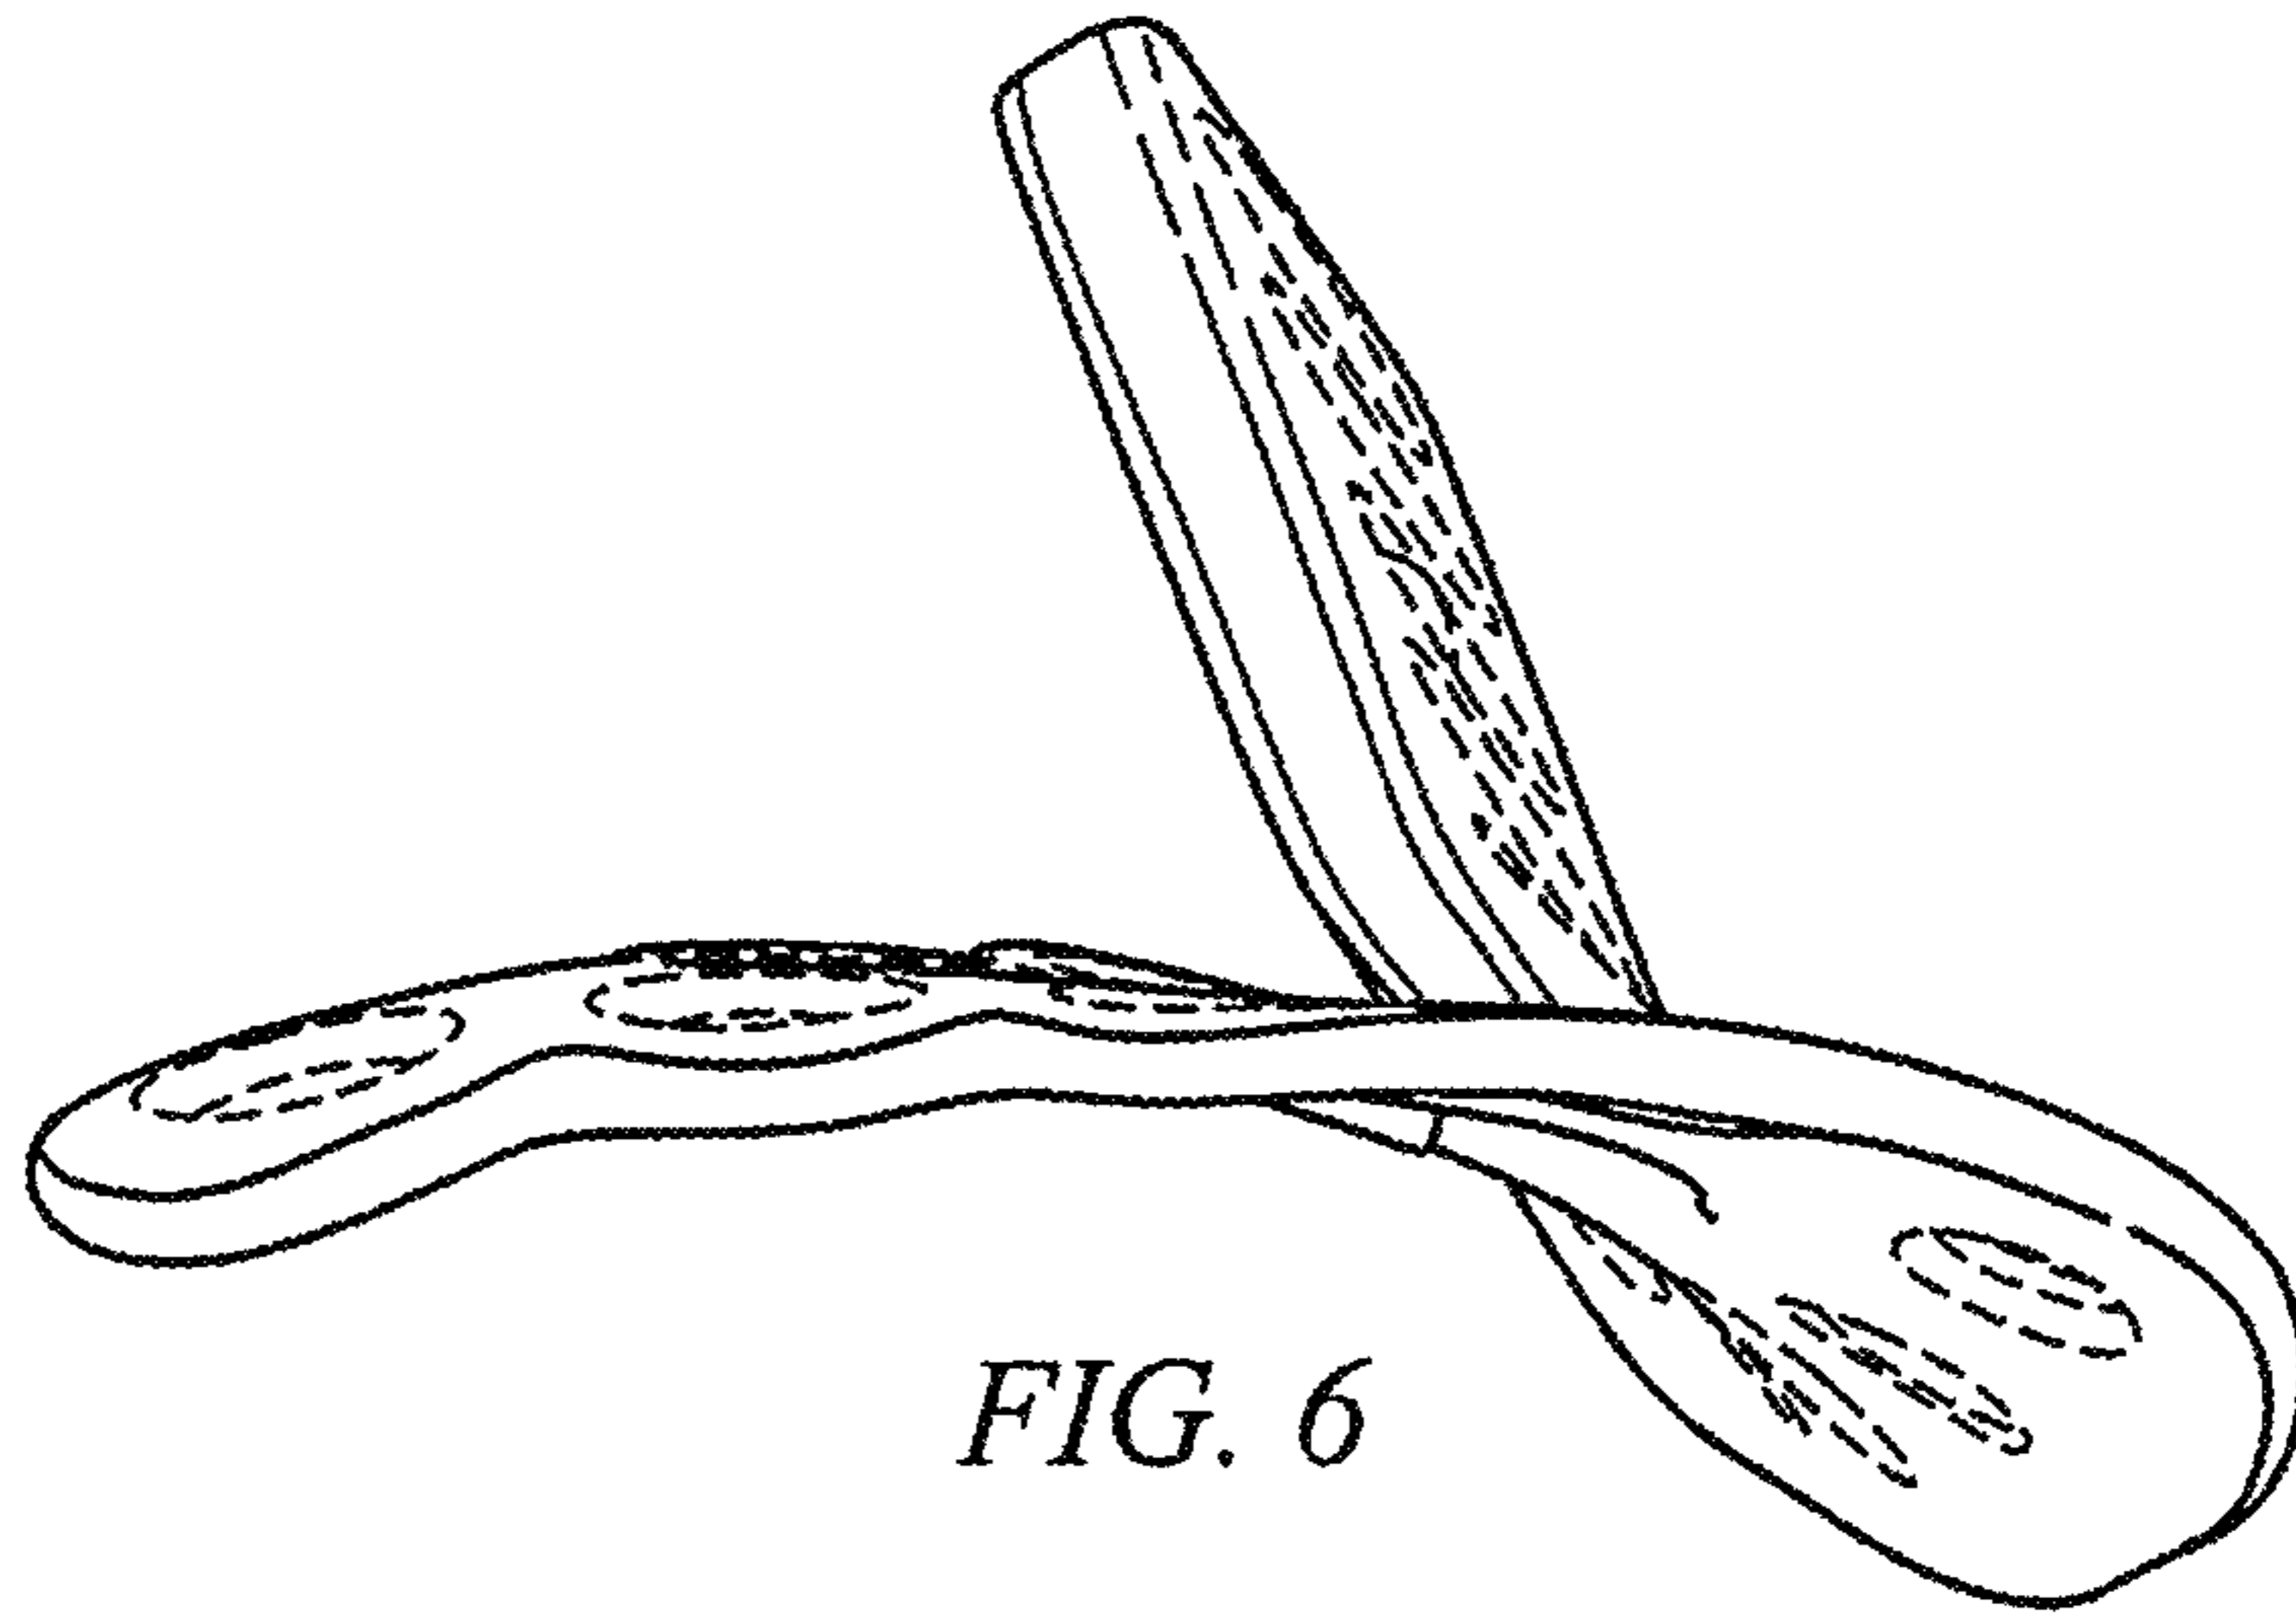


FIG. 6

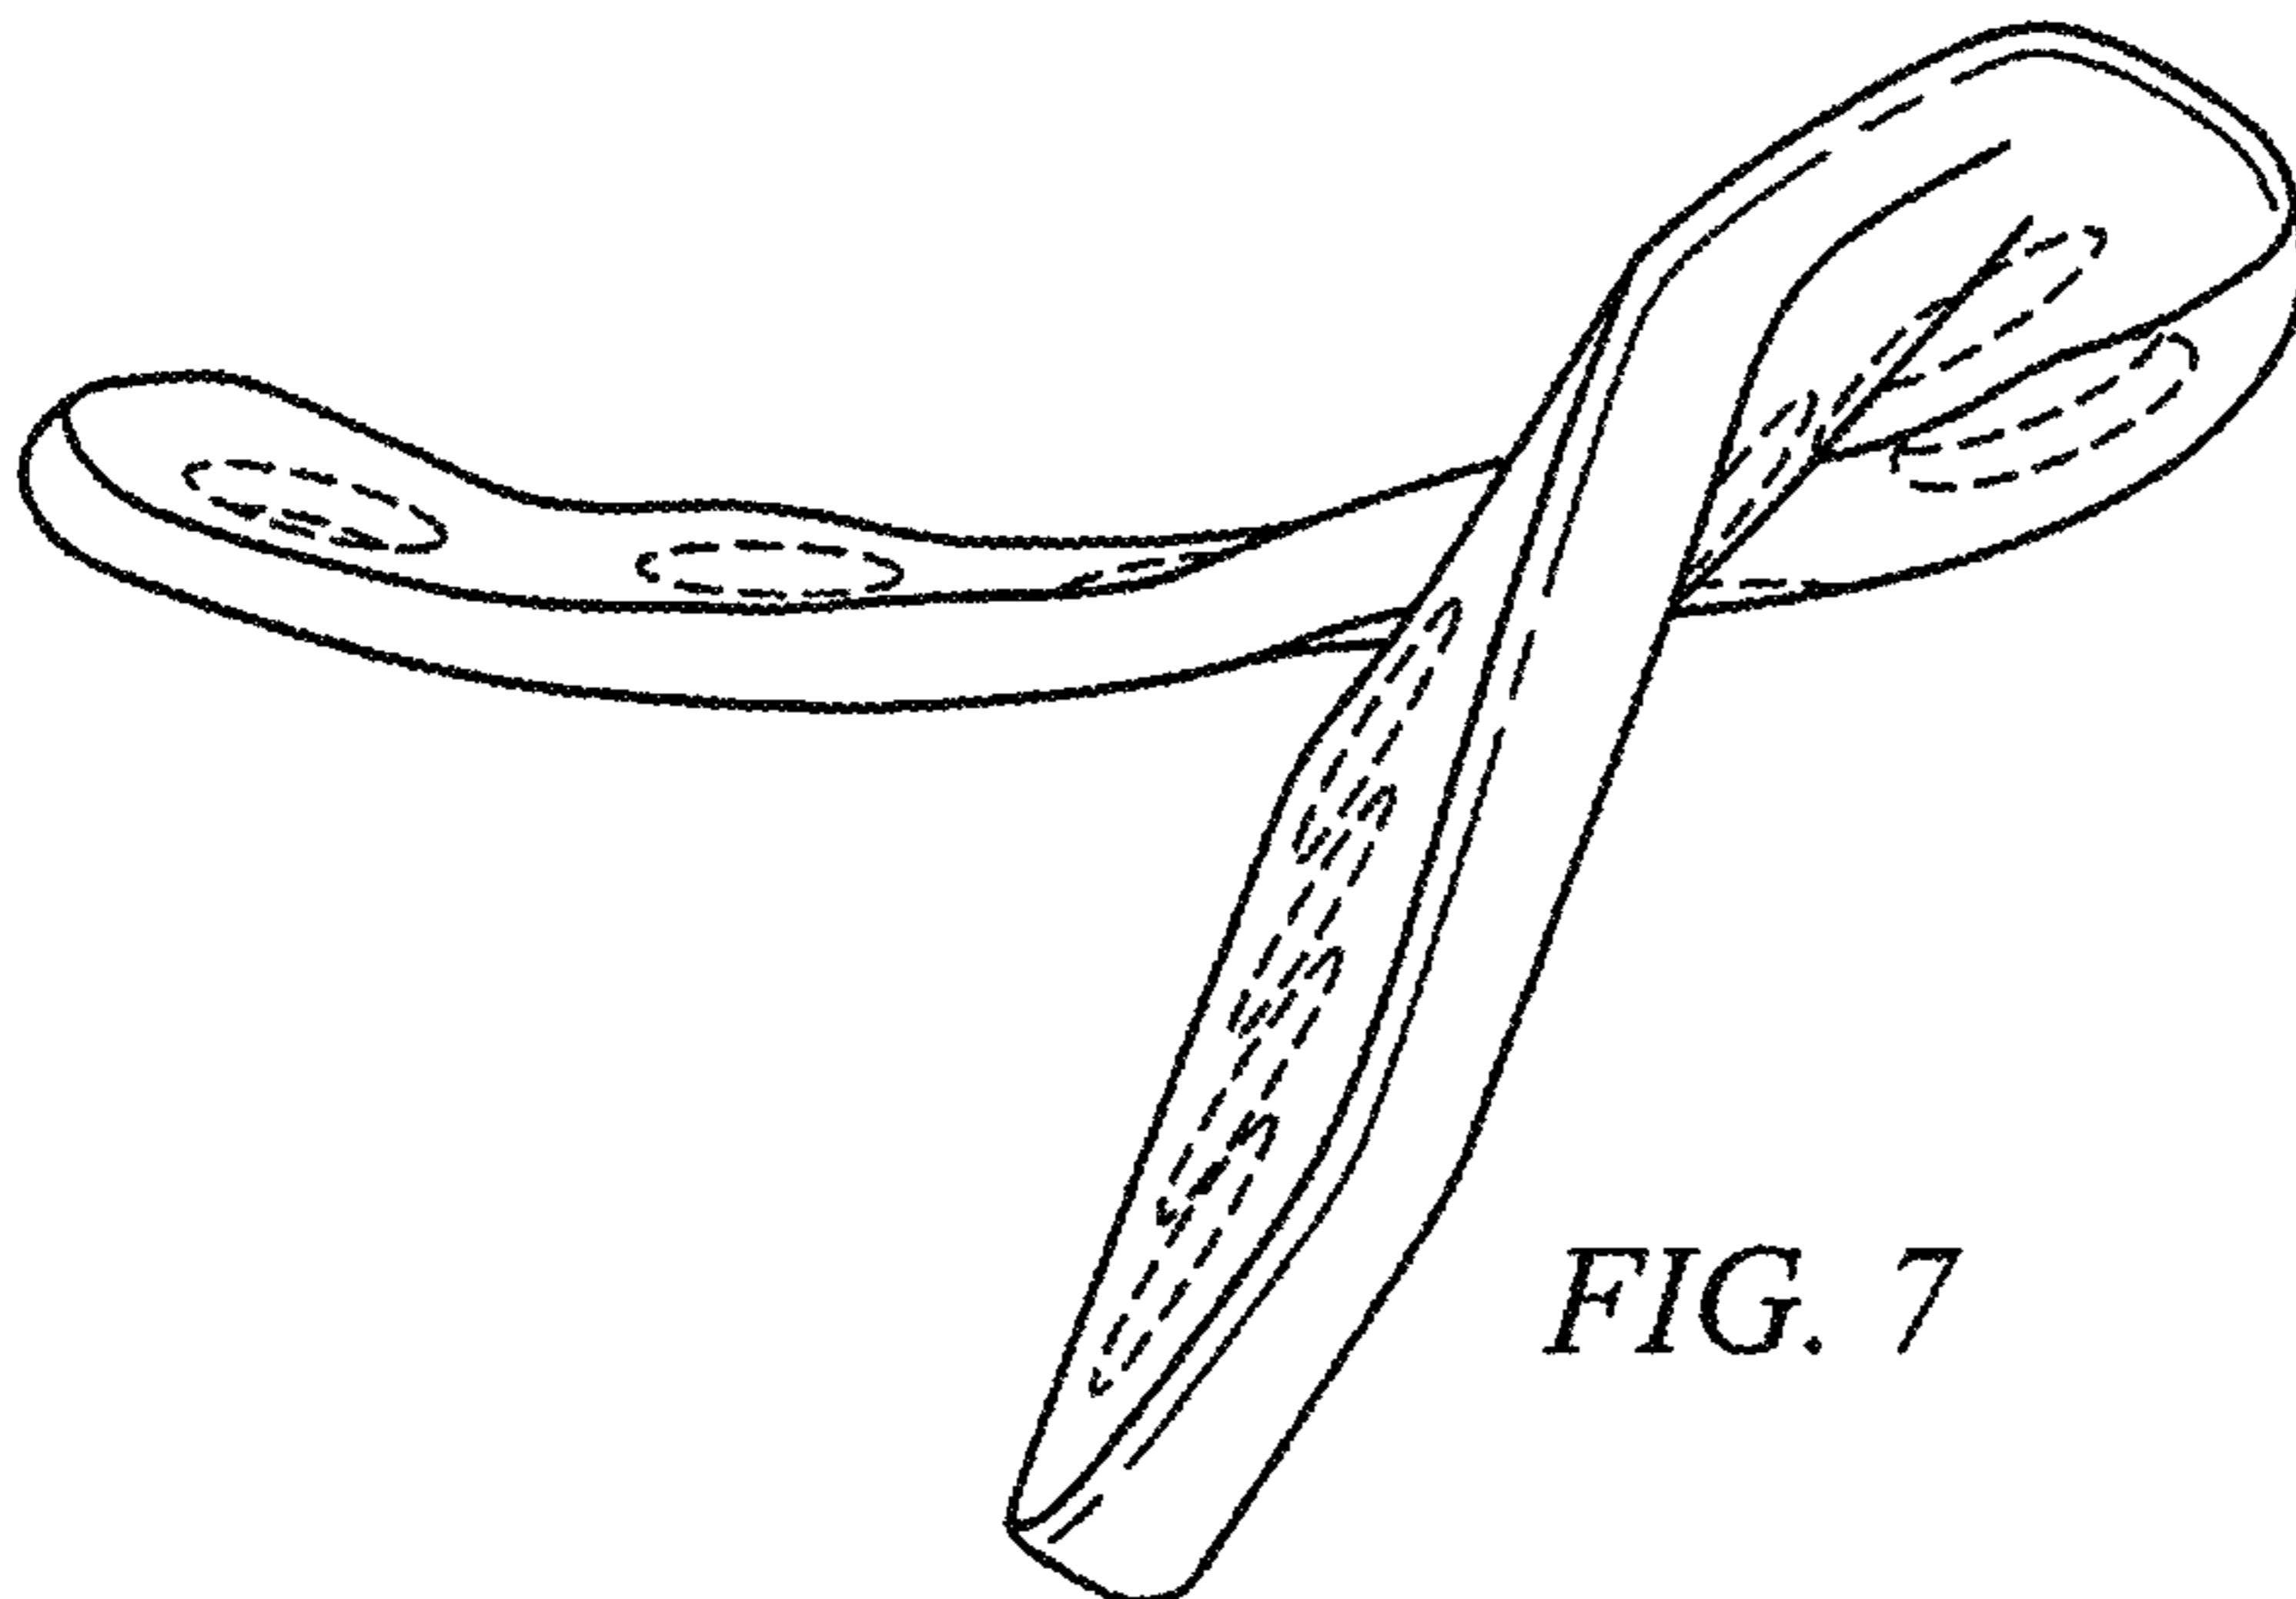


FIG. 7

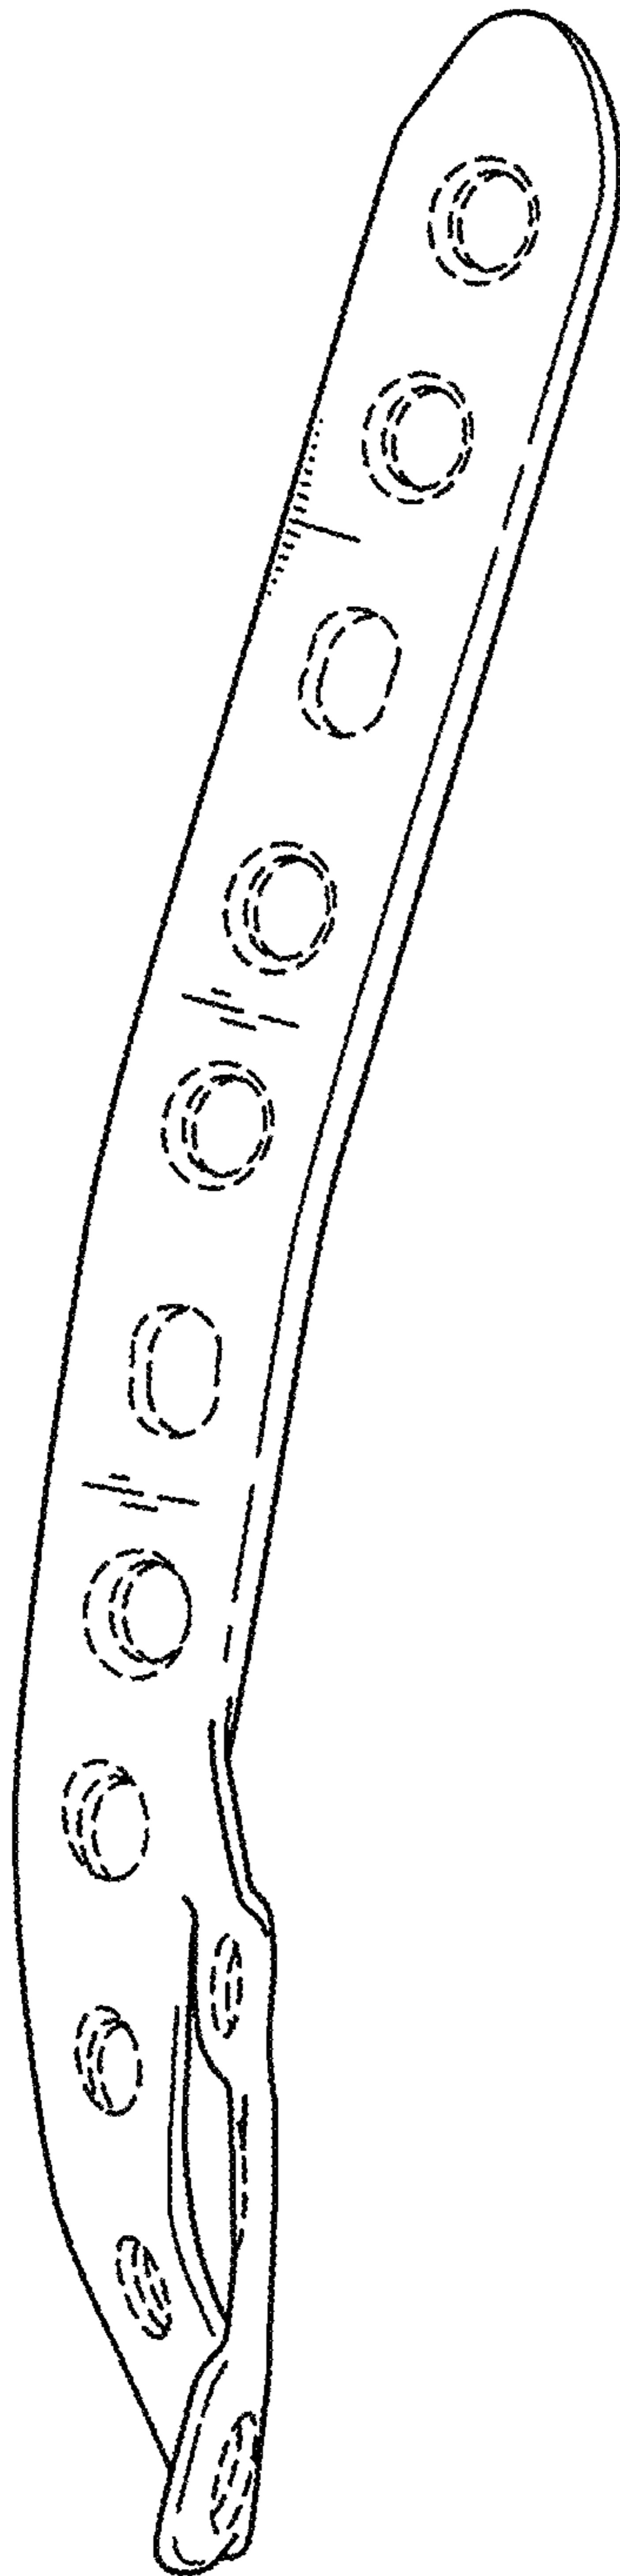


FIG. 8

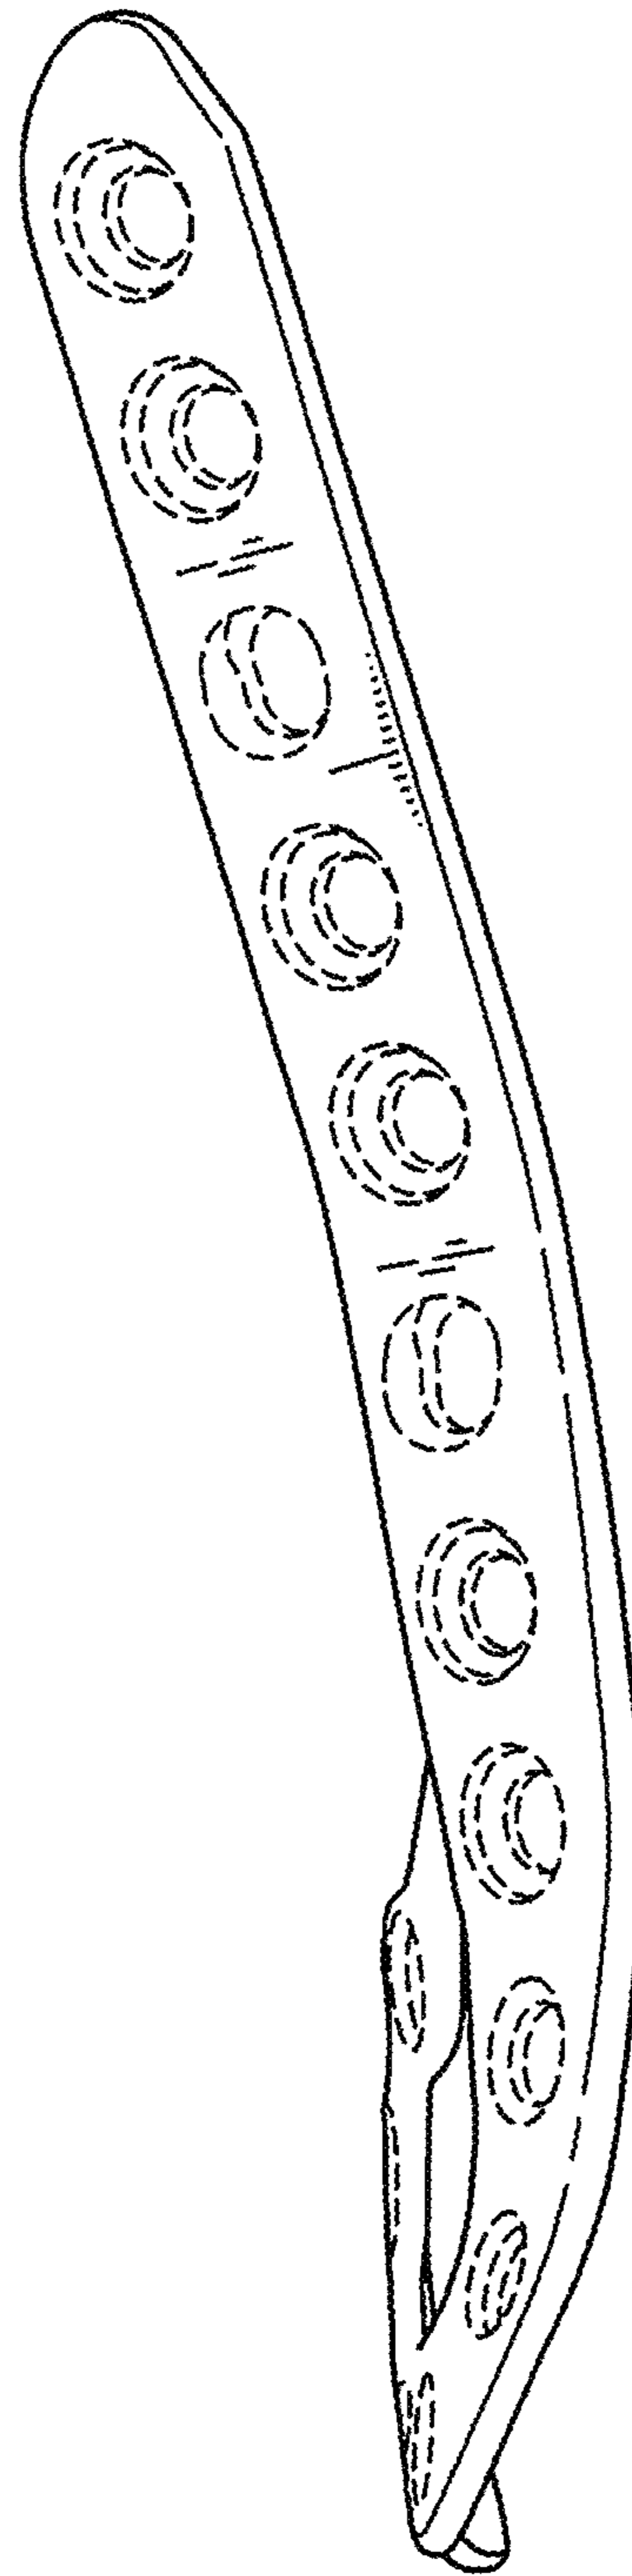


FIG. 9