



US00D767159S

(12) **United States Design Patent** (10) **Patent No.:** **US D767,159 S**
Maas (45) **Date of Patent:** **** Sep. 20, 2016**

(54) **IN VITRO DIAGNOSTIC MEDICAL DEVICE**

(71) Applicant: **Eurotrol B.V.**, Ede (NL)

(72) Inventor: **Bartholomeus Henricus Antonius Maas**, Ede (NL)

(73) Assignee: **EUROTROL B.V.**, Ede (NL)

(**) Term: **14 Years**

(21) Appl. No.: **29/518,906**

(22) Filed: **Feb. 27, 2015**

(30) **Foreign Application Priority Data**

Sep. 4, 2014 (EM) 002531152-0001

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/224**

(58) **Field of Classification Search**

USPC D24/216–230, 231, 232, 107, 169, 186;
D10/81

CPC G01N 21/0483; G01N 21/0303;
G01N 35/00029; G01N 2035/00019; G01N
2035/00306; G01N 2035/00326; B01L
2200/10; B01L 2200/16; B01L 2300/0809;
B01L 2300/0816; B01L 2300/0822; B01L
2300/0829; B01L 2300/0832; B01L
2300/0806; B01L 2300/0861

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D564,100 S * 3/2008 O'Banion D24/216
D594,131 S * 6/2009 Nguyen D24/216
D618,362 S * 6/2010 Giraud D24/224
D697,225 S * 1/2014 Maas D24/224

D728,126 S * 4/2015 Schmidt D24/224
9,085,397 B2 * 7/2015 Maas B01L 3/502
D748,813 S * 2/2016 Ishiguro D24/224
2009/0065378 A1 * 3/2009 Maas B01L 3/502
206/219

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Abelman, Frayne & Schwab

(57) **CLAIM**


The ornamental design for in vitro diagnostic medical device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and left side perspective view of the in vitro diagnostic medical device according to my new design; FIG. 2 is a top, rear and left side perspective view thereof; FIG. 3 is a left side elevational view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is front elevational view thereof; FIG. 6 is a rear elevational view thereof; FIG. 7 is a top plan view thereof; and, FIG. 8 is a bottom plan view thereof.

The broken lines in FIG. 8 illustrate portion of the in vitro diagnostic medical device that forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

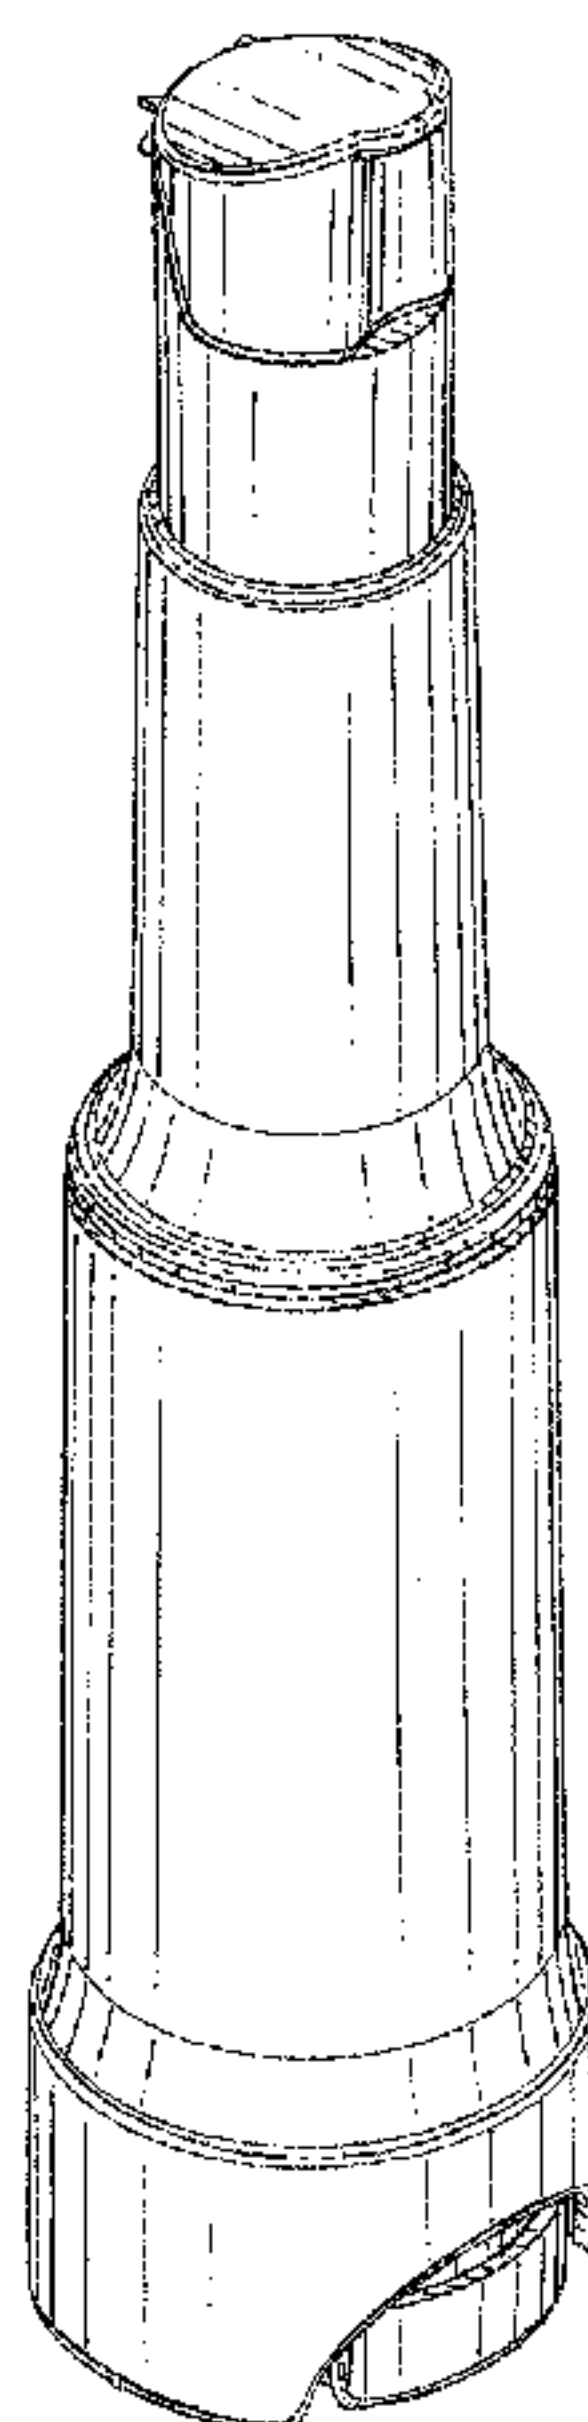

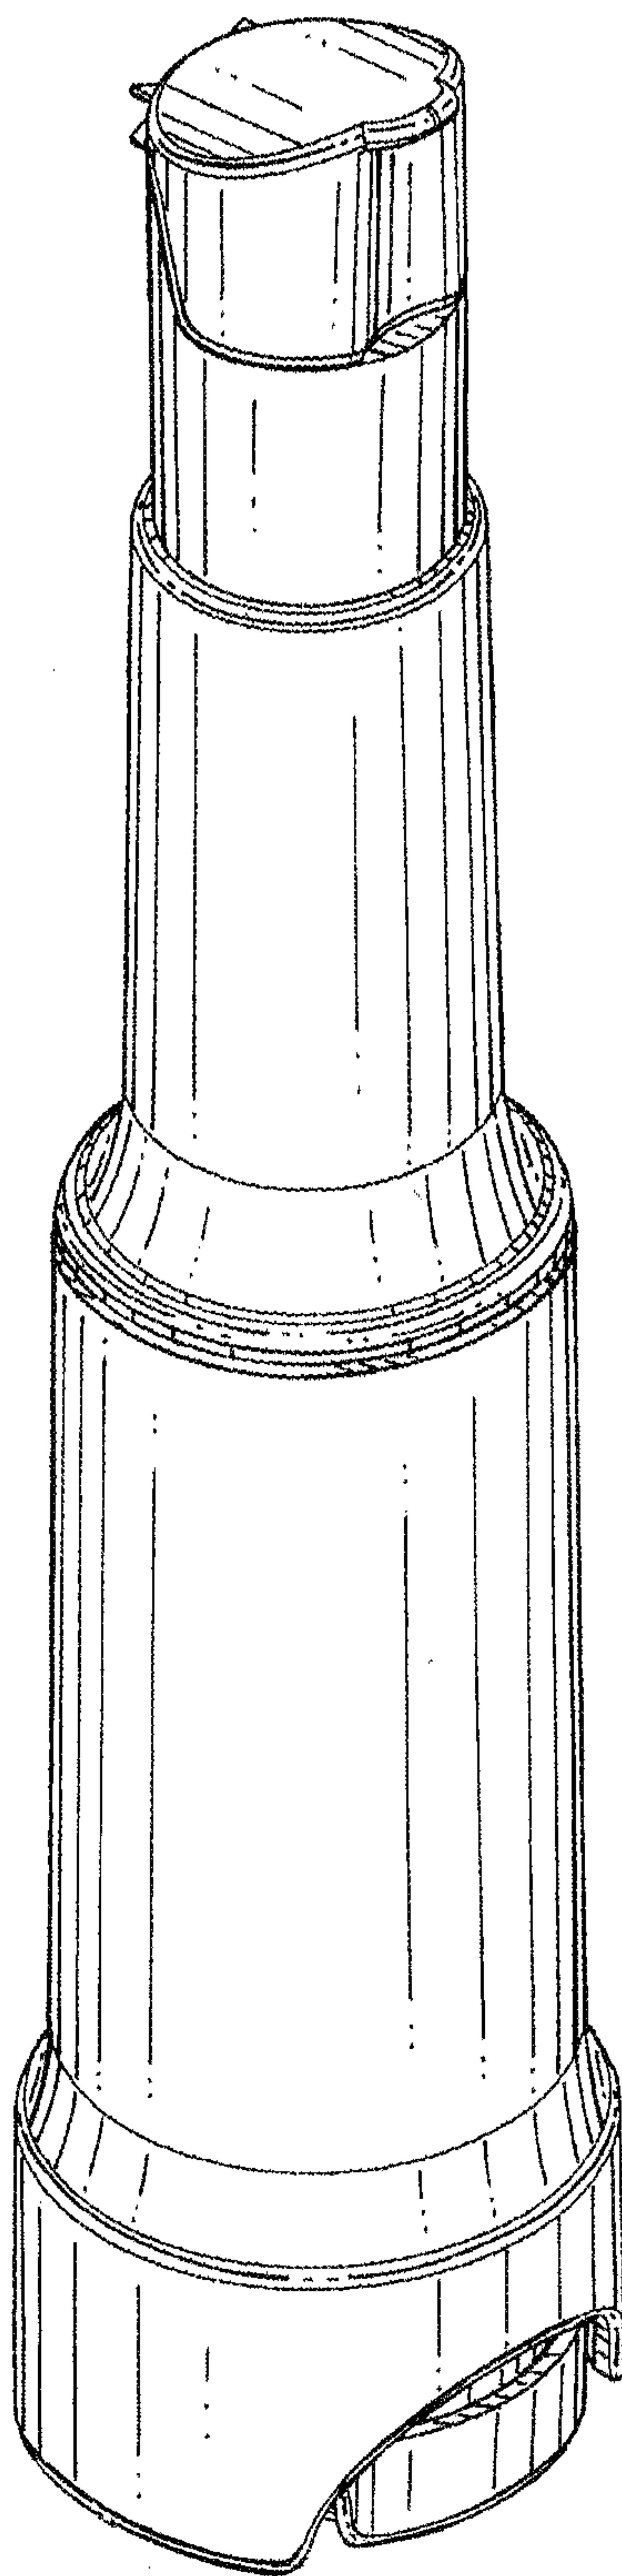


FIG. 1

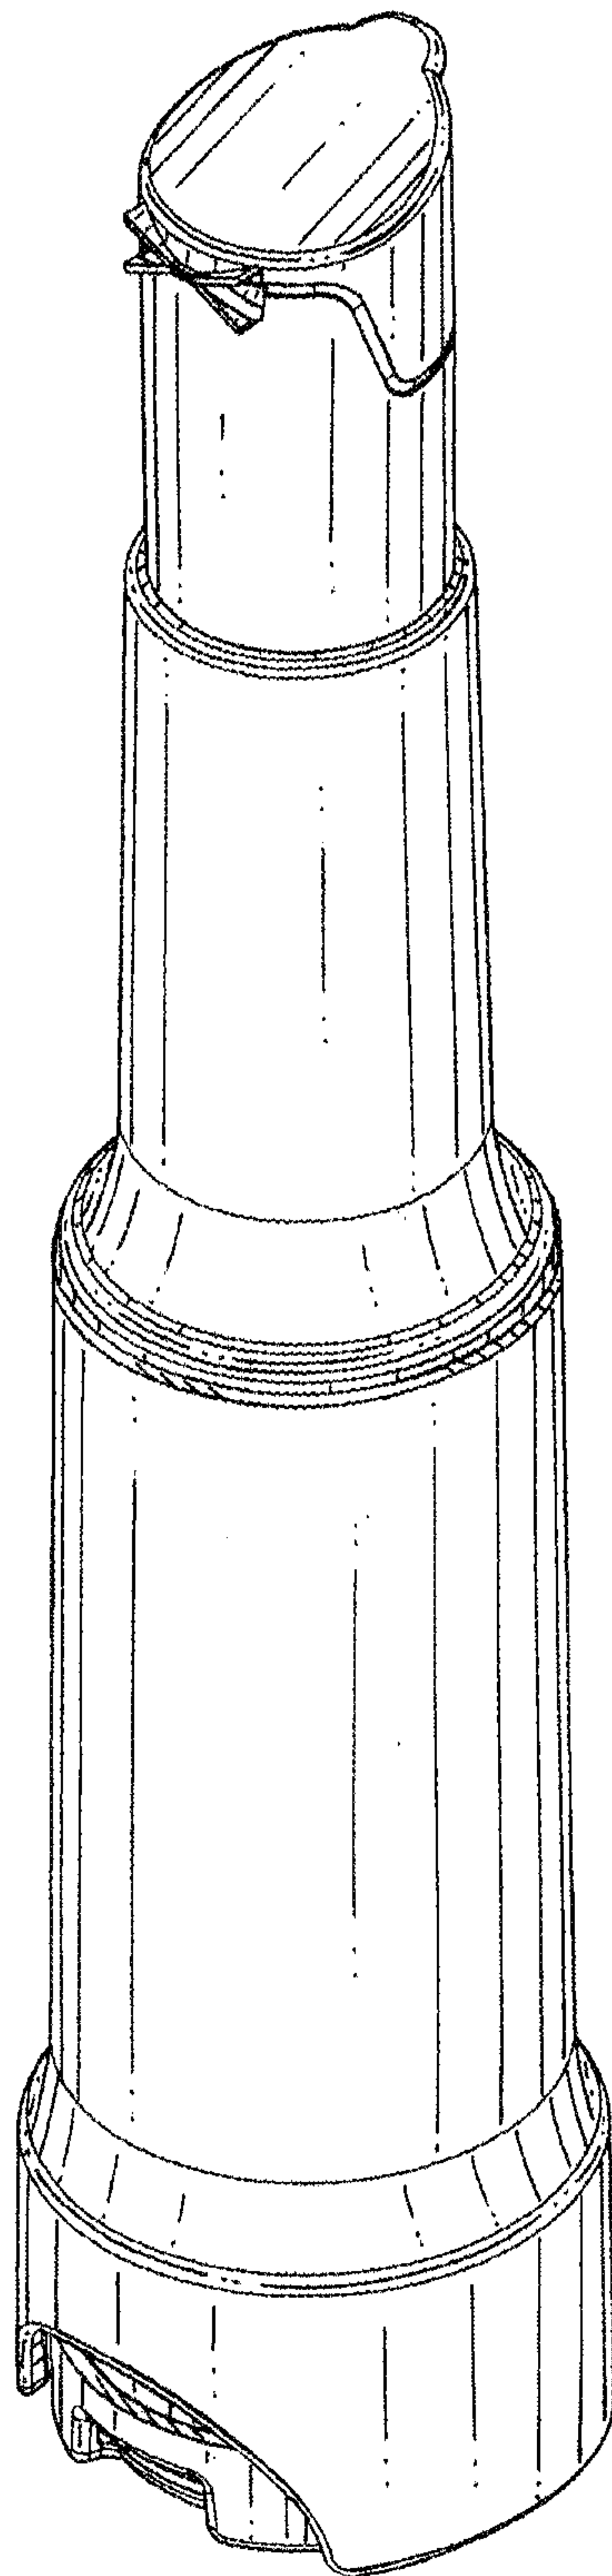
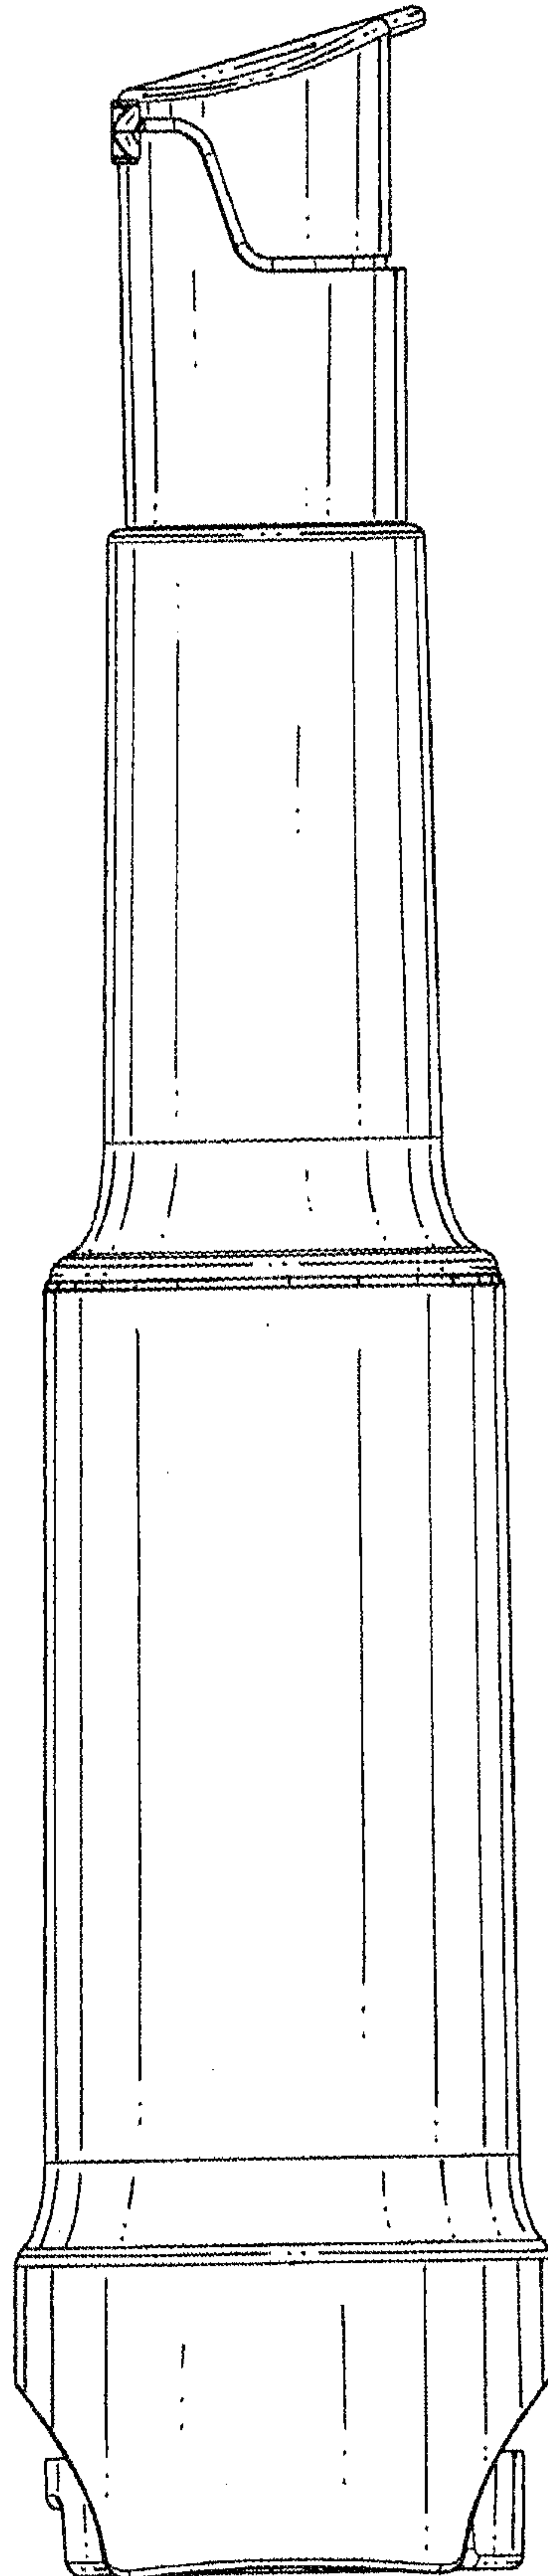


FIG. 2

FIG. 3



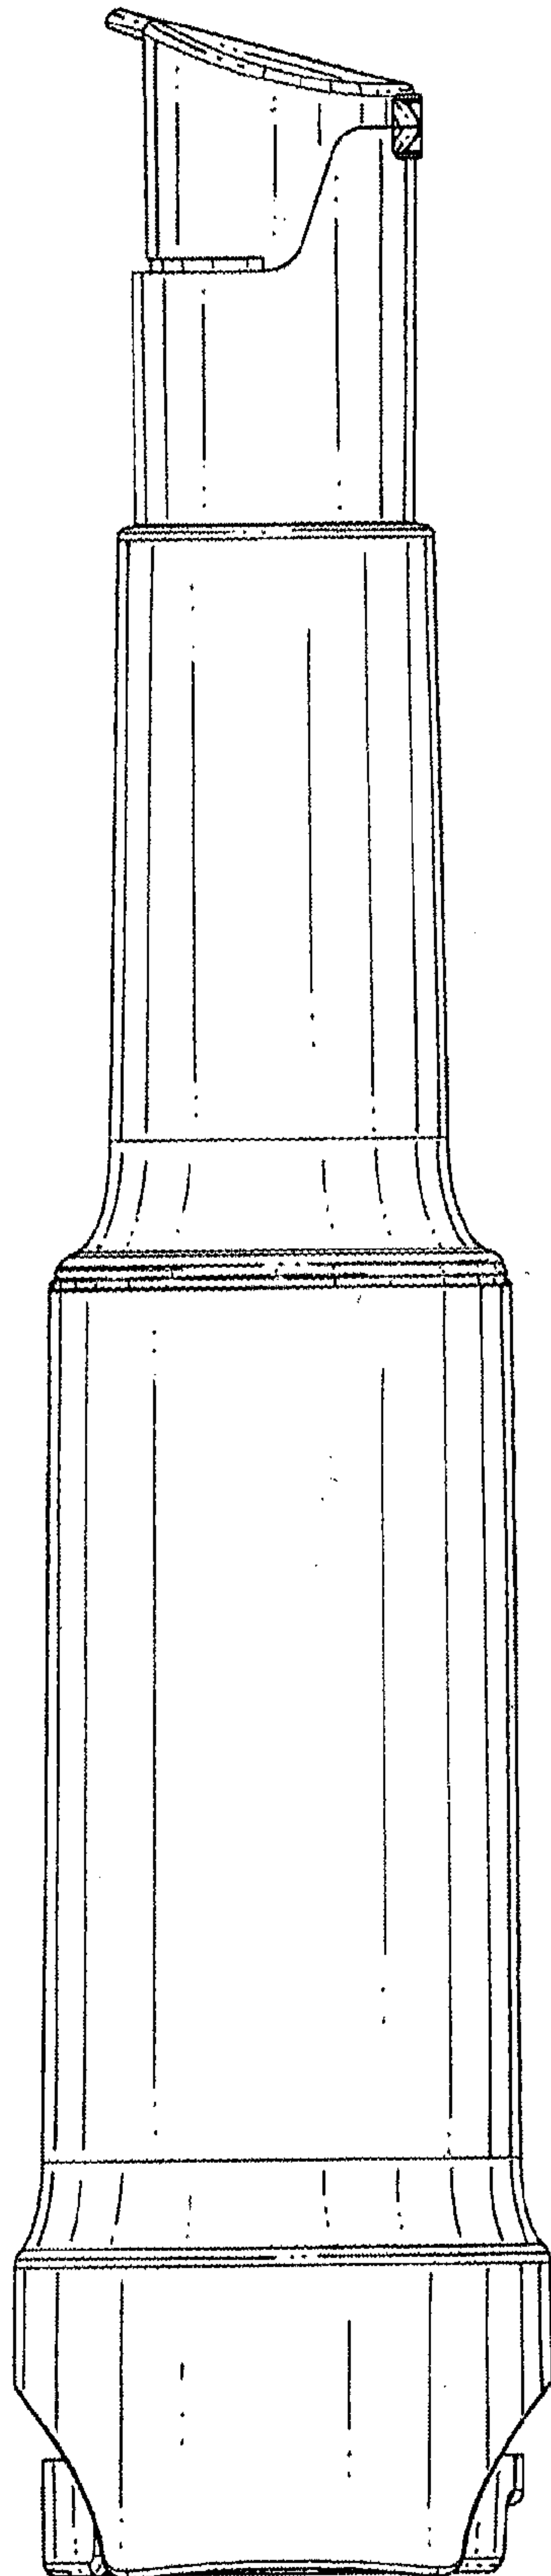
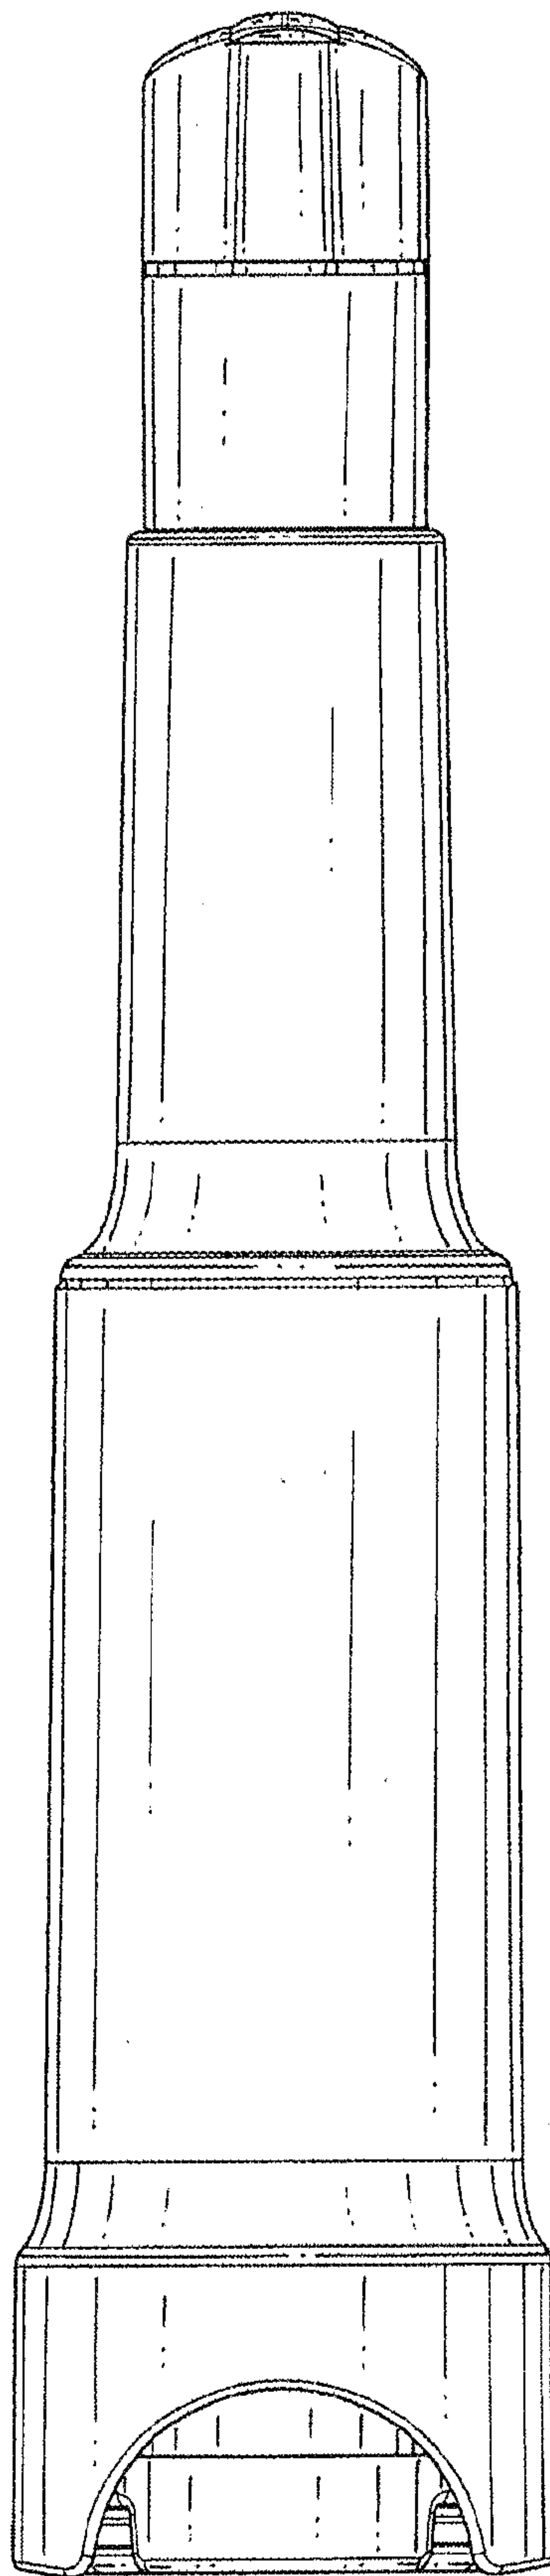


FIG. 4

FIG. 5



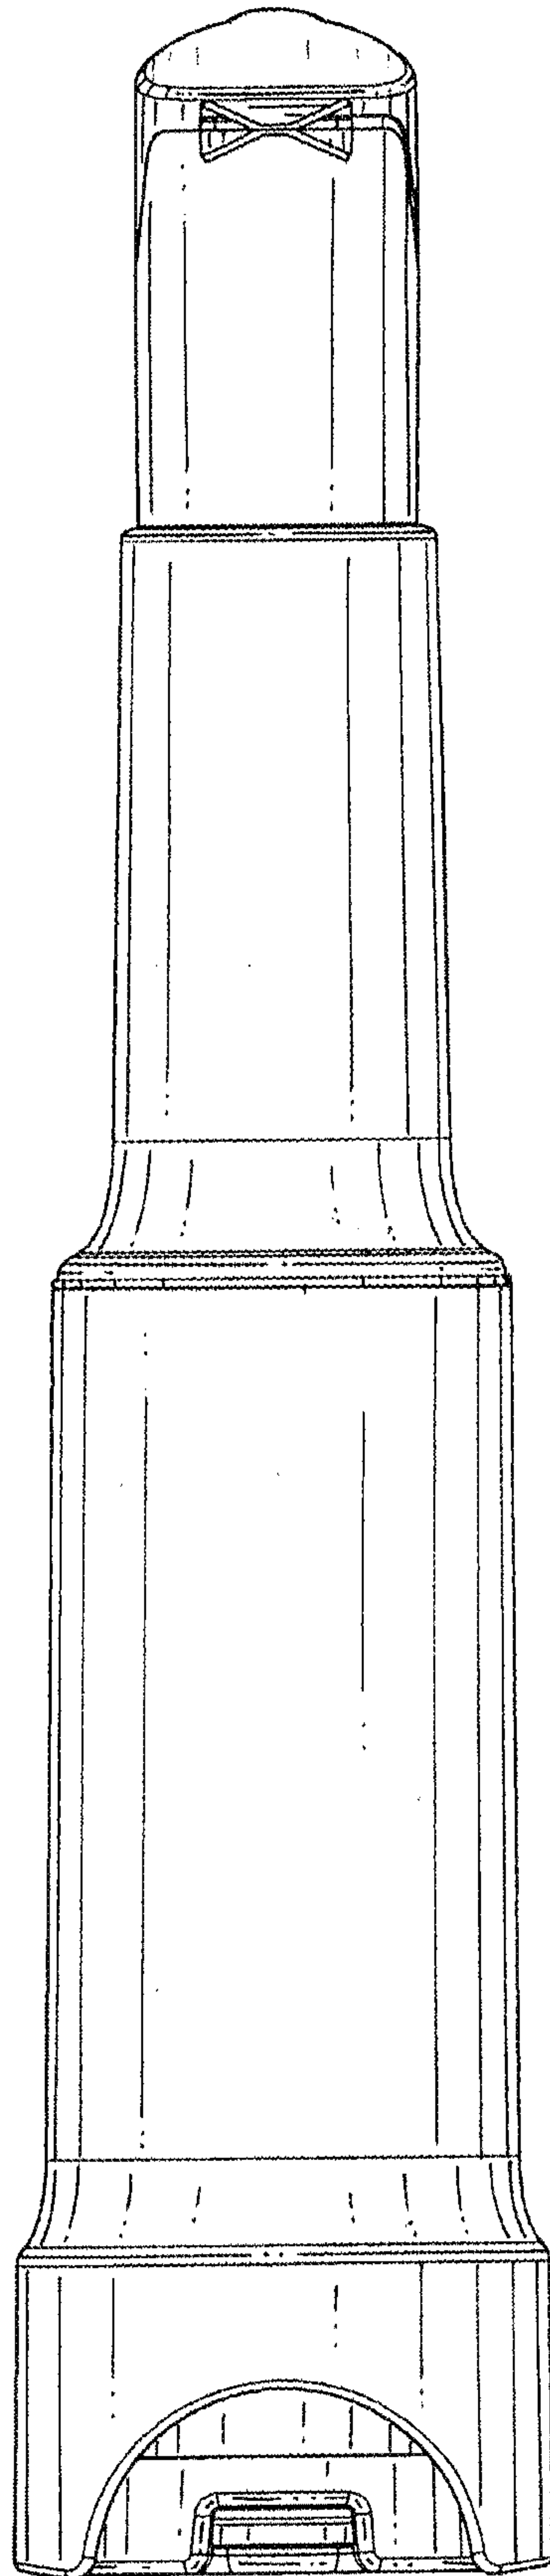


FIG. 6

FIG. 7

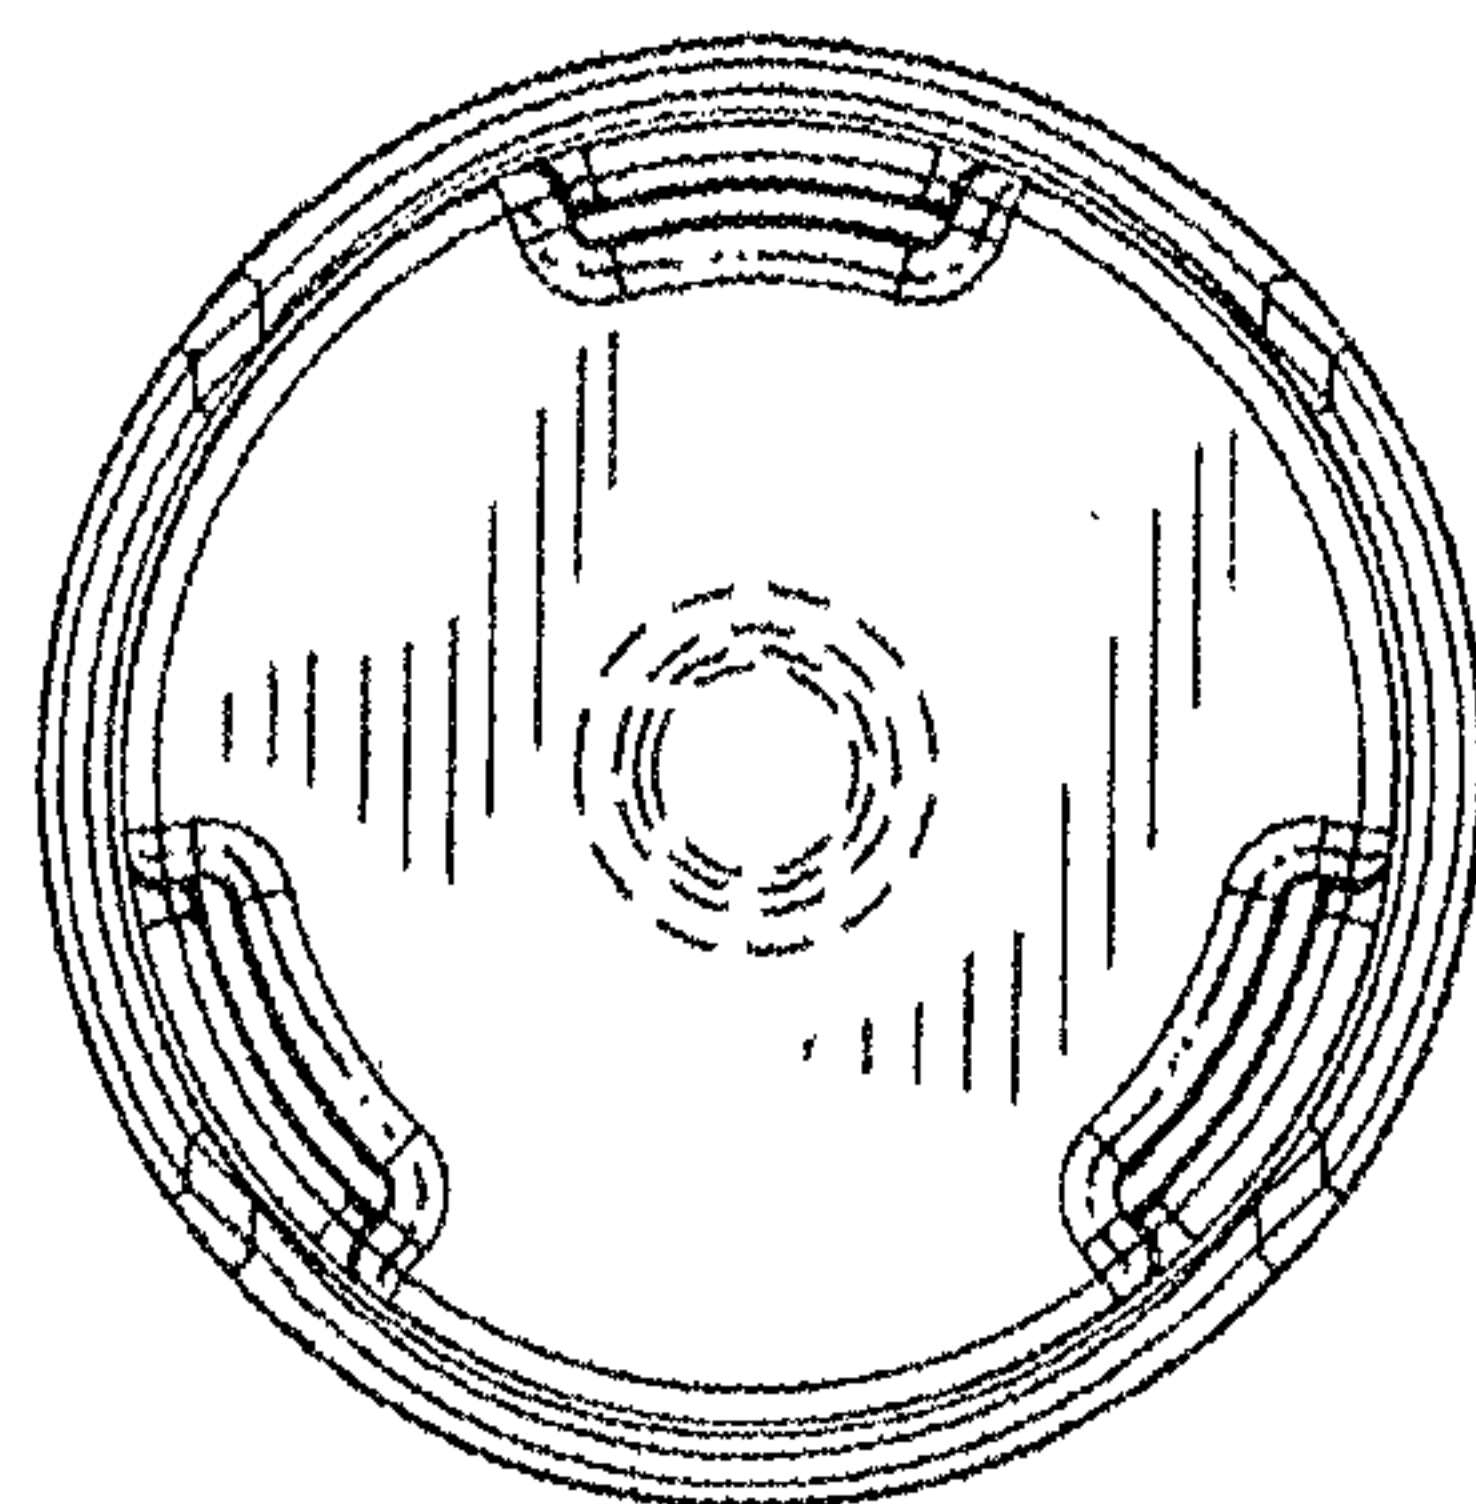
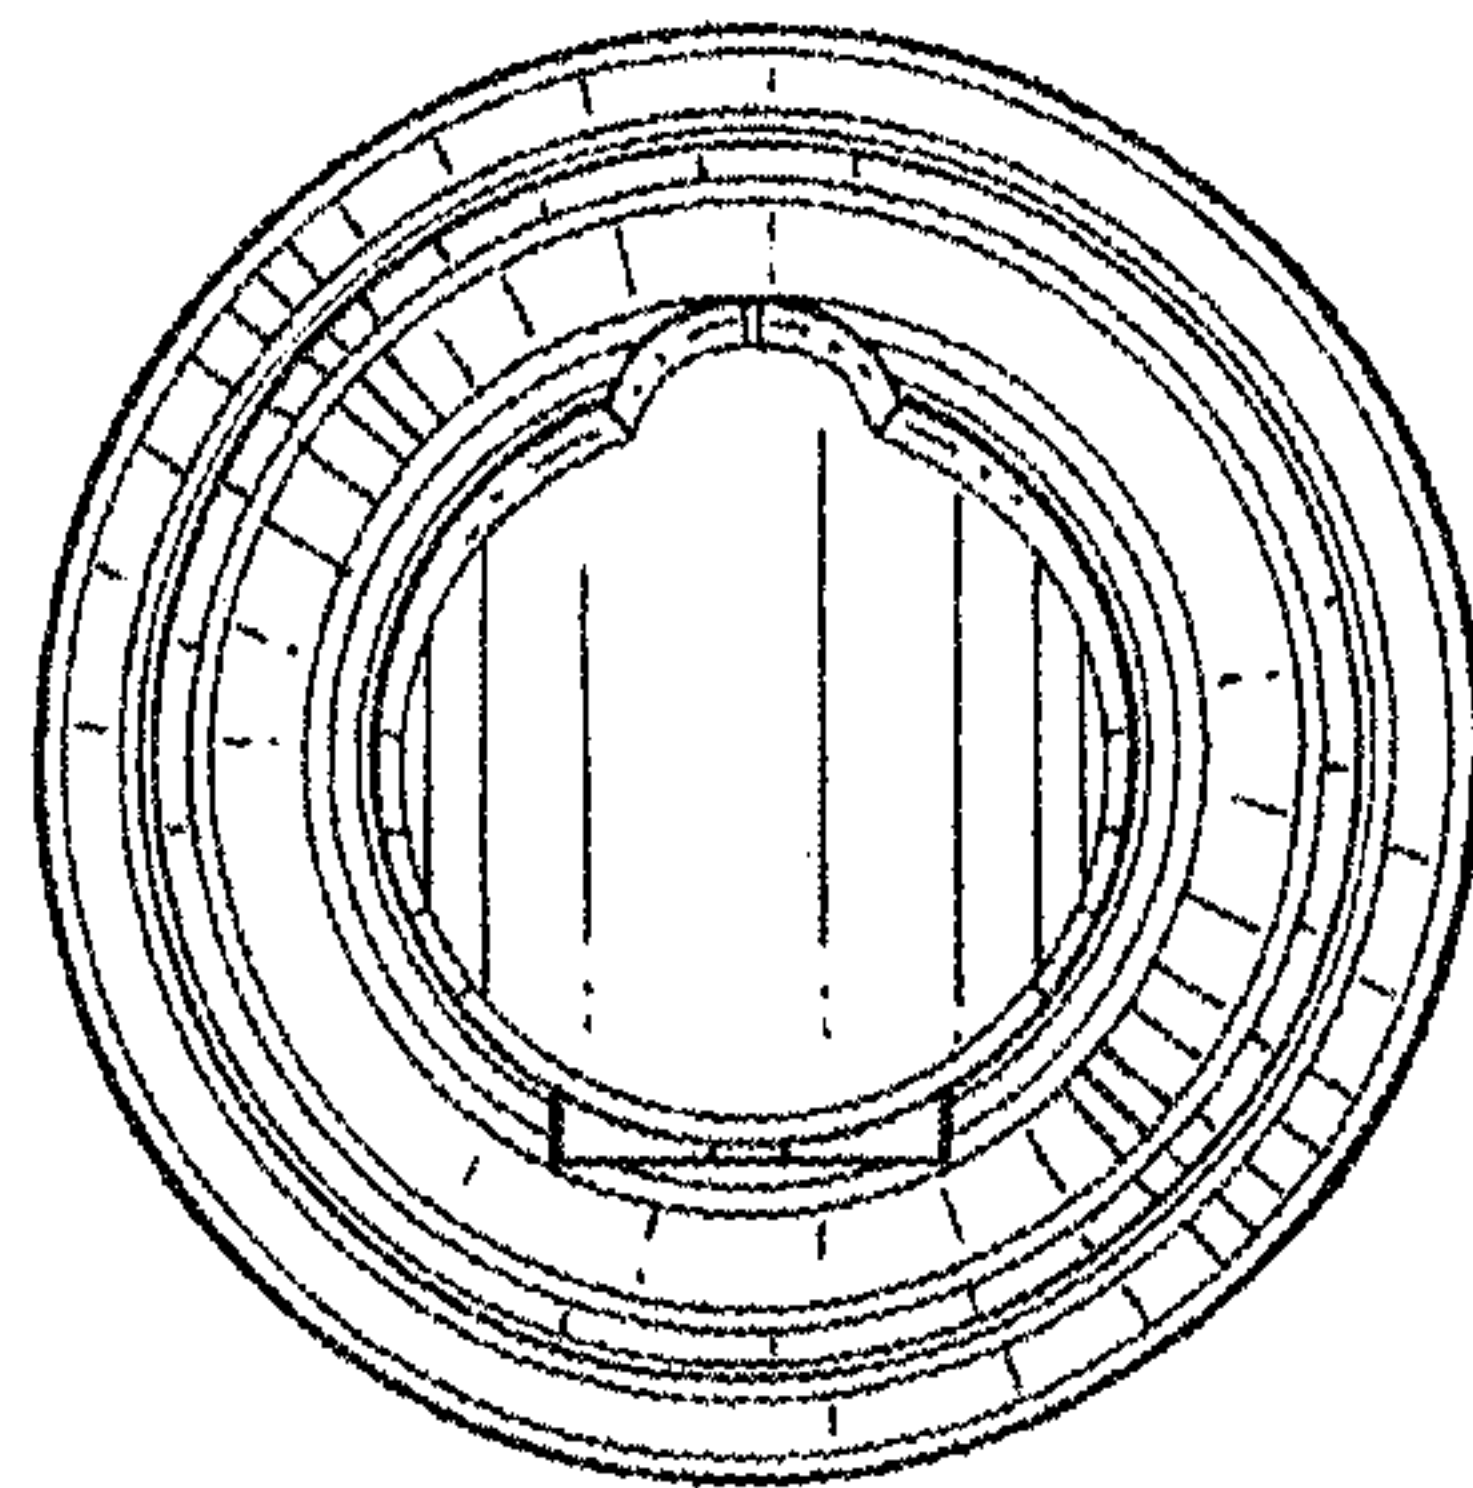


FIG. 8