



US00D768845S

(12) **United States Design Patent** (10) **Patent No.:** **US D768,845 S**  
**Burkes** (45) **Date of Patent:** **\*\* Oct. 11, 2016**

(54) **EXPIRATORY MUSCLE STRENGTH TRAINER ADAPTER**  
(71) Applicant: **M. LaQuisha Burkes**, Jackson, MS (US)  
(72) Inventor: **M. LaQuisha Burkes**, Jackson, MS (US)  
(\*\*) Term: **14 Years**  
(21) Appl. No.: **29/457,745**  
(22) Filed: **Jun. 12, 2013**  
(51) **LOC (10) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/110**  
(58) **Field of Classification Search**  
USPC ..... D24/110-110.6  
CPC .... A63B 23/18; A61B 5/093; A61B 5/0871;  
A61B 5/087; A61B 5/097; A61M 16/0045  
See application file for complete search history.

5,645,049 A \* 7/1997 Foley et al. .... 128/203.29  
5,899,832 A \* 5/1999 Hougen ..... 482/13  
6,606,990 B2 \* 8/2003 Stapleton et al. .... 128/200.18  
6,612,306 B1 \* 9/2003 Mault ..... 128/204.22  
6,631,716 B1 10/2003 Robinson et al.  
D511,210 S \* 11/2005 Cardona Burrull ..... D24/110.5  
7,004,162 B1 \* 2/2006 Foley et al. .... 128/200.22  
D556,902 S \* 12/2007 Allen ..... D24/110.5  
7,861,710 B2 1/2011 Ingenito  
8,118,713 B2 2/2012 Foley  
8,161,966 B2 \* 4/2012 Foley et al. .... 128/200.24  
2002/0170557 A1 \* 11/2002 Schmidt ..... 128/200.23  
2003/0234015 A1 \* 12/2003 Bruce et al. .... 128/200.23

\* cited by examiner

*Primary Examiner* — Deanna L Pratt  
*Assistant Examiner* — Lilyana Bekic  
(74) *Attorney, Agent, or Firm* — Kirk A. Buhler; Buhler & Associates


(57) **CLAIM**  
The ornamental design for an expiratory muscle strength trainer adapter, as shown and described.



**DESCRIPTION**


FIG. 1 is a top side view thereof;  
FIG. 2 is a bottom side view thereof;  
FIG. 3 is a left side view, the right side view being a mirror image thereof;  
FIG. 4 is a side sectional view taken along lines 5-5 from FIG. 3 thereof;  
FIG. 5 is a front view thereof; and,  
FIG. 6 is a rear side view.  
The break lines indicate that the appearance of any portion of the expiratory muscle strength trainer adapter between the break lines forms no part of the claimed design.

**1 Claim, 3 Drawing Sheets**


(56) **References Cited**  
U.S. PATENT DOCUMENTS  
2,007,330 A \* 7/1935 Hicks ..... 128/203.28  
3,511,228 A \* 5/1970 Lundgren et al. .... 601/41  
3,664,337 A \* 5/1972 Lindsey et al. .... 128/200.18  
3,880,591 A \* 4/1975 Burroughs ..... 600/529  
D242,489 S \* 11/1976 Burroughs ..... D24/110  
D254,324 S 2/1980 Thead, Jr.  
D254,443 S 3/1980 Adams  
4,221,381 A 9/1980 Ericson  
D263,166 S \* 2/1982 Bushman ..... D24/110  
D266,695 S \* 10/1982 Trammll et al. .... D24/110  
D269,124 S 5/1983 McCombs et al.  
4,832,015 A \* 5/1989 Nowacki et al. .... 128/205.23  
4,854,574 A 8/1989 Larson et al.

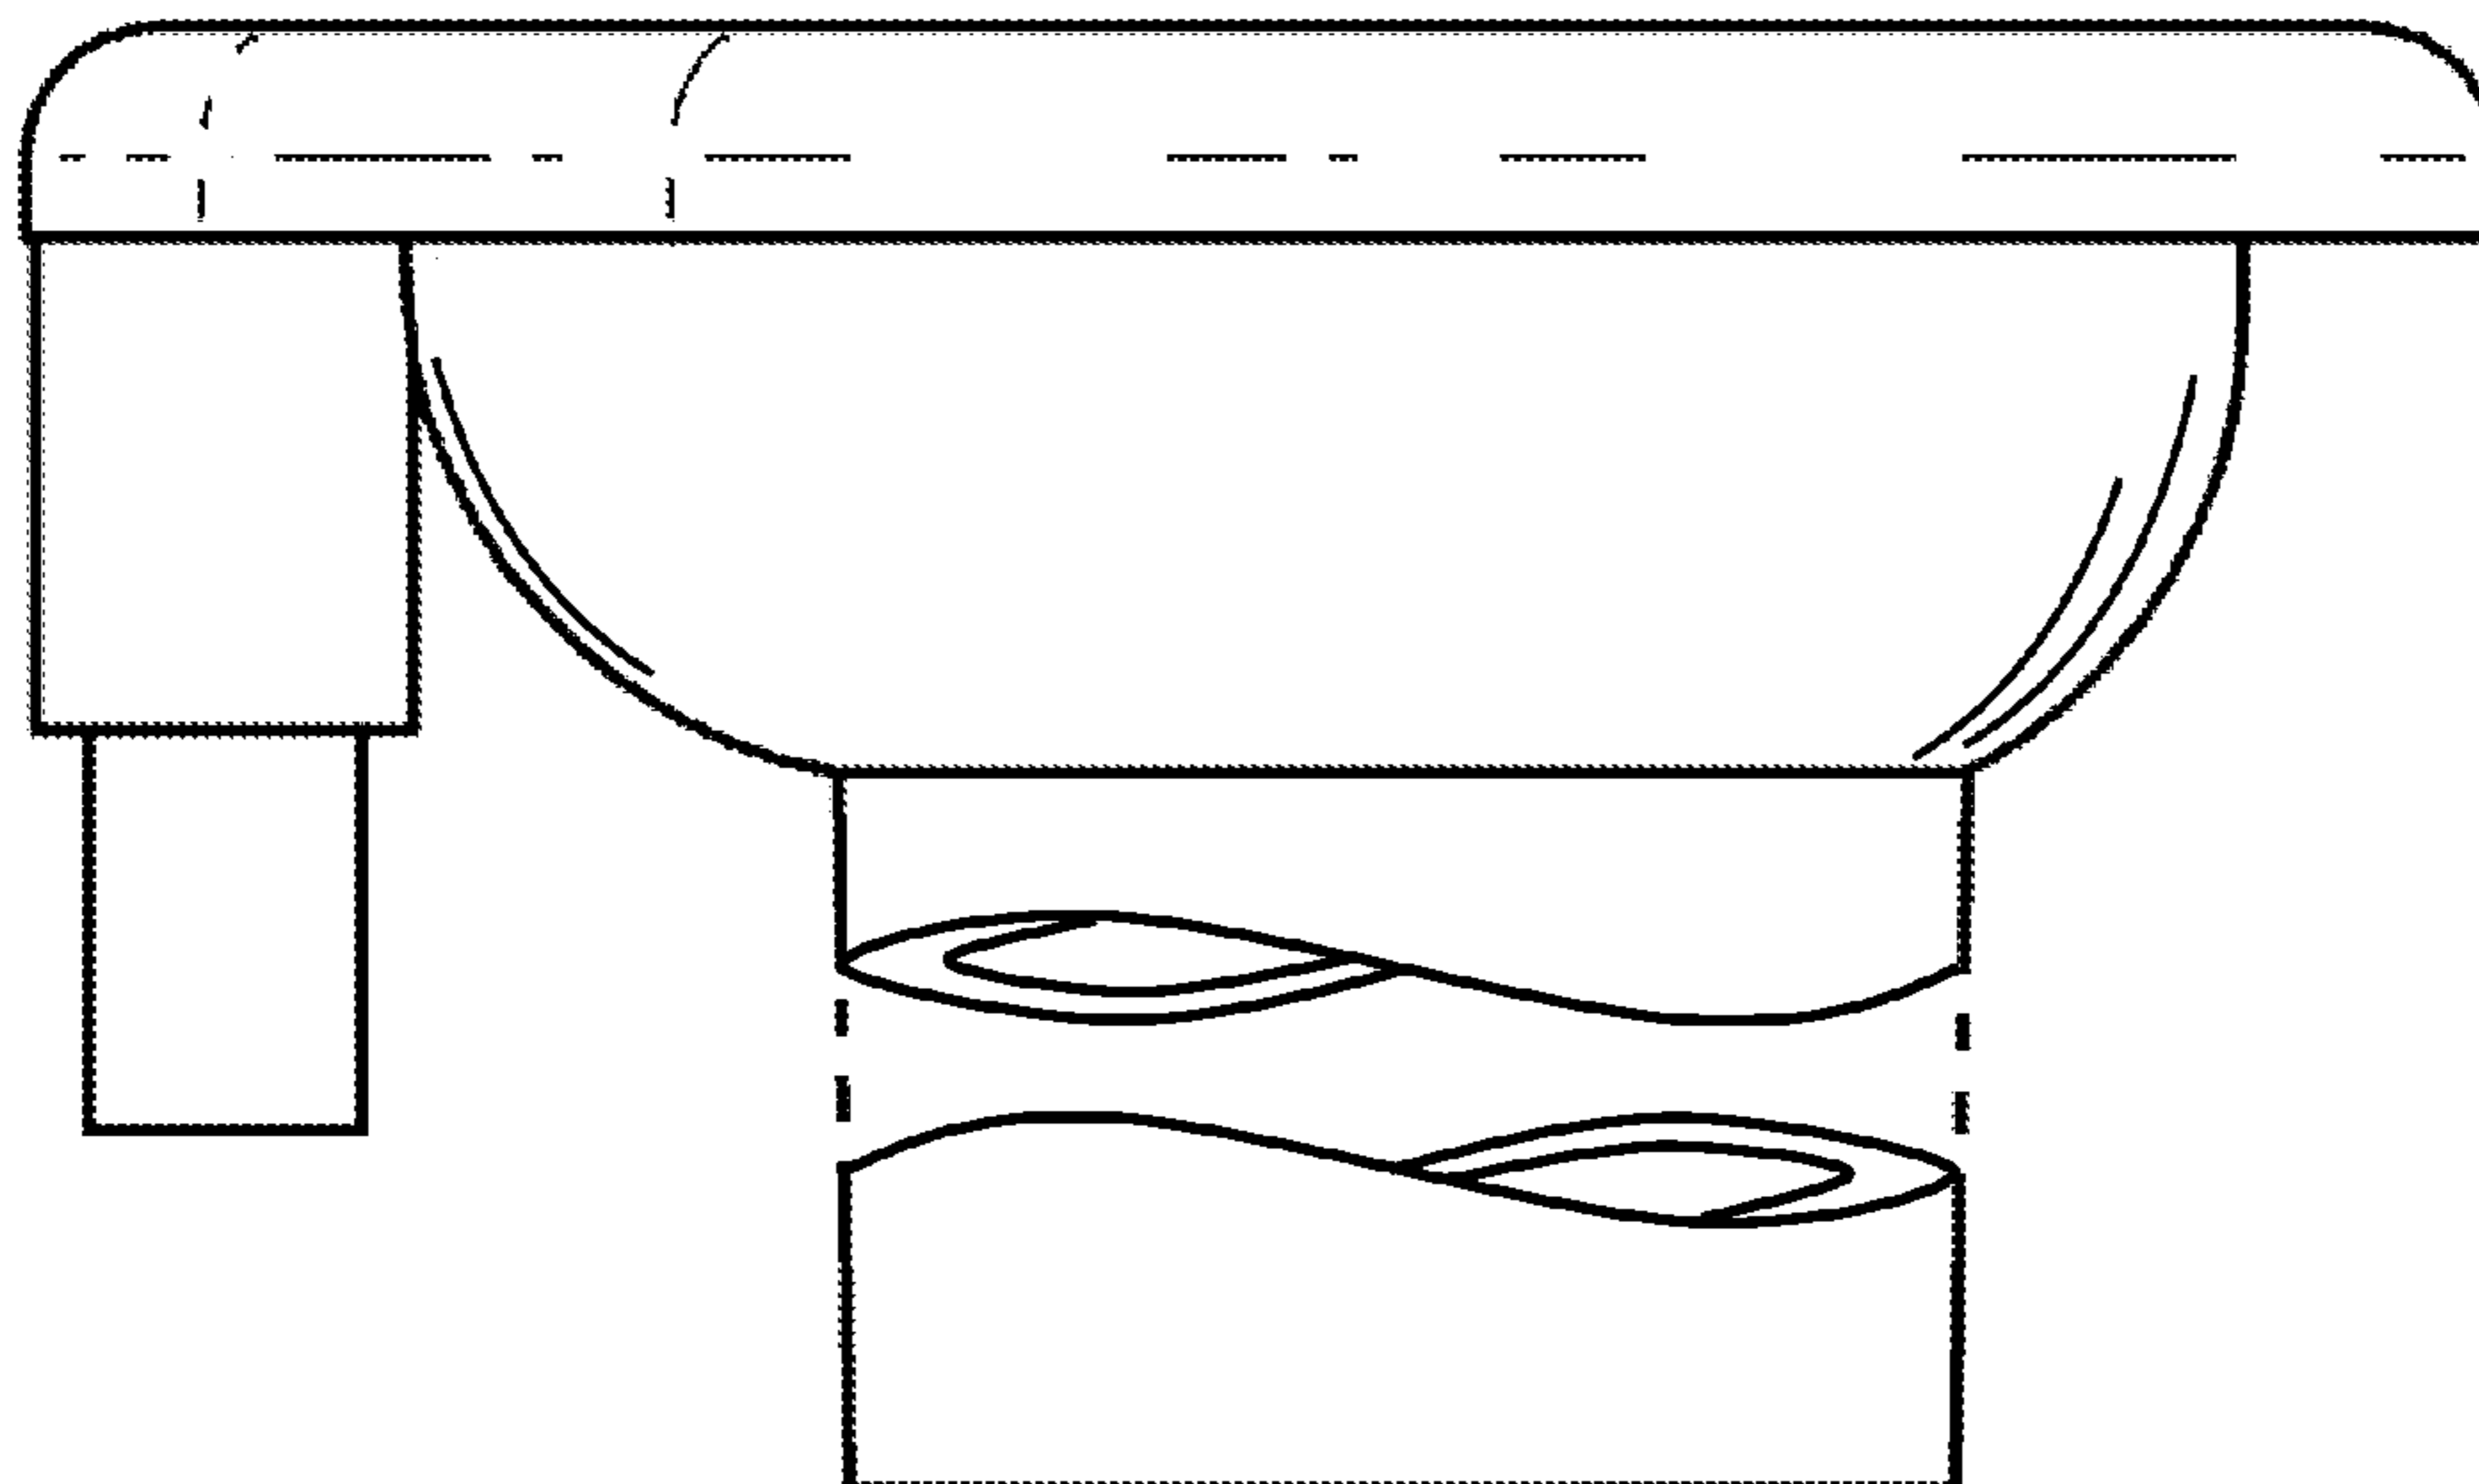

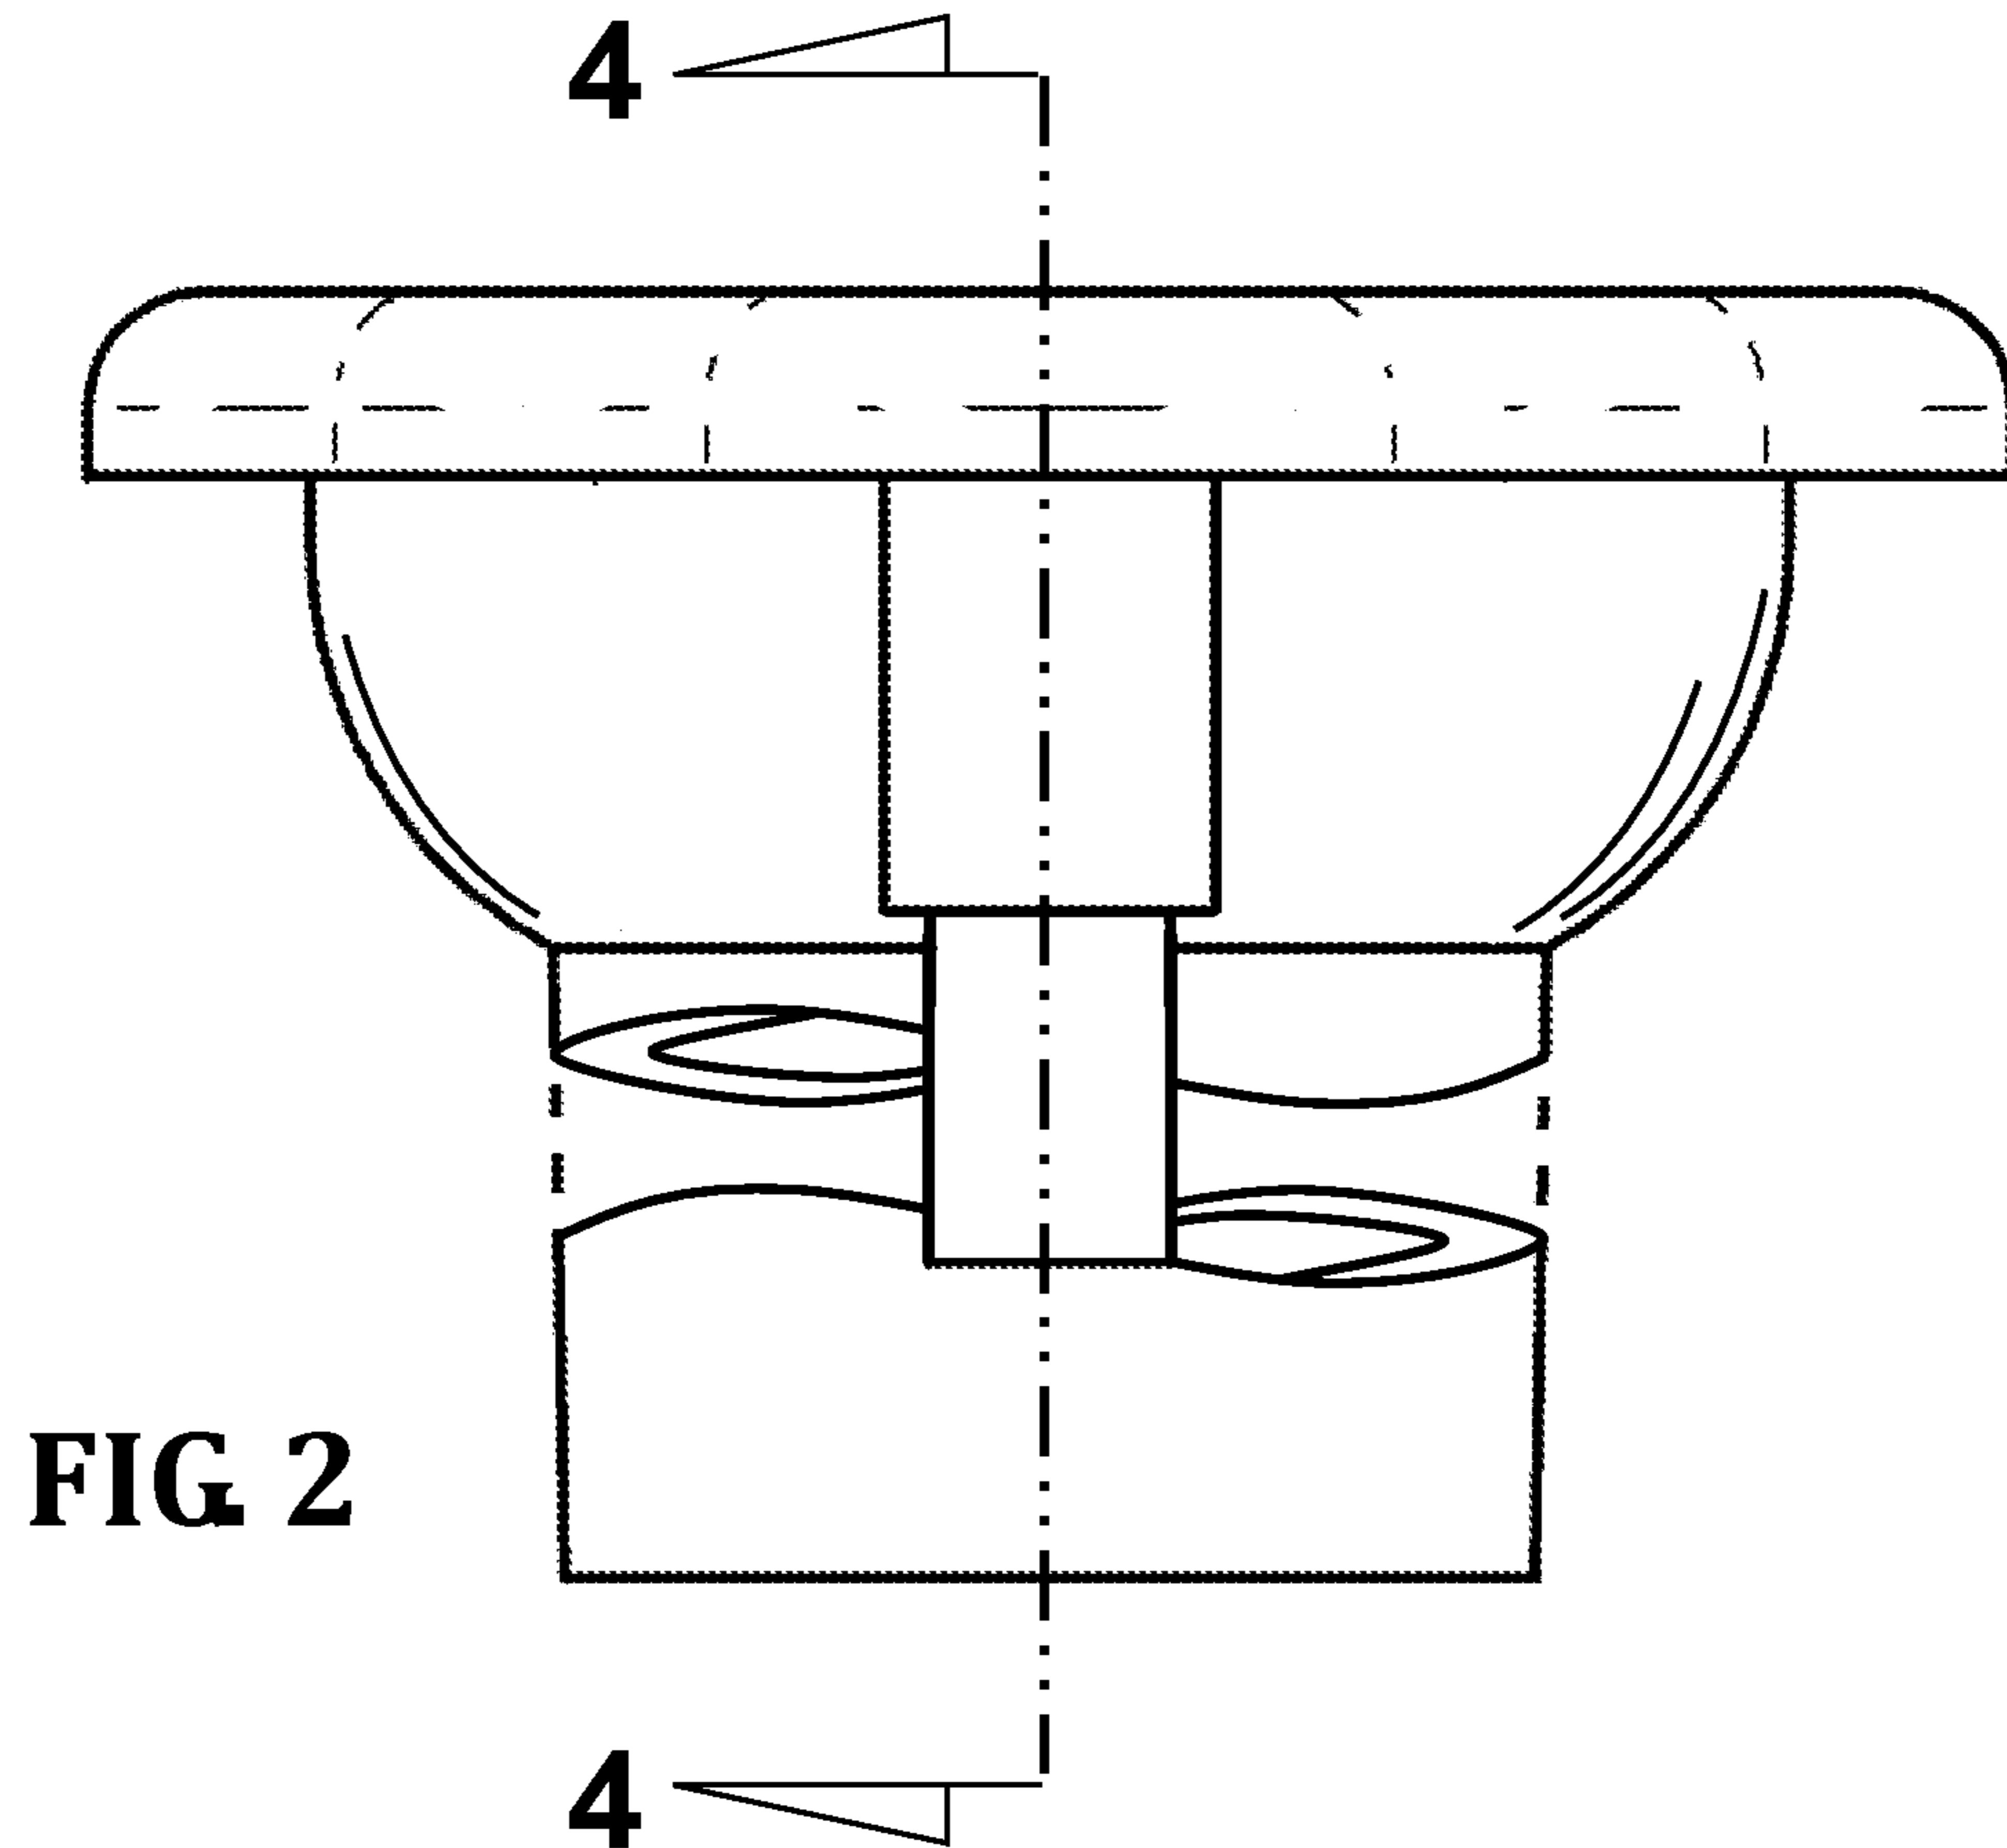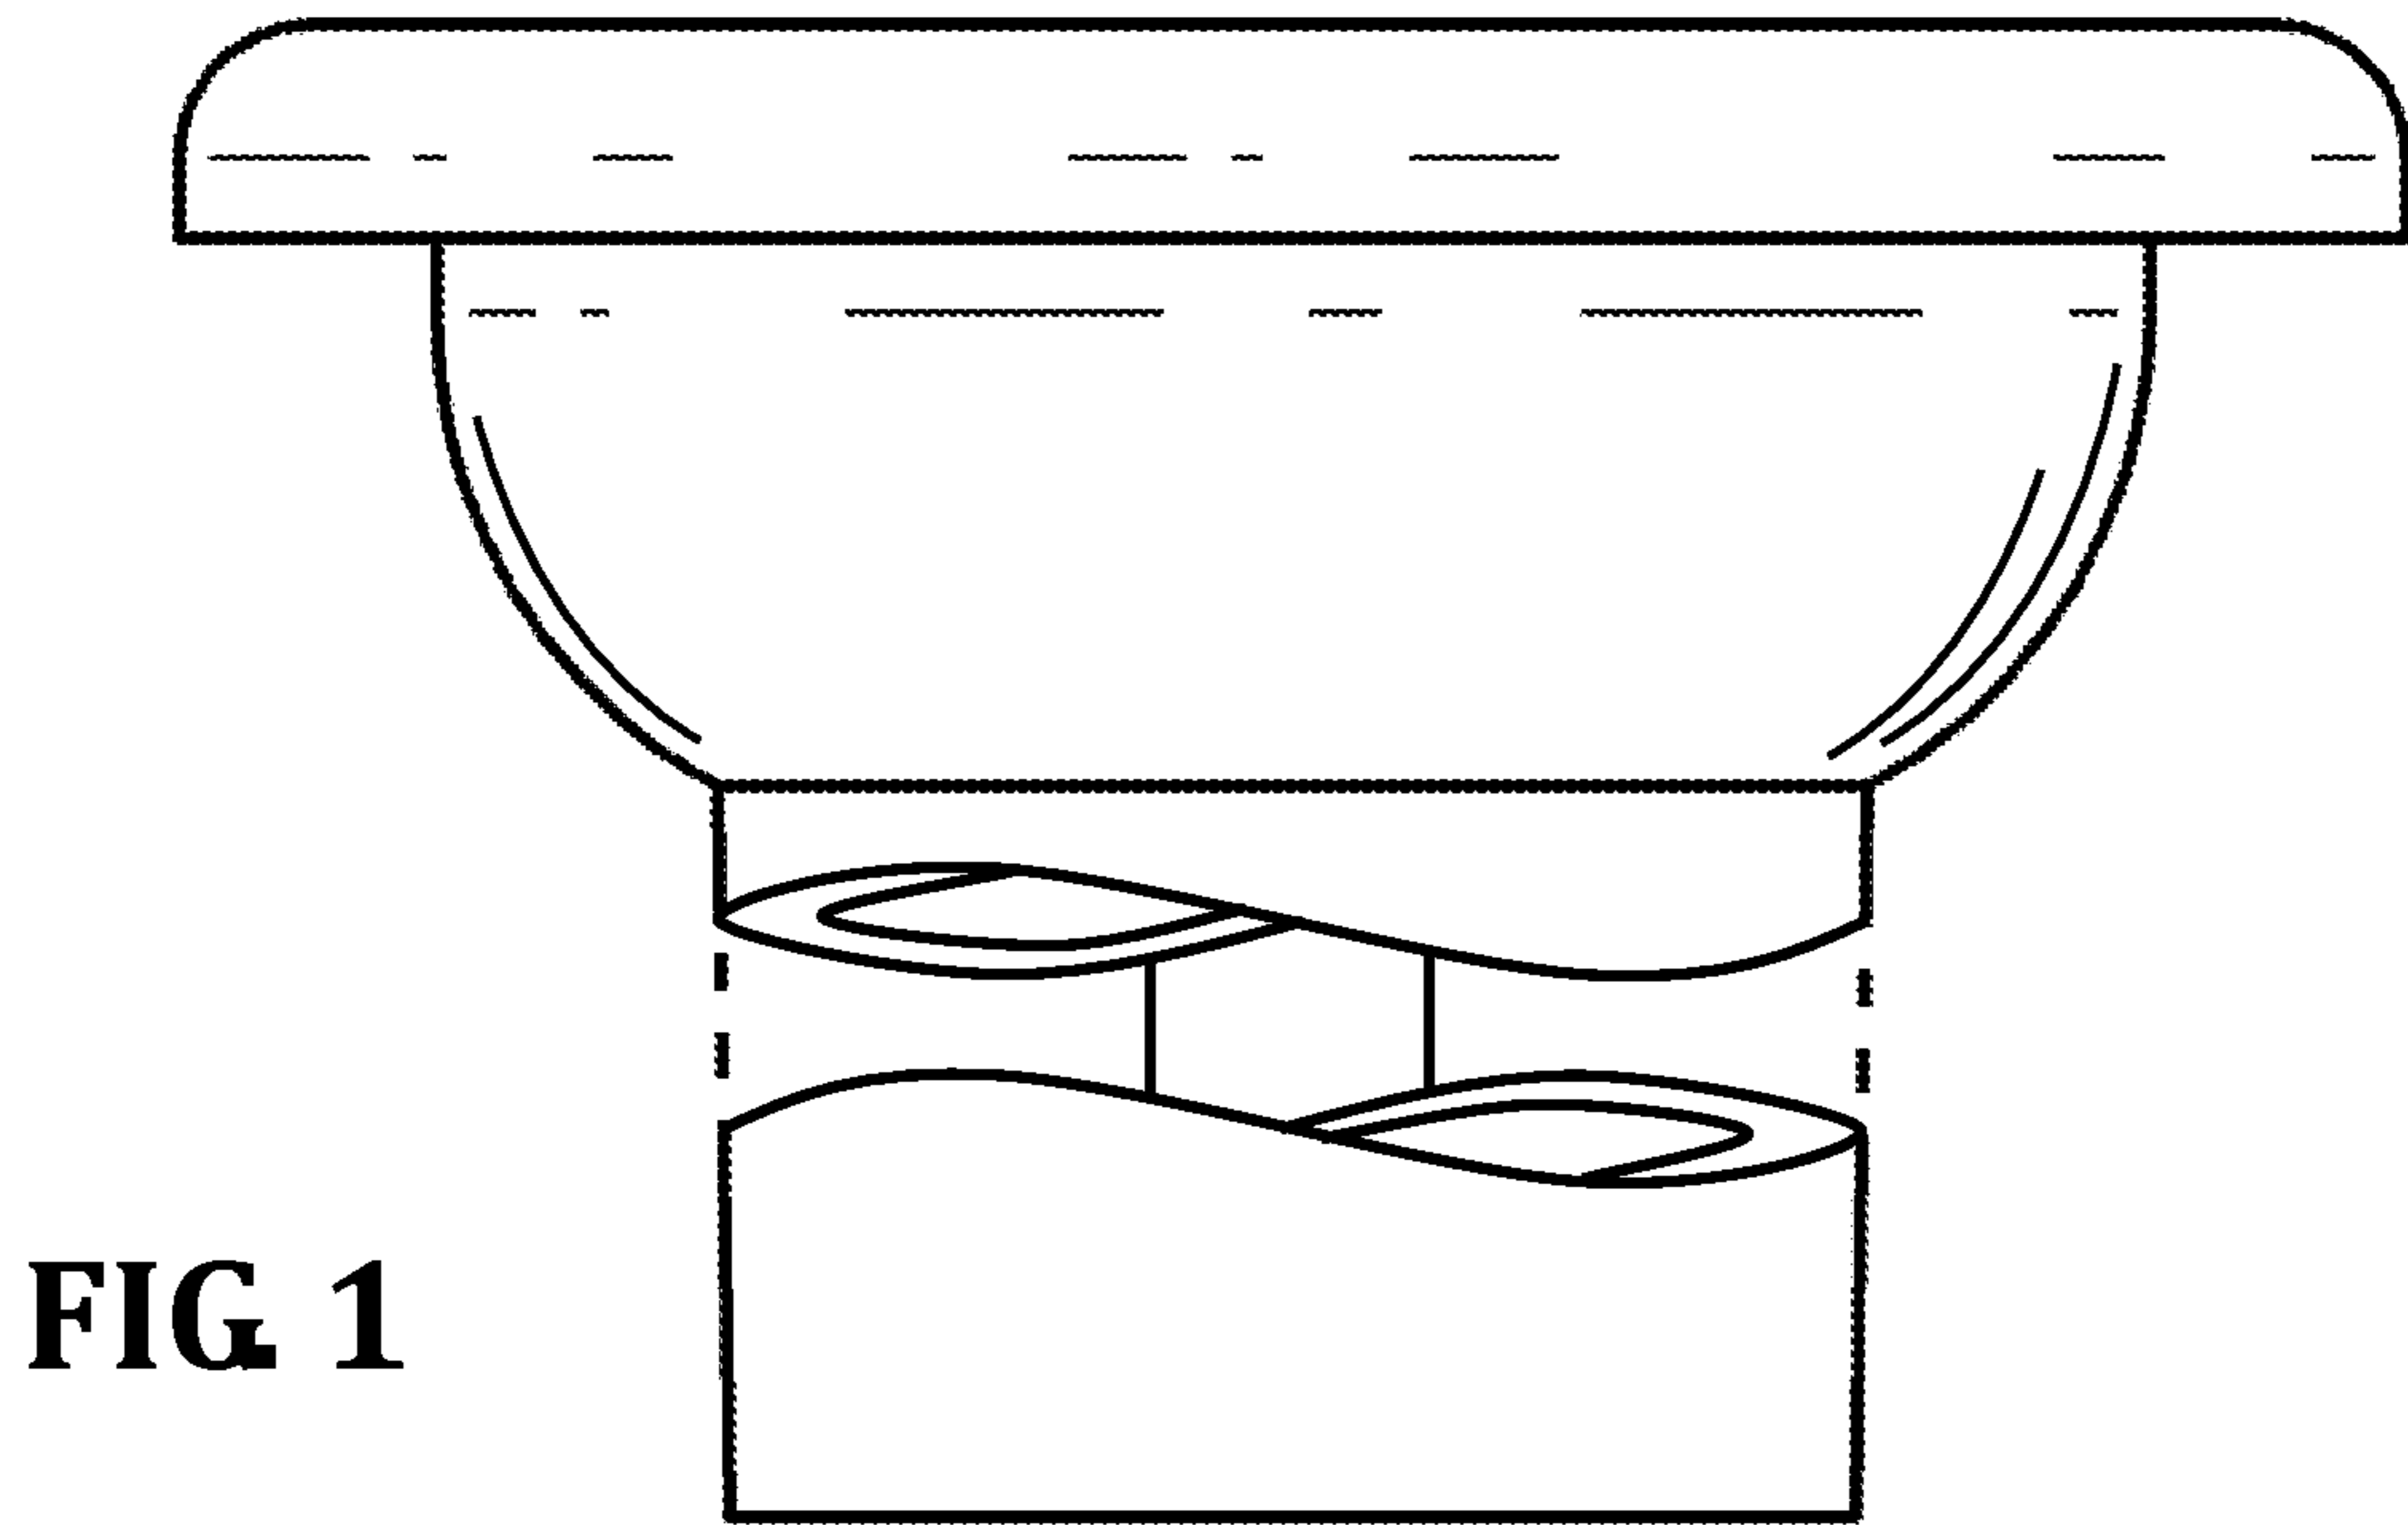


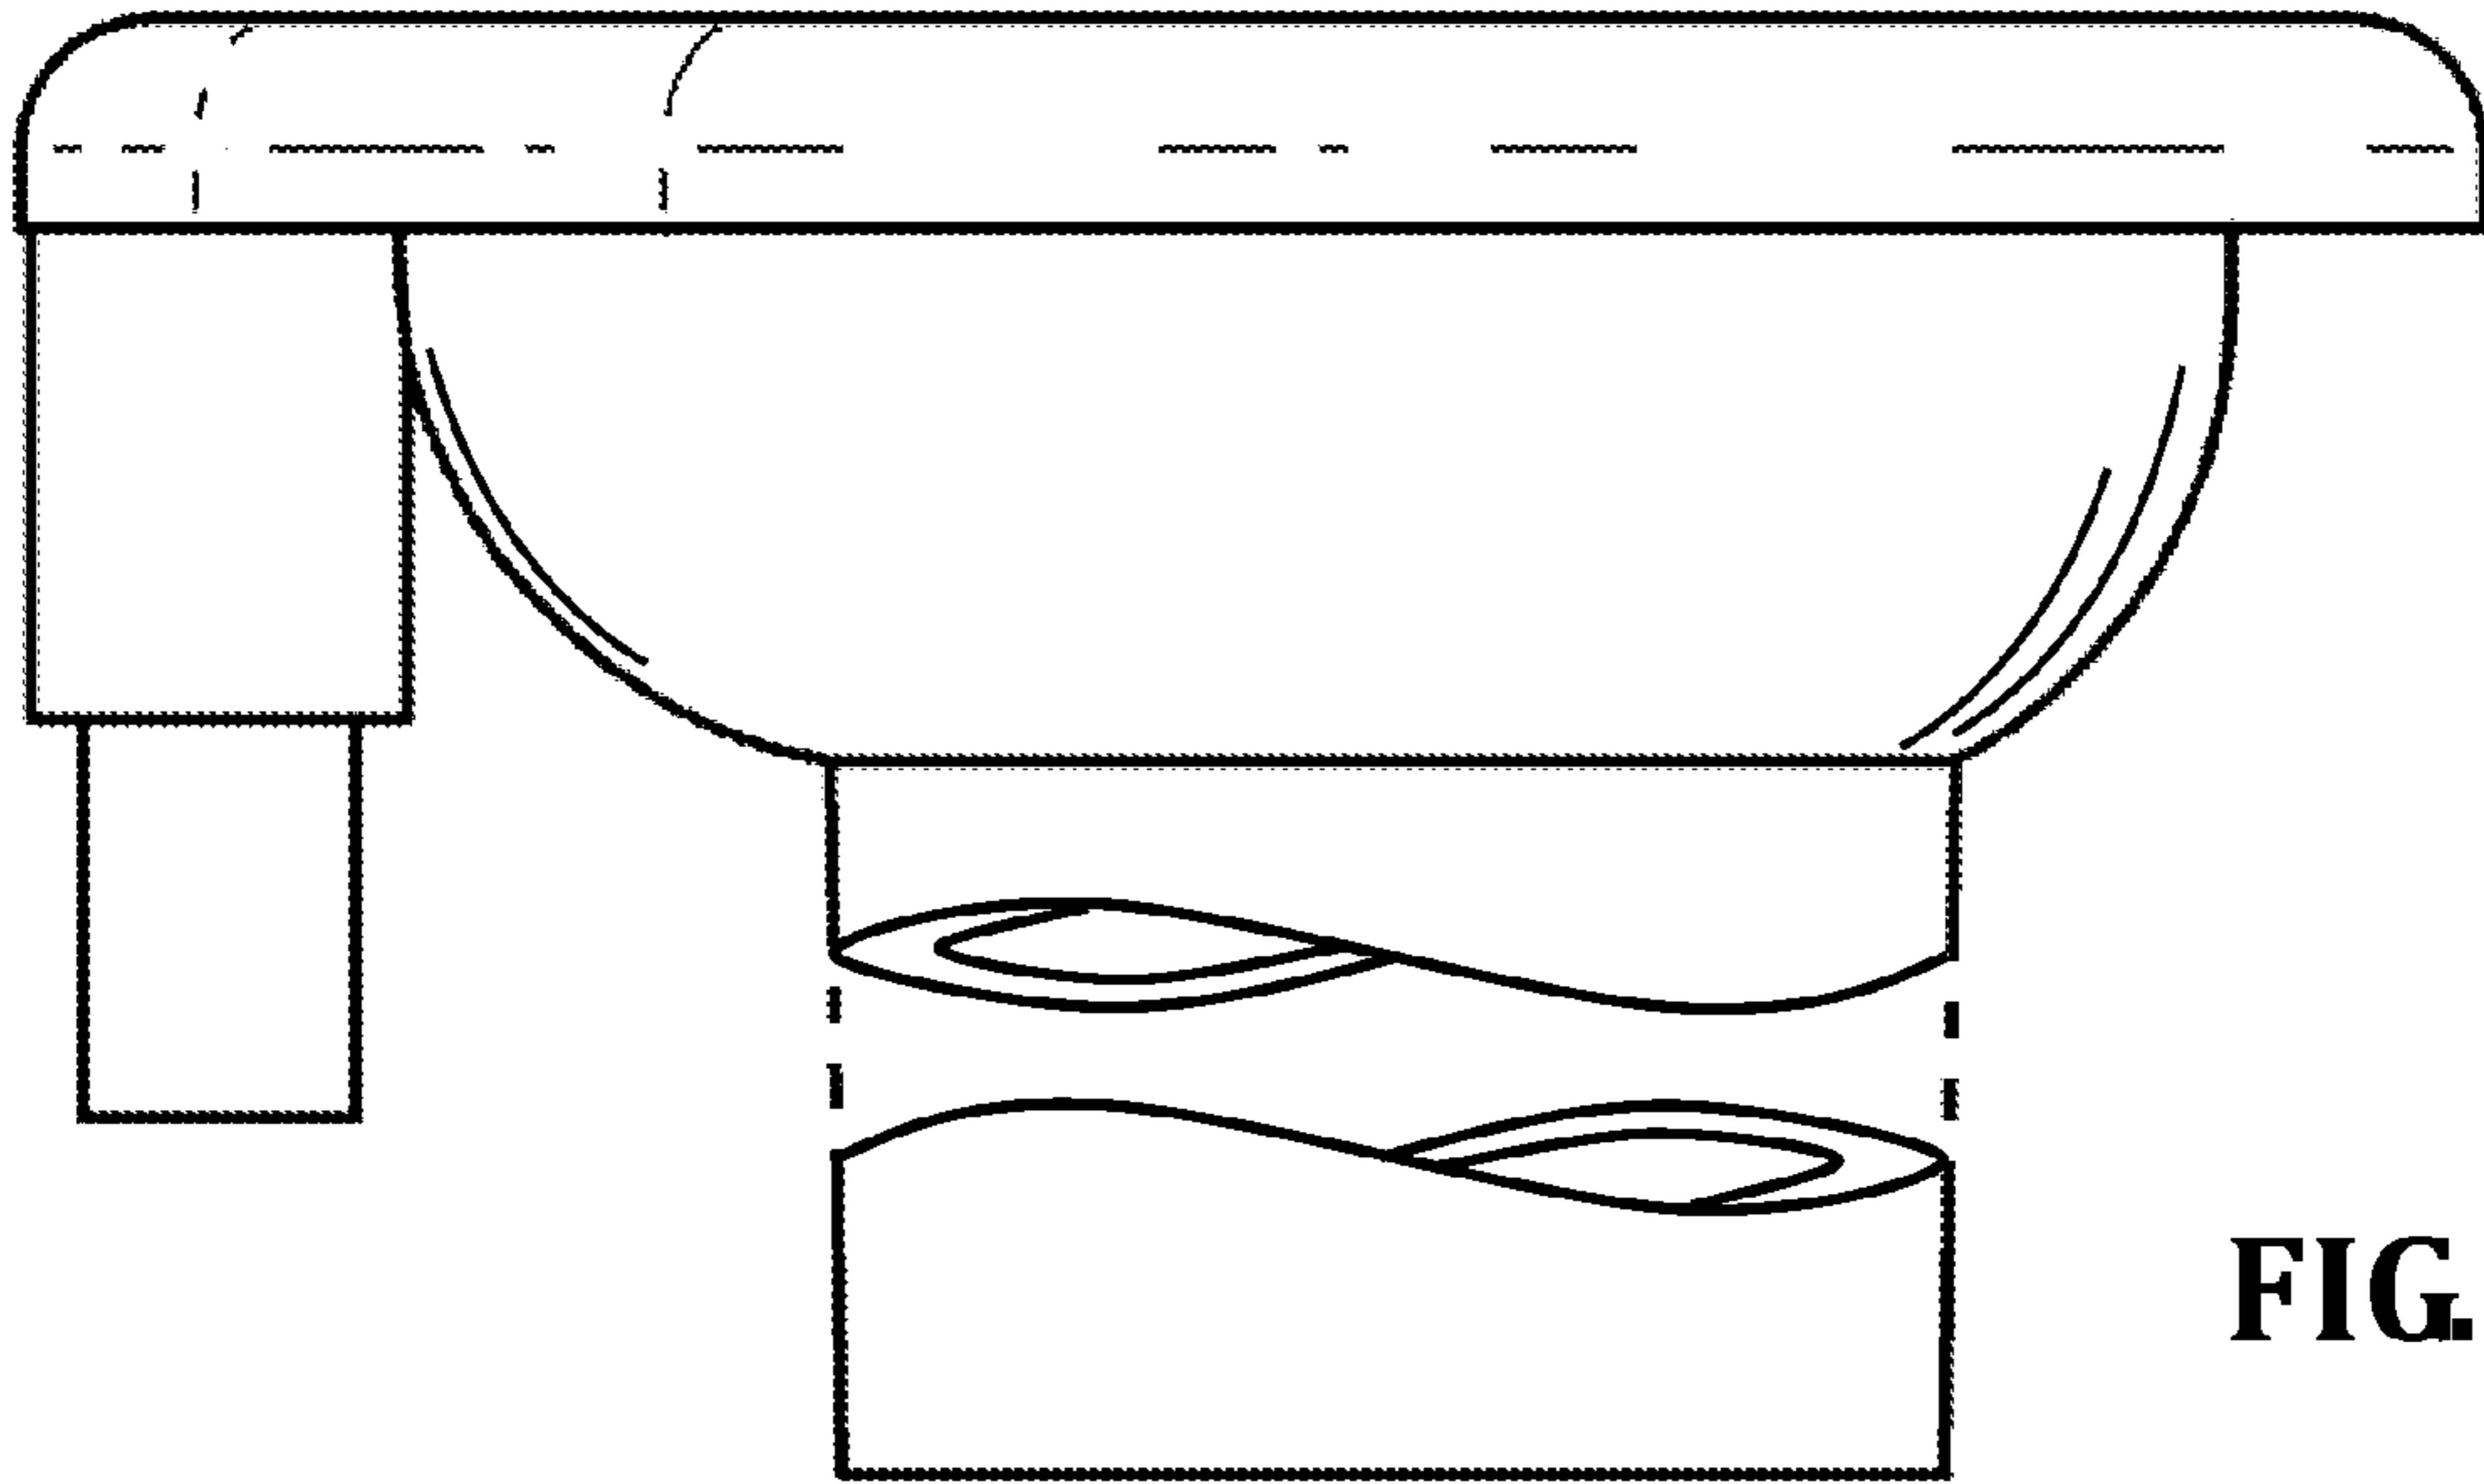


**FIG. 3**

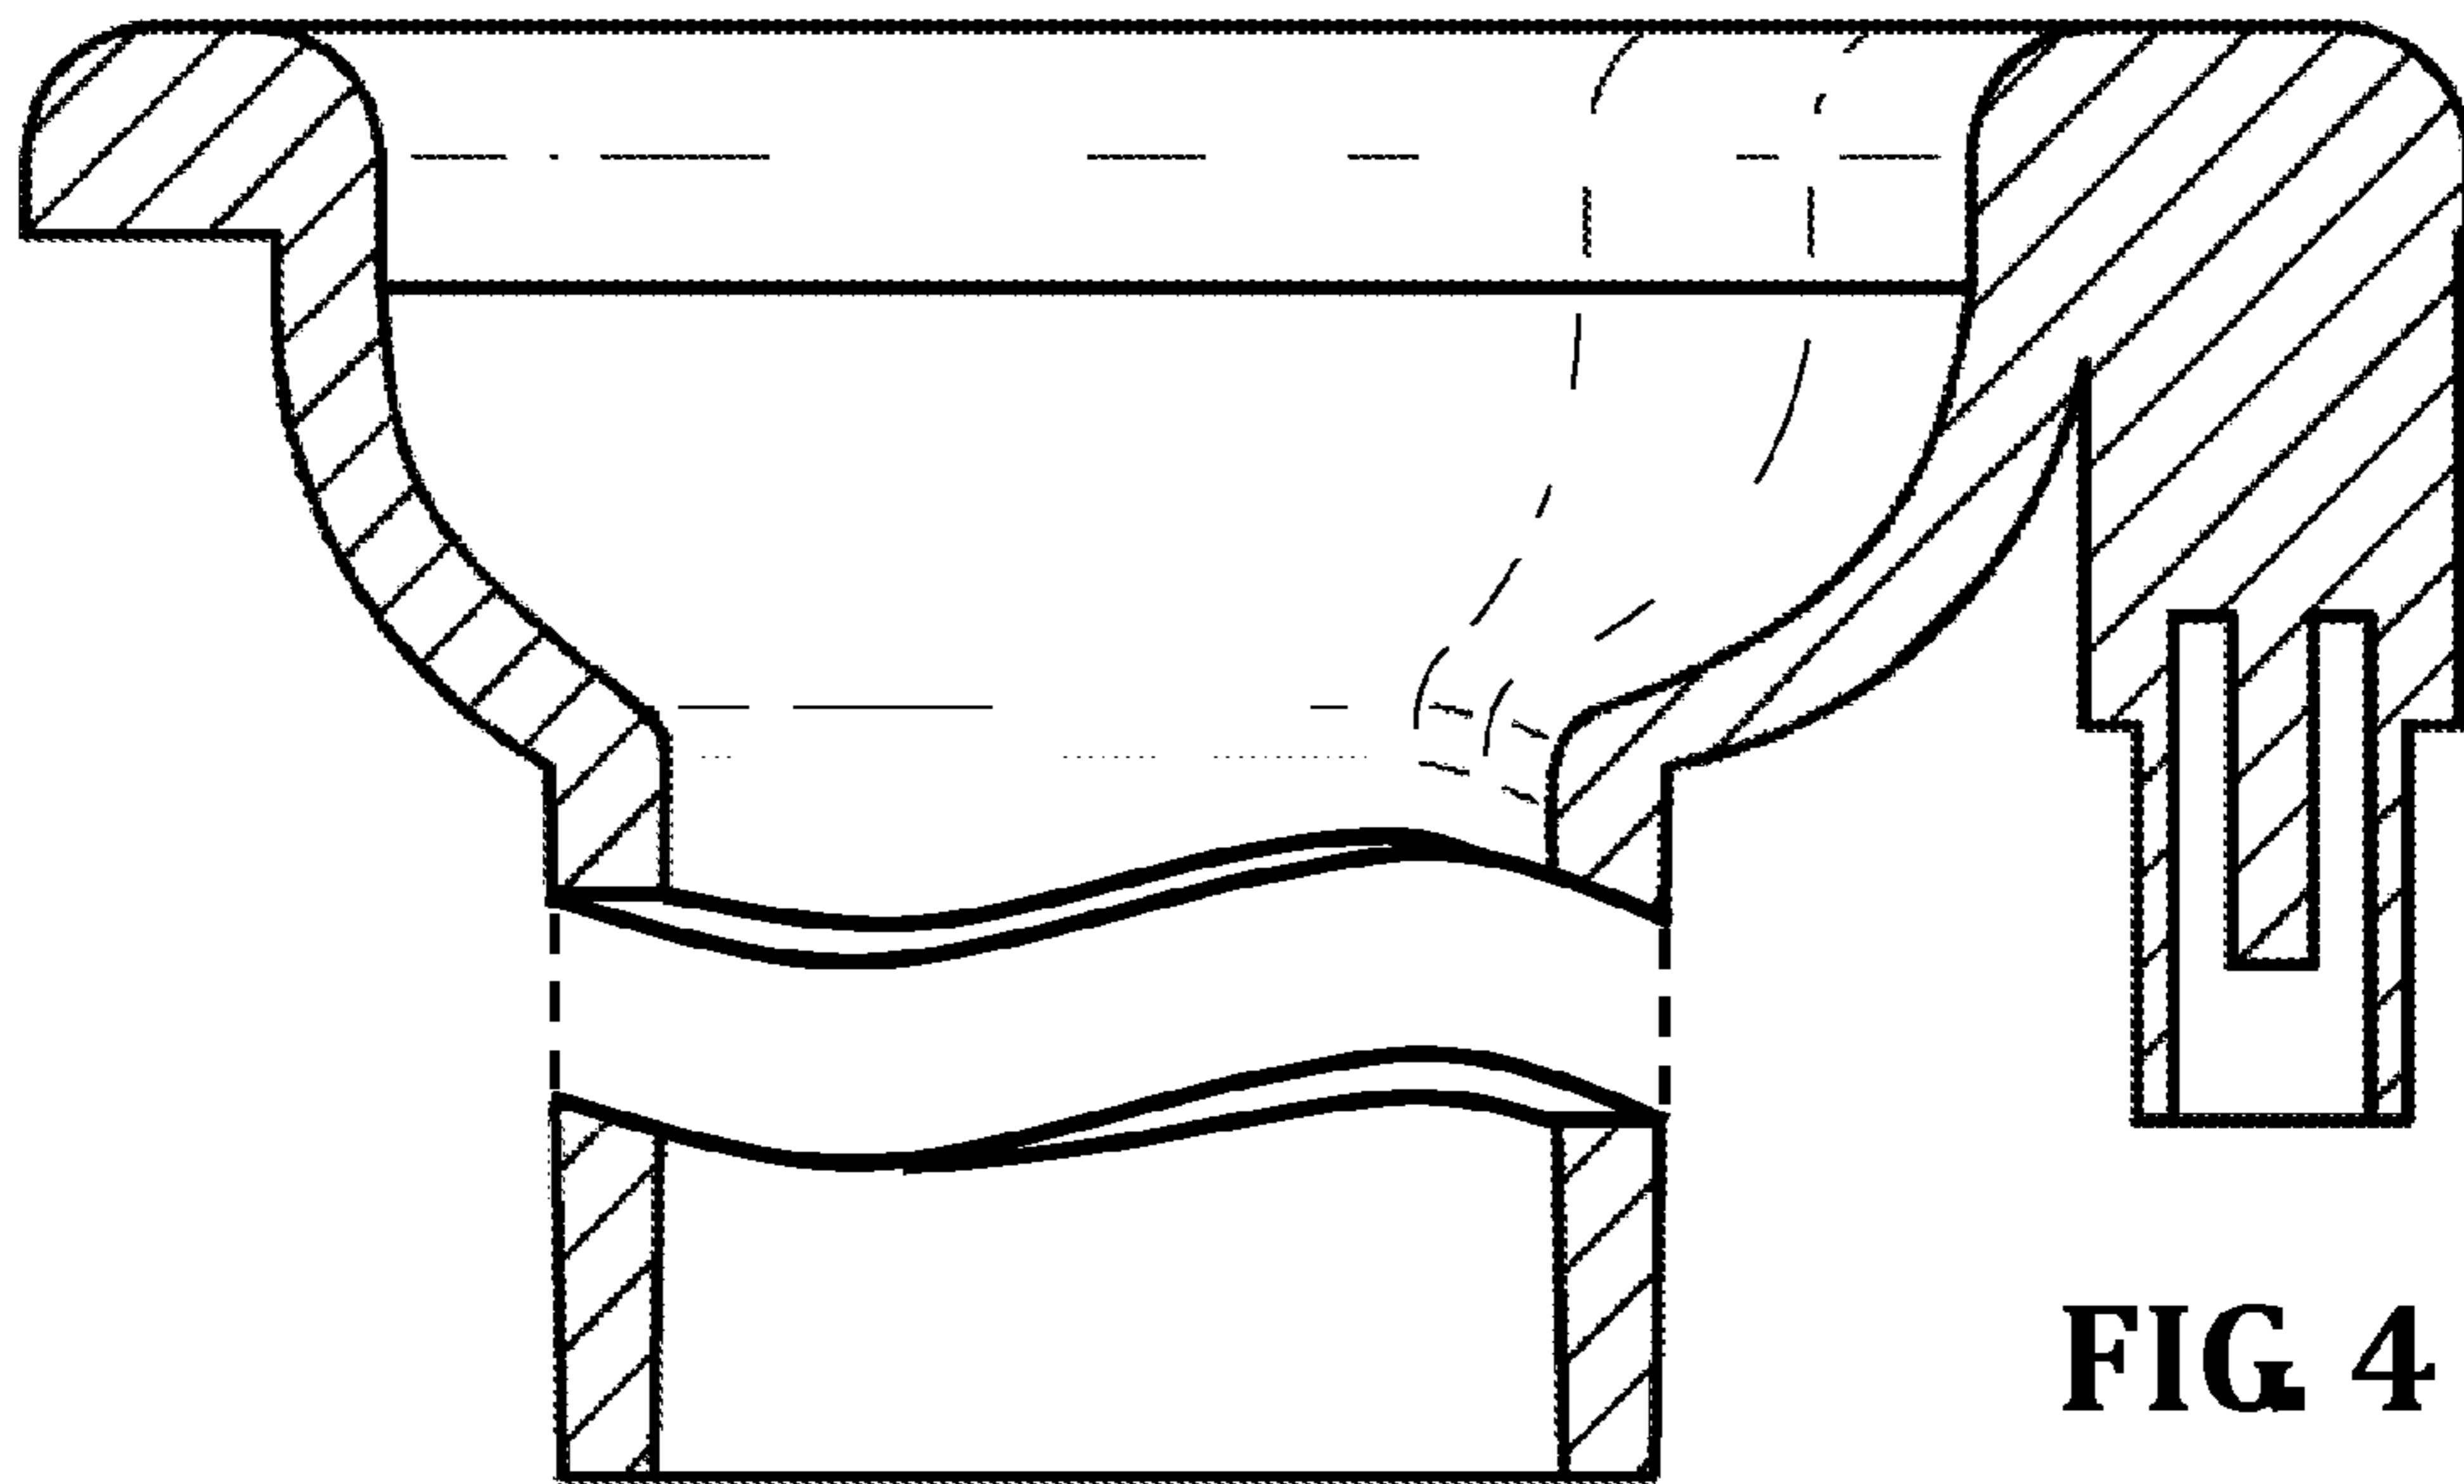

**FIG. 4**

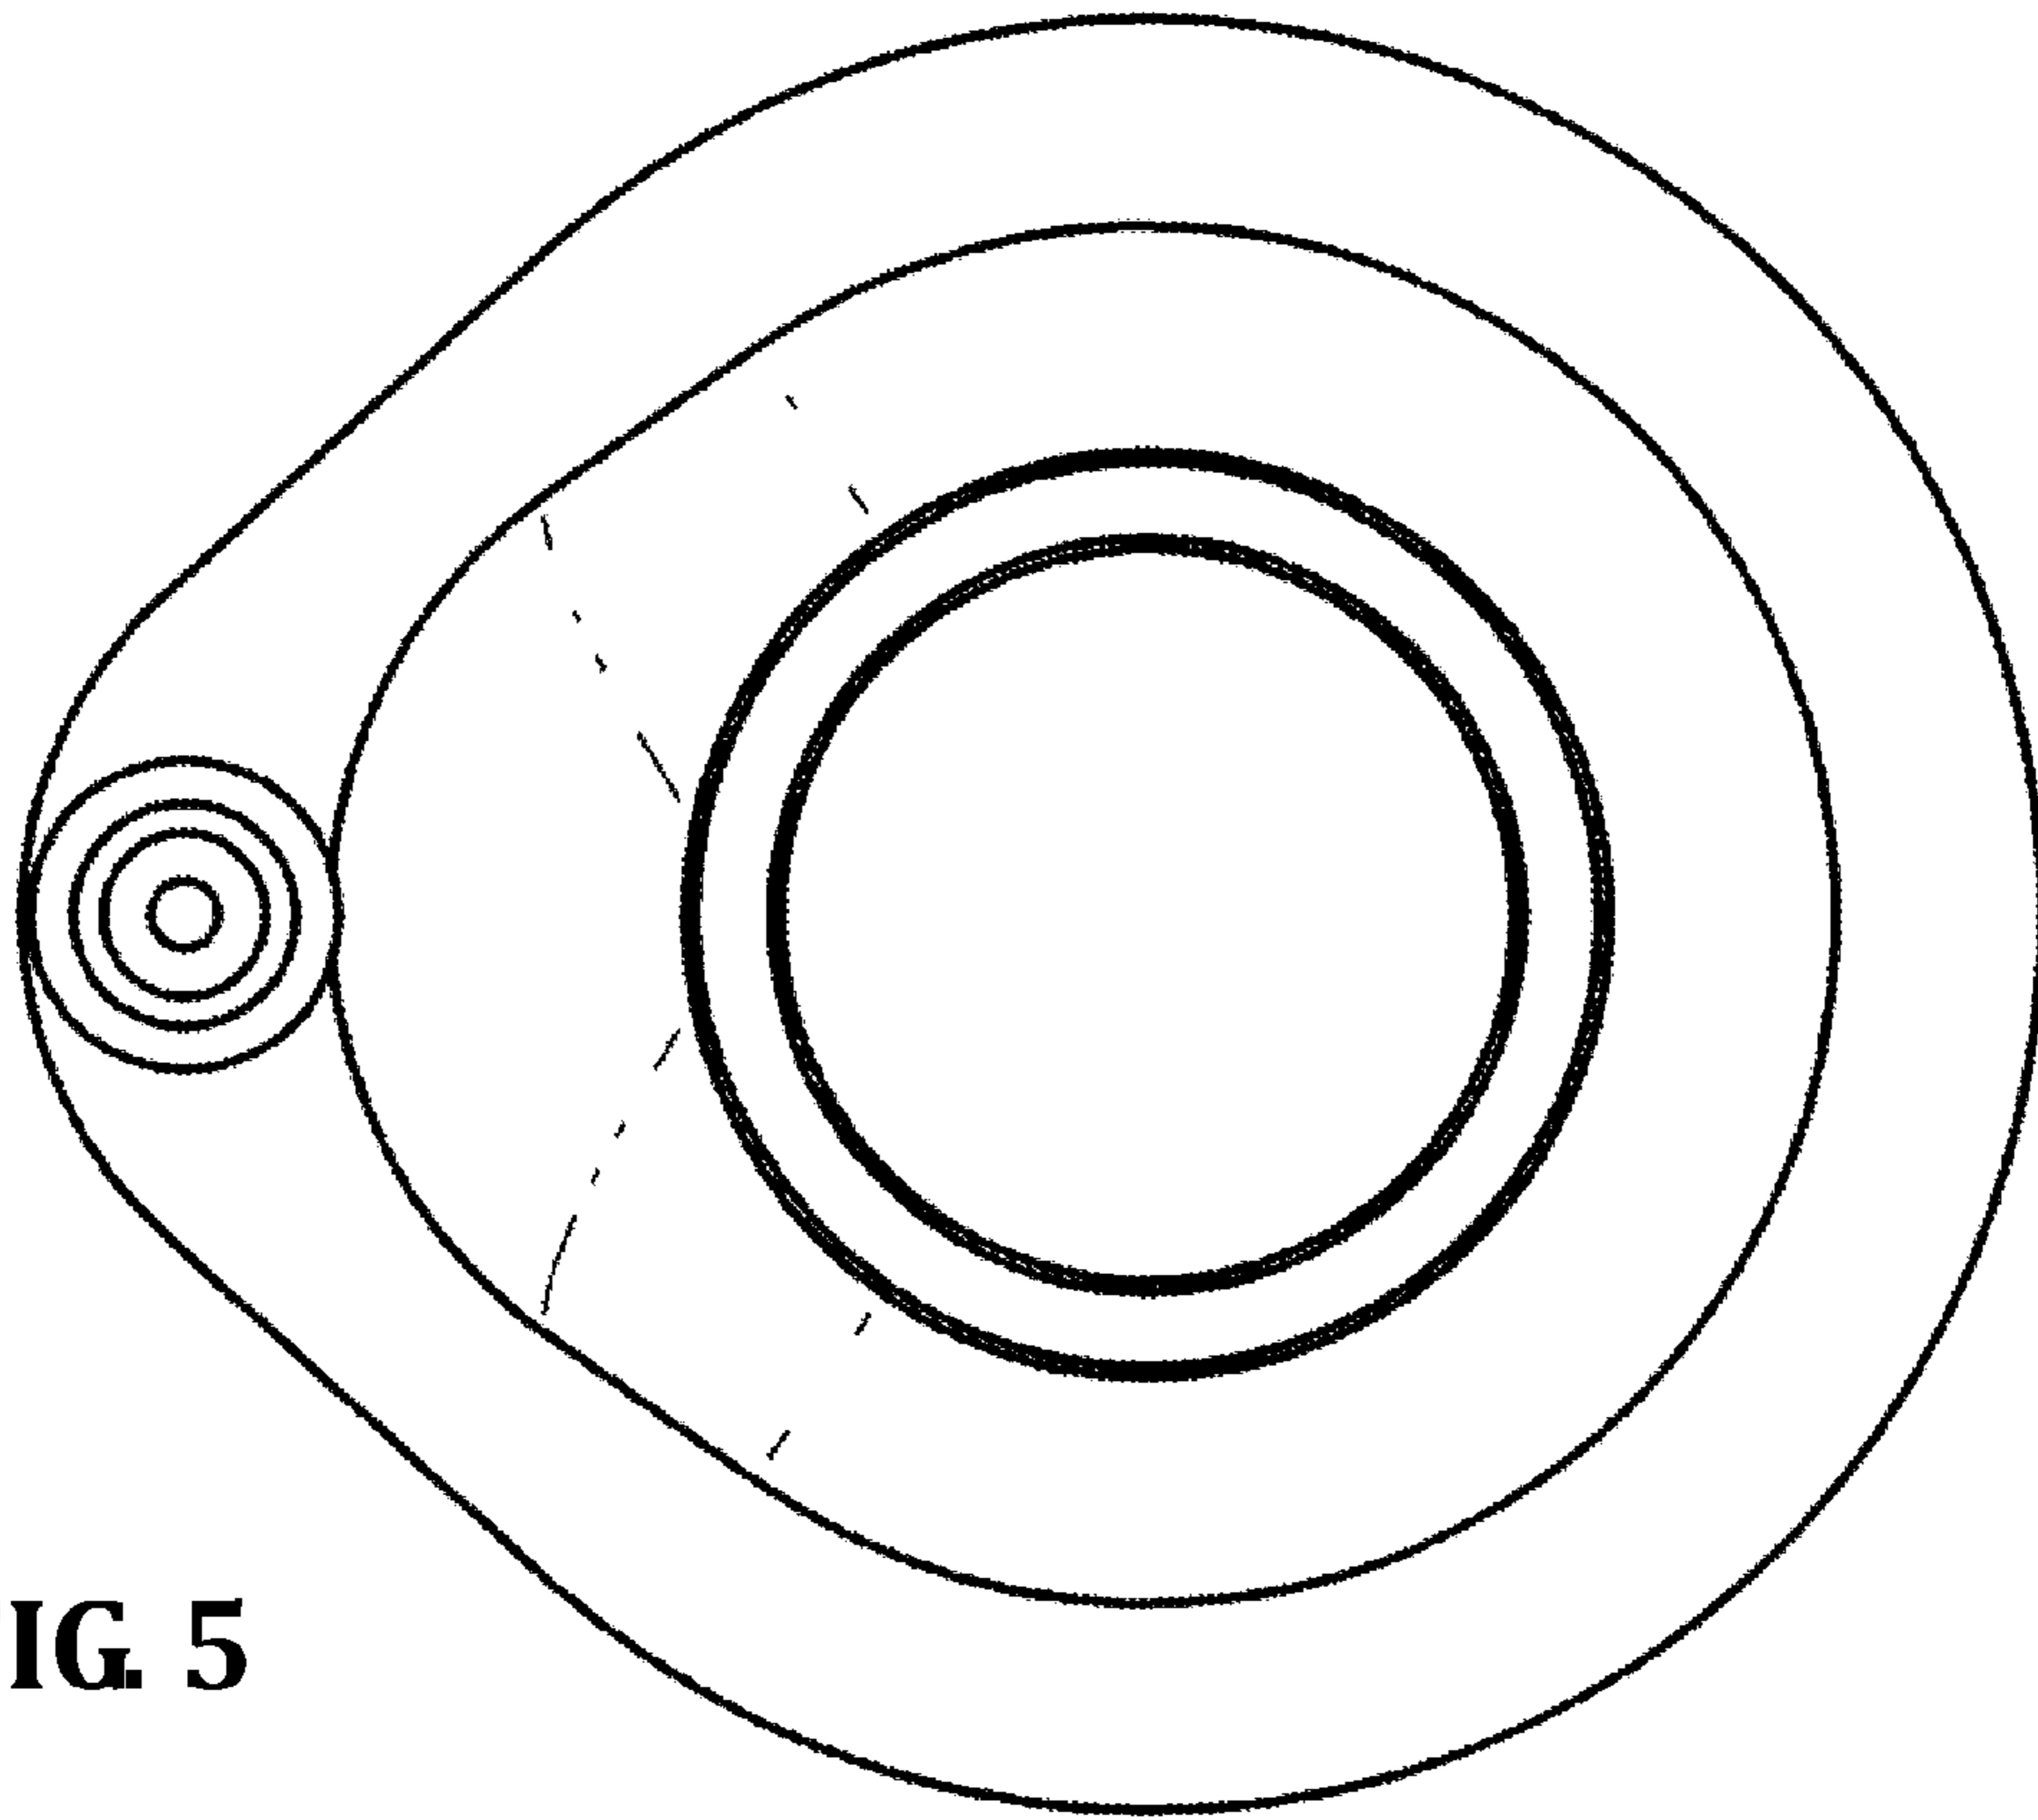

**FIG. 5**

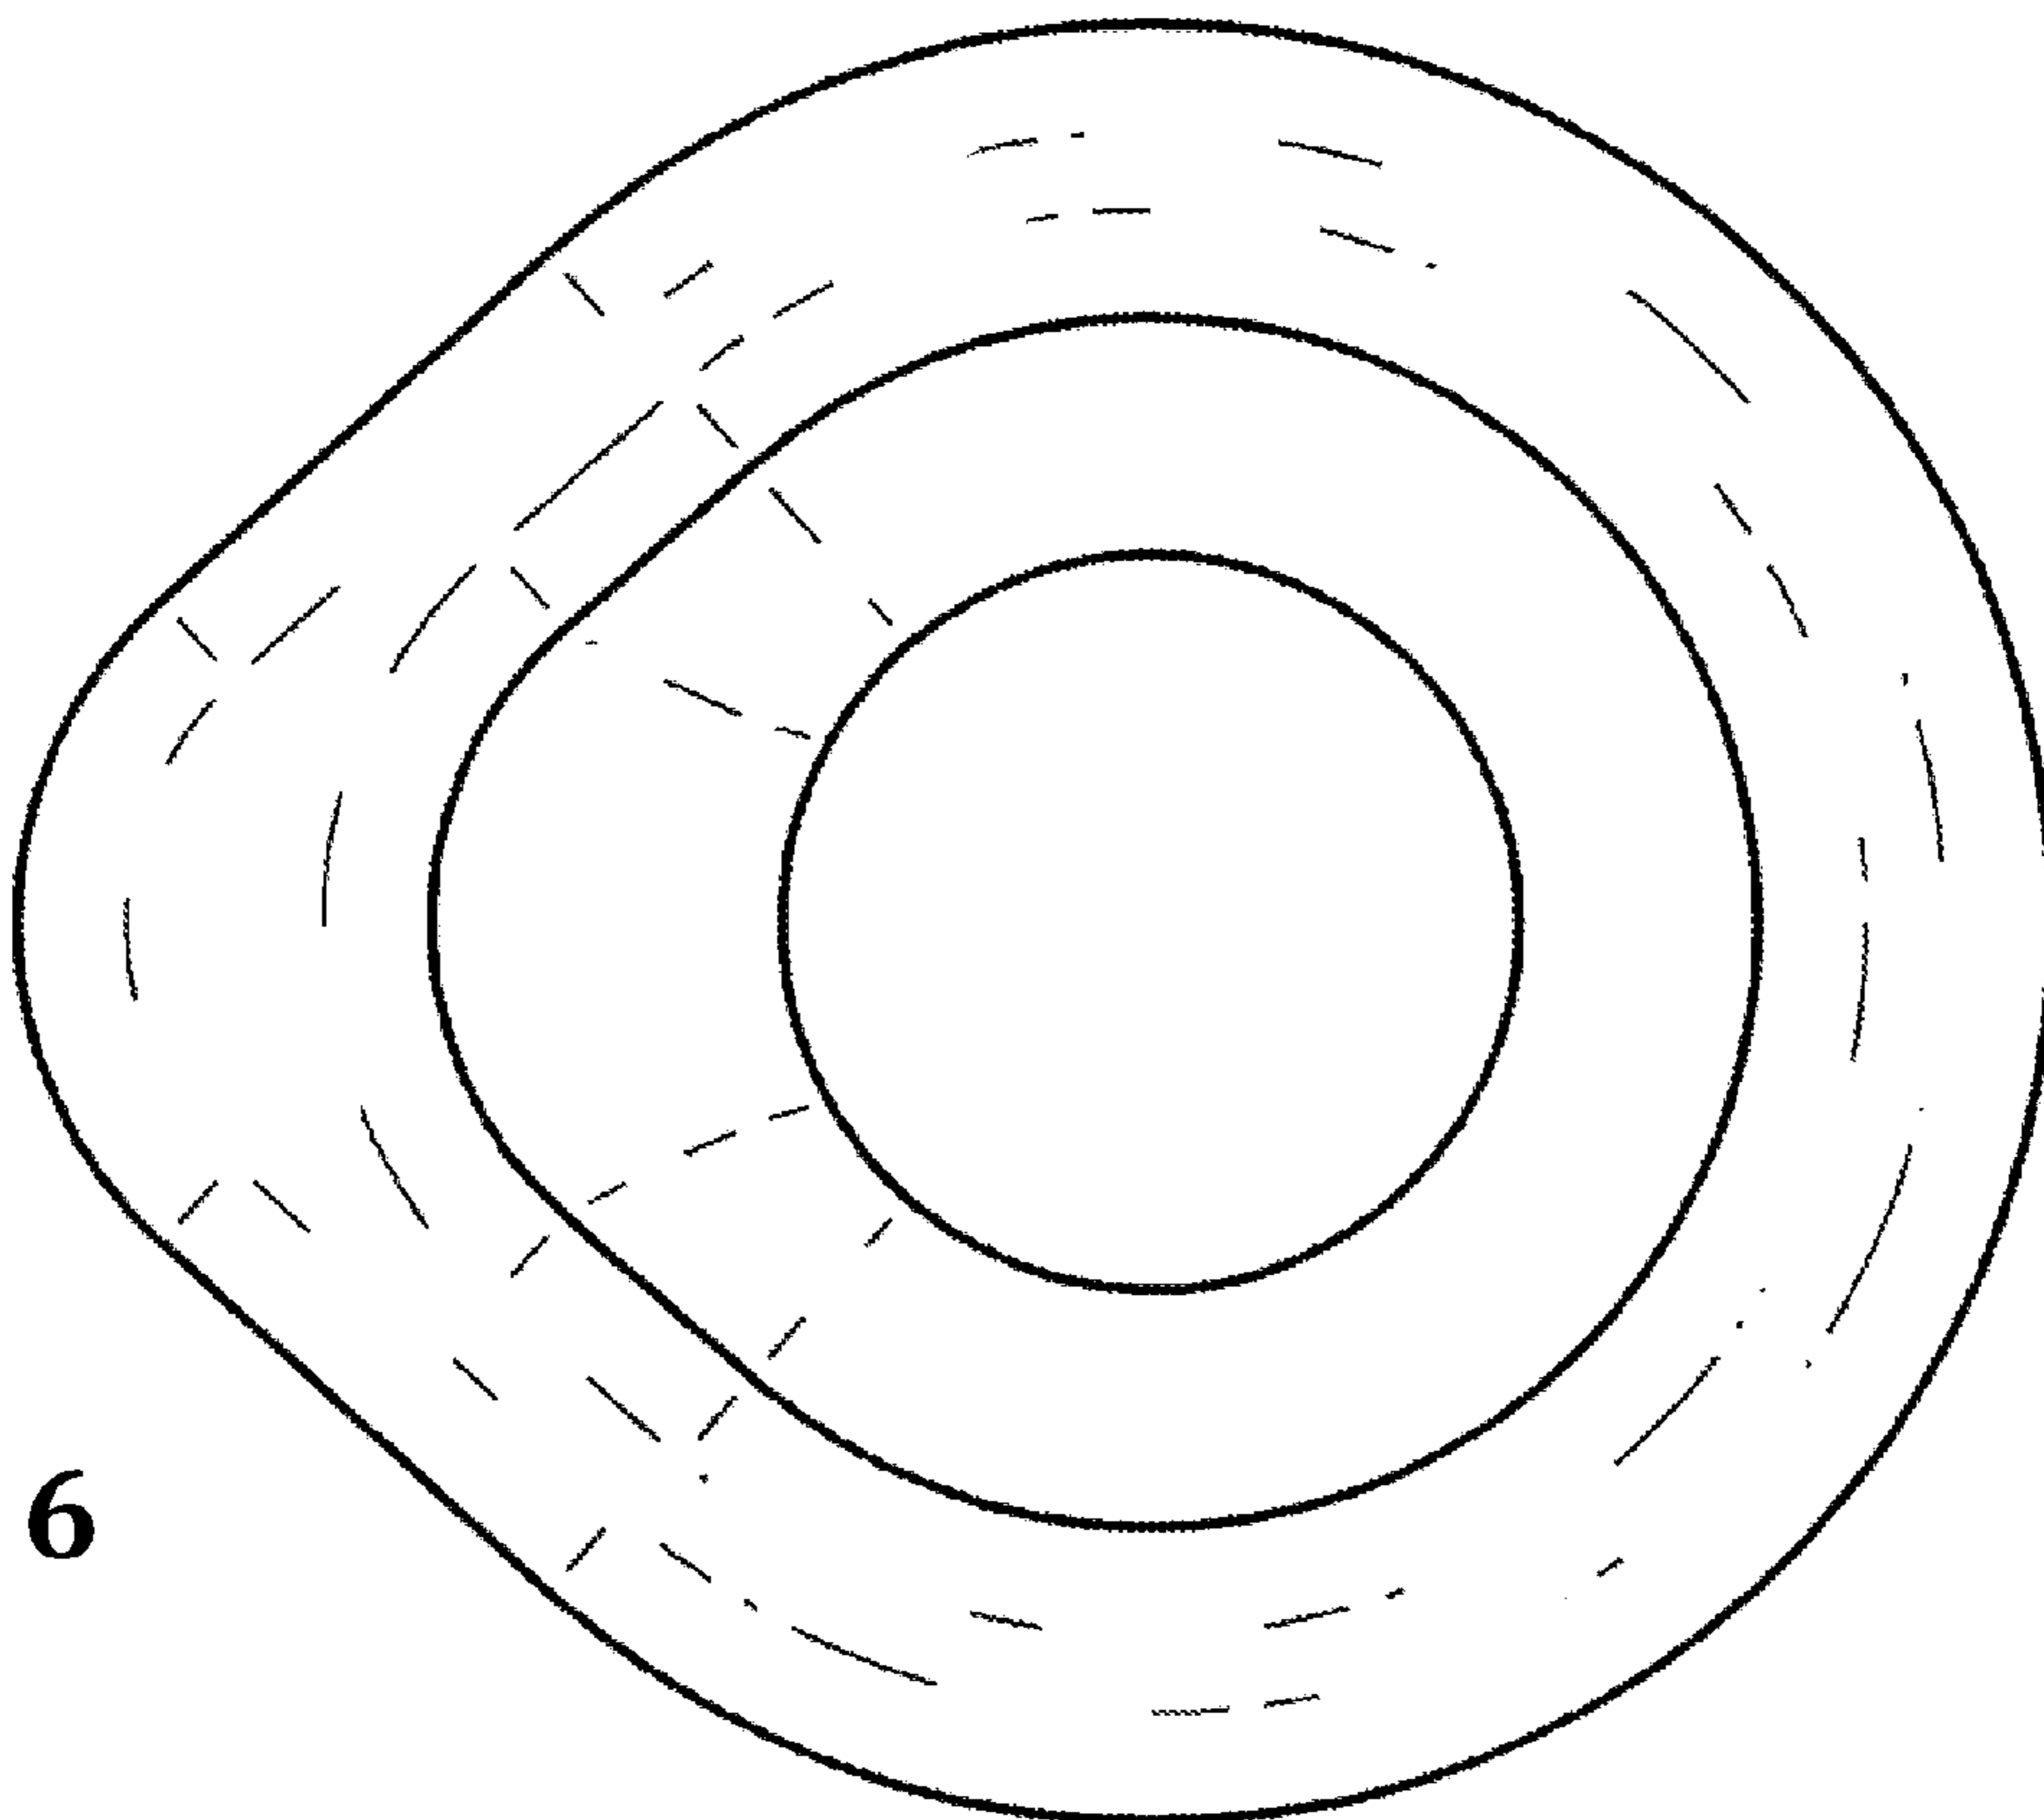

**FIG. 6**