



US00D770617S

(12) **United States Design Patent** (10) **Patent No.:** **US D770,617 S**  
**Huang et al.** (45) **Date of Patent:** **\*\* Nov. 1, 2016**

(54) **ENDOSCOPE SYSTEM WORKSTATION**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **OLYMPUS (BEIJING) SALES & SERVICE CO., LTD.**, Beijing (CN)

CN 201054478 4/2008  
CN 201353210 12/2009

(Continued)

(72) Inventors: **Xin Huang**, Beijing (CN); **Ye Hong**, Beijing (CN); **Junwei Xu**, Beijing (CN); **Han Xu**, Beijing (CN); **Tengfei Yang**, Beijing (CN)

OTHER PUBLICATIONS

United States Patent and Trademark Office, "Restriction Requirement," issued in connection with U.S. Appl. No. 29/398,222, on Nov. 16, 2012 (5 pages).

(Continued)

(73) Assignee: **OLYMPUS (BEIJING) SALES SERVICE CO., LTD.**, Beijing (CN)

(\*\*) Term: **14 Years**

*Primary Examiner* — Wan Laymon  
*Assistant Examiner* — Mark Booker

(21) Appl. No.: **29/509,378**

(74) *Attorney, Agent, or Firm* — Hanley, Flight & Zimmerman, LLC

(22) Filed: **Nov. 17, 2014**

(30) **Foreign Application Priority Data**

May 19, 2014 (CN) ..... 2014 3 0137803

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/138**

(58) **Field of Classification Search**  
USPC ..... D24/130, 143, 150, 164, 170, 171, 172, D24/177, 183, 185, 186, 188, 190, 221, D24/234; 351/206, 224, 226; D6/559, 567  
CPC ..... A61B 6/12; A61B 8/12  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D264,873 S \* 6/1982 Olson ..... D10/81  
D369,564 S \* 5/1996 Whitby ..... D10/81  
D395,085 S 6/1998 Kenley et al.  
D528,216 S 9/2006 Korner  
D563,115 S 3/2008 Atkins  
D628,701 S 12/2010 Nordgren et al.  
D631,551 S 1/2011 Nordgren et al.  
D662,208 S \* 6/2012 Otoha ..... D24/185

(Continued)


(57) **CLAIM**

The ornamental design for an "endoscope system workstation," as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of an endoscope system workstation. FIG. 2 is a rear view of the endoscope system workstation of FIG. 1. FIG. 3 is a left side view of the endoscope system workstation of FIG. 1. FIG. 4 is a right side view of the endoscope system workstation of FIG. 1. FIG. 5 is a top view of the endoscope system workstation of FIG. 1; and, FIG. 6 is a bottom view of the endoscope system workstation of FIG. 1. The broken lines in the figures represent portions of the endoscope system workstation that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

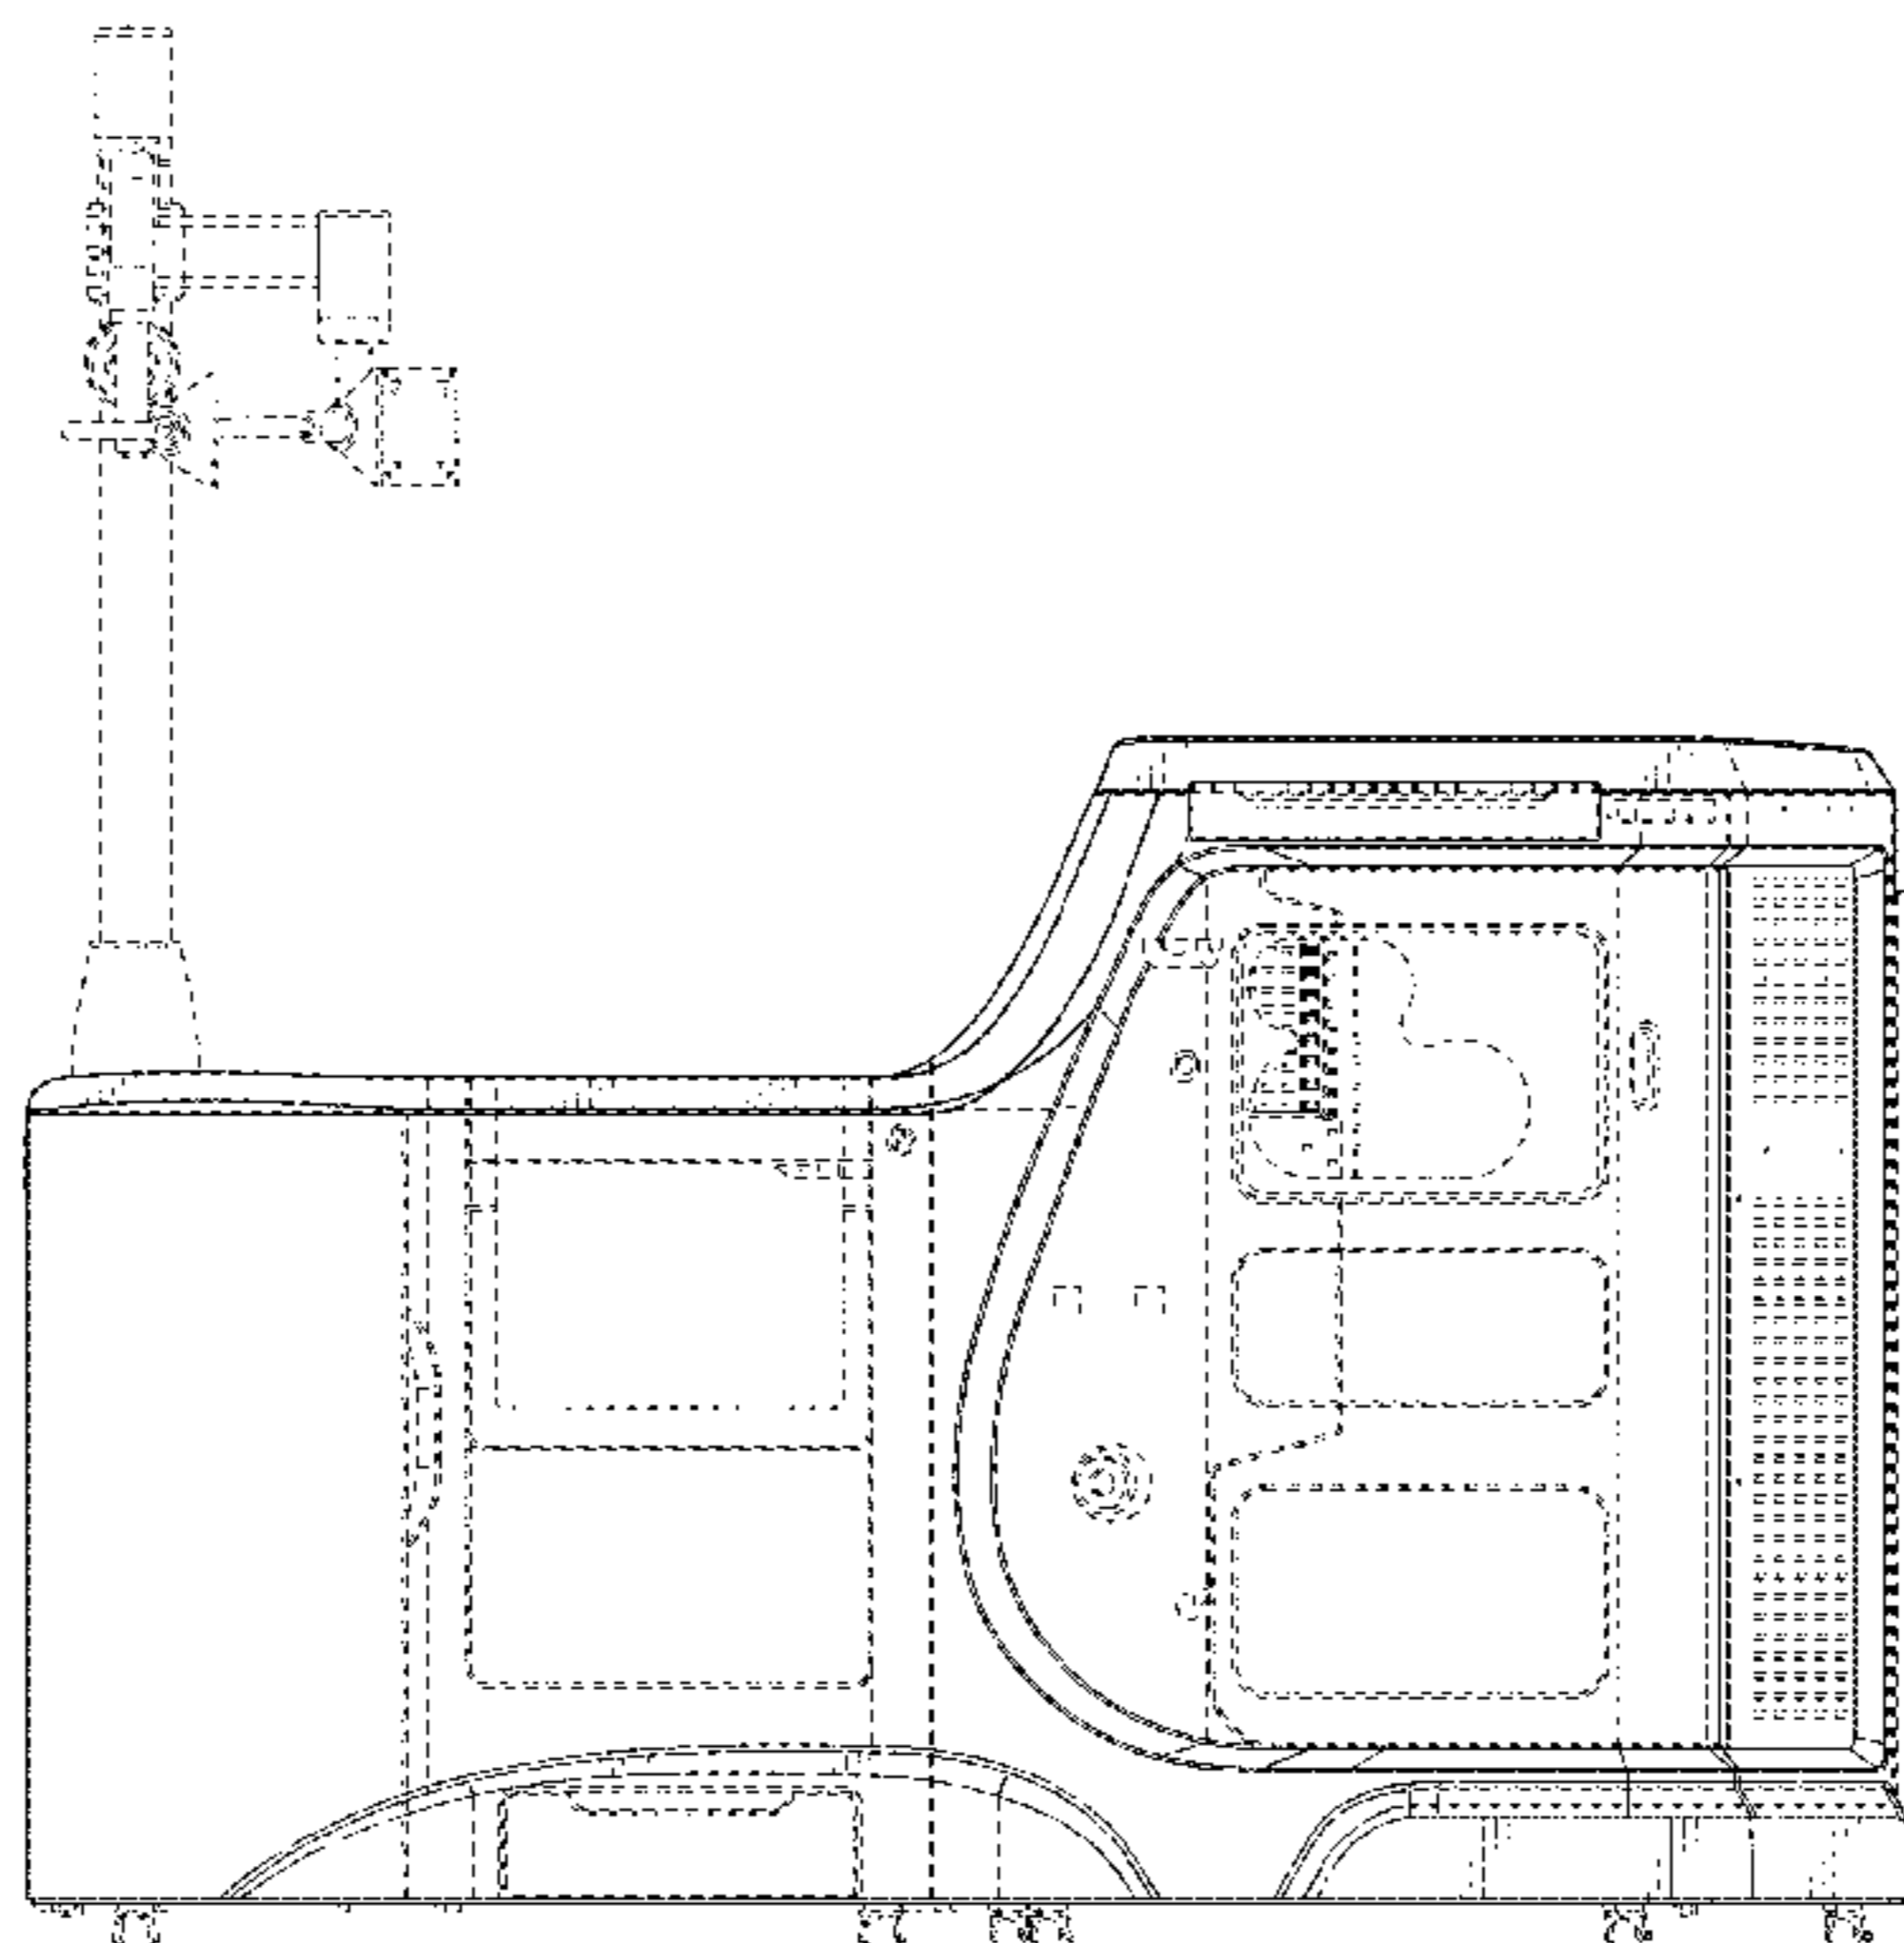

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D694,890 S *	12/2013	Bott	.....	D24/172
8,617,102 B2 *	12/2013	Moll	.....	A61B 17/062 600/114
D713,041 S	9/2014	Xu et al.		
D713,533 S	9/2014	Xu et al.		
D716,448 S *	10/2014	Kim	.....	D24/158
D722,172 S *	2/2015	Amemiya	.....	D24/185
9,039,681 B2 *	5/2015	Wang	.....	A61B 19/22 606/1
D739,947 S *	9/2015	Maier	.....	D24/186
2015/0032090 A1 *	1/2015	Gonzalez	.....	A61B 3/103 606/4

FOREIGN PATENT DOCUMENTS

CN	101664337	3/2010
JP	08-131399	5/1996
JP	2006-198237	8/2006
WO	2005/044125	5/2005
WO	2005/074806	8/2005

OTHER PUBLICATIONS

United States Patent and Trademark Office, "Non-Final Office Action," issued in connection with U.S. Appl. No. 29/398,222, on Feb. 28, 2013 (8 pages).

United States Patent and Trademark Office, "Final Rejection," issued in connection with U.S. Appl. No. 29/398,222, on Aug. 8, 2013 (6 pages).

United States Patent and Trademark Office, "Advisory Action," issued in connection with U.S. Appl. No. 29/398,222, on Nov. 14, 2013 (4 pages).

United States Patent and Trademark Office, "Final Rejection," issued in connection with U.S. Appl. No. 29/398,222, on Feb. 25, 2014 (7 pages).

United States Patent and Trademark Office, "Notice of Allowance," issued in connection with U.S. Appl. No. 29/398,222, on May 22, 2014 (5 pages).

United States Patent and Trademark Office, "Restriction Requirement," issued in connection with U.S. Appl. No. 29/428,197, on Nov. 16, 2012 (4 pages).

United States Patent and Trademark Office, "Non-Final Office Action," issued in connection with U.S. Appl. No. 29/428,197, on Mar. 7, 2013 (8 pages).

United States Patent and Trademark Office, "Final Rejection," issued in connection with U.S. Appl. No. 29/428,197, on Jul. 24, 2013 (8 pages).

United States Patent and Trademark Office, "Advisory Action," issued in connection with U.S. Appl. No. 29/428,197, on Oct. 3, 2013 (4 pages).

United States Patent and Trademark Office, "Final Rejection," issued in connection with U.S. Appl. No. 29/428,197, on Feb. 21, 2014 (6 pages).

United States Patent and Trademark Office, "Advisory Action," issued in connection with U.S. Appl. No. 29/428,197, on May 12, 2014 (4 pages).

United States Patent and Trademark Office, "Notice of Allowance," issued in connection with U.S. Appl. No. 29/428,197, on Jun. 6, 2014 (5 pages).

"Anesthesia Workstations," retrieved from <http://www.medicalexpo.com/medical-manufacturer/anesthesia-workstation-1681.html>, 2014, (23 pages).

"Endoscope Workstation—ENT 500," retrieved from <http://gmedpro.com/endoscopeworkstation.html>, 2010, (1 page).

Atmos, "ENT workstation / modular / with chair", retrieved from <http://www.medicalexpo.com/prod/atmos-medizintechnik/ent-workstations-modular-chair-67678-443374.html>, 2014, (13 pages).

\* cited by examiner

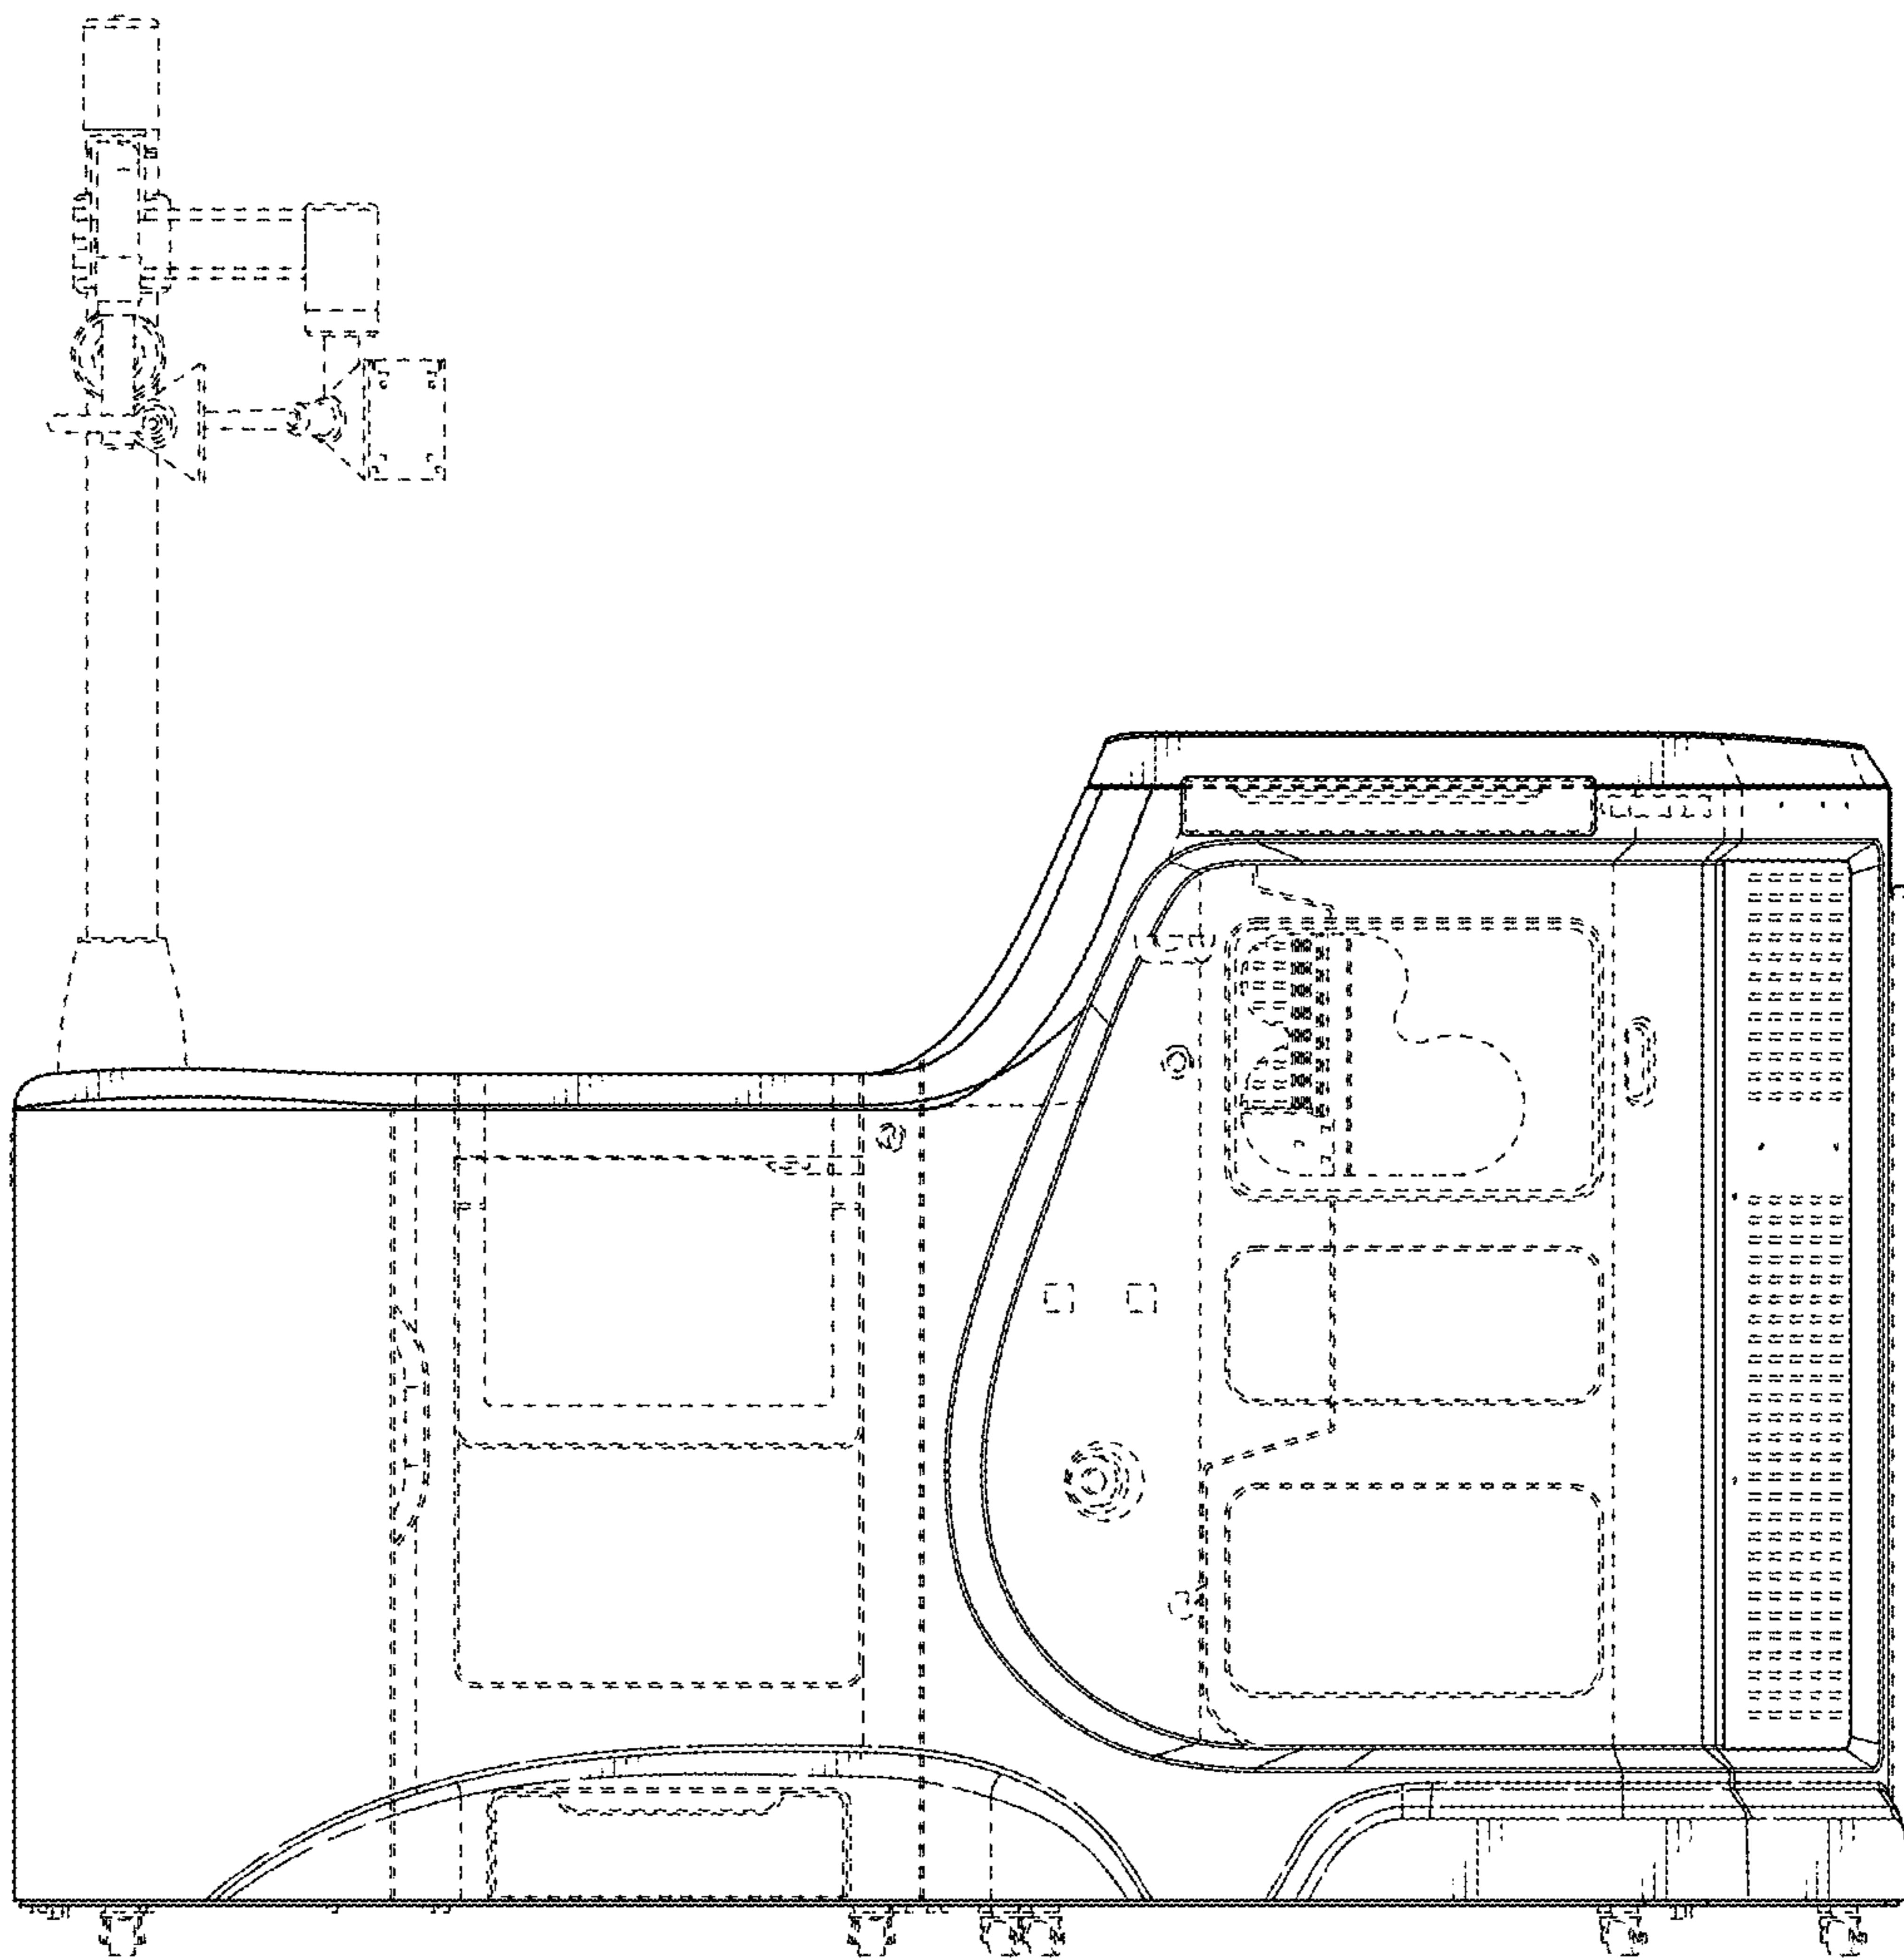


FIG. 1

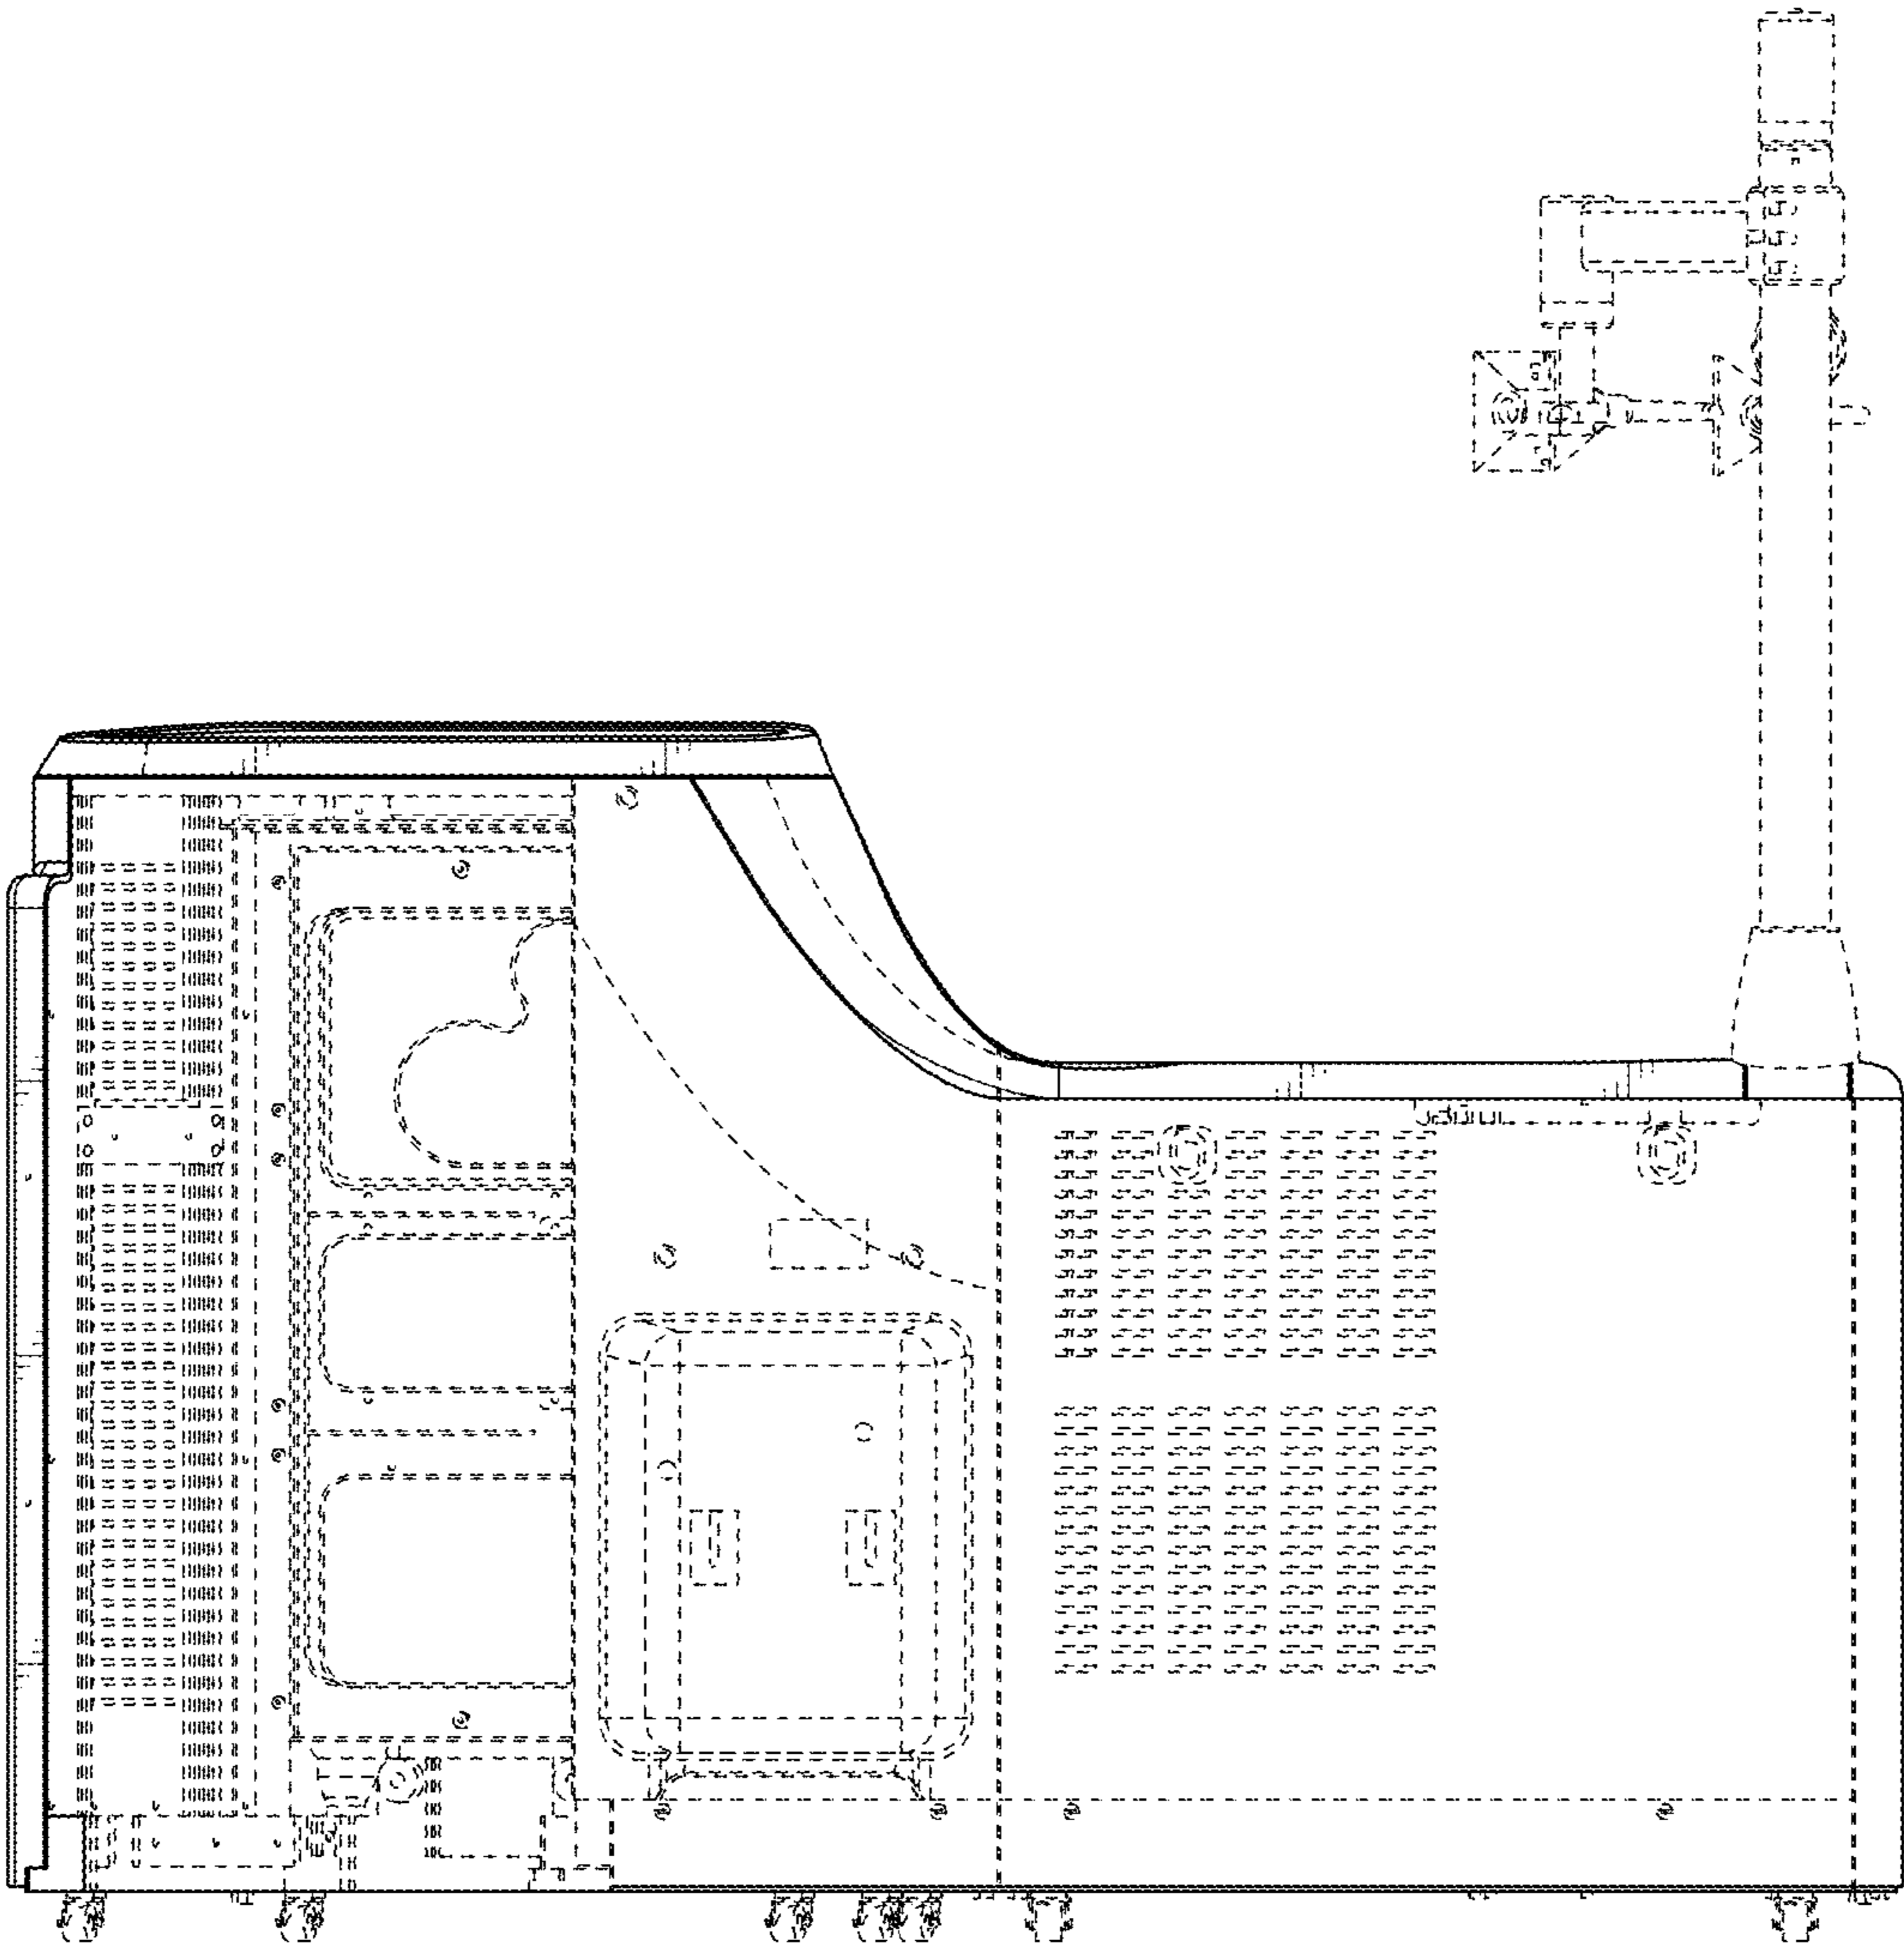


FIG. 2

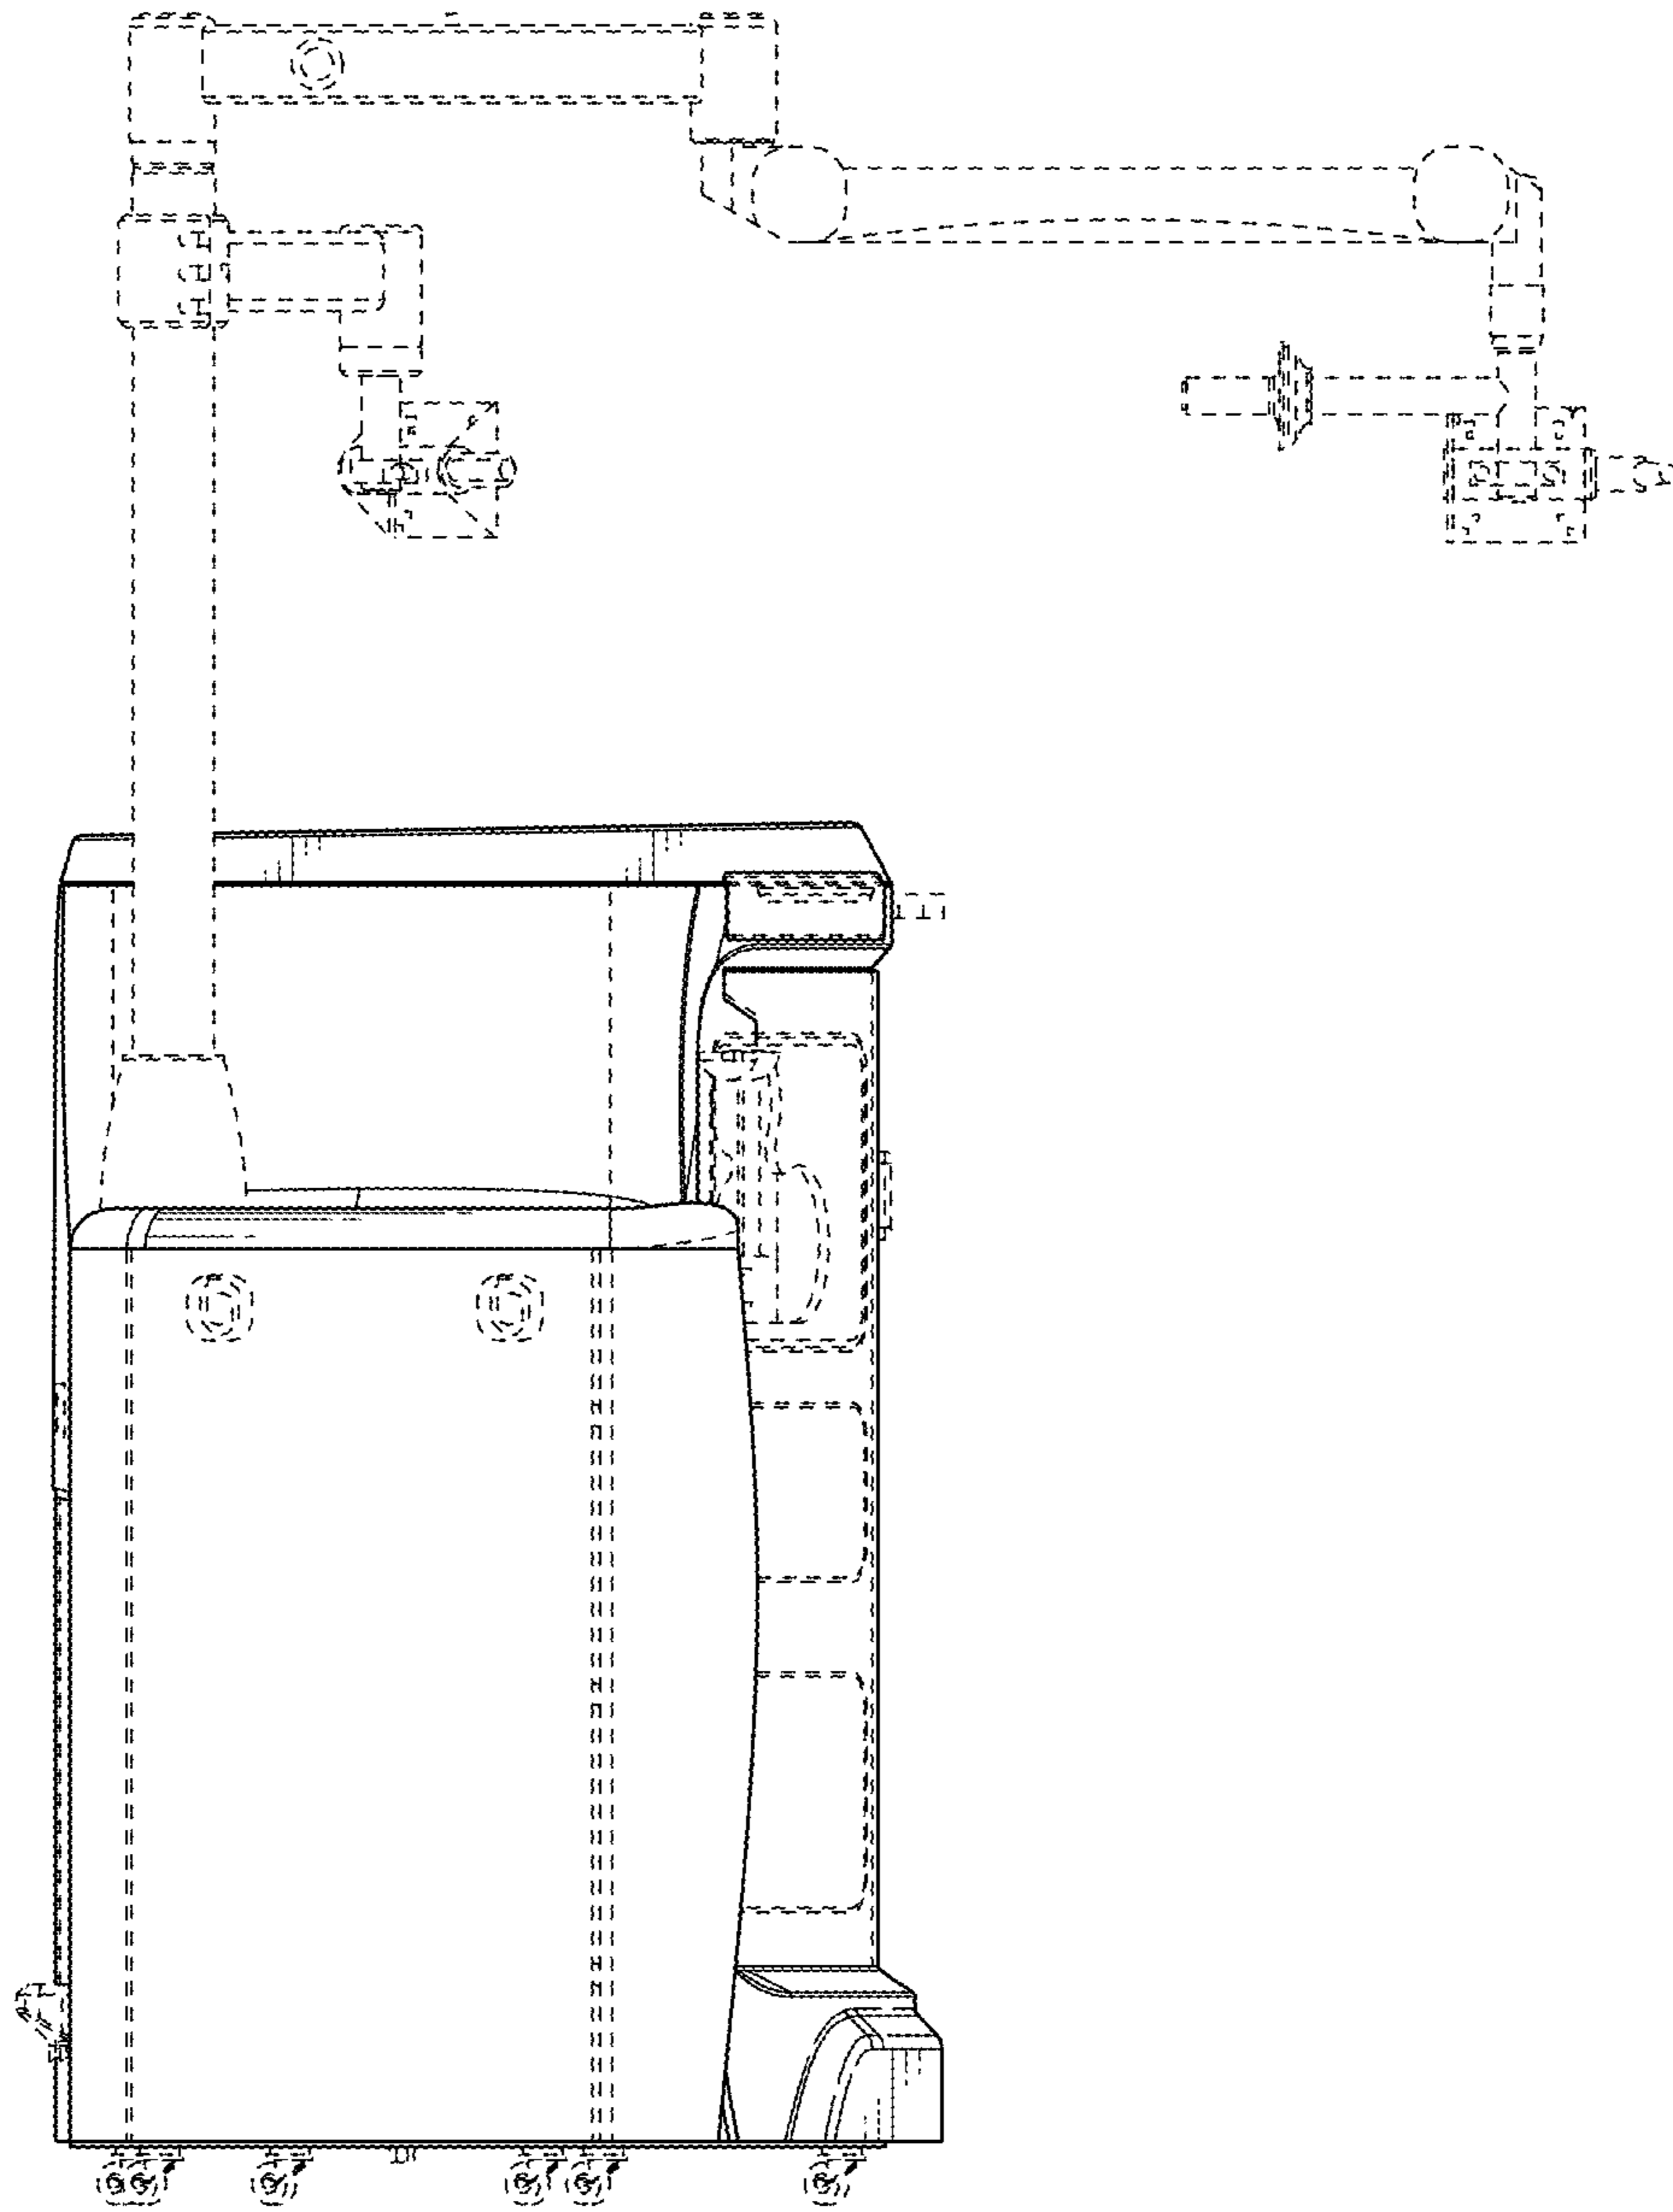


FIG. 3

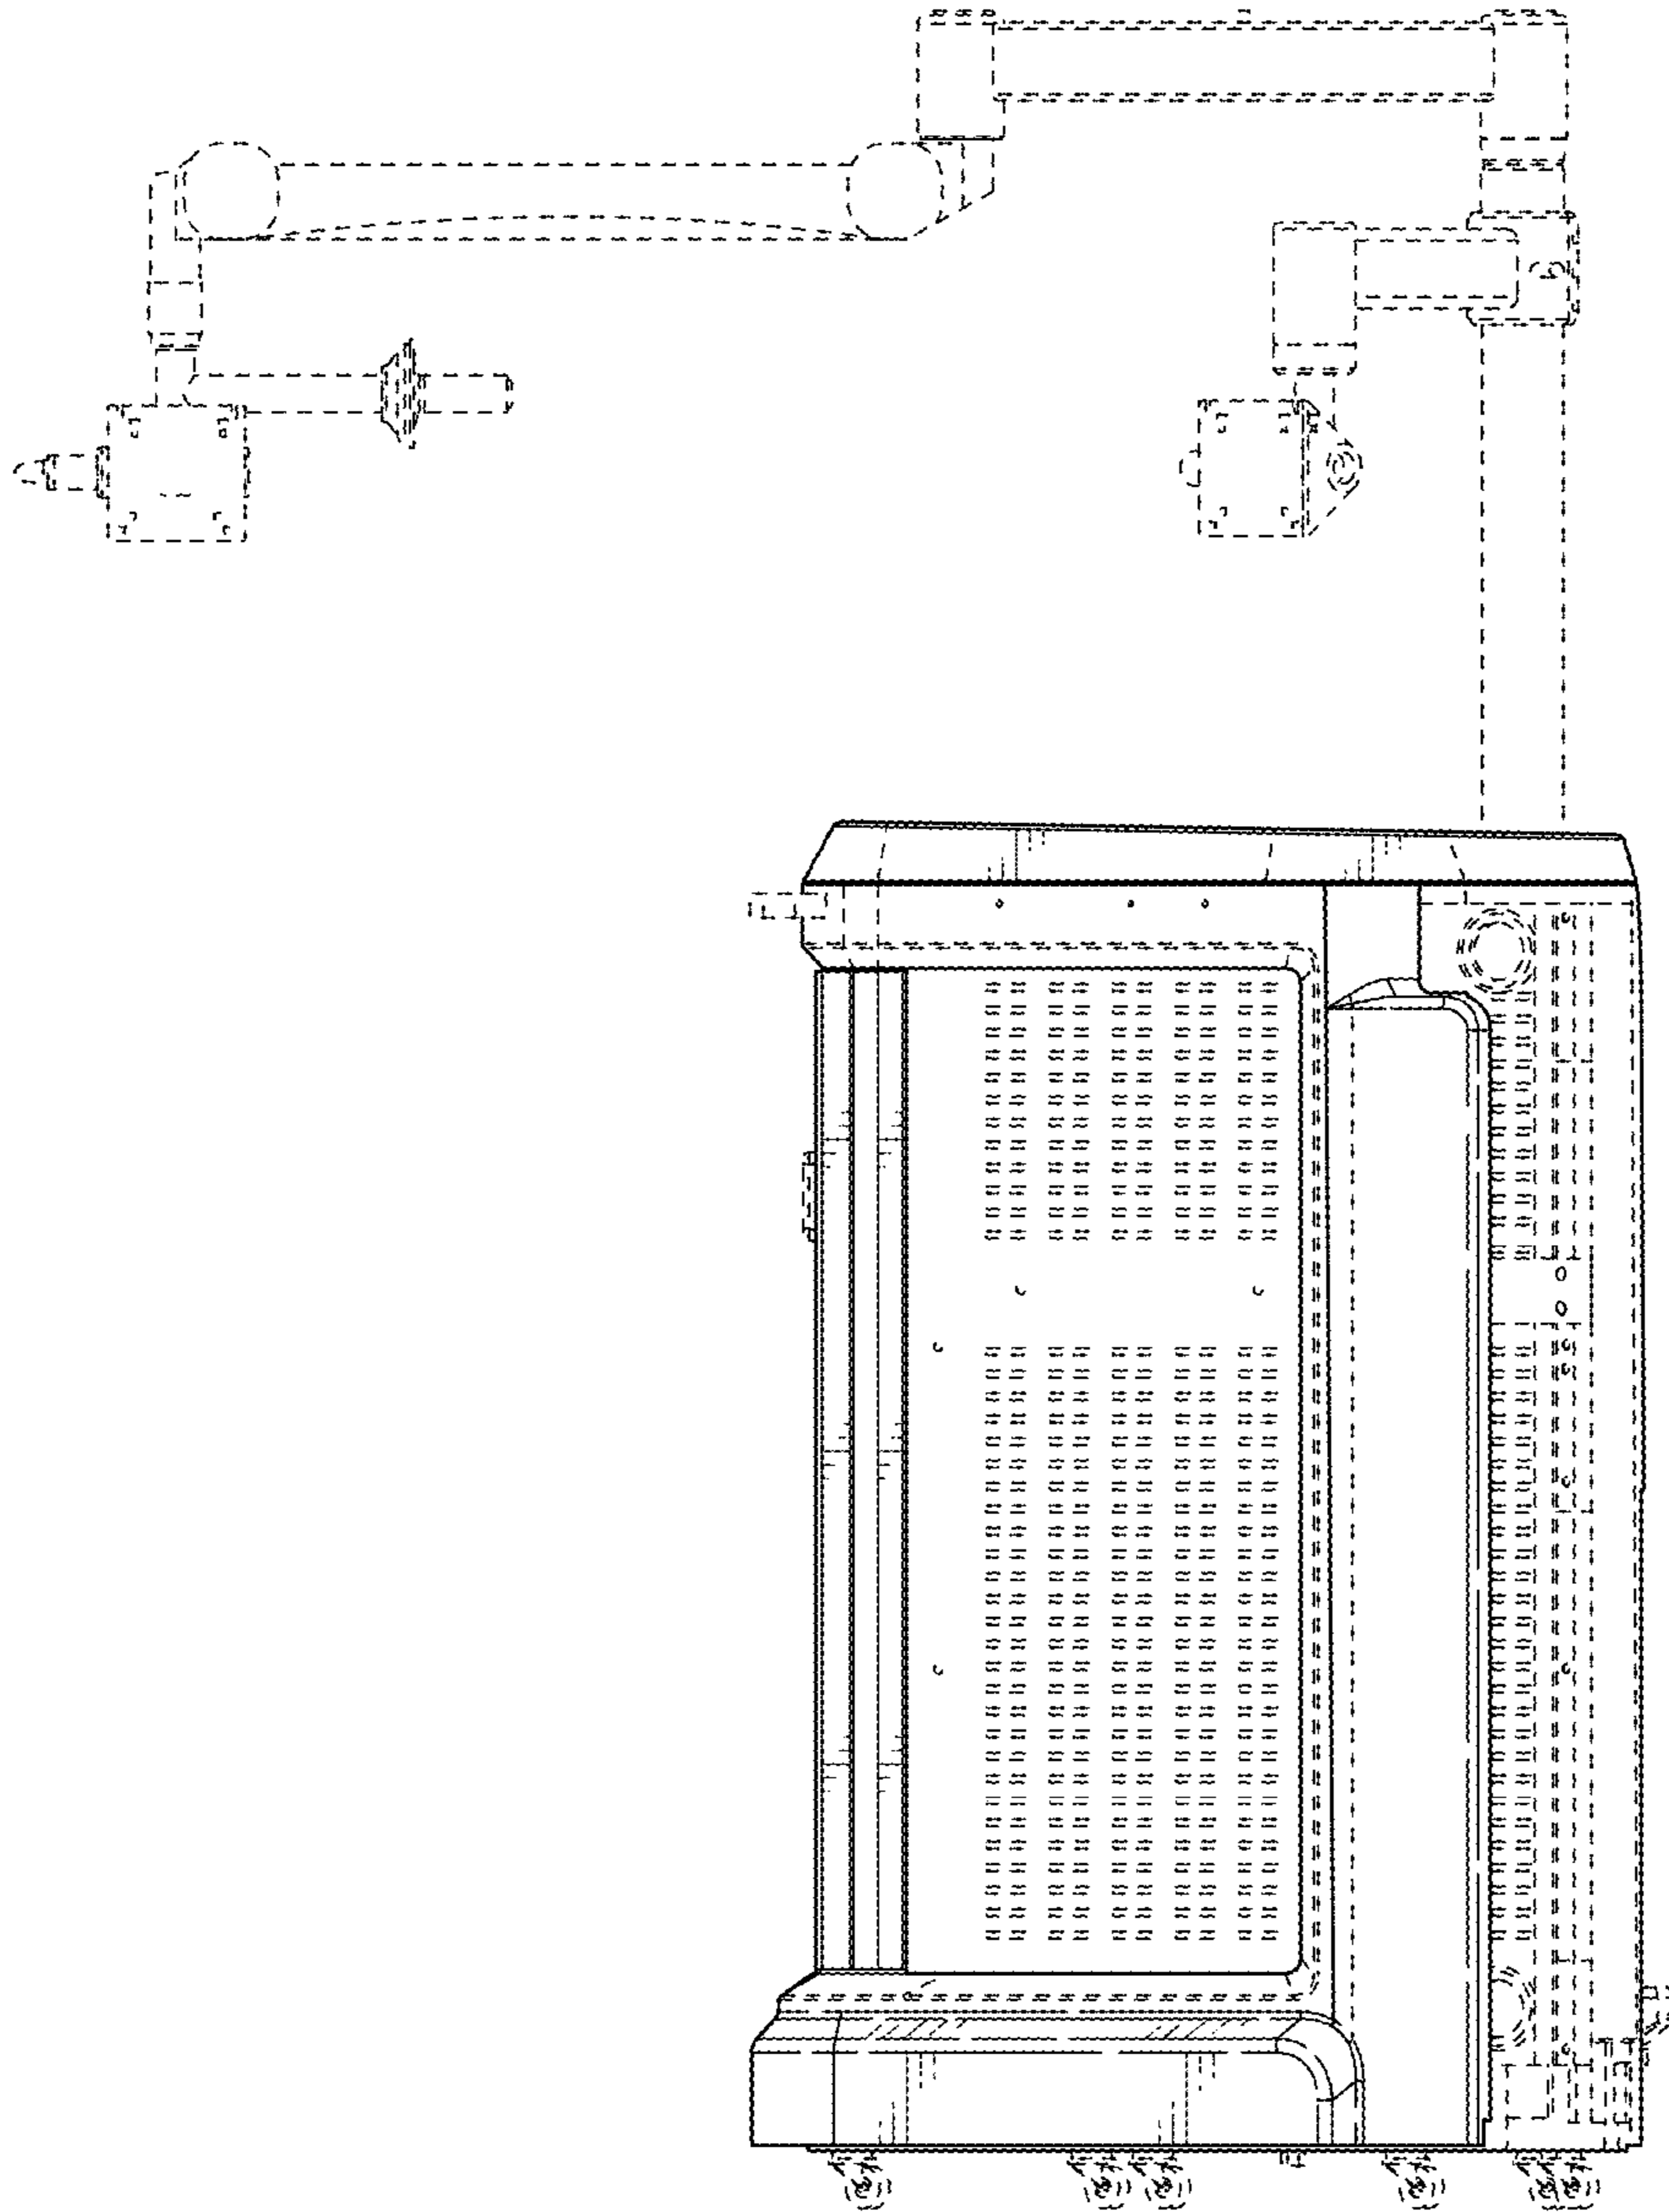


FIG. 4

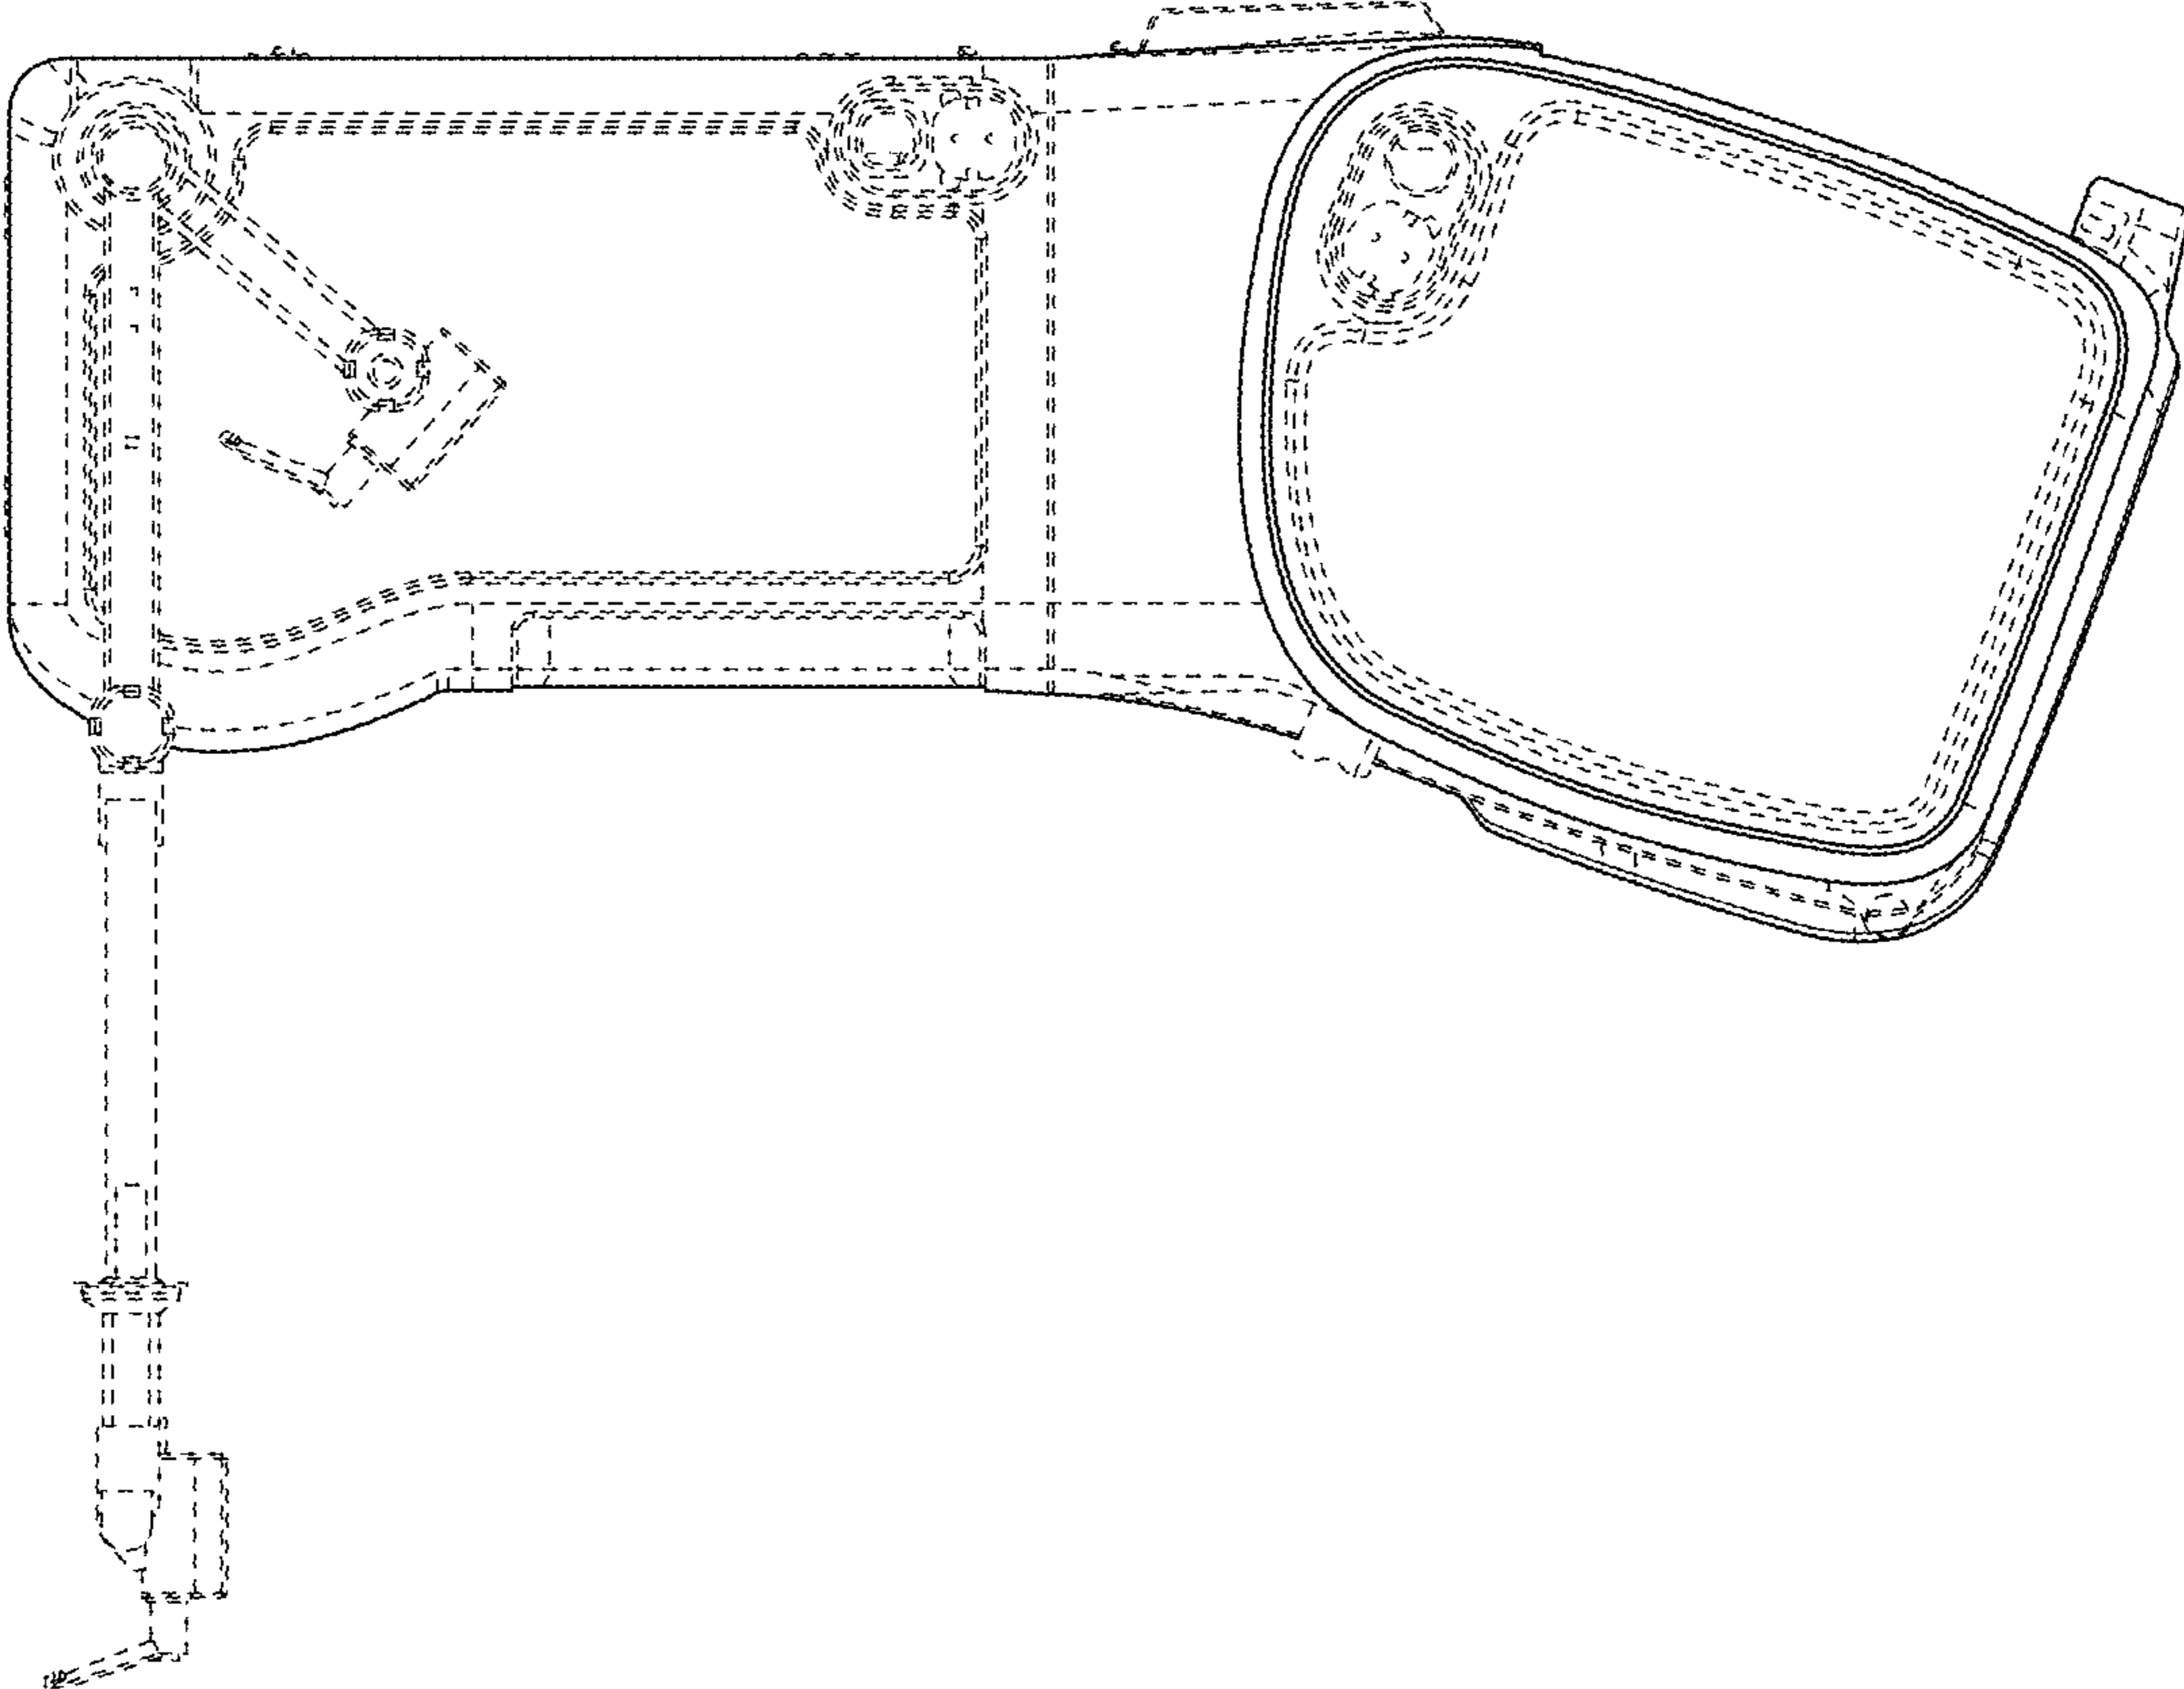


FIG. 5

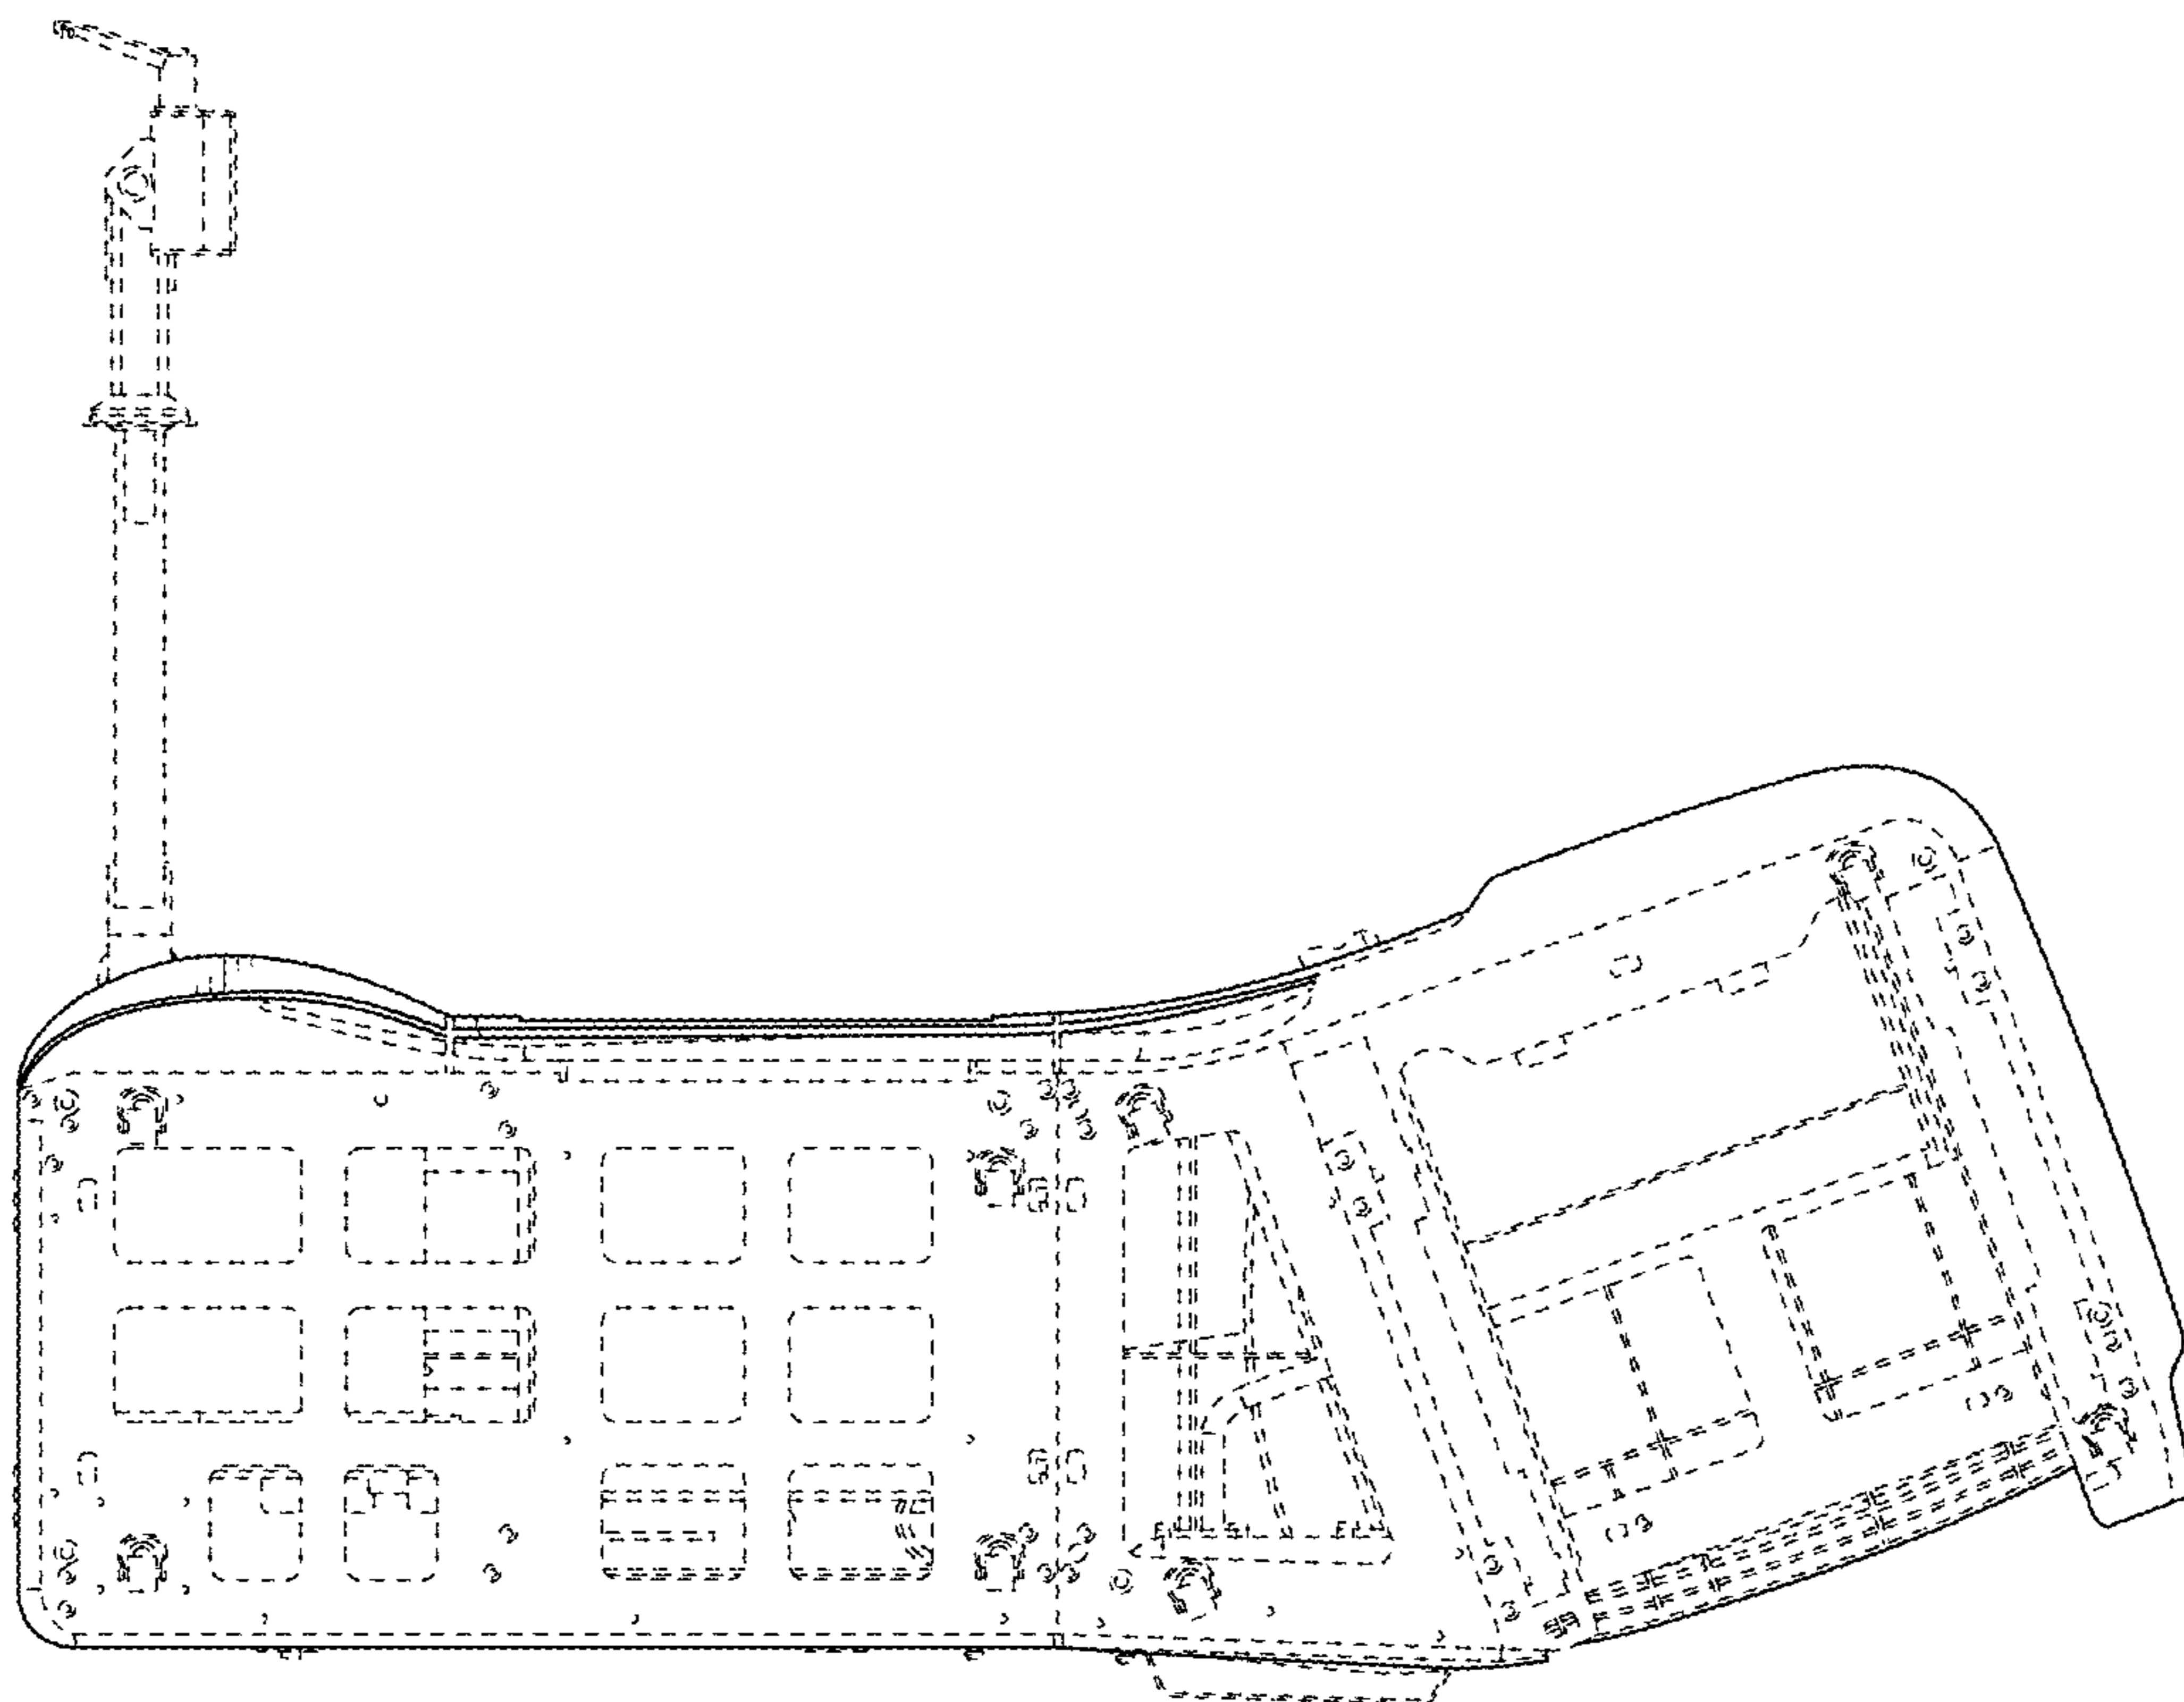


FIG. 6