



US00D772559S

(12) **United States Design Patent** (10) **Patent No.:** **US D772,559 S**  
**Binder et al.** (45) **Date of Patent:** **\*\* Nov. 29, 2016**

(54) **PACKAGING FOR A WOUND THERAPY SYSTEM**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Smith & Nephew PLC**, London (GB)

FR 1 163 907 10/1958

(72) Inventors: **Ian Binder**, Chippenham (GB); **John Cowan-Hughes**, Bristol (GB); **Beverley Love**, Hessle (GB); **Mark Russell**, Hull (GB); **Peter Sleight**, Cottingham (GB); **Philip Walsh**, Bristol (GB)

OTHER PUBLICATIONS

Packaging for Pico Single Use Negative Pressure Wound Therapy System (2012) in 1 page.

(Continued)

(73) Assignee: **Smith & Nephew PLC**, London (GB)

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Keith Frank

(\*\*) Term: **15 Years**

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson & Bear LLP

(21) Appl. No.: **29/563,987**

(57) **CLAIM**

The ornamental design for packaging for a wound therapy system, as shown and described.

(22) Filed: **May 10, 2016**

**DESCRIPTION**

**Related U.S. Application Data**

(63) Continuation of application No. 29/492,878, filed on Jun. 3, 2014, now Pat. No. Des. 758,851.

FIG. 1 is a top, front and left side perspective view of the packaging for a wound therapy system showing my new design;

(51) **LOC (10) Cl.** ..... **03-01**

(52) **U.S. Cl.**  
USPC ..... **D3/203.6**; D9/432

FIG. 2 is a front elevation view thereof;

FIG. 3 is a rear elevation view thereof;

(58) **Field of Classification Search**

USPC ..... D9/414, 420-423, 432, 456, 721;  
229/103.2; 220/4.26; 206/321, 322,  
206/449, 450, 472, 473; D3/203.1, 203.6,  
D3/203.7, 203.8

FIG. 4 is a right side elevation view thereof;

FIG. 5 is a left side elevation view thereof;

FIG. 6 is a top plan view thereof

FIG. 7 is a bottom plan view thereof;

CPC B65D 85/48; B65D 5/0245; B65D 77/0433;  
B65D 85/46

See application file for complete search history.

FIG. 8 is a top, front and left side perspective view of the packaging for a wound therapy system in a partially open configuration;

FIG. 9 is a front elevation view of a packaging for a wound therapy system in a fully open configuration;

FIG. 10 is a rear elevation view thereof;

FIG. 11 is a right side elevation view thereof;

FIG. 12 is a left side elevation view thereof;

FIG. 13 is a top plan view thereof; and,

FIG. 14 is a bottom plan view thereof.

The broken lines in the drawings depict unclaimed subject matter and form no part of the claimed design.



(56) **References Cited**

U.S. PATENT DOCUMENTS

D134,249 S \* 11/1942 Button ..... 206/564  
2,874,707 A \* 2/1959 Koppel ..... A45D 29/20  
132/315

(Continued)

**1 Claim, 13 Drawing Sheets**

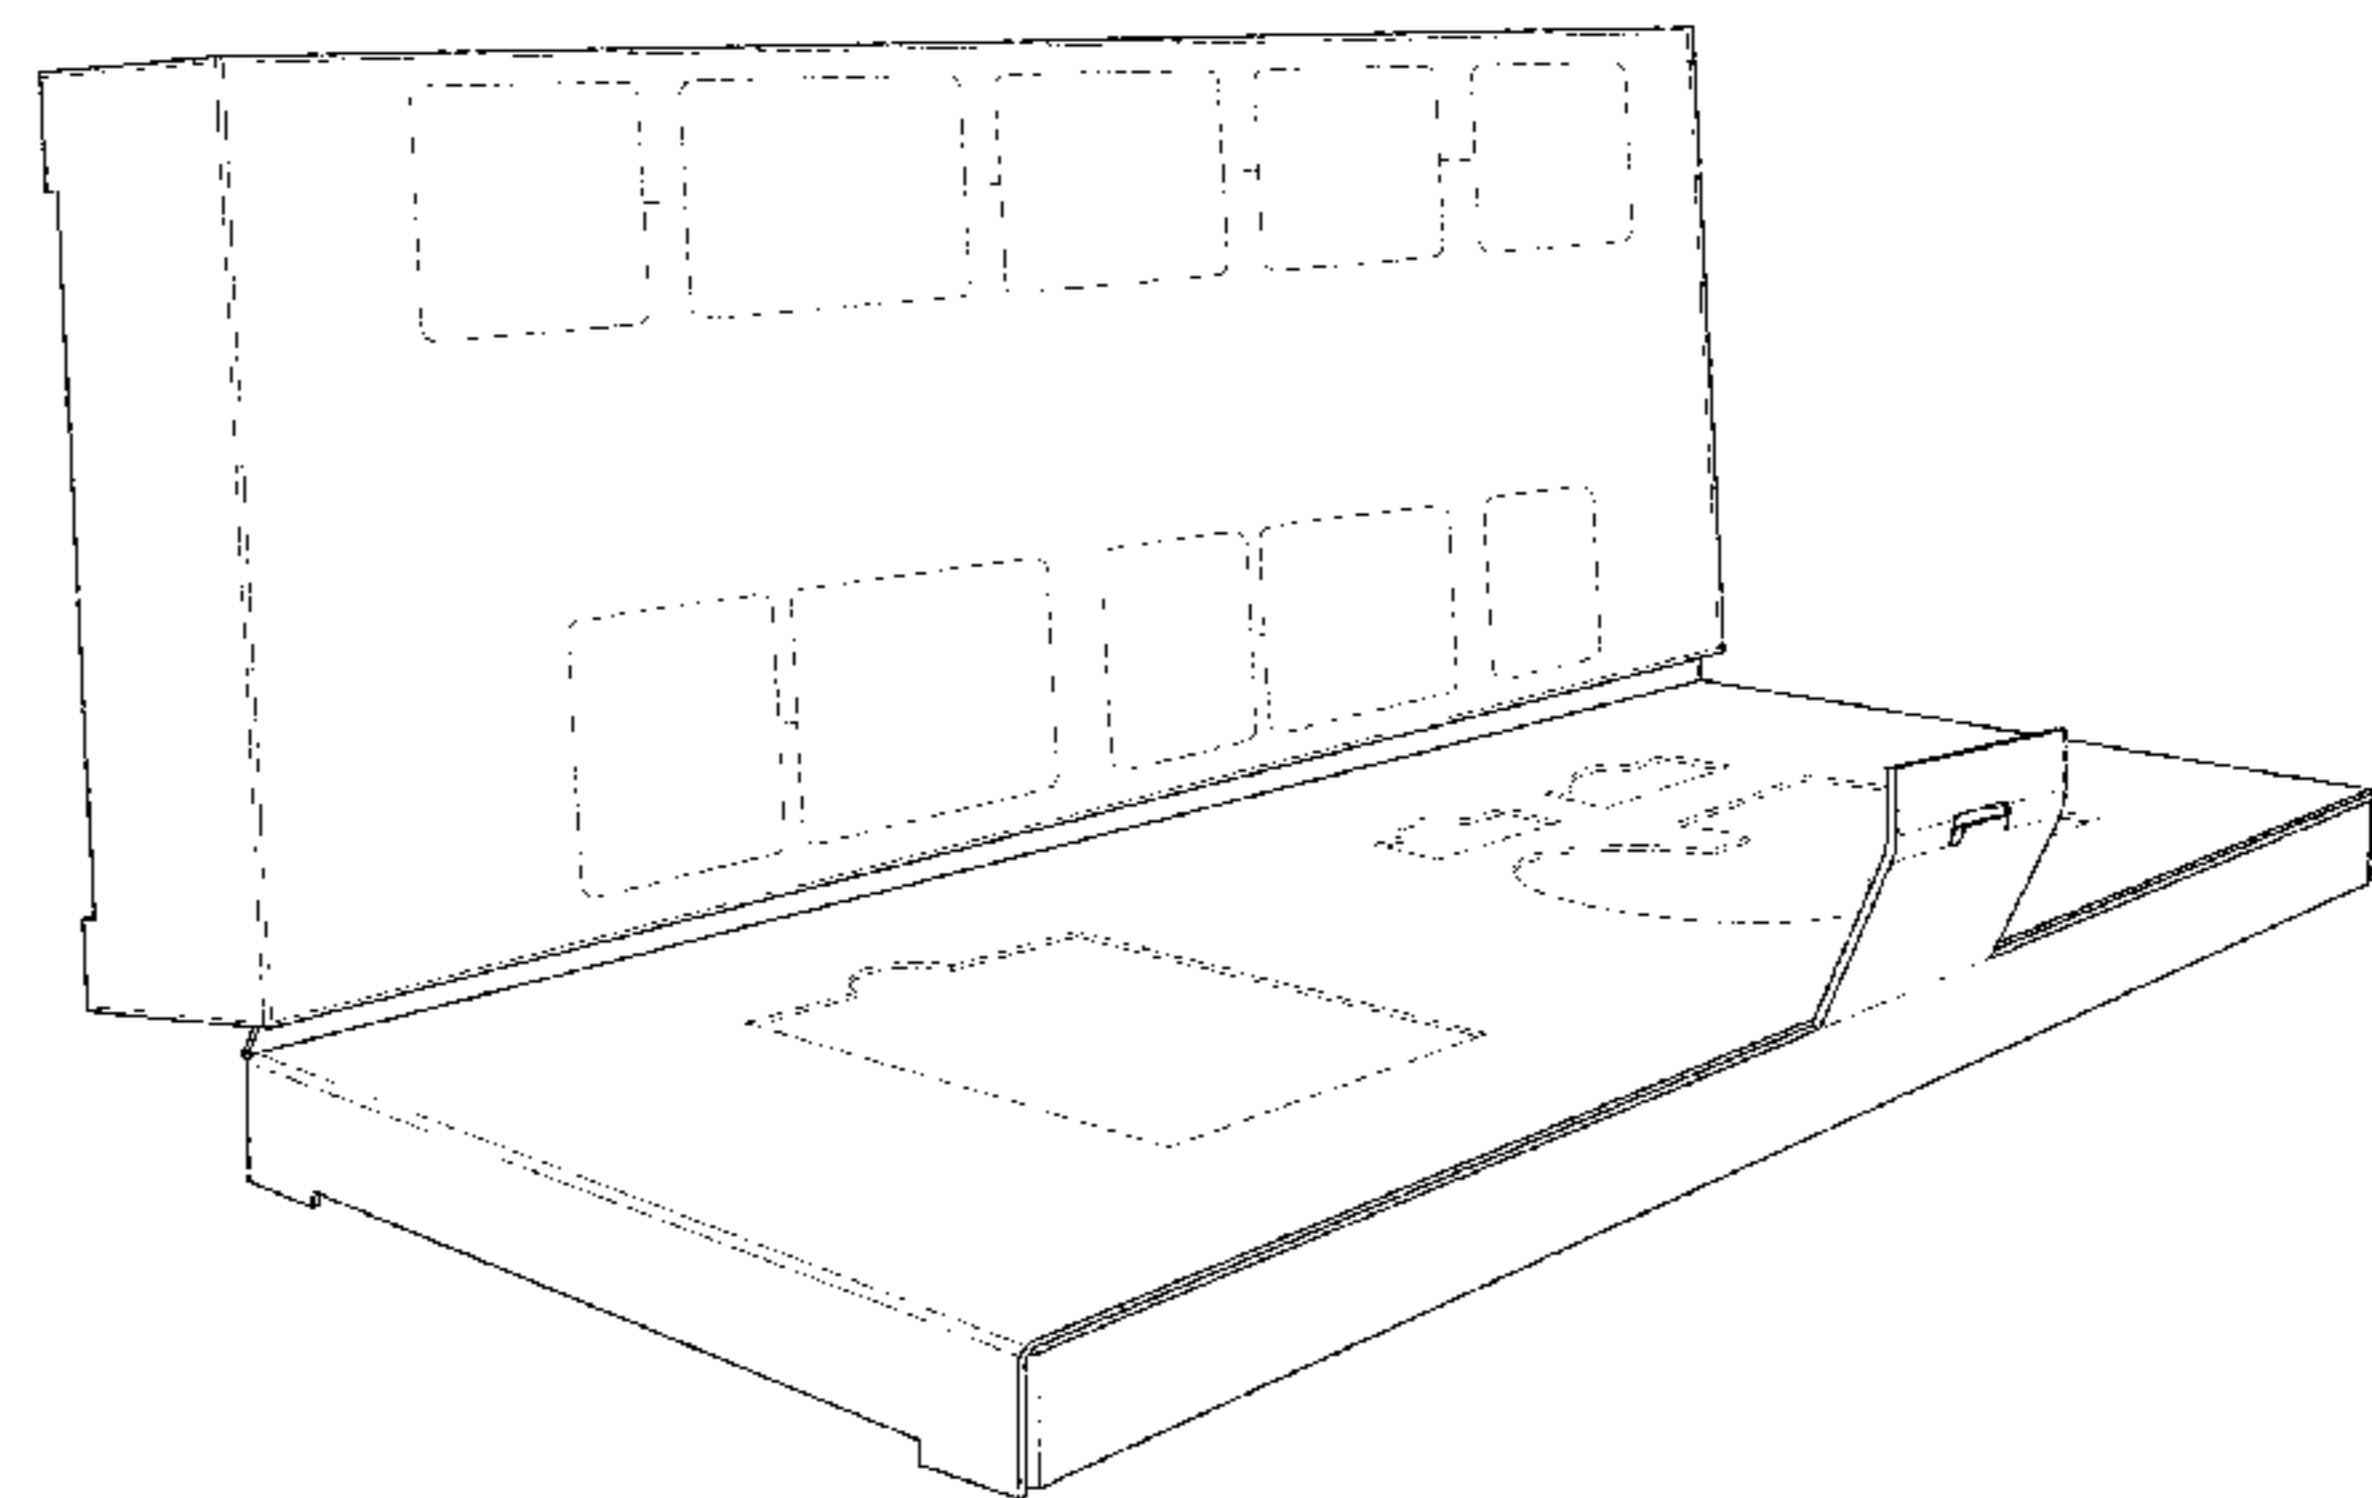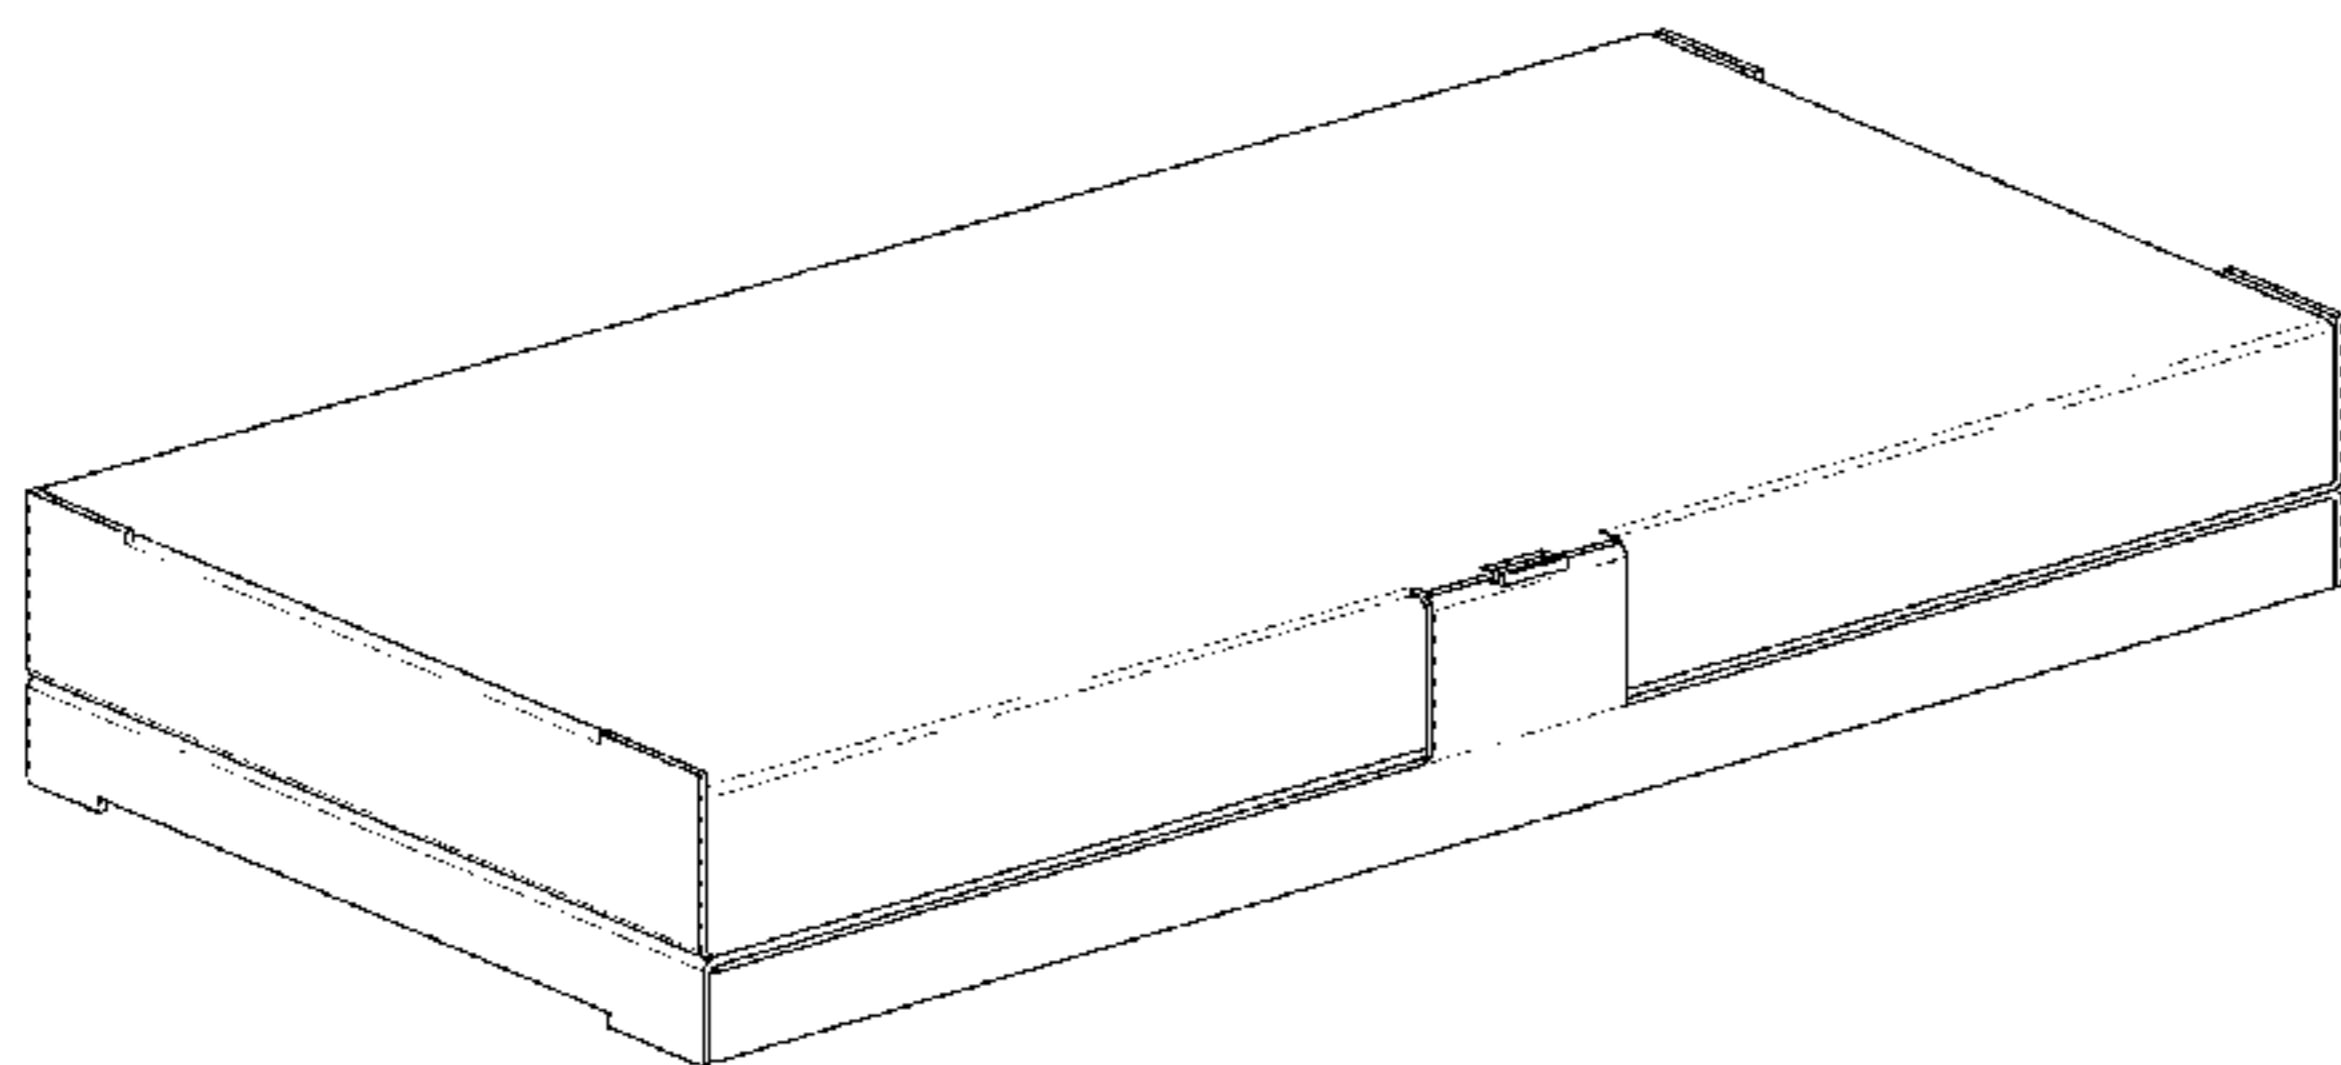

(56)

References Cited

U.S. PATENT DOCUMENTS

3,640,379 A \* 2/1972 Weingarden ..... G11B 23/0236  
206/387.13

3,972,328 A 8/1976 Chen  
D254,219 S \* 2/1980 Papciak ..... D3/203.7  
D267,834 S \* 2/1983 Yew ..... D3/203.7  
D268,098 S \* 3/1983 Brown ..... D9/418  
D275,425 S \* 9/1984 Briggs ..... D28/78  
D281,836 S \* 12/1985 Sparkman ..... D3/203.7  
D289,461 S \* 4/1987 Humphries ..... 30/1  
4,977,483 A \* 12/1990 Perretta ..... H05K 9/0067  
206/232

D313,505 S \* 1/1991 Leopoldi ..... D3/203.8  
D316,181 S 4/1991 Clifton  
D320,308 S \* 10/1991 Whitworth ..... D3/203.7  
D327,363 S \* 6/1992 Farb ..... D19/75  
5,238,732 A 8/1993 Krishnan  
D339,287 S 9/1993 Levin  
5,344,024 A \* 9/1994 Cohu ..... A45C 5/03  
206/526


D365,754 S 1/1996 Plassier  
5,549,584 A 8/1996 Gross  
D389,639 S \* 1/1998 Priebe ..... D3/203.8  
D393,591 S \* 4/1998 Baryshyan ..... D9/753  
5,759,570 A 6/1998 Arnold  
D396,750 S \* 8/1998 Slater ..... D3/284  
D397,869 S \* 9/1998 Minhas ..... D3/274  
D398,527 S 9/1998 Maceachern et al.  
D420,586 S 2/2000 Maceachern et al.  
6,626,891 B2 9/2003 Ohmstede  
7,361,184 B2 4/2008 Joshi  
7,381,859 B2 6/2008 Hunt et al.  
D579,195 S \* 10/2008 Kagawa ..... D3/203.1  
7,569,742 B2 8/2009 Haggstrom et al.  
7,615,036 B2 11/2009 Joshi et al.

D606,394 S 12/2009 Stewart  
D607,717 S 1/2010 Hodges  
7,699,823 B2 4/2010 Haggstrom et al.  
D618,546 S 6/2010 Easterbrook et al.  
7,775,998 B2 8/2010 Riesinger  
7,811,269 B2 10/2010 Boynton et al.  
7,846,141 B2 12/2010 Weston  
7,910,791 B2 3/2011 Coffey  
7,922,703 B2 4/2011 Riesinger  
7,964,766 B2 6/2011 Blott et al.  
D645,735 S 9/2011 Clark et al.  
D661,188 S 6/2012 Fahy  
D661,189 S 6/2012 Fahy  
D661,190 S 6/2012 Fahy  
D663,944 S \* 7/2012 Bouskill ..... D3/203.1  
D668,948 S 10/2012 LaTrobe  
D687,300 S \* 8/2013 Jones ..... D9/456  
D708,055 S 7/2014 Elston et al.  
D723,792 S \* 3/2015 Anderson ..... D3/201  
D730,728 S \* 6/2015 Fath ..... D9/432  
9,241,873 B2 \* 1/2016 Upchurch ..... A61J 1/035  
D750,478 S \* 3/2016 Kiss ..... D9/423  
D761,023 S \* 7/2016 Tramontana ..... D3/203.1  
2007/0225663 A1 9/2007 Watt et al.  
2008/0306456 A1 12/2008 Riesinger


OTHER PUBLICATIONS

Protz, Kerstin: "Modern Wundauflagen unterstützen Heilungsprozess", Wundversorgung: Indikation und Anwendung, Geriatrie Journal Apr. 2005, pp. 3333-3339.  
Smith & Nephew, "PICO packaging reduction", Jun. 2014, <http://www.smith-nephew.com/news-and-media/case-studies/picosntm-packaging-reduction/>.


\* cited by examiner

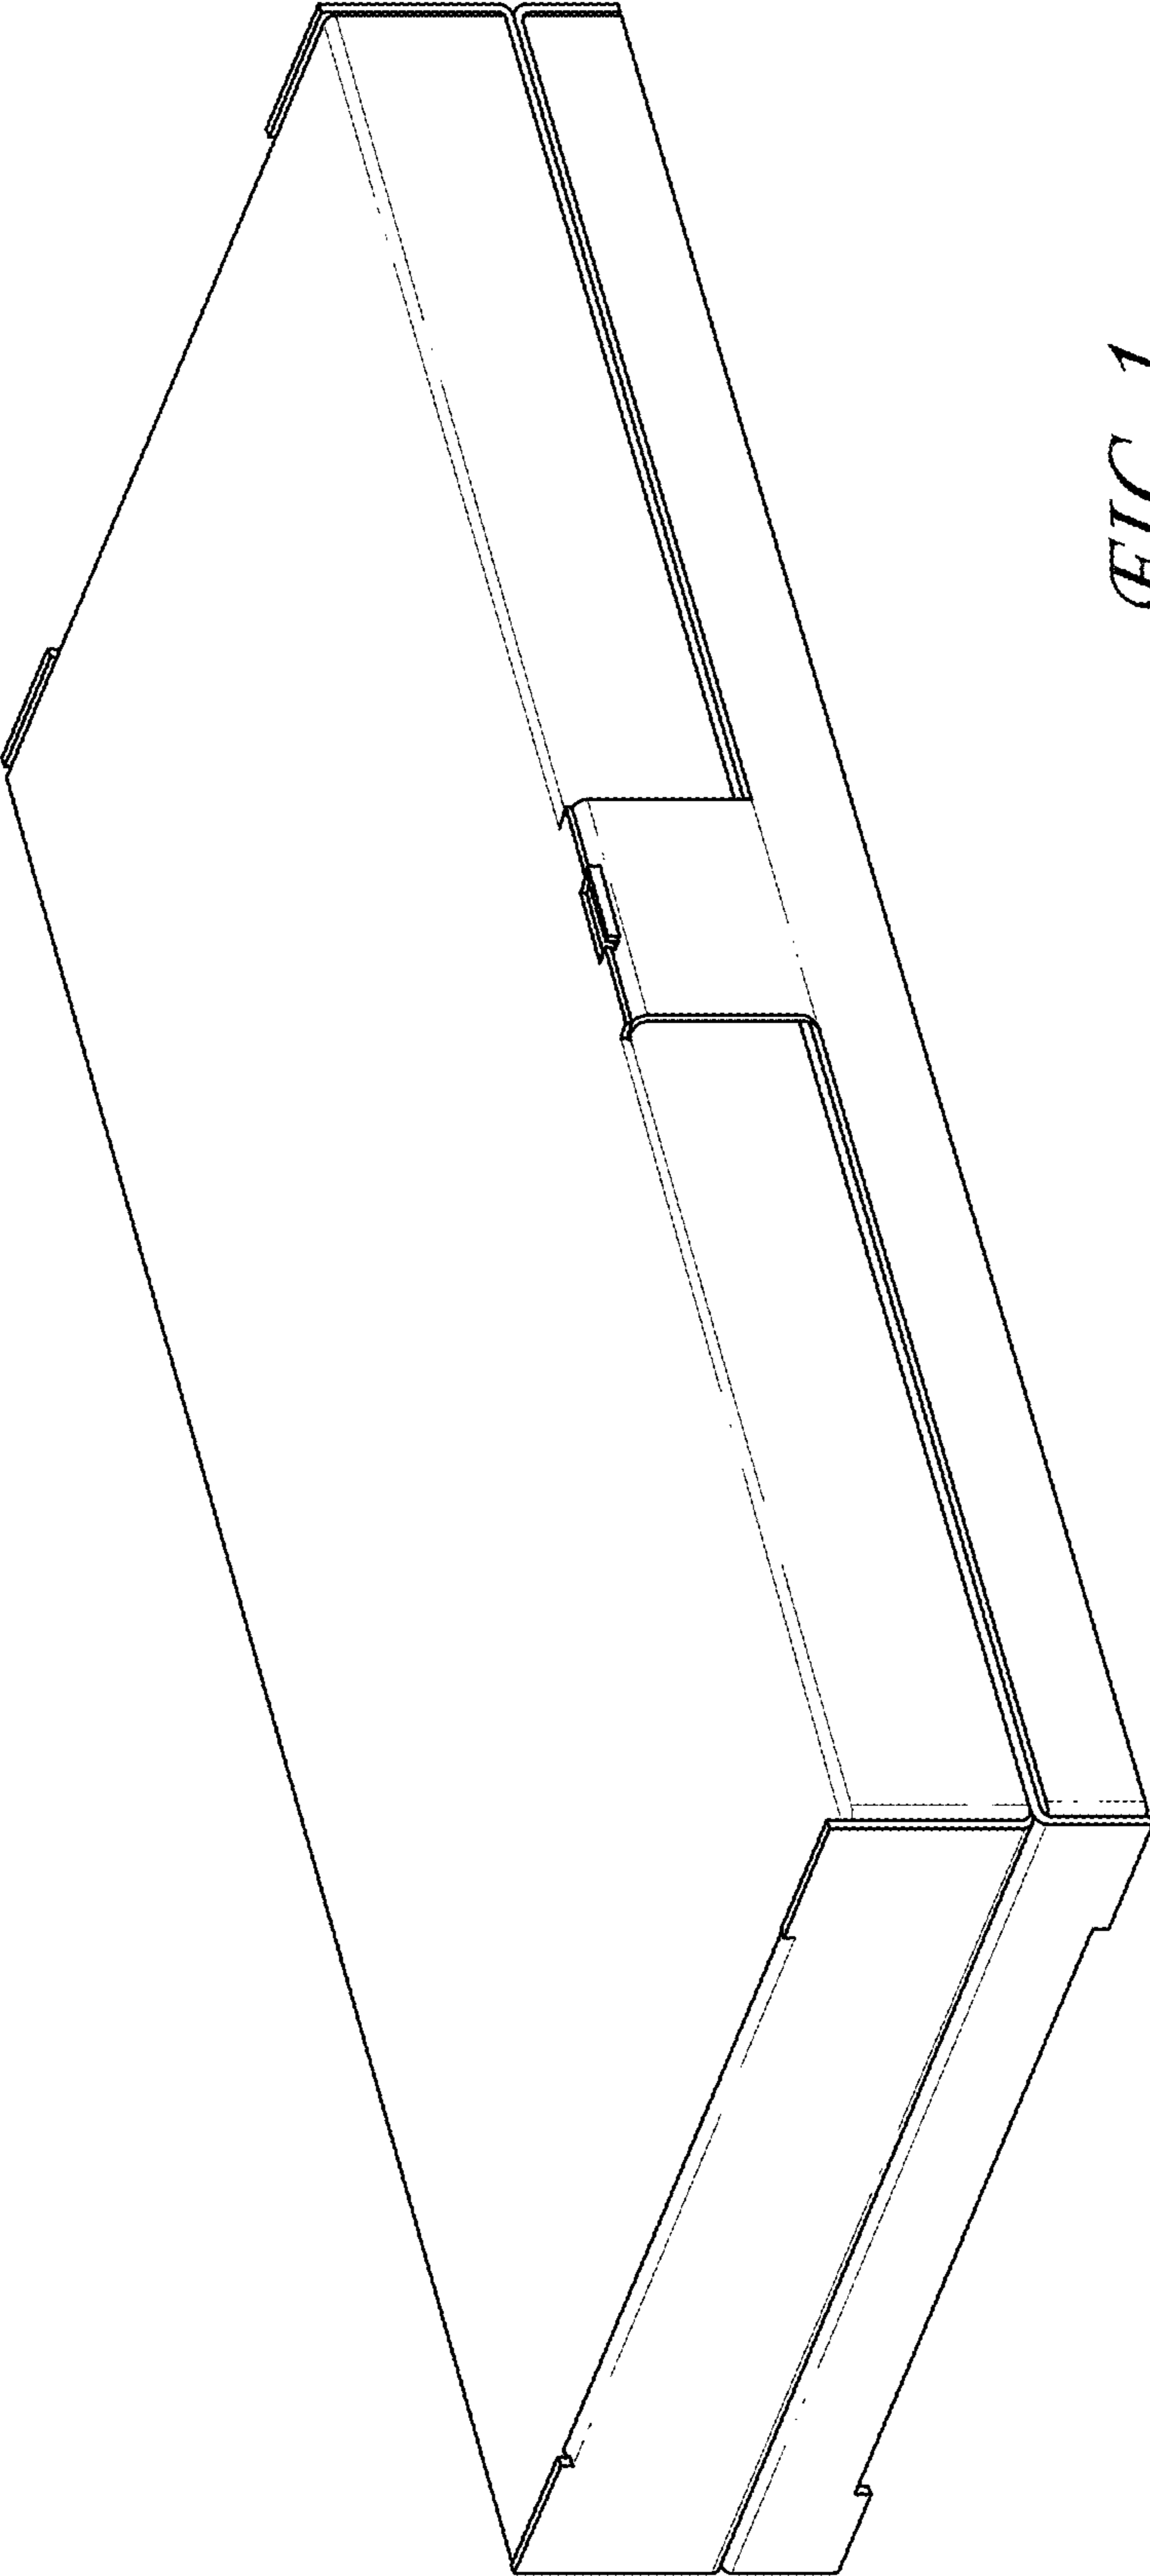


*FIG. 1*

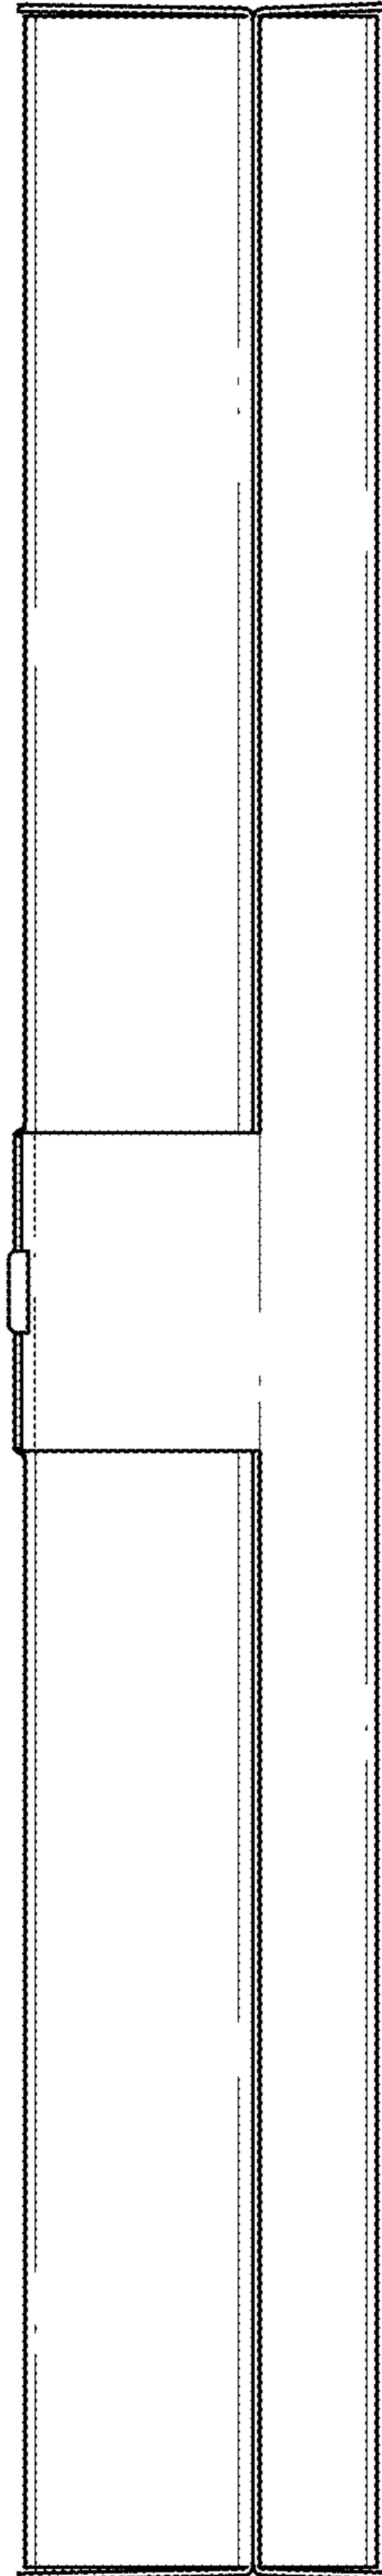


*FIG. 2*

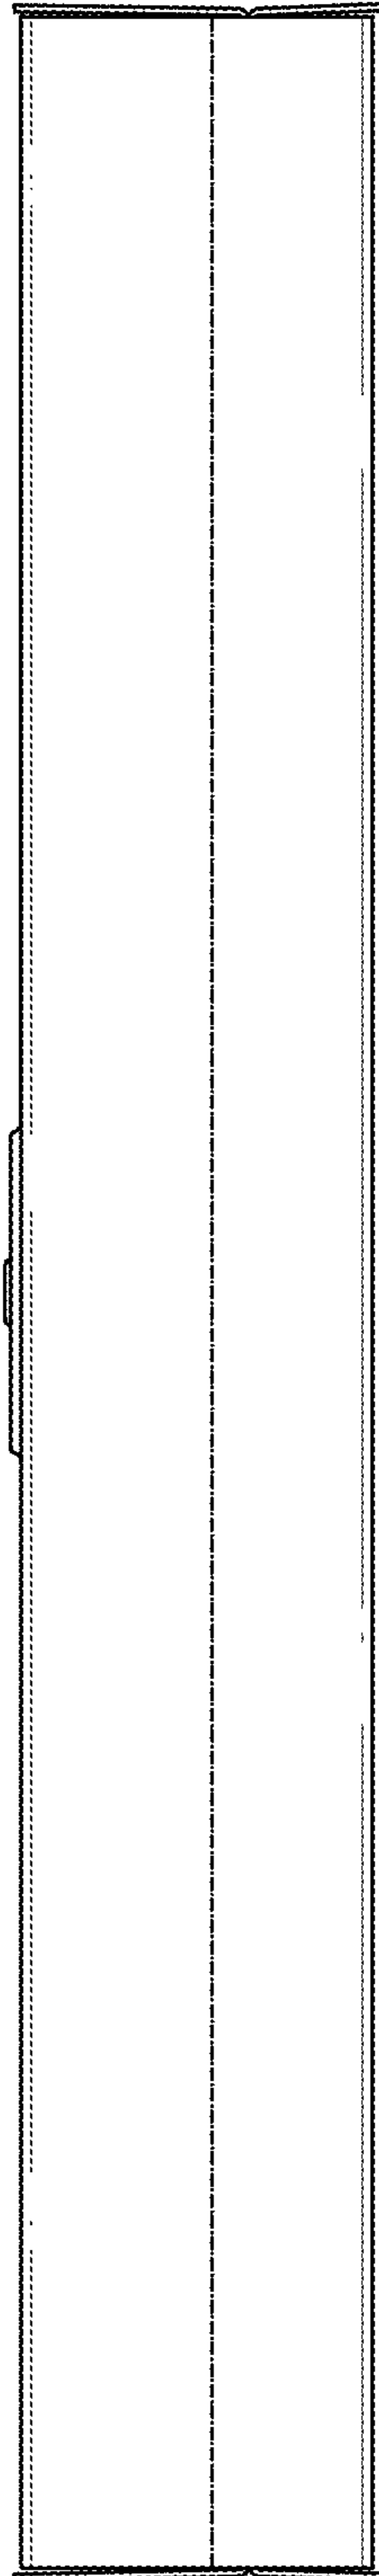


*FIG. 3*

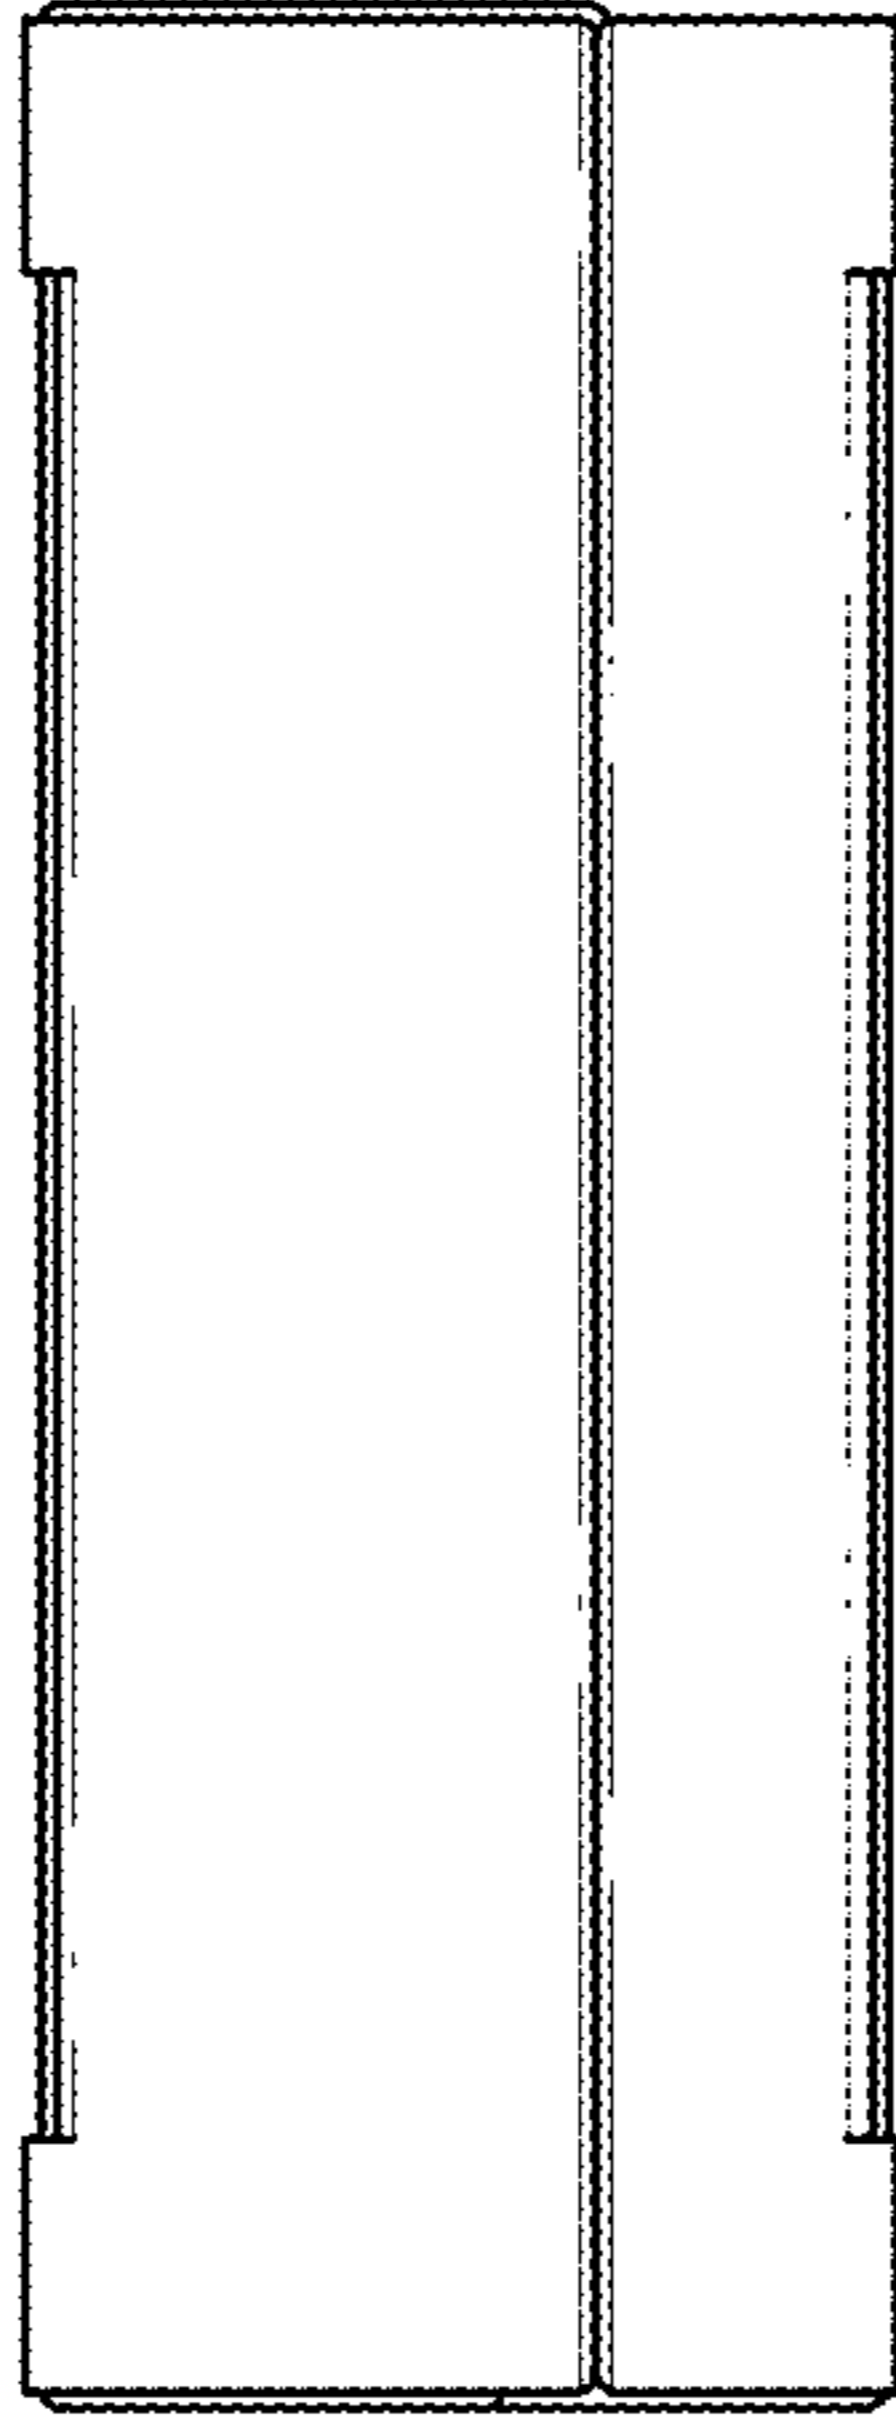


*FIG. 5*

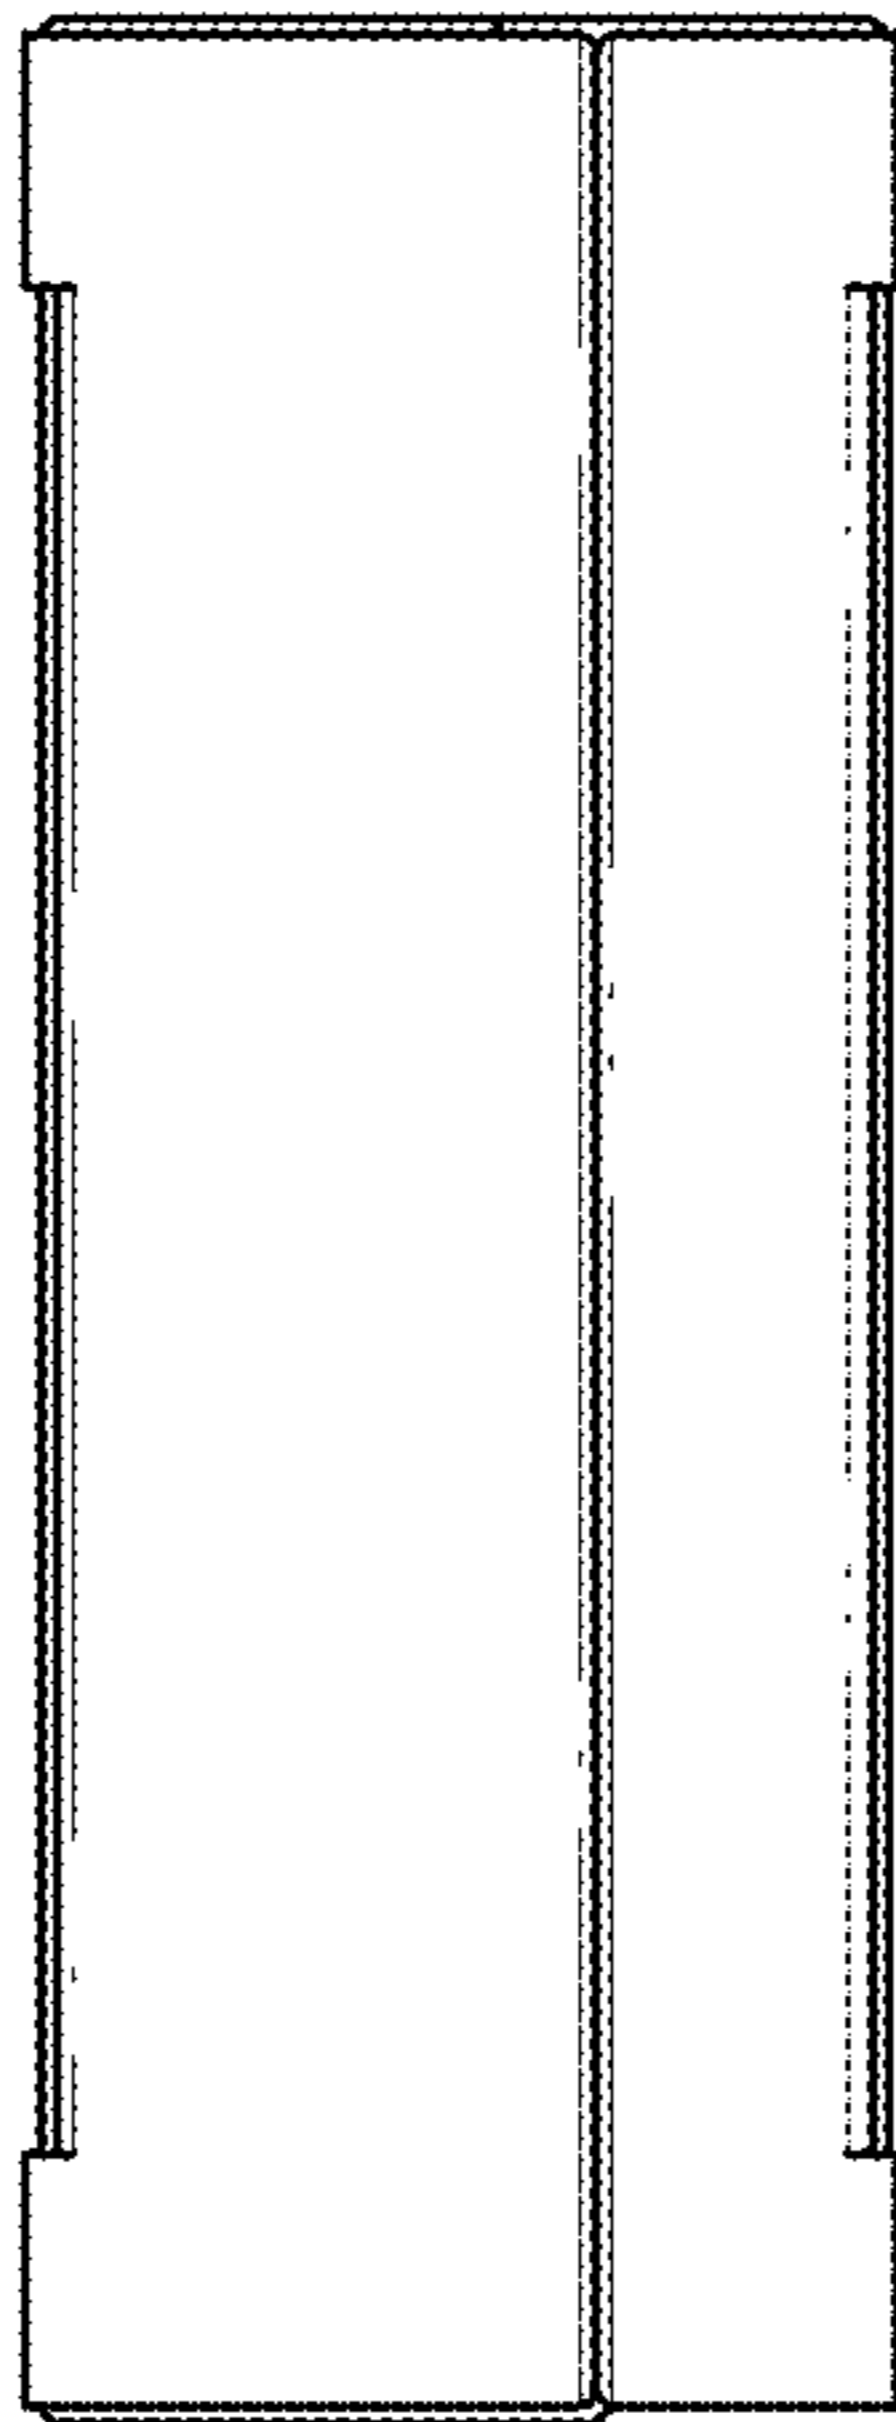

*FIG. 4*

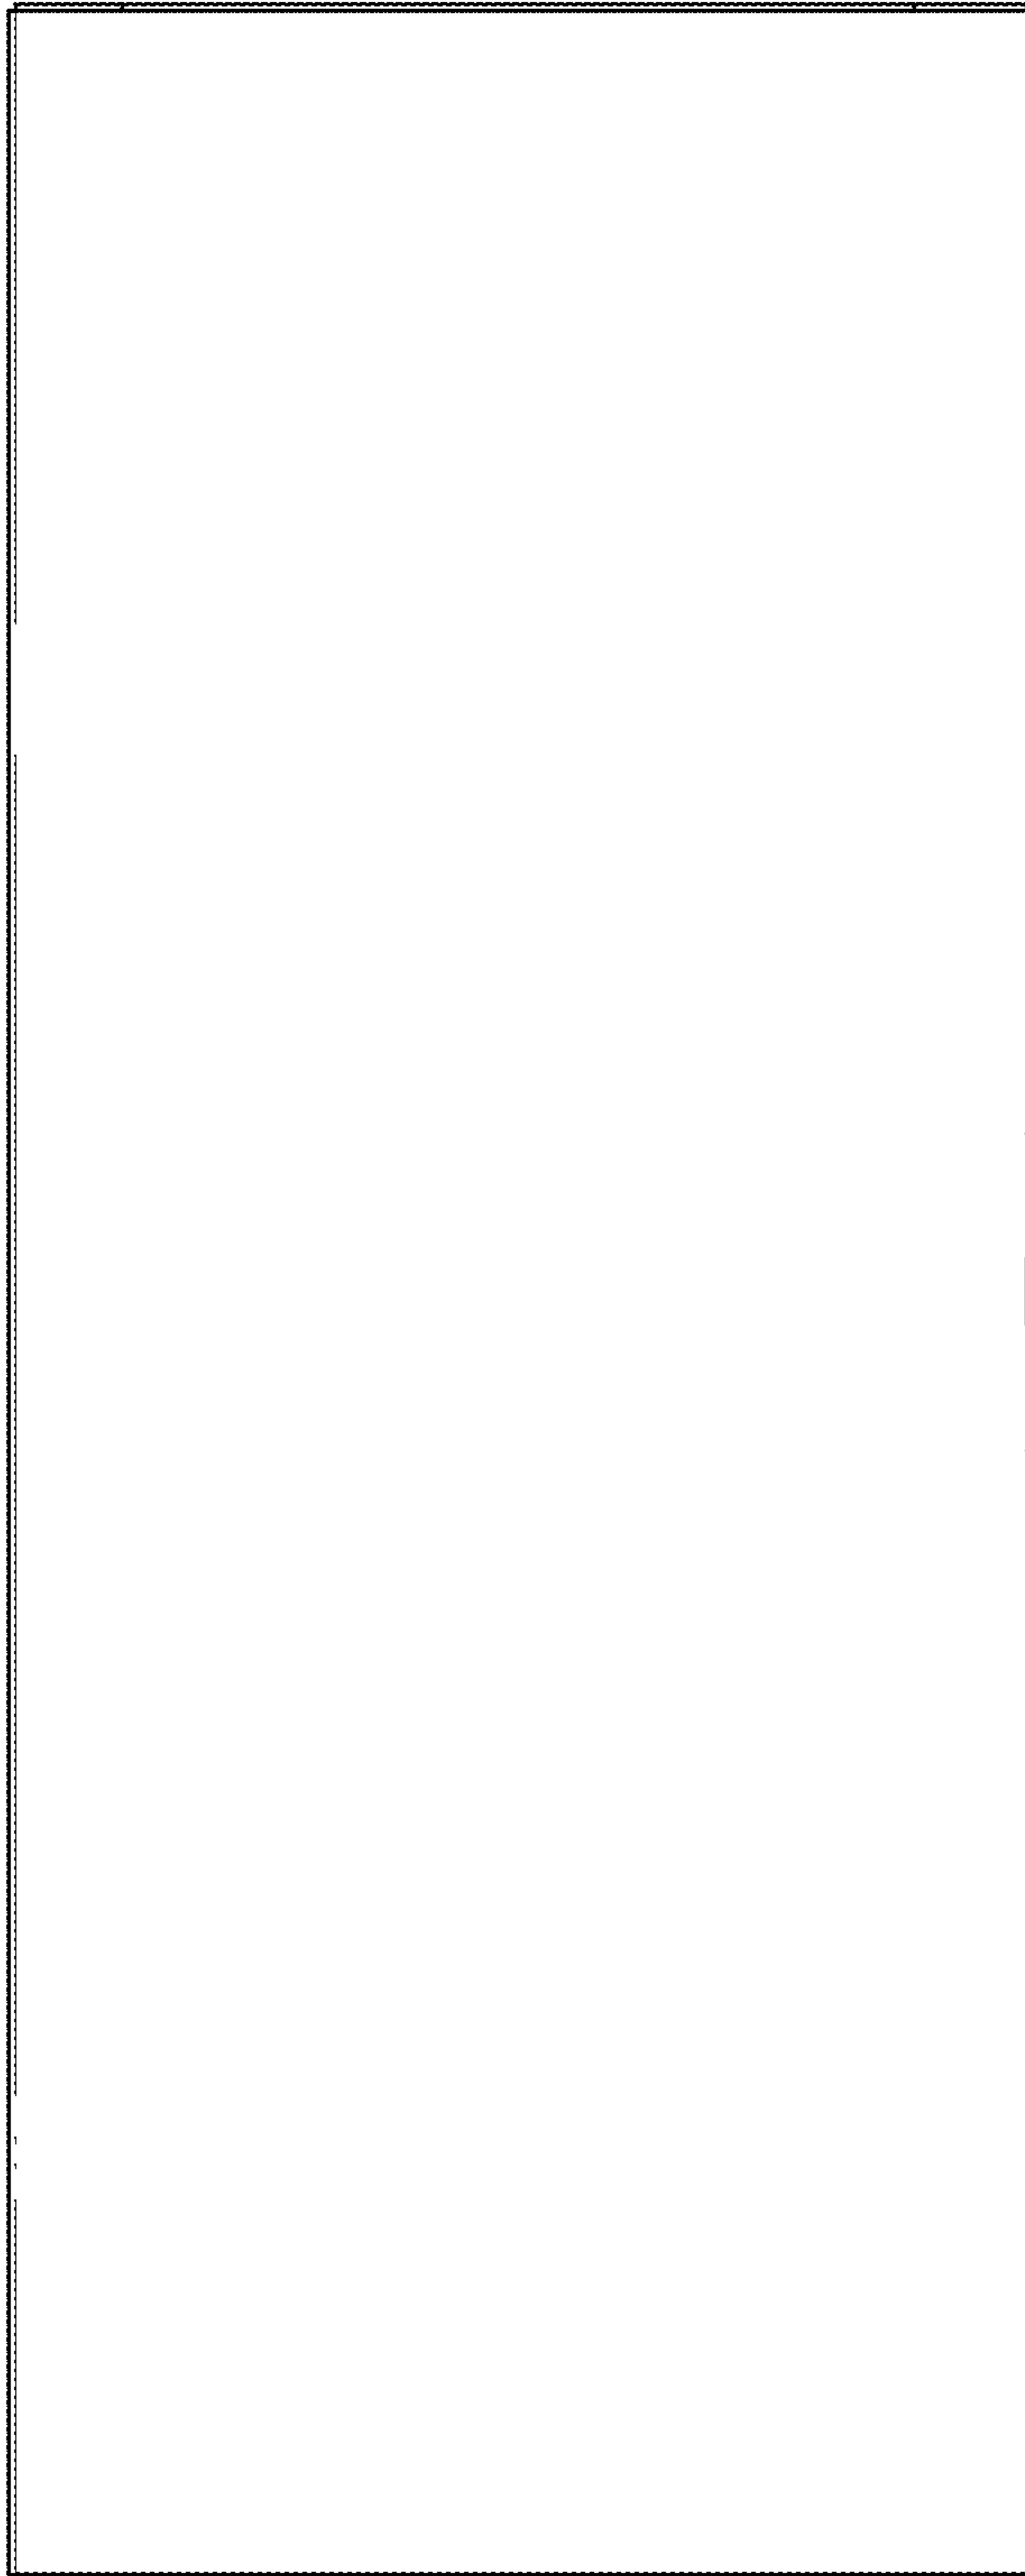

*FIG. 6*

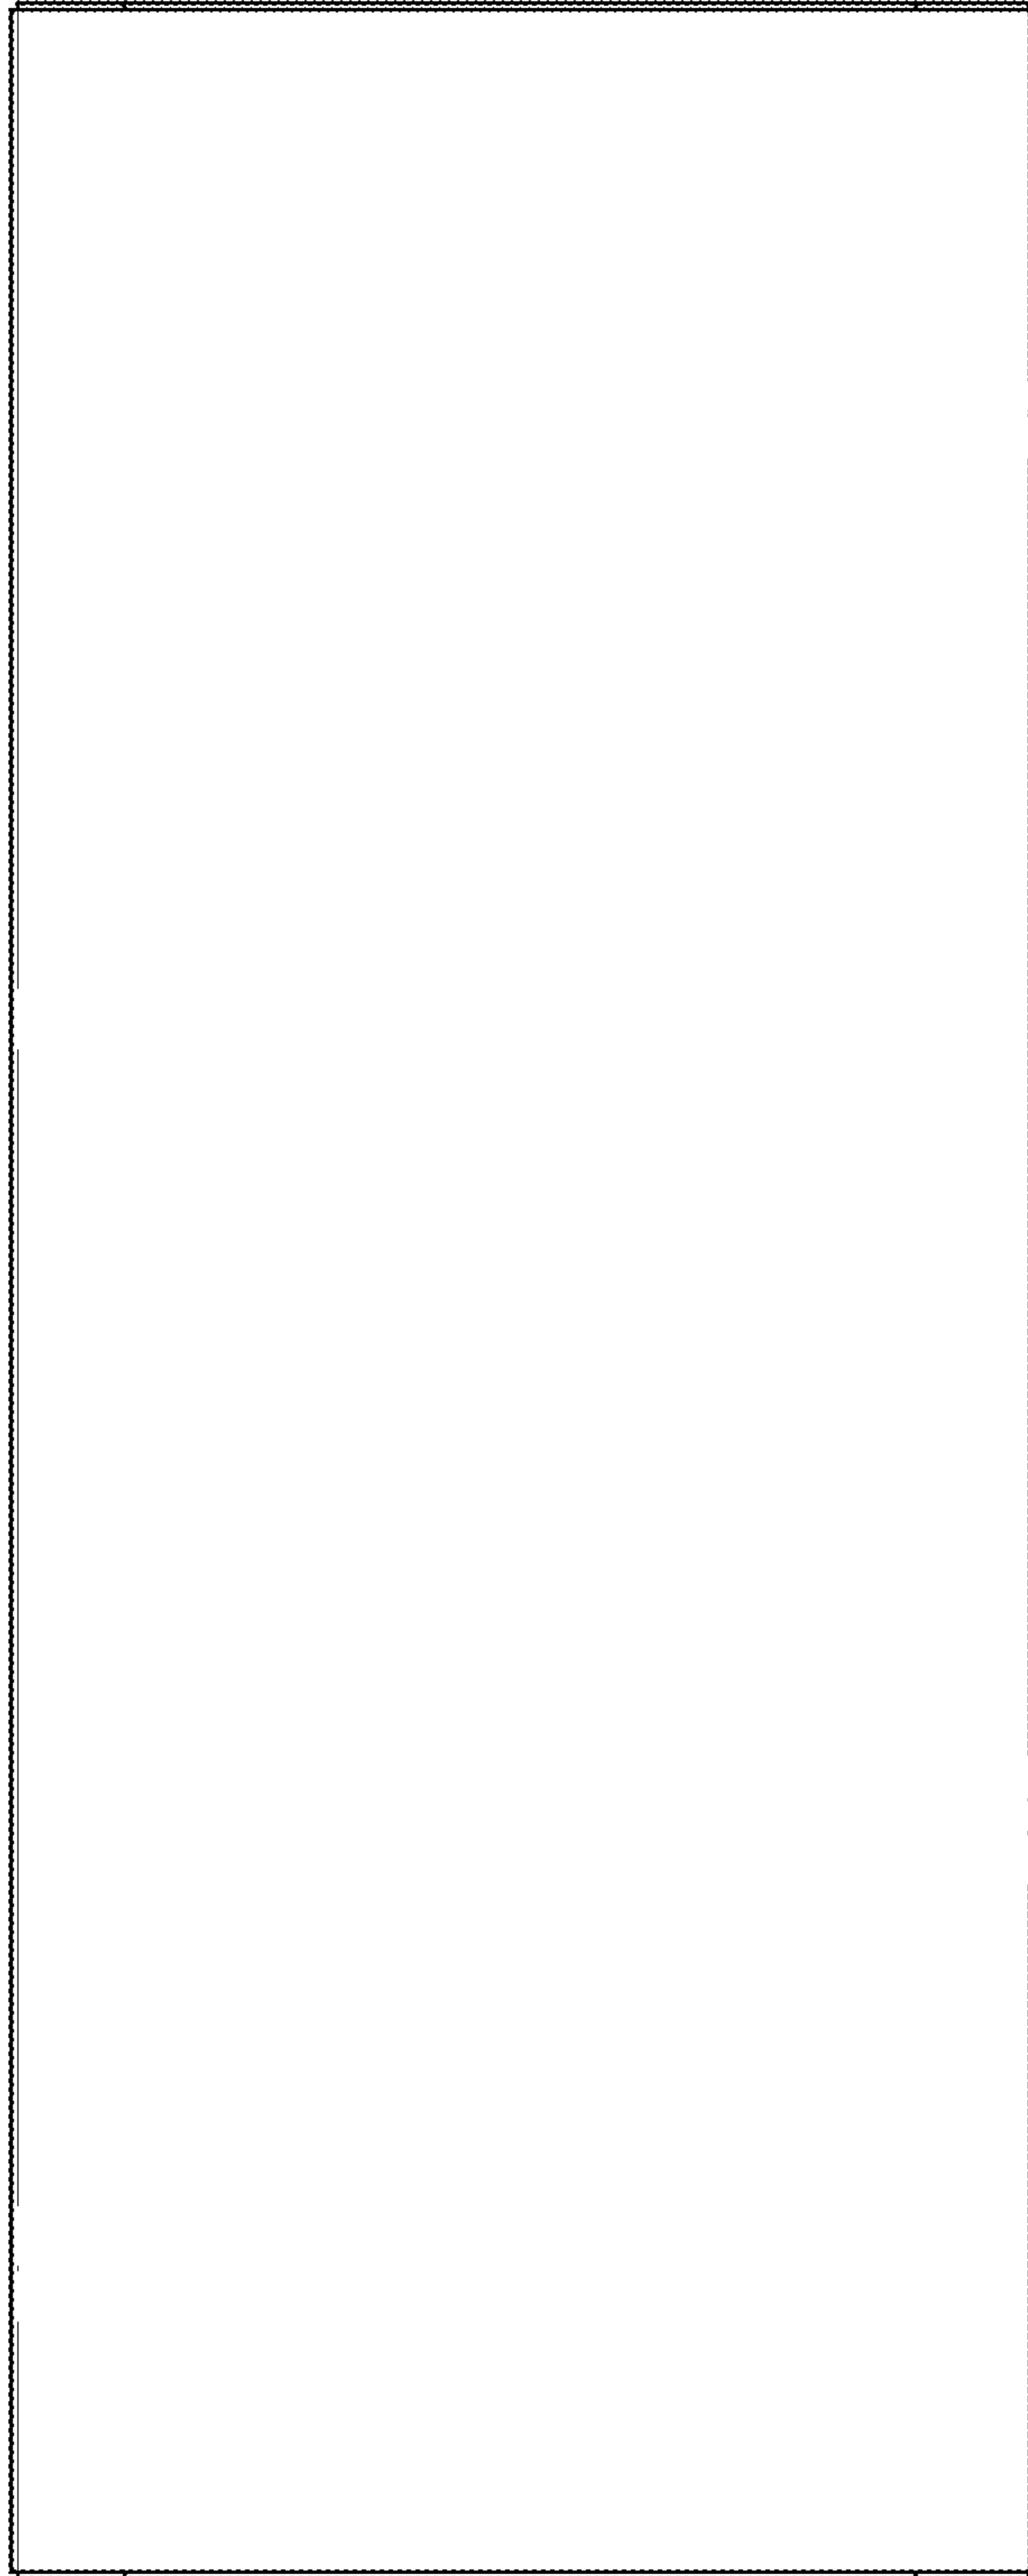

*FIG. 7*





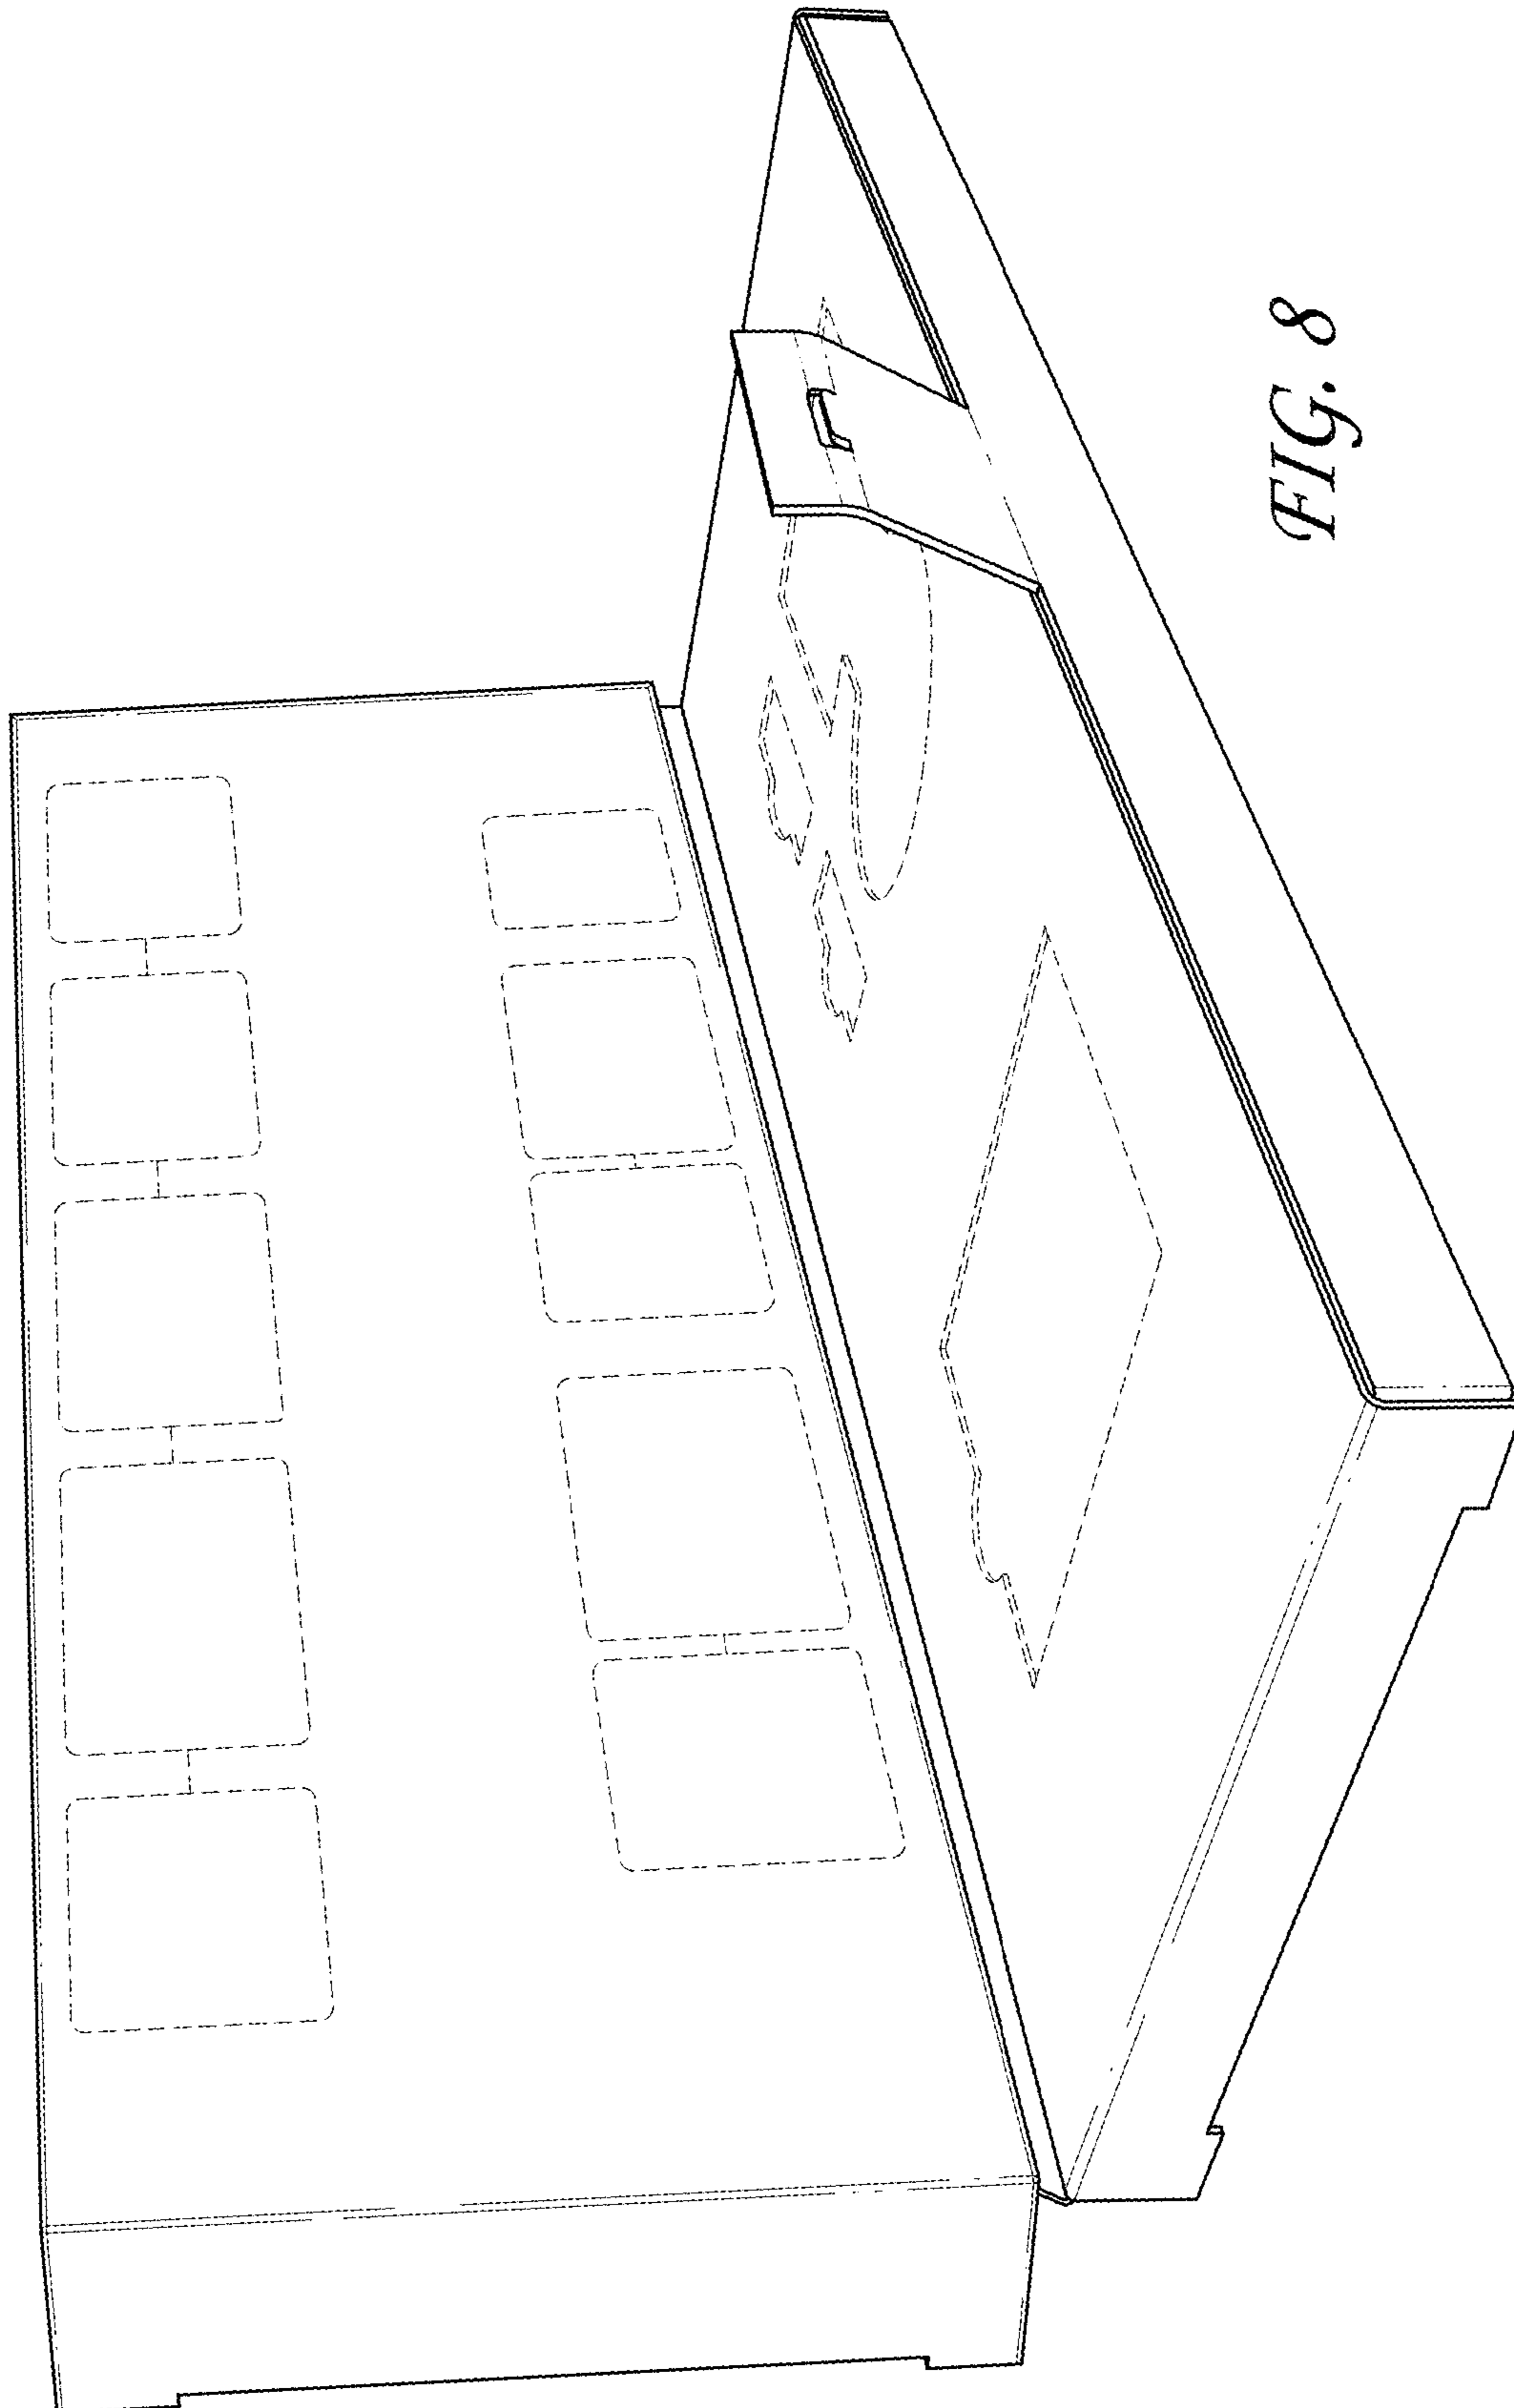



FIG. 8

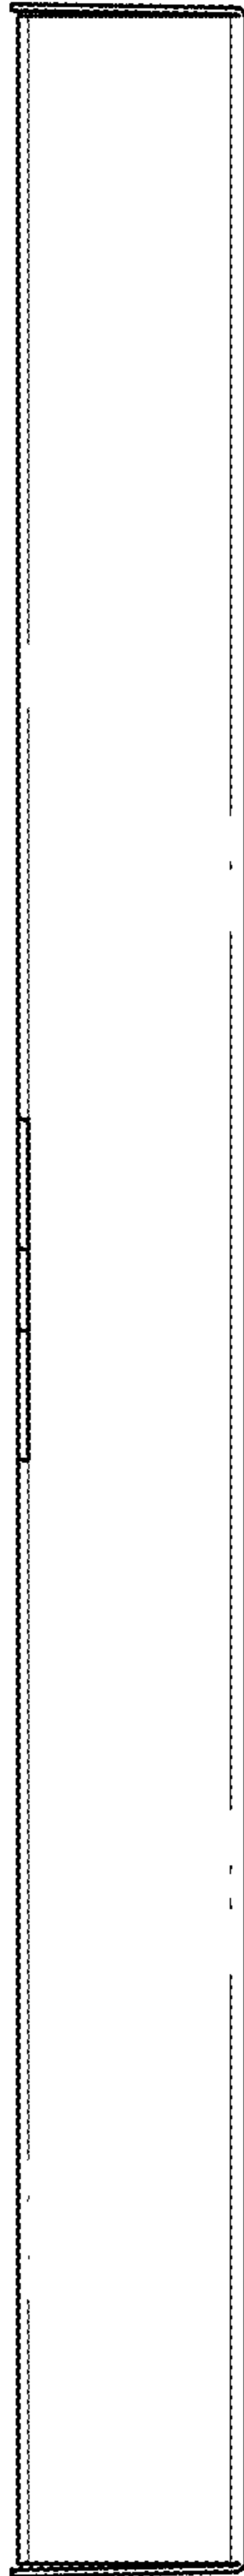


*FIG. 9*

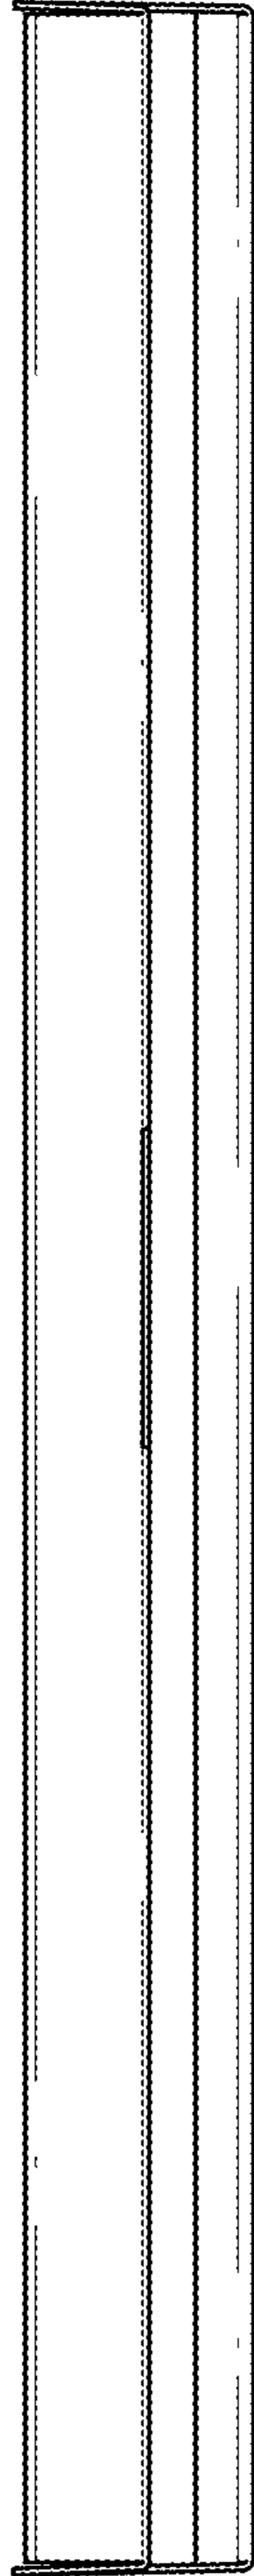


*FIG. 10*

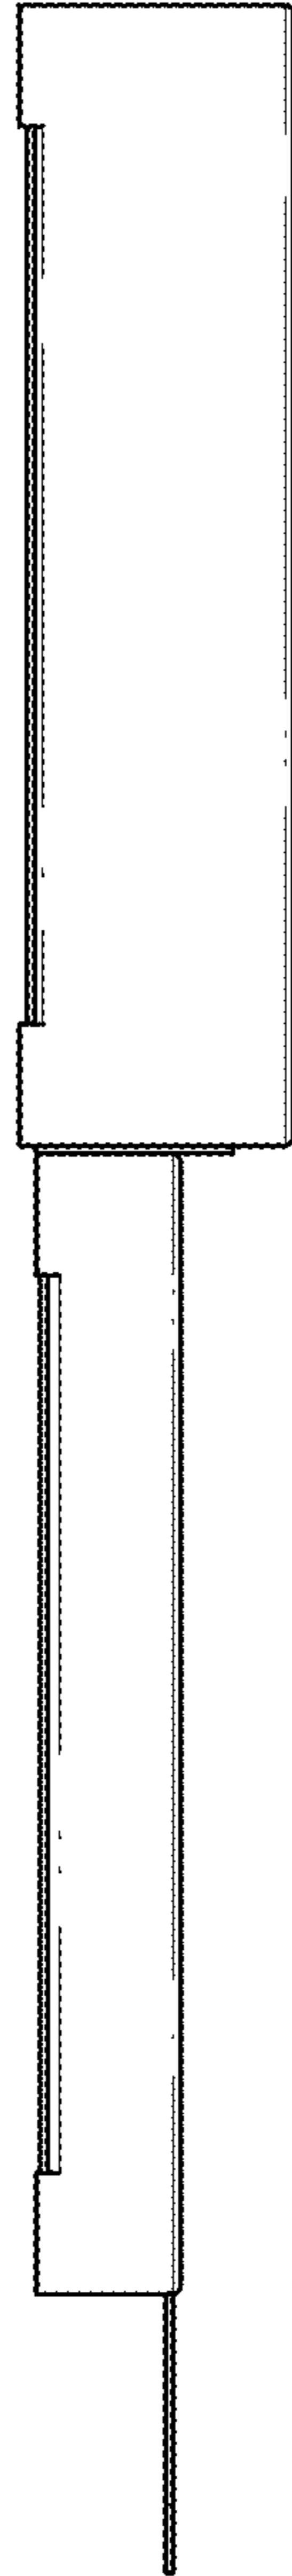

*FIG. 11*

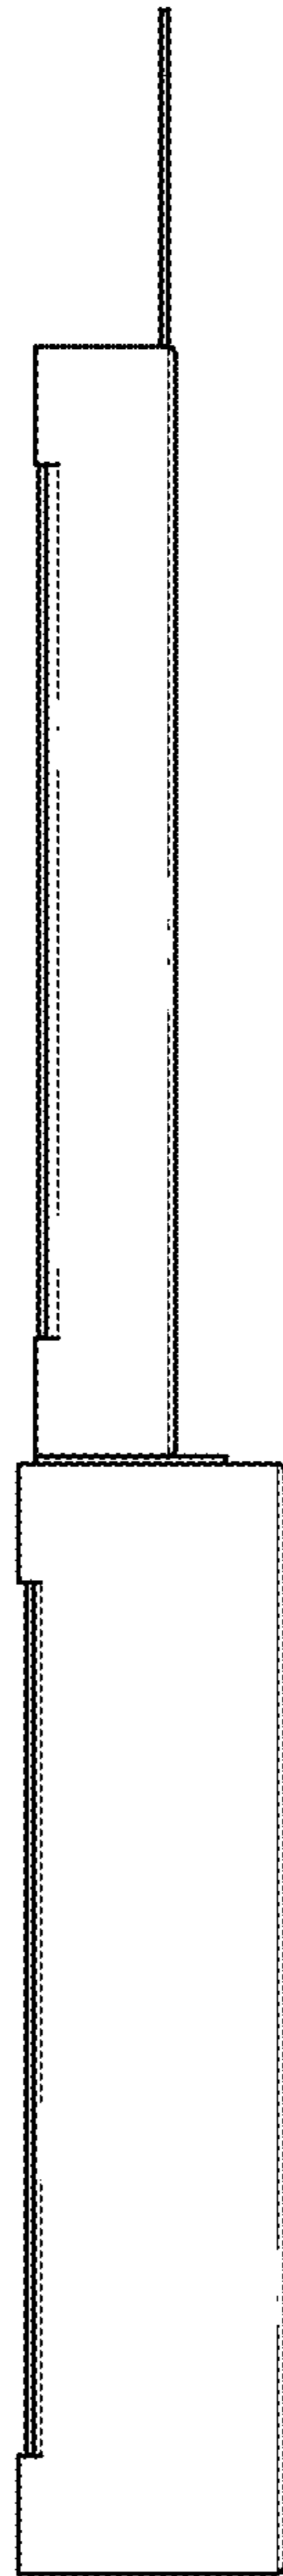

*FIG. 12*

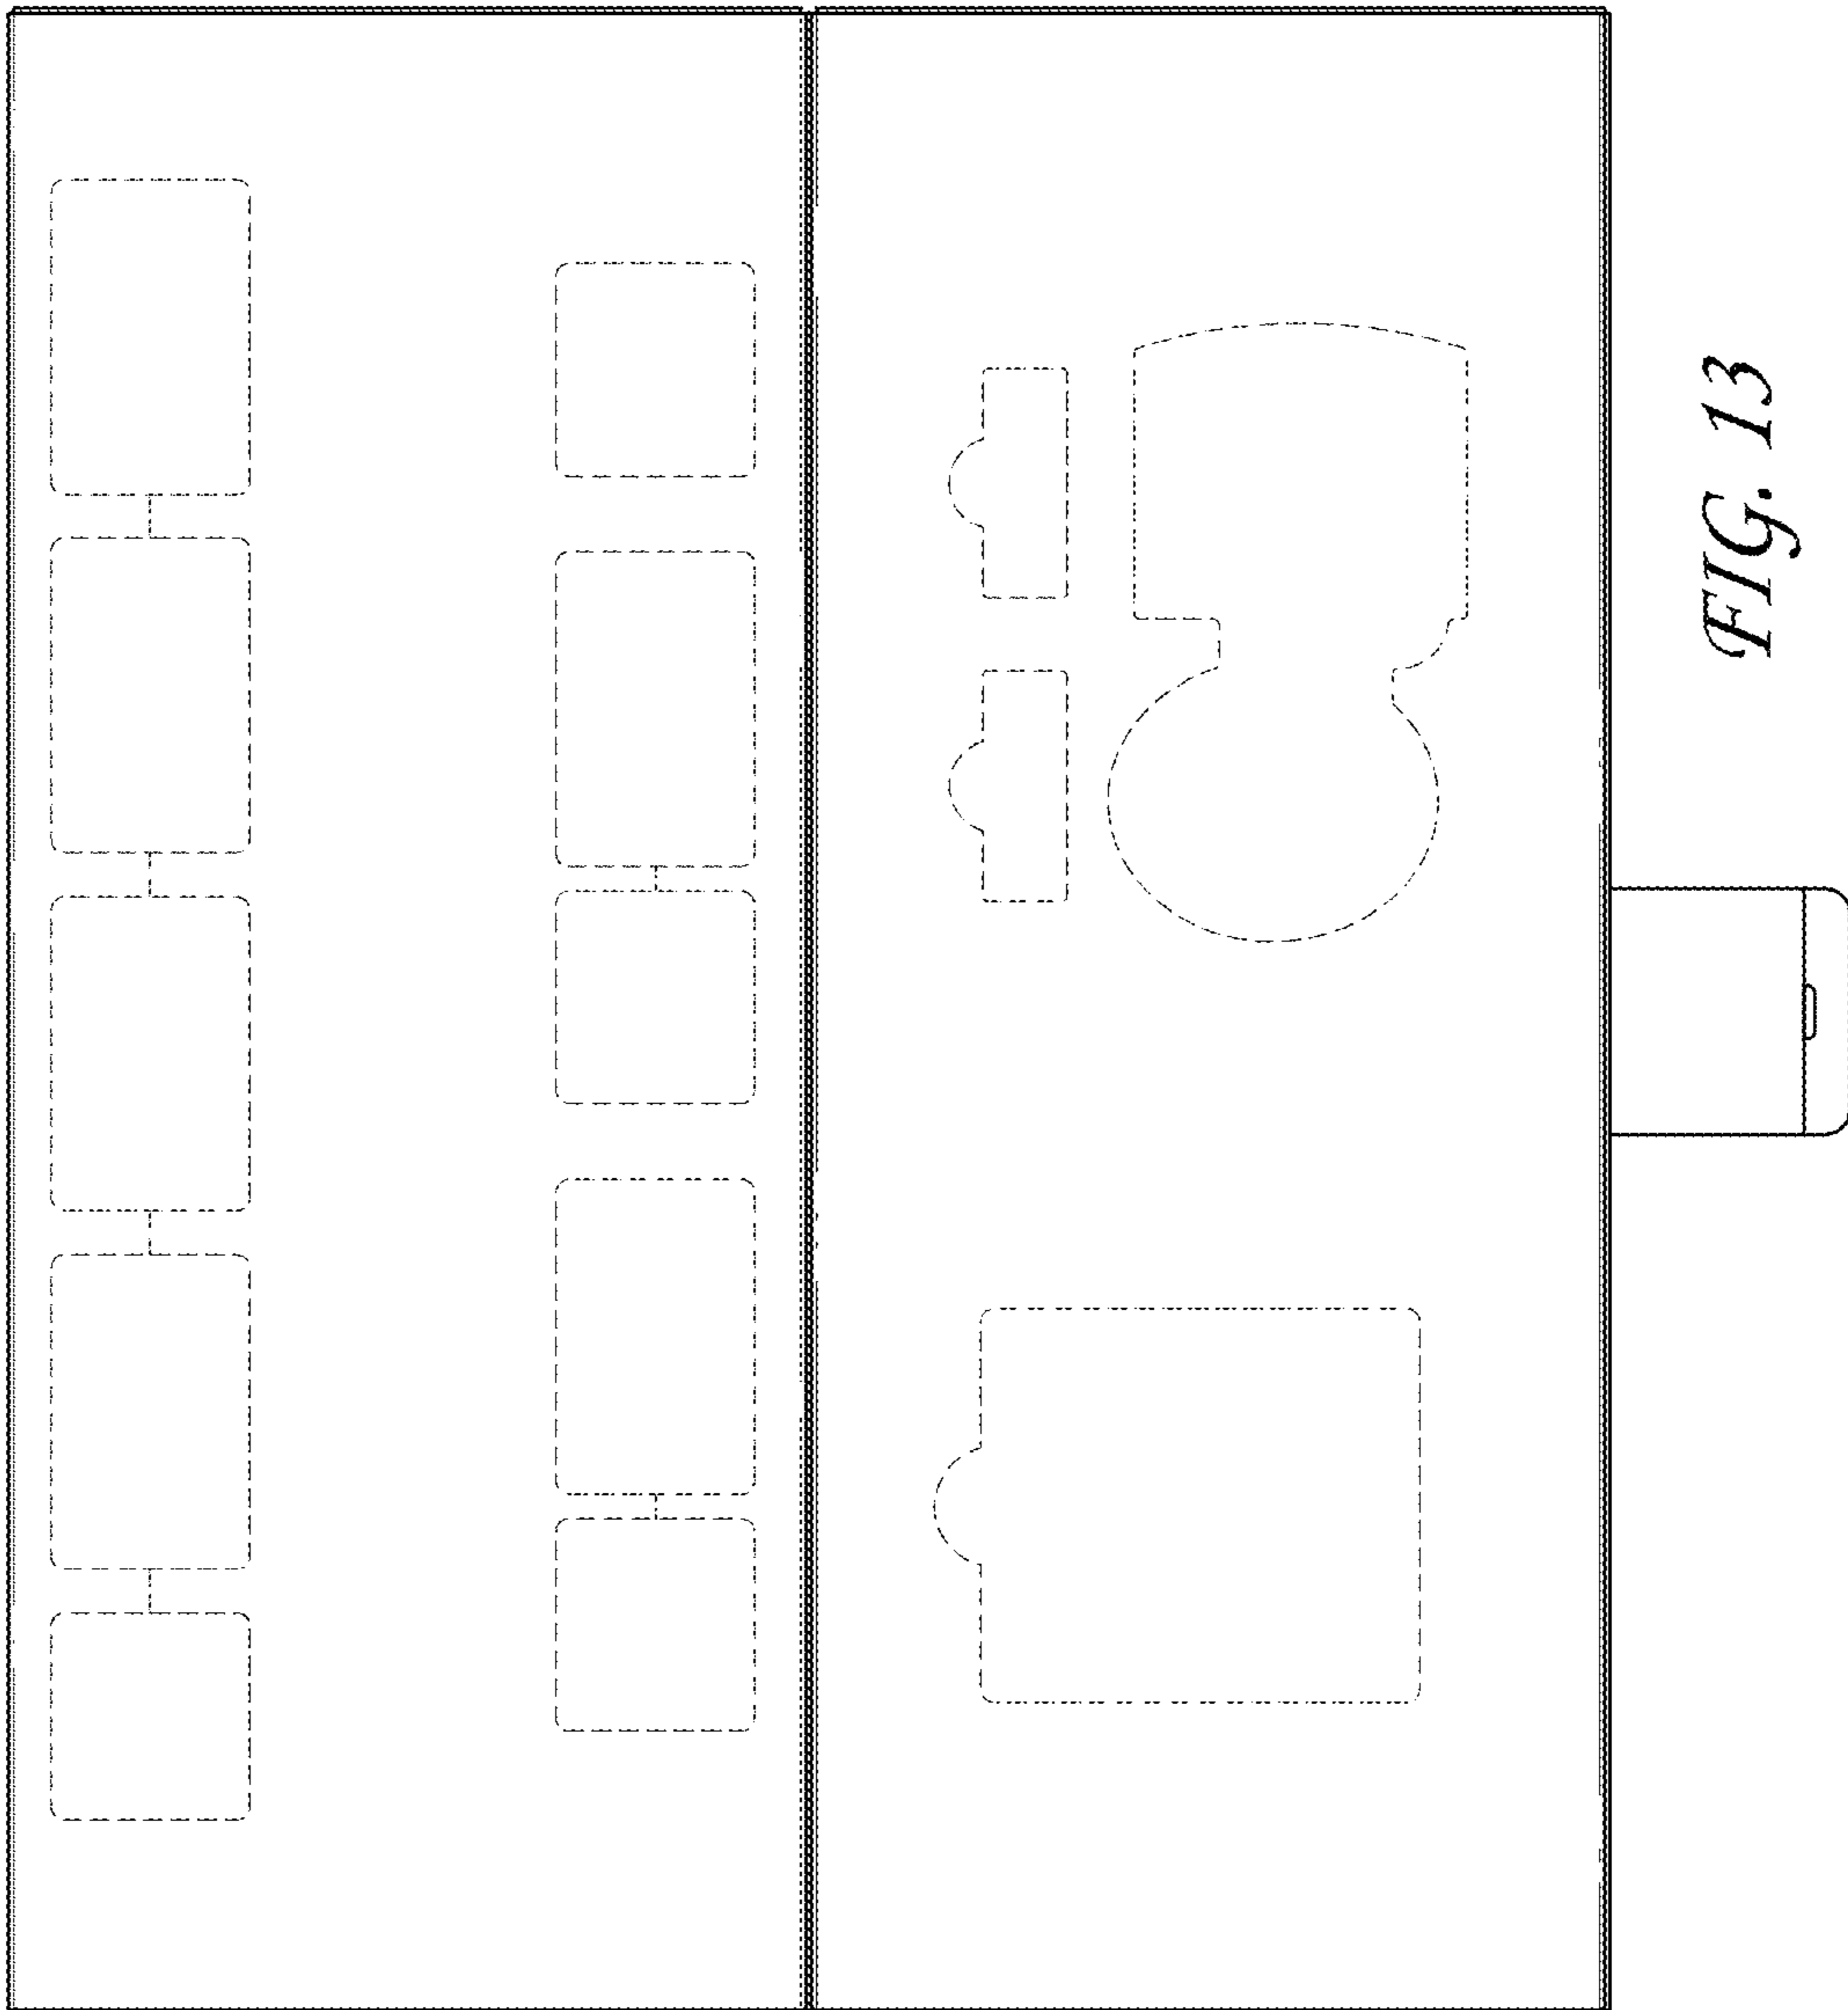

*FIG. 14*

