



US00D777315S

(12) **United States Design Patent** (10) **Patent No.:** **US D777,315 S**
Christman et al. (45) **Date of Patent:** **** Jan. 24, 2017**

(54) **EVACUATED AIR CHAMBER** 3,410,300 A 11/1968 Mondano
3,426,745 A 2/1969 Farr
(71) Applicant: **QUINTRON INSTRUMENT** 3,544,273 A 12/1970 McConnaughey
COMPANY INC., Milwaukee, WI 3,602,531 A 8/1971 Patry
(US) 3,676,073 A * 7/1972 Luckey G01N 33/497
422/510

(72) Inventors: **Norbert John Thomas Christman**,
Wauwatosa, WI (US); **Steven D**
Hamilton, Greenfield, WI (US);
Katherine M Ross, West Allis, WI
(US)

(Continued)

FOREIGN PATENT DOCUMENTS

DE 4028387 3/1992
FR 1294835 4/1962

(Continued)

(73) Assignee: **QuinTron Instrument Company, Inc.**,
Milwaukee, WI (US)

OTHER PUBLICATIONS

(**) Term: **14 Years**

Sucrose Intolerance/Deficiency Home Breath Test Kit. Quintron.
www.breathtests.com. Date accessed: Sep. 13, 2016. <<http://www.breathtests.com/breath-tests-home/sucrose-breath-test.html>>.*

(21) Appl. No.: **29/525,440**

(Continued)

(22) Filed: **Apr. 29, 2015**

Related U.S. Application Data

(63) Continuation of application No. 13/221,446, filed on
Aug. 30, 2011, now abandoned.

(51) **LOC (10) Cl.** **29-02**

(52) **U.S. Cl.**
USPC **D24/110; D24/224**

(58) **Field of Classification Search**
USPC D24/107, 110-110.1, 110.5, 121, 127,
D24/164, 216, 224; D9/516, 544,
D9/572-575

CPC A61B 5/08; A61B 5/082; A61B 5/097;
G01N 33/497

See application file for complete search history.

Primary Examiner — Barbara Fox
Assistant Examiner — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Ryan Kromholz &
Manion, S.C.

(57) **CLAIM**

The ornamental design for an evacuated air chamber, as
shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an evacuated air chamber
showing the new design;

FIG. 2 is a front elevation view, the rear elevation view, the
right side elevation view and the left side elevation view
being identical;

FIG. 3 is a top plan view thereof; and,

FIG. 4 is a bottom plan view thereof.


The broken lines in the drawings illustrate portions of the
evacuated air chamber that form no part of the claimed
design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,191,700 A 7/1910 Howes
1,467,615 A 9/1923 Fairbanks
2,893,683 A 7/1959 Lane
3,303,840 A 2/1967 Etzlinger
3,388,705 A 6/1968 Grosshandler

1 Claim, 1 Drawing Sheet

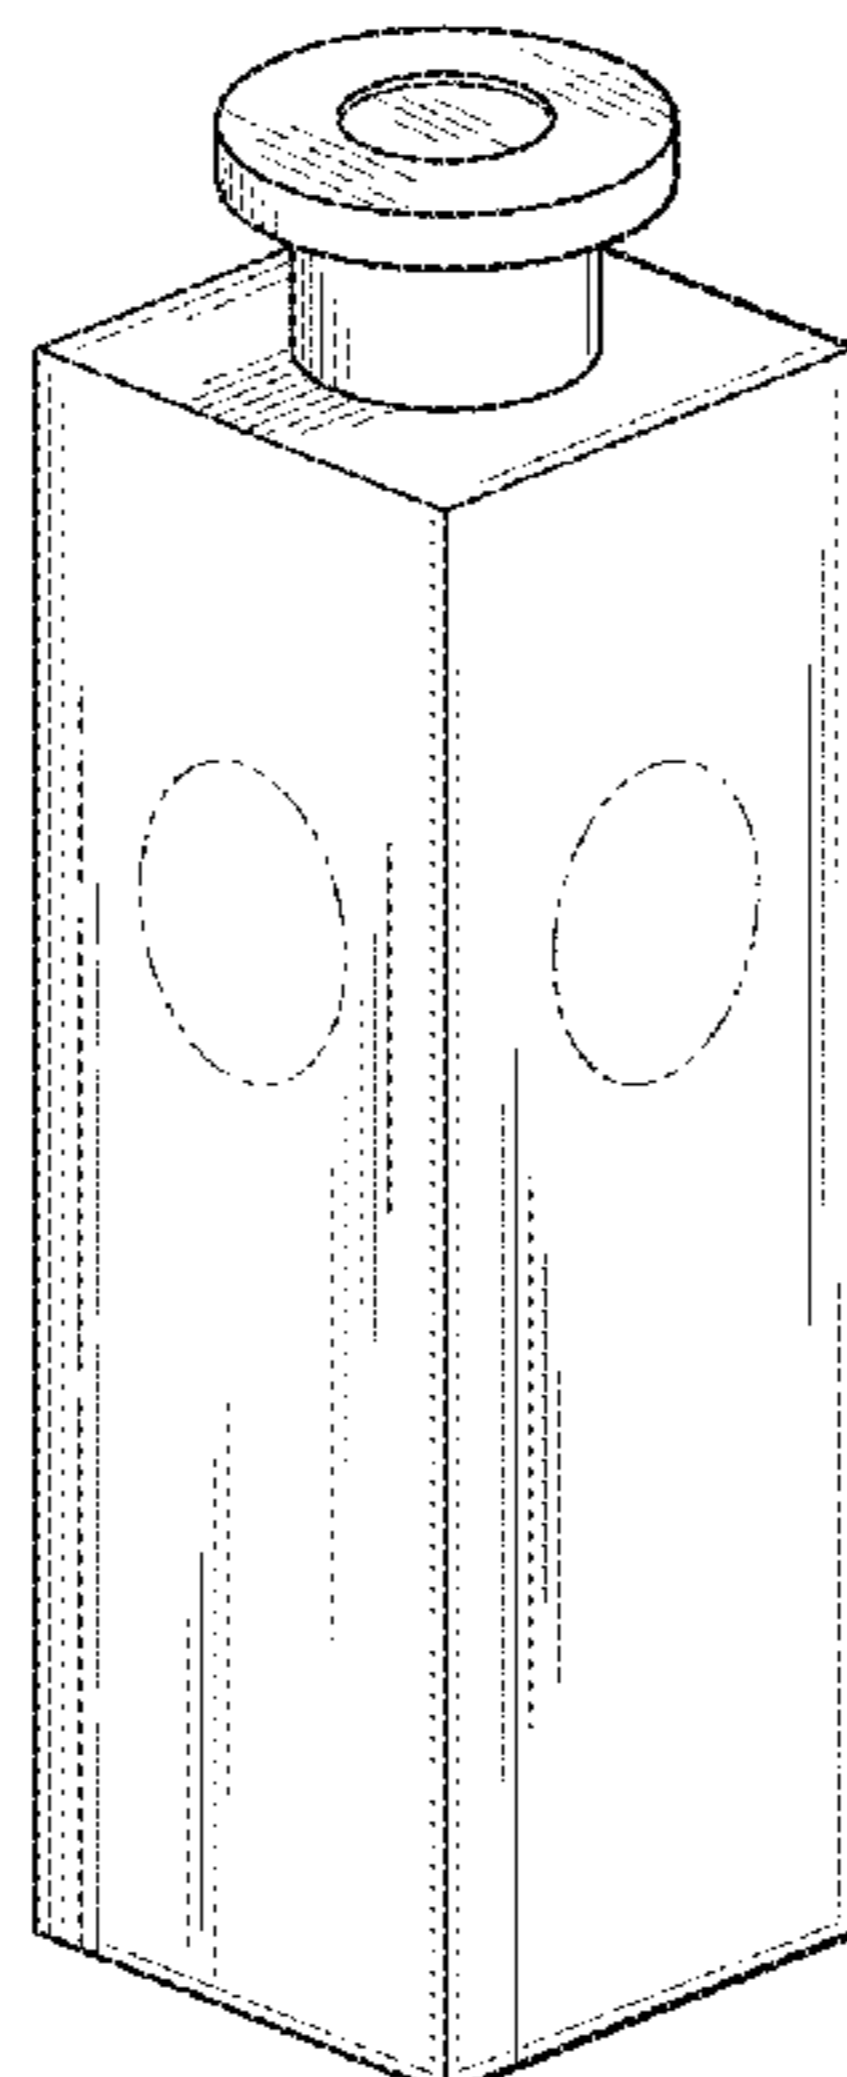

(56)

References Cited

U.S. PATENT DOCUMENTS

3,734,692 A 5/1973 Lucker et al.
 3,777,571 A 12/1973 Jaeger
 3,817,108 A 6/1974 Principe et al.
 3,858,573 A 1/1975 Ryan et al.
 3,923,043 A 12/1975 Yanda
 3,924,832 A 12/1975 Babcock
 4,076,044 A 2/1978 Schindling
 4,161,307 A 7/1979 Clinch et al.
 4,327,741 A 5/1982 Watson
 4,470,412 A 9/1984 Nowacki et al.
 4,506,665 A 3/1985 Andrews et al.
 4,544,273 A 10/1985 Berndt
 4,579,826 A 4/1986 Bolton et al.
 4,580,556 A 4/1986 Kondur
 4,582,054 A 4/1986 Ferrer
 4,585,254 A 4/1986 Adams
 4,587,989 A 5/1986 Mayhew, Jr.
 4,646,786 A 3/1987 Herder et al.
 4,671,298 A 6/1987 Babb et al.
 4,809,692 A 3/1989 Nowacki et al.
 4,821,737 A 4/1989 Nelson
 4,827,921 A 5/1989 Rugheimer
 4,832,015 A 5/1989 Nowacki et al.
 4,852,563 A 8/1989 Gross
 4,852,583 A 8/1989 Walker
 4,919,127 A 4/1990 Pell
 4,938,210 A 7/1990 Shene
 4,947,861 A * 8/1990 Hamilton A61B 5/097
 128/898
 4,953,547 A 9/1990 Poole, Jr.
 5,012,803 A 5/1991 Foley et al.
 5,012,804 A 5/1991 Foley et al.
 5,042,500 A 8/1991 Norlien et al.
 D321,227 S * 10/1991 Norell D21/662
 5,062,423 A 11/1991 Matson et al.
 5,066,597 A 11/1991 Stinson et al.
 5,100,005 A 3/1992 Noble et al.
 5,137,520 A 8/1992 Maxson et al.
 5,140,993 A * 8/1992 Opekun, Jr. A61B 5/097
 422/84
 5,165,393 A 11/1992 Kawaguchi
 5,211,181 A * 5/1993 Delente A61B 5/097
 422/84
 5,327,901 A * 7/1994 Delente A61B 5/097
 422/84
 5,346,089 A 9/1994 Brown
 5,350,078 A 9/1994 Potts et al.
 5,361,772 A * 11/1994 Murnick G01N 33/497
 600/543
 5,432,094 A * 7/1995 Delente A61B 5/097
 422/413
 5,467,776 A * 11/1995 Hamilton A61B 5/097
 600/543
 5,711,306 A * 1/1998 Guilluy A61B 5/097
 215/228

D395,895 S 7/1998 Flinn
 5,834,626 A 11/1998 De Castro et al.
 5,957,839 A 9/1999 Kruse et al.
 6,017,317 A 1/2000 Newby et al.
 6,016,122 A 2/2000 Chen
 6,171,811 B1 * 1/2001 Becerro
 De Bengoa Vallejo . C12Q 1/16
 435/29
 6,368,558 B1 4/2002 Suslick et al.
 6,468,477 B1 10/2002 Hamilton et al.
 6,495,102 B1 12/2002 Suslick et al.
 D469,185 S * 1/2003 Lodge D24/224
 6,632,402 B2 10/2003 Blazewicz et al.
 D487,862 S 3/2004 Tincher
 6,712,770 B2 3/2004 Lin et al.
 D553,254 S * 10/2007 Colin D24/224
 D581,800 S * 12/2008 Rica D9/544
 D689,774 S * 9/2013 Ford D9/544
 D755,957 S * 5/2016 Larson D24/121
 2004/0157281 A1 8/2004 Hulkower et al.
 2004/0222345 A1 11/2004 Lindsay
 2007/0066928 A1 3/2007 Lannoy
 2008/0053439 A1 3/2008 Lighton
 2009/0318823 A1 * 12/2009 Christman A61B 5/097
 600/532
 2010/0182606 A1 7/2010 Prenner et al.
 2012/0226183 A1 * 9/2012 Christman G01N 33/497
 600/543
 2016/0022946 A1 * 1/2016 Sislian G01N 1/2202
 600/543
 2016/0242674 A1 * 8/2016 Ahmad A61B 5/082
 2016/0245797 A1 * 8/2016 Ahmad G01N 33/52

FOREIGN PATENT DOCUMENTS

FR 2497686 7/1982
 GB 2230456 10/1990
 WO 9311817 6/1993

OTHER PUBLICATIONS

Aerodiagnostics Easy Sampler Breath Collection Kit. Date accessed: Sep. 13, 2016. <<https://nebula.wsimg.com/b0933154914d3502099648ec3335e5b4?AccessKeyId=28AC0744C4440494CAA5&disposition=0&alloworigin=1>>.*
 Monaghan Medical Corp Brochure, "Topical Dosage for Young Asthmatic Children with M.D.I. Aerosol Medications", Apr. 1989.
 Rakow, N.A.; Suslick, K.S. "A Colorimetric Sensor Array for Odour Visualization" Nature, 2000, 406, 710-714; Suslick, K.S. Rakow, N.A.
 mvw.chemsensing.com/hepatotoxicity.html—ChemSensing, Hepatotoxicity, 2004.
 www.chemsensing.com/elisa.html—ChemSensing, ELISA, 2004.

* cited by examiner

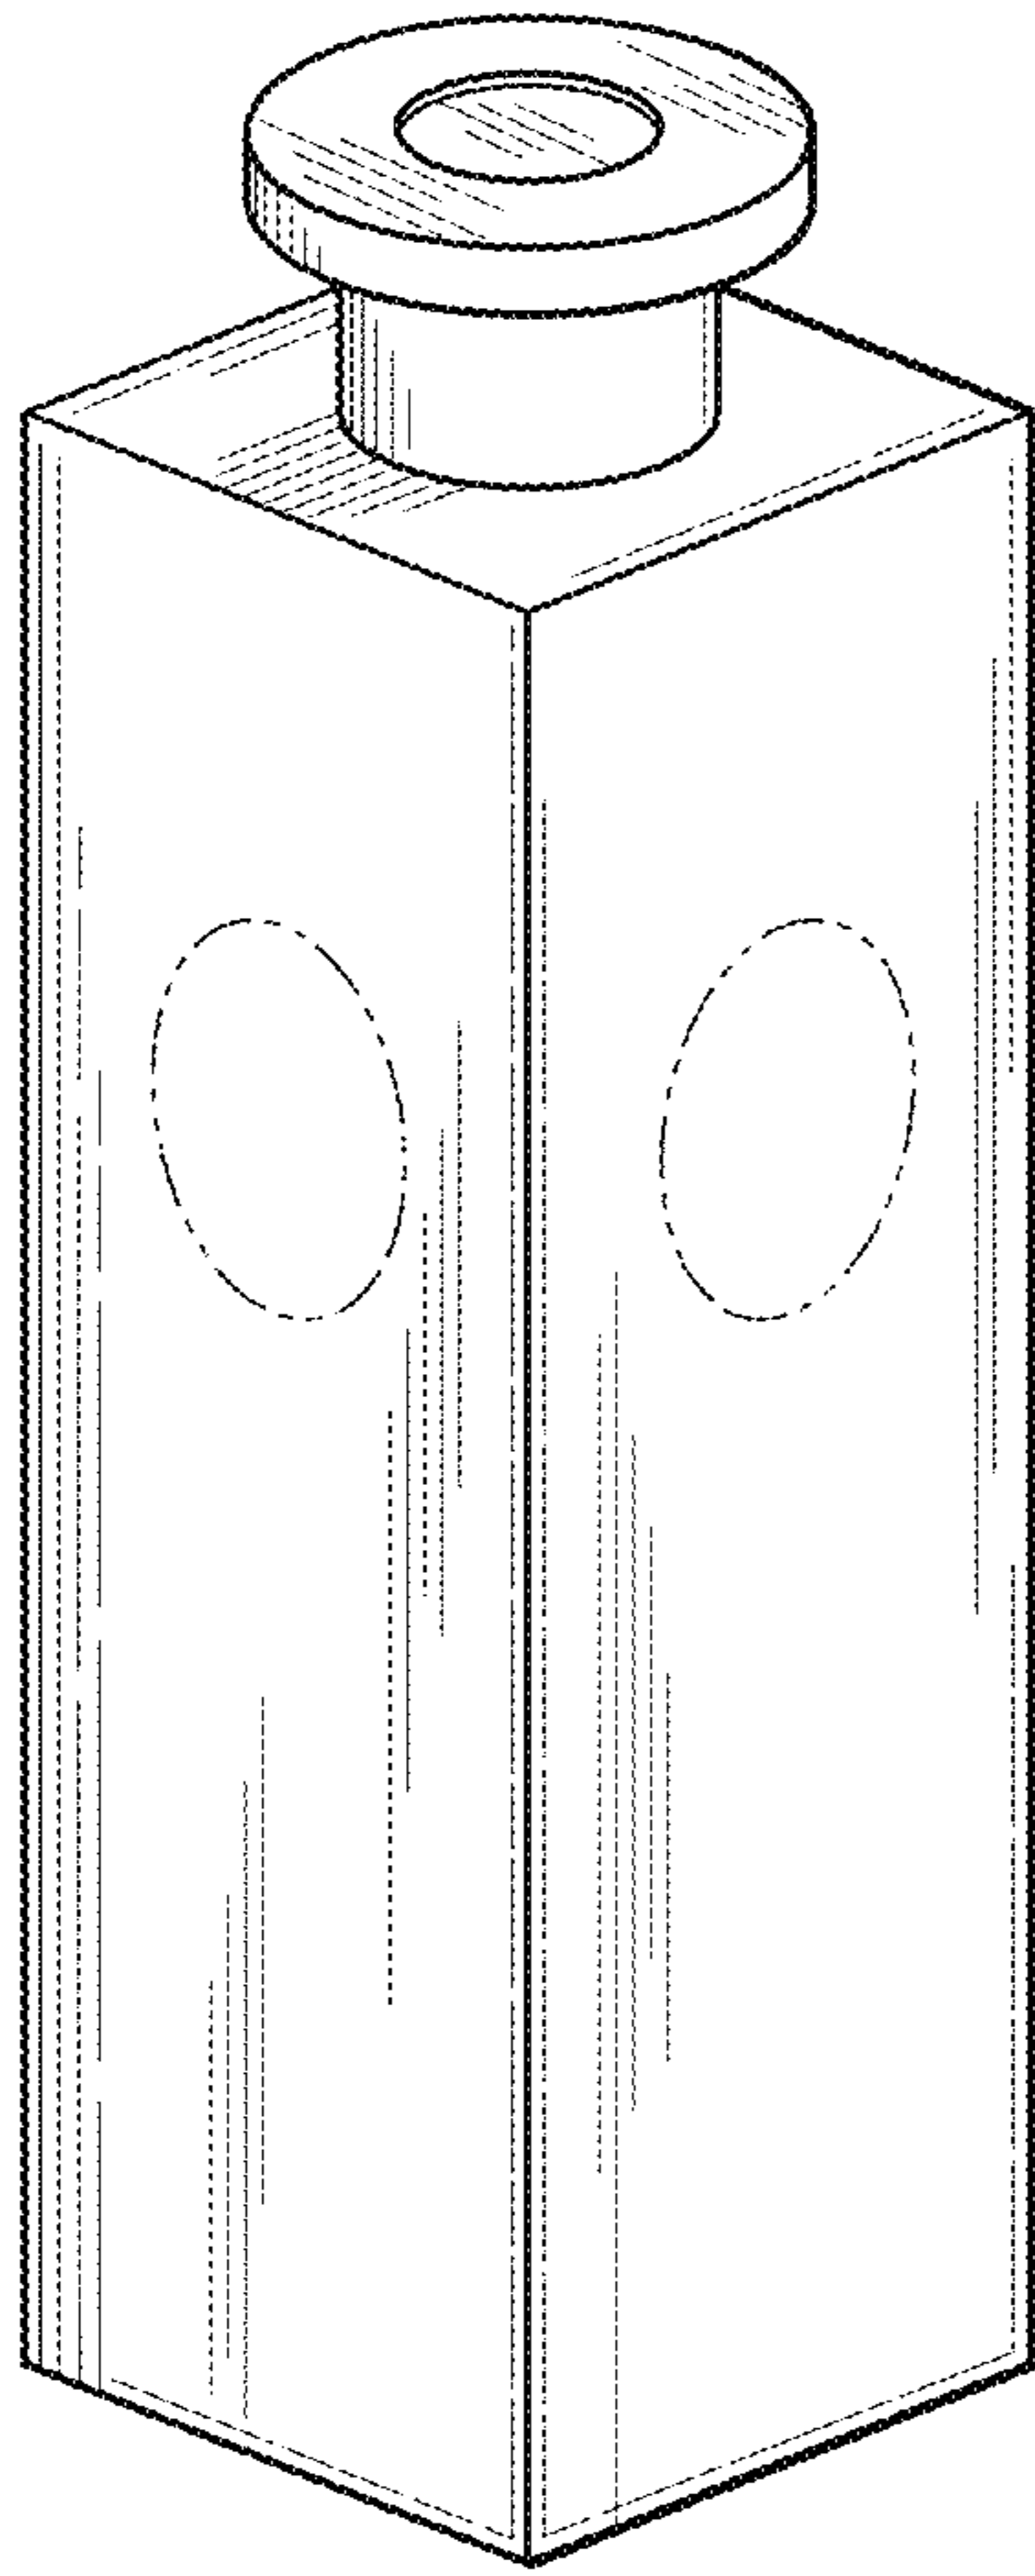


Fig. 1

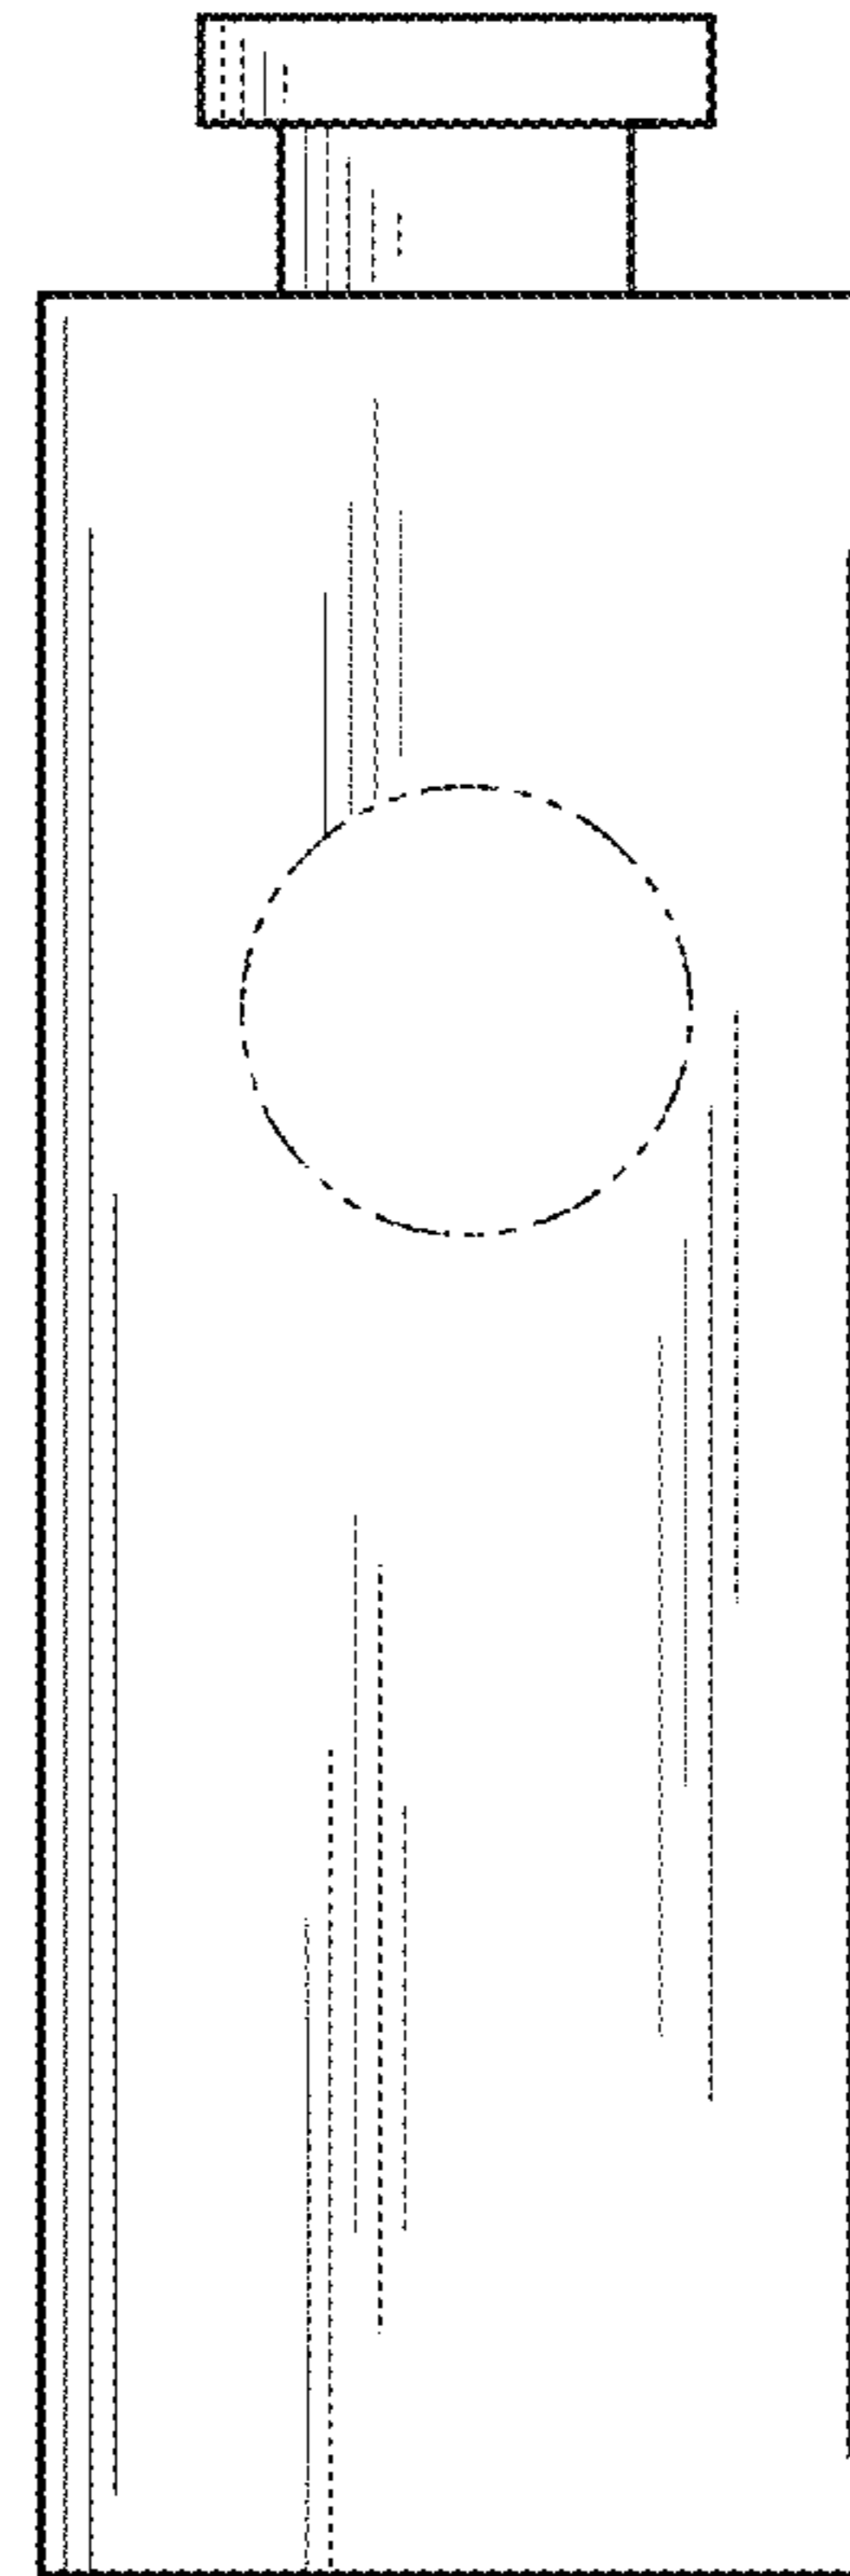


Fig. 2

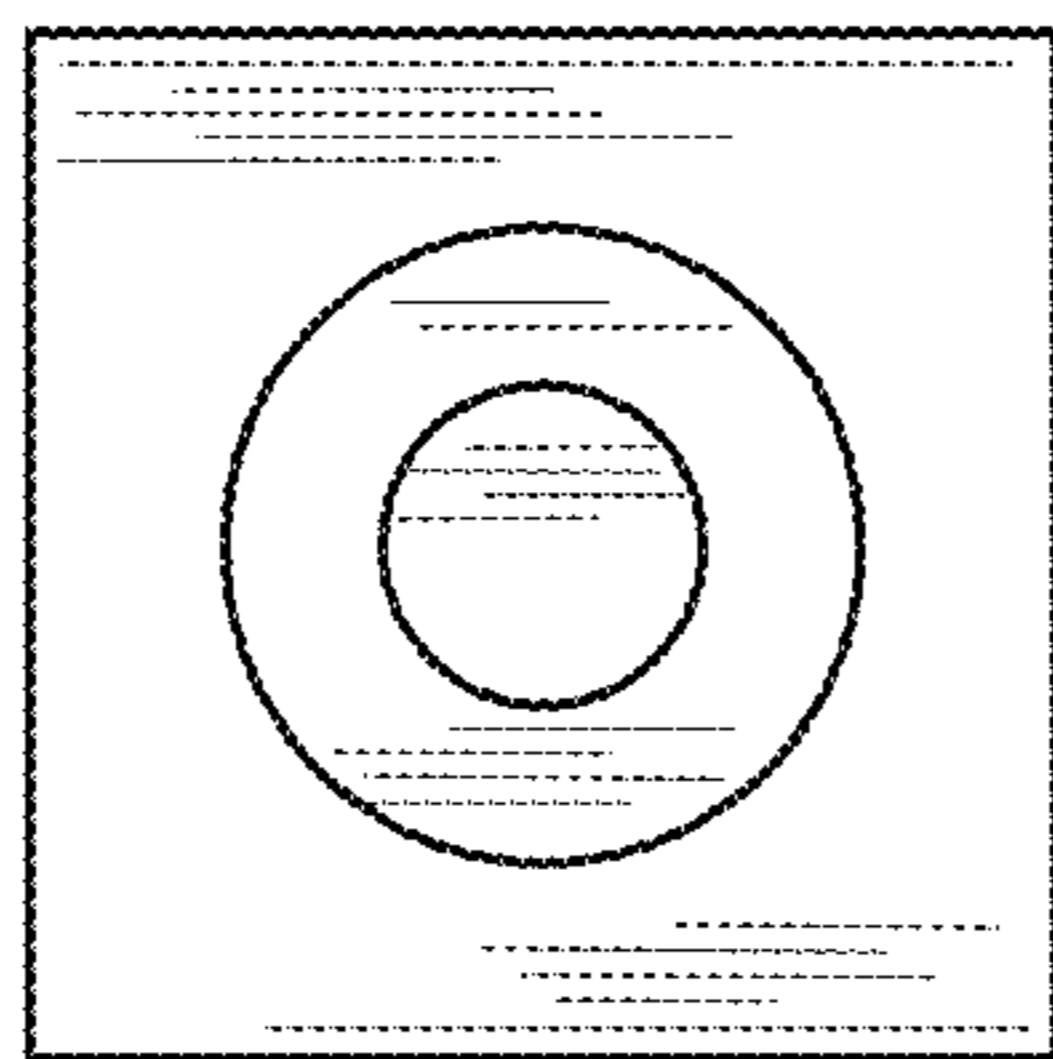


Fig. 3

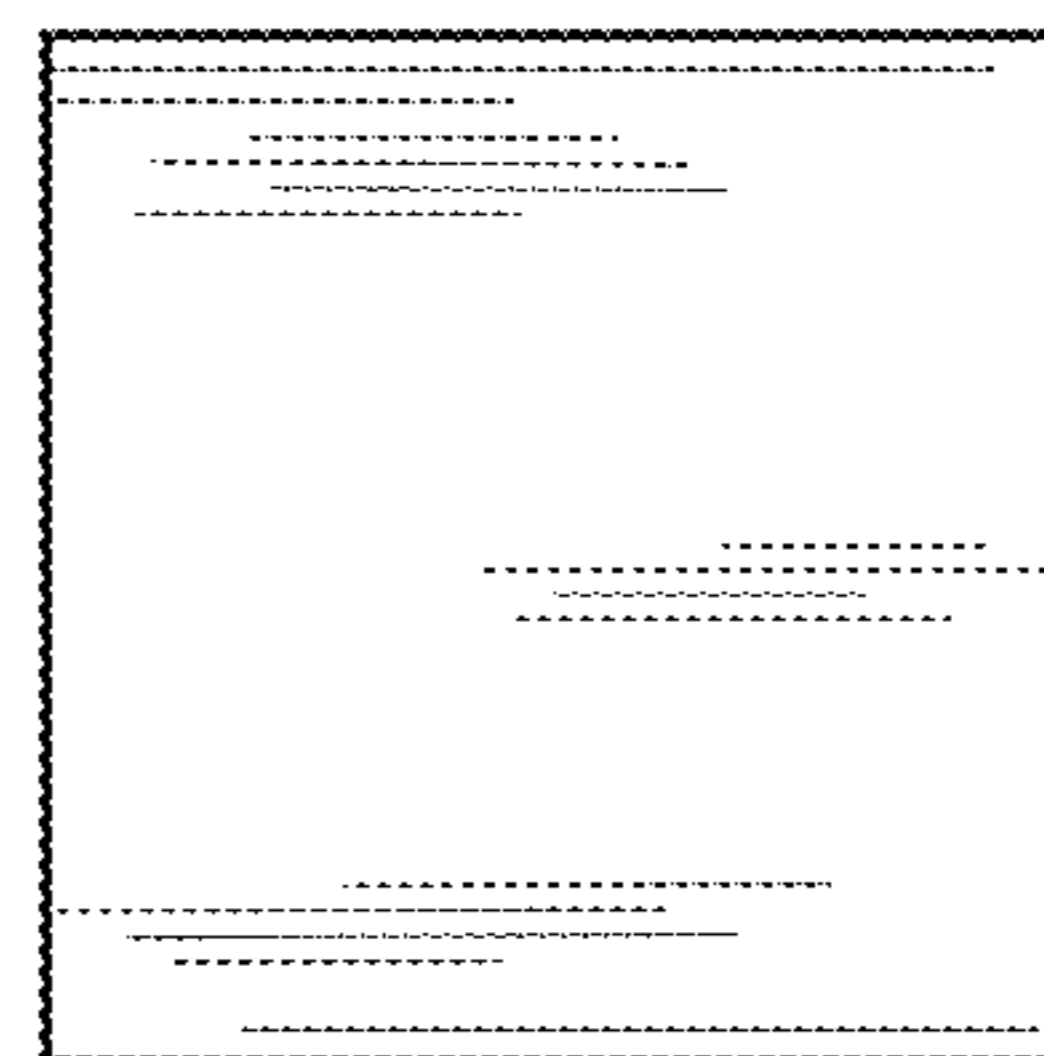


Fig. 4

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D777,315 S
APPLICATION NO. : 29/525440
DATED : January 24, 2017
INVENTOR(S) : Norbert John Thomas Christman et al.


Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On Page 2 (56) References Cited; Other Publications:

“mvw.chemsensing.com/hepatotoxicity.html-ChemSensing, Hepatotoxicity, 2004” should read
--www.chemsensing.com/hepatotoxicity.html-ChemSensing, Hepatotoxicity, 2004--

Signed and Sealed this
Sixth Day of June, 2017

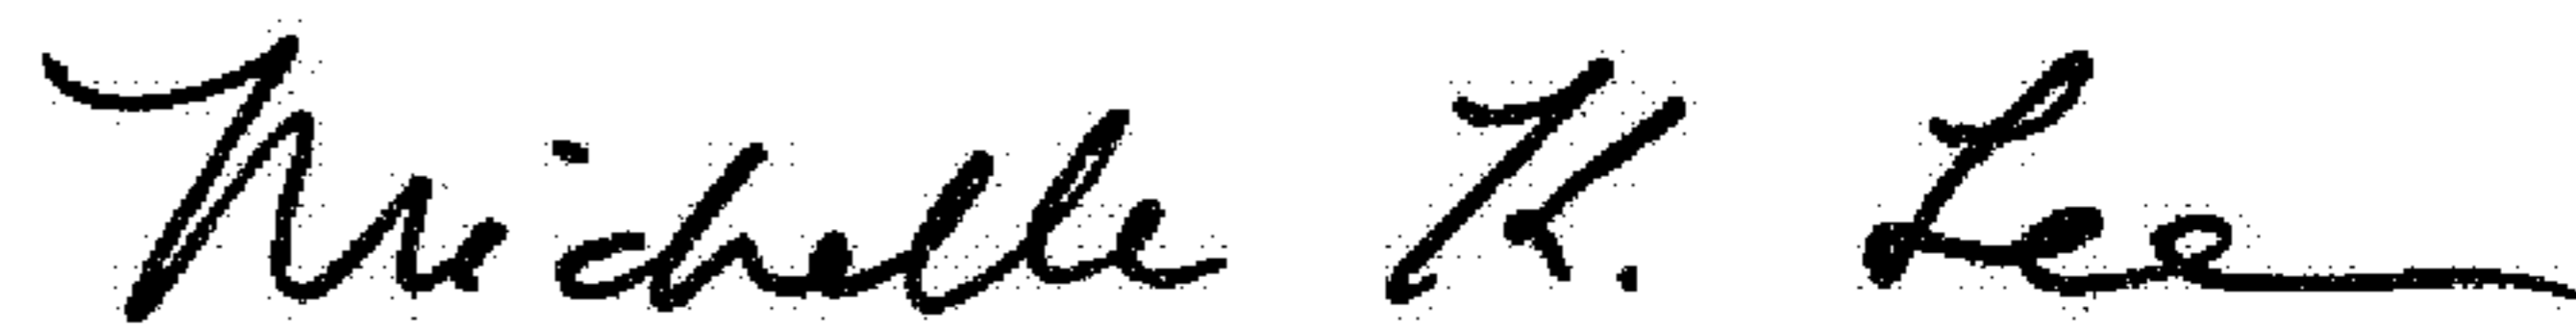

Michelle K. Lee
Director of the United States Patent and Trademark Office