

US00D777335S

(12) **United States Design Patent** (10) **Patent No.:** **US D777,335 S**
Rurling et al. (45) **Date of Patent:** **** Jan. 24, 2017**

(54) **FRAME FOR NEUROLOGICAL FIXATION DEVICE**
(71) Applicant: **ELEKTA AB (PUBL)**, Stockholm (SE)
(72) Inventors: **Erik Rurling**, Bromma (SE); **Anna Wik**, Hägersten (SE); **Malin Svensson**, Stockholm (SE); **Ivars Alksnis**, Trångsund (SE); **Marianne Plantz**, Stockholm (SE); **Mathias Stavervik**, Stockholm (SE)

D676,139 S * 2/2013 Golzari D24/200
D750,264 S * 2/2016 Guarraia D24/200
D752,236 S * 3/2016 Guarraia D24/200
D752,766 S * 3/2016 Guarraia D24/200
2008/0097195 A1 4/2008 Urquhart et al.
2012/0060847 A1* 3/2012 Stratton A61B 19/203
128/845

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2013/011443 A1 1/2013

OTHER PUBLICATIONS

An OEM Partner With a Medical Quality System Already in Place [online]. SHL Group, 2009 [retrieved on Sep. 12, 2016]. Retrieved from the Internet:< <http://www.shl-group.com/product/neurosurgical-equipment/>>.*

Primary Examiner — Eric Goodman
Assistant Examiner — Sloan Rozin

(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch & Birch, LLP

(73) Assignee: **ELEKTA AB PUBL**, Stockholm (SE)

(**) Term: **14 Years**

(21) Appl. No.: **29/504,731**

(22) Filed: **Oct. 8, 2014**

(30) **Foreign Application Priority Data**

Oct. 2, 2014 (EM) 002549915-0002

(51) **LOC (10) Cl.** **24-04**

(52) **U.S. Cl.**
USPC **D24/191**

(58) **Field of Classification Search**
USPC D24/143, 171, 183–185, 188, 190–191,
D24/200

CPC ... A61B 8/40; A61B 19/203; A61B 2017/681;
A61B 5/702; A61B 5/704; A61B 5/706;
A61B 5/708; A61B 6/04; A61B 5/150748;
A47C 20/027; A47C 20/025; A47G 9/10;
A47G 2009/1018; A61G 13/0036; A61F
5/04

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,612,930 A 9/1986 Bremer
5,456,266 A 10/1995 Brown

(57) **CLAIM**


The ornamental design for frame for neurological fixation device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right view of frame for neurological fixation device showing my new design;
FIG. 2 is a bottom, left, rear perspective view thereof;
FIG. 3 is a right side view thereof;
FIG. 4 is a left side view thereof;
FIG. 5 is a front view thereof;
FIG. 6 is a top view thereof; and,
FIG. 7 is a bottom view thereof.

The portions of the drawings illustrated in broken lines are directed to the boundary of the design and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

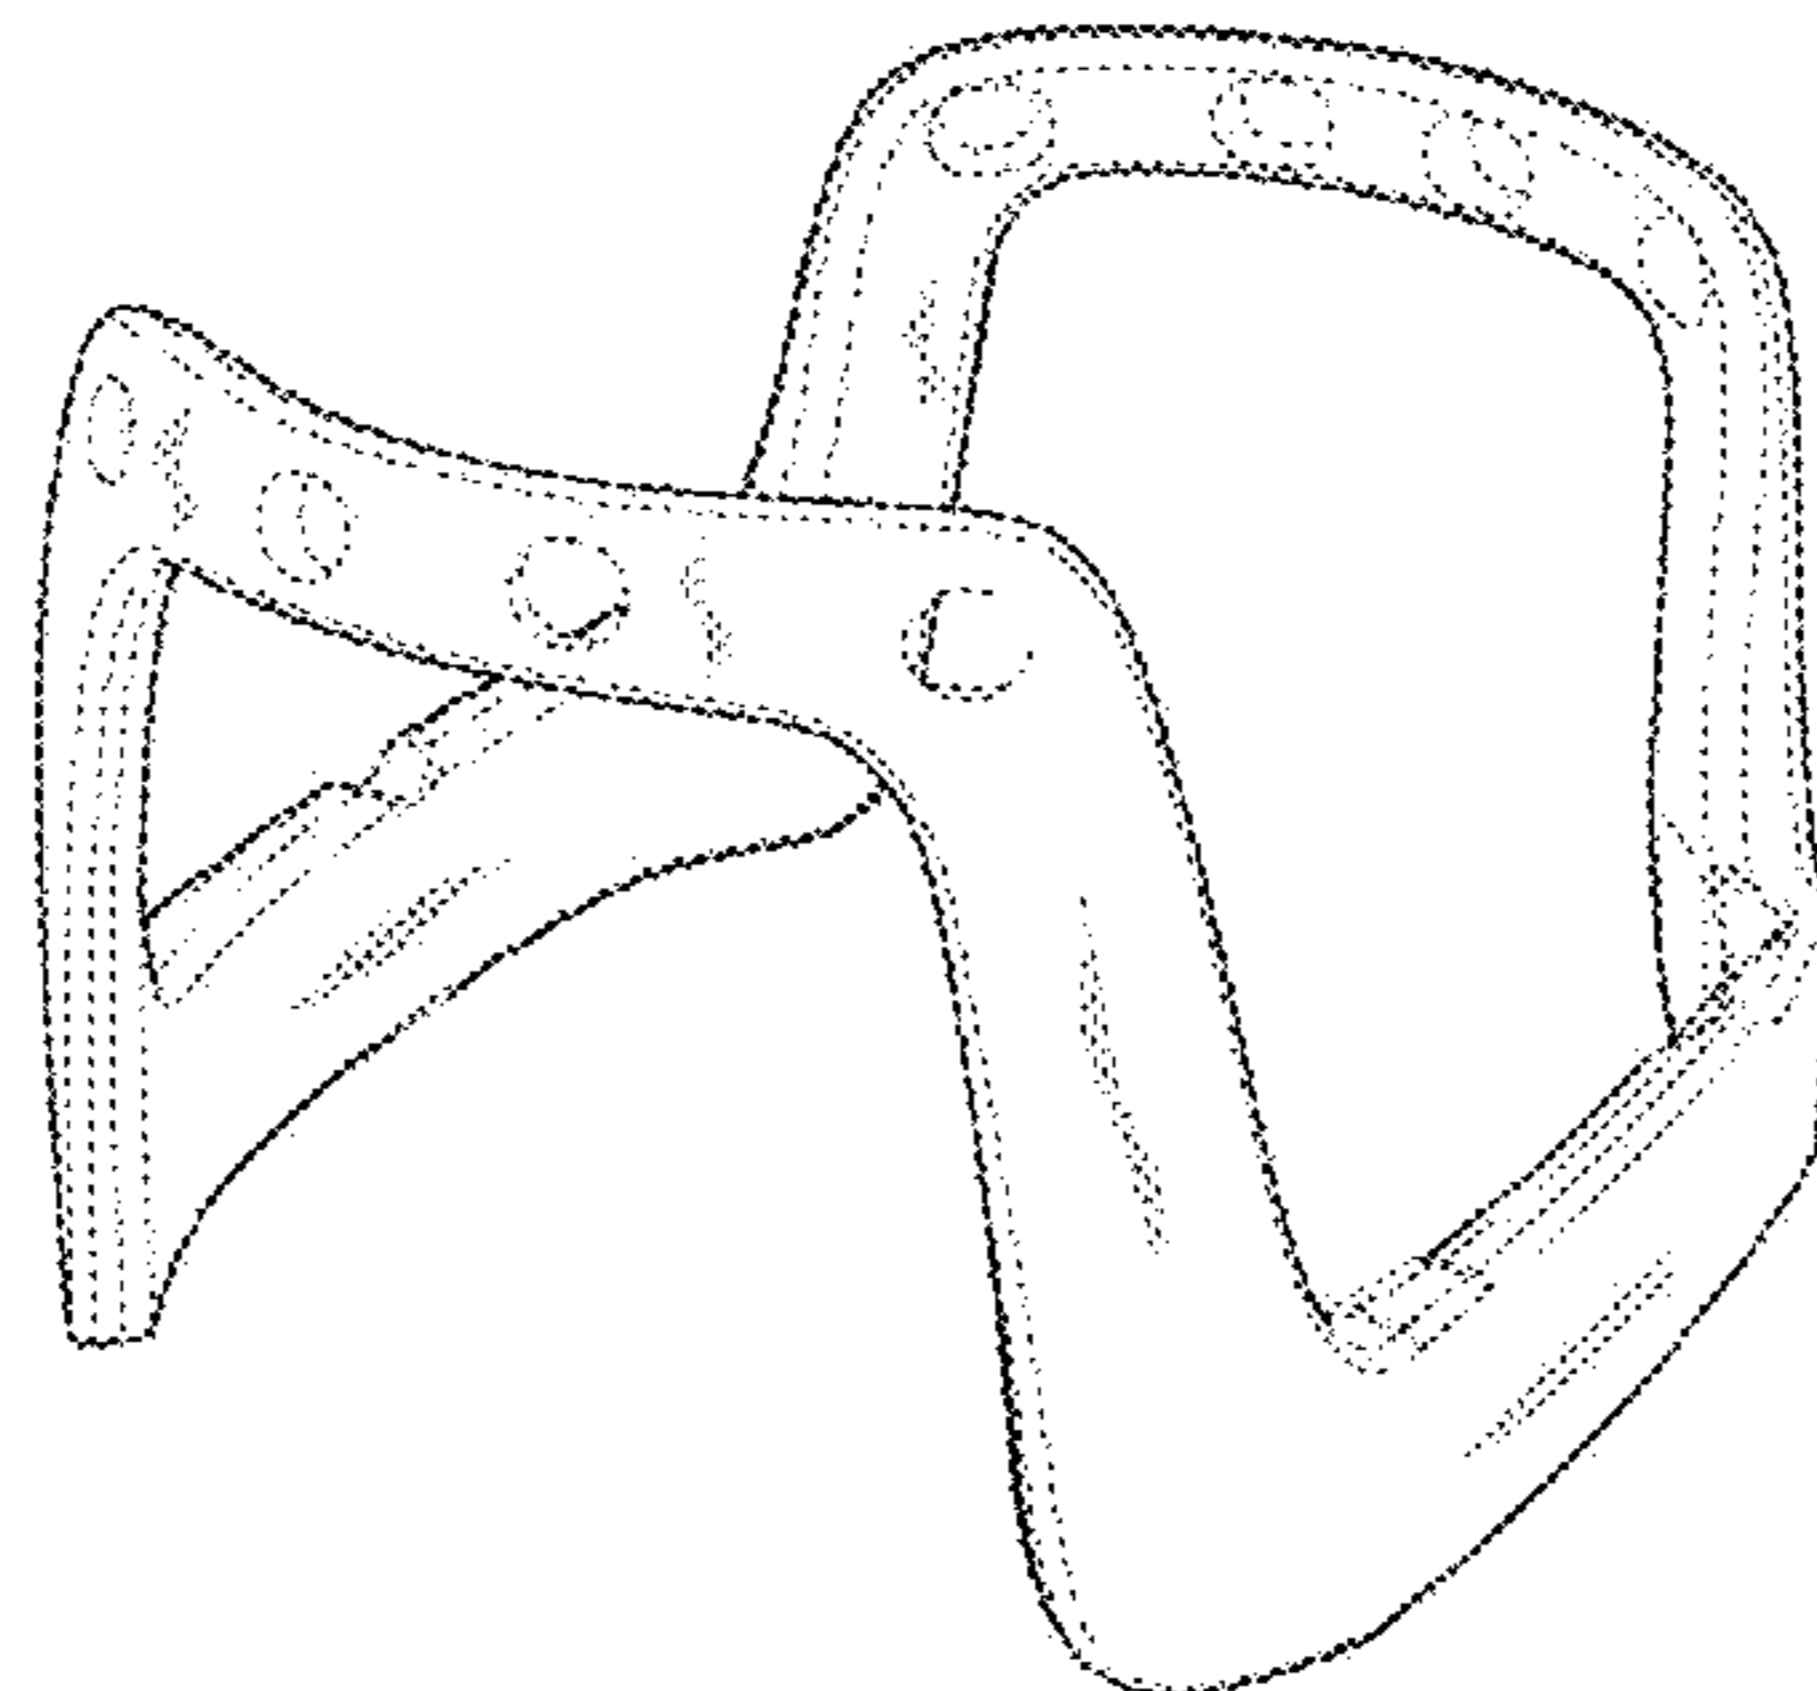

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0138066 A1* 6/2012 Akram A61B 19/203
128/845
2014/0135765 A1* 5/2014 Schuele A61B 90/14
606/57
2015/0119902 A1* 4/2015 Rurling A61B 90/14
606/130

* cited by examiner

FIG. 1

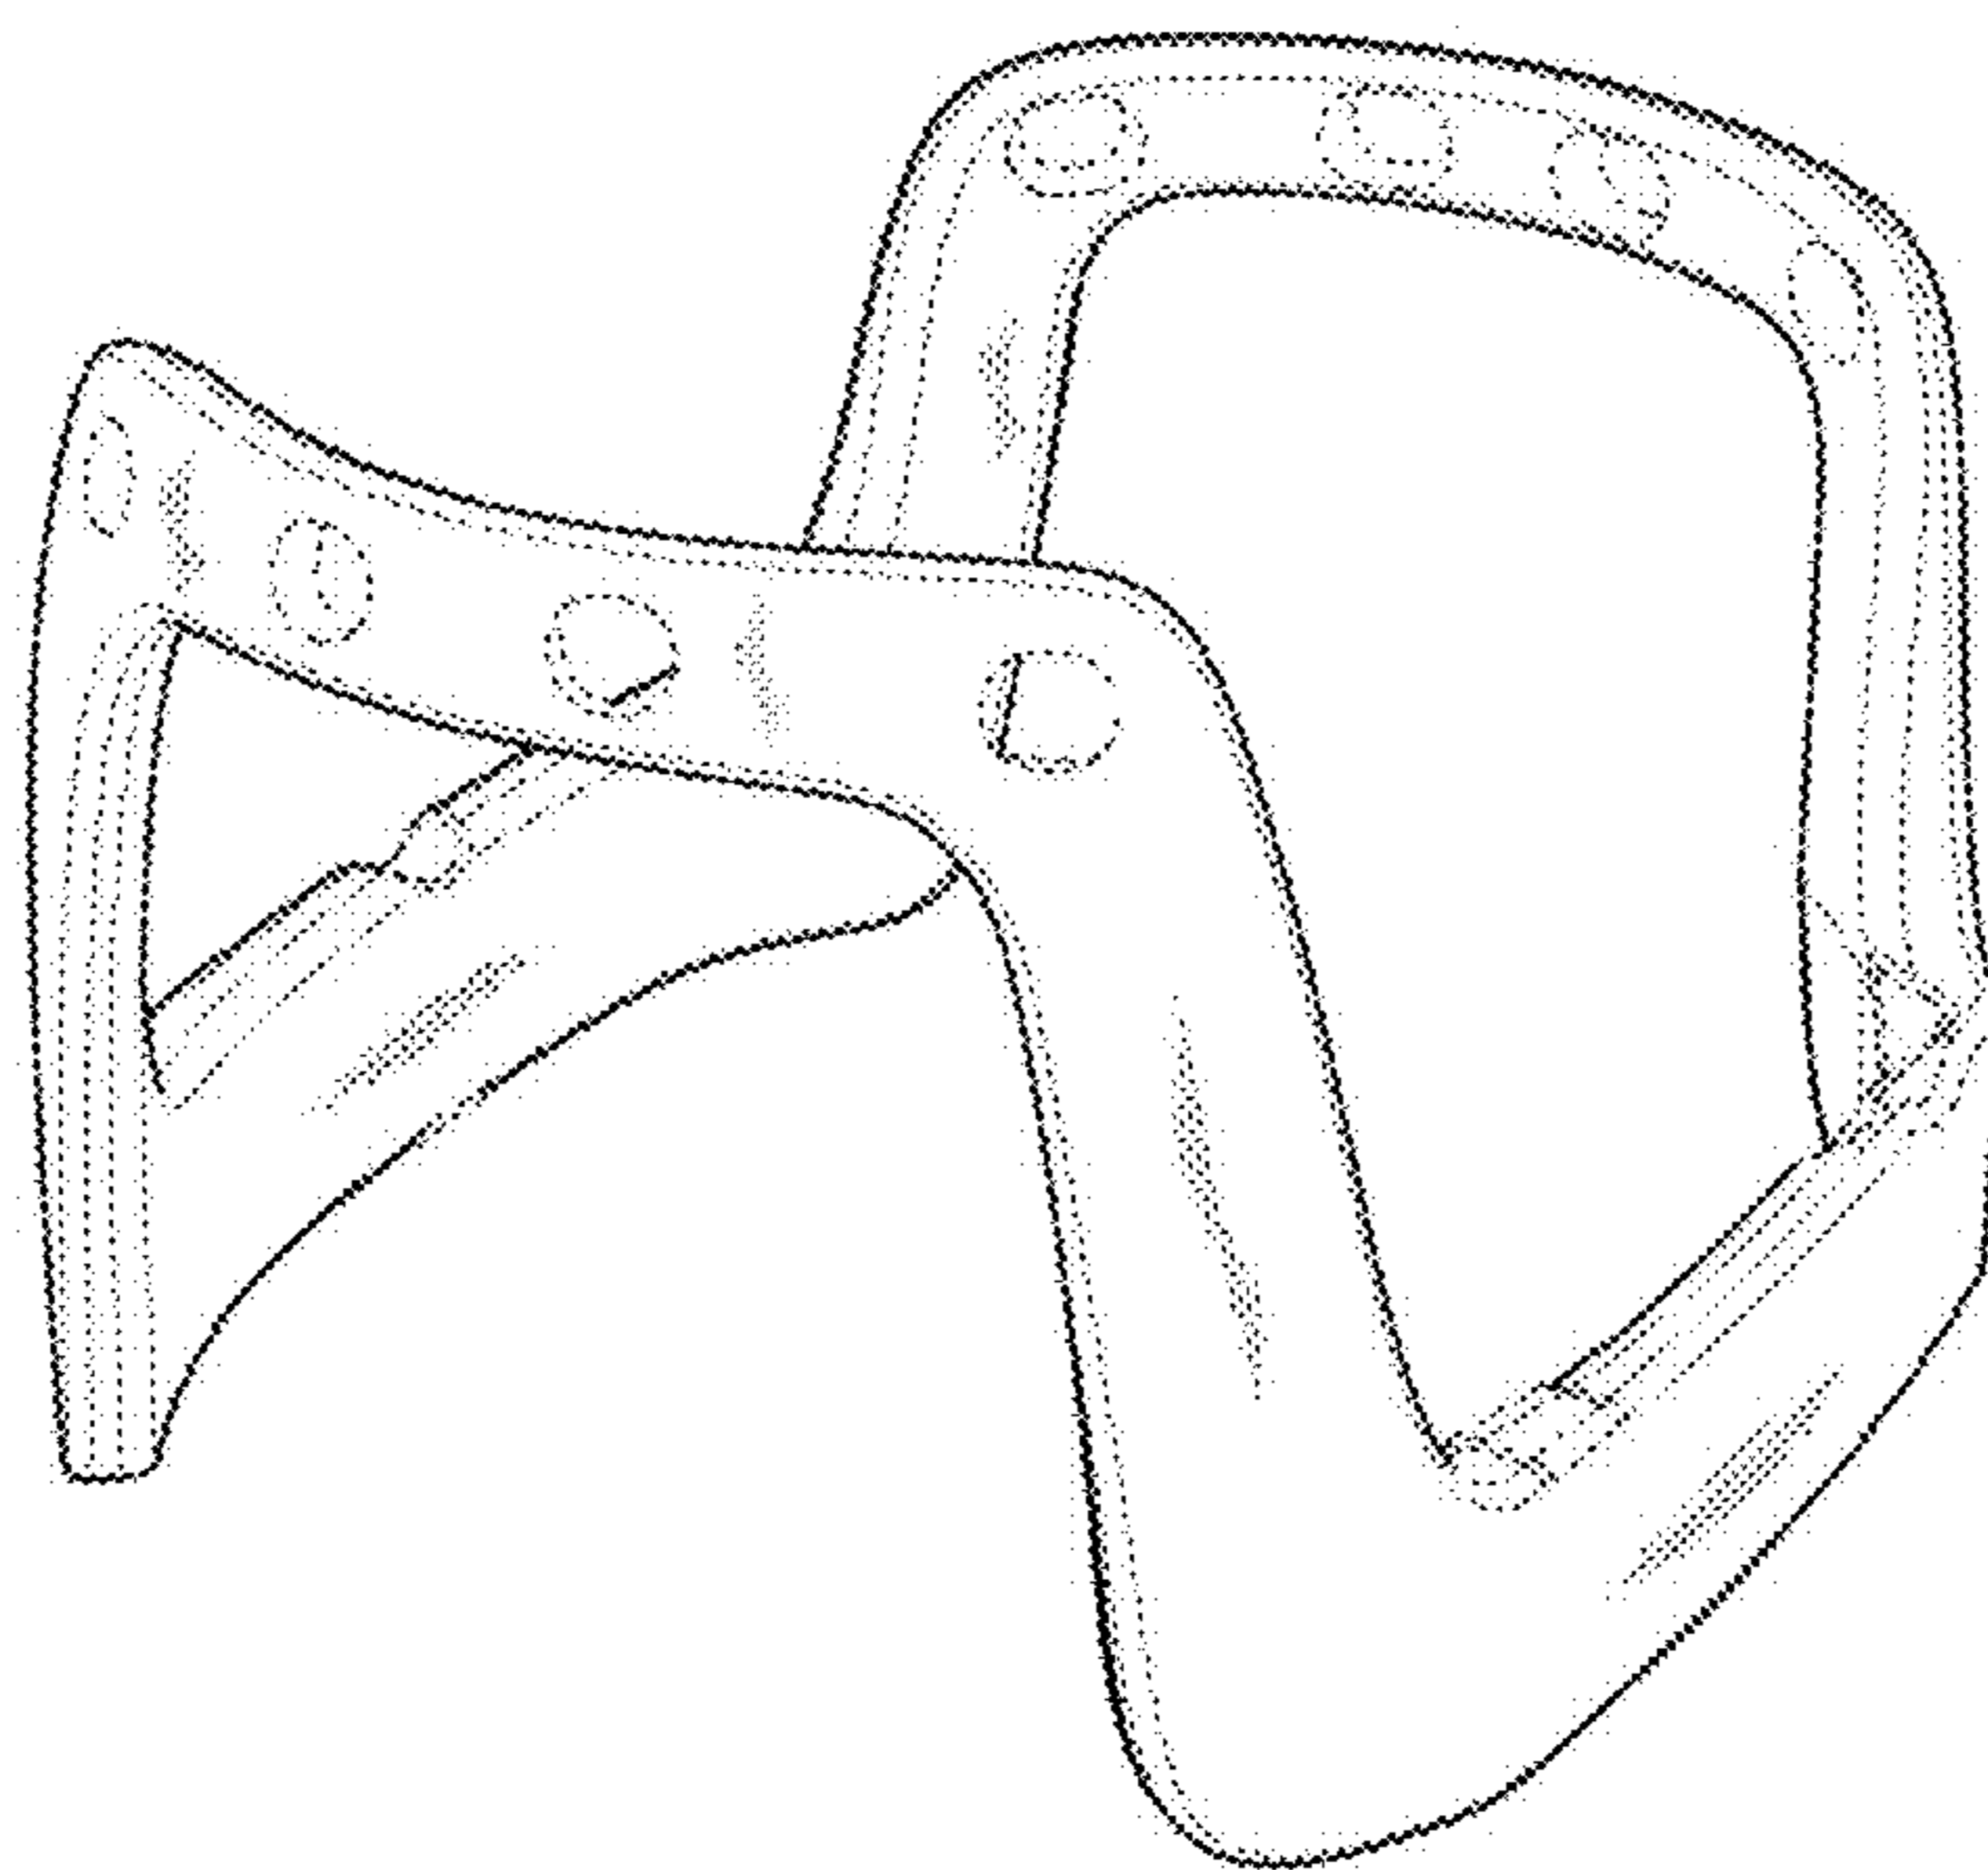


FIG. 2

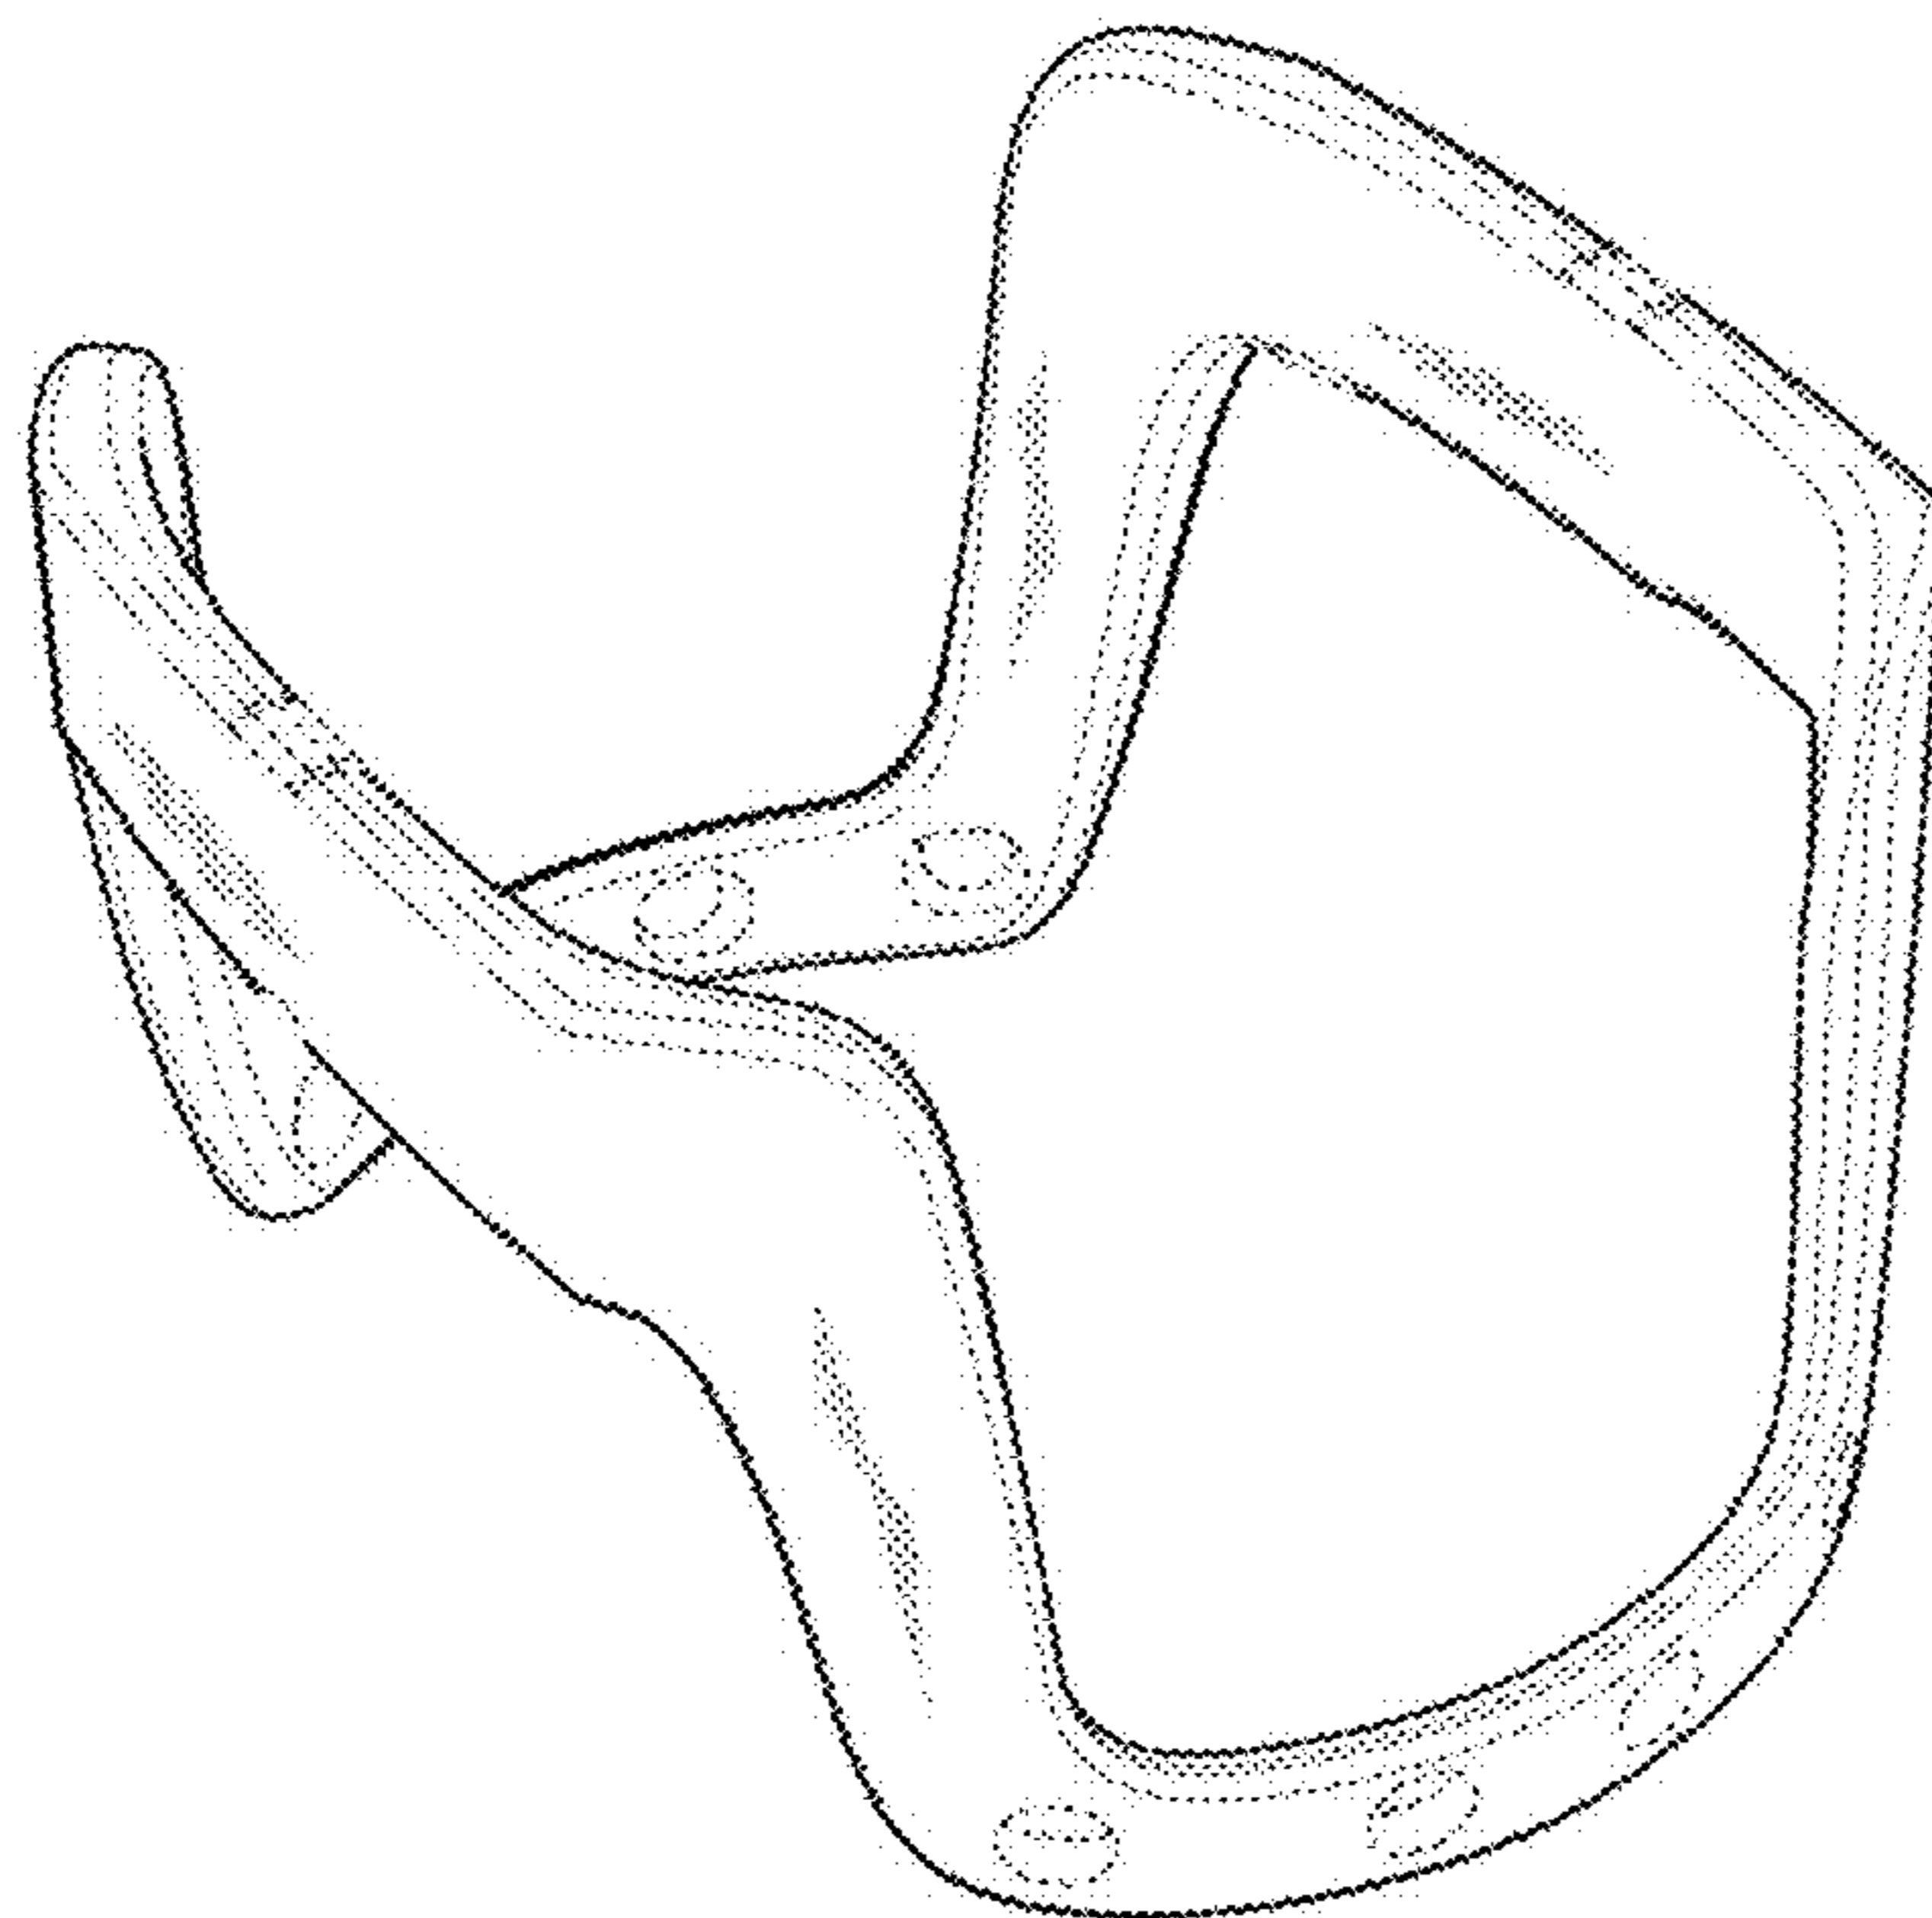


FIG. 3

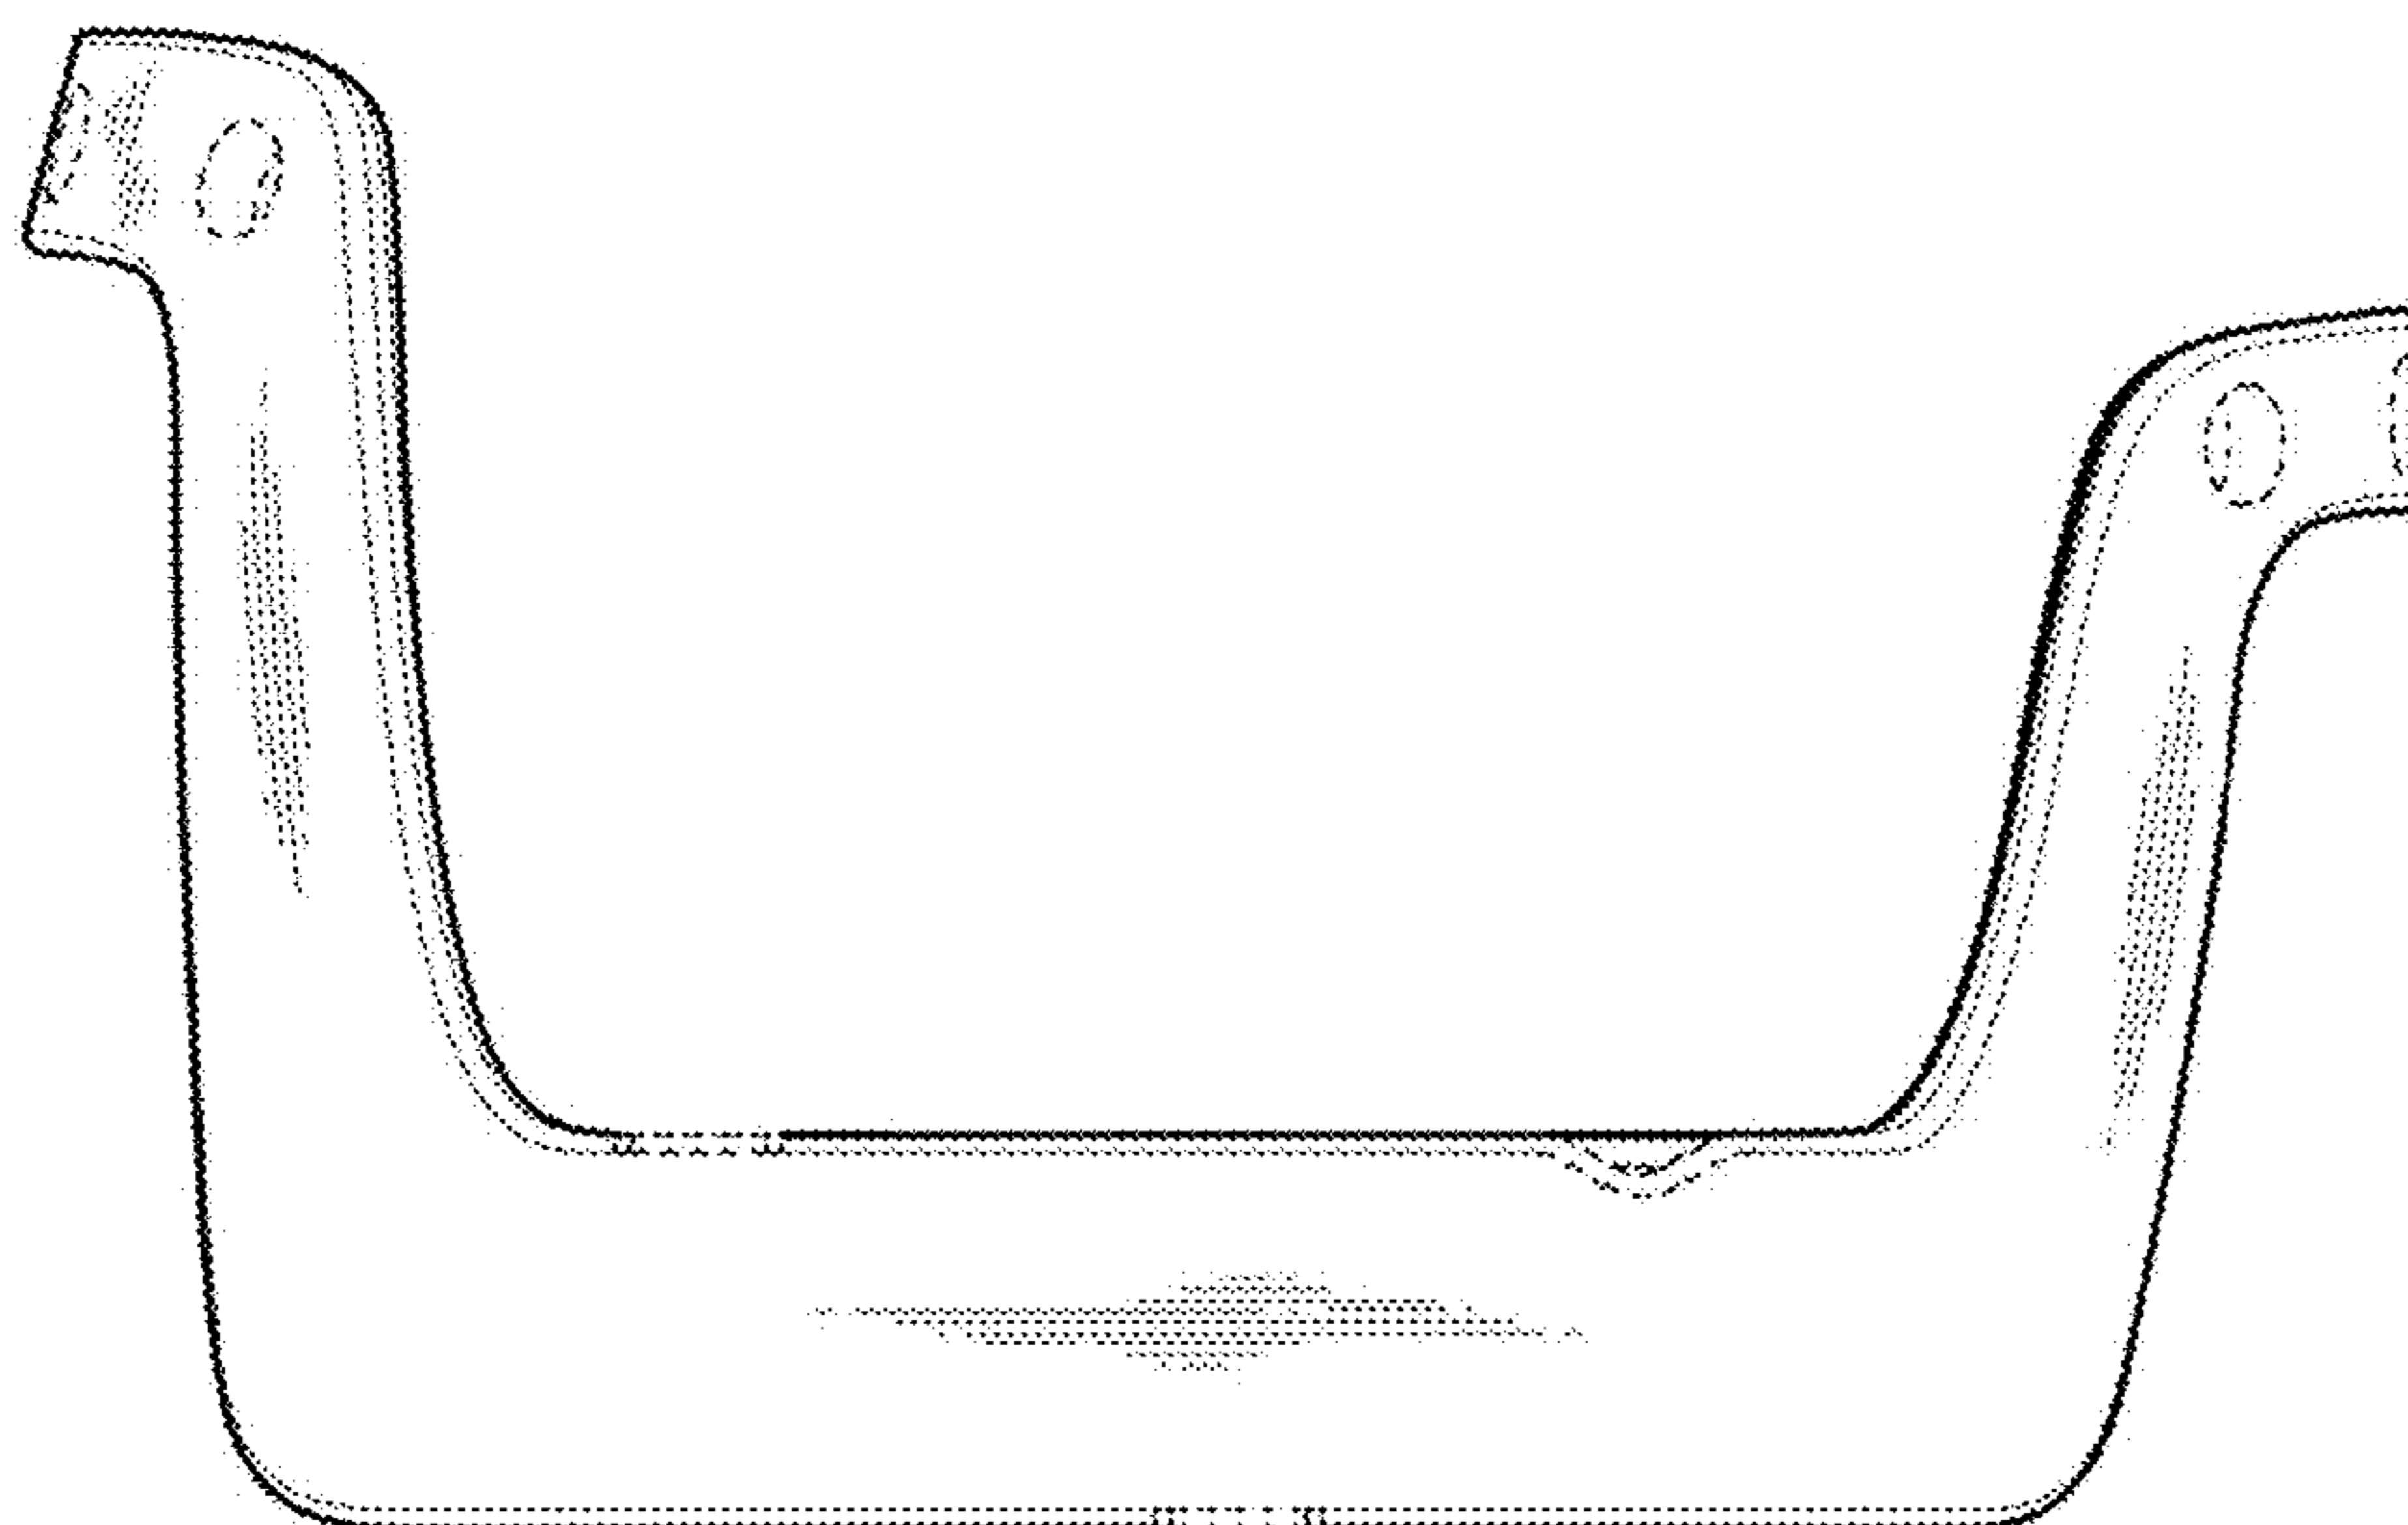


FIG. 4

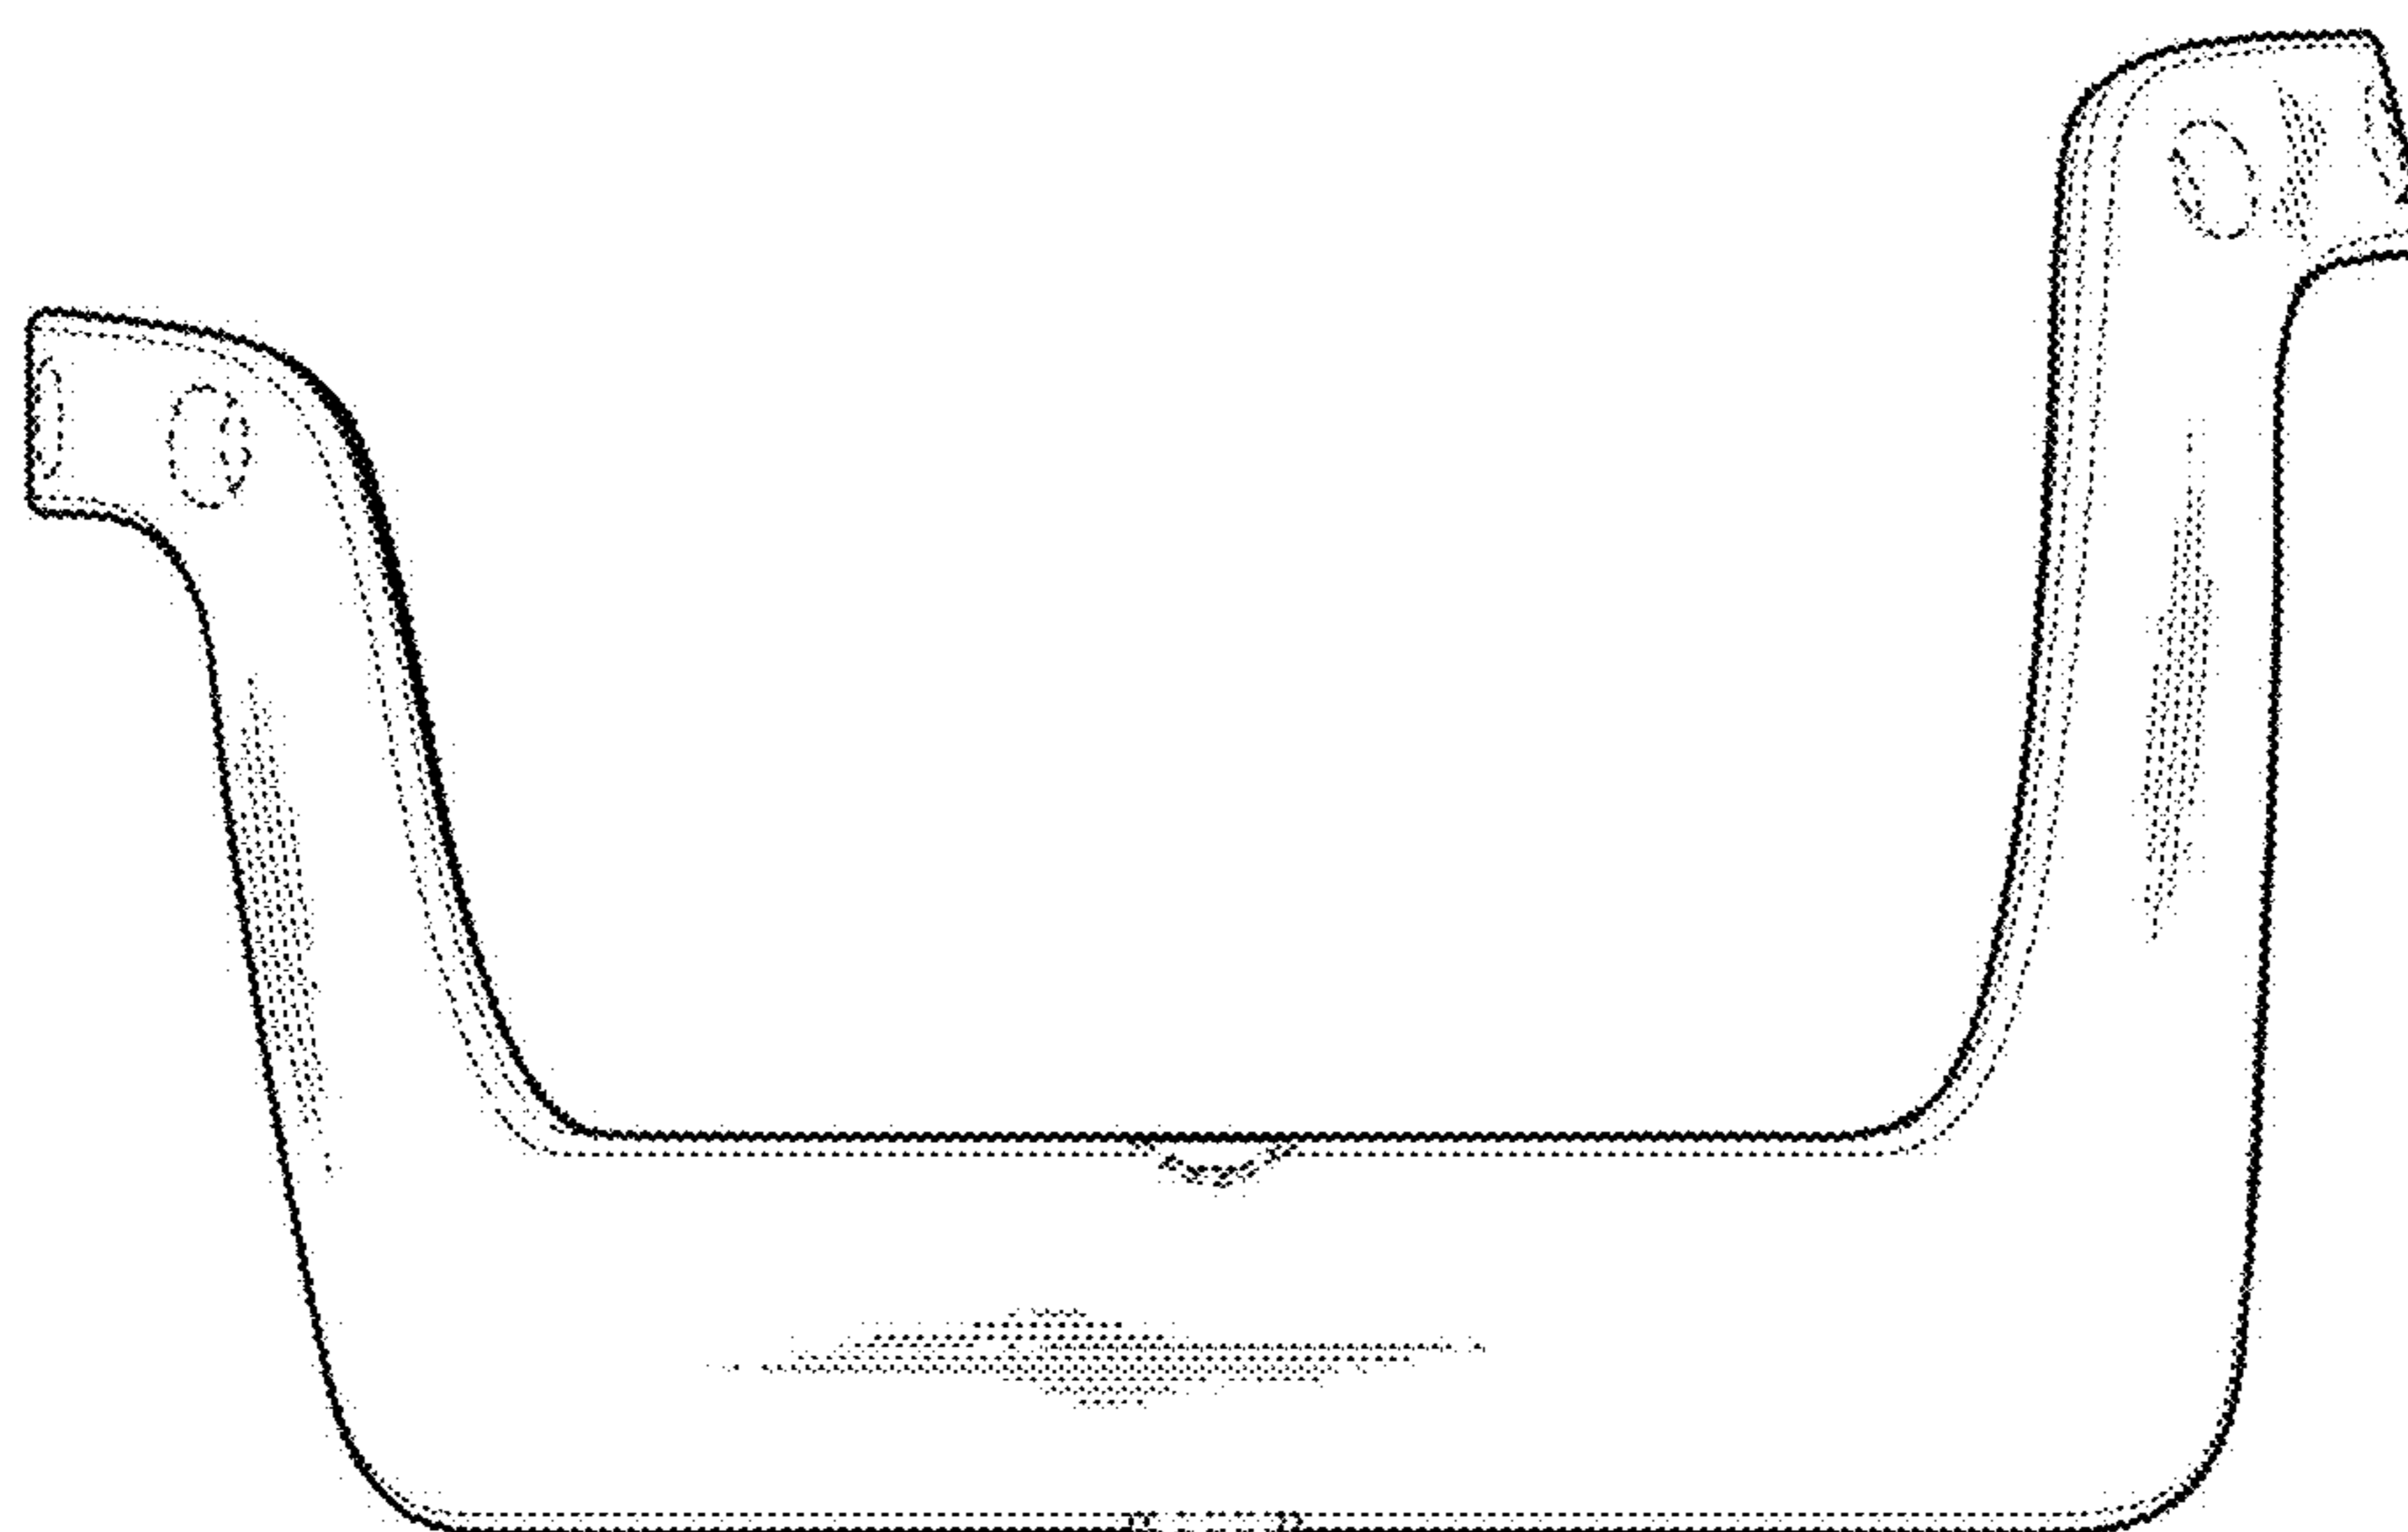


FIG. 5

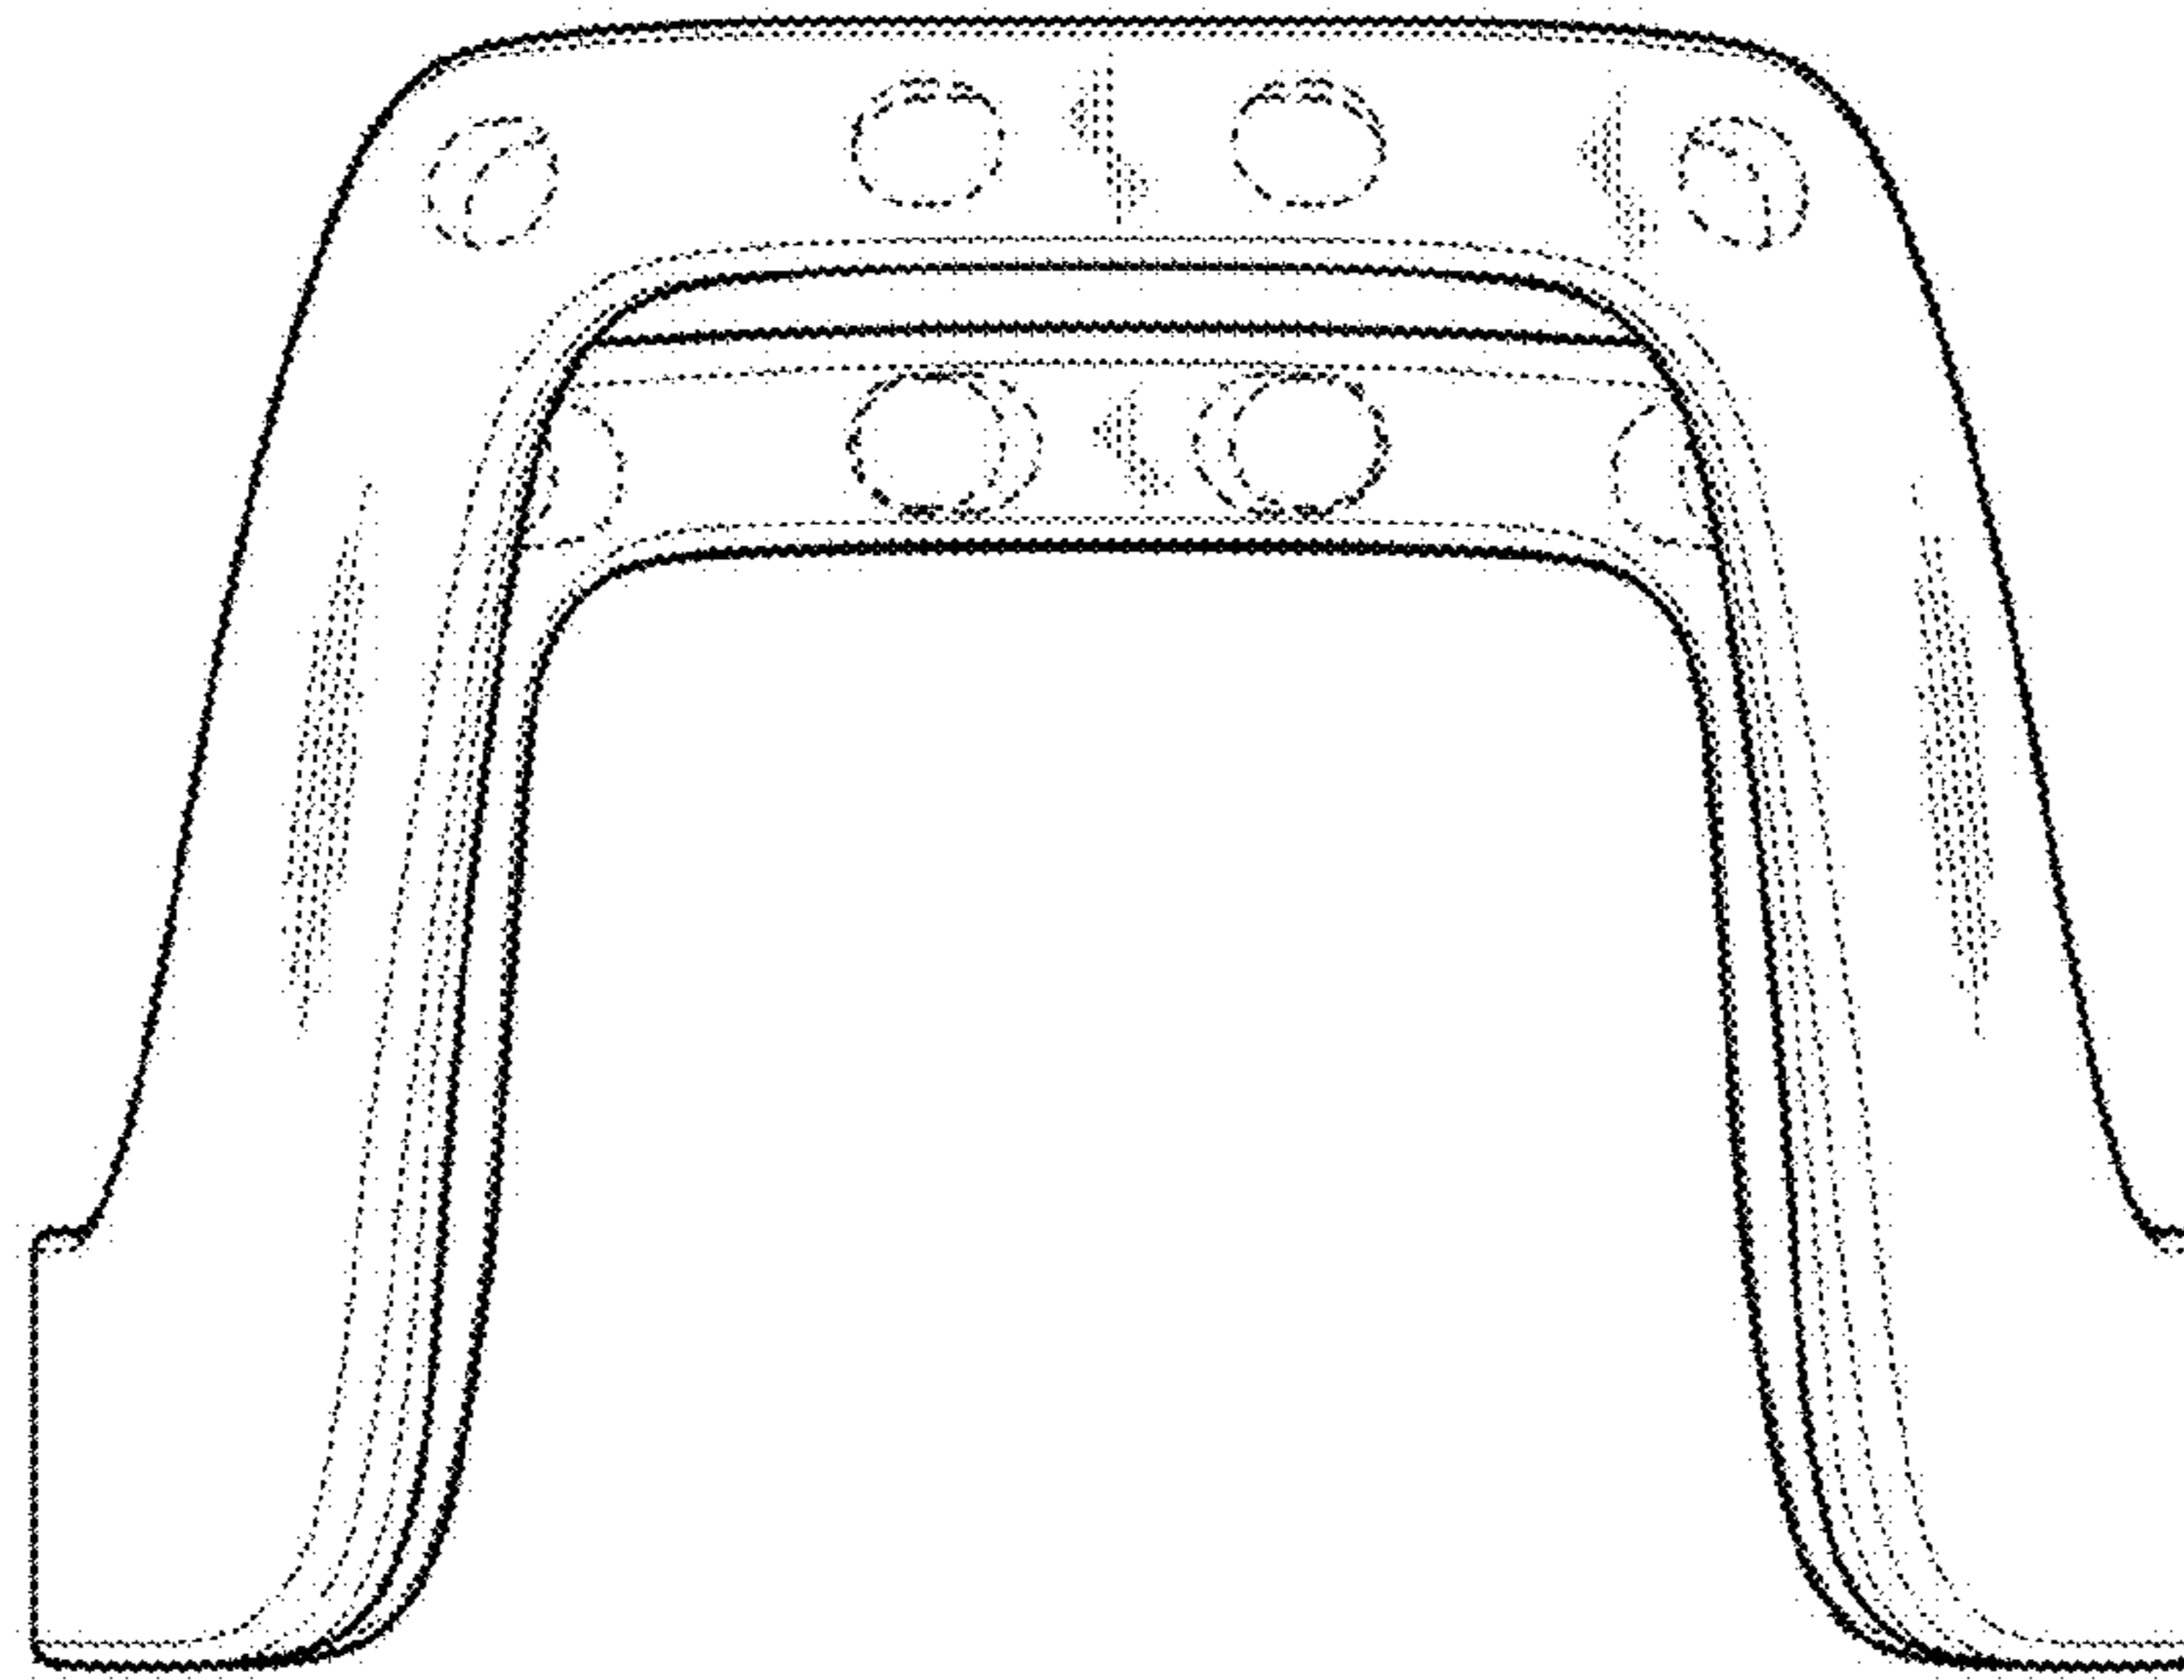


FIG. 6

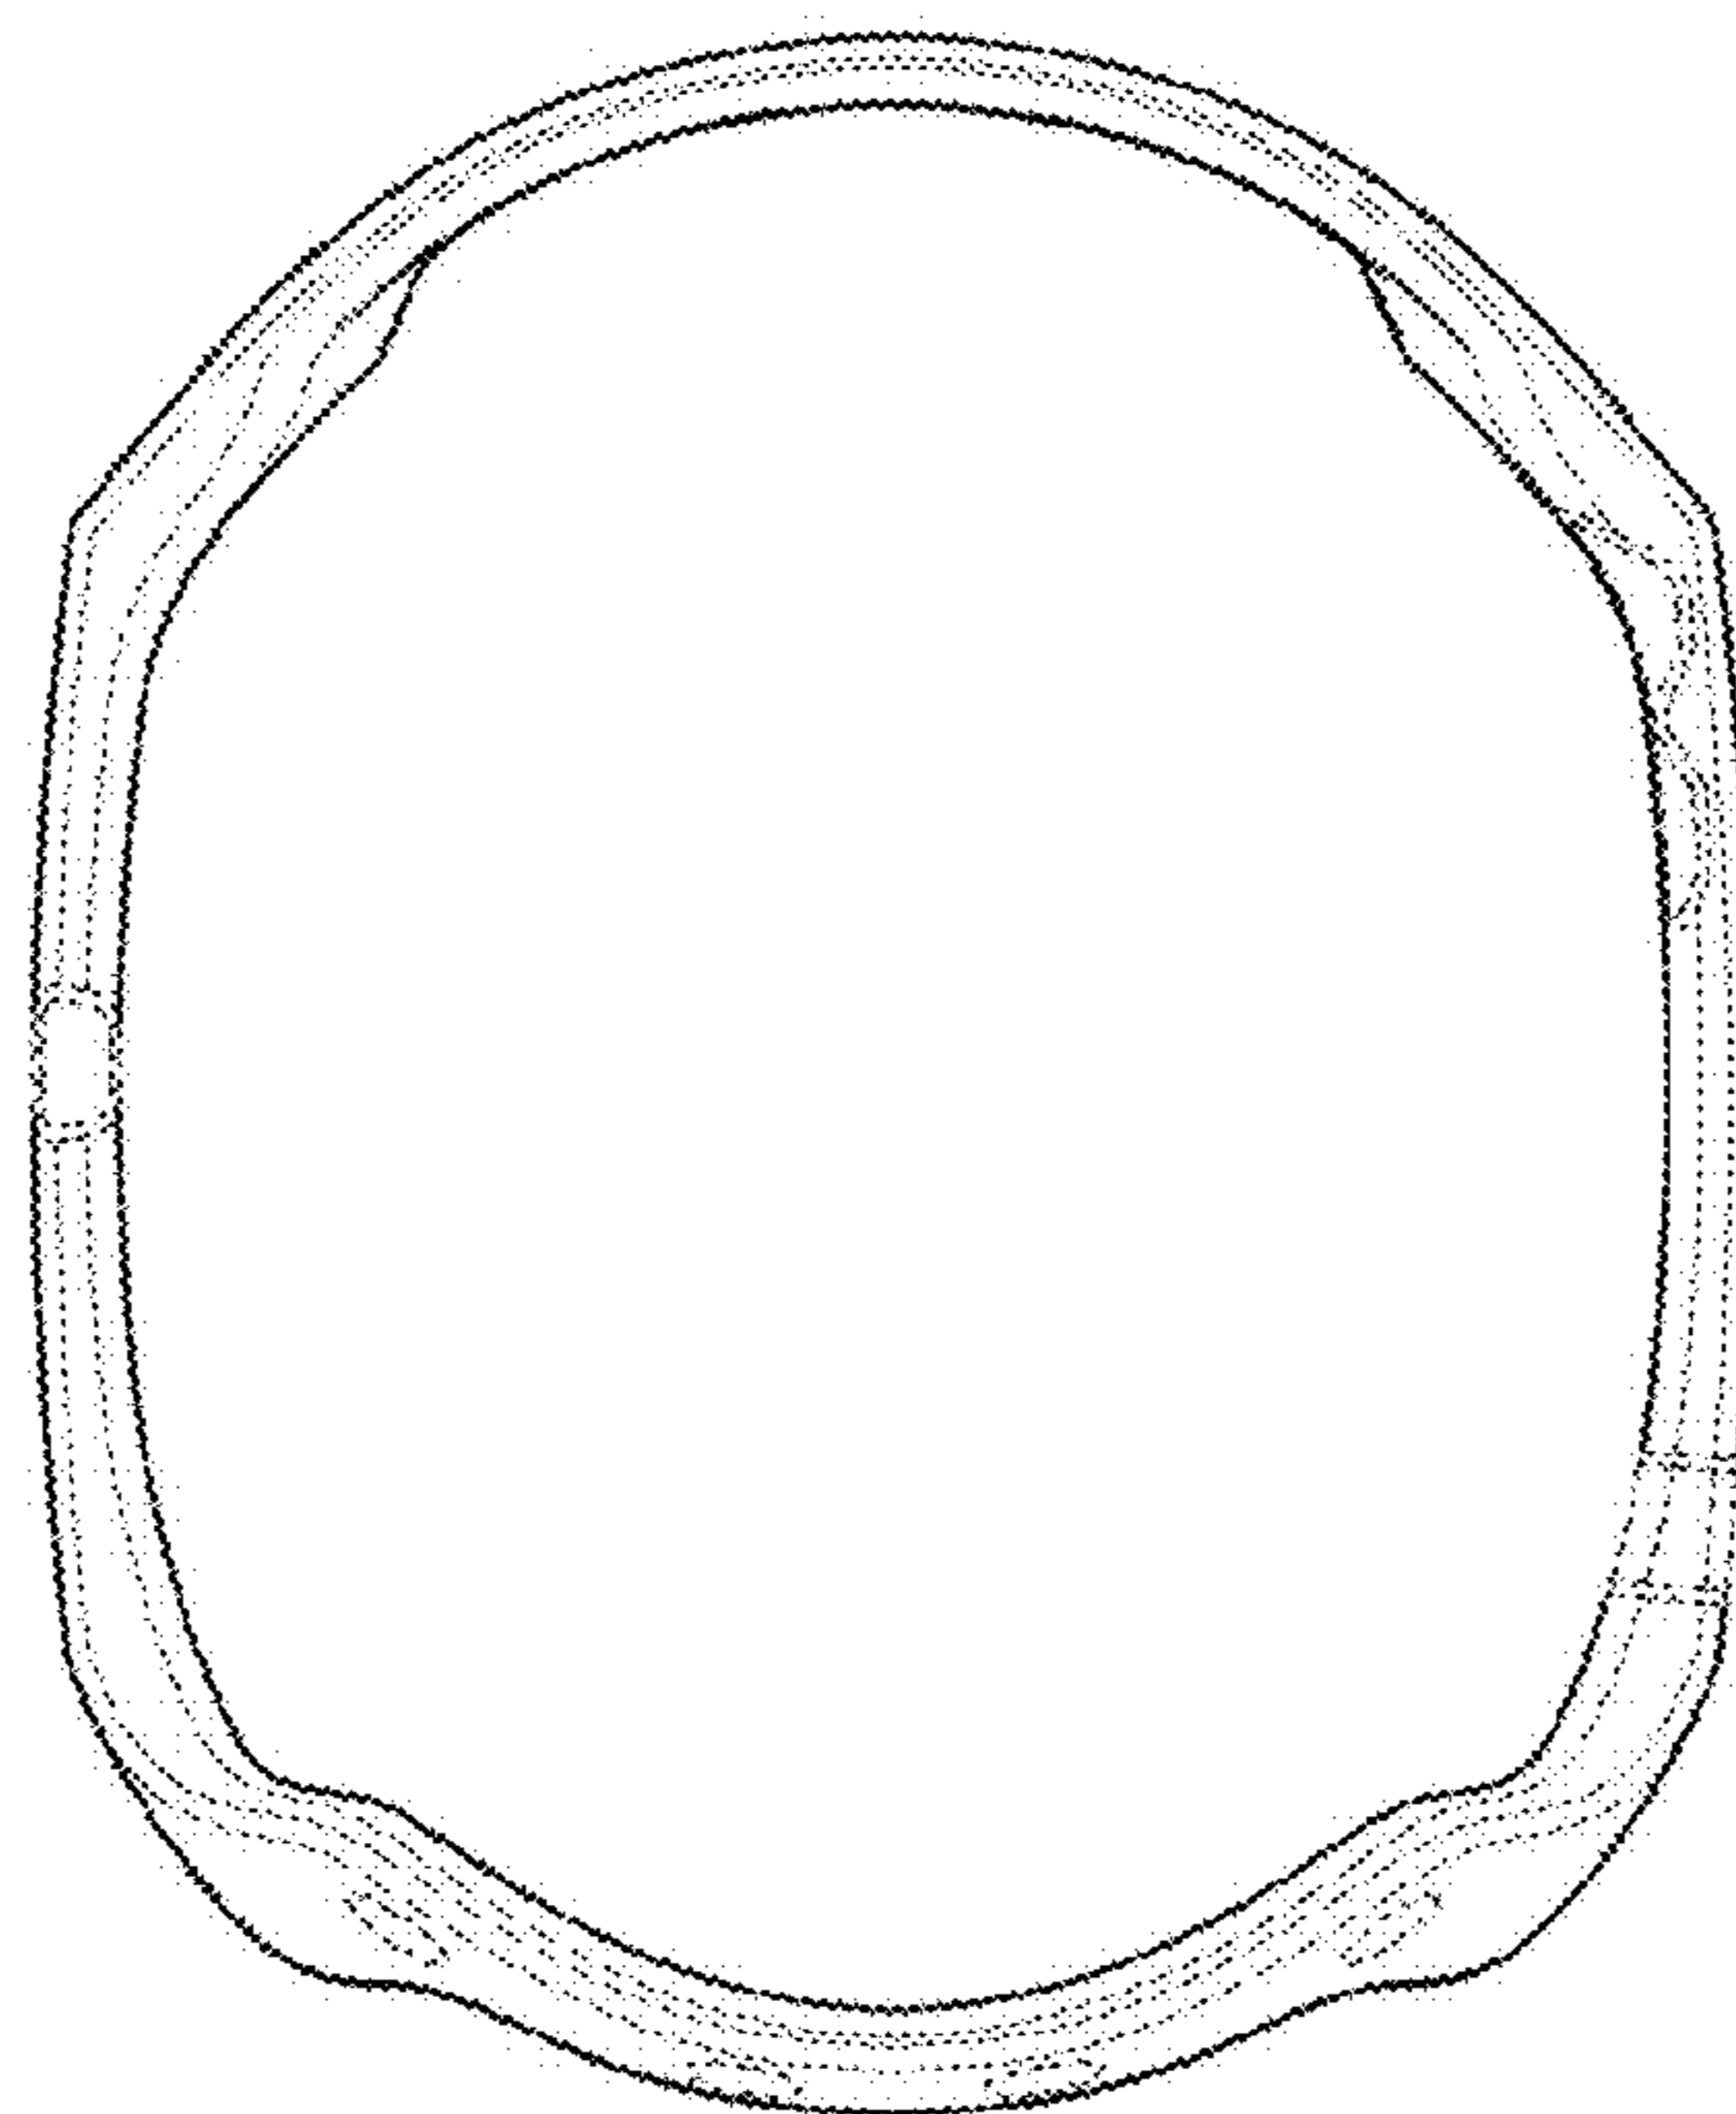


FIG. 7

