



US00D778451S

(12) **United States Design Patent**  
**Takizawa et al.**

(10) **Patent No.:** **US D778,451 S**  
(45) **Date of Patent:** **\*\* Feb. 7, 2017**

(54) **CONDUCTIVE SEAL OF A BIOMEDICAL SIGNAL RECORDER**

(71) Applicant: **TDK Corporation**, Tokyo (JP)

(72) Inventors: **Minoru Takizawa**, Sagamihara (JP);  
**Yasushi Sasaki**, Tokyo (JP); **Fongru Lin**, Yokohama (JP)

(73) Assignee: **TDK Corporation**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/508,781**

(22) Filed: **Nov. 11, 2014**

(30) **Foreign Application Priority Data**

May 13, 2014 (JP) ..... 2014-010185

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC . D24/186-187, 232, 168, 200, 189; D20/27  
CPC . A61B 5/0408; A61B 5/04085; A61B 5/0404;  
A61B 5/04087; A61B 5/04082; A61B  
5/05

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,606,881 A \* 9/1971 Woodson ..... A61B 5/0416  
600/392
- 4,852,571 A \* 8/1989 Gadsby ..... A61B 5/04087  
600/396
- 5,402,780 A \* 4/1995 Faasse, Jr. .... A61B 5/0408  
29/877
- 5,511,548 A \* 4/1996 Riazzi ..... A61B 5/0408  
600/391

- 5,921,925 A \* 7/1999 Cartmell ..... A61B 5/0408  
600/391
- 6,129,666 A \* 10/2000 DeLuca ..... A61B 5/04085  
600/372
- 9,162,045 B2 \* 10/2015 Jones ..... A61B 5/0408
- D749,748 S \* 2/2016 Suzuki ..... D24/232

FOREIGN PATENT DOCUMENTS

- IN 256193-0001 \* 9/2013
- JP S1485504 12/2013
- JP S1485505 12/2013
- JP S1485726 12/2013

\* cited by examiner

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.


(57) **CLAIM**


The ornamental design for a conductive seal of a biomedical signal recorder, as shown and described.

**DESCRIPTION**


FIG. 1 is a front view of a conductive seal of a biomedical signal recorder, showing our new design;  
 FIG. 2 is a rear view thereof;  
 FIG. 3 is a top view thereof;  
 FIG. 4 is a bottom view thereof;  
 FIG. 5 is a right side view thereof, the left side being symmetrical;  
 FIG. 6 is a cross-sectional view thereof, taken along the line 6-6 of FIG. 1; and,  
 FIG. 7 is an exploded perspective view thereof, showing a state of separate components of the conductive seal of a biomedical signal recorder.

**1 Claim, 3 Drawing Sheets**

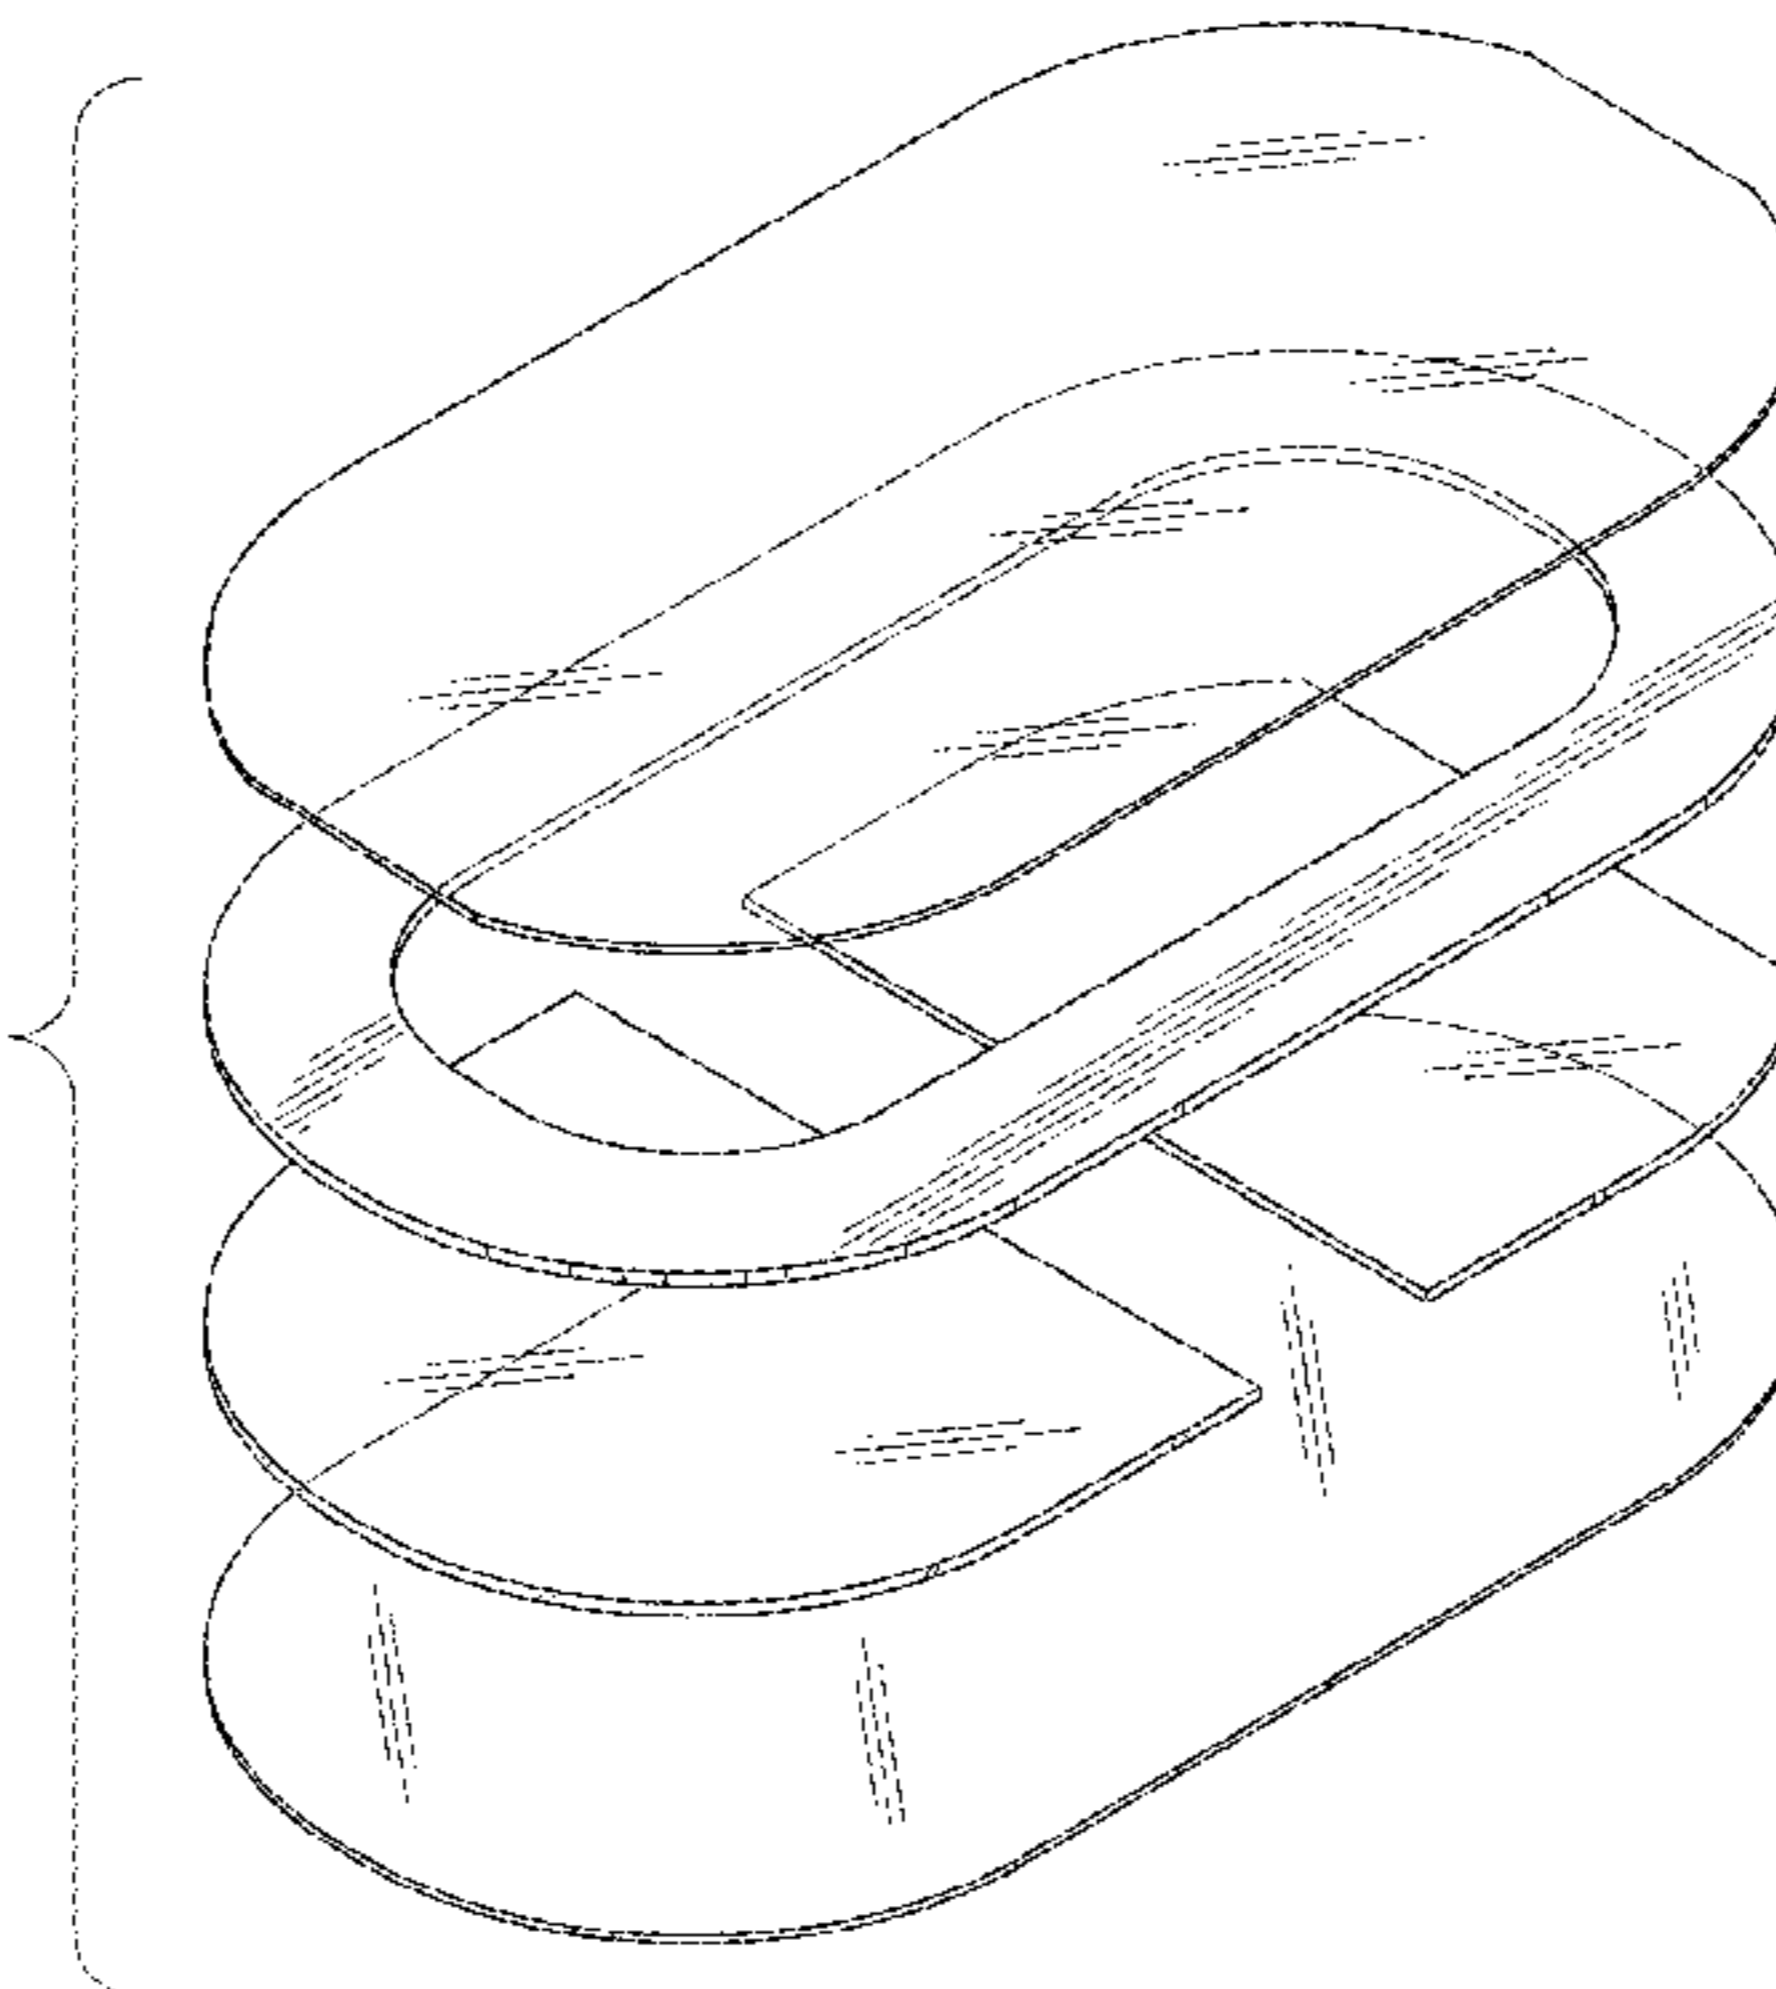

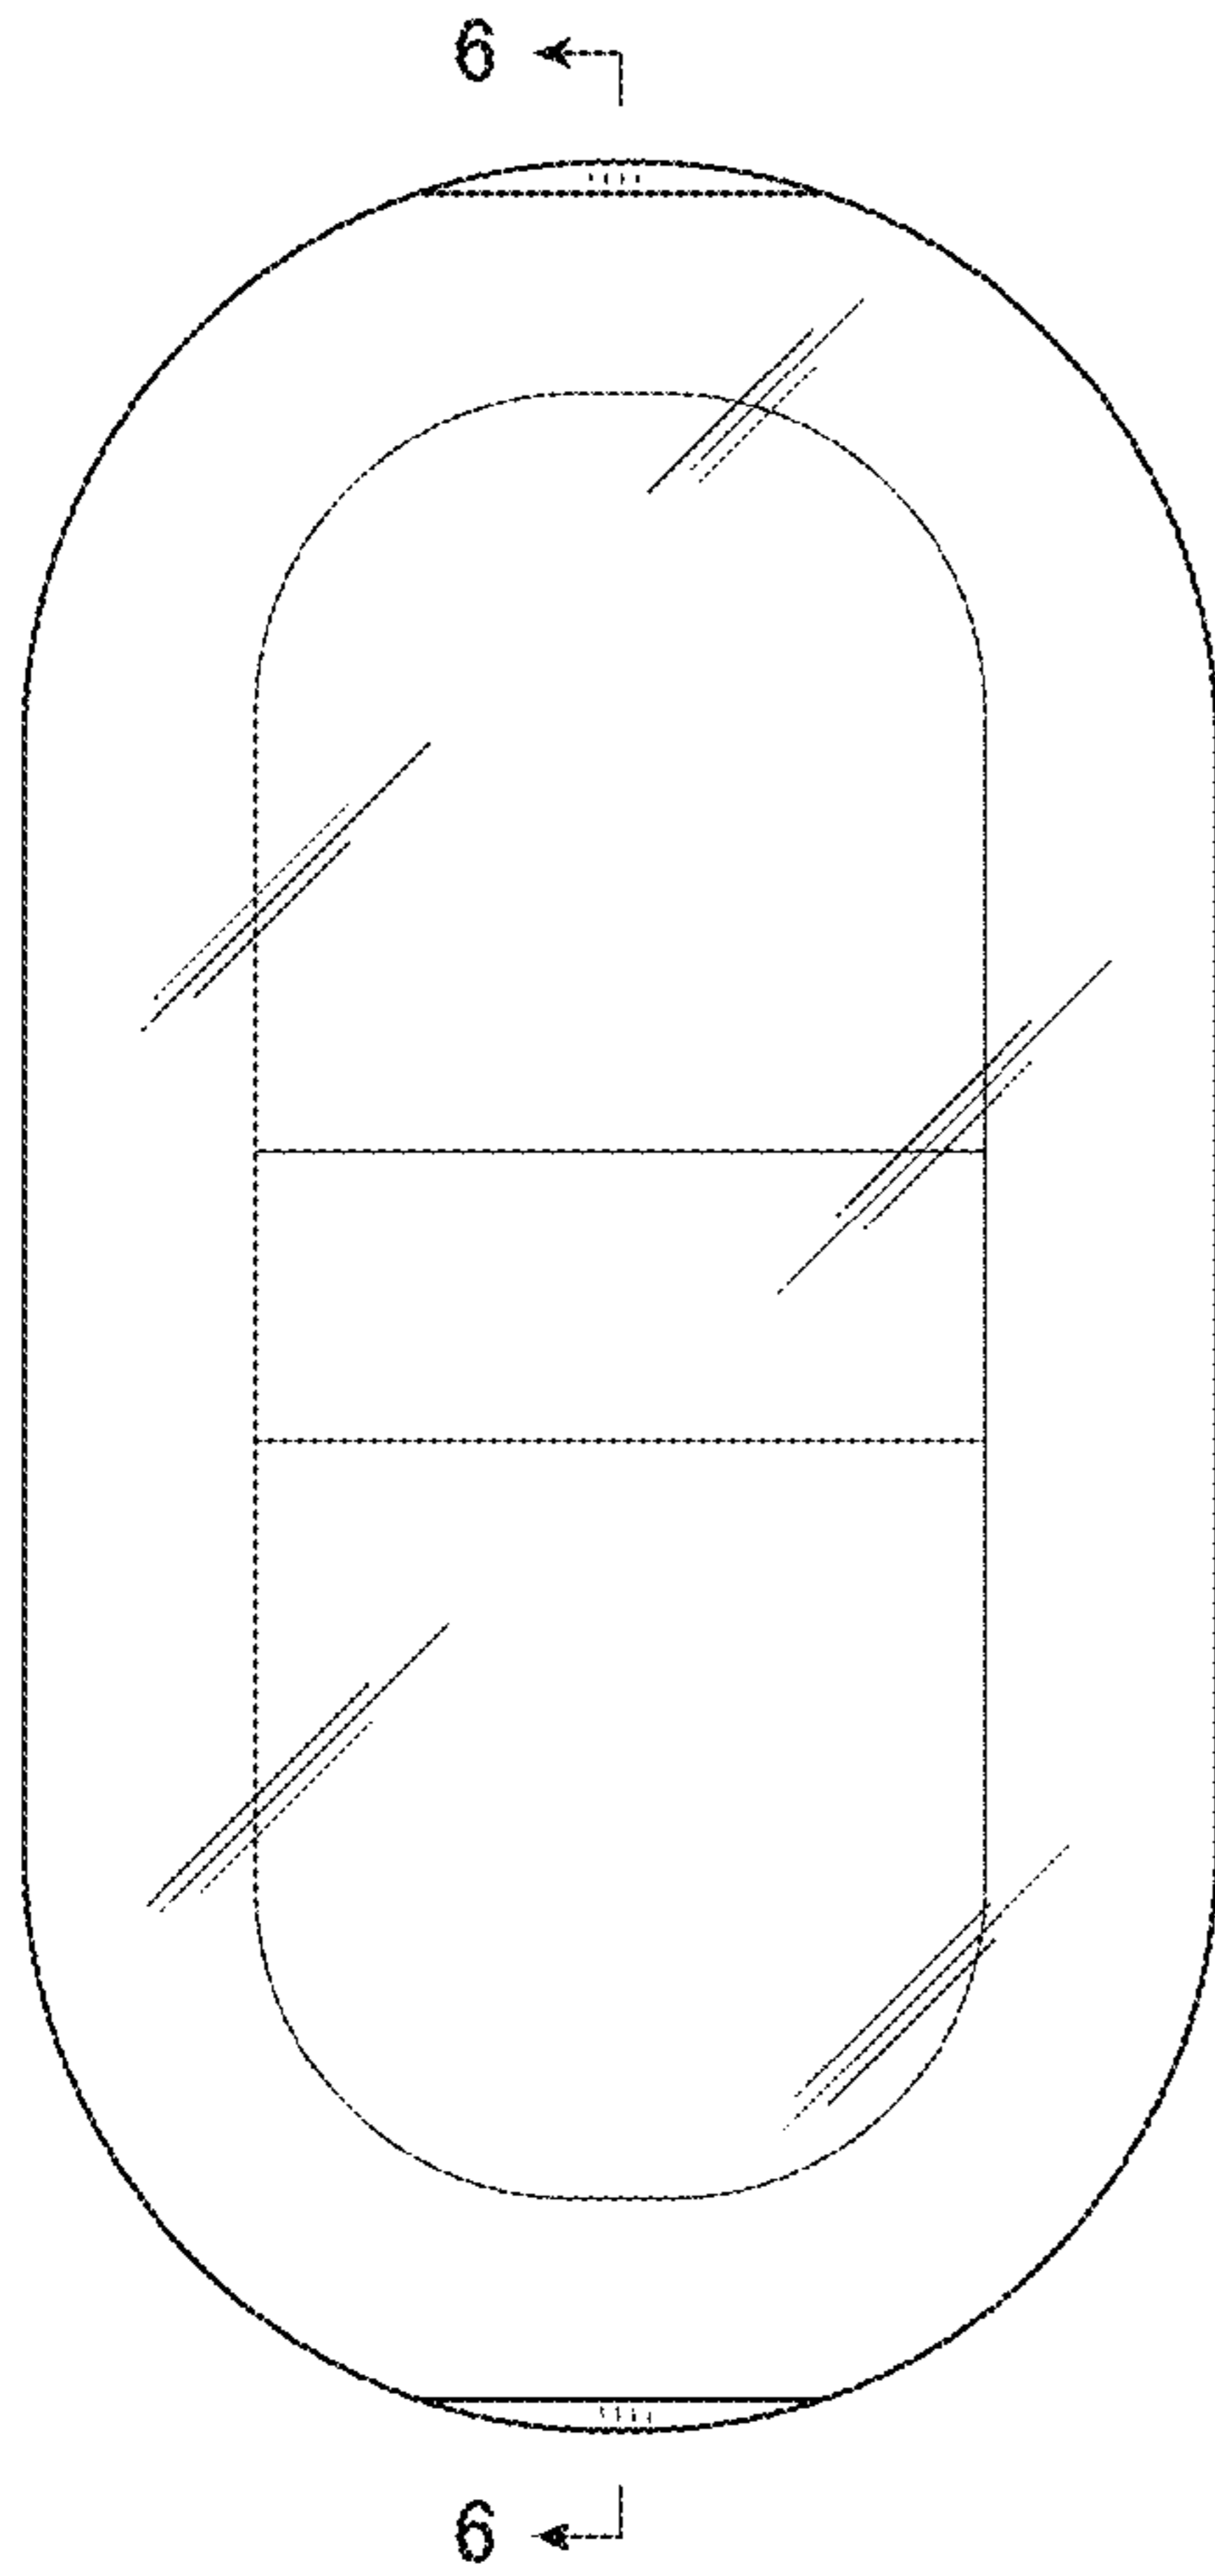


*Fig. 1*

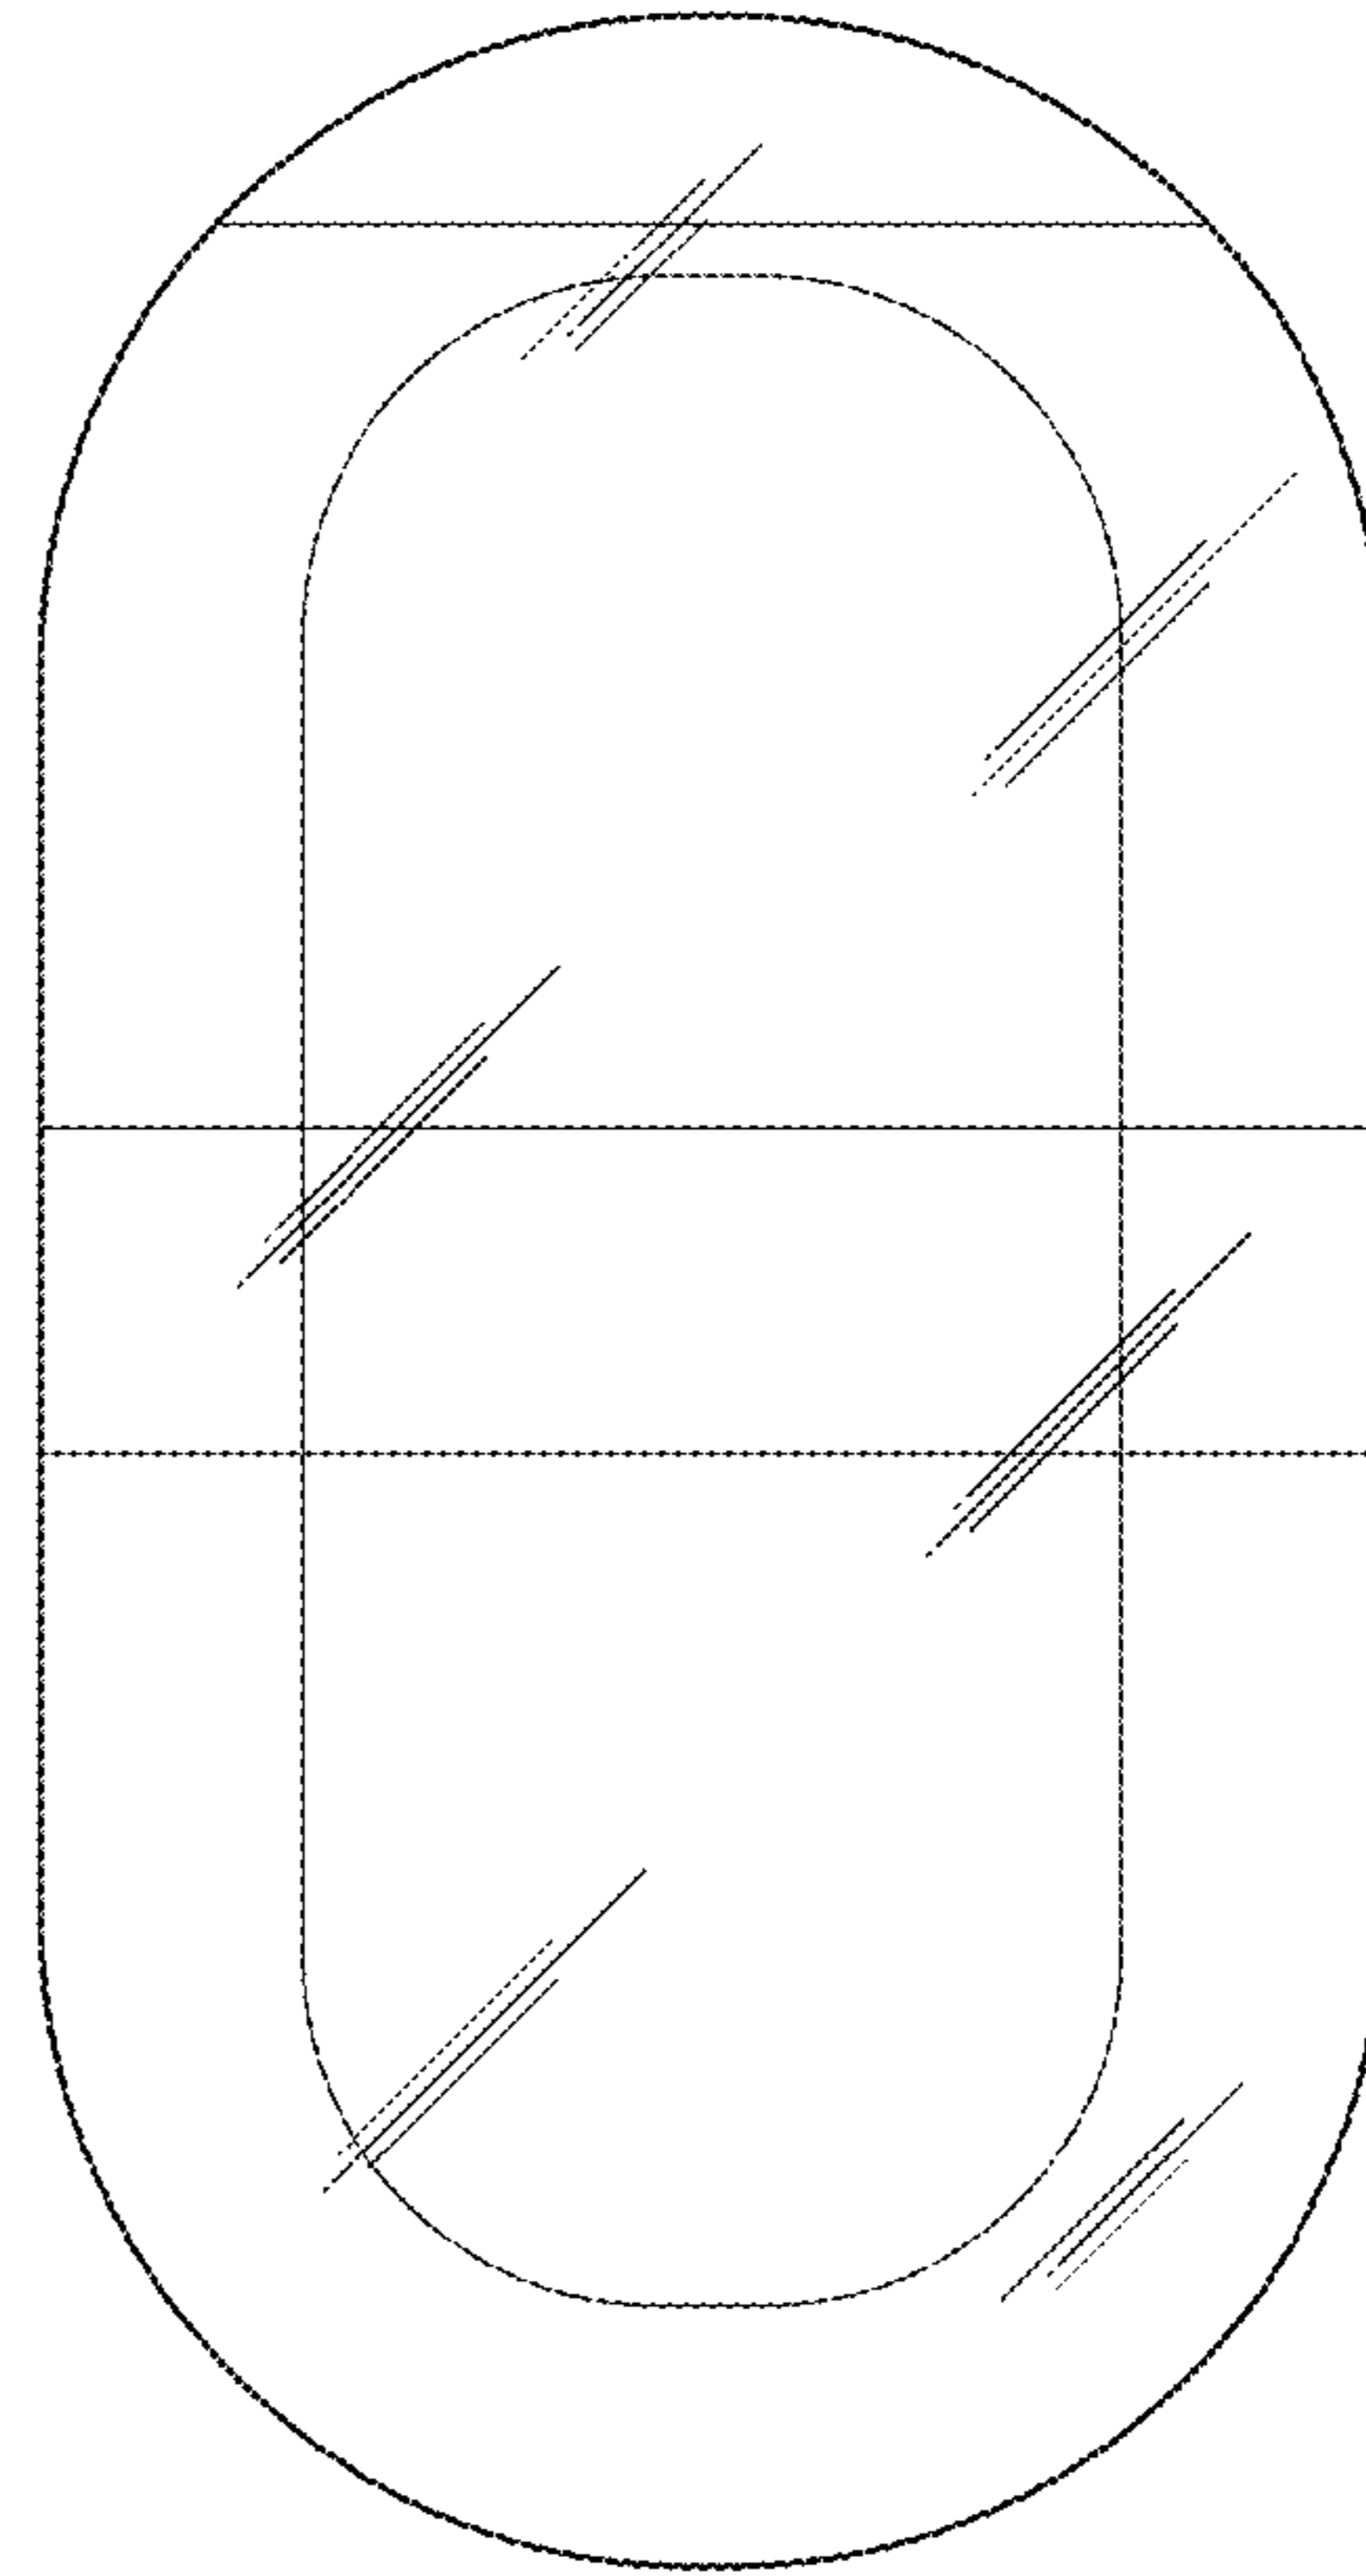


*Fig. 2*




*Fig. 3*

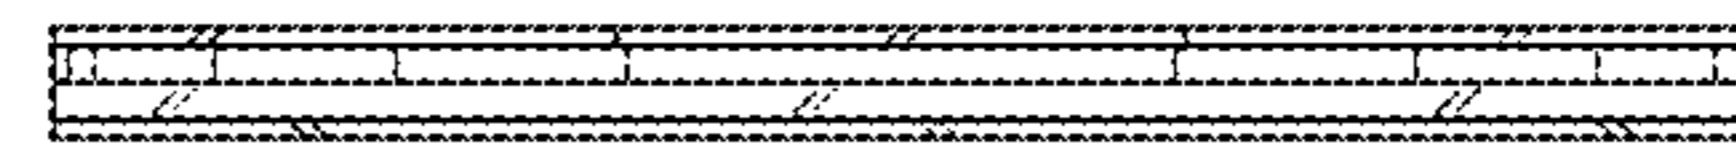


*Fig. 4*

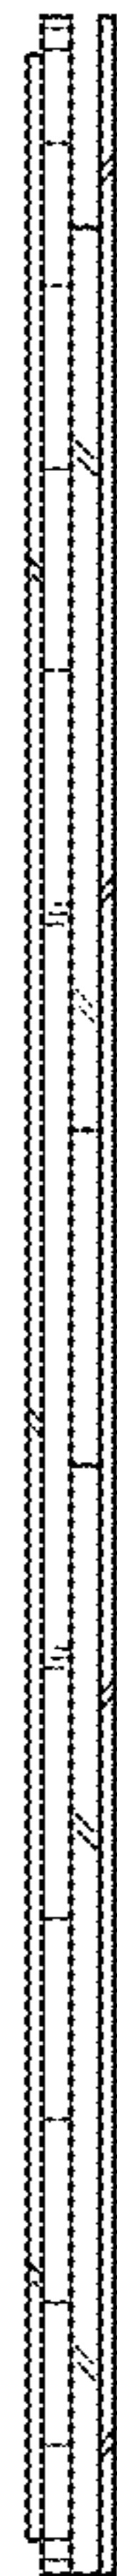

*Fig. 5*

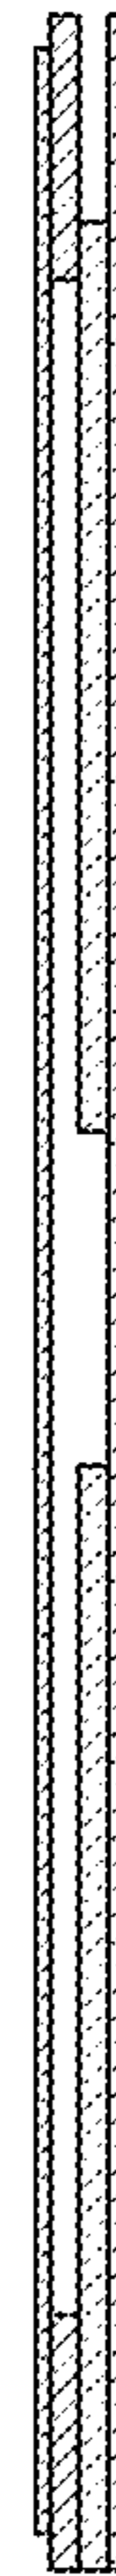

*Fig. 6*

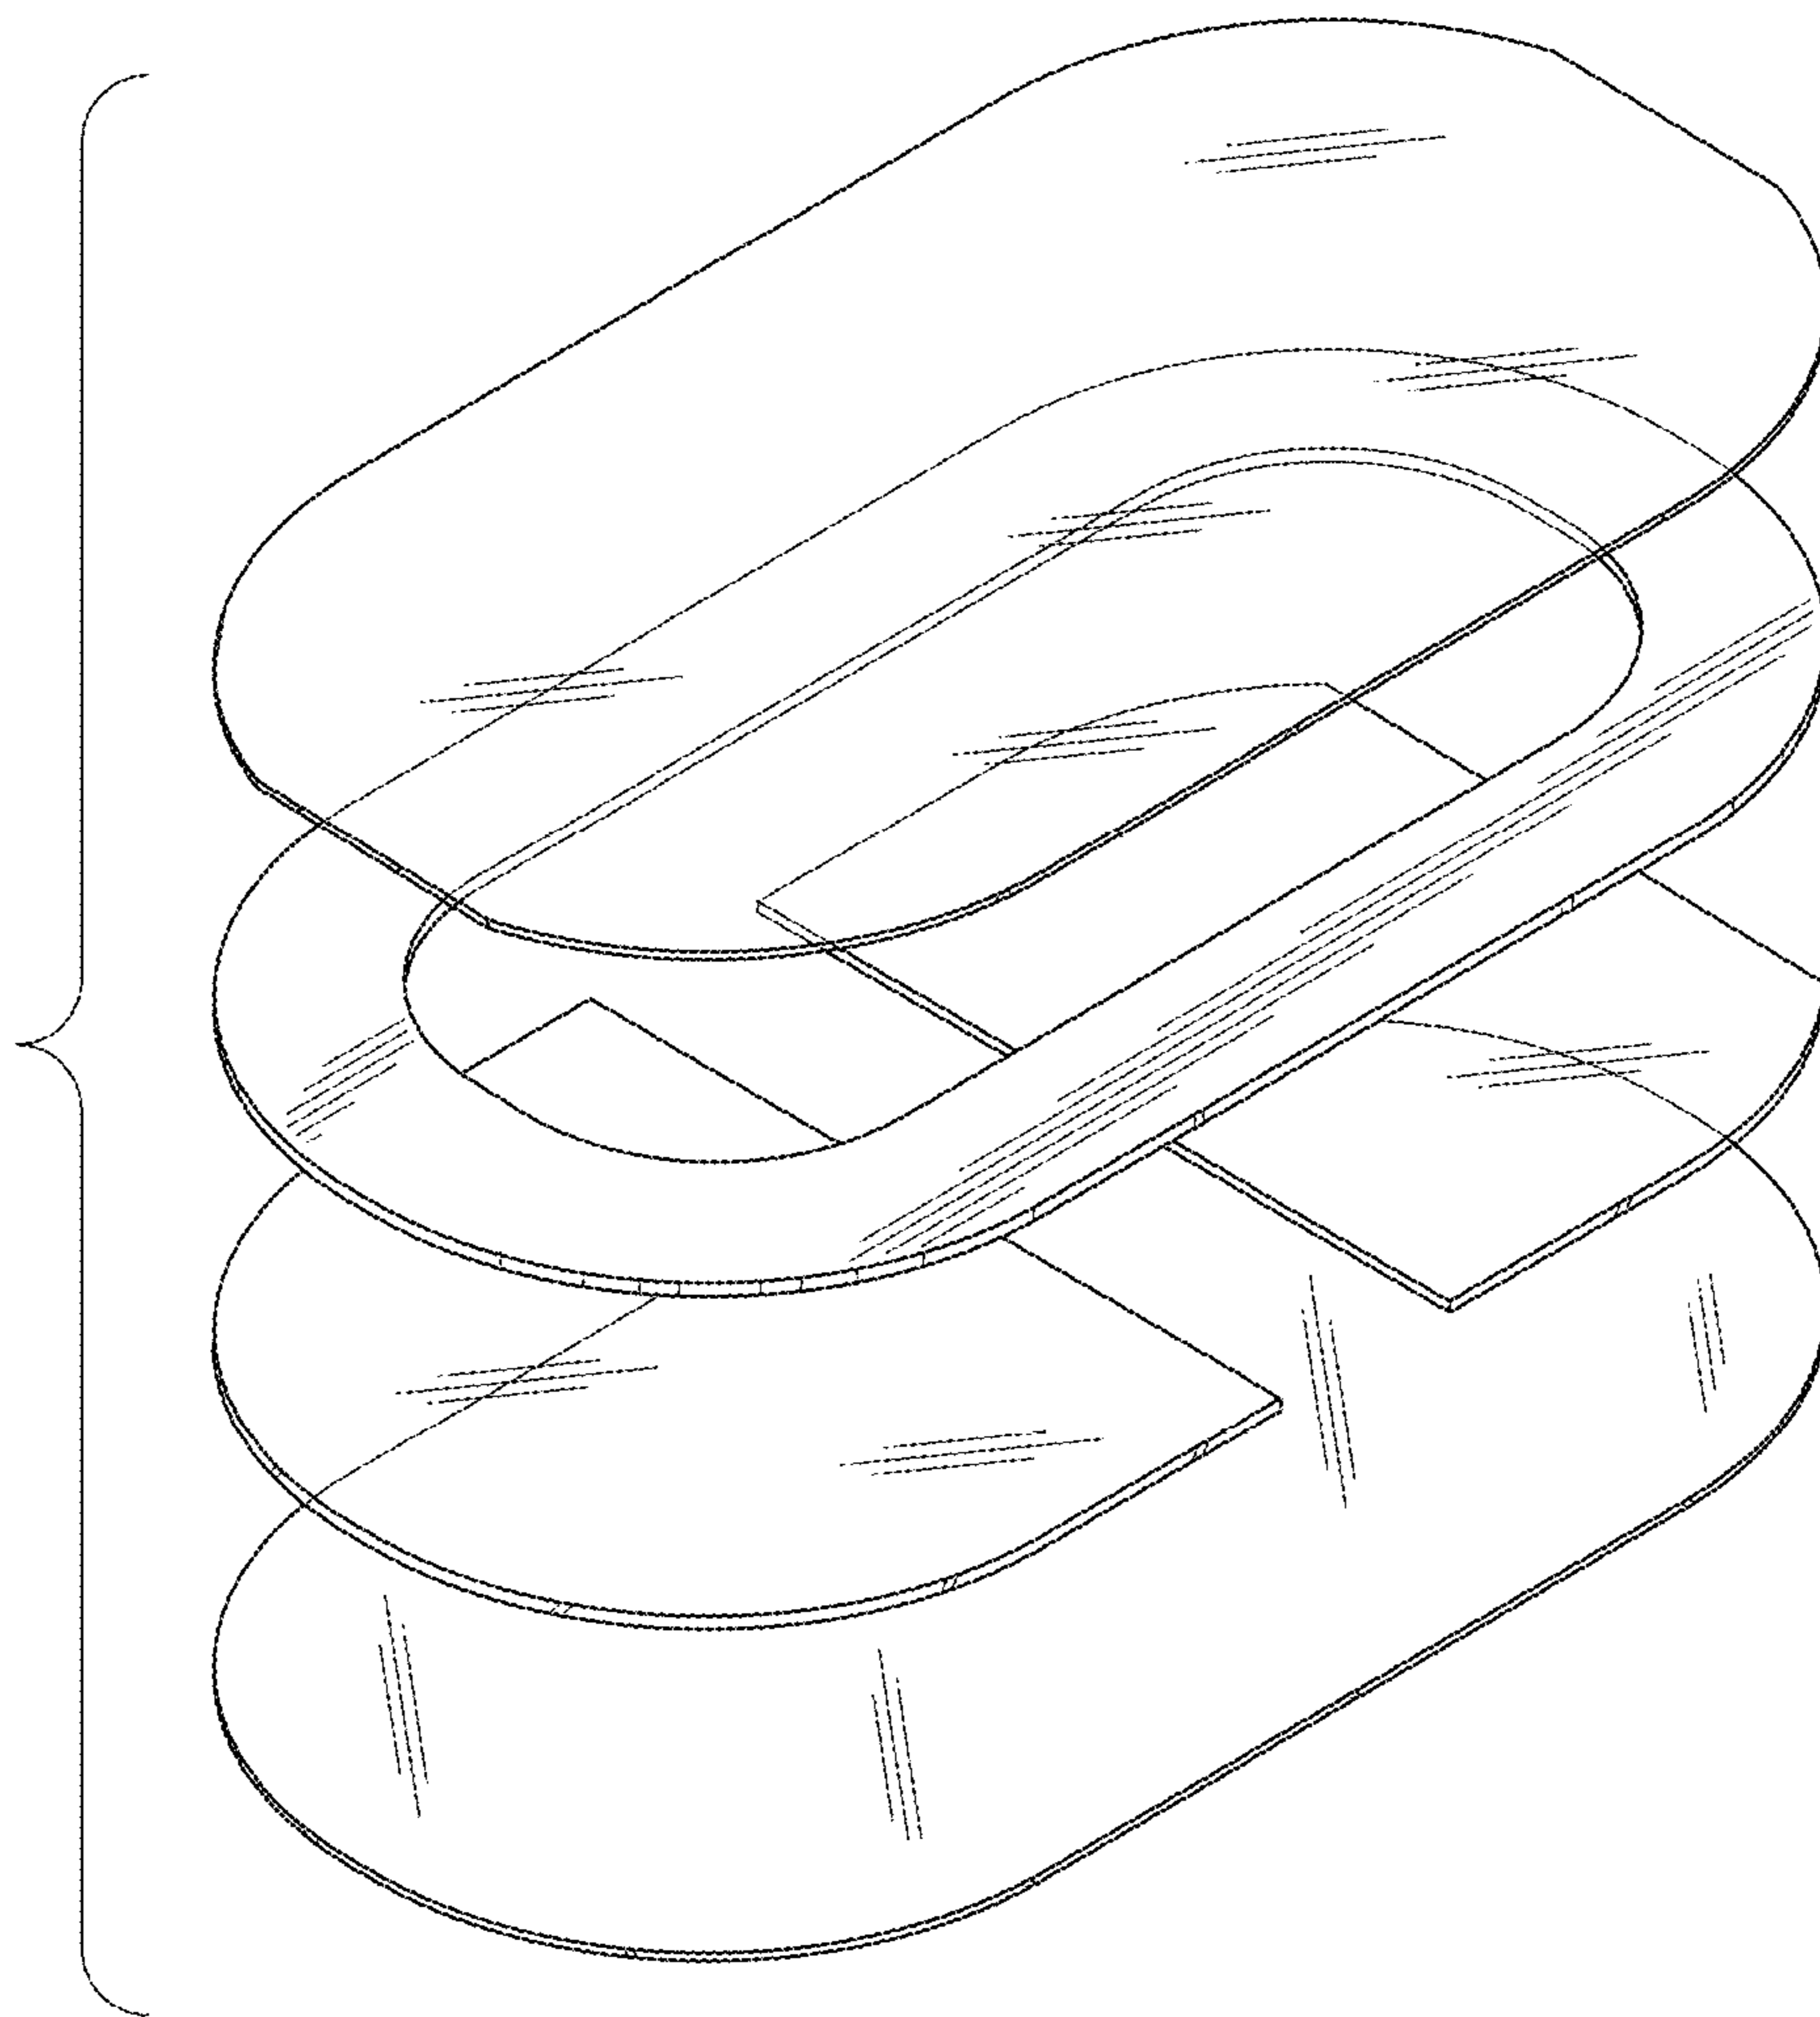

*Fig. 7*