



US00D780921S

(12) **United States Design Patent**  
**Burkinshaw et al.**(10) **Patent No.:** US D780,921 S  
(45) **Date of Patent:** \*\* Mar. 7, 2017(54) **SPINAL DISC IMPLANT WITH CONIC PROTRUSIONS**(71) Applicants: **Brian D. Burkinshaw**, Pflugerville, TX (US); **Jonathan Stupka**, Lakeway, TX (US)(72) Inventors: **Brian D. Burkinshaw**, Pflugerville, TX (US); **Jonathan Stupka**, Lakeway, TX (US)(\*\*) Term: **15 Years**(21) Appl. No.: **29/559,752**(22) Filed: **Mar. 31, 2016****Related U.S. Application Data**

(63) Continuation of application No. 29/481,785, filed on Feb. 10, 2014, now Pat. No. Des. 753,306.

(51) **LOC (10) Cl.** ..... **24-02**(52) **U.S. Cl.**USPC ..... **D24/155**(58) **Field of Classification Search**USPC ..... D24/155-157  
CPC ..... A61F 2/4611; A61F 2/442; A61F 2/447;  
A61F 2220/0025; A61F 2310/00023;  
A61F 2310/00017; A61F 2002/4475;  
A61F 2002/30841; A61F 2002/2835;  
A61F 2002/30904; A61F 2002/30785;  
A61F 2002/443; A61F 2002/30578

See application file for complete search history.

(56) **References Cited**

## U.S. PATENT DOCUMENTS

5,071,437 A 12/1991 Steffee  
7,025,787 B2 \* 4/2006 Bryan ..... A61B 17/1671  
623/17.15  
D598,105 S \* 8/2009 Krishna ..... D24/1557,601,174 B2 \* 10/2009 Kelly ..... A61B 17/02  
623/17.13  
7,901,459 B2 \* 3/2011 Hodges ..... A61F 2/4405  
623/17.14  
8,038,920 B2 \* 10/2011 Denoziere ..... A61L 27/16  
264/101  
8,092,542 B2 \* 1/2012 Bryan ..... A61B 17/02  
623/16.11  
8,226,723 B2 \* 7/2012 Conti ..... A61F 2/442  
623/17.16  
8,603,171 B2 \* 12/2013 McClellan, III ..... A61F 2/442  
623/17.16  
8,926,703 B2 \* 1/2015 Michelson ..... A61F 2/4455  
623/17.16  
2005/0251260 A1 \* 11/2005 Gerber ..... A61F 2/441  
623/17.13  
2006/0276790 A1 12/2006 Dawson  
2009/0216331 A1 8/2009 Grotz  
2012/0191193 A1 7/2012 Trieu

\* cited by examiner

*Primary Examiner* — Charles Hanson(74) *Attorney, Agent, or Firm* — ClearPat Services, LLC;  
Brian Burkinshaw

(57)

**CLAIM**

The ornamental design for a spinal disc implant with conic protrusions, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan elevation view of a spinal disc implant, showing our new design;

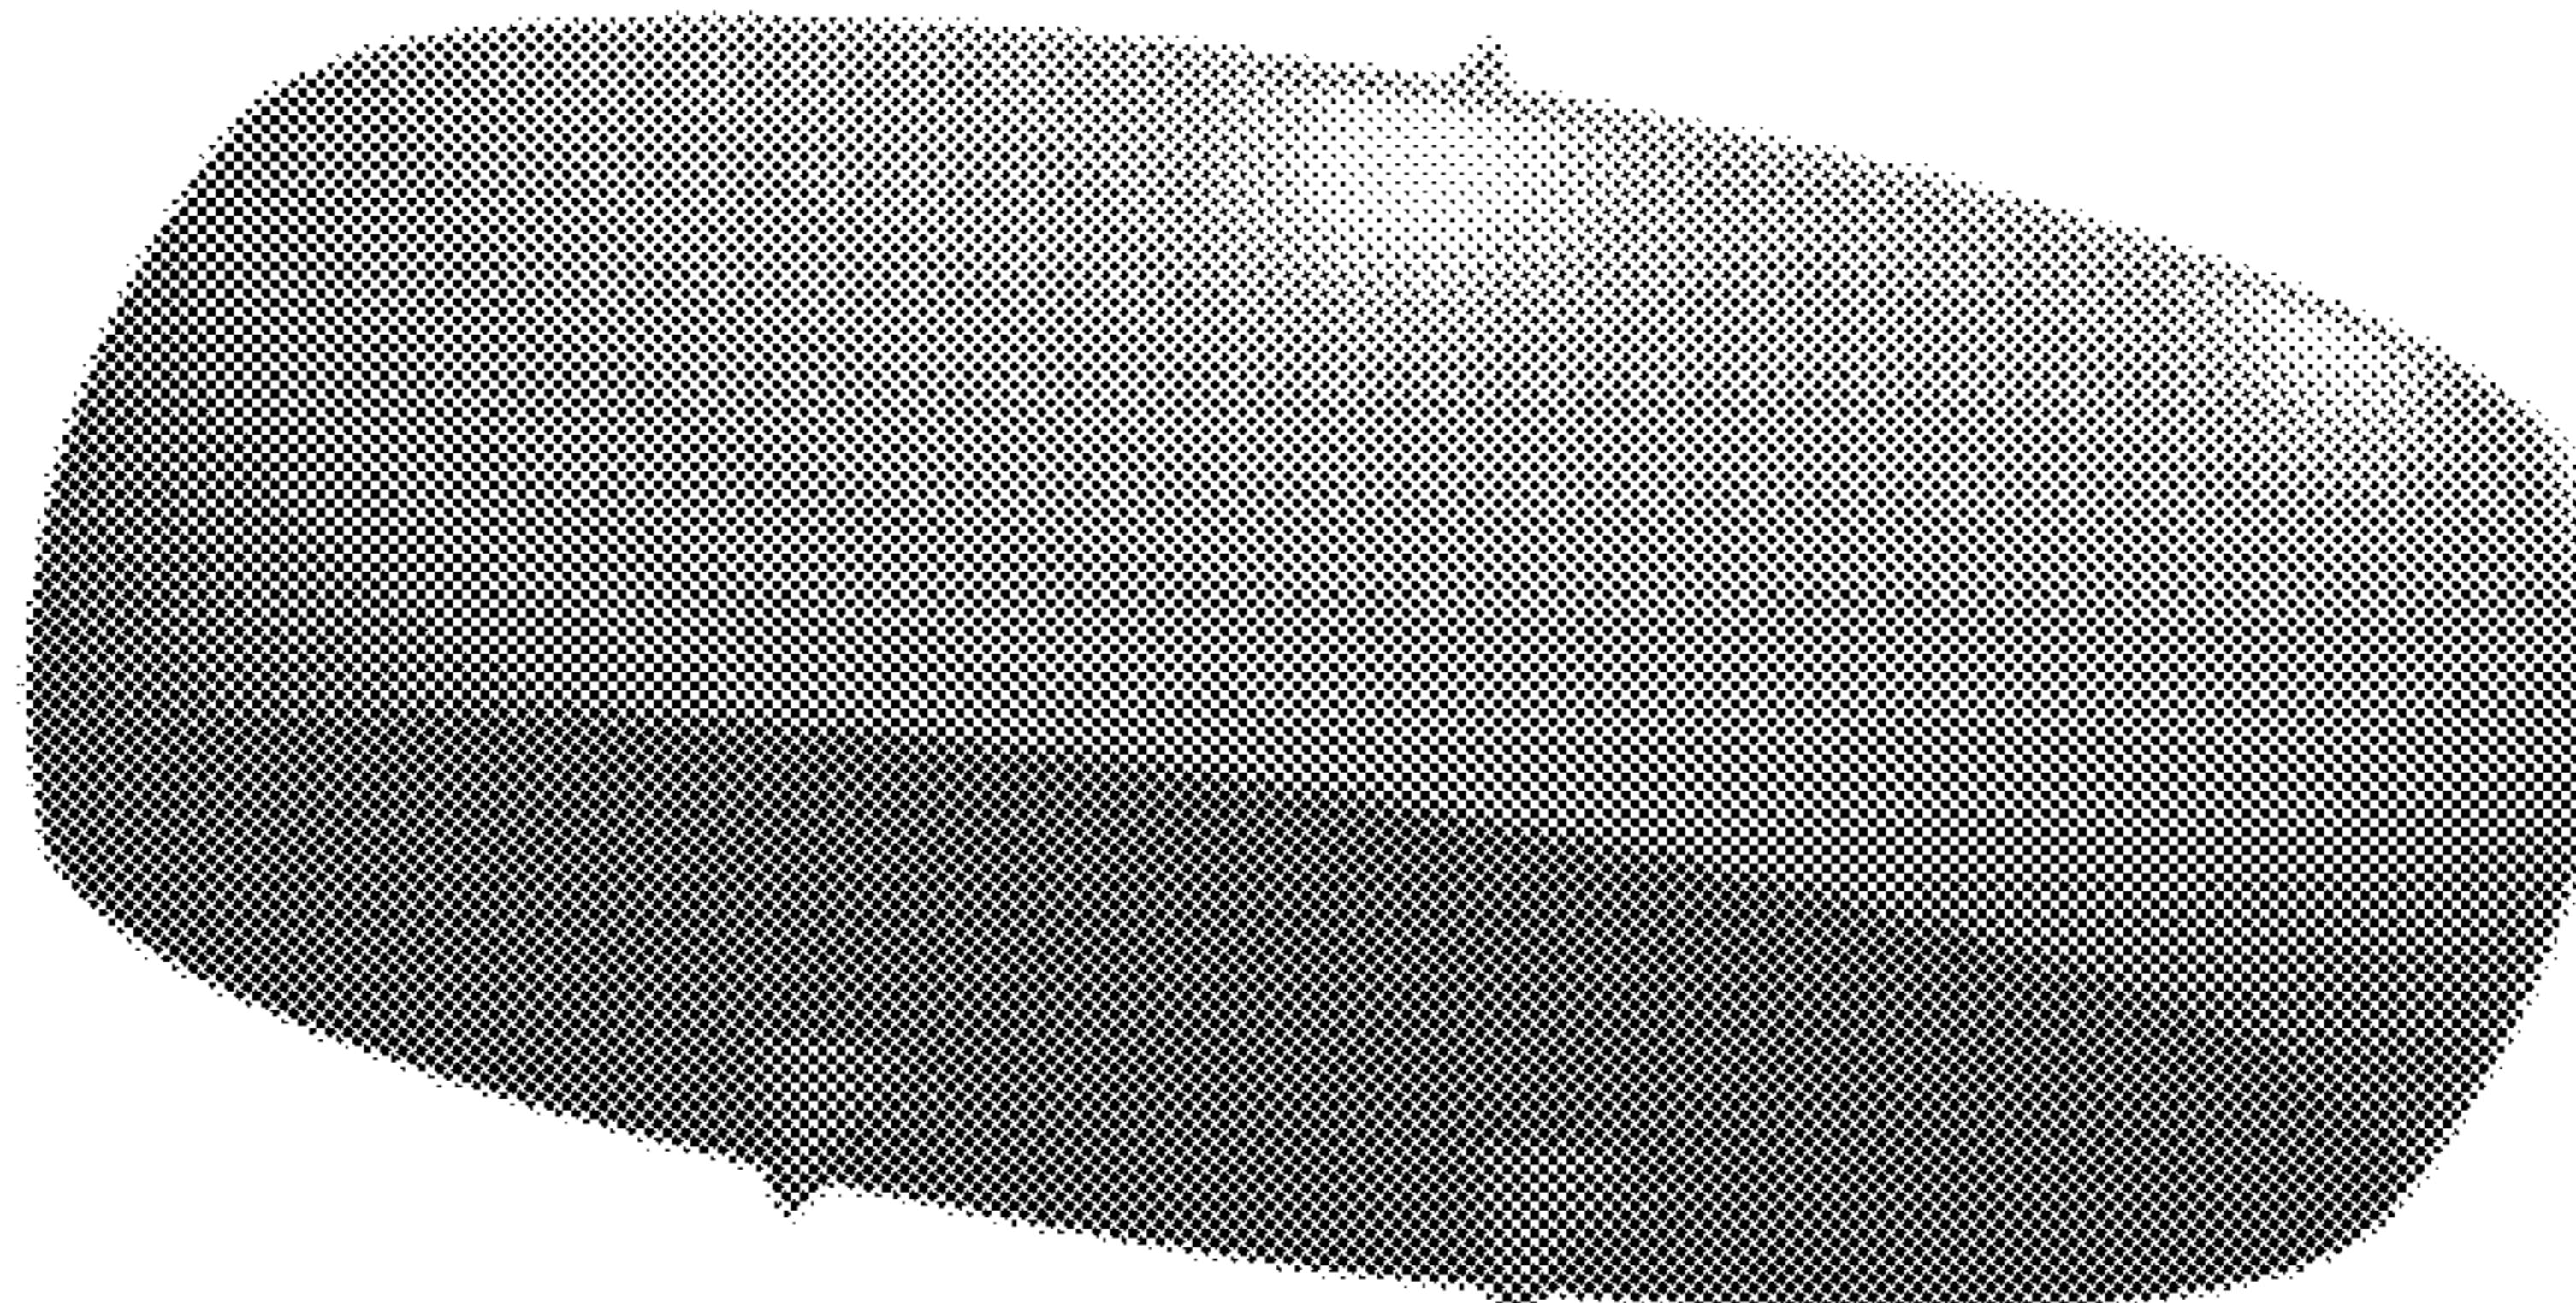
FIG. 2 is a bottom plan view thereof;


FIG. 3 is a side elevation view thereof;

FIG. 4 is a side perspective view of thereof;


FIG. 5 is a non-textured bottom perspective view thereof; and,

FIG. 6 is an alternate textured bottom perspective view thereof.


**1 Claim, 1 Drawing Sheet**

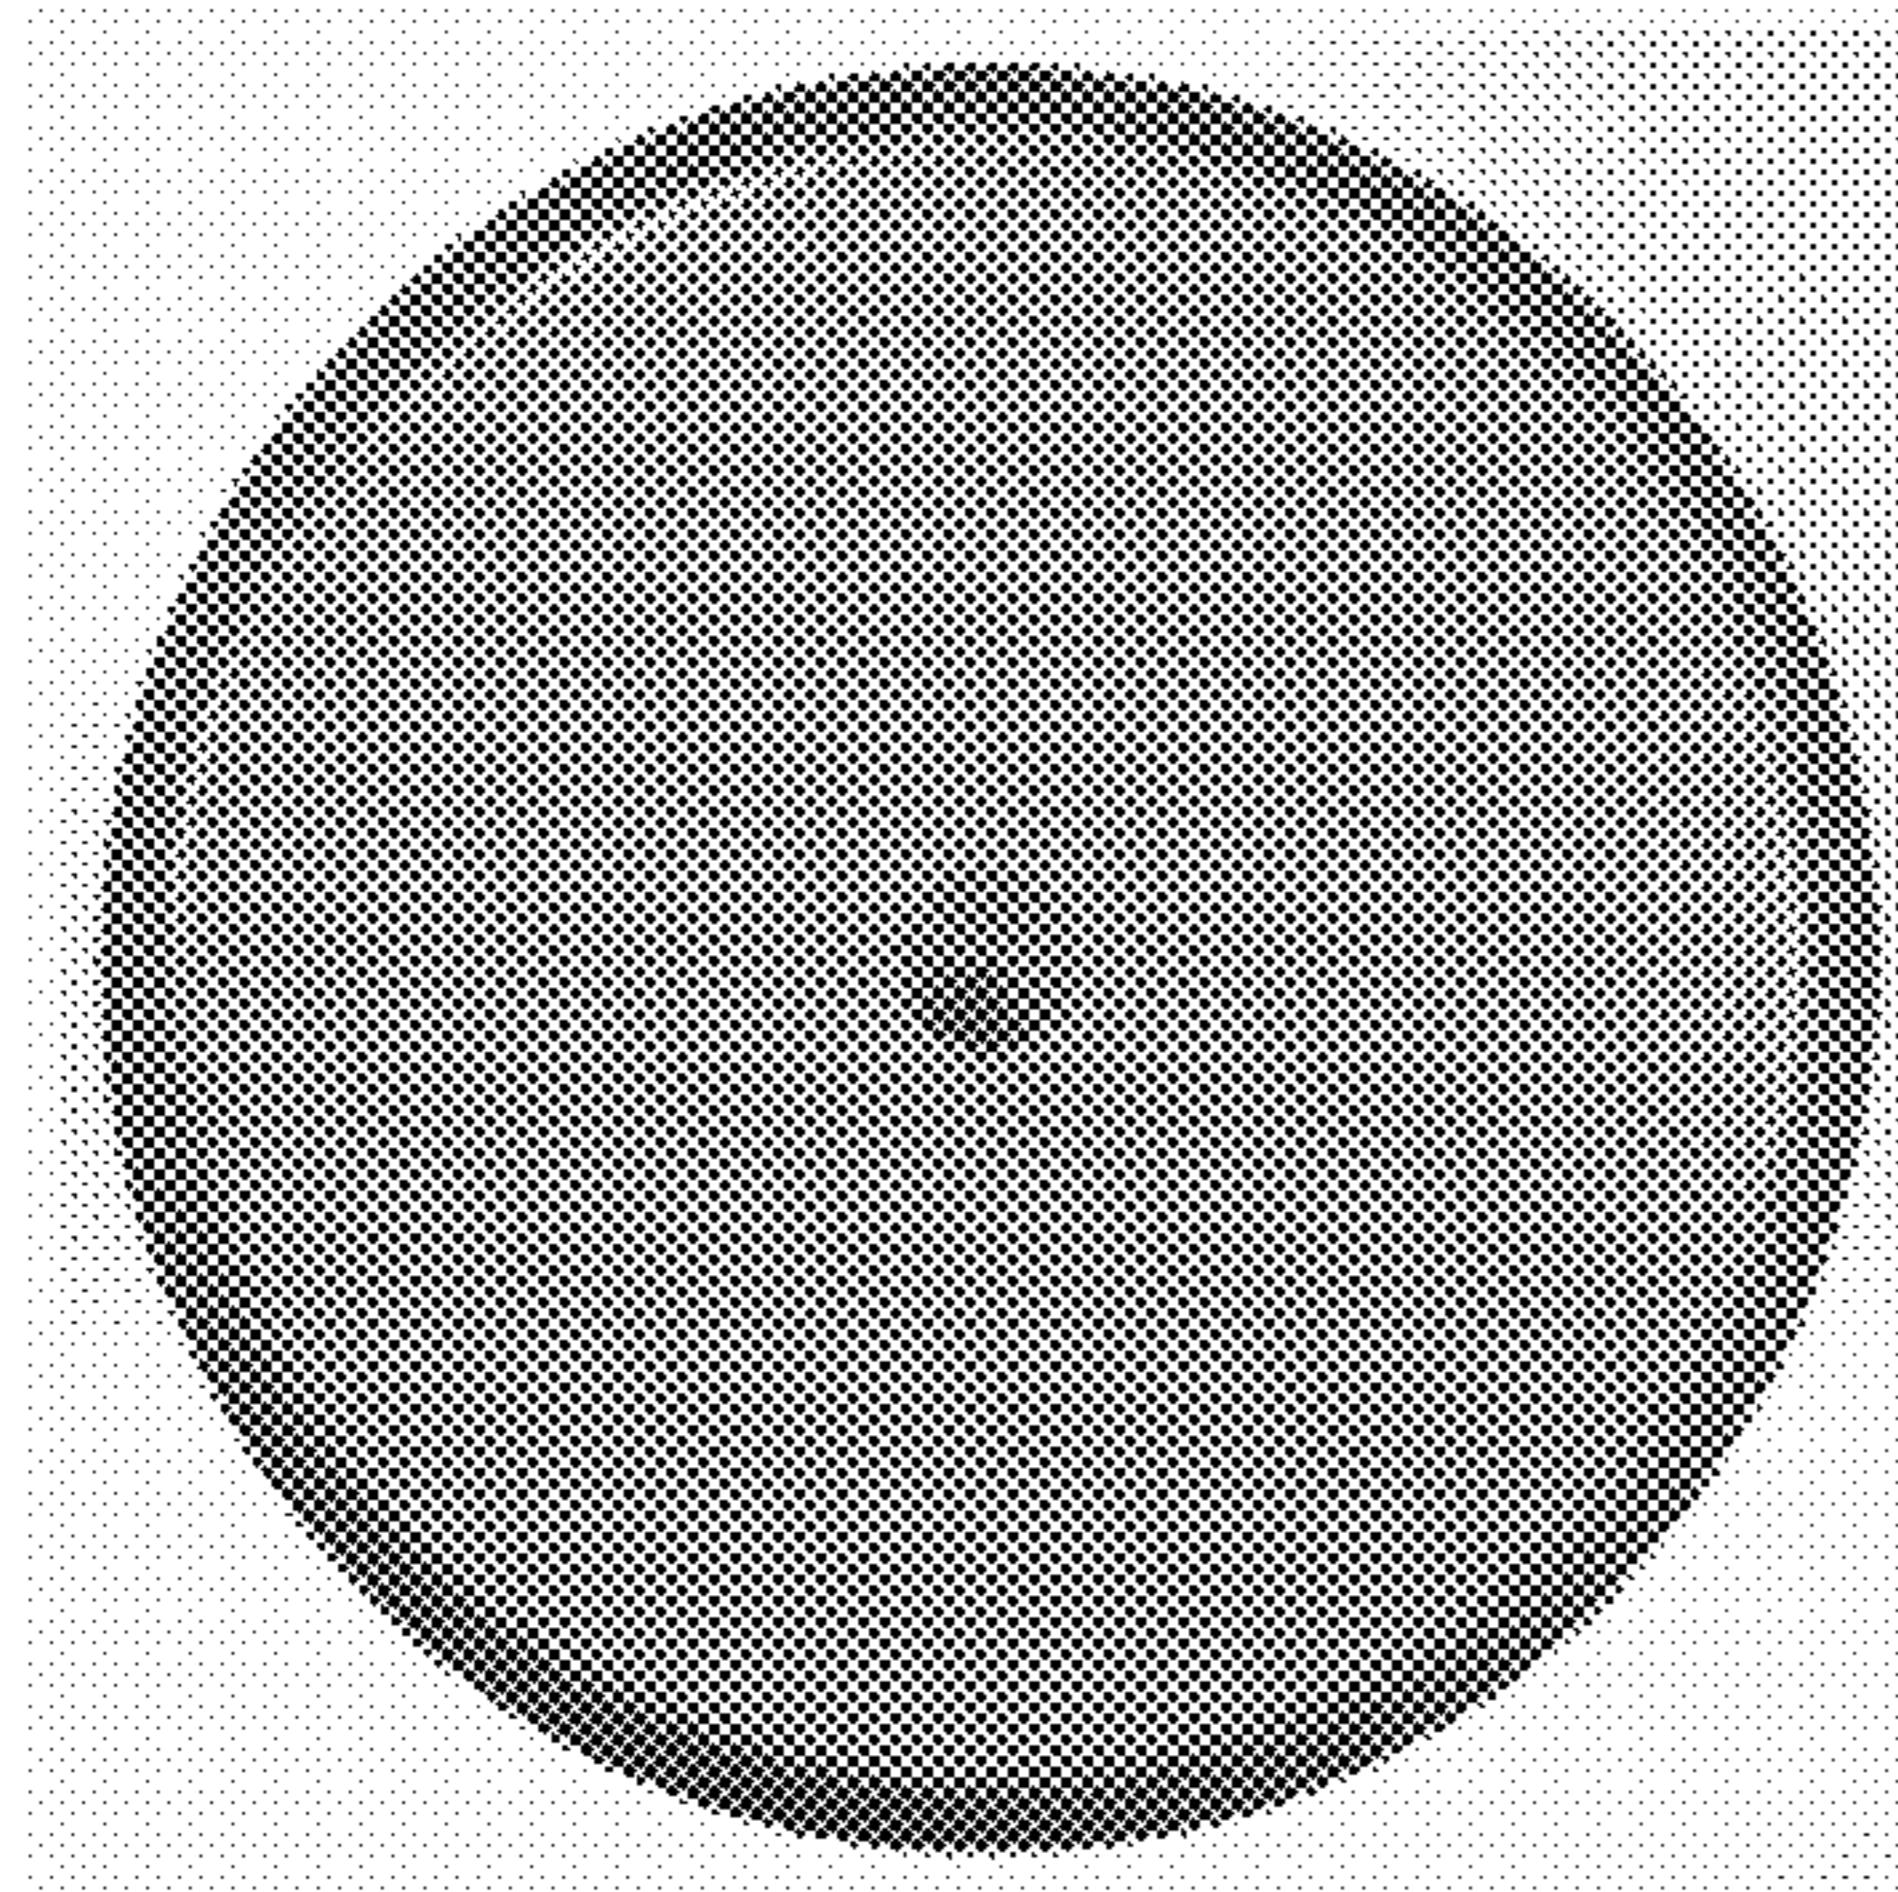


**FIG. 1**

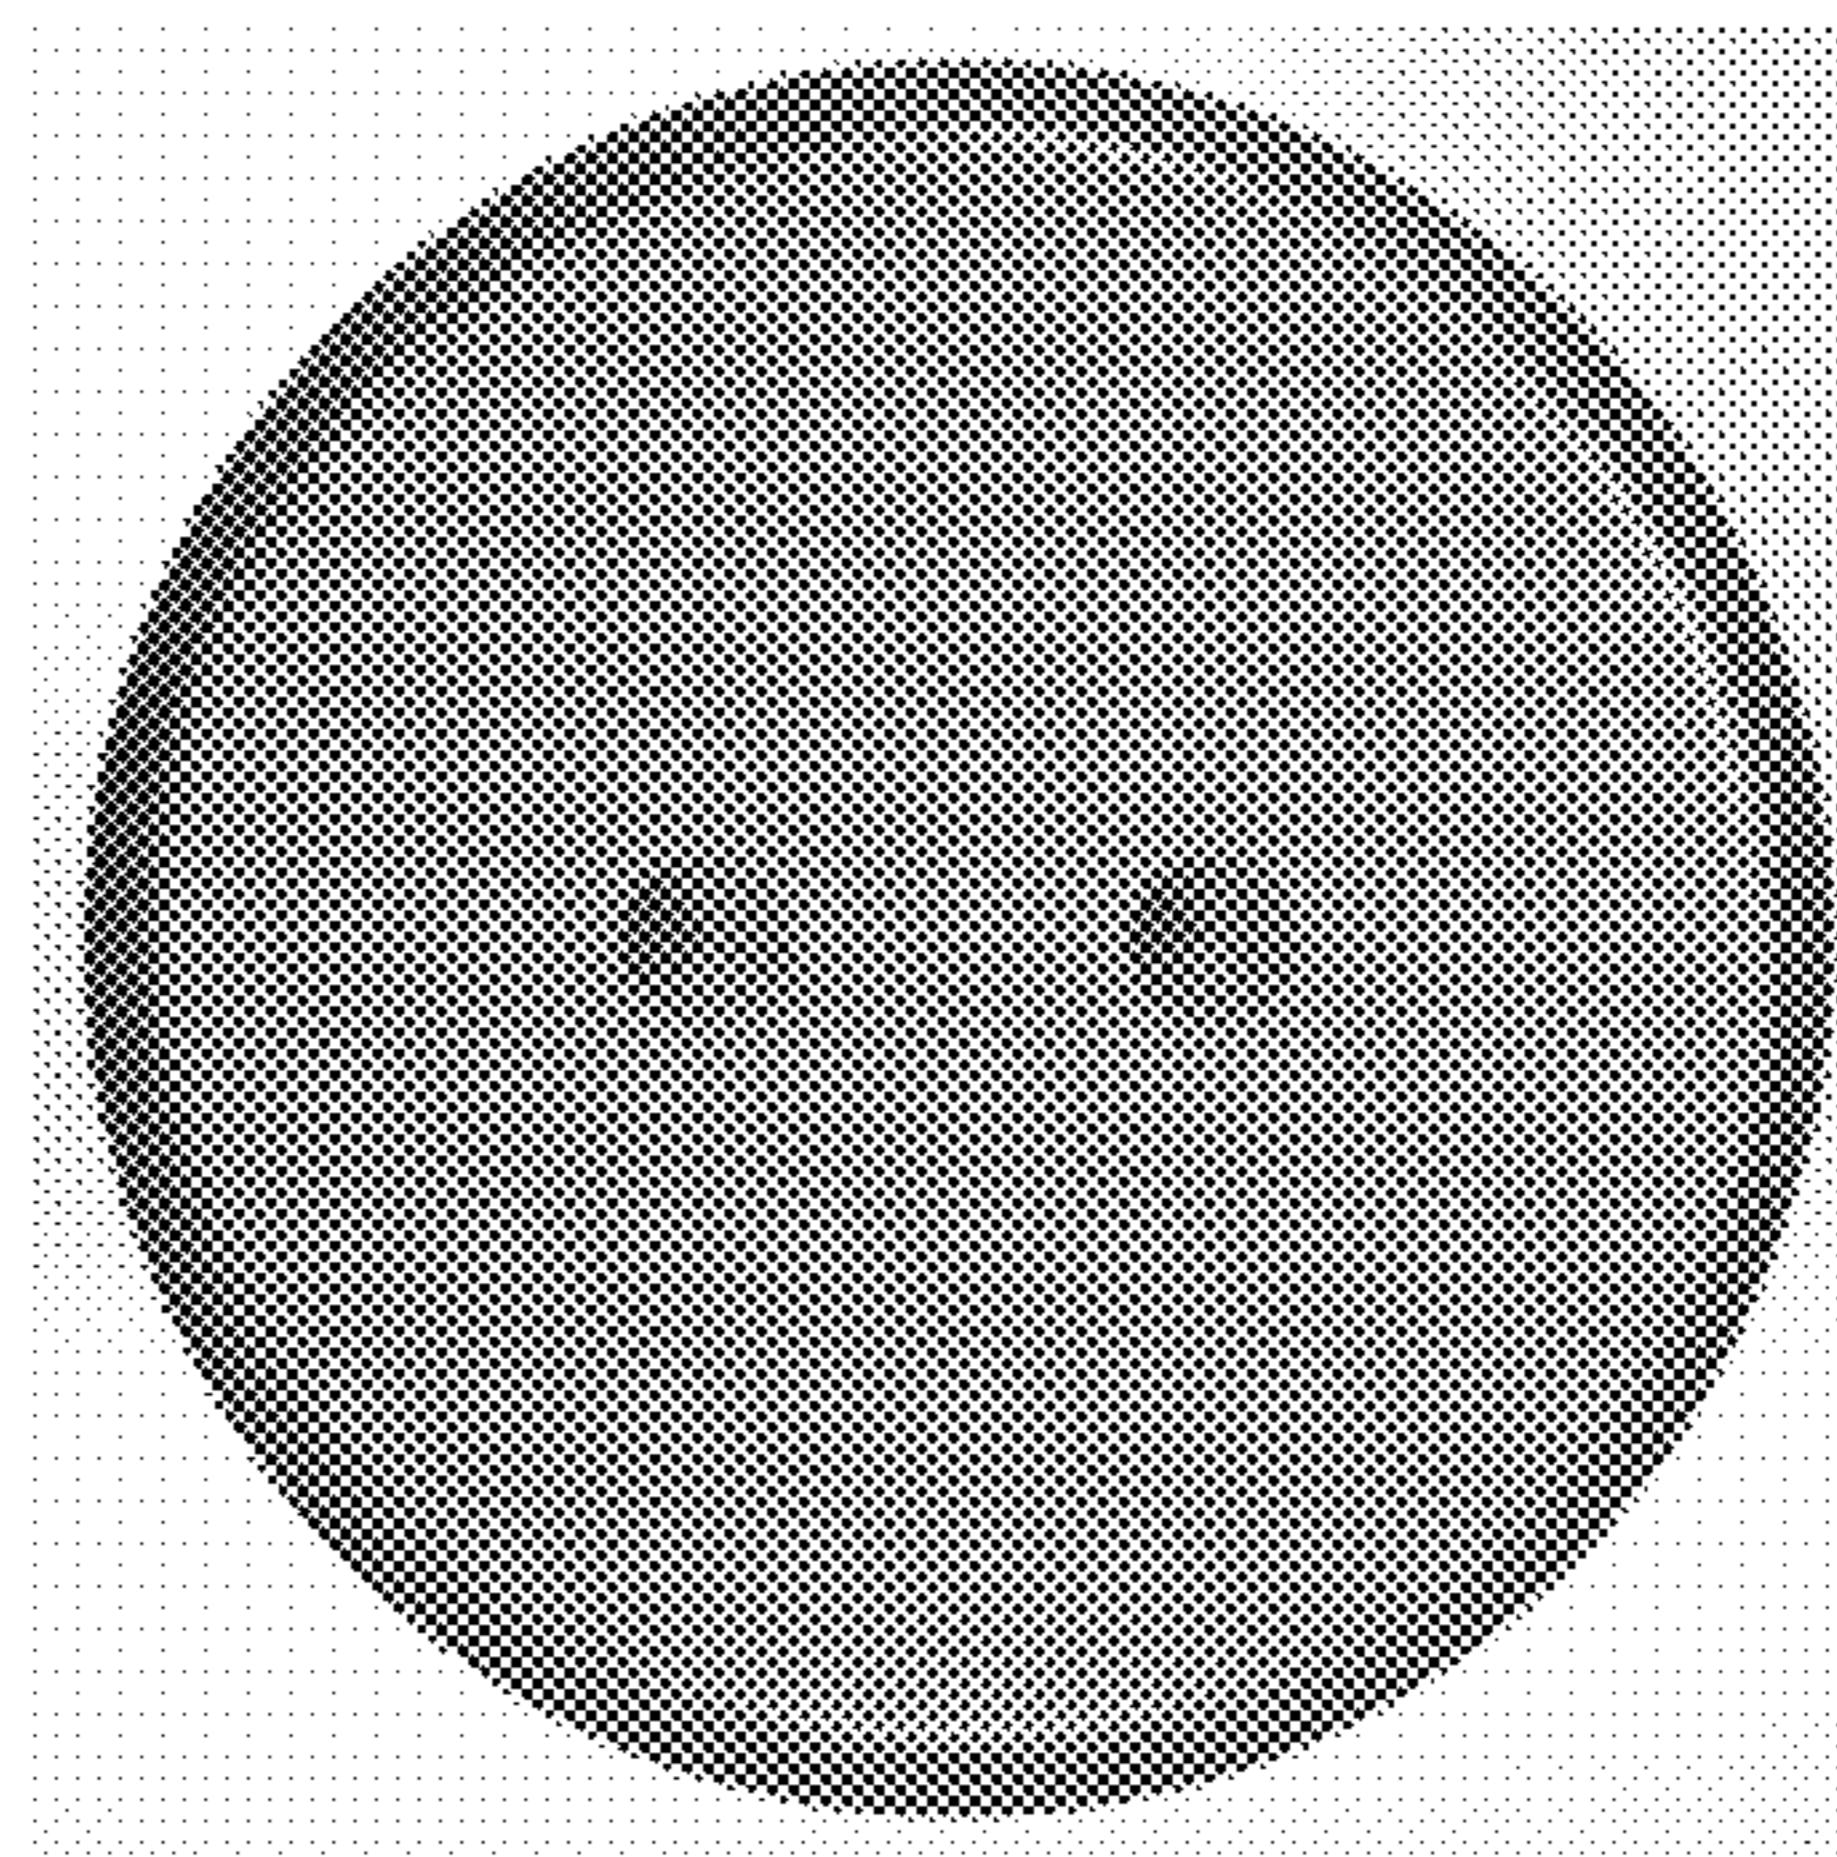


**FIG. 2**

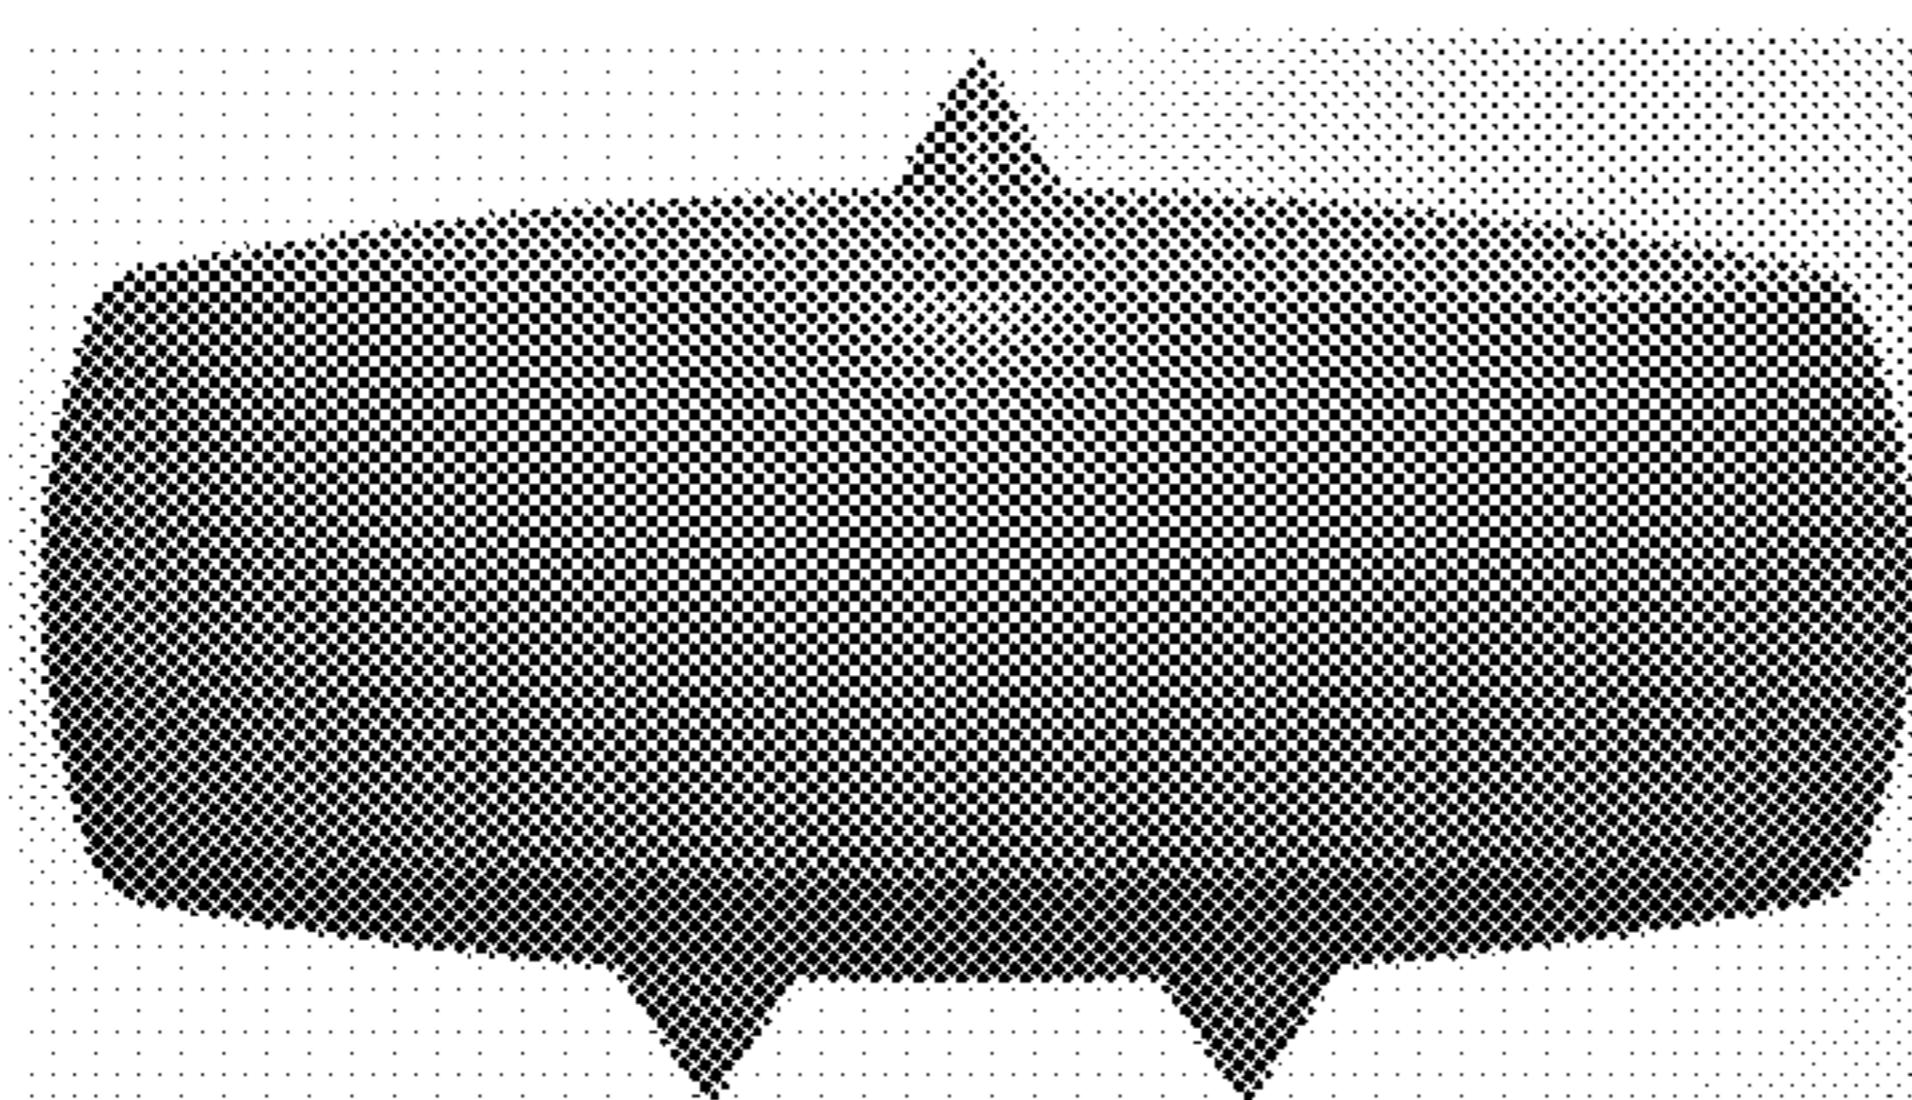


**FIG. 3**

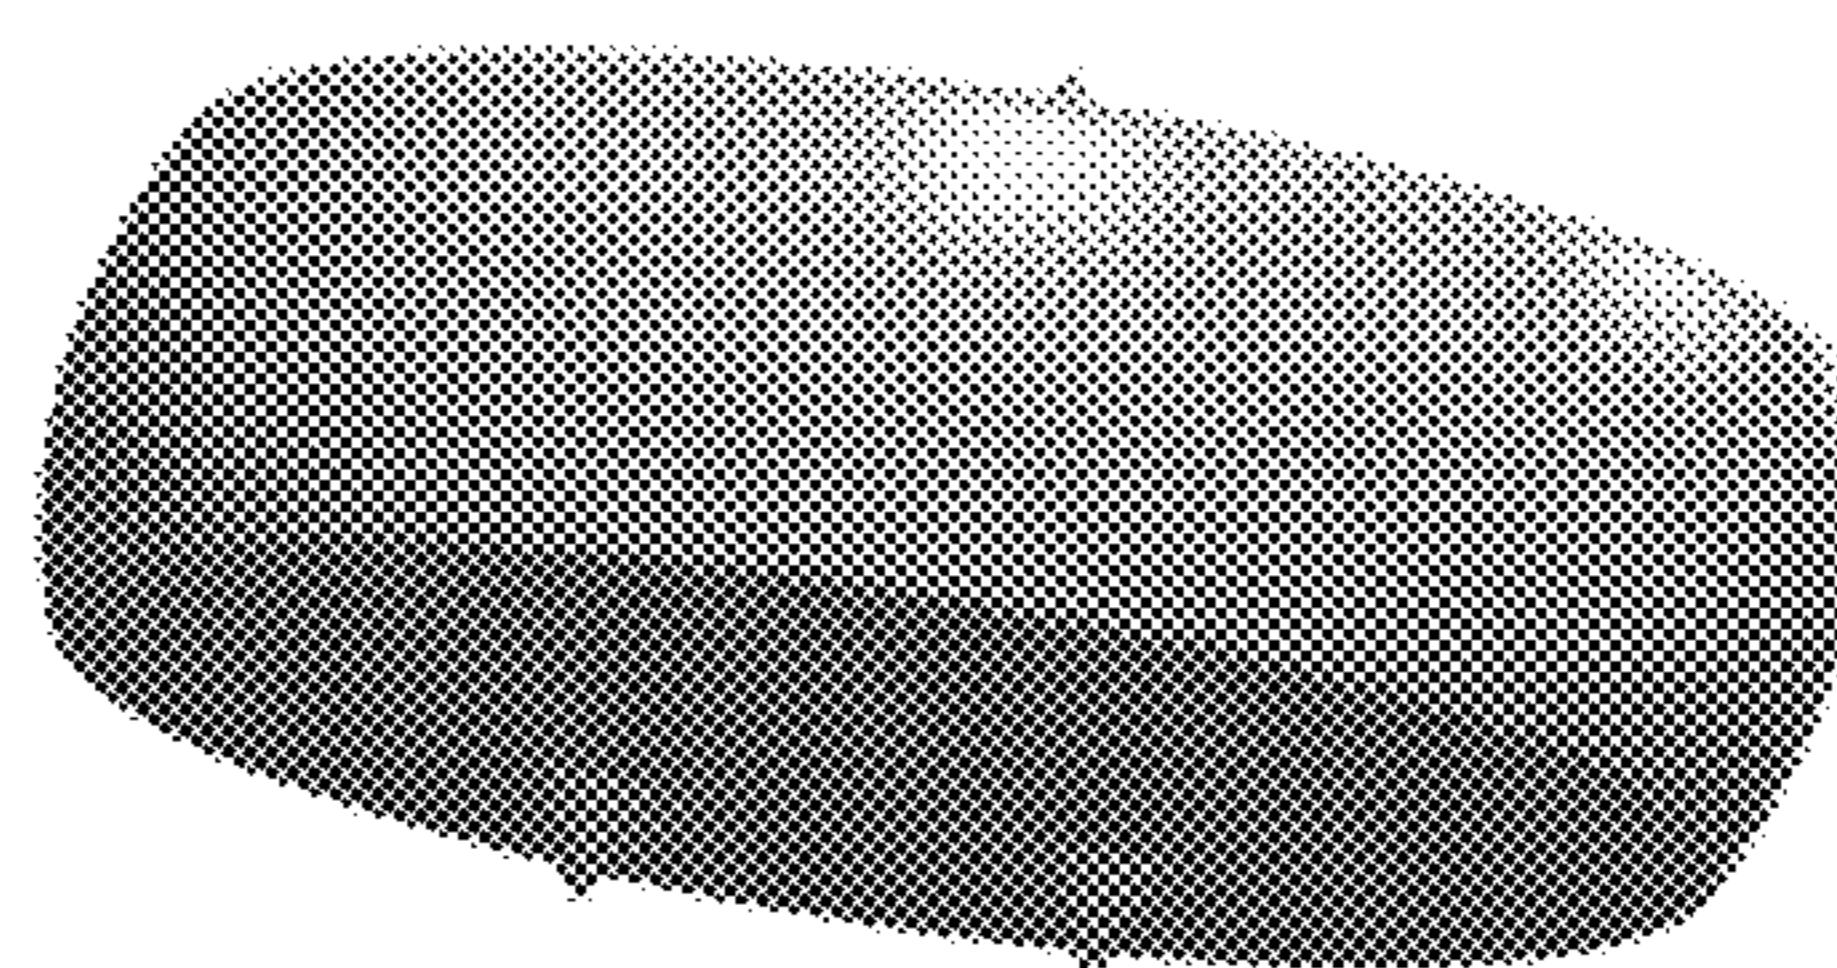

**FIG. 4**

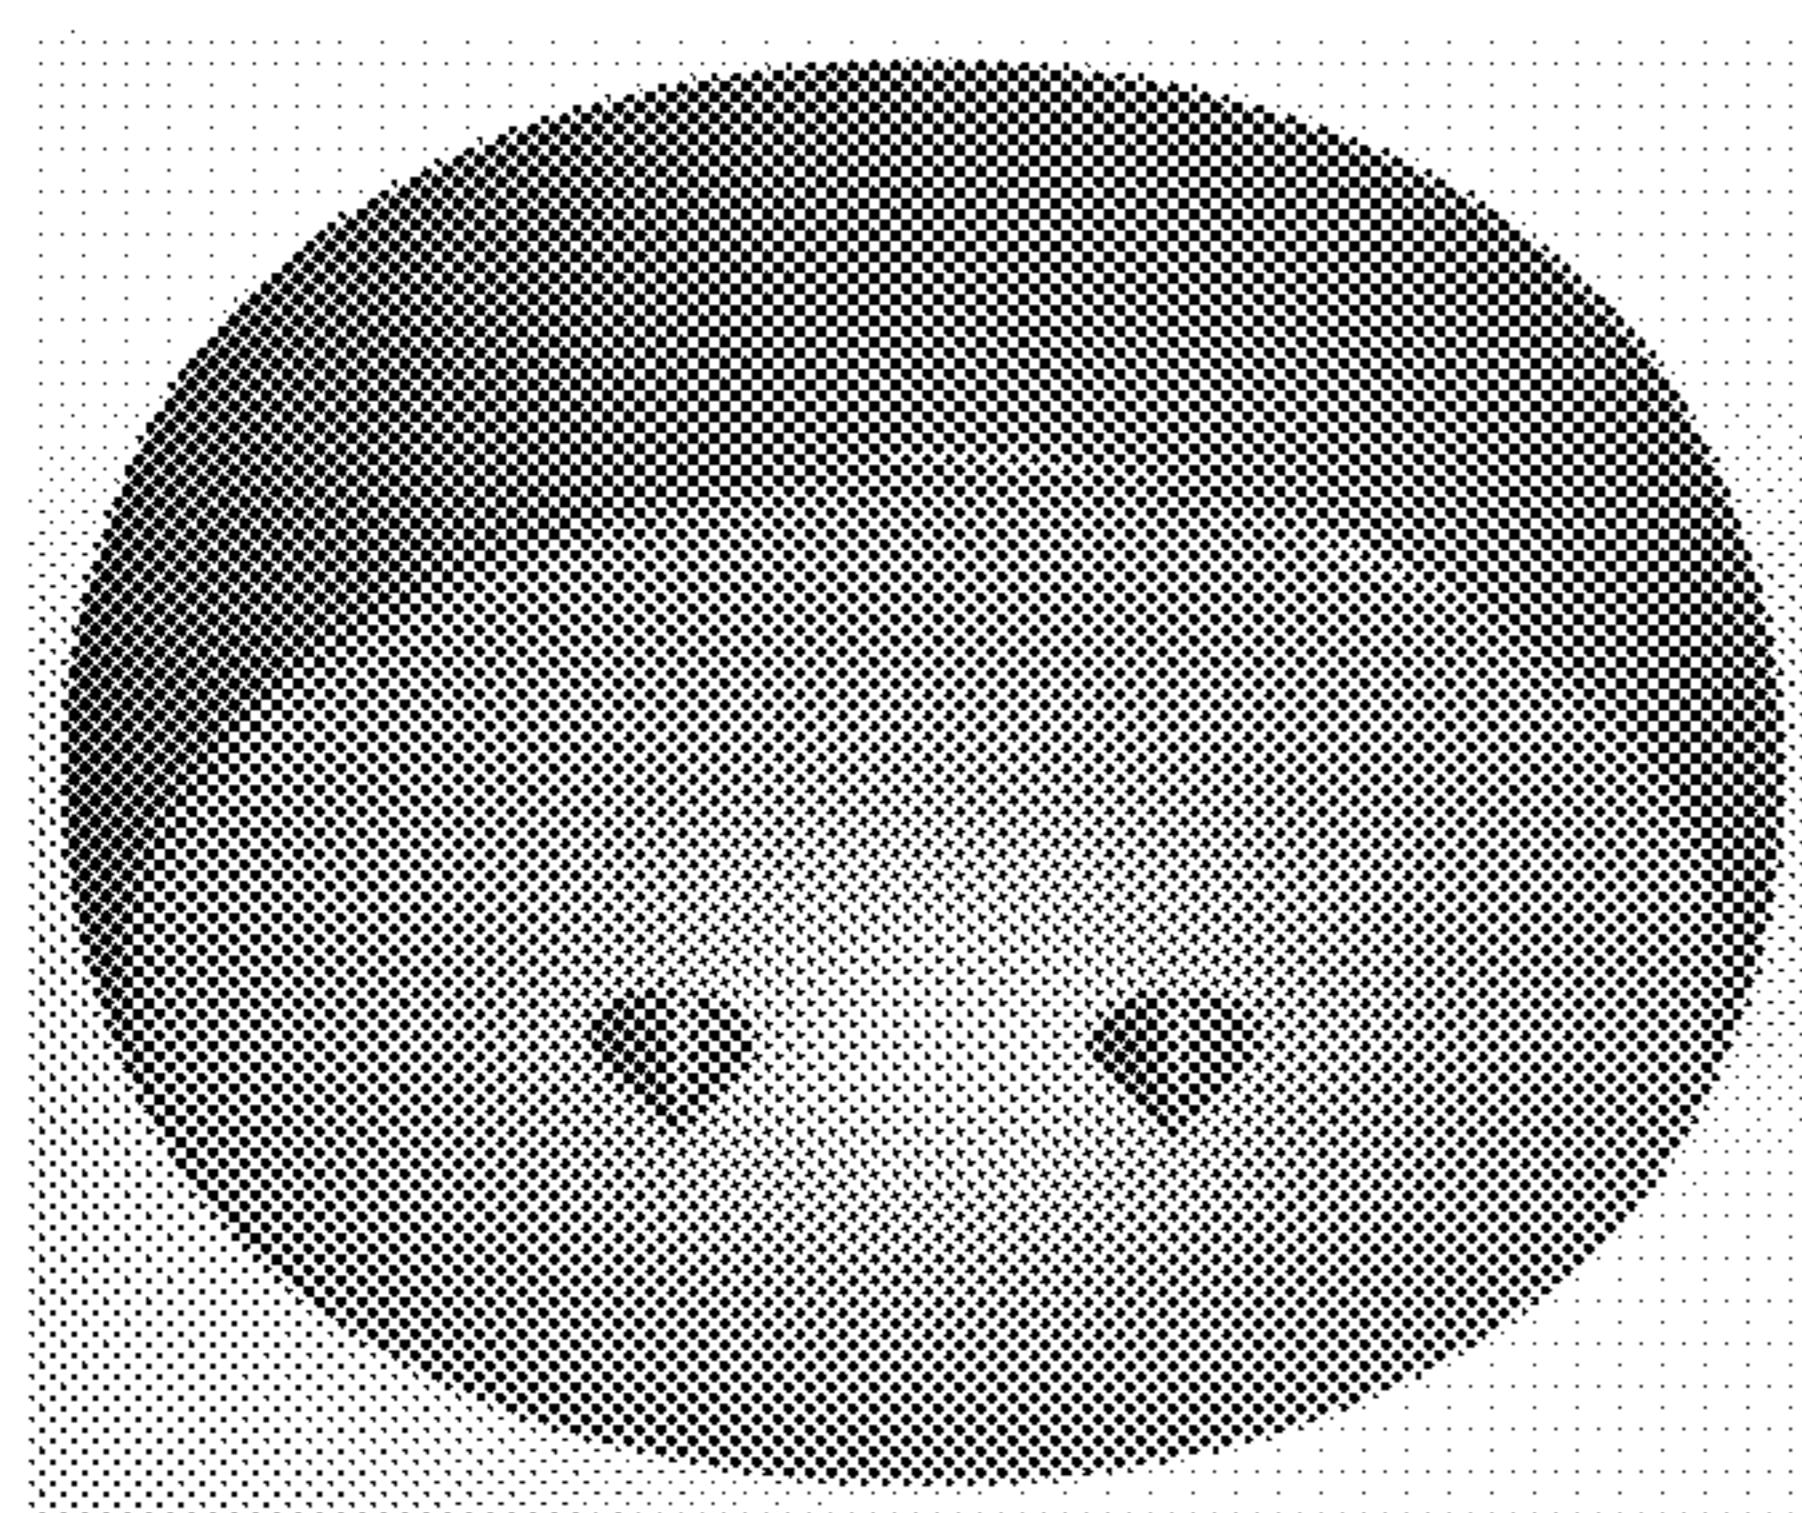

**FIG. 5**

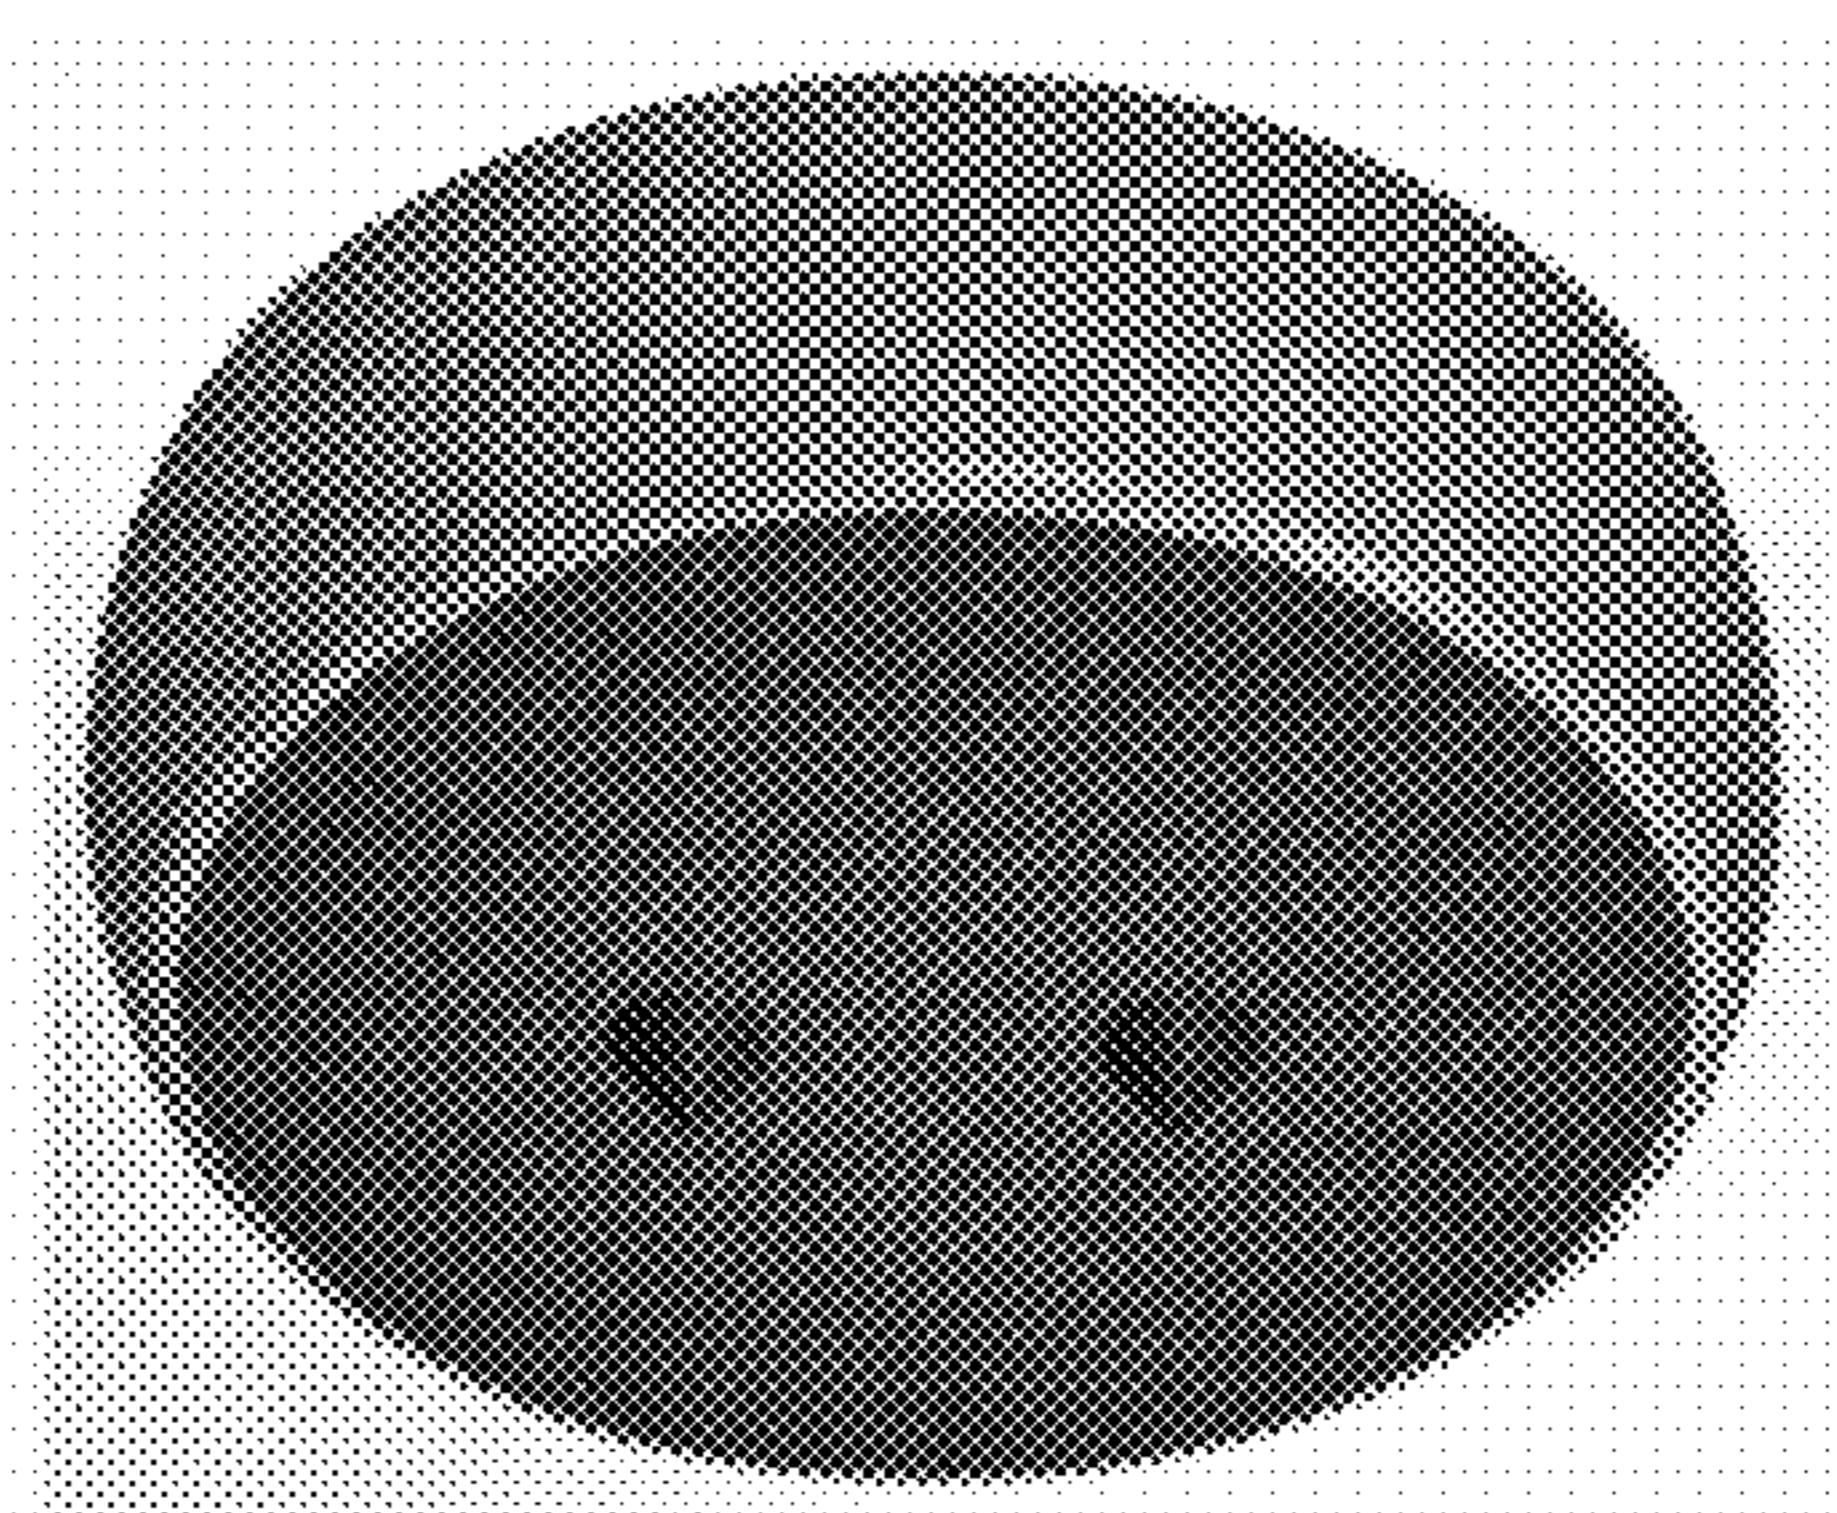

**FIG. 6**