



US00D783832S

(12) **United States Design Patent**  
**Dascoli et al.**

(10) **Patent No.:** **US D783,832 S**

(45) **Date of Patent:** **\*\* Apr. 11, 2017**

(54) **AUTOMATED EXTERNAL DEFIBRILLATOR  
ELECTRODE PAD**

(71) Applicant: **ZOLL Medical Corporation**,  
Chelmsford, MA (US)

(72) Inventors: **Melissa M. Dascoli**, Wakefield, MA  
(US); **George Reilly**, Chelmsford, MA  
(US); **Ian Durrant**, Arlington, MA  
(US); **Deborah T. Jones**, Dartmouth,  
MA (US); **Mark Bates**, West Newton,  
MA (US); **David N. Craige, III**,  
Attleboro, MA (US); **Brian  
Stonecipher**, Thousand Oaks, CA (US);  
**James Wilson**, Norwood, MA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/556,122**

(22) Filed: **Feb. 26, 2016**

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/167**

(58) **Field of Classification Search**  
USPC ..... D24/165–168, 186, 187, 107; D10/75;  
D3/203.1

CPC ..... A61N 1/39; A61N 1/3925; A61N 1/3968;  
A61N 1/3987; A61N 1/3993; A61N  
1/046; A61N 1/0484; A61N 1/0492

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D409,752 S \* 5/1999 Bishay ..... D24/187  
D425,203 S \* 5/2000 Sheehan ..... D24/187  
D492,782 S \* 7/2004 Faller ..... D24/167

6,782,293 B2 \* 8/2004 Dupelle ..... A61N 1/0492  
607/142  
D498,848 S \* 11/2004 Vaisnys ..... D24/187  
D524,943 S \* 7/2006 Faller ..... D24/167  
D675,739 S \* 2/2013 McCormack ..... D24/168  
9,091,718 B2 \* 7/2015 Craige, III ..... A61N 1/046  
9,314,610 B2 \* 4/2016 Khuon ..... A61N 1/046  
2014/0012360 A1 \* 1/2014 Griesser ..... A61N 1/046  
607/142  
2014/0170622 A1 \* 6/2014 Pastrick ..... G09B 23/288  
434/265  
2016/0082246 A1 \* 3/2016 Piazza ..... A61N 1/0404  
607/5

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Fish & Richardson P.C.

(57) **CLAIM**

The ornamental design for an automated external defibril-  
lator electrode pad, substantially as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the automated external  
defibrillator electrode pad.

FIG. 2 is a front view thereof.

FIG. 3 is a back view thereof.

FIG. 4 is right side view thereof as shown from FIG. 2.


FIG. 5 is left side view thereof as shown from FIG. 2.

FIG. 6 is top view thereof as shown from FIG. 2; and,

FIG. 7 is bottom view thereof as shown from FIG. 2.

The broken lines immediately adjacent the shaded areas  
represent the bounds of the claim, while all other broken  
lines are directed to environment and are for illustrative  
purposes only; the broken lines form no part of the claimed  
design.

**1 Claim, 5 Drawing Sheets**

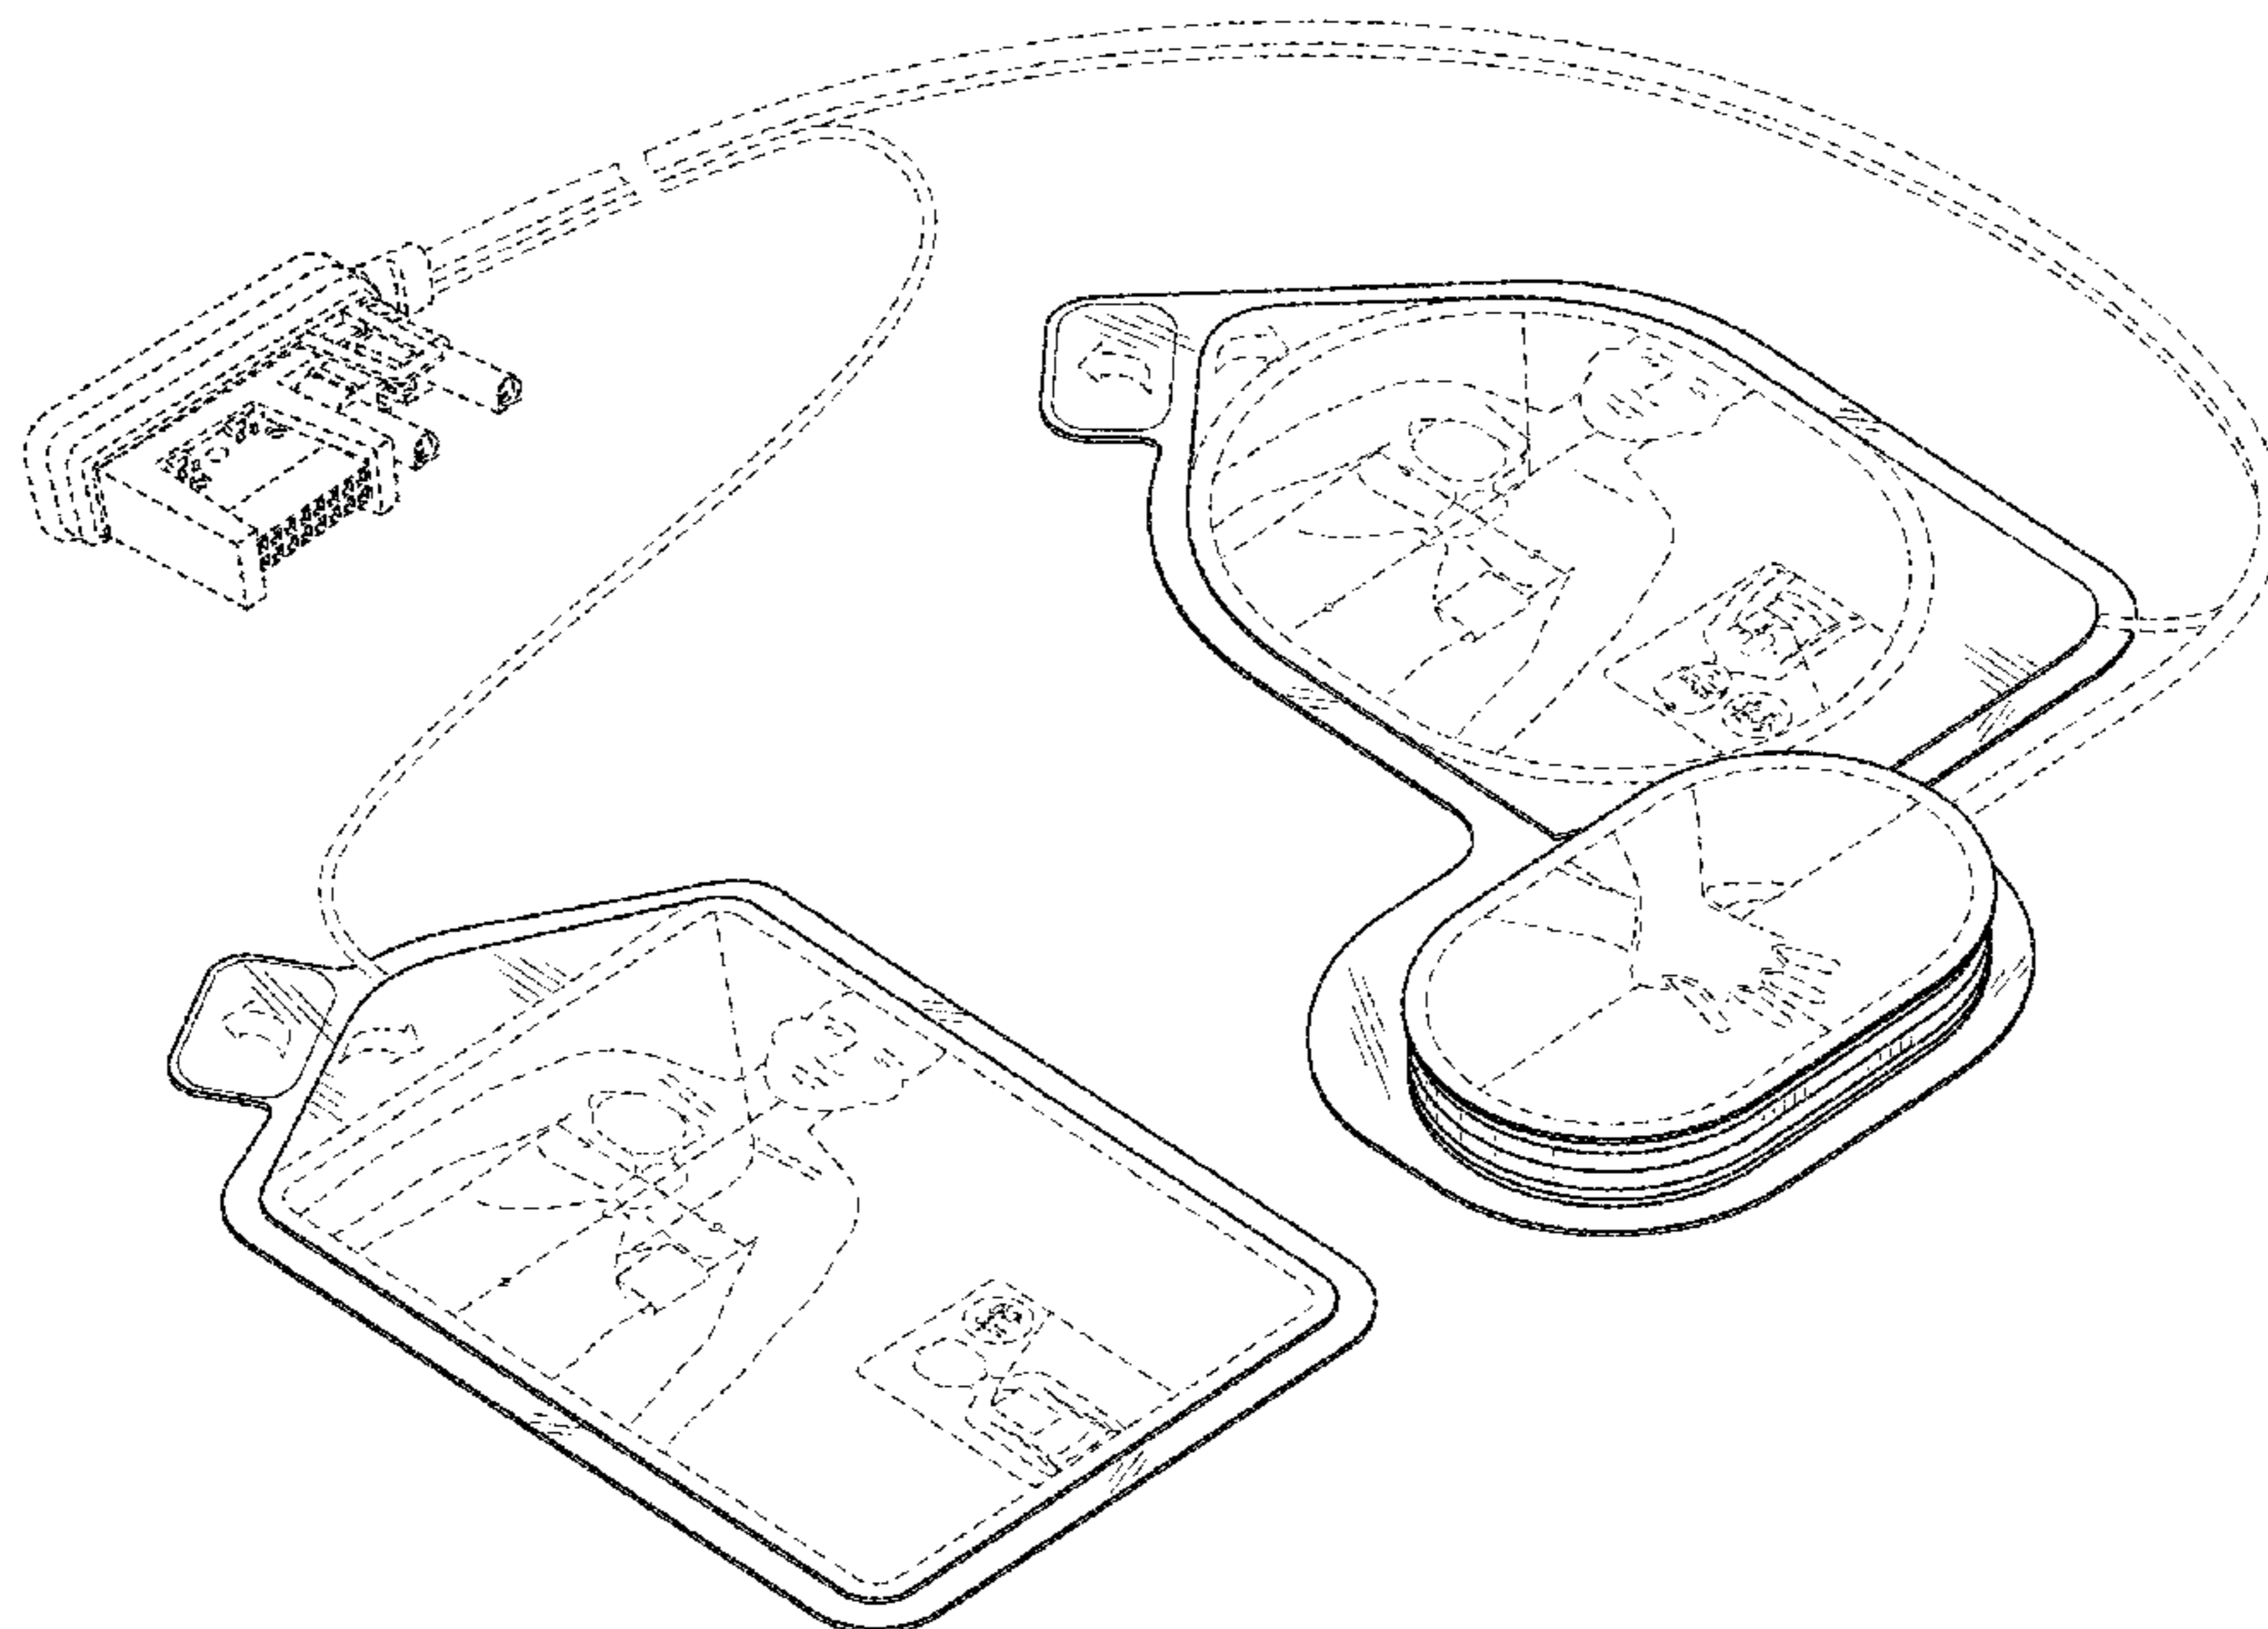

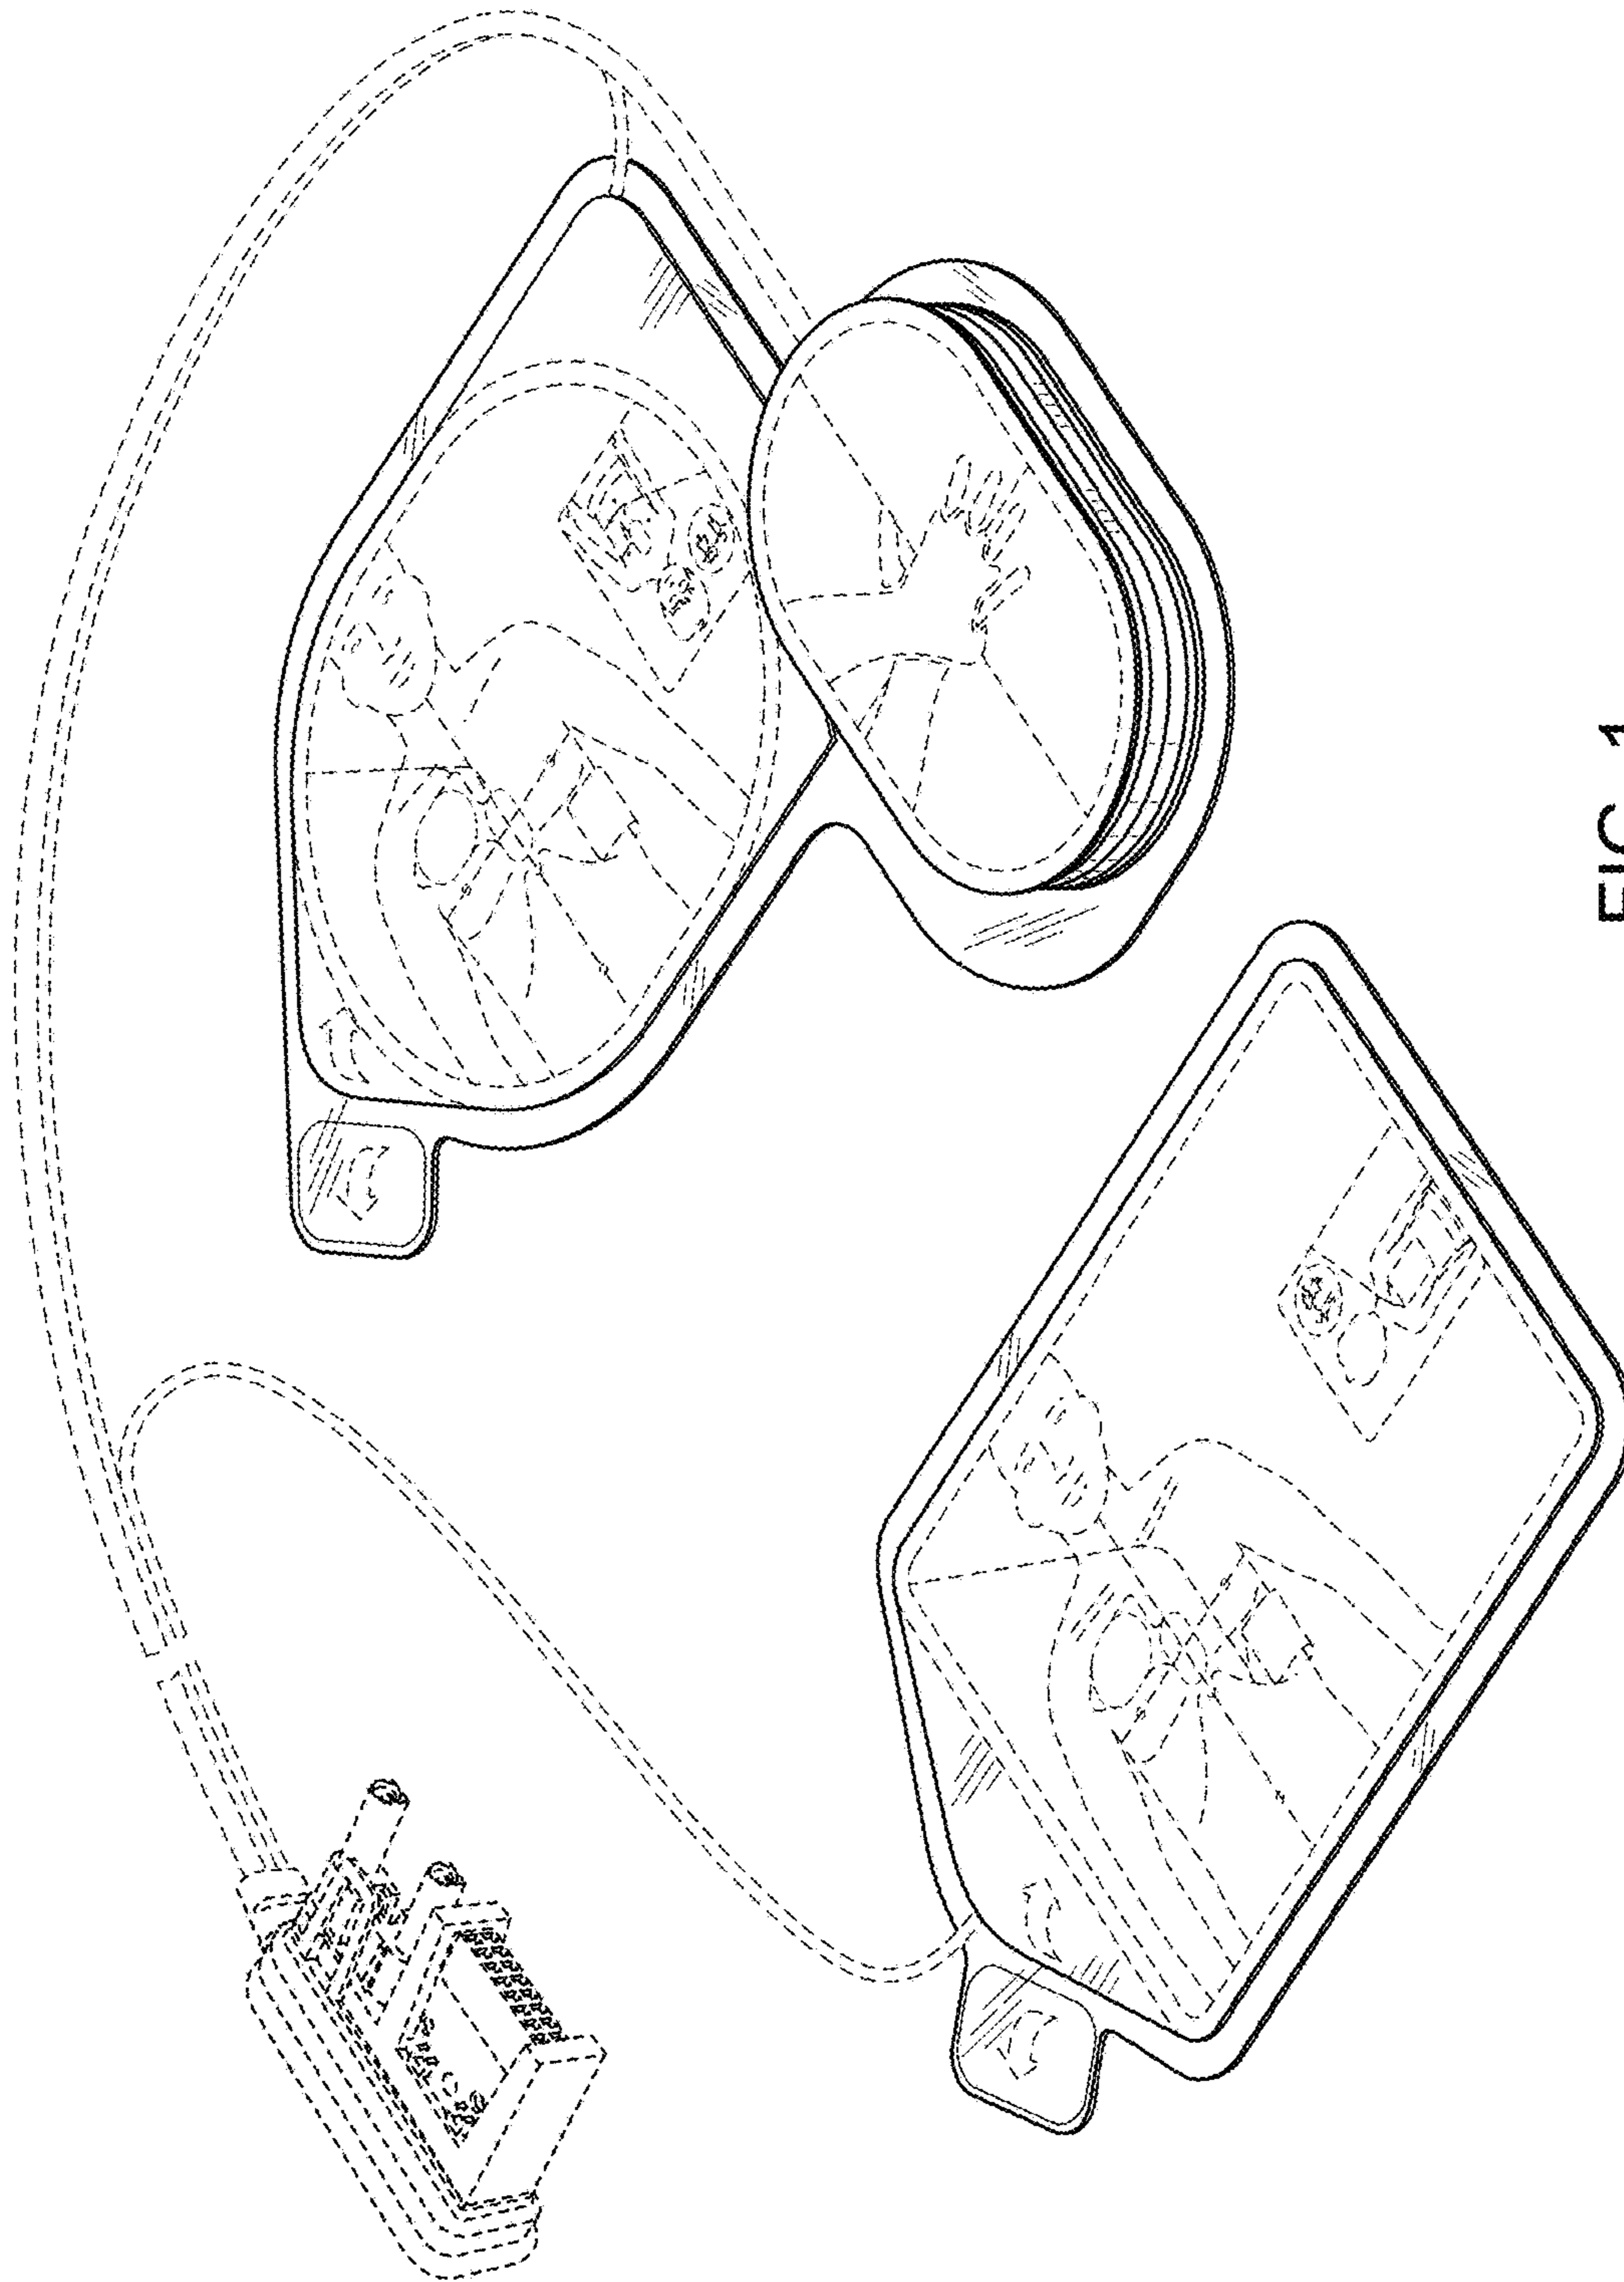


FIG. 1

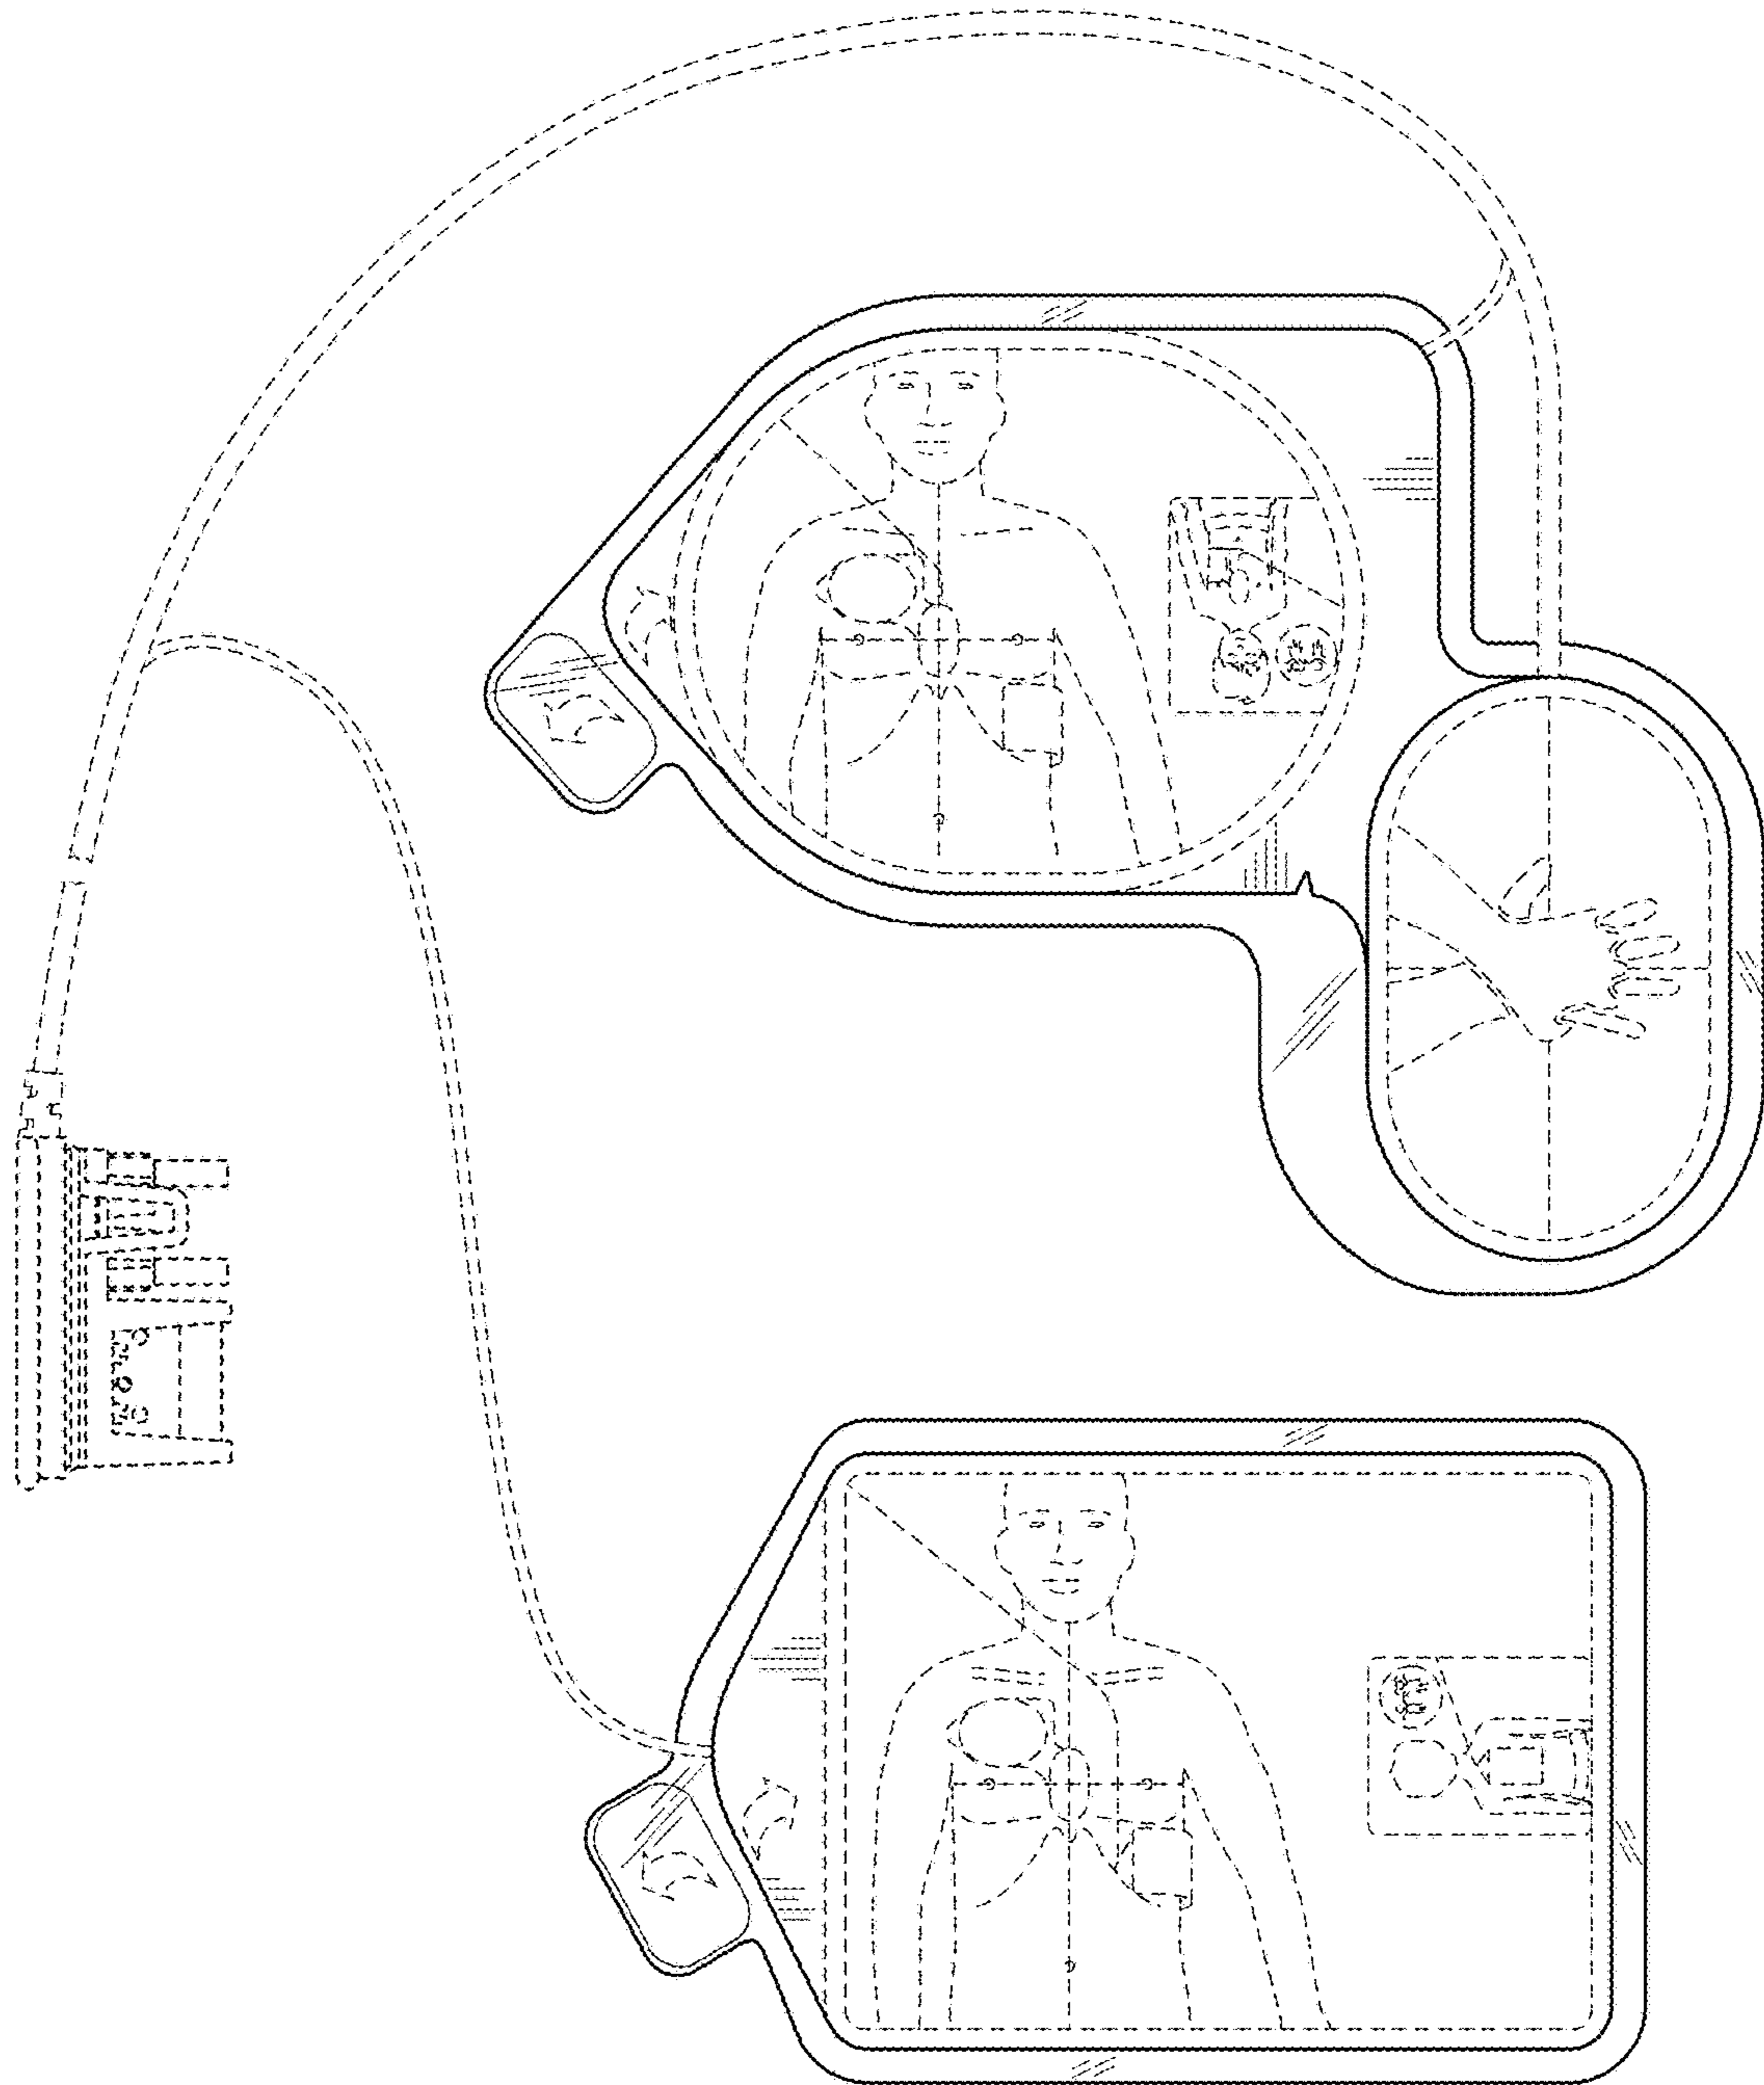


FIG. 2

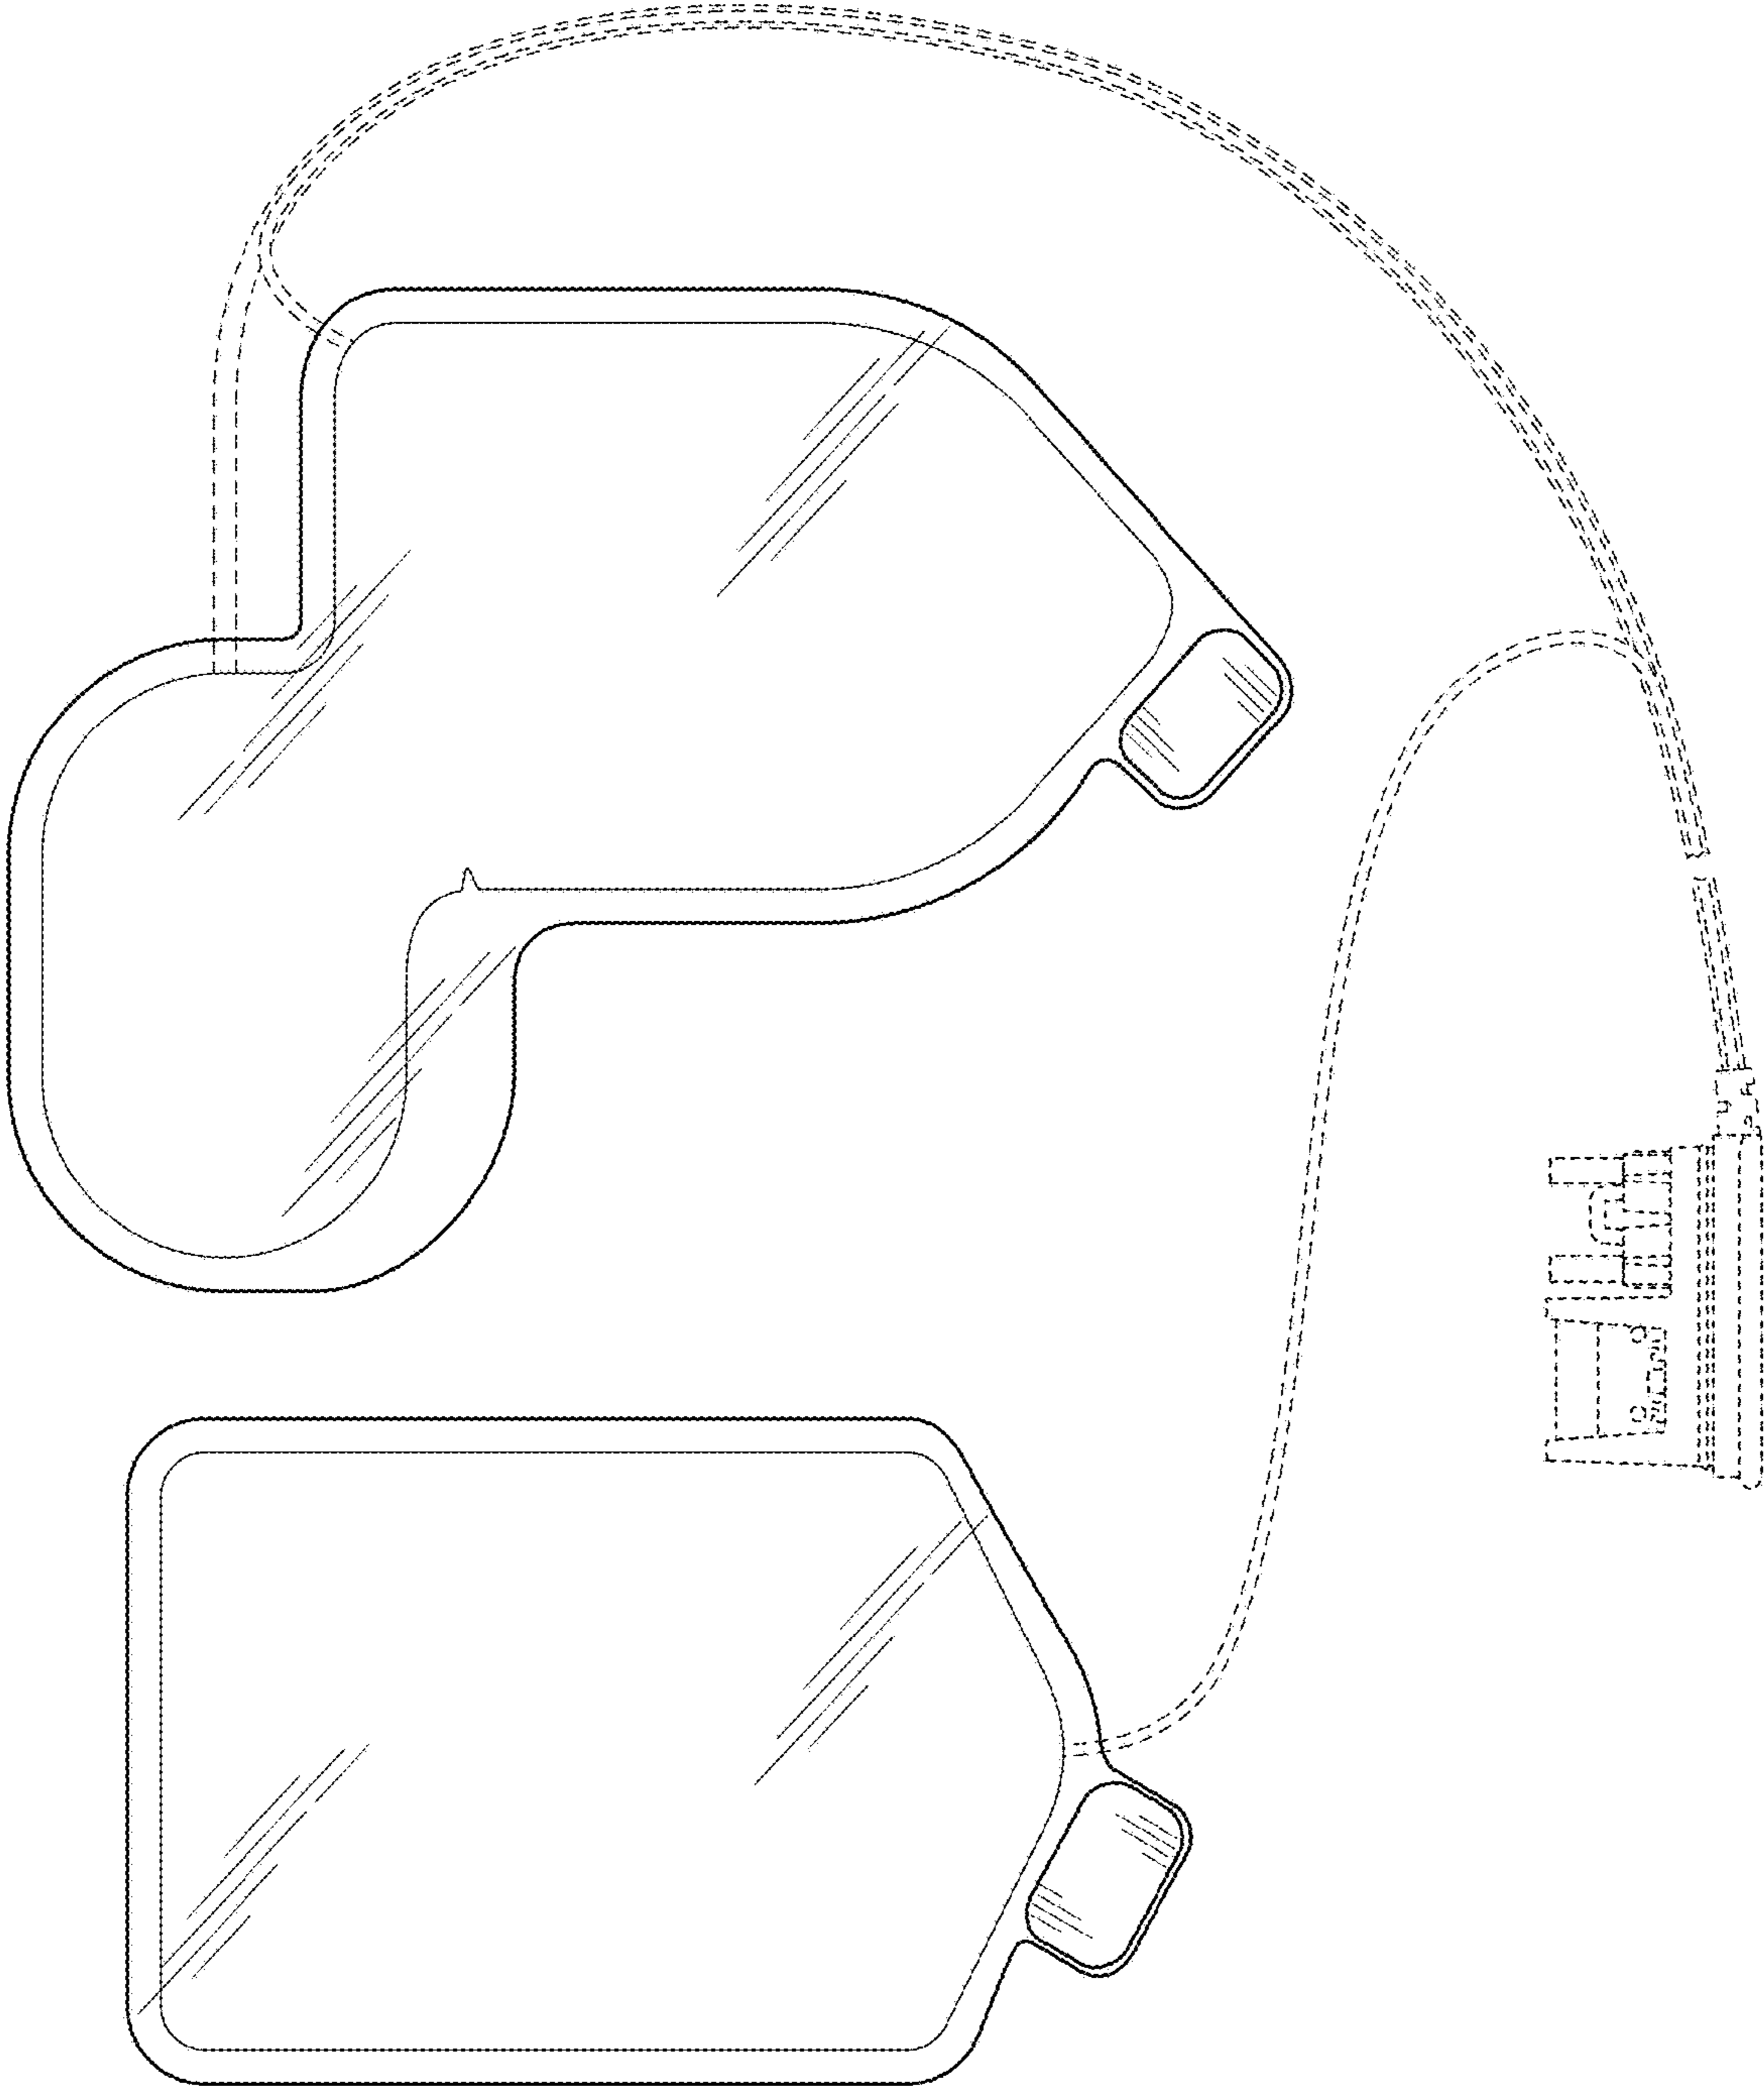


FIG. 3

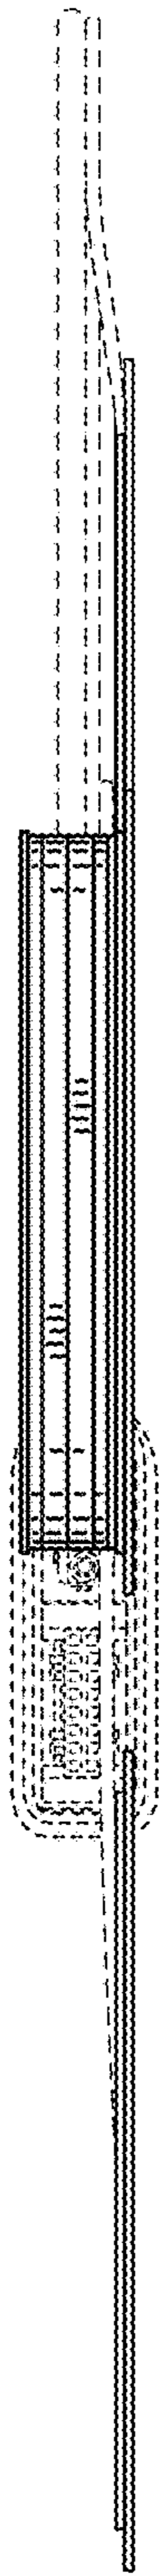


FIG. 4



FIG. 5

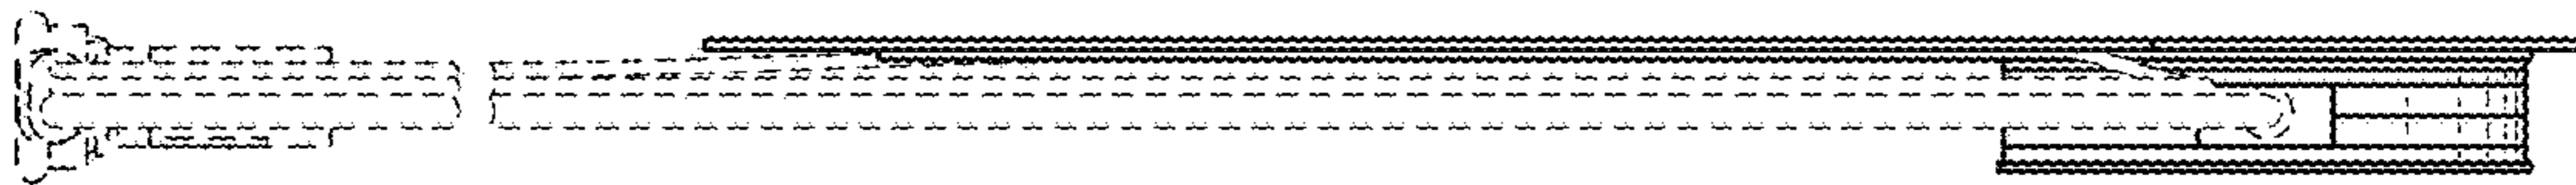


FIG. 6

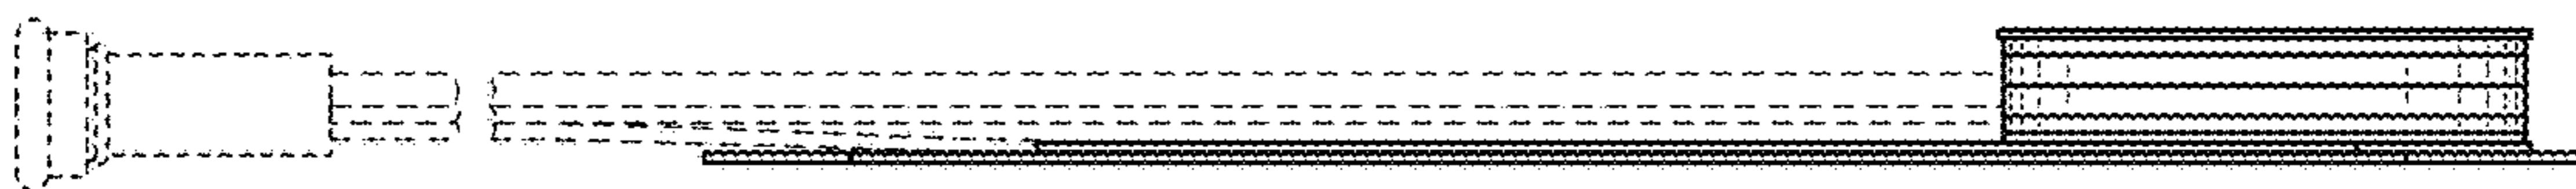


FIG. 7