



US00D784540S

(12) **United States Design Patent**
Boudville et al.

(10) **Patent No.:** **US D784,540 S**
(45) **Date of Patent:** **** Apr. 18, 2017**

(54) **FOOT PROFILING DEVICE**

D630,336 S * 1/2011 Park D24/213
D696,971 S * 1/2014 Ammon D10/70
D702,573 S * 4/2014 Schwartz D10/70

(71) Applicant: **Re-Align Performance Pty Ltd**,
Prestons, New South Wales (AU)

(Continued)

(72) Inventors: **Paul Boudville**, Prestons (AU); **Adrian Cursio**, Dandenong South (AU)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Re-Align Performance Pty Ltd** (AU)

EM 002955690-00 01 * 1/2016
WO WO 2005060782 A1 * 7/2005 A43D 1/025

(**) Term: **15 Years**

OTHER PUBLICATIONS

(21) Appl. No.: **29/552,563**

Foot Profiling Device, Go-tec® Software Foot Mapping System, posted at Sensorprod.com, posted on Jan. 12, 2012, site visited Oct. 28, 2016, <<http://www.sensorprod.com/pdf/go-tec-foot-plate.pdf>>.*

(22) Filed: **Jan. 22, 2016**

(Continued)

(30) **Foreign Application Priority Data**

Jul. 23, 2015 (AU) 201513682

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**

USPC **D24/186**

(58) **Field of Classification Search**

USPC D24/185–188, 160–161, 158, 200, 213
CPC . A63B 24/00; A47K 3/022; A61F 2/66; A61F 2002/6614; A61F 2002/6657; A61B 5/103; A61B 5/1074; A61B 5/0064; A61B 5/1036; A61B 5/107; A43D 1/00; A43D 1/02; A43D 1/022; A43D 1/025; A43D 1/027; G01B 11/02; G01B 7/02; G06F 3/041; G06F 3/04842

See application file for complete search history.

Primary Examiner — Barbara Fox

Assistant Examiner — Messina L Smith

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57)

CLAIM

The ornamental design for a foot profiling device, as shown and described.

DESCRIPTION

FIG. 1 is a top, back and right side perspective view of a foot profiling device embodying our new design;

FIG. 2 is a top, back and left side perspective view thereof;

FIG. 3 is a top, front and right side perspective view thereof;

FIG. 4 is a top view thereof;

FIG. 5 is a left side view thereof, the right side being a mirror image; and,

FIG. 6 is a bottom view thereof.


Broken lines are used to illustrate features of the foot profiling device which form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,332,292 A * 10/1943 Bliss A43D 1/02 33/3 A
D478,670 S * 8/2003 Tsai D24/212
D601,254 S * 9/2009 Weichert D24/161

1 Claim, 6 Drawing Sheets

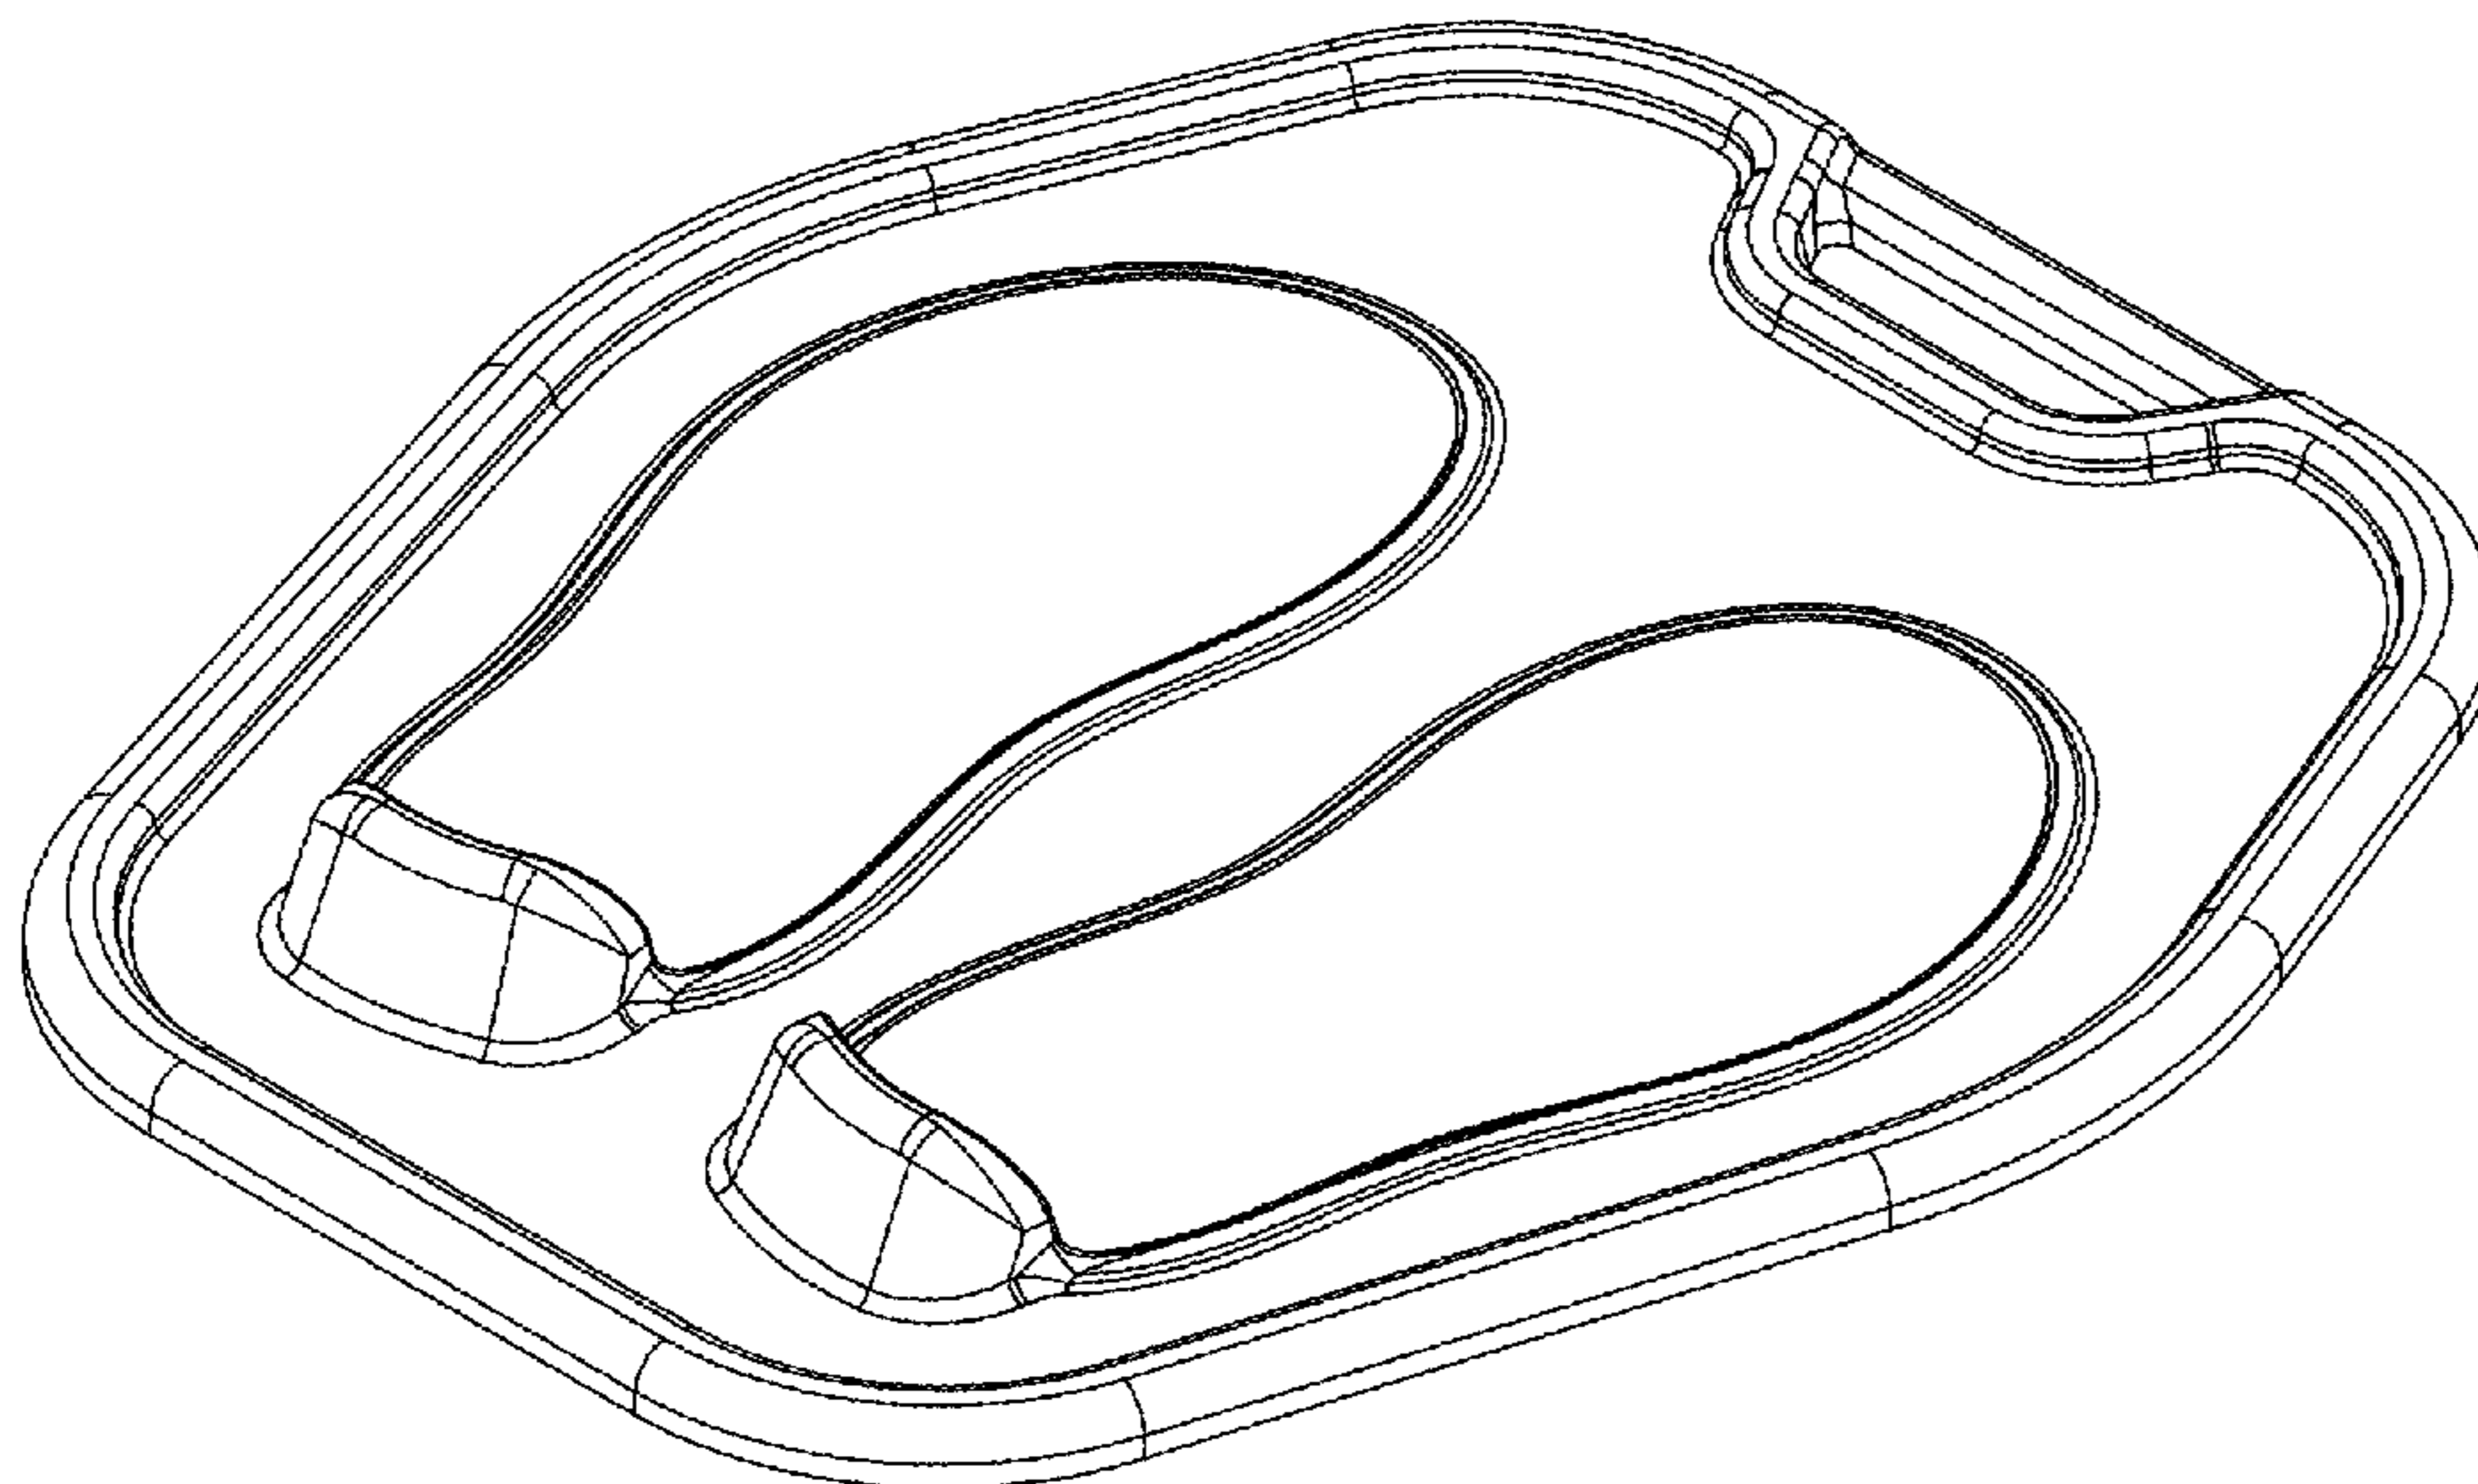

(56)

References Cited

U.S. PATENT DOCUMENTS

D712,287 S * 9/2014 Michaelian D10/70
D713,969 S * 9/2014 Robinson D24/200
D746,482 S * 12/2015 Ho D24/213
D751,715 S * 3/2016 Bostley D24/161
D754,358 S * 4/2016 Krullaards D24/188
2014/0152450 A1* 6/2014 Hjort A63B 23/0458
340/665
2014/0309534 A1* 10/2014 Pichler A61B 5/1036
600/476
2016/0015298 A1* 1/2016 Danenberg A61B 5/1079
600/476

OTHER PUBLICATIONS

Foot Profiling Device, iStep Foot Scanner Demonstration by Sonoma Boot Company, posted at Youtube.com, posted on Jun. 15, 2015, site visited Oct. 28, 2016, <<https://www.youtube.com/watch?v=QWJdMf6M0YM>>.*

Foot Measuring, Foot analysis with FOOTDISC thermo scan, posted at Youtube.com, posted on Oct. 25, 2010, site visited Oct. 28, 2016, <https://www.youtube.com/watch?v=Tt3eooe27_I>.*

Orthotic Device, Pedicure Machine Electric, posted at Aliexpress.com, no posting date given, © 2010-2016, site visited Oct. 28, 2016, <<https://www.aliexpress.com/item/Pedicure-Machine-Electric-Far-infrared-foot-massage-apparatus-Vibration-magnetic-wave-heat-ing-foot-physiotherapy-instrument/32742198348.html?spm=2114.40010308.4.17.ptwzlw>>.*

* cited by examiner

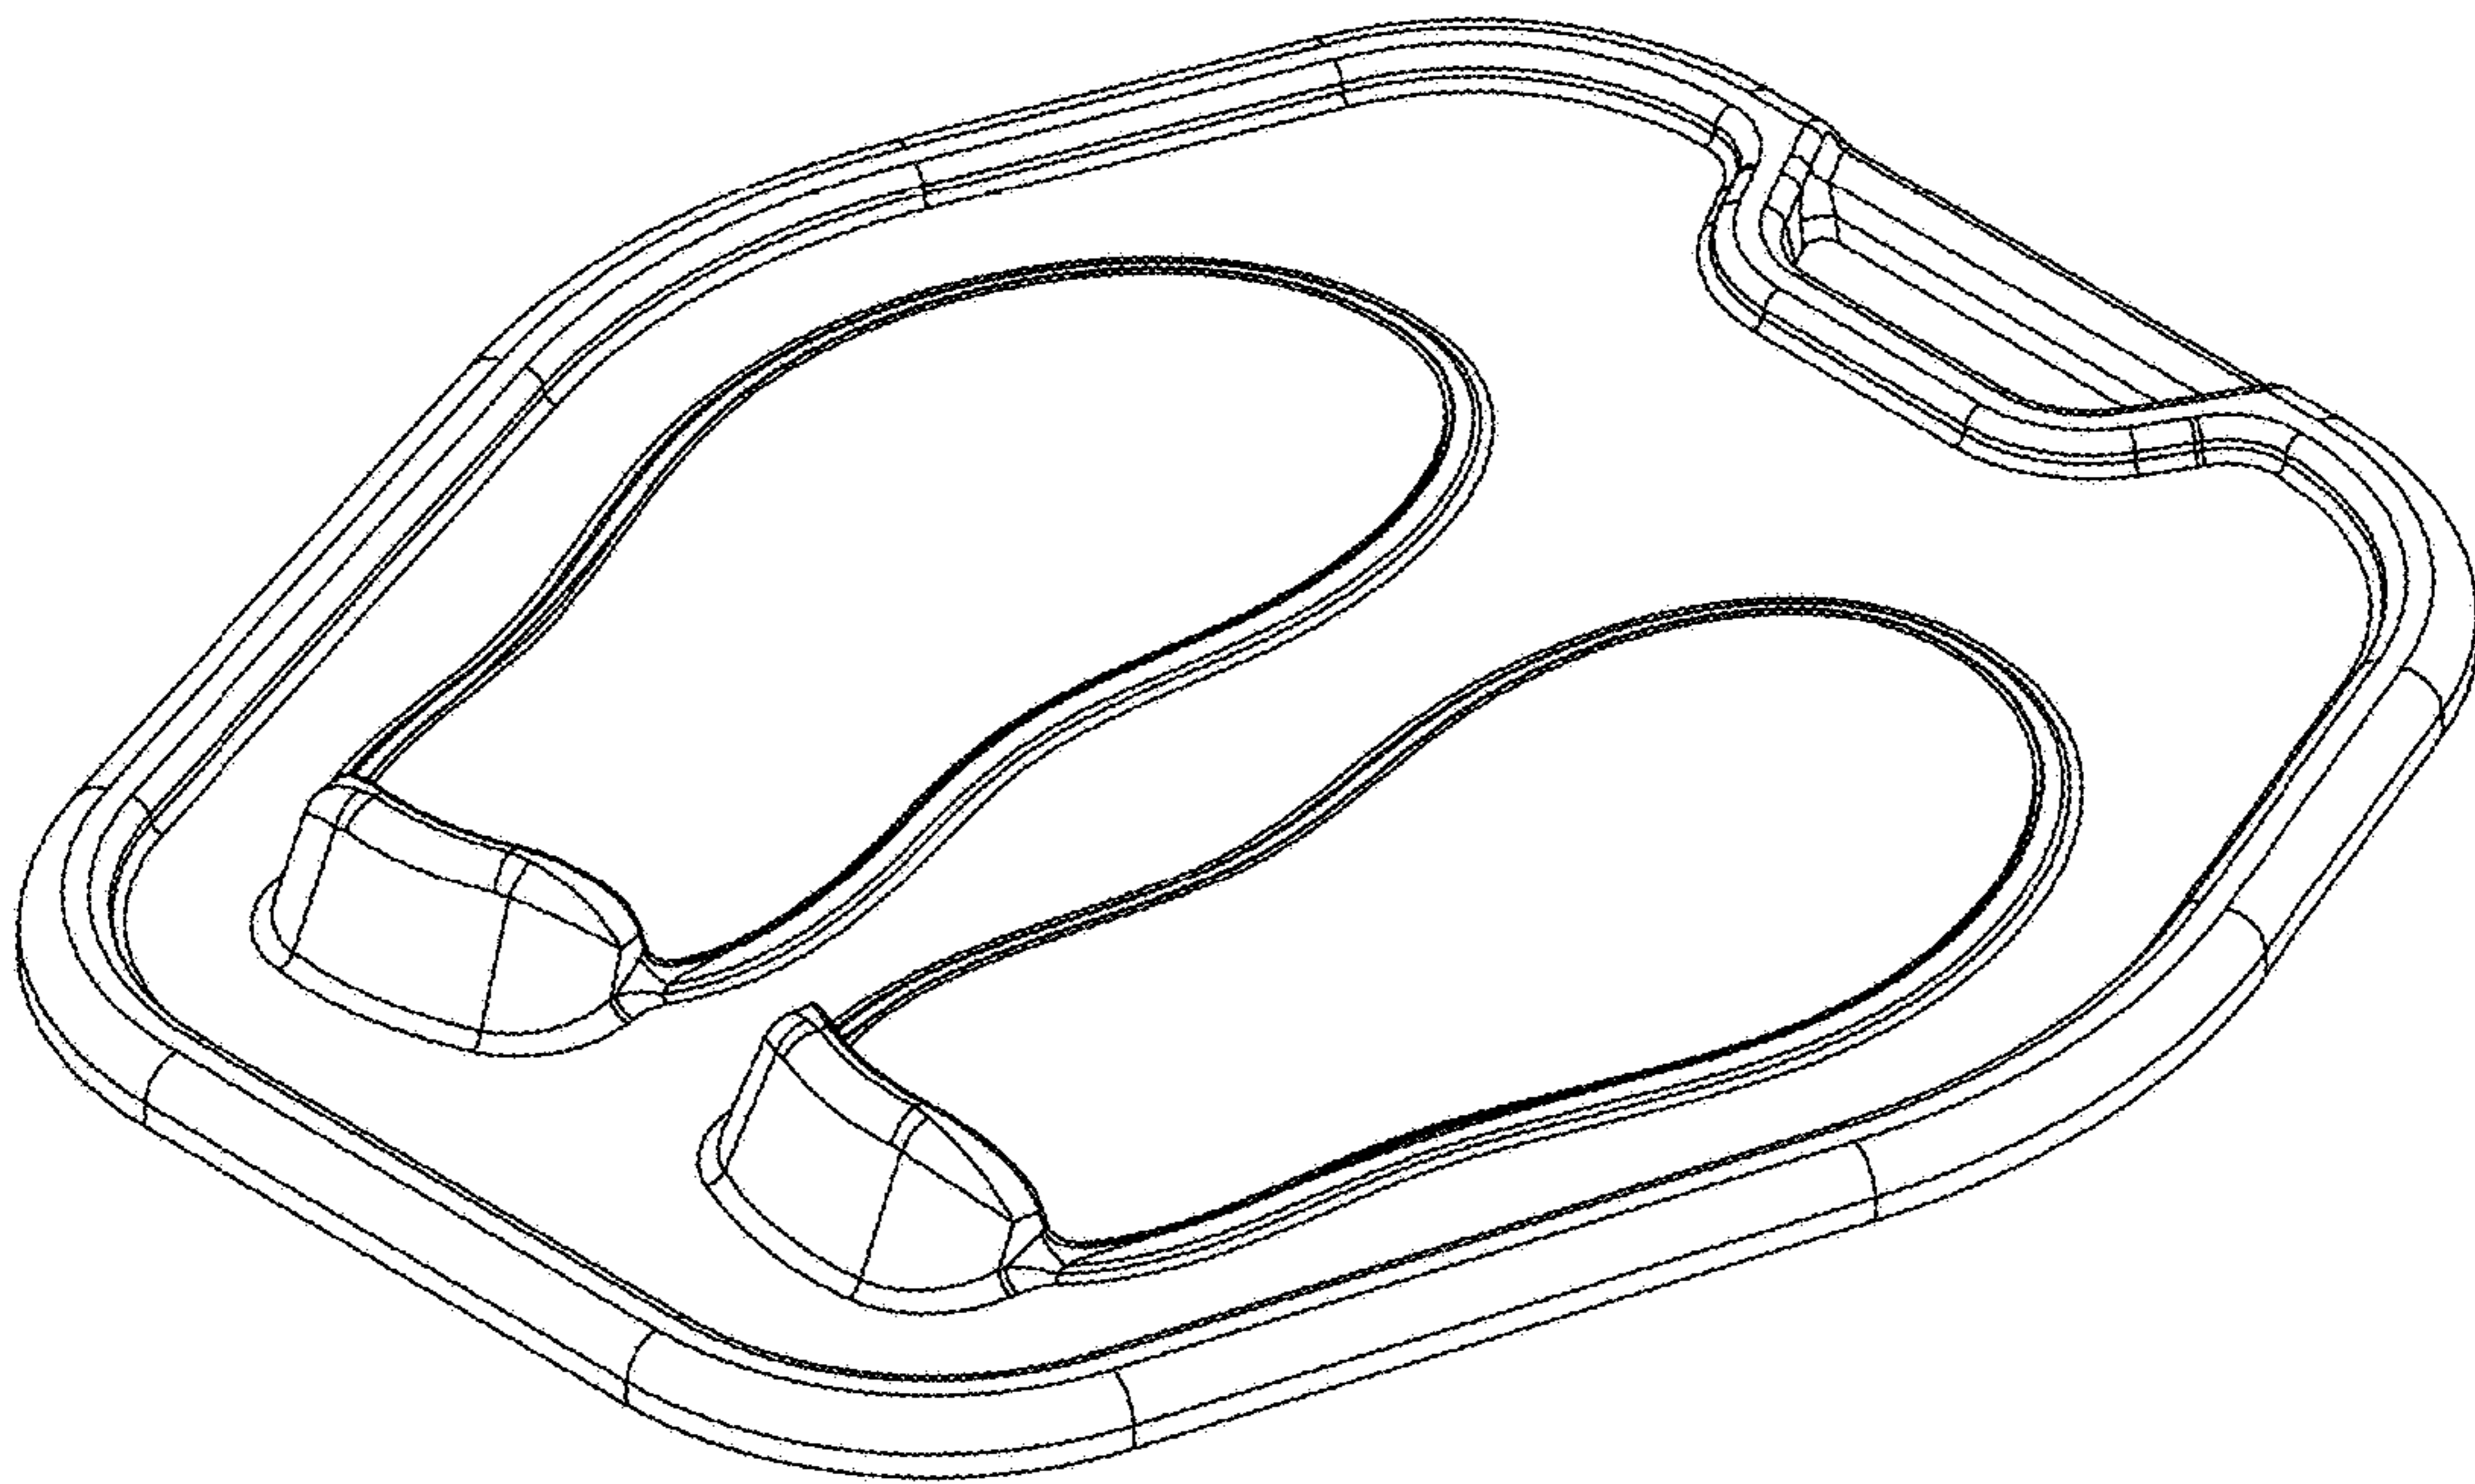


FIG. 1

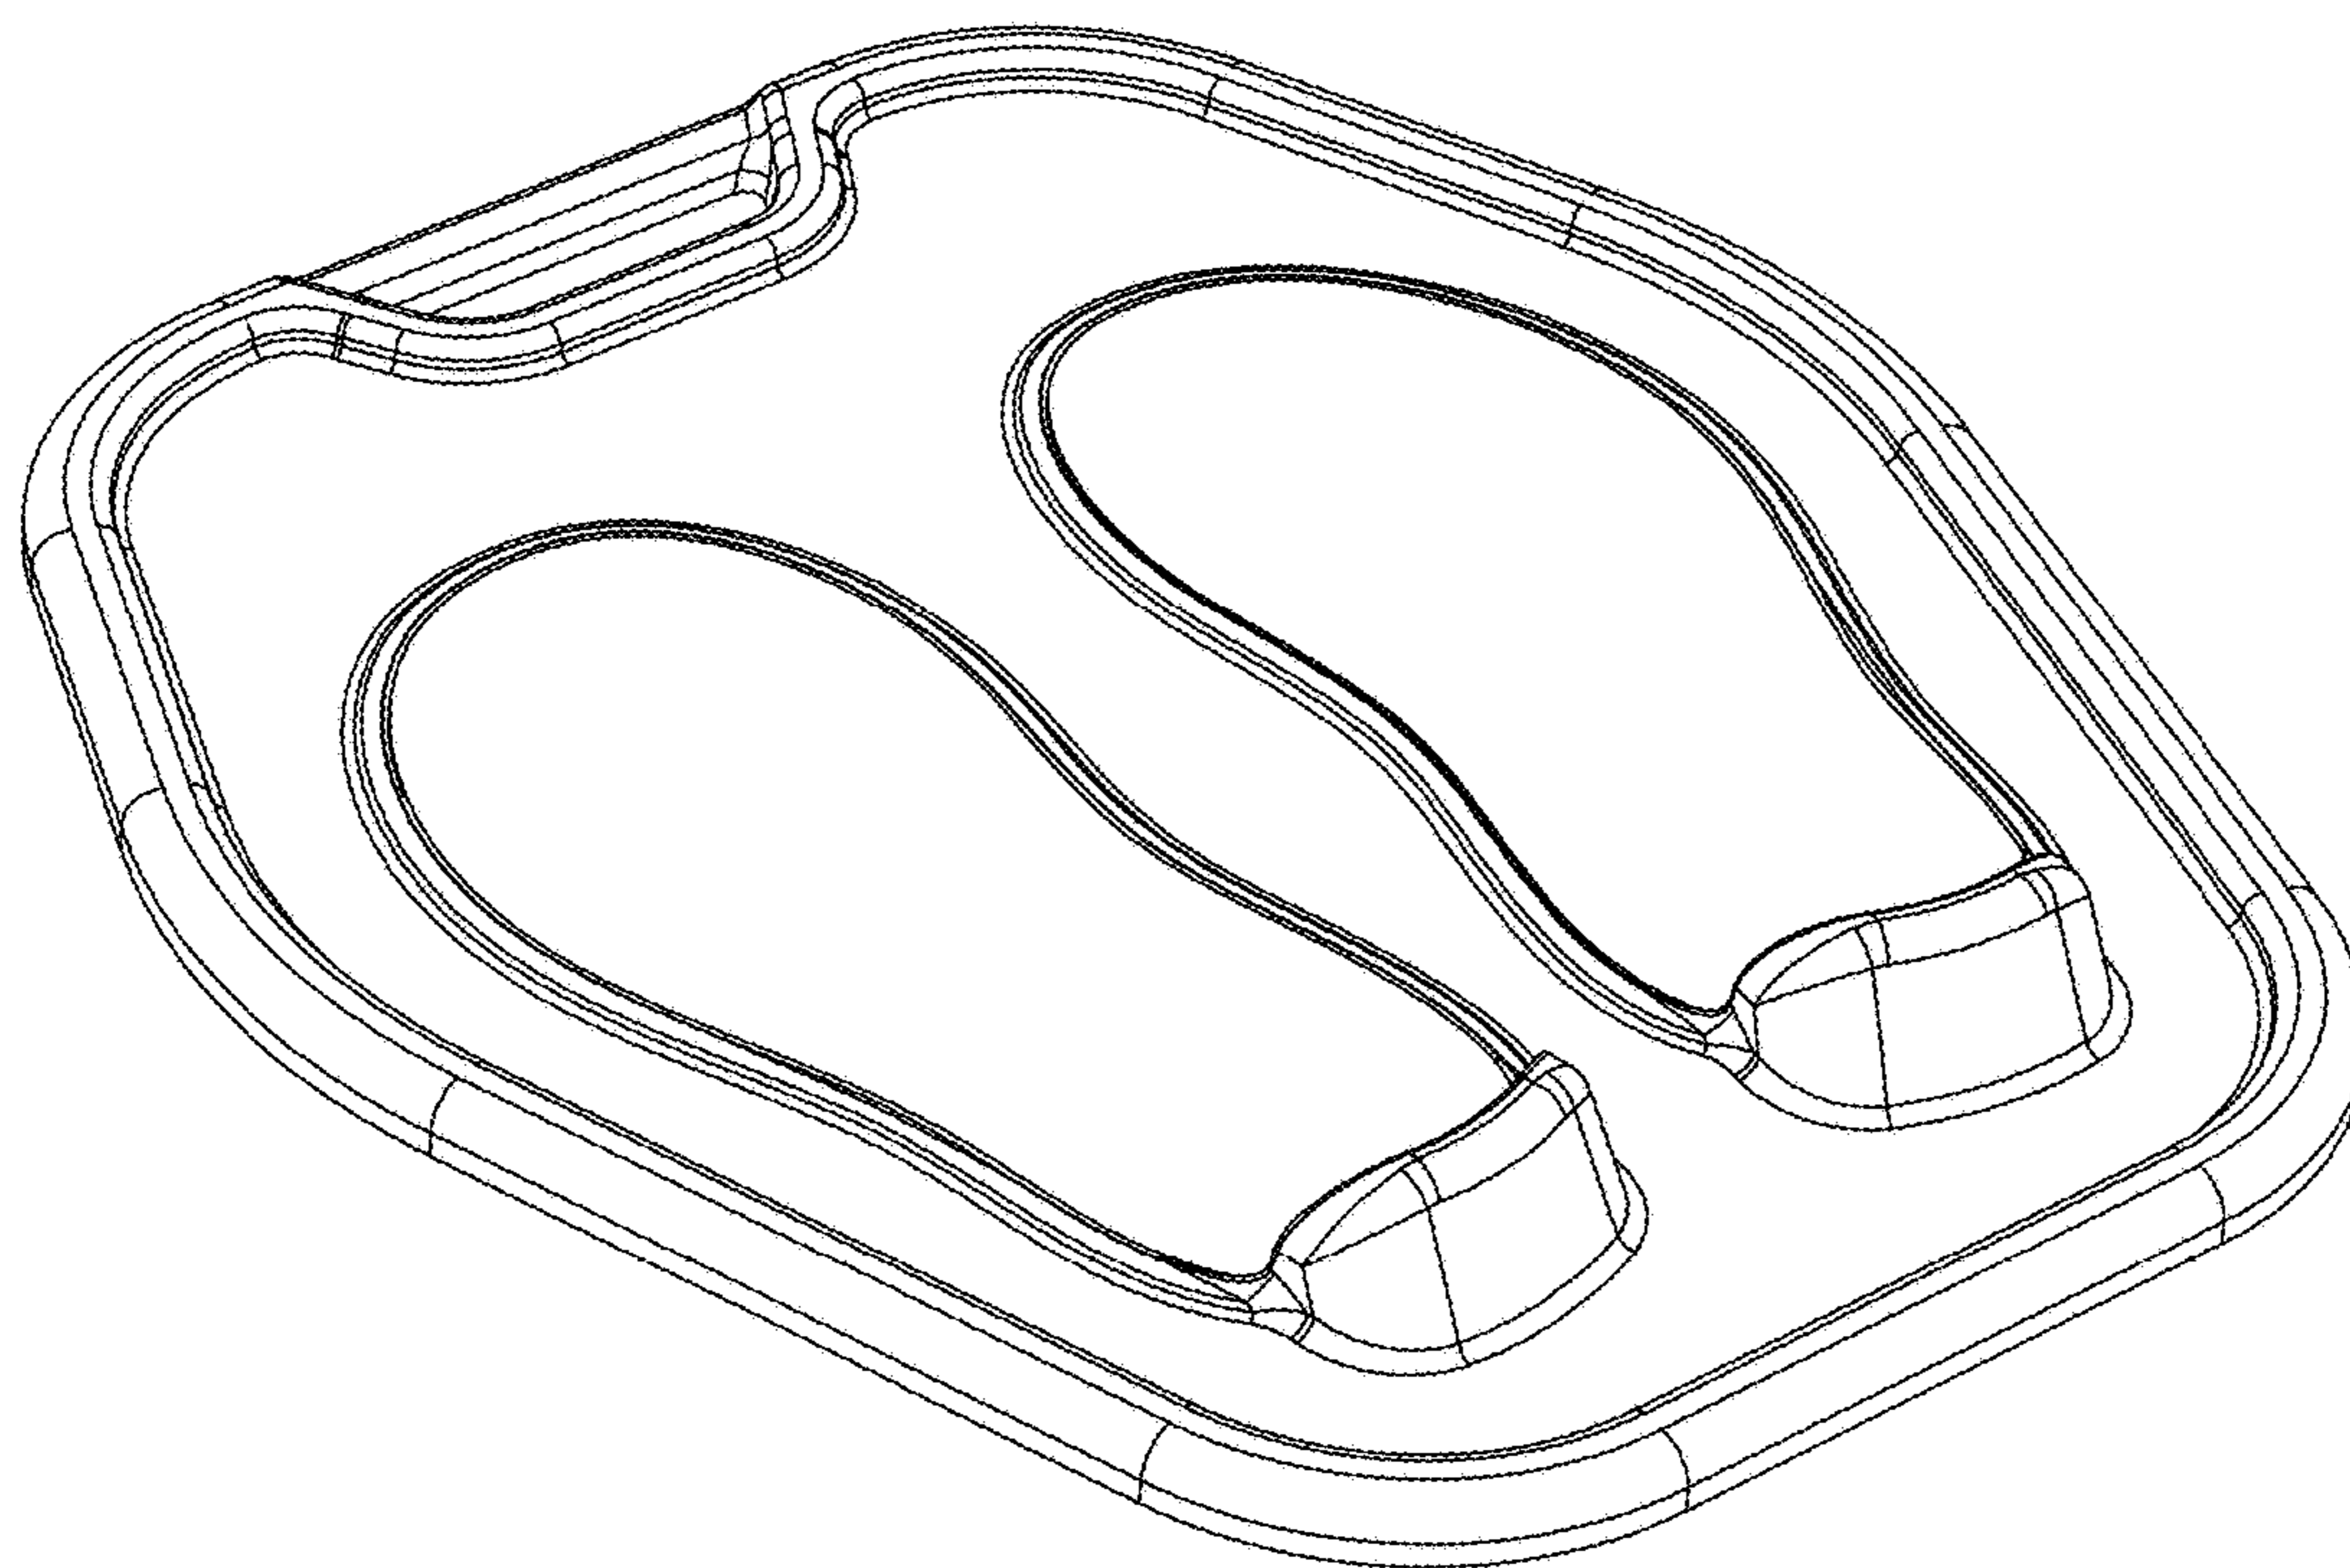


FIG. 2

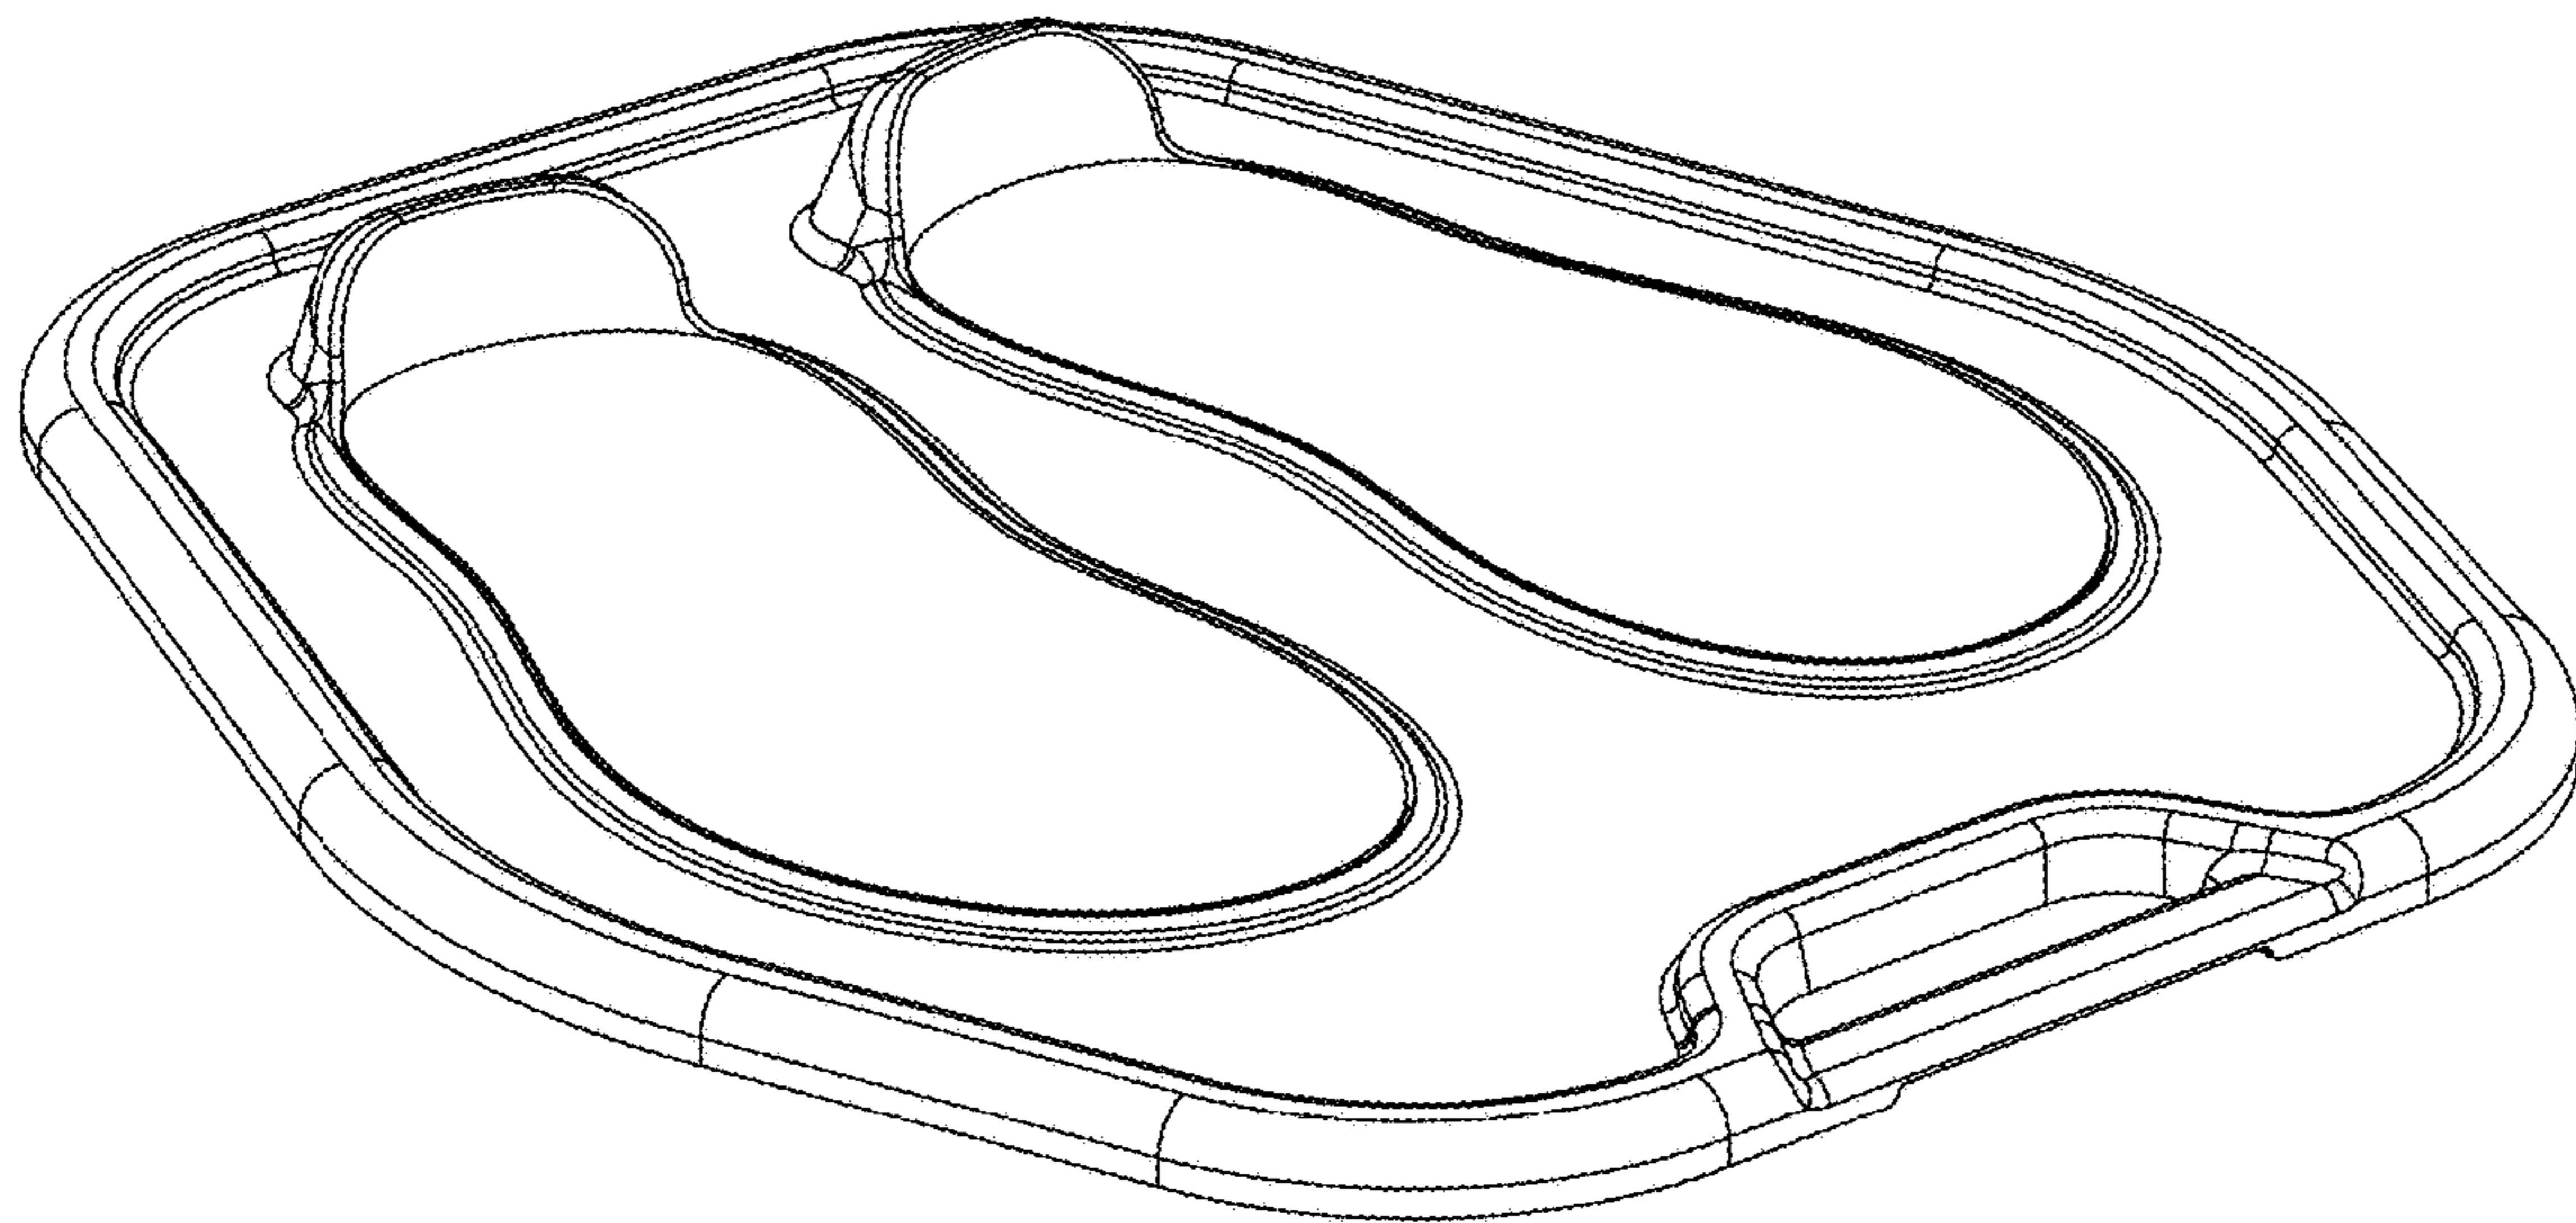


FIG. 3

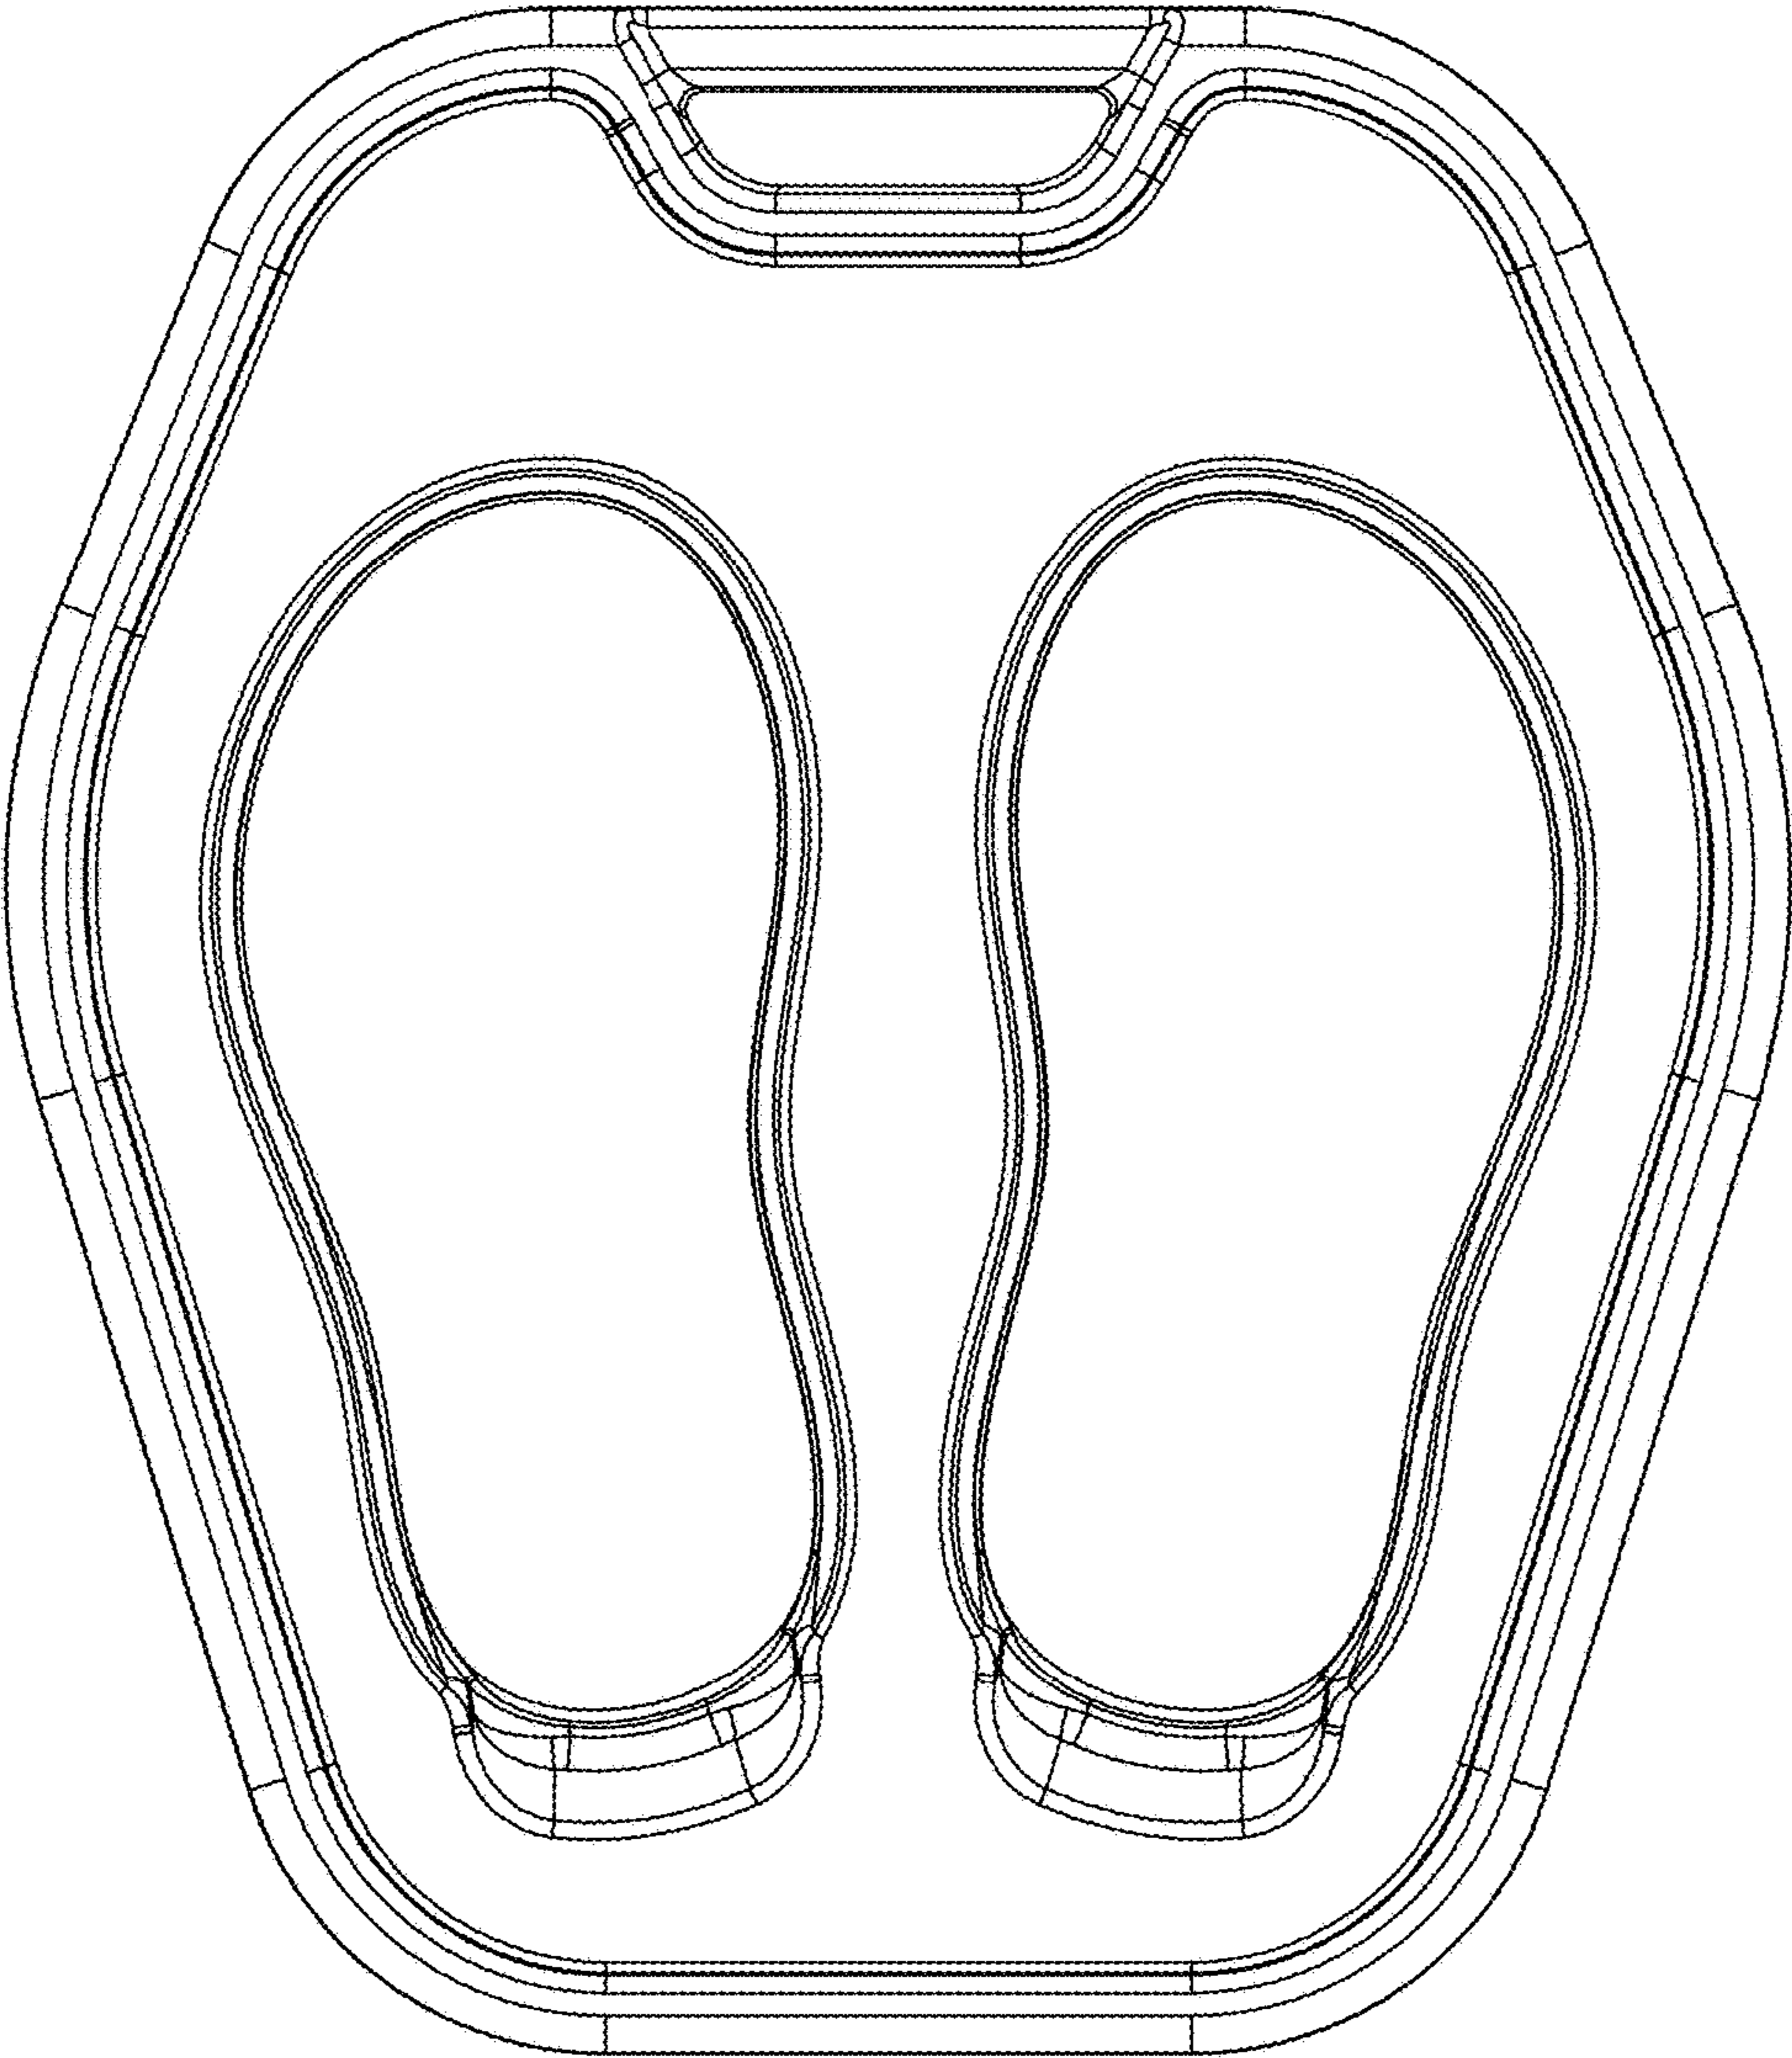


FIG. 4

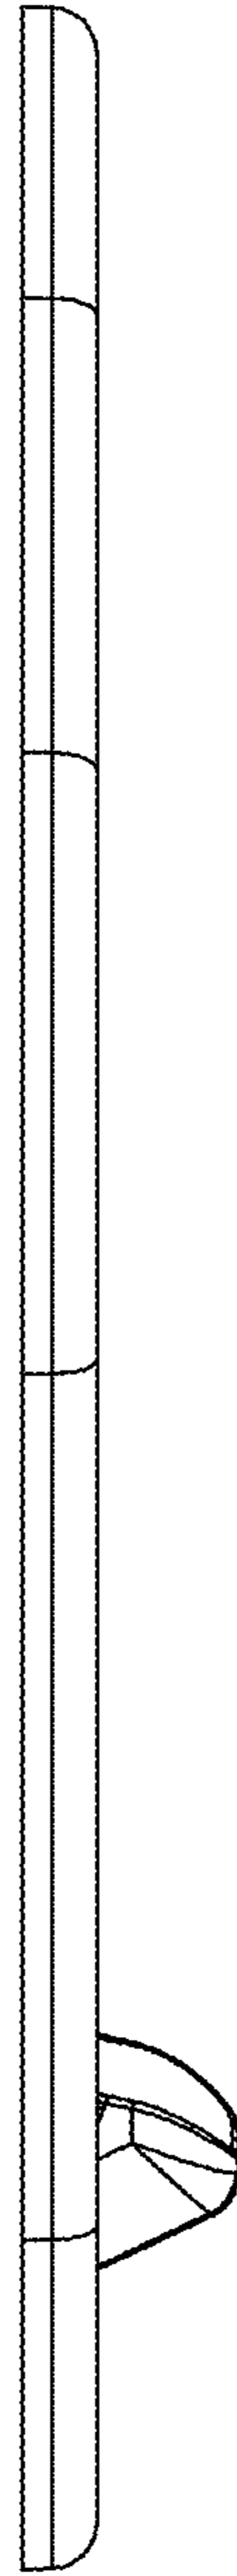


FIG. 5

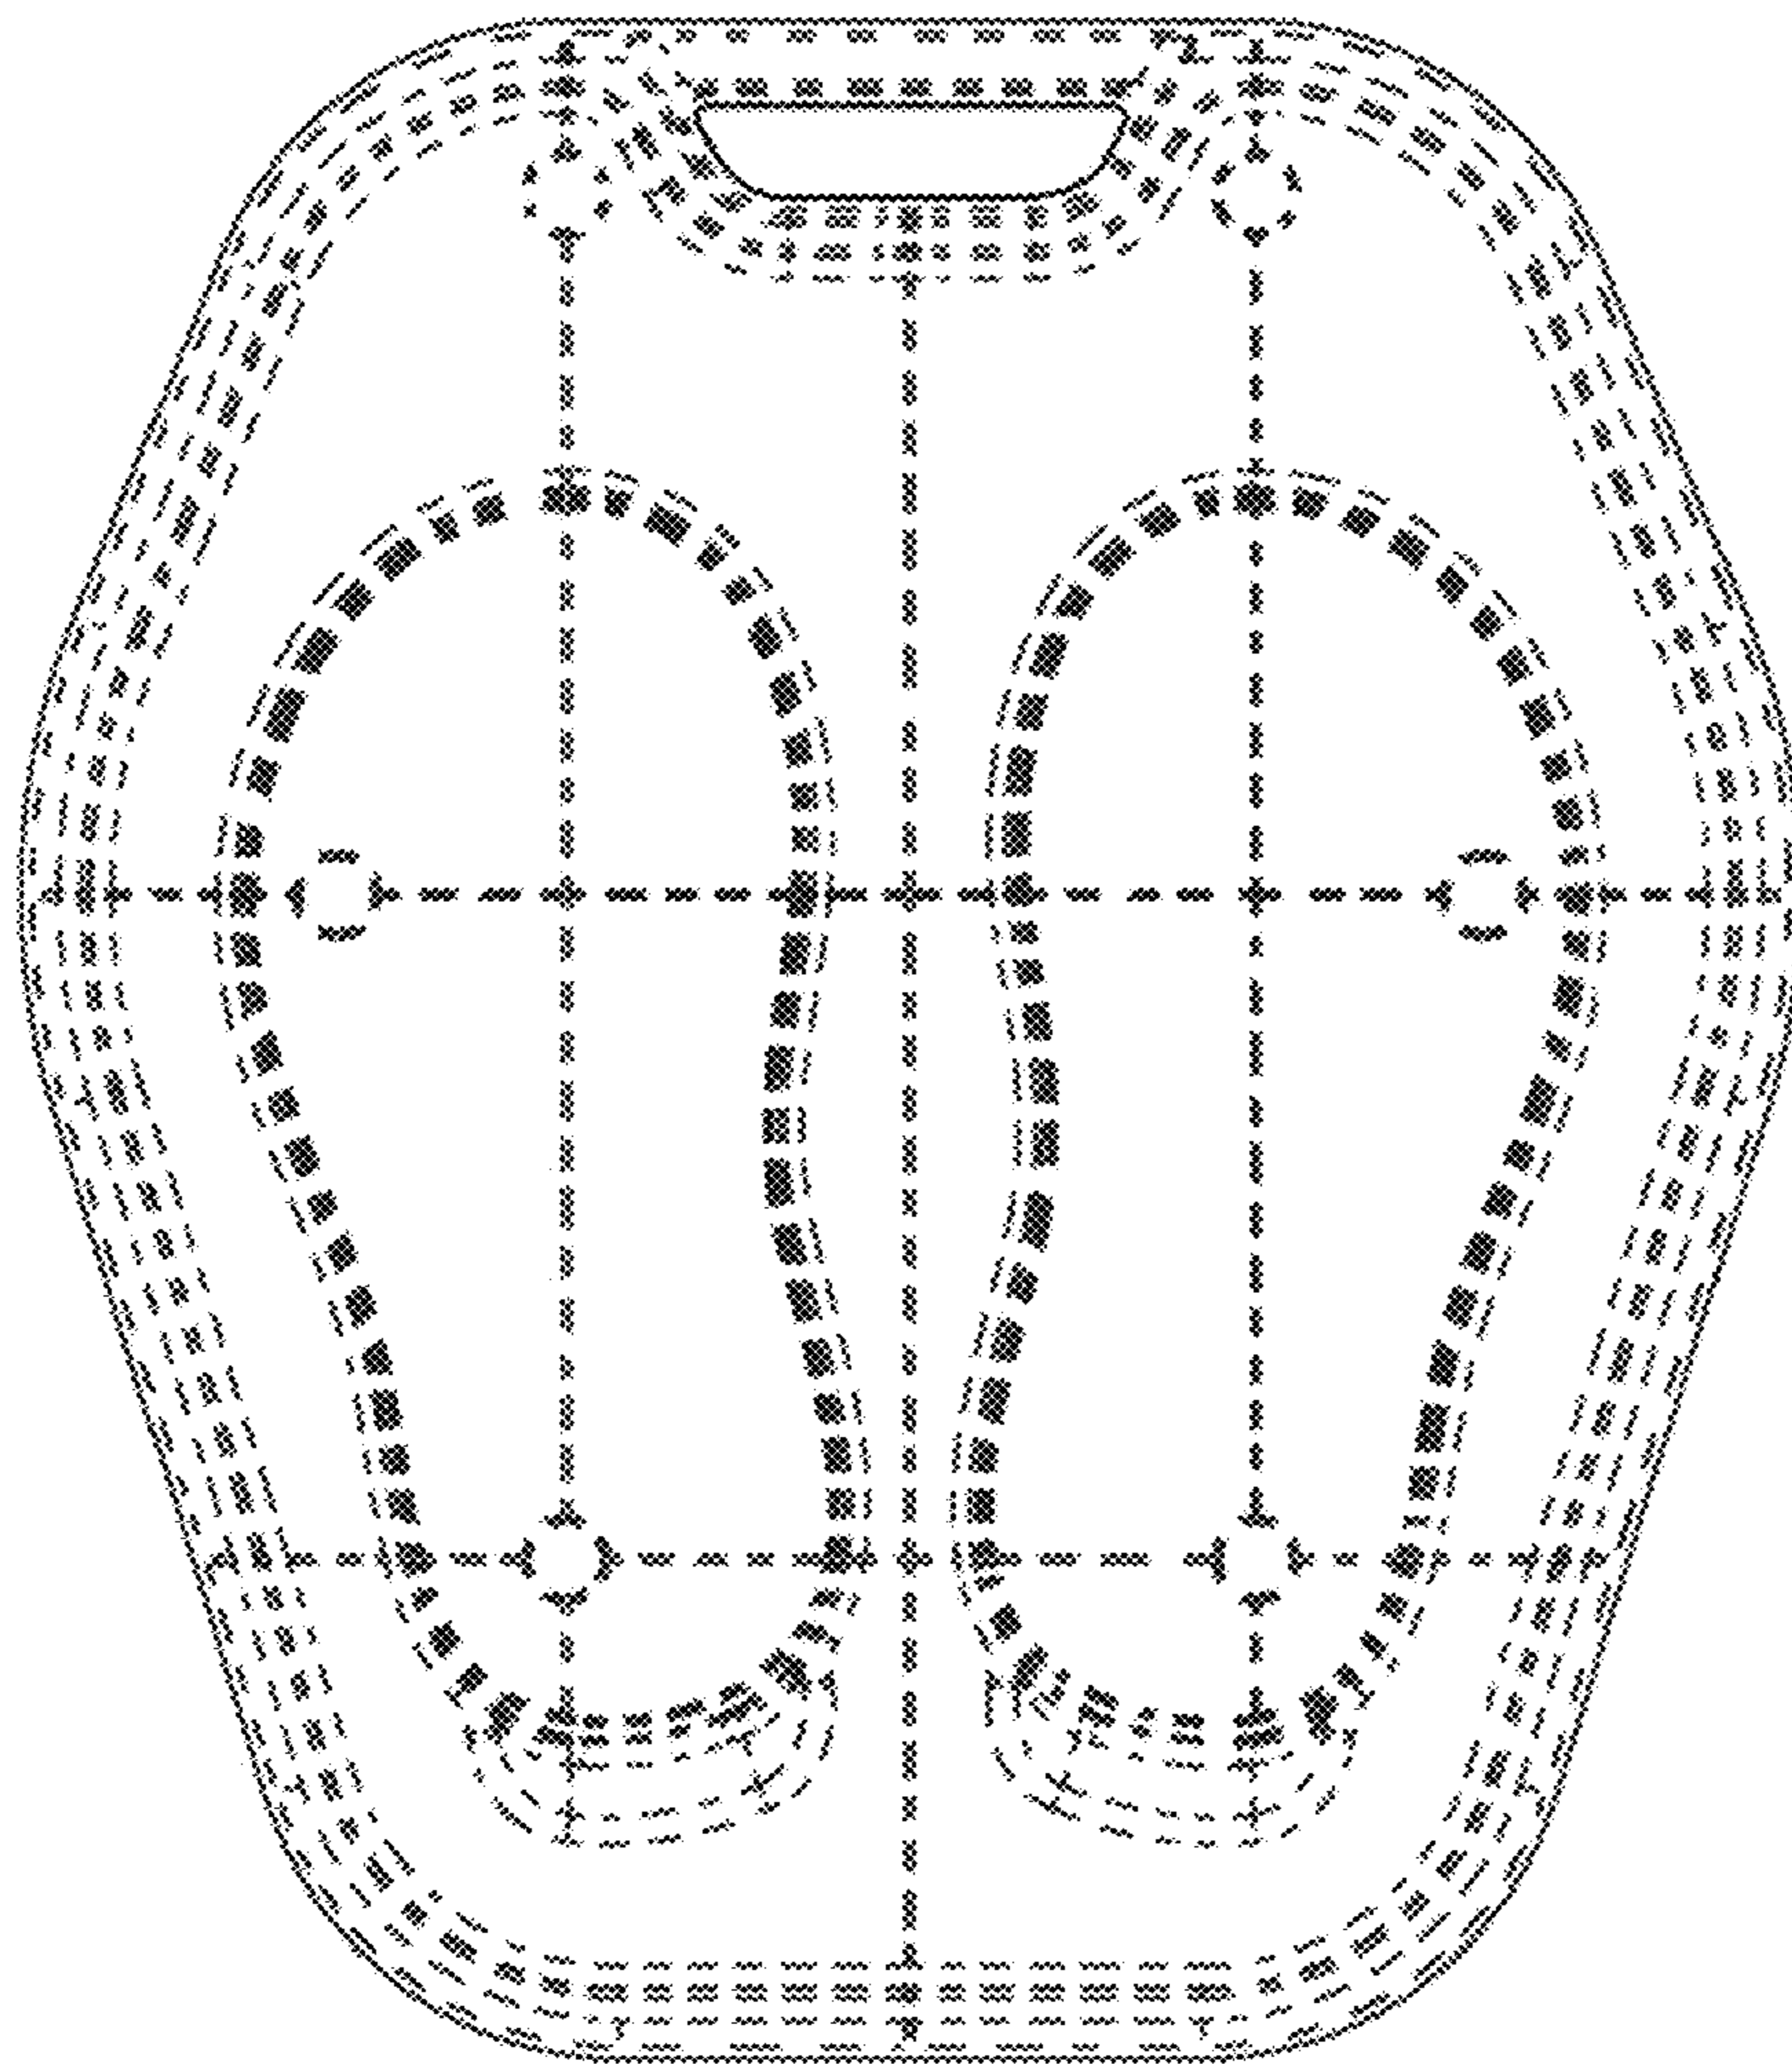


FIG. 6