



US00D785185S

(12) **United States Design Patent**  
**Yang et al.**

(10) **Patent No.:** **US D785,185 S**  
(45) **Date of Patent:** **\*\* Apr. 25, 2017**

(54) **PHYSIOLOGICAL SIGNAL DETECTOR**

(71) Applicant: **APODX TECHNOLOGY, INC.**,  
Taipei (TW)

(72) Inventors: **Tzu-Chieh Yang**, Taipei (TW);  
**Jyh-Ren Ho**, Taipei (TW)

(73) Assignee: **Apodx Technology, Inc.**, Taipei (TW)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/517,080**

(22) Filed: **Feb. 10, 2015**

(30) **Foreign Application Priority Data**

Nov. 14, 2014 (TW) ..... 103306667

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

(58) **Field of Classification Search**  
USPC ..... D24/184, 185, 186, 187, 188, 164-168;  
600/595; D10/70, 71, 75, 78, 80, 94, 129  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D348,618 S \* 7/1994 Leslie ..... D10/64
- D377,832 S \* 2/1997 Jacober ..... D24/186
- 6,468,231 B2 \* 10/2002 Sarvazyan ..... A61B 5/061  
600/587
- 6,595,933 B2 \* 7/2003 Sarvazyan ..... A61B 5/061  
600/587
- D633,814 S \* 3/2011 Nishiyama ..... D10/81
- D712,541 S \* 9/2014 Brigham ..... D24/167
- D760,903 S \* 7/2016 Lin ..... D24/165

- 2004/0267165 A1\* 12/2004 Sarvazyan ..... A61B 5/0002  
600/587
- 2007/0251531 A1\* 11/2007 Khouri ..... A61B 19/24  
128/898
- 2011/0237924 A1\* 9/2011 McGusty ..... A61B 5/0006  
600/391
- 2013/0165768 A1\* 6/2013 Biber ..... G01R 33/3642  
600/422
- 2015/0089824 A1\* 4/2015 Moore ..... A41H 1/02  
33/512

\* cited by examiner

*Primary Examiner* — Ian Simmons

*Assistant Examiner* — Samantha Q Lawrence

(74) *Attorney, Agent, or Firm* — Rosenberg, Klein & Lee


(57) **CLAIM**

The ornamental design for a physiological signal detector, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a physiological signal detector of the new design;  
 FIG. 2 is a front elevation view thereof;  
 FIG. 3 is a rear elevation view thereof;  
 FIG. 4 is a left side view thereof;  
 FIG. 5 is a right side view thereof;  
 FIG. 6 is a top plan view thereof;  
 FIG. 7 is a bottom plan view thereof; and,  
 FIG. 8 is a front elevation view thereof in an environment of use.  
 The additional broken lines shown in FIG. 8 illustrate environment and form no part of the claimed design.  
 The broken lines shown in FIGS. 1-8 illustrate portions of the physiological signal detector that form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

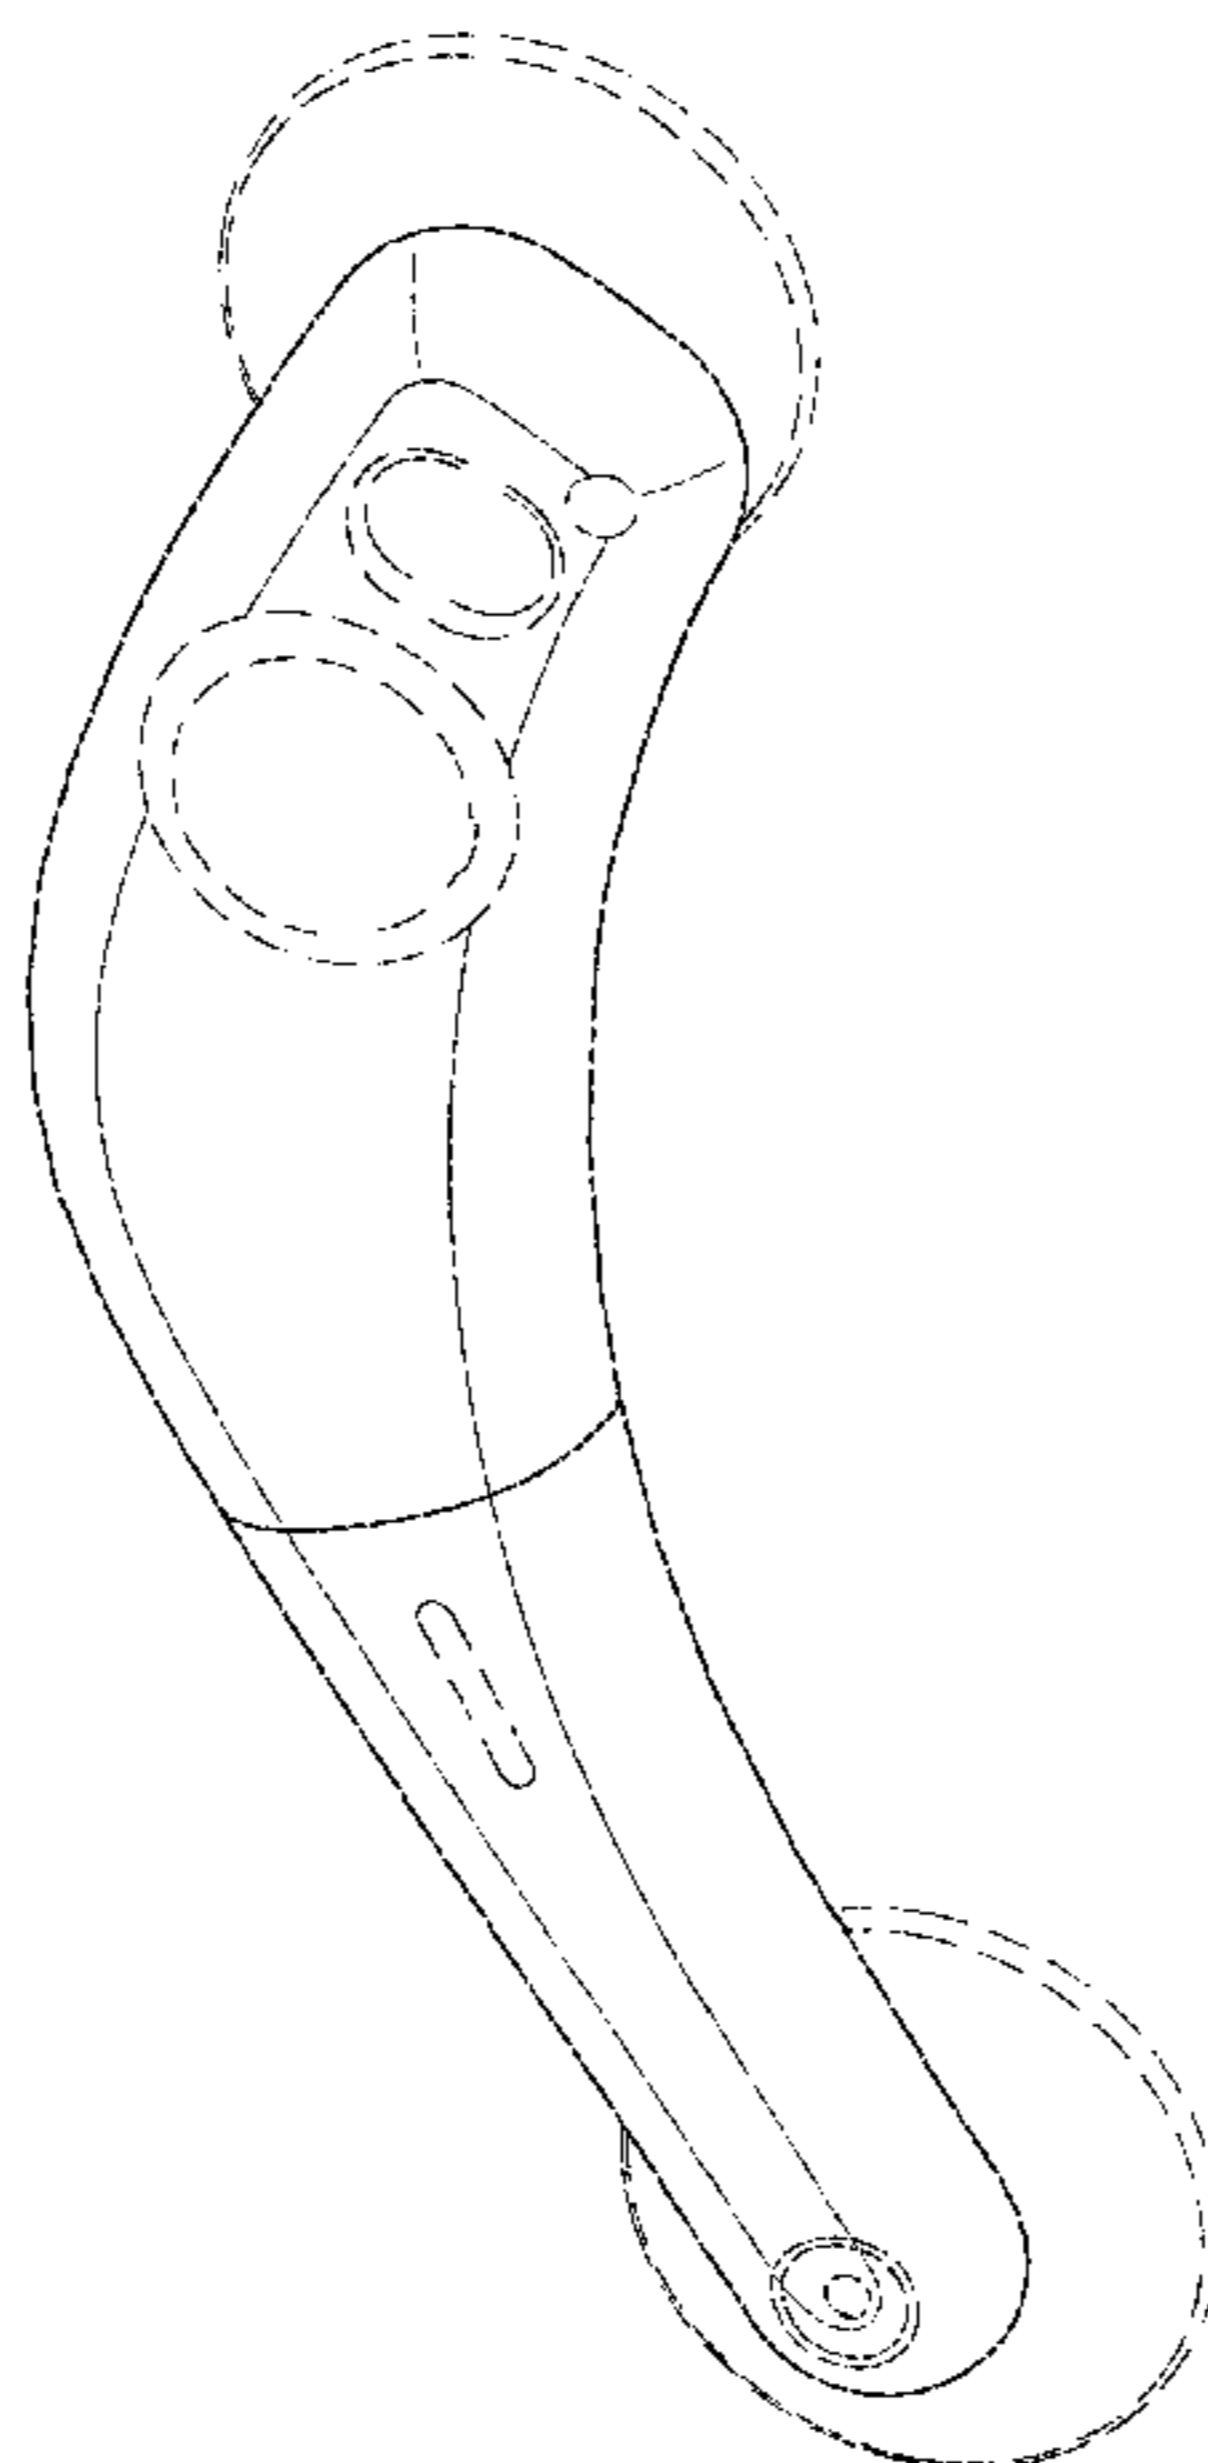

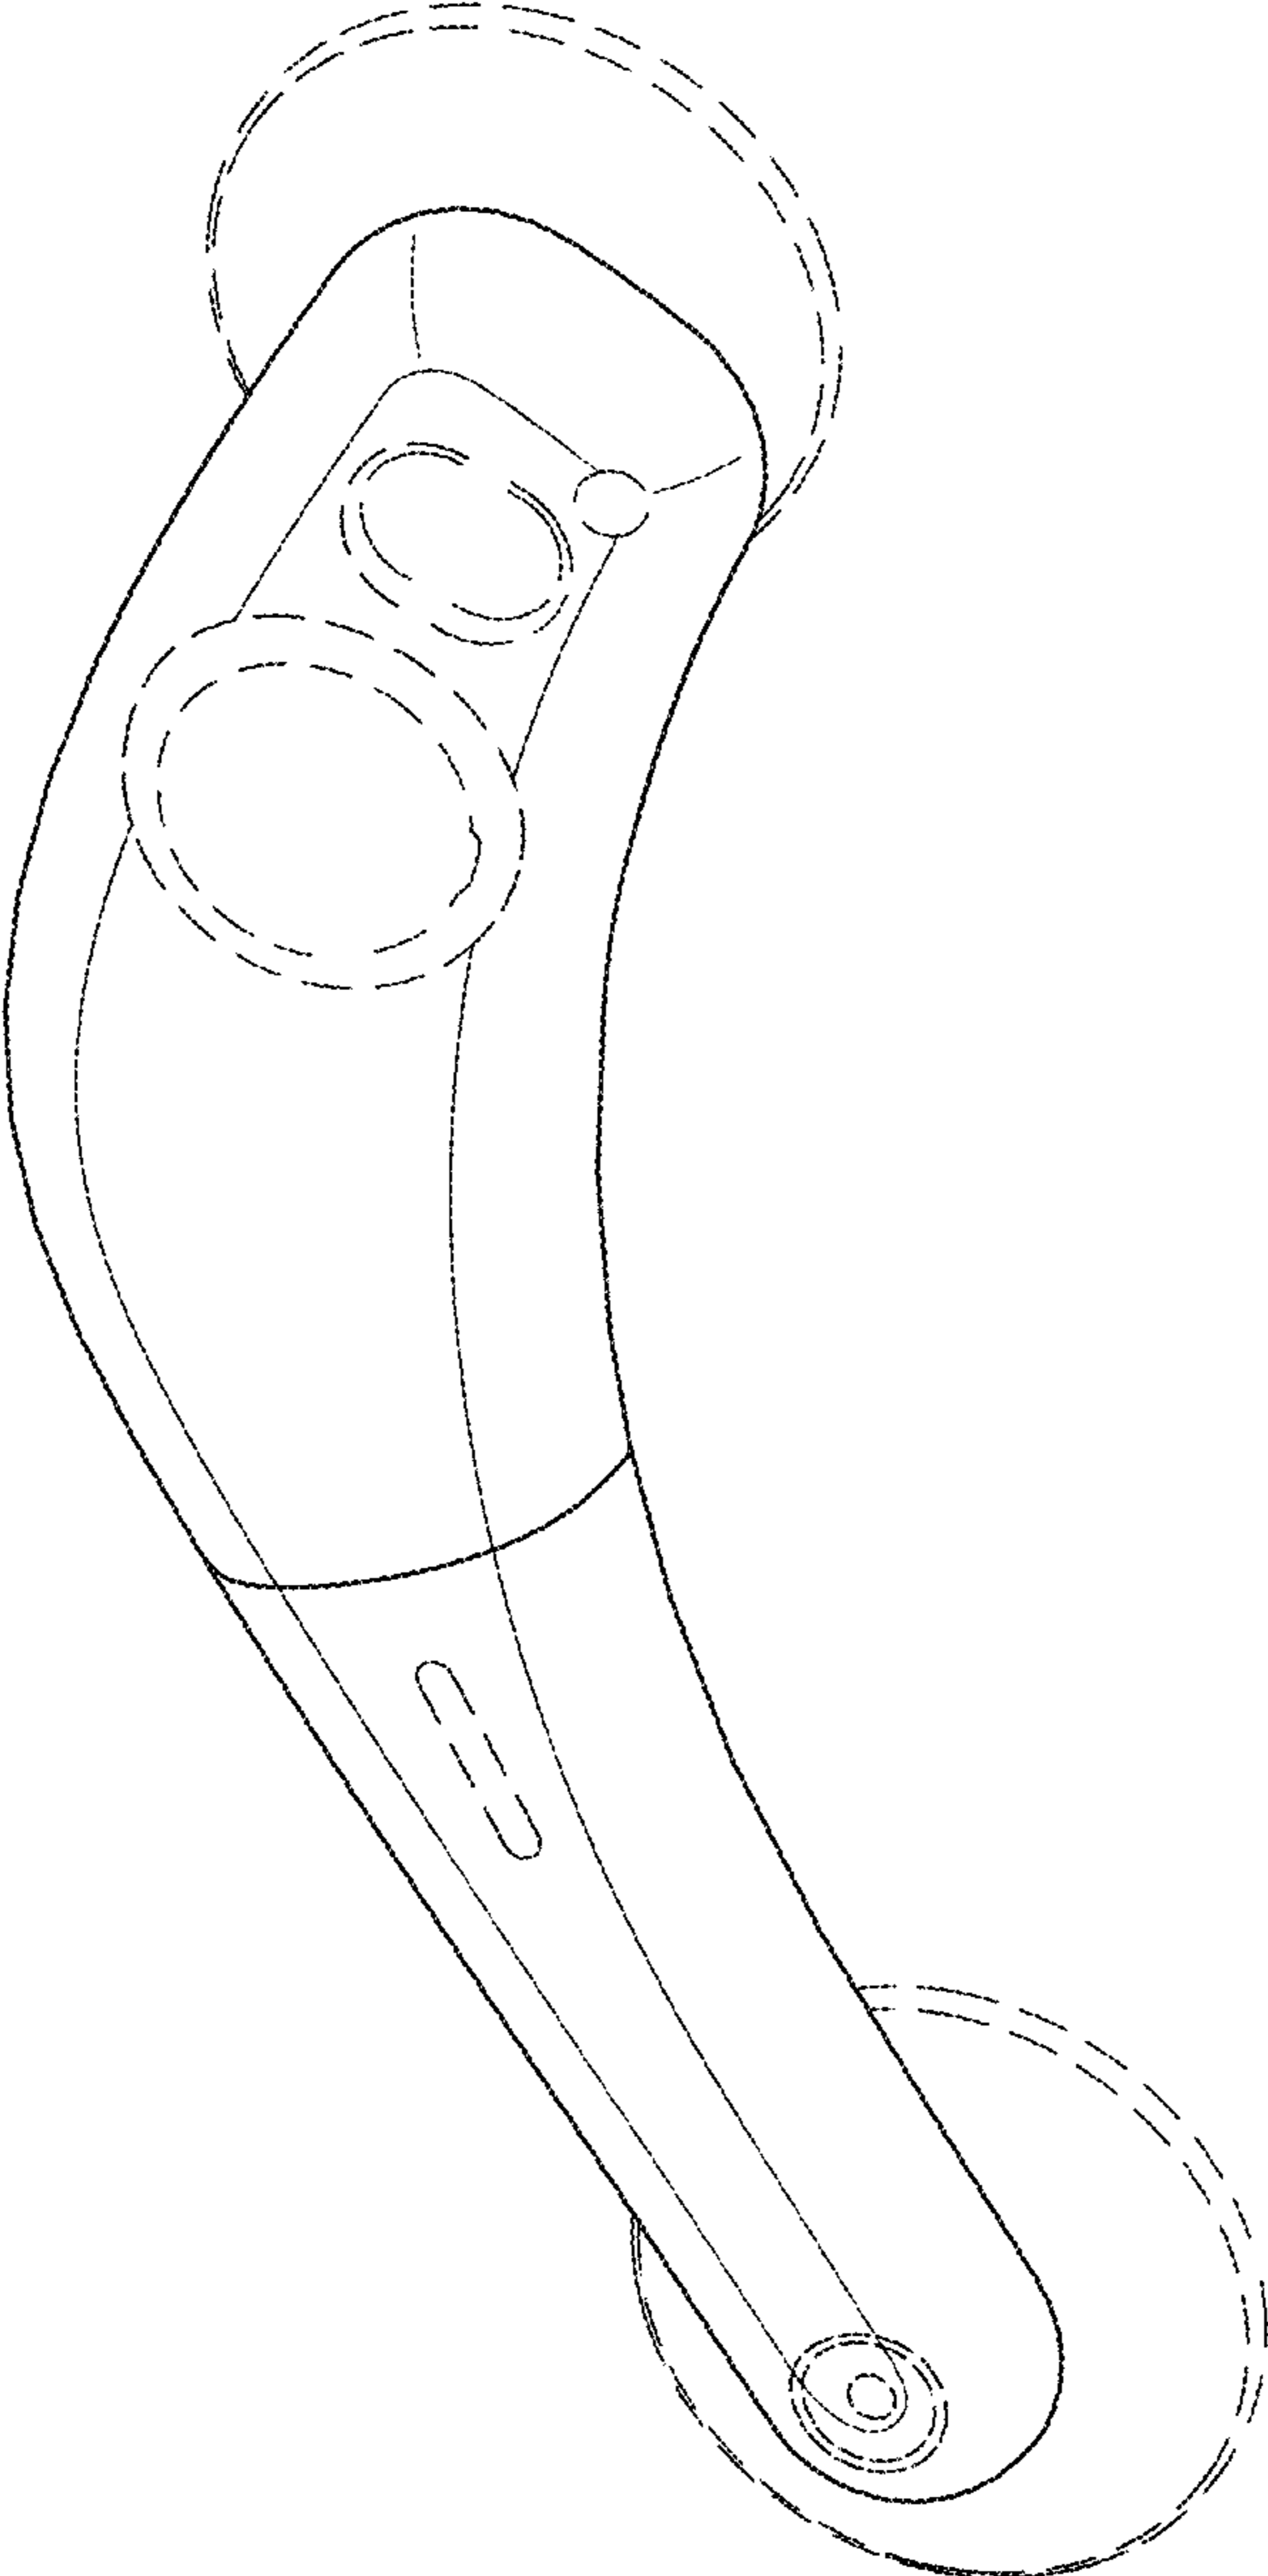


FIG. 1

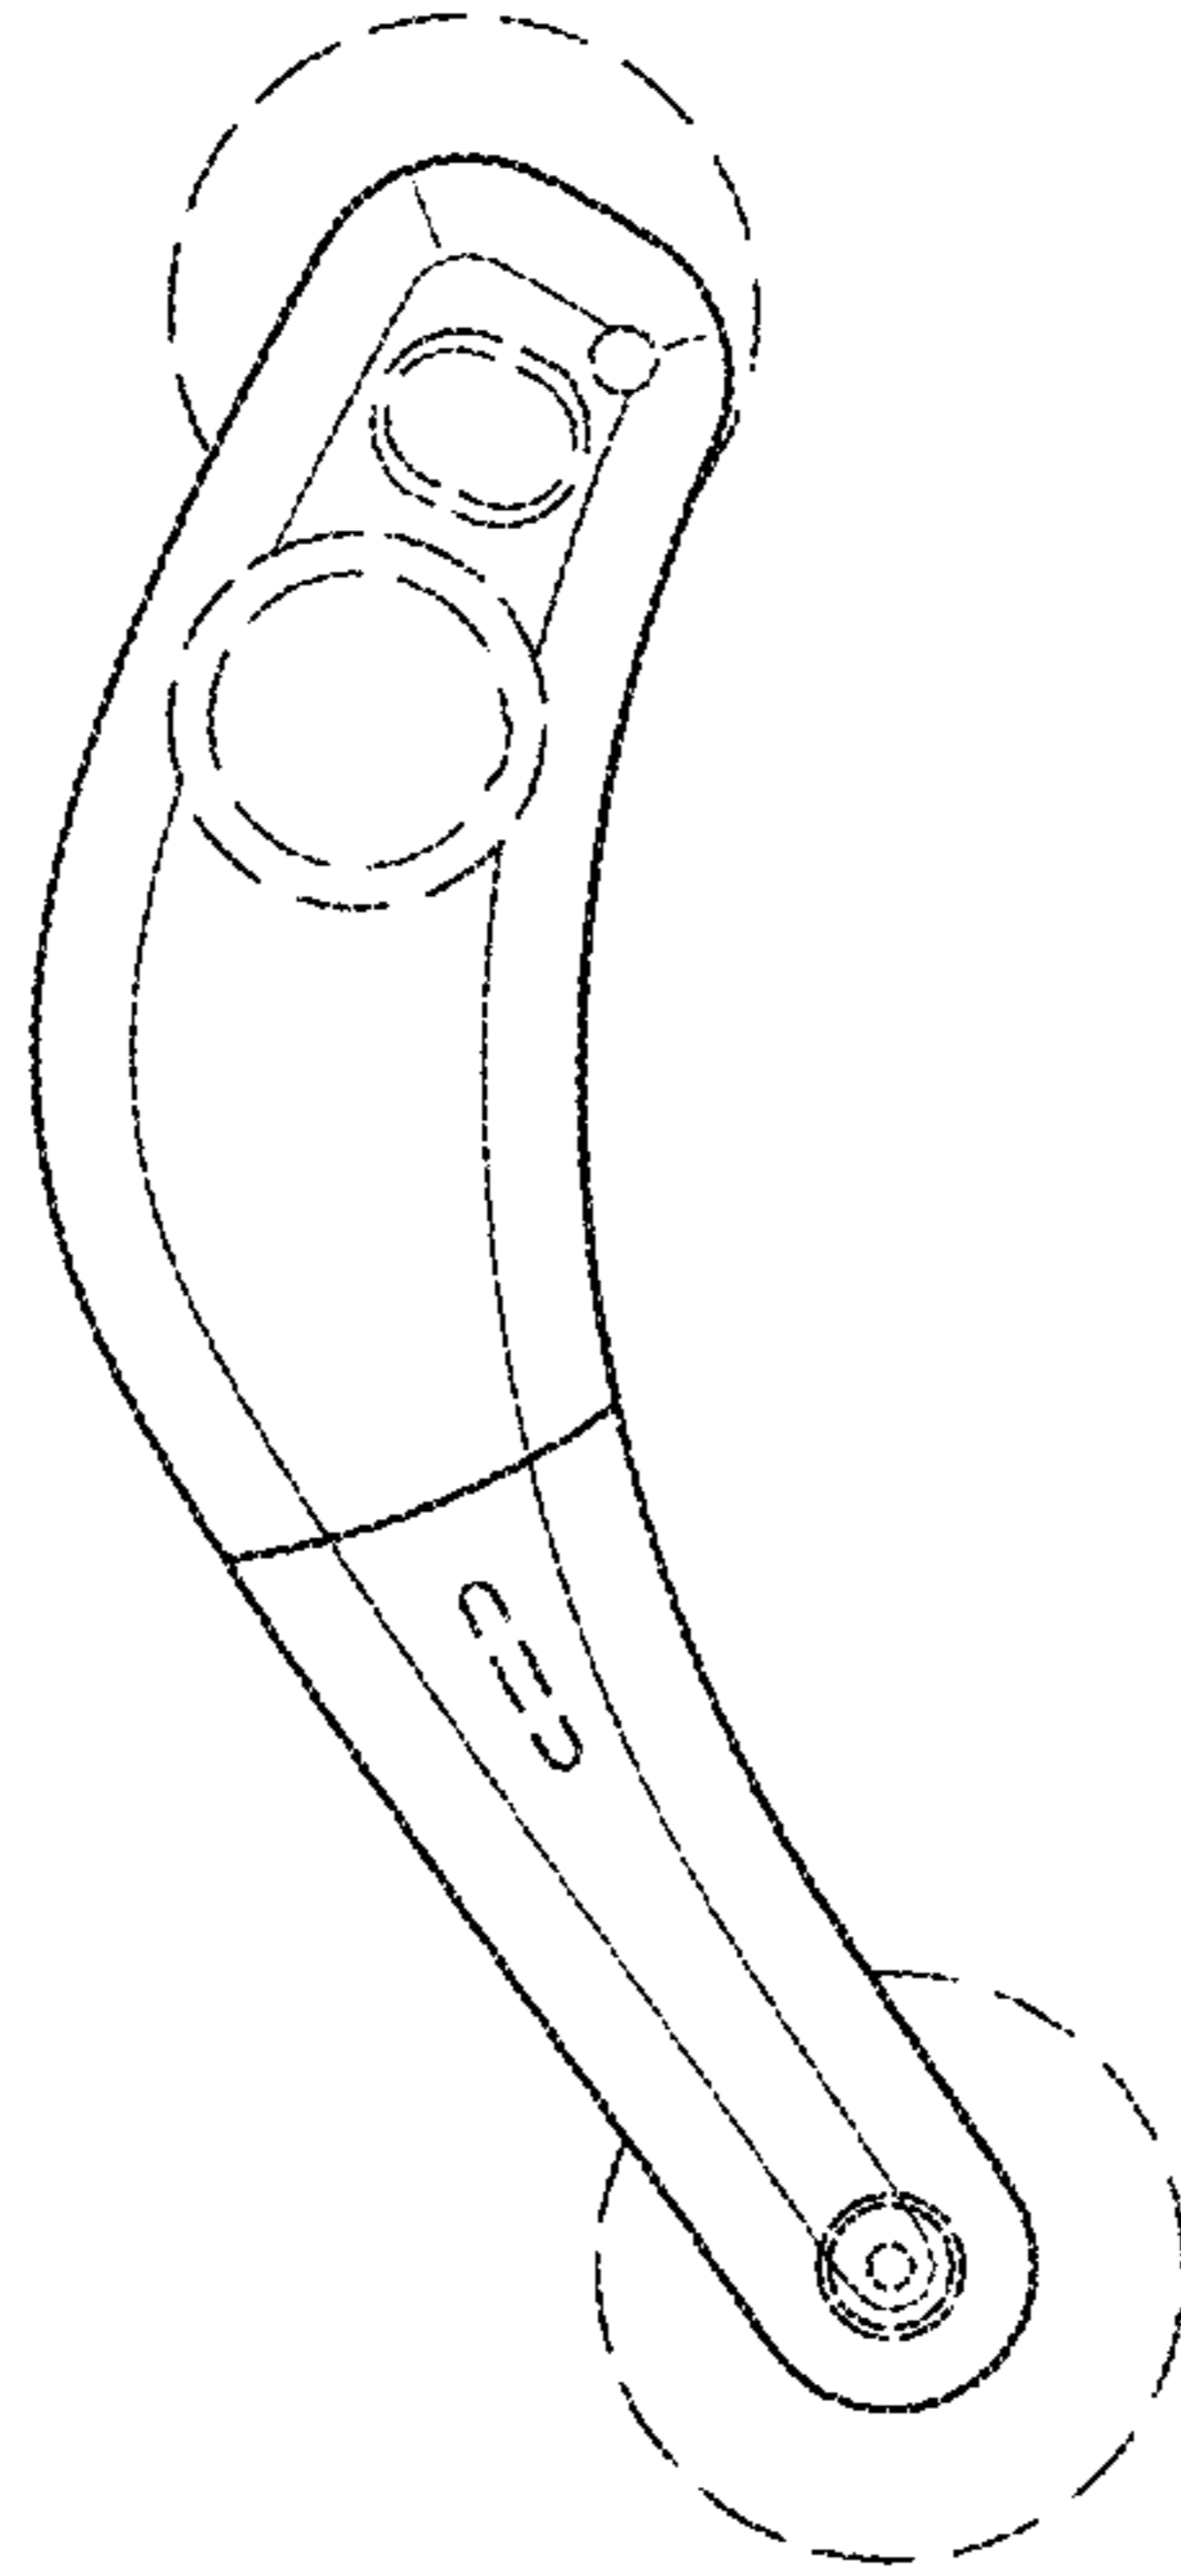


FIG. 2

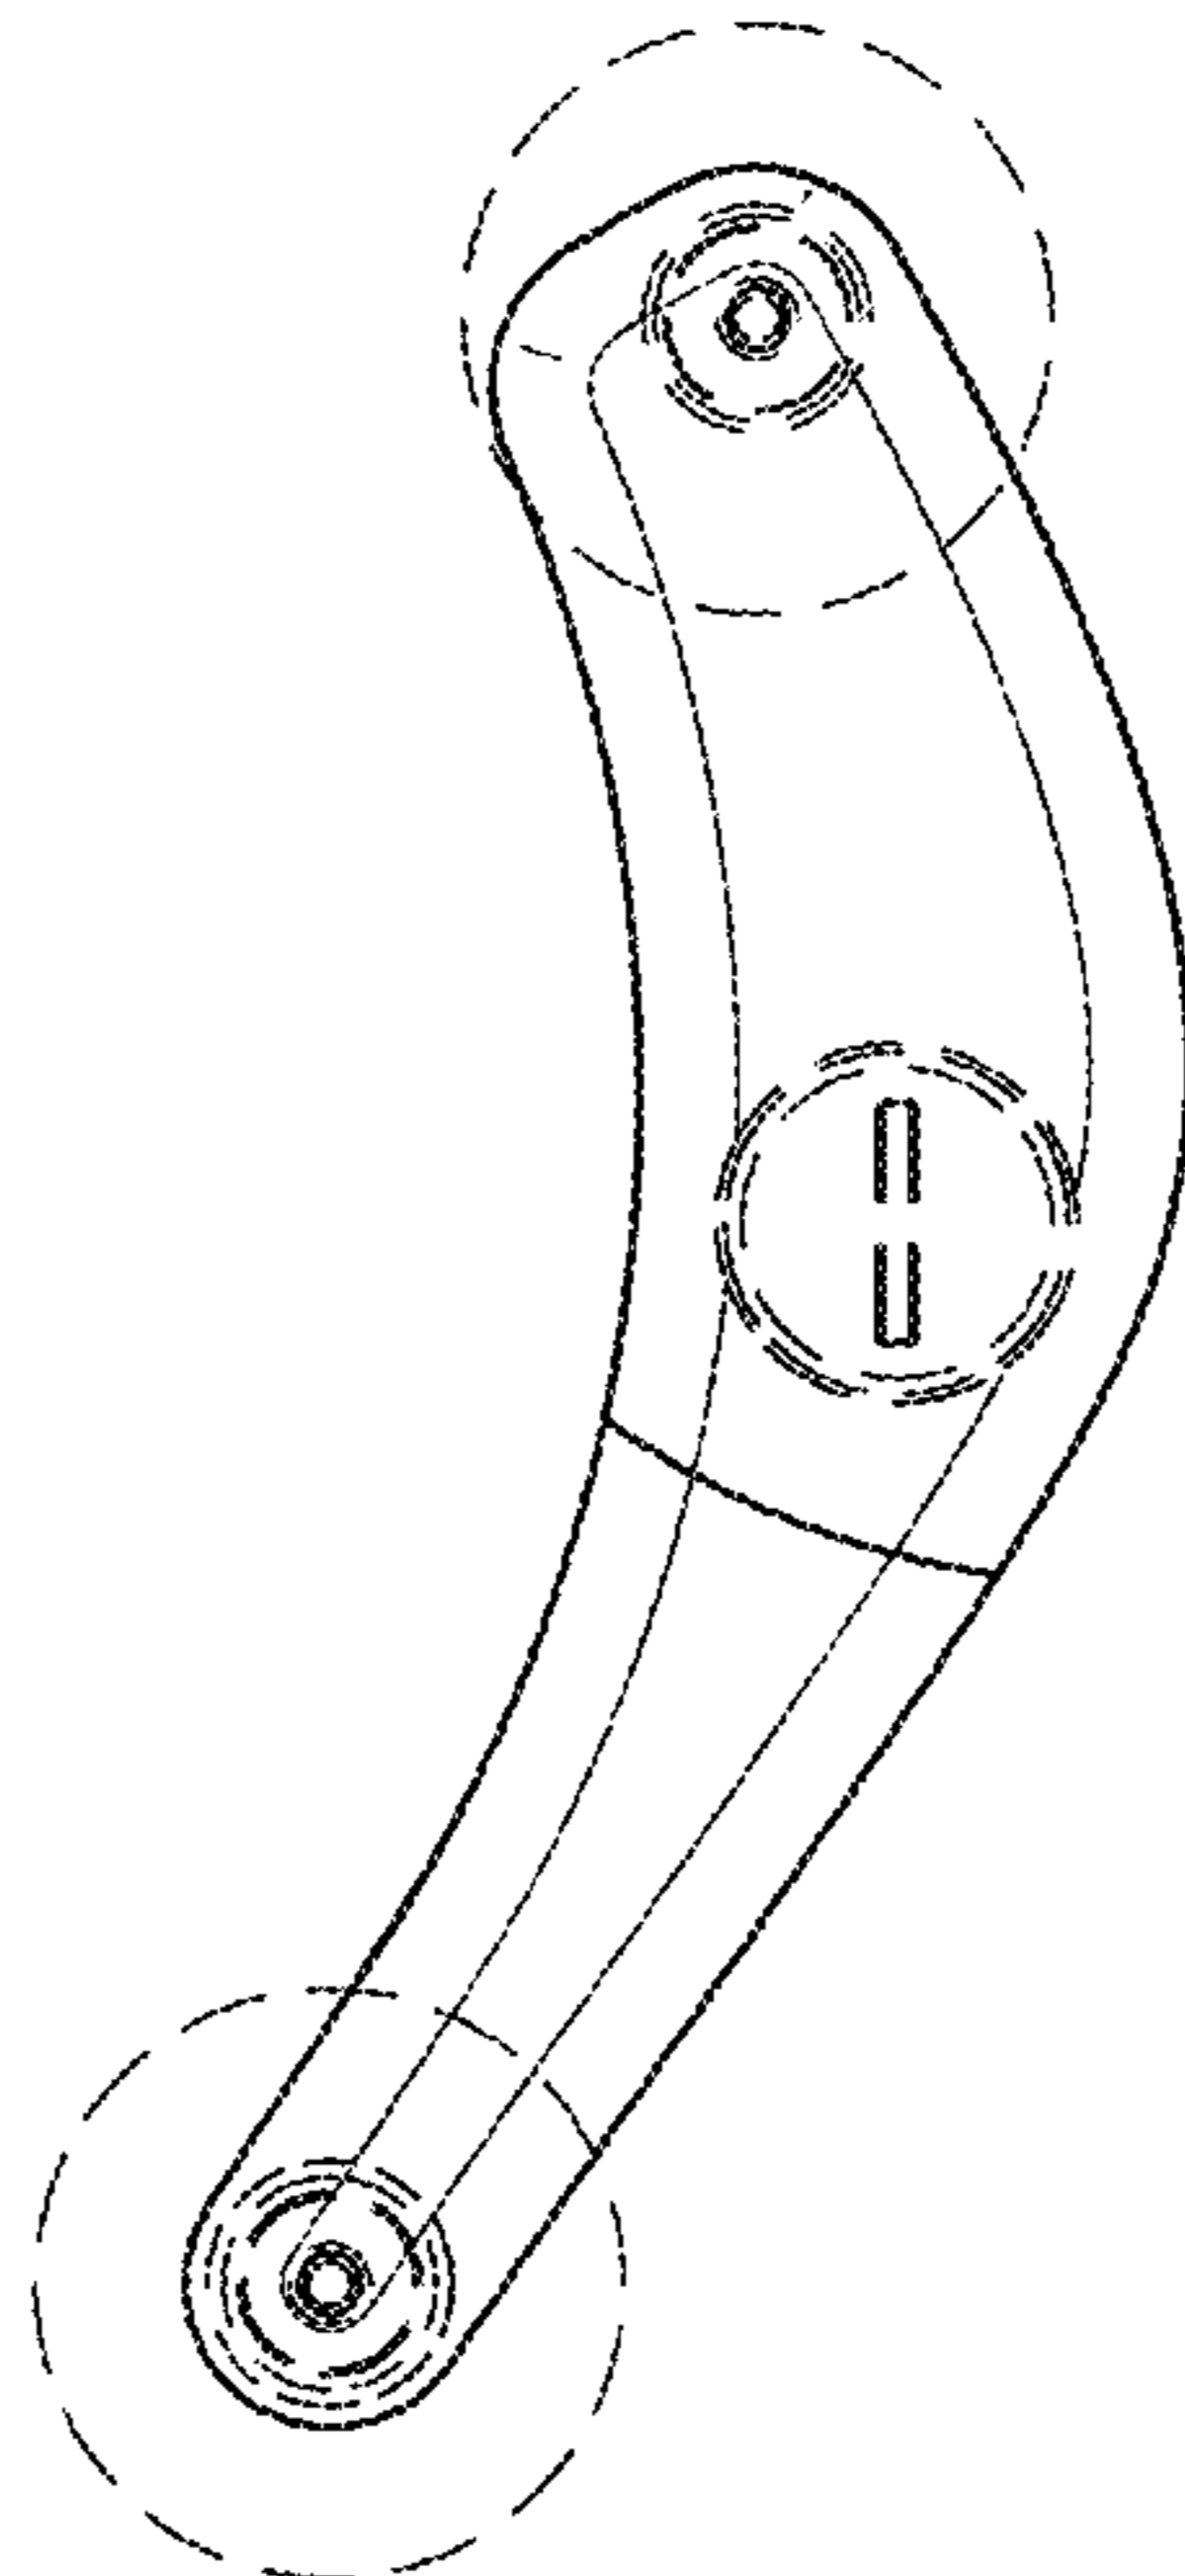


FIG. 3

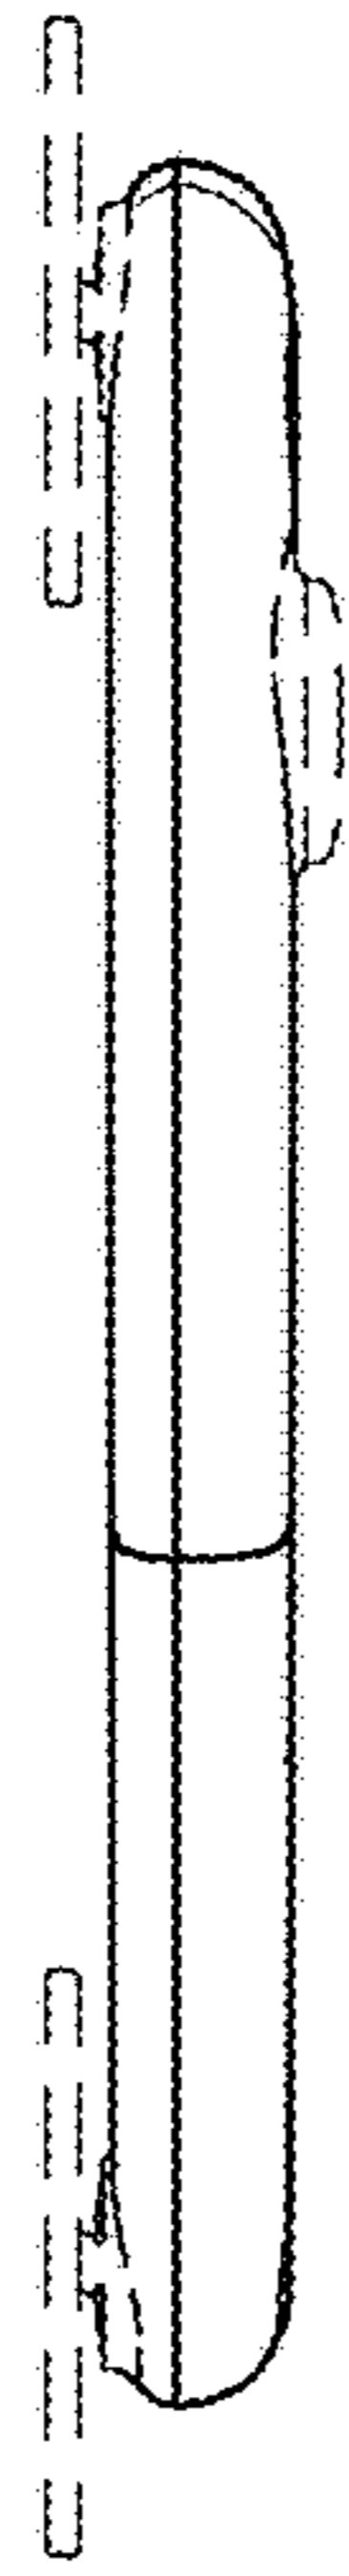


FIG. 4

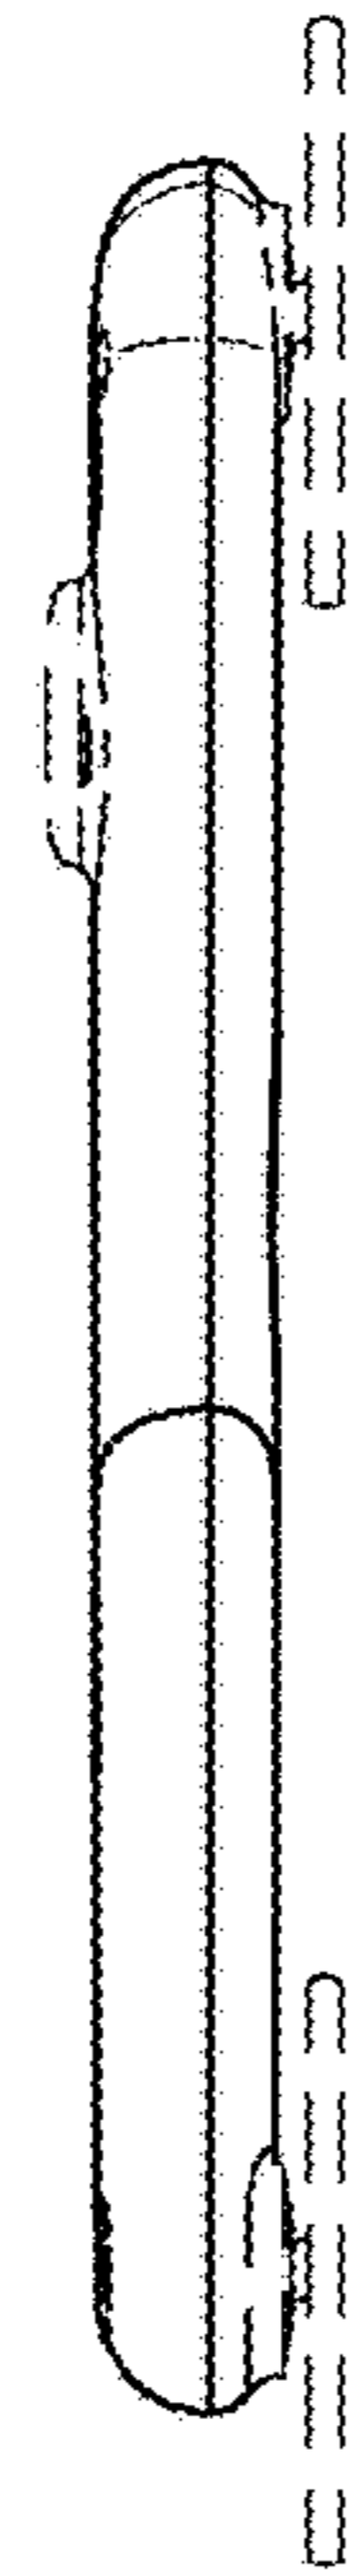


FIG. 5

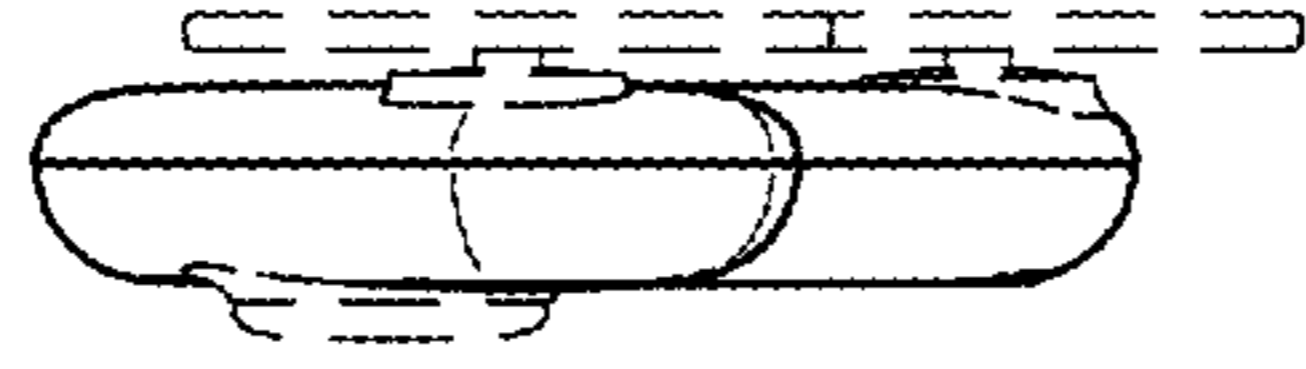


FIG. 6

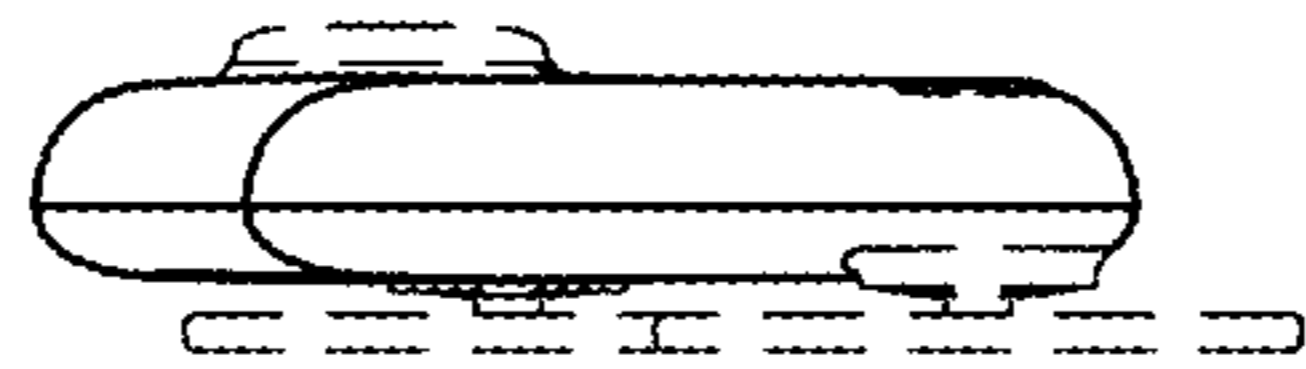


FIG. 7

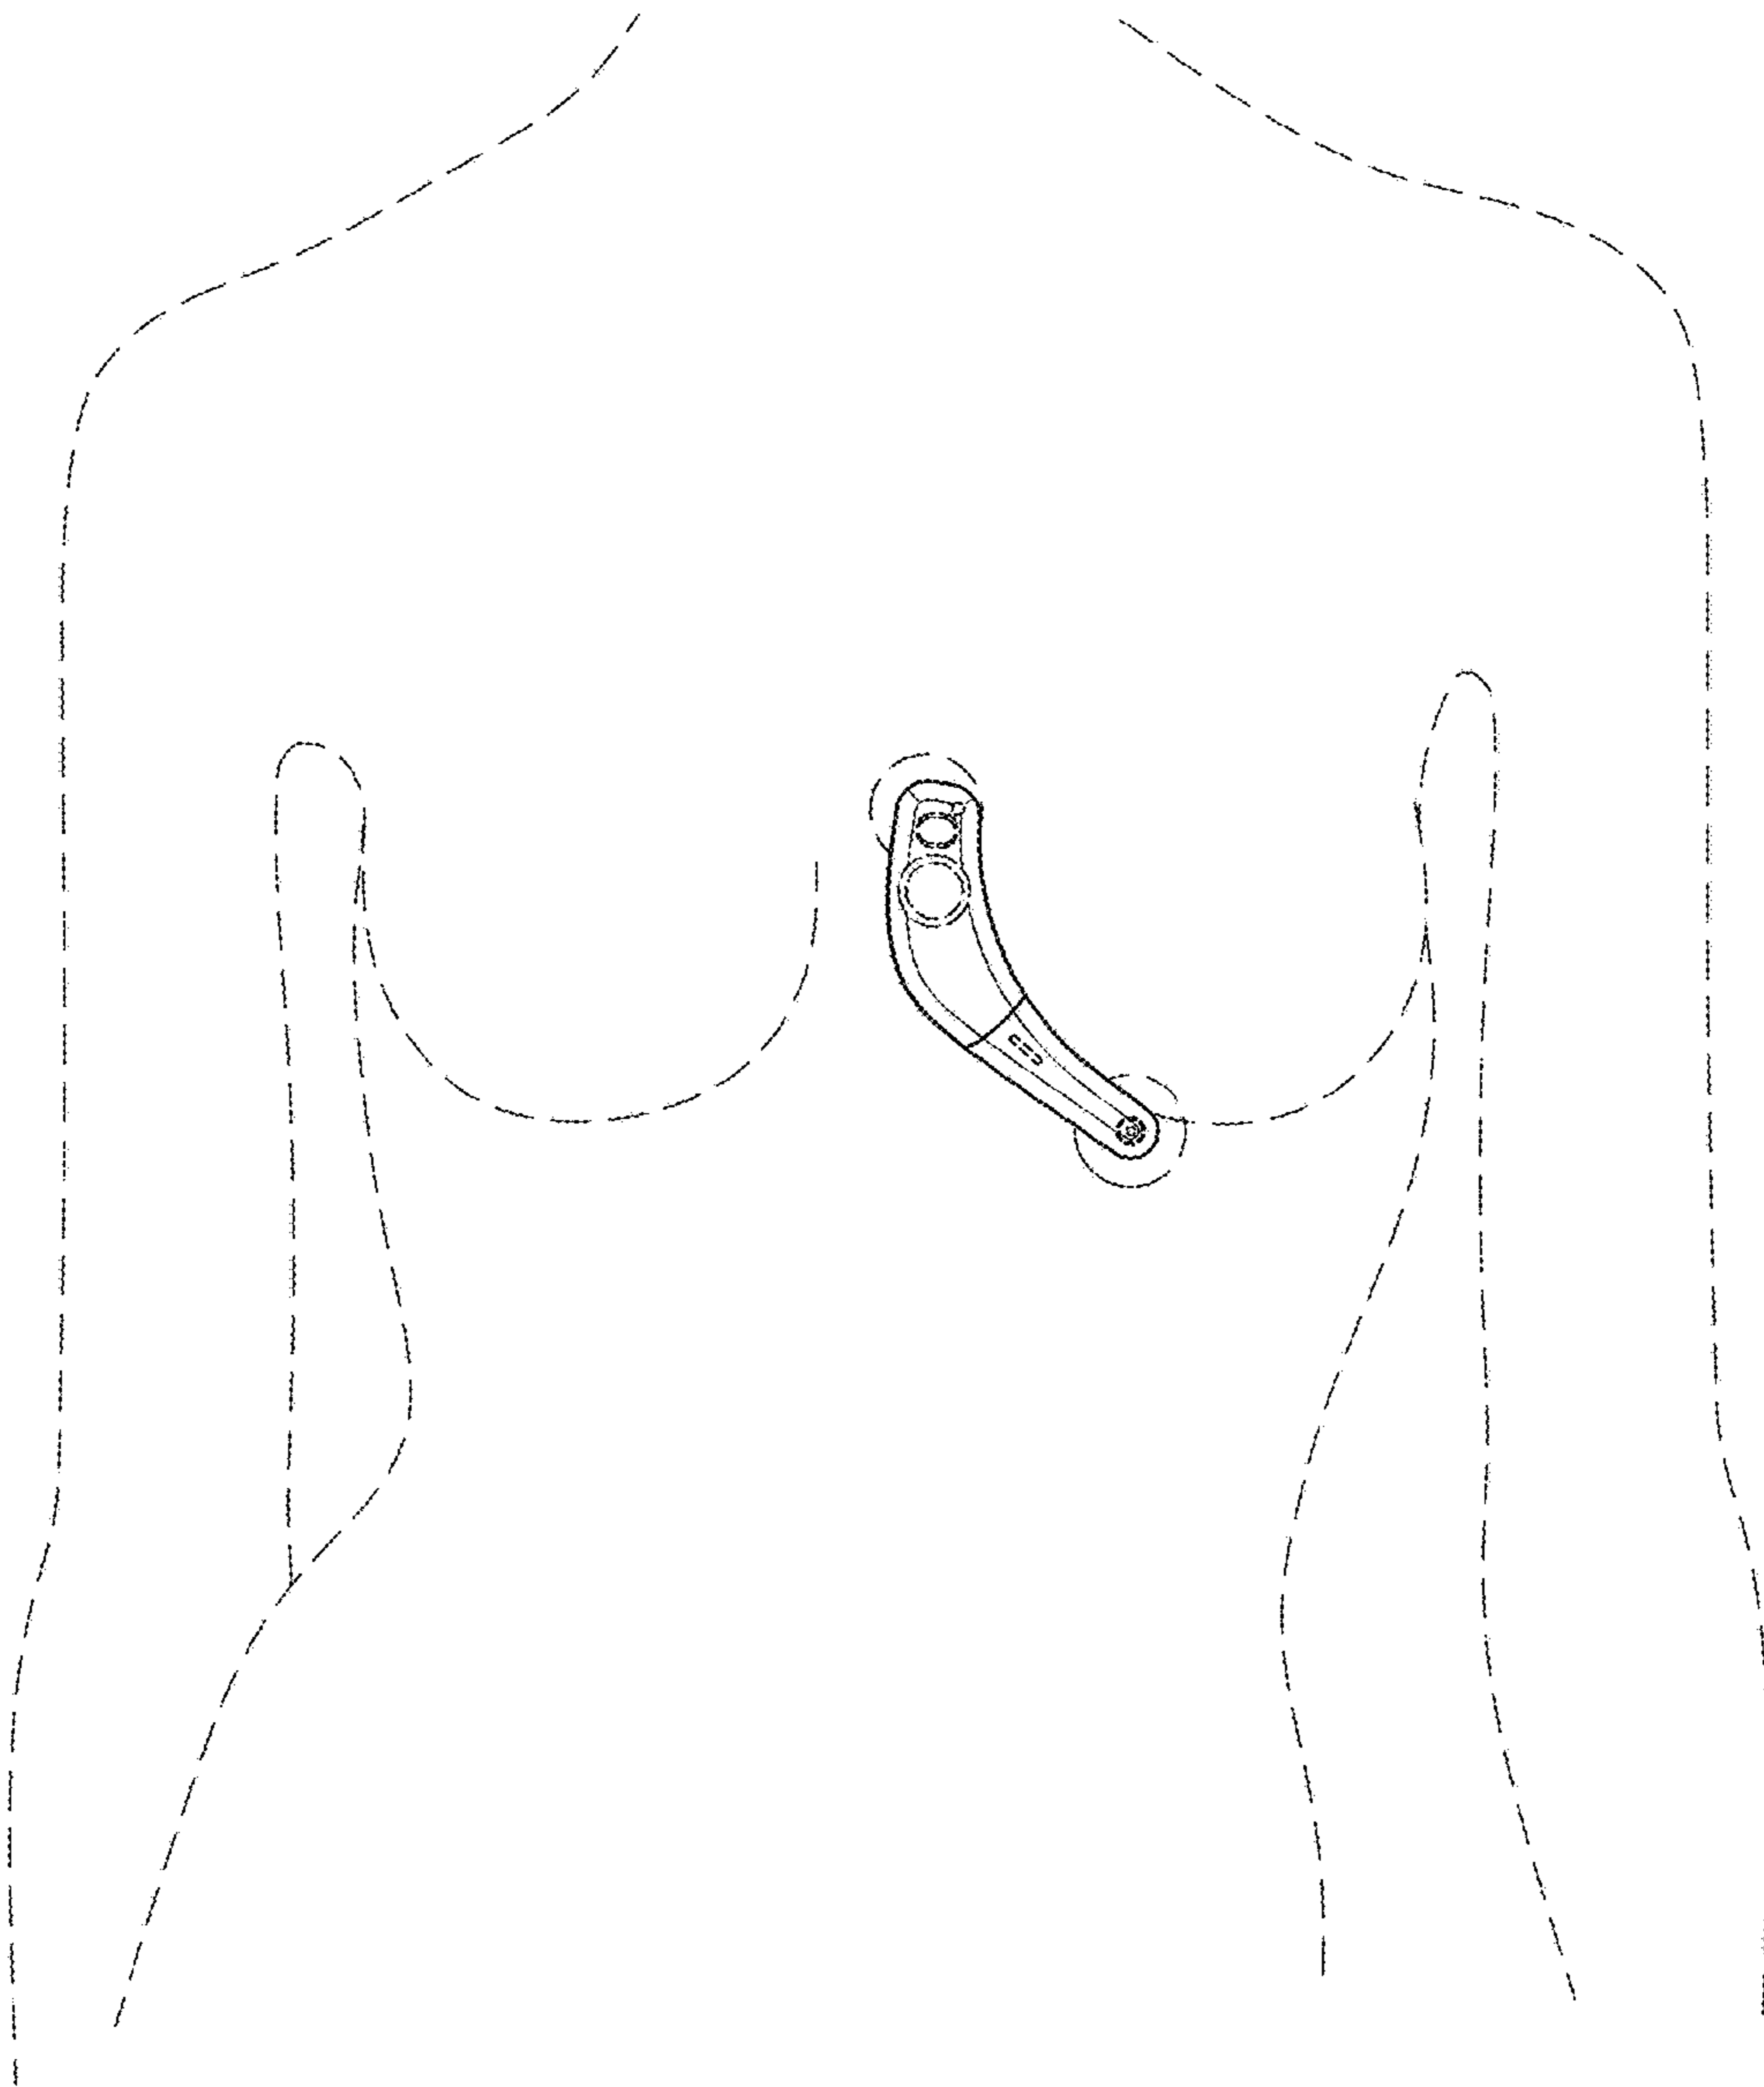


FIG. 8