



US00D787701S

(12) **United States Design Patent**
Wilson et al.

(10) **Patent No.:** **US D787,701 S**

(45) **Date of Patent:** **** May 23, 2017**

(54) **FLOW CYTOMETER SYSTEM SHELF UNIT**

35/04; G01N 15/1404; G01N 15/1425;
A47L 9/0009; A47B 81/005

See application file for complete search history.

(71) Applicant: **Intellicyt Corporation**, Albuquerque,
NM (US)

(56) **References Cited**

(72) Inventors: **Garrett S. Wilson**, Lafayette, CO (US);
Braden L. Smith, Lafayette, CO (US);
Michael A. Artinger, Boulder, CO
(US)

U.S. PATENT DOCUMENTS

D251,644 S * 4/1979 Ravn D6/571
D257,710 S * 12/1980 Basler D24/185
D269,121 S * 5/1983 Pollard D24/128

(Continued)

(73) Assignee: **Intellicyt Corporation**, Albuquerque,
NM (US)

Primary Examiner — Ian Simmons

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Marsh Fischmann &
Breyfogle LLP; Ross E. Breyfogle

(**) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/485,766**

The ornamental design for a flow cytometer system shelf
unit, as shown and described.

(22) Filed: **Mar. 21, 2014**

DESCRIPTION

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**


USPC **D24/227**

(58) **Field of Classification Search**

USPC D24/216–232, 127–128, 130, 133, 185,
D24/177, 161, 134, 158, 164, 107;
D3/203.1–203.8, 304, 313; 211/85.13,
211/126.14, 70.6; D6/571, 406.1, 310,
D6/567, 513, 574, 553, 514, 675.3;
422/297, 401, 560–564; 206/528,
206/538–539, 438, 485, 557; D10/81, 97;
D12/407; 356/36; D8/354; 73/1.79,
73/864.91; 435/287.1, 288.7; 250/435
CPC ... A61L 2/26; B01L 9/06; B01L 3/502; B01L
9/52; A61B 19/0256; A61B 2019/0258;
A61B 19/026; B65D 85/42; B65D 1/34;
B65D 75/327; G01N 15/1459; G01N

FIG. 1 is a top, front and right side perspective view of the
flow cytometer system shelf unit;
FIG. 2 is a top, rear and right side perspective view of the
flow cytometer system shelf unit;
FIG. 3 is a bottom, front and left side perspective view of the
flow cytometer system shelf unit;
FIG. 4 is a top, rear and left side perspective view of the flow
cytometer system shelf unit;
FIG. 5 is a front view of the flow cytometer system shelf
unit;
FIG. 6 is a rear view of the flow cytometer system shelf unit;
FIG. 7 is a right side view of the flow cytometer system shelf
unit;
FIG. 8 is a left side view of the flow cytometer system shelf
unit;
FIG. 9 is a top view of the flow cytometer system shelf unit;
FIG. 10 is a bottom view of the flow cytometer system shelf
unit; and,
FIG. 11 is an enlarged fragmented view of the flow cytom-
eter system shelf unit as indicated by the notation in FIG. 1.

(Continued)

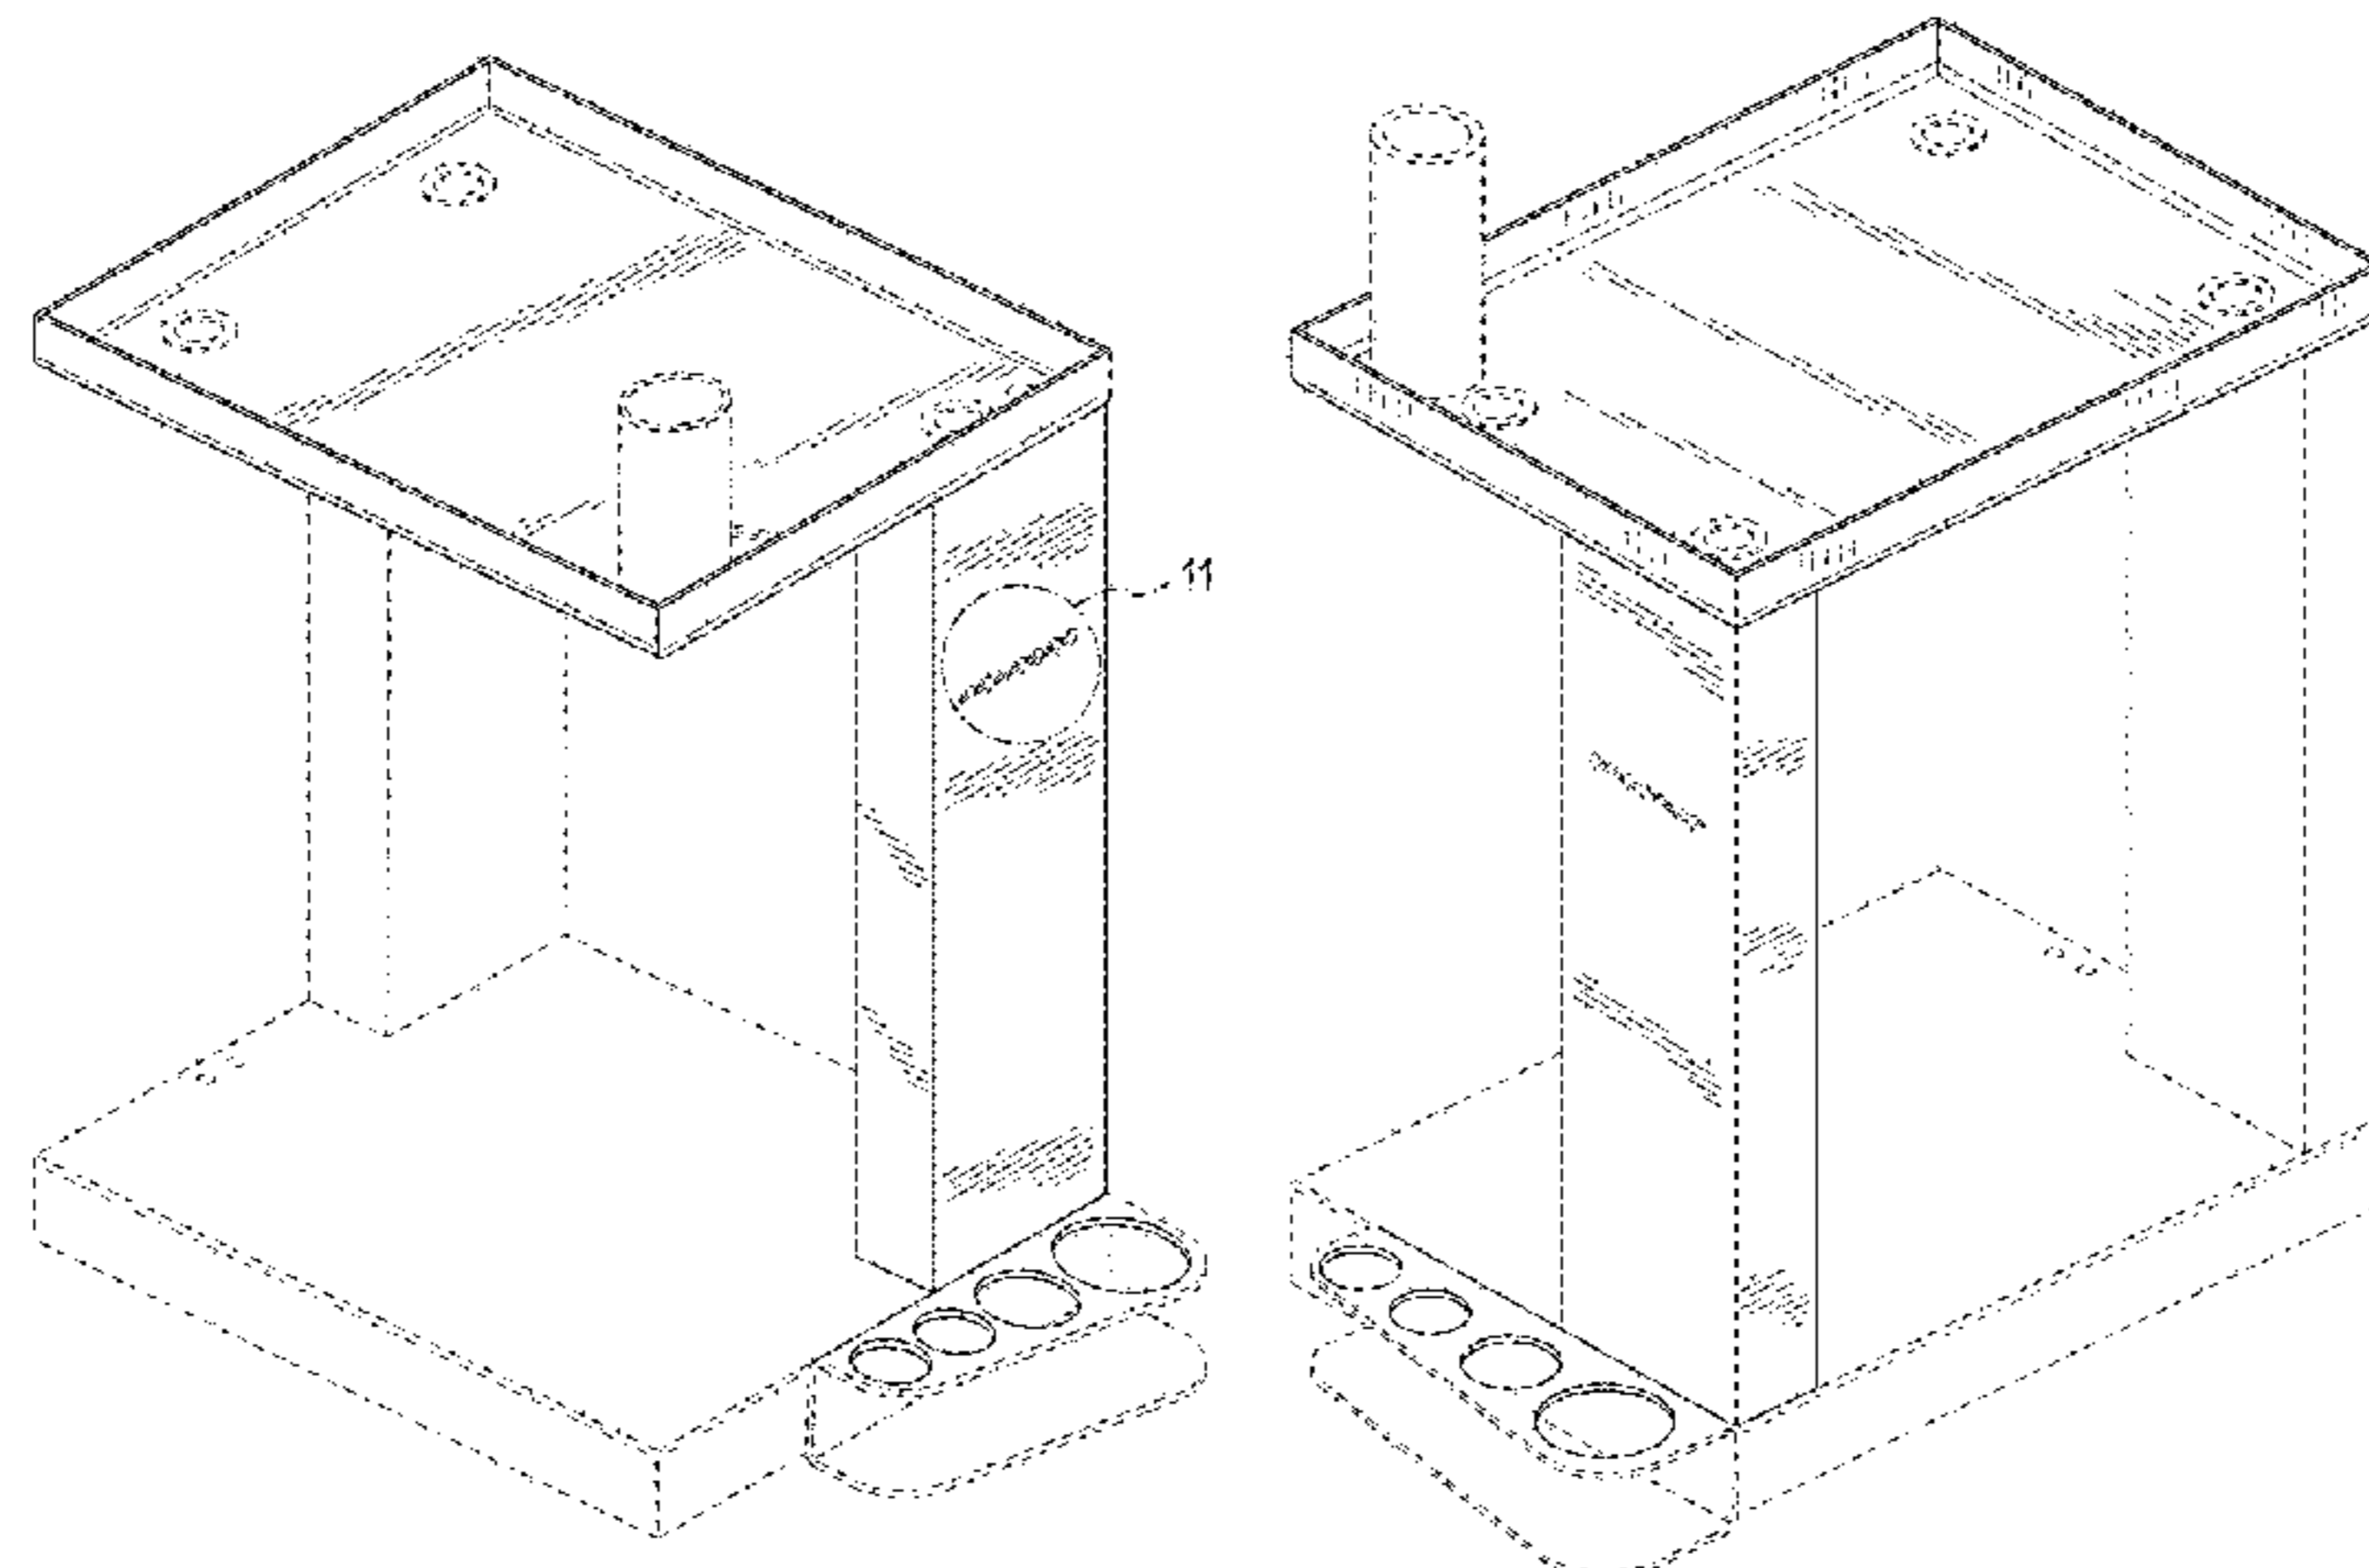

The broken lines in the drawings show portions of the flow cytometer system shelf unit that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

(56)

References Cited

U.S. PATENT DOCUMENTS

D283,049	S *	3/1986	Pandya	D24/223
D283,163	S *	3/1986	Pandya	D24/230
D283,164	S *	3/1986	Pandya	D24/223
D288,122	S *	2/1987	McGaha	D24/177
D292,153	S *	10/1987	Delaney, Sr.	D6/406.1
D298,054	S *	10/1988	Moore	D24/161
D301,575	S *	6/1989	Crawford, Jr.	D24/229
D331,967	S *	12/1992	Flower	D6/310
D337,822	S *	7/1993	Janke	D24/185
D354,874	S *	1/1995	Burch	D6/567
D366,170	S *	1/1996	Temple	D6/513
D392,827	S *	3/1998	Yemini	D6/574
D393,543	S *	4/1998	Wilkening	D3/313
D394,775	S *	6/1998	Anderson	D6/574
D404,831	S *	1/1999	Yamazaki	D24/224
D433,662	S *	11/2000	Fanshaw	D12/407
D442,287	S *	5/2001	Pogorzelski	D24/227
D442,814	S *	5/2001	Sterling	D6/553
D445,185	S *	7/2001	Najmi	D24/134
D486,580	S *	2/2004	Abdel-Model	D24/229
D550,007	S *	9/2007	Westra	D6/514
D575,972	S *	9/2008	Shiao	D6/567
7,506,770	B2 *	3/2009	Rief	A47L 9/0009 211/70.6

D595,423	S *	6/2009	Johansson	D24/229
D598,730	S *	8/2009	Luo	D8/354
D602,724	S *	10/2009	Liu	D6/567
D606,202	S *	12/2009	Banryu	D24/185
D609,349	S *	2/2010	Pelissier	D24/186
D617,990	S *	6/2010	Liao	D3/313
D628,299	S *	11/2010	Held	D24/185
D650,482	S *	12/2011	Kim	D24/158
D652,932	S *	1/2012	Petteway	D24/164
D655,410	S *	3/2012	Chu	D24/128
D674,506	S *	1/2013	Labrasca	D24/227
D687,561	S *	8/2013	Iseki	D24/216
D696,783	S *	12/2013	Chung	D24/185
D706,558	S *	6/2014	Yates	D6/675.3
D708,341	S *	7/2014	Ikegame	D24/185
D725,406	S *	3/2015	Olszewski	D6/567
9,033,162	B2 *	5/2015	Brotzman	A61B 19/0256 211/126.14
D738,243	S *	9/2015	Selberg	D10/81
D746,433	S *	12/2015	Smith	D24/107
9,282,817	B2 *	3/2016	Yates	A47B 81/005
D764,956	S *	8/2016	Selberg	D10/97
2004/0025602	A1 *	2/2004	Norton	G01N 15/1459 356/36
2010/0014947	A1 *	1/2010	Kehrer	G01N 35/04 73/1.79
2011/0300618	A1 *	12/2011	Lieblein	B01L 3/502 435/287.1
2013/0020498	A1 *	1/2013	Ebi	G01N 15/1404 250/435
2013/0340539	A1 *	12/2013	Gaskill-Fox	B01L 9/52 73/864.91
2015/0050688	A1 *	2/2015	Thrasher	G01N 15/1425 435/288.7

* cited by examiner

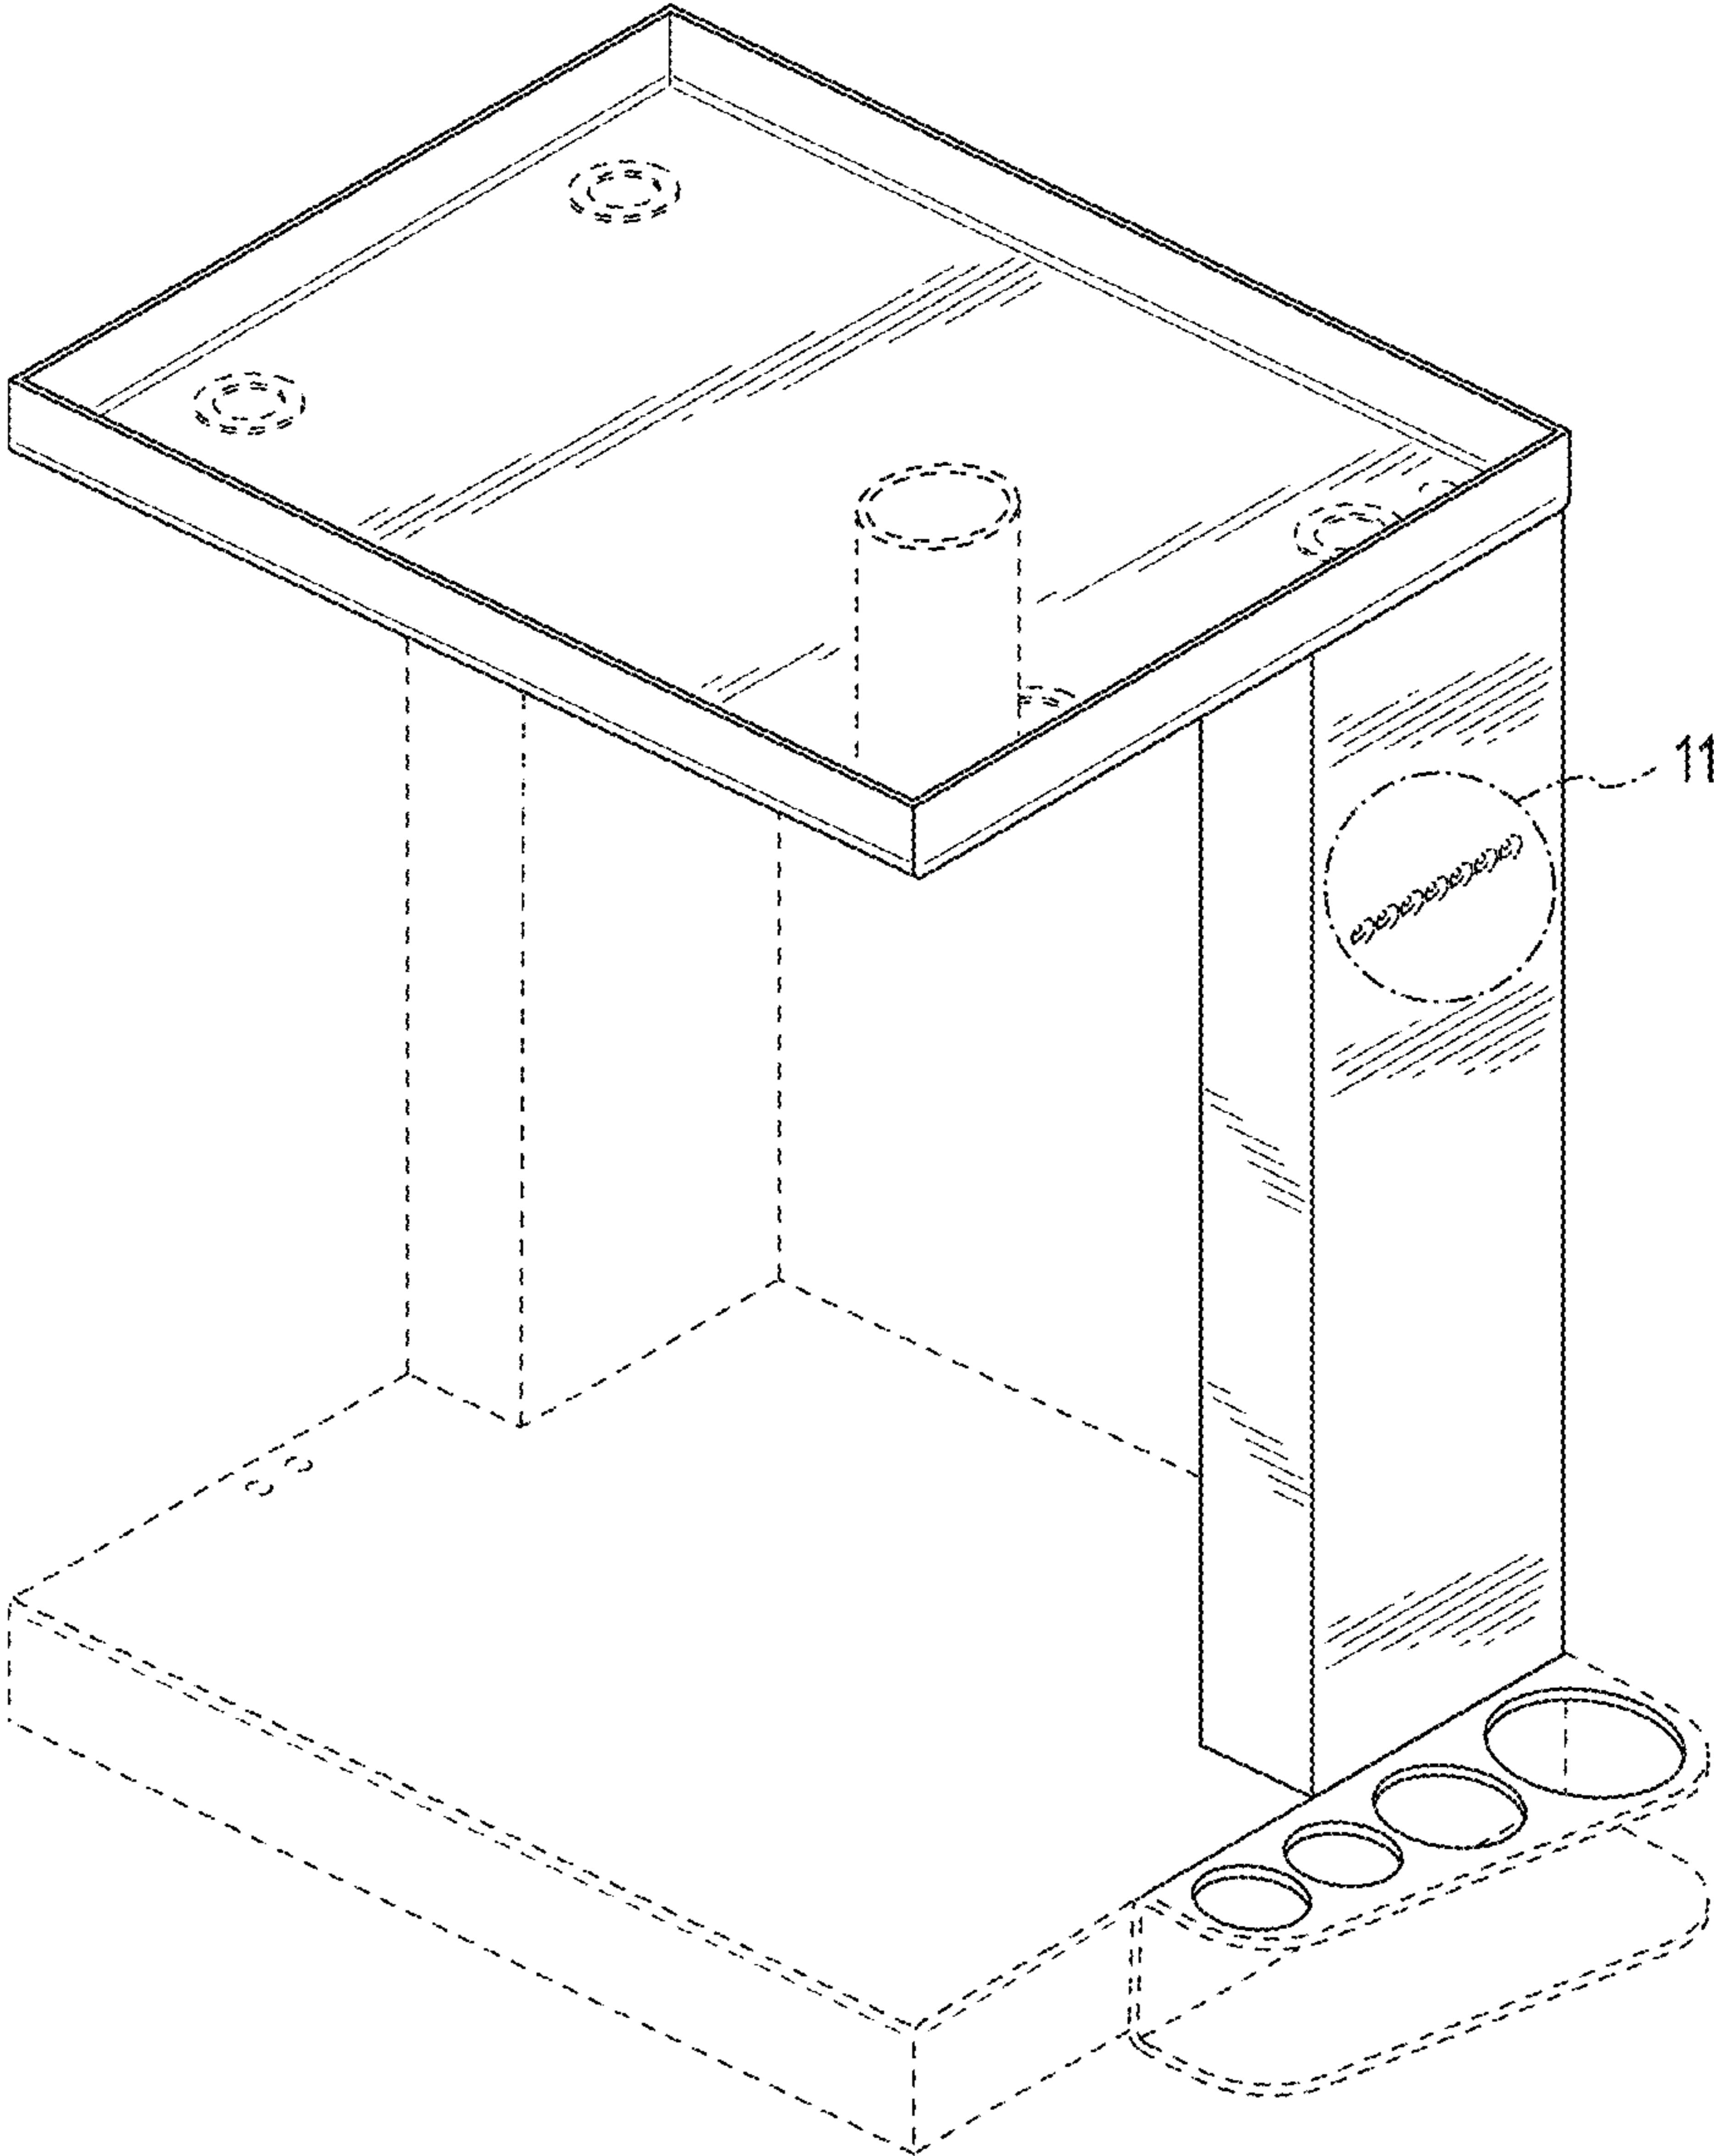


FIG.1

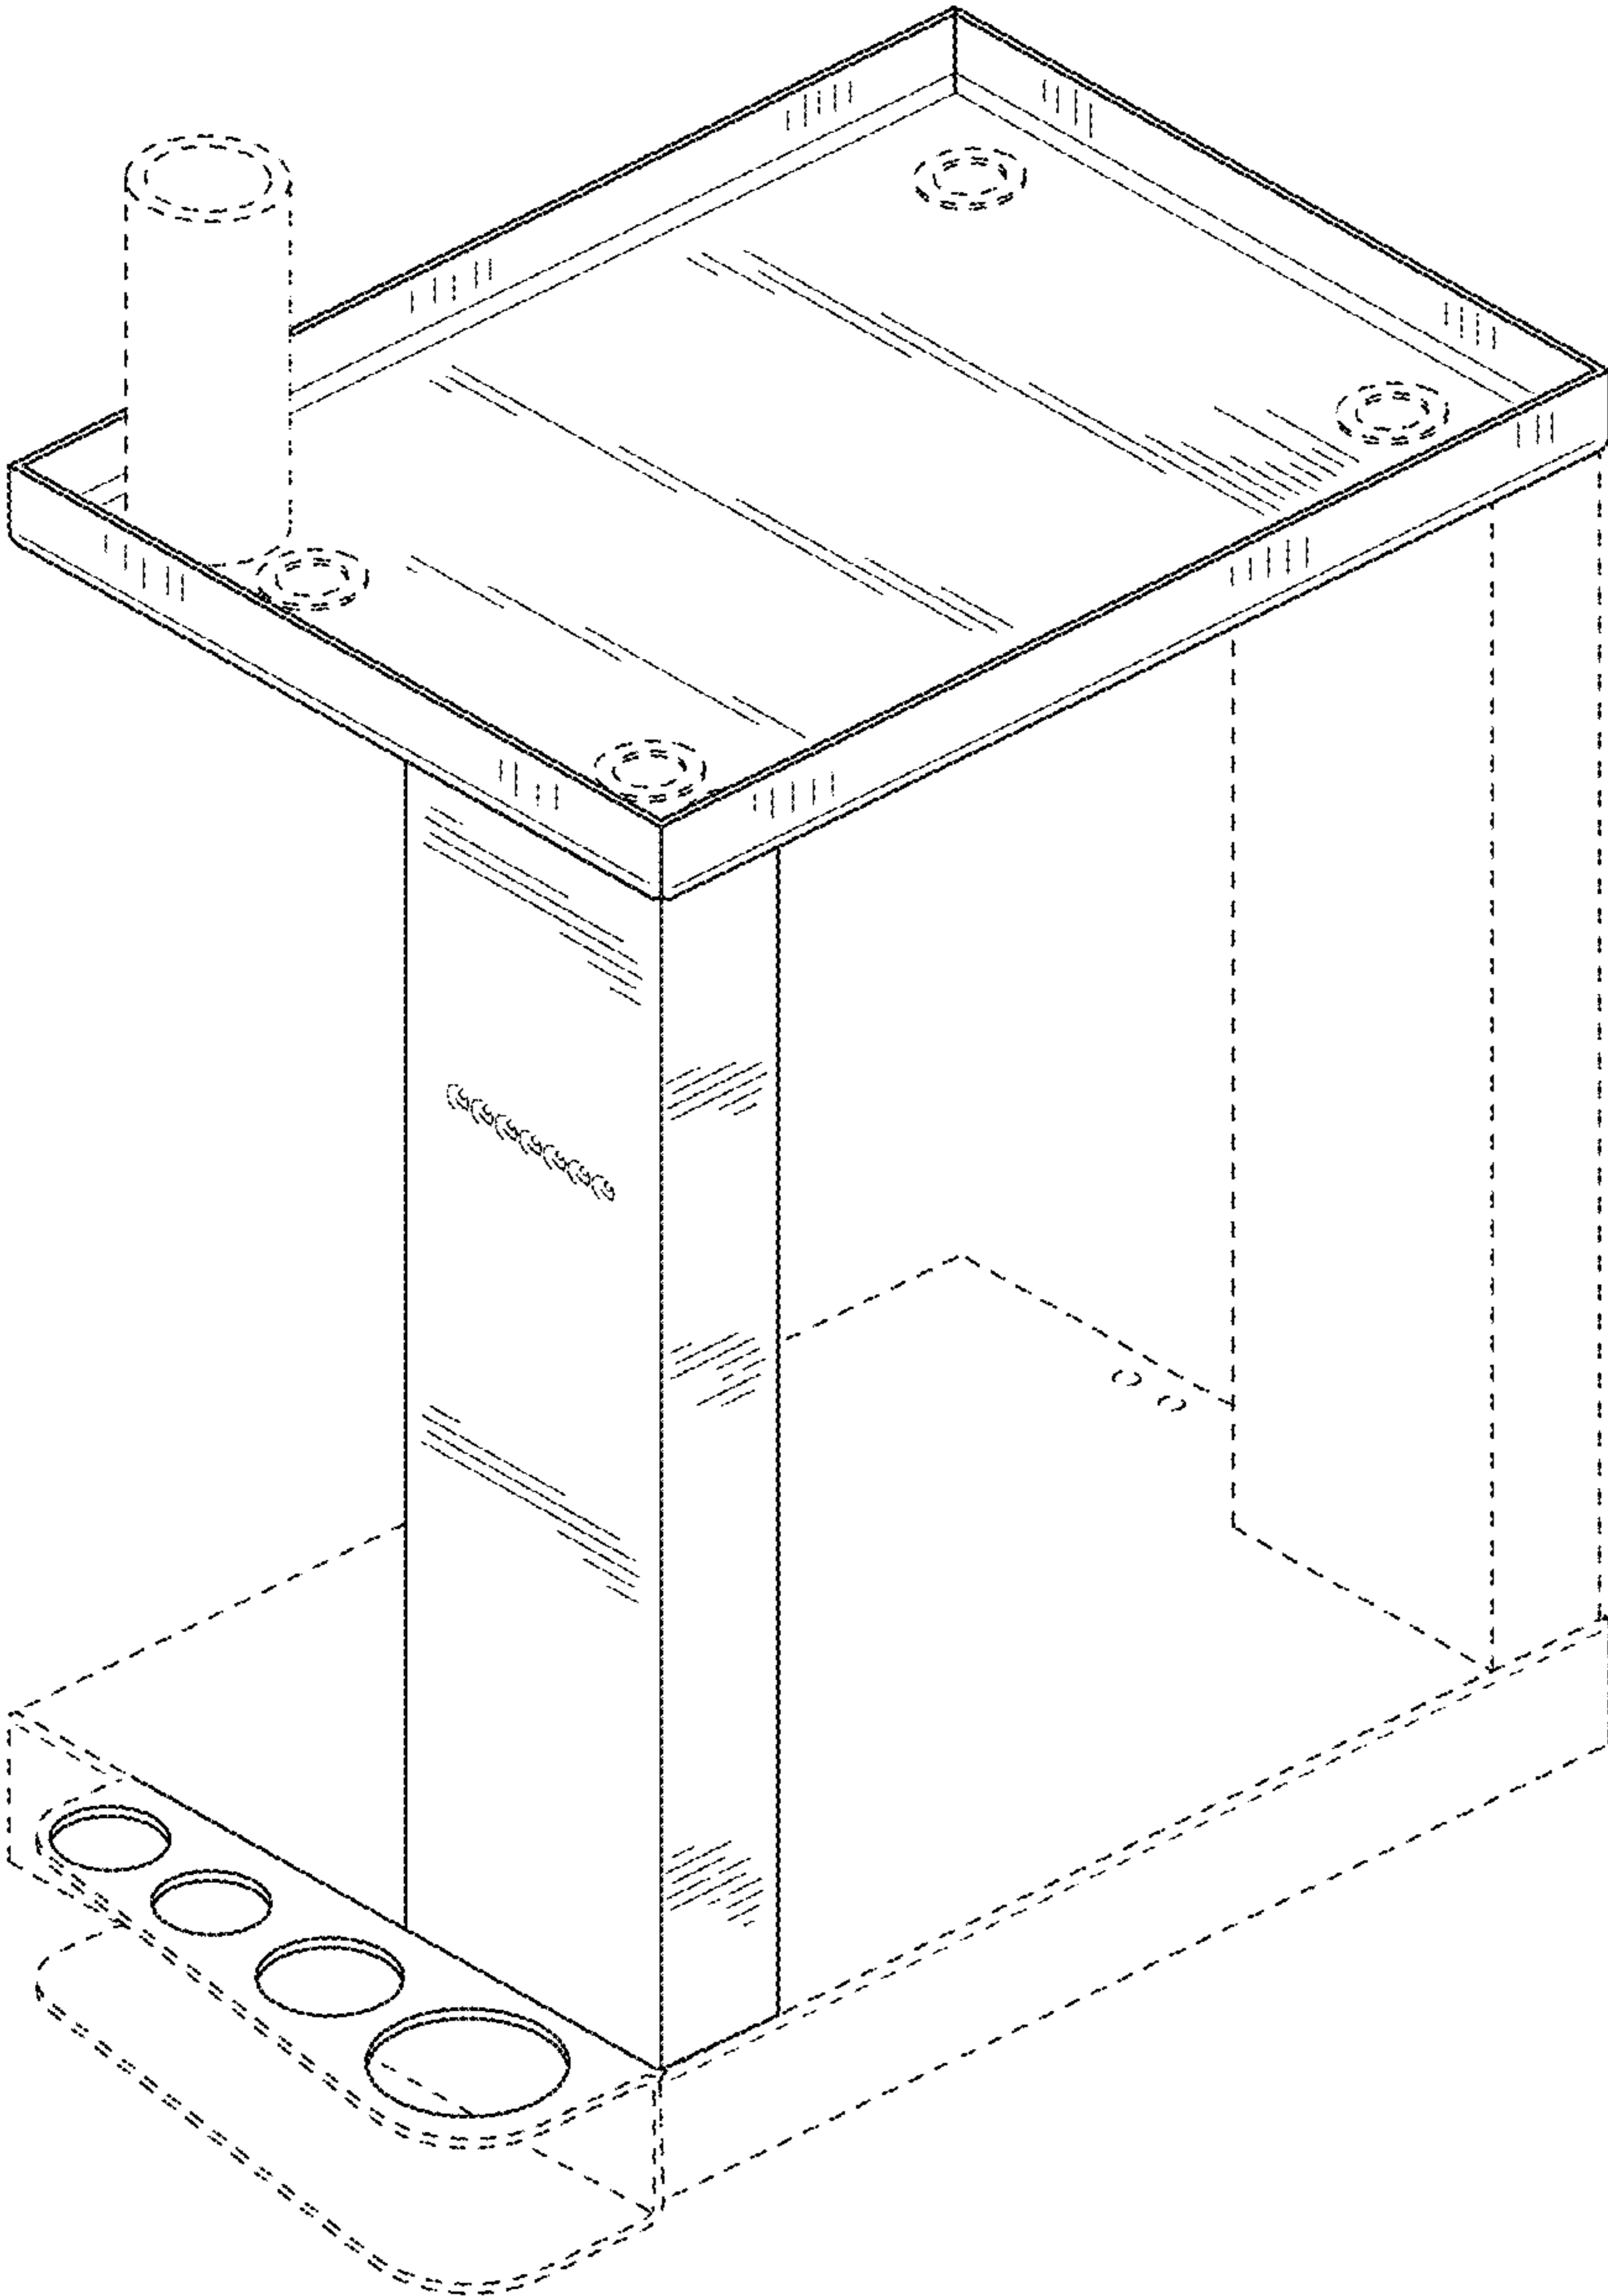


FIG.2

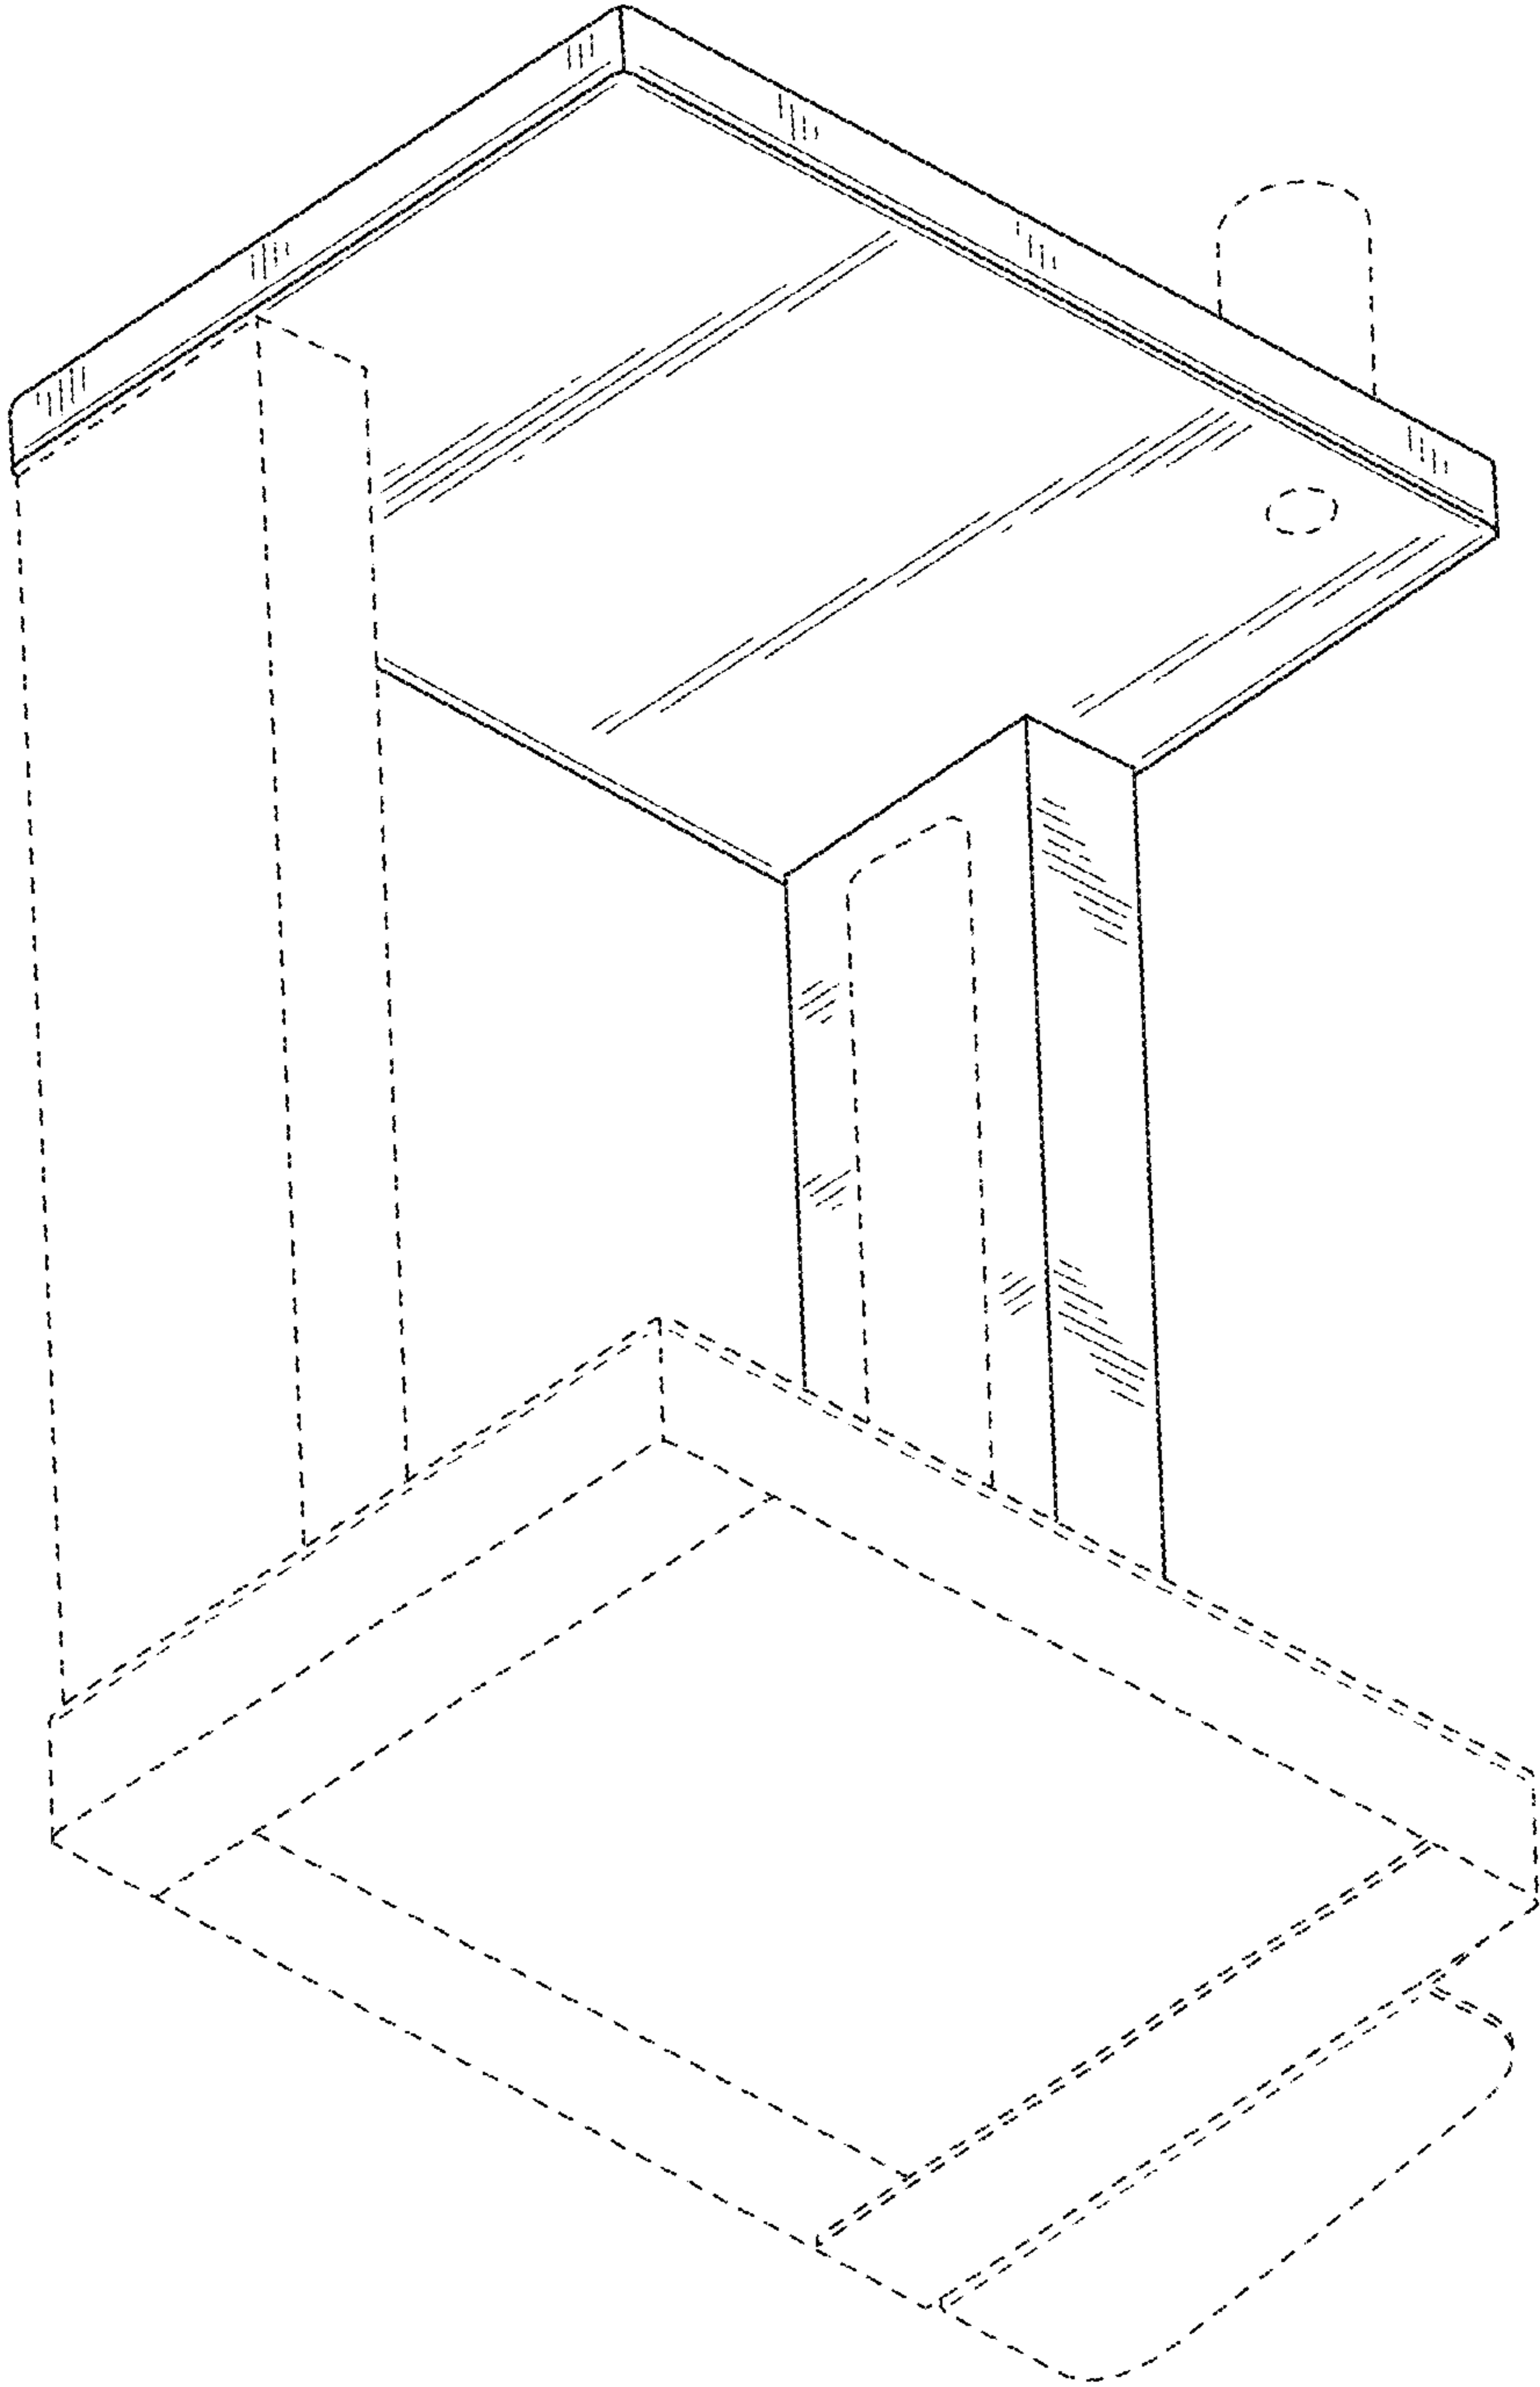


FIG.3

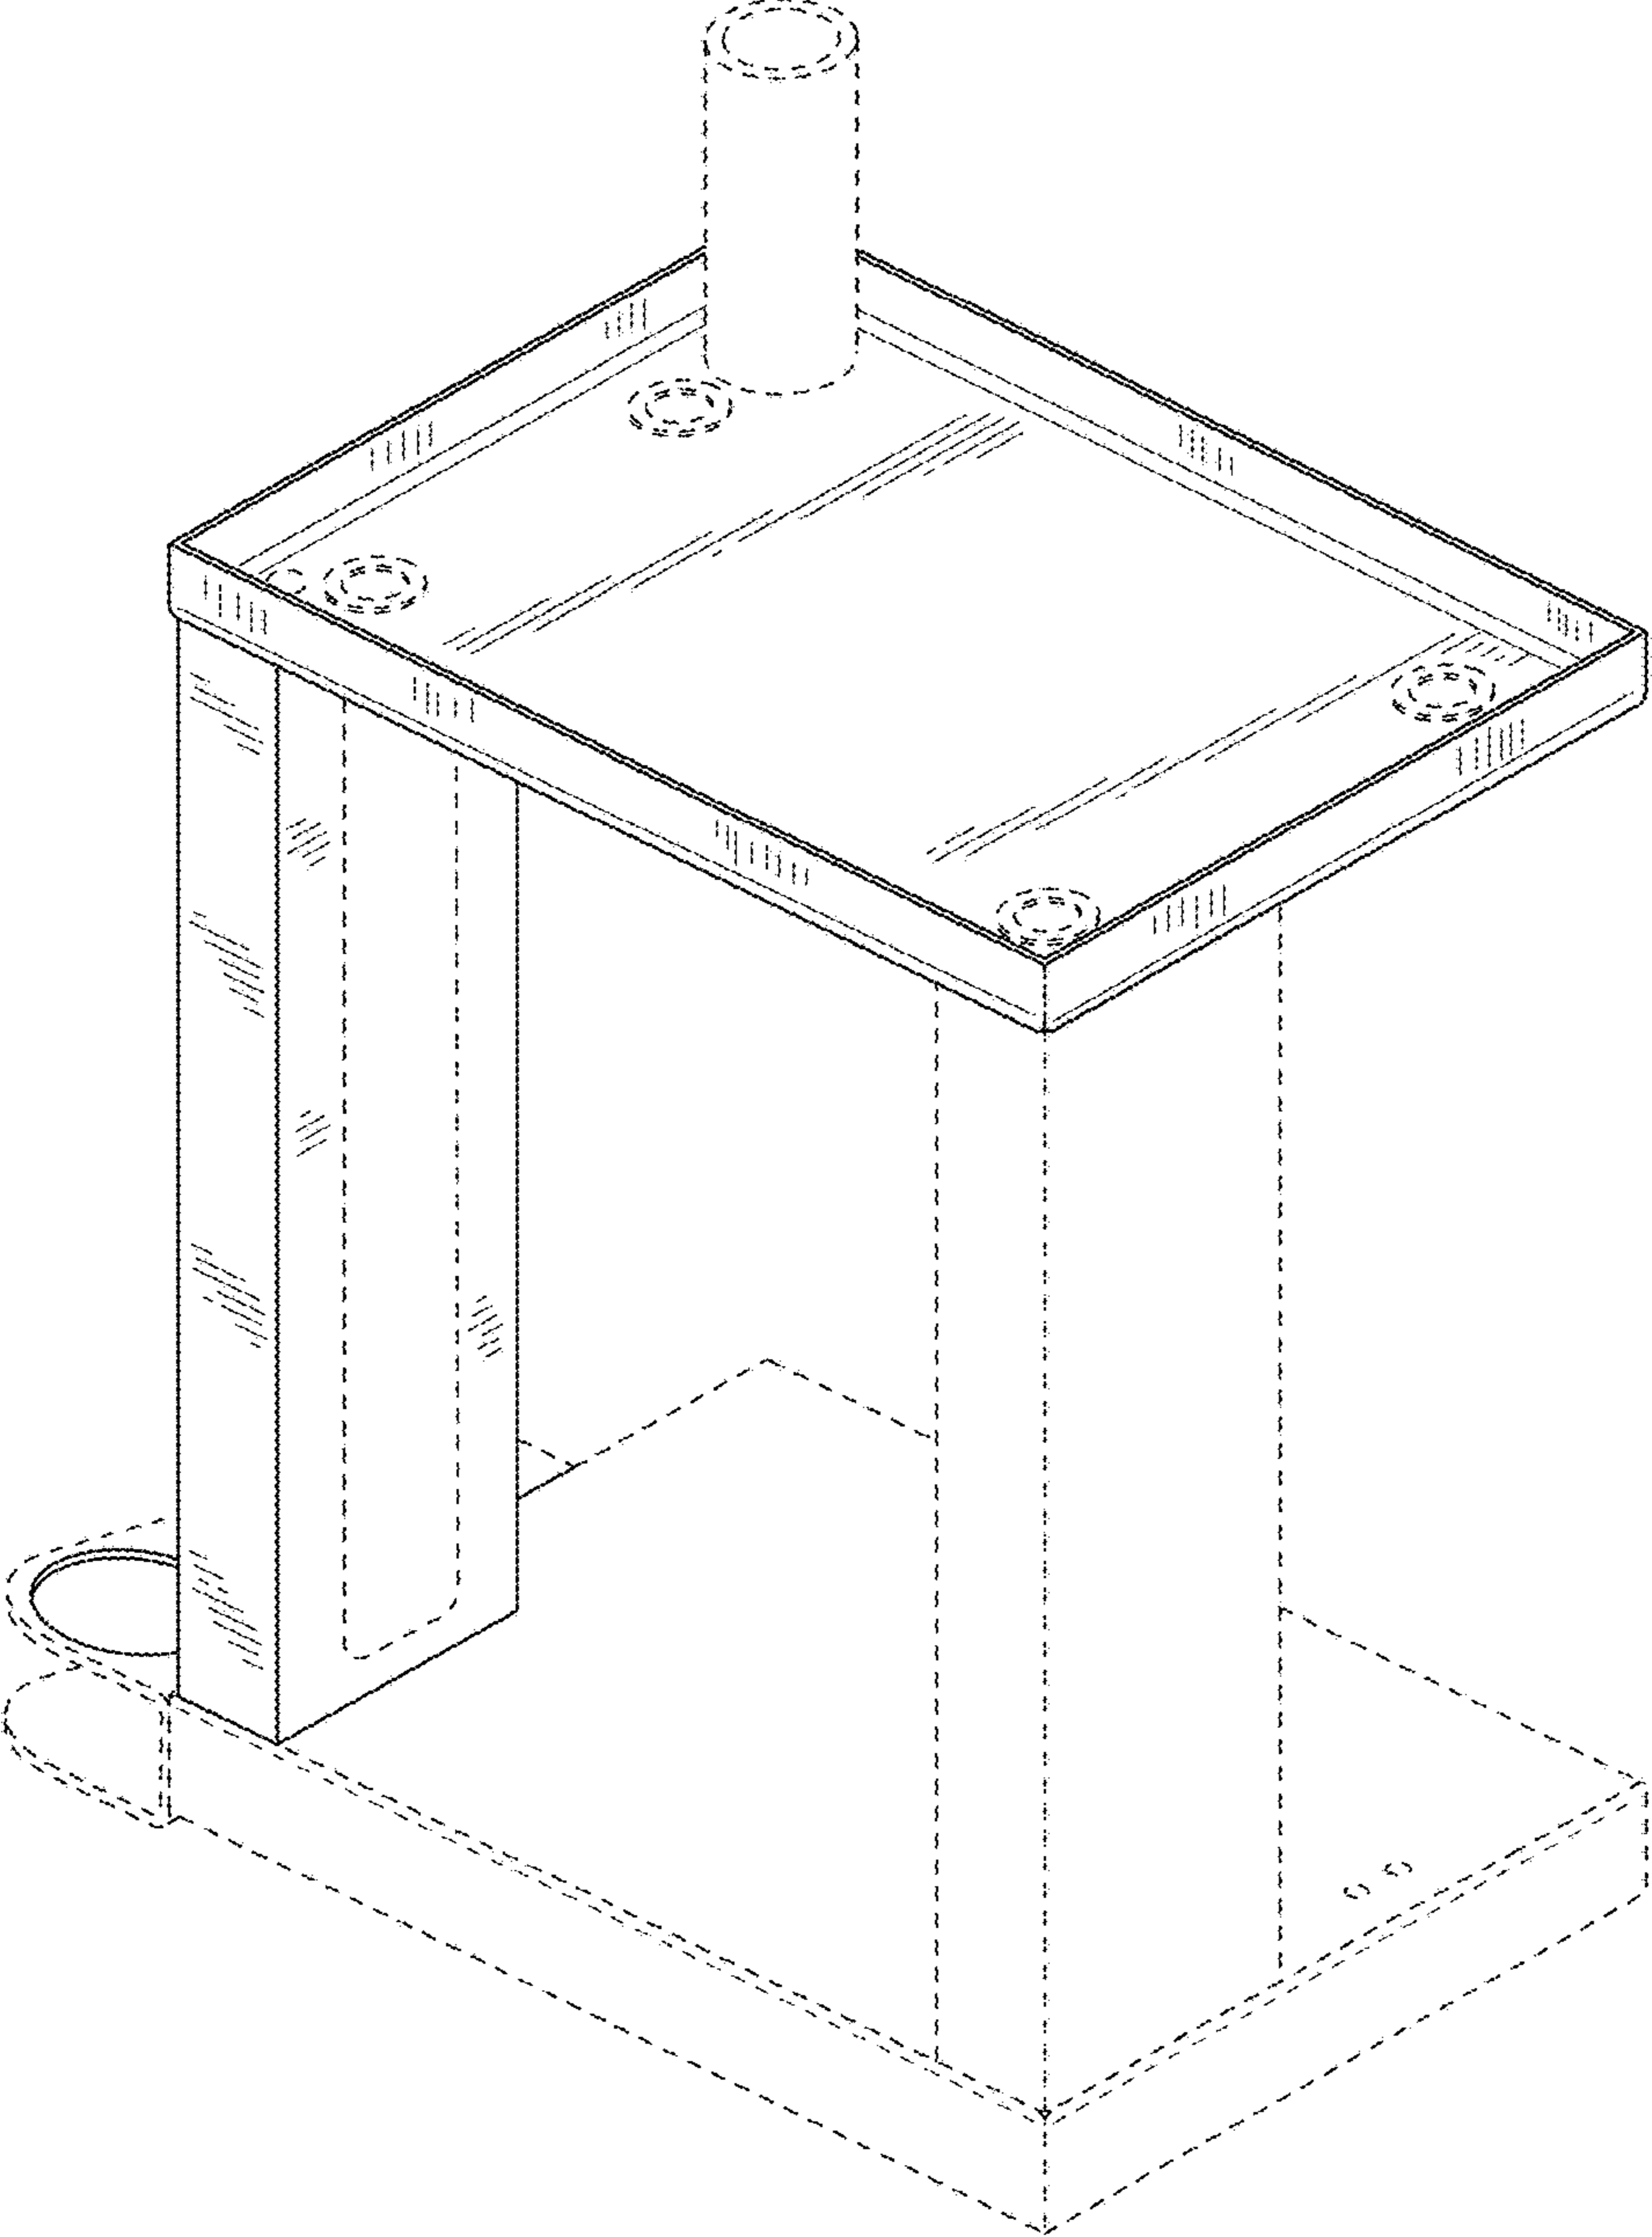


FIG.4

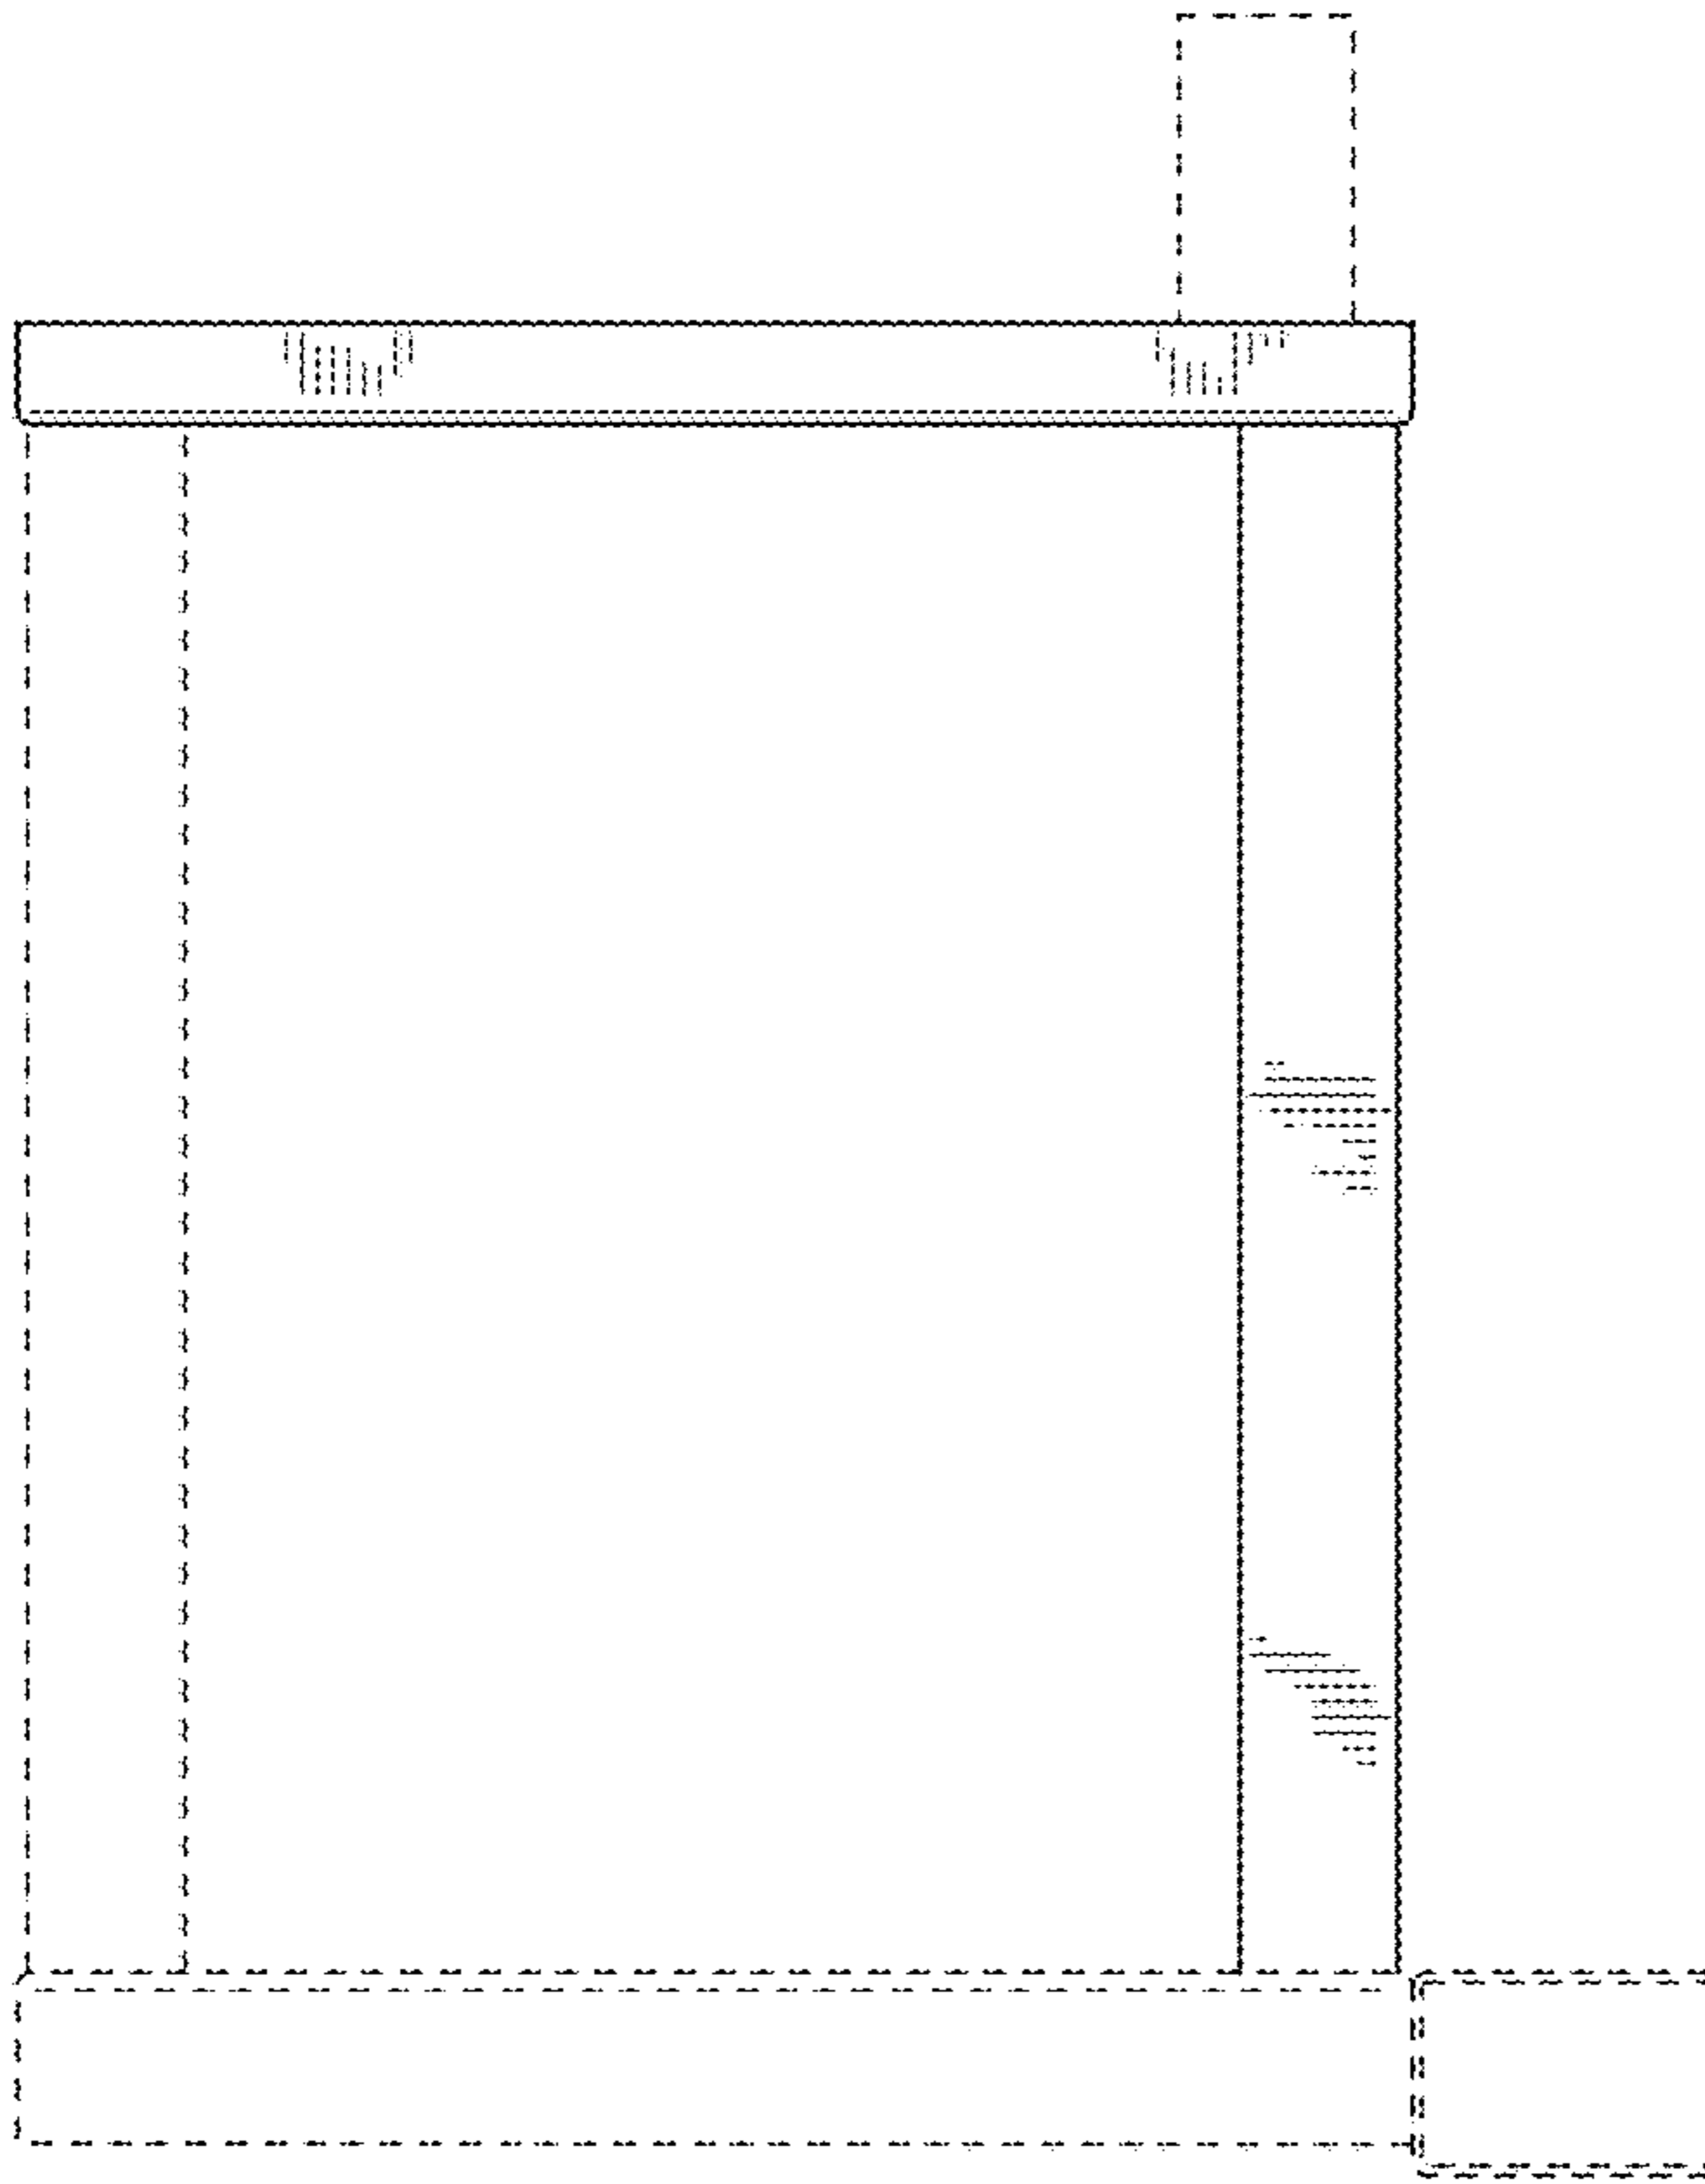


FIG.5

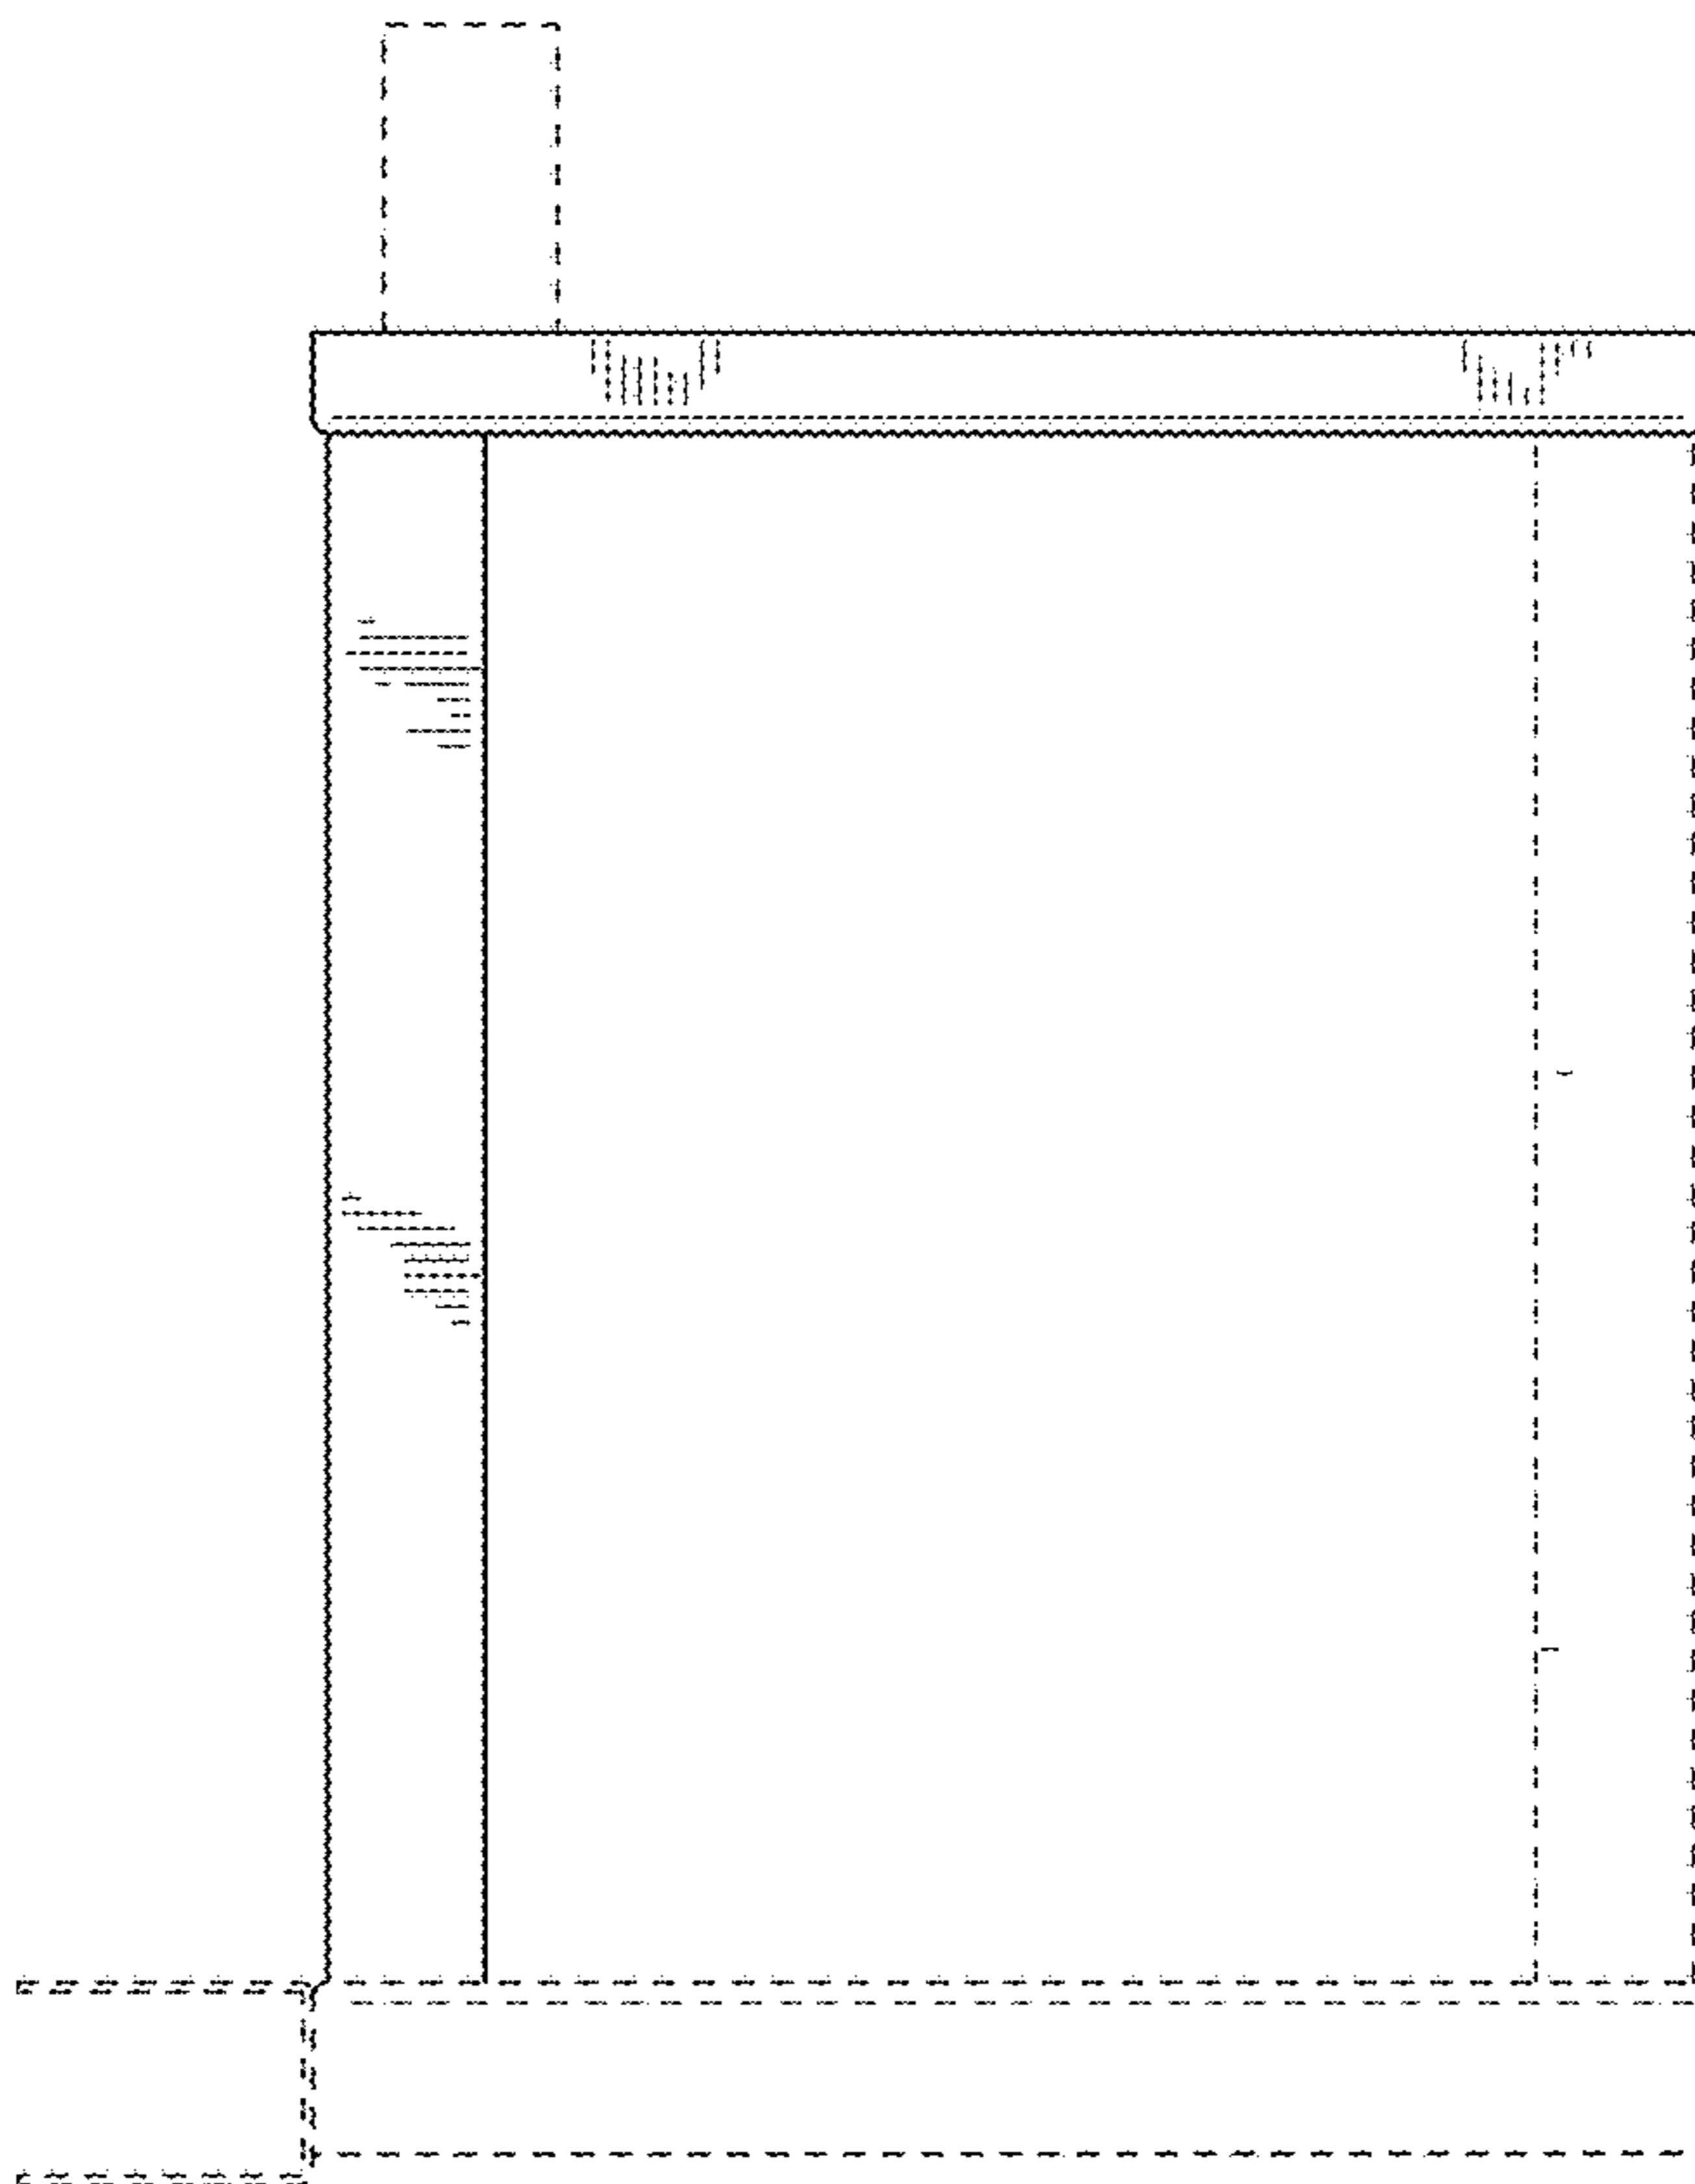


FIG.6

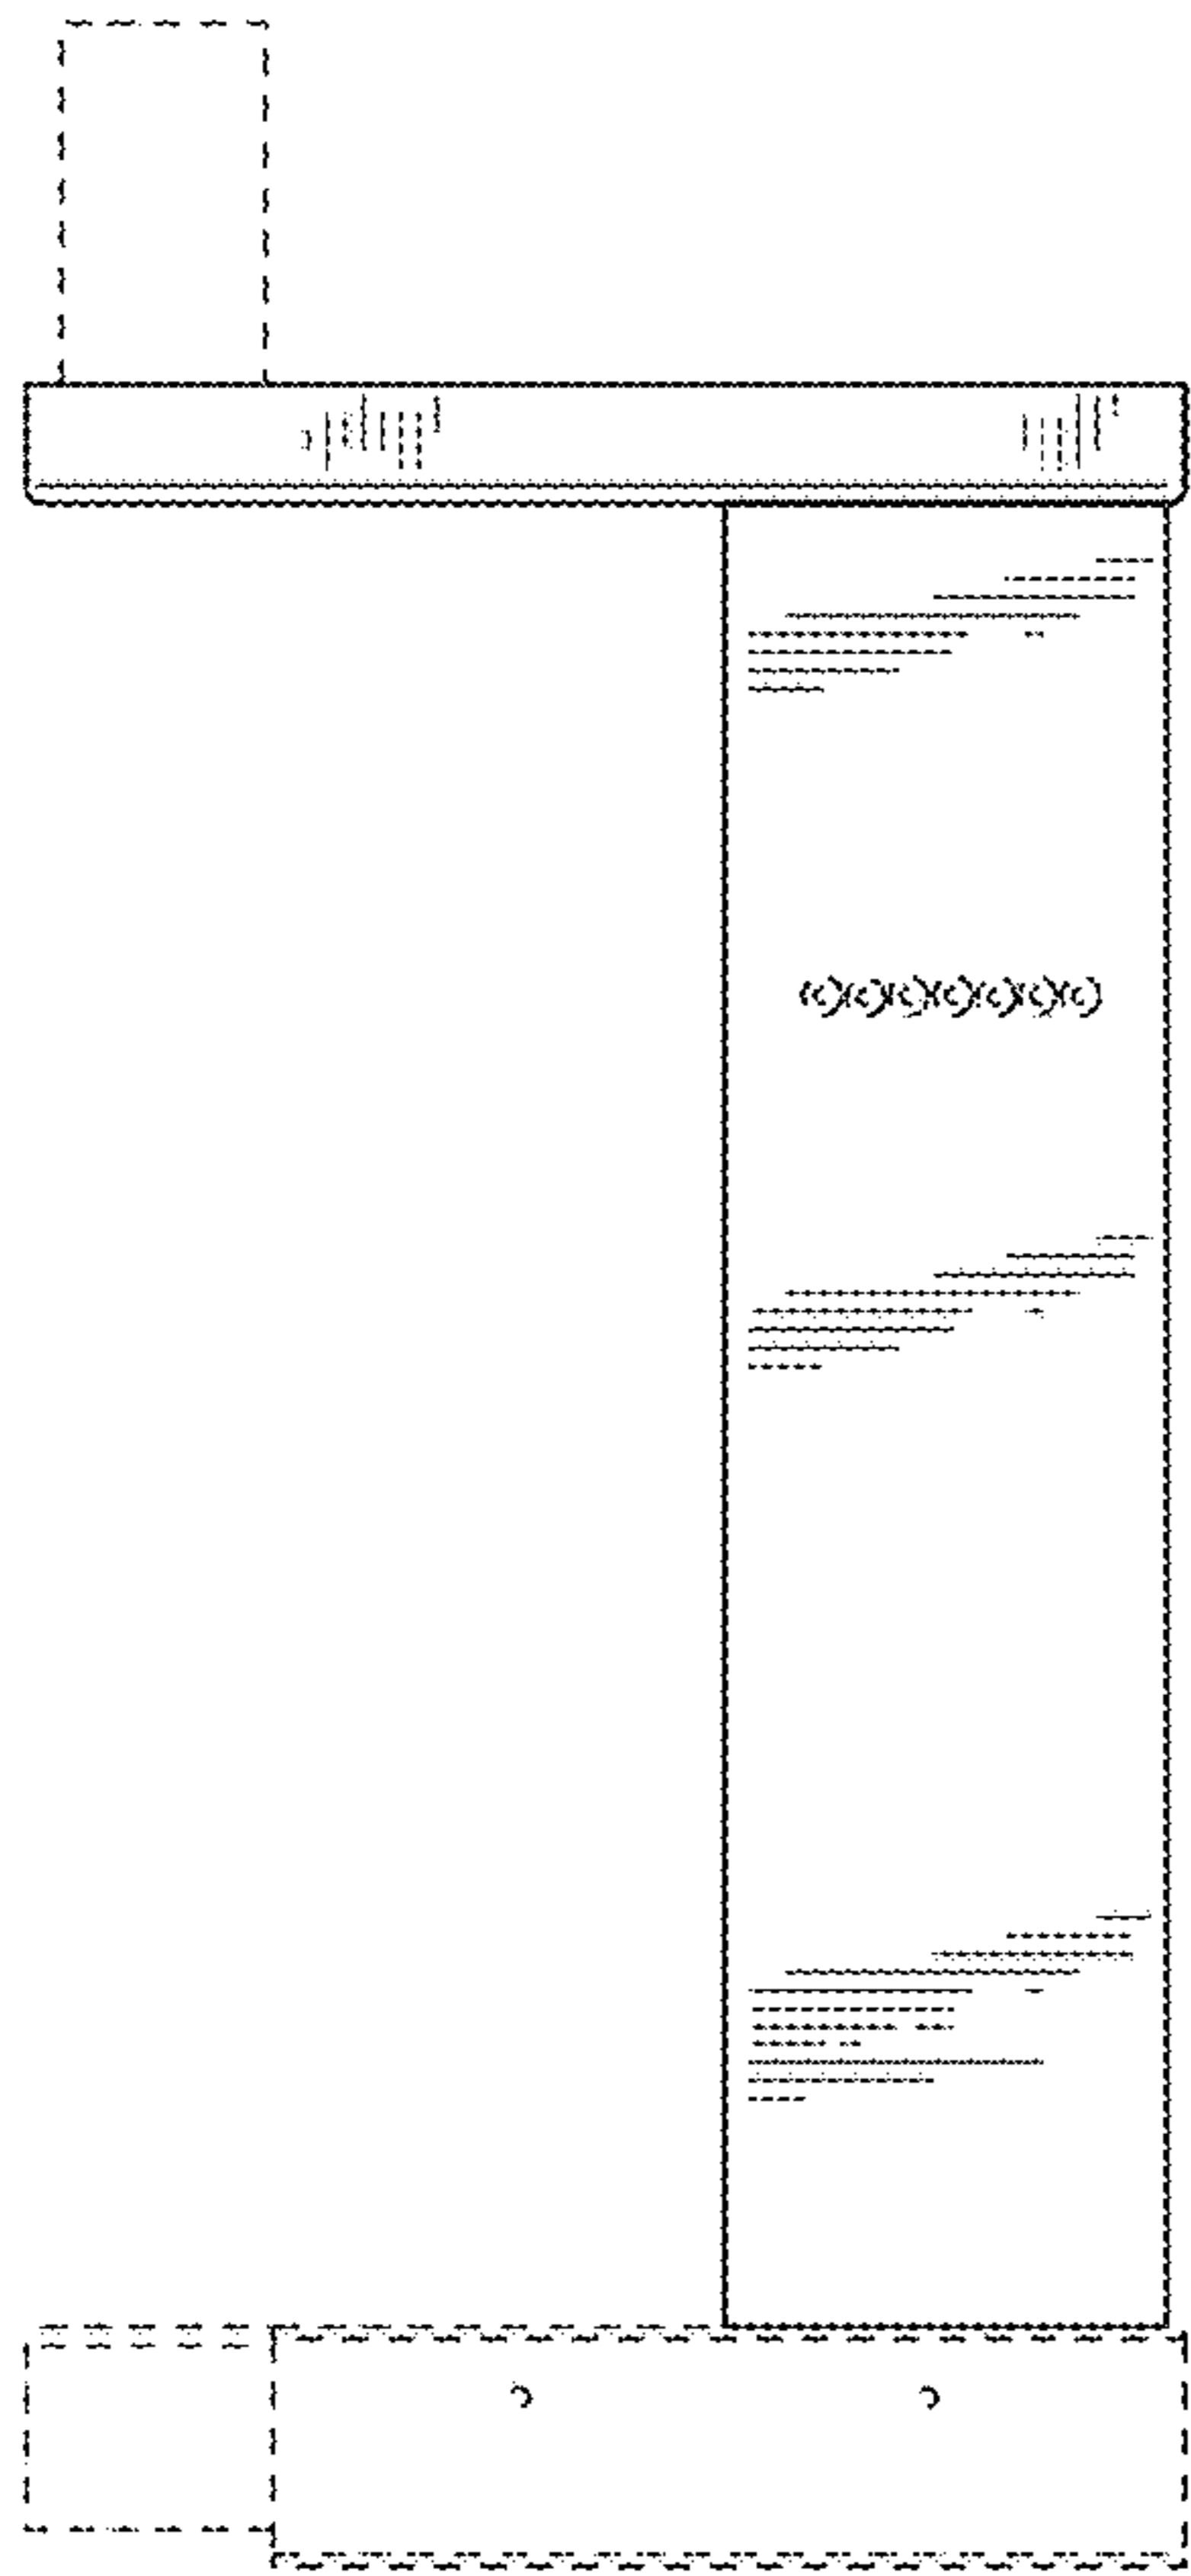


FIG. 7

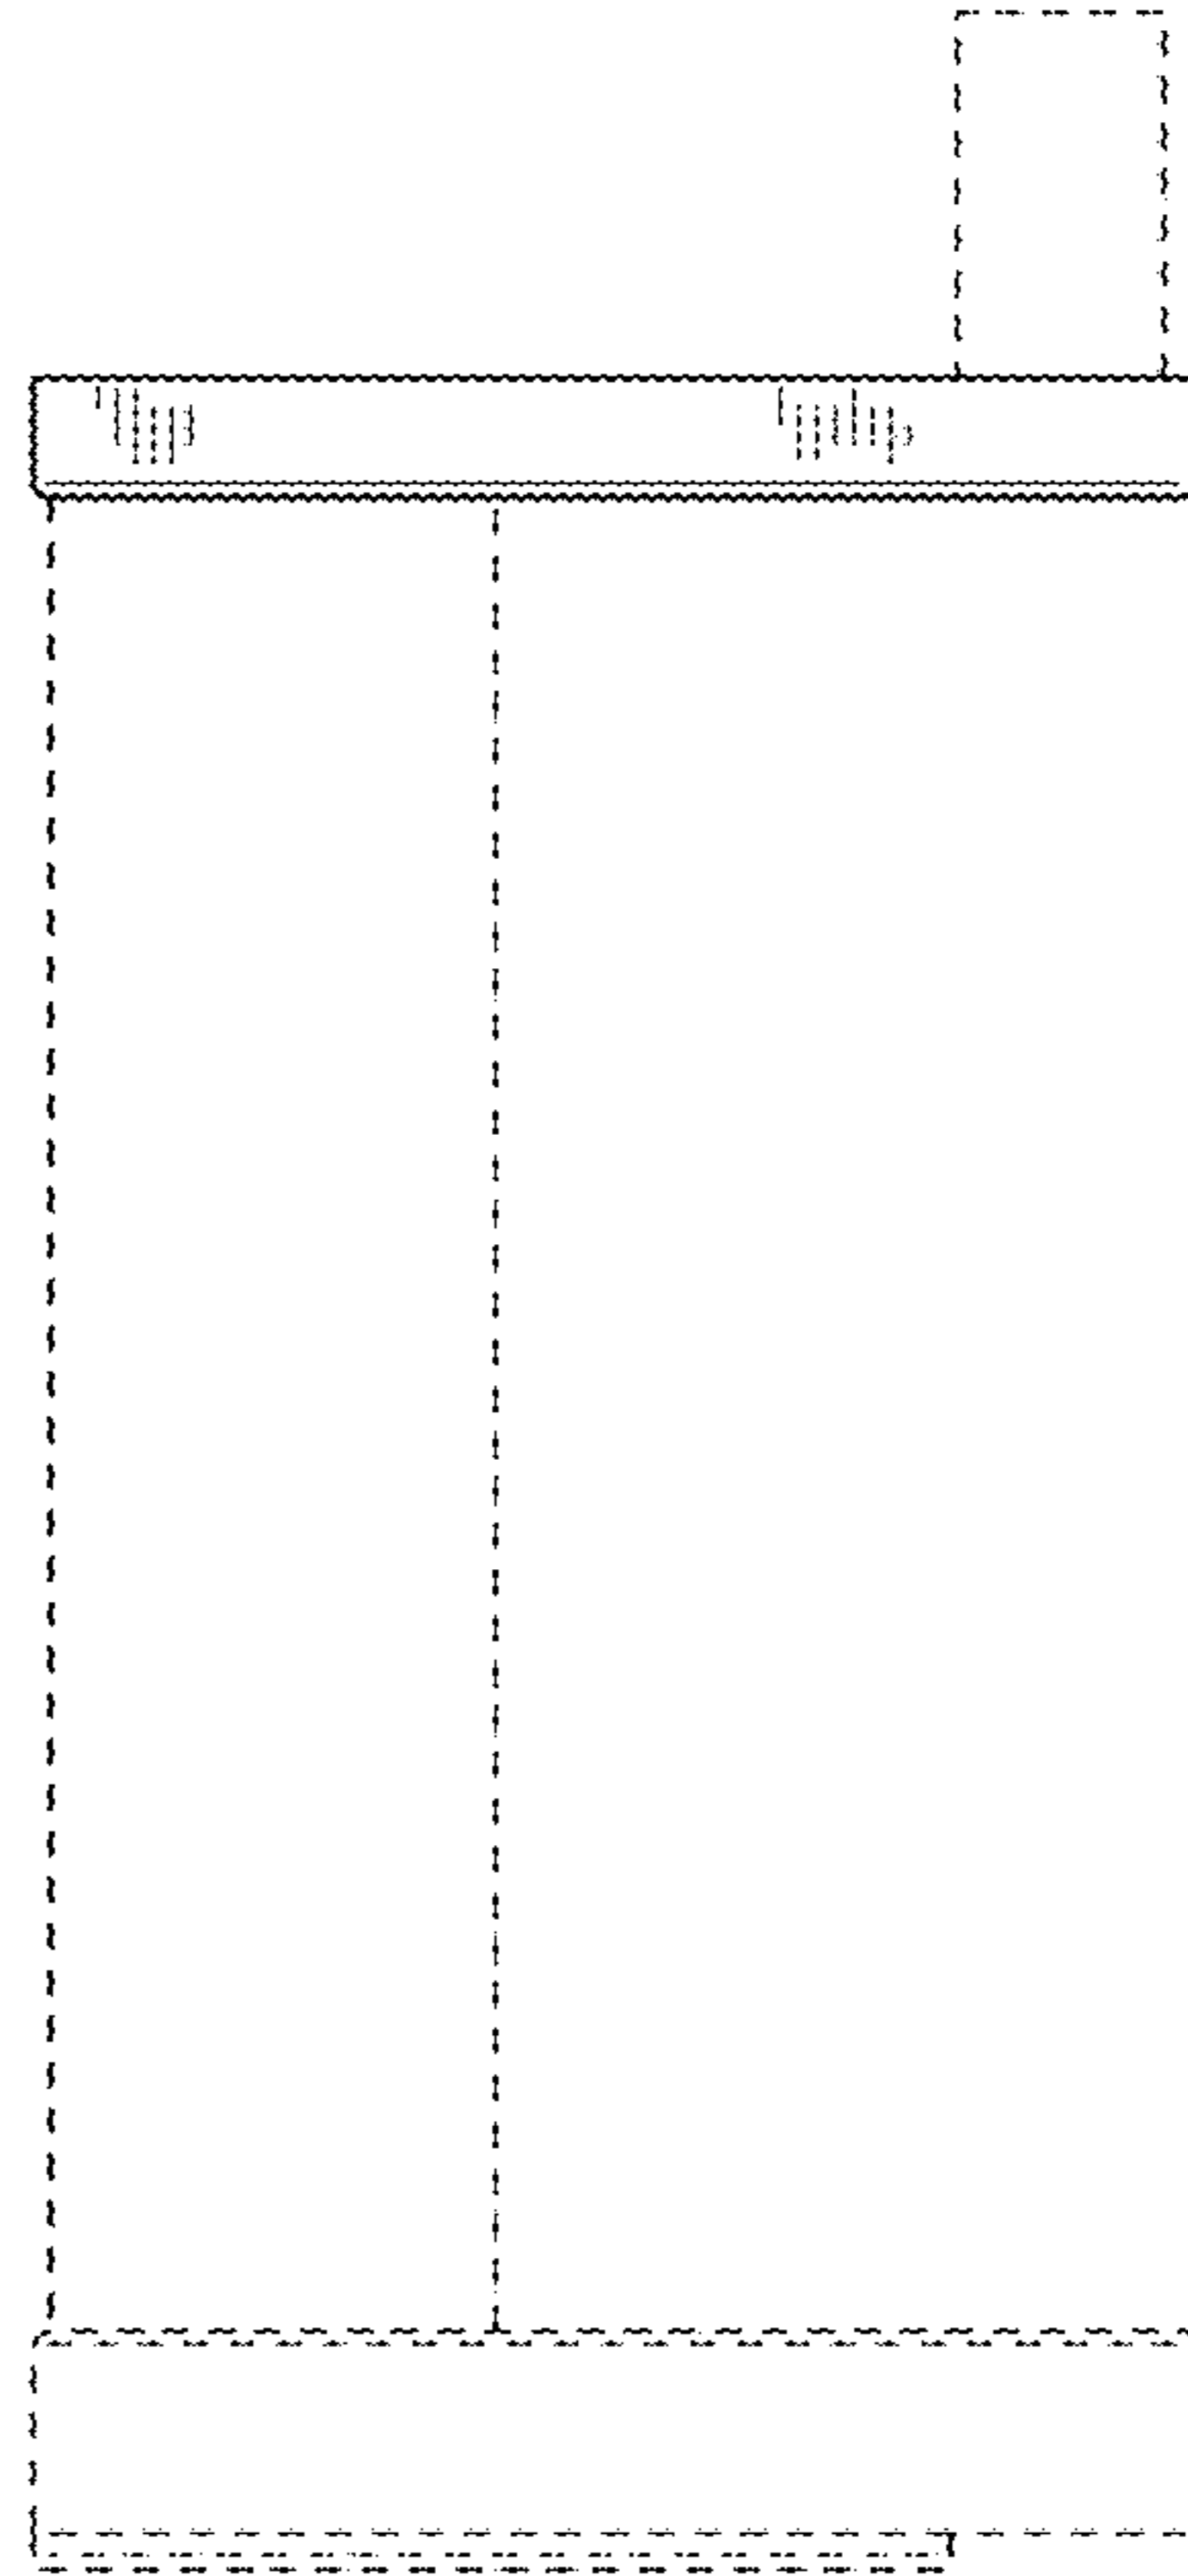


FIG. 8

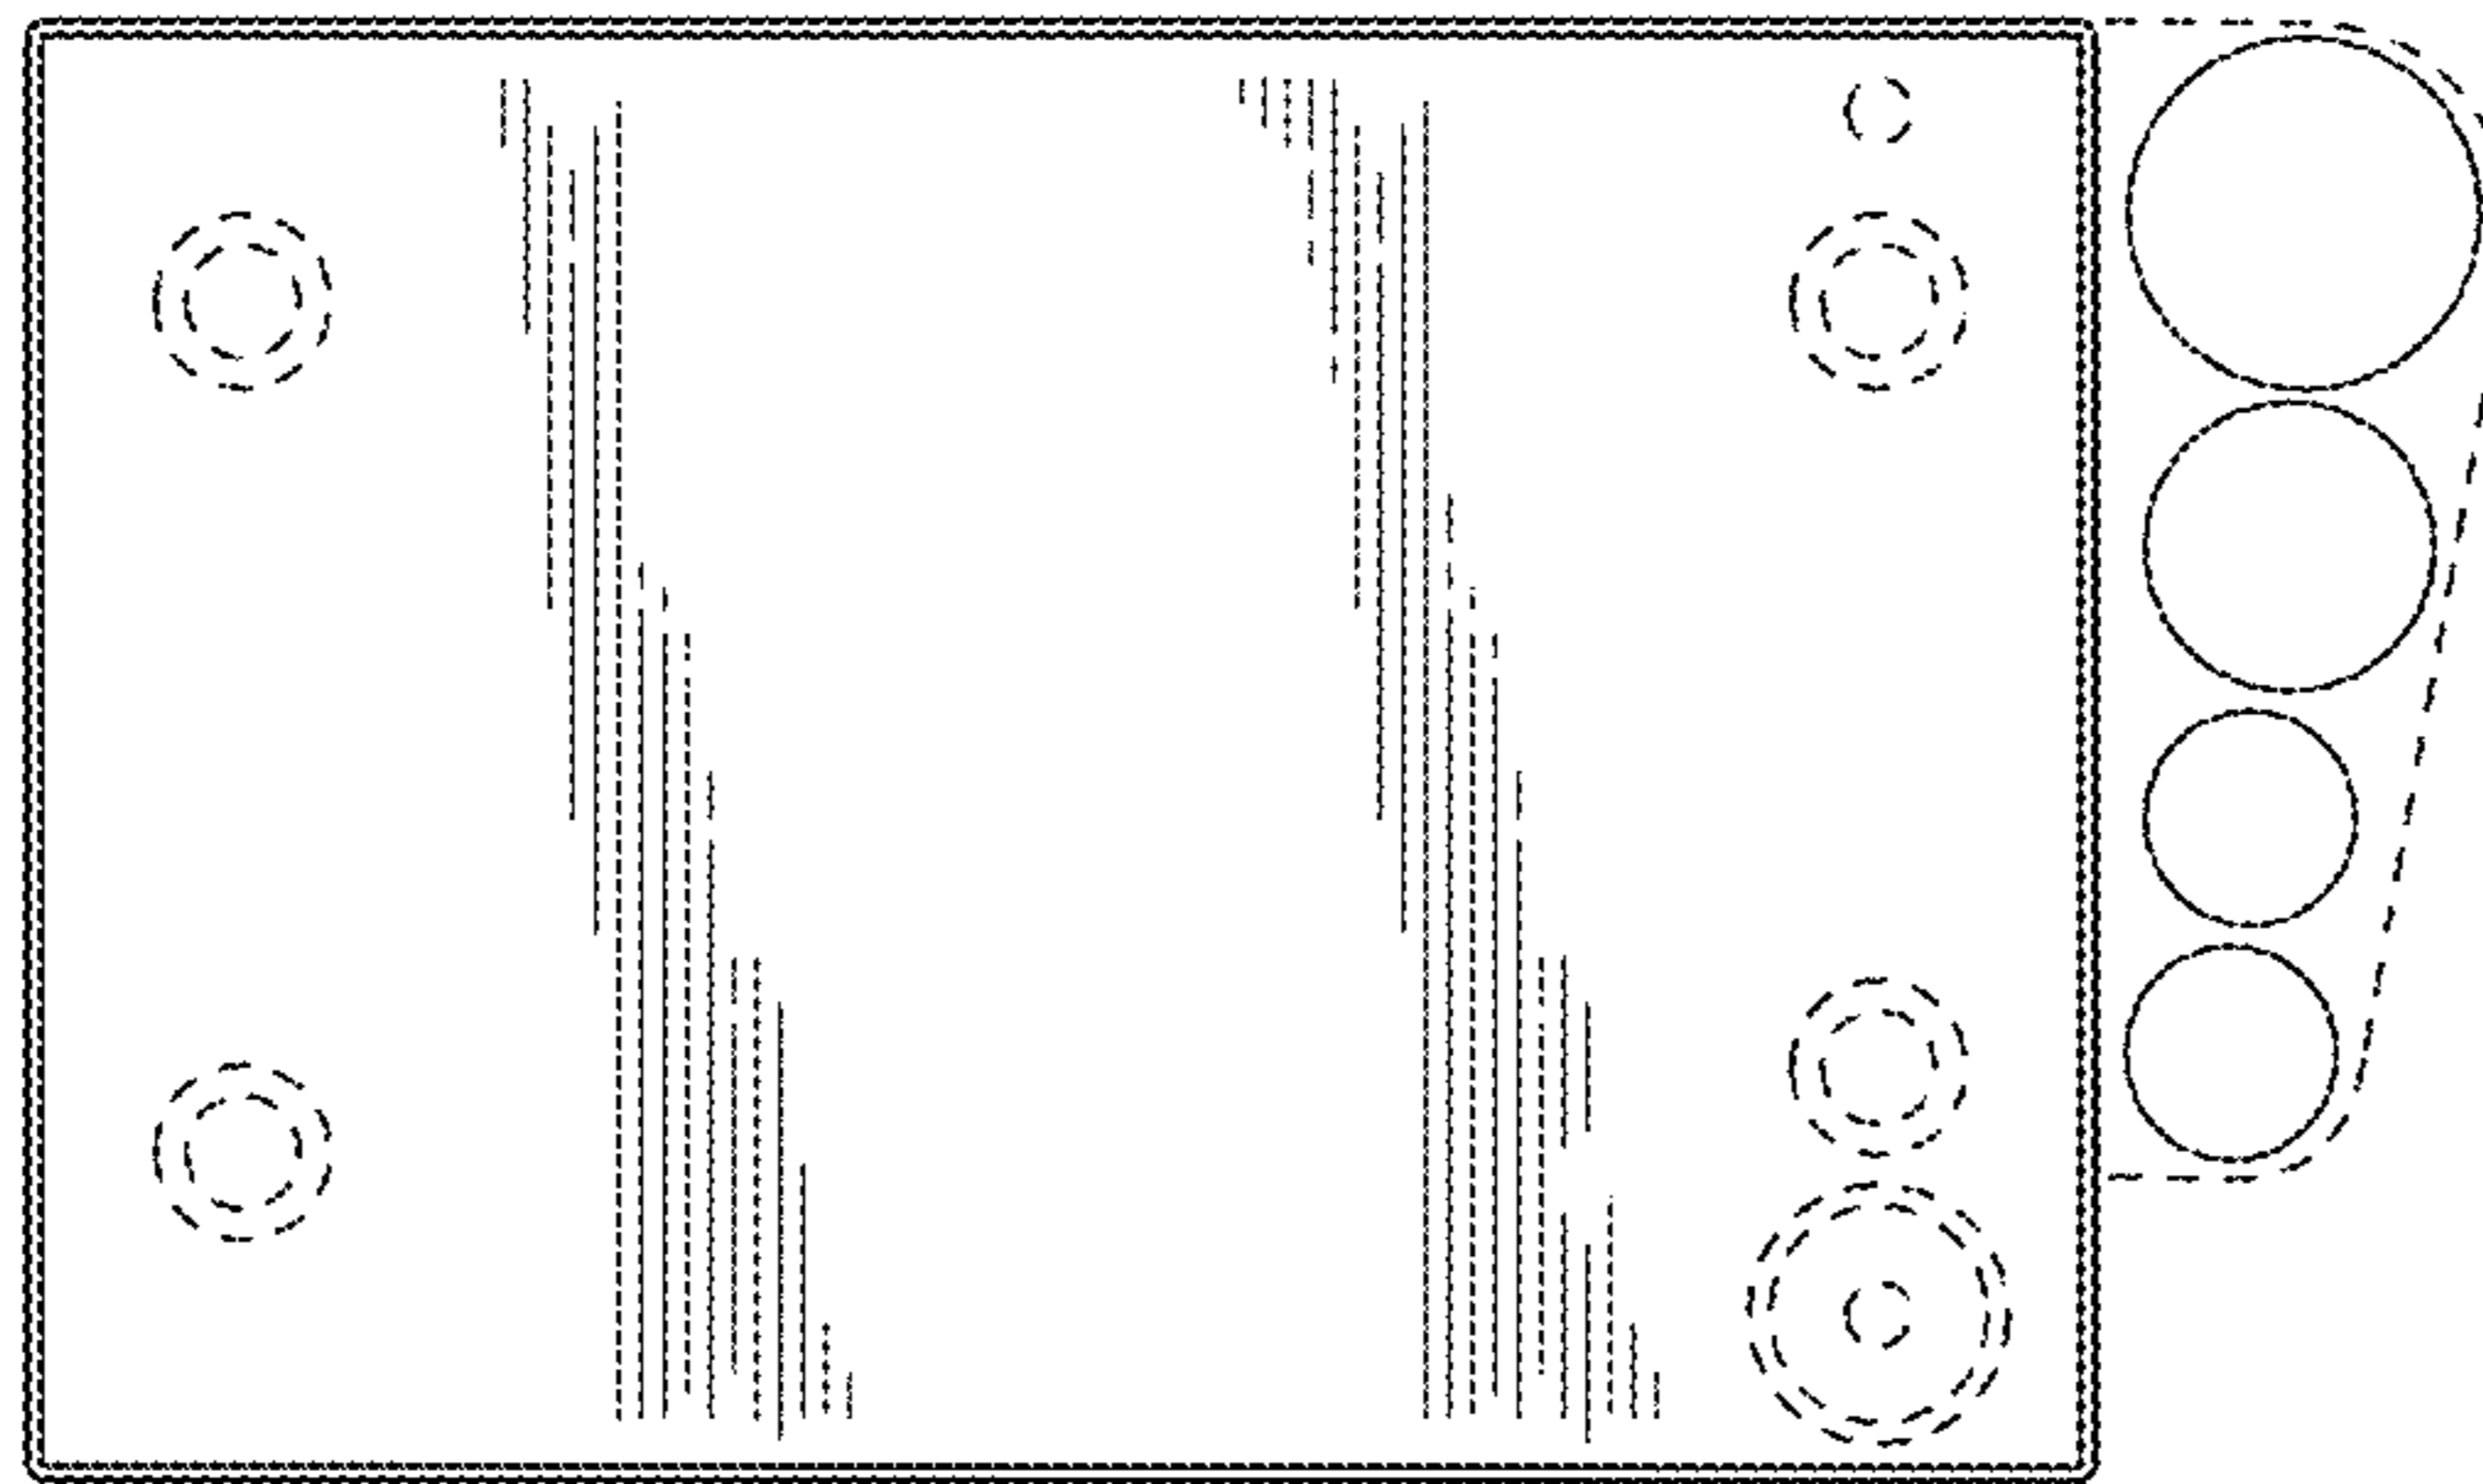


FIG. 9

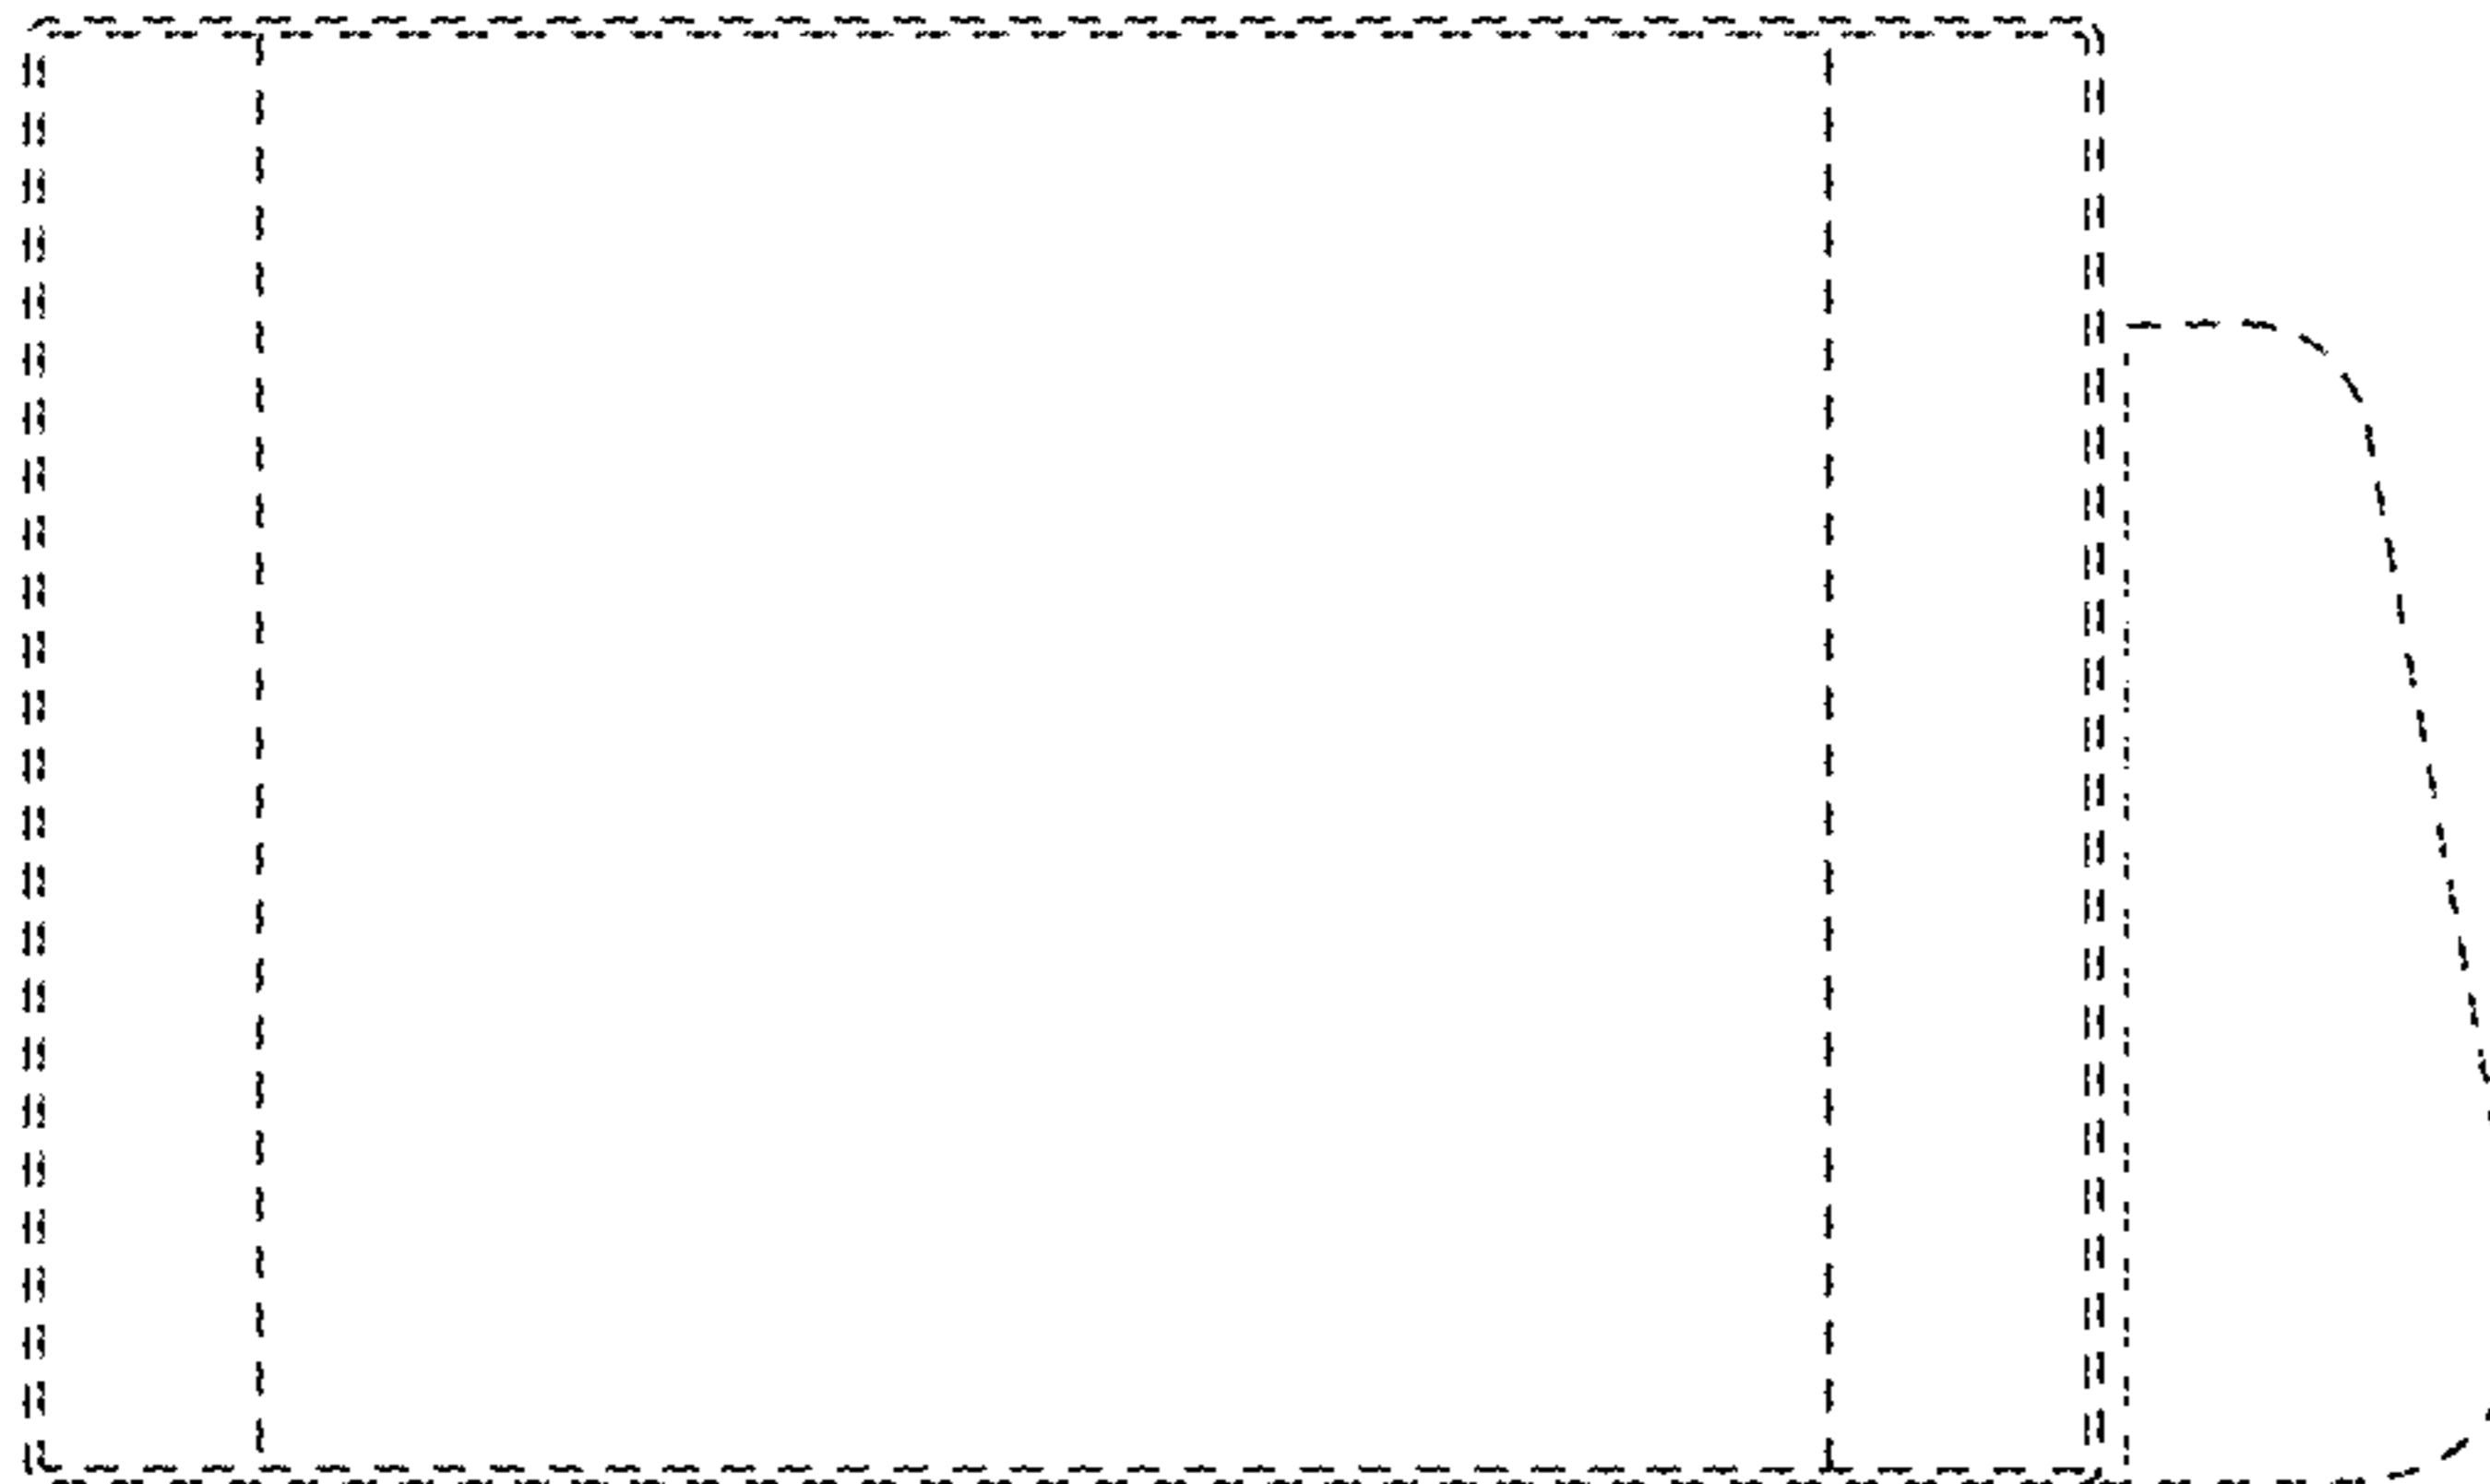


FIG. 10

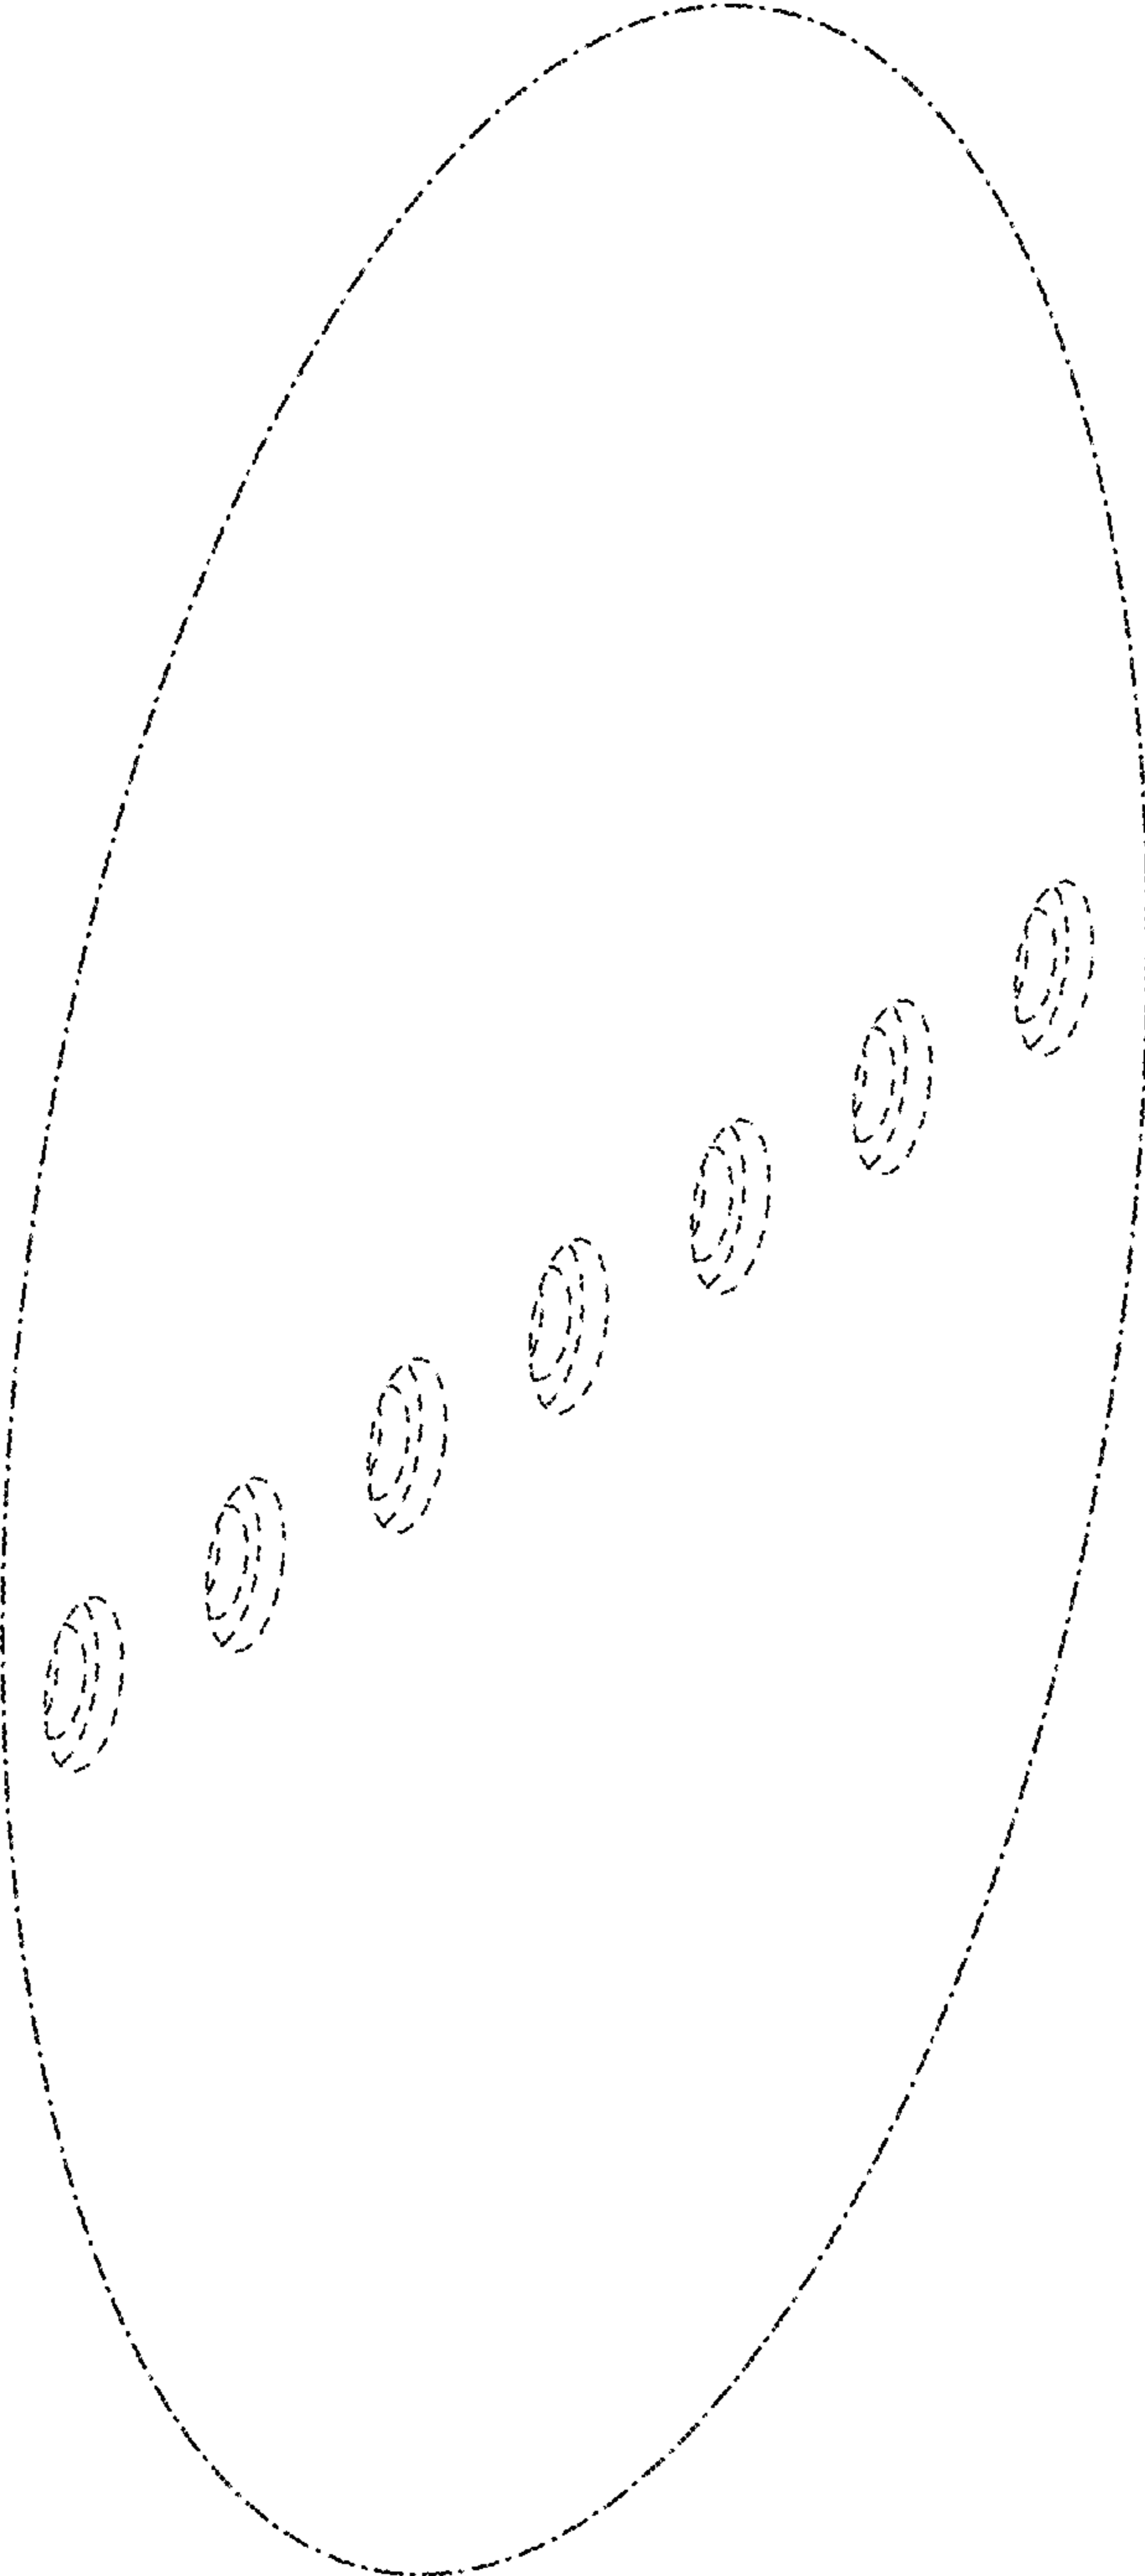


FIG.11