



US00D790690S

(12) **United States Design Patent**  
**Hayamizu**

(10) **Patent No.:** **US D790,690 S**  
(45) **Date of Patent:** **\*\* Jun. 27, 2017**

(54) **HOLDER OF A DETECTION DEVICE FOR ENDOSCOPE**

(71) Applicant: **HOYA CORPORATION**, Tokyo (JP)

(72) Inventor: **Eiji Hayamizu**, Tokyo (JP)

(73) Assignee: **HOYA CORPORATION**, Tokyo (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/568,774**

(22) Filed: **Jun. 21, 2016**

(30) **Foreign Application Priority Data**

Apr. 13, 2016 (JP) ..... 2016-008206

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/128**

(58) **Field of Classification Search**

USPC ..... D24/108, 112, 113-114, 127, 133, 137,  
D24/138, 143, 145, 128; D6/540, 546,  
D6/554, 556; D19/1; D22/108; D8/16,  
D8/19, 300, 303, 372, 314, 394

CPC ..... A47G 7/045; A47G 7/044; A47G 7/047;  
A47G 7/07; A61B 17/00; A61B 18/00;  
A61B 1/0052; A01G 9/12

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D229,744 S \* 1/1974 Oletti ..... D7/407  
D318,608 S \* 7/1991 Schenker ..... D8/371

D327,641 S \* 7/1992 Hoskinson ..... D8/367  
D443,503 S \* 6/2001 Harvey ..... D8/367  
D613,589 S \* 4/2010 Goodman ..... D8/367  
D618,023 S \* 6/2010 Goodman ..... D6/513  
D628,410 S \* 12/2010 Parisi ..... D6/526  
D715,627 S \* 10/2014 Pan ..... D8/371  
D716,641 S \* 11/2014 Goodman ..... D8/371  
D727,718 S \* 4/2015 McLaren Hall ..... D8/373  
D770,190 S \* 11/2016 Wirth ..... D6/328  
D771,464 S \* 11/2016 Loso ..... D8/71

\* cited by examiner

*Primary Examiner* — Manpreet Matharu

*Assistant Examiner* — Yolanda Robinson

(74) *Attorney, Agent, or Firm* — Cantor Colburn LLP

(57) **CLAIM**

The ornamental design for a holder of a detection device for endoscope, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a holder of a detection device for endoscope showing my new design;  
FIG. 2 is a rear perspective view thereof;  
FIG. 3 is a front view thereof;  
FIG. 4 is a rear view thereof;  
FIG. 5 is a top plan view thereof;  
FIG. 6 is a bottom plan view thereof; and,  
FIG. 7 is a right side view thereof, the left side view being a mirror image of FIG. 7.

The broken lines illustrate portions of the holder of a detection device for endoscope and form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

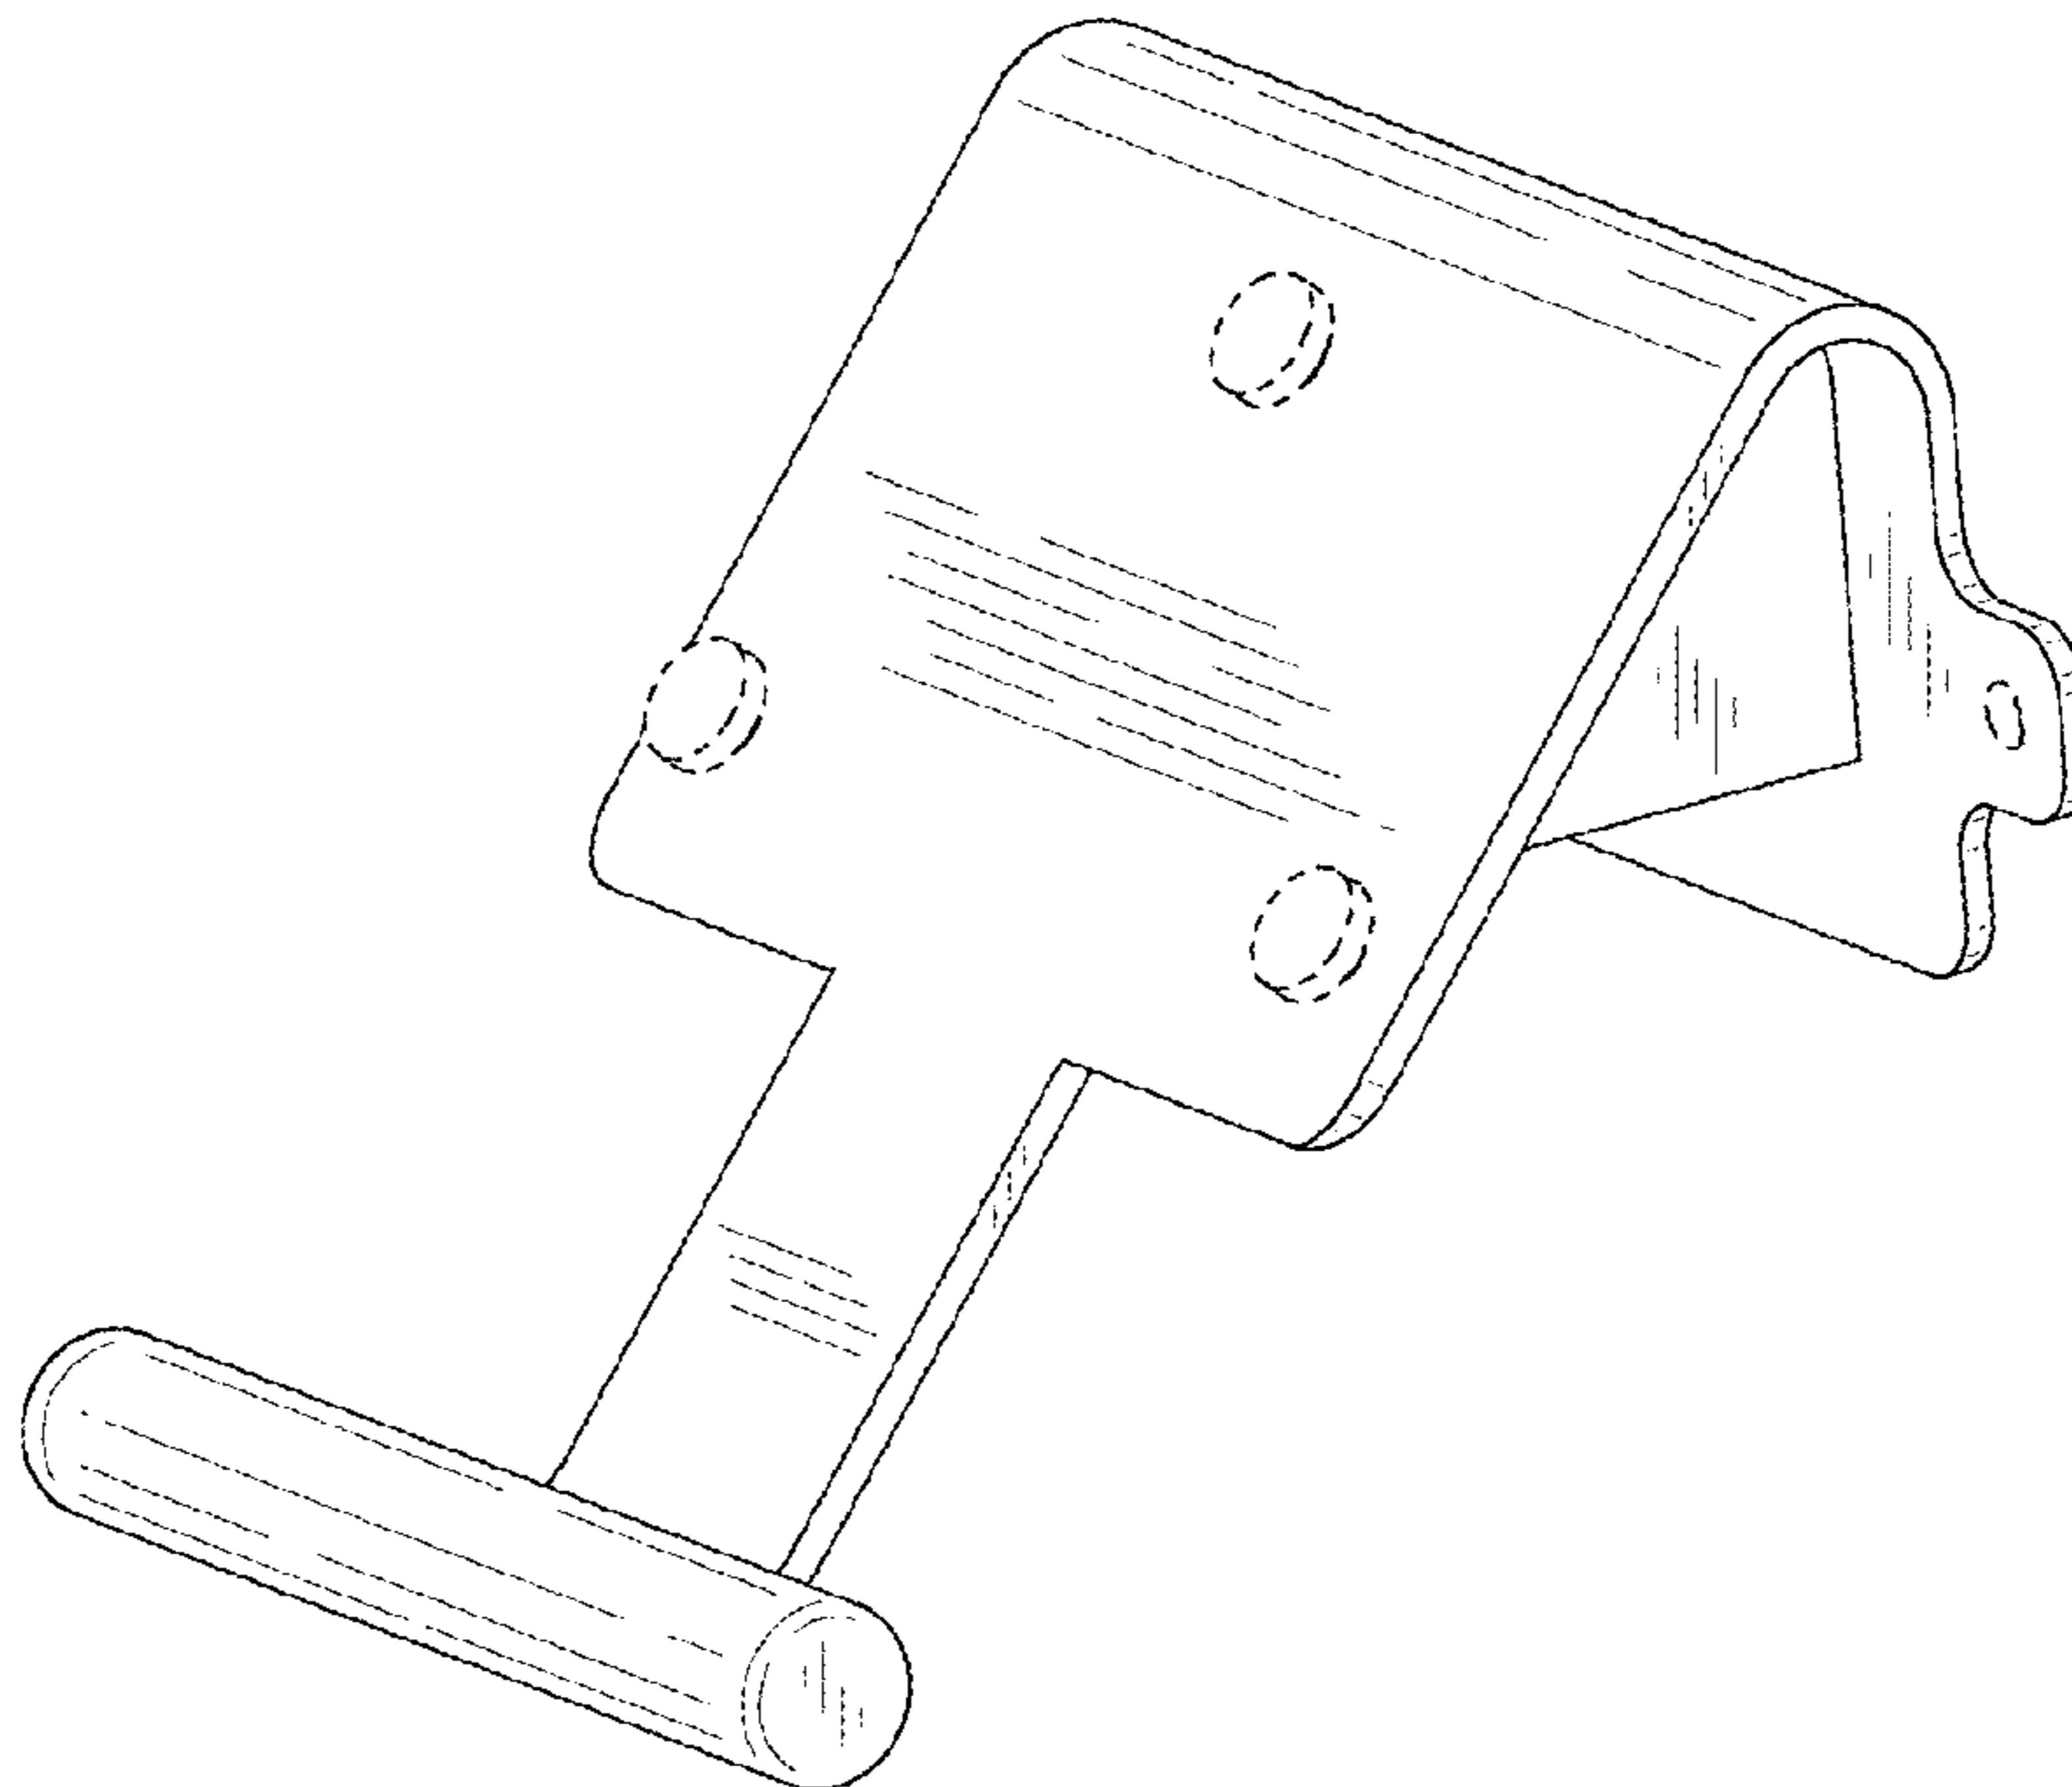


Fig.1

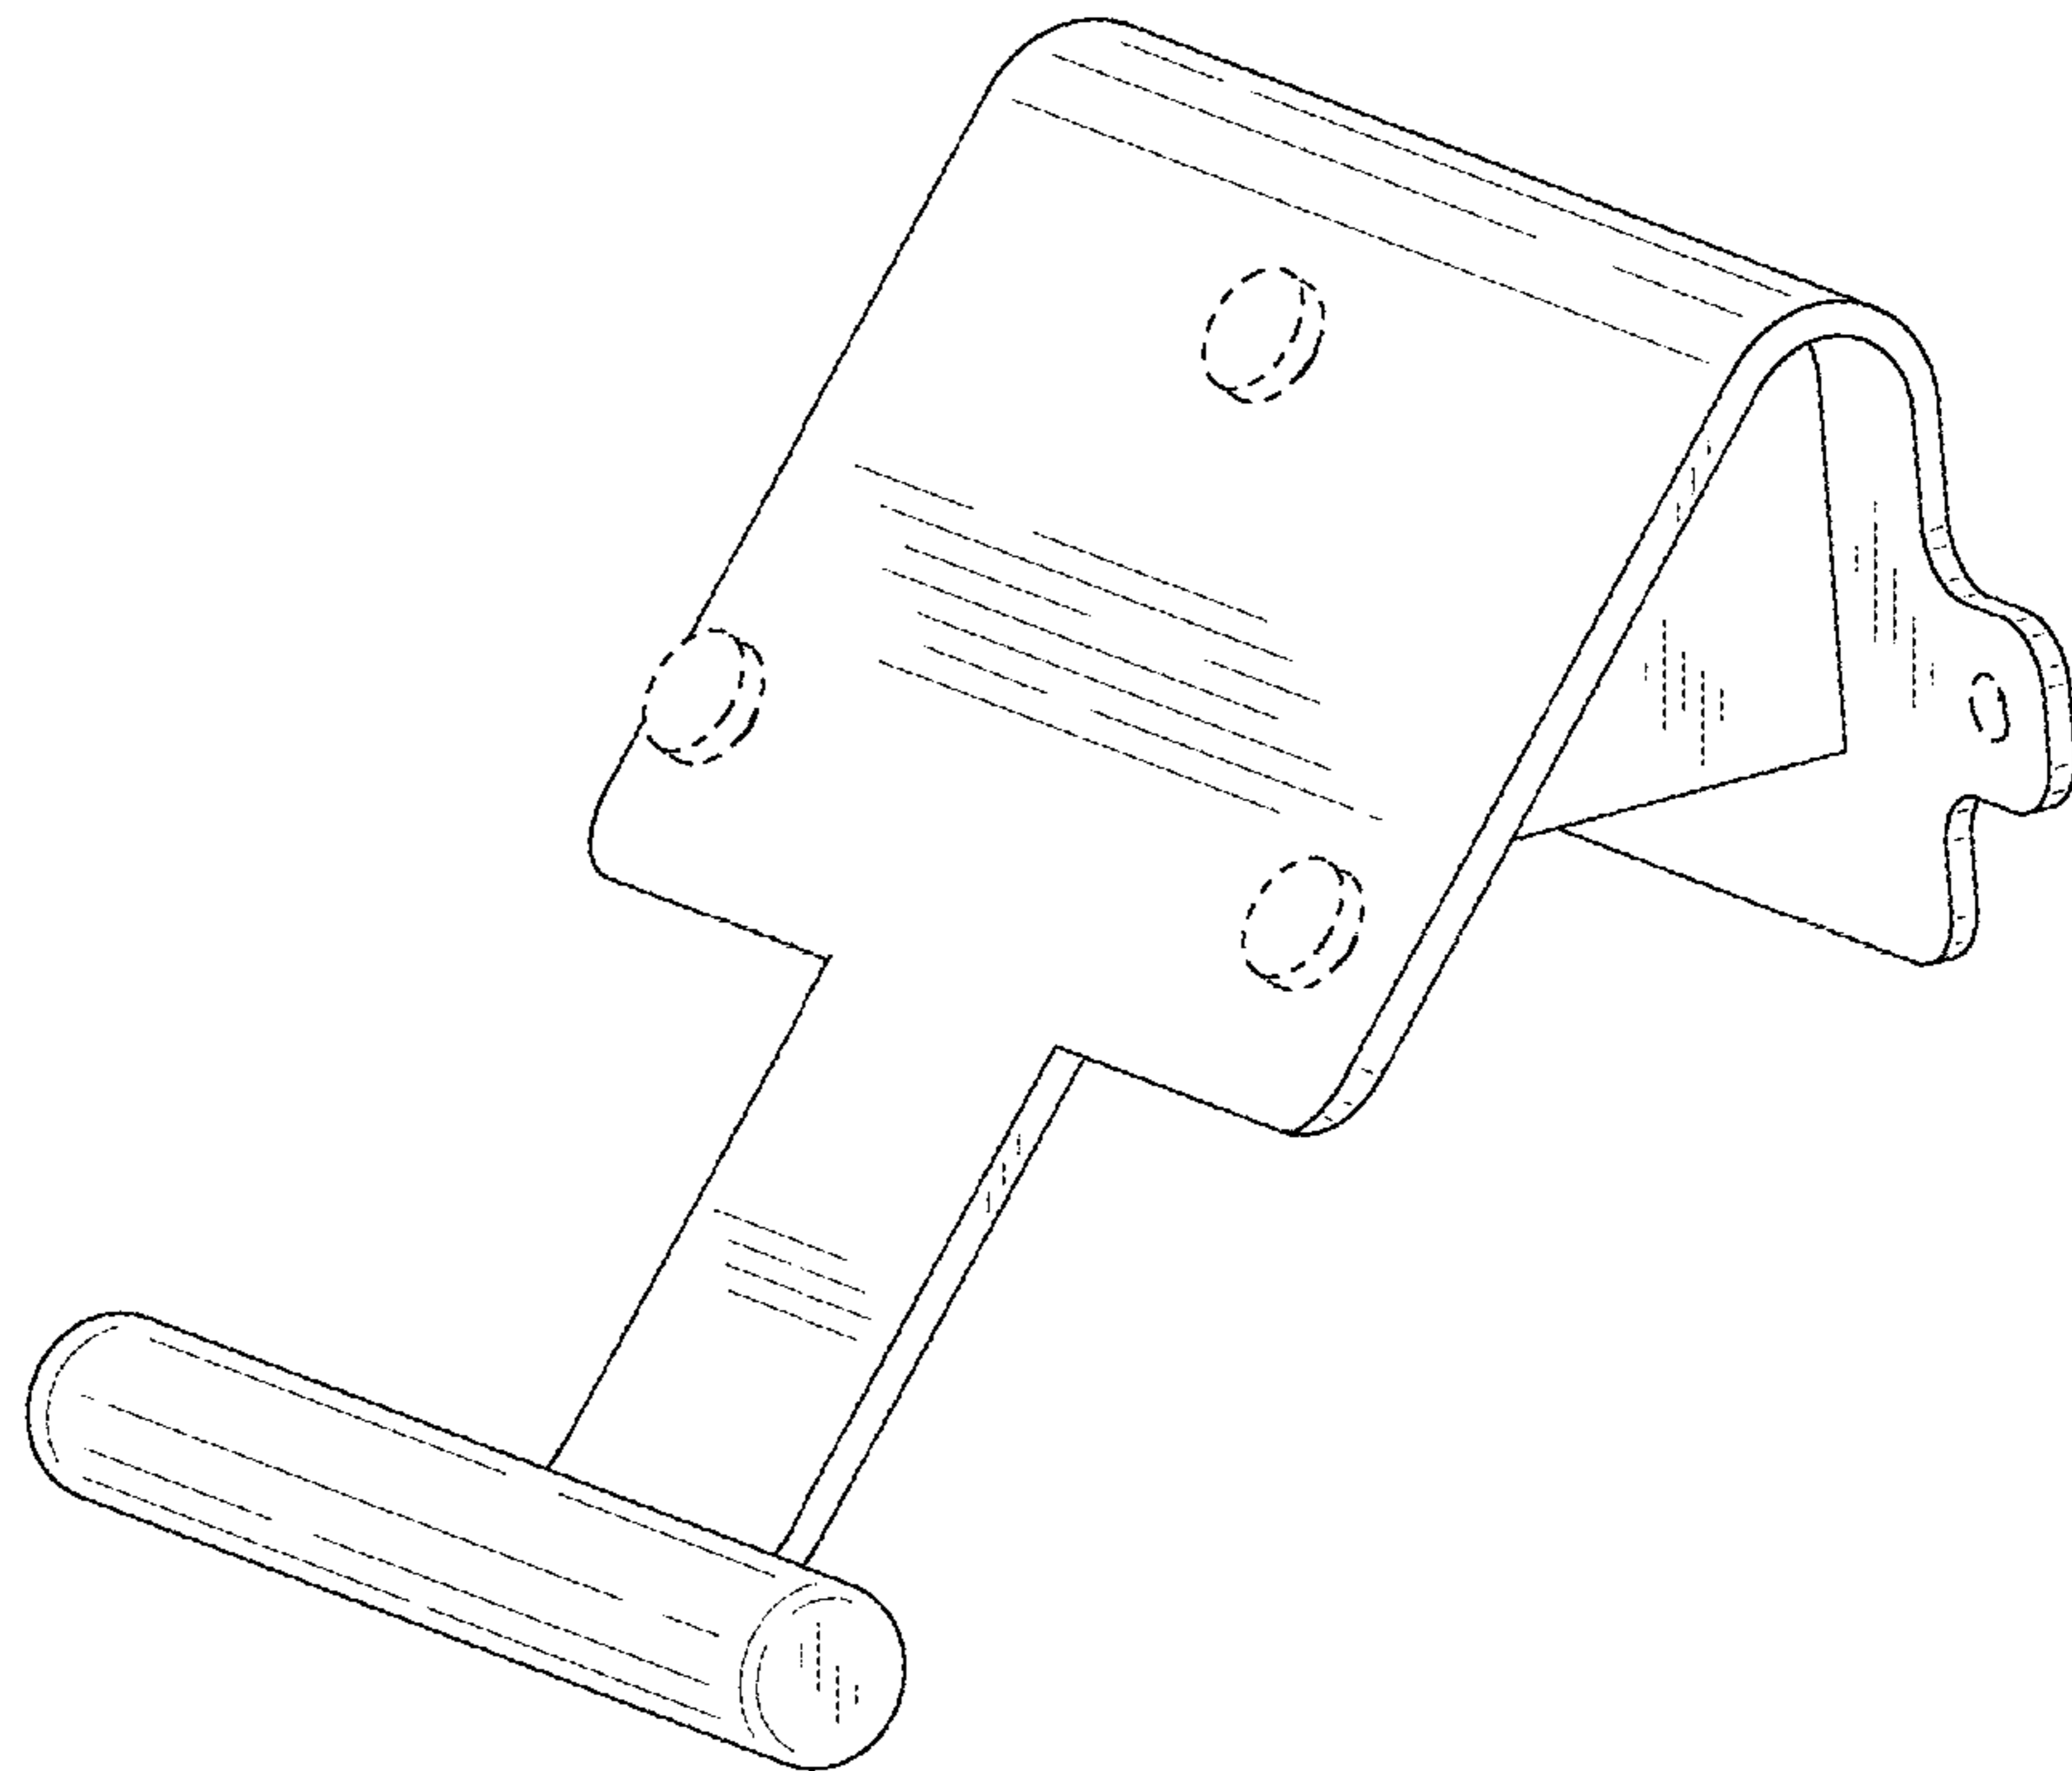


Fig.2

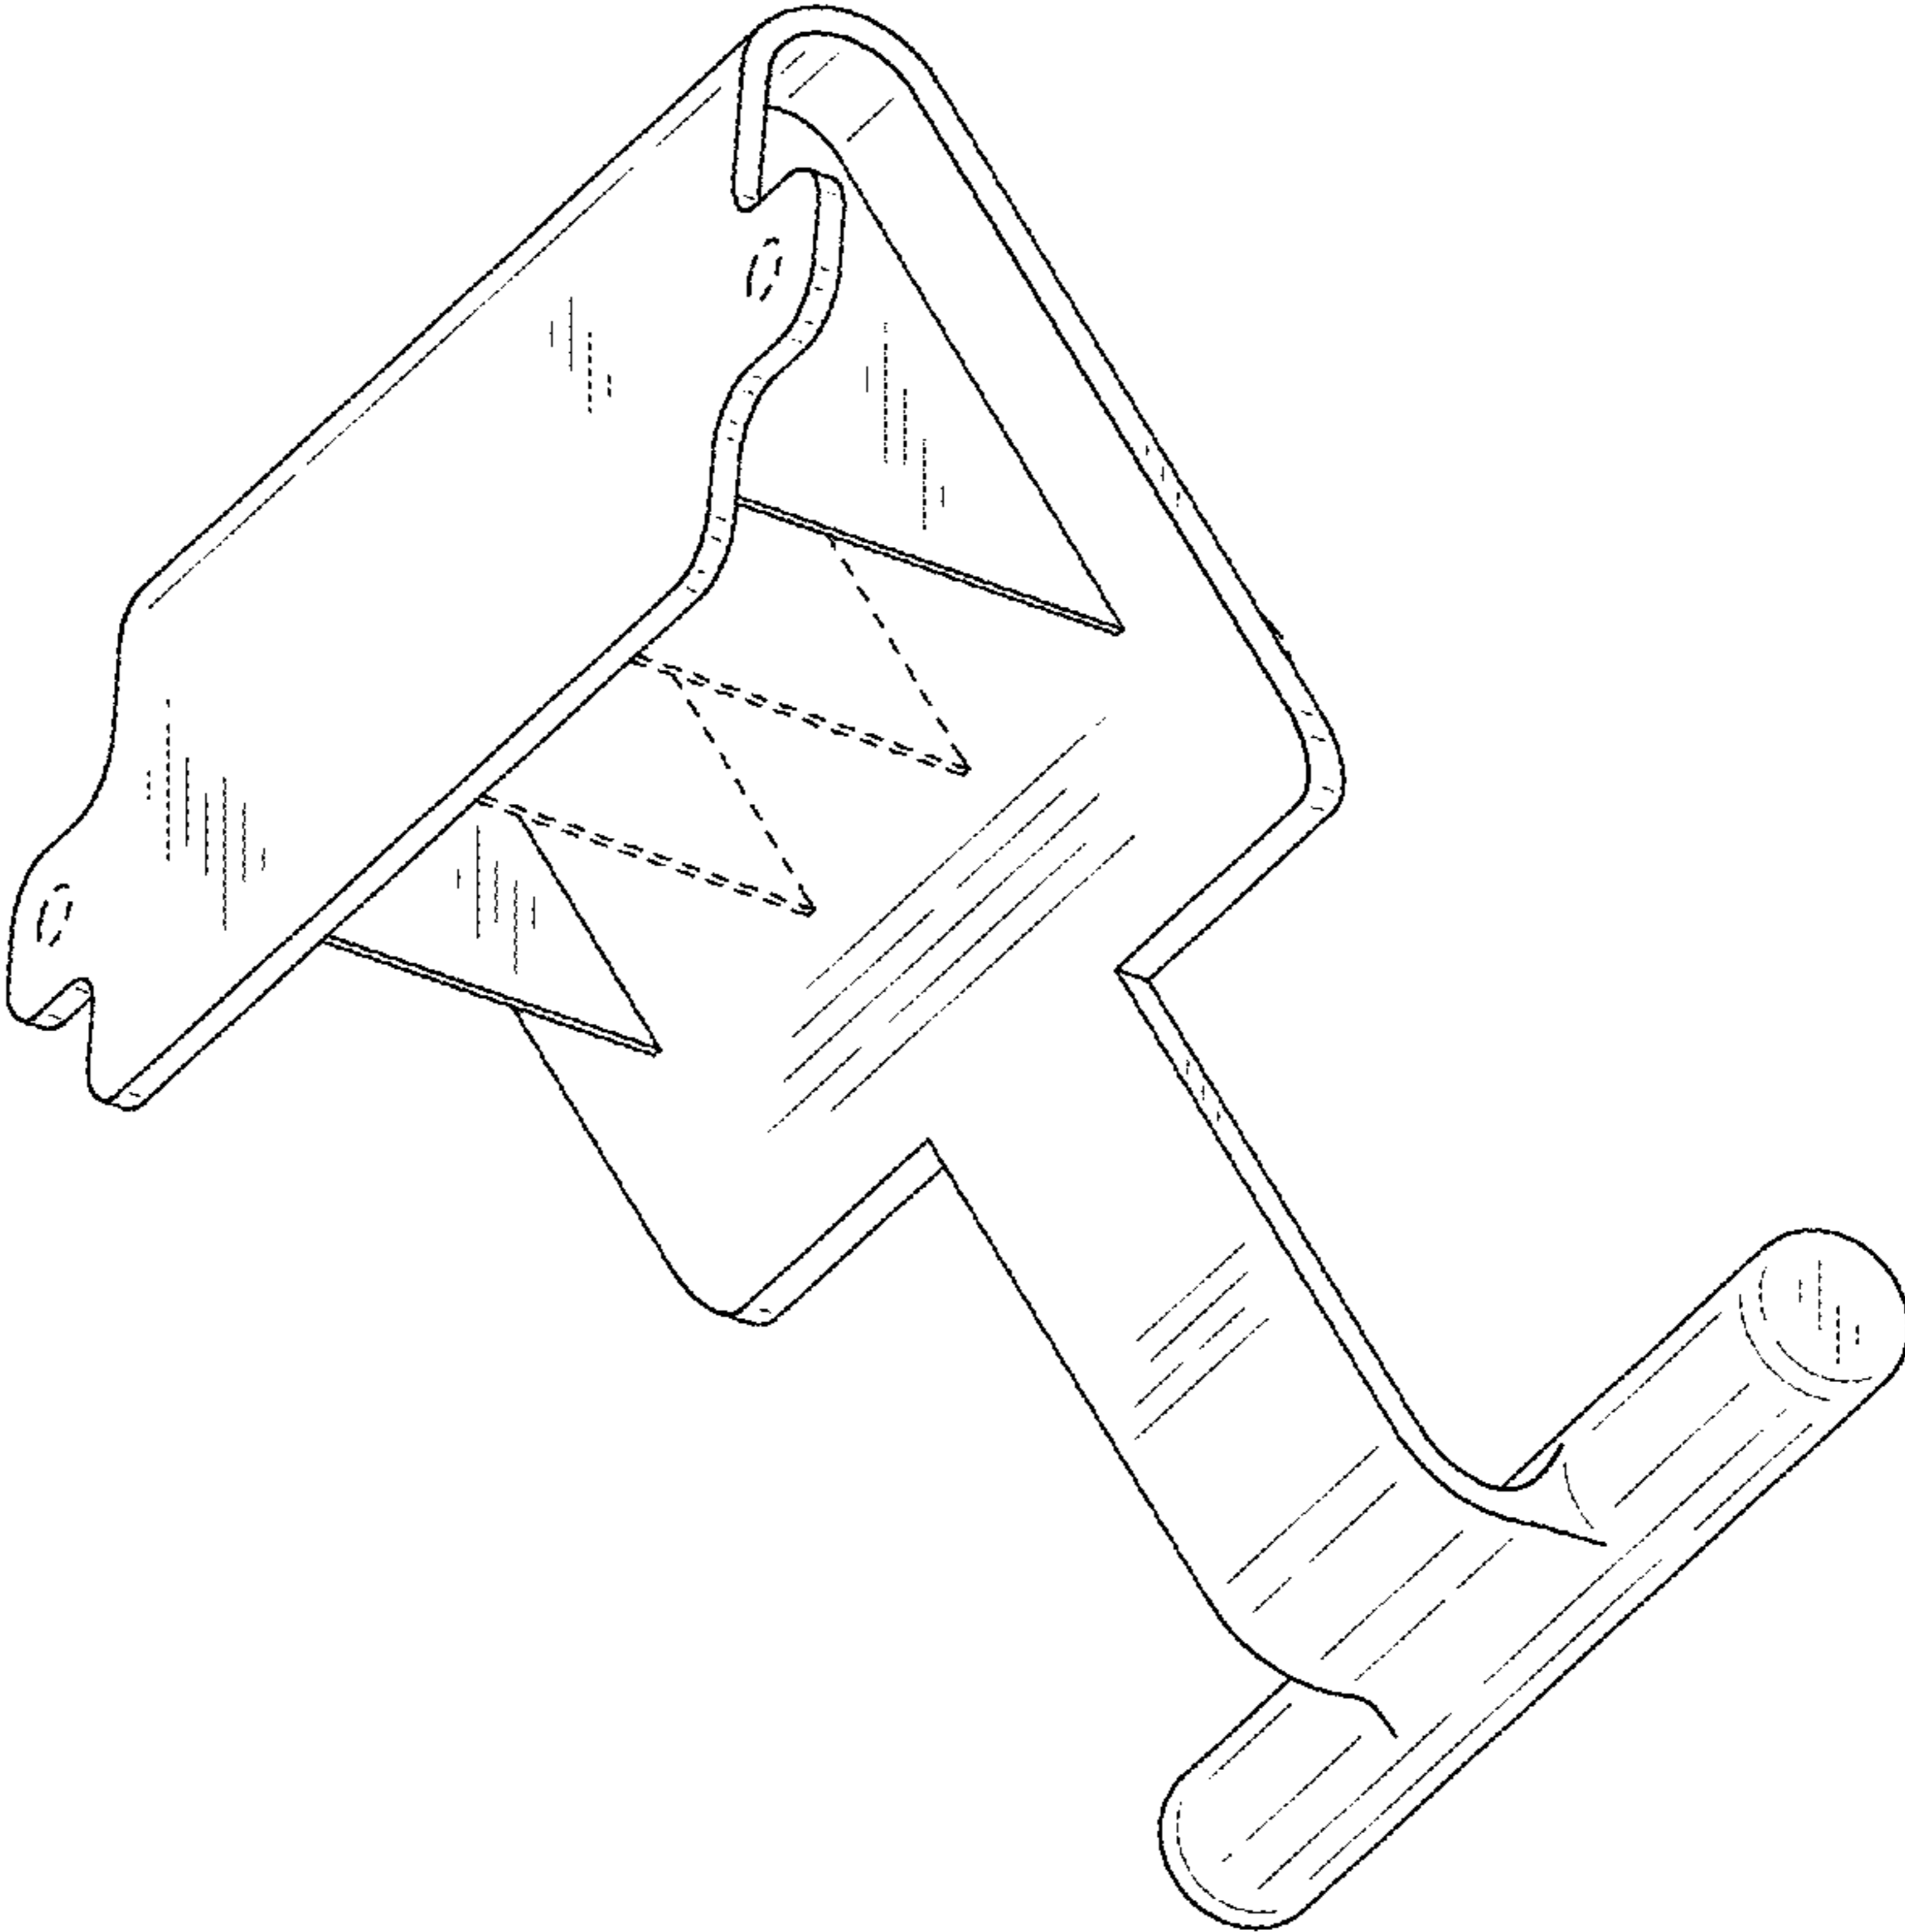


Fig.3

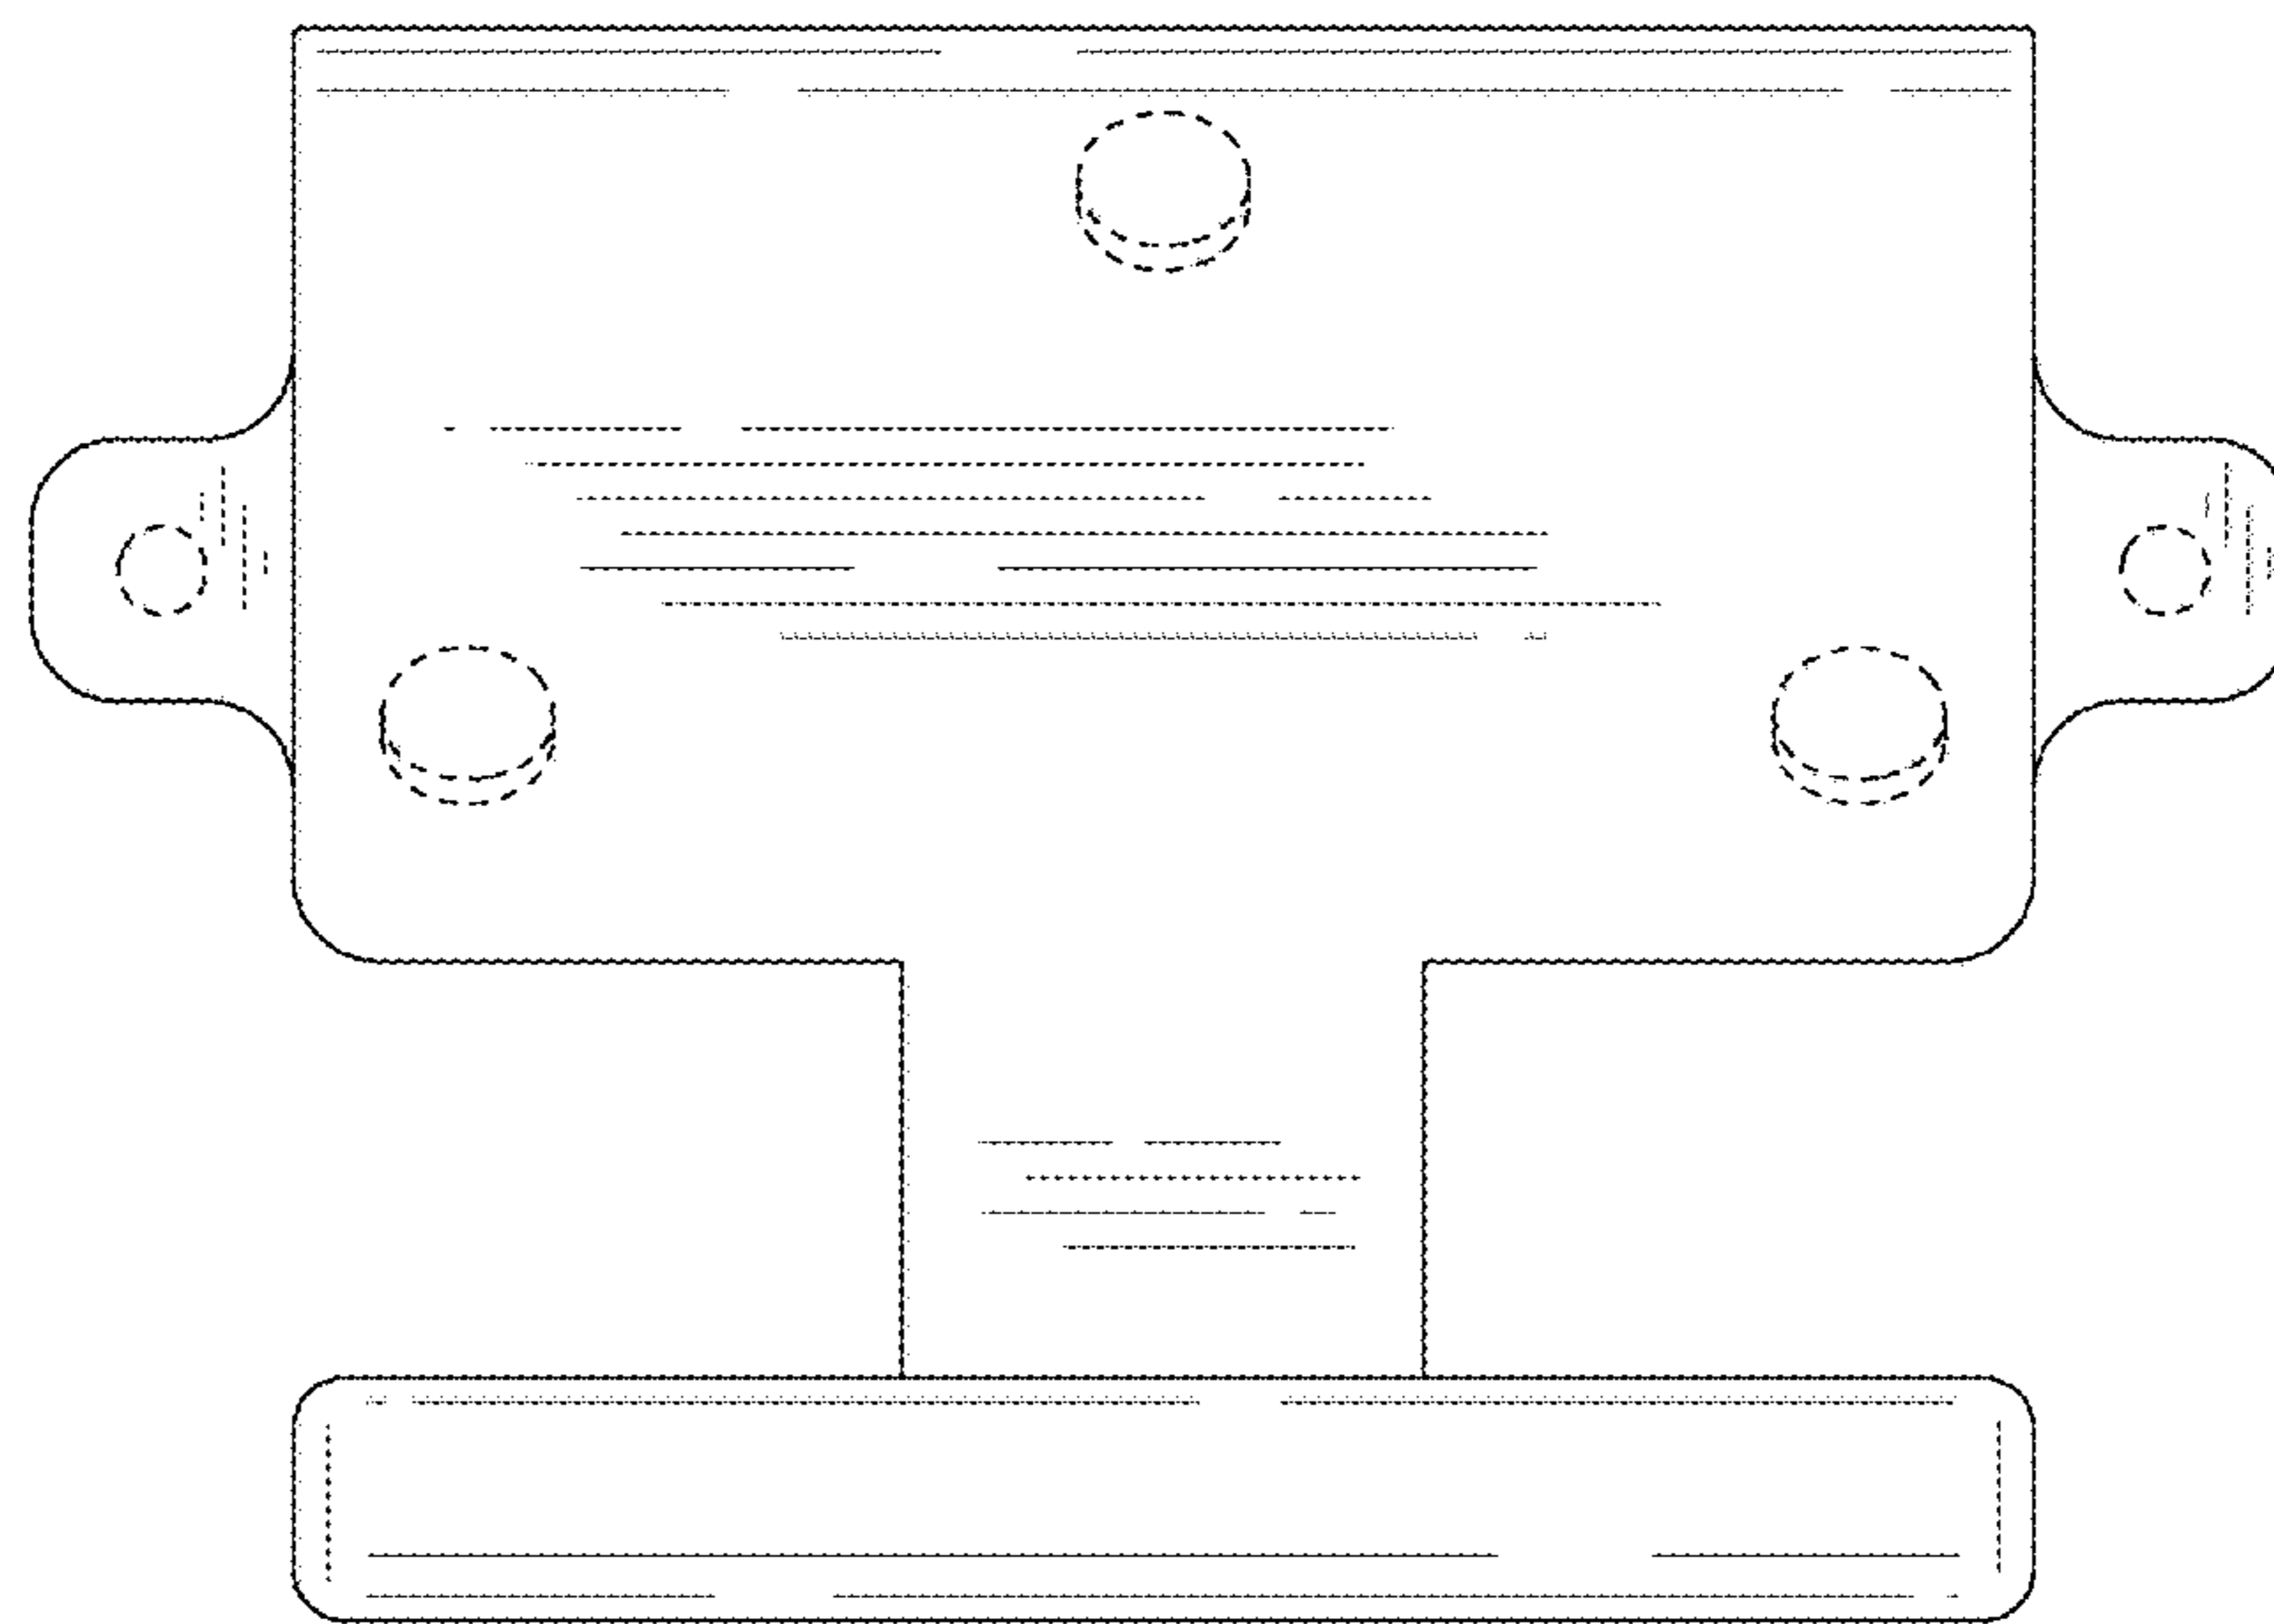


Fig.4

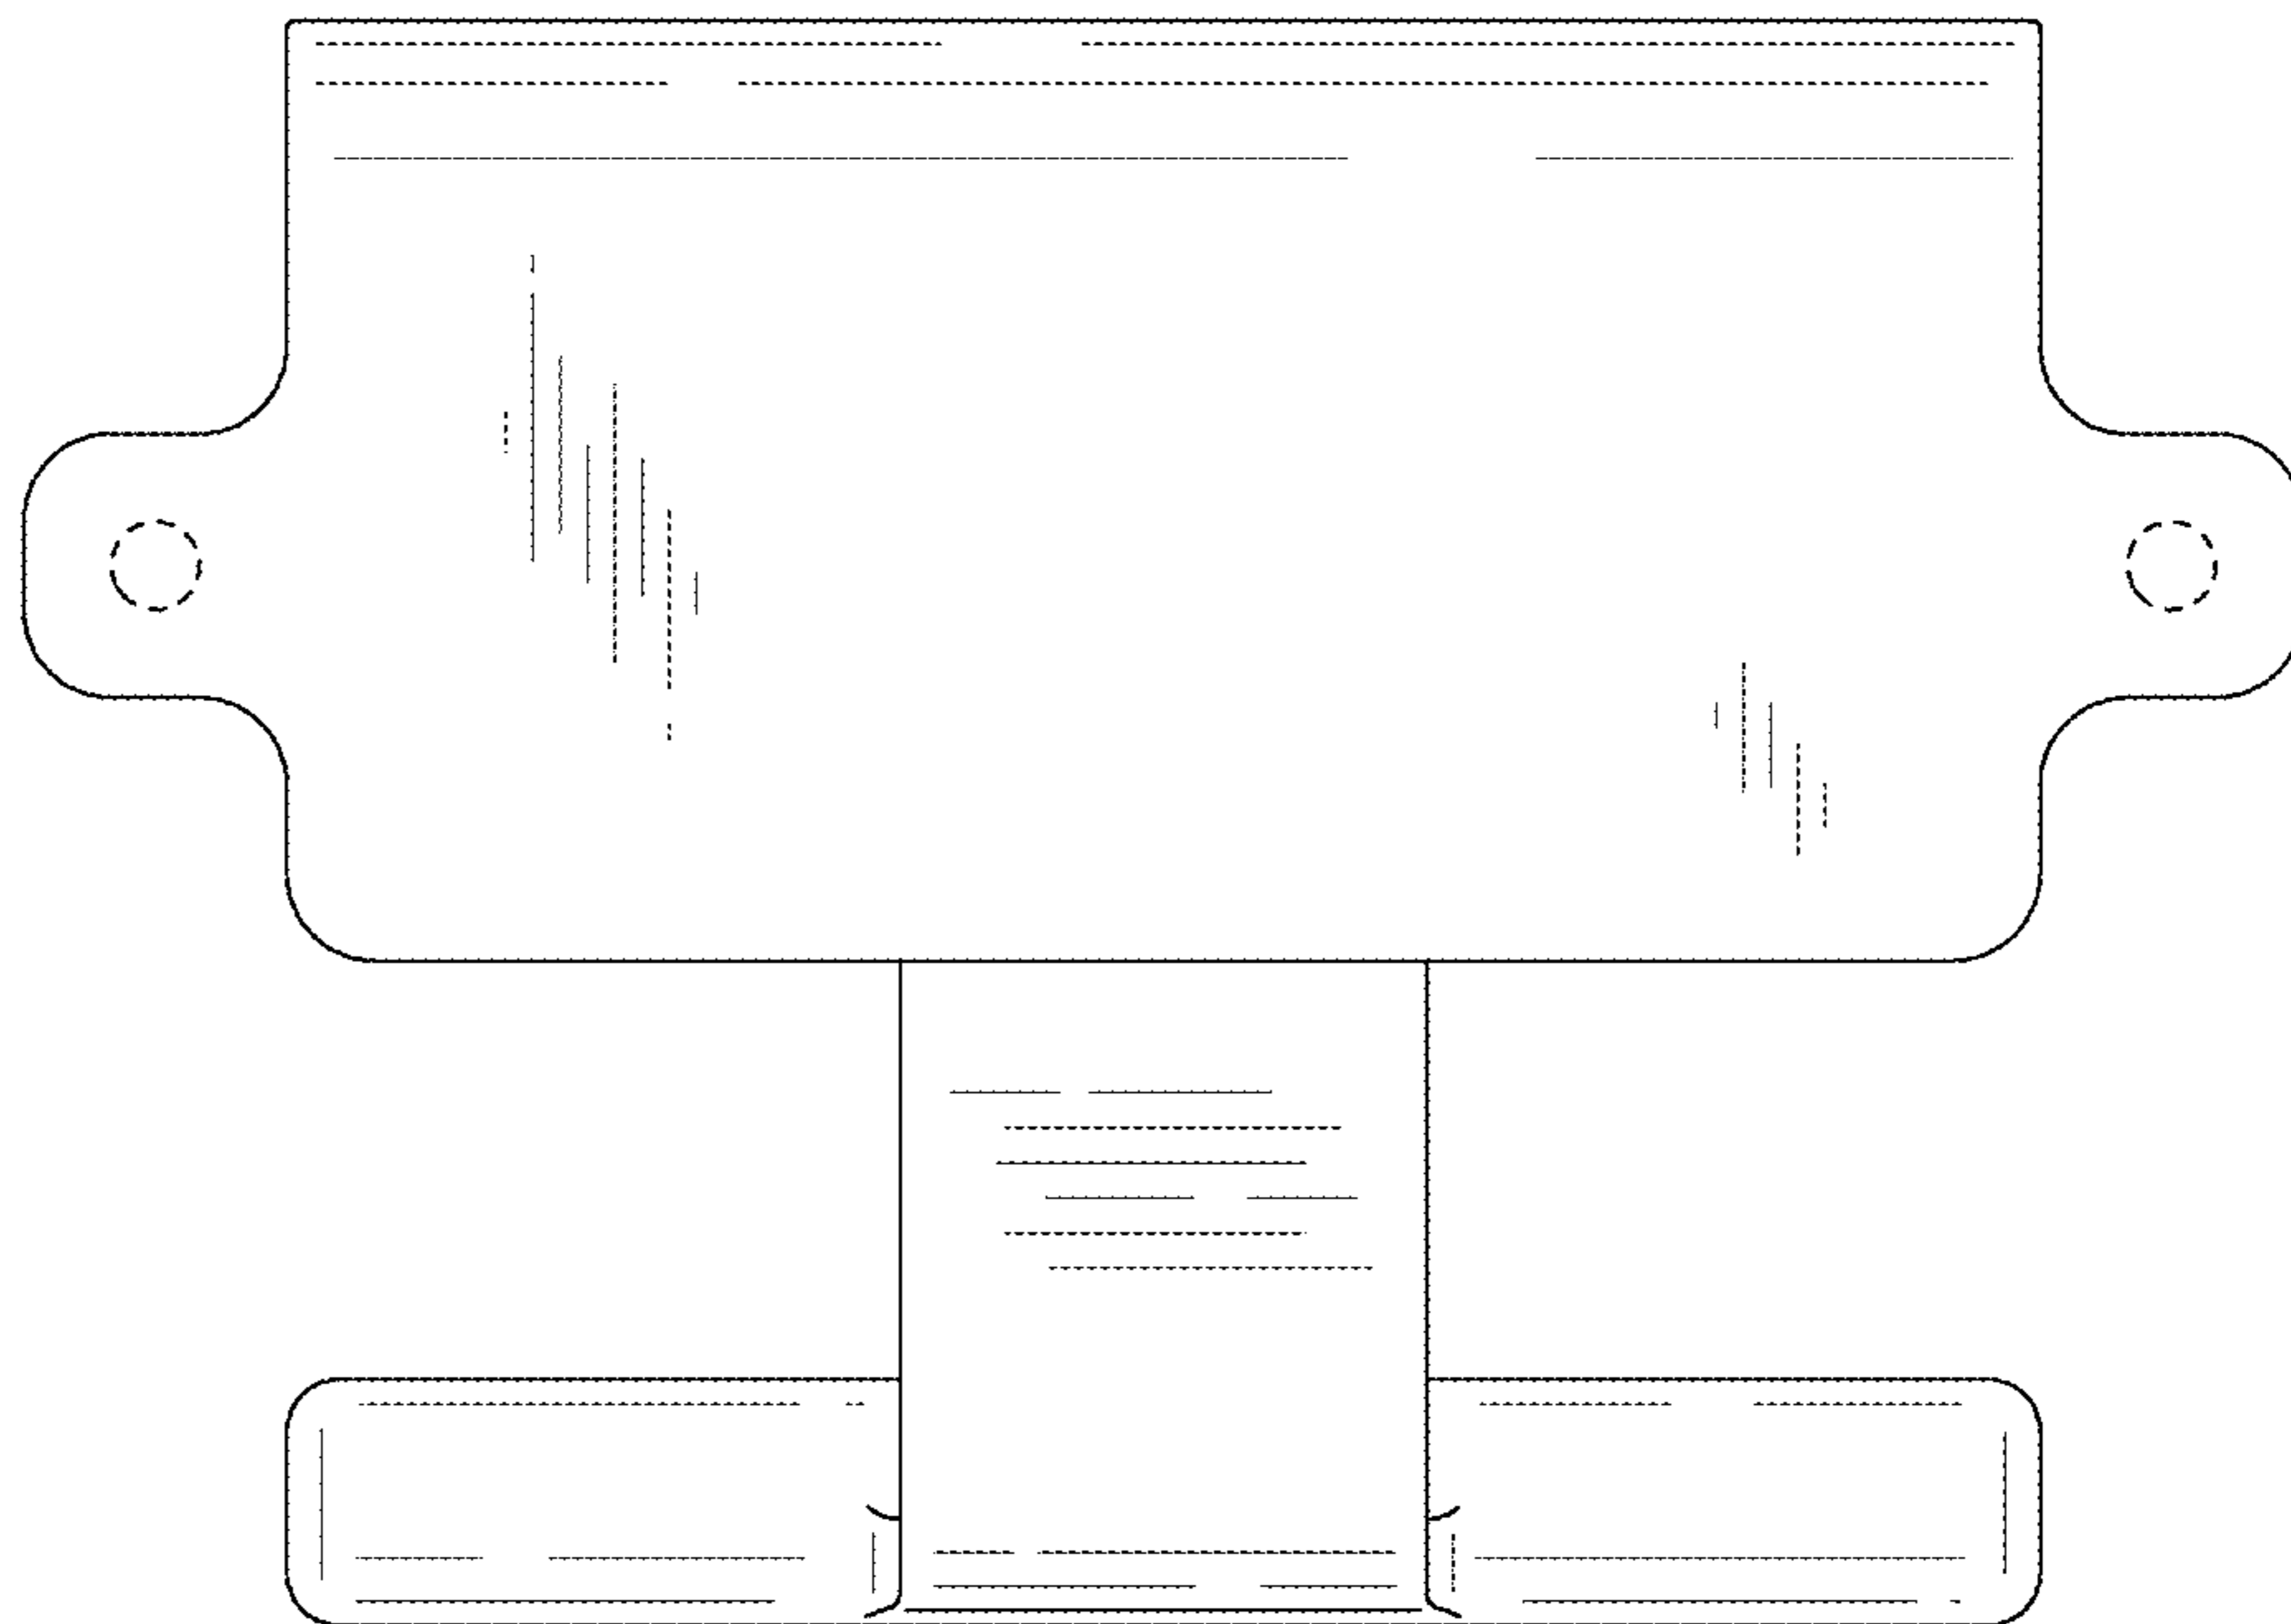


Fig.5

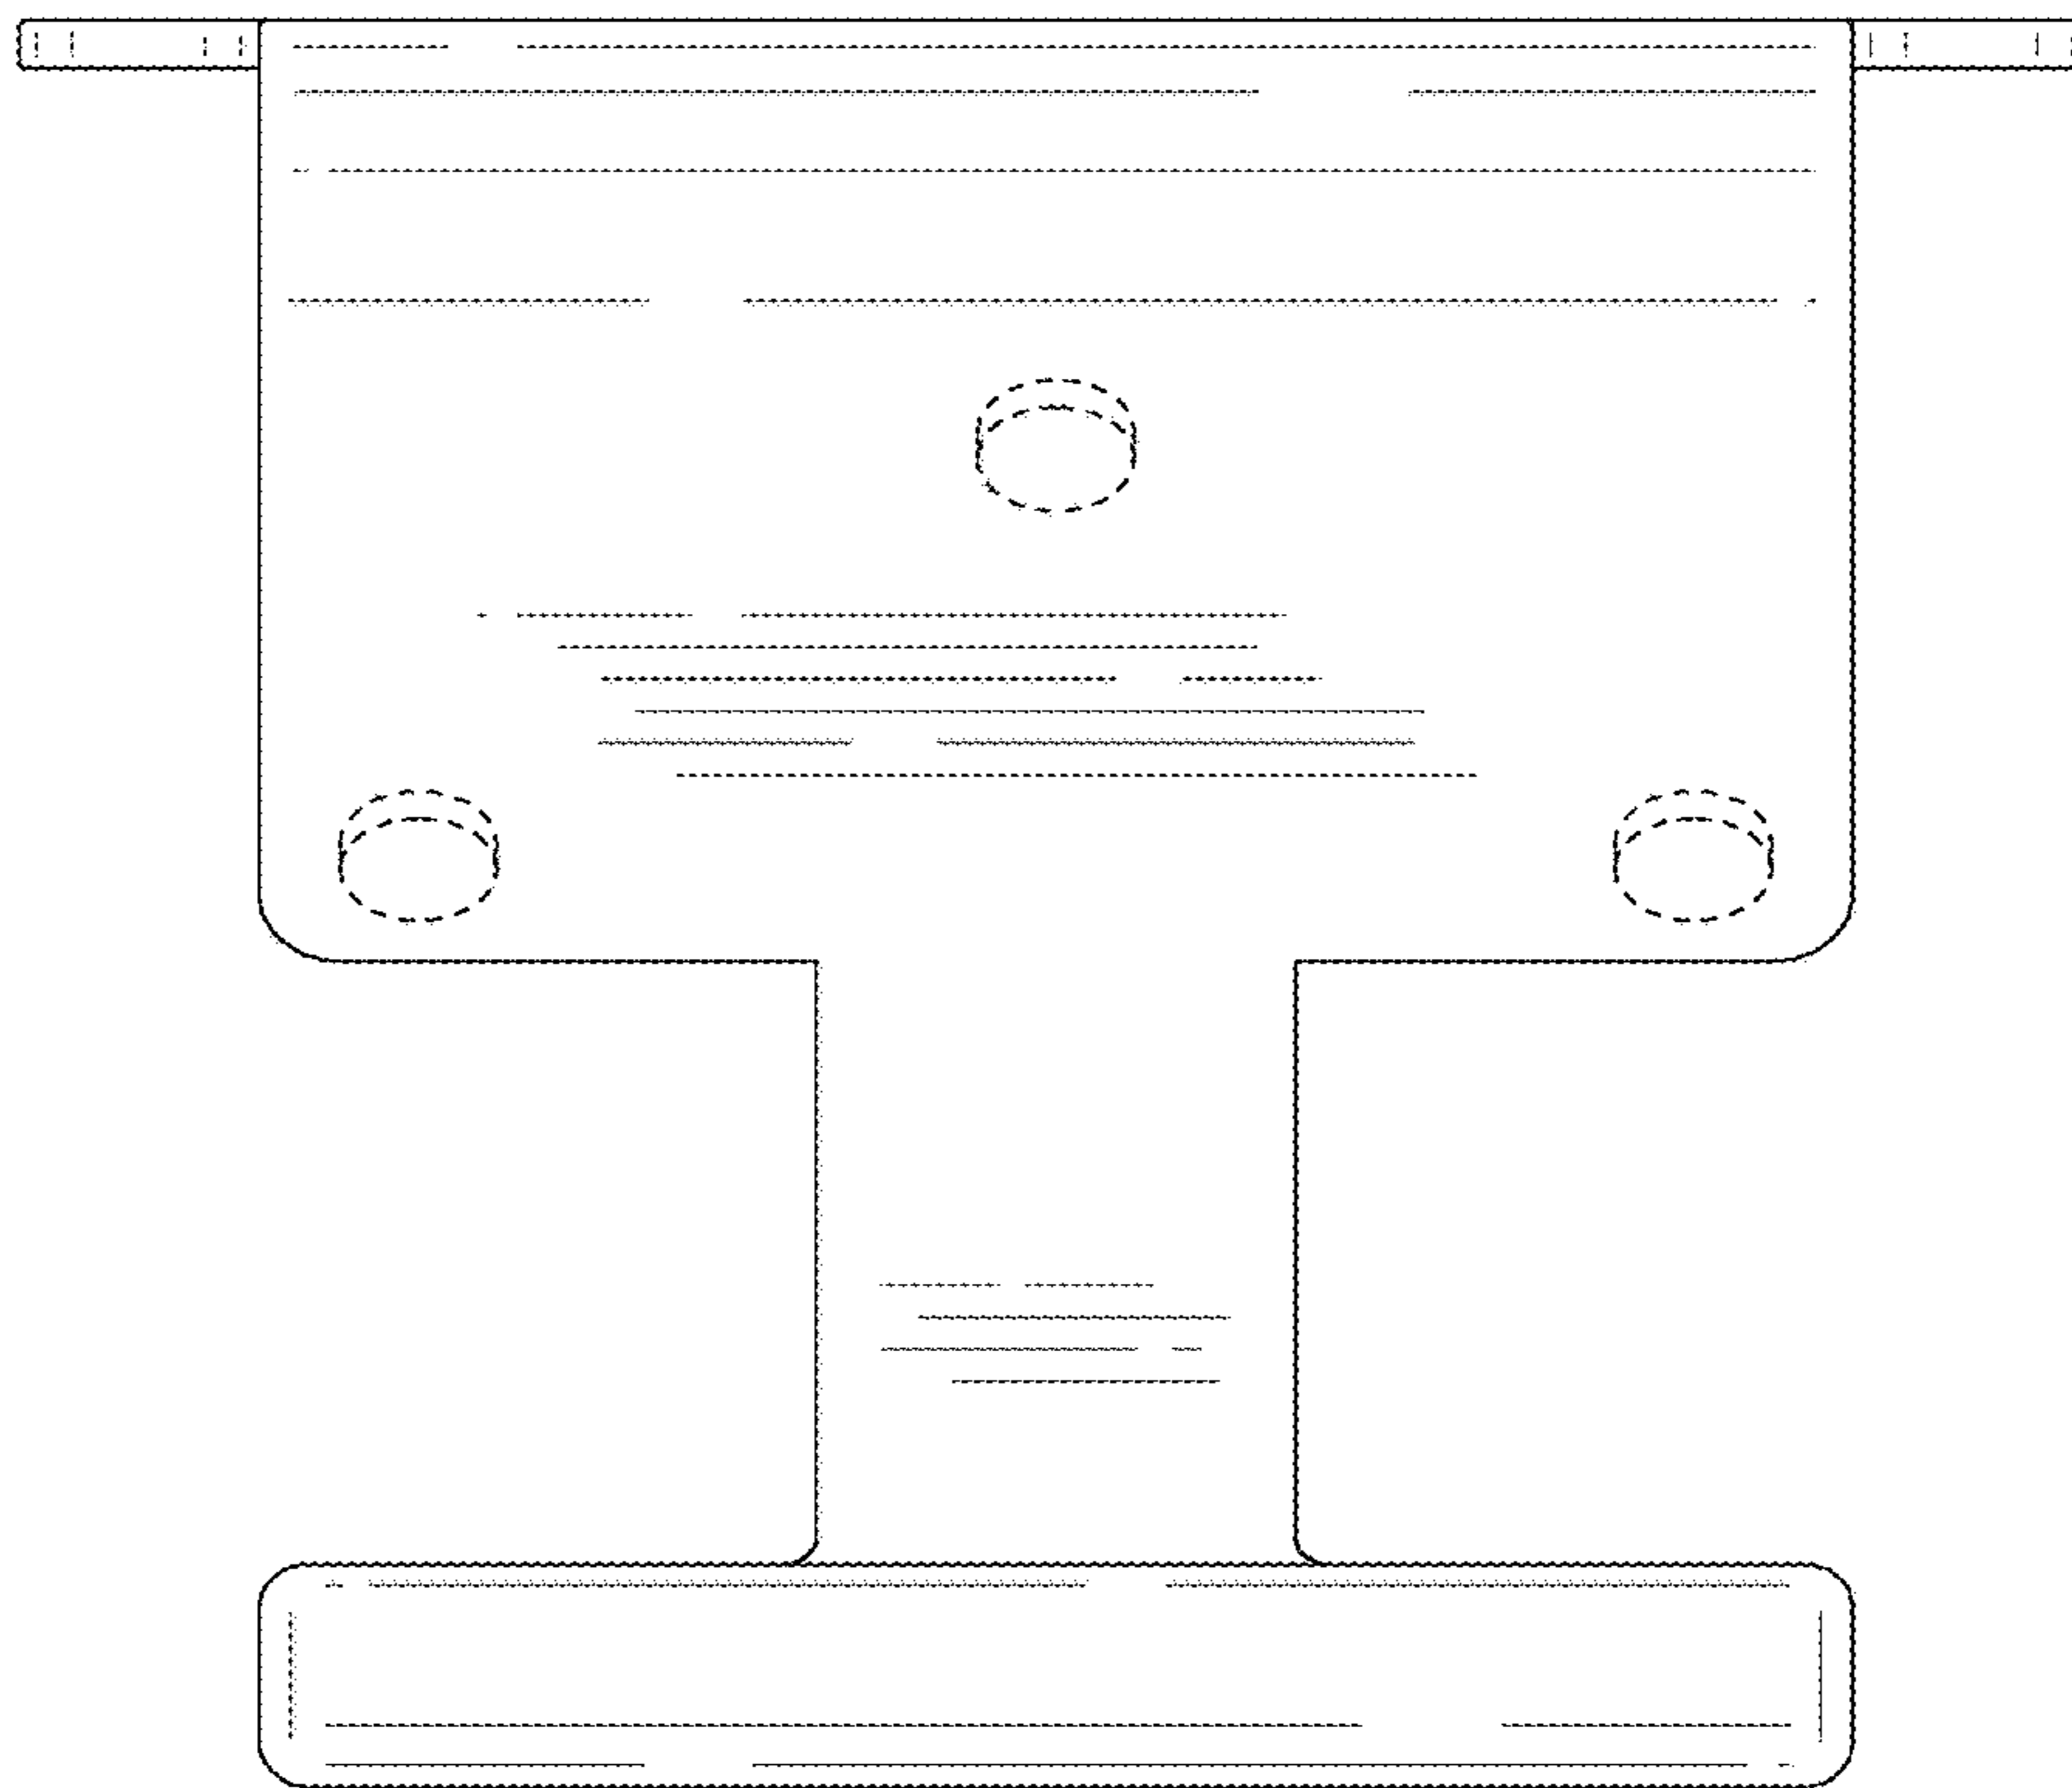


Fig.6

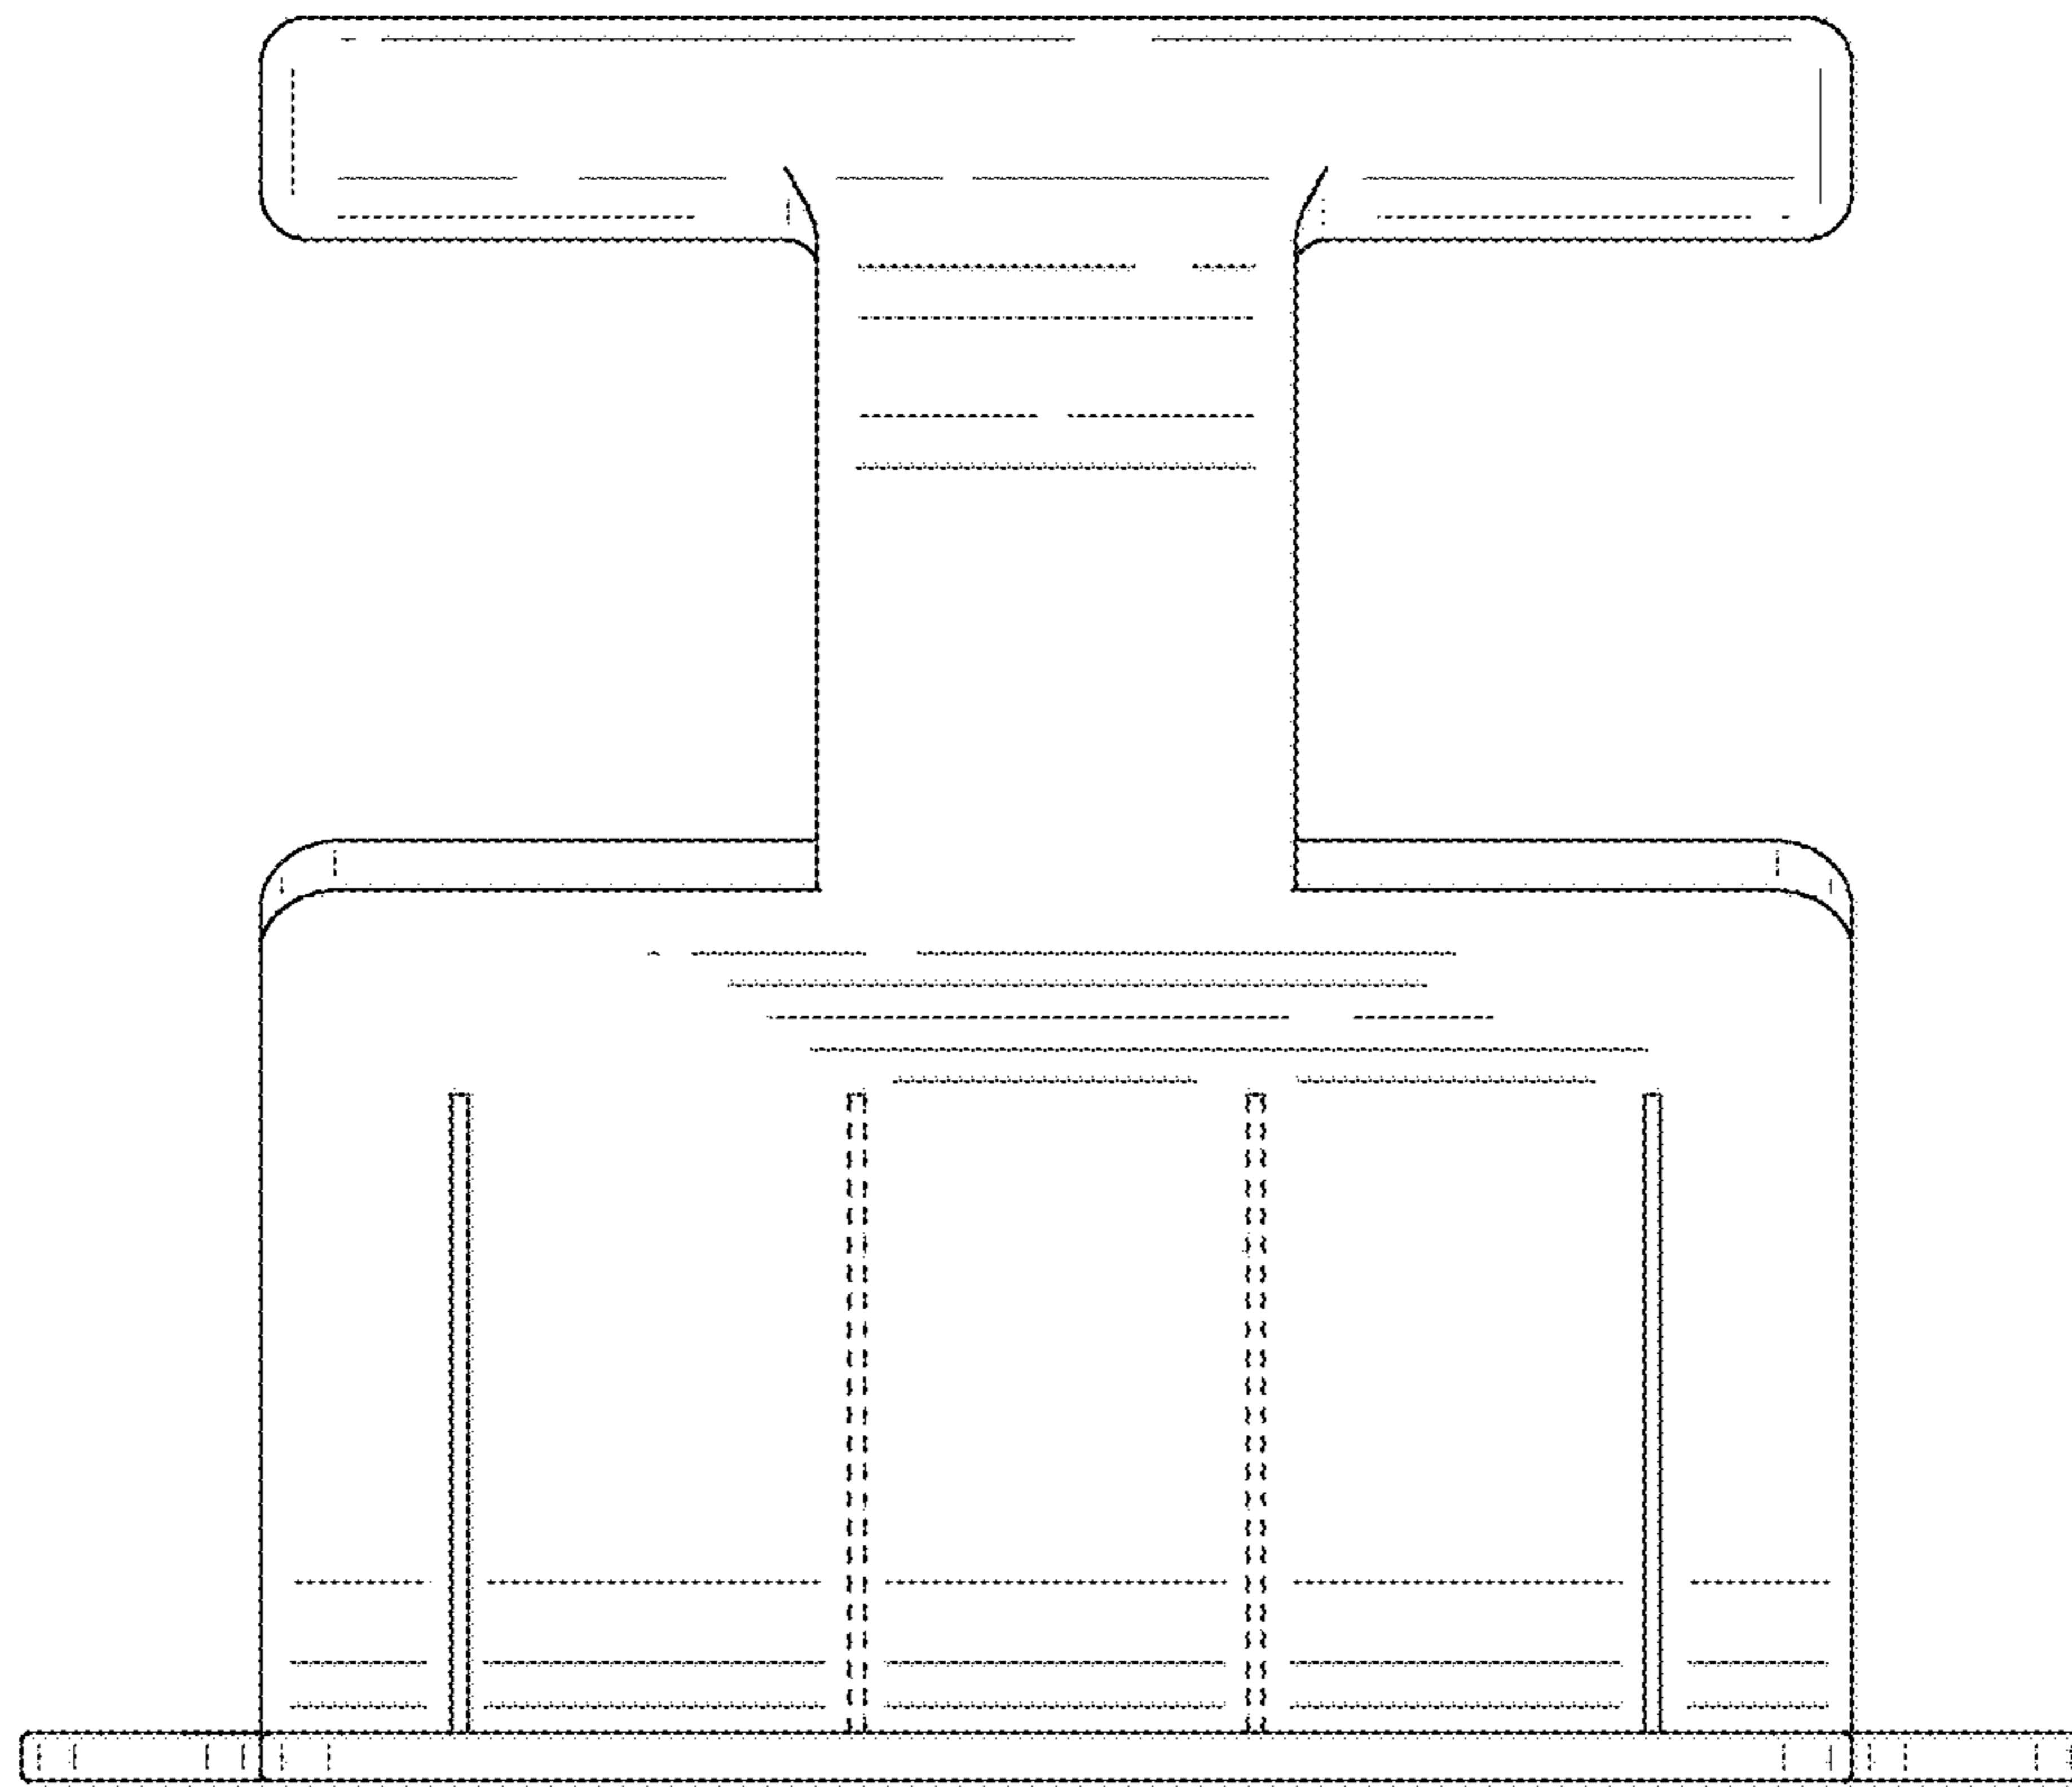


Fig.7

