



US00D793557S

(12) **United States Design Patent** (10) **Patent No.:** **US D793,557 S**  
**Thoma et al.** (45) **Date of Patent:** **\*\* Aug. 1, 2017**

(54) <b>X-RAY IMAGING DEVICE</b>	D585,554 S	1/2009	Suzuki	
	D597,210 S	7/2009	Hirabayashi	
(71) Applicant: <b>Sirona Dental Systems GmbH,</b> Bensheim (DE)	7,785,006 B2	8/2010	Kim	
	D659,833 S	5/2012	Ogura	
	8,251,583 B2 *	8/2012	Cekov	A61B 6/14 378/191
(72) Inventors: <b>Dieter Thoma,</b> Einhausen (DE); <b>Stefan Maier,</b> Darmstadt (DE)	2007/0297571 A1 *	12/2007	Beckhaus	A61B 6/14 378/147
	2011/0142198 A1 *	6/2011	Cekov	A61B 6/14 378/38
(73) Assignee: <b>Sirona Dental Systems GmbH,</b> Bensheim (DE)	2011/0305320 A1 *	12/2011	Suuronen	A61B 6/00 378/98.5

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/546,065**

(22) Filed: **Nov. 18, 2015**

**Related U.S. Application Data**

(63) Continuation of application No. 29/509,262, filed on Nov. 14, 2014, now abandoned.

(30) **Foreign Application Priority Data**

May 16, 2014 (EM) ..... 002465500-0001

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/158**

(58) **Field of Classification Search**  
USPC ..... D24/158-161, 185, 186, 107, 176  
CPC ..... A61B 6/14; A61B 6/4411; A61B 6/4441;  
A61B 6/032; A61B 5/4504; A61B 5/4547  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D480,142 S	9/2003	Chikuma
D554,257 S	10/2007	Ogiwara
D563,553 S	3/2008	Saito et al.
D571,471 S	6/2008	Stockl

**OTHER PUBLICATIONS**

“Orthophos XG List of Spare Parts” dated Sep. 8, 2013, pp. 1-102, printed in Germany.  
Orthophos XG 3D and Orthophos XG 3D ready Brochure, pp. 1-11, Rev. 02/11.  
Orthophos XG 3D/Ceph, Orthophos XG 3D ready/Ceph, Operating Instructions, pp. 1, 30, 104, 109, Jun. 2014.

(Continued)

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Fitzpatrick, Cella, Harper & Scinto


(57) **CLAIM**

The ornamental design for an X-ray imaging device, as shown and described.

**DESCRIPTION**

FIG. 1 is a right and rear perspective view of our design; FIG. 2 is a front elevation thereof; FIG. 3 is a rear elevation thereof; FIG. 4 is a top, right, and rear perspective view thereof; FIG. 5 is a bottom, left, and rear perspective view thereof; FIG. 6 is a left side view thereof; and, FIG. 7 is a right side view thereof.

**1 Claim, 7 Drawing Sheets**

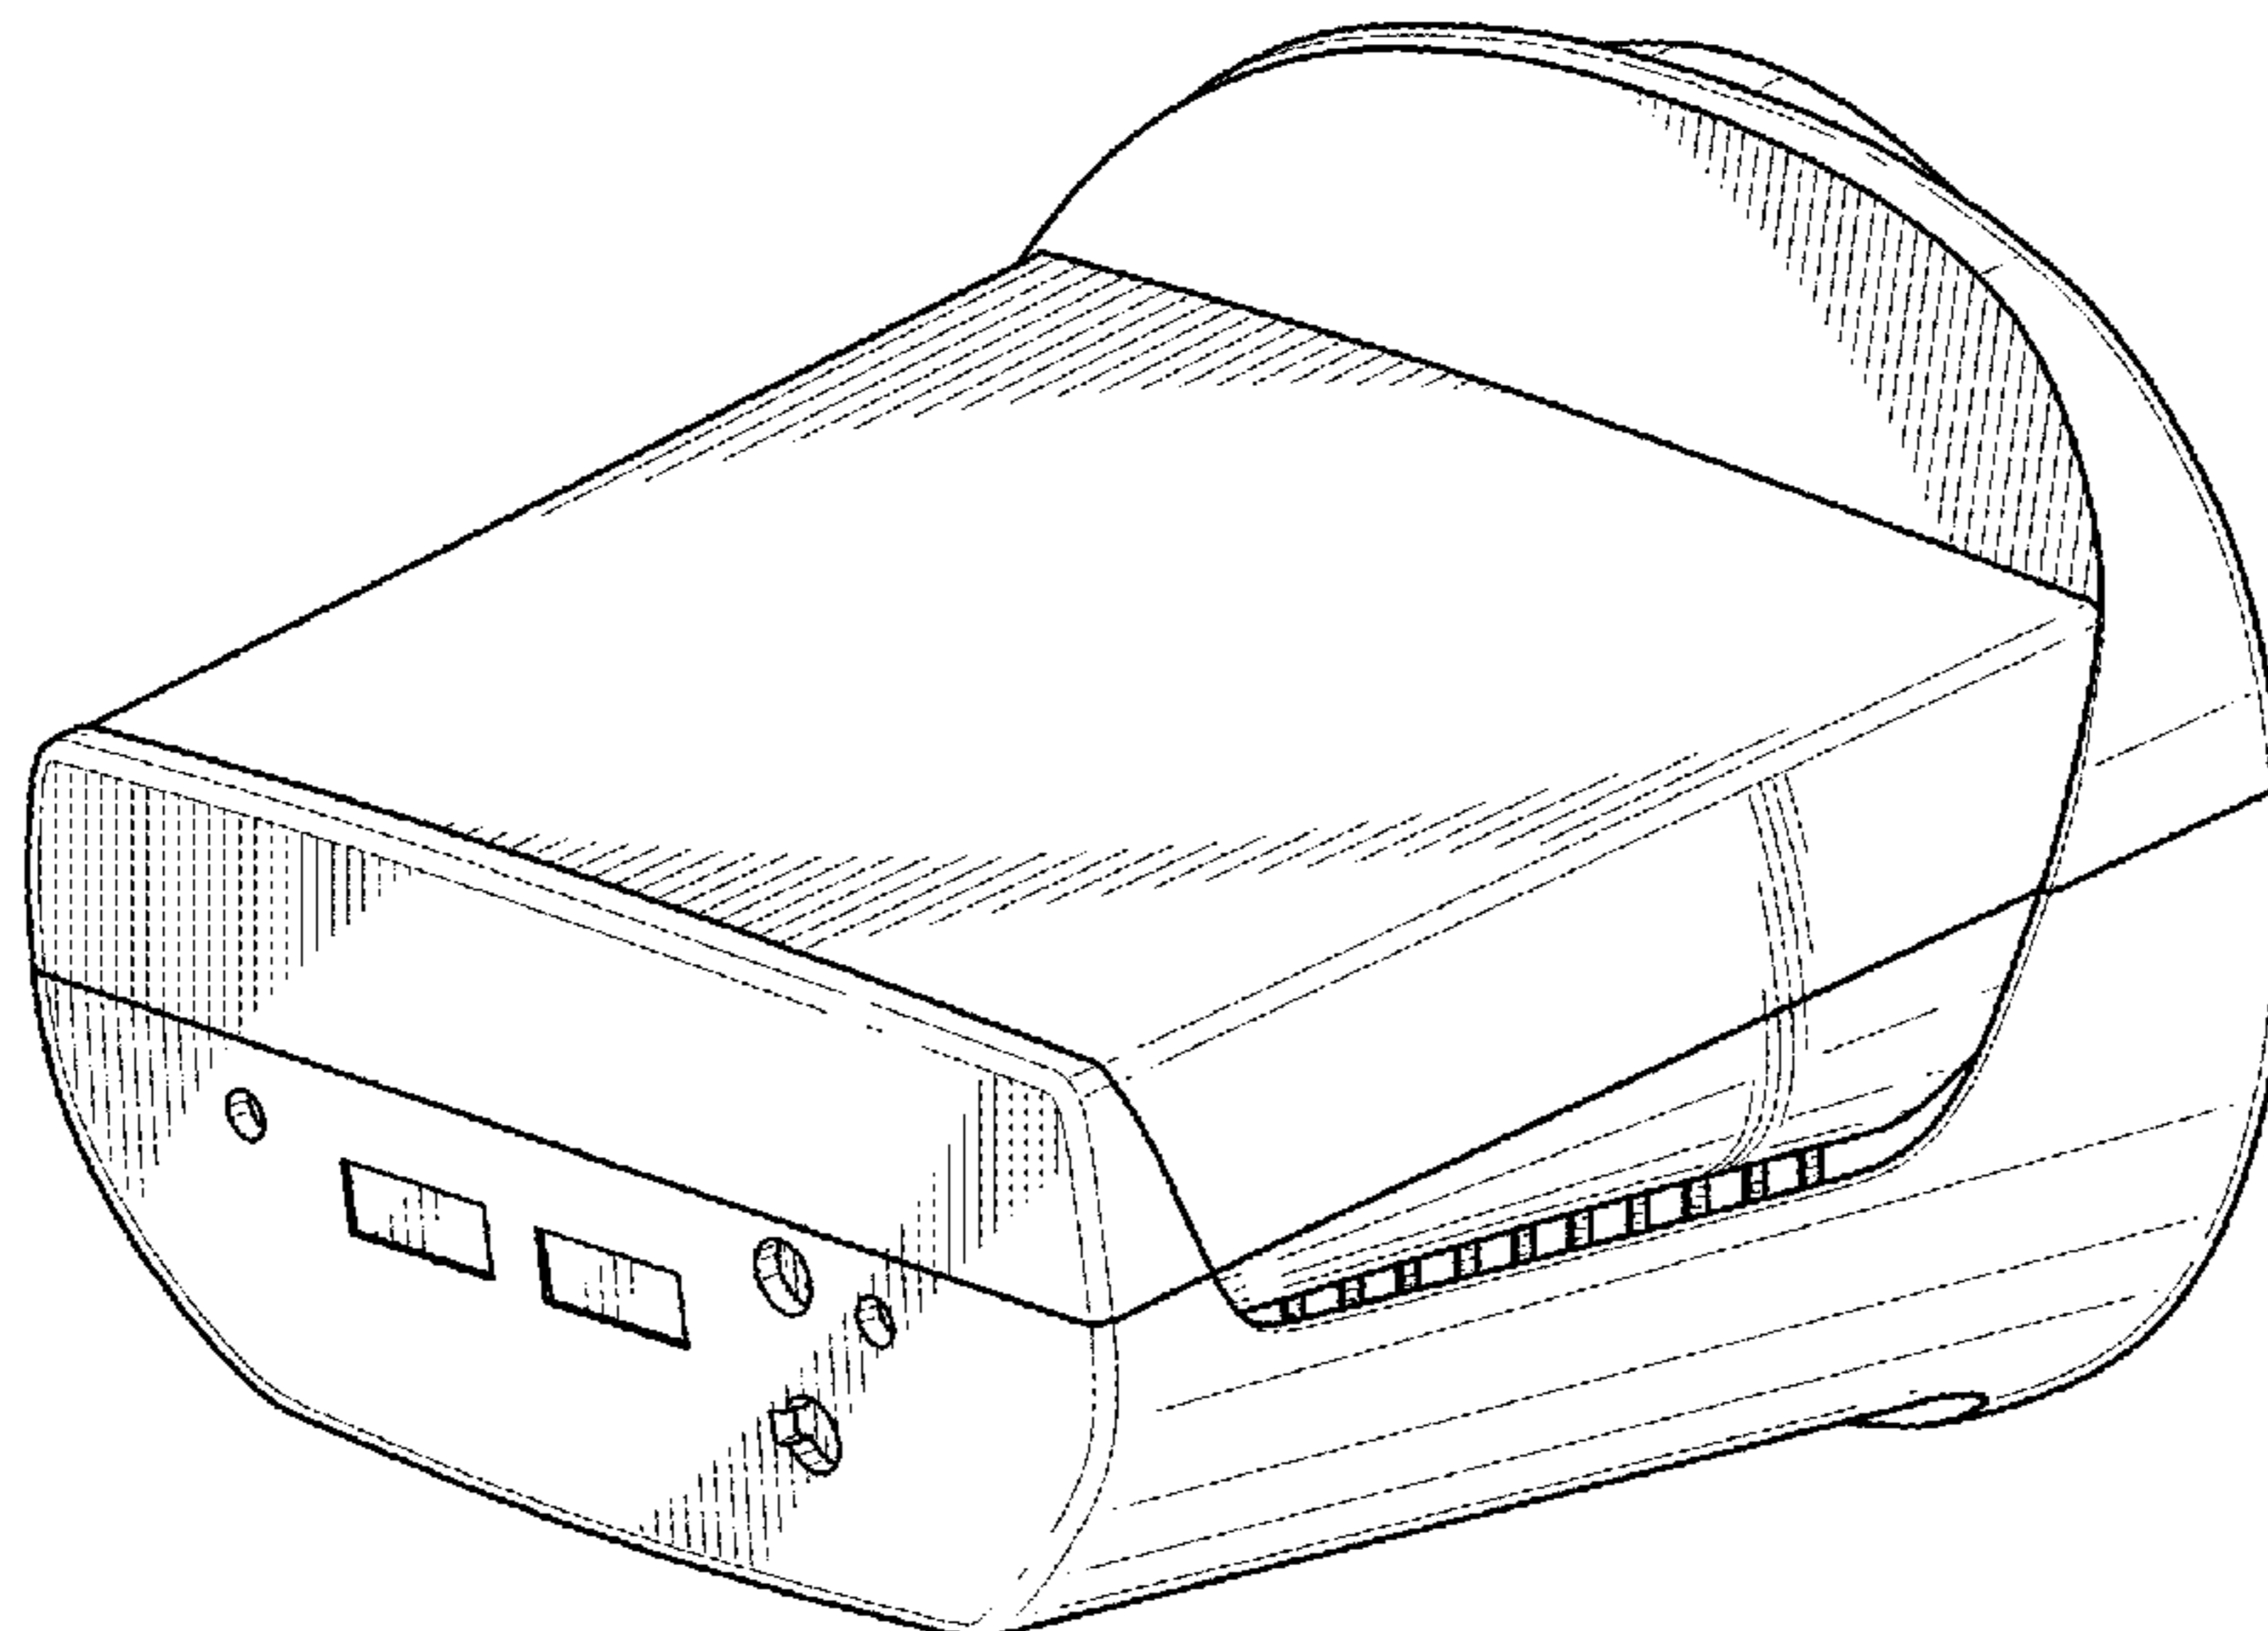

(56)


**References Cited**

OTHER PUBLICATIONS


Orthophos XG 5/Ceph, Orthophos XG 5 DS/Ceph, Operating Instructions, pp. 1, 23, 24, 45, Aug. 2013.

Orthophos Plus DS, Operating Instructions, pp. 1, 11, 24, 26, Jul. 2003.


\* cited by examiner

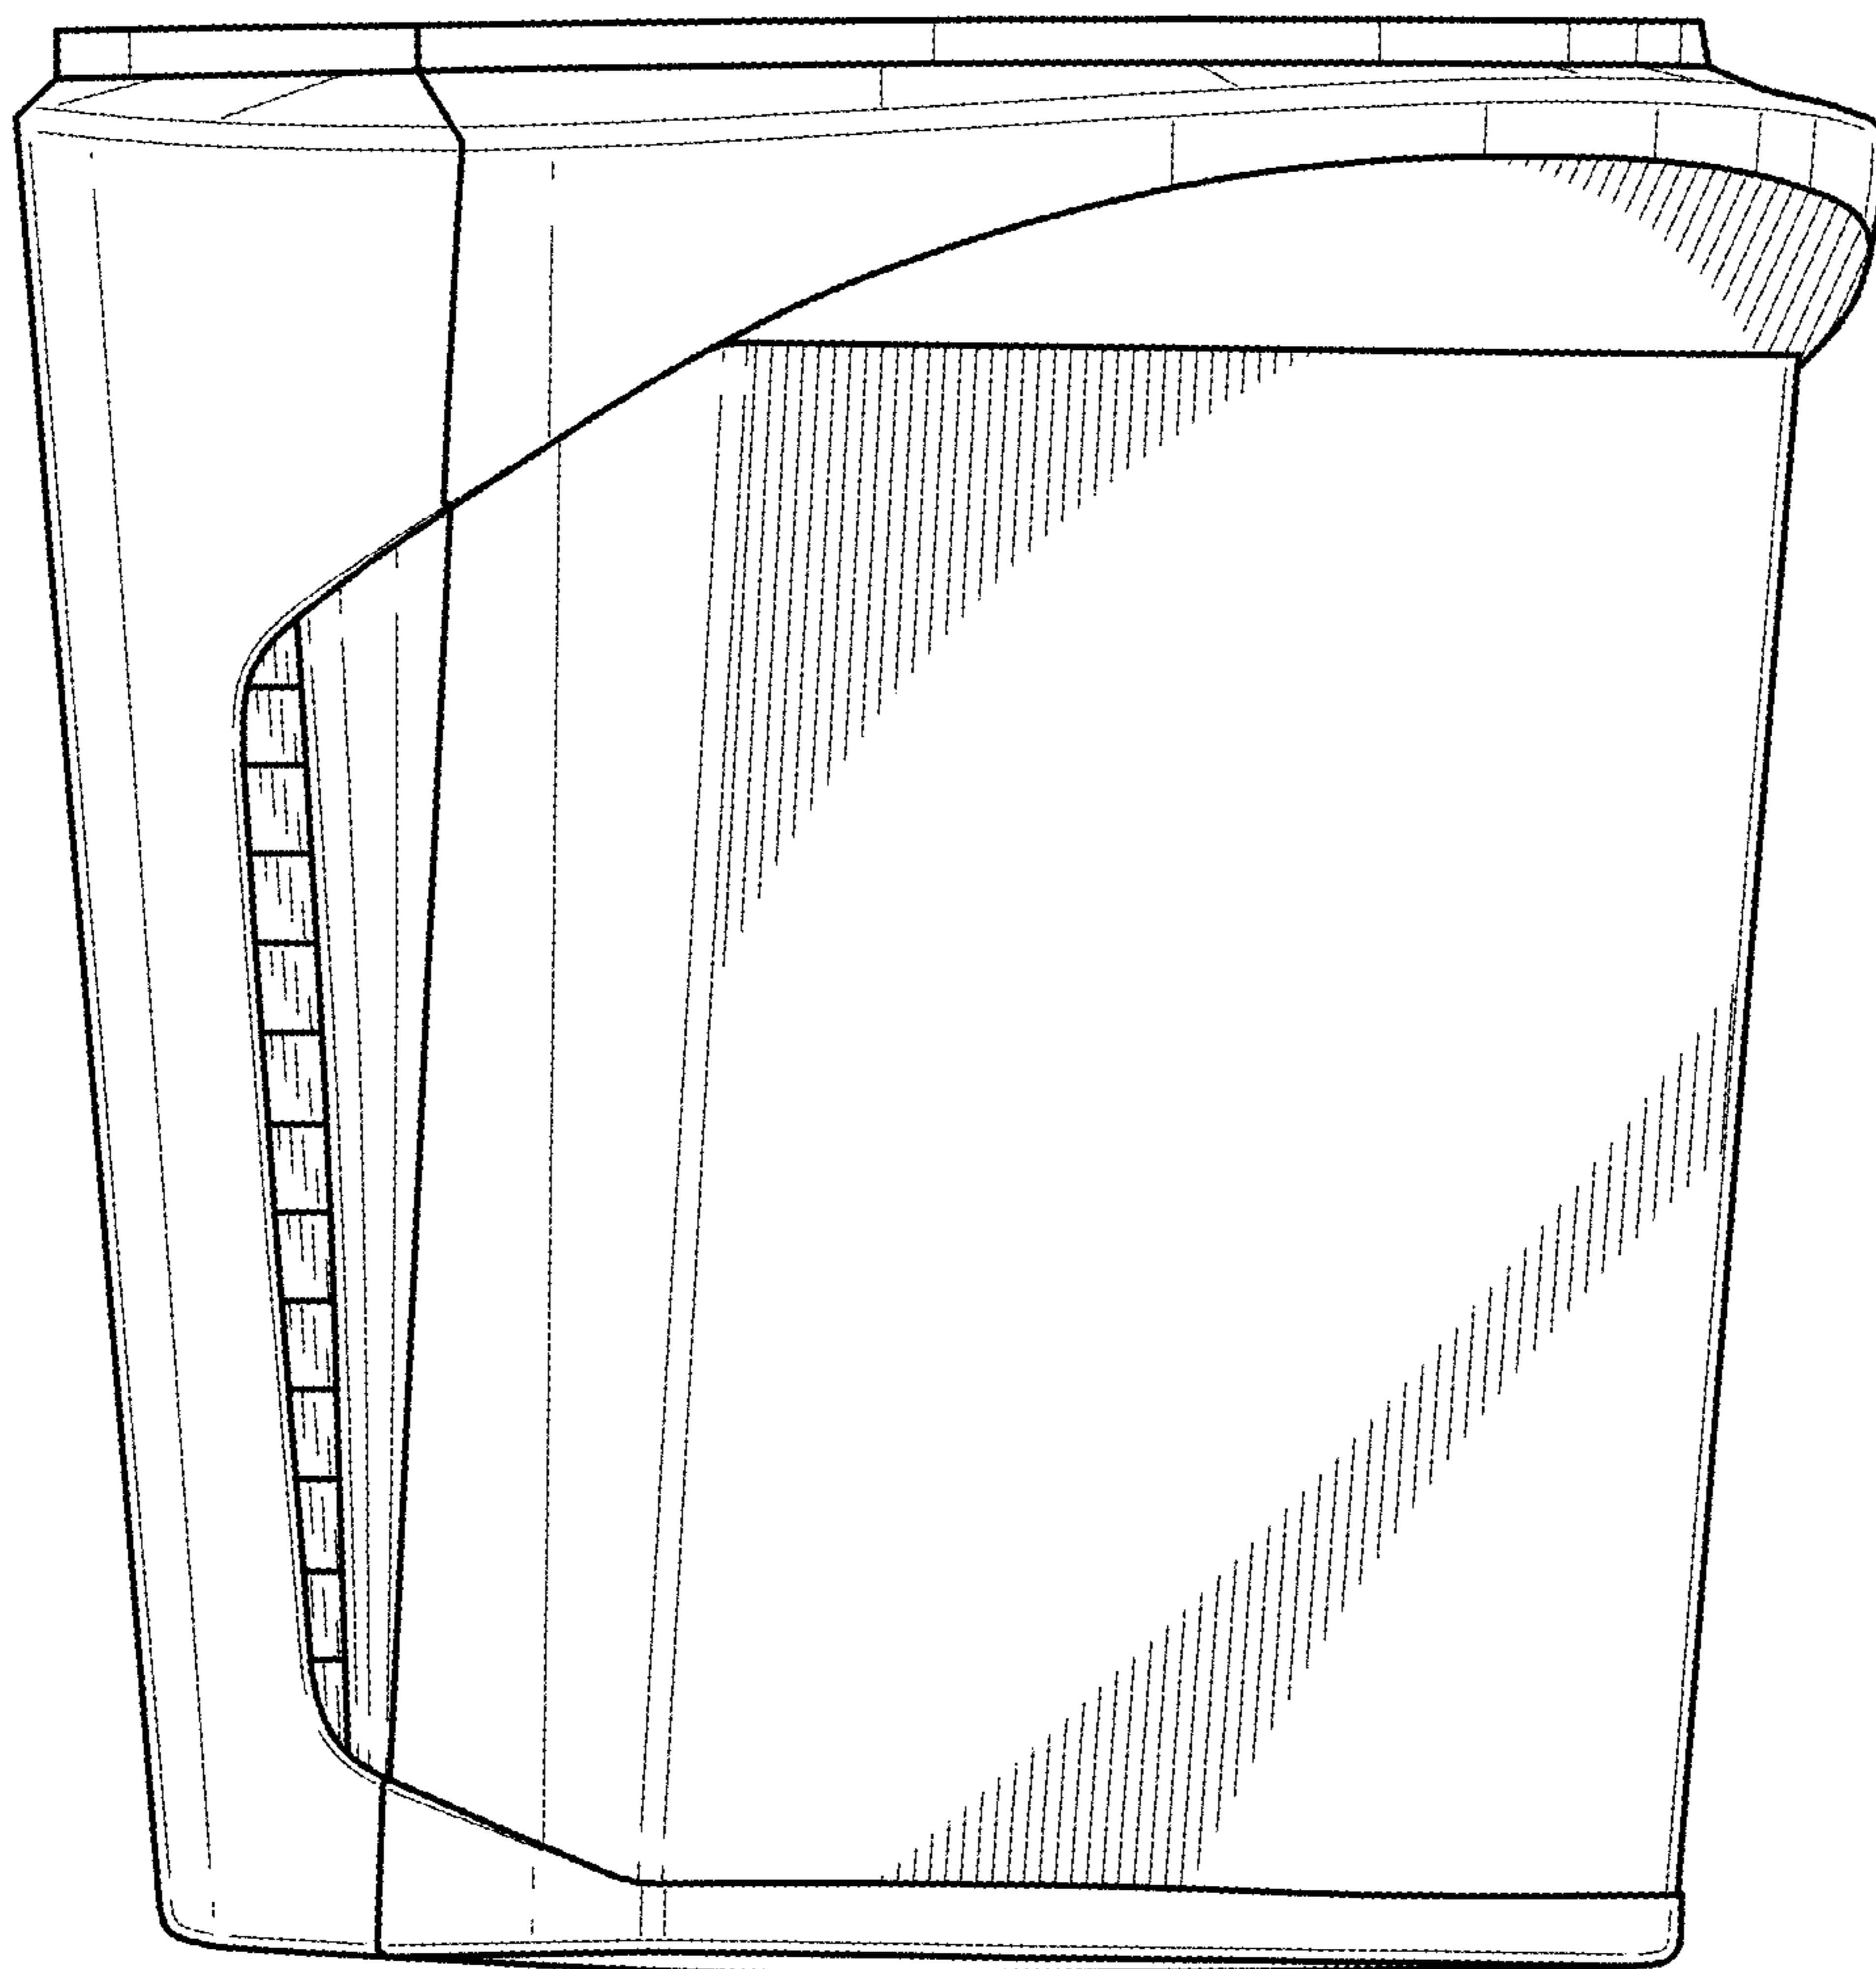


**FIG. 1**

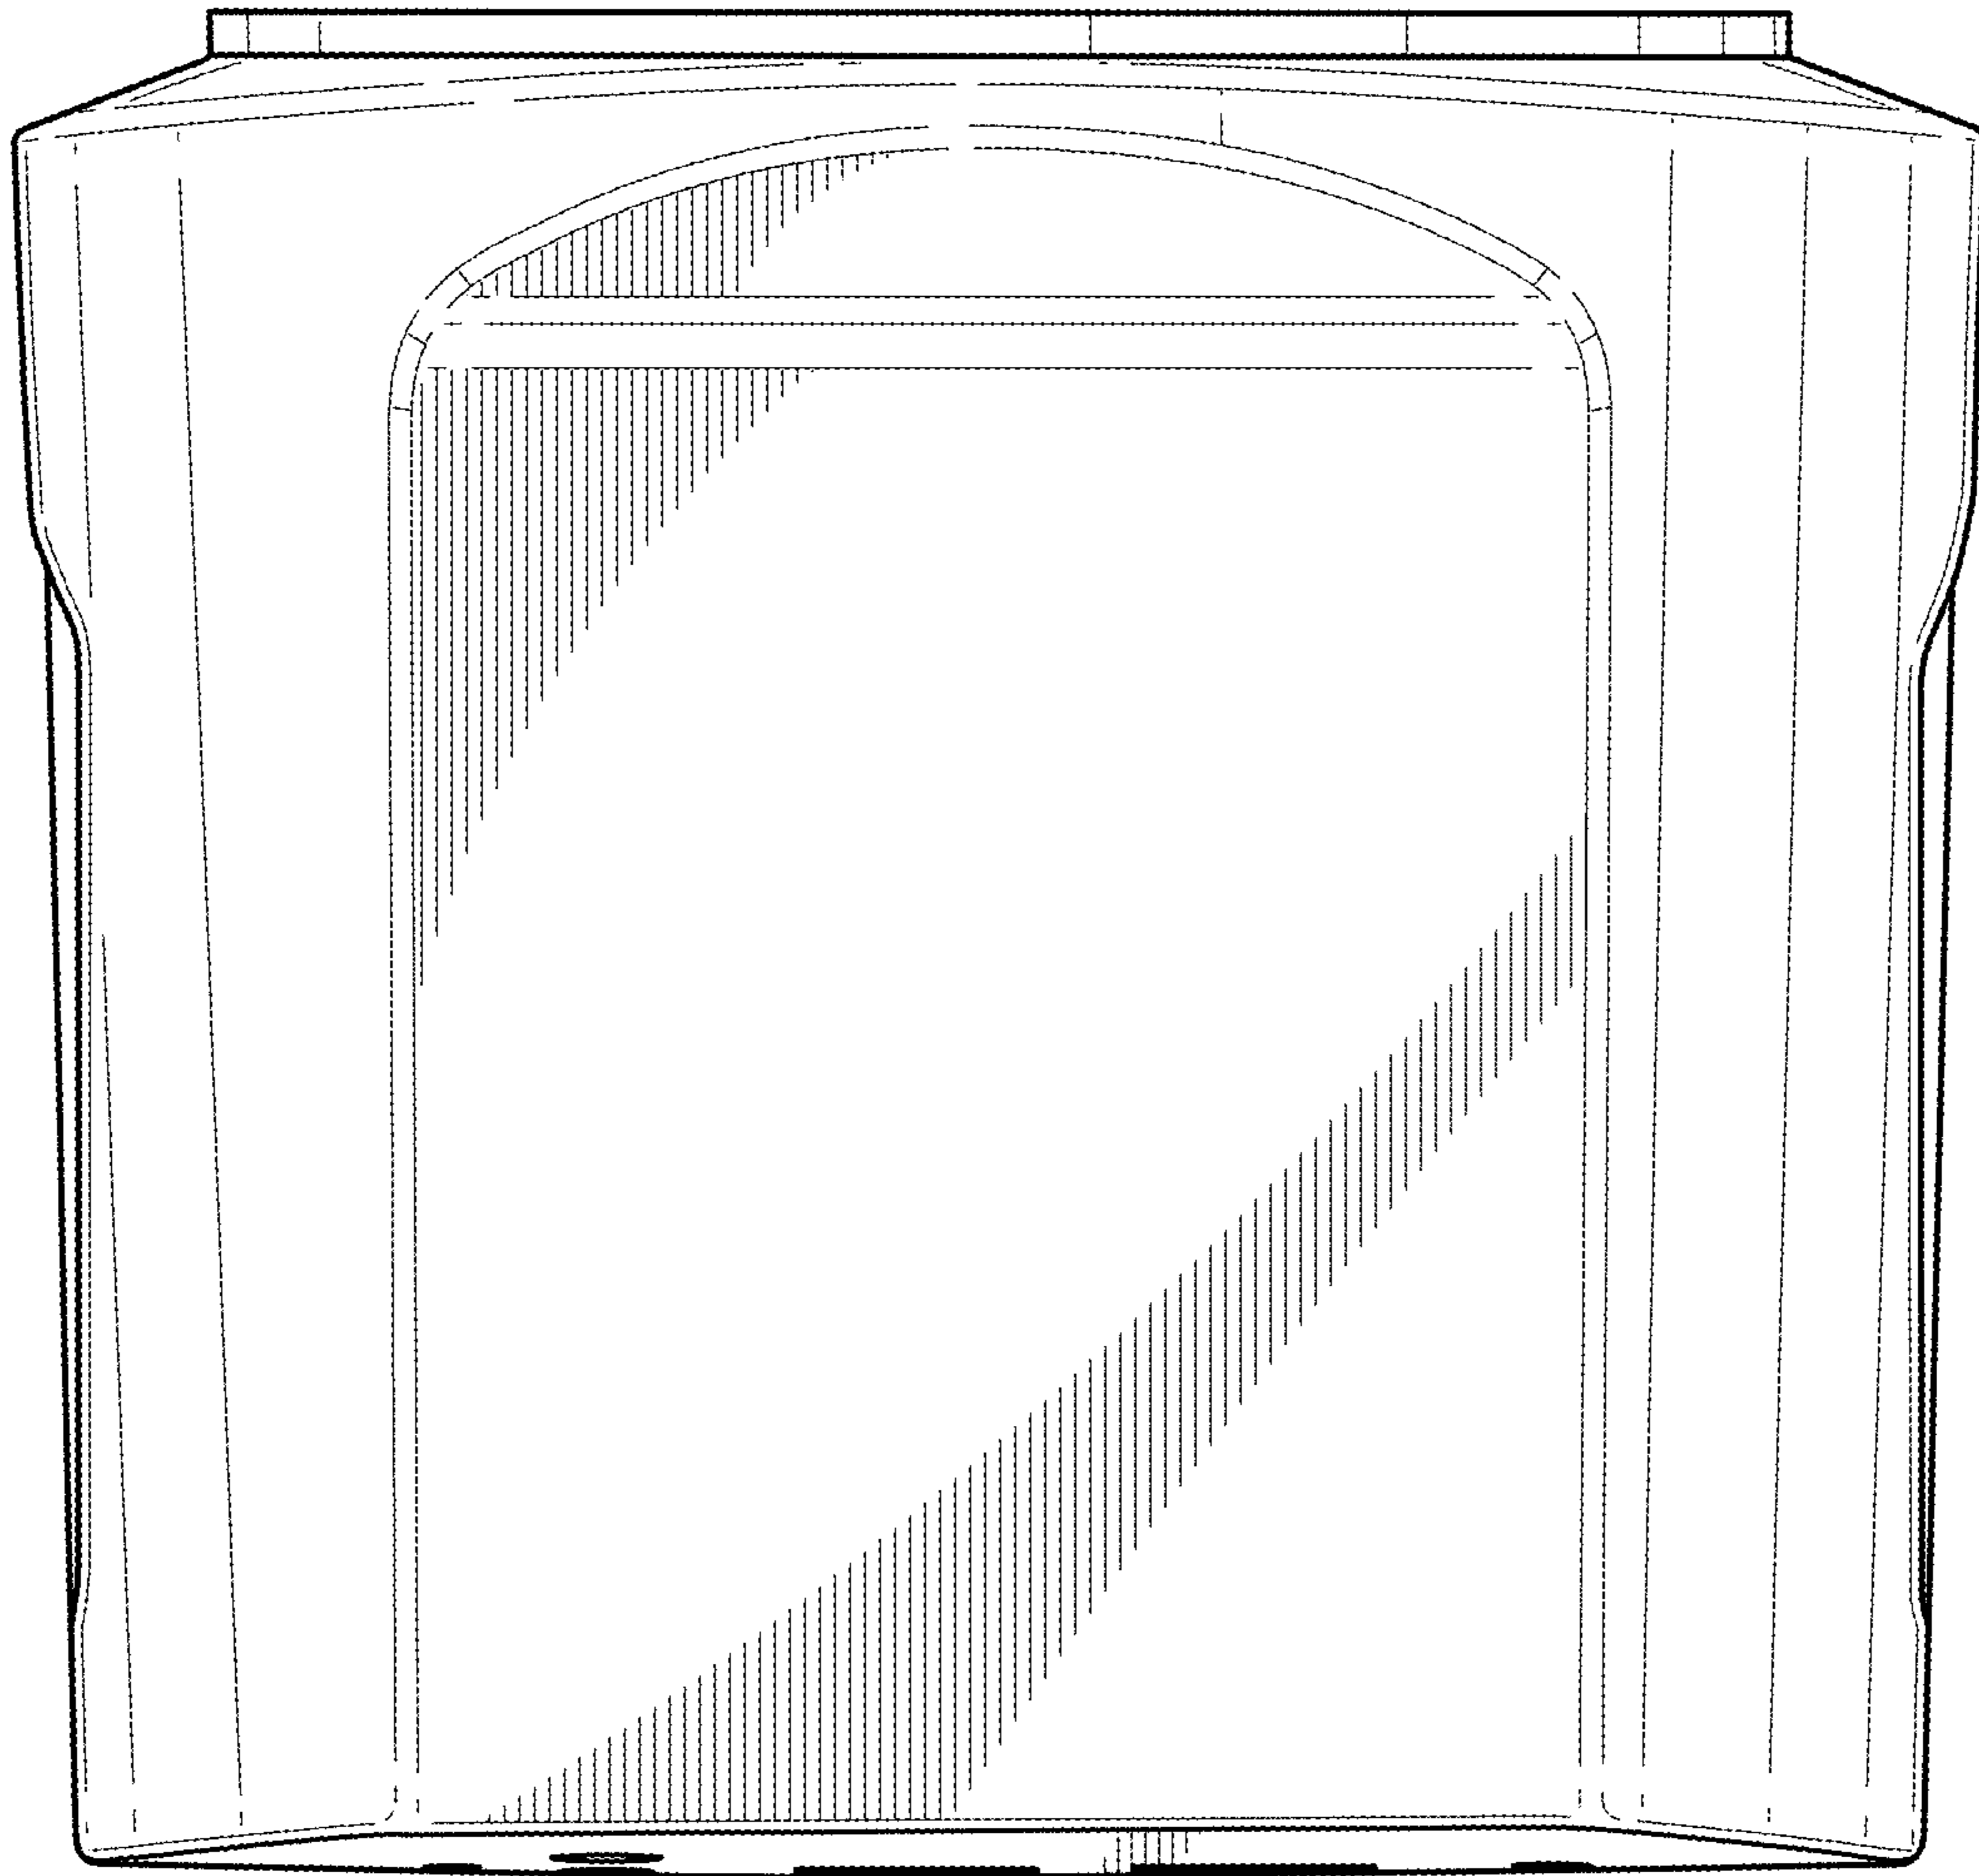


**FIG. 2**

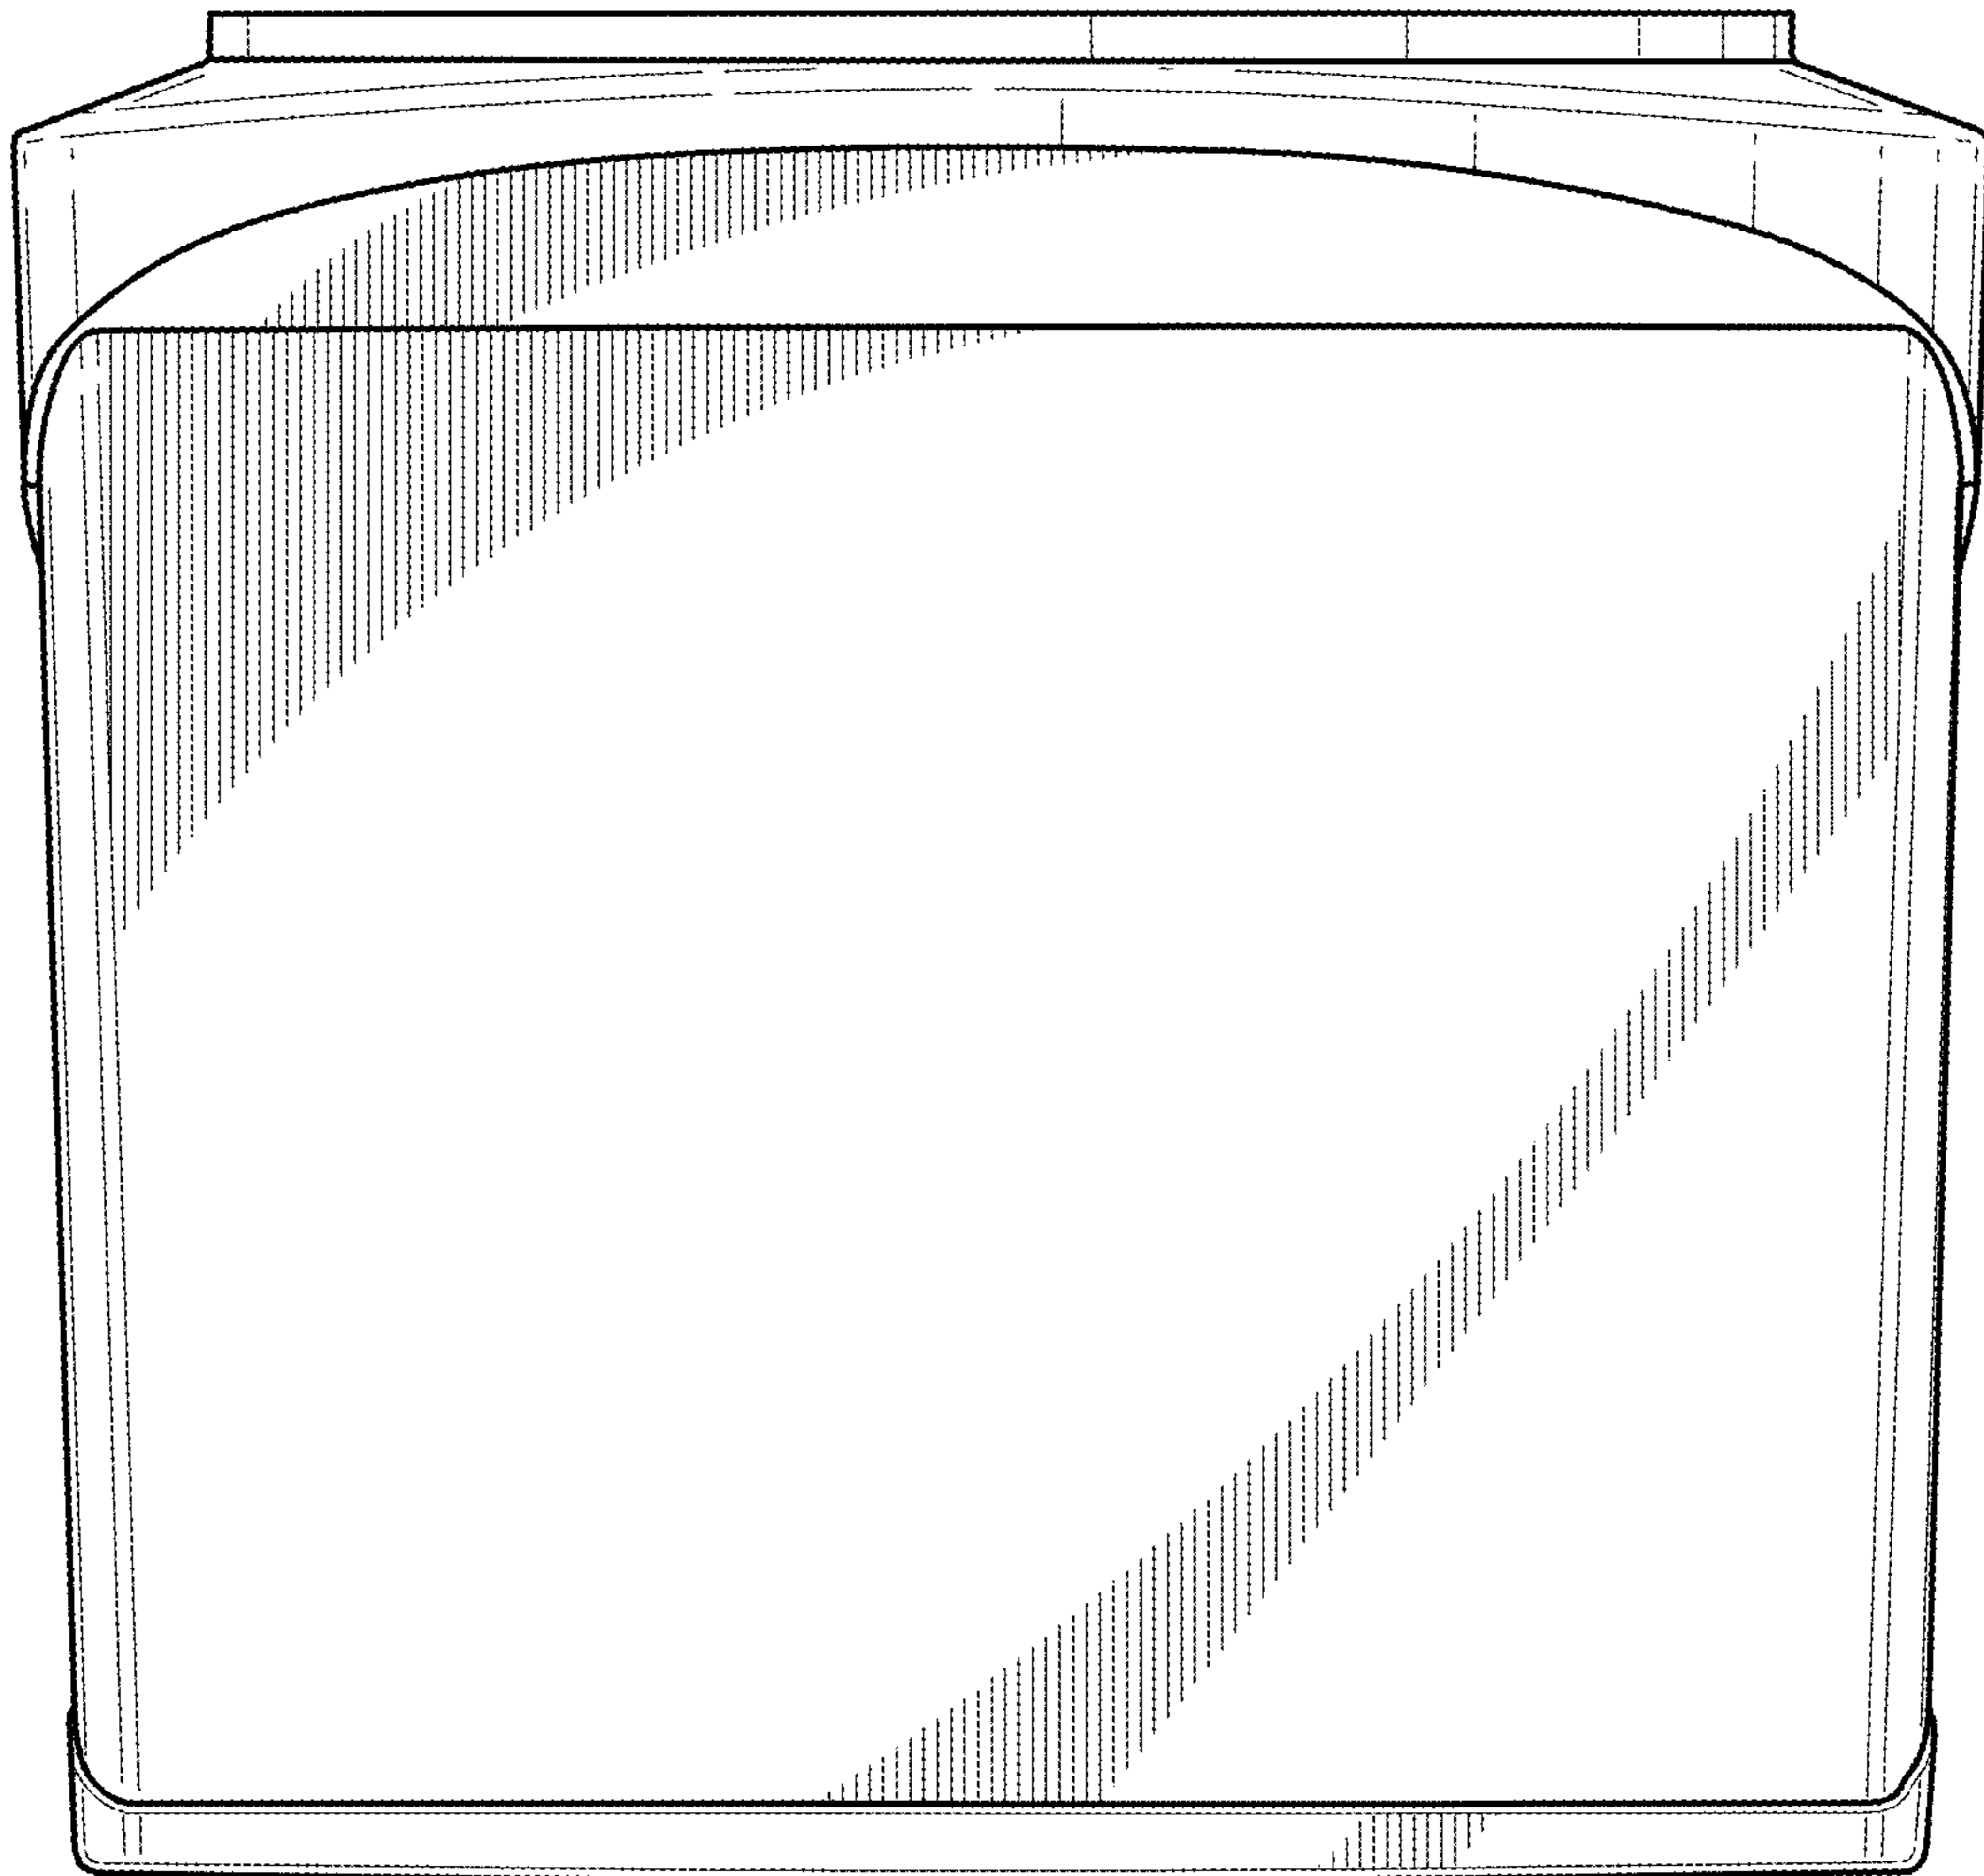


**FIG. 3**

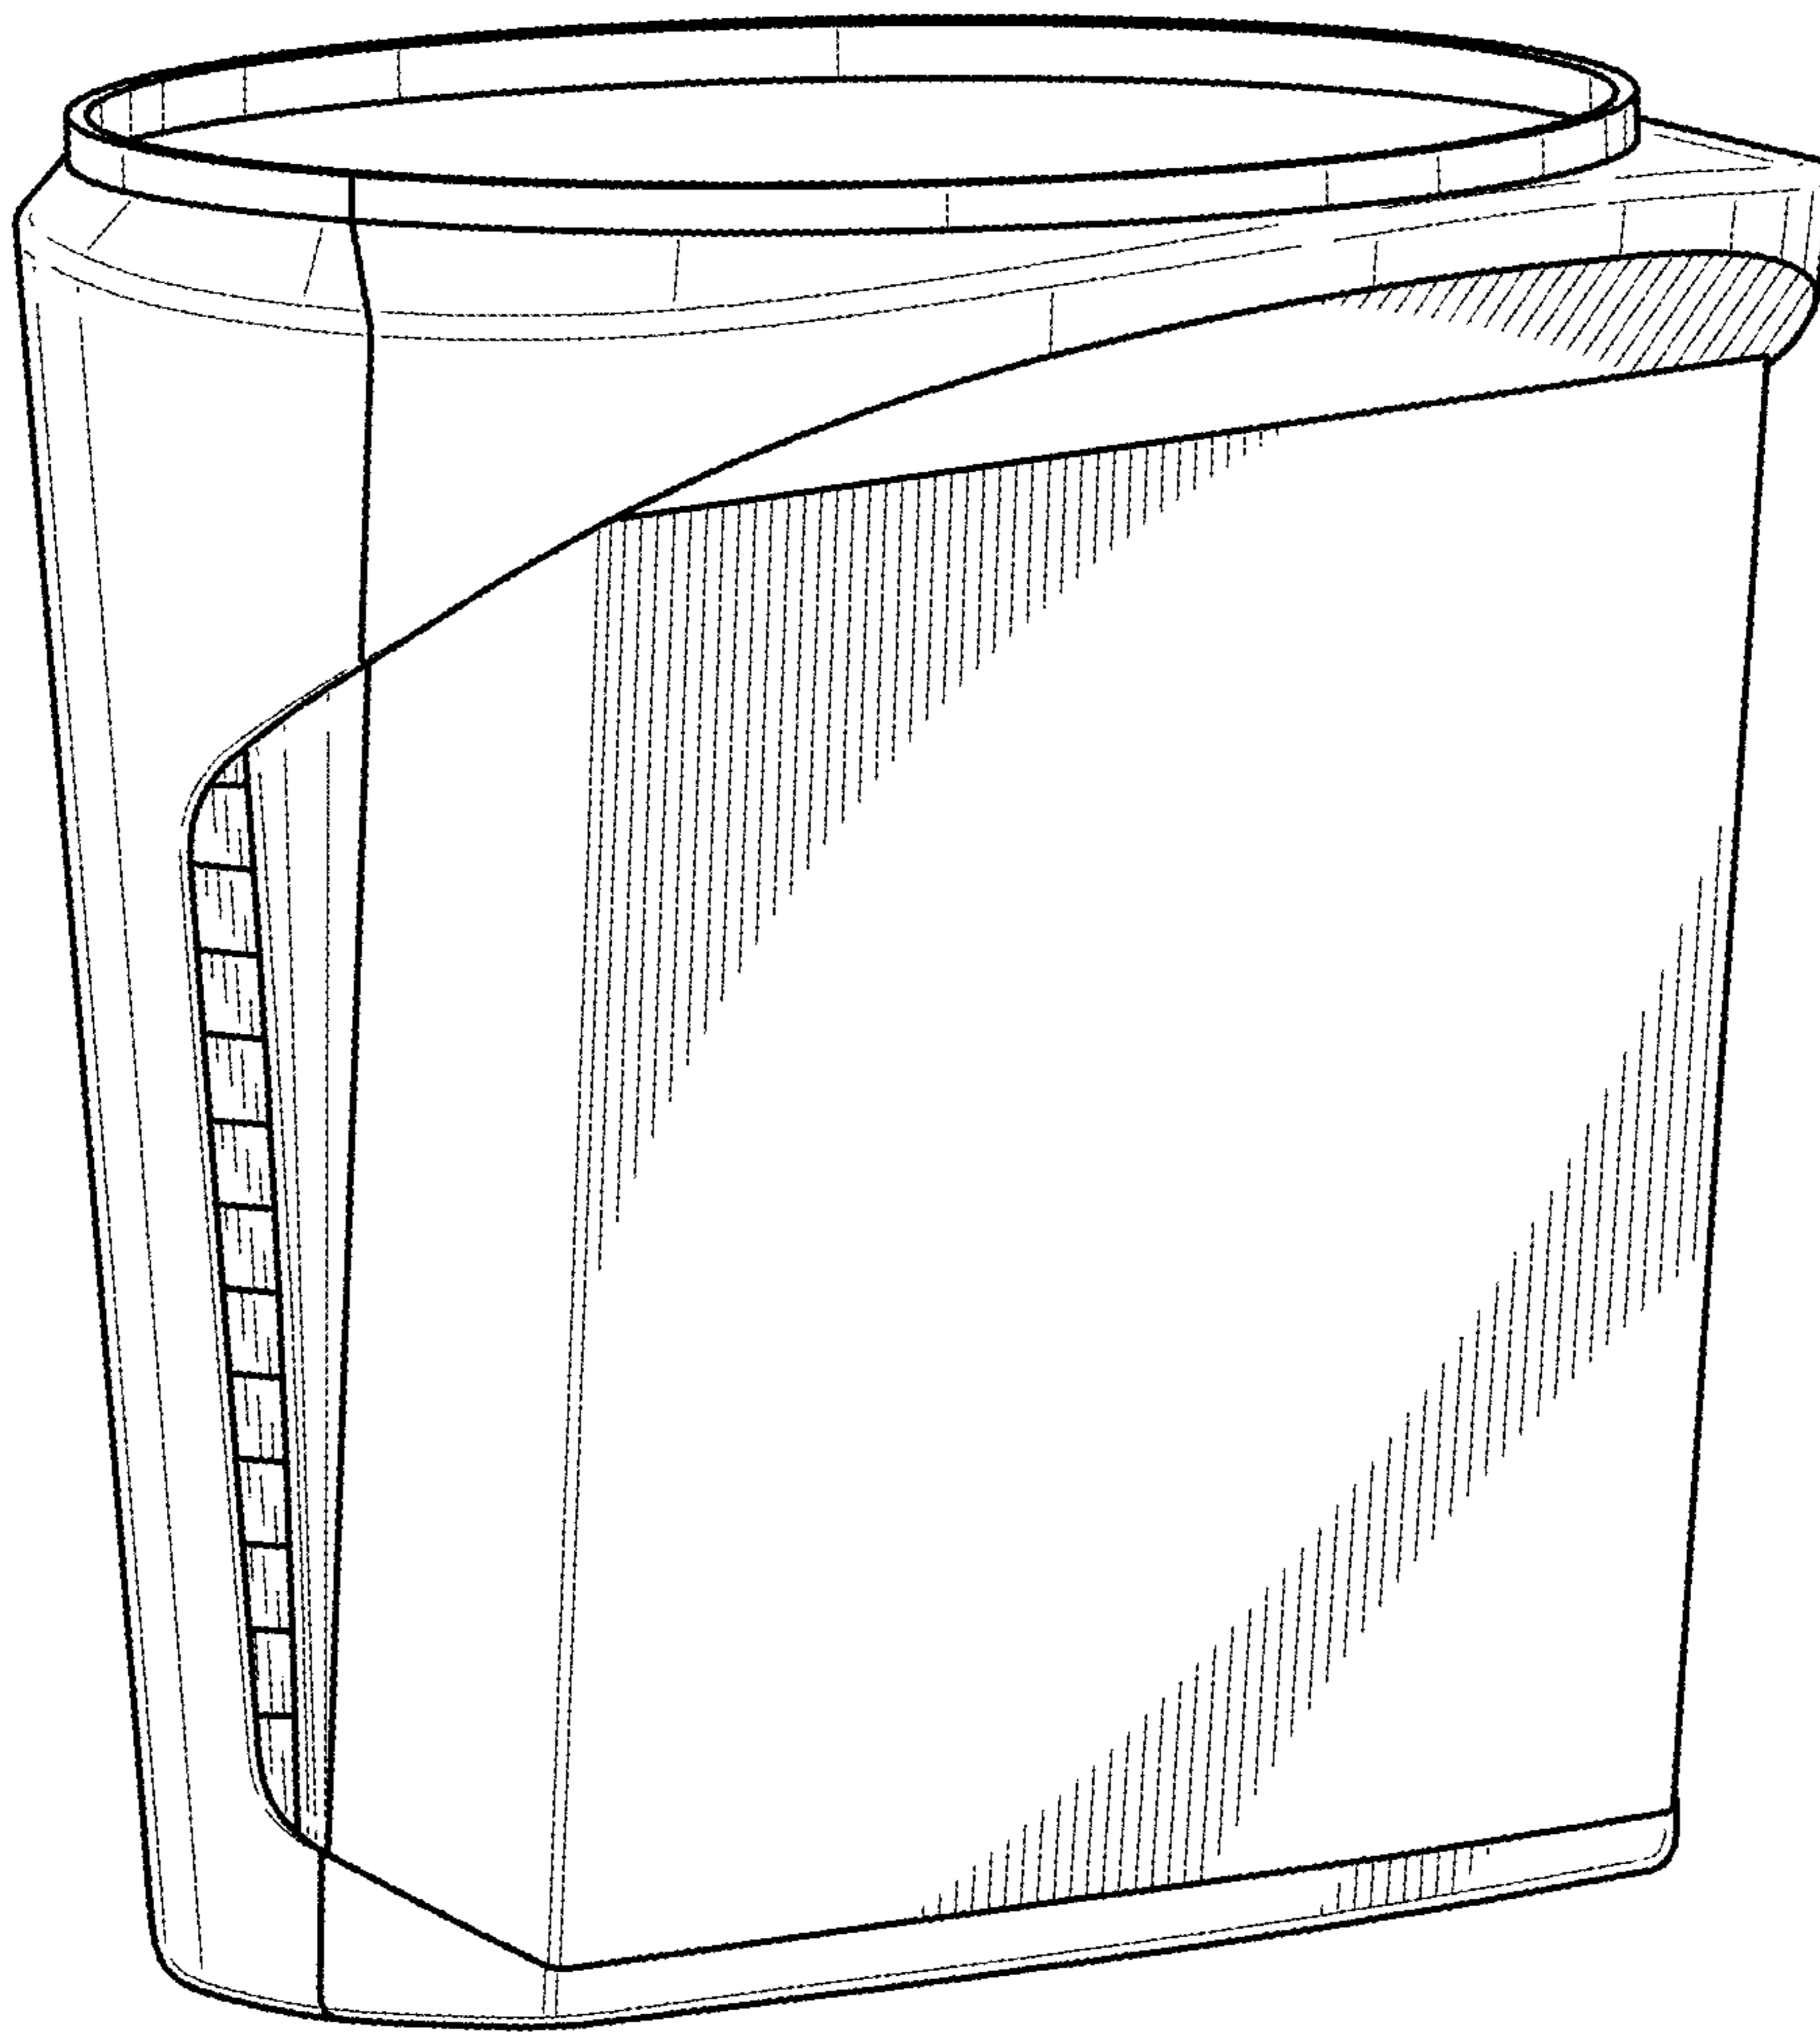

**FIG. 4**

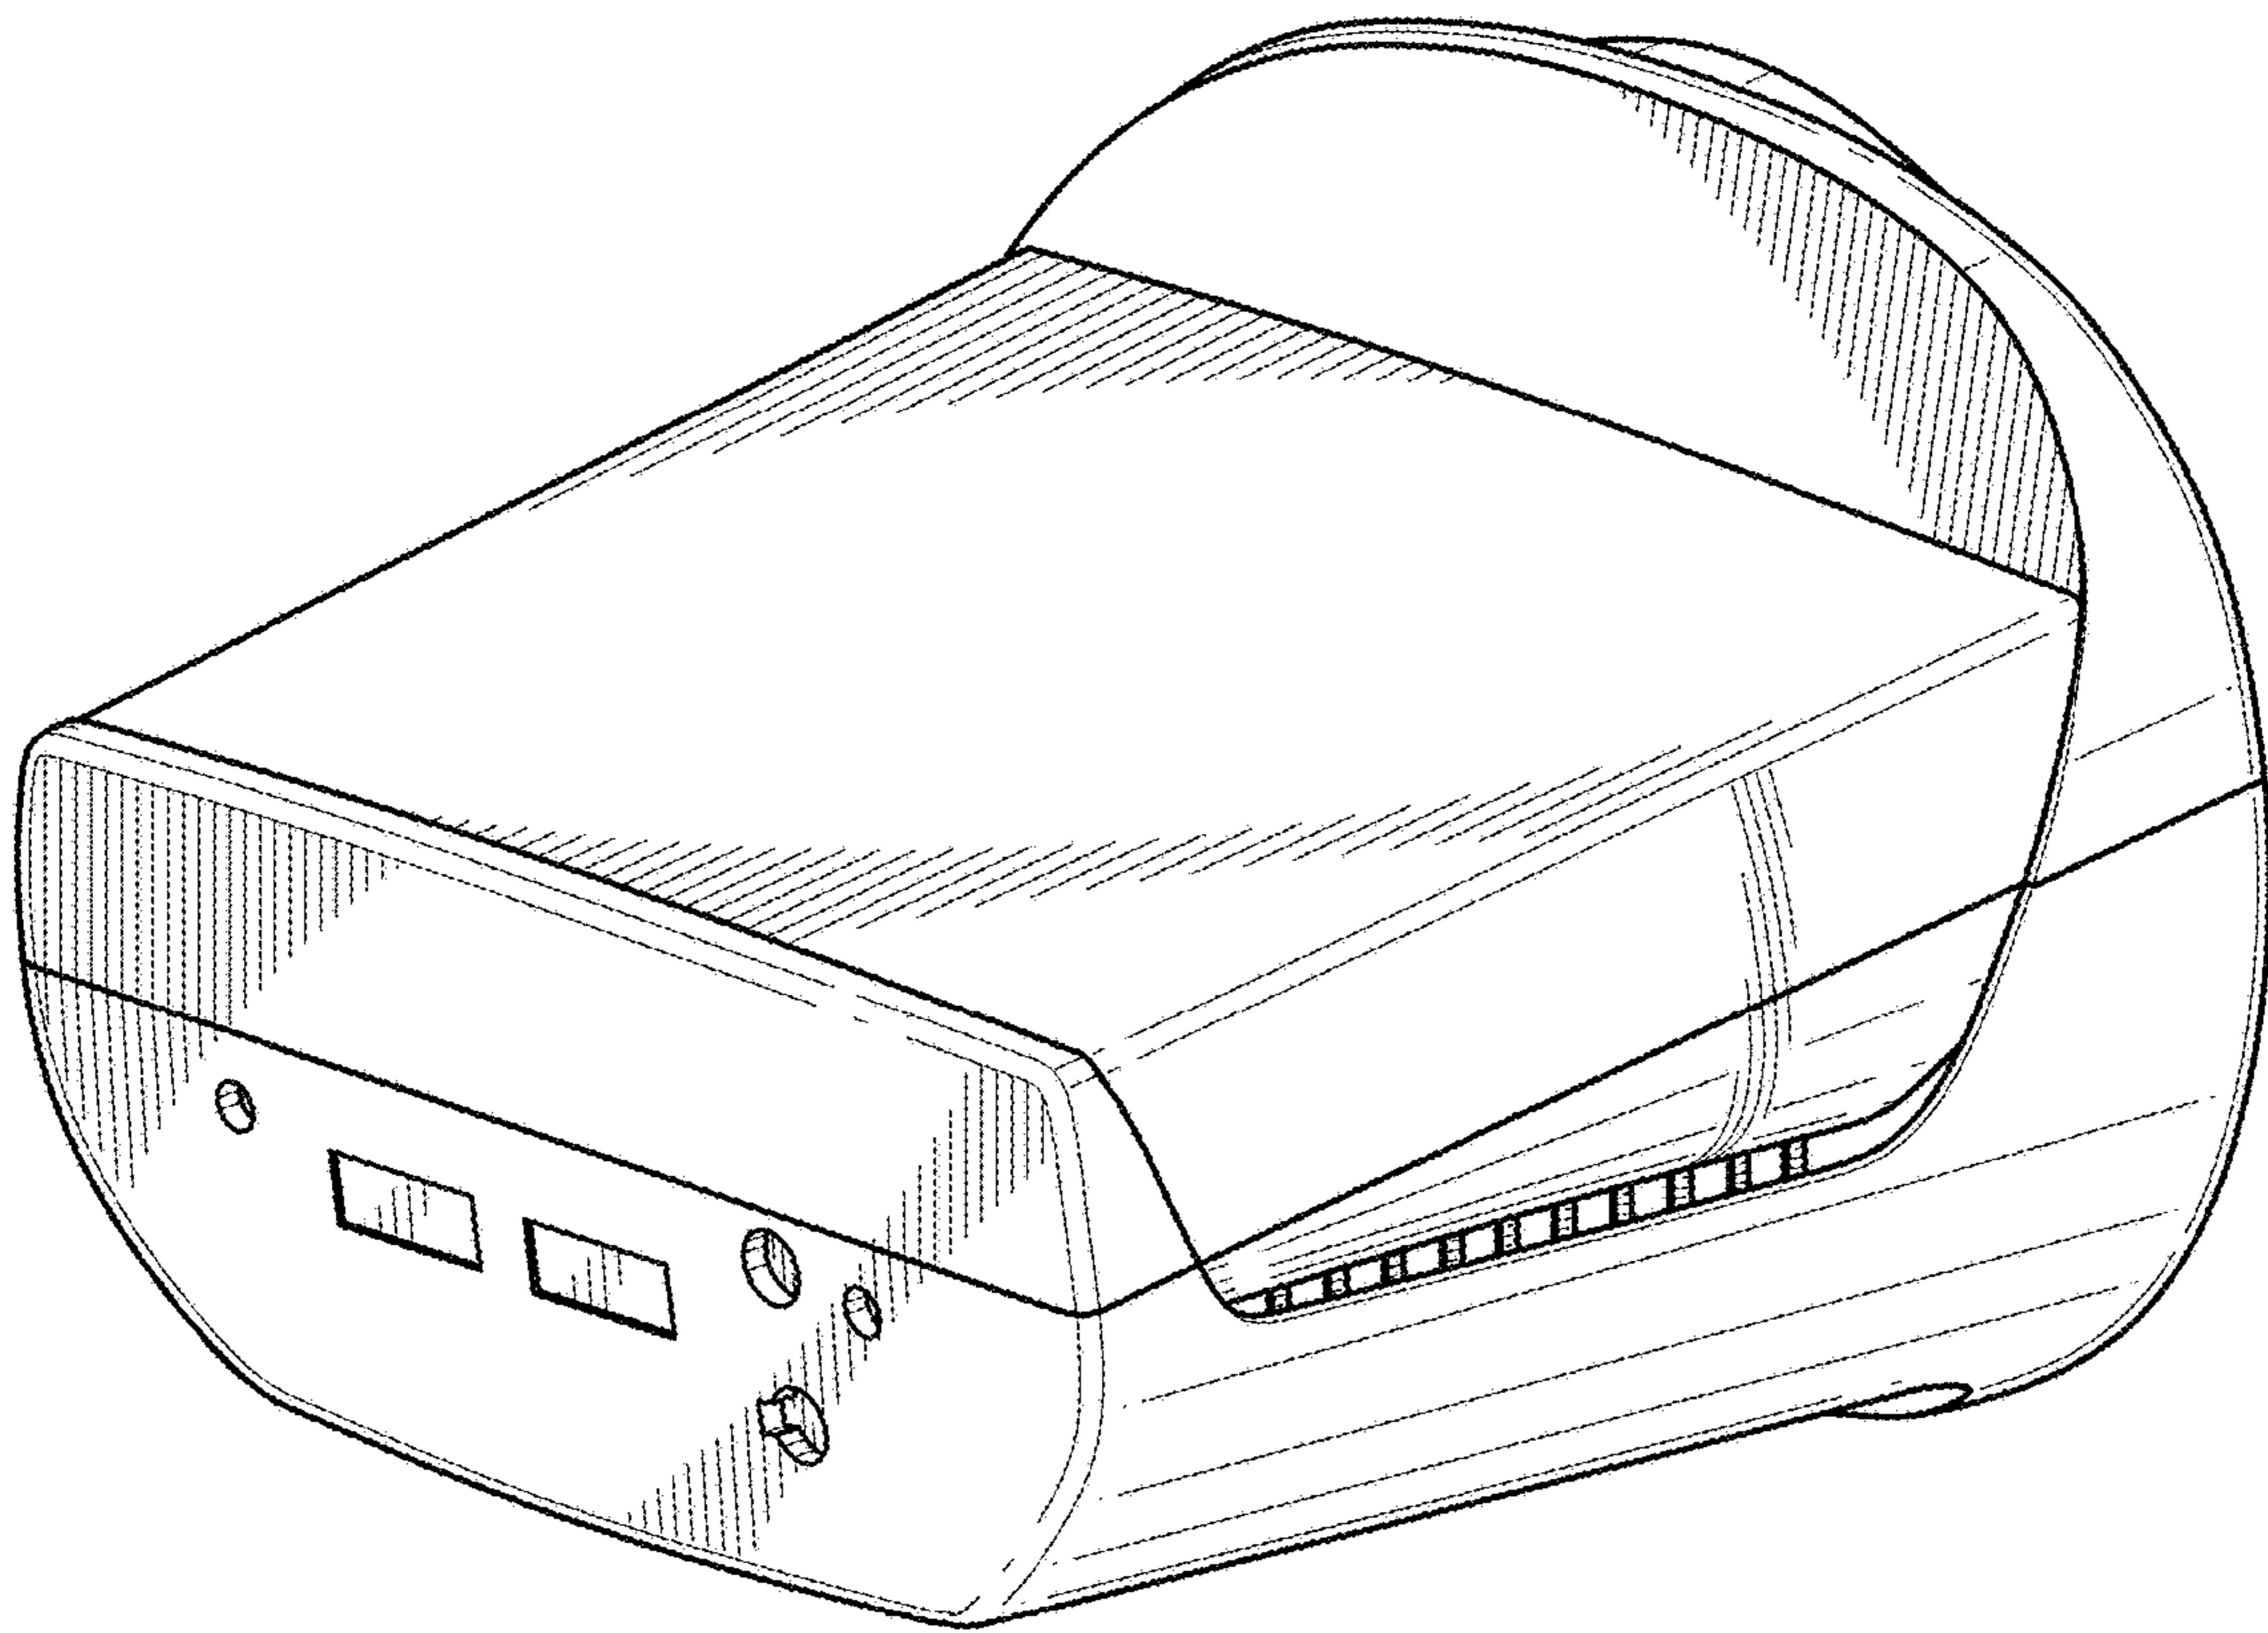


**FIG. 5**

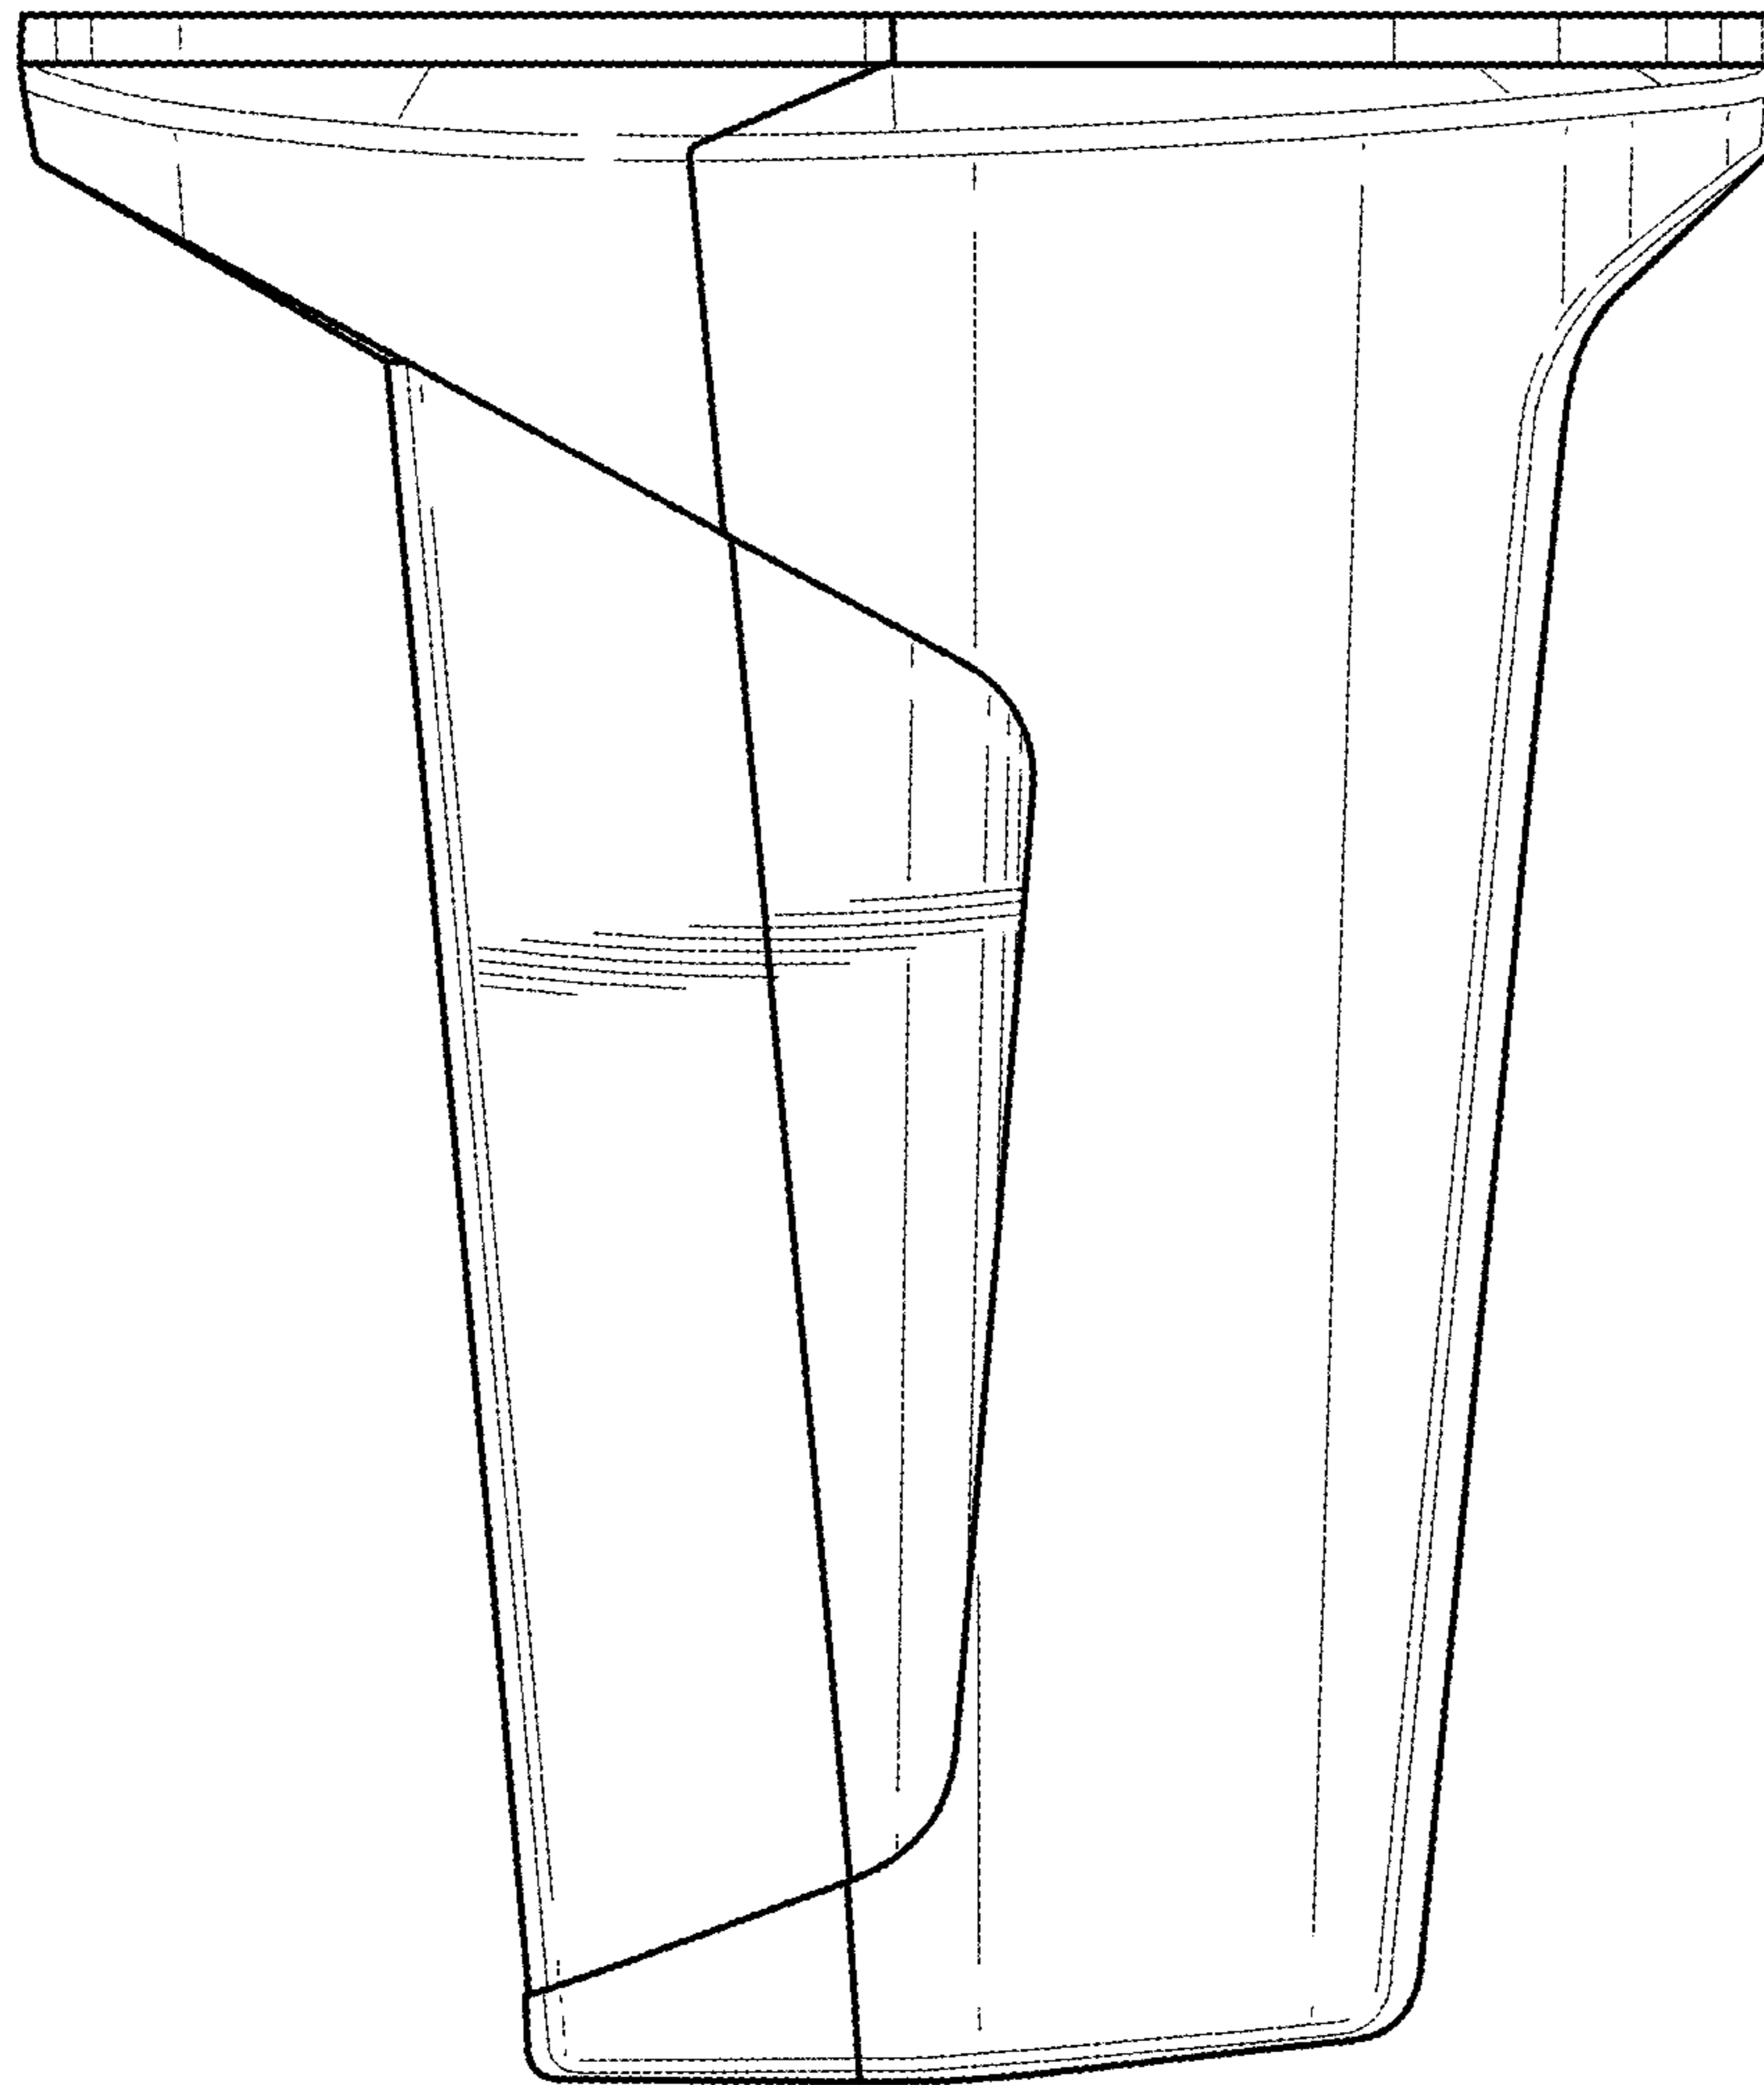

**FIG. 6**



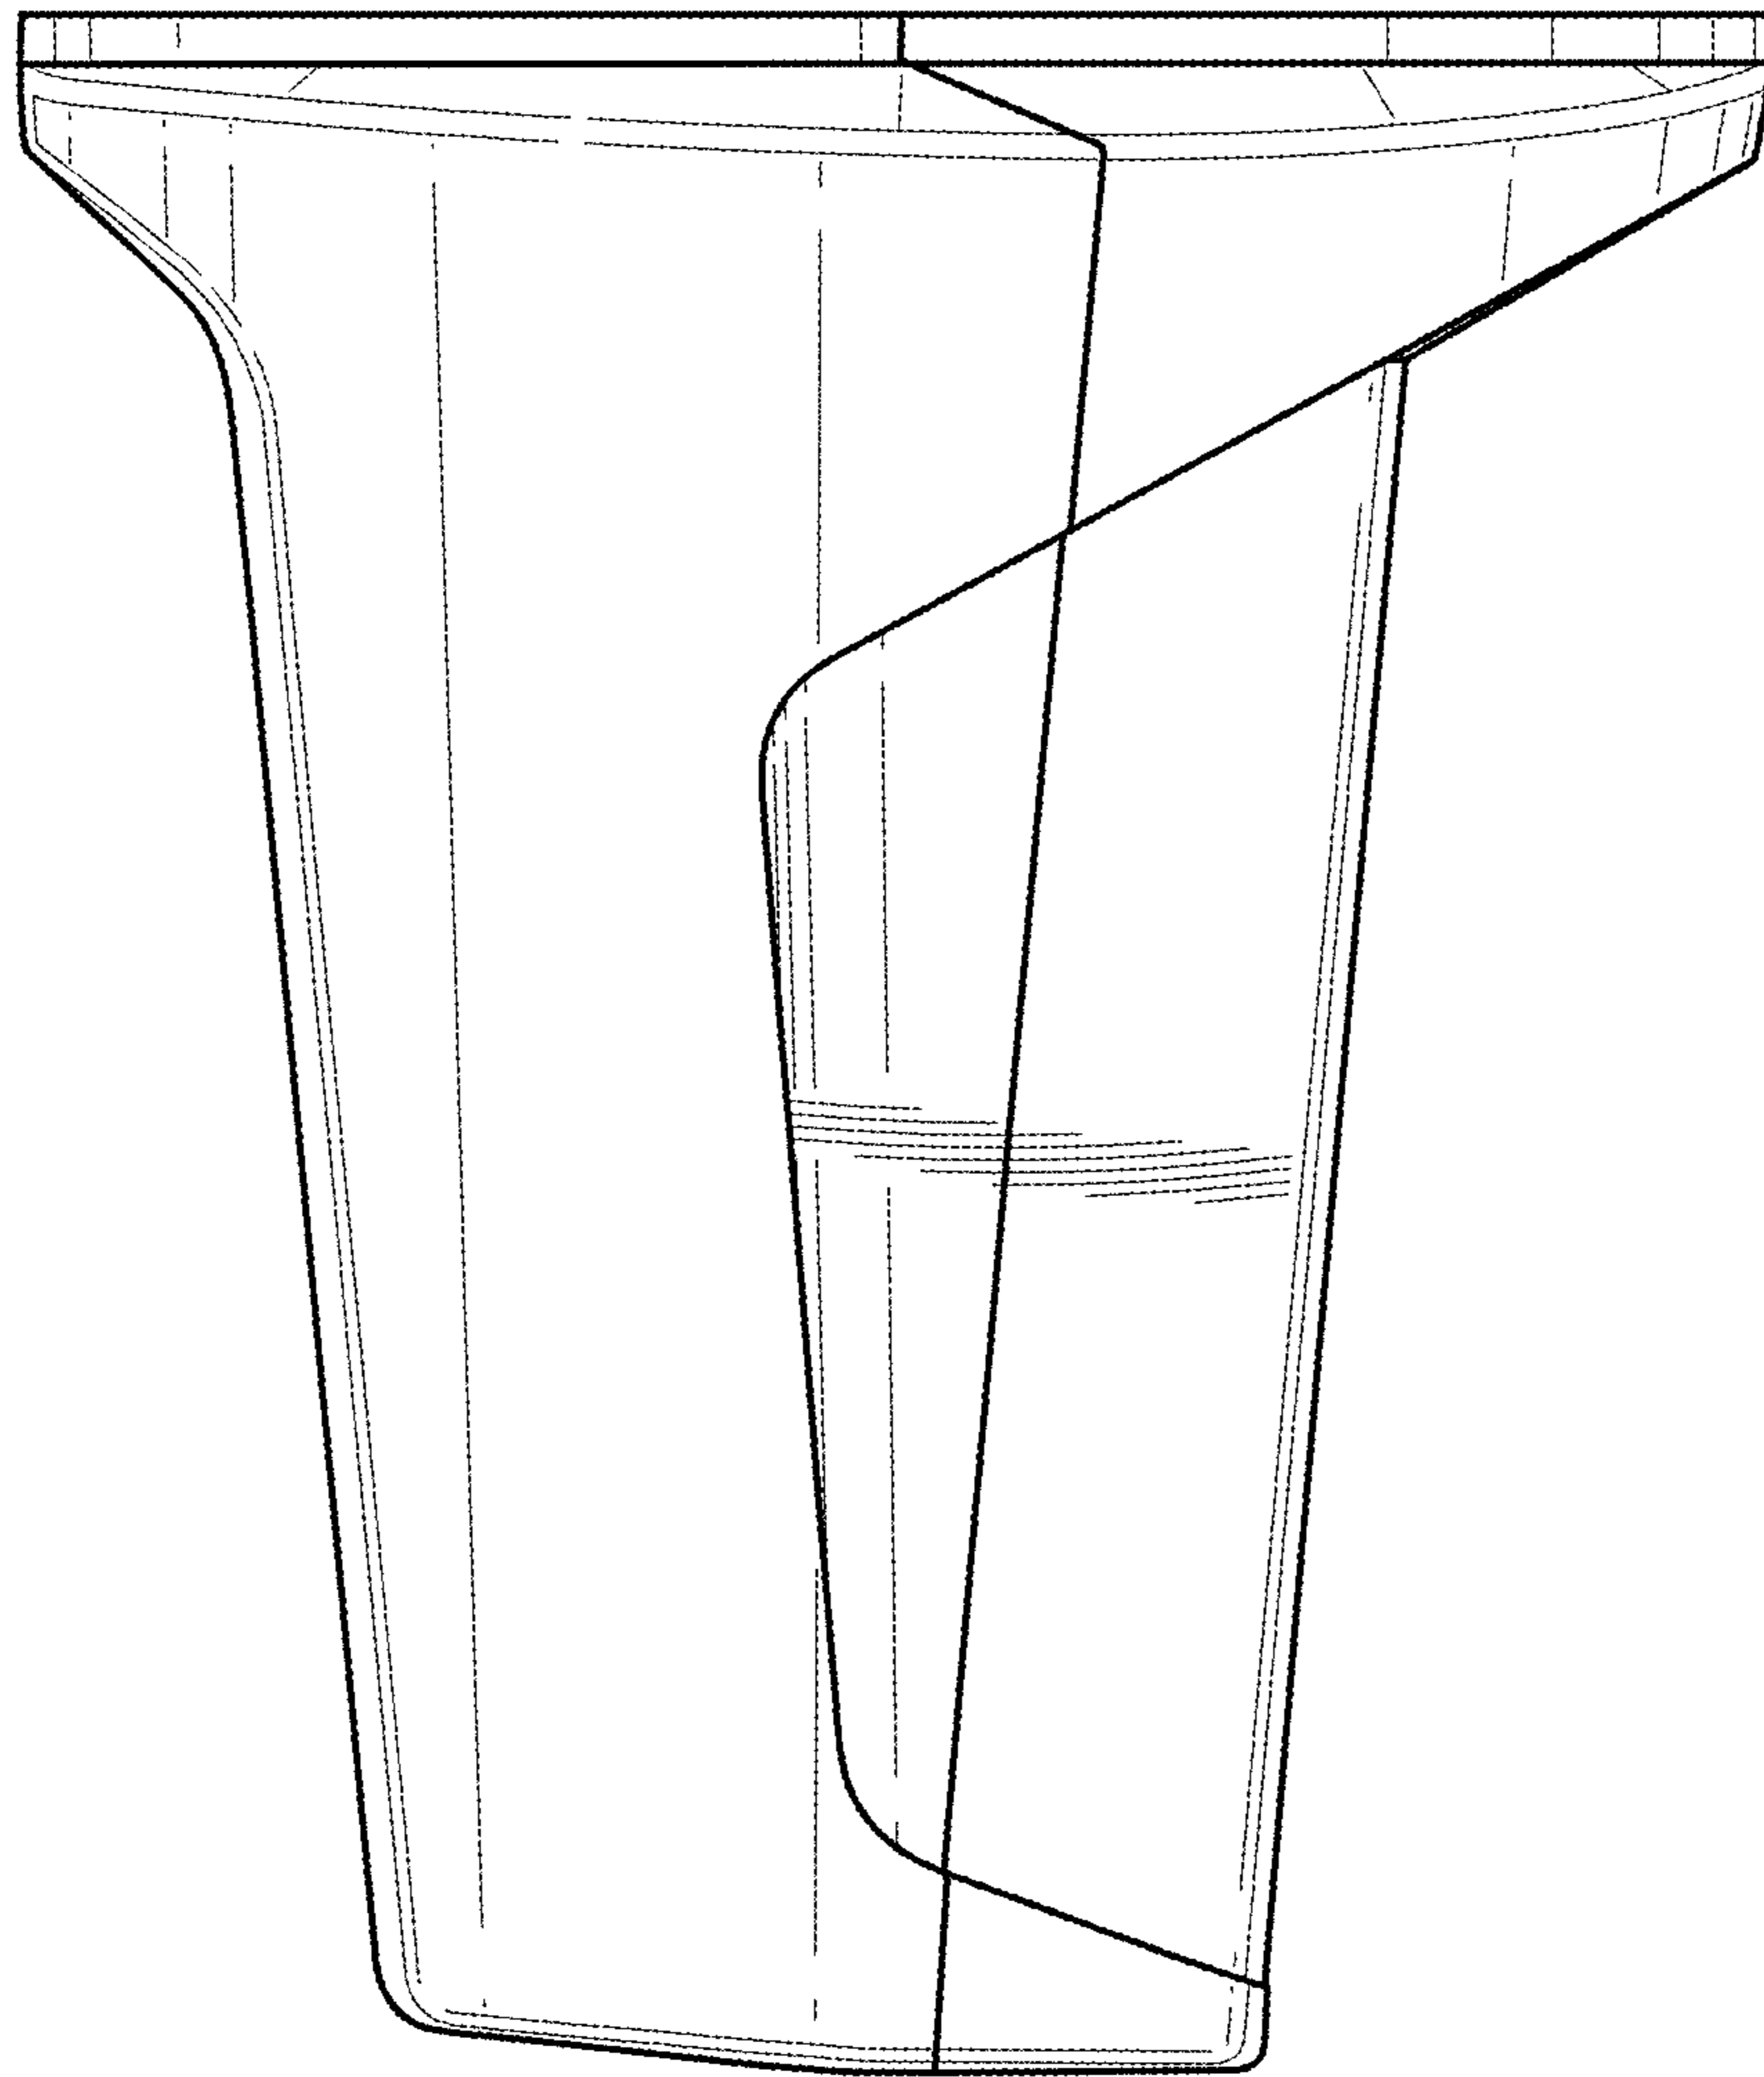

**FIG. 7**