

US00D794664S

(12) **United States Design Patent** (10) **Patent No.:** **US D794,664 S**
Okabe et al. (45) **Date of Patent:** **** Aug. 15, 2017**

(54) **DISPLAY SCREEN FOR MEDICAL INFORMATION MANAGEMENT APPARATUS WITH GRAPHICAL USER INTERFACE**

D664,971 S * 8/2012 Lee D14/486
D666,625 S * 9/2012 Gilmore D14/485
D675,224 S * 1/2013 Lee D14/488

(Continued)

(71) Applicant: **FUJIFILM Corporation**, Minato-ku, Tokyo (JP)

(72) Inventors: **Yuki Okabe**, Tokyo (JP); **Yasuyo Nenoki**, Tokyo (JP)

(73) Assignee: **FUJIFILM Corporation**, Minato-ku, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/514,338**

(22) Filed: **Jan. 12, 2015**

(30) **Foreign Application Priority Data**

Jul. 14, 2014 (JP) 2014-015355

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495; 348/14.01; 715/769, 784; D20/11; D21/324, 325
CPC G06F 3/048; G06F 3/04817; G06F 3/0482; G06F 3/04842; G06F 3/0485; G06F 3/04883; G06F 19/321; G06F 21/10; H04L 67/22; G06K 9/6212; A61B 5/055; A61B 6/3217

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D579,456 S * 10/2008 Chen D14/485
D598,923 S * 8/2009 Chen D14/485
D658,196 S * 4/2012 Wood D14/486
D658,673 S * 5/2012 Velasco D14/488
D664,967 S * 8/2012 Lee D14/485
D664,968 S * 8/2012 Lee D14/485

OTHER PUBLICATIONS

“CXDI Control Software NE”, posted at virtualimaging-fl.com, Oct. 31, 2010, [site visited Mar. 29, 2016]. Available from Internet: <http://www.virtualimaging-fl.com/Healthcare_Products/Software_Solutions/CXDI_Control_Software_NE/CXDI_Control_Software_tabbedLandingPage.shtml>.*

“Nurses: Spend More Time in Direct Patient Care with RTLS”, posted at versustech.com, Feb. 28, 2013, [site visited Mar. 29, 2016]. Available from Internet: <<http://www.versustech.com/rtls-benefits/nurses>>.*

(Continued)

Primary Examiner — Karen Kearney

Assistant Examiner — John M Otte

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for a display screen for medical information management apparatus with graphical user interface, as shown and described.


DESCRIPTION

FIG. 1 is a front view of a display screen for medical information management apparatus with graphical user interface showing a first embodiment of our new design; FIG. 2 is an enlarged partial view of FIG. 1, shown for clarity of illustration; and,

FIG. 3 is a front view of a second embodiment of a display screen for medical information management apparatus with graphical user interface.

The broken line showing of the display screen is included for the purpose of illustrating portions of the display screen for medical information management apparatus with graphical user interface and form no part of the claimed design. The perimeters of the underlying portion of the display screen and the graphical user interface are understood to be flush.

1 Claim, 3 Drawing Sheets

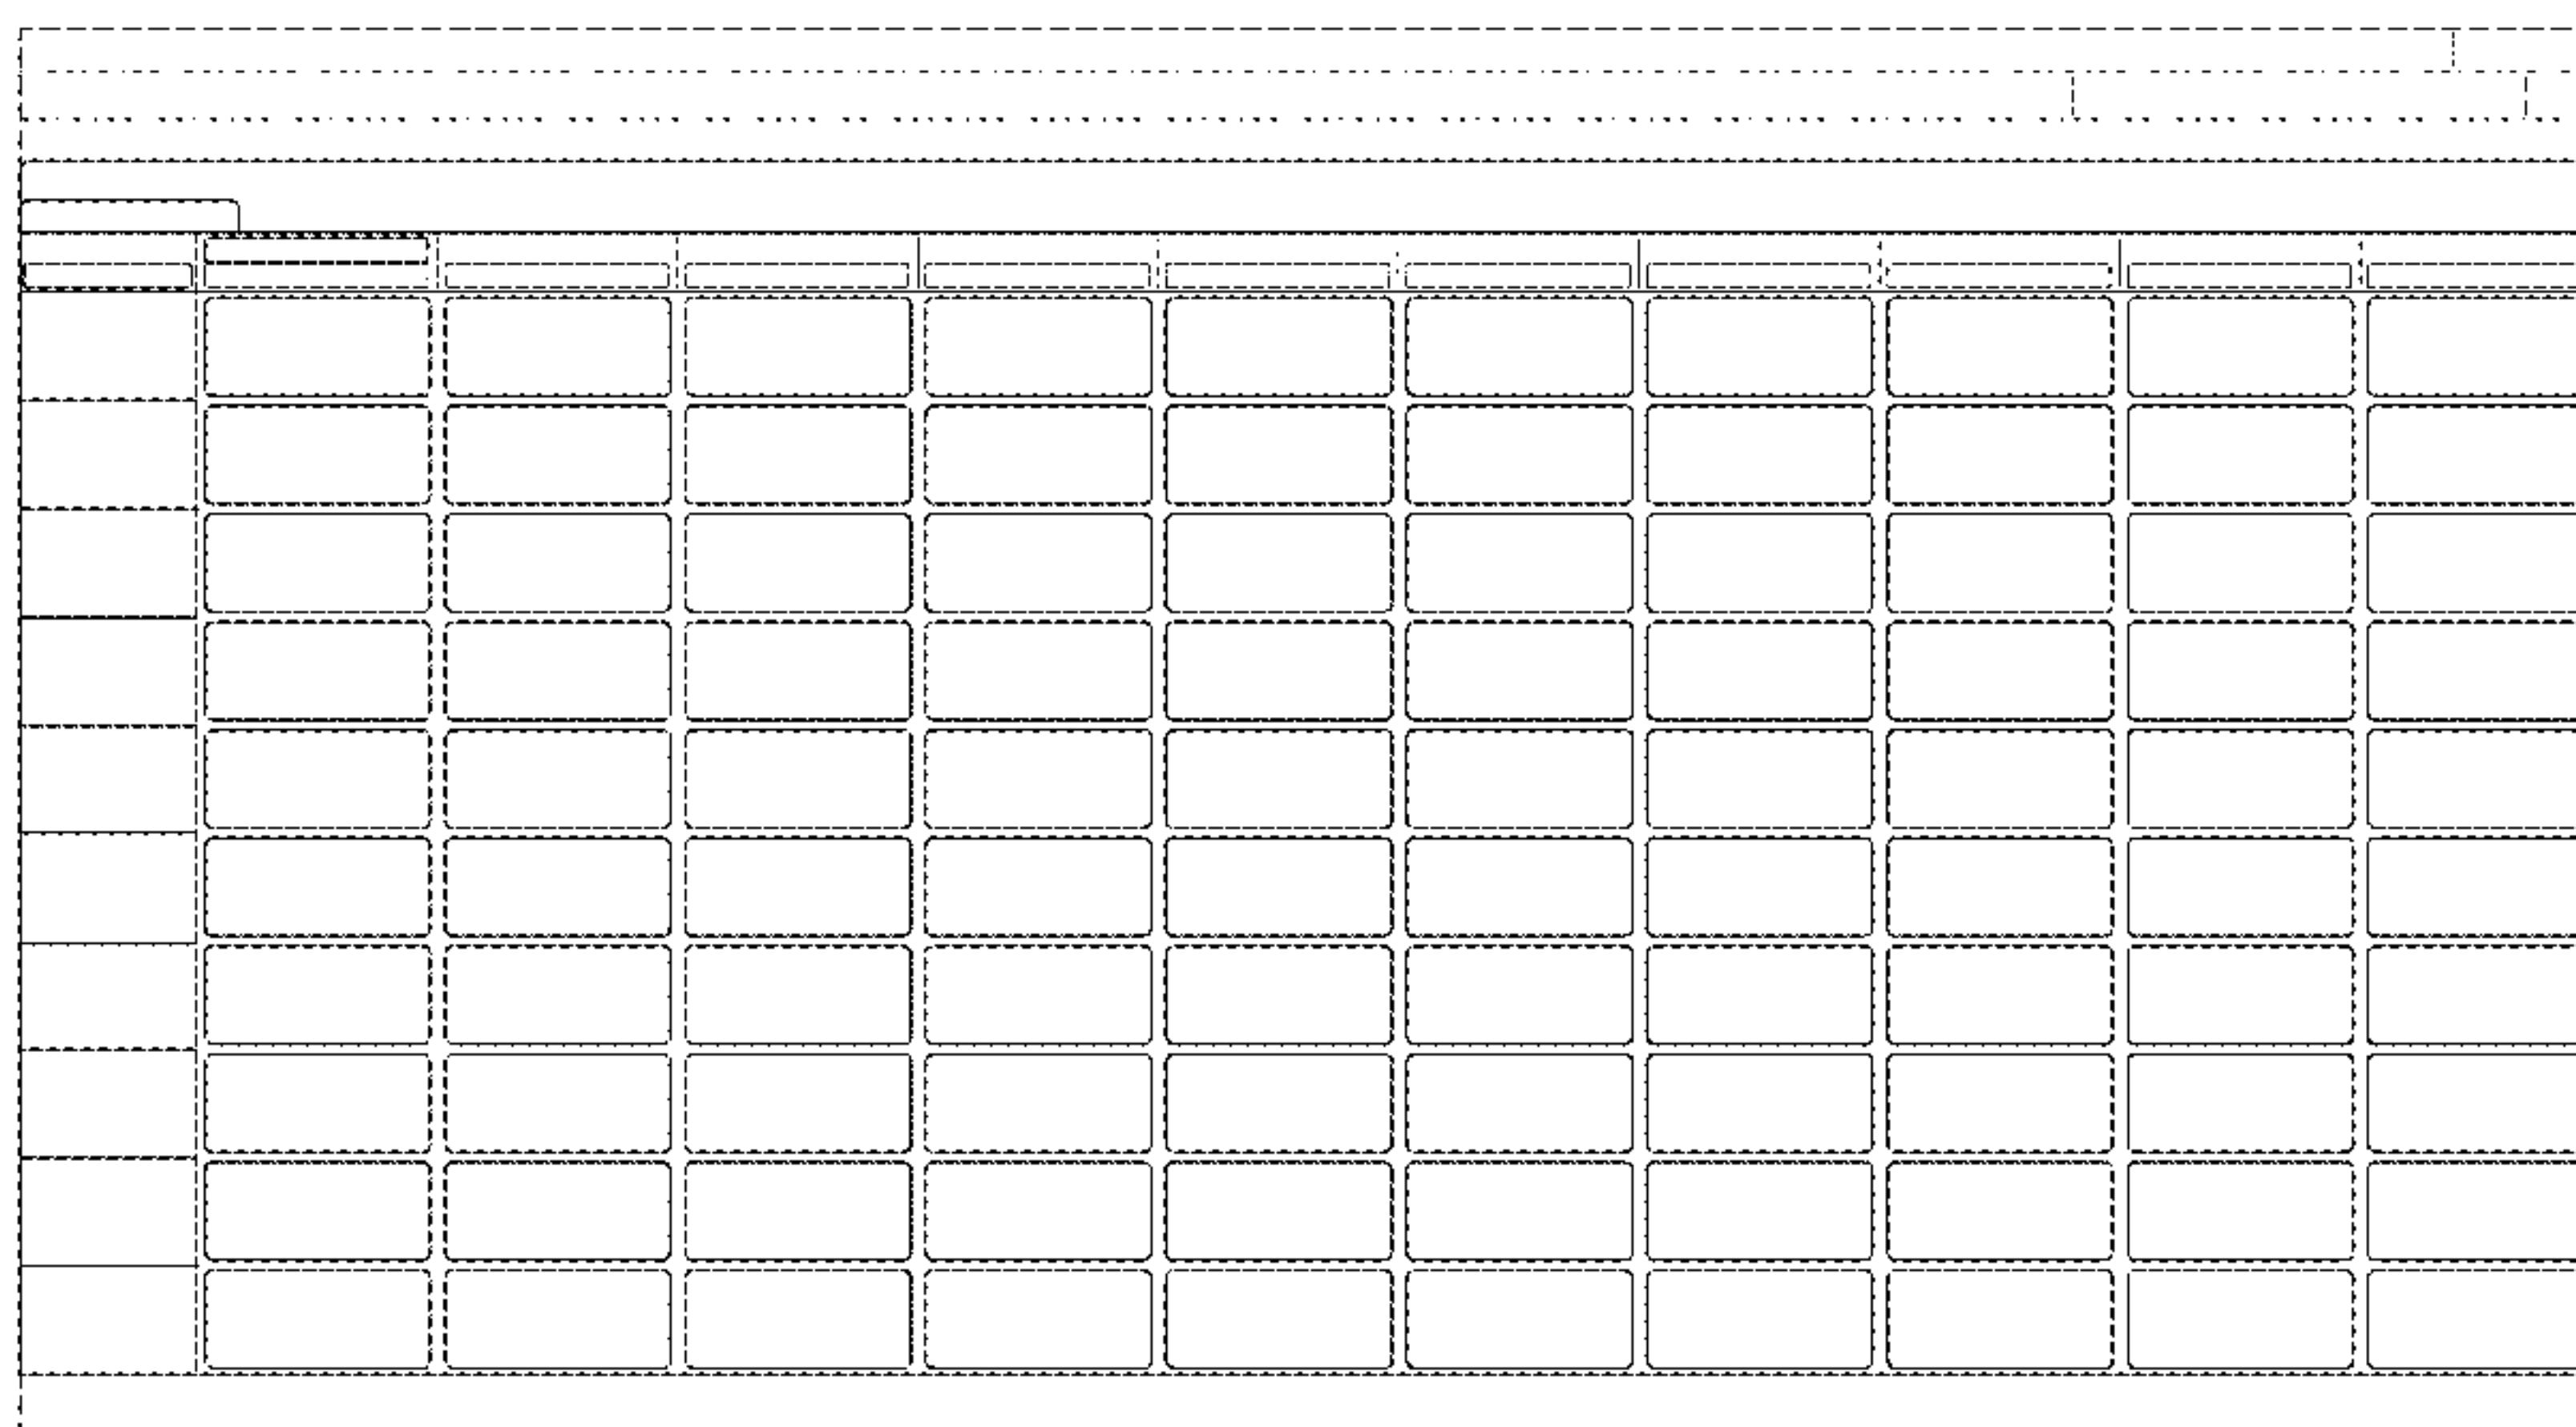

(56)

References Cited

U.S. PATENT DOCUMENTS

D680,548	S *	4/2013	Goldstein	D14/485
D705,787	S *	5/2014	Talbot	D14/485
D707,704	S *	6/2014	Capua	D14/488
D710,879	S *	8/2014	Elston	D14/488
8,863,016	B2 *	10/2014	Victor	715/769
D717,312	S *	11/2014	Matas	G06F 3/04883 D14/485
D737,831	S *	9/2015	Lee	D14/485
D738,384	S *	9/2015	Kim	D14/485
D741,339	S *	10/2015	Jung	D14/485
D759,669	S *	6/2016	Matsumiya	D14/485
D762,655	S *	8/2016	Kai	D14/485
D764,481	S *	8/2016	Omiya	D14/485
D765,136	S *	8/2016	Lee	D14/488
D768,159	S *	10/2016	McRae	D14/486
2011/0141218	A1 *	6/2011	Stancato	G06F 21/10 348/14.01
2014/0096070	A1 *	4/2014	Mishima	G06F 3/0485 715/784
2016/0239854	A1 *	8/2016	Neal	H04L 67/22

OTHER PUBLICATIONS

“Patient & Retail Management Software for Optometrists”, posted at samaansystems.com, Apr. 18, 2008, [site visited Mar. 29, 2016]. Available from Internet: <<http://samaansystems.com/index.php?page=best-practice---optical>>.*

“SkyDesk”, posted at skydesk.jp, Nov. 3, 2013, [site visited Oct. 24, 2016]. Available from Internet: <<http://web.archive.org/web/20131103065120/https://www.skydesk.jp/en/suites/collaboration/calendar.html>>.*

“Synapse® RIS 6.2 Automates, Streamlines Workflow for Dozens of Radiology Information System Tasks”, posted at prnewswire.com, Nov. 25, 2012, [site visited Oct. 24, 2016]. Available from Internet: <<http://www.prnewswire.com/news-releases/synapse-ris-62-automates-streamlines-workflow-for-dozens-of-radiology-information-system-tasks-180757301.html>>.*

“Screen Shots of the Cottage Med EMR Open Source Software”, posted at ehcreenshots.com, May 24, 2011, [site visited Oct. 24, 2016]. Available from Internet: <<http://www.ehcreenshots.com/tag/cottage-med>>.*

* cited by examiner

FIG. 1

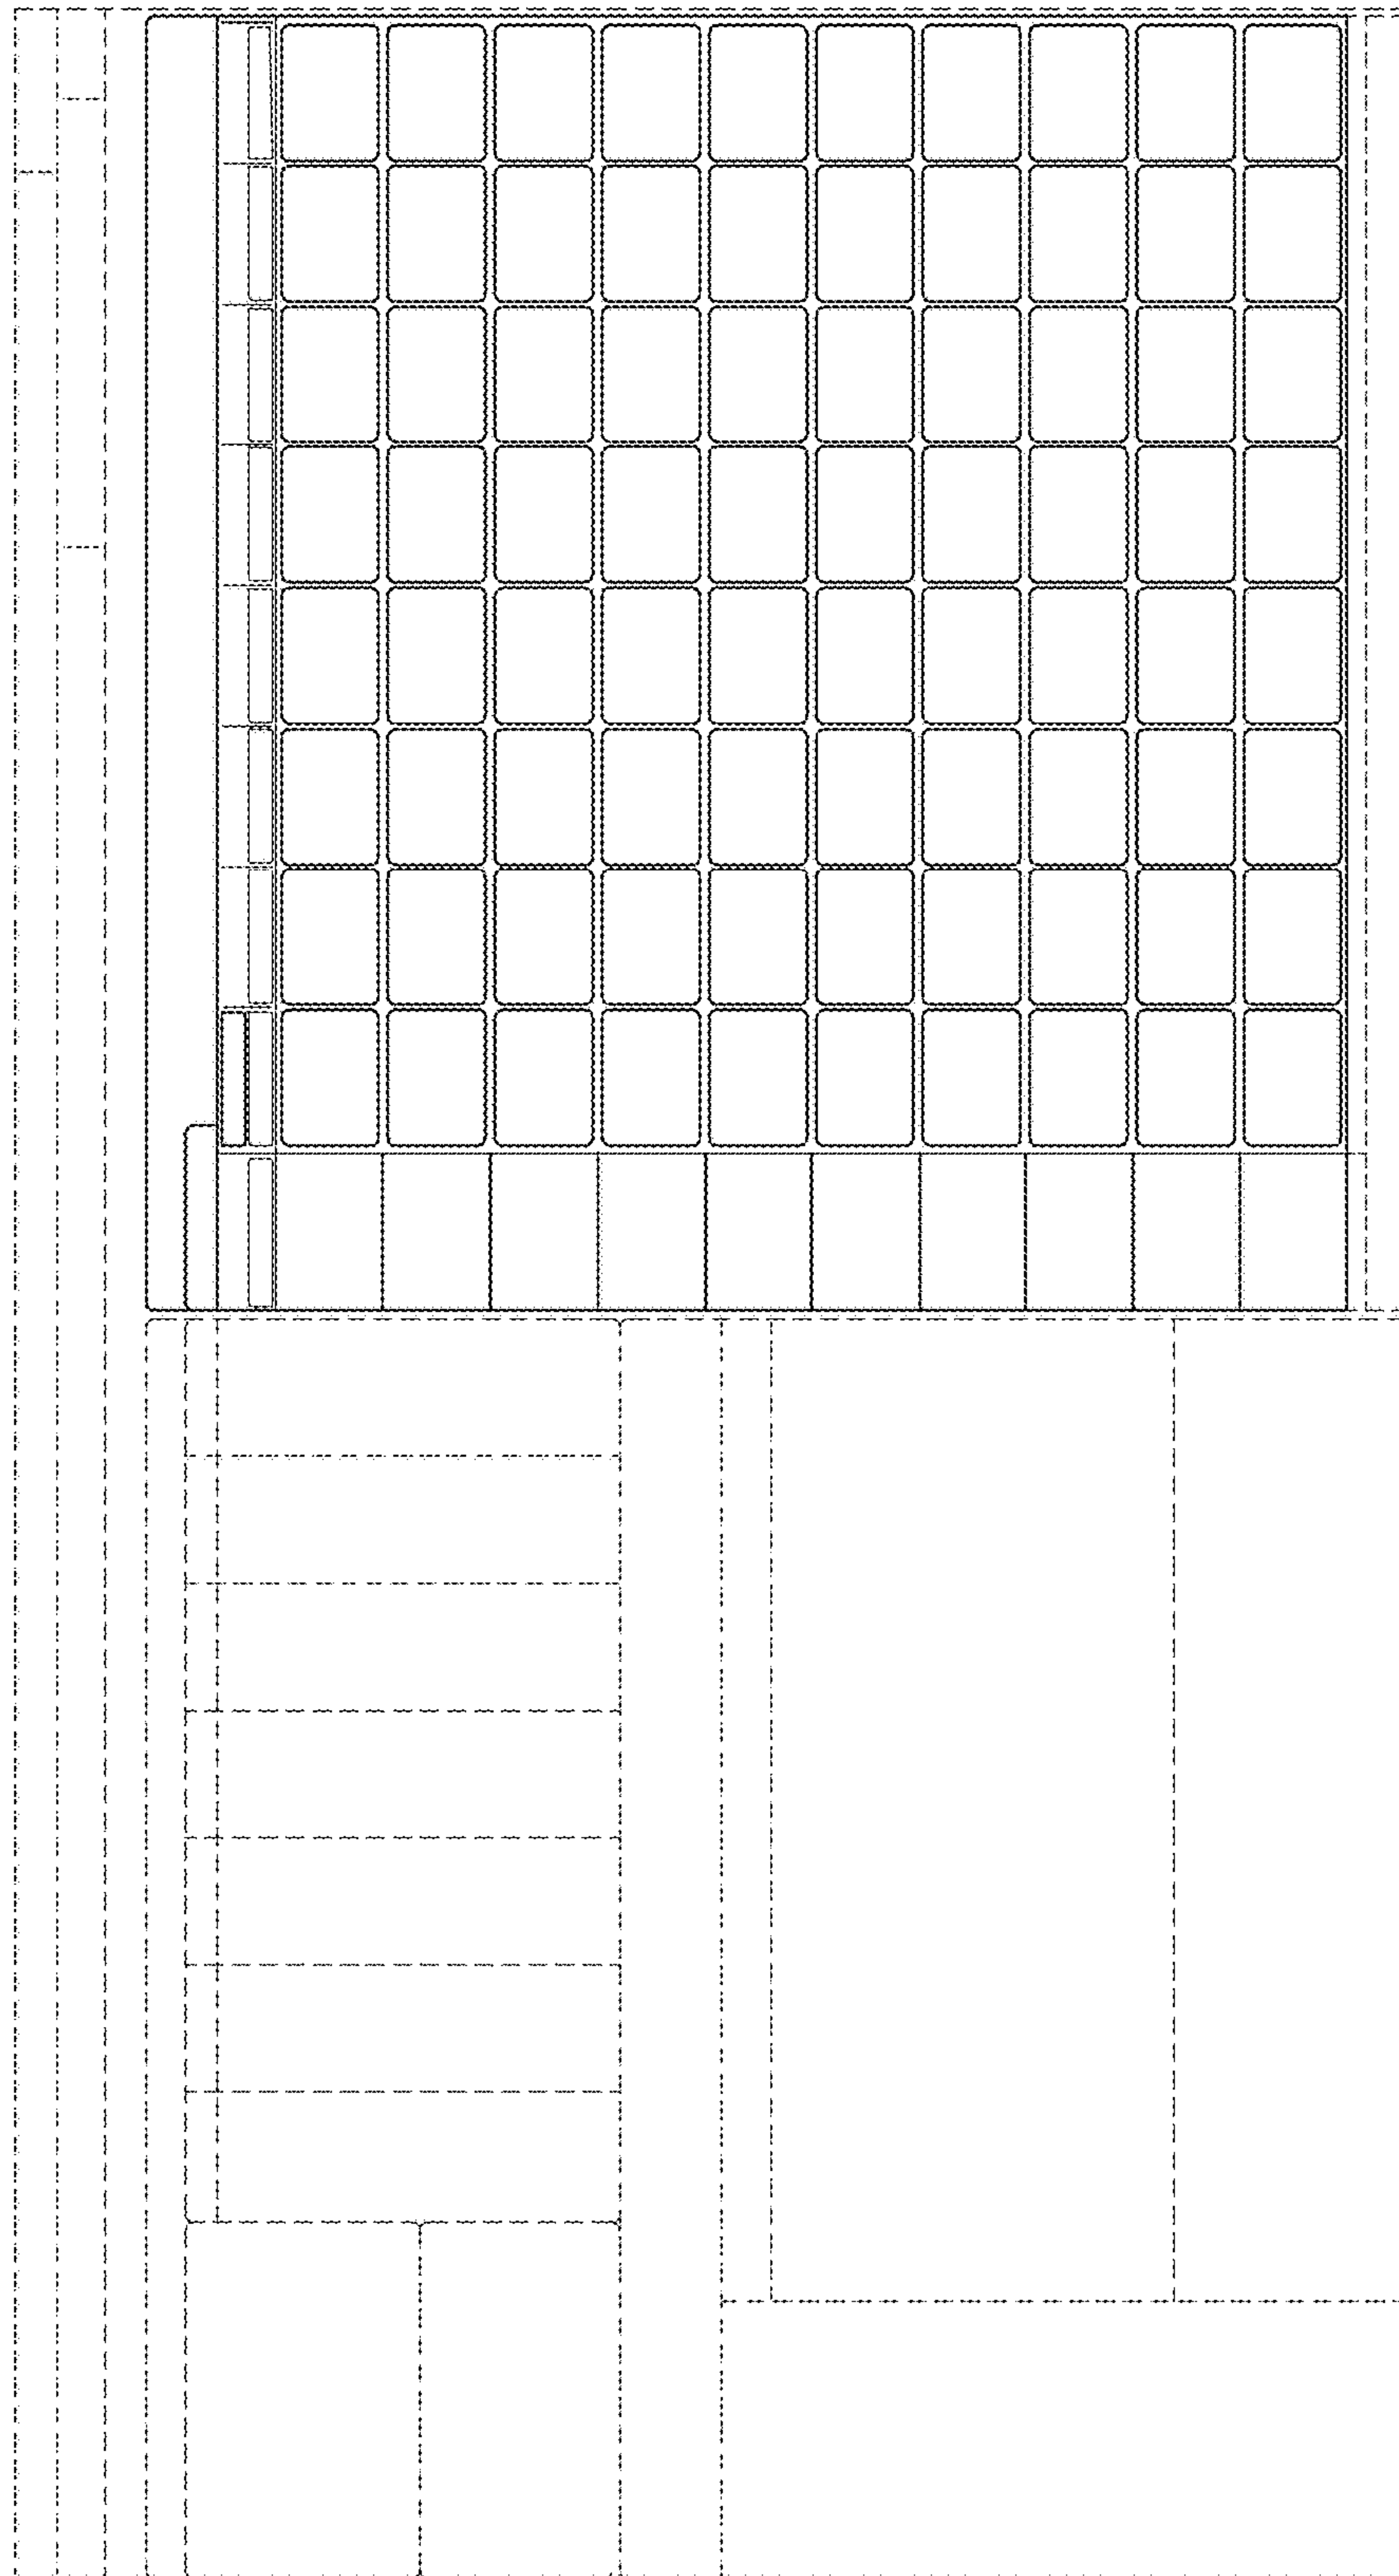


FIG. 2

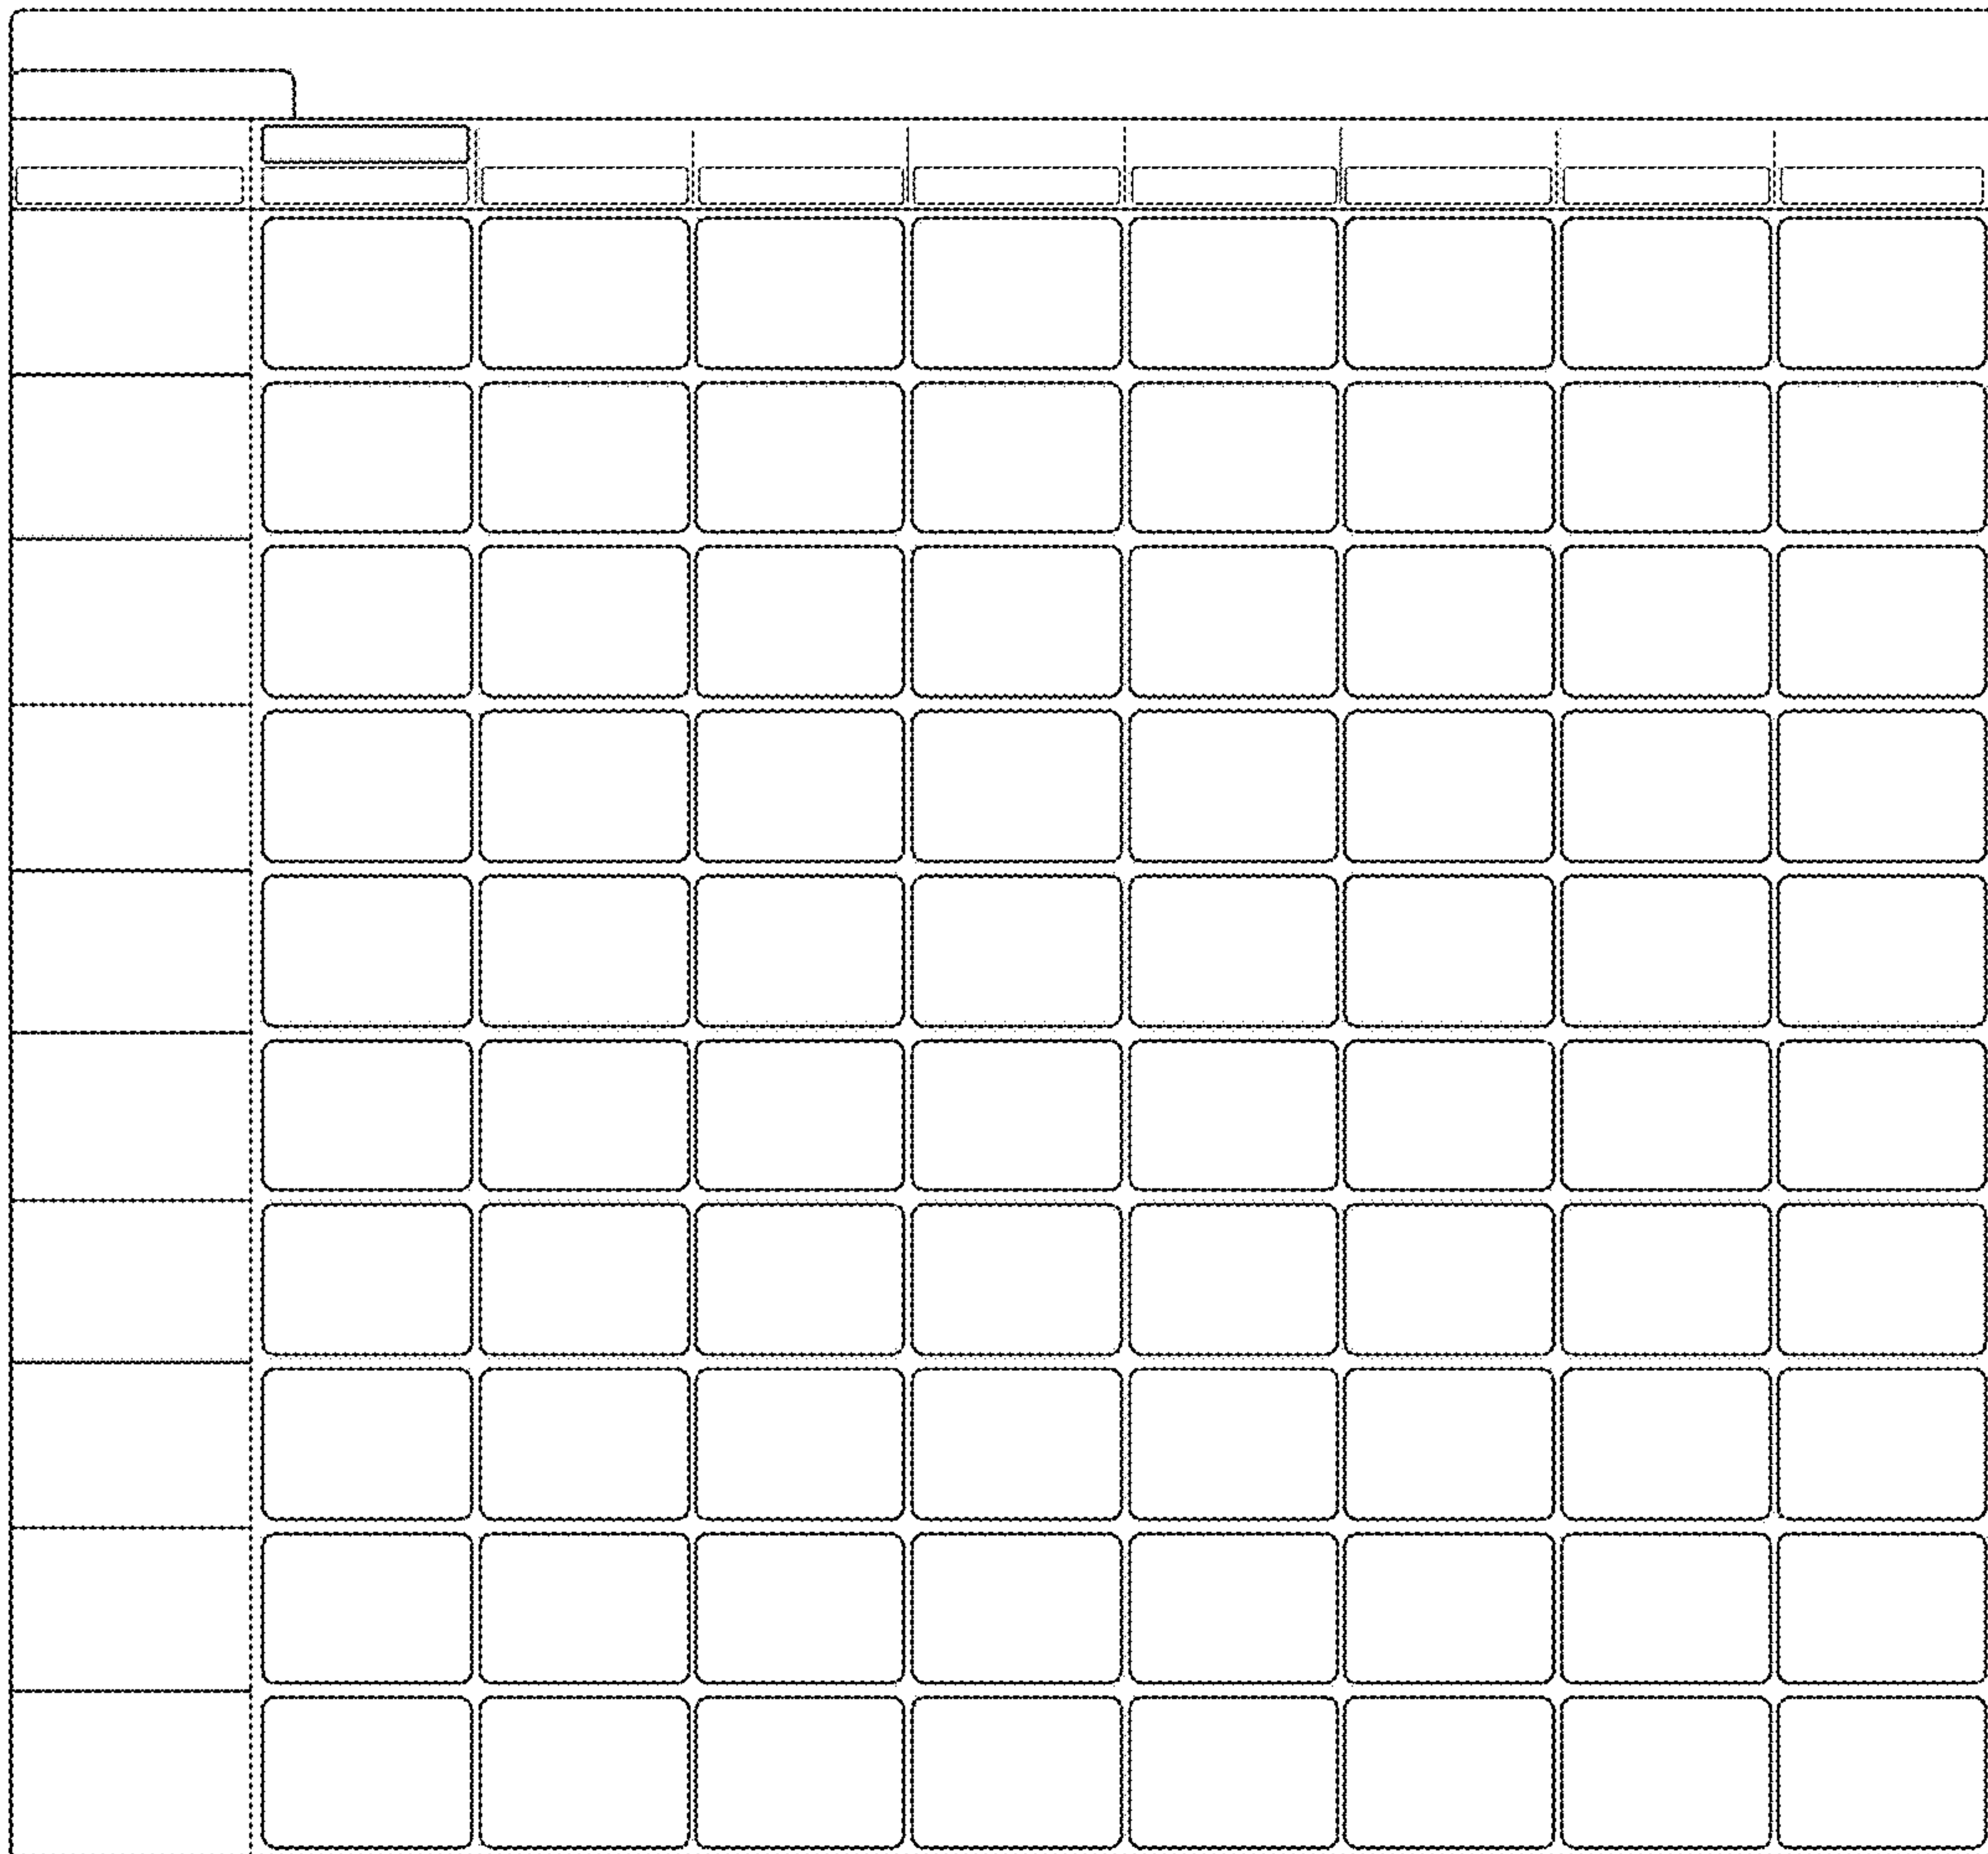


FIG. 3

