

US00D794664S

(12) **United States Design Patent** (10) **Patent No.:** **US D794,664 S**  
**Okabe et al.** (45) **Date of Patent:** **\*\* Aug. 15, 2017**

(54) **DISPLAY SCREEN FOR MEDICAL INFORMATION MANAGEMENT APPARATUS WITH GRAPHICAL USER INTERFACE**

D664,971 S \* 8/2012 Lee ..... D14/486  
D666,625 S \* 9/2012 Gilmore ..... D14/485  
D675,224 S \* 1/2013 Lee ..... D14/488

(Continued)

(71) Applicant: **FUJIFILM Corporation**, Minato-ku, Tokyo (JP)

(72) Inventors: **Yuki Okabe**, Tokyo (JP); **Yasuyo Nenoki**, Tokyo (JP)

(73) Assignee: **FUJIFILM Corporation**, Minato-ku, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/514,338**

(22) Filed: **Jan. 12, 2015**

(30) **Foreign Application Priority Data**

Jul. 14, 2014 (JP) ..... 2014-015355

(51) **LOC (10) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/486**

(58) **Field of Classification Search**  
USPC ..... D14/485-495; 348/14.01; 715/769, 784; D20/11; D21/324, 325  
CPC .... G06F 3/048; G06F 3/04817; G06F 3/0482; G06F 3/04842; G06F 3/0485; G06F 3/04883; G06F 19/321; G06F 21/10; H04L 67/22; G06K 9/6212; A61B 5/055; A61B 6/3217

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D579,456 S \* 10/2008 Chen ..... D14/485  
D598,923 S \* 8/2009 Chen ..... D14/485  
D658,196 S \* 4/2012 Wood ..... D14/486  
D658,673 S \* 5/2012 Velasco ..... D14/488  
D664,967 S \* 8/2012 Lee ..... D14/485  
D664,968 S \* 8/2012 Lee ..... D14/485

**OTHER PUBLICATIONS**

“CXDI Control Software NE”, posted at virtualimaging-fl.com, Oct. 31, 2010, [site visited Mar. 29, 2016]. Available from Internet: <[http://www.virtualimaging-fl.com/Healthcare\\_Products/Software\\_Solutions/CXDI\\_Control\\_Software\\_NE/CXDI\\_Control\\_Software\\_tabbedLandingPage.shtml](http://www.virtualimaging-fl.com/Healthcare_Products/Software_Solutions/CXDI_Control_Software_NE/CXDI_Control_Software_tabbedLandingPage.shtml)>.\*

“Nurses: Spend More Time in Direct Patient Care with RTLS”, posted at versustech.com, Feb. 28, 2013, [site visited Mar. 29, 2016]. Available from Internet: <<http://www.versustech.com/rtls-benefits/nurses>>.\*

(Continued)

*Primary Examiner* — Karen Kearney

*Assistant Examiner* — John M Otte

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for a display screen for medical information management apparatus with graphical user interface, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of a display screen for medical information management apparatus with graphical user interface showing a first embodiment of our new design; FIG. 2 is an enlarged partial view of FIG. 1, shown for clarity of illustration; and,

FIG. 3 is a front view of a second embodiment of a display screen for medical information management apparatus with graphical user interface.

The broken line showing of the display screen is included for the purpose of illustrating portions of the display screen for medical information management apparatus with graphical user interface and form no part of the claimed design. The perimeters of the underlying portion of the display screen and the graphical user interface are understood to be flush.

**1 Claim, 3 Drawing Sheets**

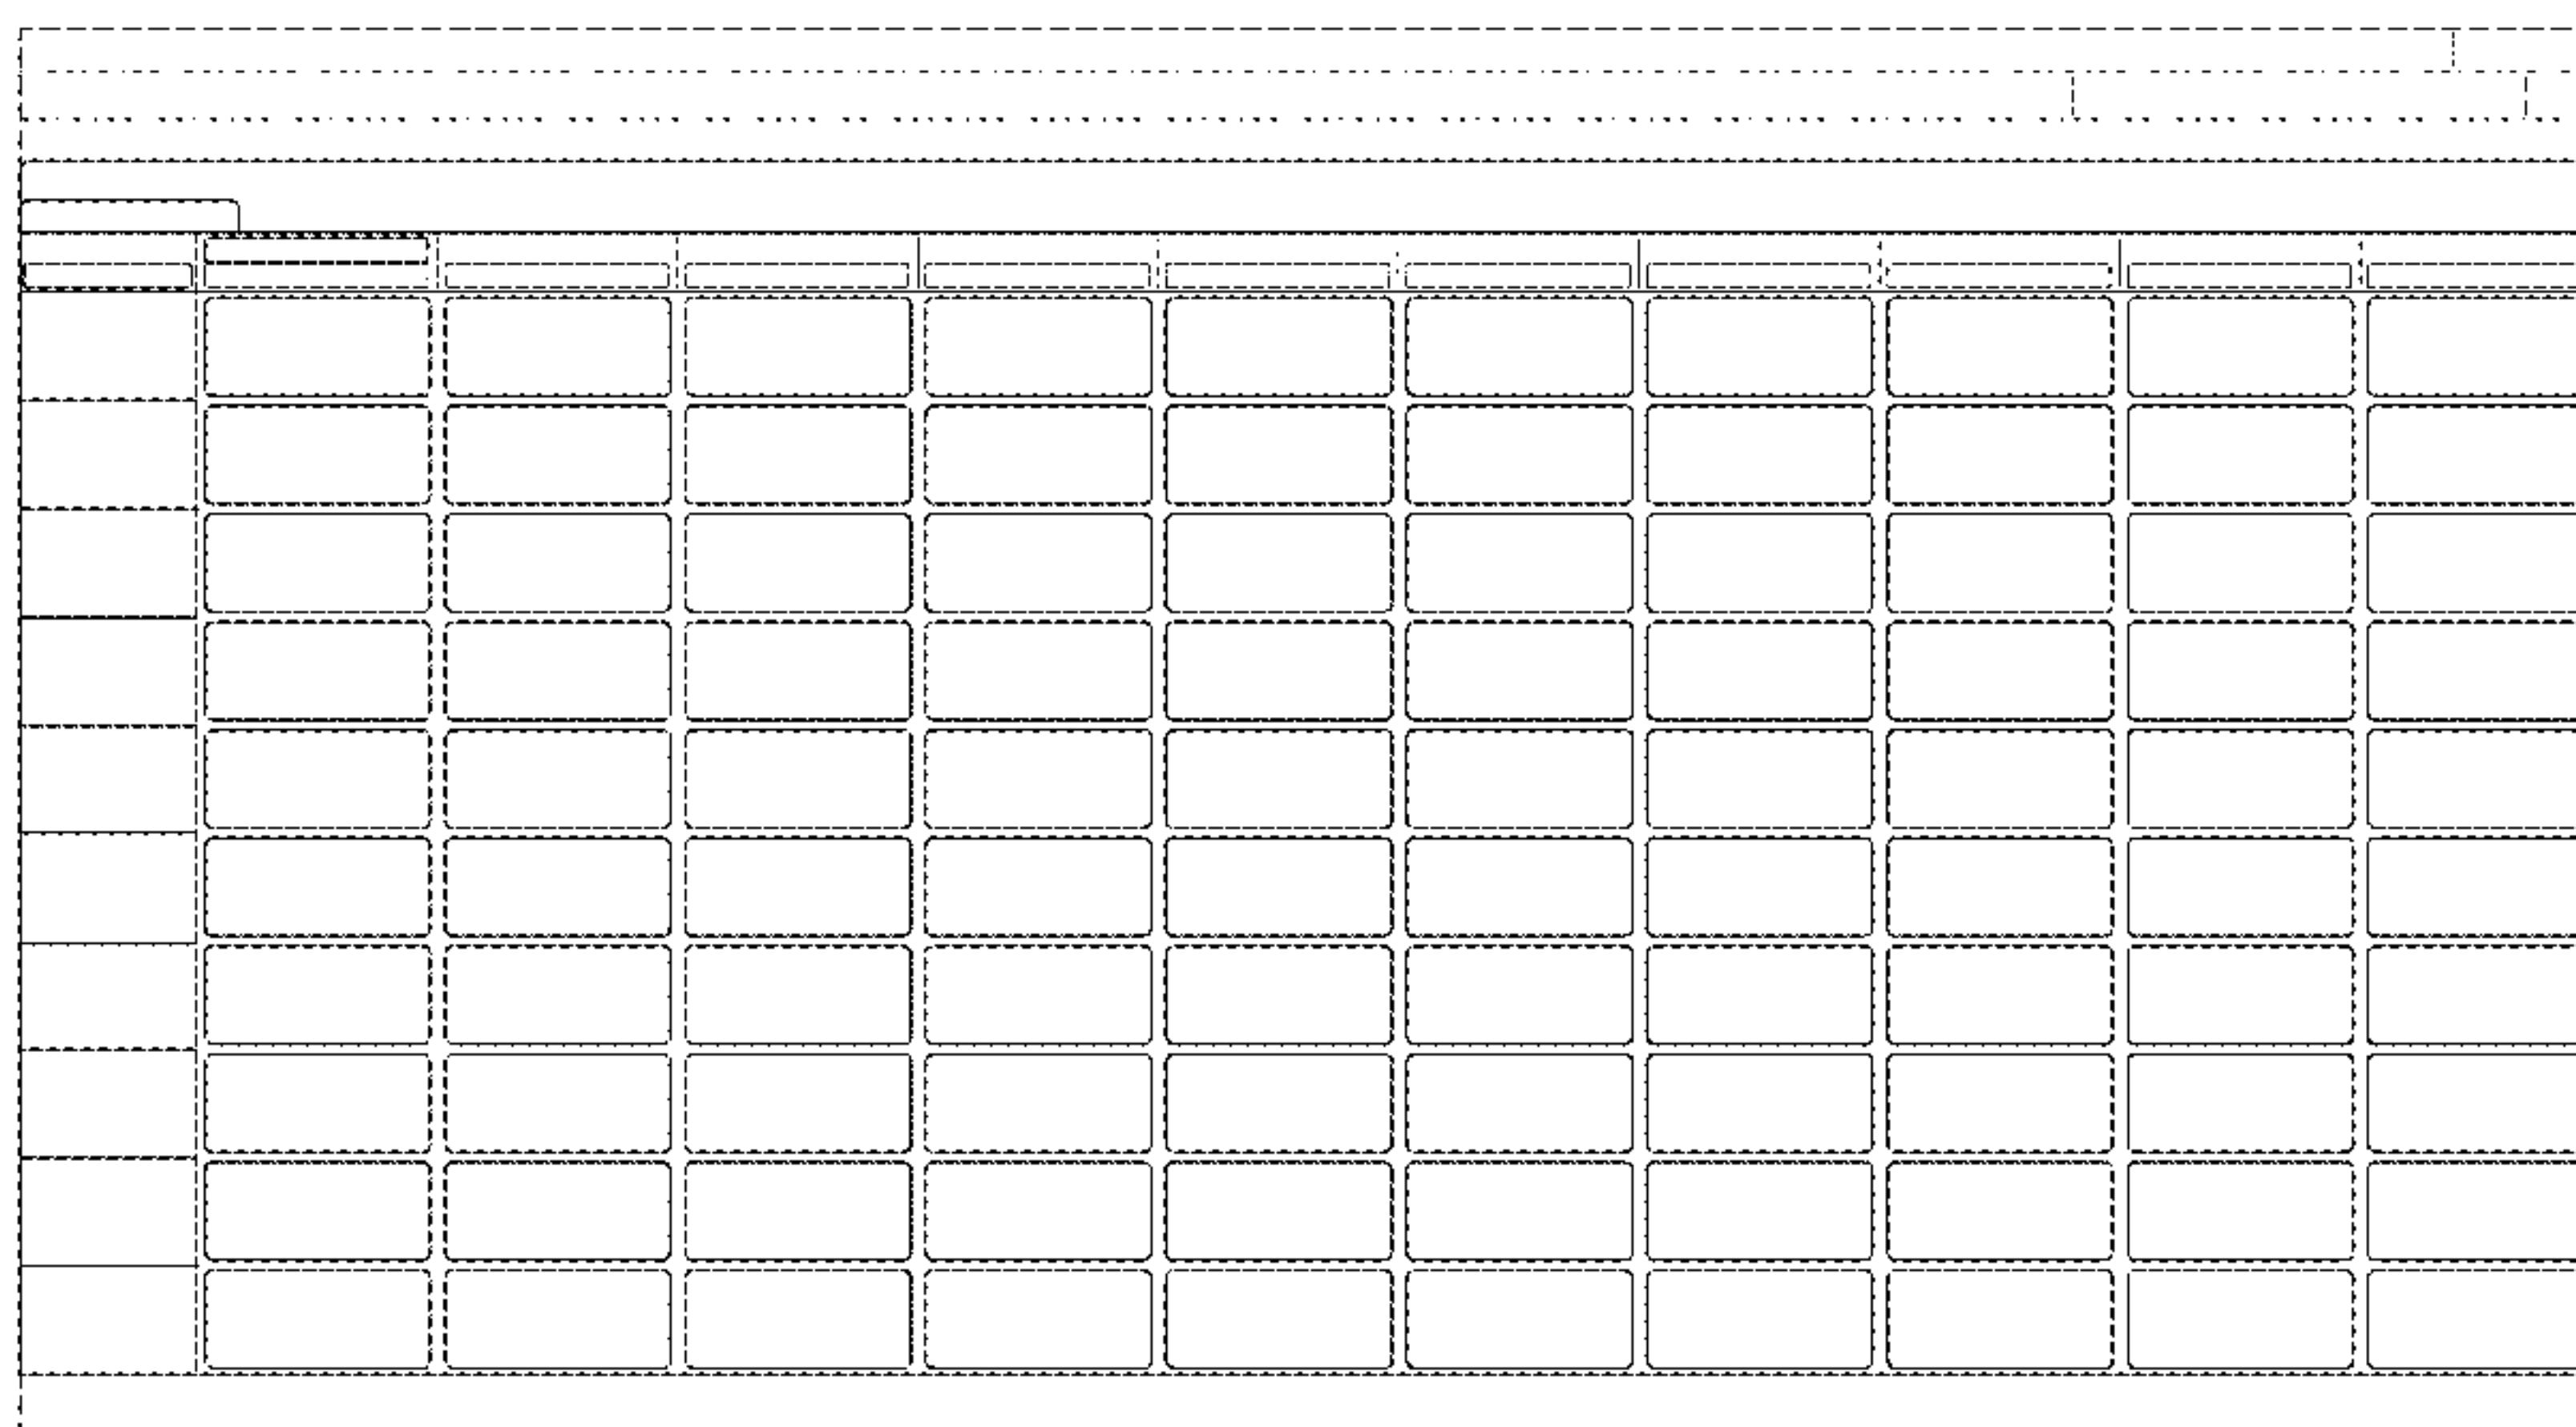




FIG. 1

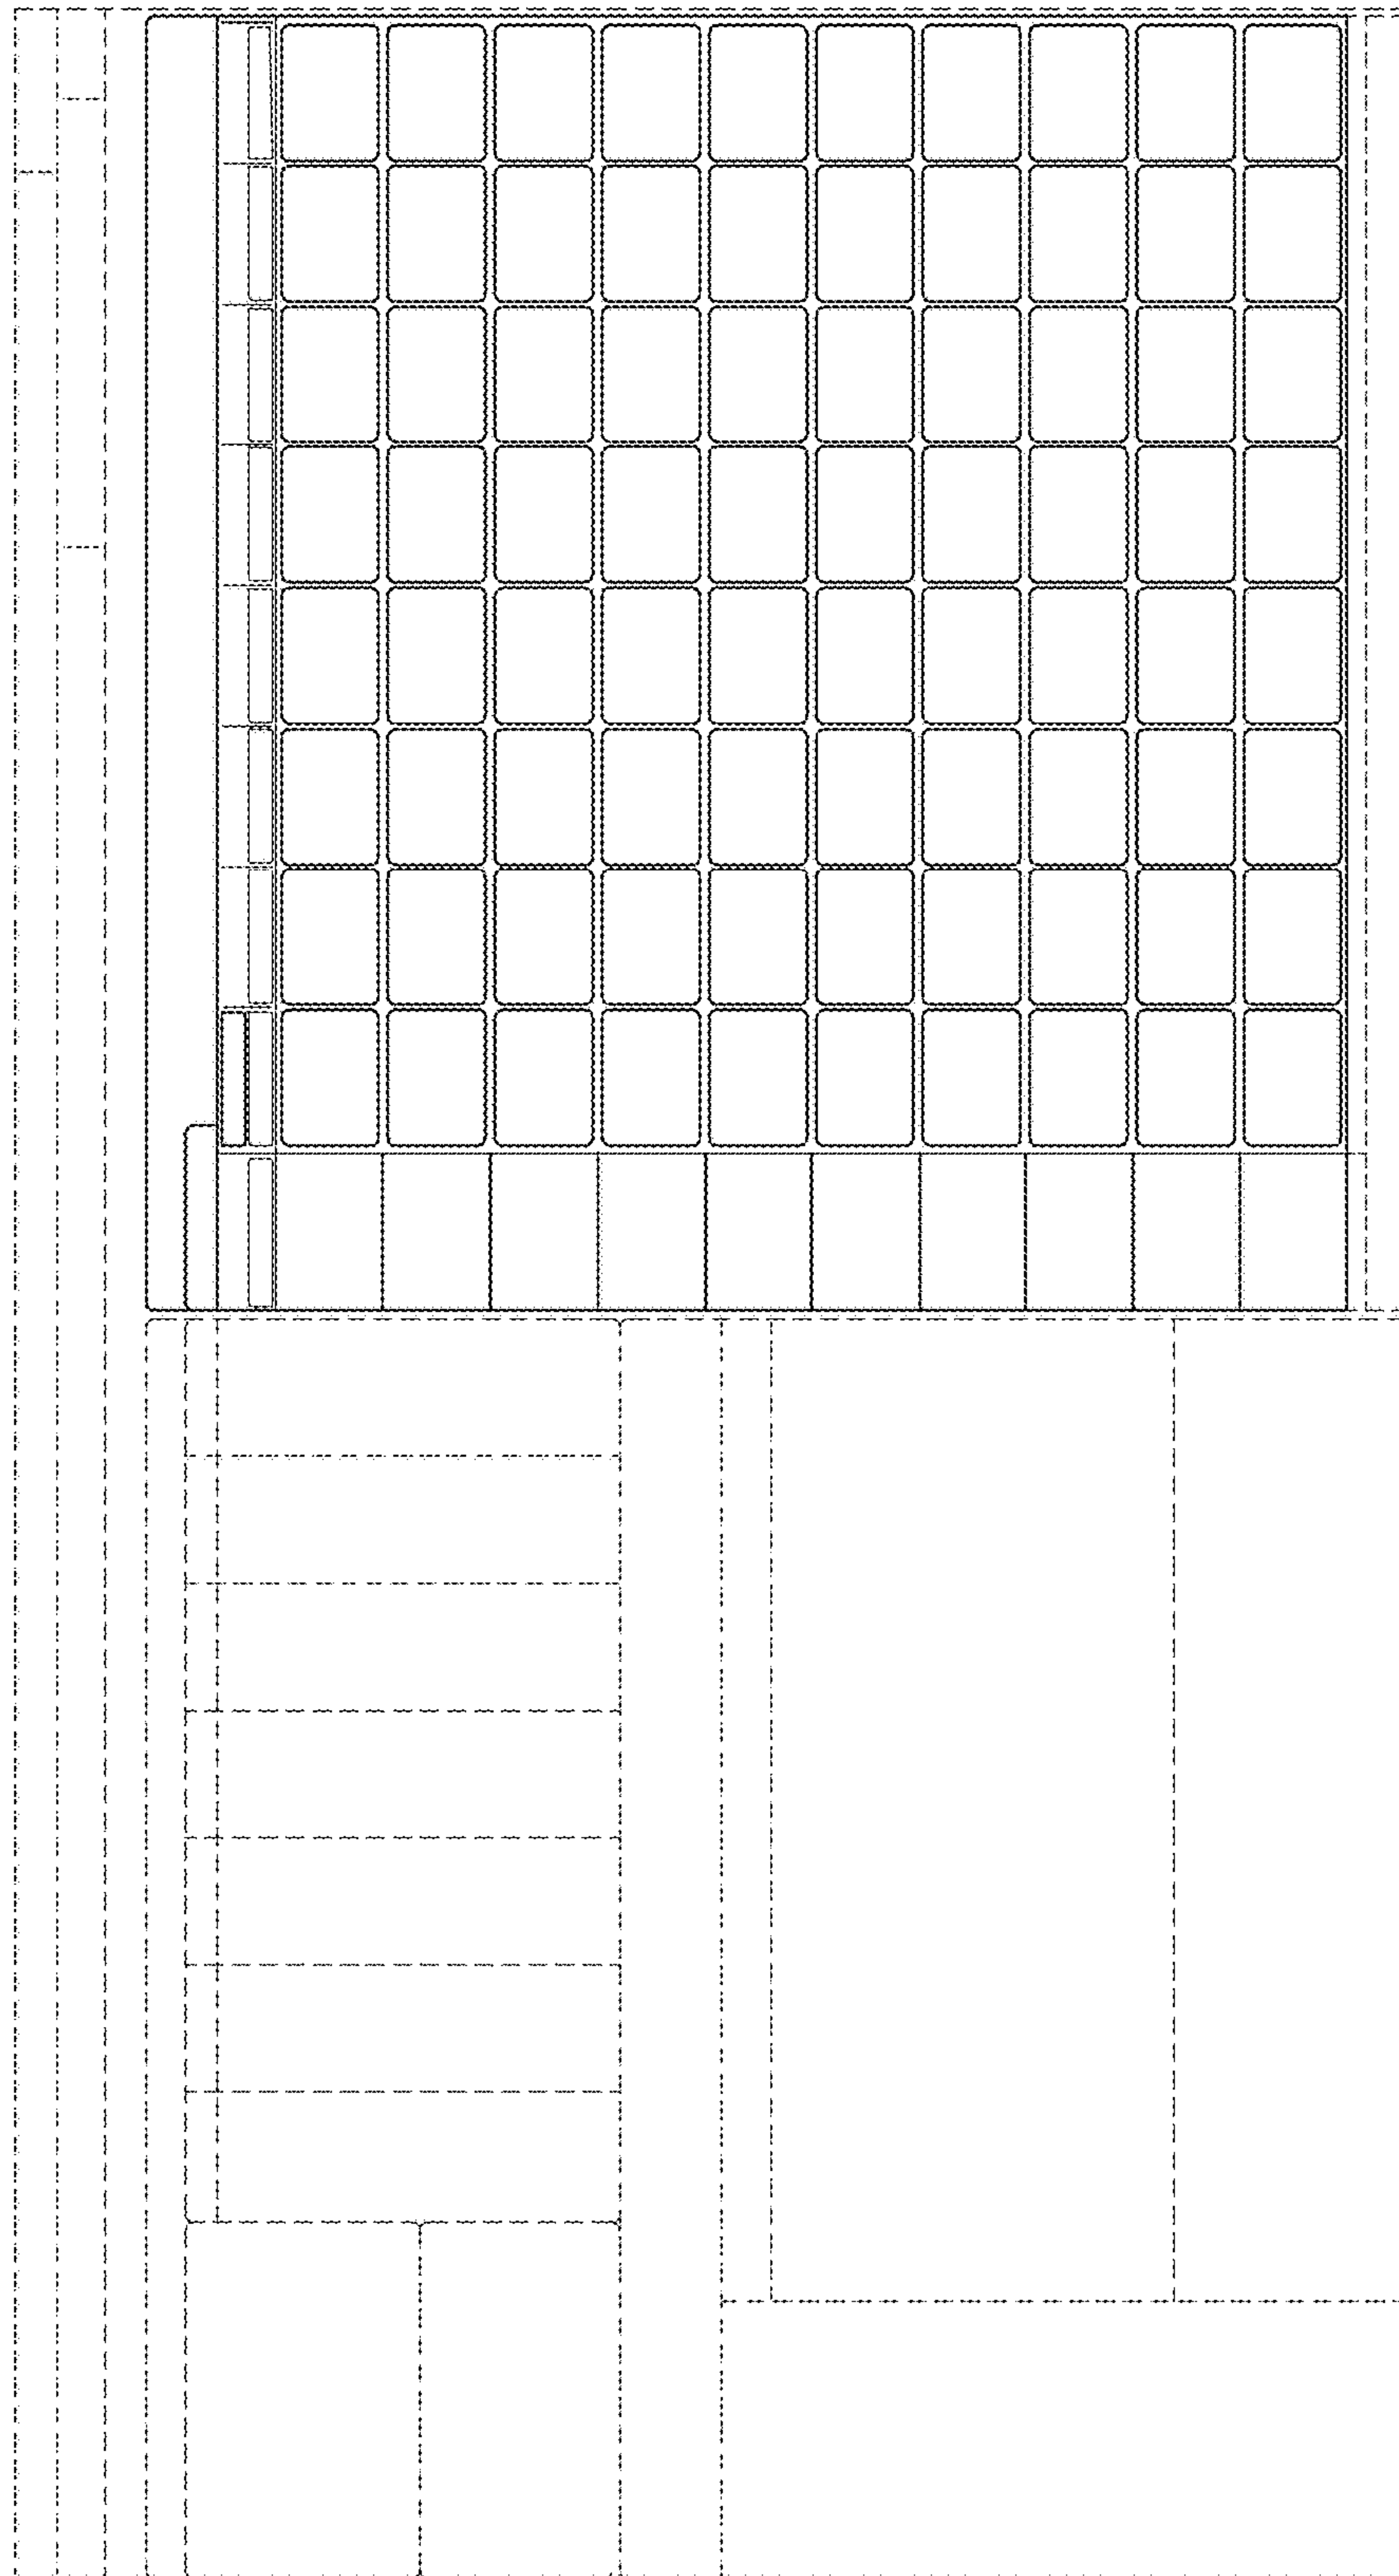




FIG. 2

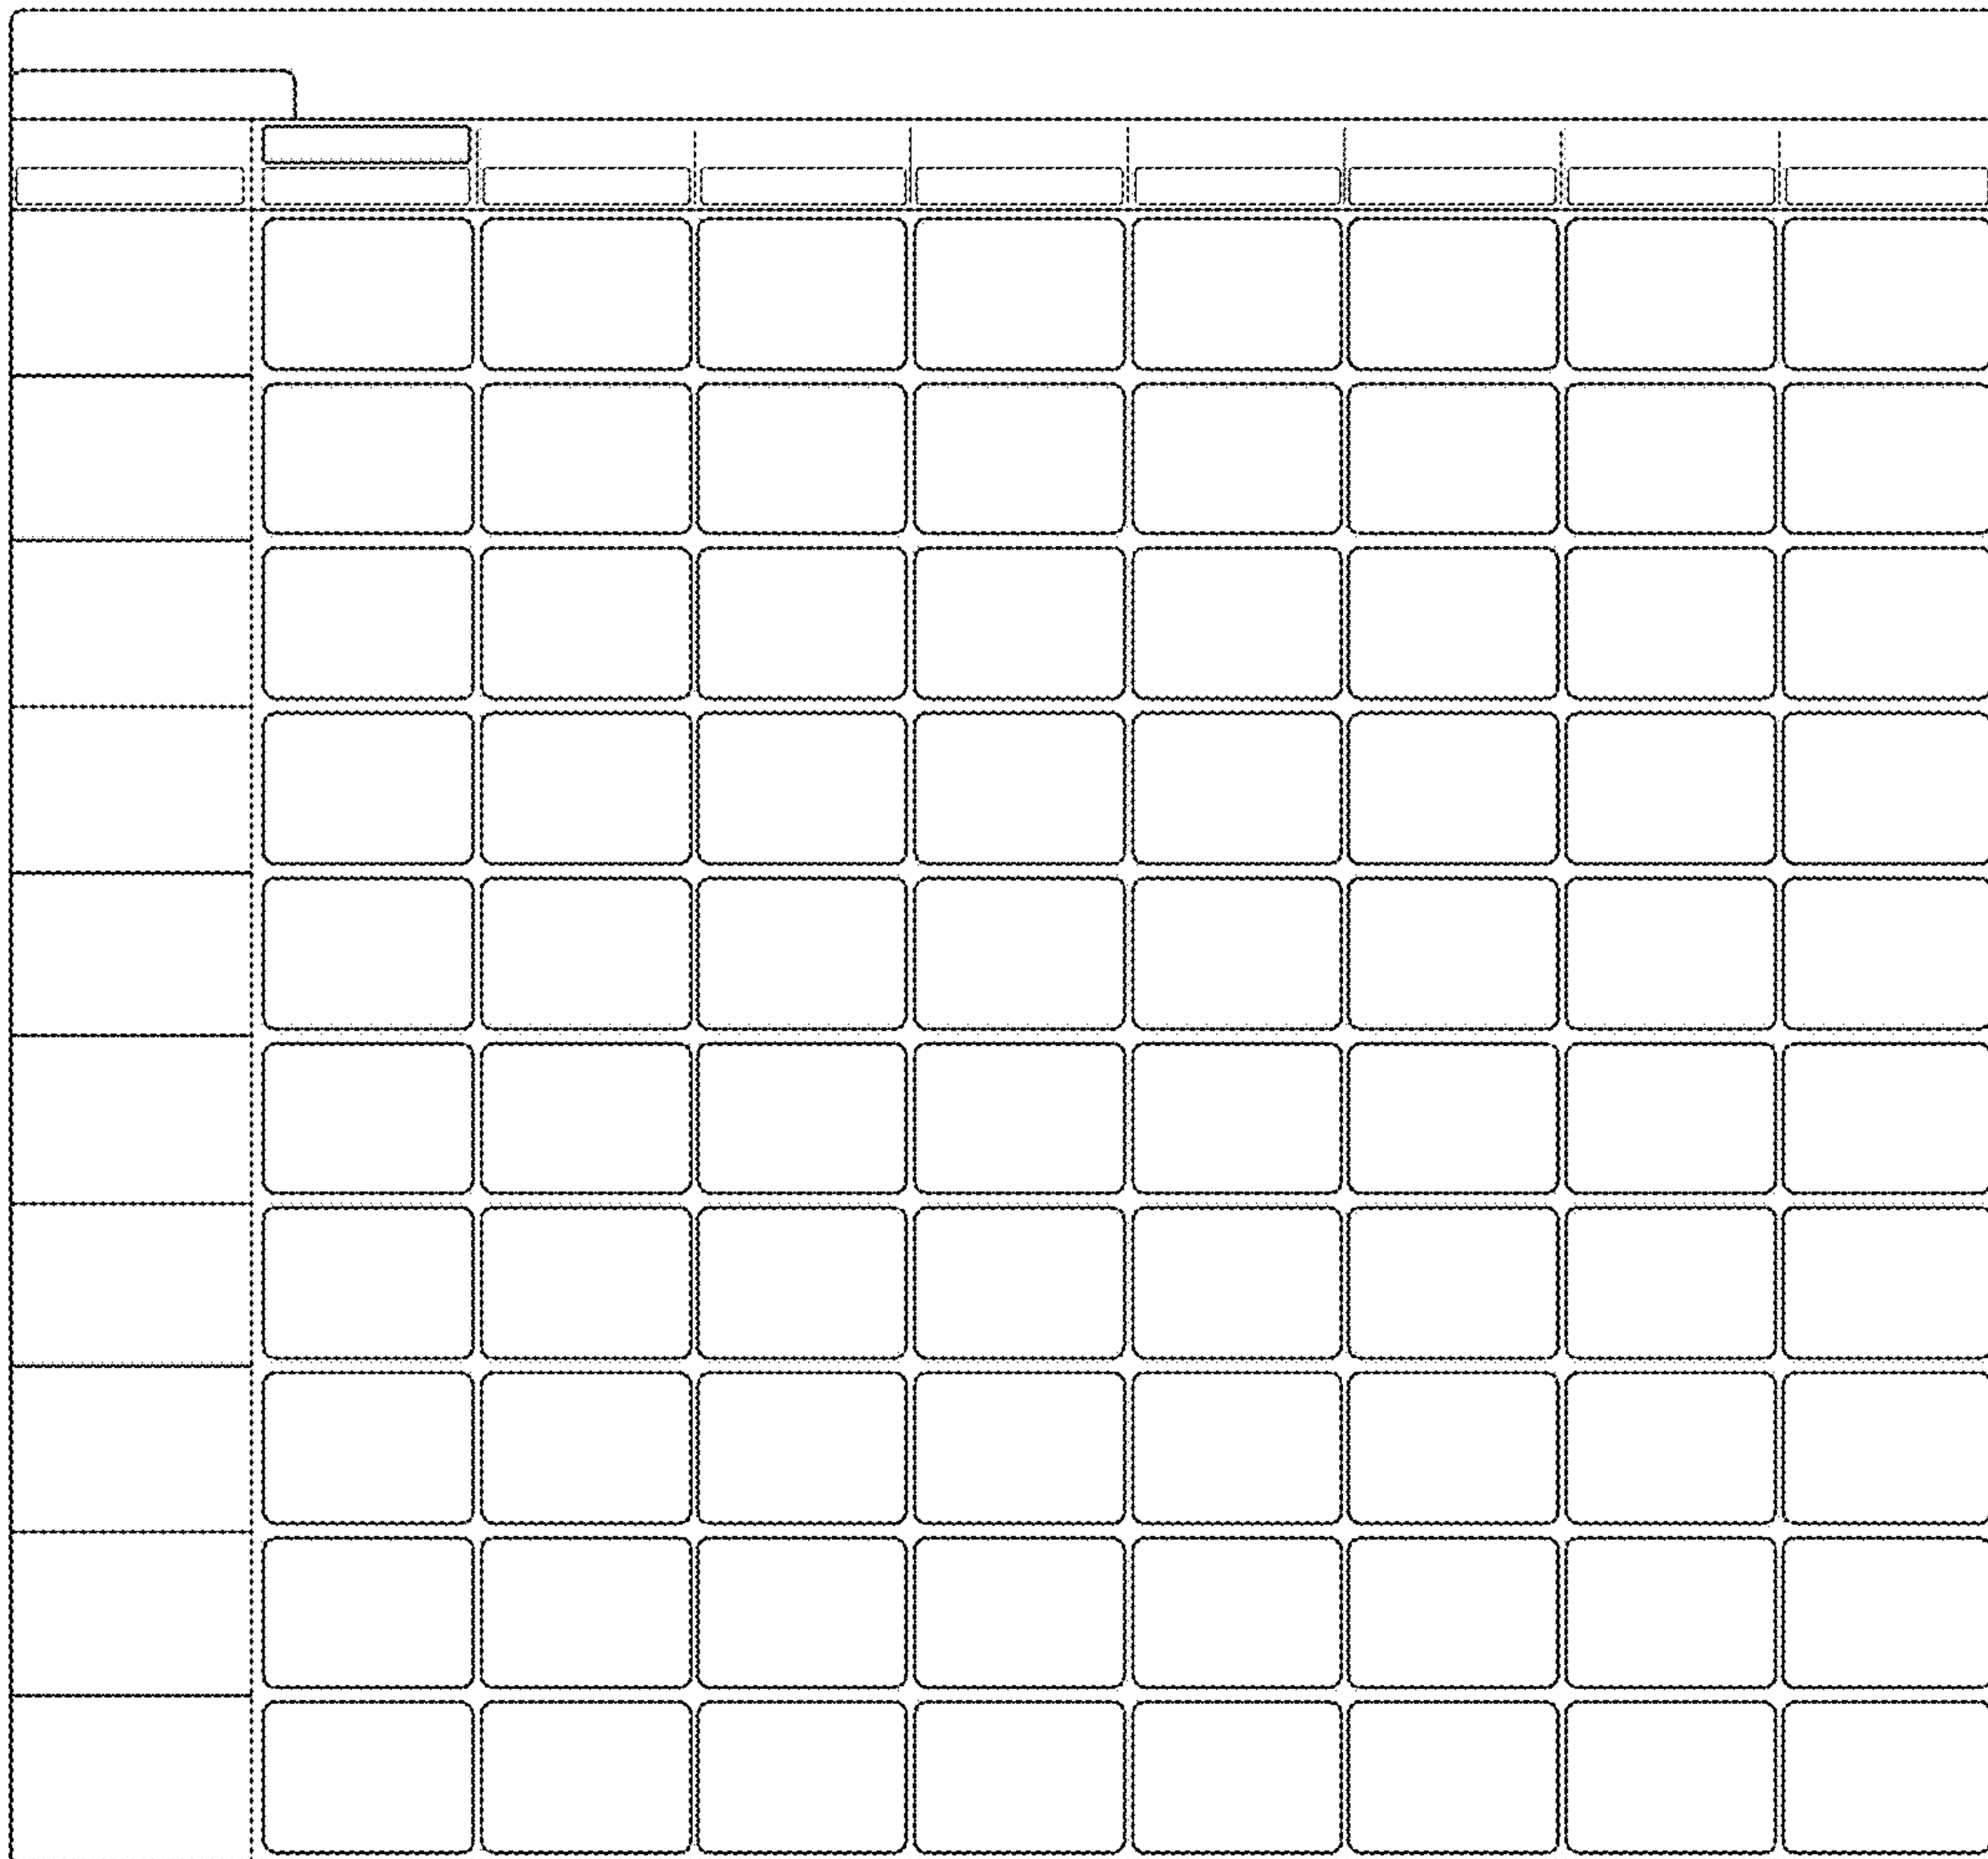


FIG. 3

