



US00D794775S

(12) **United States Design Patent**  
**Bainton et al.**

(10) **Patent No.:** **US D794,775 S**  
(45) **Date of Patent:** **\*\* Aug. 15, 2017**

(54) **INJECTION DEVICE**

(71) Applicant: **SANOFI SA**

(72) Inventors: **Mike Cameron Bainton**, Warwickshire (GB); **Robert F. Veasey**, Warwickshire (GB)

(73) Assignee: **SANOFI SA**, Paris (FR)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/520,734**

(22) Filed: **Mar. 17, 2015**

(30) **Foreign Application Priority Data**

Sep. 23, 2014 (EM) ..... 002542852

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/112**

(58) **Field of Classification Search**

USPC ..... D24/127–131, 112–114, 133, 186;  
606/181, 185; 604/264, 523–528, 272,  
604/187, 158, 164.01–164.11, 181, 184,  
604/227; 600/101, 139, 143;  
128/200.24, 207.14, 207.15

CPC ..... A61M 5/178; A61M 3/00; A61M 5/20;  
A61M 5/31; A61M 5/3146; A61M  
5/3129; A61M 5/3148; A61M 5/315

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D365,881 S \* 1/1996 Tiefenthal ..... D24/158  
D371,605 S \* 7/1996 Wong ..... D24/169

D393,271 S \* 4/1998 Conner ..... D16/130  
D439,657 S \* 3/2001 Bridle ..... D24/113  
D440,309 S \* 4/2001 Whiteside ..... D24/131  
D447,282 S \* 8/2001 Yiu ..... D24/133  
6,379,339 B1 \* 4/2002 Klitgaard ..... A61M 5/3129  
604/207  
D623,740 S \* 9/2010 Harris ..... D24/133  
D633,201 S \* 2/2011 Lee ..... D24/129  
D676,549 S \* 2/2013 Lovell ..... D24/113  
8,394,117 B2 \* 3/2013 Hein ..... A61B 5/1411  
606/181  
D681,195 S \* 4/2013 Skulley ..... D24/113  
D725,261 S \* 3/2015 Barrett ..... D24/129

\* cited by examiner

*Primary Examiner* — David Muller

(74) *Attorney, Agent, or Firm* — McDonnell Boehnen  
Hulbert & Berghoff LLP


(57) **CLAIM**

The ornamental injection device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the injection device from the front and right;  
FIG. 2 is top end view of the injection device; and  
FIG. 3 is a bottom end view of the injection device;  
FIG. 4 is a right side view of the injection device;  
FIG. 5 is a left side view of the injection device;  
FIG. 6 is a front end view of the injection device; and,  
FIG. 7 is a back end view of the injection device.

**1 Claim, 6 Drawing Sheets**

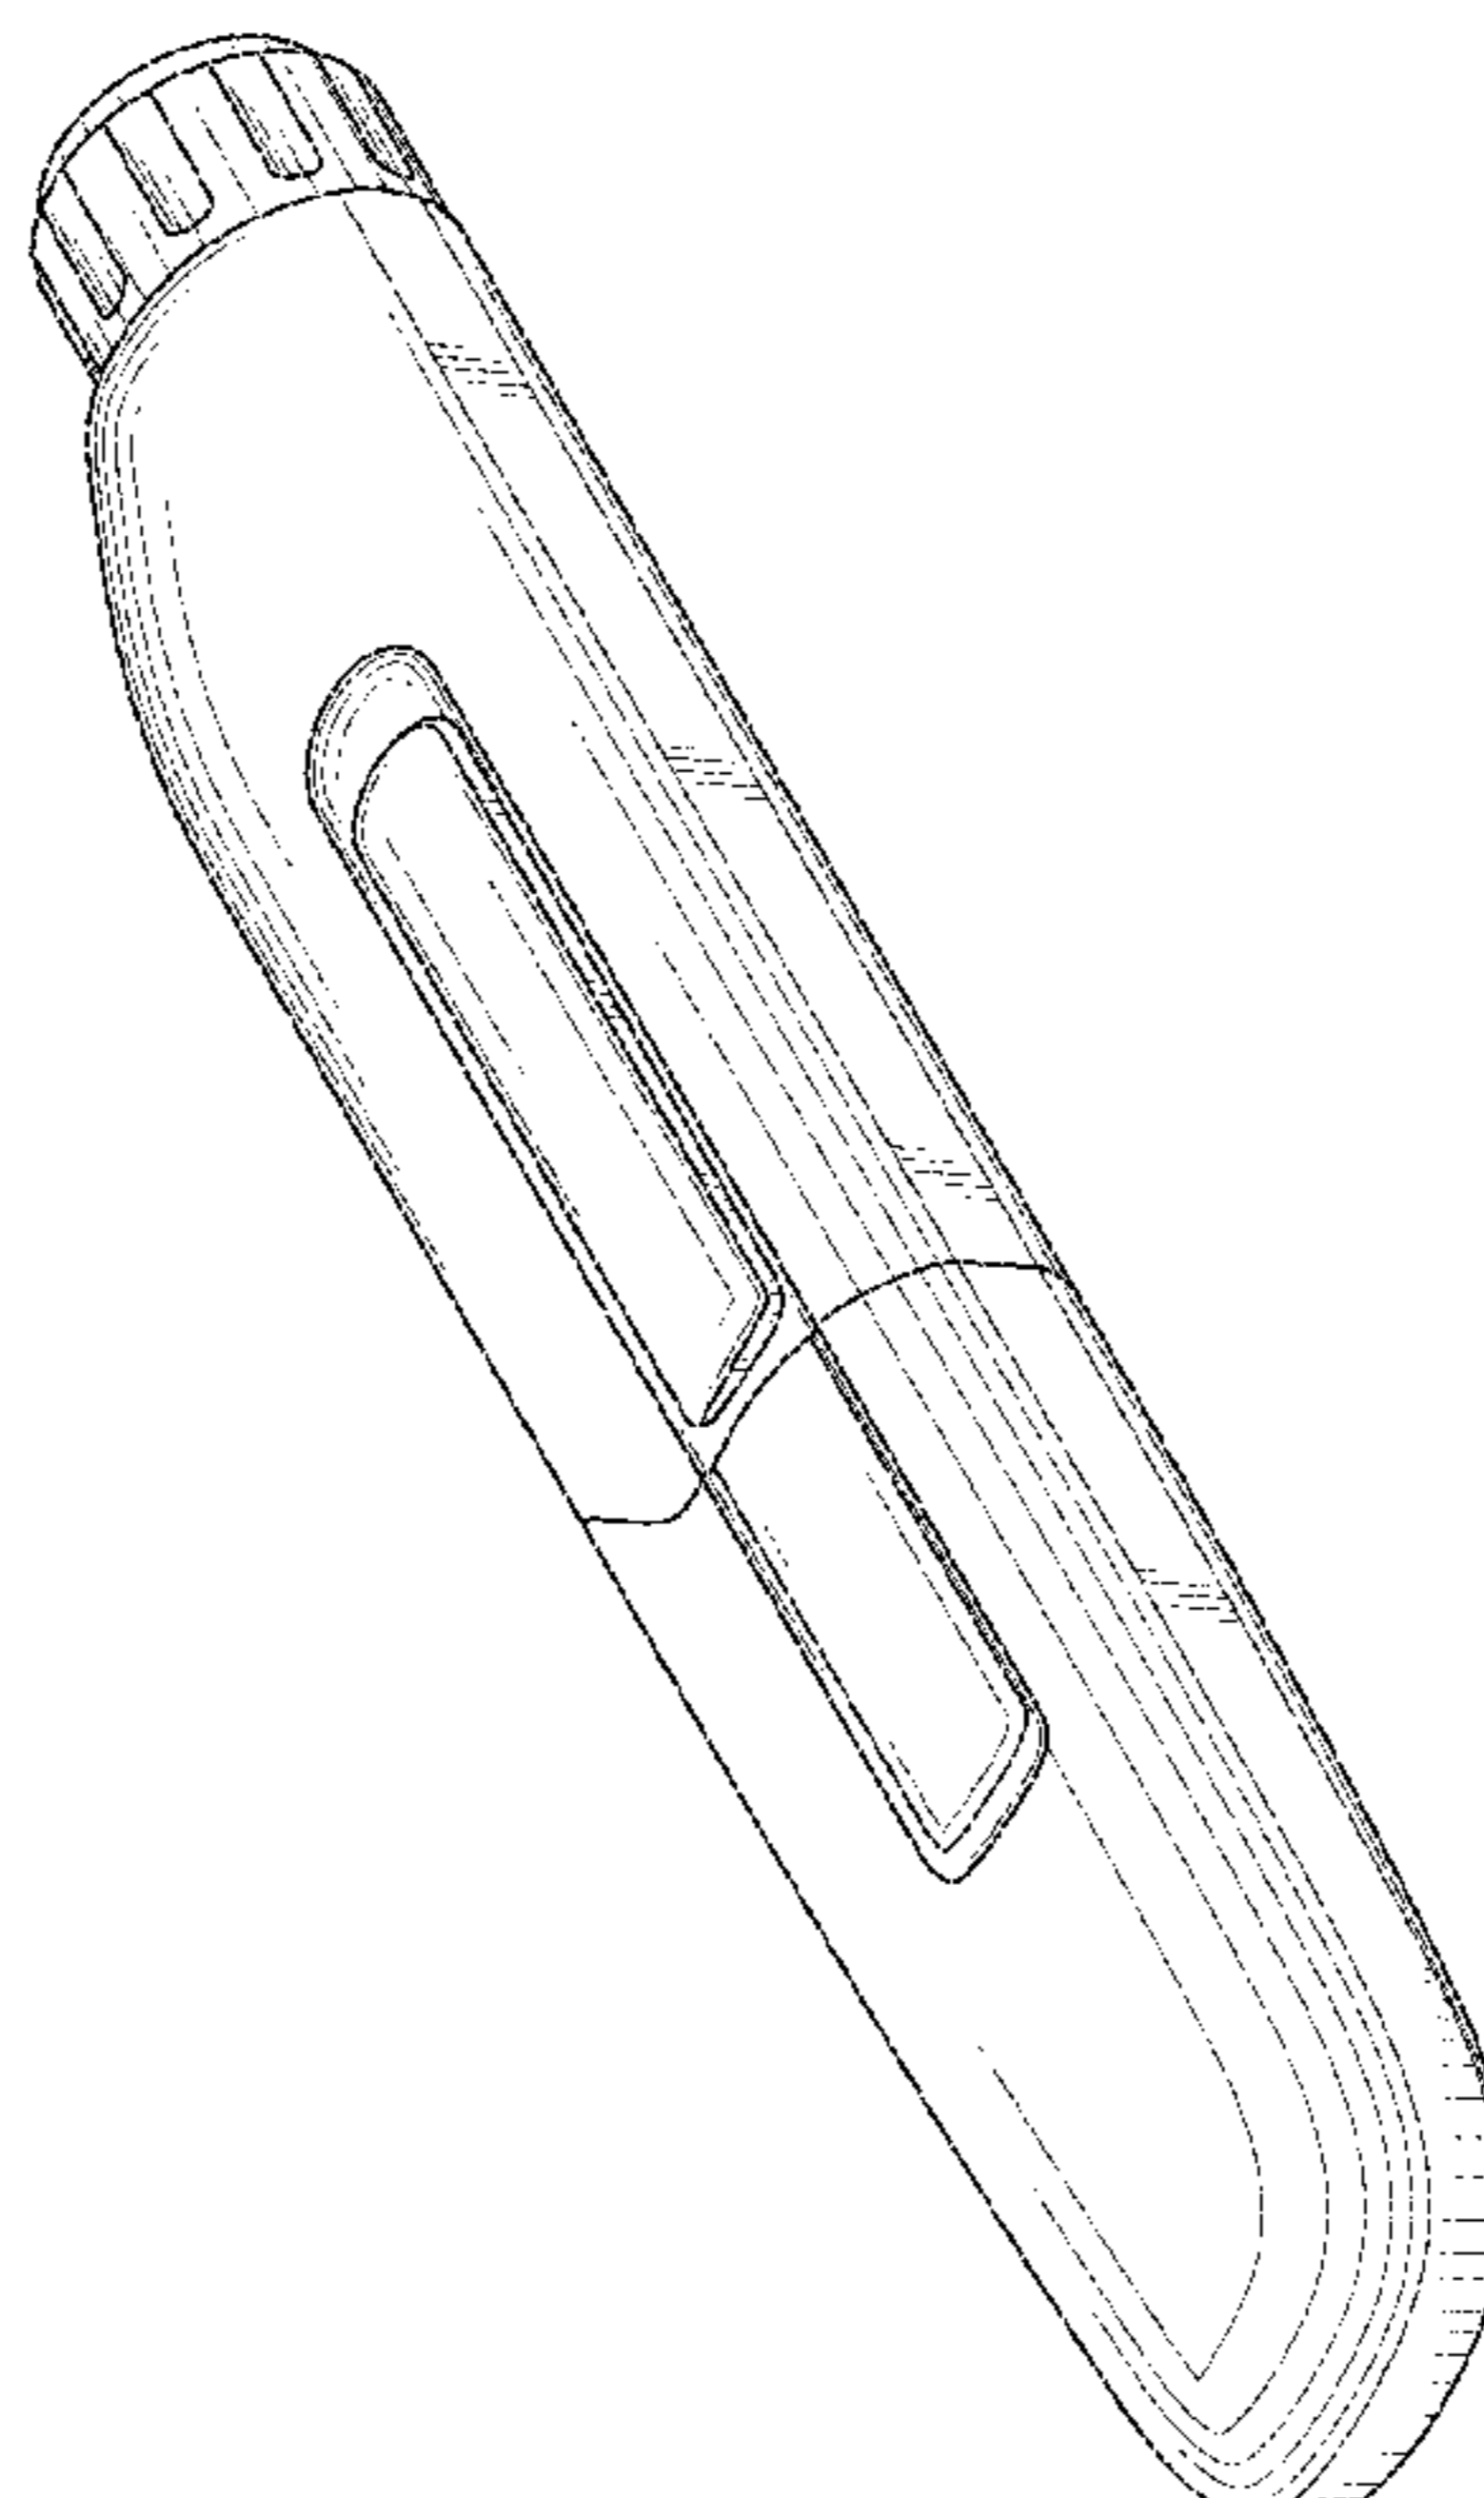

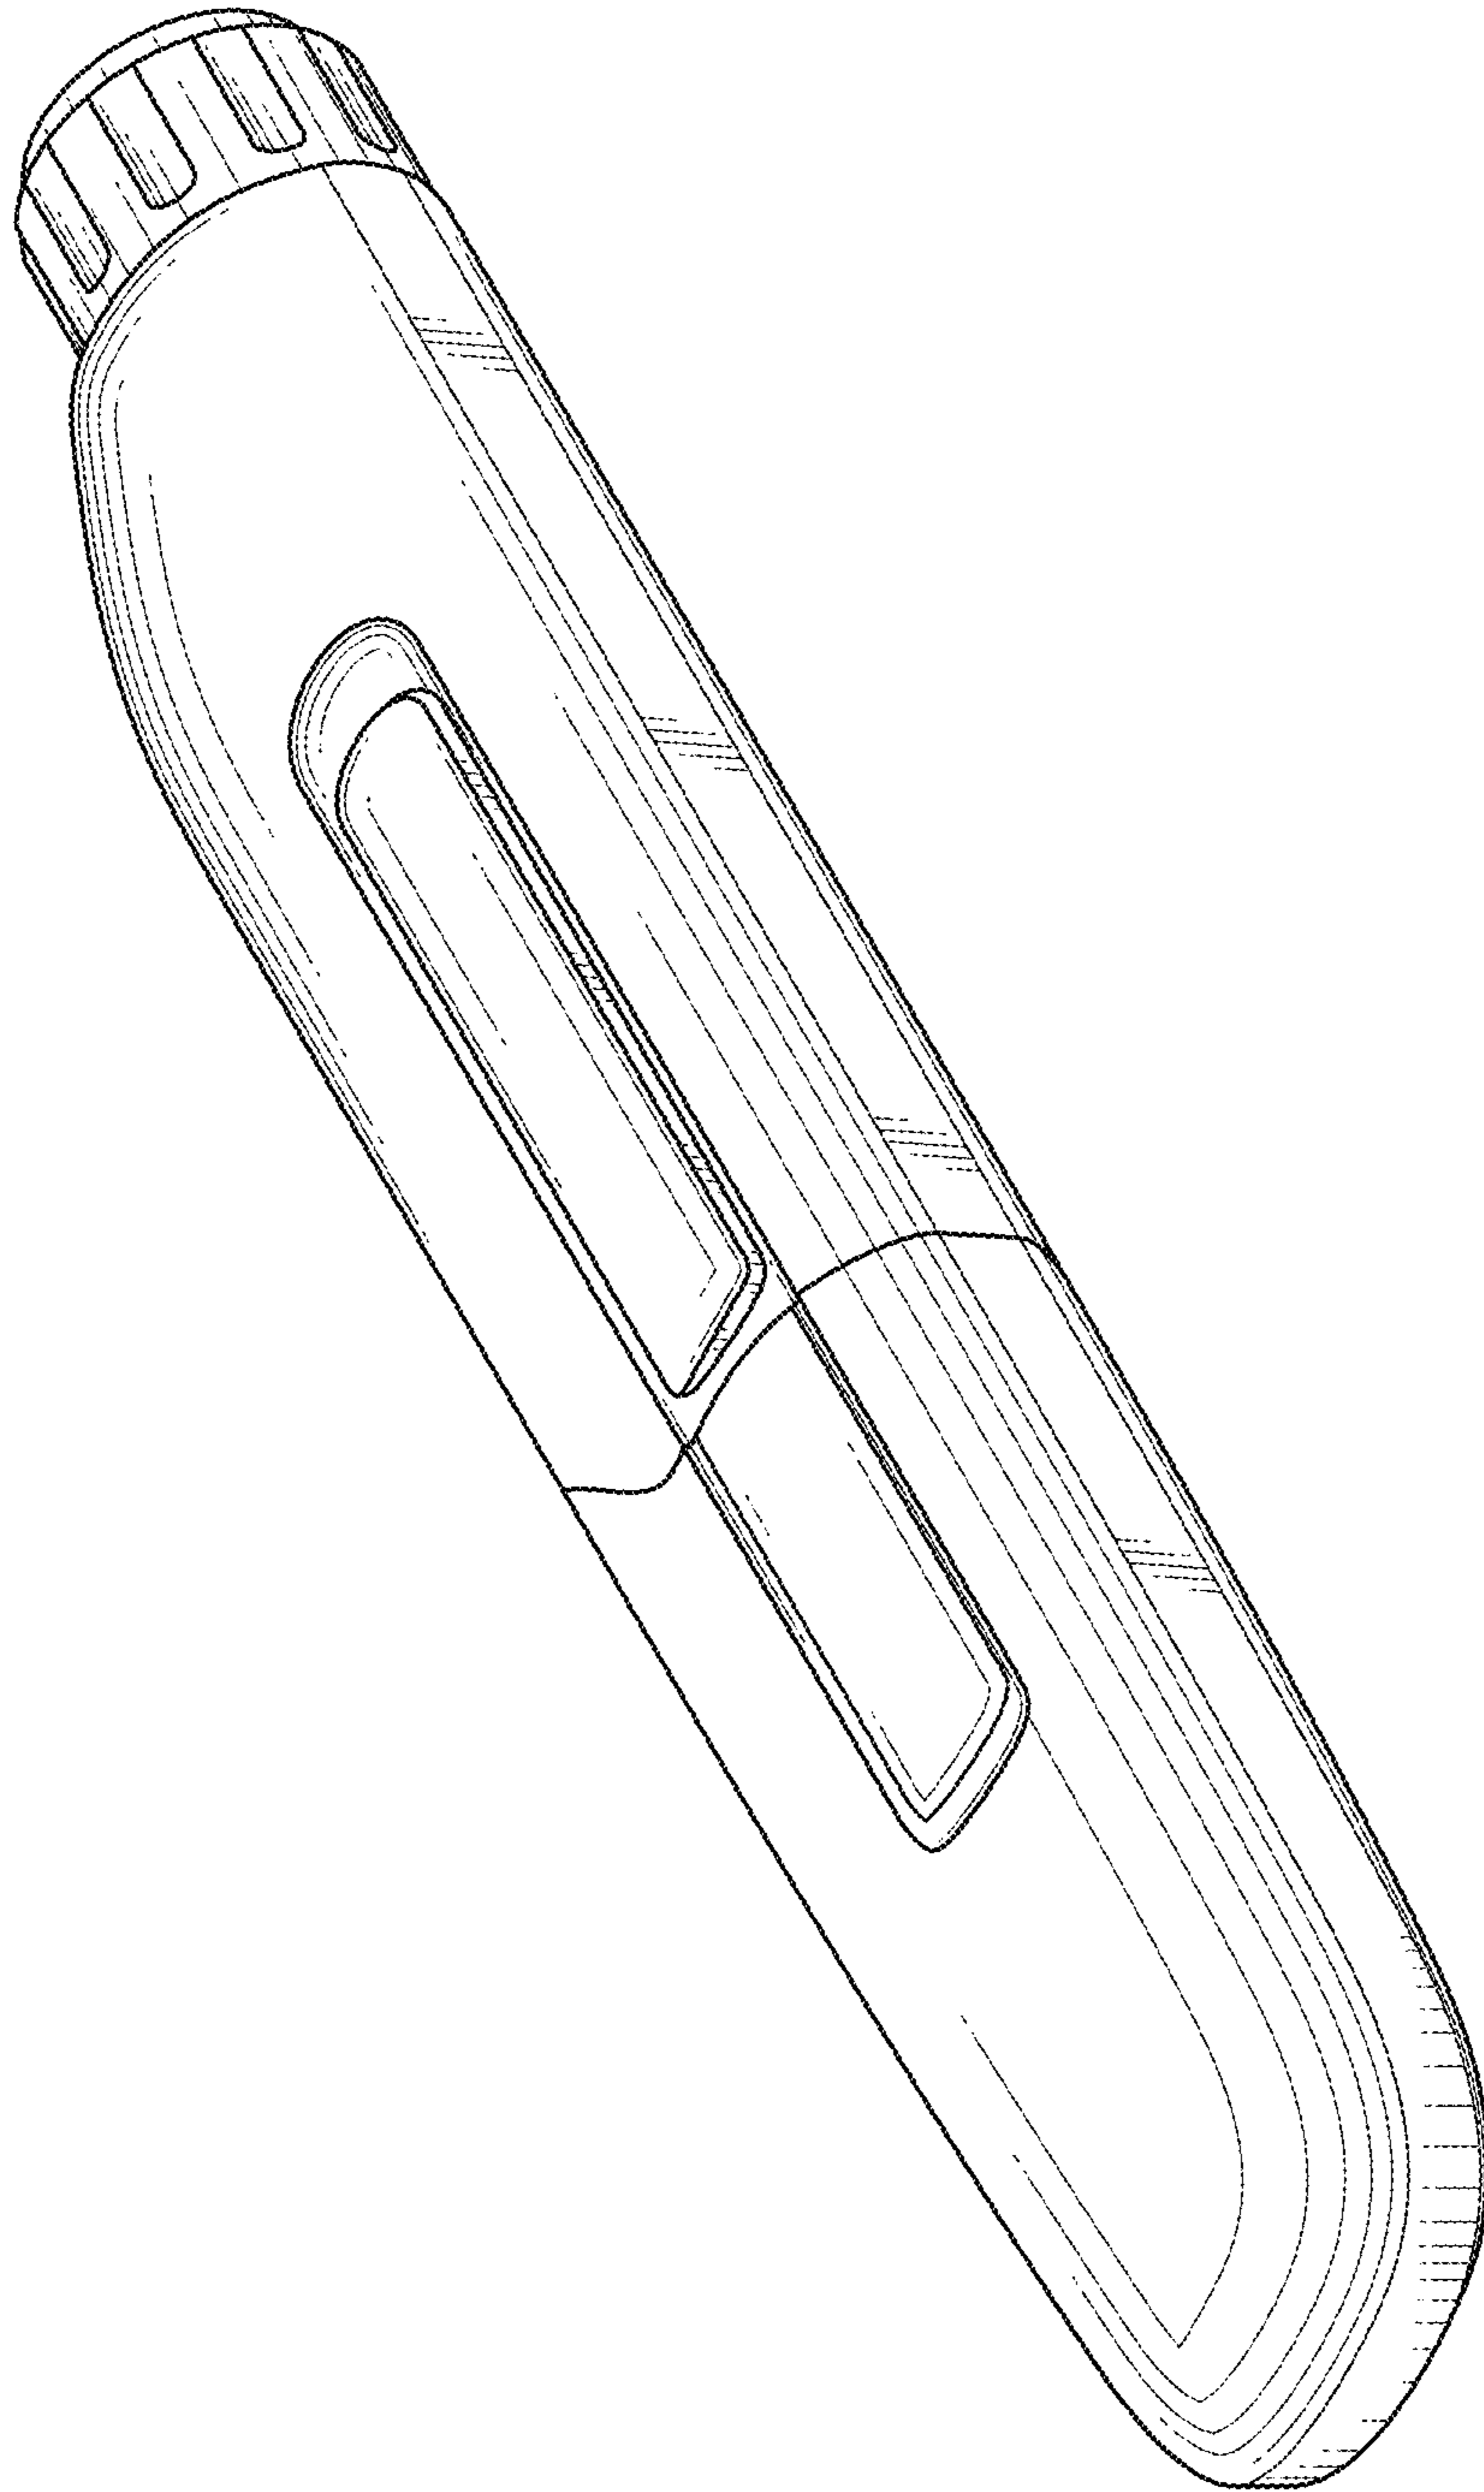


FIG. 1

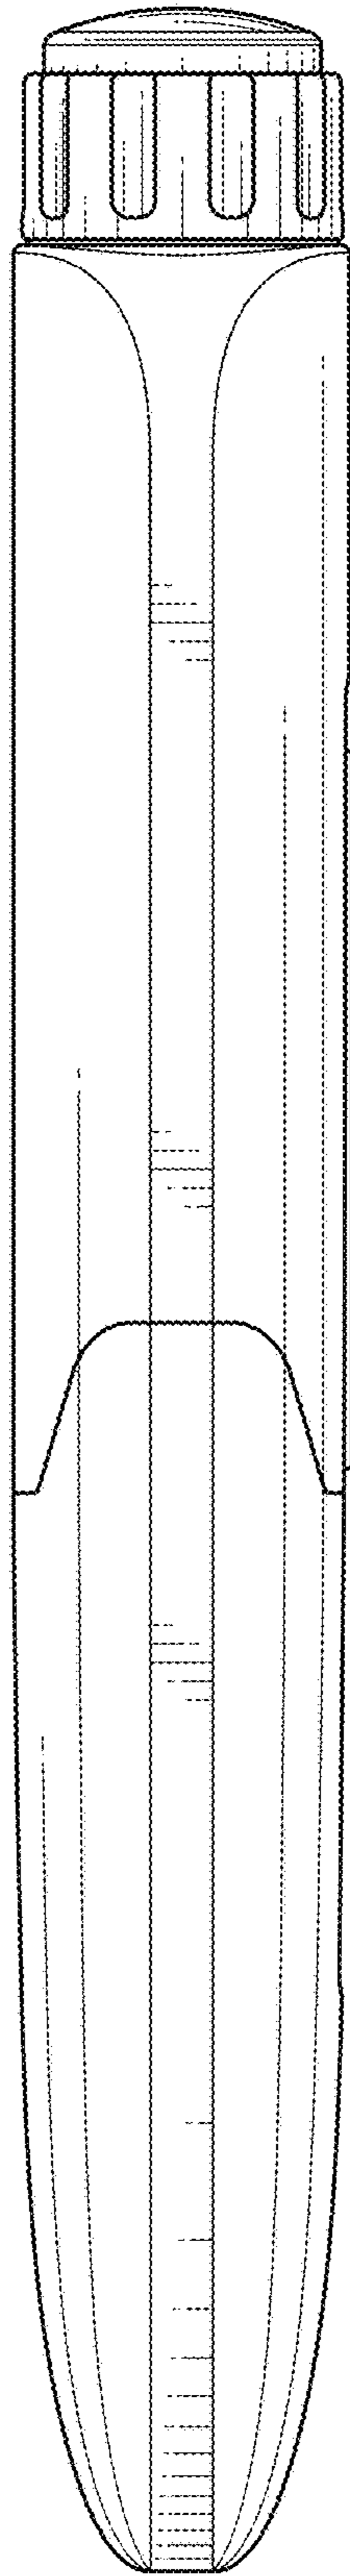


FIG. 2

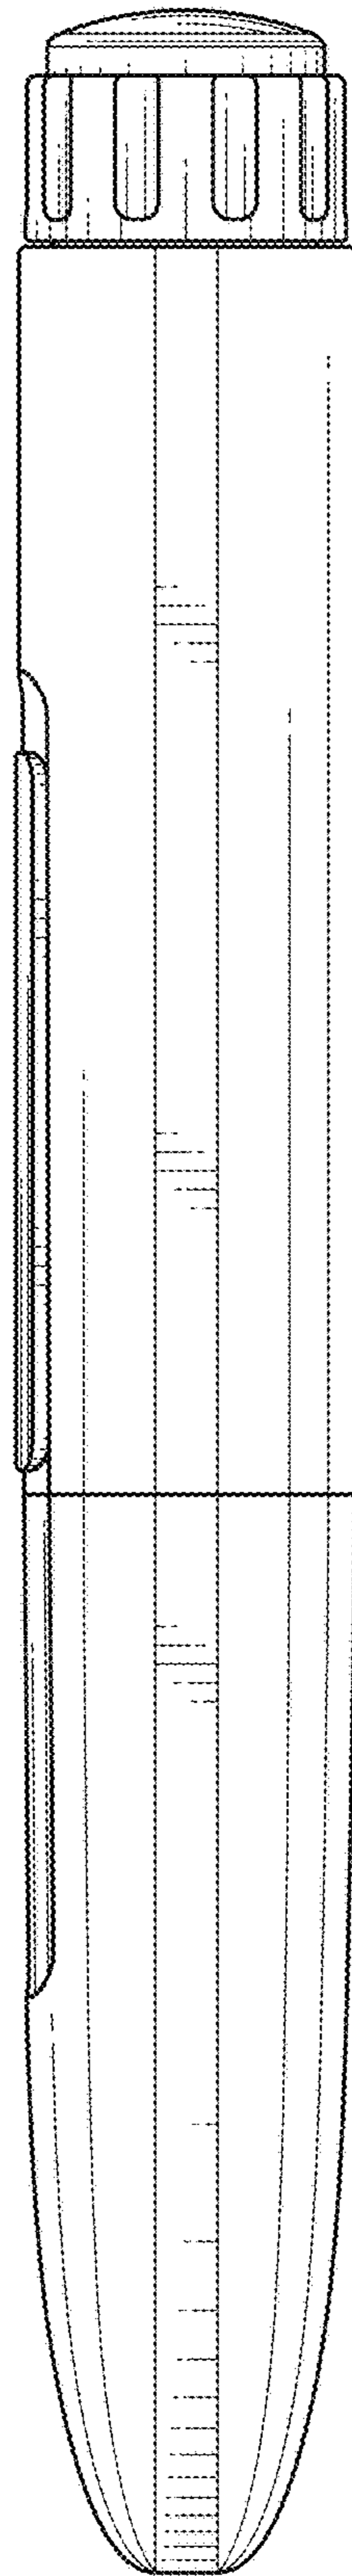


FIG. 3

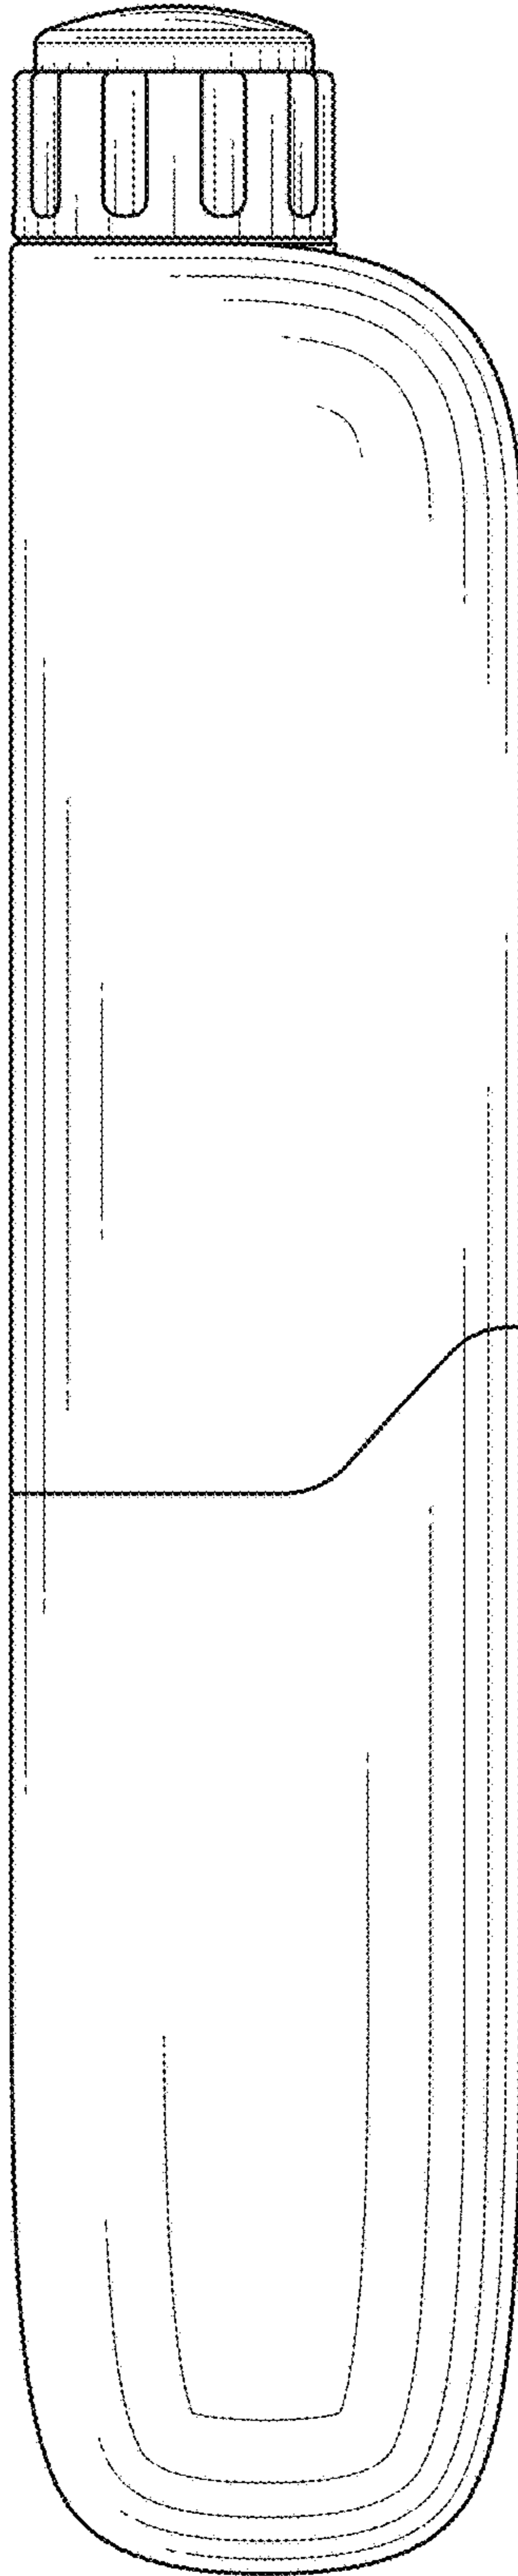


FIG. 4



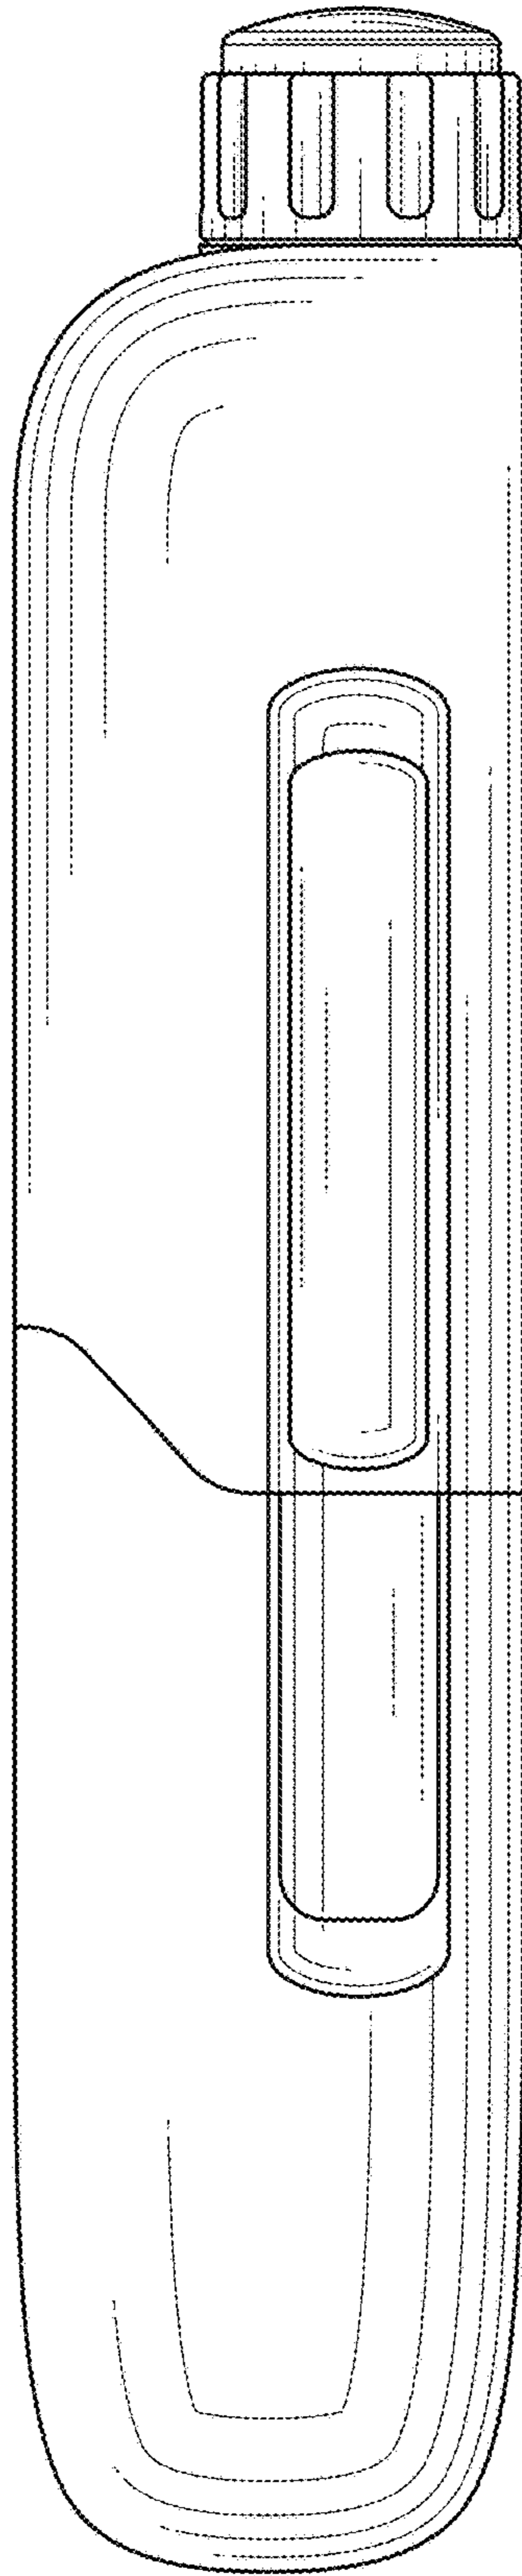
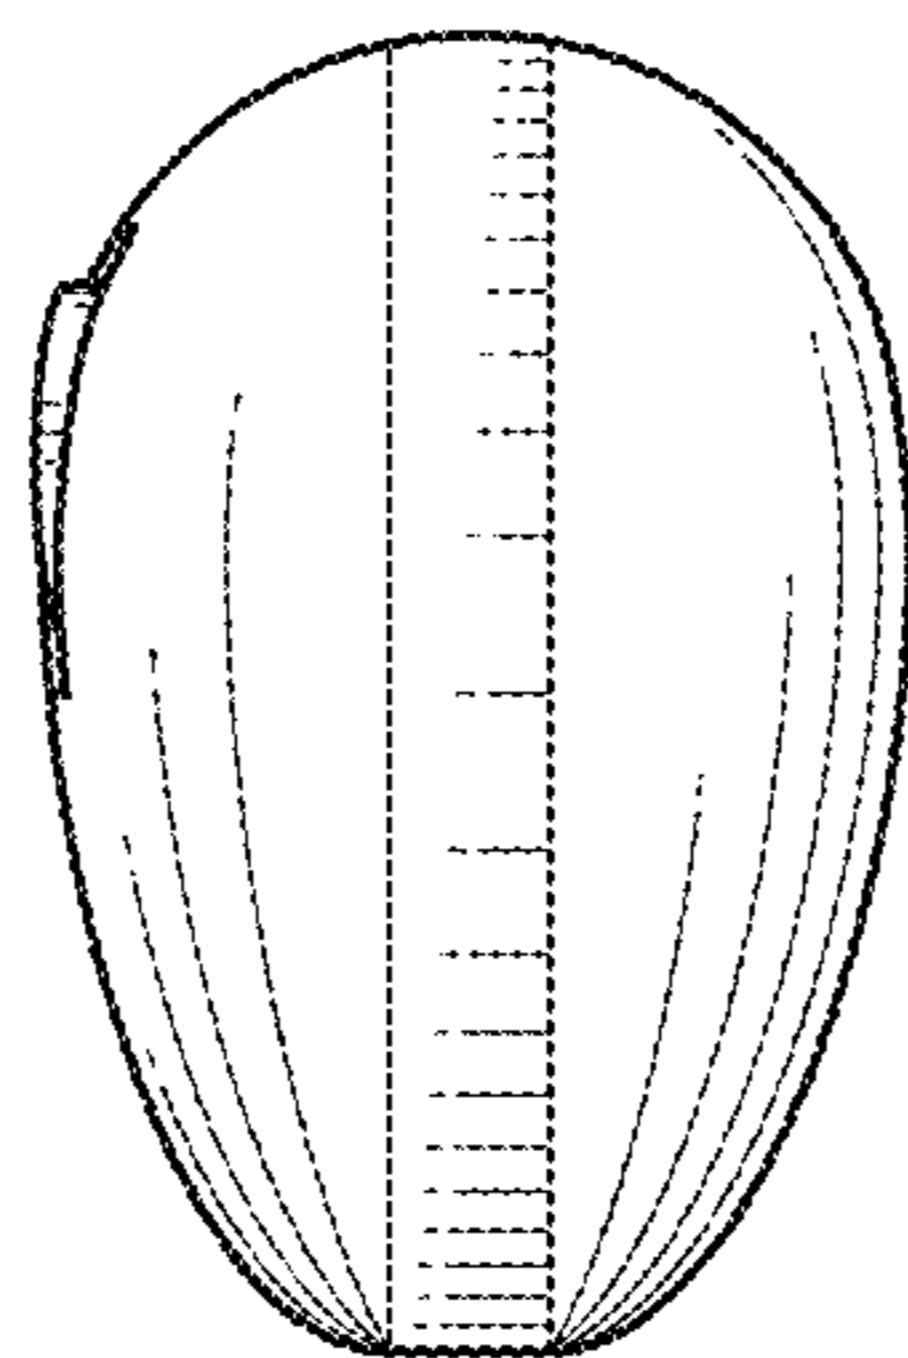
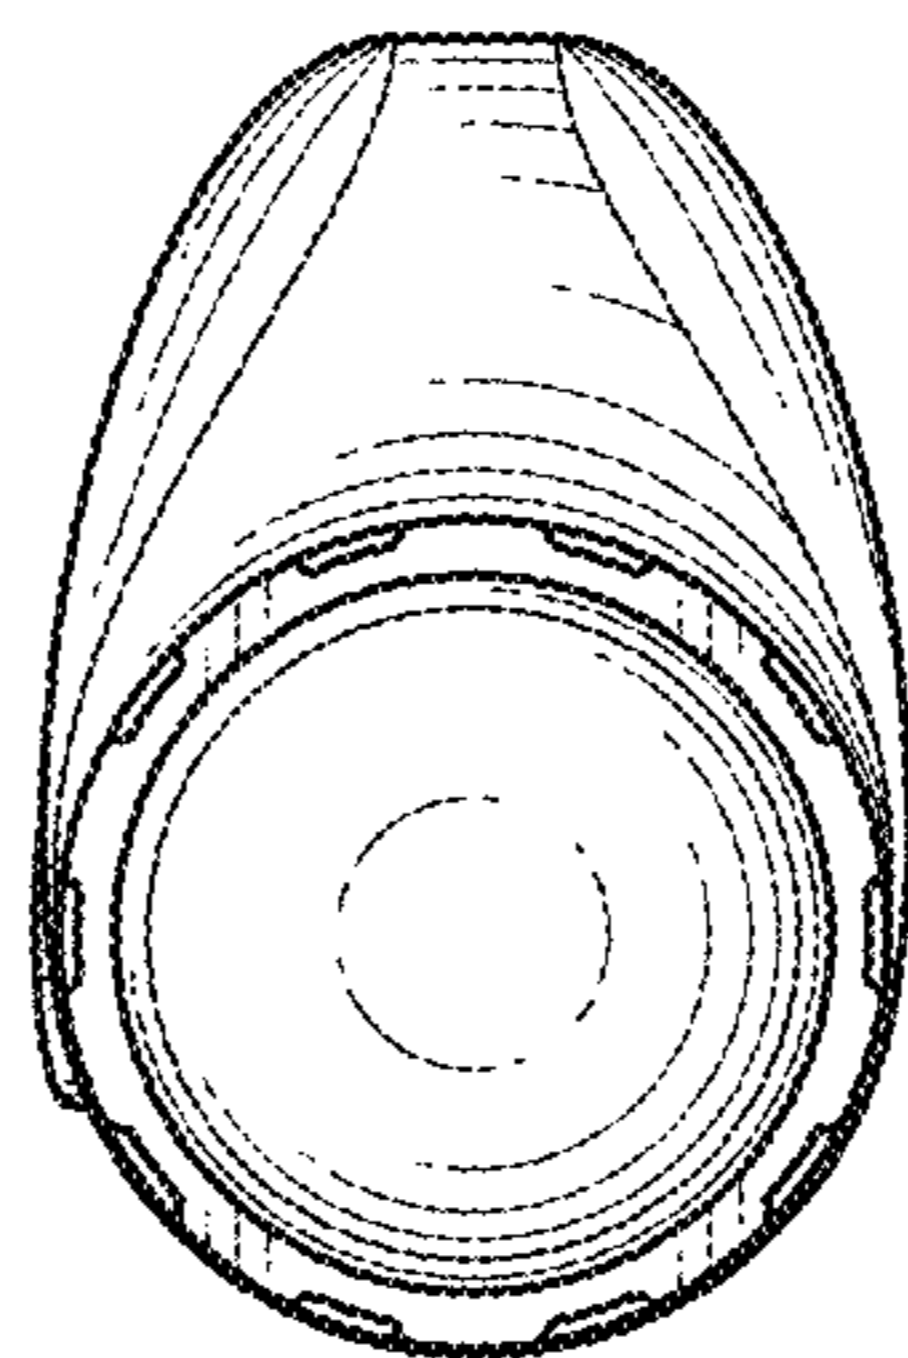


FIG. 5



**FIG. 6**



**FIG. 7**