



US00D795436S

(12) **United States Design Patent** (10) **Patent No.:** **US D795,436 S**
Ogura (45) **Date of Patent:** **** Aug. 22, 2017**

(54) **MEDICAL X-RAY IMAGING APPARATUS**
(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)
(72) Inventor: **Ryosuke Ogura**, Kanagawa (JP)
(73) Assignee: **FUJIFILM Corporation**, Tokyo (JP)
(**) Term: **15 Years**
(21) Appl. No.: **29/565,715**
(22) Filed: **May 24, 2016**
(30) **Foreign Application Priority Data**

Nov. 27, 2015 (JP) 2015-026552
(51) **LOC (10) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/158**
(58) **Field of Classification Search**
USPC D24/158-161, 186, 107, 185; D34/19,
D34/20, 25; D6/662
CPC .. A61B 5/05; A61B 5/055; A61B 6/03; A61B
6/035; A61B 6/4405; A61B 6/4411; A61B
6/4435; A61B 6/4441; A61B 6/4447
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
6,126,314 A * 10/2000 Morasse G03B 42/045
378/167
D546,453 S * 7/2007 McNair, Jr. D24/161
D599,480 S * 9/2009 Weichert D24/158
D617,906 S * 6/2010 Nakahara D24/158
D690,012 S * 9/2013 Yanase D24/158
D710,012 S * 7/2014 Polhamus D24/158
D724,738 S * 3/2015 Dorris D24/158
D769,446 S * 10/2016 Liu D24/158
2007/0133753 A1 * 6/2007 Jakob A61B 6/4405
378/198

2010/0329426 A1* 12/2010 Oda A61B 6/4405
378/98.2
2014/0098941 A1* 4/2014 Konkle A61B 6/4405
378/189
2016/0120489 A1* 5/2016 Yang A61B 6/4405
378/62

* cited by examiner
Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Young & Thompson

(57) **CLAIM**
The ornamental design for a medical X-ray imaging apparatus, as shown and described.

DESCRIPTION
FIG. 1 is a top, front and left side perspective view of a medical X-ray imaging apparatus showing my new design; FIG. 2 is a top, rear and left side perspective view thereof; FIG. 3 is a front elevational view thereof; FIG. 4 is a rear elevational view thereof; FIG. 5 is a top plan view thereof; FIG. 6 is a bottom plan view thereof; FIG. 7 is a left side elevational view thereof; FIG. 8 is a right side elevational view thereof; FIG. 9 is a front elevational view thereof in a state that an arm having an X-ray irradiation device at its distal end is folded; FIG. 10 is an enlarged cross-sectional view thereof taken along lines X-X of FIG. 9, in which an internal mechanism is omitted; and, FIG. 11 is a top, rear and left side perspective view thereof, showing a state that an electronic cassette is put in a housing section such that the electronic cassette is charged. The broken line portions of the X-ray imaging apparatus throughout the drawings are shown to illustrate environment only and form no part of the claimed design.

1 Claim, 11 Drawing Sheets

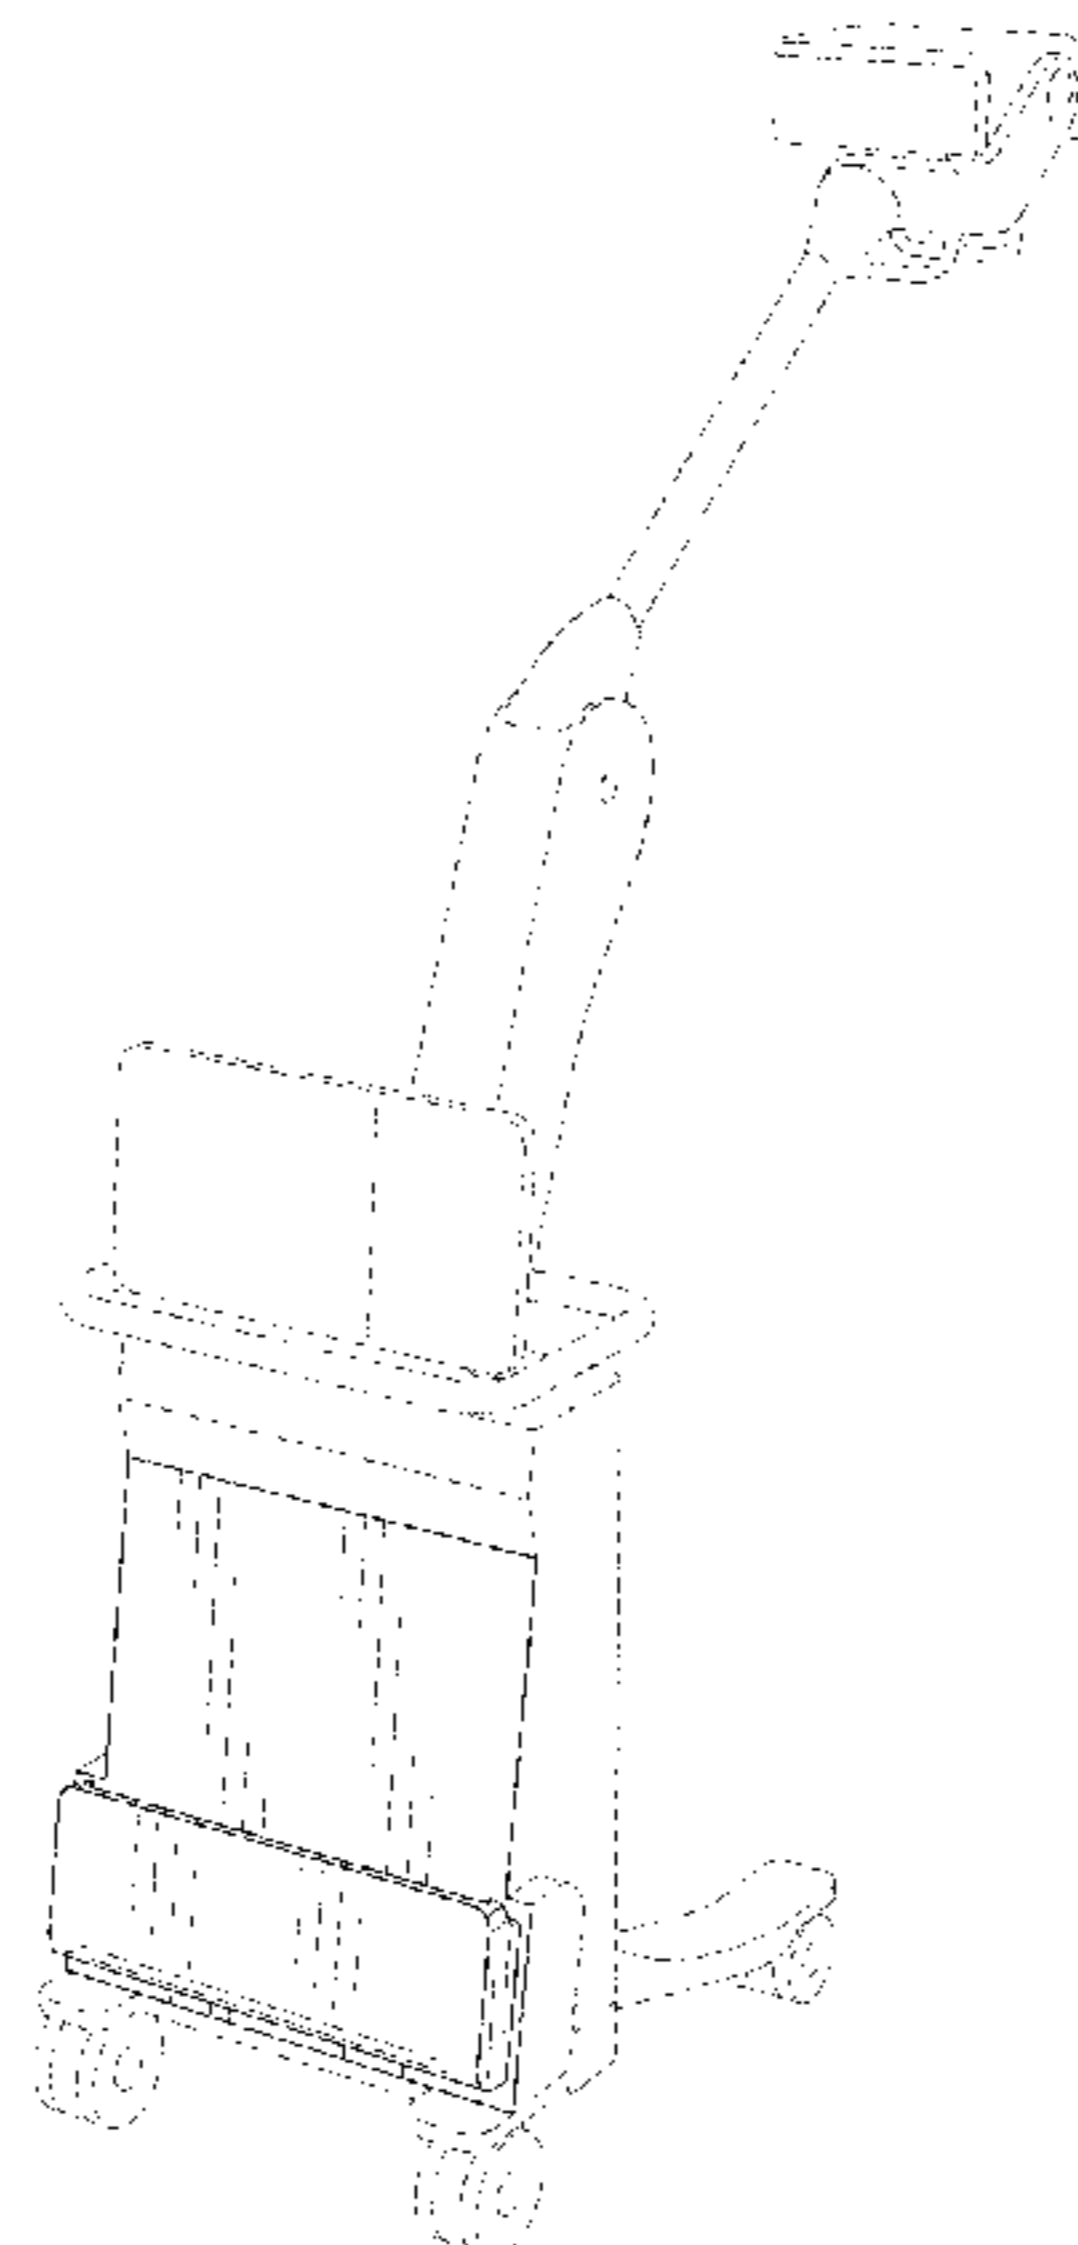


FIG. 1

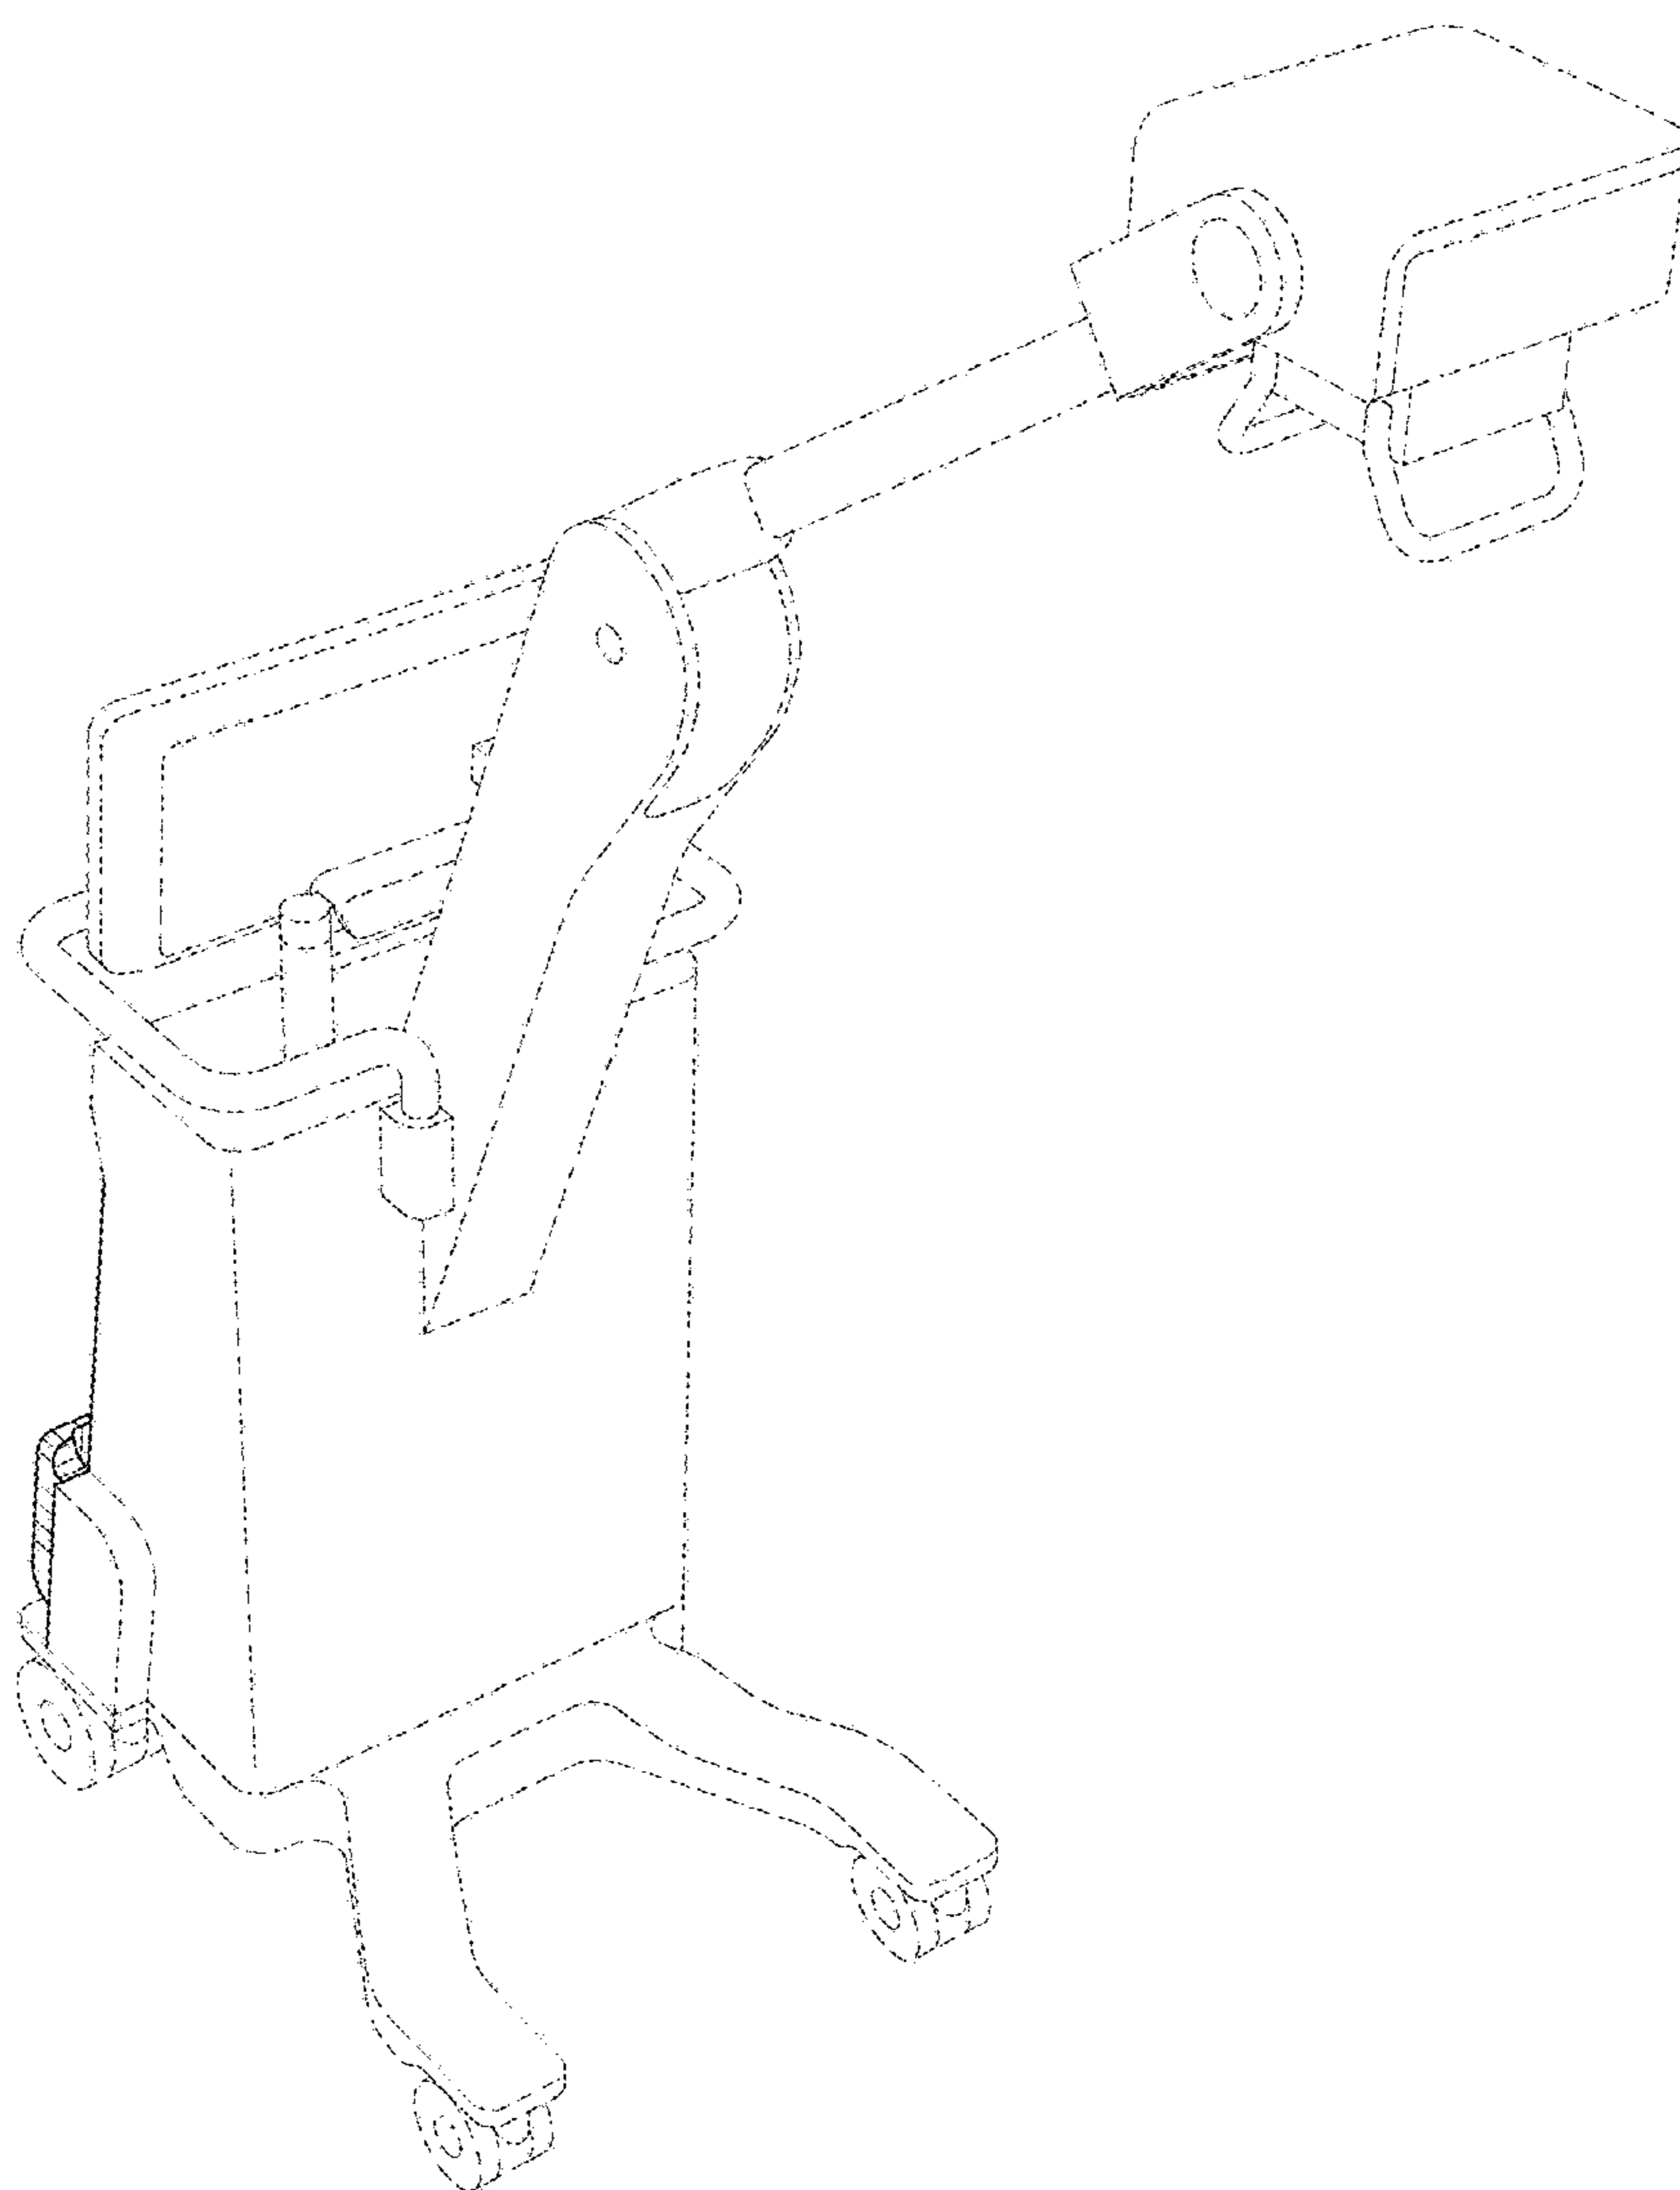


FIG. 2

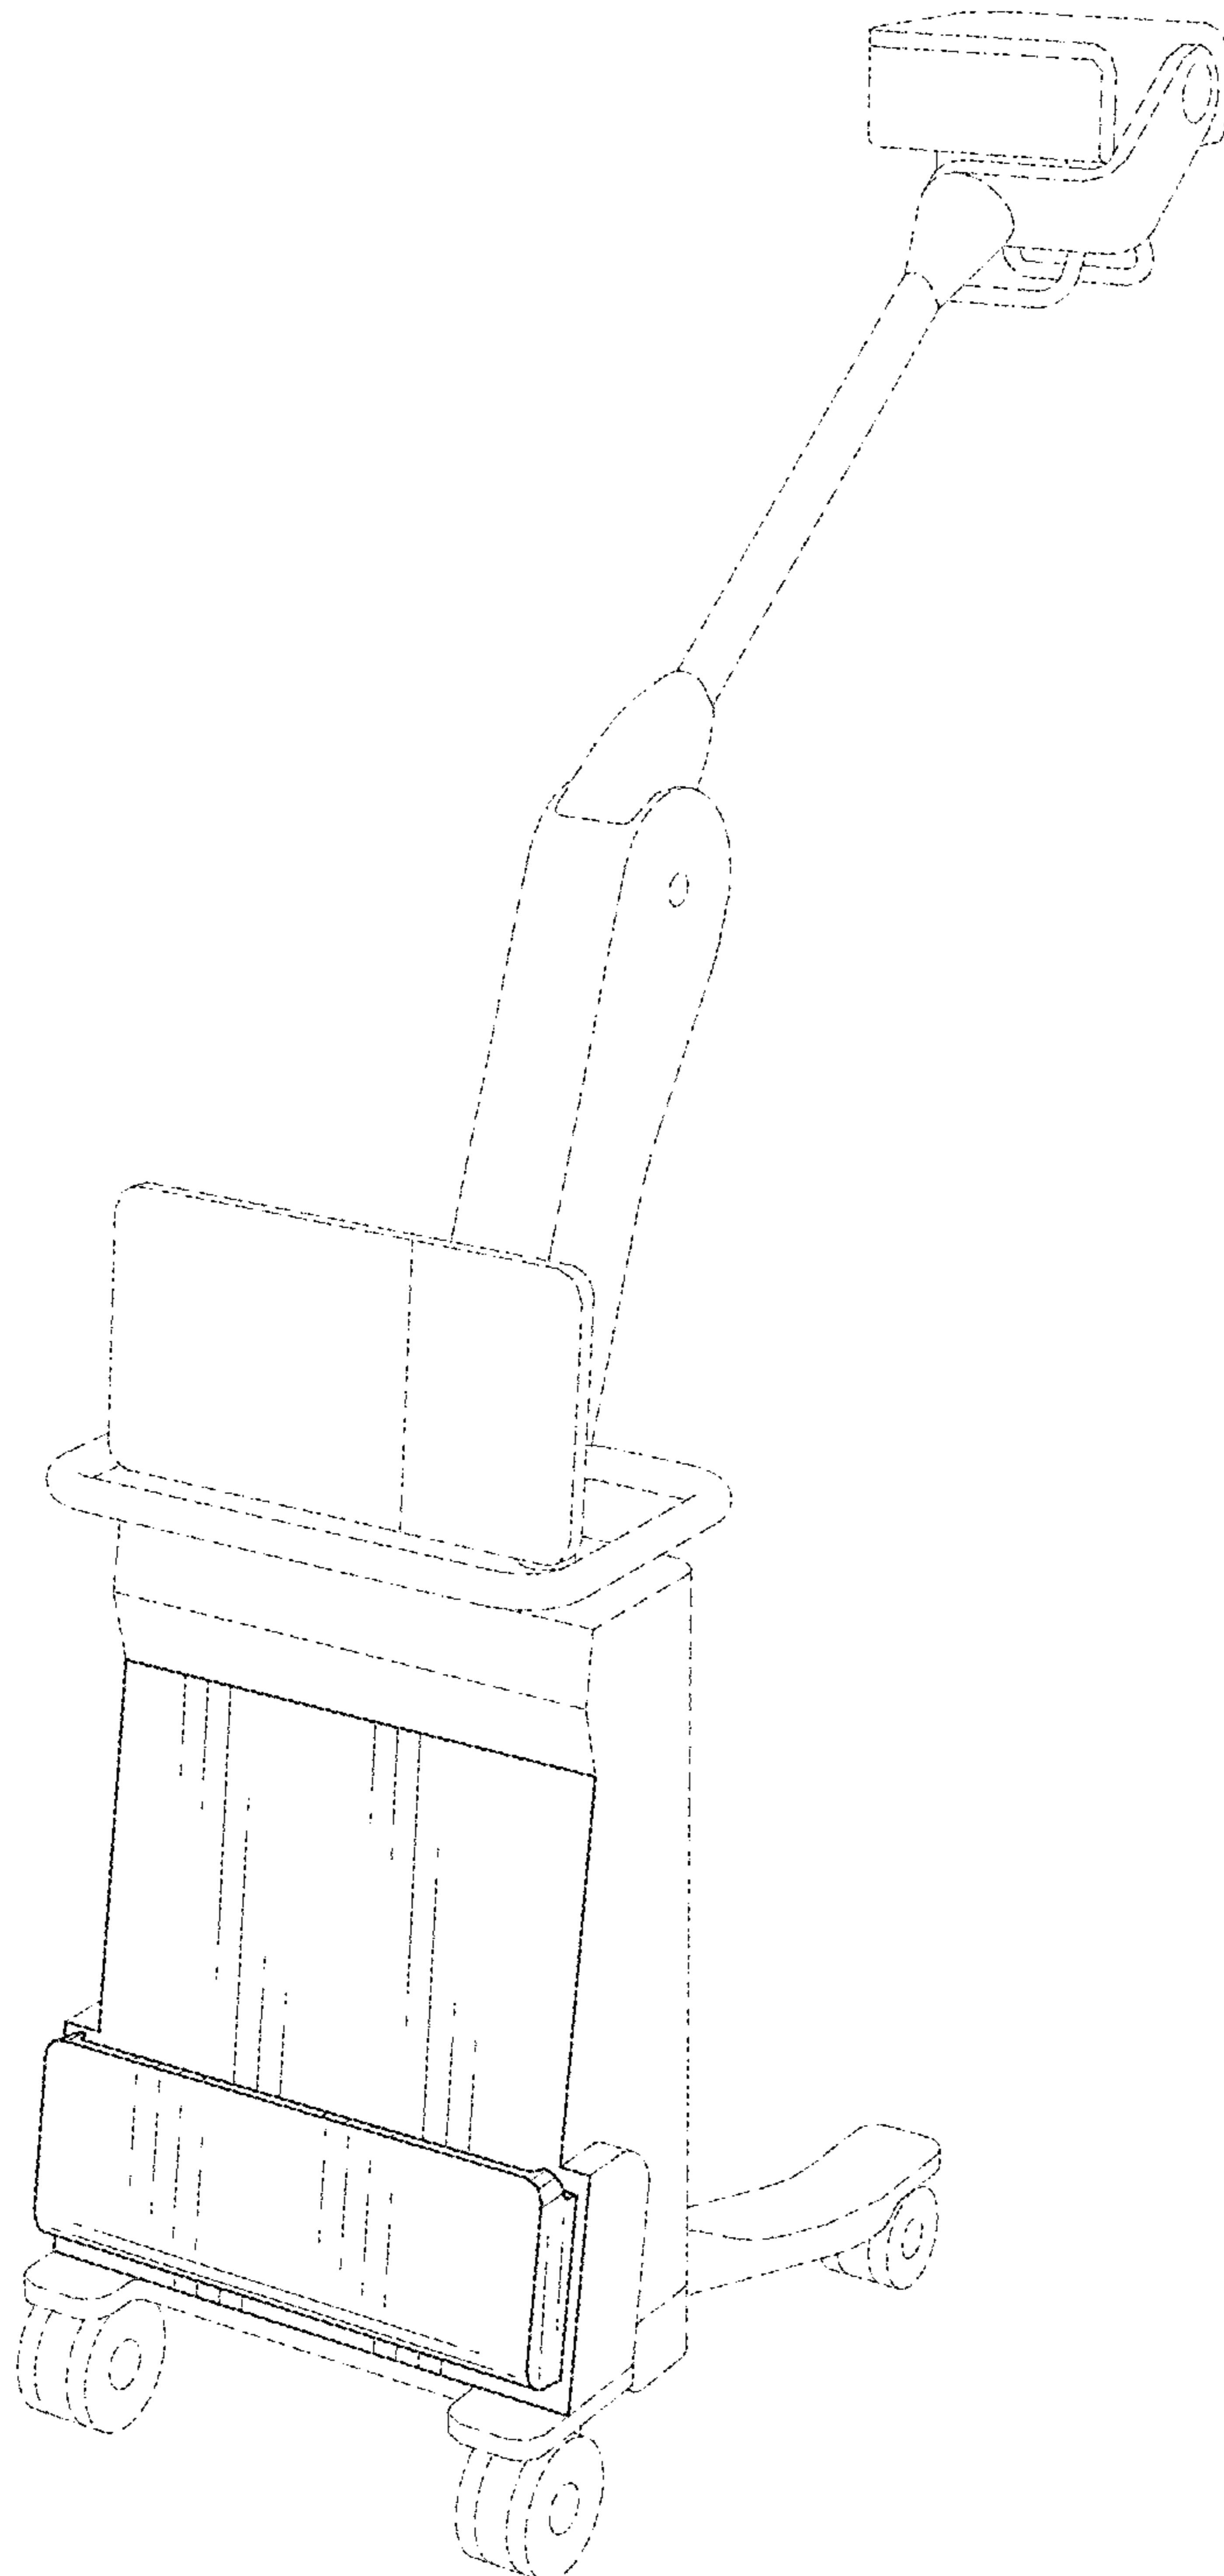


FIG. 3

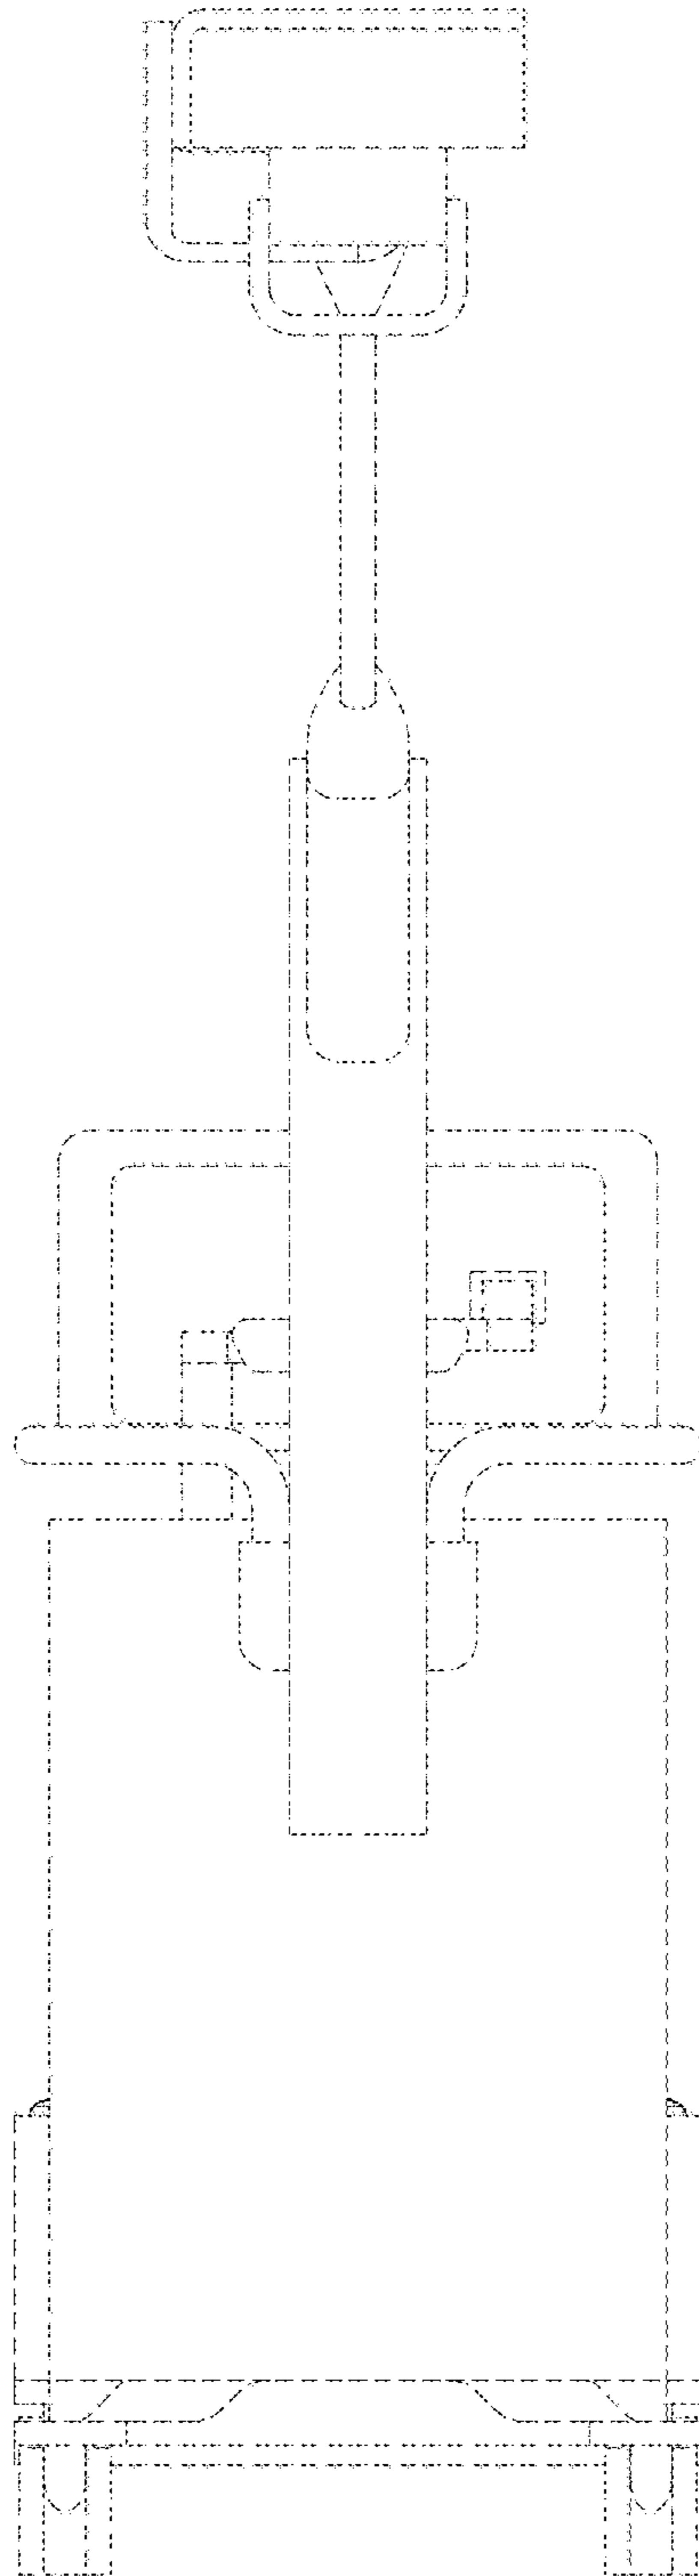


FIG. 4

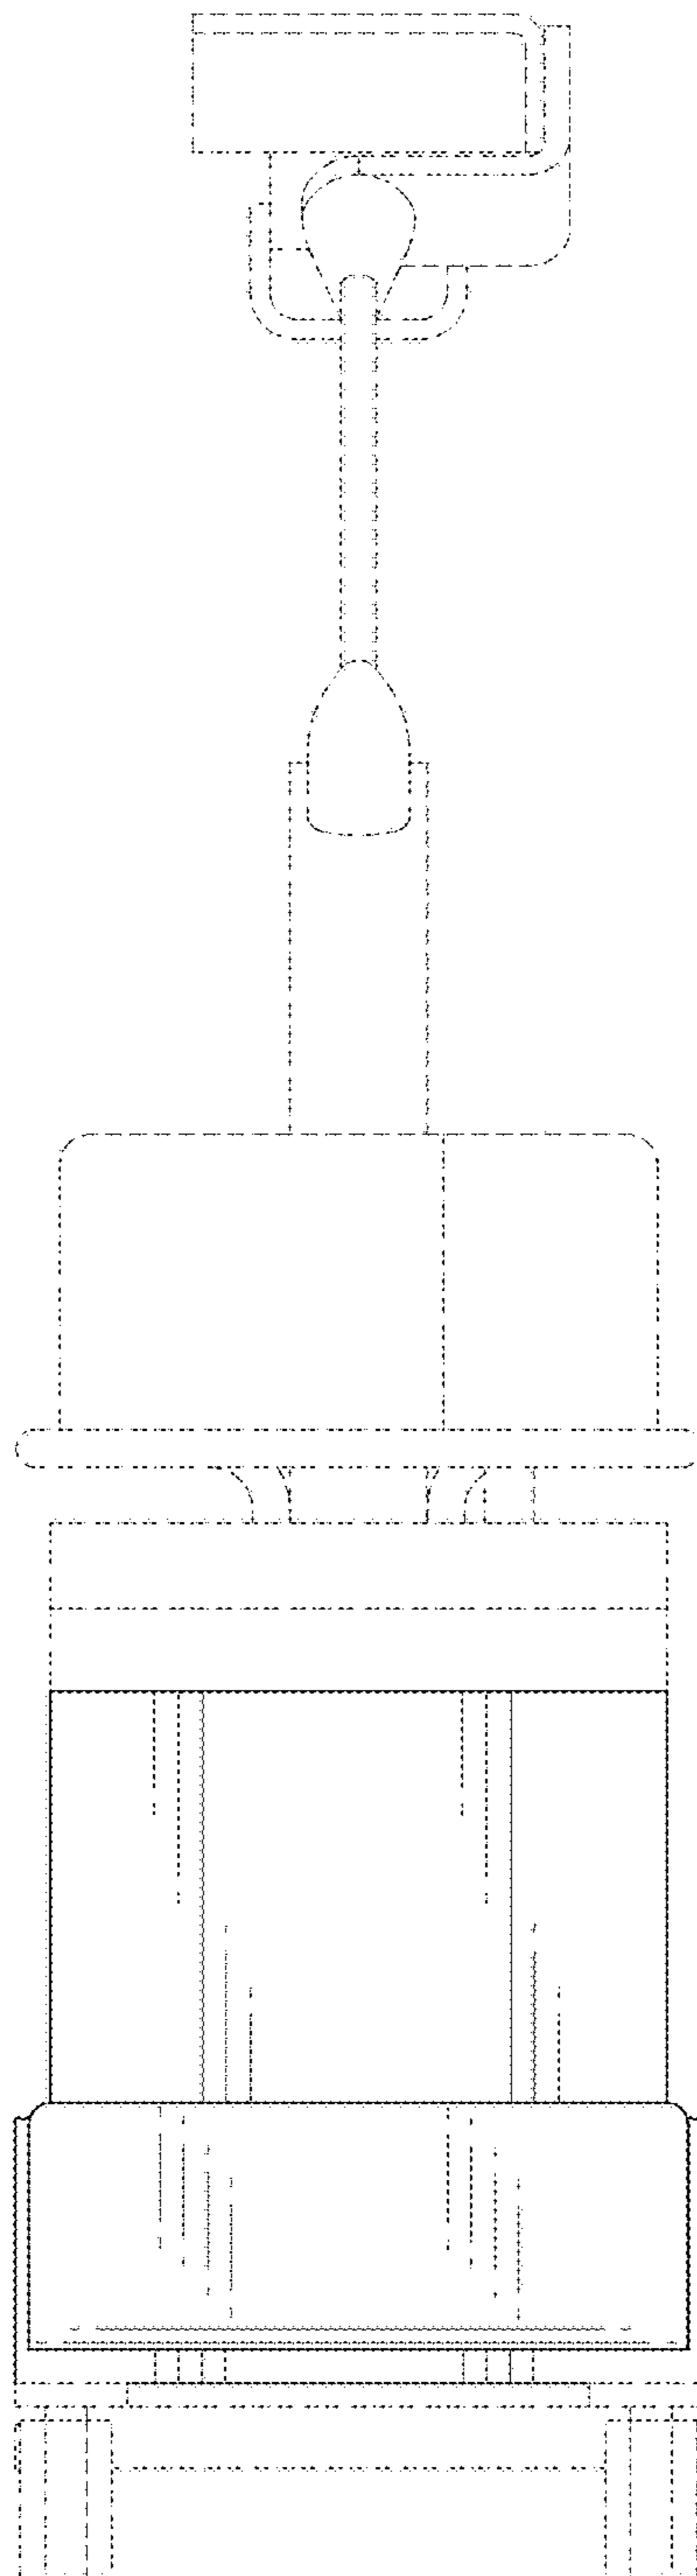


FIG. 5

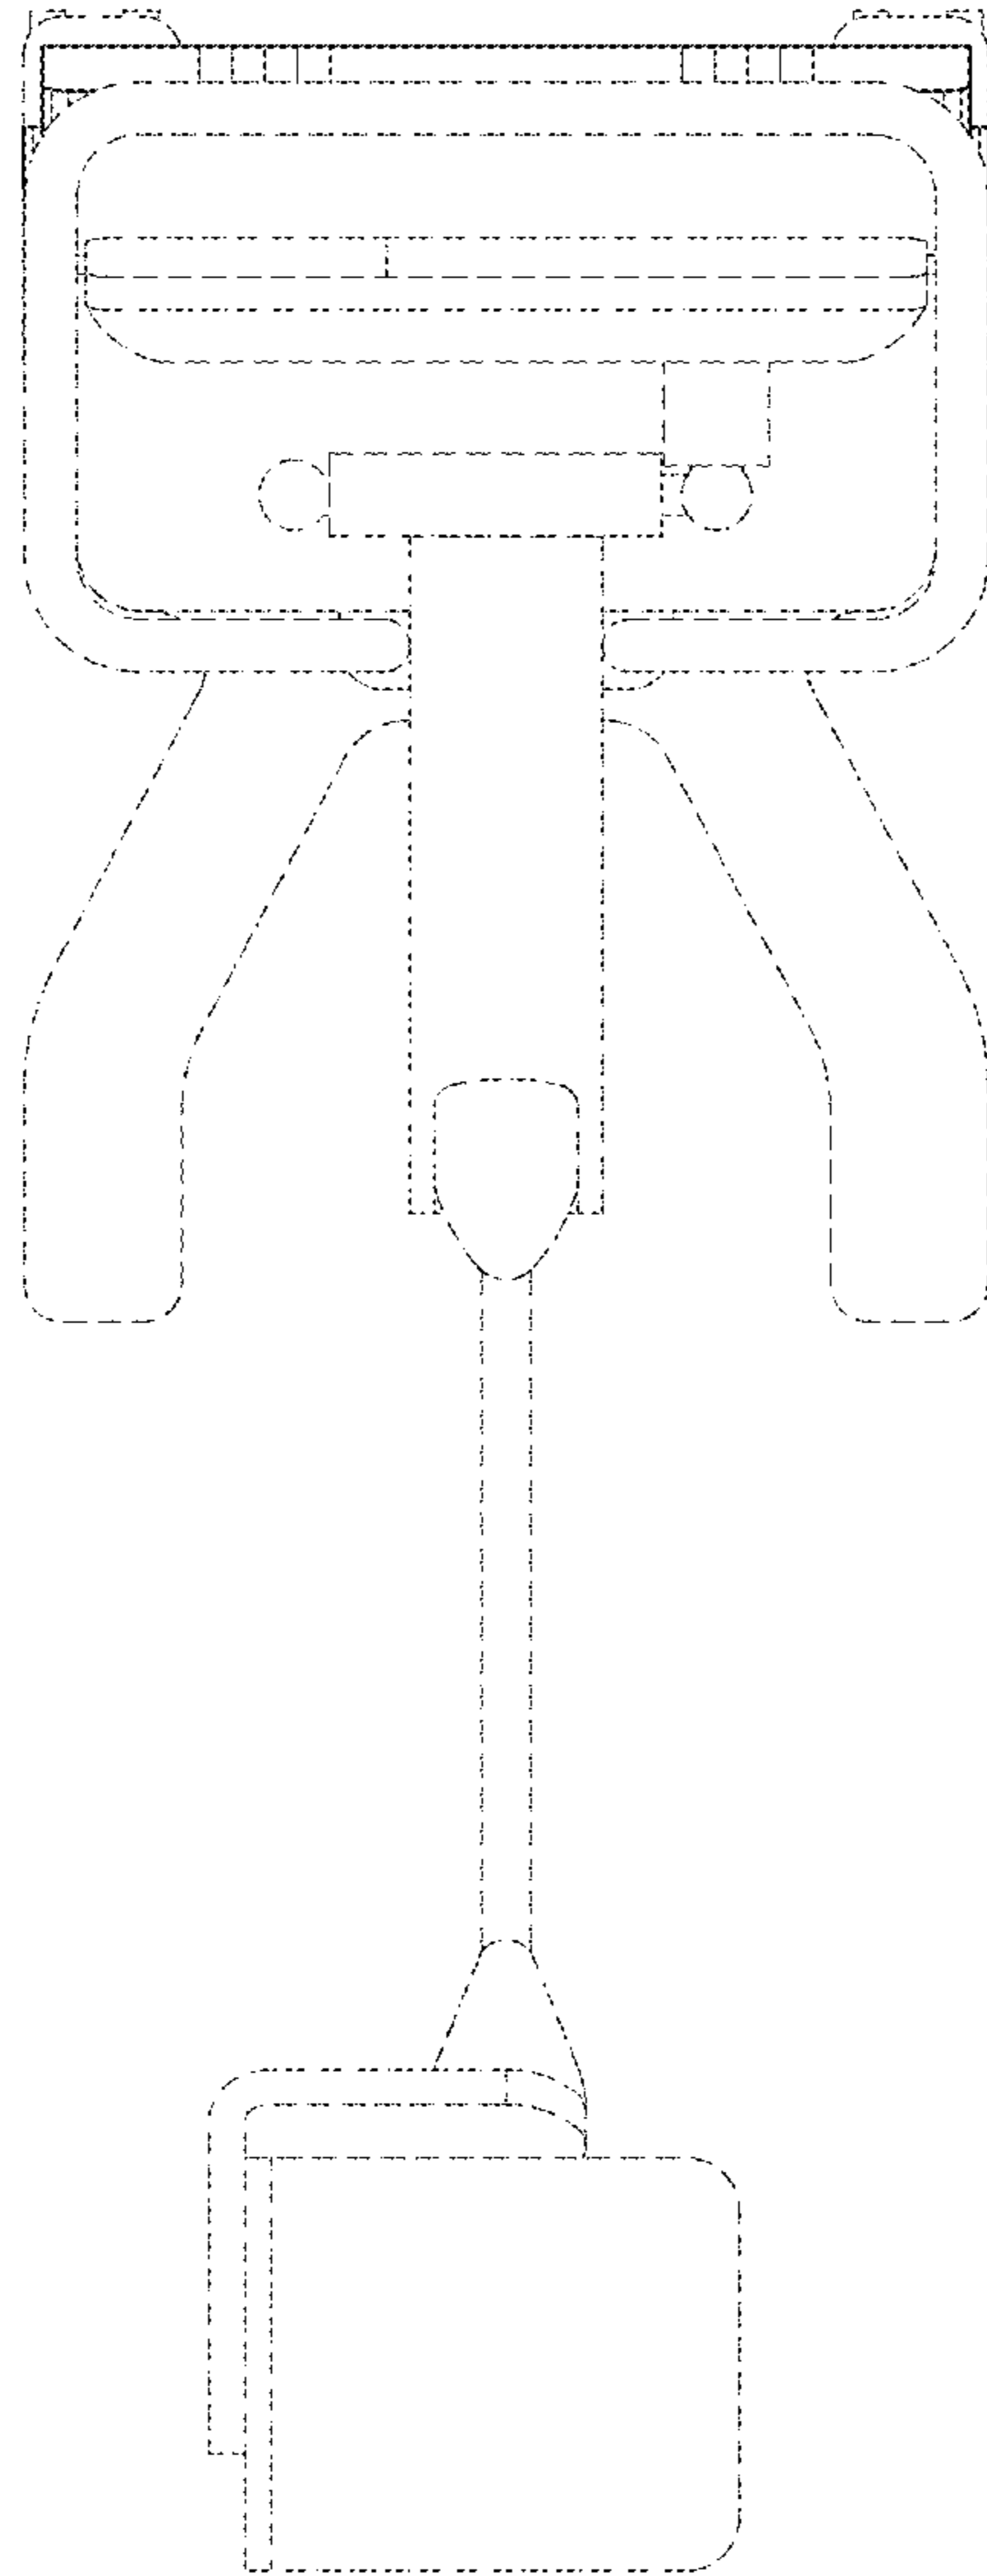


FIG. 6

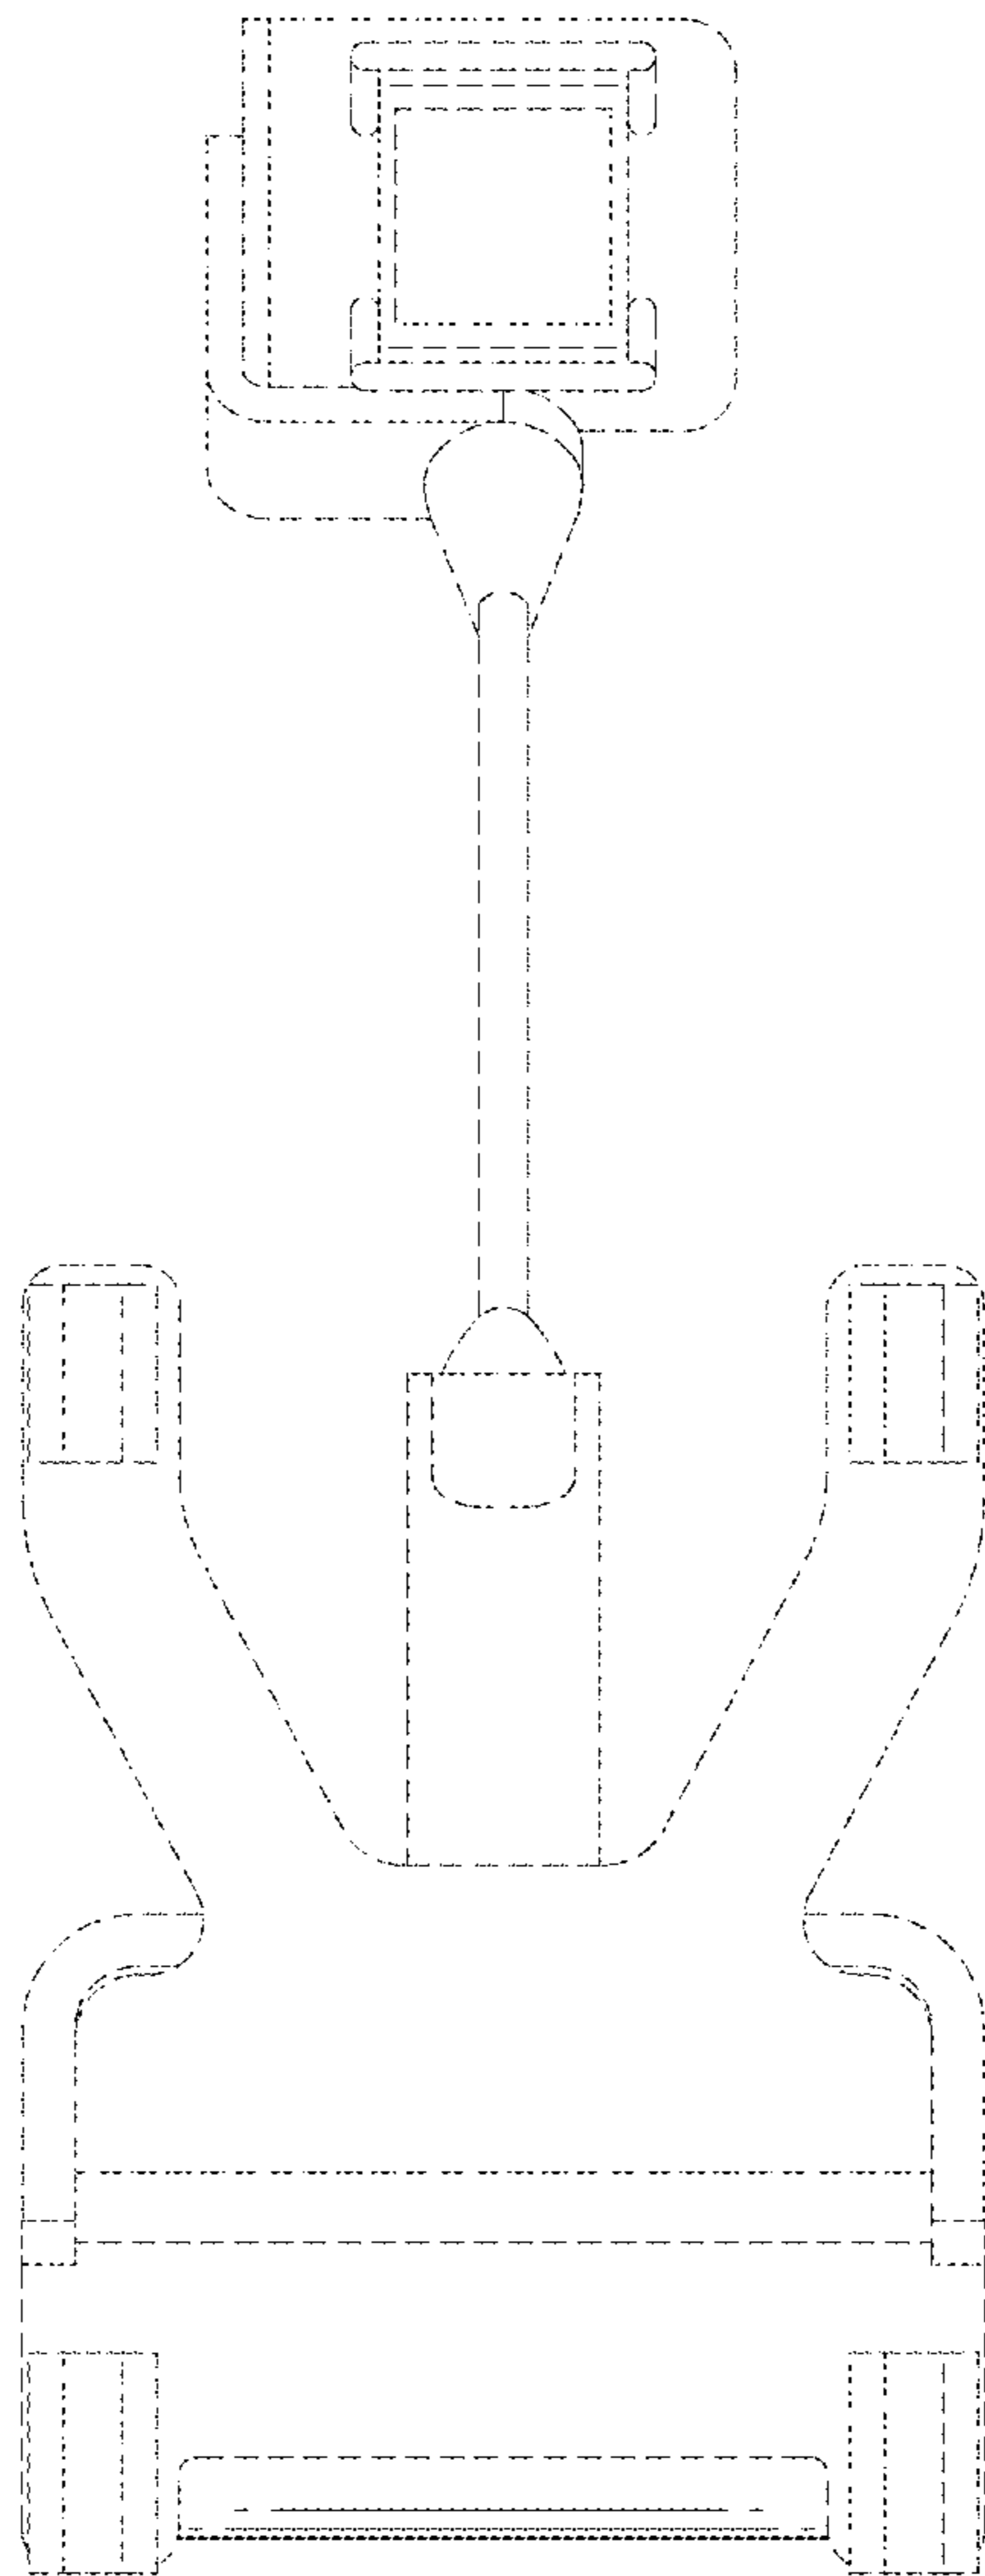


FIG. 7

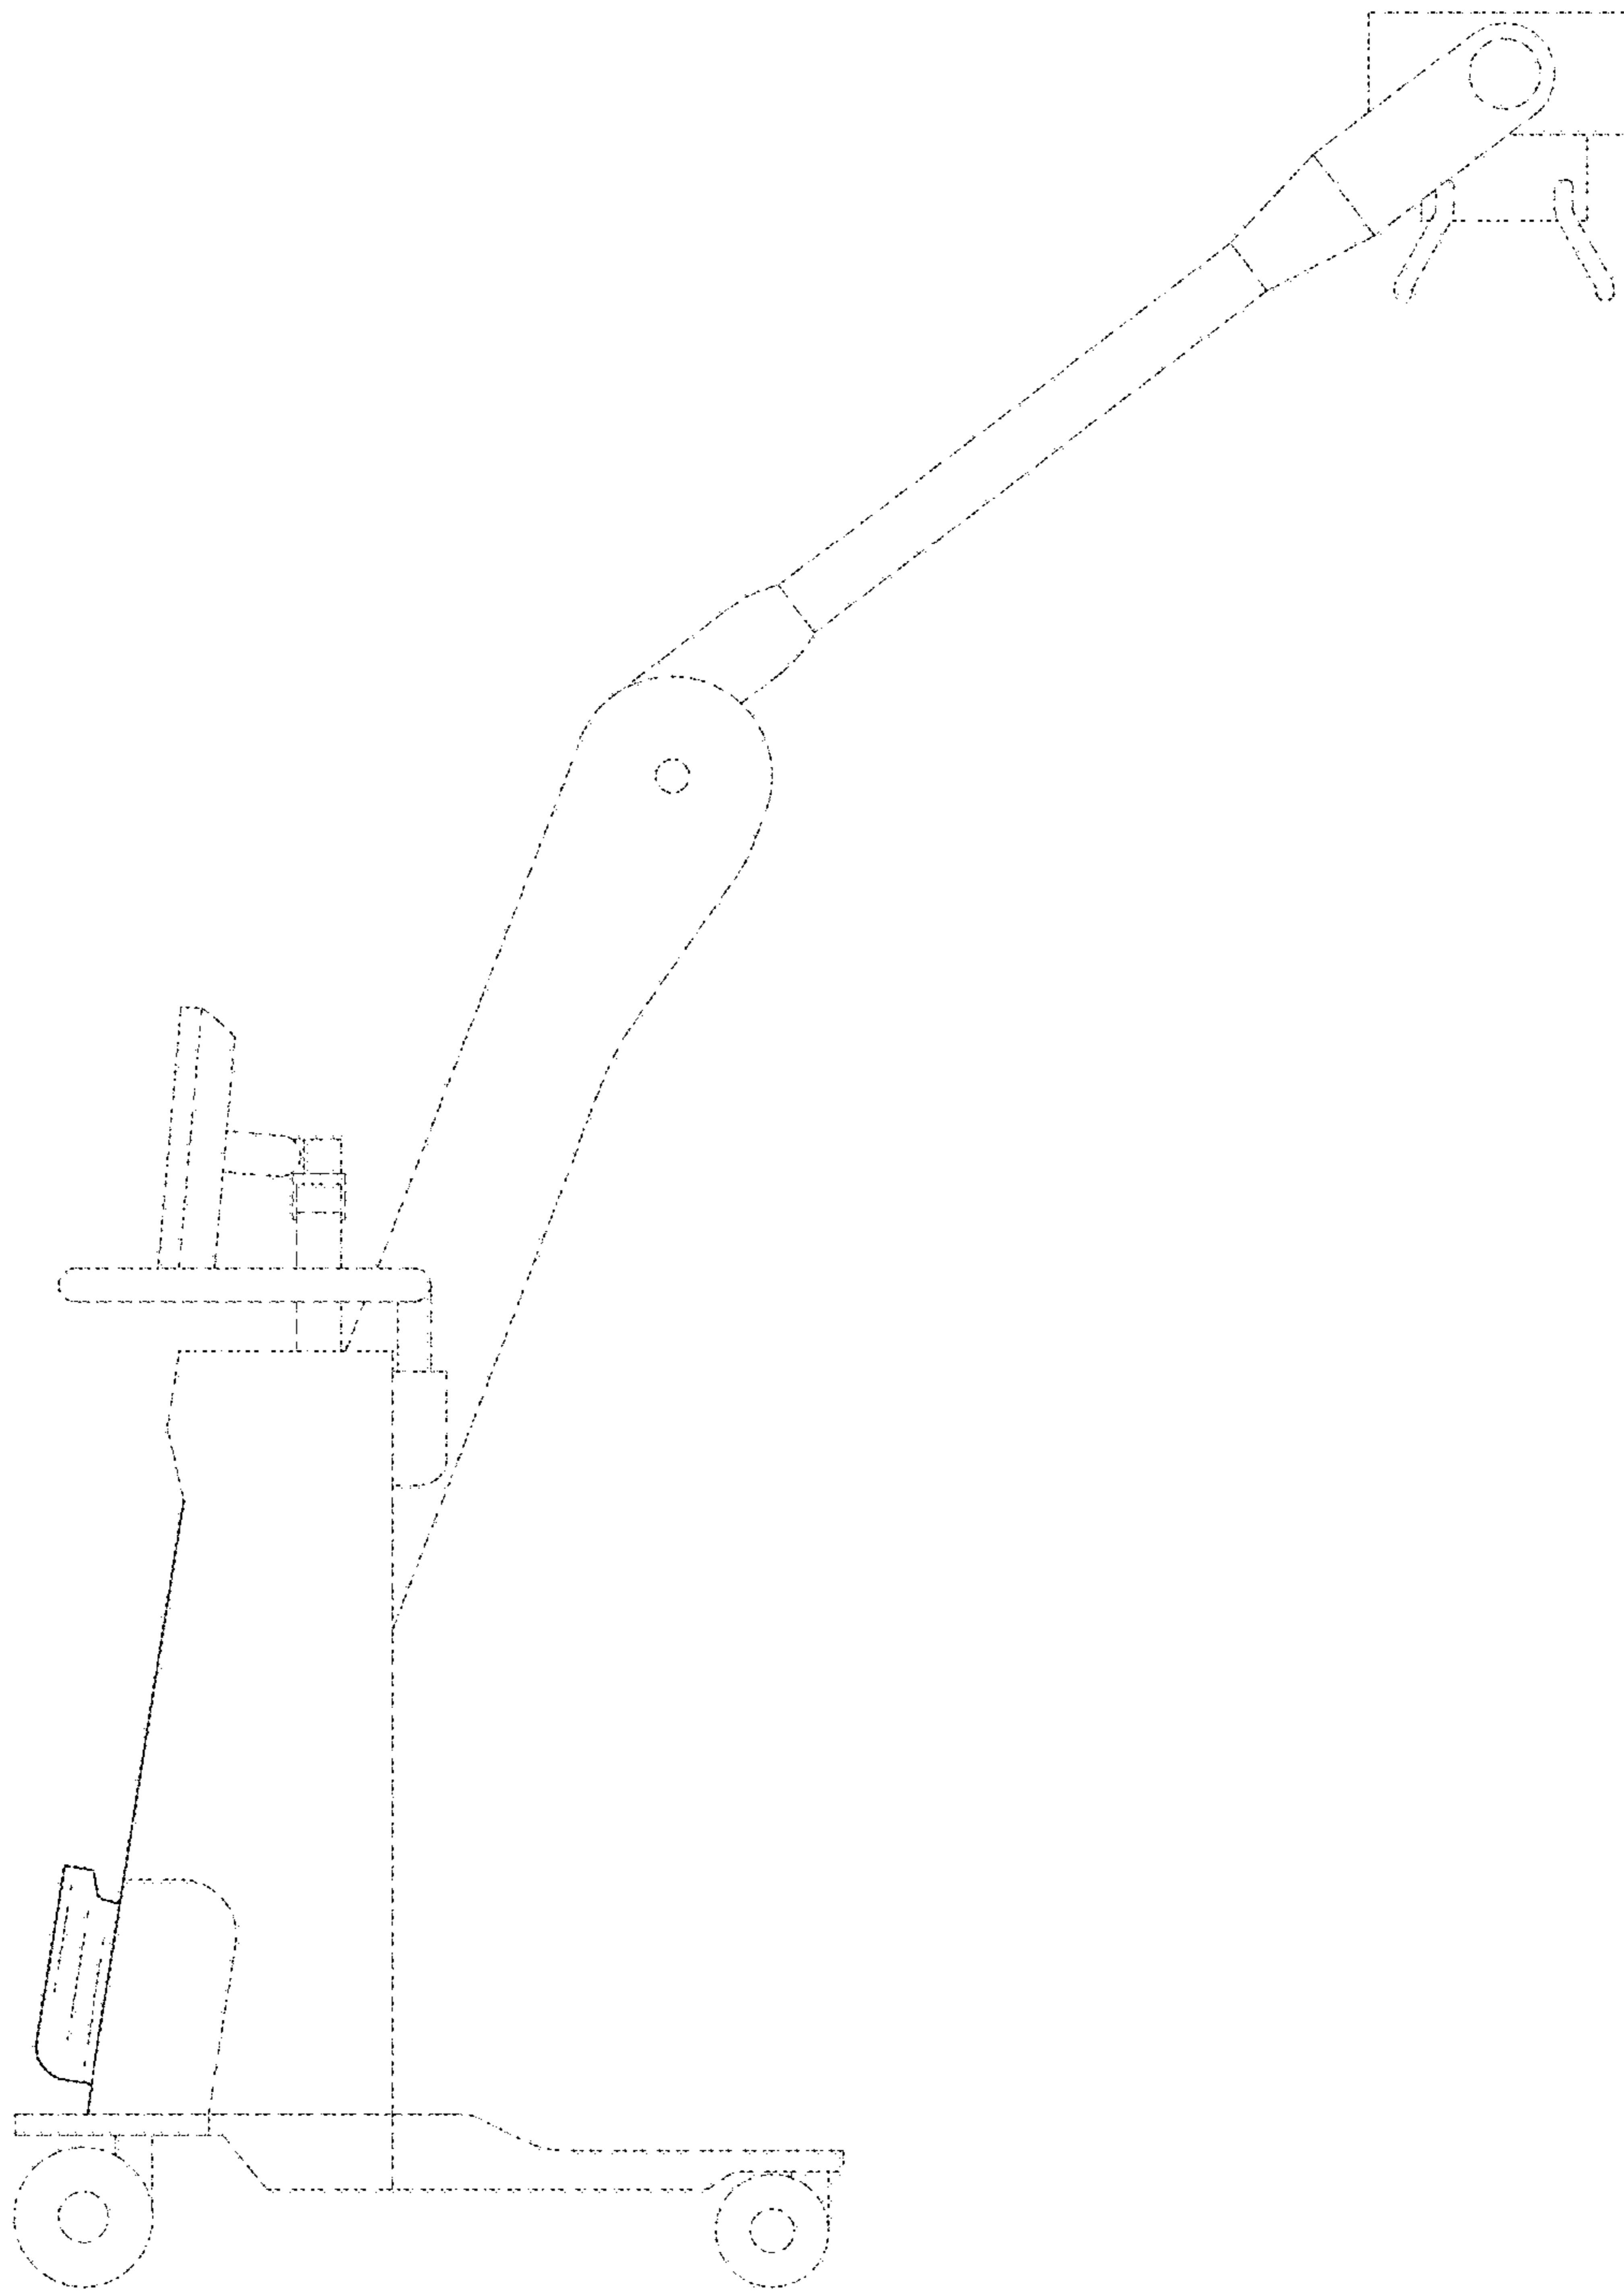


FIG. 8

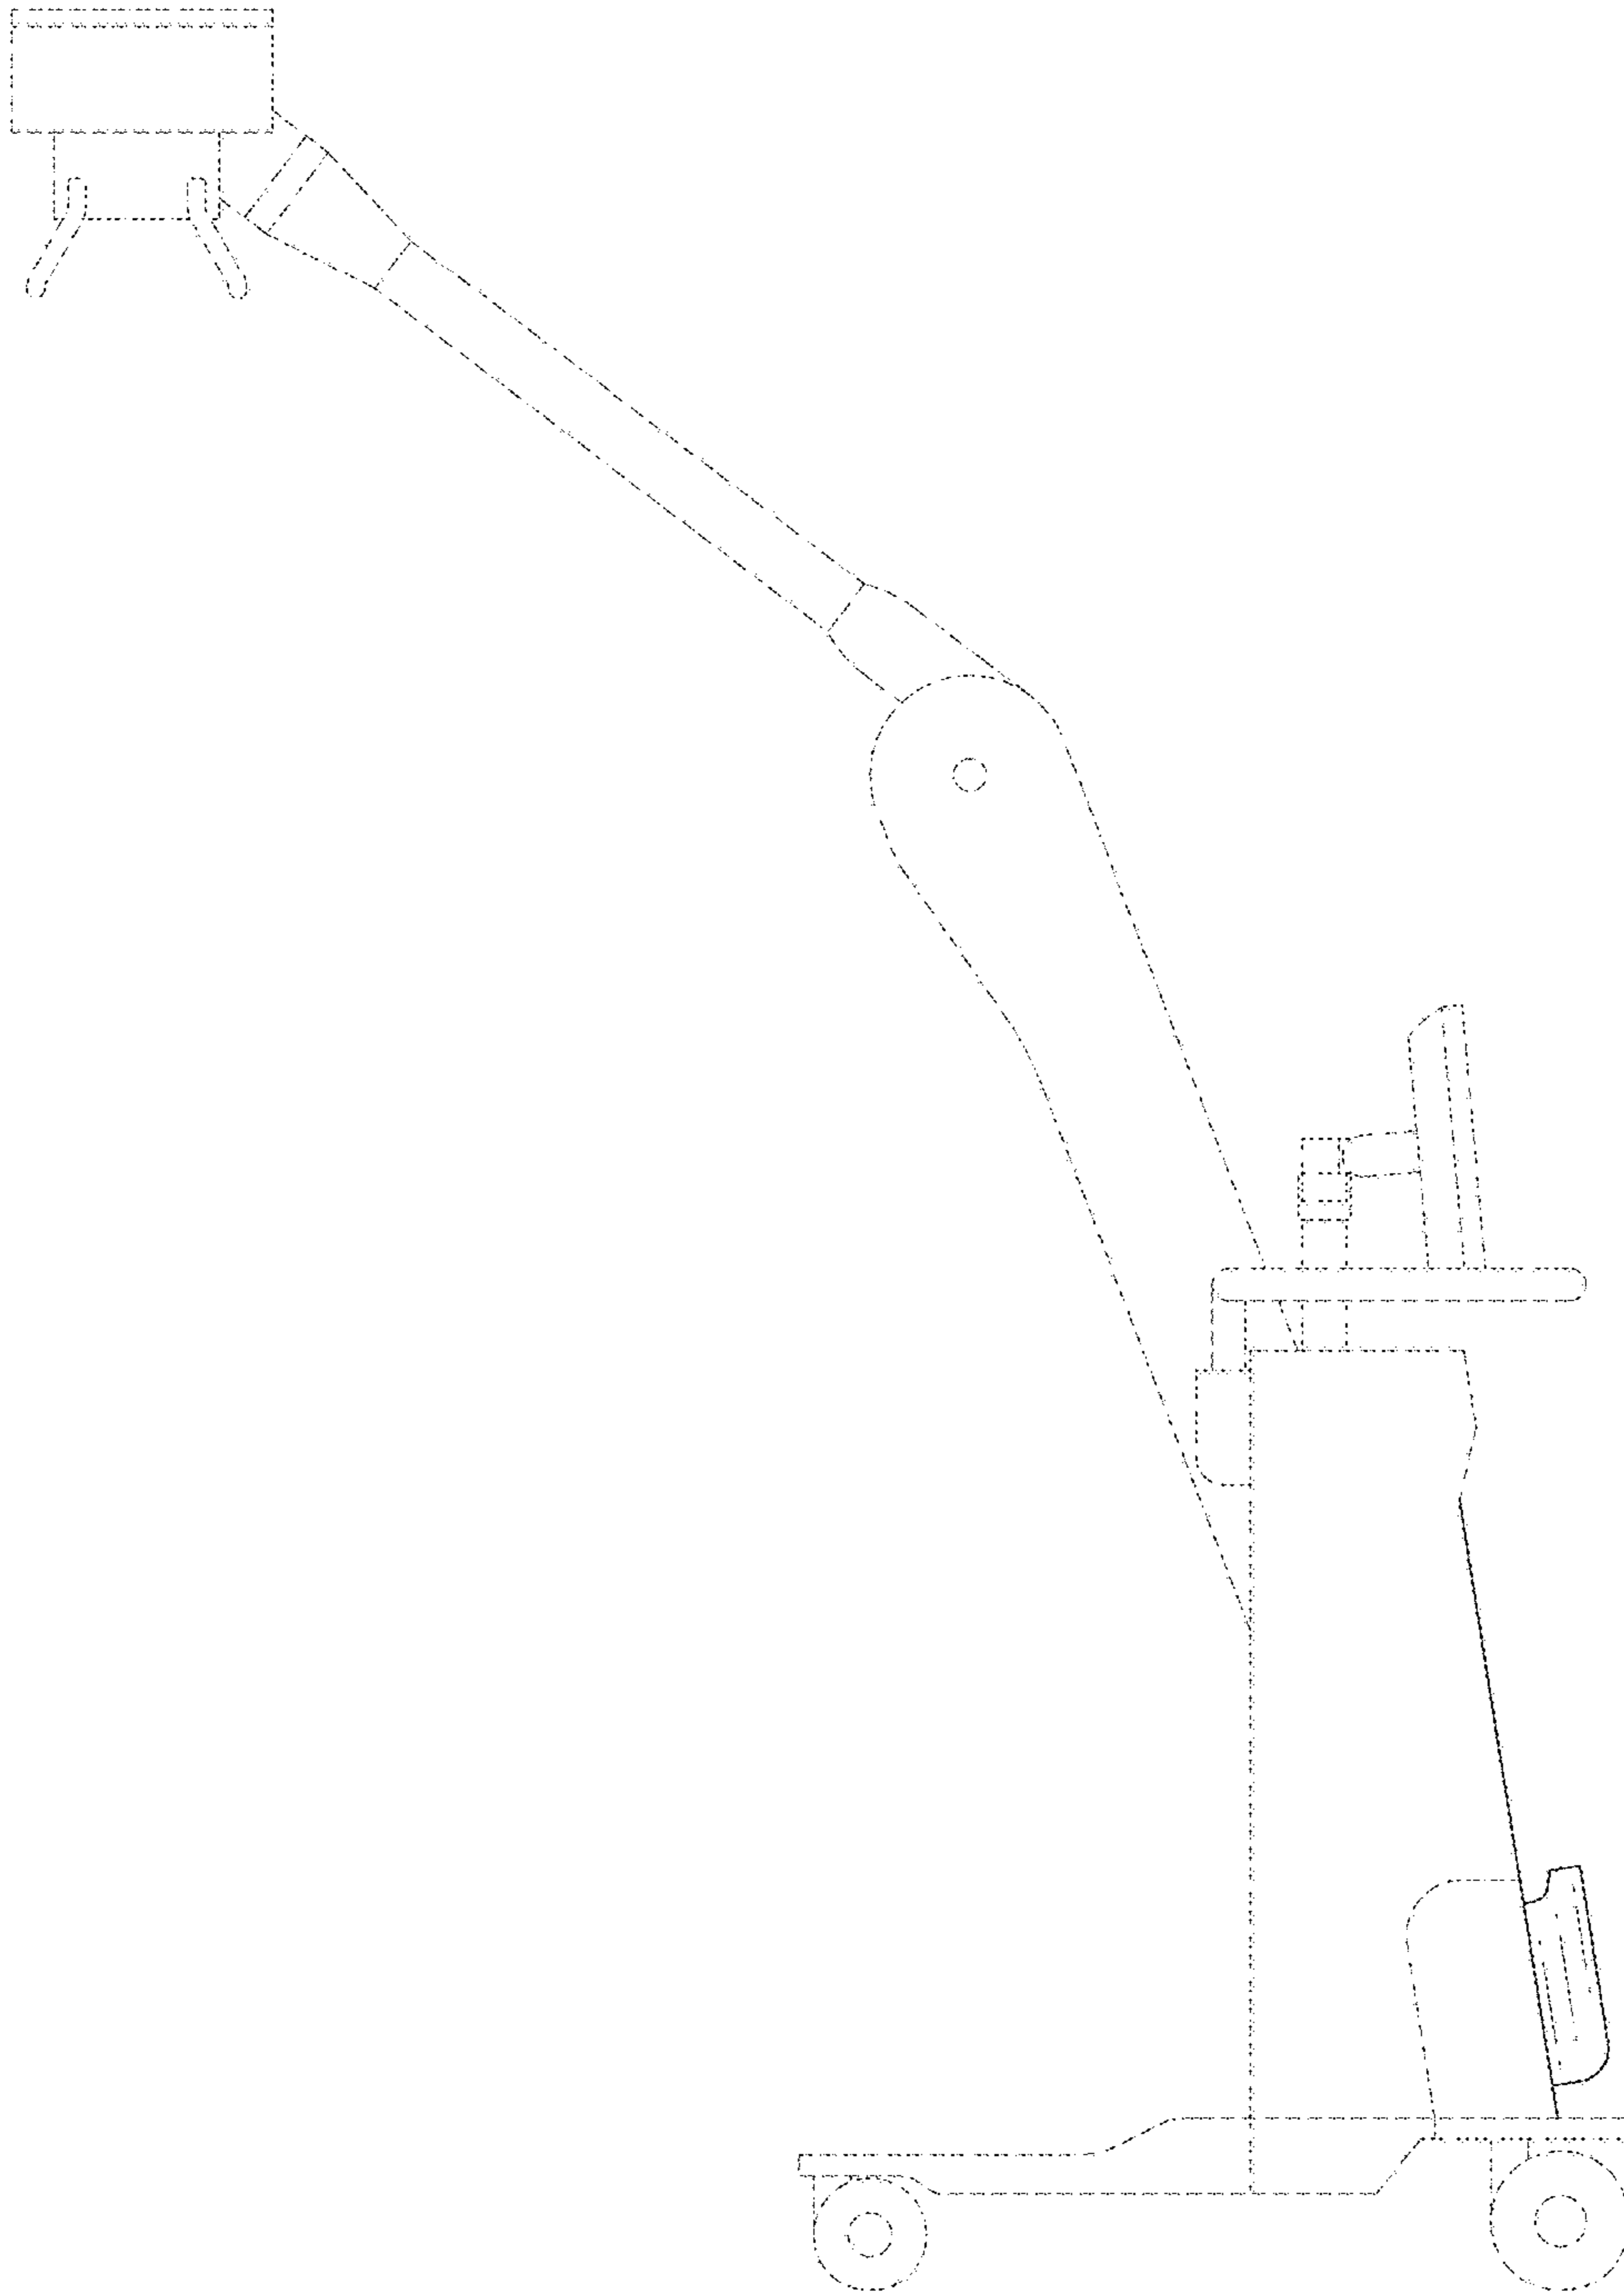


FIG. 9

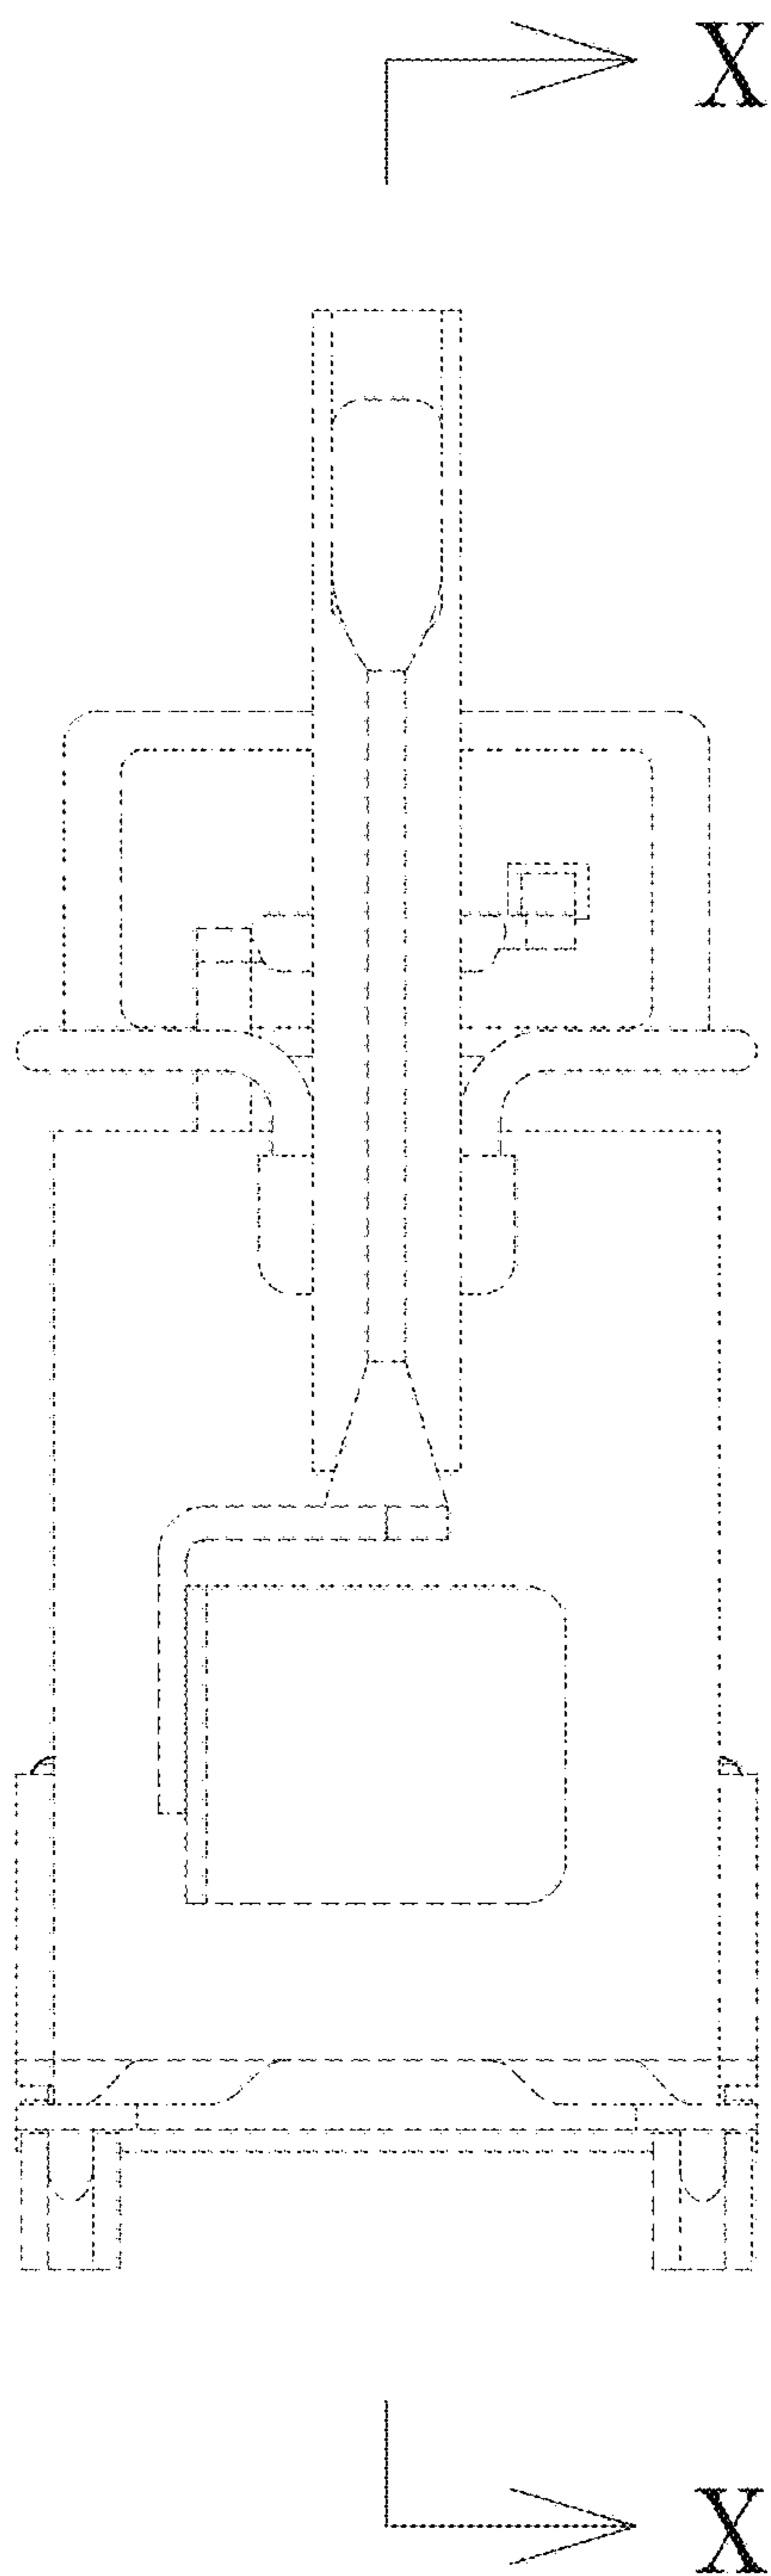


FIG. 10

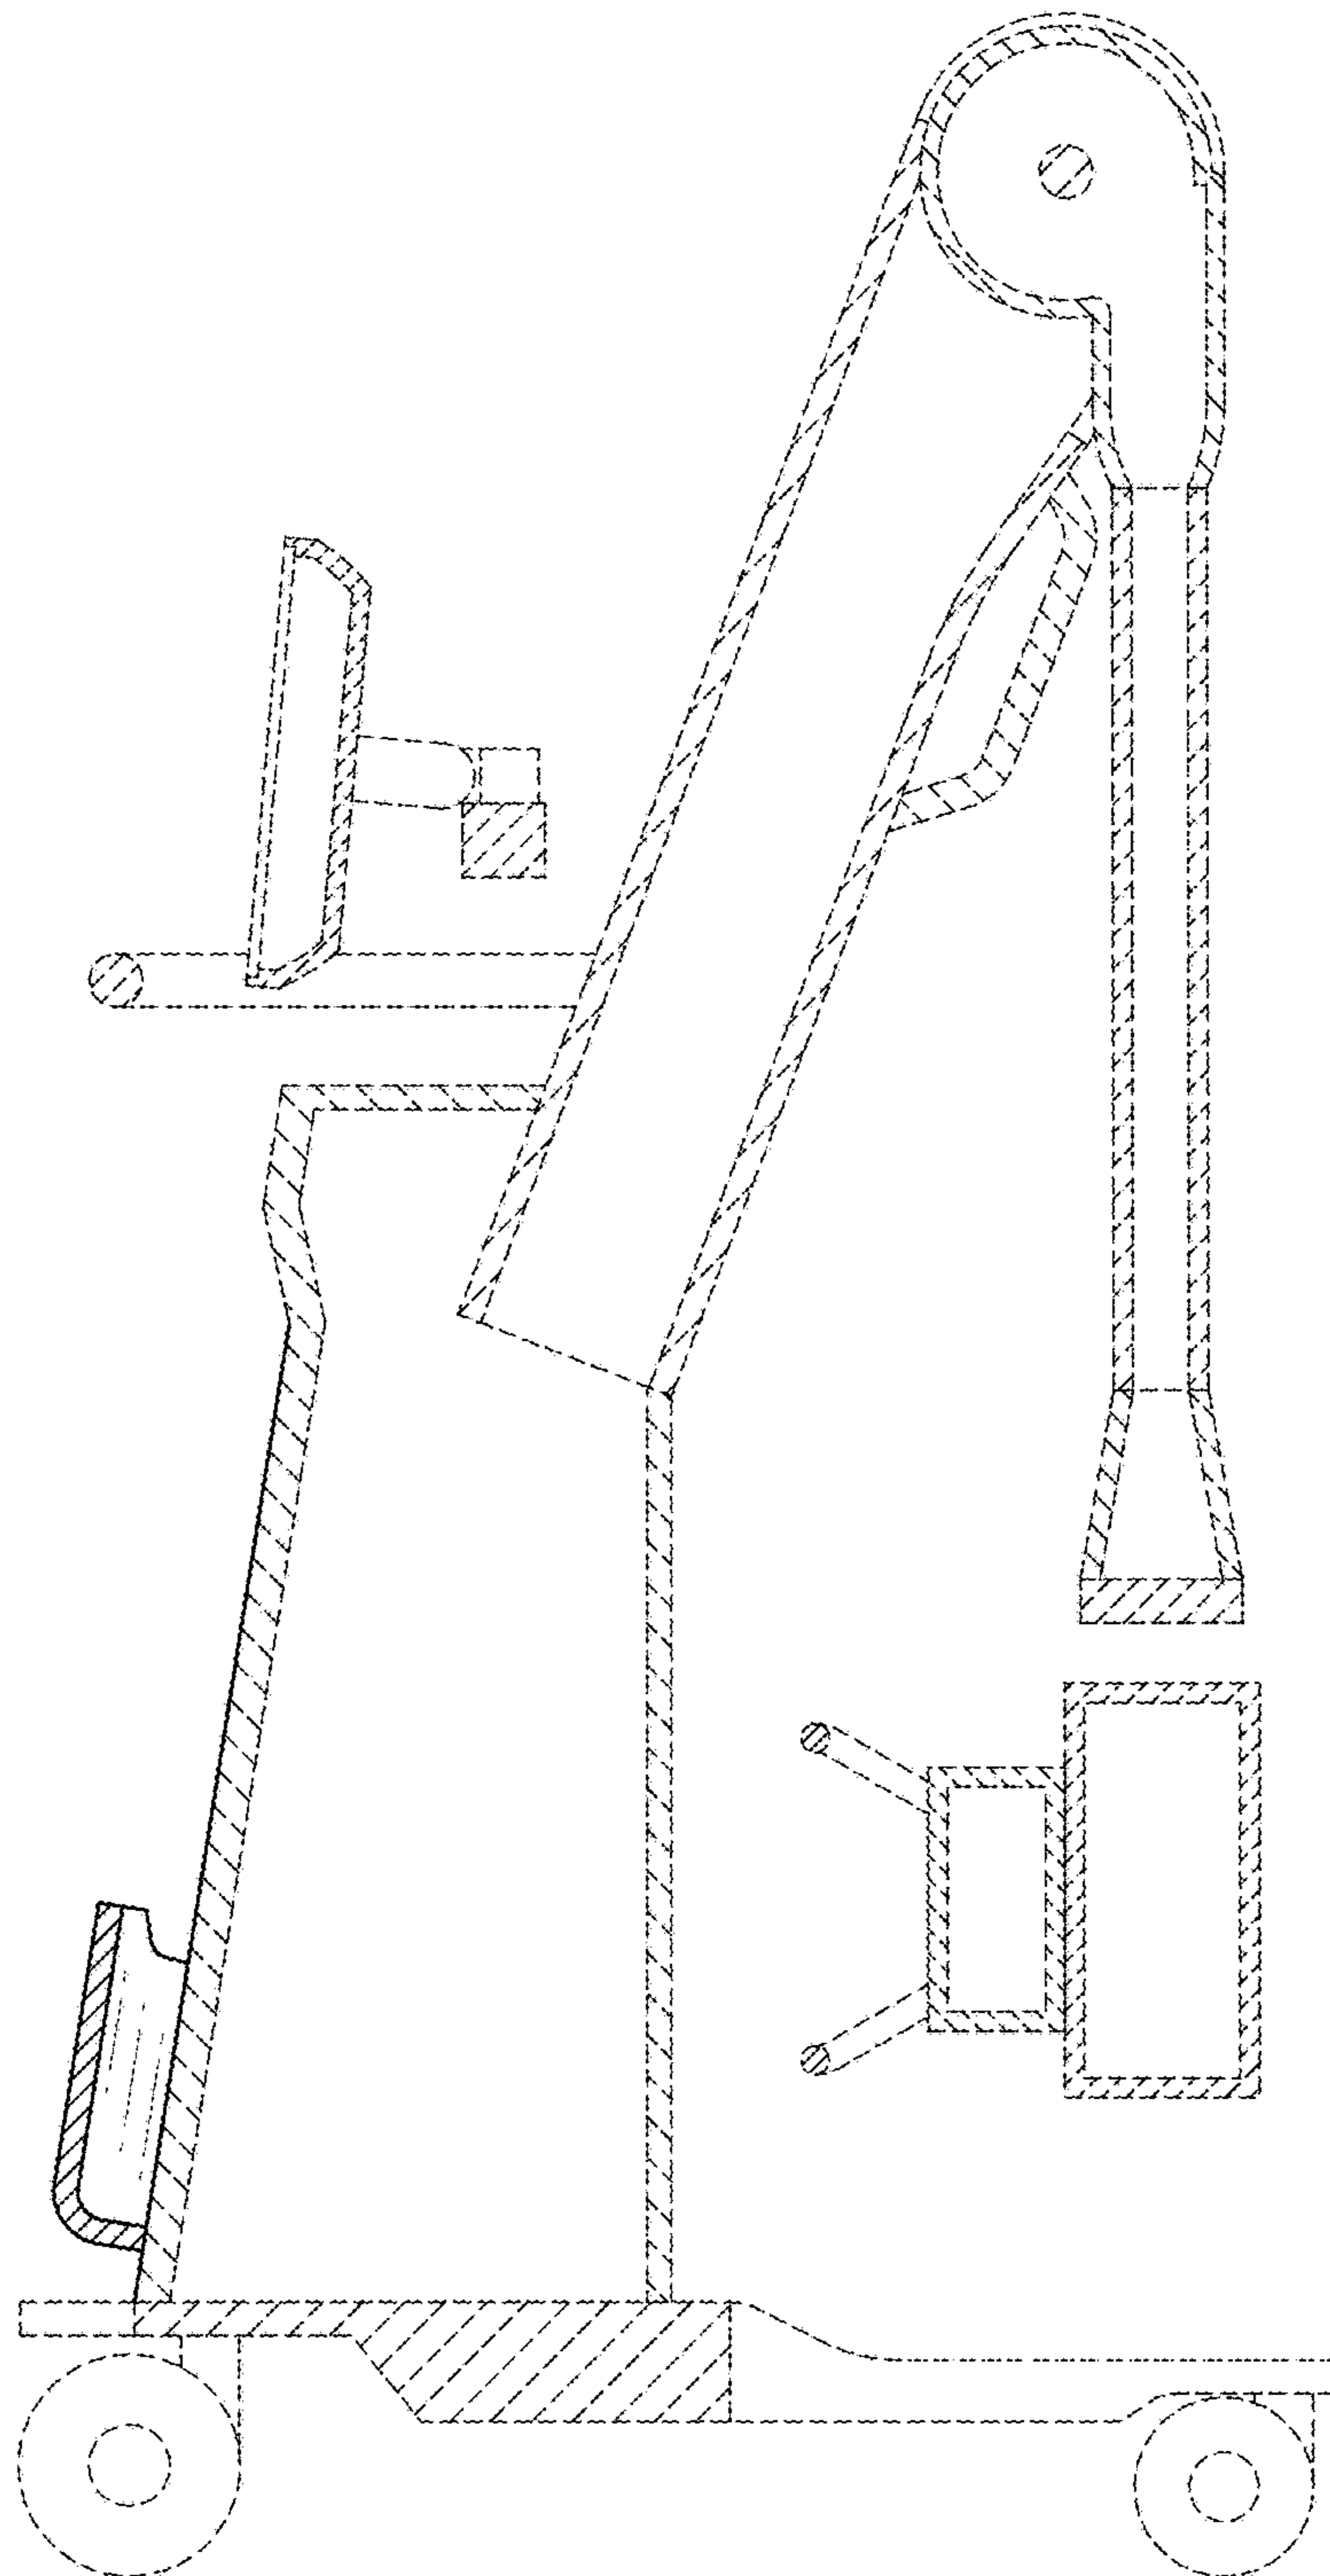


FIG. 11

