



US00D797280S

(12) **United States Design Patent** (10) **Patent No.:** **US D797,280 S**  
**Kyvik** (45) **Date of Patent:** **\*\* Sep. 12, 2017**

(54) **CATHETER ANCHOR PAD WITH RELEASE LAYER**

D616,983 S 6/2010 Kyvik et al.  
D625,002 S \* 10/2010 Kyvik ..... D24/128  
D715,927 S \* 10/2014 Kyvik ..... D24/128  
D717,946 S \* 11/2014 Kyvik ..... D24/128  
D720,849 S \* 1/2015 Kyvik ..... D24/128

(Continued)

(71) Applicant: **Kurt T. Kyvik**, Satellite Beach, FL (US)

*Primary Examiner* — David Muller  
(74) *Attorney, Agent, or Firm* — Thomas C. Saitta

(72) Inventor: **Kurt T. Kyvik**, Satellite Beach, FL (US)

(73) Assignee: **KT KYVIK, LLC**, Satellite Beach, FL (US)

(57) **CLAIM**

The ornamental design for a catheter anchor pad with release layer, as shown and described.

(\*\*) Term: **15 Years**

**DESCRIPTION**

(21) Appl. No.: **29/576,776**

(22) Filed: **Sep. 7, 2016**

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/128**

(58) **Field of Classification Search**  
USPC ..... D24/127–131, 112–114, 133, 186;  
606/181, 185; 604/264, 523–528, 272,  
604/187, 158, 164.01–164.11, 181, 184,  
604/227; 600/101, 139, 143;  
128/200.24, 207.14, 207.15  
CPC .. A61M 25/065; A61M 5/42; A61M 25/0612;  
A61M 25/00; A61M 39/00; A61M 27/00;  
A61M 25/0043; A61M 25/0067; A61M  
25/0097; A61F 2/958

See application file for complete search history.


FIG. 1 is a perspective view of the catheter anchor pad with release layer, shown in the open position.  
FIG. 2 is a top view of the catheter anchor pad with release layer, shown in the closed position.  
FIG. 3 is a bottom view of the catheter anchor pad with release layer, shown in the closed position.  
FIG. 4 is a left side view of the catheter anchor pad with release layer, shown in the closed position.  
FIG. 5 is a right side view of the catheter anchor pad with release layer, shown in the closed position.  
FIG. 6 is a front view of the catheter anchor pad with release layer, shown in the closed position, the rear view being a mirror image.  
FIG. 7 is a top view of the catheter anchor pad with release layer removed, shown in the closed position.  
FIG. 8 is a bottom view of the catheter anchor pad with release layer removed, shown in the closed position.  
FIG. 9 is a left side view of the catheter anchor pad with release layer removed, shown in the closed position.  
FIG. 10 is a right side view of the catheter anchor pad with release layer removed, shown in the closed position; and,  
FIG. 11 is a front view of the catheter anchor pad with release layer removed, shown in the closed position, the rear view being a mirror image.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D375,356 S \* 11/1996 Bierman ..... 604/180  
D492,411 S \* 6/2004 Bierman ..... D24/128  
D503,977 S \* 4/2005 Bierman ..... D24/128  
D528,206 S \* 9/2006 Bierman ..... D24/128  
D608,887 S \* 1/2010 Kyvik ..... D24/130  
D616,091 S \* 5/2010 Kyvik ..... D24/128  
D616,542 S \* 5/2010 Kyvik ..... D24/128

**1 Claim, 5 Drawing Sheets**

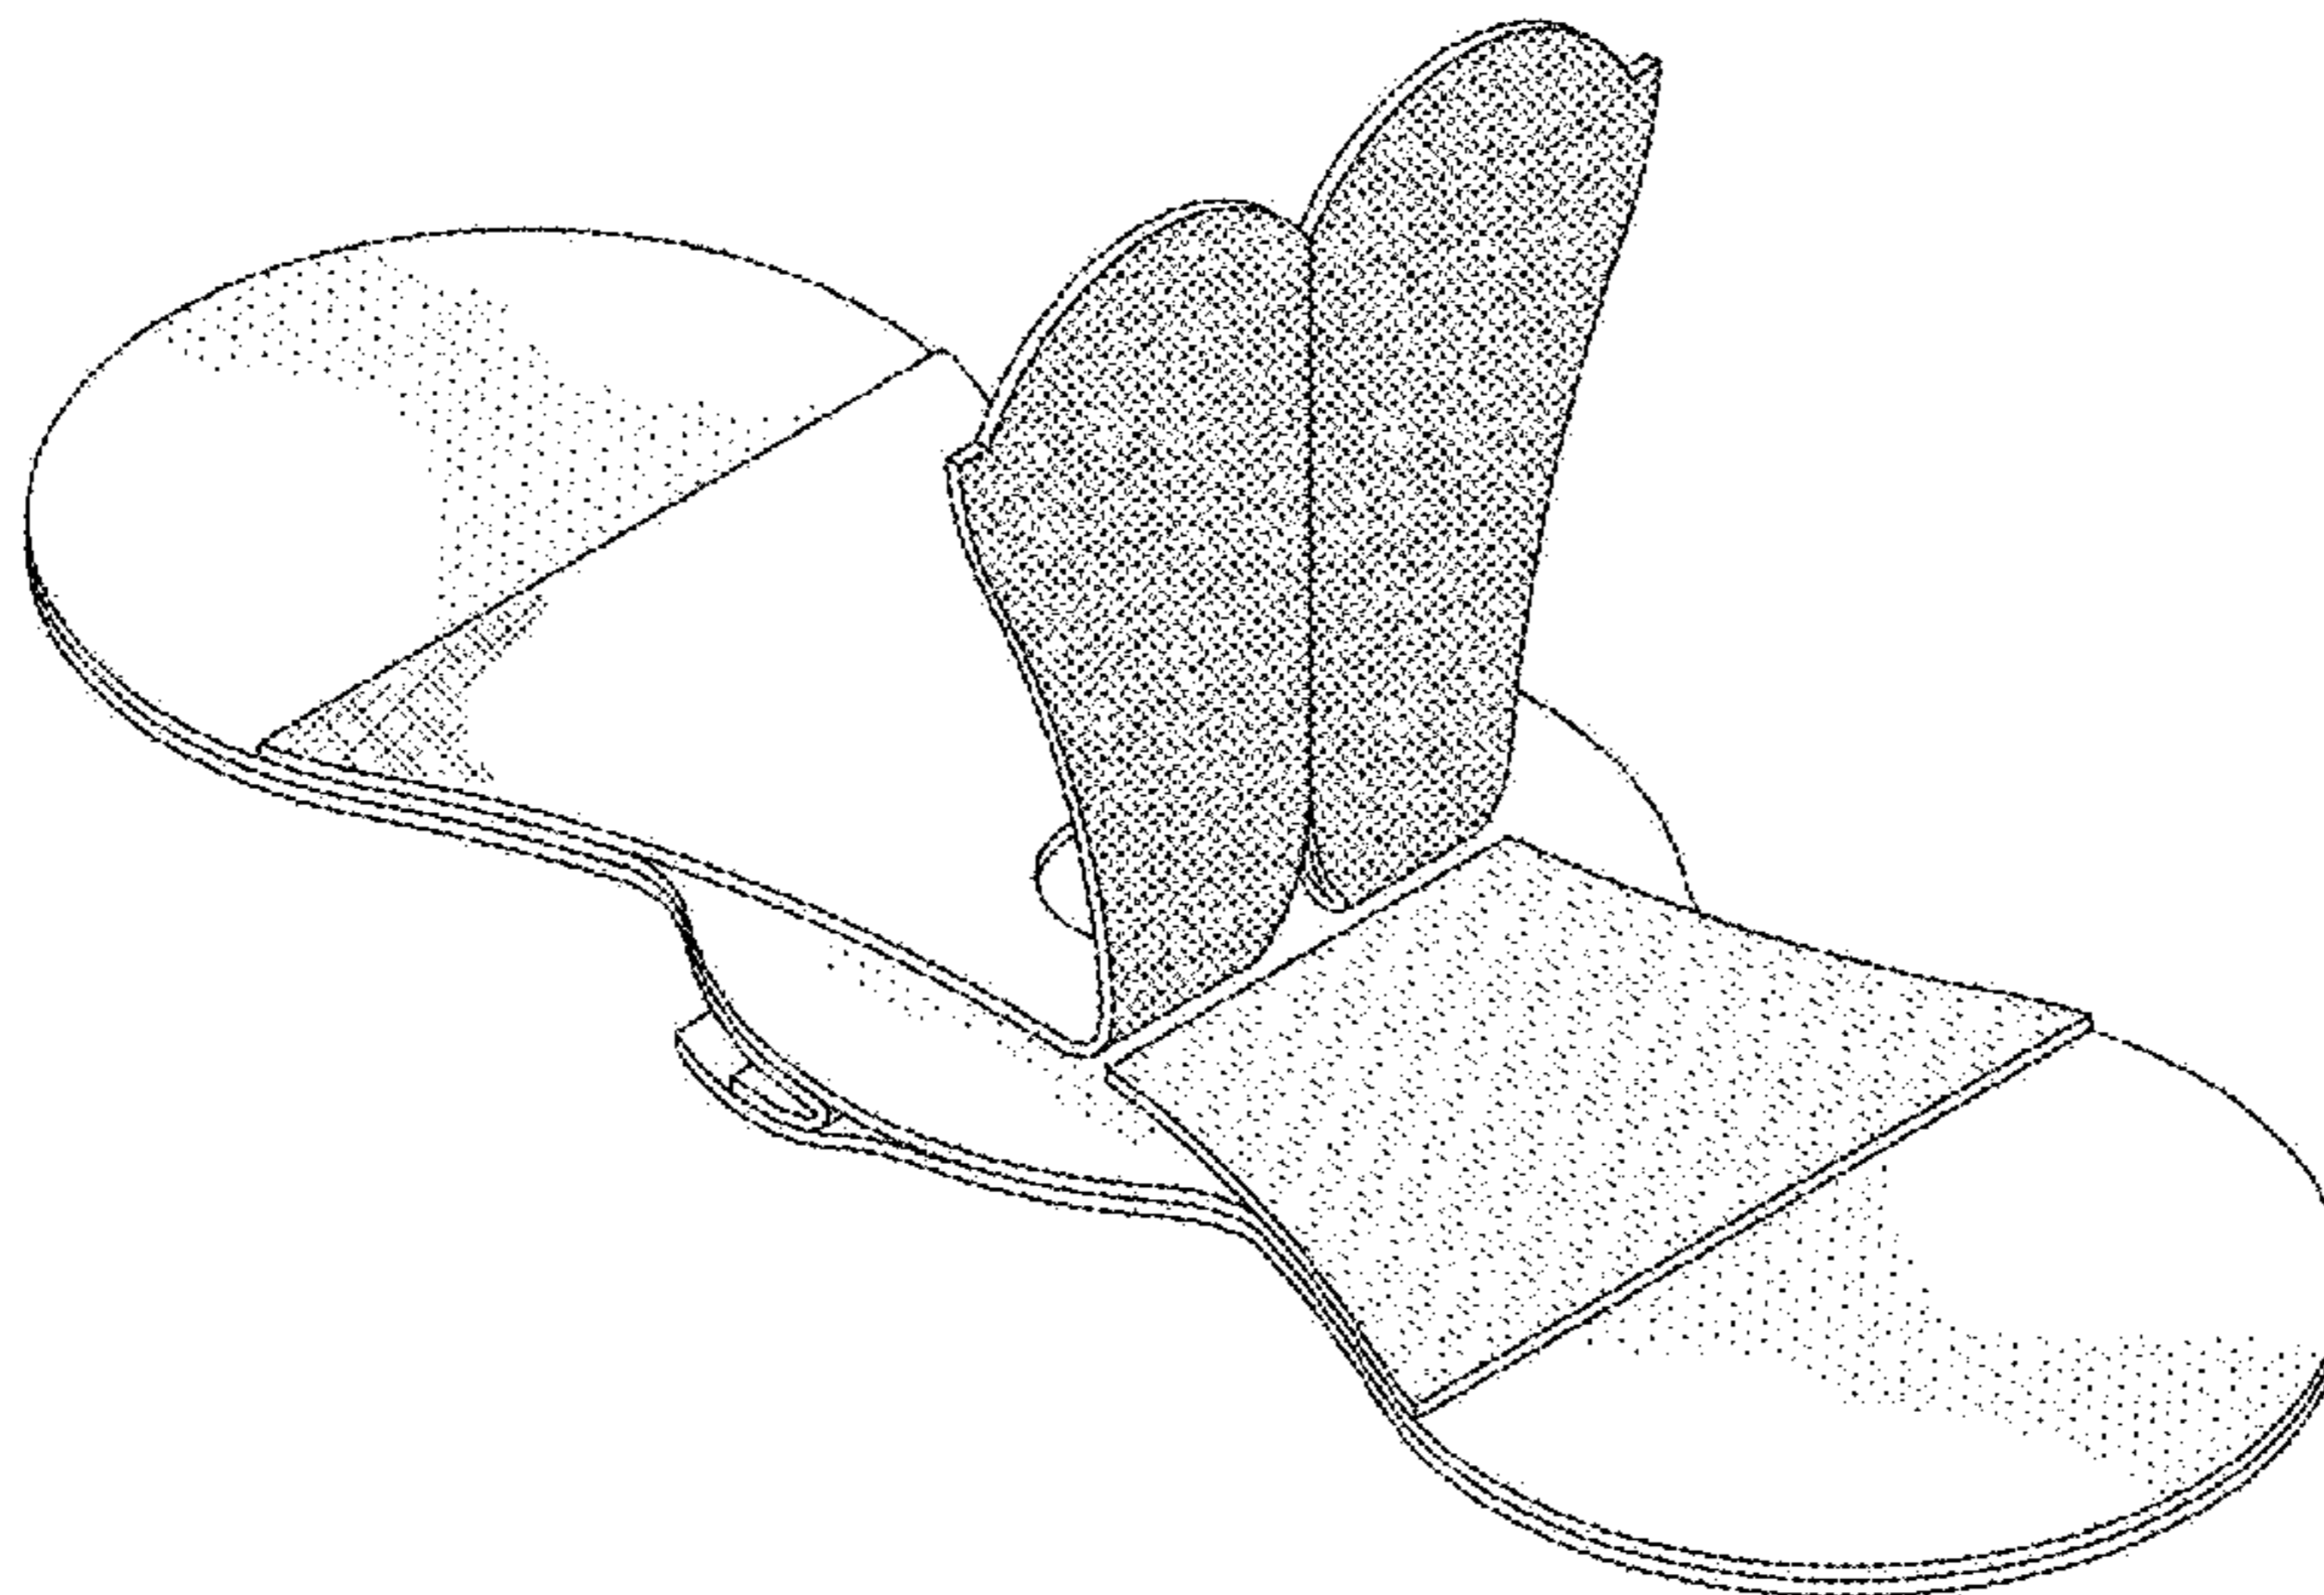


(56)

**References Cited**


U.S. PATENT DOCUMENTS

D755,962 S \* 5/2016 Adams ..... D24/128  
D780,914 S \* 3/2017 Kyvik ..... D24/130


\* cited by examiner

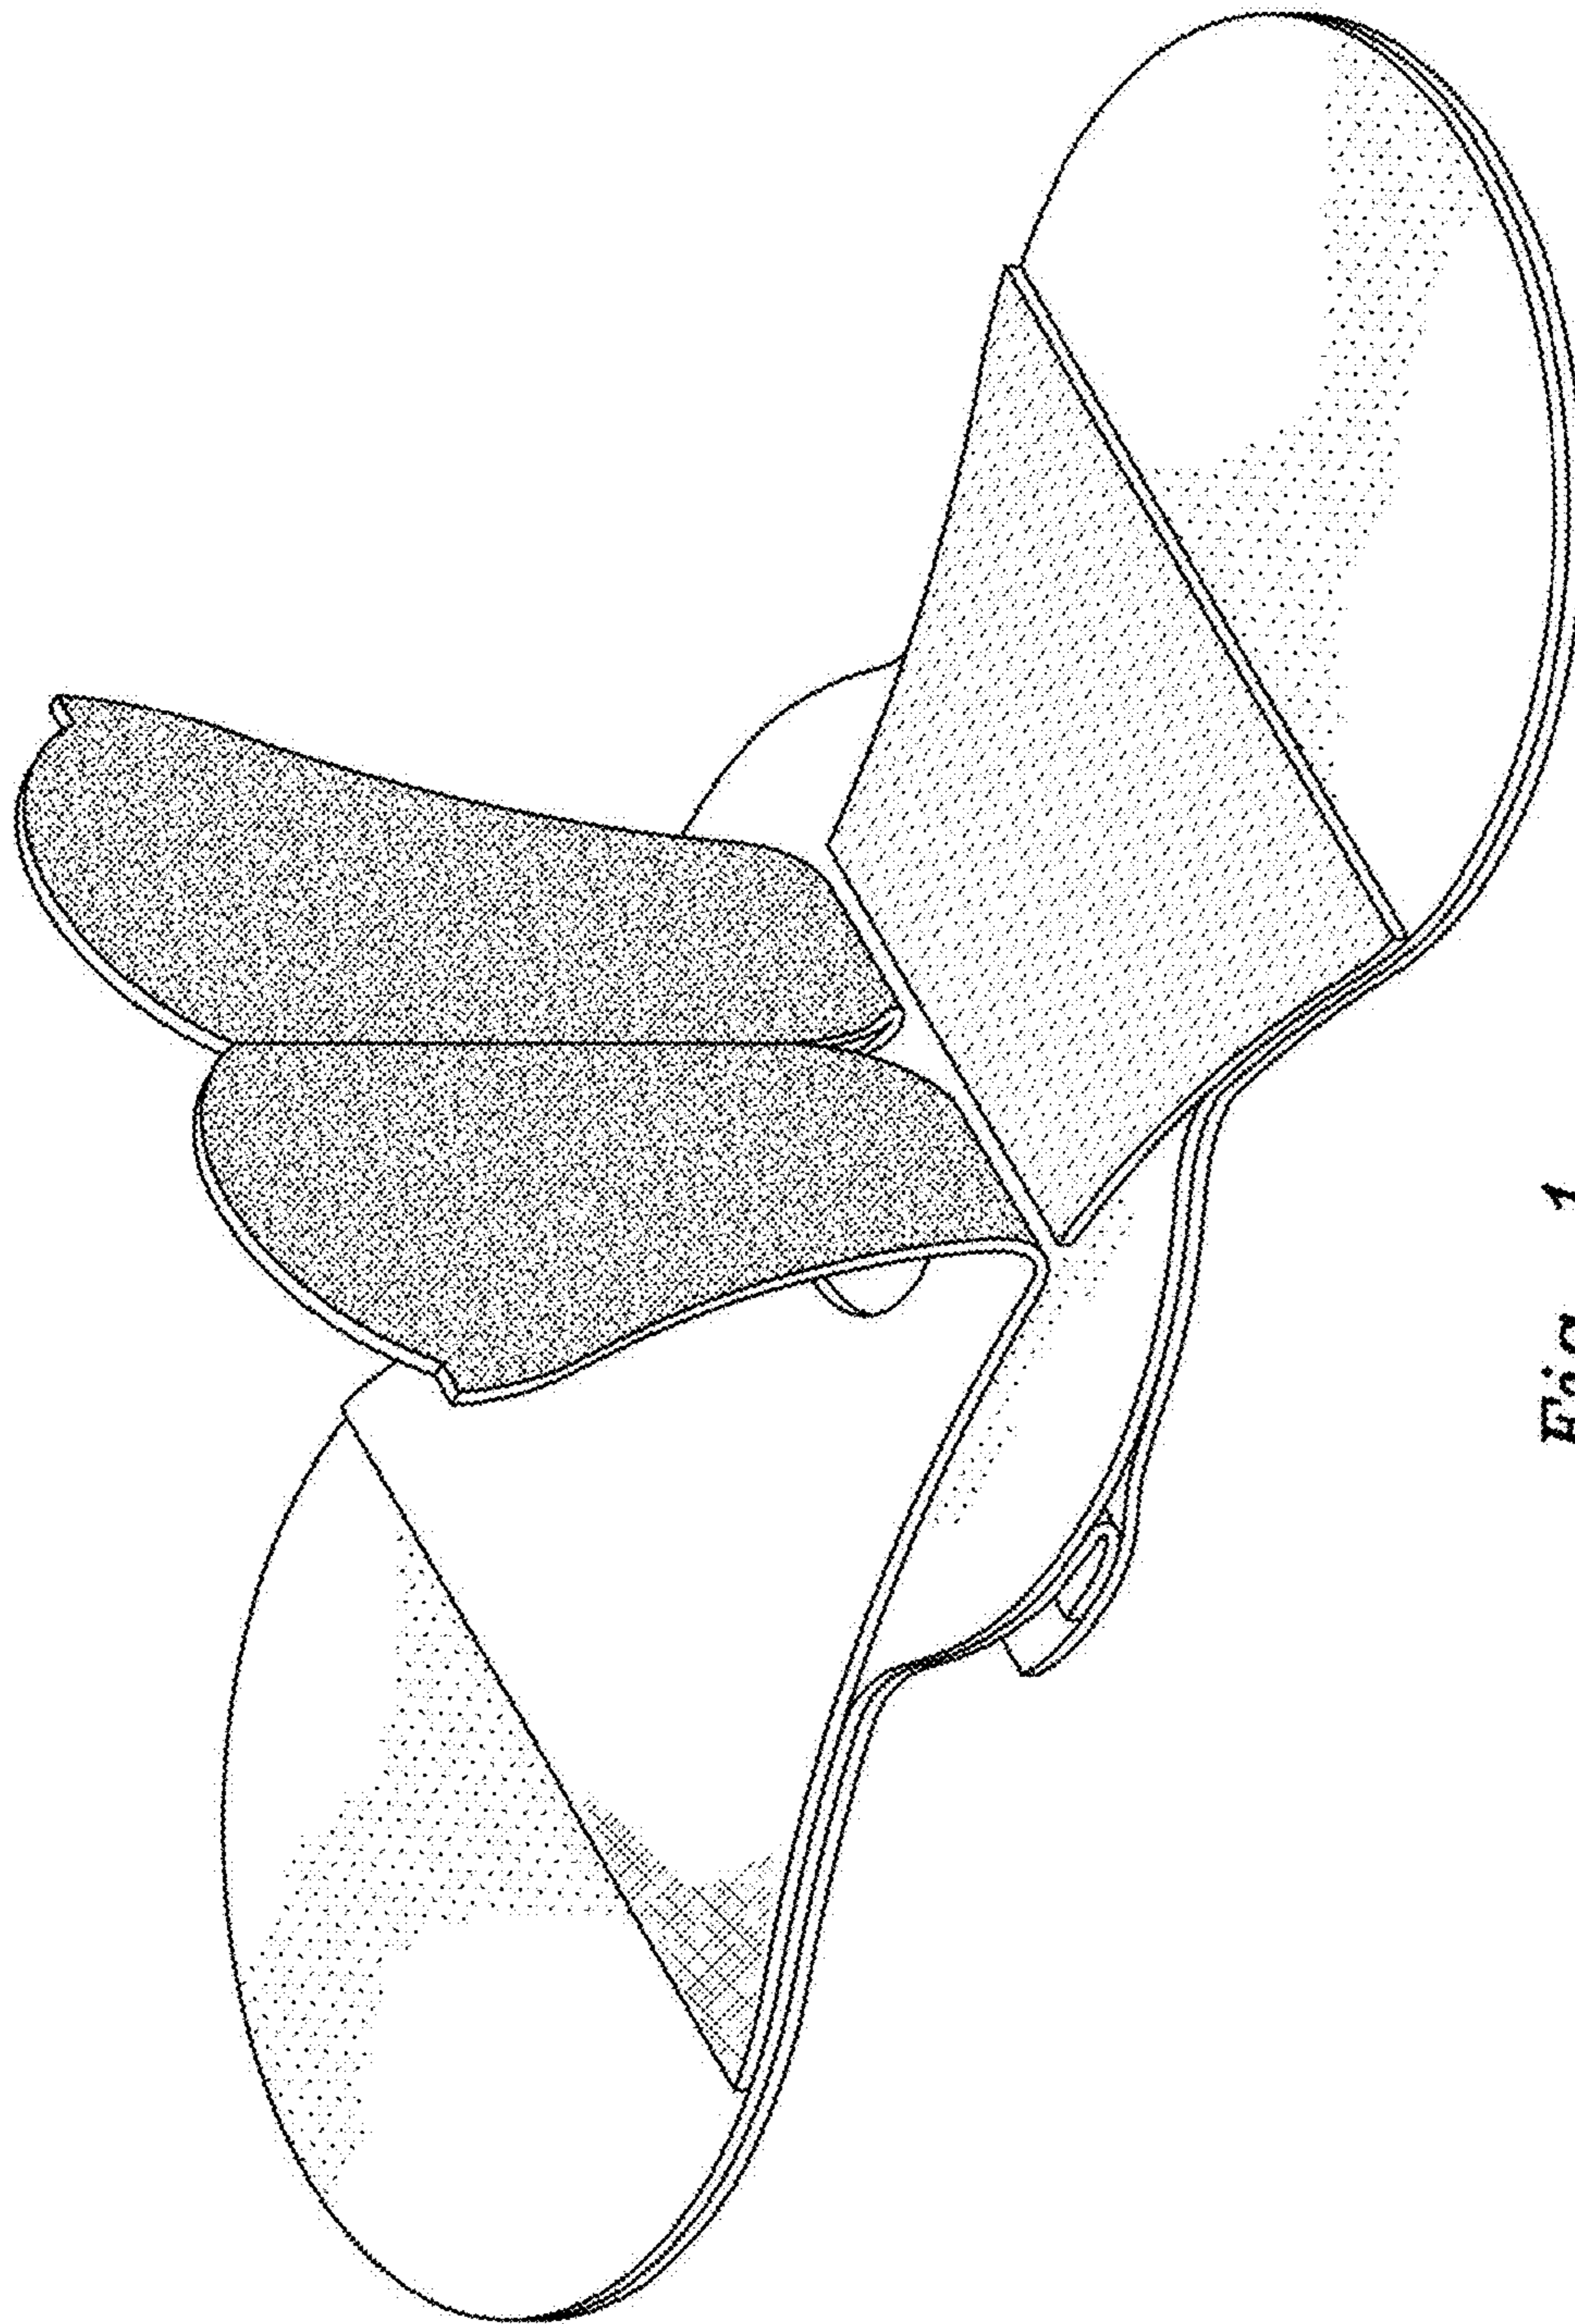


*Fig. 1*

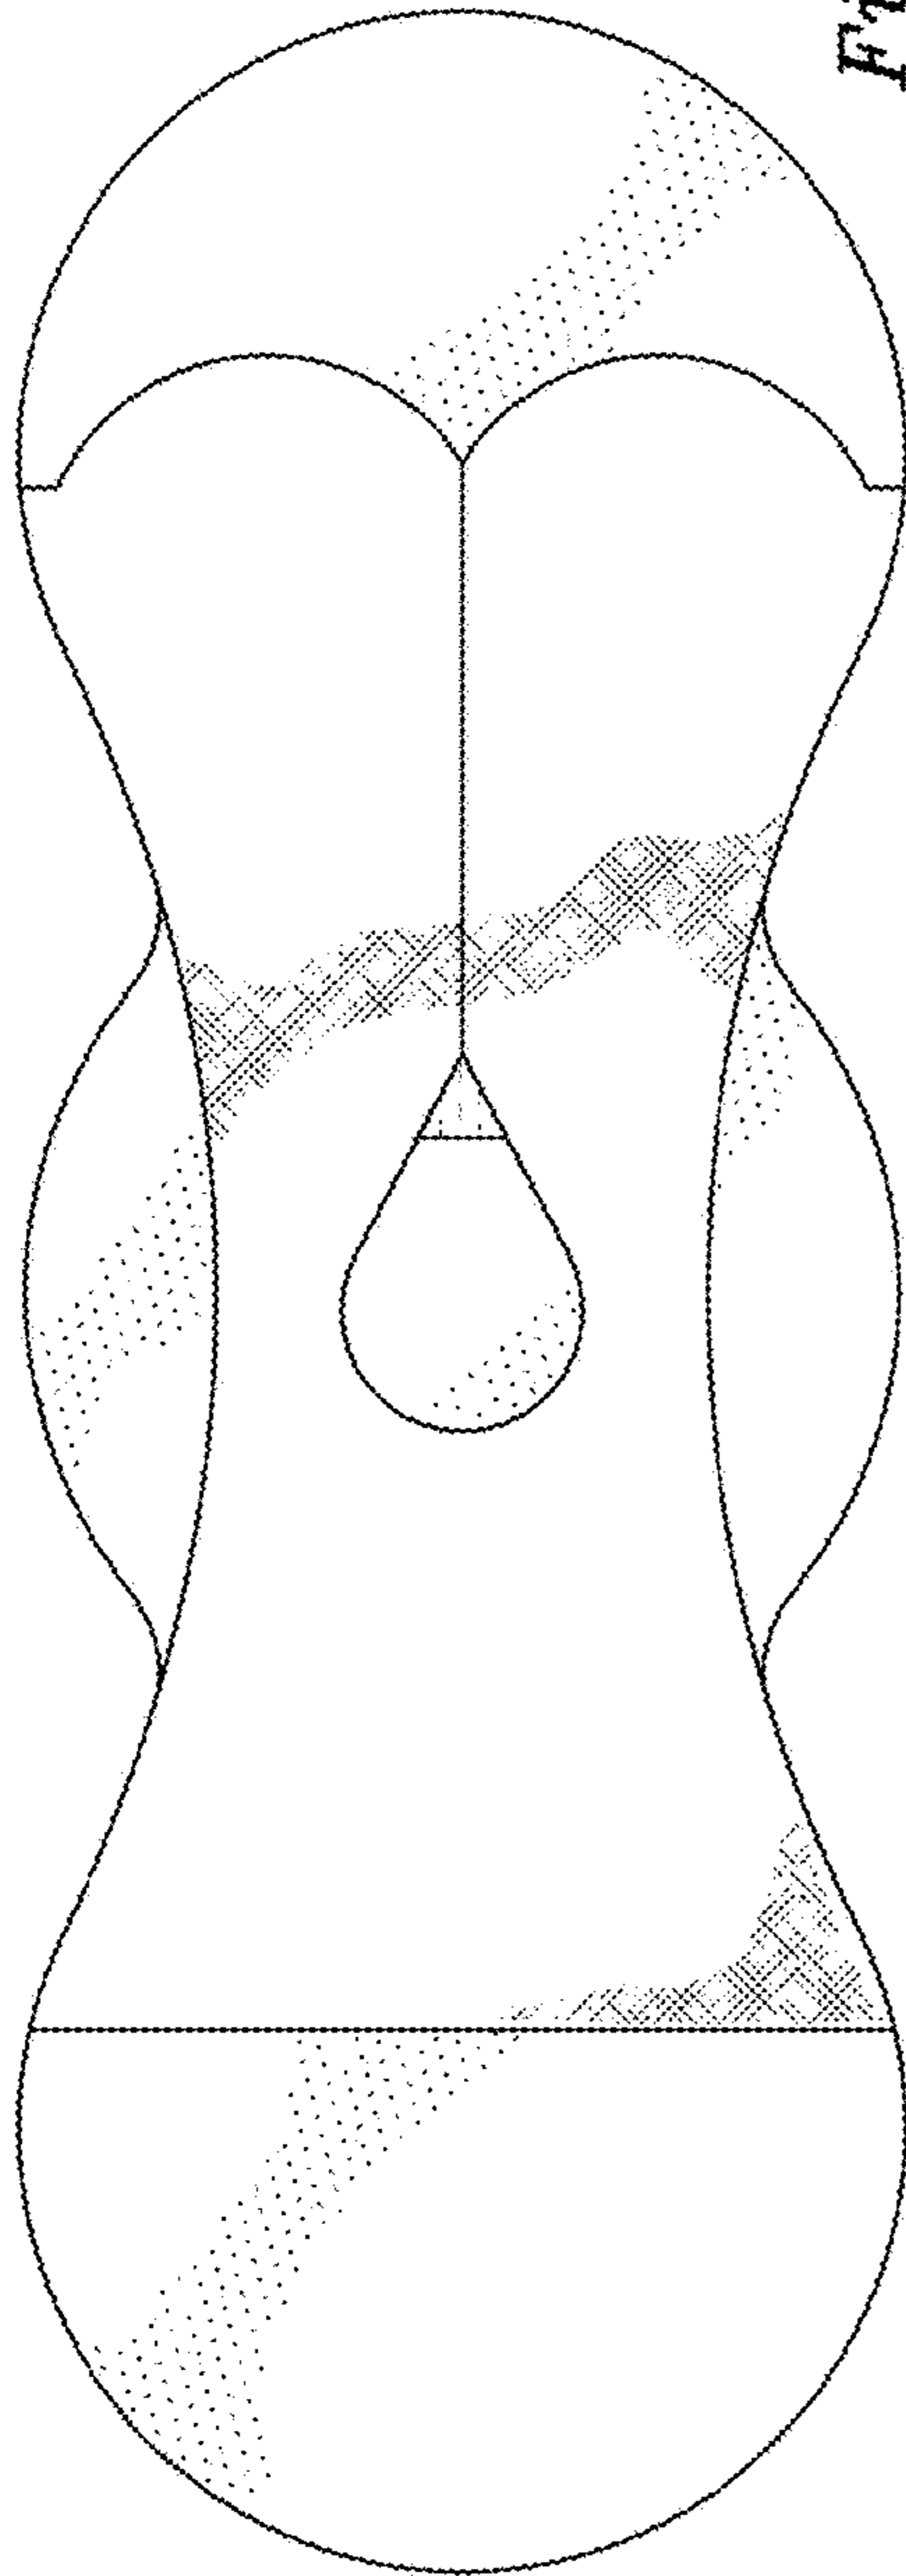


*Fig. 2*

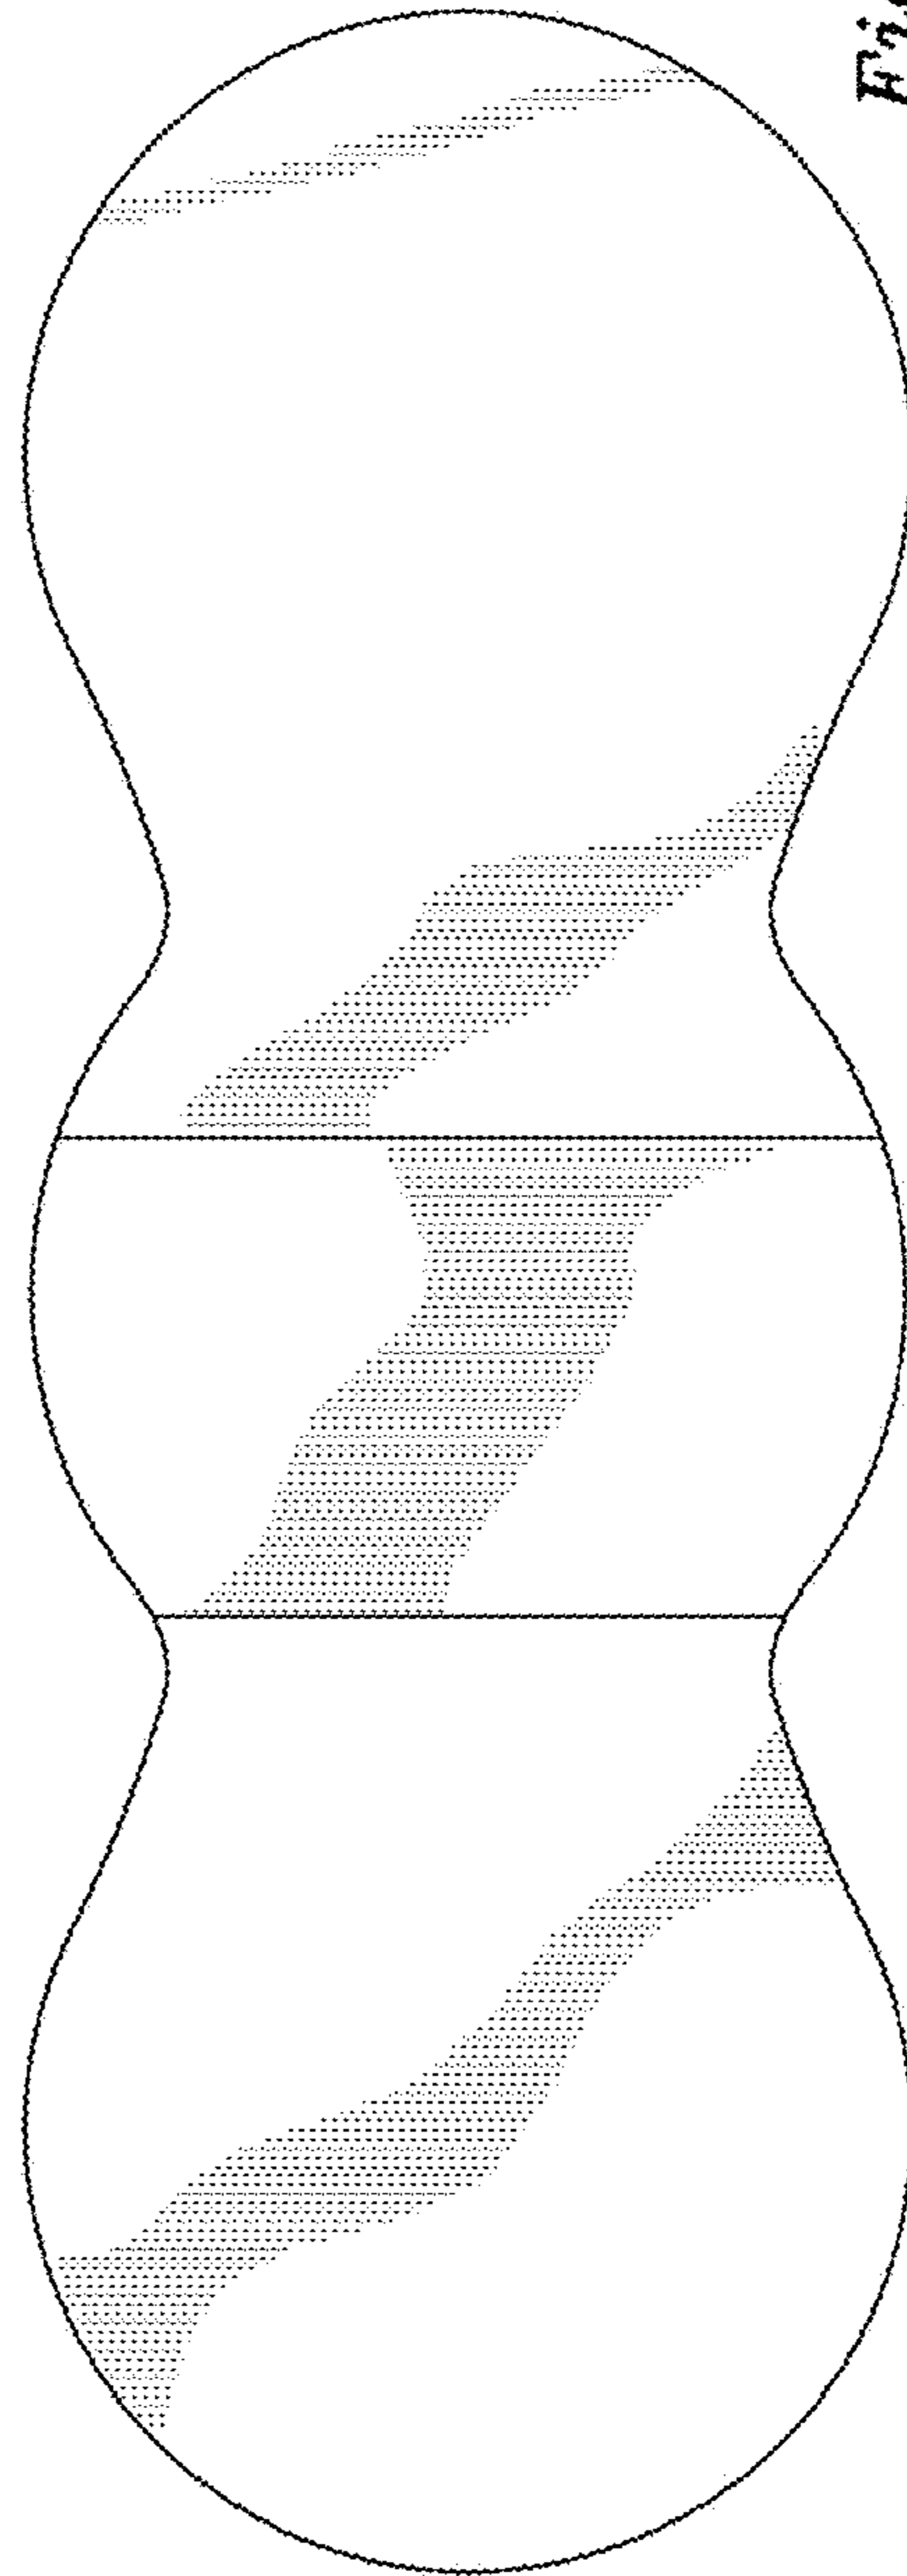


*Fig. 3*

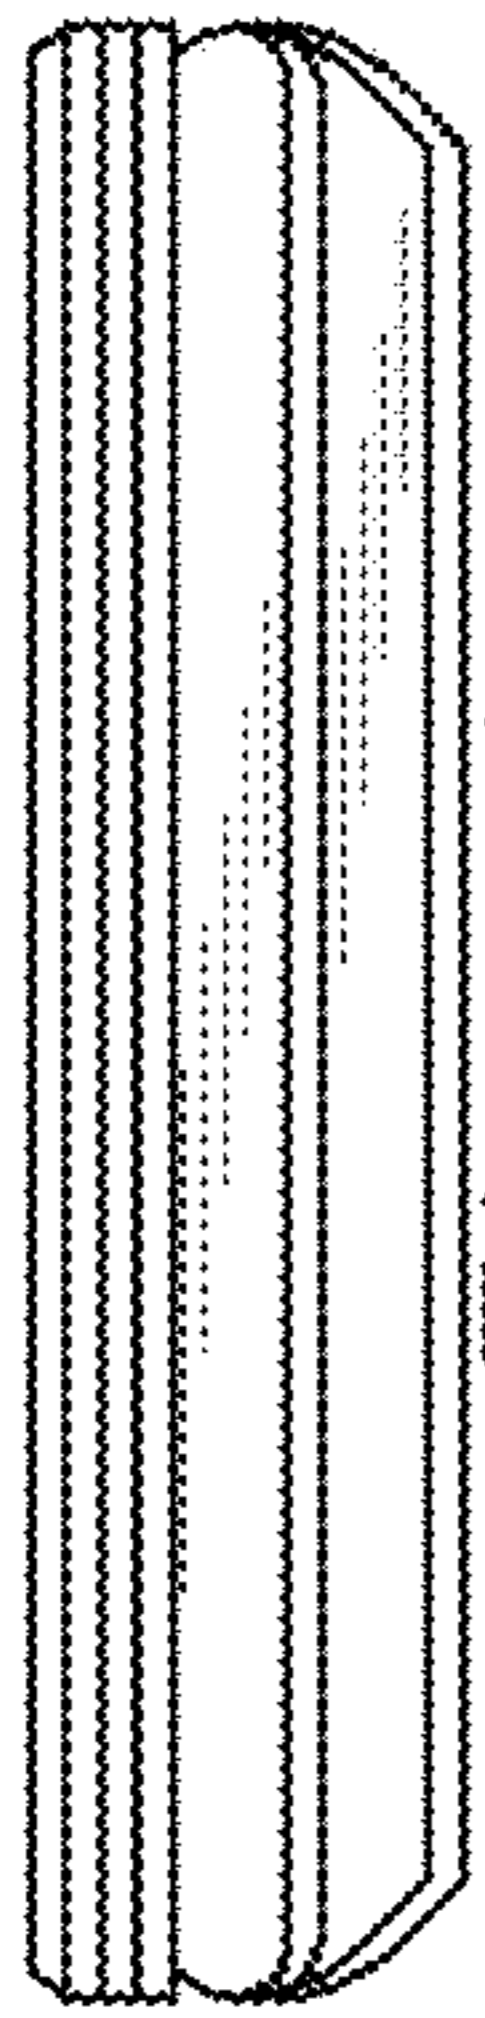



*Fig. 4*

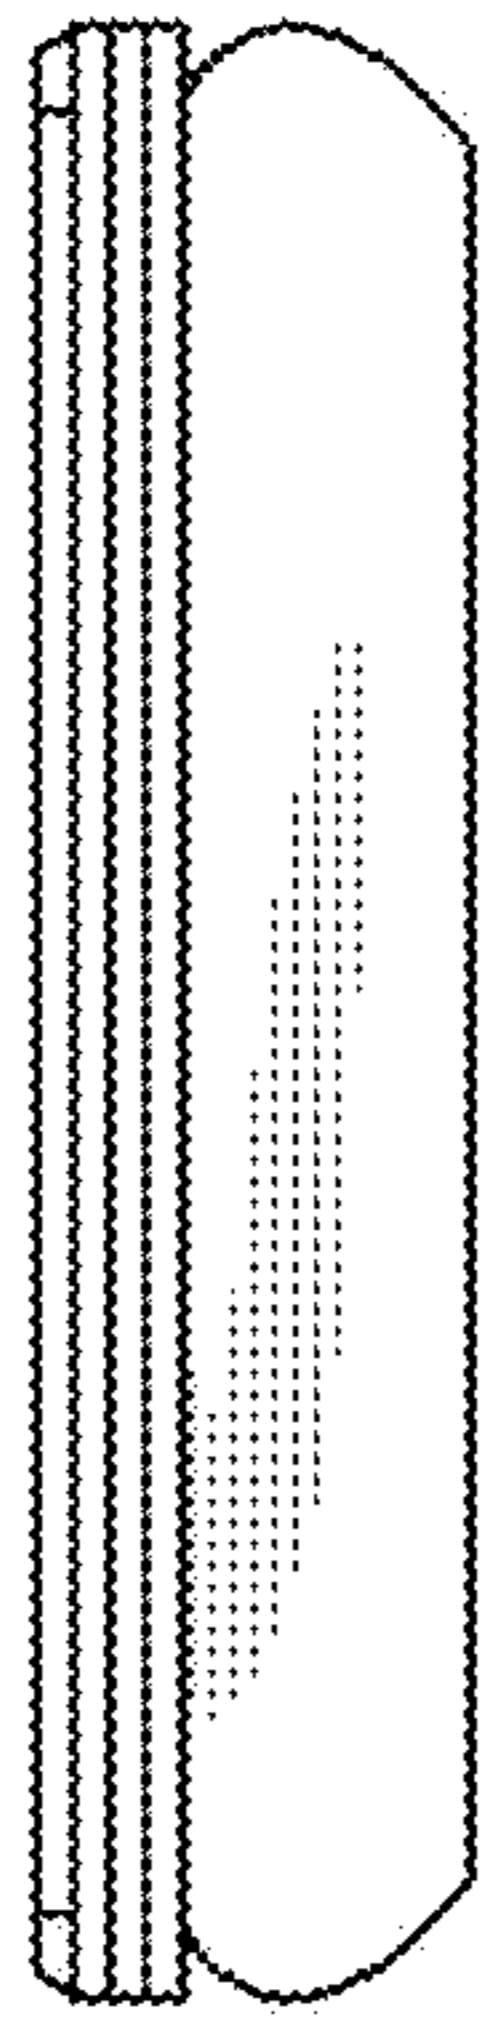


*Fig. 5*

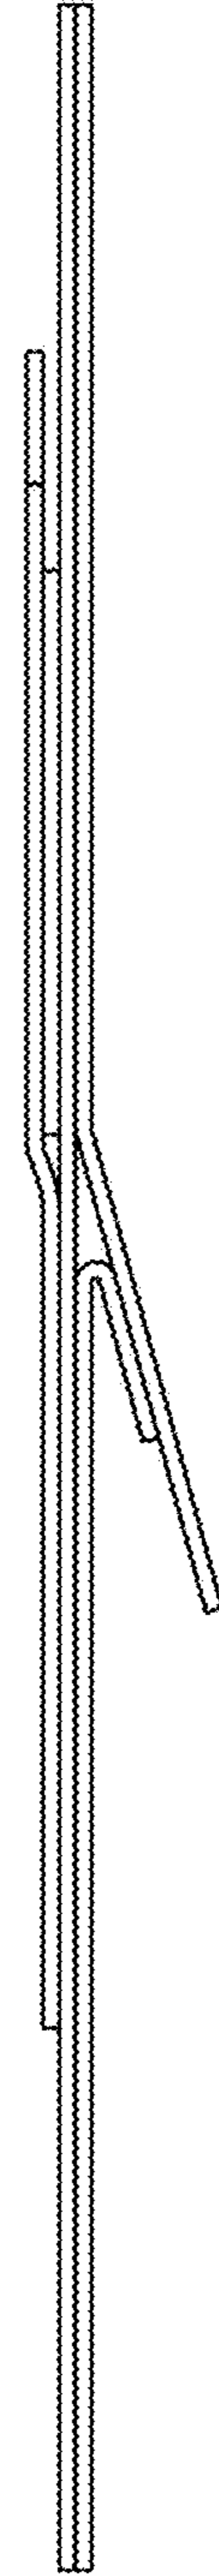

*Fig. 6*

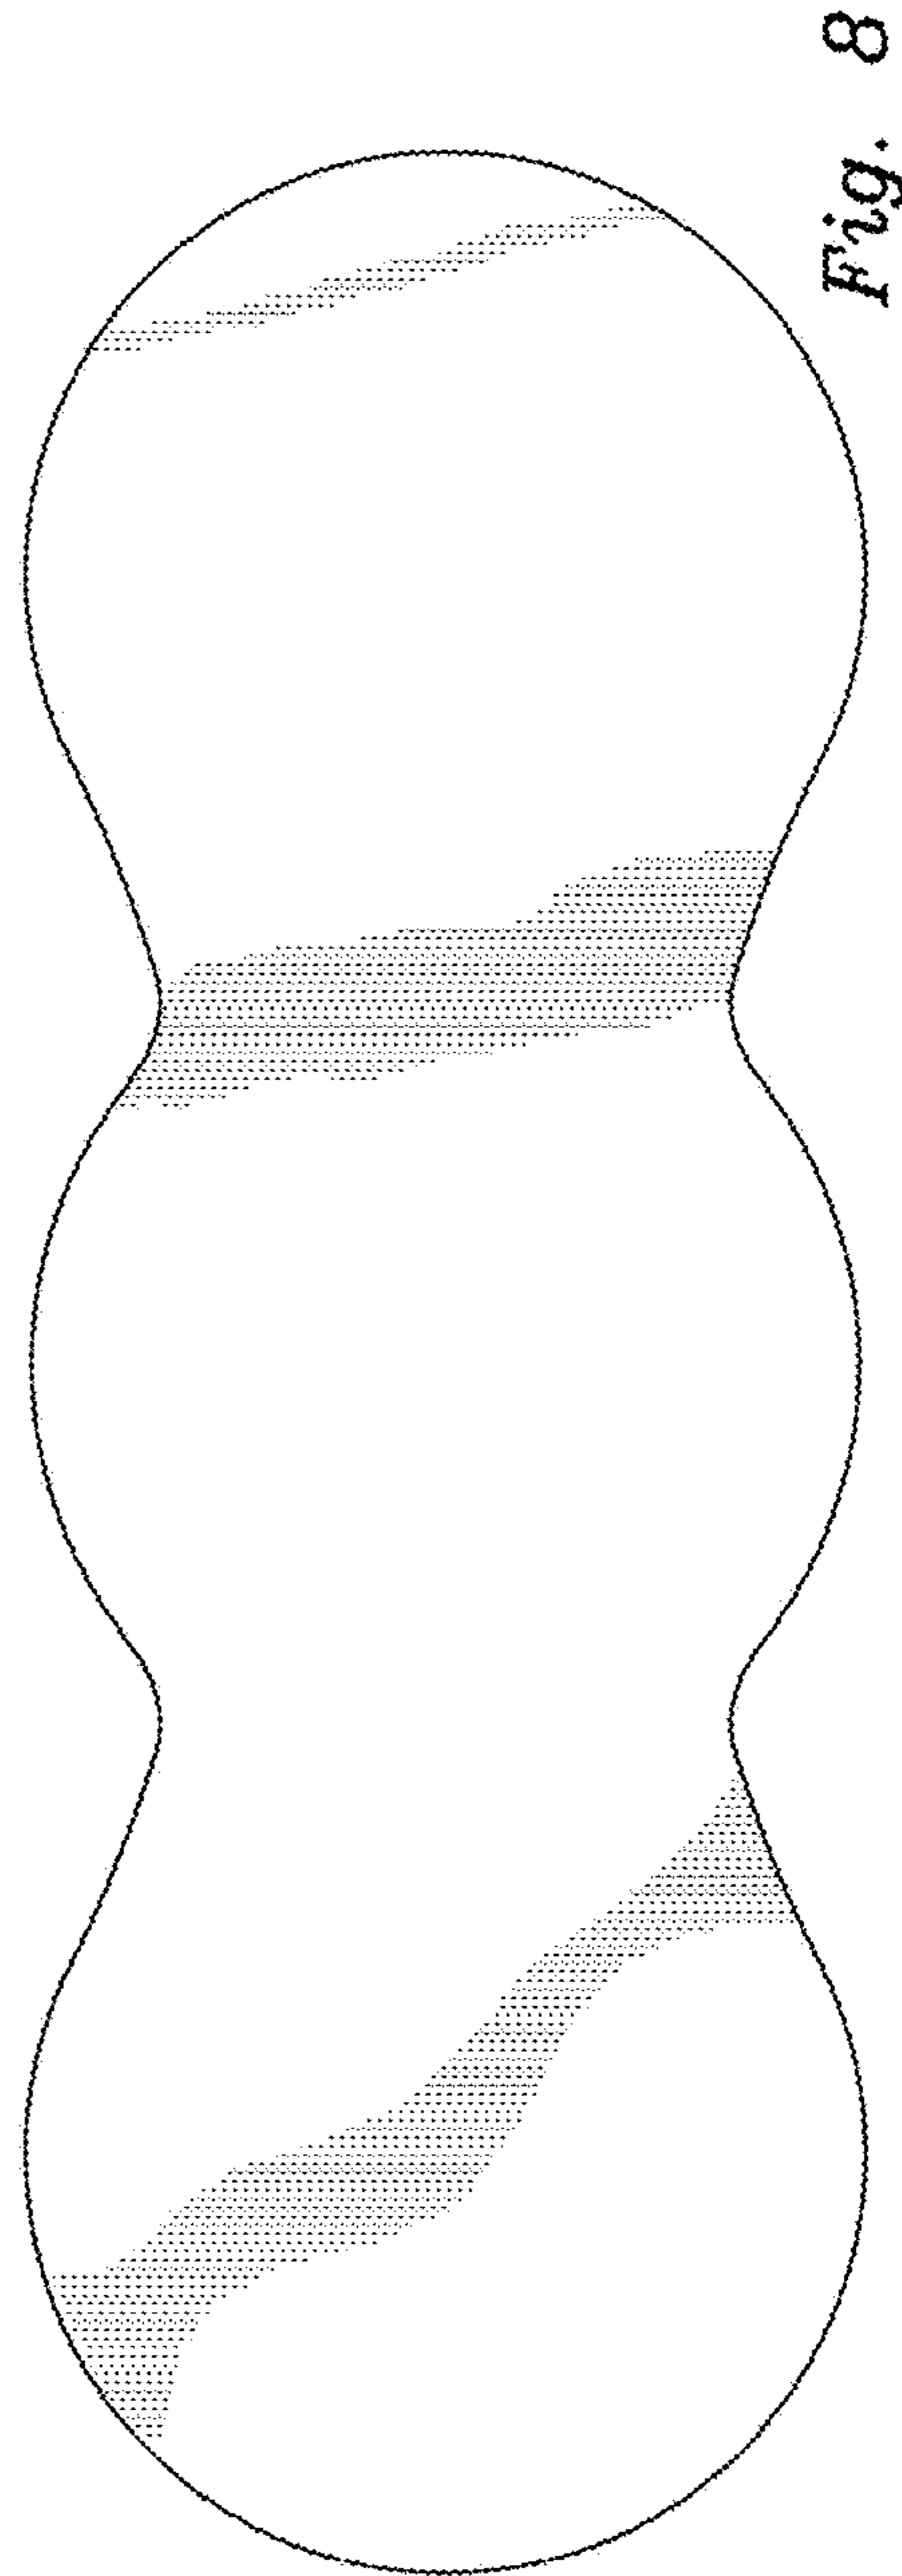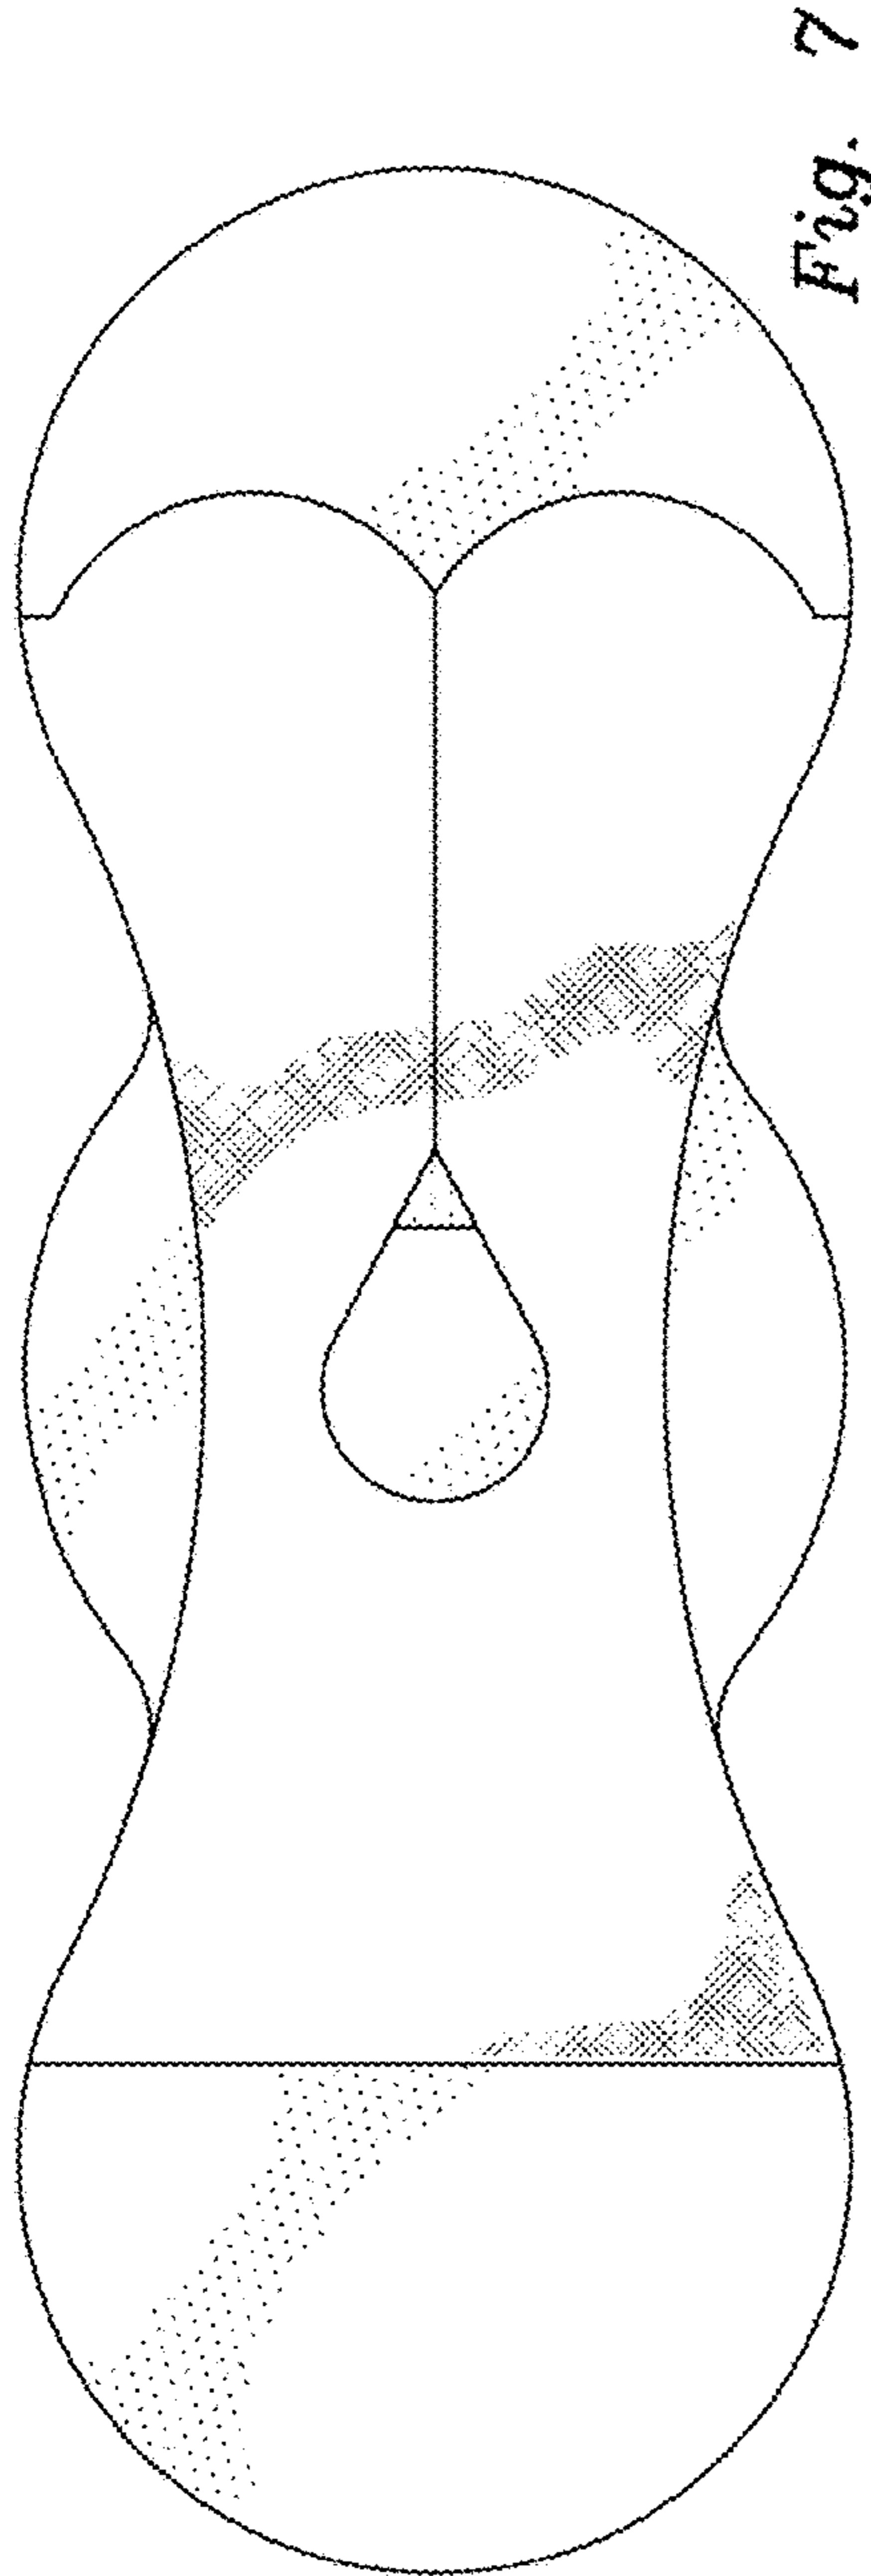



*Fig. 9*



*Fig. 10*



*Fig. 11*