



US00D797288S

(12) **United States Design Patent** (10) **Patent No.:** **US D797,288 S**  
**Zhou et al.** (45) **Date of Patent:** **\*\* Sep. 12, 2017**

(54) **TROCAR**  
(71) Applicant: **Guangzhou T.K Medical Instrument Co., Ltd.**, Guangzhou (CN)  
(72) Inventors: **Xing Zhou**, Guangzhou (CN); **Shaoming Zhu**, Guangzhou (CN); **Jiajiang Wei**, Guangzhou (CN); **Huaping Xu**, Guangzhou (CN); **Lifei Luo**, Guangzhou (CN)  
(73) Assignee: **GUANGZHOU T.K MEDICAL INSTRUMENT CO., LTD.**, Guangzhou (CN)

D700,326 S \* 2/2014 Minelli ..... D24/146  
D713,033 S \* 9/2014 Sauer ..... D24/146  
D753,303 S \* 4/2016 Dannaher ..... D24/146  
2004/0230161 A1 \* 11/2004 Zeiner ..... A61B 17/34  
604/167.06  
2005/0070946 A1 \* 3/2005 Franer ..... A61B 17/3498  
606/185  
2006/0264992 A1 \* 11/2006 Franer ..... A61B 17/3462  
606/167  
2007/0066988 A1 \* 3/2007 Datta ..... A61B 17/3417  
606/185  
2007/0185453 A1 \* 8/2007 Michael ..... A61B 17/3462  
604/164.01

(Continued)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/550,322**

(22) Filed: **Dec. 31, 2015**

(30) **Foreign Application Priority Data**

Jul. 3, 2015 (CN) ..... 2015 3 0233903  
Jul. 3, 2015 (CN) ..... 2015 3 0233909

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/146**

(58) **Field of Classification Search**  
USPC ..... D7/649; D8/93, 97, 300, 310, 311, 313;  
D19/110, 115; D24/146, 147, 148  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D541,417 S \* 4/2007 Albrecht ..... D24/146  
D542,918 S \* 5/2007 Albrecht ..... D24/146  
8,206,411 B2 \* 6/2012 Thompson ..... A61B 17/3462  
600/184

**OTHER PUBLICATIONS**

Guangzhou, Office Action, JP 2015028162, Apr. 4, 2016, 3 pgs.

(Continued)

*Primary Examiner* — Thomas Johannes  
*Assistant Examiner* — Samantha Q Lawrence  
(74) *Attorney, Agent, or Firm* — Morgan, Lewis & Bockius LLP


(57) **CLAIM**

The ornamental design for a trocar, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a trocar;  
FIG. 2 is a first side view of the design of FIG. 1;  
FIG. 3 is a second side view of the design of FIG. 1;  
FIG. 4 is a third side view of the design of FIG. 1;  
FIG. 5 is a fourth side view of the design of FIG. 1;  
FIG. 6 is a top view of the design of FIG. 1; and  
FIG. 7 is a bottom view of the design of FIG. 1.  
The broken lines shown in the drawings represent portions of the trocar that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

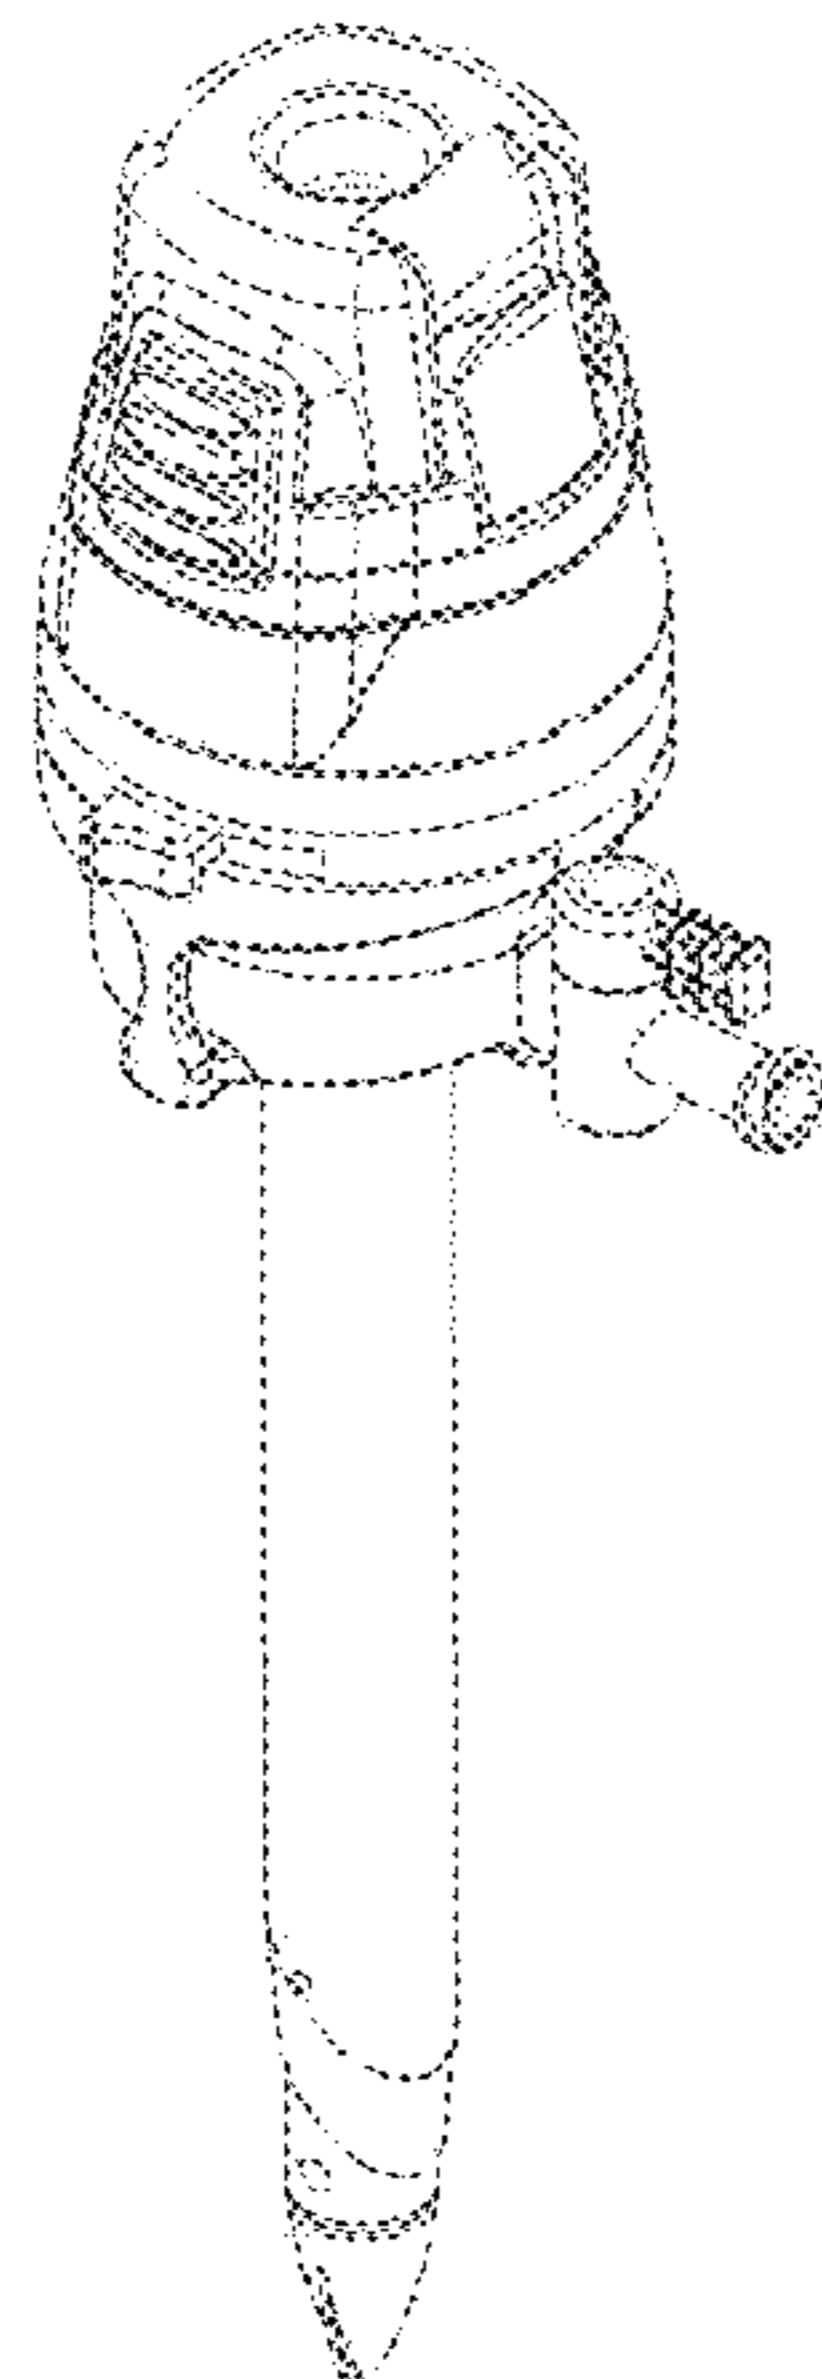

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2007/0260273 A1\* 11/2007 Cropper ..... A61B 1/00087  
606/185  
2008/0228214 A1\* 9/2008 Hoan ..... A61B 17/34  
606/185  
2010/0016878 A1\* 1/2010 Smith ..... A61B 17/3417  
606/185  
2013/0237902 A1\* 9/2013 McGinley ..... A61B 17/3462  
604/26  
2013/0338694 A1\* 12/2013 Fischvogt ..... A61B 17/3494  
606/185

OTHER PUBLICATIONS

Guangzhou, Office Action, CA 166189, May 11, 2016, 1 pg.  
Guangzhou, Certificate of Grant, HK1502637.0, Apr. 8, 2016, 12  
pg.  
Guangzhou, Notice of Allowance, TW104307030, Jul. 11, 2016, 3  
pgs.  
Guangzhou, Certificate of Registration, KR30-2015-0066540, Nov.  
2, 2016, 11 pgs.  
Guangzhou, Certificate of Registration, CA166189, Nov. 16, 2016,  
1 pg.  
Guangzhou, Patent Certificate, TW104307030 Dec. 11, 2016, 2 pgs.

\* cited by examiner

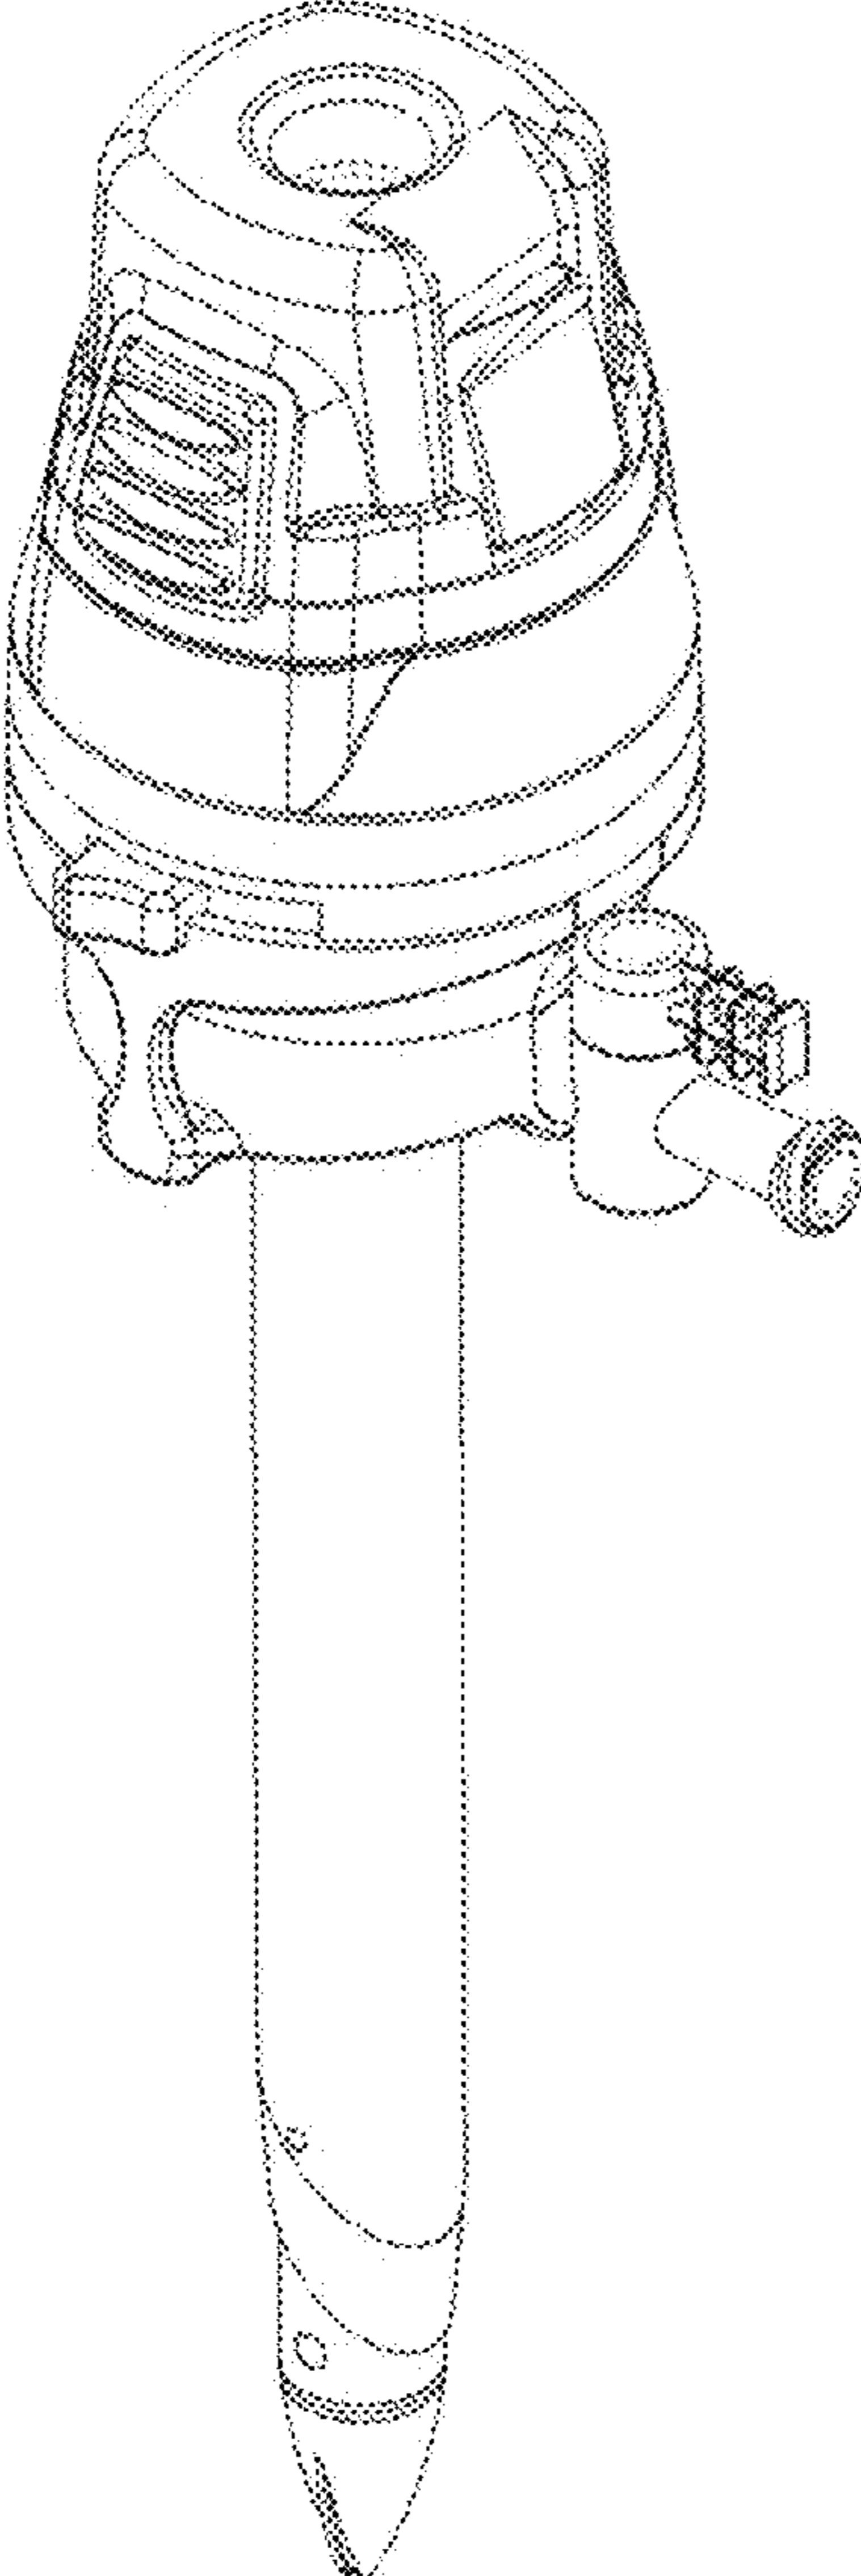


FIG. 1

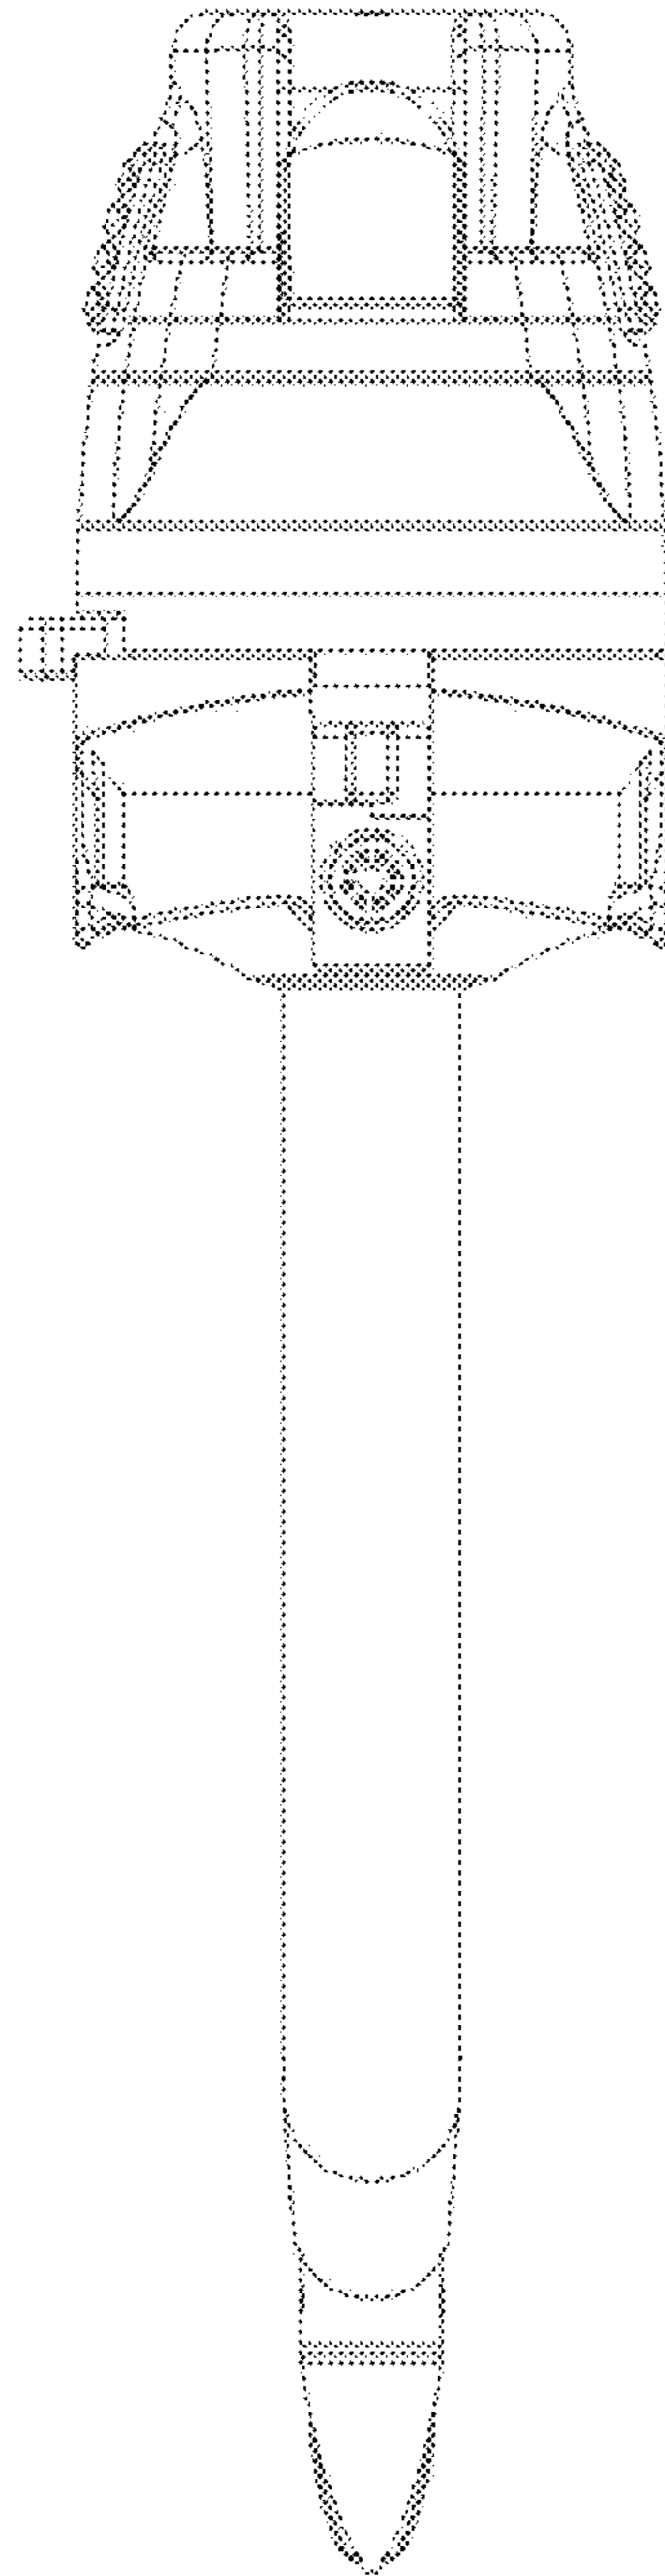


FIG. 2

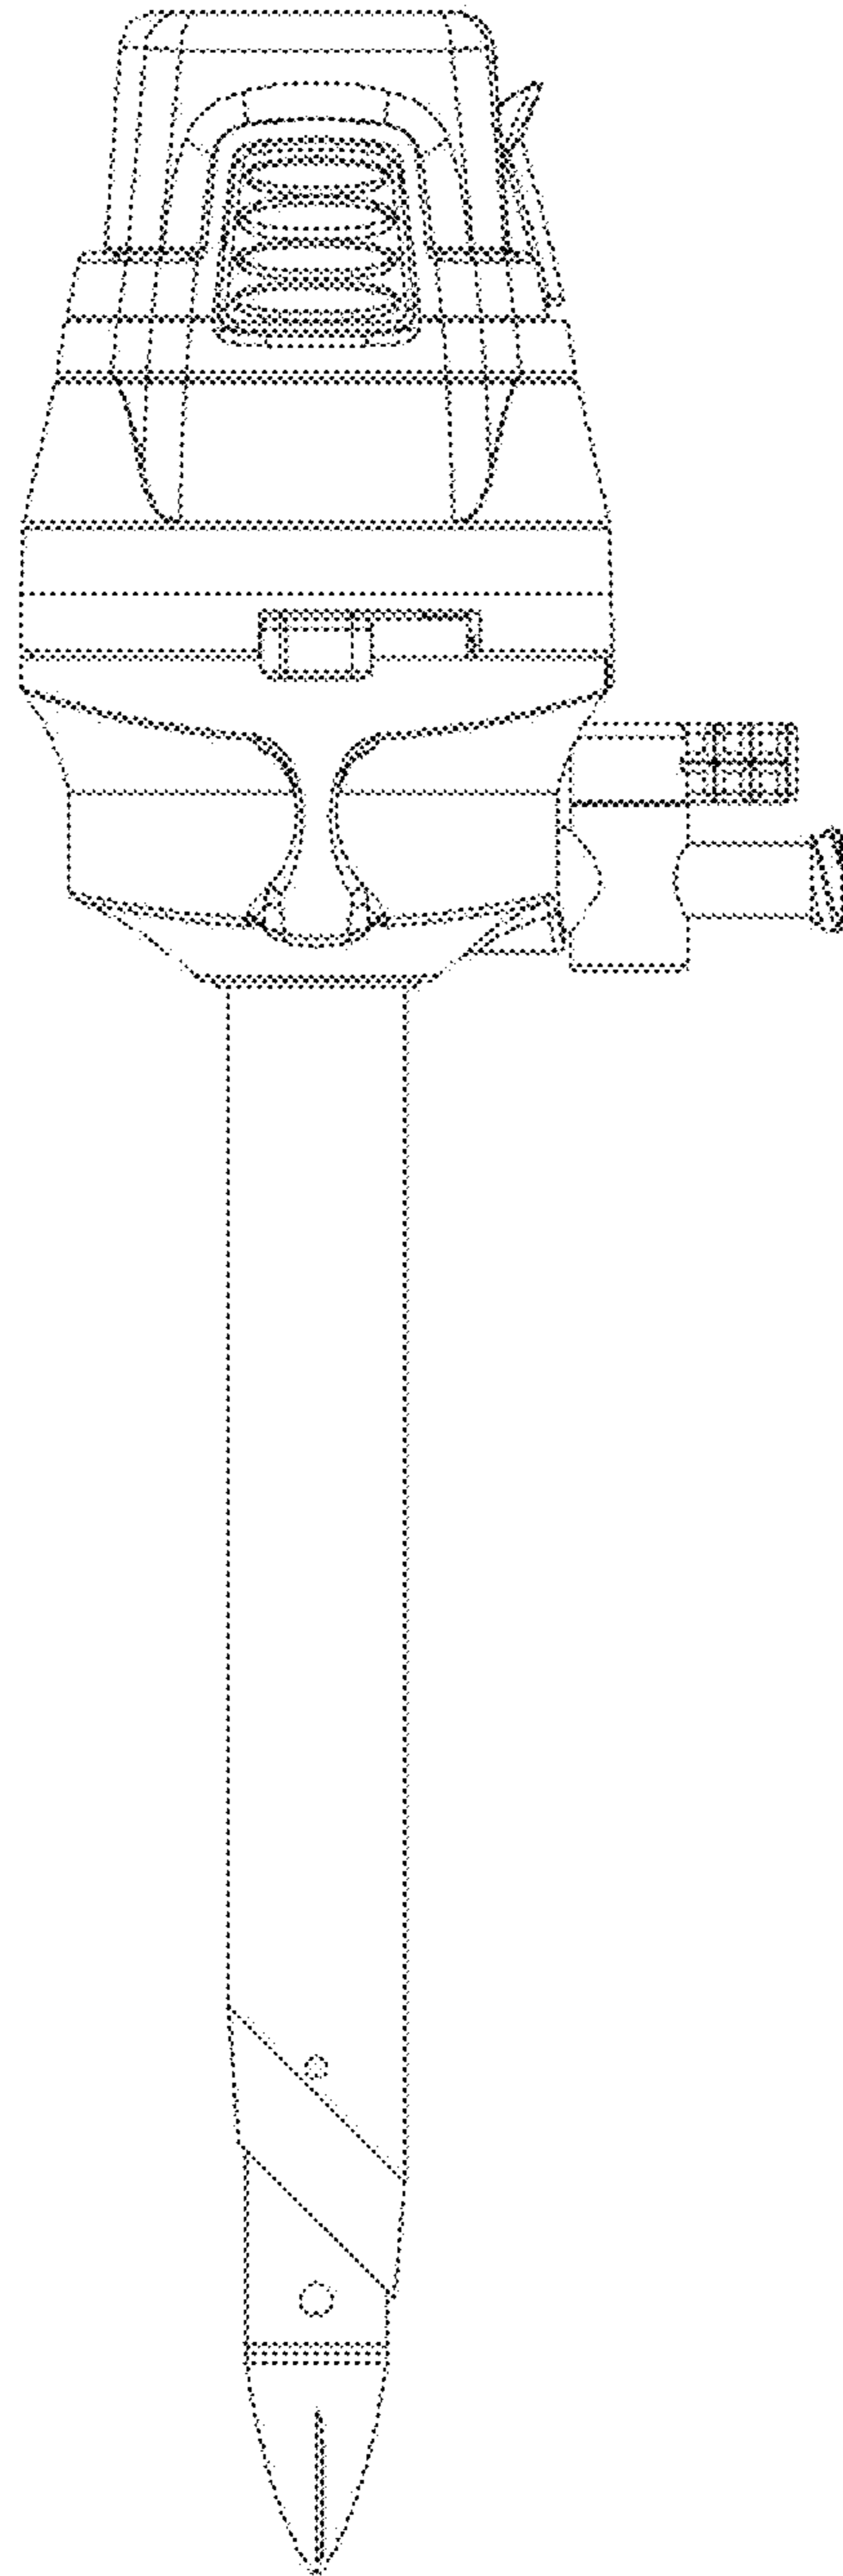


FIG. 3

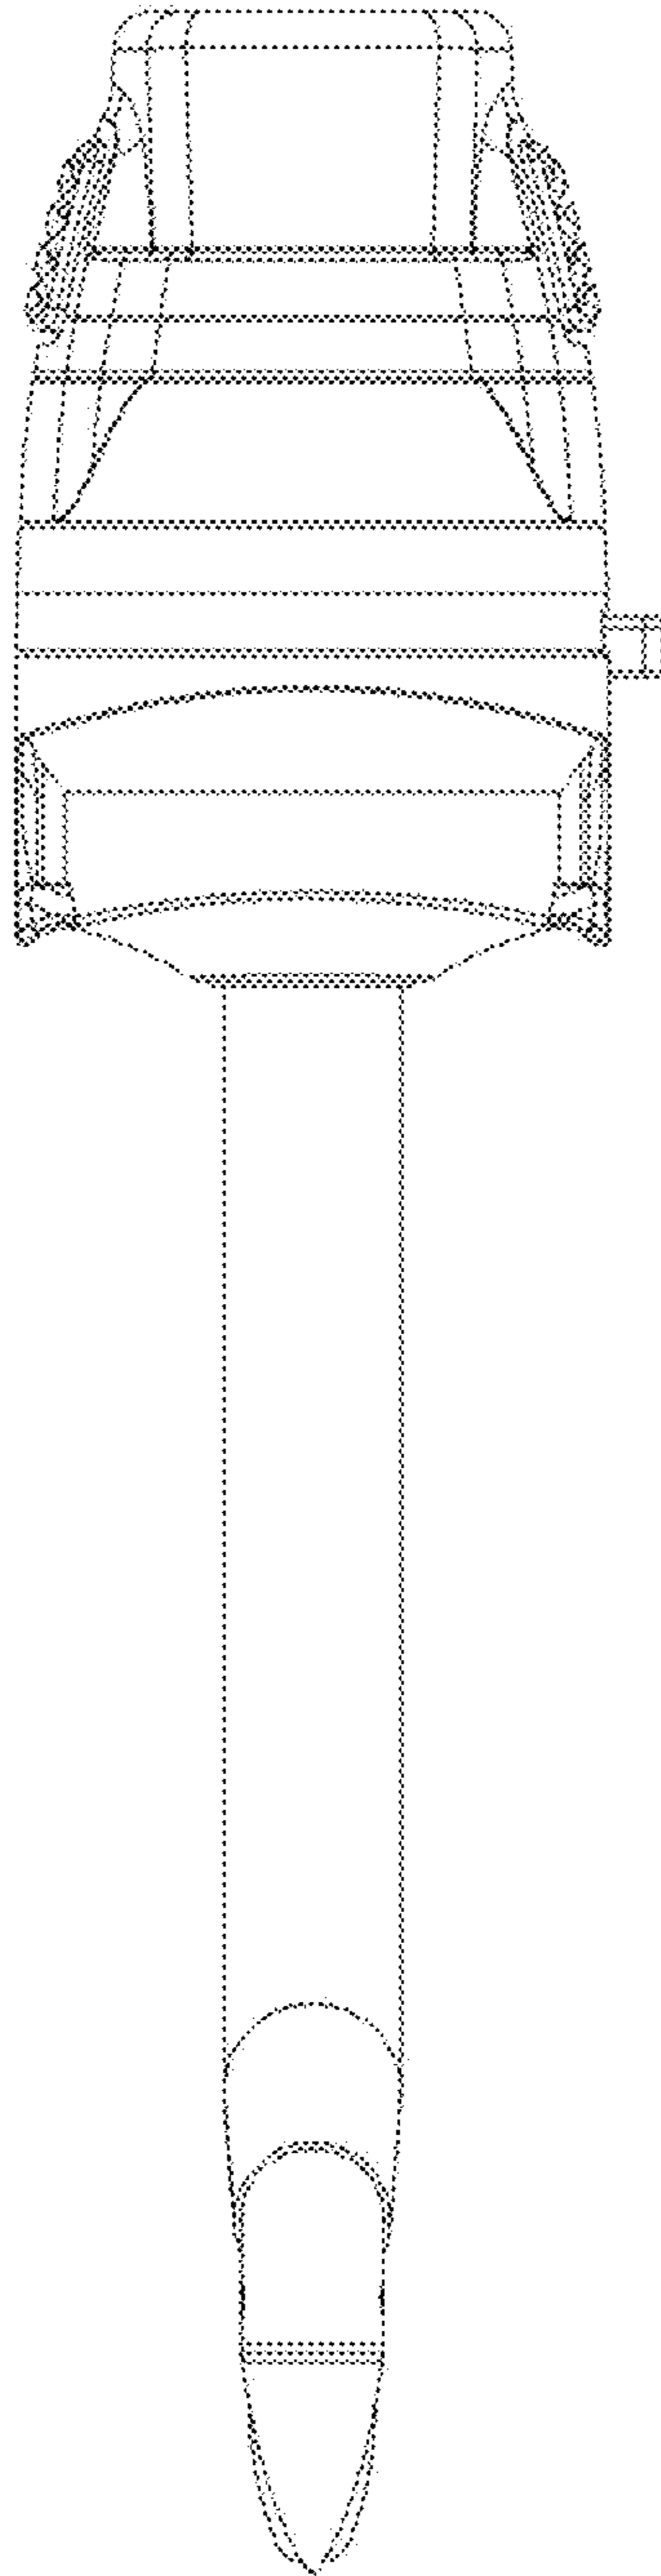


FIG. 4

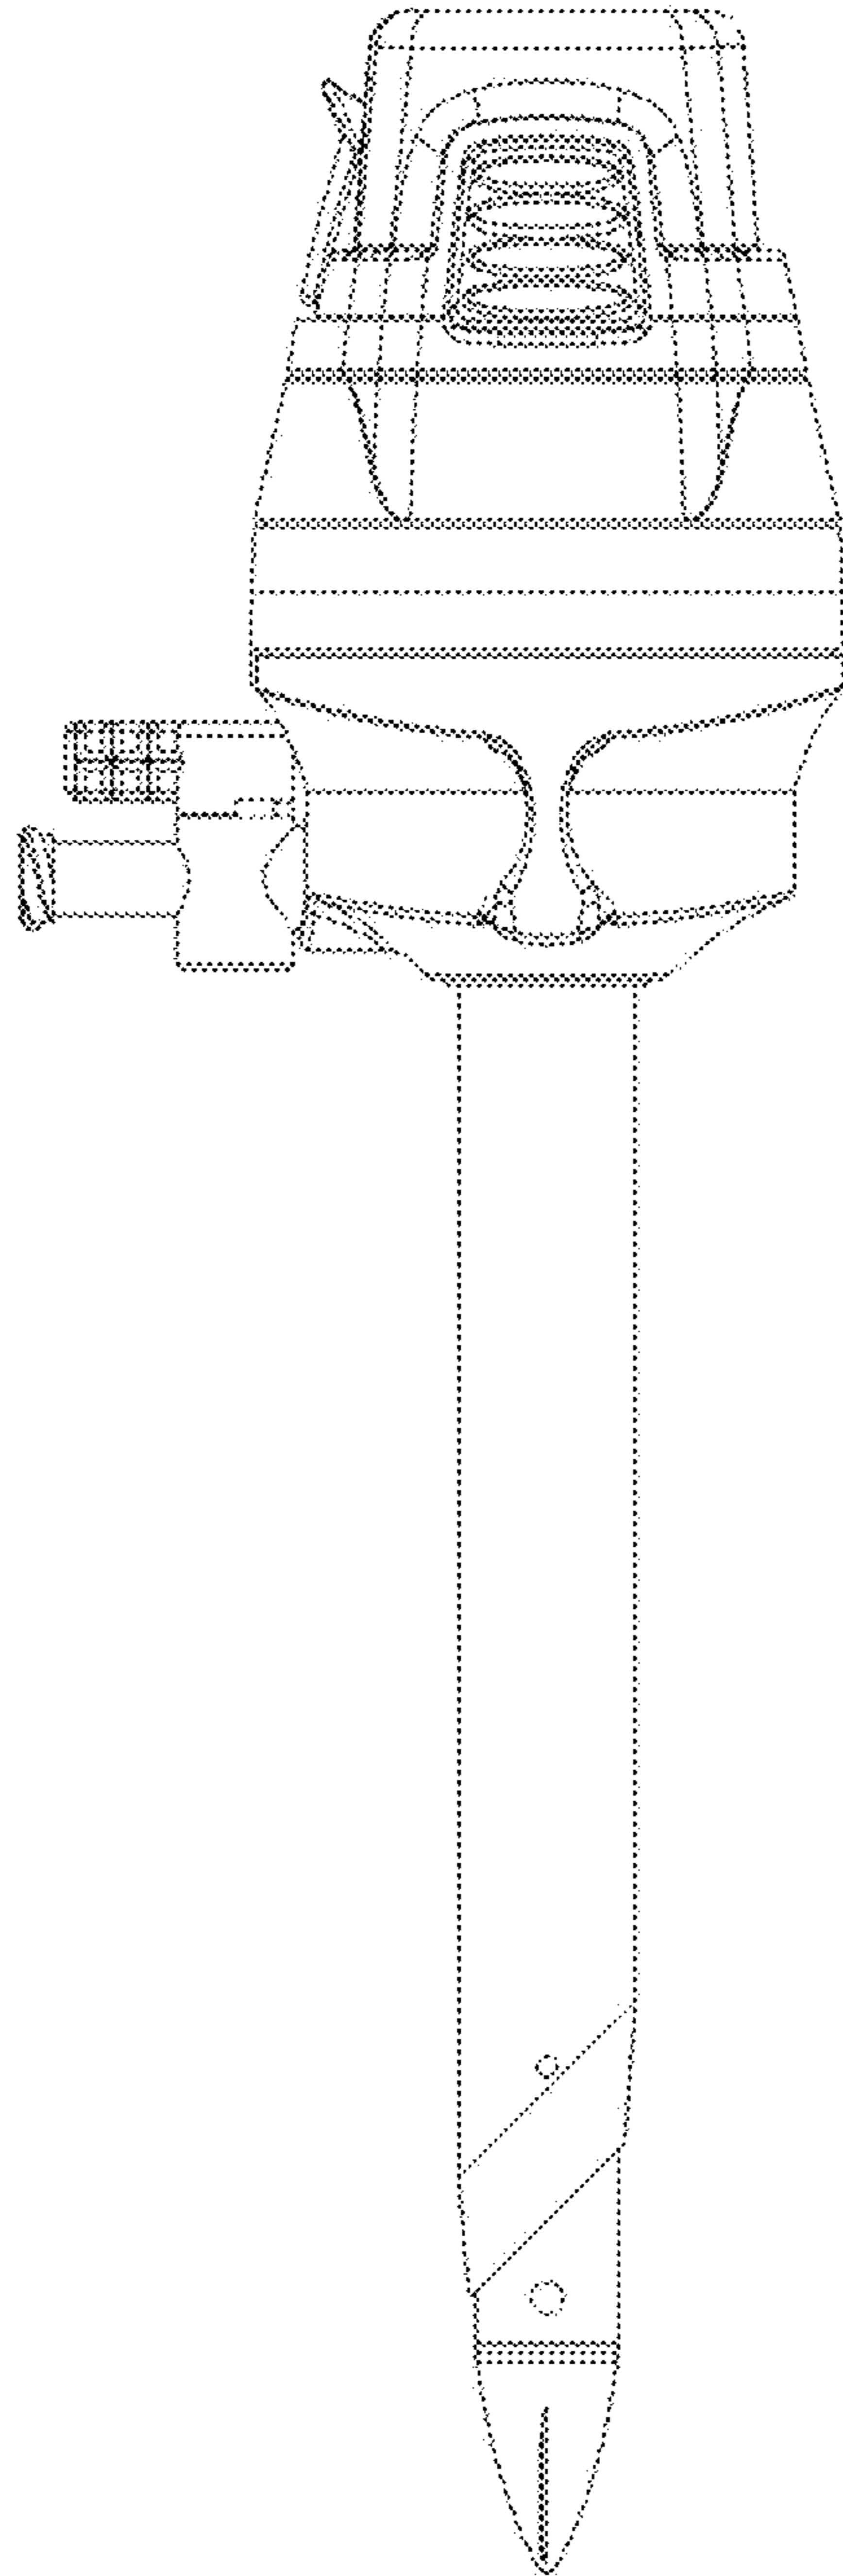


FIG. 5

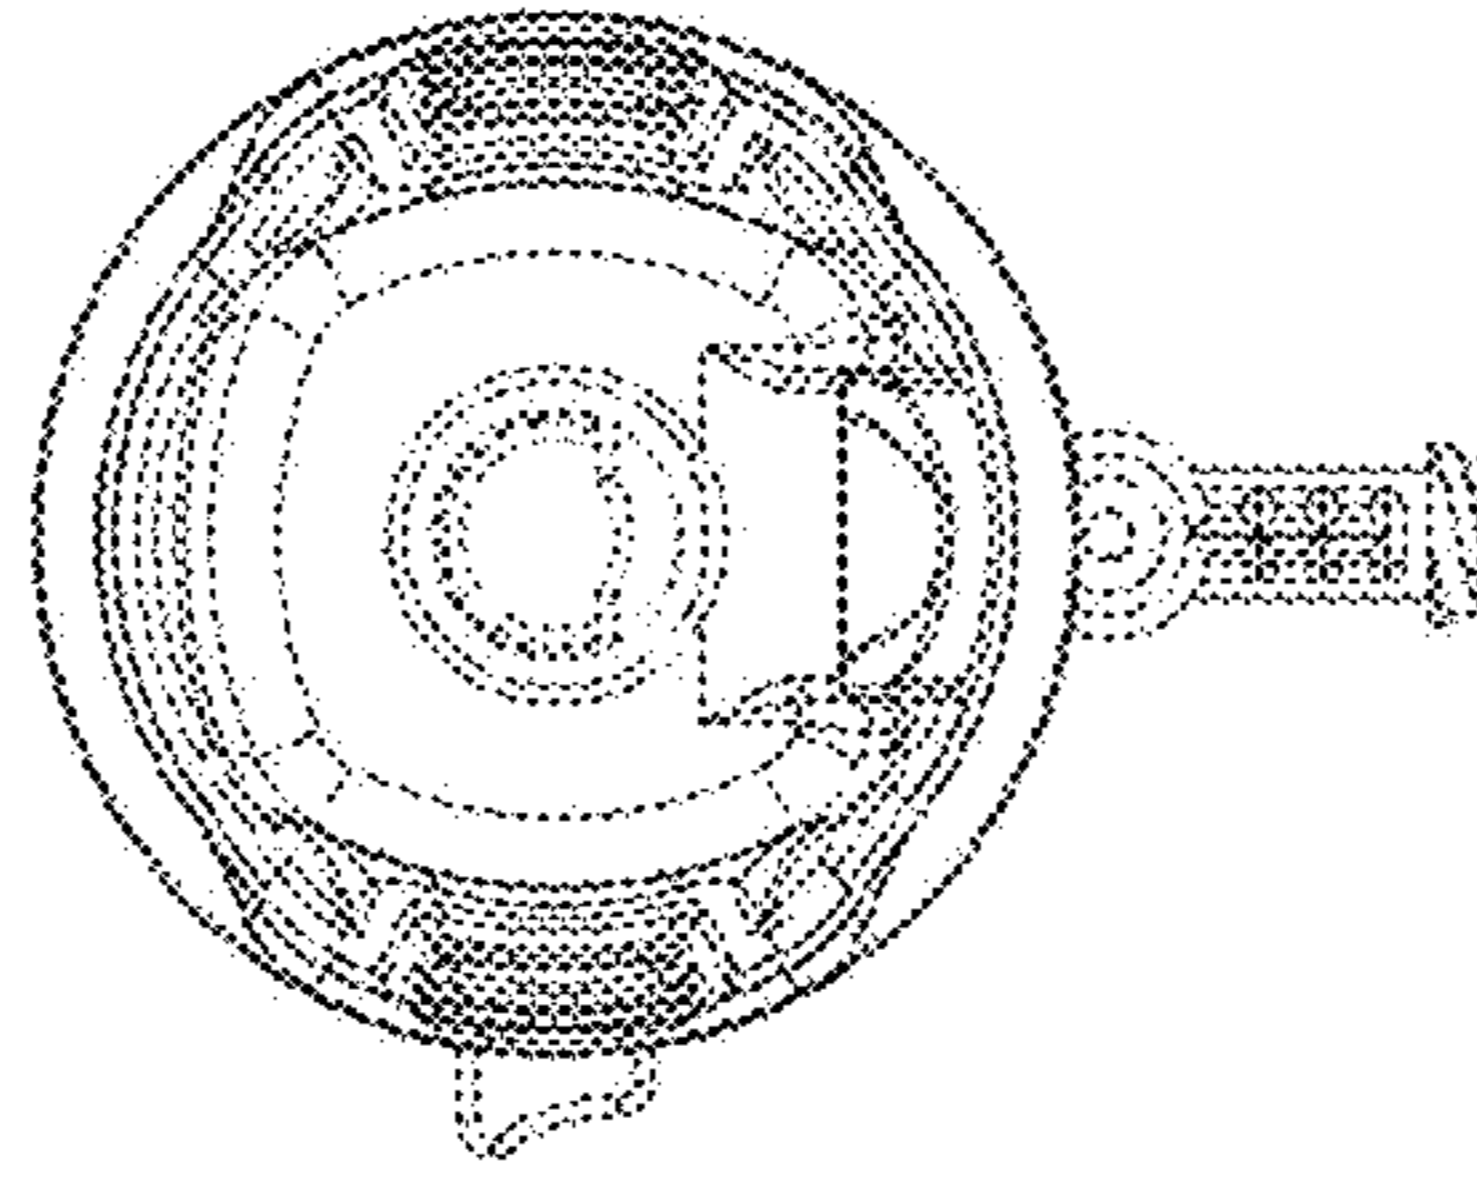


FIG. 6

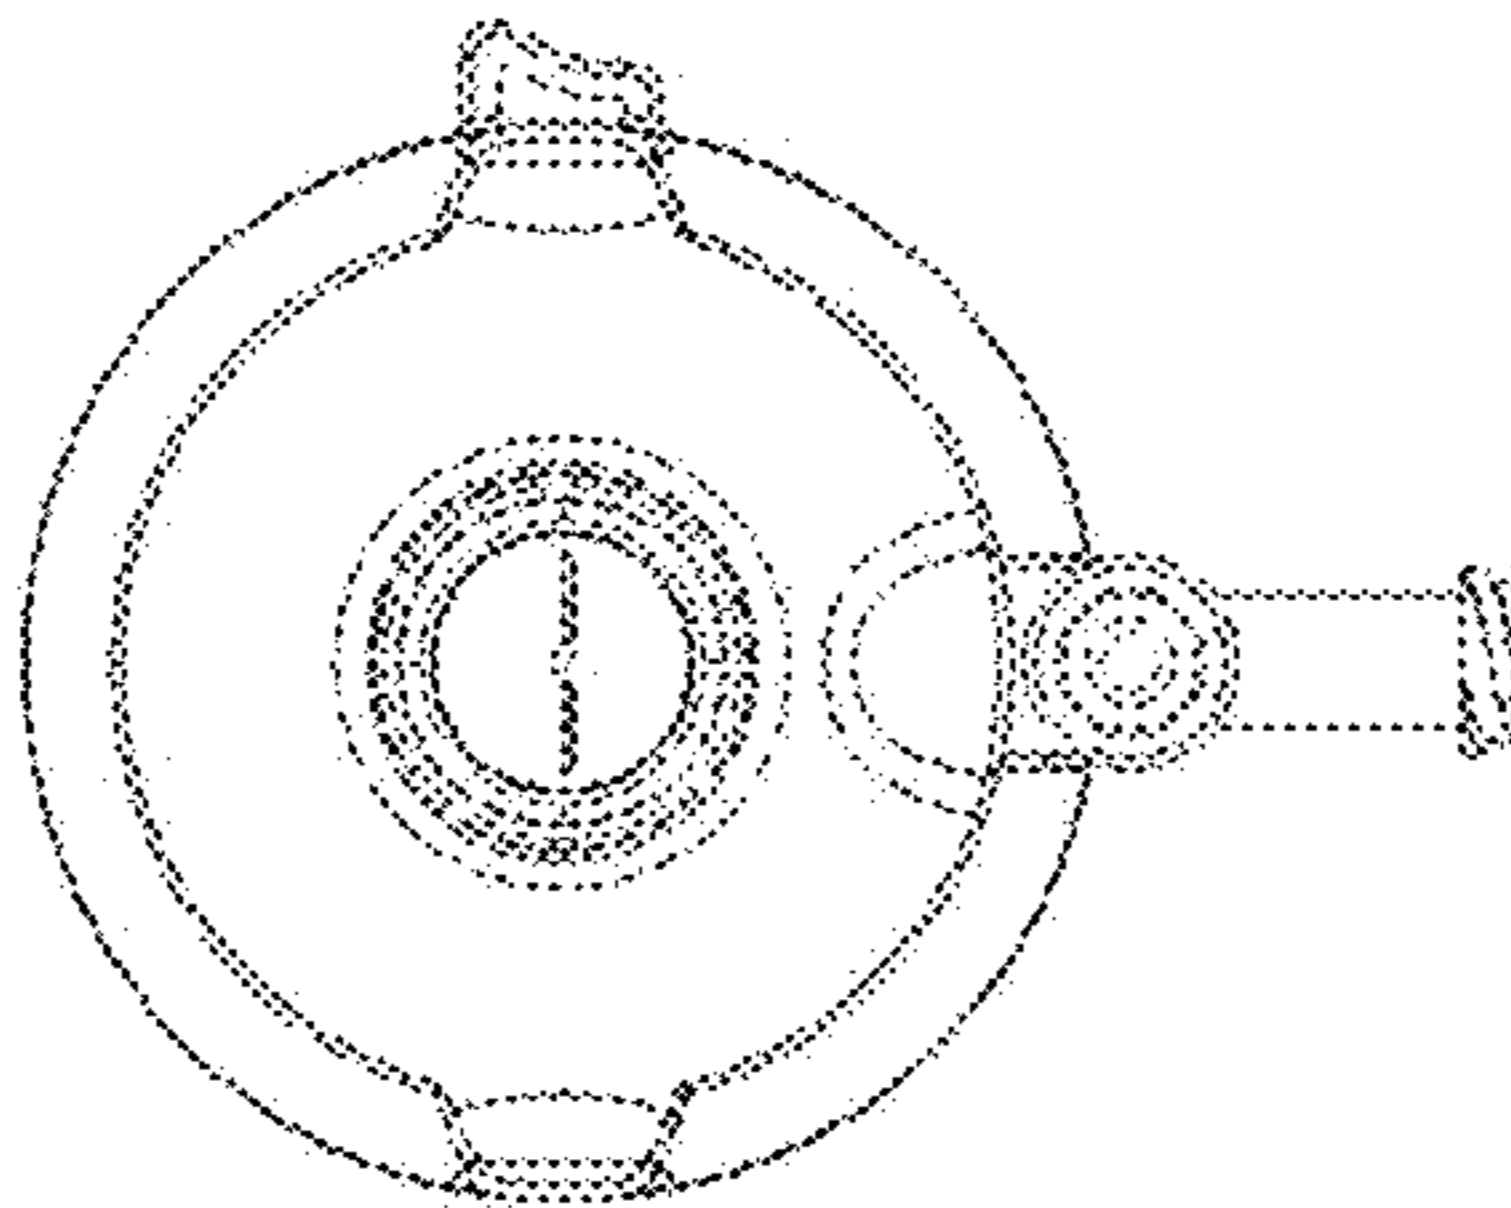


FIG. 7