



US00D798040S

(12) **United States Design Patent** (10) **Patent No.:** **US D798,040 S**
Binder et al. (45) **Date of Patent:** **** Sep. 26, 2017**

(54) **PACKAGING FOR A WOUND THERAPY SYSTEM**

(71) Applicant: **Smith & Nephew PLC**, London (GB)

(72) Inventors: **Ian Binder**, Chippenham (GB); **John Cowan-Hughes**, Bristol (GB); **Beverley Love**, Hessele (GB); **Mark Russell**, Hull (GB); **Peter Sleight**, Cottingham (GB); **Philip Walsh**, Bristol (GB)

(73) Assignee: **Smith & Nephew PLC** (GB)

(**) Term: **15 Years**

(21) Appl. No.: **29/584,531**

(22) Filed: **Nov. 15, 2016**

Related U.S. Application Data

(63) Continuation of application No. 29/563,987, filed on May 10, 2016, now Pat. No. Des. 772,559, which is (Continued)

(51) **LOC (10) Cl.** **03-01**

(52) **U.S. Cl.**
USPC **D3/203.6; D9/432**

(58) **Field of Classification Search**
USPC D9/414, 420-423, 432, 456, 721;
D3/203.1, 203.6, 203.7, 203.8
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D134,249 S 11/1942 Button
2,874,707 A 2/1959 Koppel
(Continued)

FOREIGN PATENT DOCUMENTS

FR 1 163 907 10/1958

OTHER PUBLICATIONS

Packaging for Pico Single Use Negative Pressure Wound Therapy System (2012) in 1 page.

(Continued)

Primary Examiner — Ian Simmons

Assistant Examiner — Keith Frank

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57) **CLAIM**

The ornamental design for packaging for a wound therapy system, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, and left side perspective view of a packaging for a wound therapy system showing my new design in a closed configuration;

FIG. 2 is a front elevation view thereof;

FIG. 3 is a rear elevation view thereof;

FIG. 4 is a right side elevation view thereof;

FIG. 5 is a left side elevation view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof;

FIG. 8 is a top, front, and left side perspective view of the packaging for a wound therapy system of FIG. 1 in a partially open configuration.

FIG. 9 is a front elevation view of the packaging for a wound therapy system of FIG. 1 in a fully open configuration;

FIG. 10 is a rear elevation view thereof;

FIG. 11 is a right side elevation view thereof;



FIG. 12 is a left side elevation view of the packaging of FIG. 1 in a fully open configuration.

FIG. 13 is a top plan view thereof; and,

FIG. 14 is a bottom plan view thereof.

The broken lines in the drawings depict unclaimed subject matter and form no part of the claimed design.

1 Claim, 13 Drawing Sheets

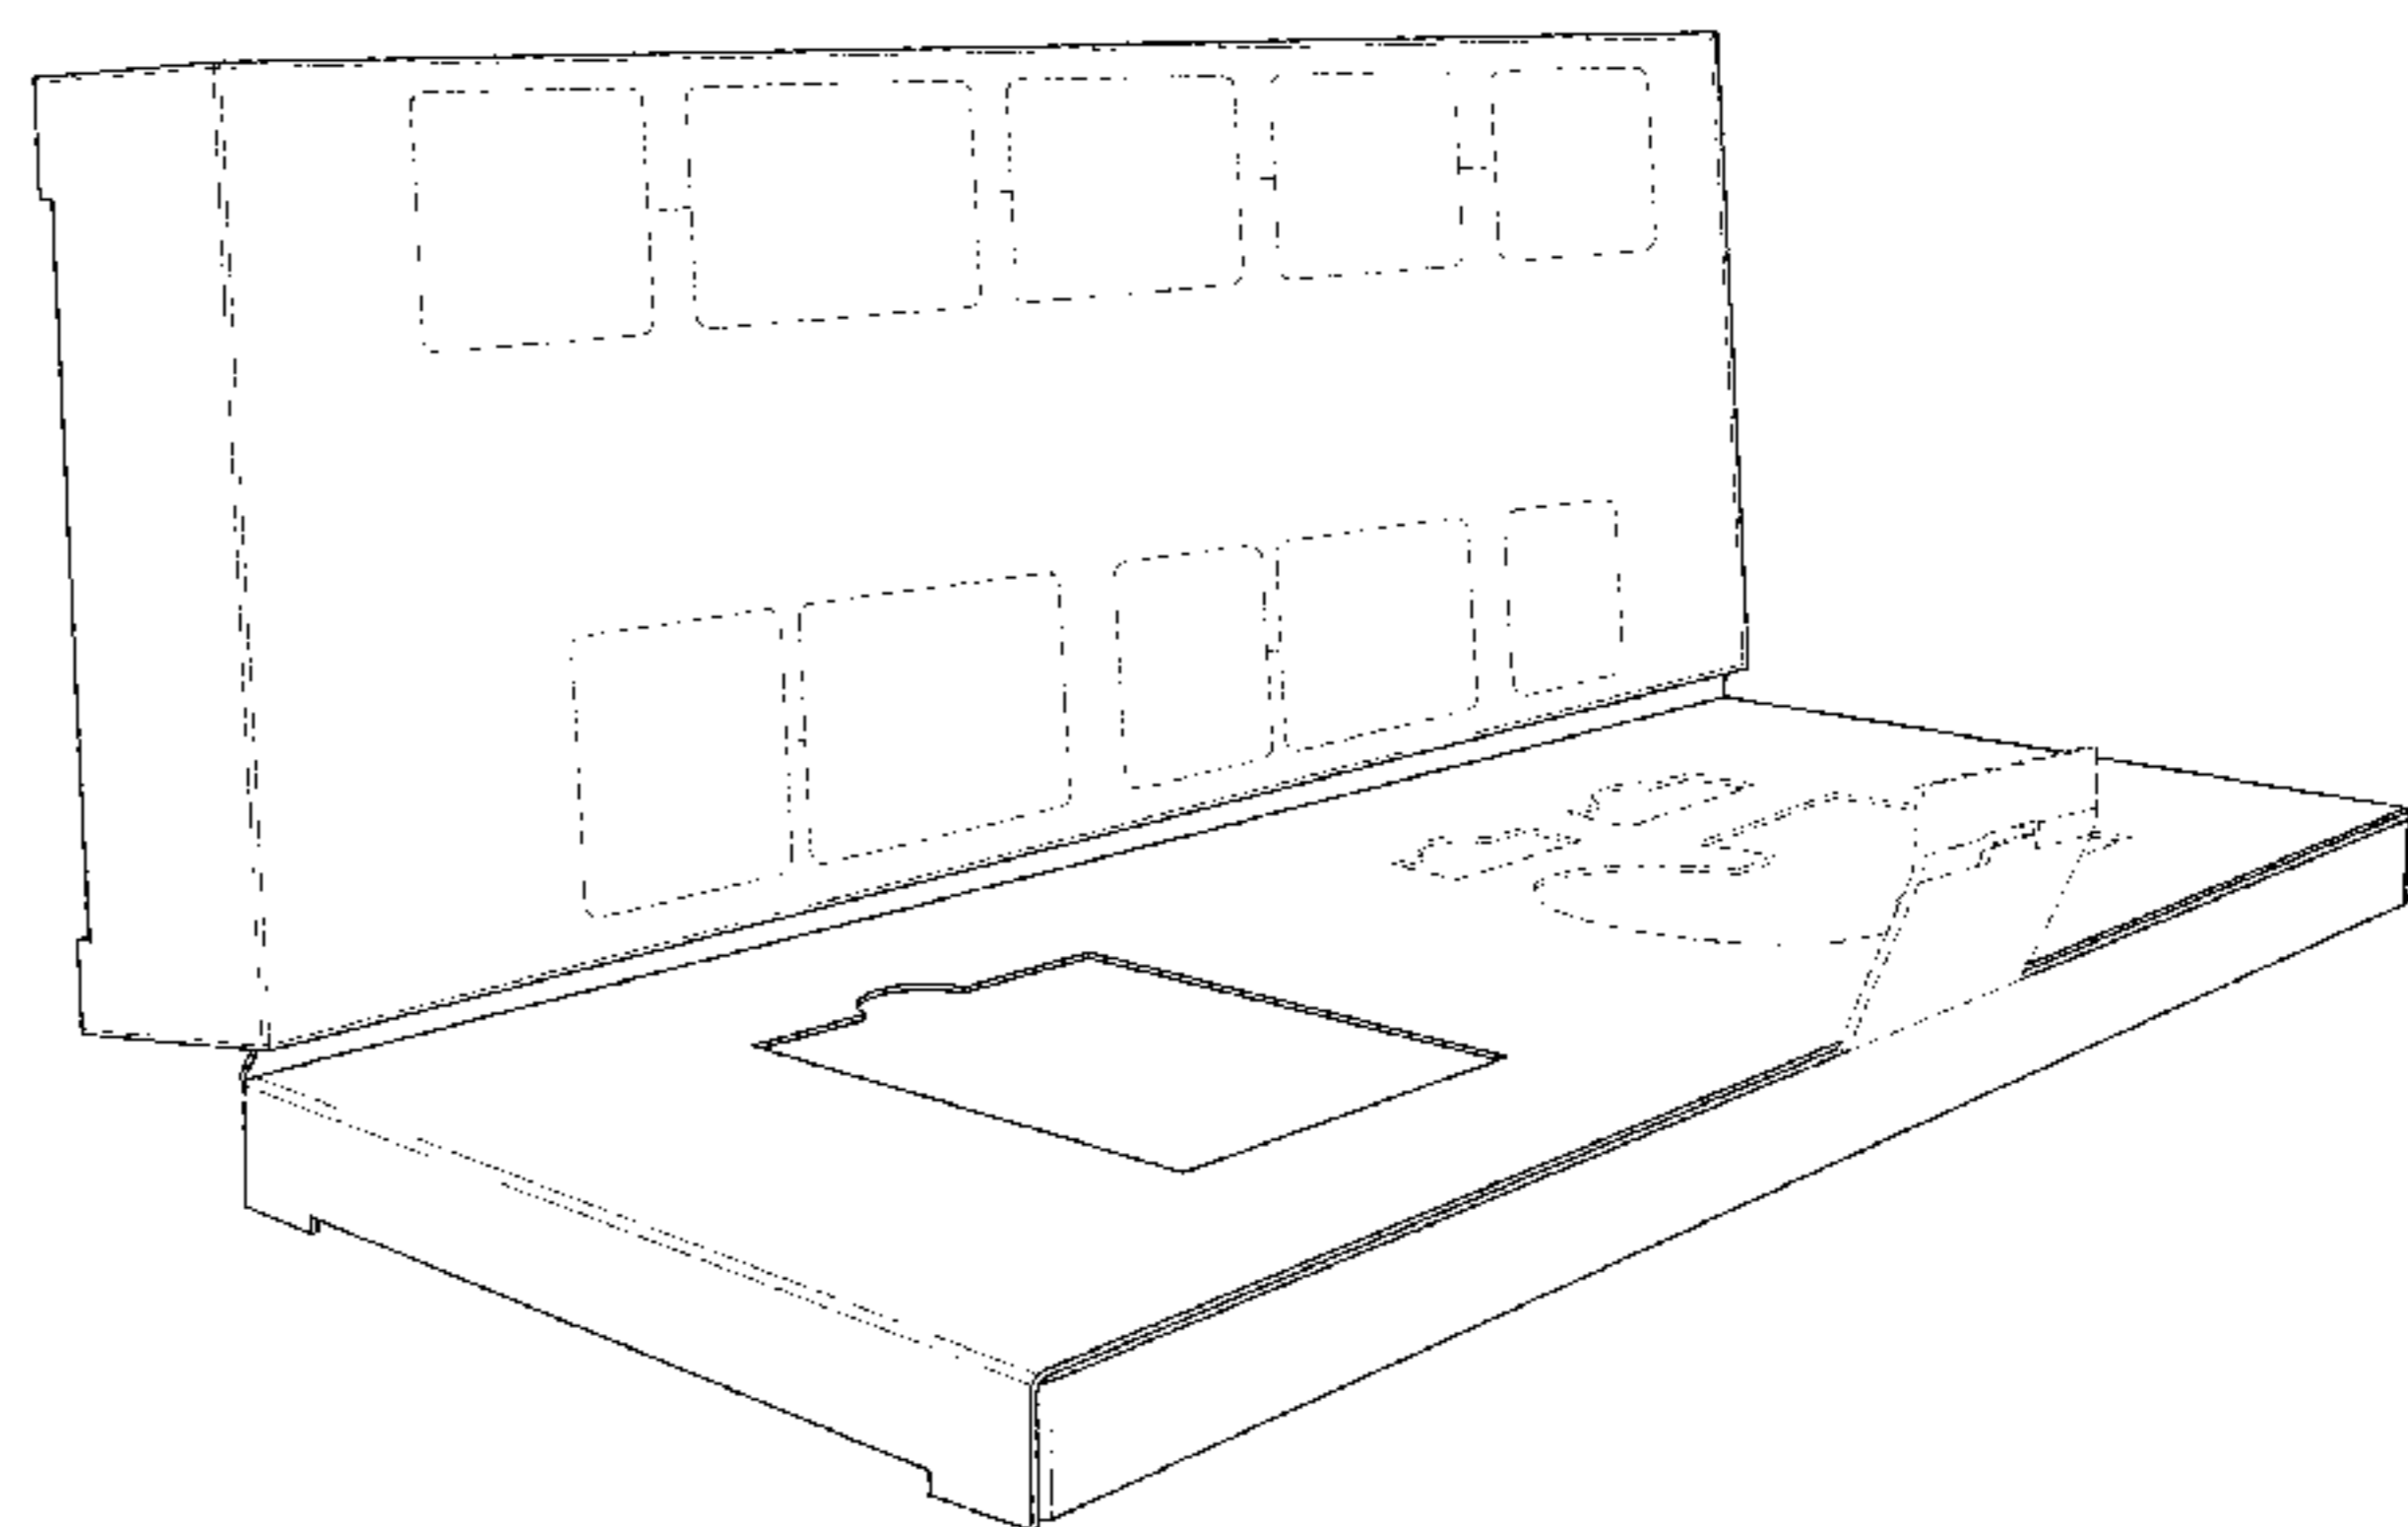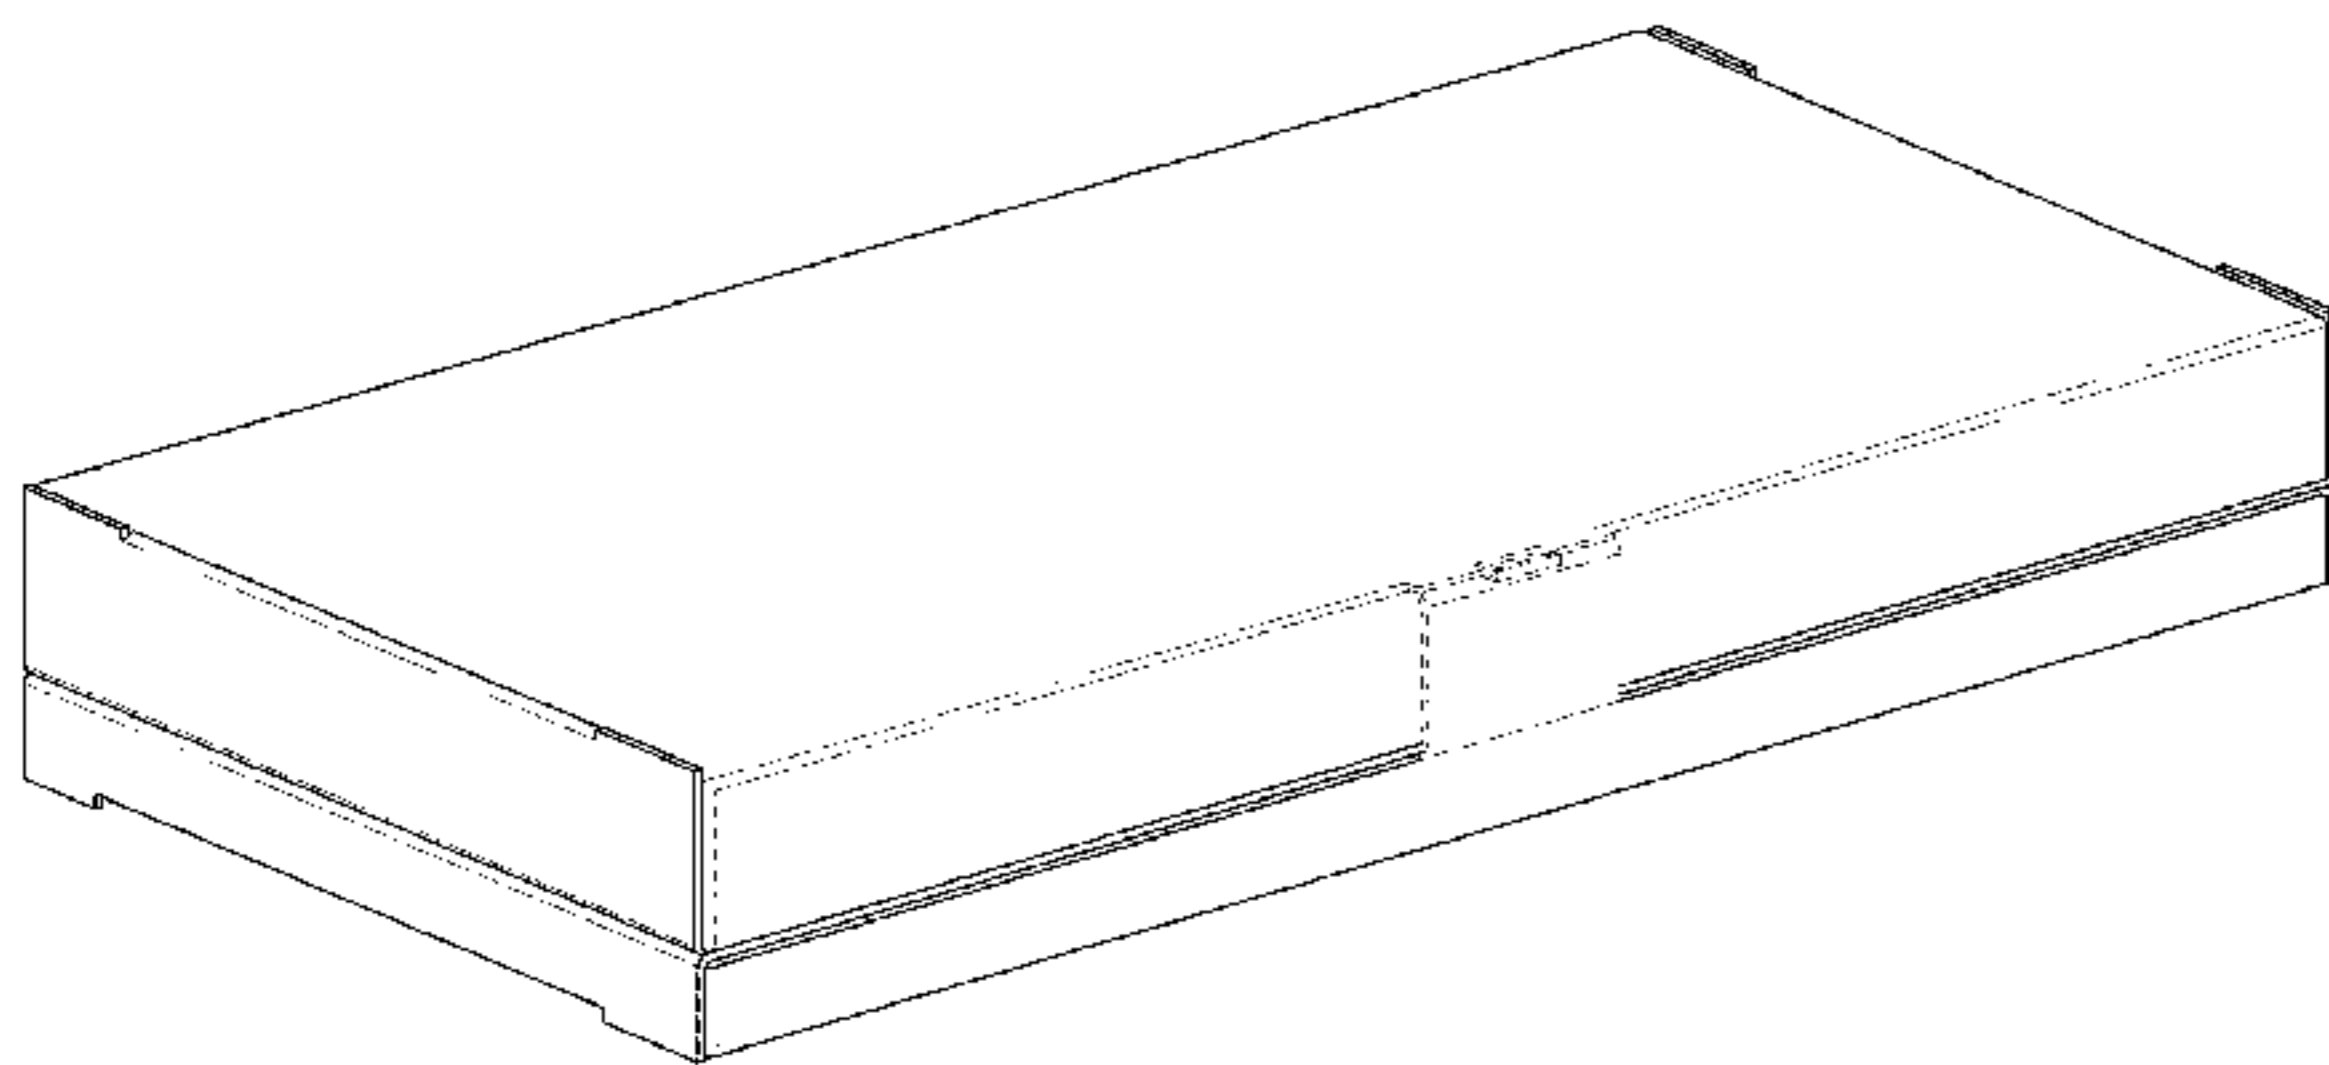

Related U.S. Application Data

a continuation of application No. 29/492,878, filed on Jun. 3, 2014, now Pat. No. Des. 758,851.

(58) **Field of Classification Search**

CPC .. B65D 85/48; B65D 5/0245; B65D 77/0433; B65D 85/46

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,640,379	A	2/1972	Weingarden	
3,972,328	A	8/1976	Chen	
D254,219	S	2/1980	Papciak	
D267,834	S	2/1983	Yew	
D268,098	S	3/1983	Brown	
D275,425	S	9/1984	Briggs	
D281,836	S	12/1985	Sparkman	
D289,461	S	4/1987	Humphries	
4,977,483	A	12/1990	Perretta	
D313,505	S	1/1991	Leopoldi et al.	
D316,181	S	4/1991	Clifton	
D320,308	S	10/1991	Whitworth	
D327,363	S	6/1992	Farb	
5,238,732	A	8/1993	Krishnan	
D339,287	S	9/1993	Levin	
5,344,024	A	9/1994	Cohu	
D365,754	S	1/1996	Plassier	
D369,295	S *	4/1996	Kobari	D9/423
5,549,584	A	8/1996	Gross	
D389,639	S	1/1998	Priebe	
D393,591	S	4/1998	Baryshyan	
5,759,570	A	6/1998	Arnold	
D396,750	S	8/1998	Slater et al.	
D397,869	S	9/1998	Minhas	
D398,527	S	9/1998	Maceachern et al.	
D420,586	S	2/2000	Maceachern et al.	
D431,902	S *	10/2000	Mellin	D3/203.1
D455,312	S *	4/2002	Myszka	D6/407
6,626,891	B2	9/2003	Ohmstede	
6,913,149	B2 *	7/2005	Gelardi	B65D 50/045 206/1.5
7,361,184	B2	4/2008	Joshi	
7,381,859	B2	6/2008	Hunt et al.	
D579,195	S	10/2008	Kagawa	

D589,798	S *	4/2009	Liipola	D9/456
7,569,742	B2	8/2009	Haggstrom et al.	
7,615,036	B2	11/2009	Joshi et al.	
D606,394	S	12/2009	Stewart	
D607,717	S	1/2010	Hodges	
7,699,823	B2	4/2010	Haggstrom et al.	
D618,546	S	6/2010	Easterbrook et al.	
D621,125	S *	8/2010	Heintzelman	D99/28
7,775,998	B2	8/2010	Riesinger	
7,811,269	B2	10/2010	Boynton et al.	
7,846,141	B2	12/2010	Weston	
7,910,791	B2	3/2011	Coffey	
7,922,703	B2	4/2011	Riesinger	
7,964,766	B2	6/2011	Blott et al.	
D644,514	S *	9/2011	Robins	D9/456
D645,735	S	9/2011	Clark et al.	
D661,188	S	6/2012	Fahy	
D661,189	S	6/2012	Fahy	
D661,190	S	6/2012	Fahy	
D663,944	S	7/2012	Bouskill	
D668,948	S	10/2012	LaTrobe	
D678,067	S *	3/2013	Jones	D9/456
D682,279	S *	5/2013	Fuchs	D14/440
D687,300	S	8/2013	Jones et al.	
D704,442	S *	5/2014	Chen	D3/294
D708,055	S	7/2014	Elston et al.	
D723,792	S	3/2015	Anderson et al.	
D729,515	S *	5/2015	Slimane	D3/242
D730,728	S	6/2015	Fath	
9,241,873	B2	1/2016	Upchurch et al.	
D750,478	S	3/2016	Kiss	
D761,023	S	7/2016	Tramontana	
D766,713	S *	9/2016	Kiss	D9/421
2003/0230509	A1 *	12/2003	Fitzgerald	B42F 7/14 206/472
2007/0225663	A1	9/2007	Watt et al.	
2008/0306456	A1	12/2008	Riesinger	

OTHER PUBLICATIONS

Protz, Kerstin: "Modern Wundauflagen unterstützen Heilungsprozess", Wundversorgung: Indikation and Anwendung, Geriatrie Journal Apr. 2005, pp. 3333-3339.

Smith & Nephew, "PICO packaging reduction", Jun. 2014, <http://www.smith-nephew.com/news-and-media/case-studies/picosntm-packaging-reduction/>.

* cited by examiner

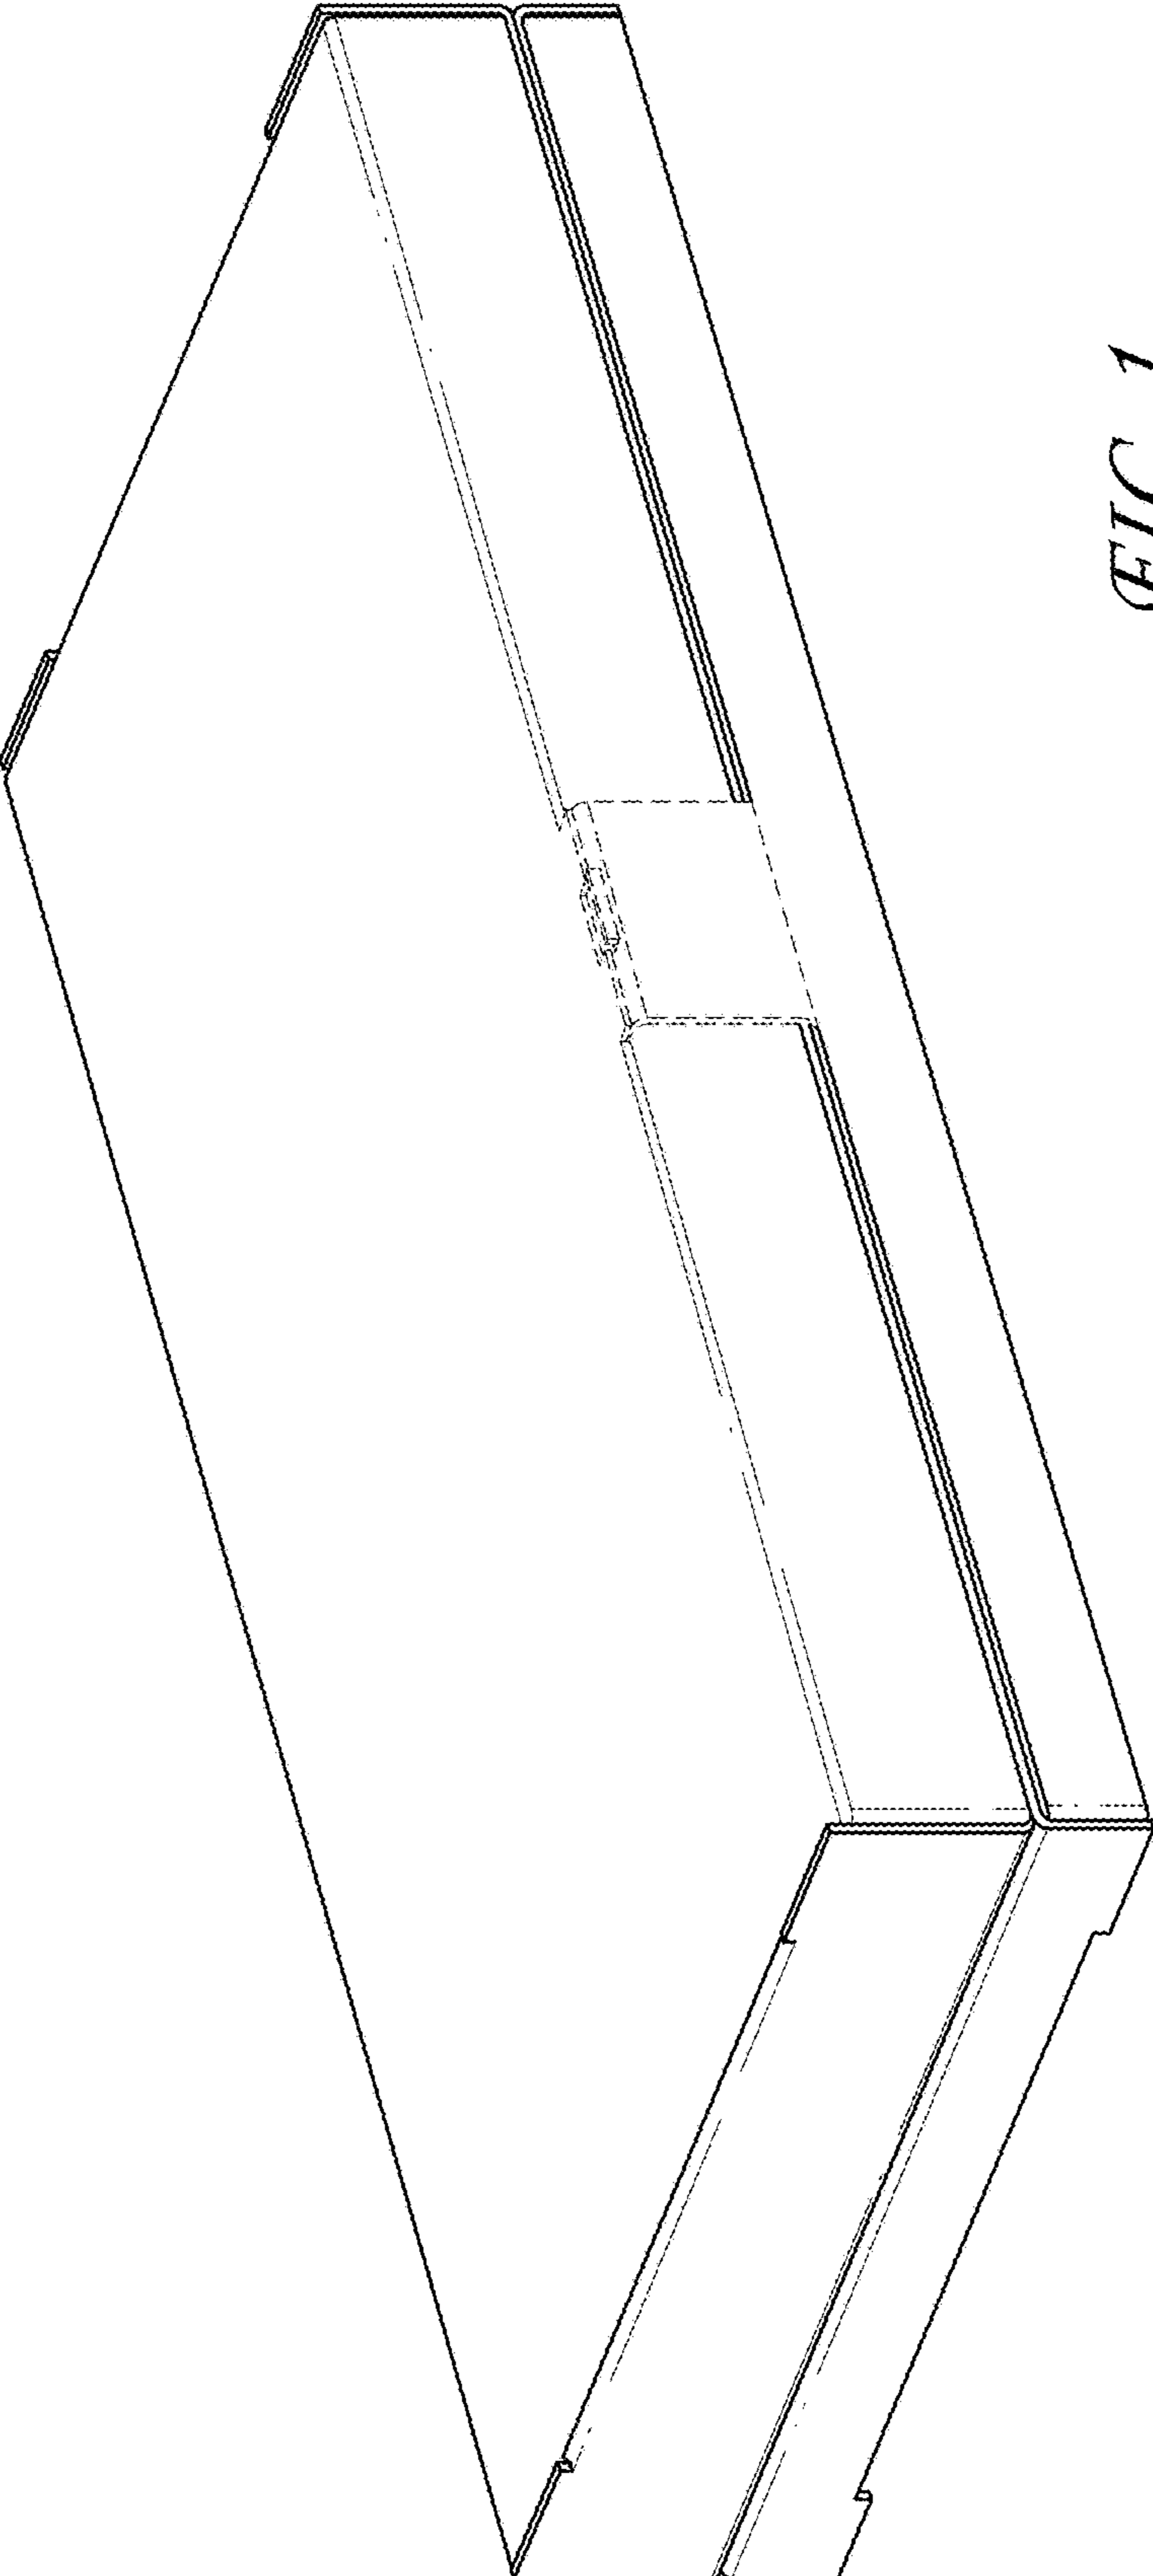


FIG. 1

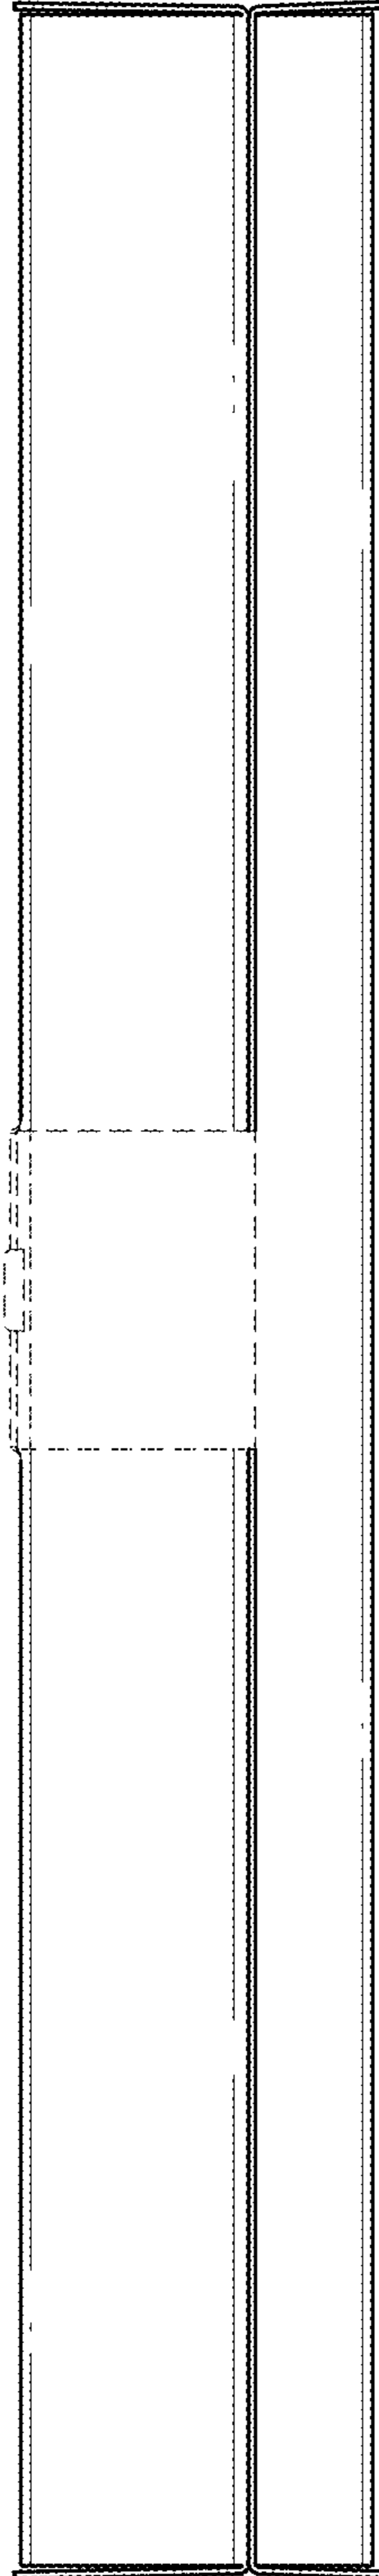


FIG. 2

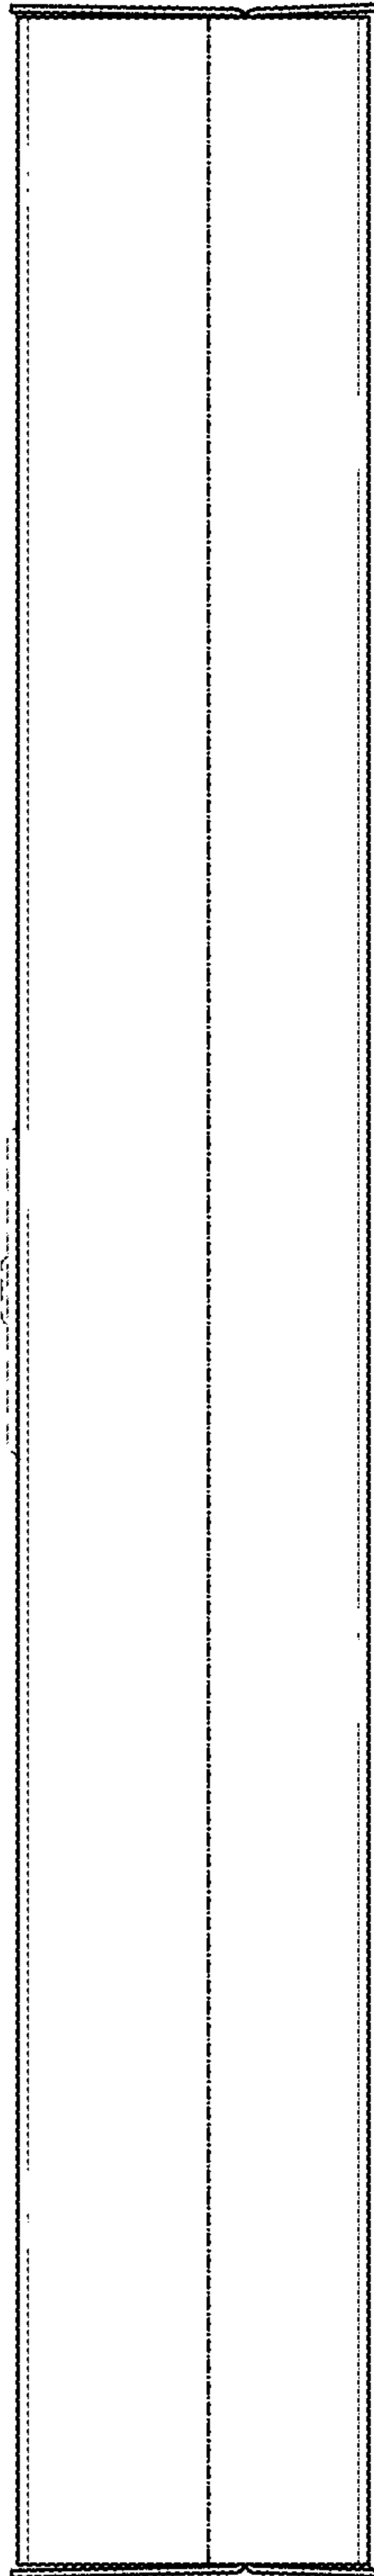


FIG. 3

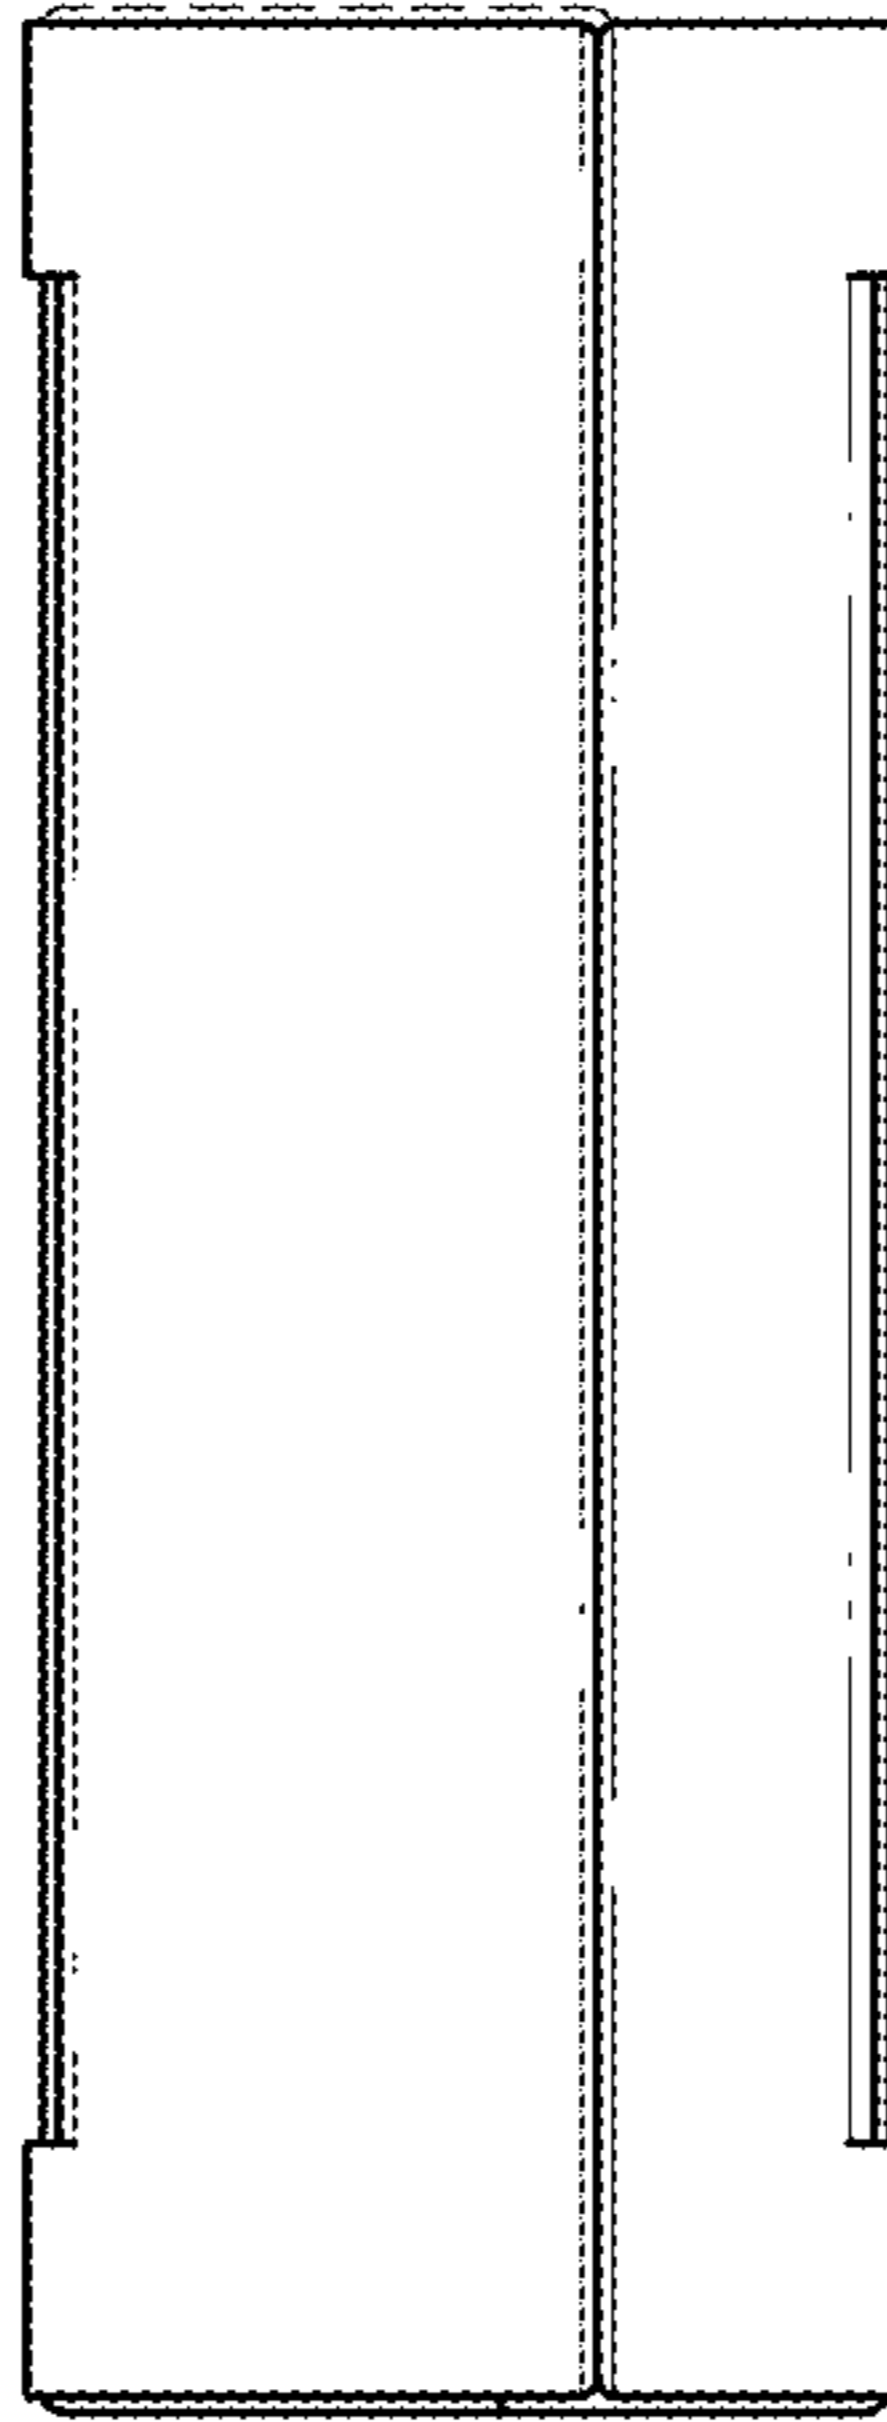


FIG. 4

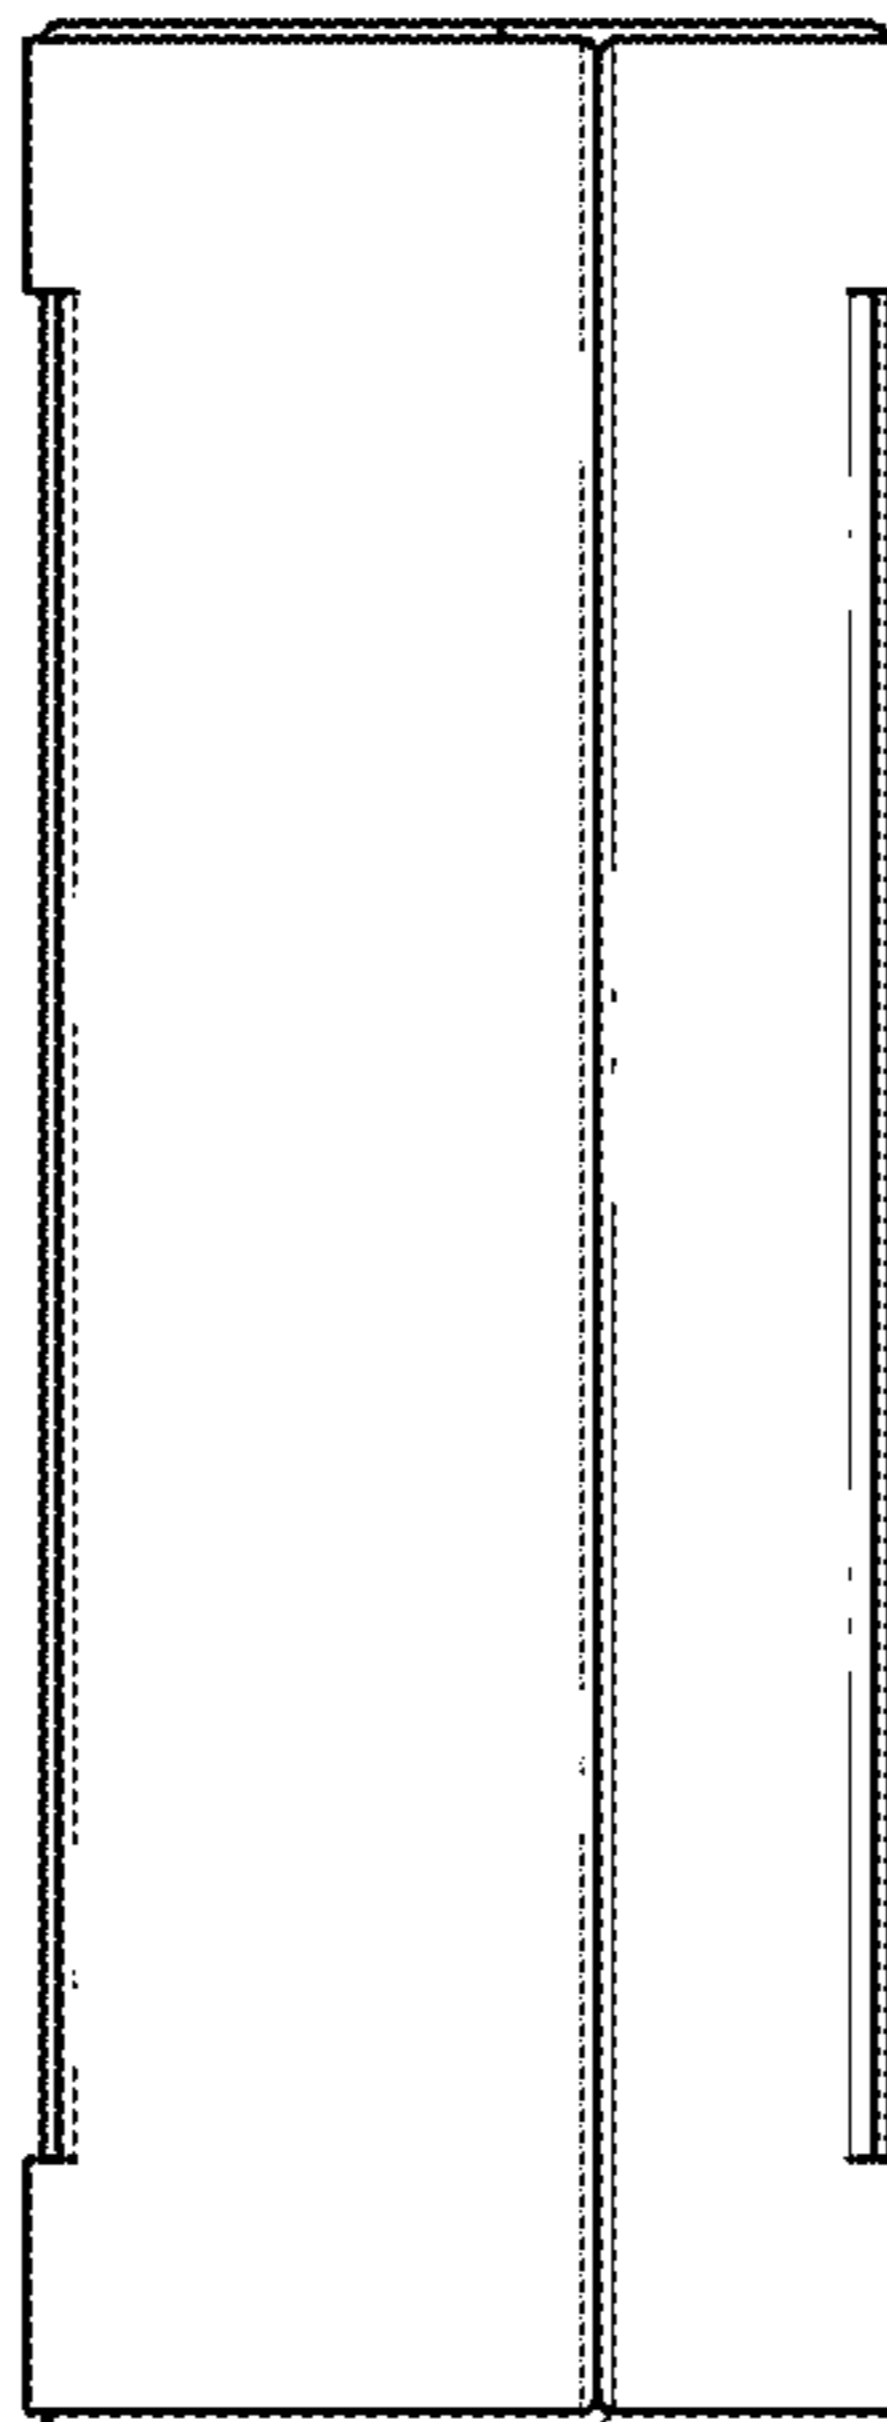


FIG. 5

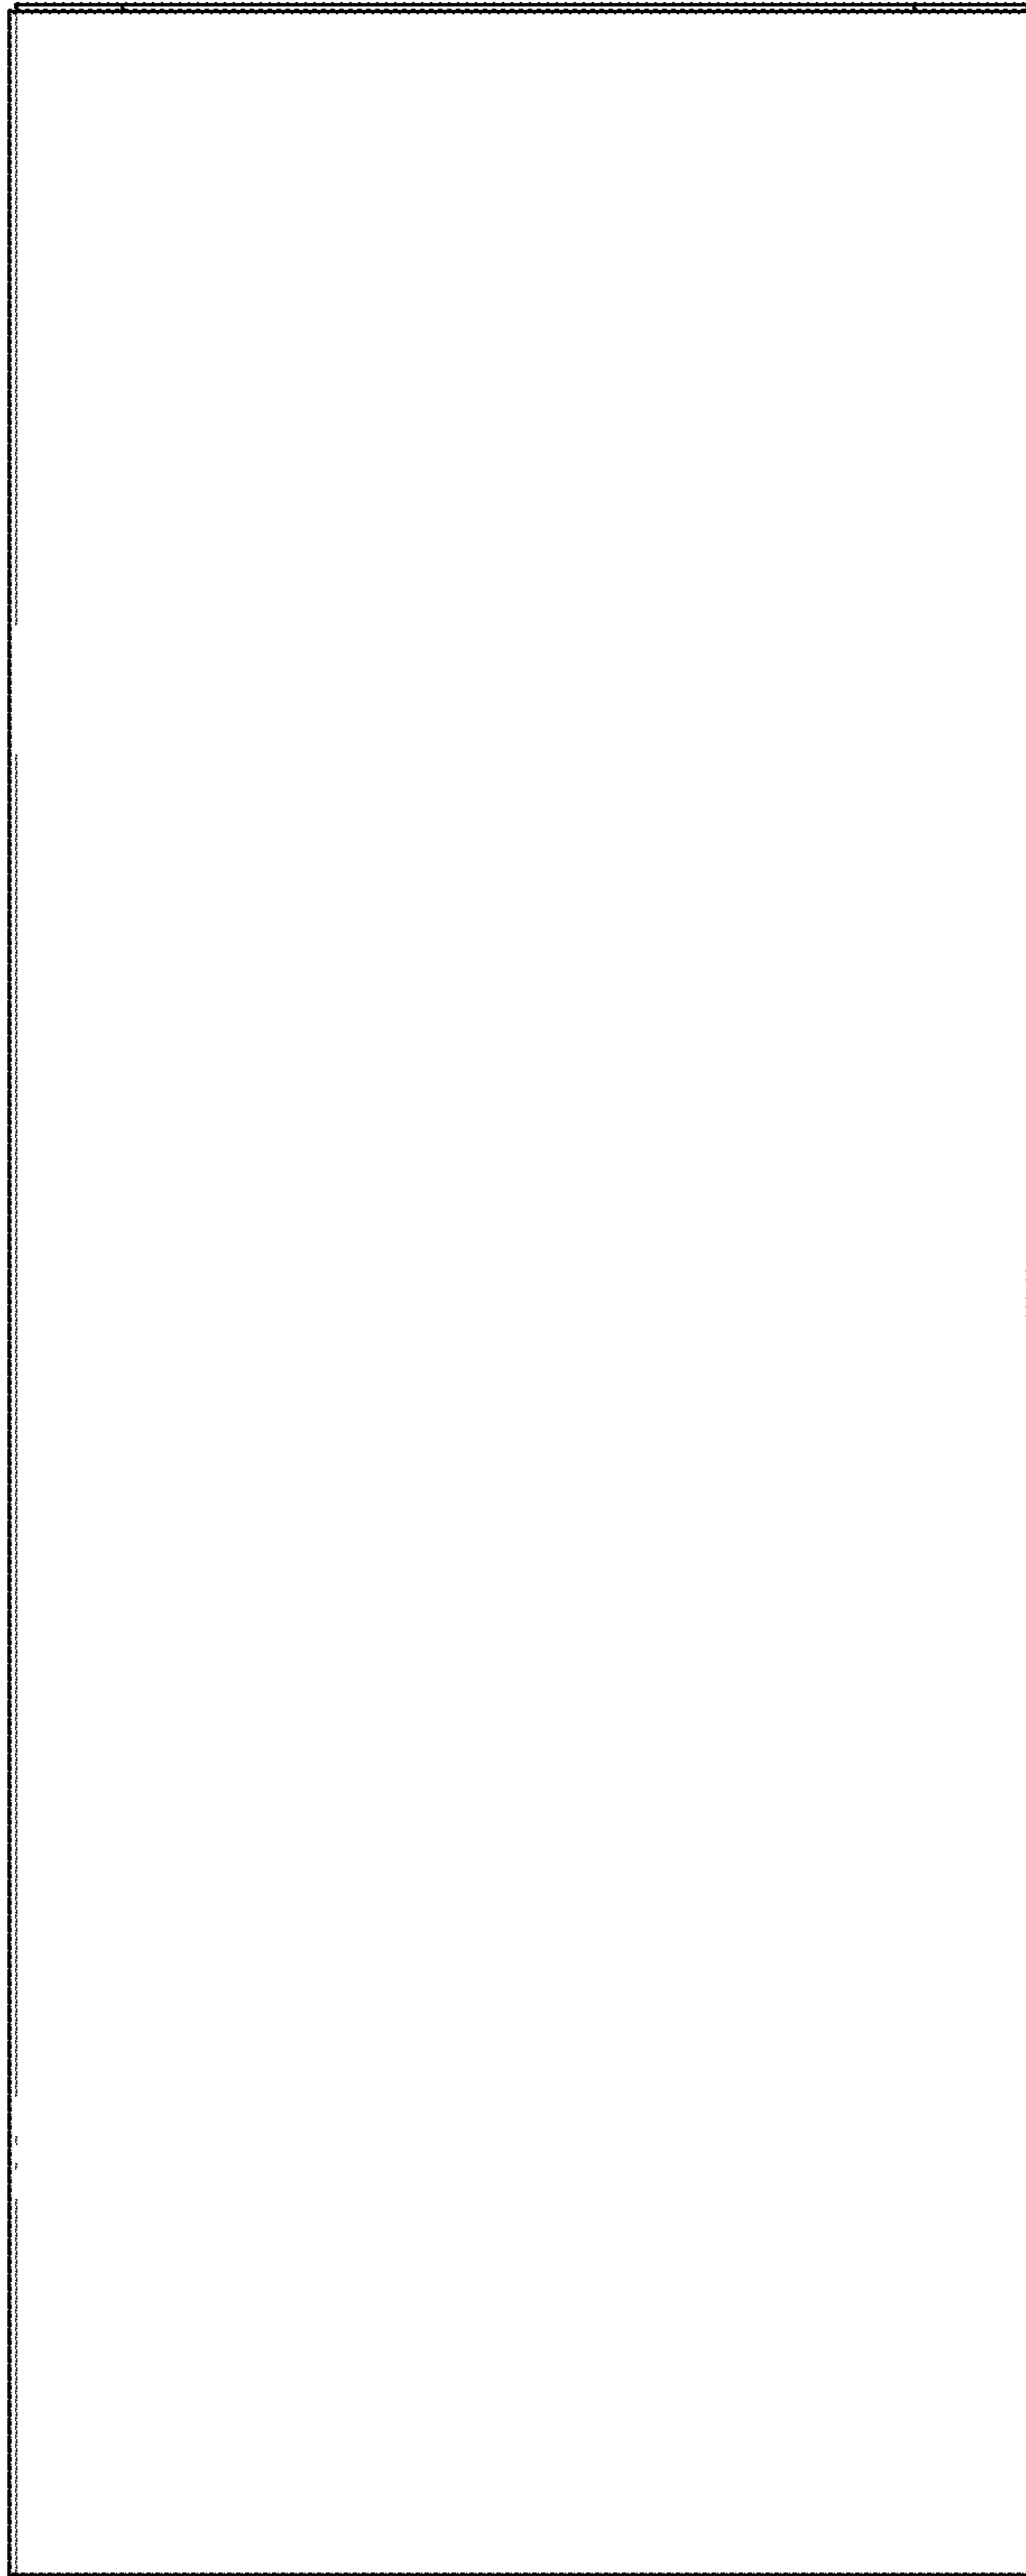


FIG. 6

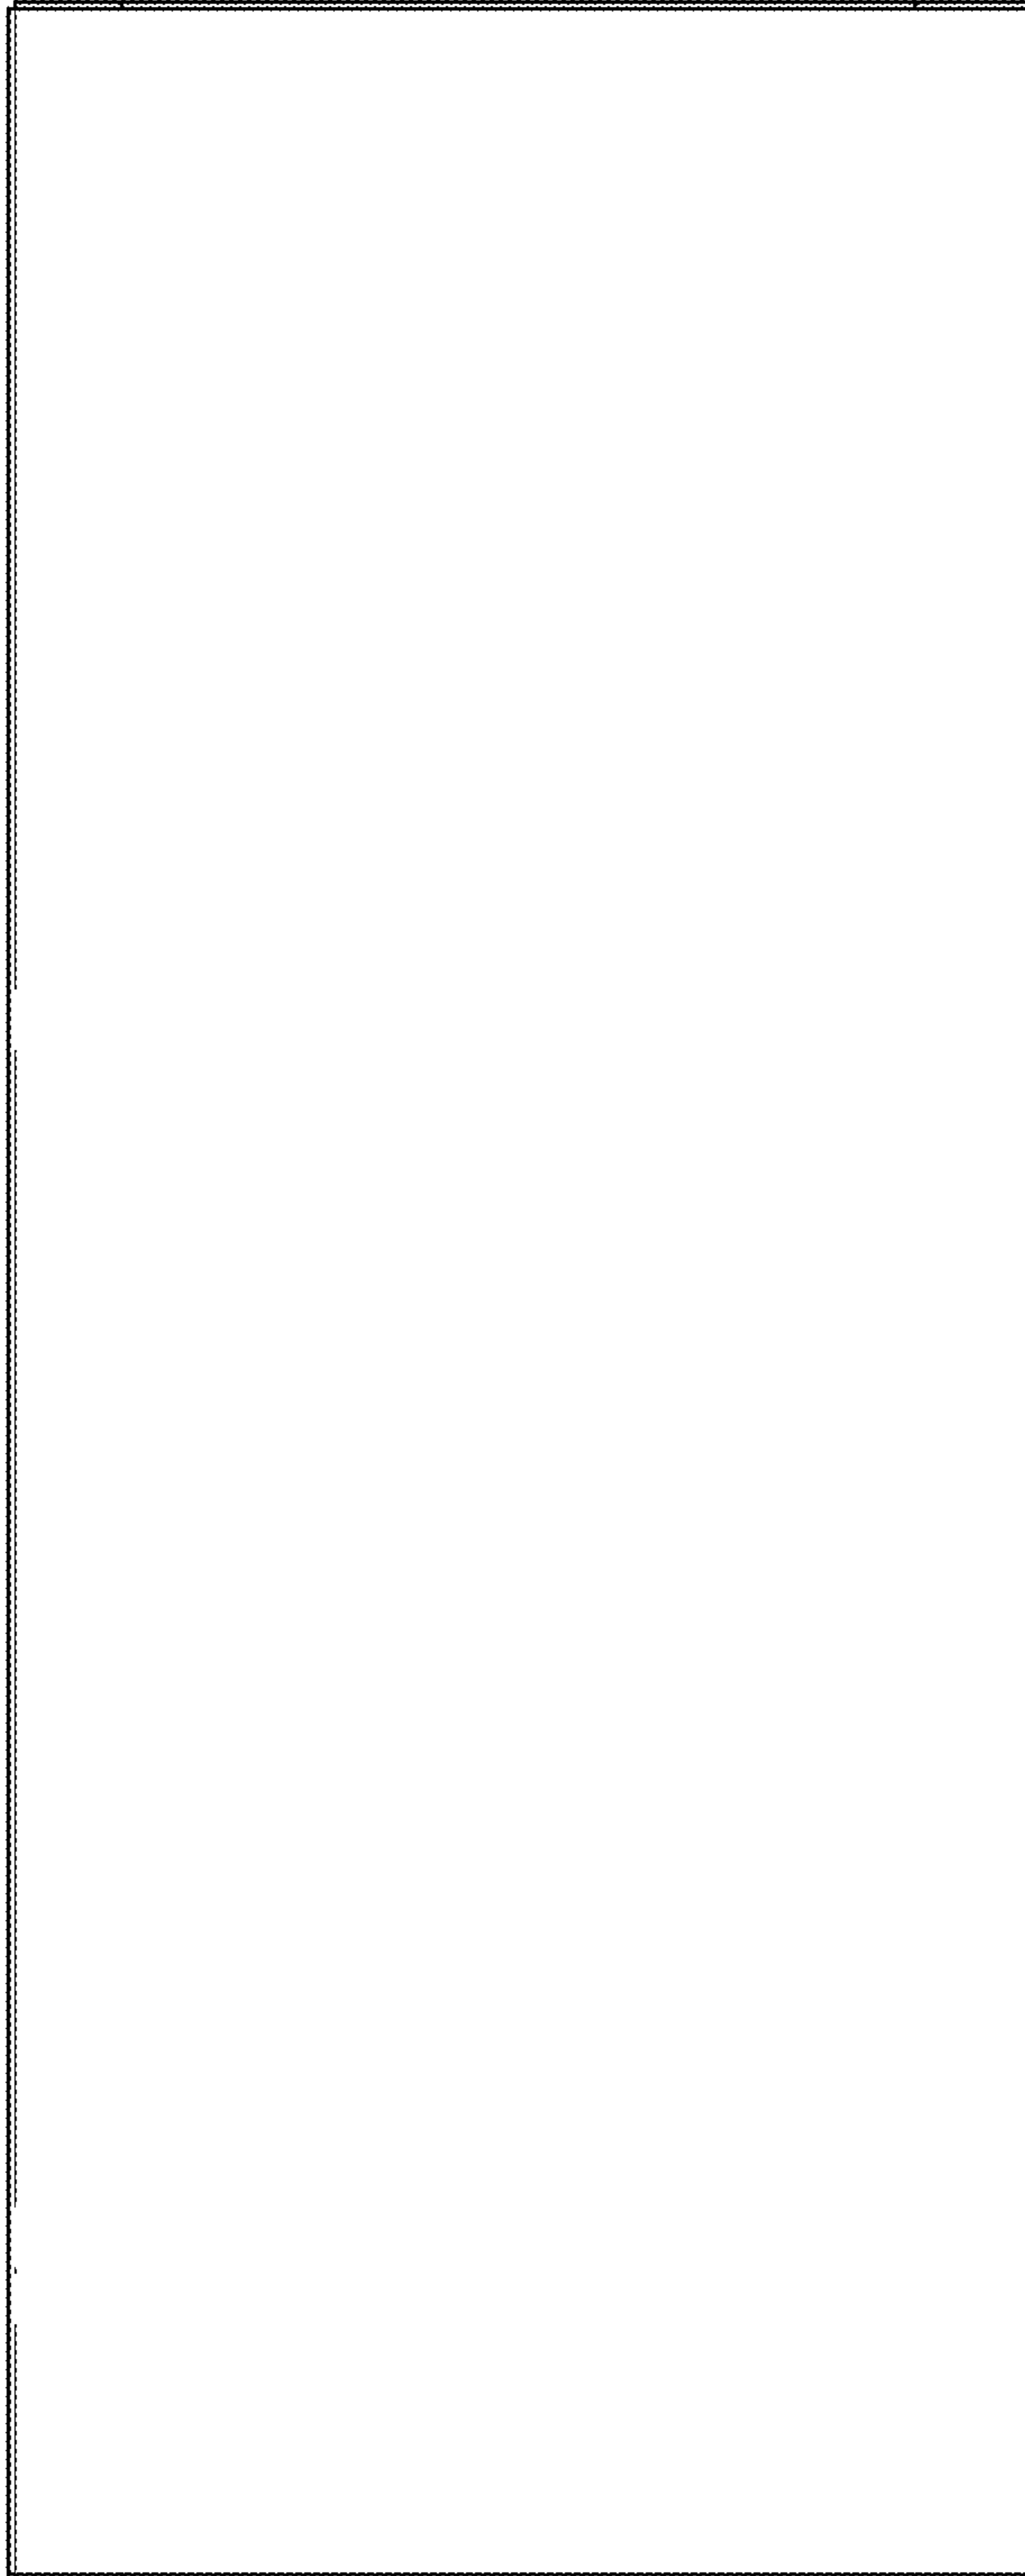


FIG. 7

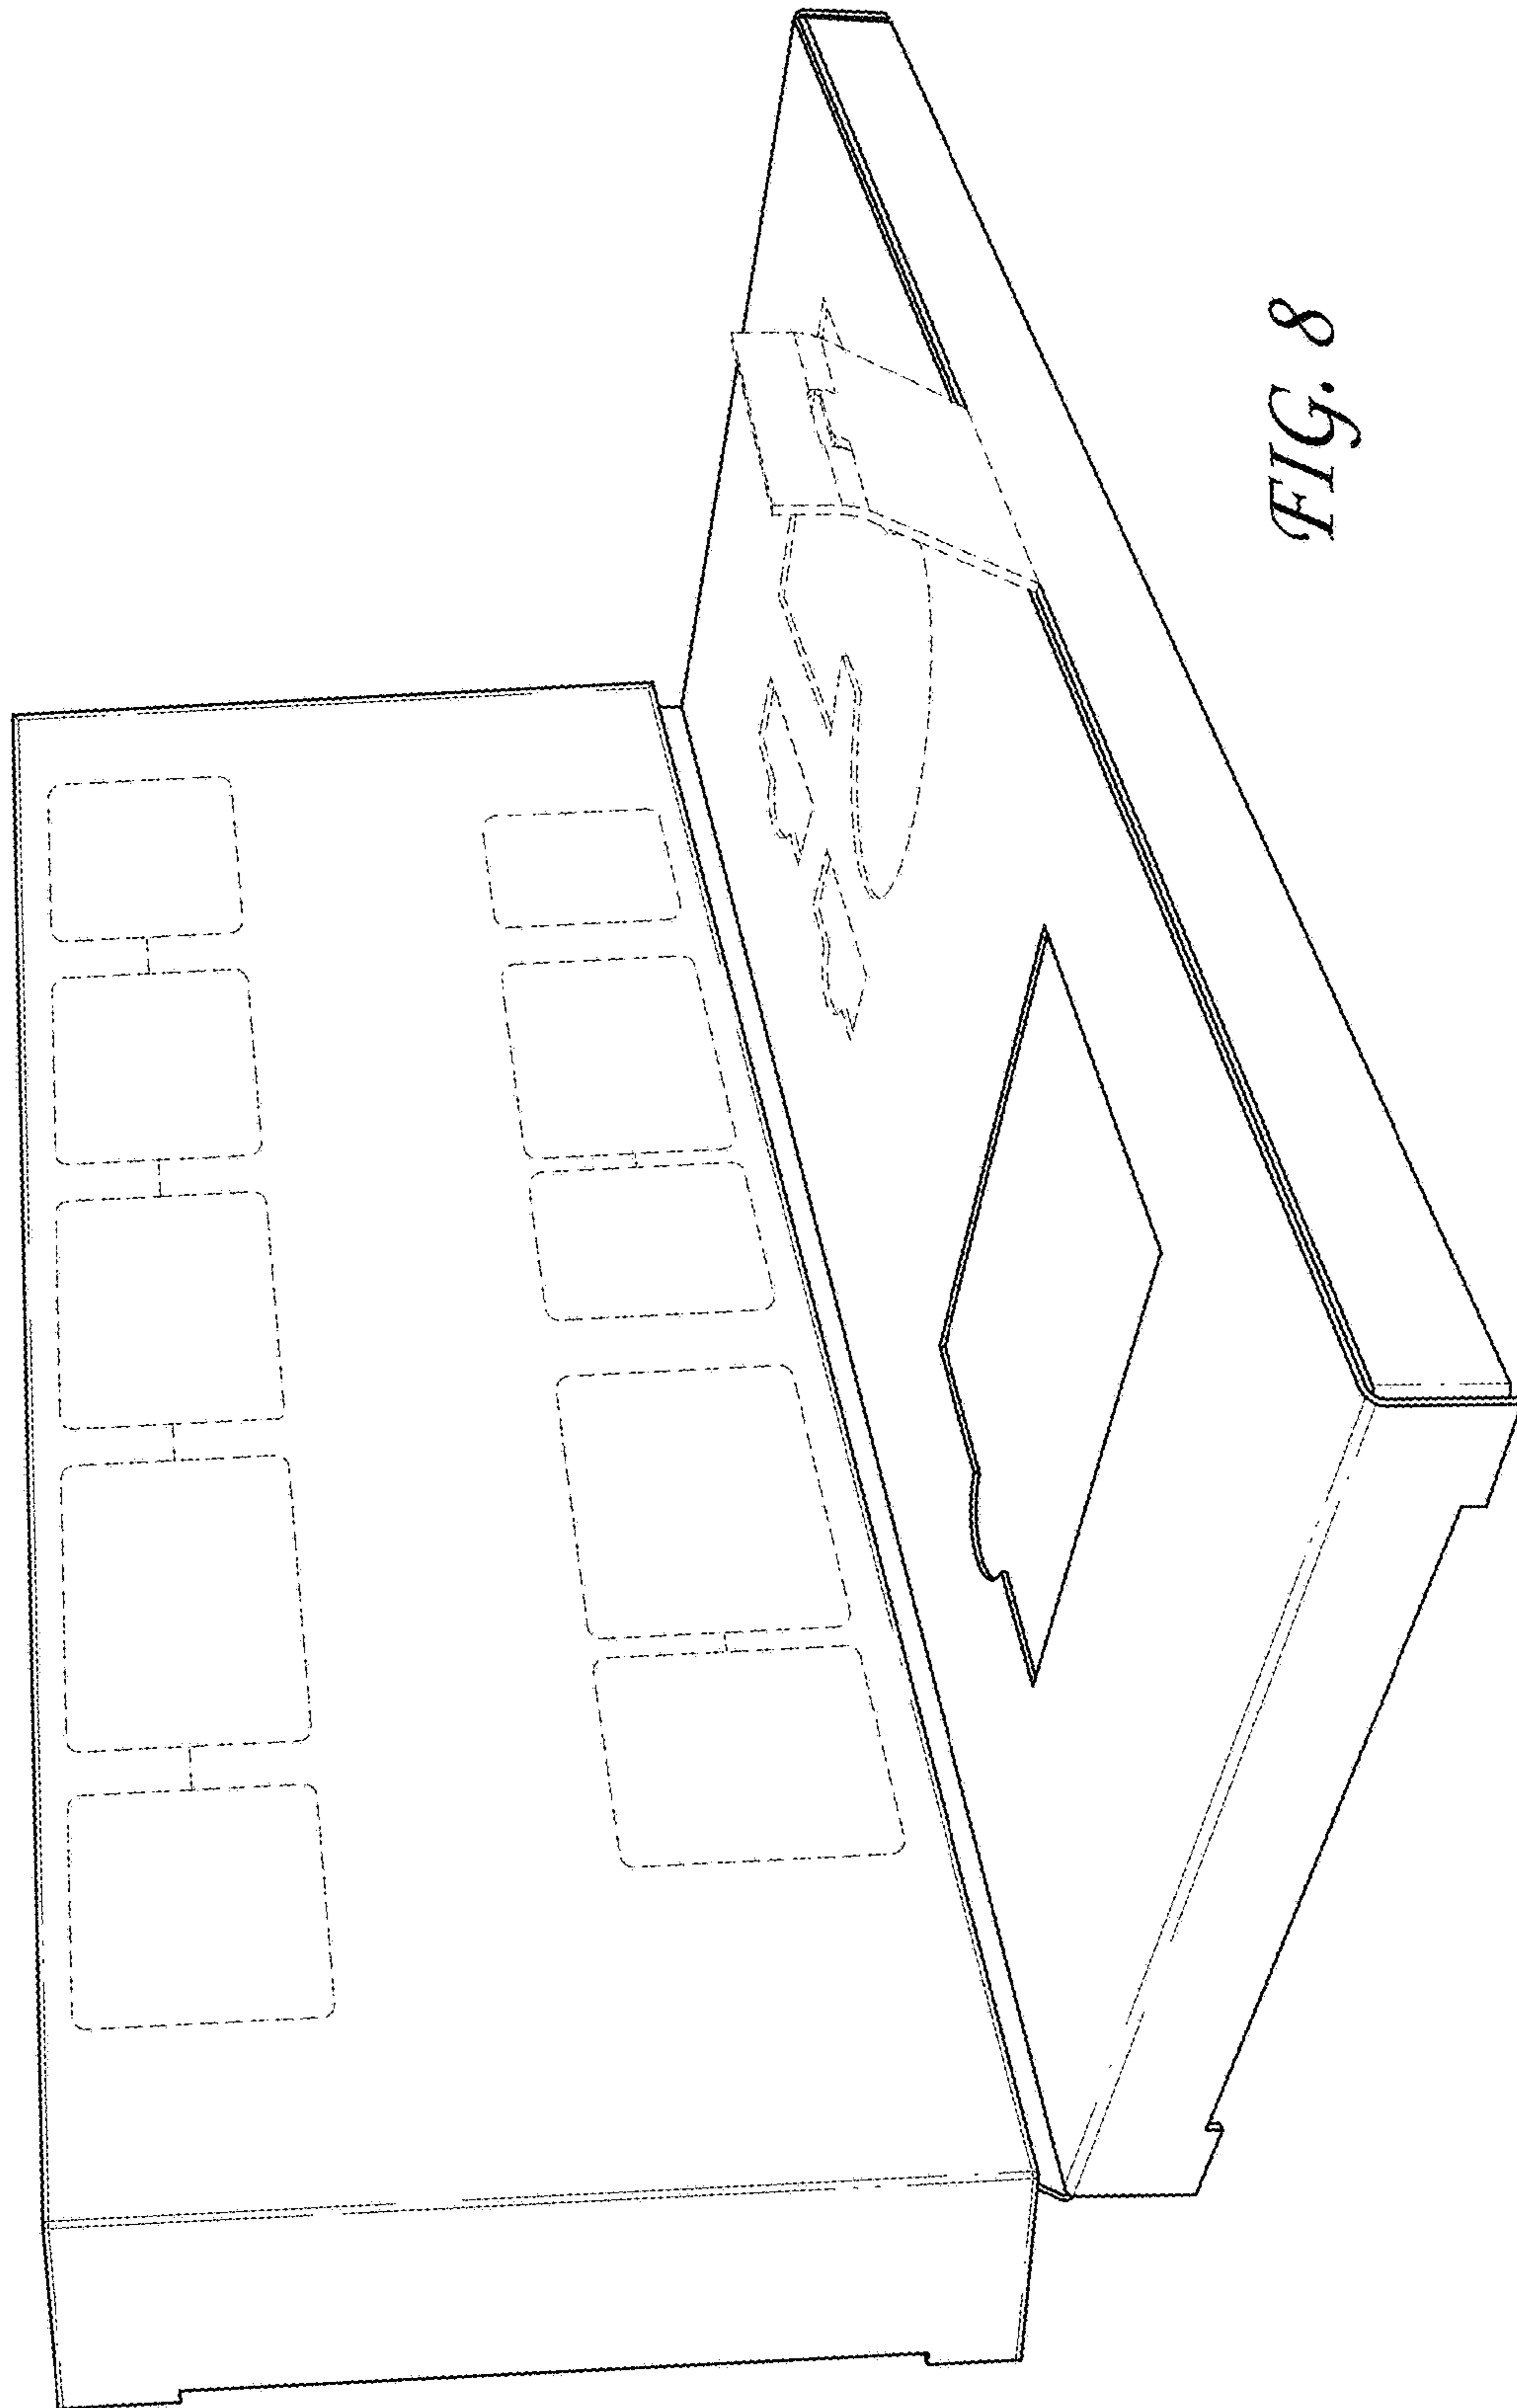


FIG. 8

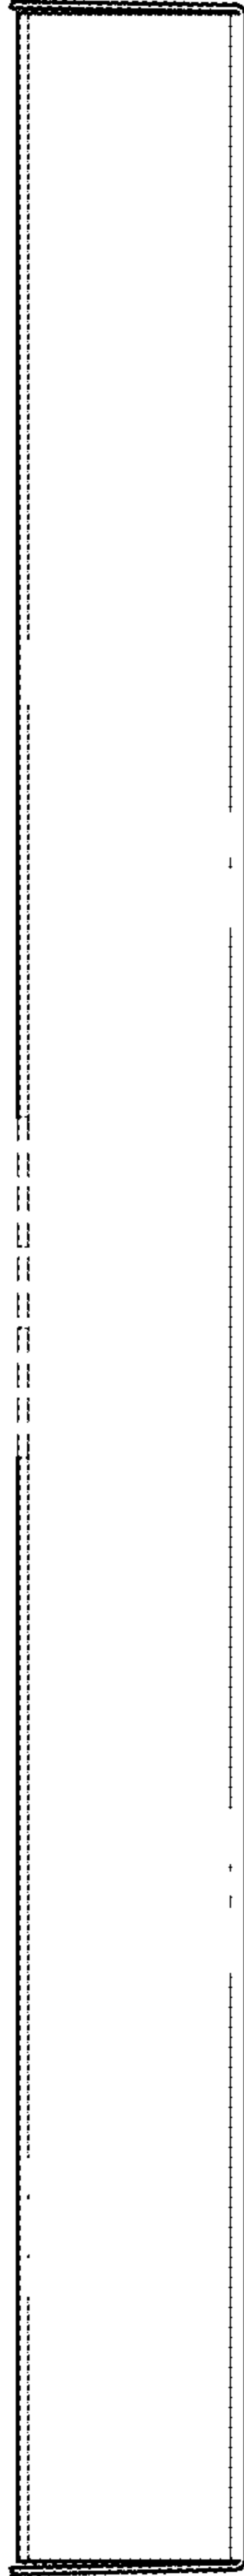


FIG. 9

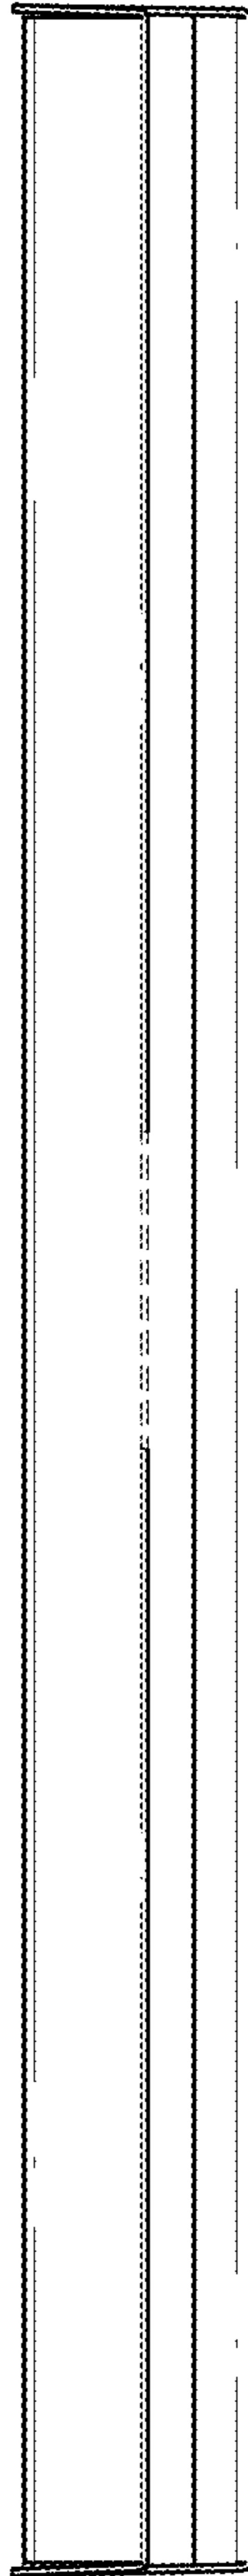


FIG. 10

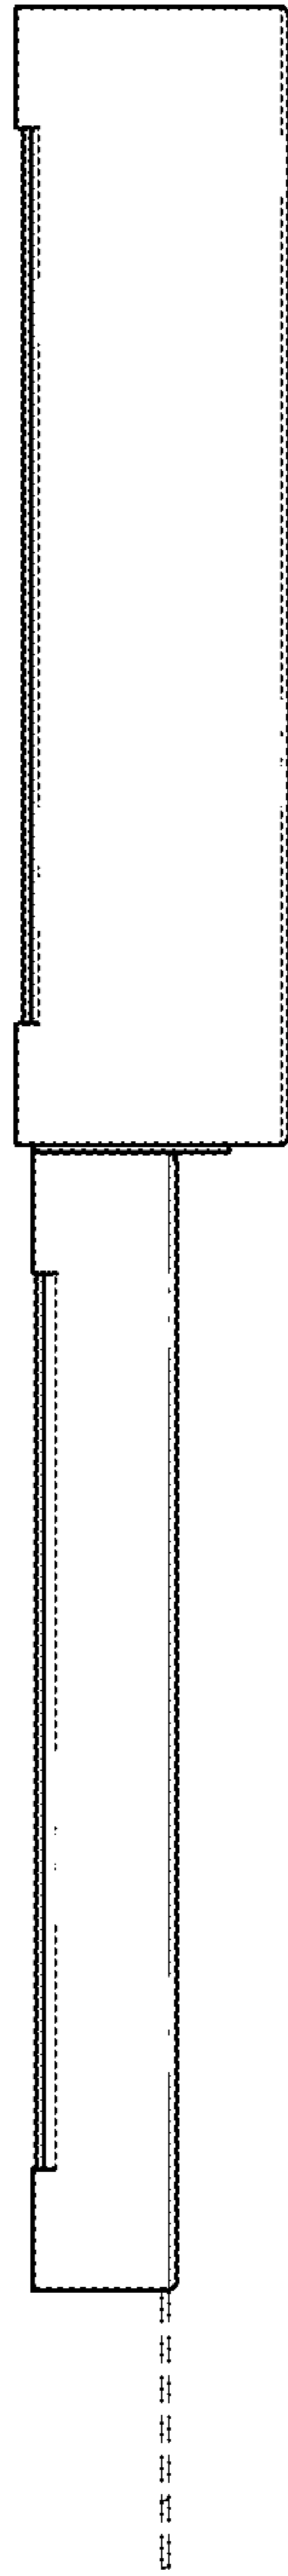


FIG. 11

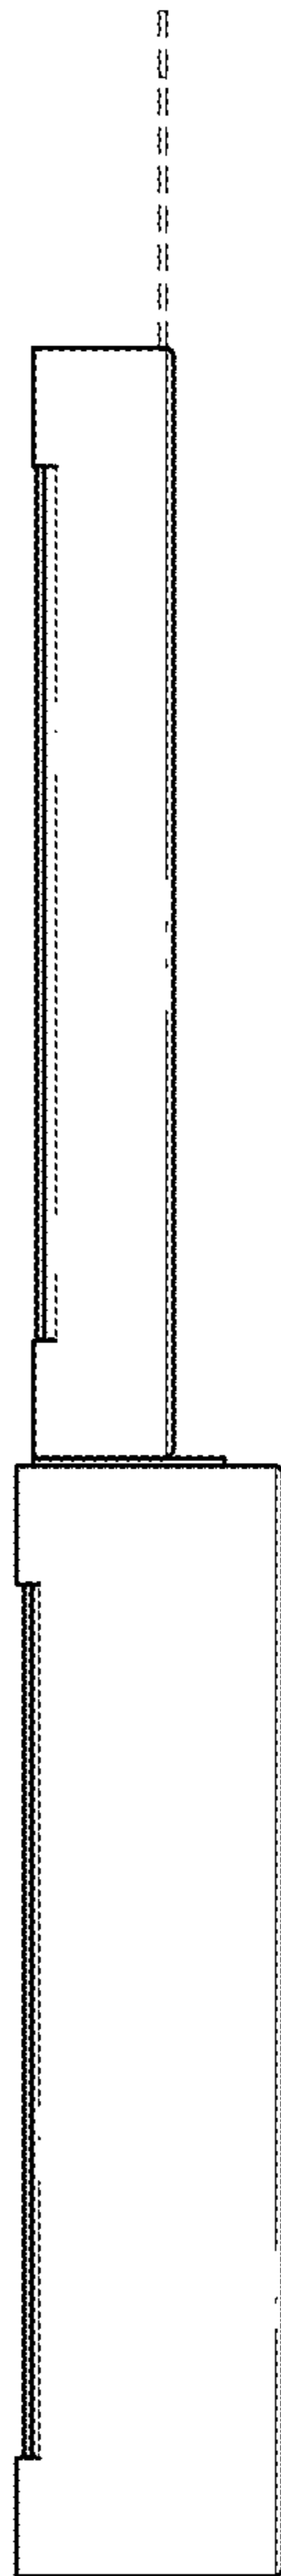


FIG. 12

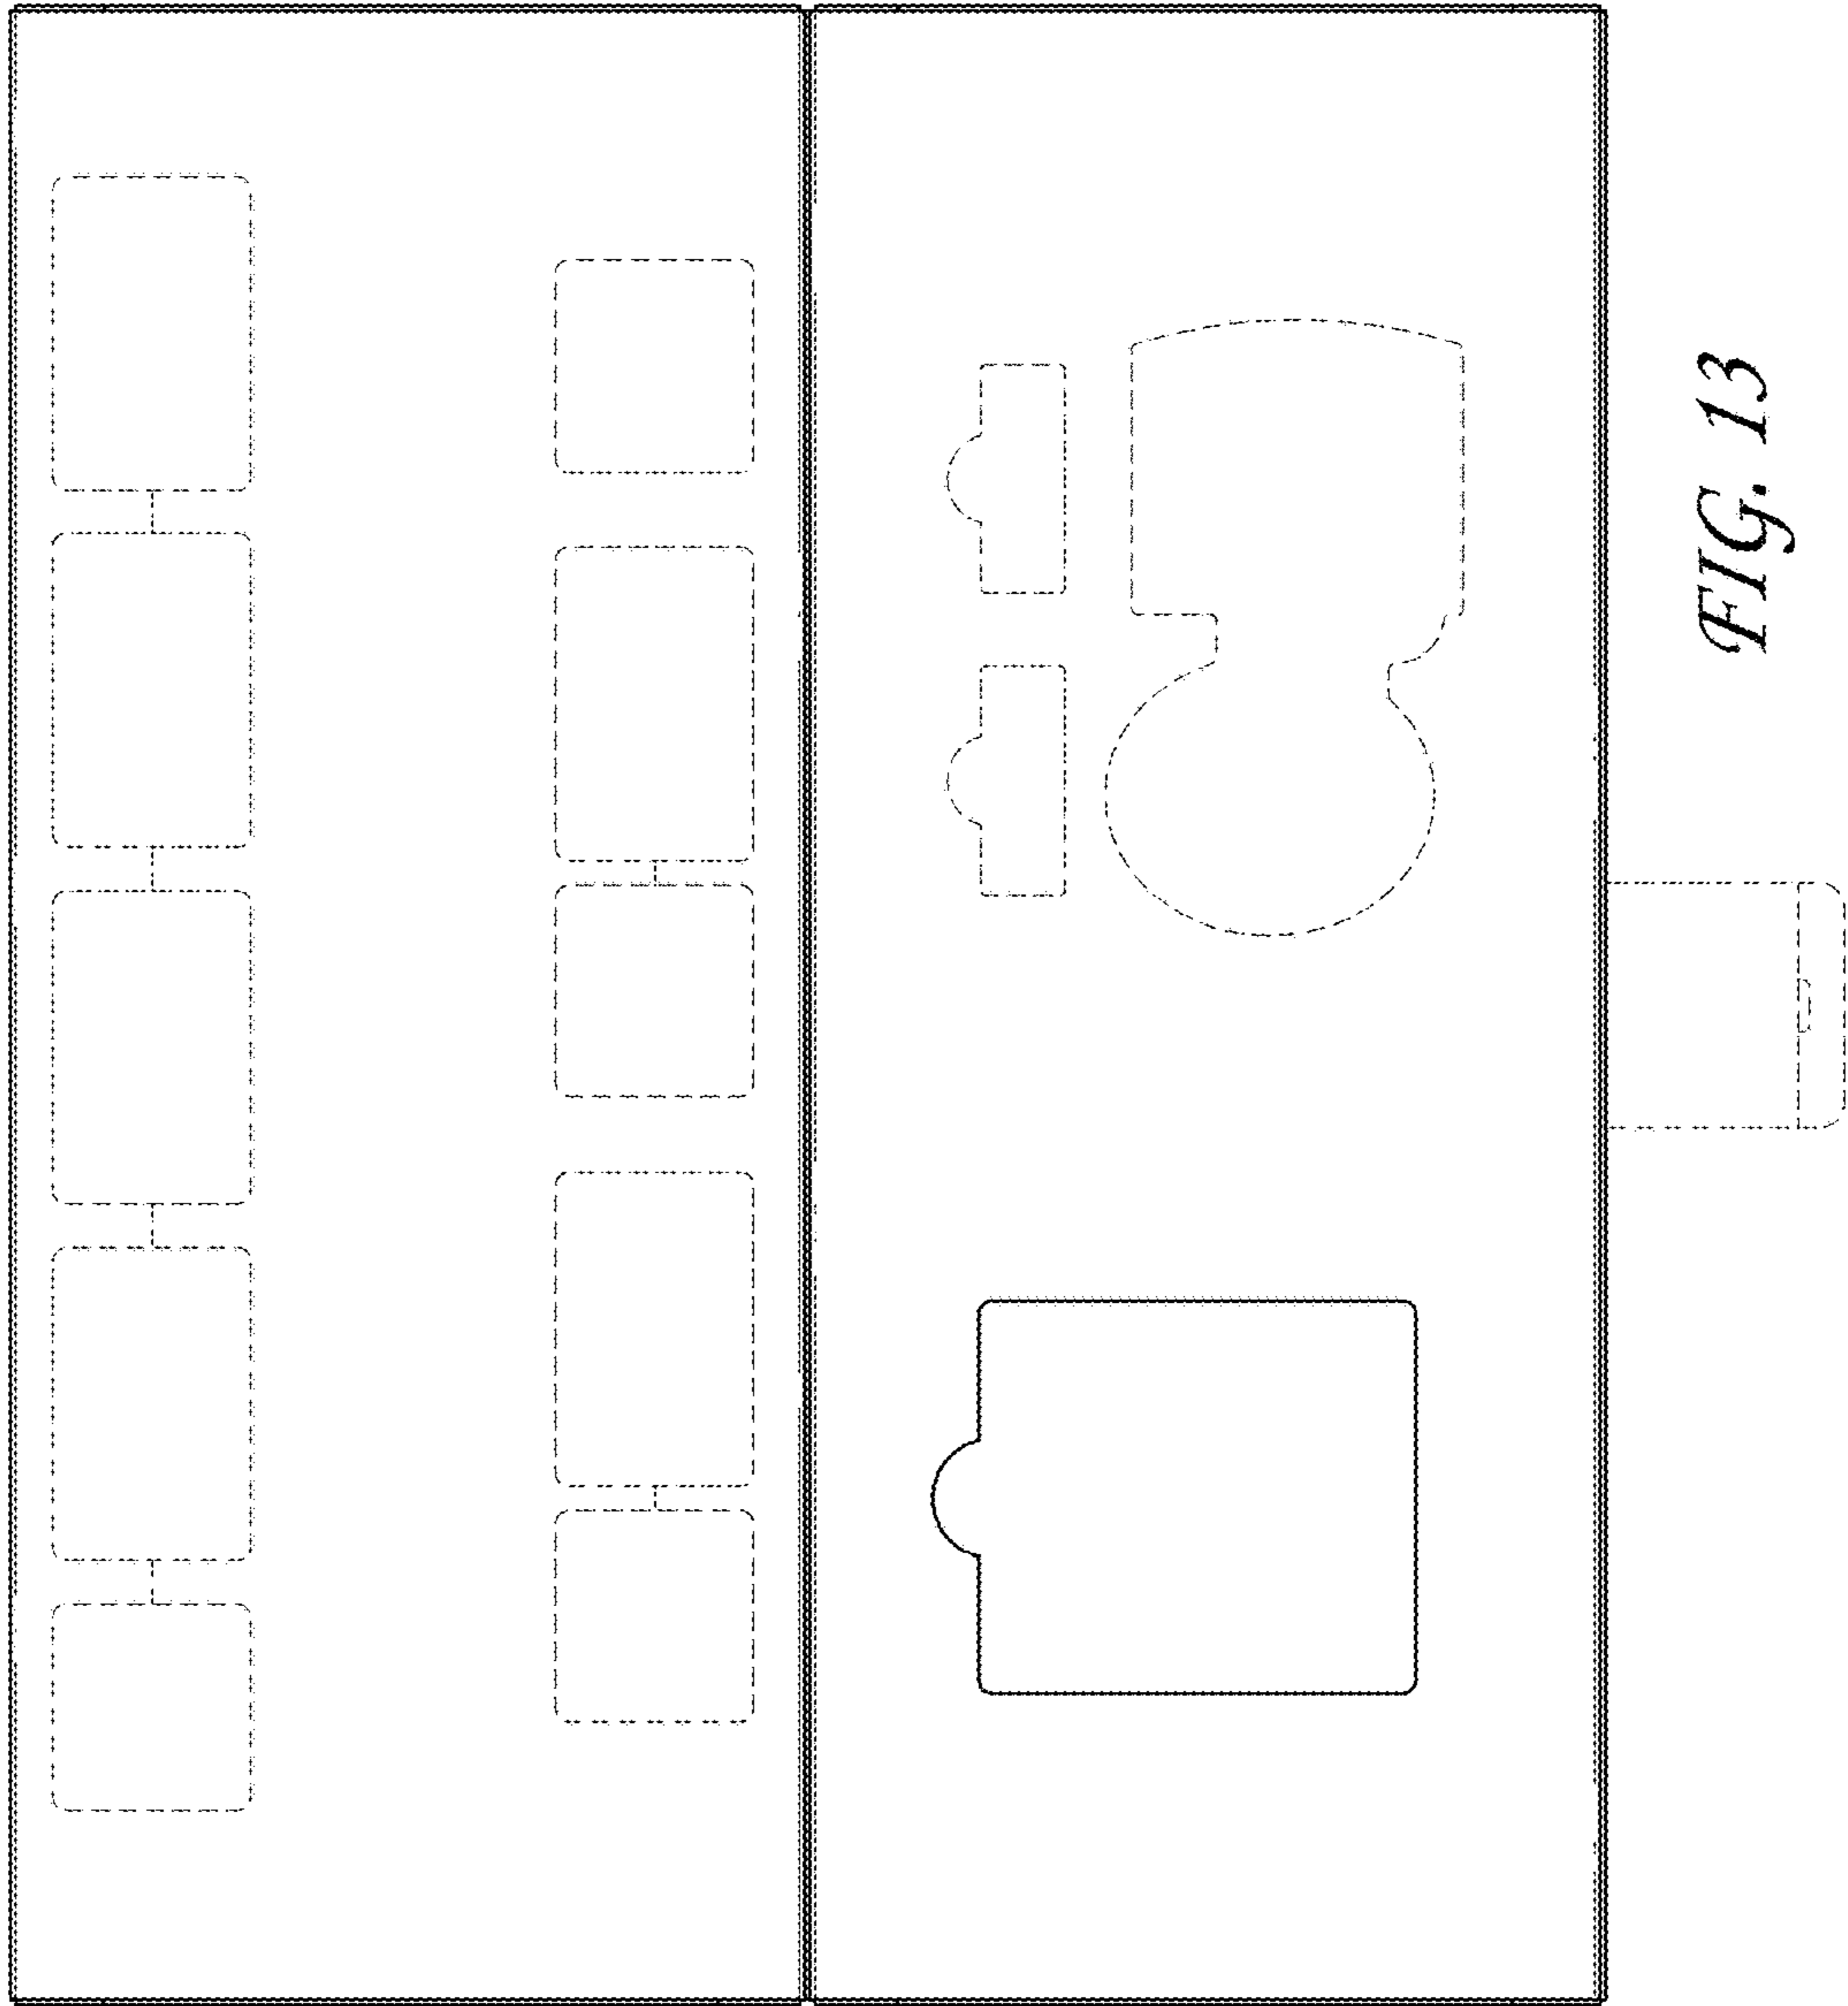


FIG. 13

FIG. 14

