



US00D799042S

(12) **United States Design Patent** (10) **Patent No.:** **US D799,042 S**
Perkins et al. (45) **Date of Patent:** **** Oct. 3, 2017**

(54) **ORTHOPEDIC IMPLANT SIZING DEVICE**

(56) **References Cited**

(71) Applicant: **BioMedical Enterprises, Inc.**, San Antonio, TX (US)

U.S. PATENT DOCUMENTS

(72) Inventors: **Luke A. Perkins**, Bulverde, TX (US);
Adam T. Knight, San Antonio, TX (US); **John K. Ellington**, Charlotte, NC (US)

2,788,816	A	*	4/1957	Dargols	B25B 13/56
						7/165
D197,915	S	*	4/1964	Ayars	7/164
3,191,649	A	*	6/1965	Dzus	B25B 15/00
						81/439
D229,390	S	*	11/1973	Hart	D8/85
D302,514	S	*	8/1989	Gates	D8/105
D344,664	S	*	3/1994	Malkinson	D8/85
D486,051	S	*	2/2004	Parry	D8/82
D634,010	S	*	3/2011	DeCarlo	D24/133
D652,144	S	*	1/2012	Stotland	D24/140
D755,964	S	*	5/2016	Freudenthal	D24/140

(73) Assignee: **BioMedical Enterprises, Inc.**, San Antonio, TX (US)

(**) Term: **15 Years**

* cited by examiner

(21) Appl. No.: **29/590,424**

Primary Examiner — Charles Hanson

(22) Filed: **Jan. 10, 2017**

(74) *Attorney, Agent, or Firm* — Christopher L. Makay

Related U.S. Application Data

(62) Division of application No. 29/513,531, filed on Dec. 31, 2014, now Pat. No. Des. 780,312.

(51) **LOC (10) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/155**

(58) **Field of Classification Search**
USPC D24/155–157, 140; D8/85, 26
CPC A61B 17/0642; A61B 17/0682; A61B 17/0644; A61B 90/06; A61B 2090/061; B25B 15/00; A61F 2/4657; A61F 2002/4668; A61F 2002/4658; A61F 2220/0025

See application file for complete search history.


(57) **CLAIM**

The ornamental design for an orthopedic implant sizing device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view illustrating the orthopedic implant sizing device showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a left side elevational view thereof; FIG. 5 is a right side elevational view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof. The broken lines shown in FIGS. 1-7 represent additional portions of the orthopedic implant sizing device that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

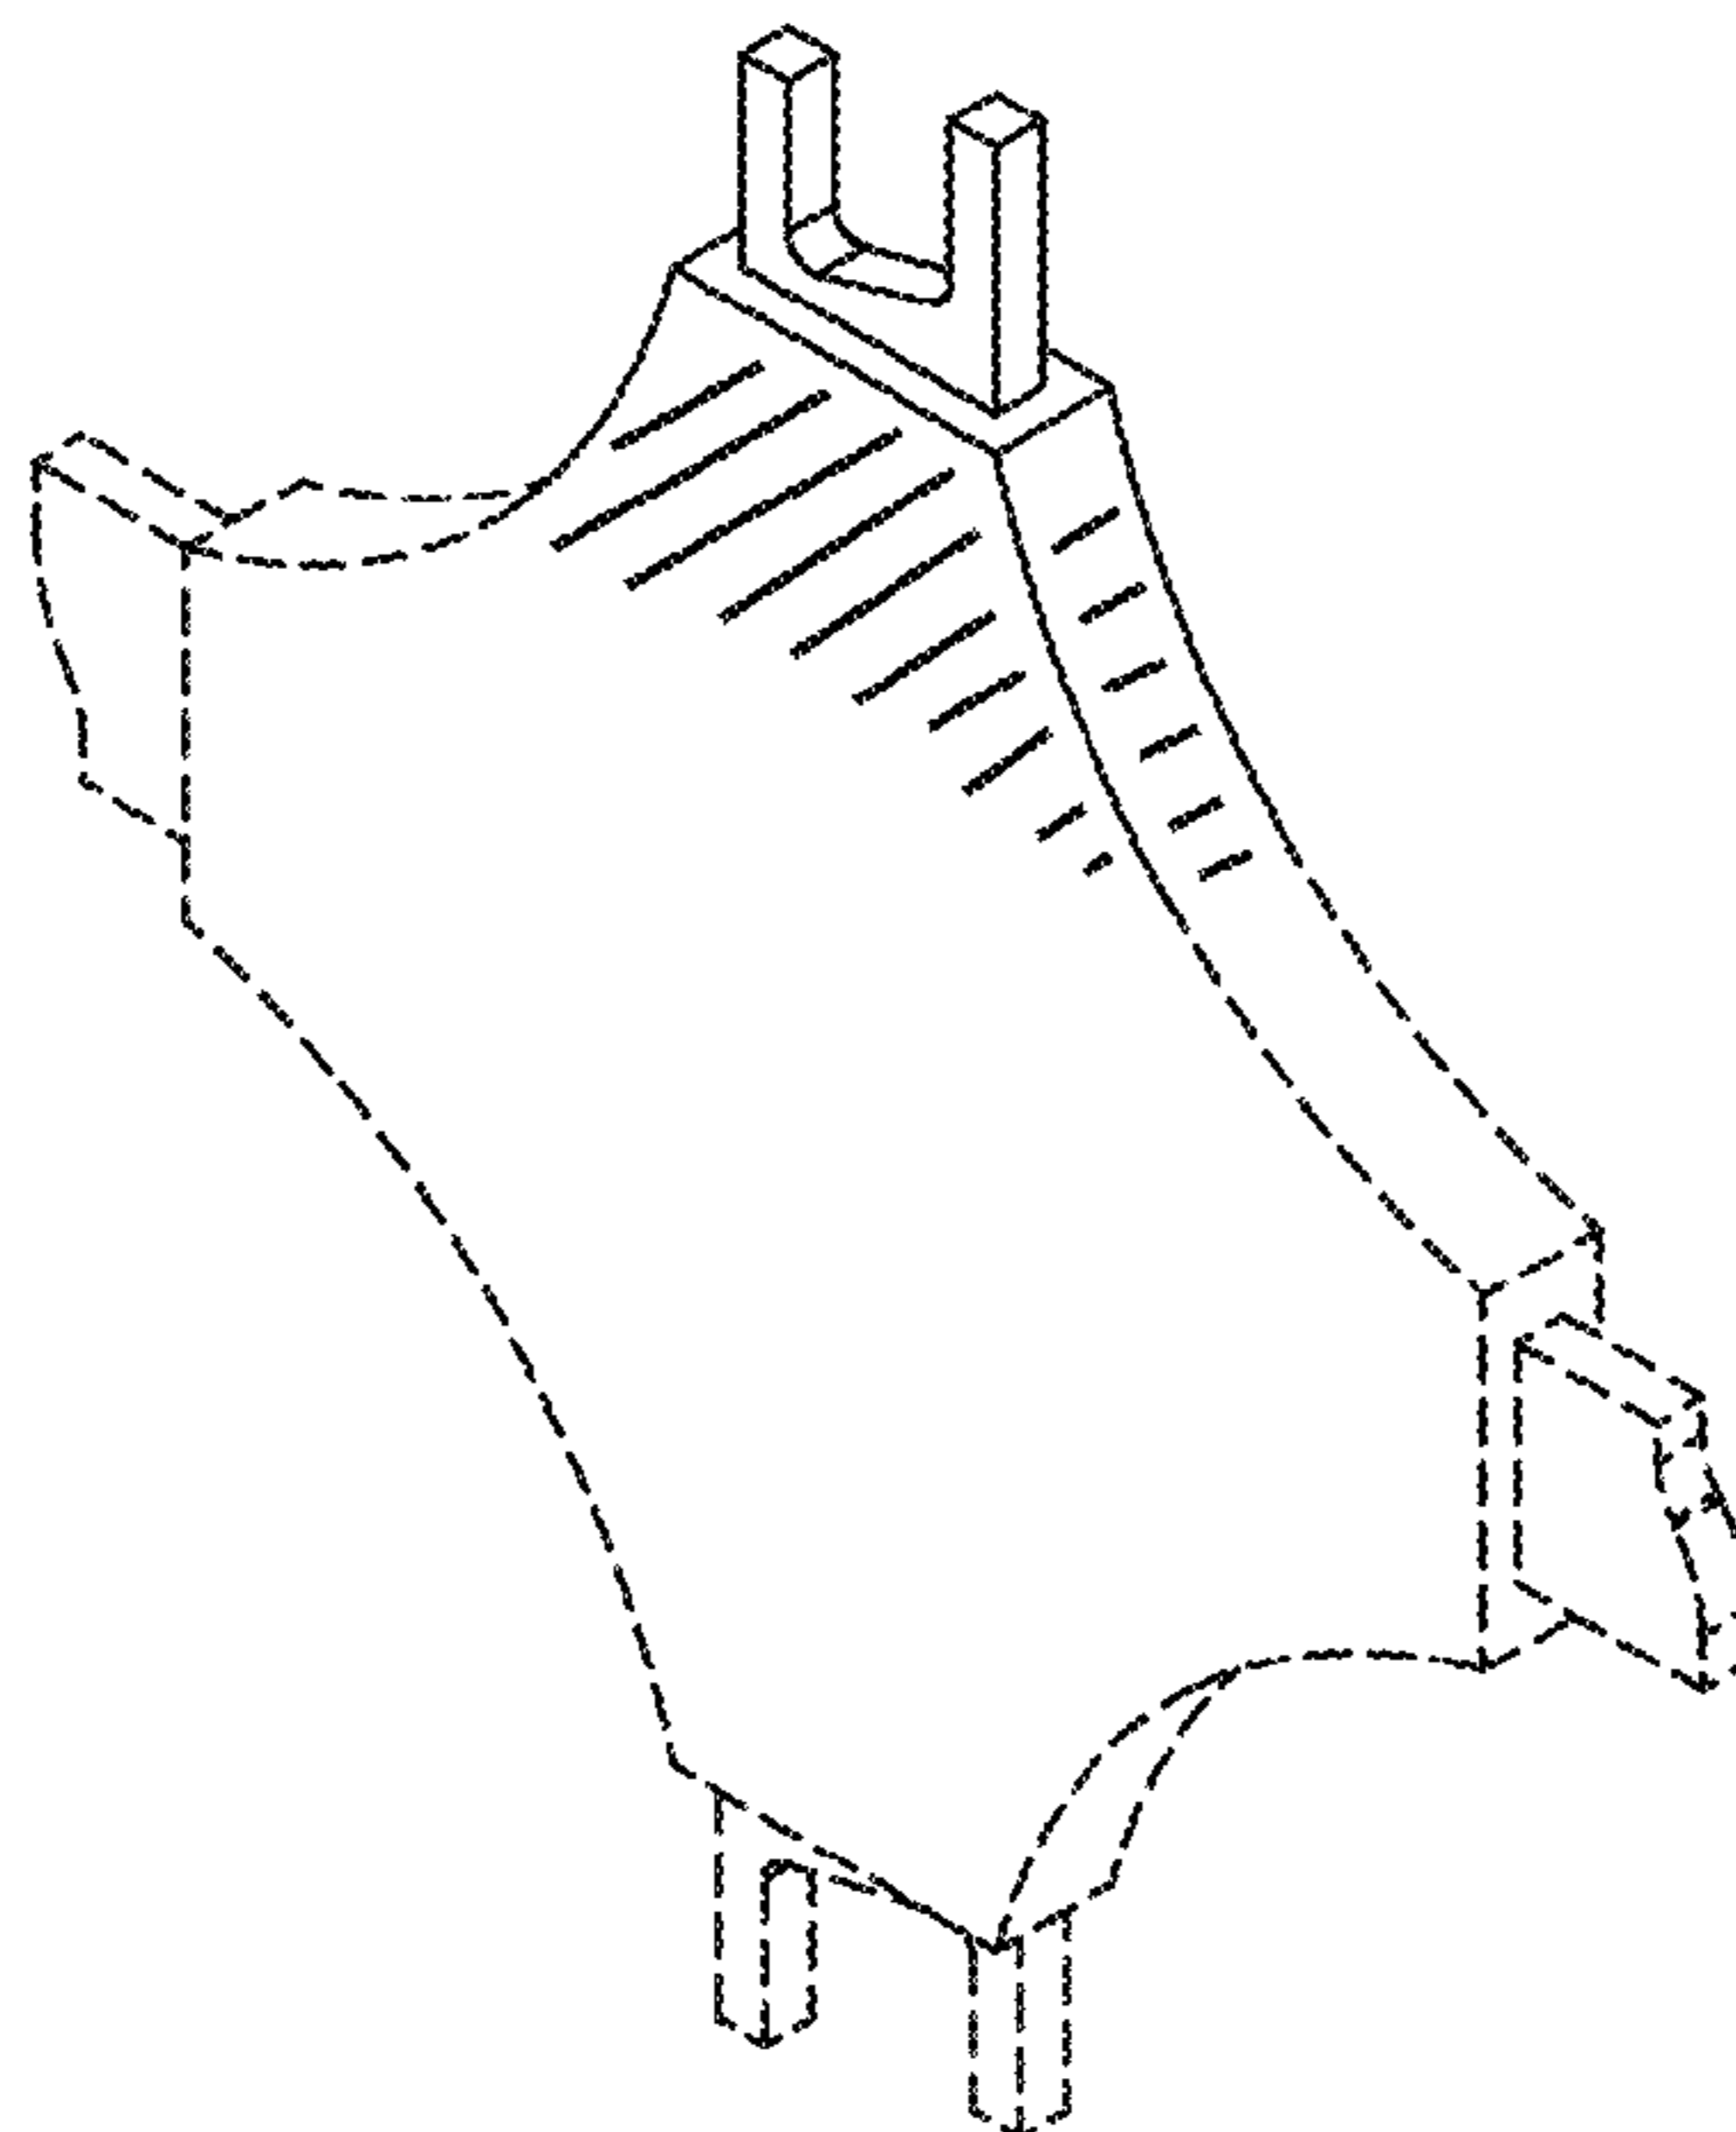

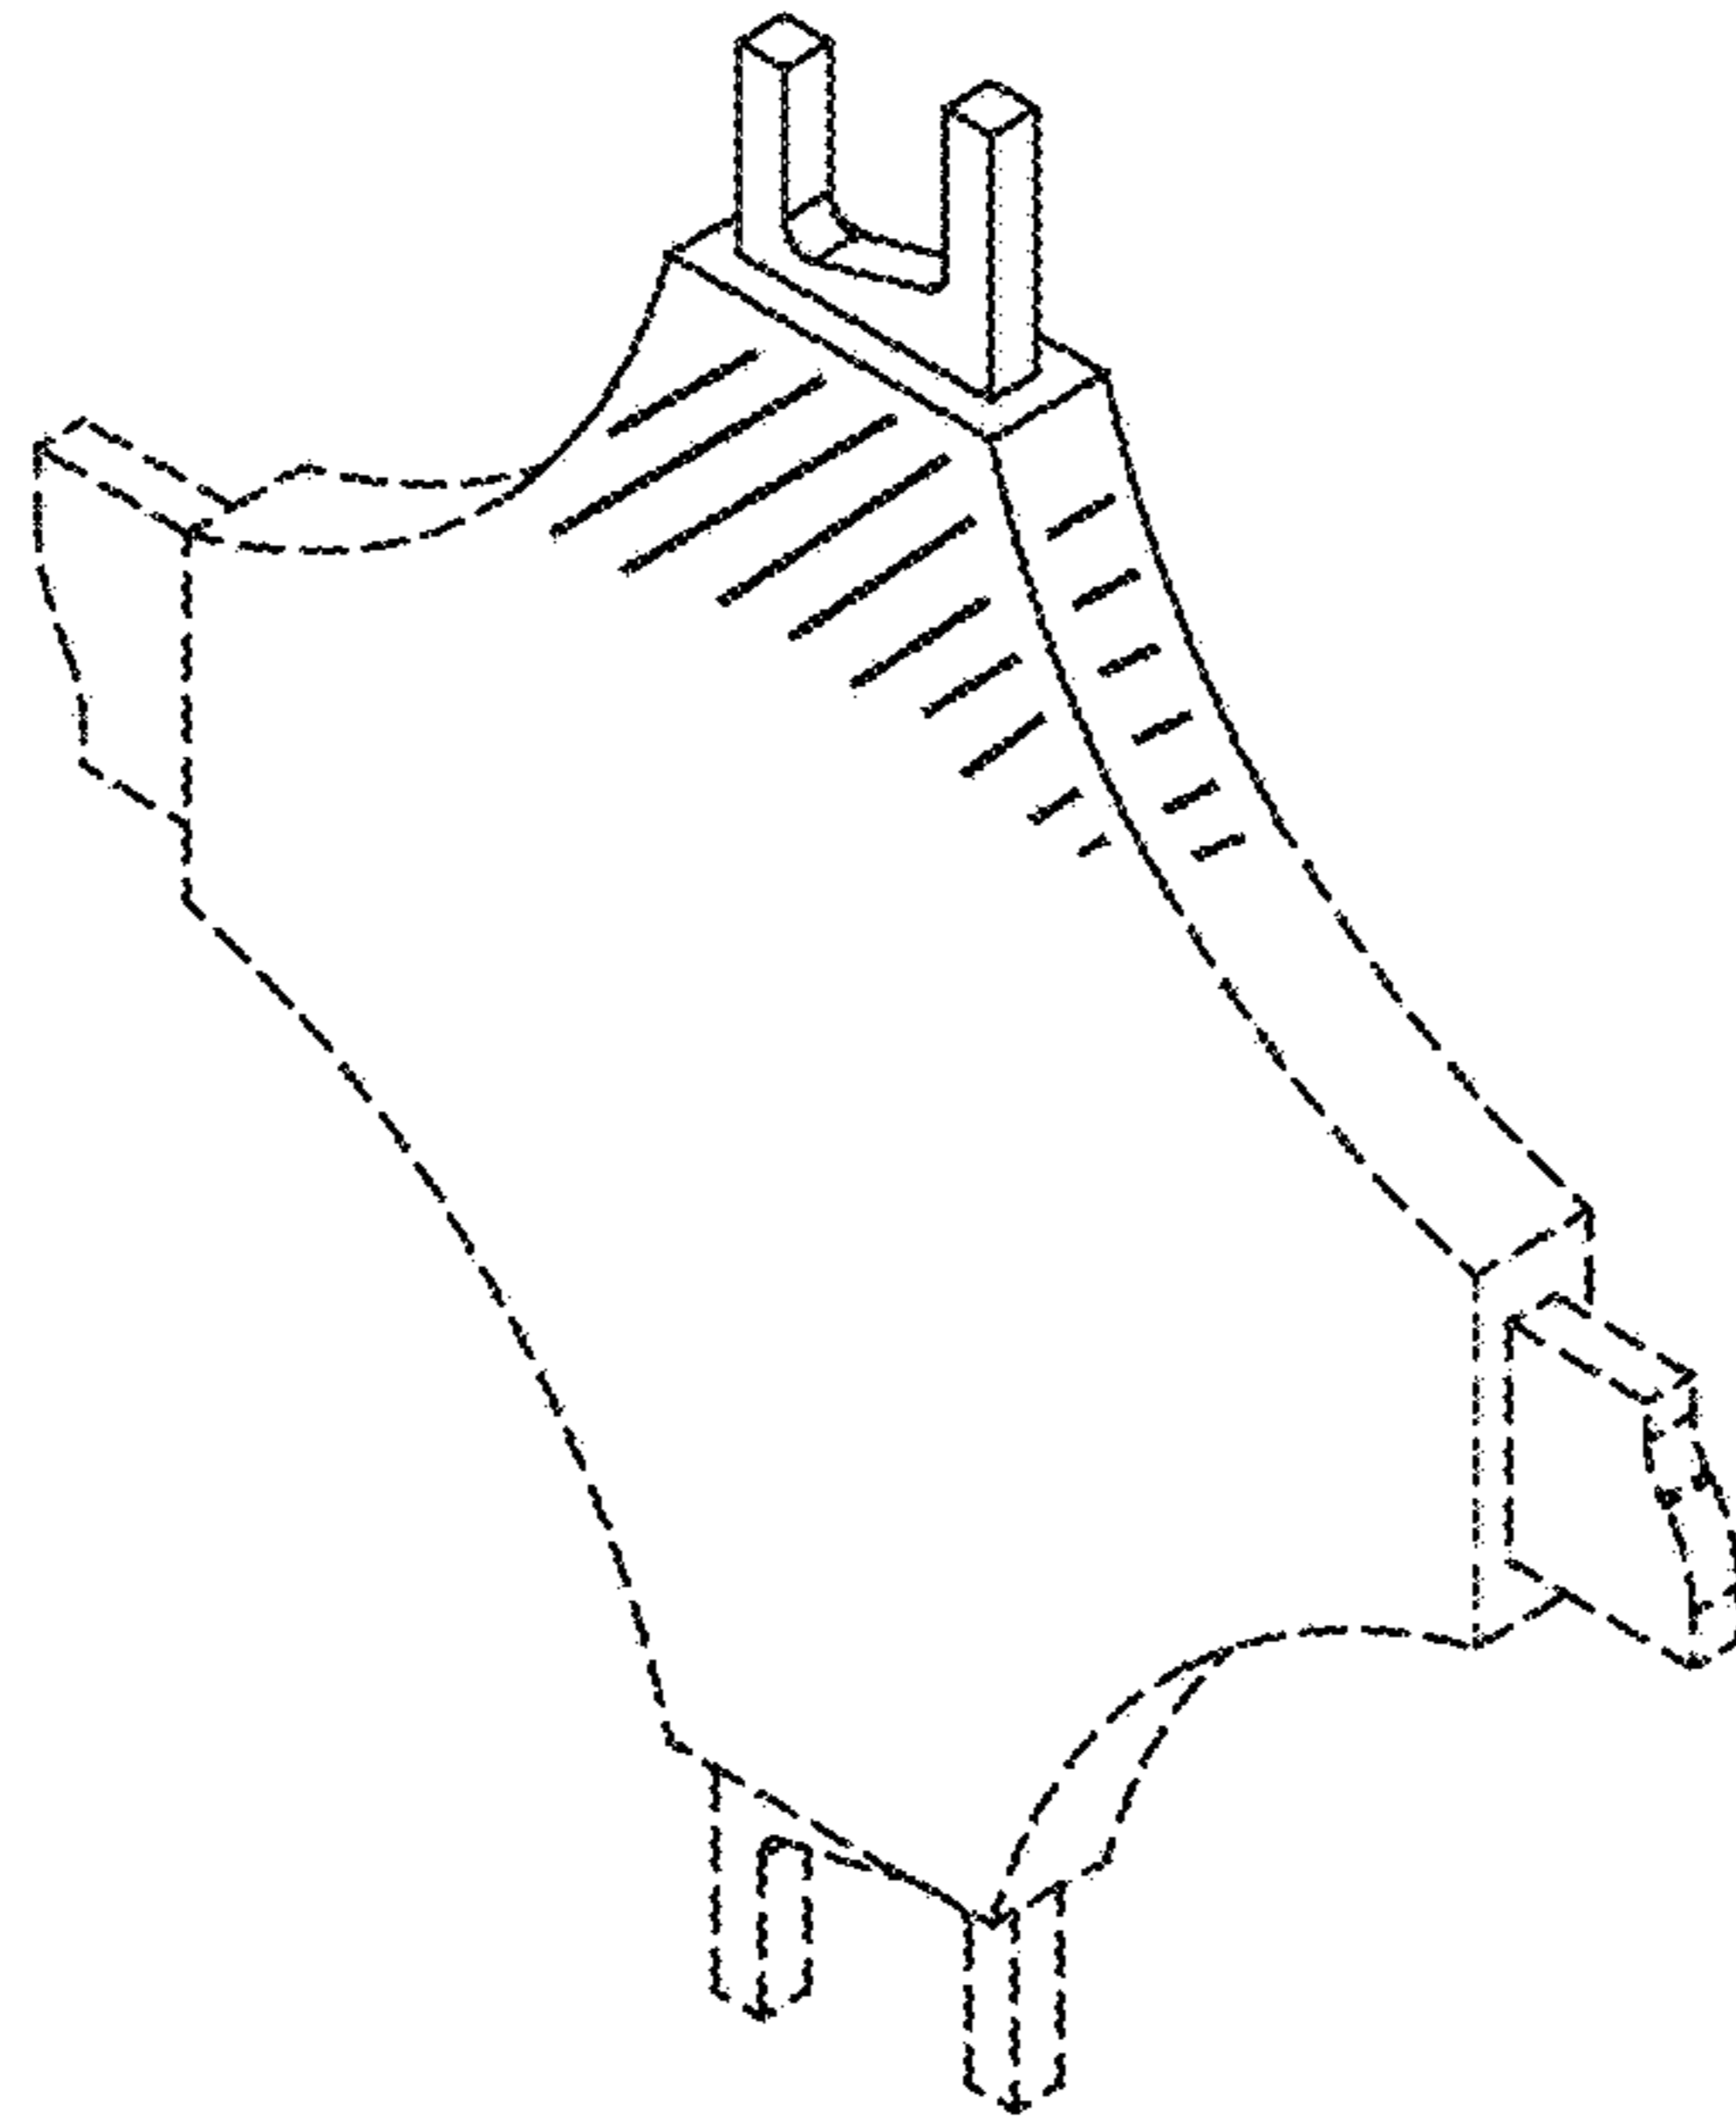


FIG. 1

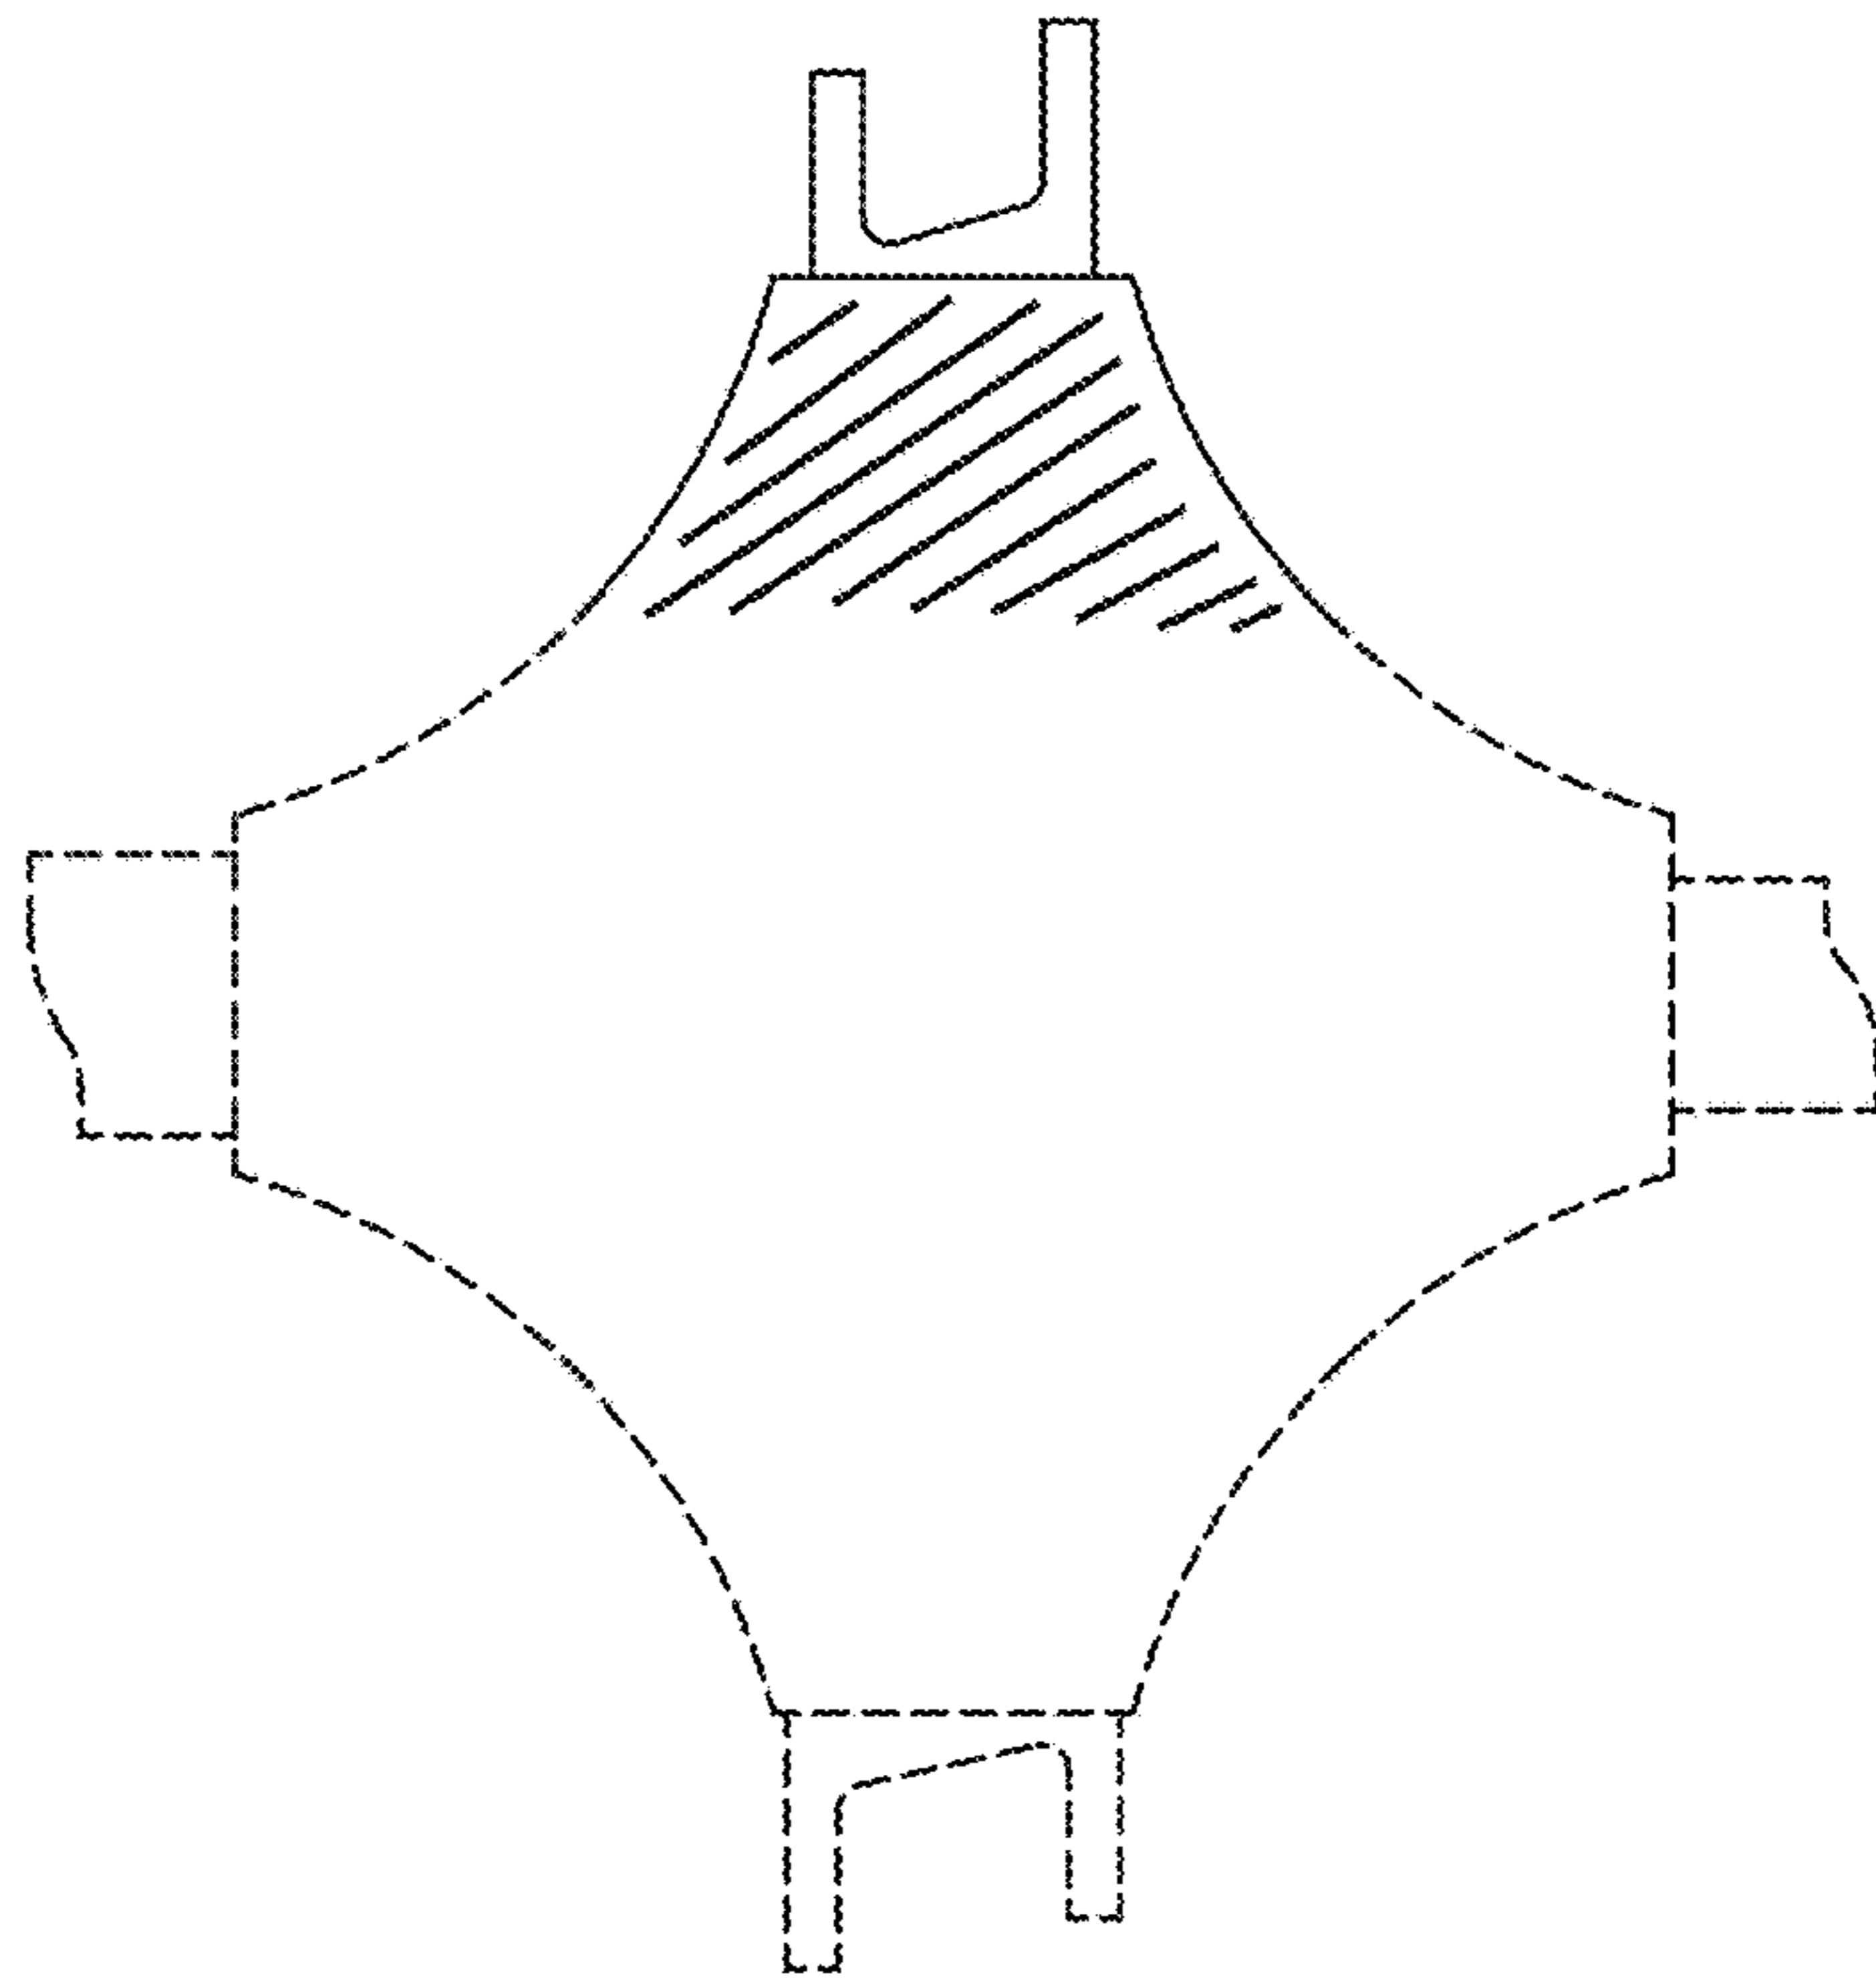


FIG. 2

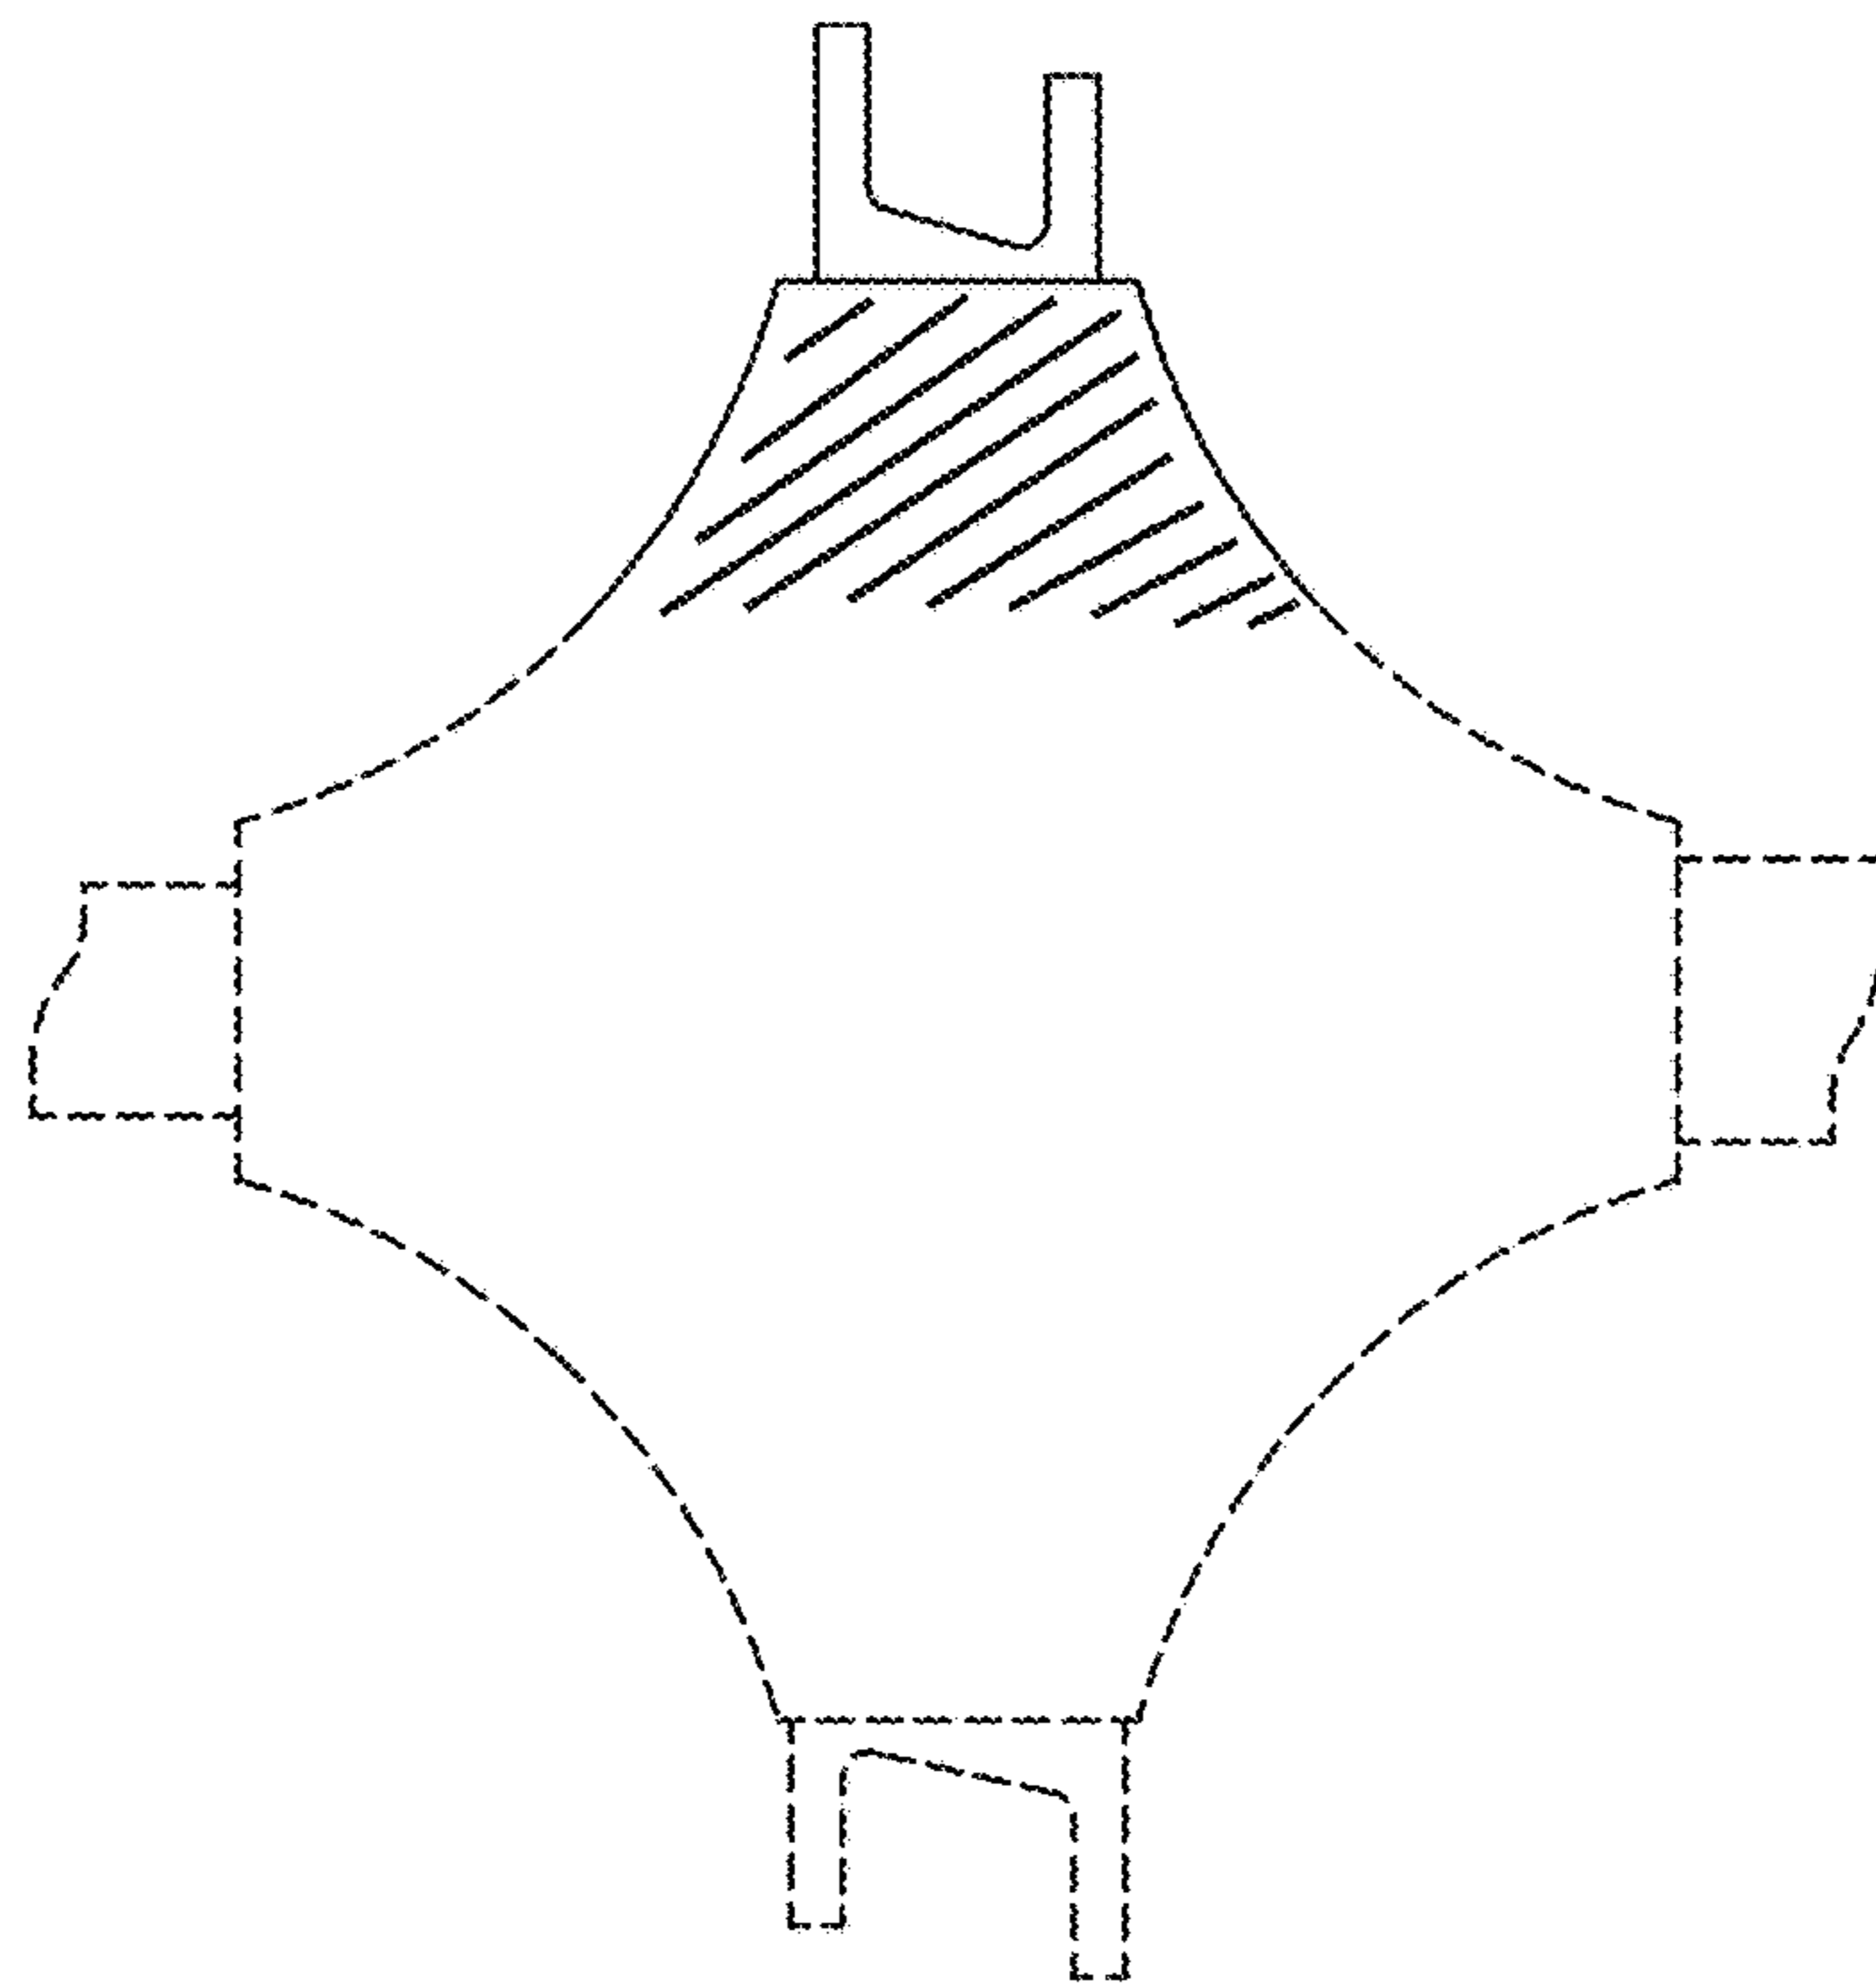


FIG. 3

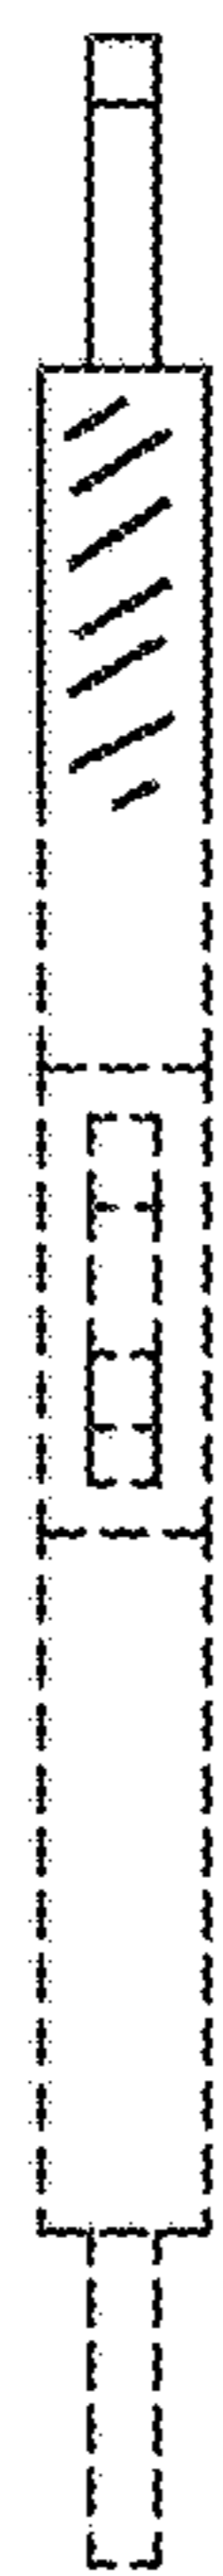


FIG. 4

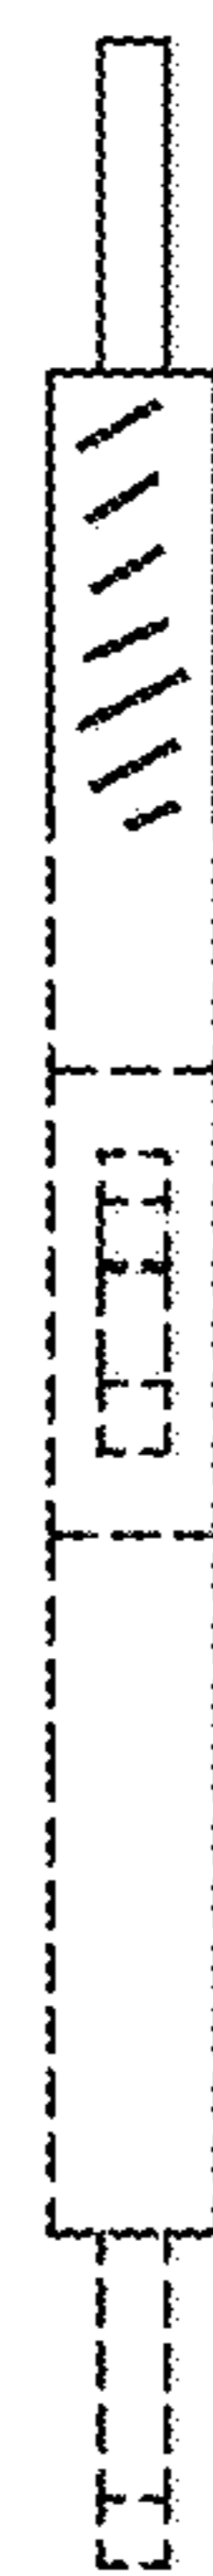


FIG. 5

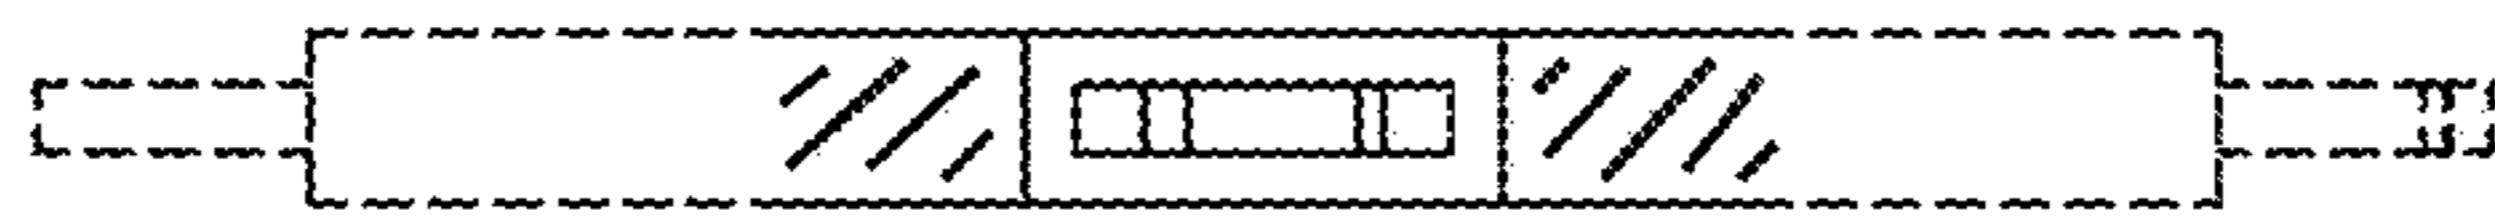


FIG. 6

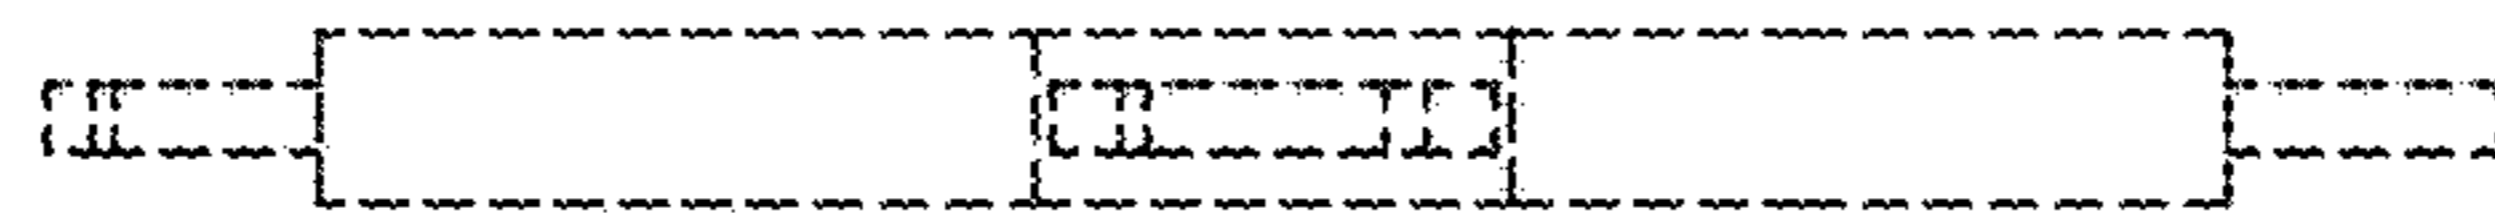


FIG. 7