



US00D799999S

(12) **United States Design Patent** (10) **Patent No.:** **US D799,999 S**
Barton et al. (45) **Date of Patent:** **** Oct. 17, 2017**

(54) **DIAGNOSTIC ANALYZER**

- (71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)
- (72) Inventors: **Christina A Barton**, Irving, TX (US); **Daniel Roger Nett**, Sun Prairie, WI (US); **Rachel Elizabeth Wallace**, Madison, WI (US); **Ami Marie Verhalen**, Sun Prairie, WI (US); **Christopher Alan Harris**, Madison, WI (US)
- (73) Assignee: **ABBOTT LABORATORIES**, Abbott Park, IL (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/549,332**
- (22) Filed: **Dec. 21, 2015**

Related U.S. Application Data

- (63) Continuation-in-part of application No. 29/531,576, filed on Jun. 26, 2015, now Pat. No. Des. 777,048.
- (51) **LOC (10) Cl.** **10-04**
- (52) **U.S. Cl.** USPC **D10/81; D24/216**
- (58) **Field of Classification Search**
USPC D24/216–219, 231, 232, 233, 107, 169, D24/186; D10/81
CPC G01N 21/00; G01N 21/01; G01N 2021/0106; G01N 2201/022; G01N 2201/0221; G01N 2201/0222; G01N
- (Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D347,396 S 5/1994 Ohnuma et al.
D755,405 S 5/2016 Zhu
D773,071 S * 11/2016 Hakoda D10/81

OTHER PUBLICATIONS

Intellectual Property Office of Japan, "Directive," issued in connection with Japanese Design Application No. 2015-28870, dated Oct. 25, 2016, 3 pages.

(Continued)

Primary Examiner — Antoine D Davis*(74) Attorney, Agent, or Firm* — McAndrews, Held & Malloy, Ltd.

(57)

CLAIM

The ornamental design for a diagnostic analyzer, as shown and described.


DESCRIPTION

The file of this patent contains at least one drawing/photograph executed in color. Copies of this patent with color drawings(s)/photograph(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front left perspective view of a first embodiment of a diagnostic analyzer showing our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a front left perspective view of a second embodiment of a diagnostic analyzer showing our new design;
FIG. 4 is a front elevation view thereof;
FIG. 5 is a rear elevation view thereof;
FIG. 6 is a right side elevation view thereof;
FIG. 7 is a left side elevation view thereof;
FIG. 8 is a top plan view thereof; and,
FIG. 9 is a bottom plan view thereof.

It is understood that the only difference between the first and second embodiments is the inclusion of a display screen and associated arm in the second embodiment, it being understood that all other surfaces are the same in the two embodiments.

1 Claim, 6 Drawing Sheets
(4 of 6 Drawing Sheet(s) Filed in Color)

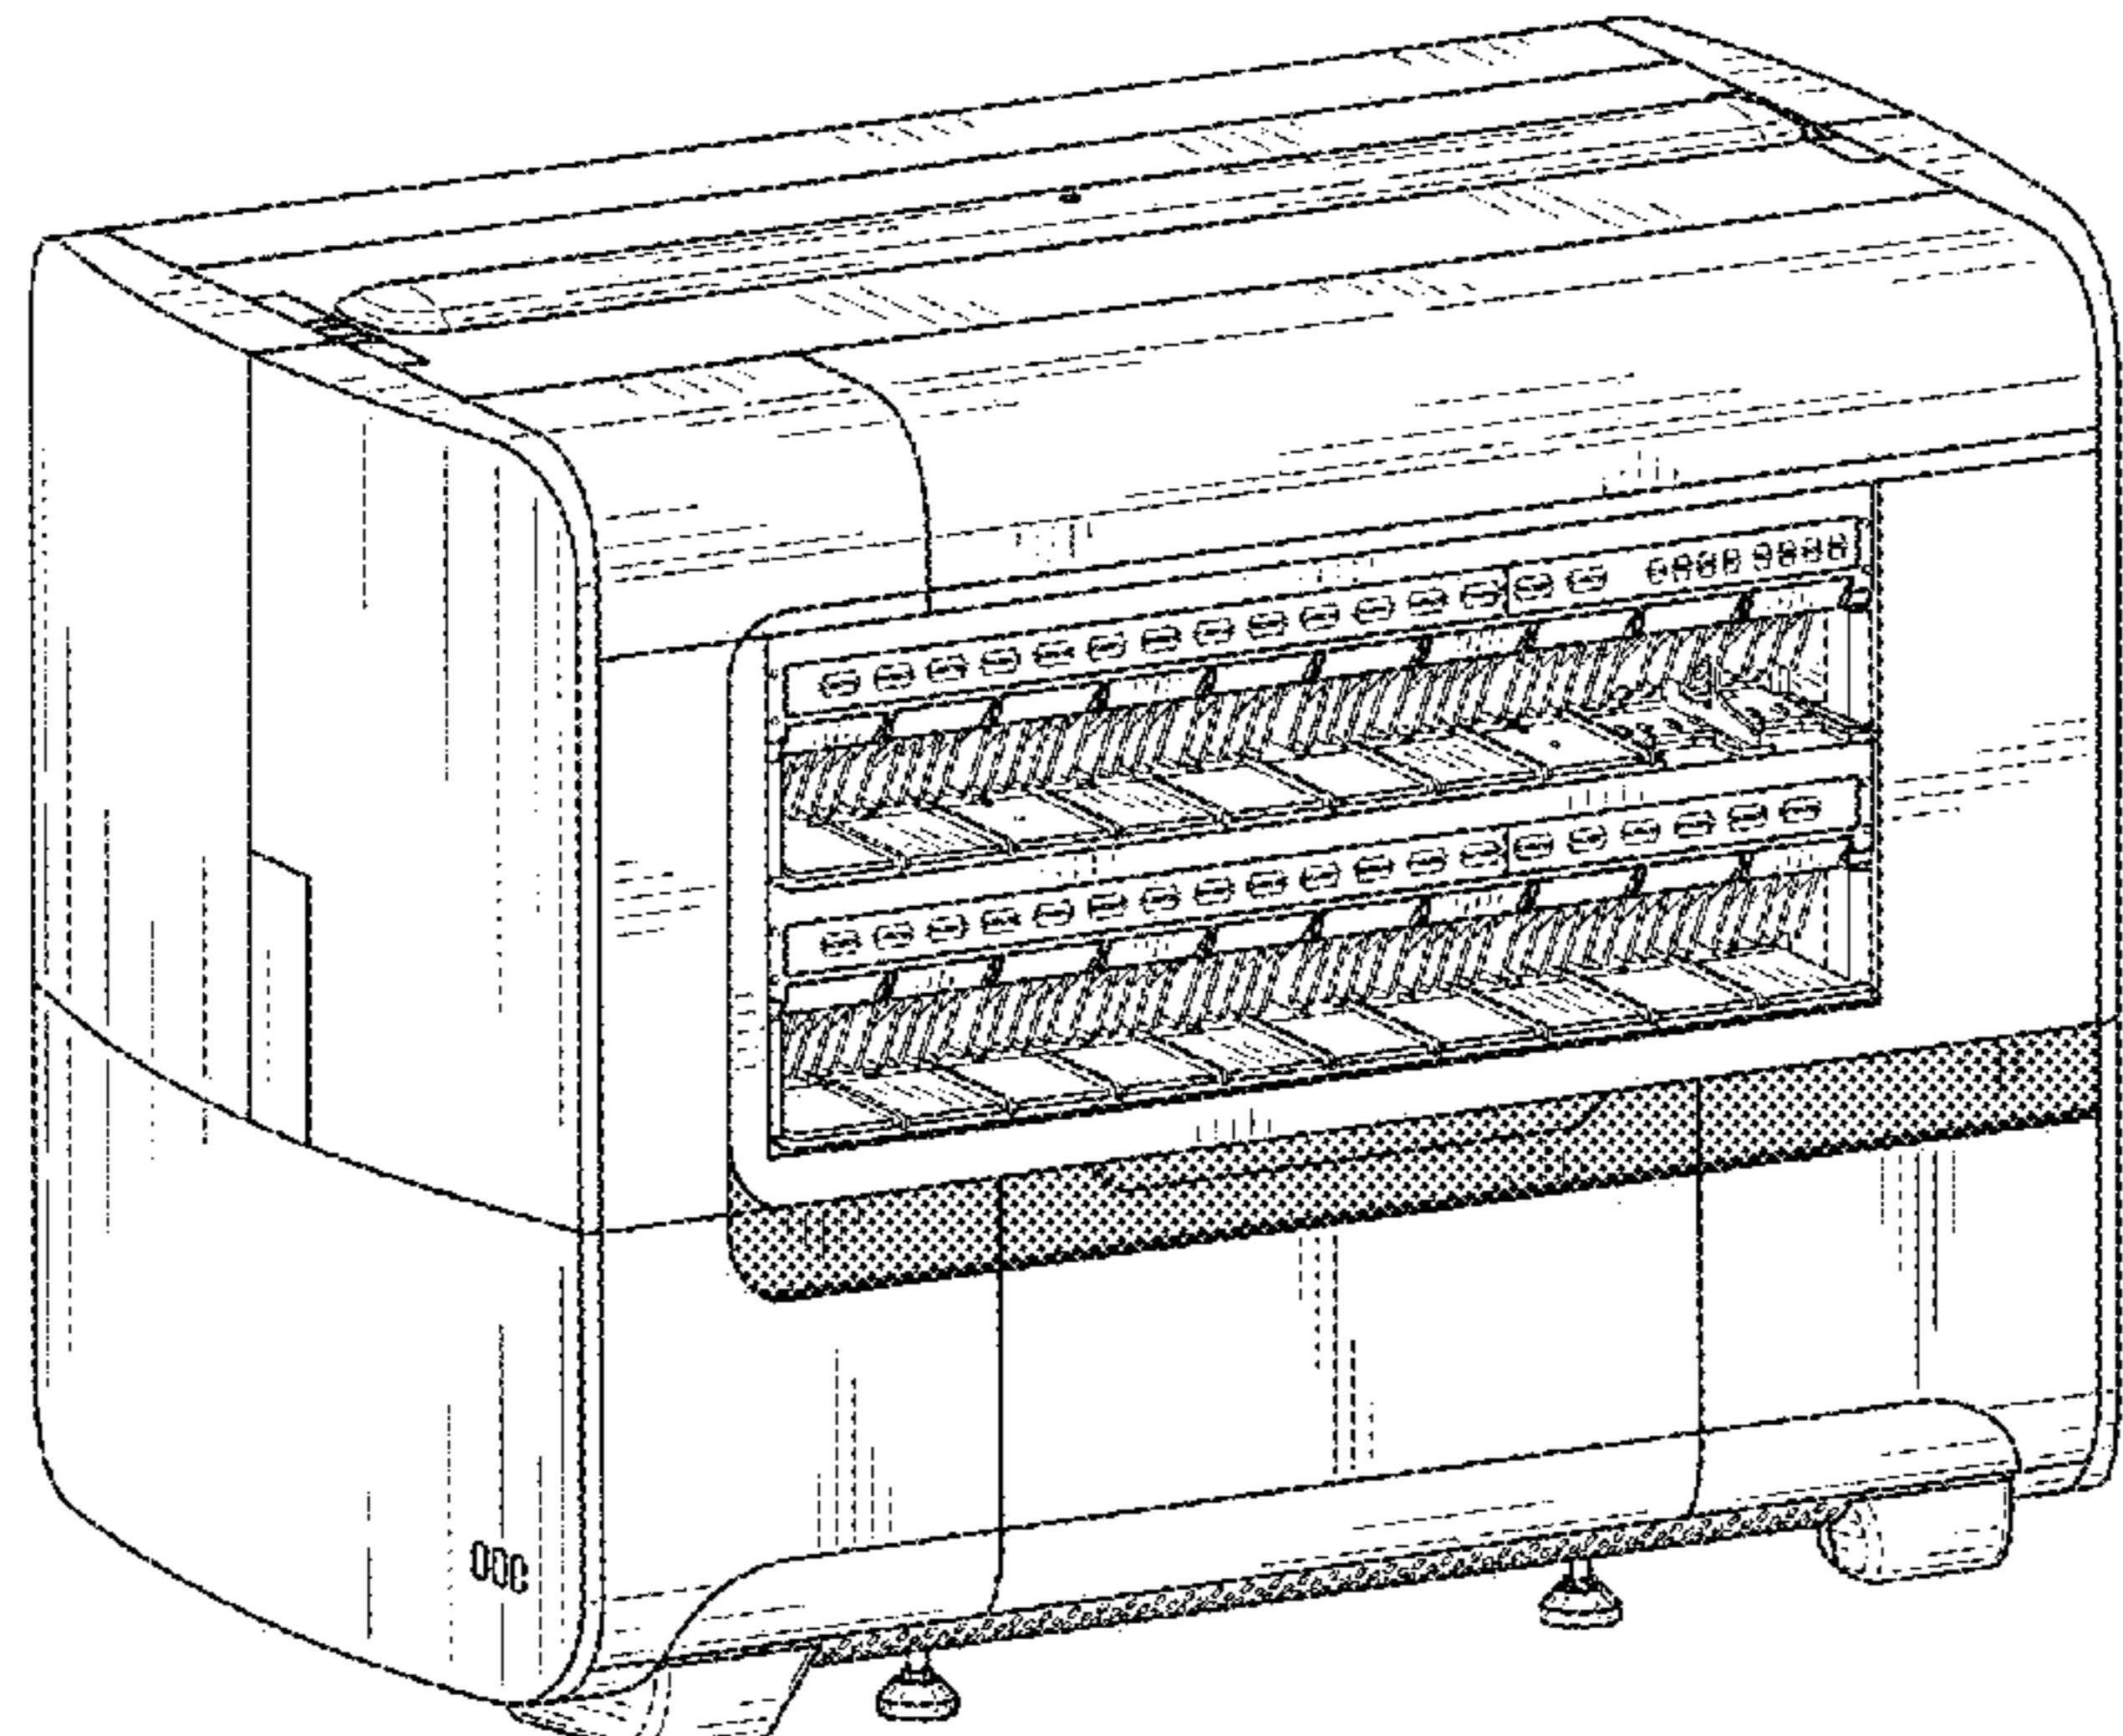

(58) **Field of Classification Search**

CPC 2201/0224; G01N 2201/0225; G01N
2201/0227; G01N 2201/0228; G01N
2201/024; G01N 2201/0245; G01N
2021/0112–21/958

See application file for complete search history.

(56)

References Cited

OTHER PUBLICATIONS

State Intellectual Property Office of China, "First Office Action," issued in connection with Chinese Patent Application No. 201530555266.8, dated Oct. 9, 2016, 3 pages.
State Intellectual Property Office of China, "Notification of First Correction," issued in connection with Chinese Patent Application No. 201530555266.8, dated Apr. 22, 2016, 3 pages.
Intellectual Property Office of Japan, "Notice for Reasons for Rejection," issued in connection with Japanese Application No. 2015-28870, mailed Jun. 14, 2016, 5 pages.

Office for Harmonization in the Internal Market, "Notification of the Registration of the Community Designs," issued in connection with European Community Design Nos. 002930230-0001 through 002930230-0029, dated Mar. 17, 2016, 6 pages.

United States Patent and Trademark Office, "Restriction and/or Election Requirement," issued in connection with U.S. Appl. No. 29/531,576, mailed Jul. 6, 2016, 12 pages.

United States Patent and Trademark Office, "Notice of Allowance," issued in connection with U.S. Appl. No. 29/531,576, mailed Sep. 8, 2016, 13 pages.

Japanese Patent Office, "Notice of Reasons for Rejection," issued in connection with Japanese Patent Application No. 2016-22305, mailed Feb. 28, 2017, 3 pages.

Japanese Patent Office, "Notice of Reasons for Rejection," issued in connection with Japanese Patent Application No. 2016-22306, mailed Feb. 28, 2017, 3 pages.

Japanese Patent Office, "Notice of Reasons for Rejection," issued in connection with Japanese Patent Application No. 2016-22307, mailed Feb. 28, 2017, 3 pages.

* cited by examiner

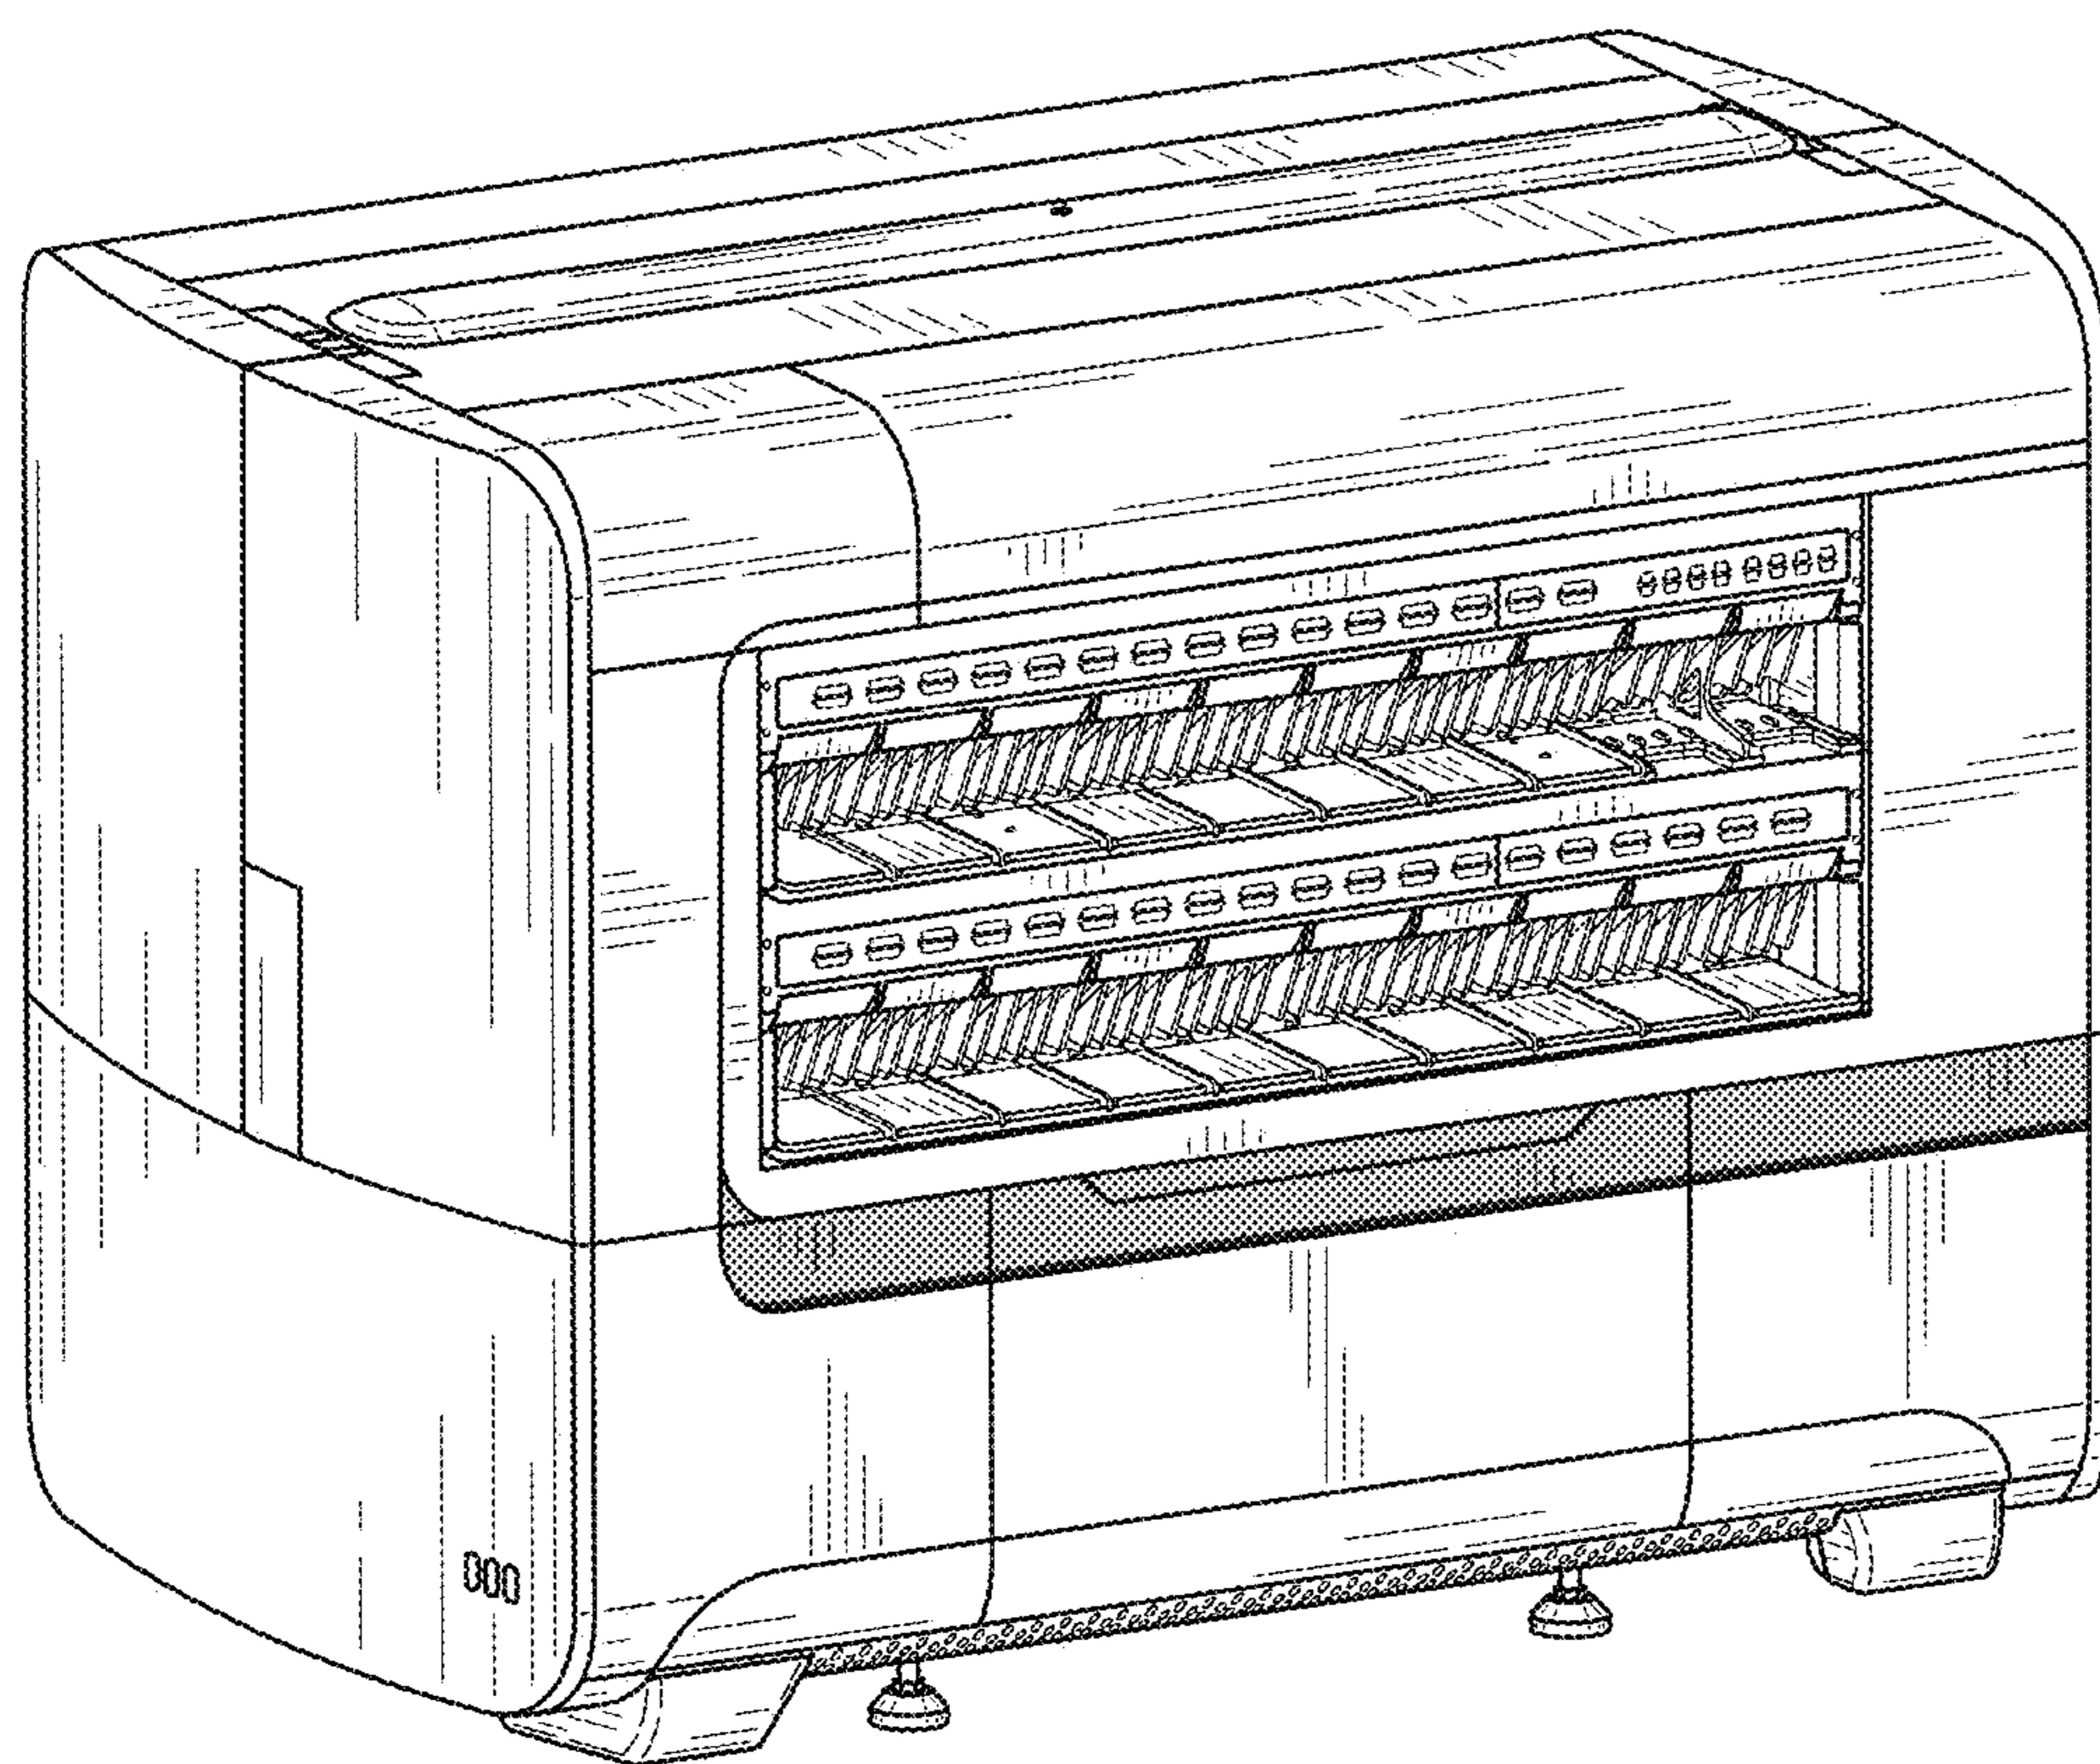
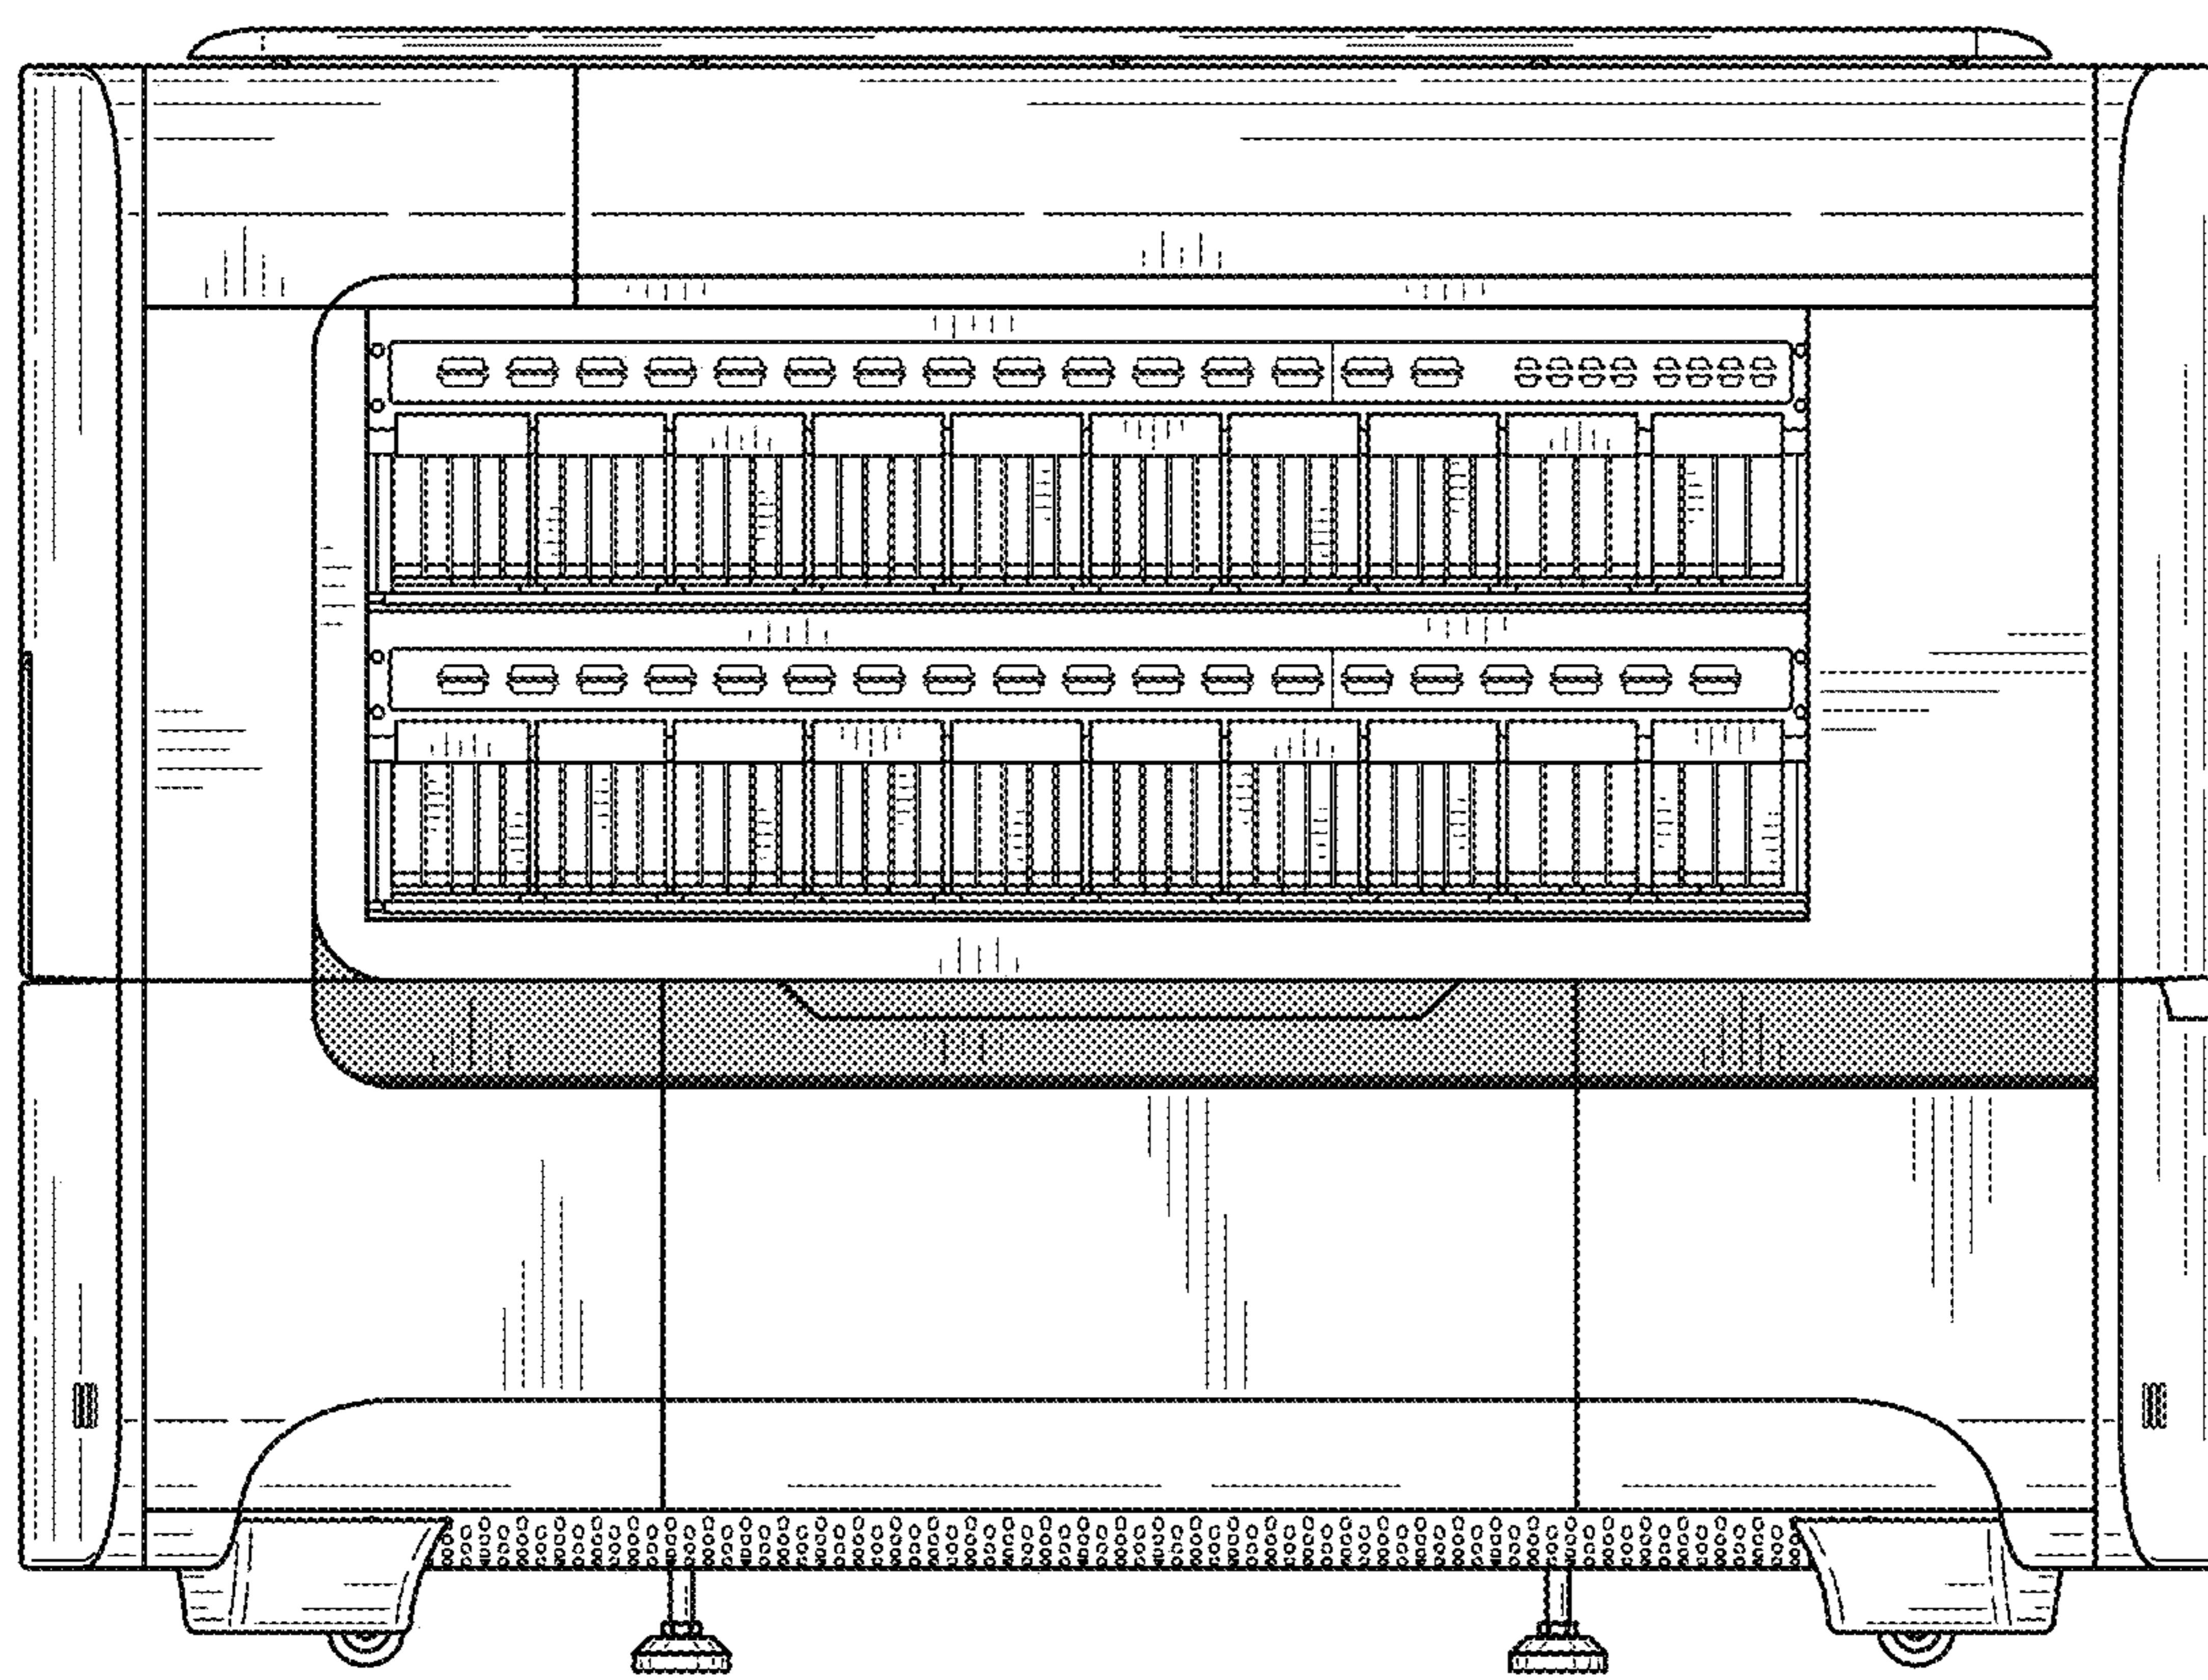


FIG. 1

**FIG. 2**

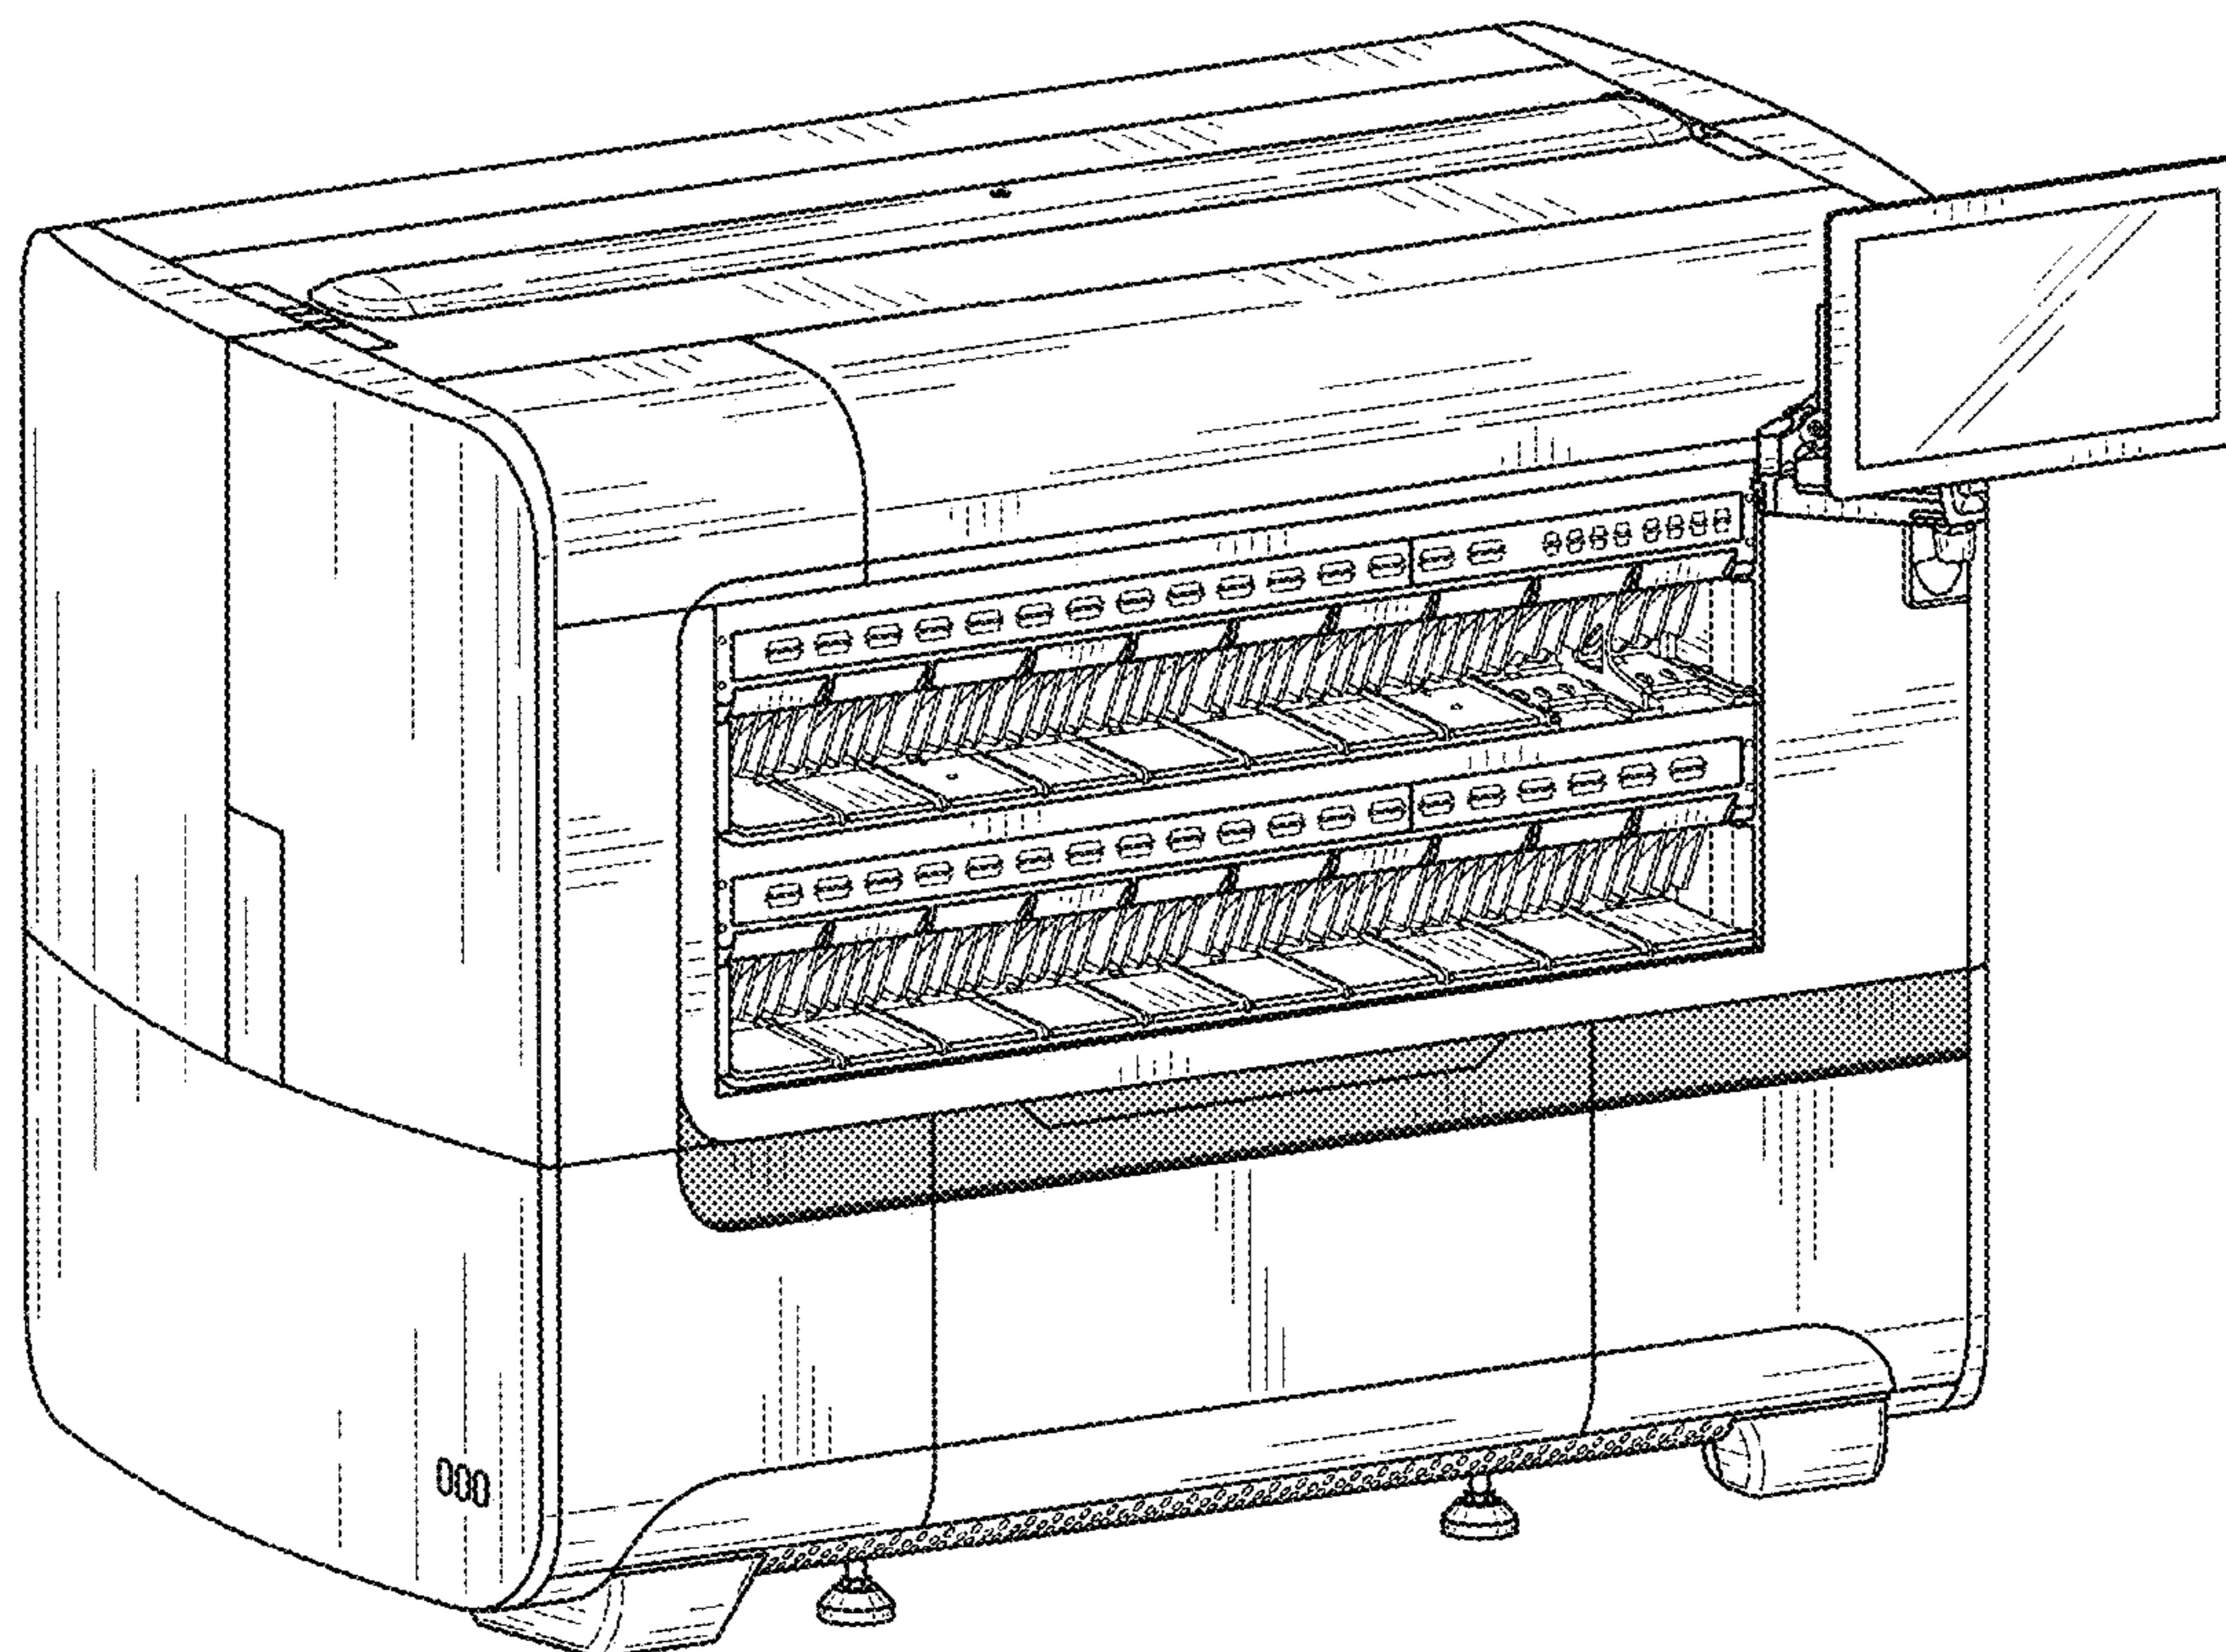
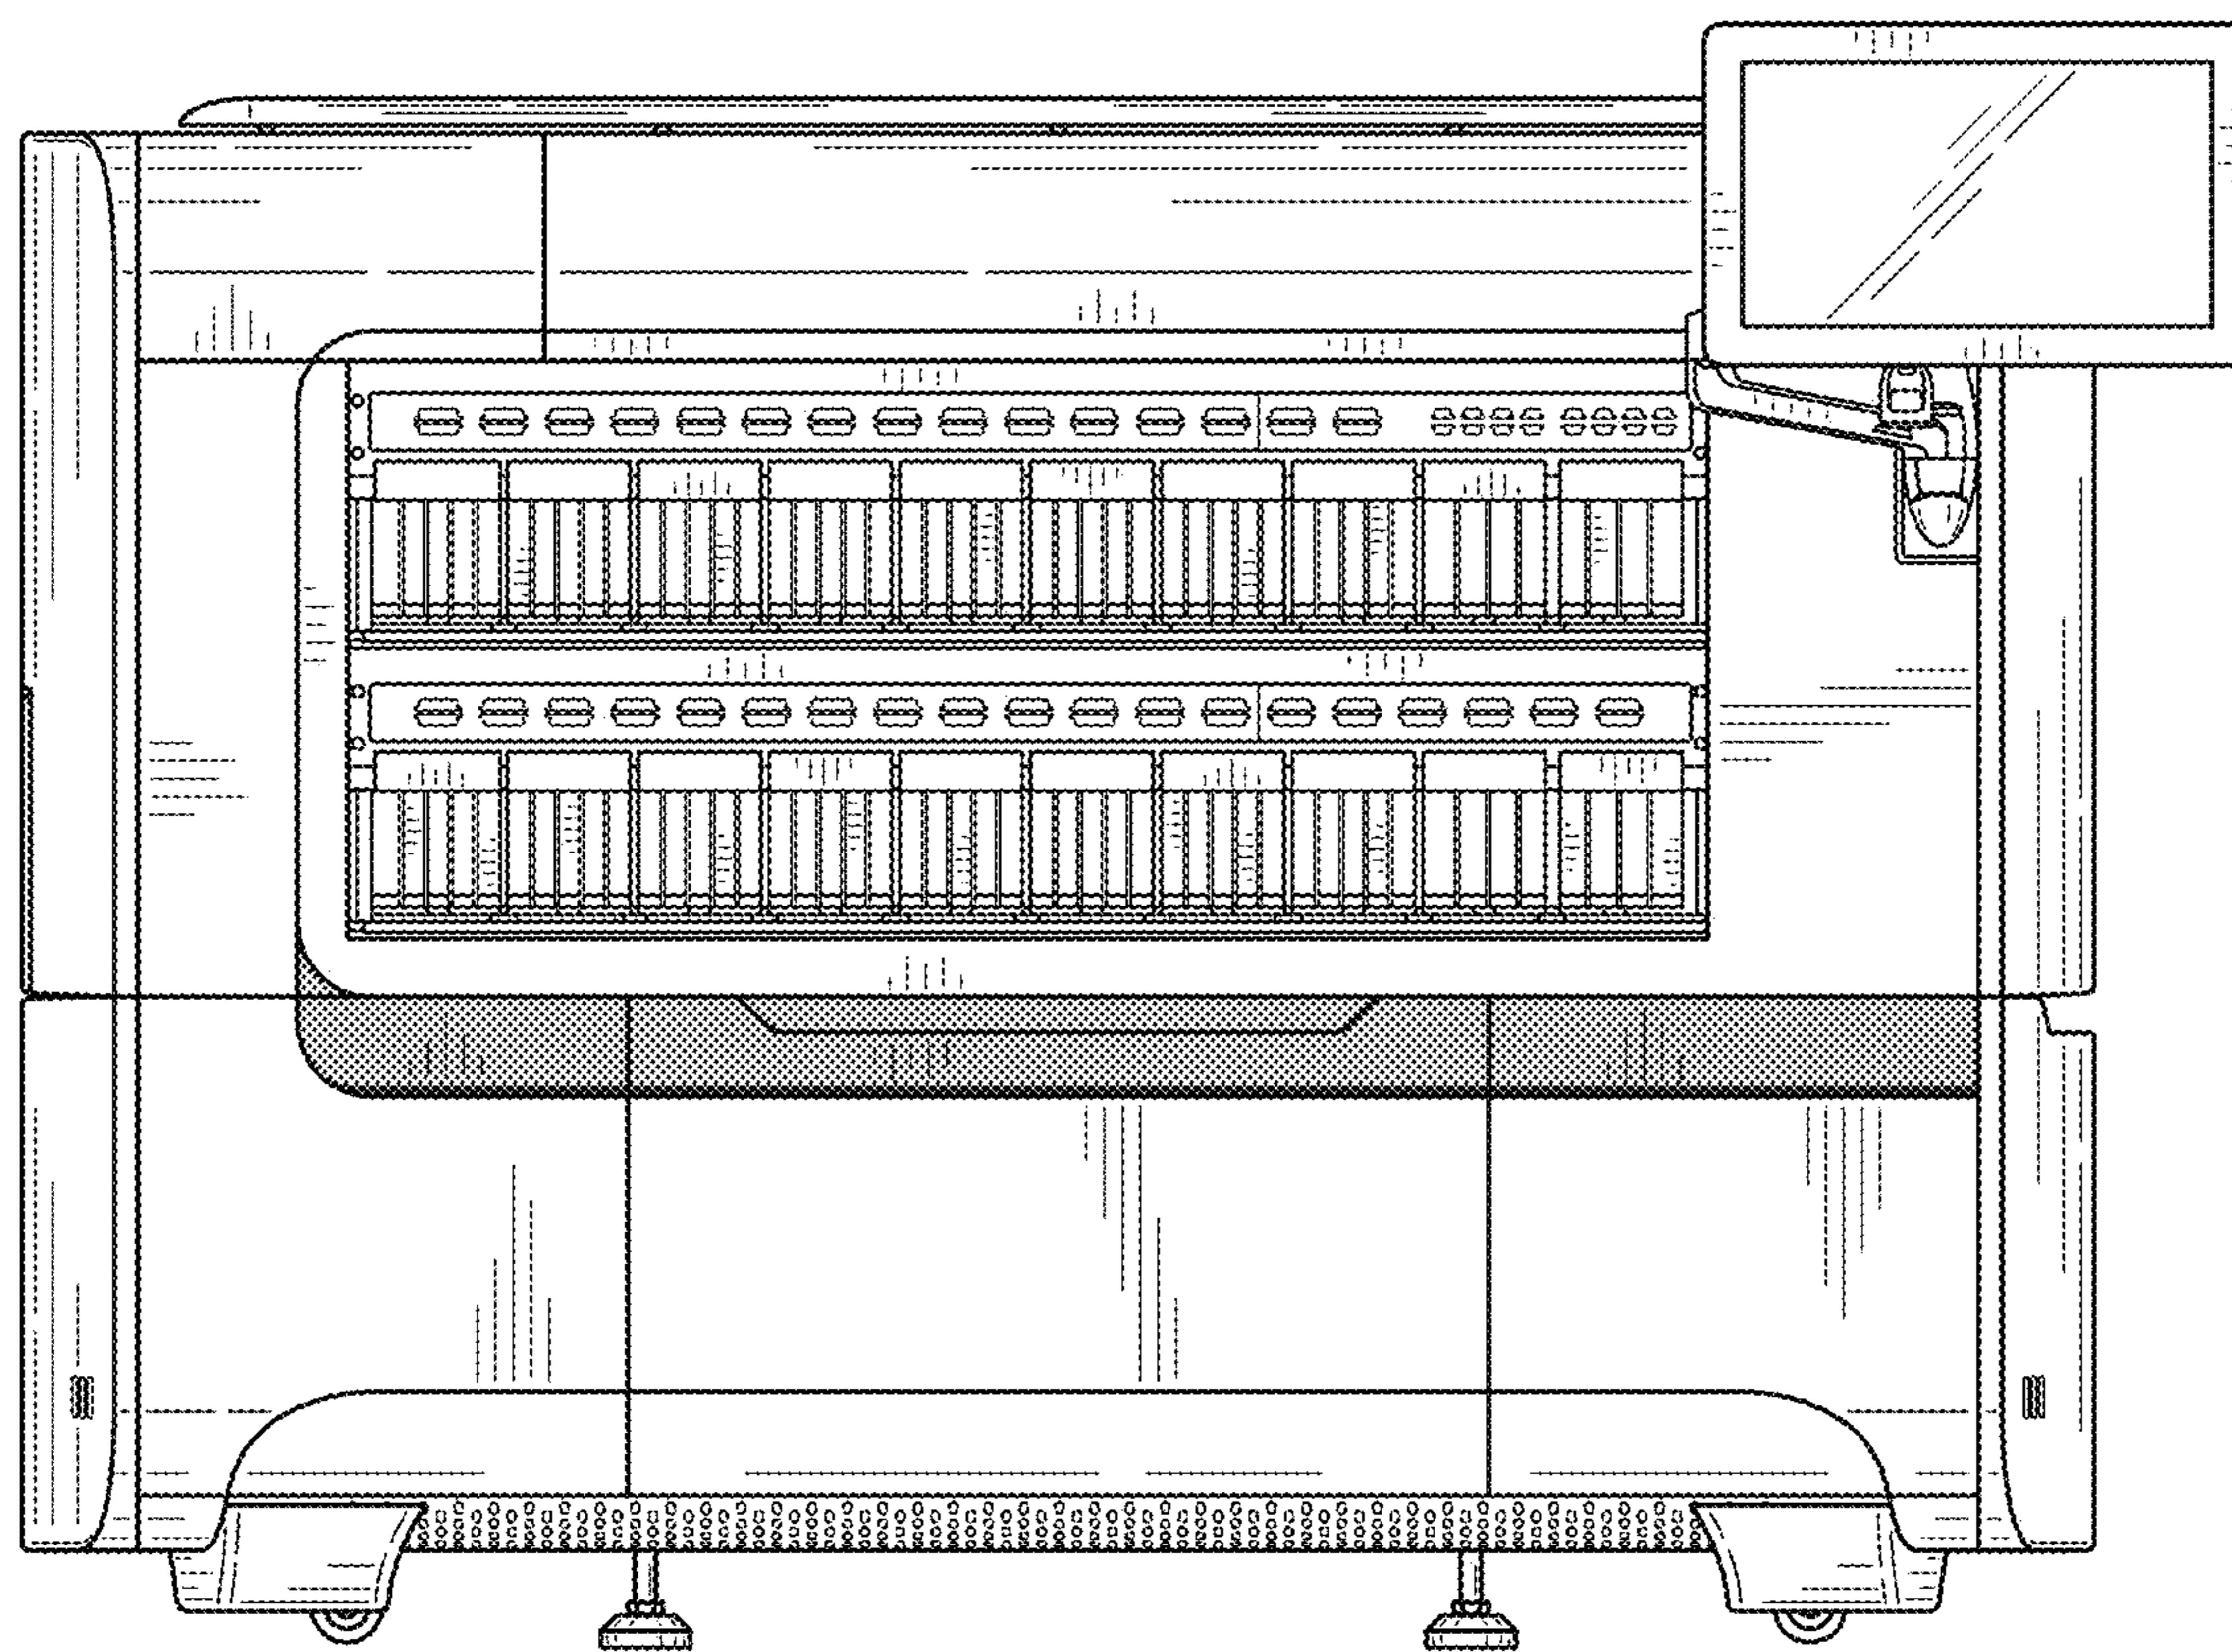
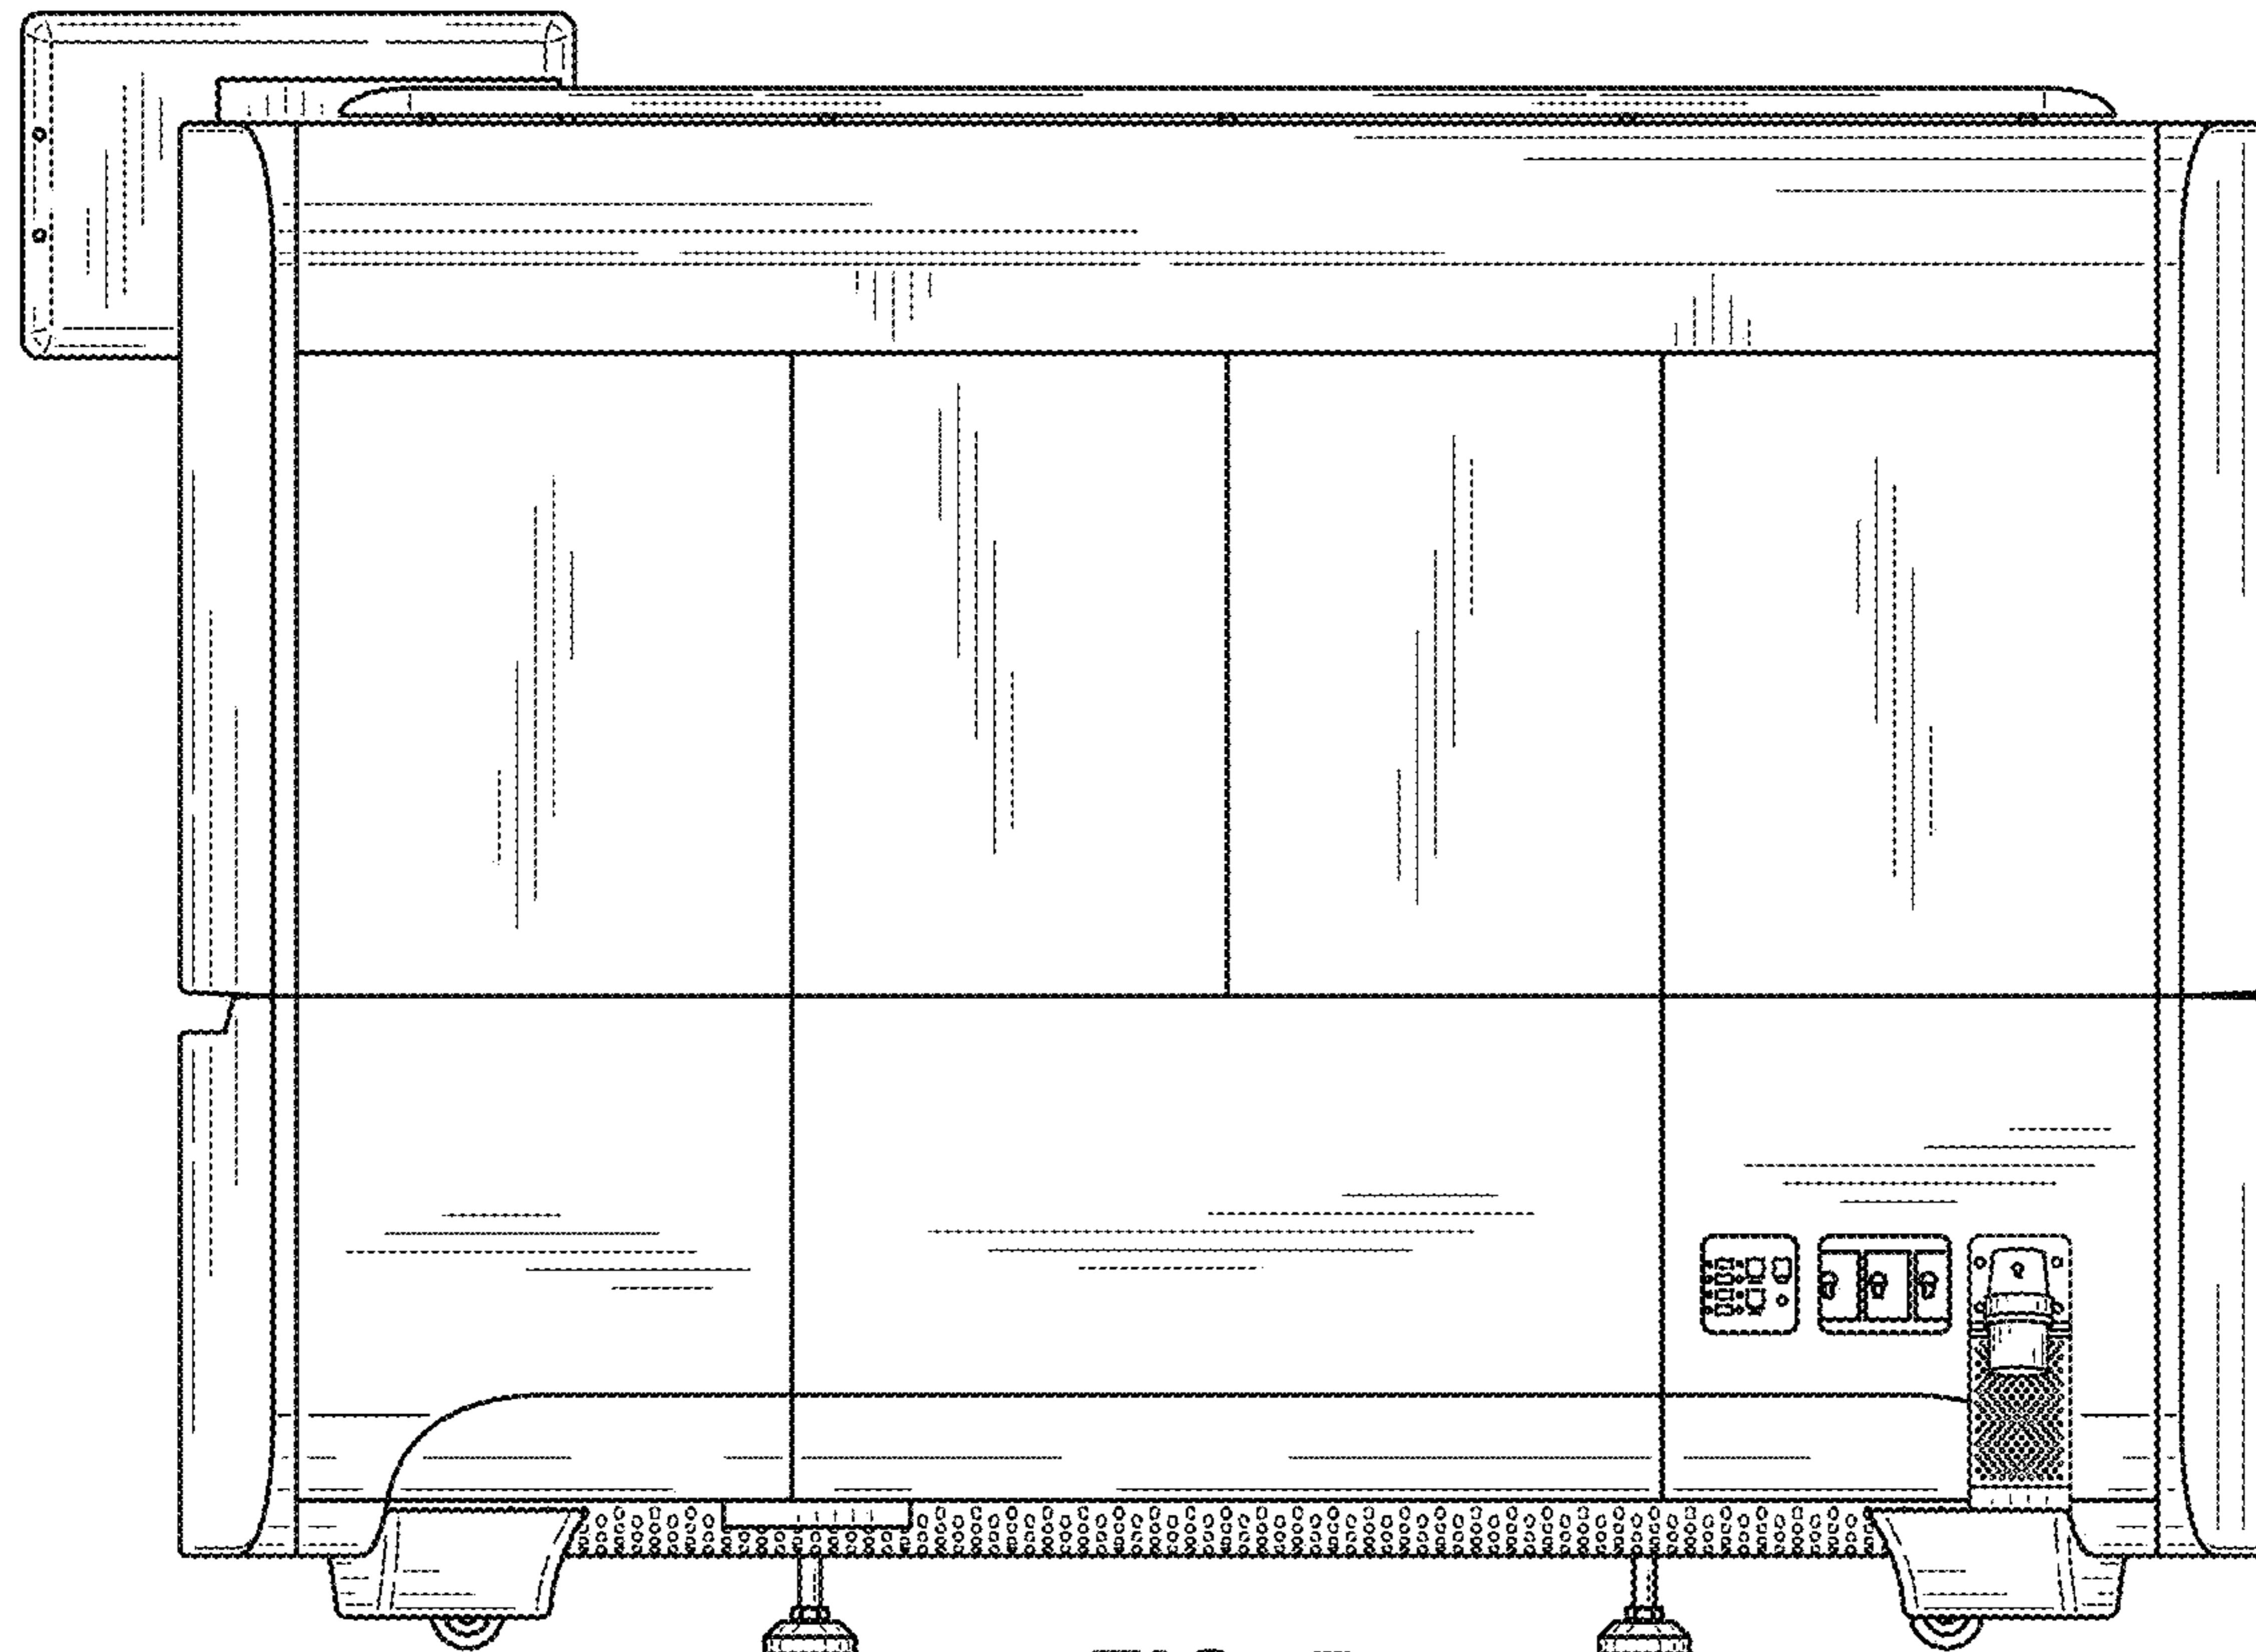
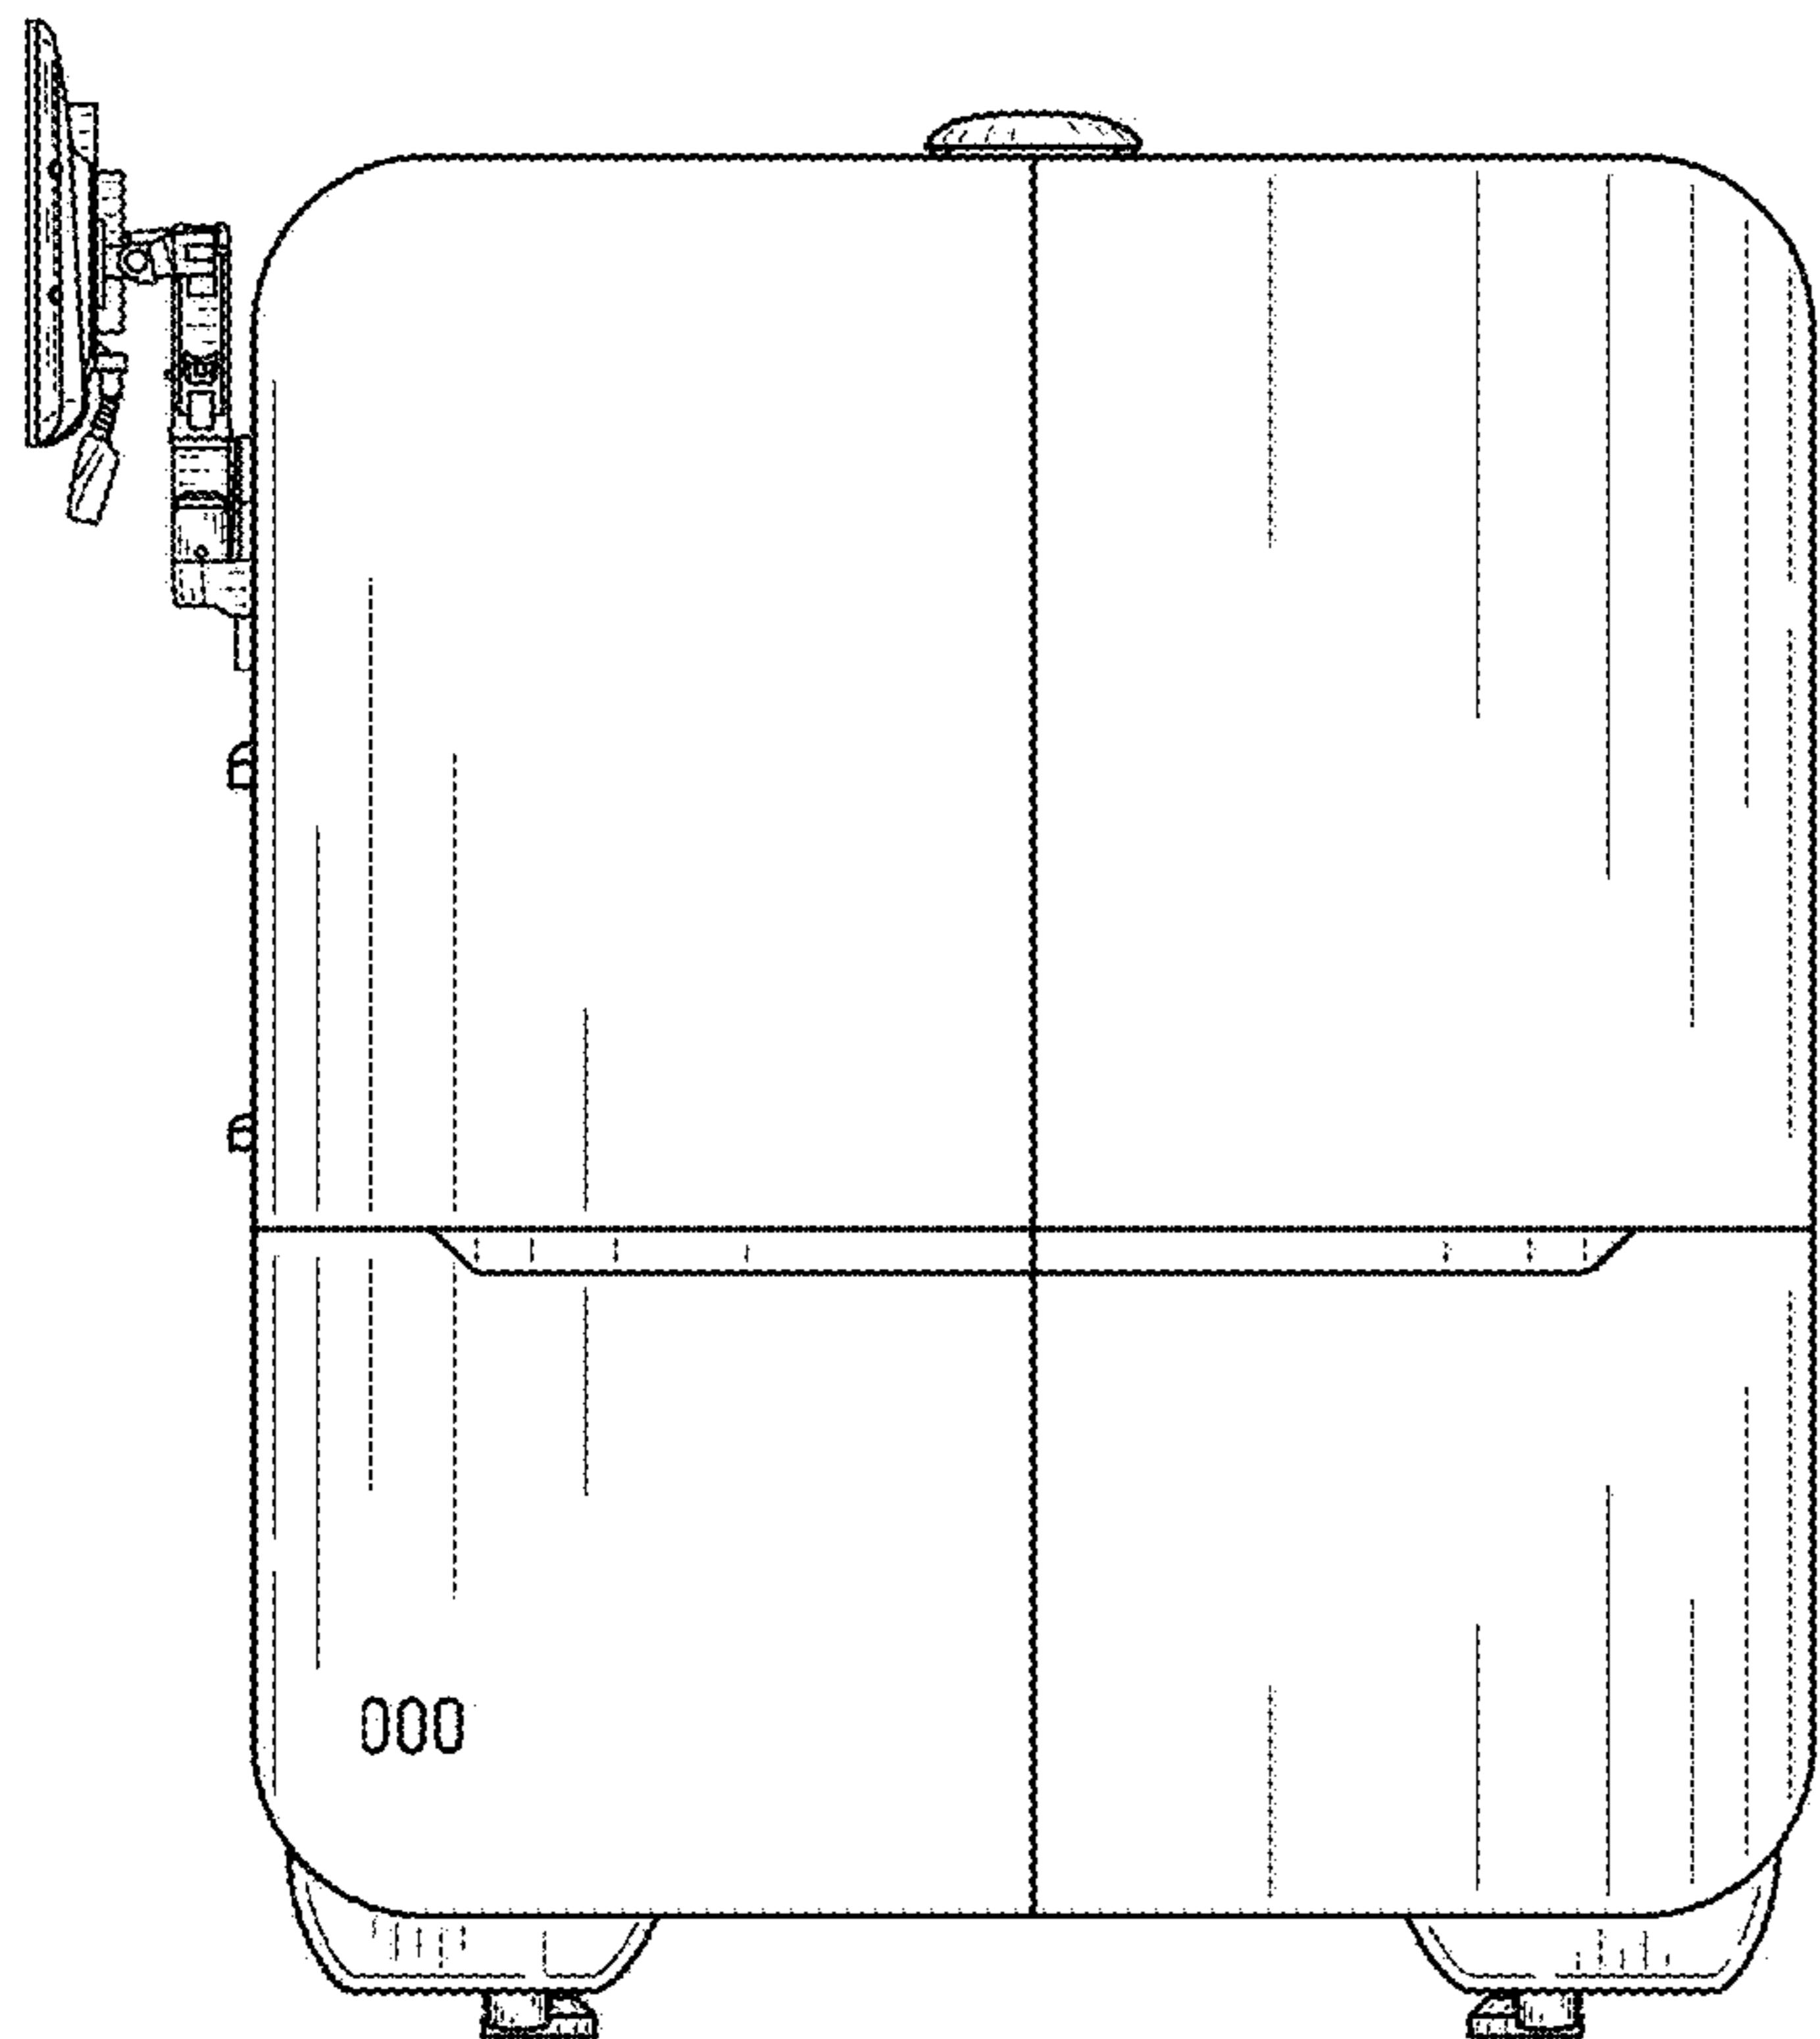
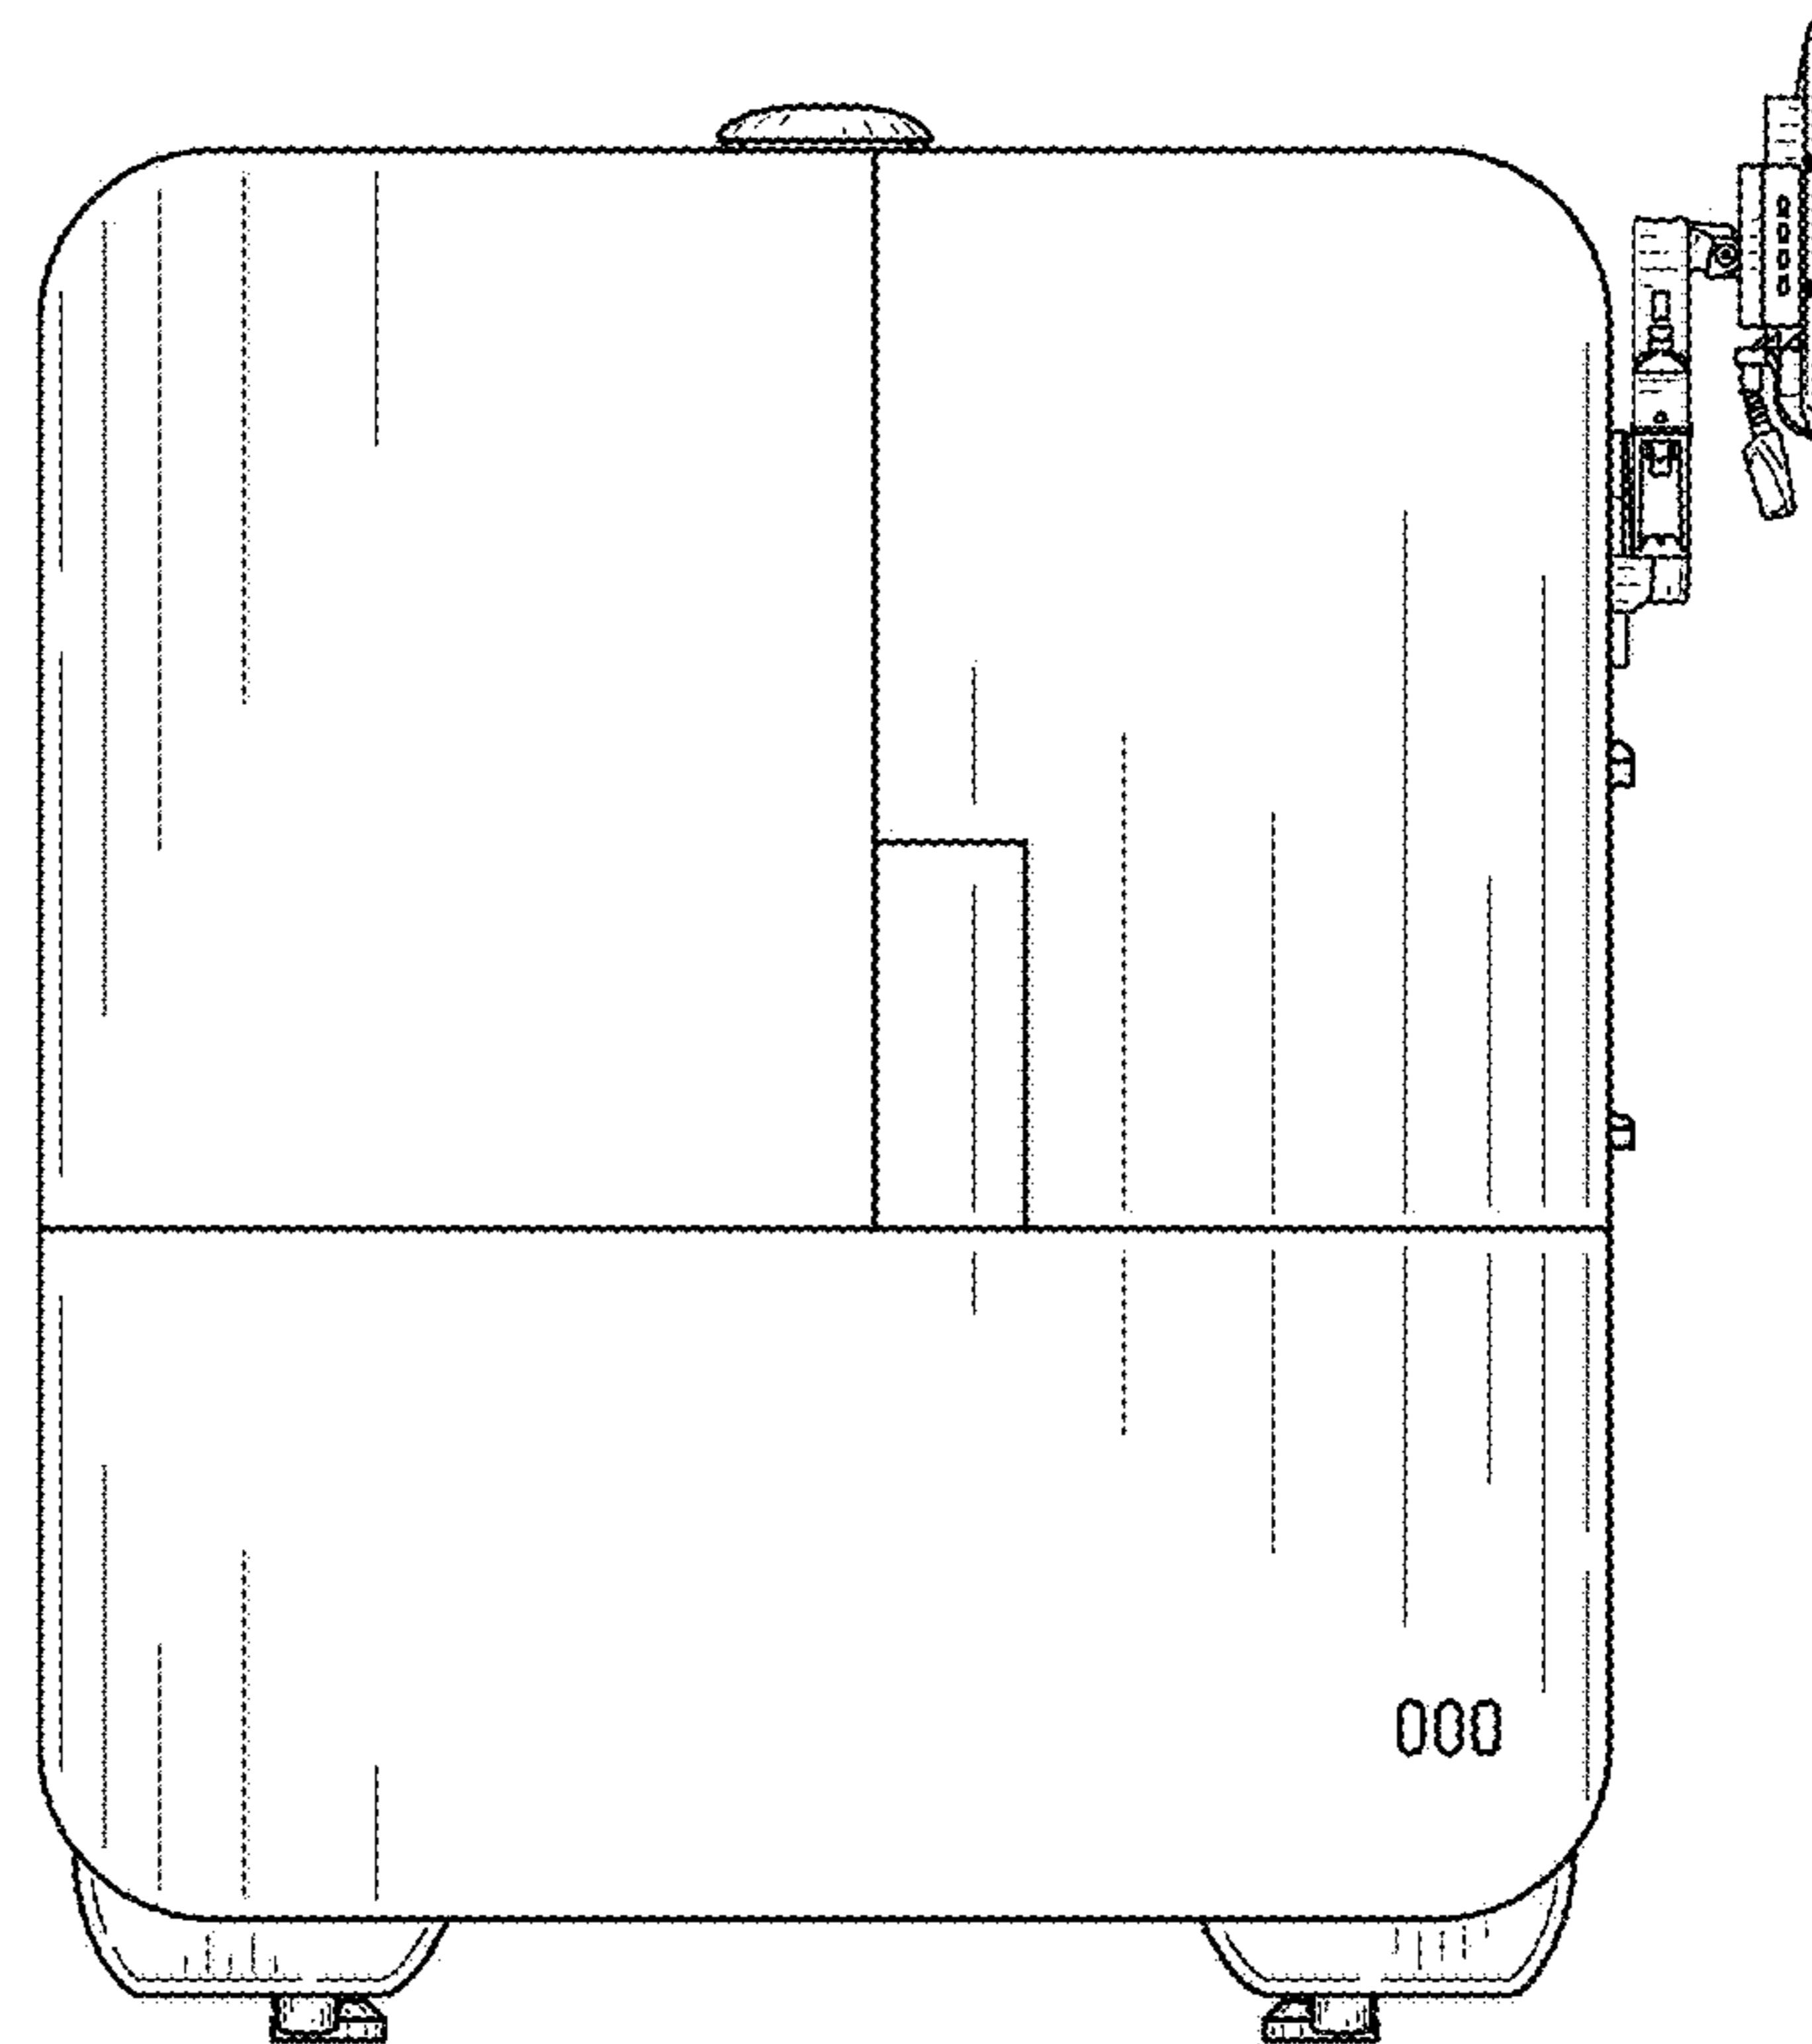
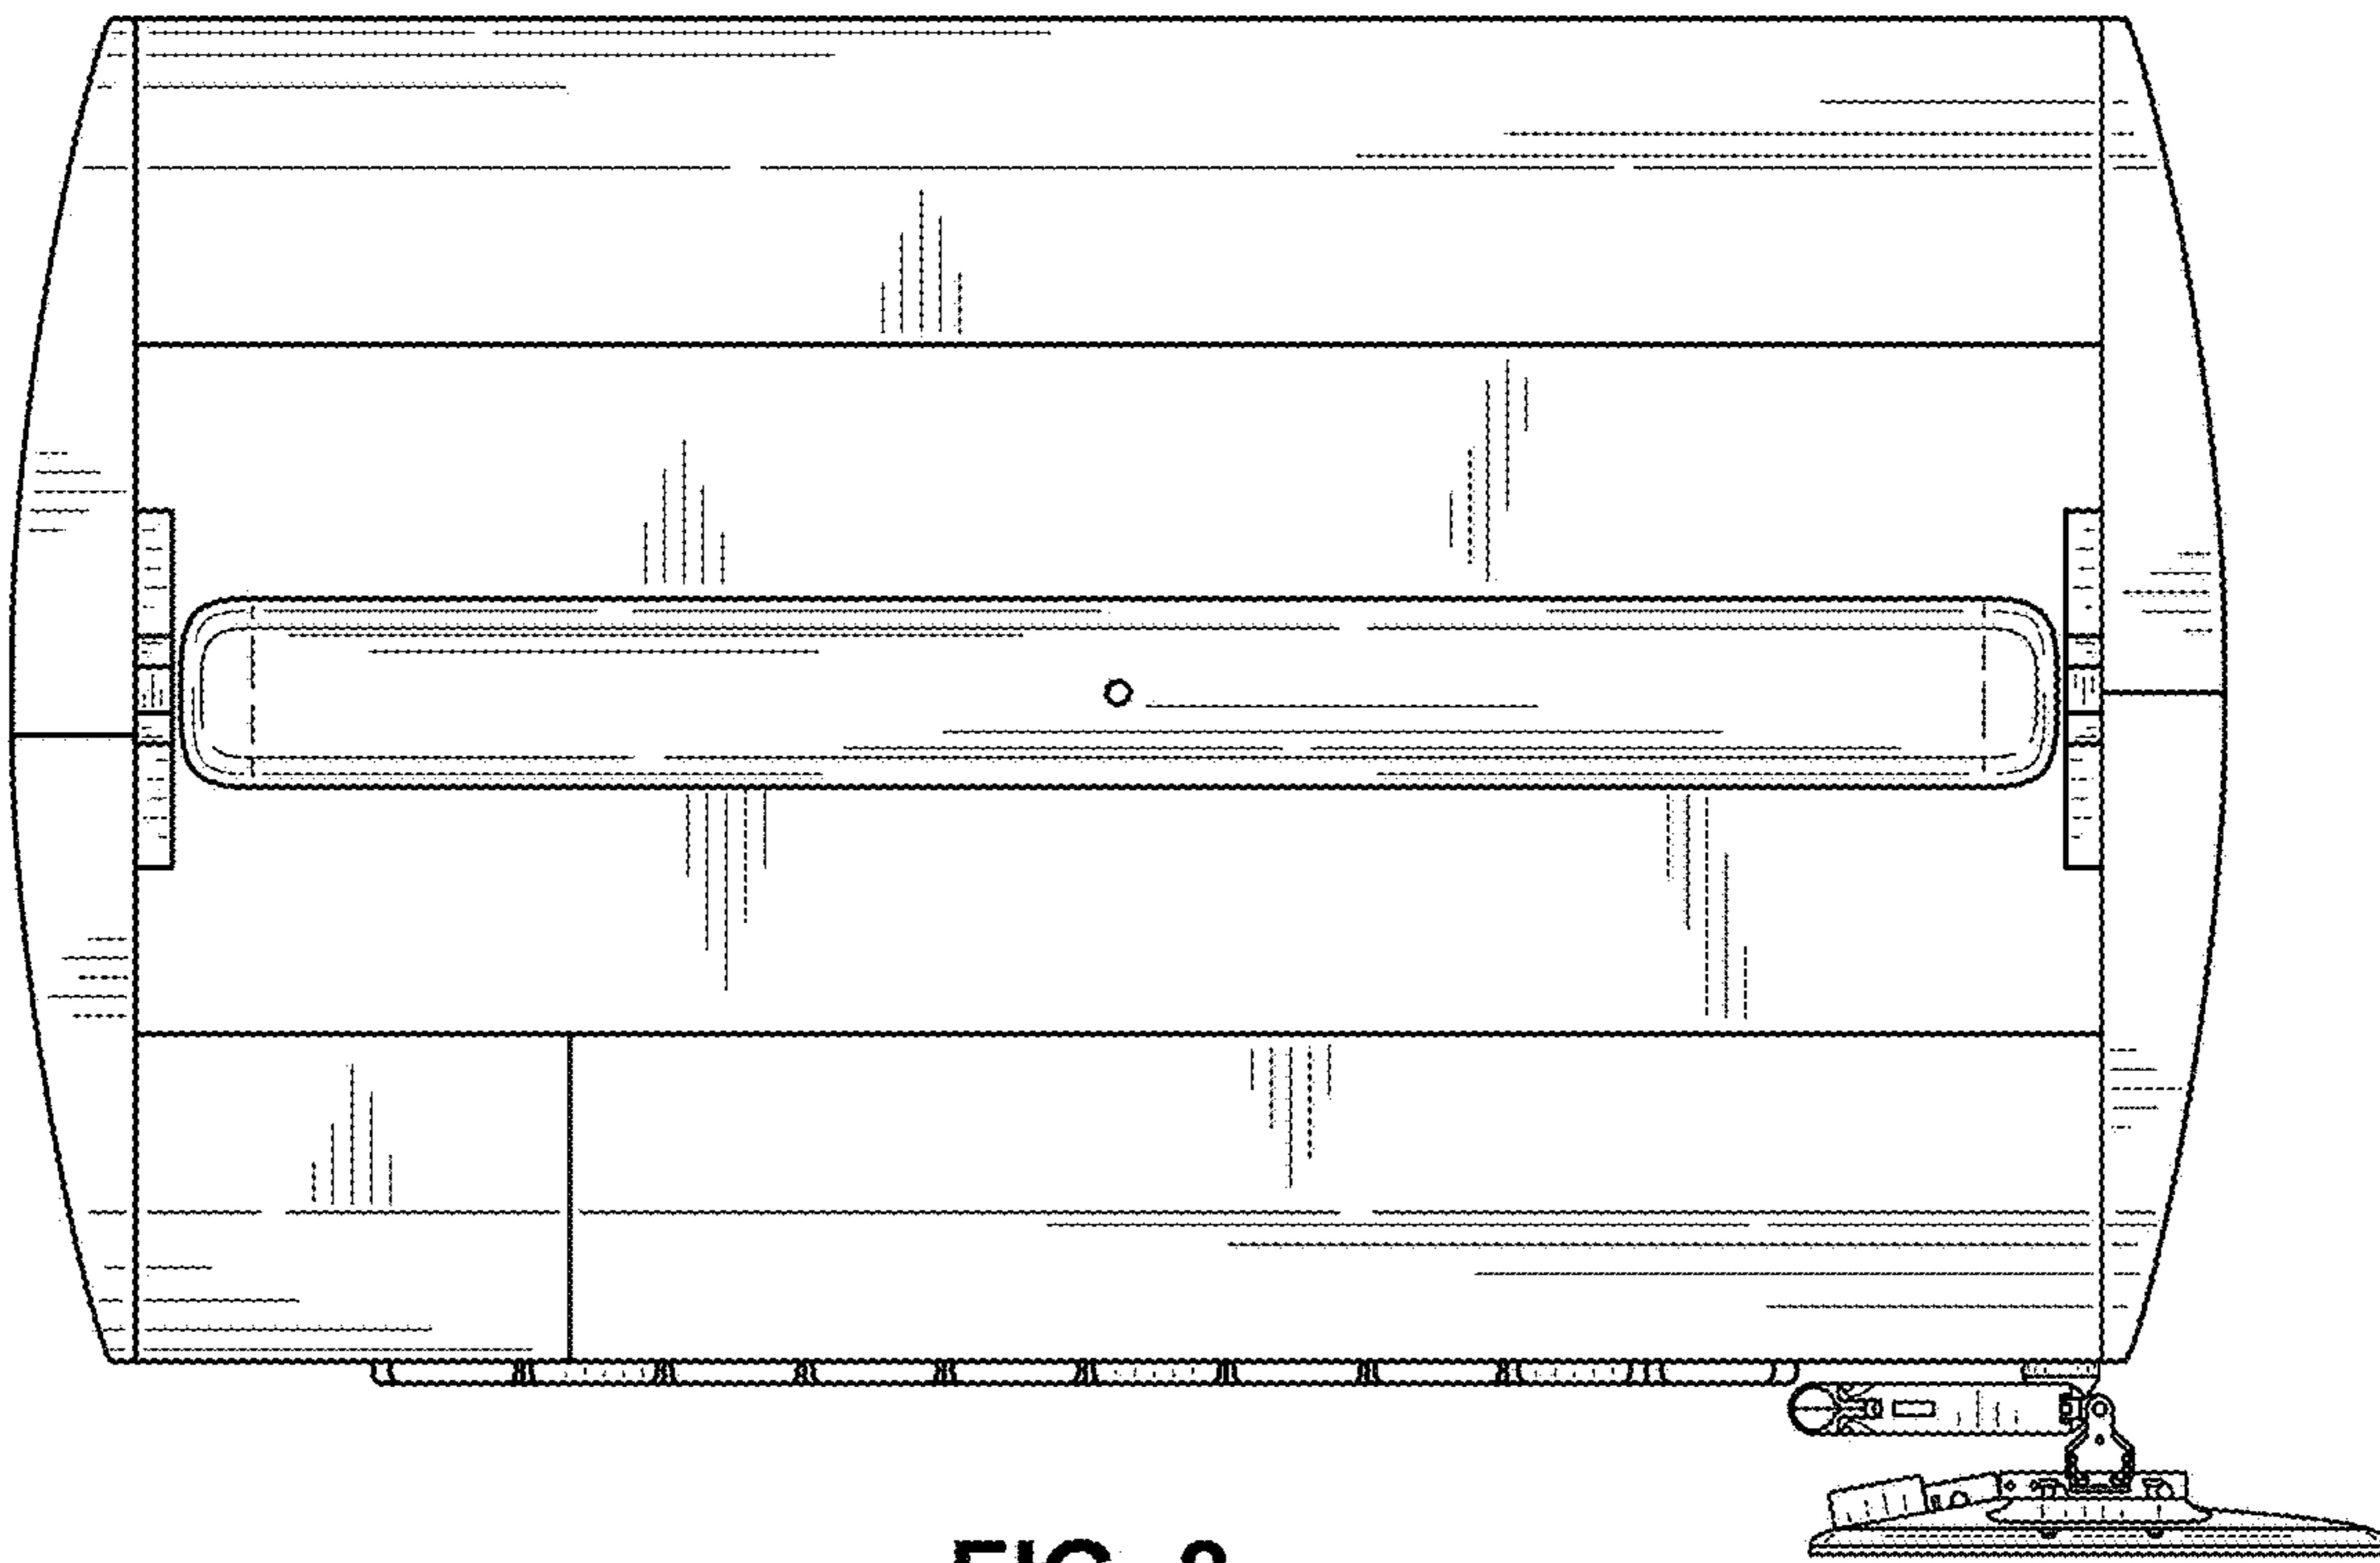
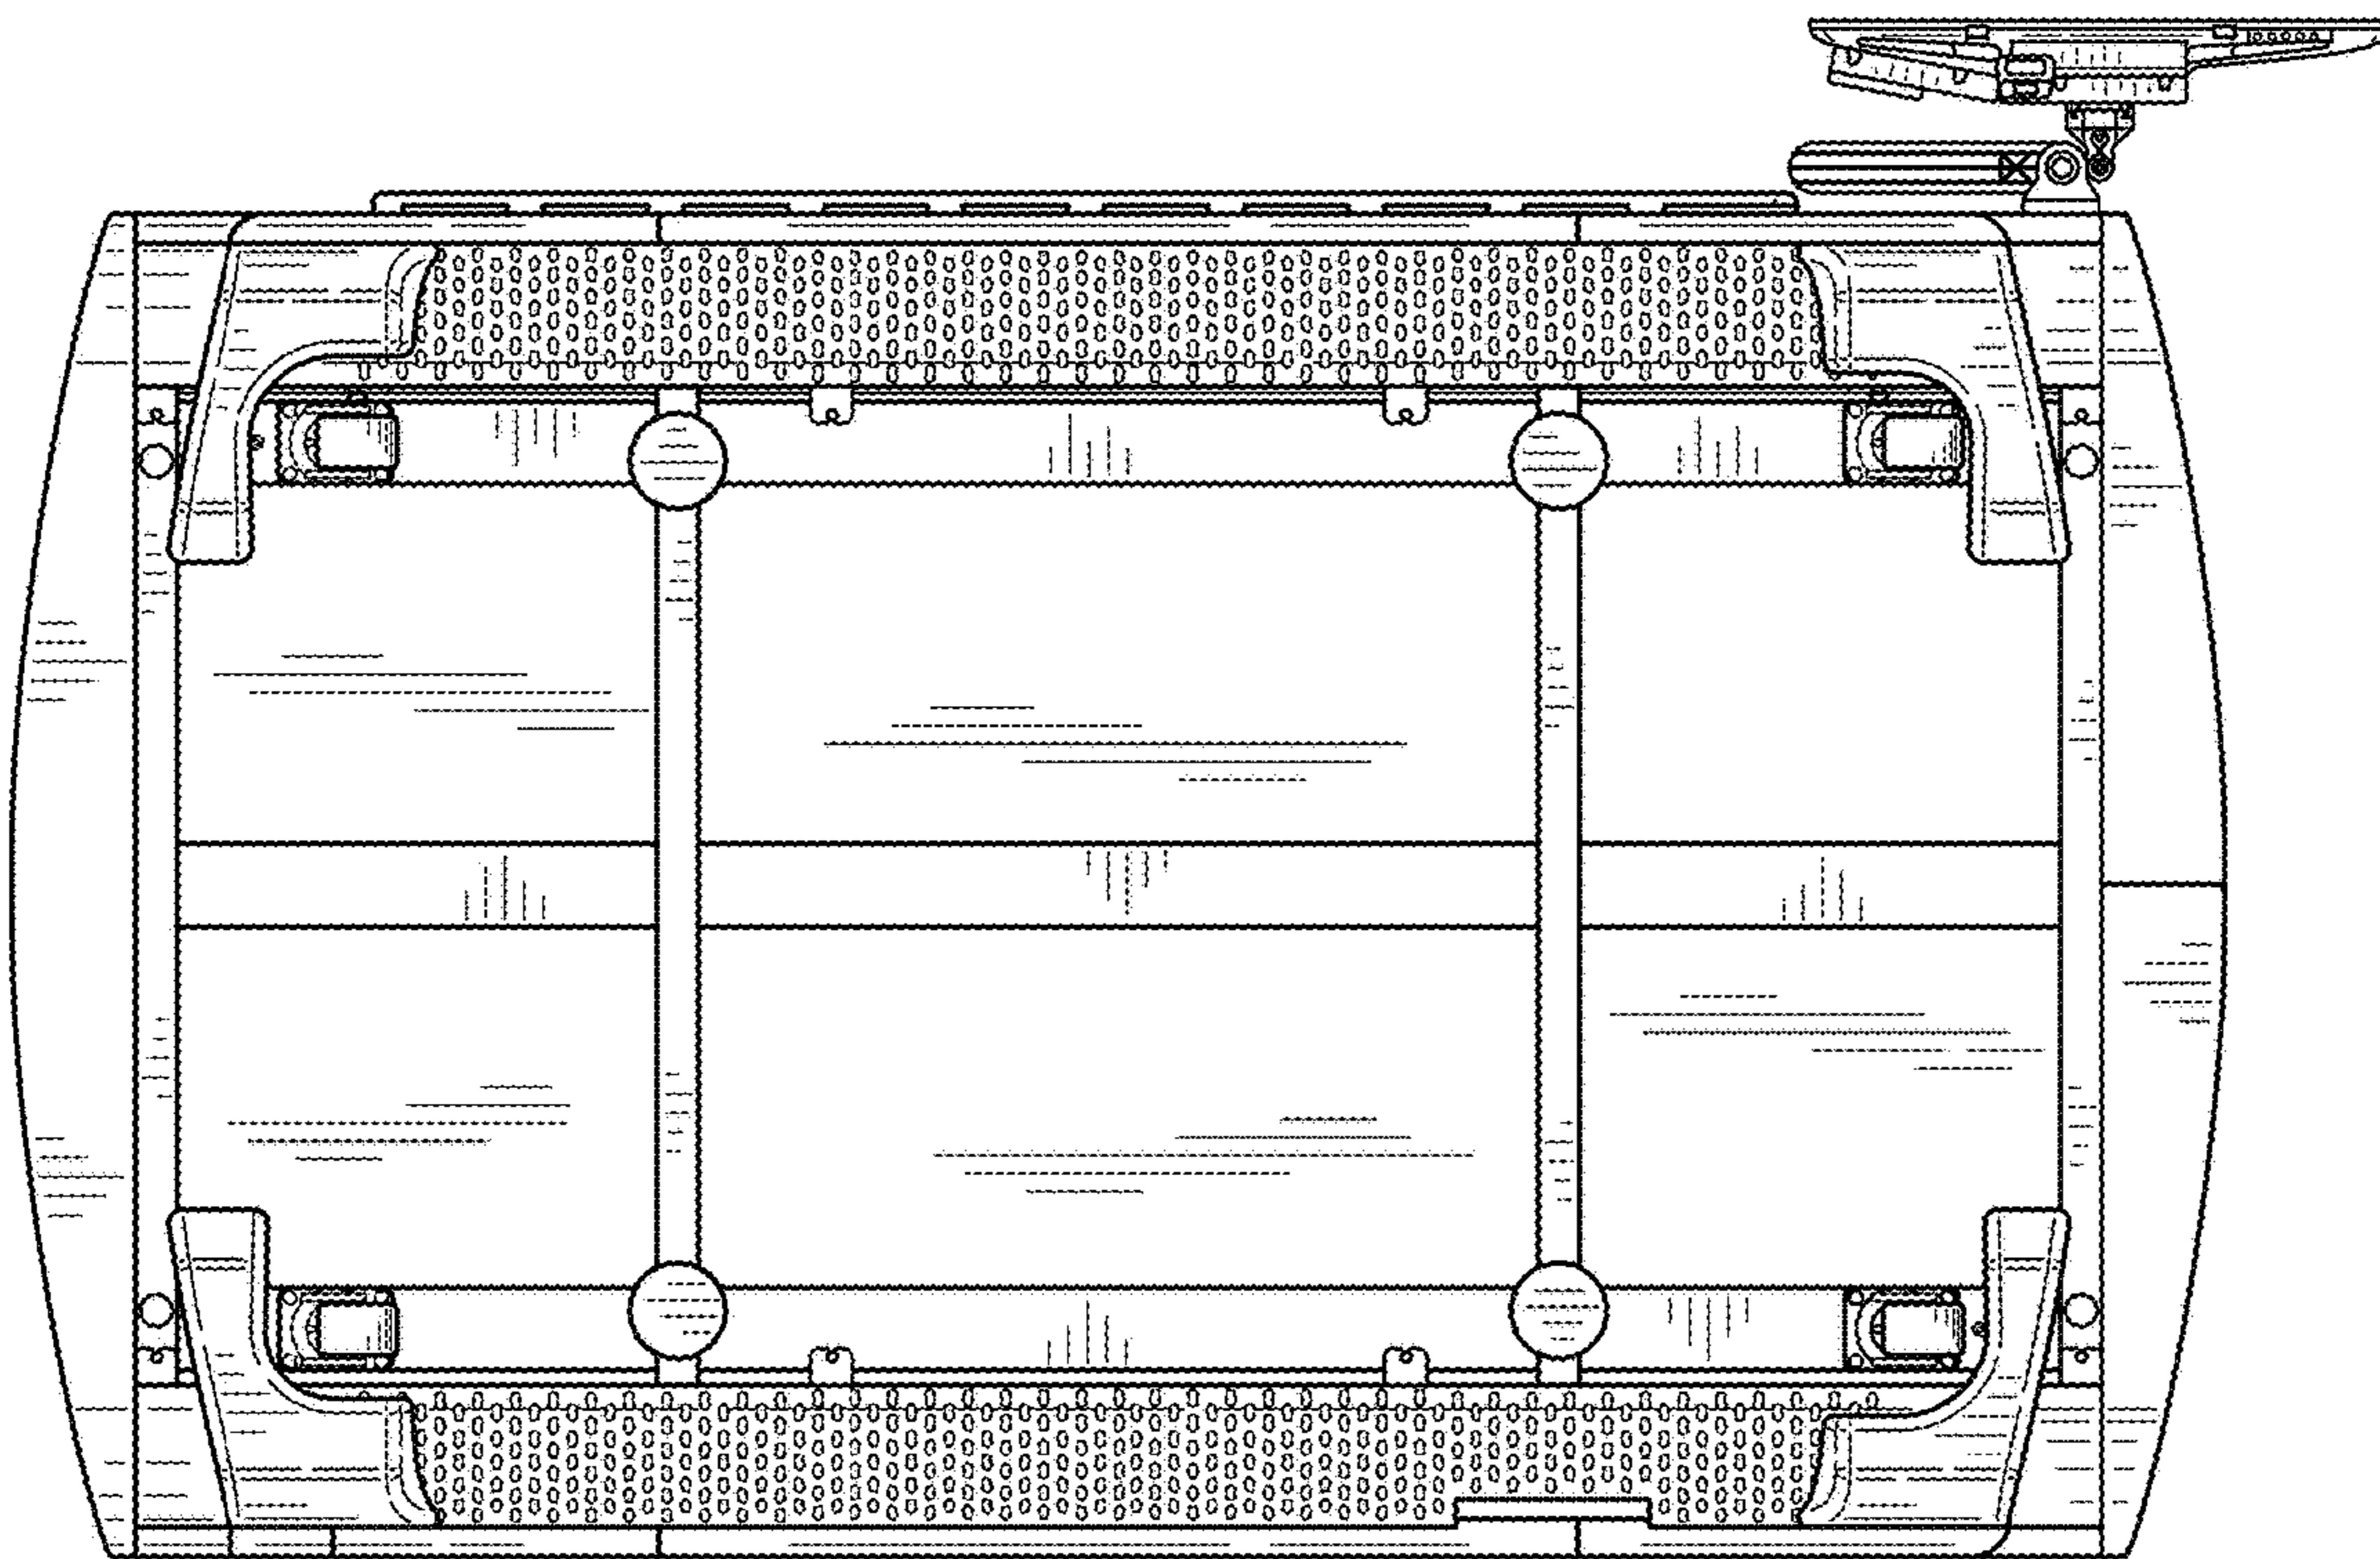


FIG. 3

**FIG. 4****FIG. 5**

**FIG. 6****FIG. 7**

**FIG. 8****FIG. 9**