



US00D800757S

(12) **United States Design Patent** (10) **Patent No.:** **US D800,757 S**
Mullen et al. (45) **Date of Patent:** **** Oct. 24, 2017**

(54) **GRAPHICAL DATA DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE FOR DISPLAY OF CONTINUOUS LOOP INSULIN AND GLUCOSE DATA**

8,041,714 B2 * 10/2011 Aymeloglu G06F 17/30398
707/726
D652,048 S * 1/2012 Joseph D14/485
D652,052 S 1/2012 Judy et al.
8,133,178 B2 3/2012 Brauker
D661,313 S 6/2012 Nenoki
D667,417 S * 9/2012 Long D14/486

(71) Applicant: **Park Nicollet Institute**, St. Louis Park, MN (US)

(Continued)

(72) Inventors: **Deborah M. Mullen**, Minneapolis, MN (US); **David M. Wesley**, Hudson, WI (US); **Richard M. Bergenstal**, Plymouth, MN (US)

OTHER PUBLICATIONS

“Recommendations . . .”, posted at researchgate.net, Feb. 2013, [site visited Jun. 1, 2017]. Available from Internet: https://www.researchgate.net/publication/235755545_Recommendations_for_Standardizing_Glucose_Reporting_and_Analysis_to_Optimize_Clinical_Decision_Making_in_Diabetes_The_Ambulatory_Glucose_Profile_AGP.*

(Continued)

(73) Assignee: **Park Nicollet Institute**, St. Louis Park, MN (US)

(**) Term: **15 Years**

Primary Examiner — Karen E Kearney

Assistant Examiner — John M Otte

(74) *Attorney, Agent, or Firm* — Merchant & Gould P.C.

(21) Appl. No.: **29/570,125**

(22) Filed: **Jul. 5, 2016**

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485–495; D20/11; D21/324.325
CPC G06F 3/04817; G06F 3/0482; G06F 3/04842; G06F 17/30398; G03G 25/2039; F01D 9/065; G01R 13/345; G06Q 10/10; G06Q 30/02; G09G 5/363; B24D 12/10
See application file for complete search history.

(57) **CLAIM**

The ornamental design for a graphical data display screen with graphical user interface for display of continuous loop insulin and glucose data, as shown and described.

DESCRIPTION


FIG. 1 is a front view of a first embodiment of a graphical data display screen with graphical user interface for display of continuous loop insulin and glucose data; and, FIG. 2 is a front view of a second embodiment thereof. The evenly spaced broken line showing of the graphical data display screen with graphical user interface for display of continuous loop insulin and glucose data is included for the purpose of illustrating portions of the article and form no part of the claimed design. The outer long dash short dash broken line represents the bounds of the claimed design and forms no part thereof.

1 Claim, 2 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,559,868 B2 * 5/2003 Alexander G01R 13/345
345/440.1
D525,264 S * 7/2006 Chotai D14/486
D573,601 S 7/2008 Gregov et al.
D589,976 S 4/2009 Hosokawa et al.
D630,648 S 1/2011 Tokunaga et al.
D630,649 S 1/2011 Tokunaga et al.
D632,699 S 2/2011 Judy et al.
D633,514 S 3/2011 Tokunaga et al.

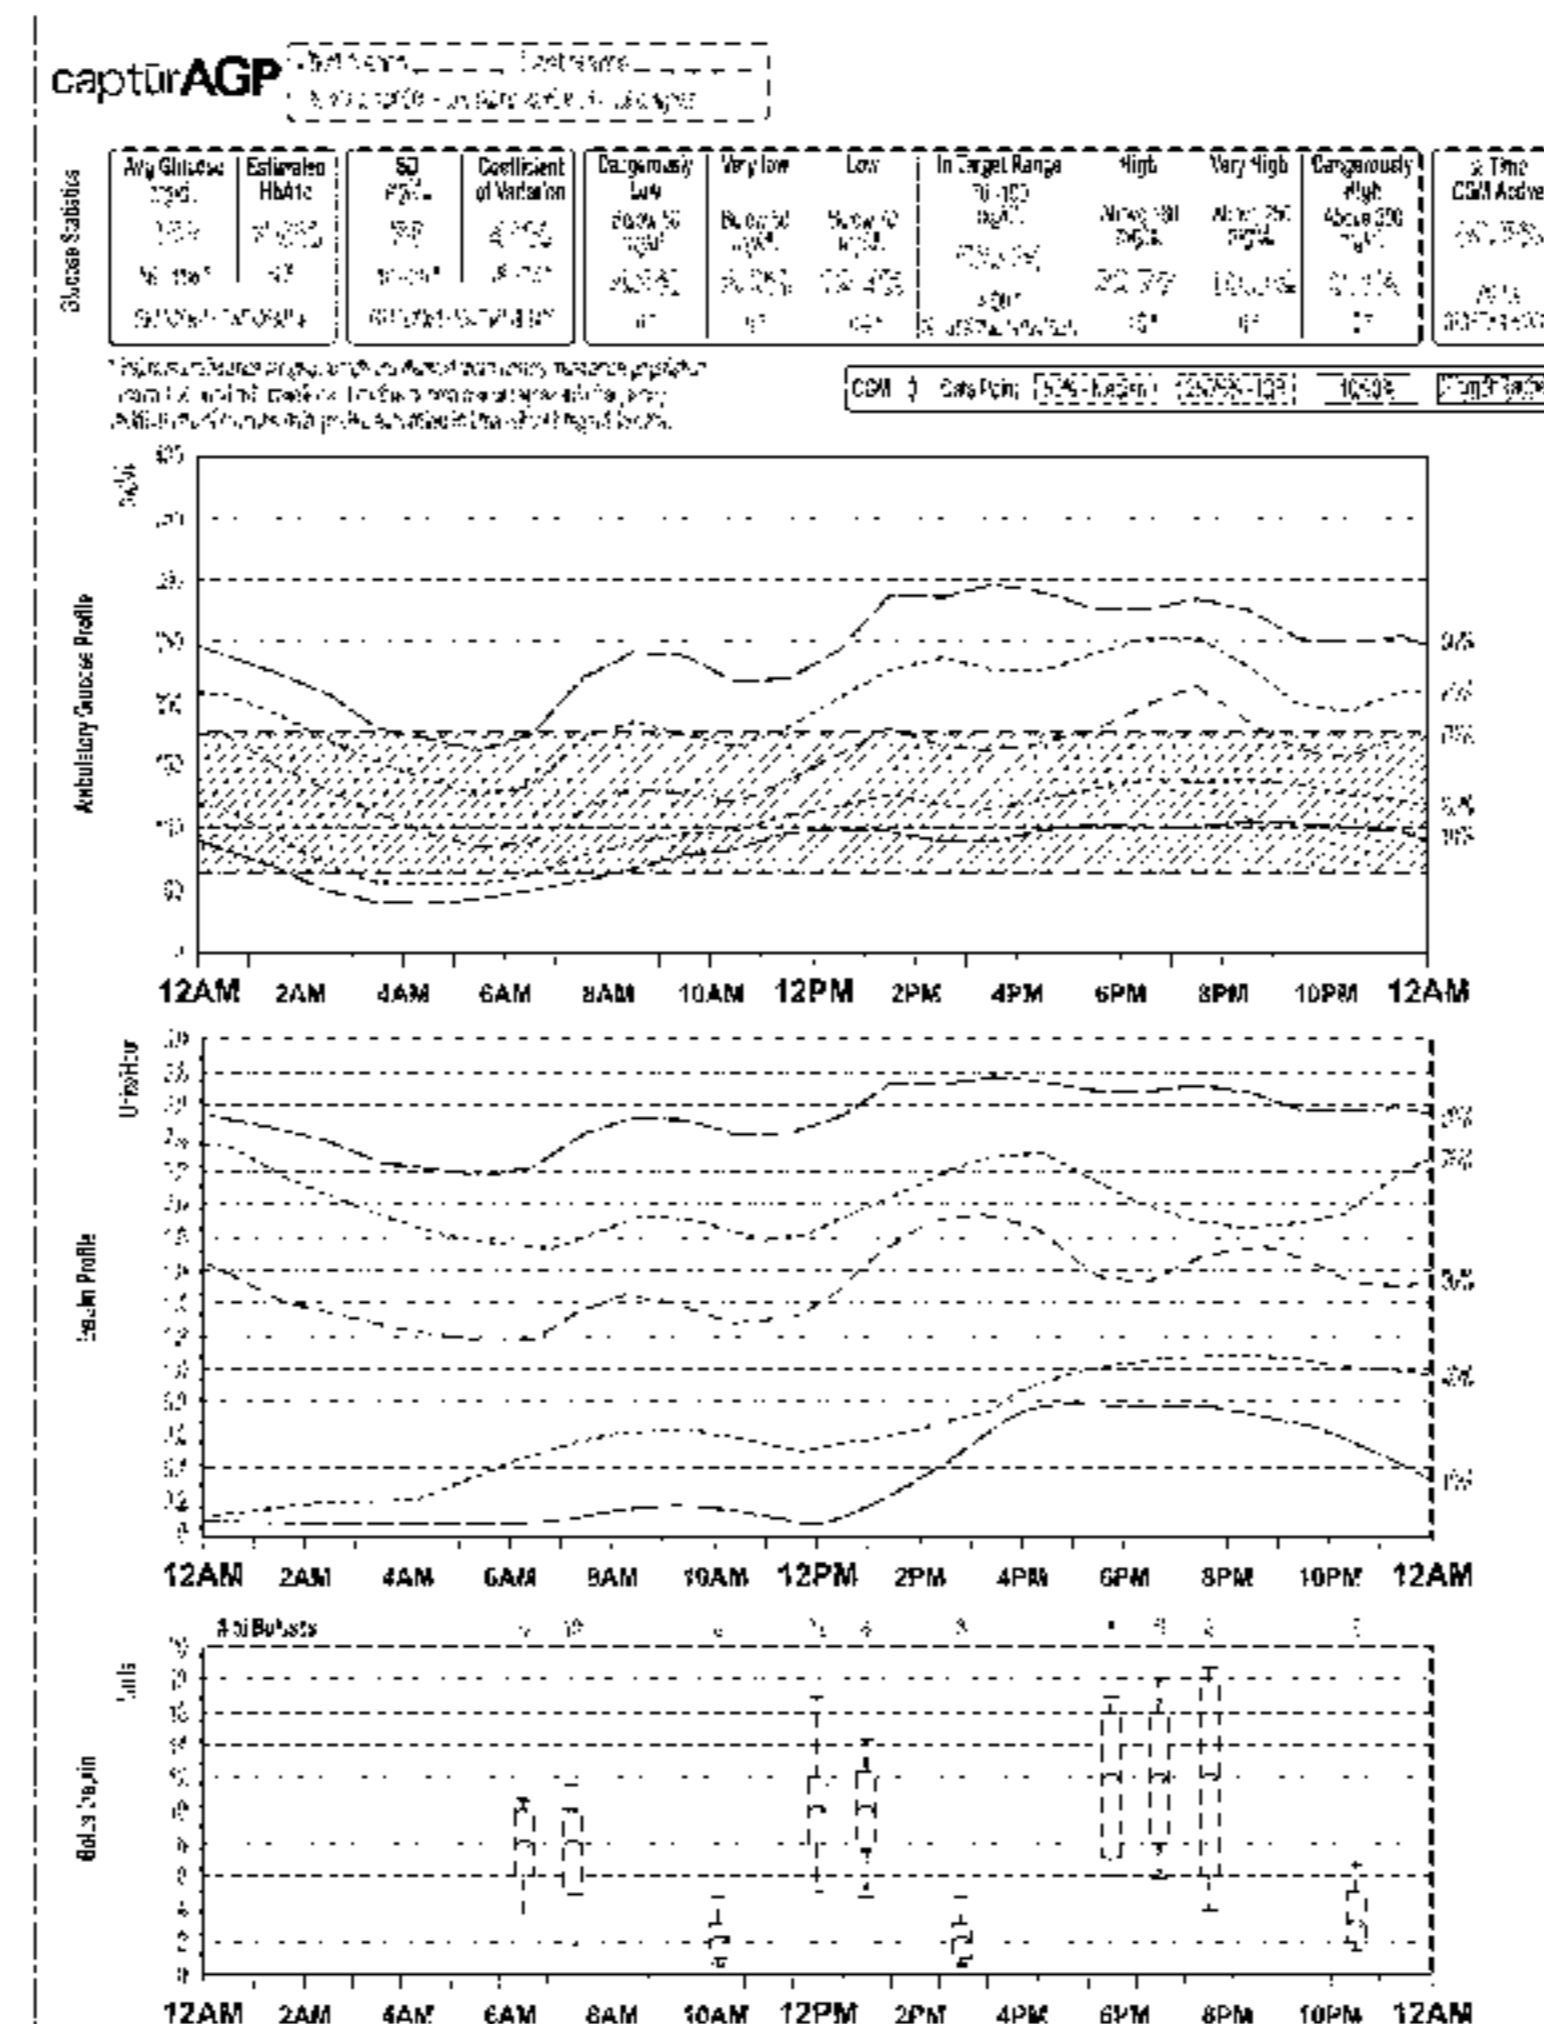

(56)

References Cited

U.S. PATENT DOCUMENTS

D674,404 S 1/2013 Pearcy et al.
 D674,812 S * 1/2013 Joseph D14/486
 D684,172 S 6/2013 Rytt et al.
 D685,810 S 7/2013 Way et al.
 D690,309 S 9/2013 Wenz et al.
 D692,911 S 11/2013 Pearcy et al.
 D709,082 S 7/2014 Meegan et al.
 D709,518 S 7/2014 Meegan et al.
 D710,373 S 8/2014 Meegan et al.
 D717,328 S * 11/2014 Lin D14/486
 D717,331 S * 11/2014 Lin D14/486
 D756,371 S * 5/2016 Bertnick D14/485
 D773,478 S * 12/2016 Wesley D14/485
 D774,058 S * 12/2016 Dias D14/486
 D775,144 S * 12/2016 Vazquez D14/485
 D780,199 S * 2/2017 Croan D14/486
 2002/0193679 A1 12/2002 Malave et al.
 2008/0127052 A1 * 5/2008 Rostoker G06Q 30/02
 717/105
 2009/0029631 A1 * 1/2009 Offer B24D 13/10
 451/28
 2009/0238597 A1 * 9/2009 Cao G03G 15/2039
 399/70
 2010/0096474 A1 * 4/2010 Zhang F01D 9/065
 239/265.17
 2010/0100470 A1 * 4/2010 Buchanan G06Q 10/10
 705/35
 2012/0004947 A1 1/2012 Dombrowski et al.

2014/0028682 A1 * 1/2014 Omiya G09G 5/363
 345/440
 2014/0188400 A1 7/2014 Dunn et al.
 2014/0206970 A1 7/2014 Wesley et al.

OTHER PUBLICATIONS

“1.2 Designing Information Systems”, posted at saylordotorg.github.io, Mar. 26, 2011, [site visited Jun. 1, 2017]. Available from Internet: https://saylordotorg.github.io/text_business-information-systems-design-an-app-for-that/s05-02-designing-information-systems.html.*
 “Ambulatory Blood Pressure and Cardiovascular Outcome in Relation to Perceived Sleep Deprivation”, posted at hyper.ahajournals.org, Mar. 21, 2007, [site visited Jun. 1, 2017]. Available from Internet: <http://hyper.ahajournals.org/content/49/4/777/tab-article-info>.*
 “Wall St. Warrior”, posted at traderjamie.blogspot.com, Sep. 3, 2011, [site visited Jun. 1, 2017]. Available from Internet: <http://traderjamie.blogspot.com/2011/09/technical-picture-bearish-island.html>.*
 PCT International Searching Authority, International Search Report and Written Opinion mailed on Sep. 5, 2014 for Int’1 Application No. PCT/US2014/012549, 11 pages.
 Bergenstal MD, Rich, SMBG & CGM in Clinical Practice, Barbara Davis Center Keystone Conference 2012, Jul. 15, 2012, 50 pages.
 Mazze, Roger S., Characterizing Glucose Exposure for Individuals with Normal Glucose Tolerance Using continuous Glucose Monitoring and Ambulatory Glucose Profile Analysis, Diabetes Technology & Therapeutics, vol. 10, No. 3, Jun. 1, 2008, pp. 149-159.

* cited by examiner

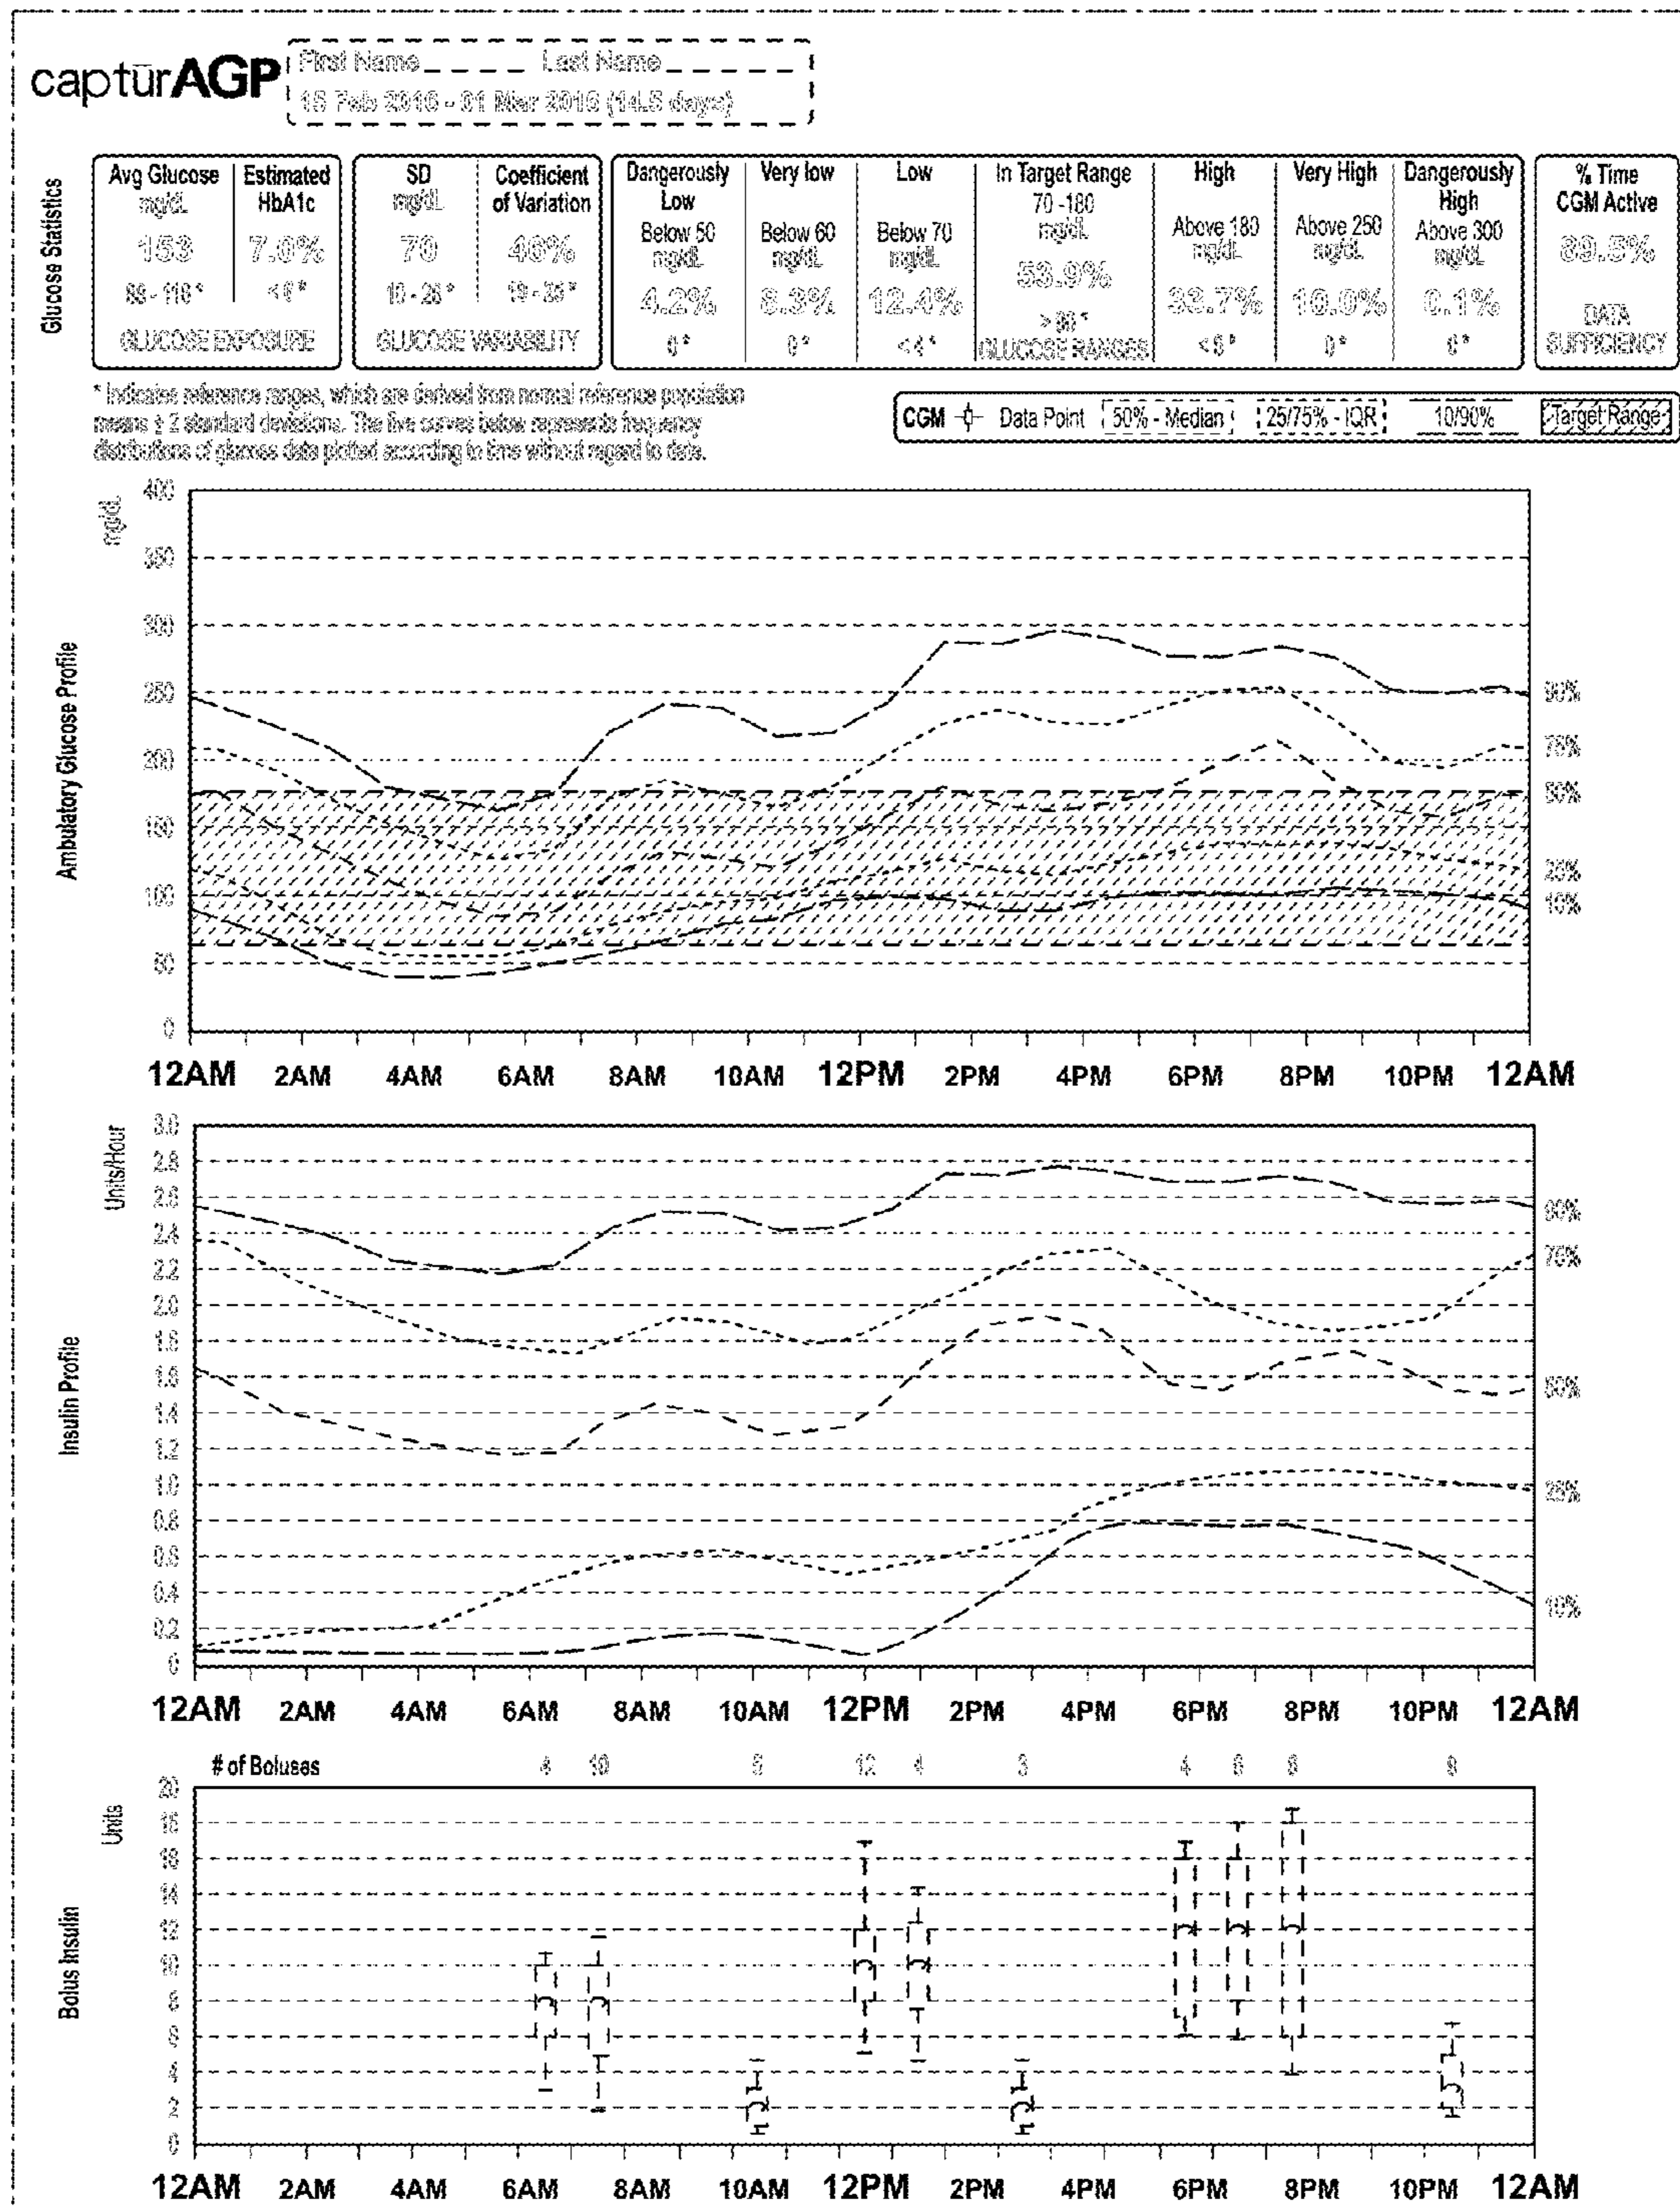


FIG. 1

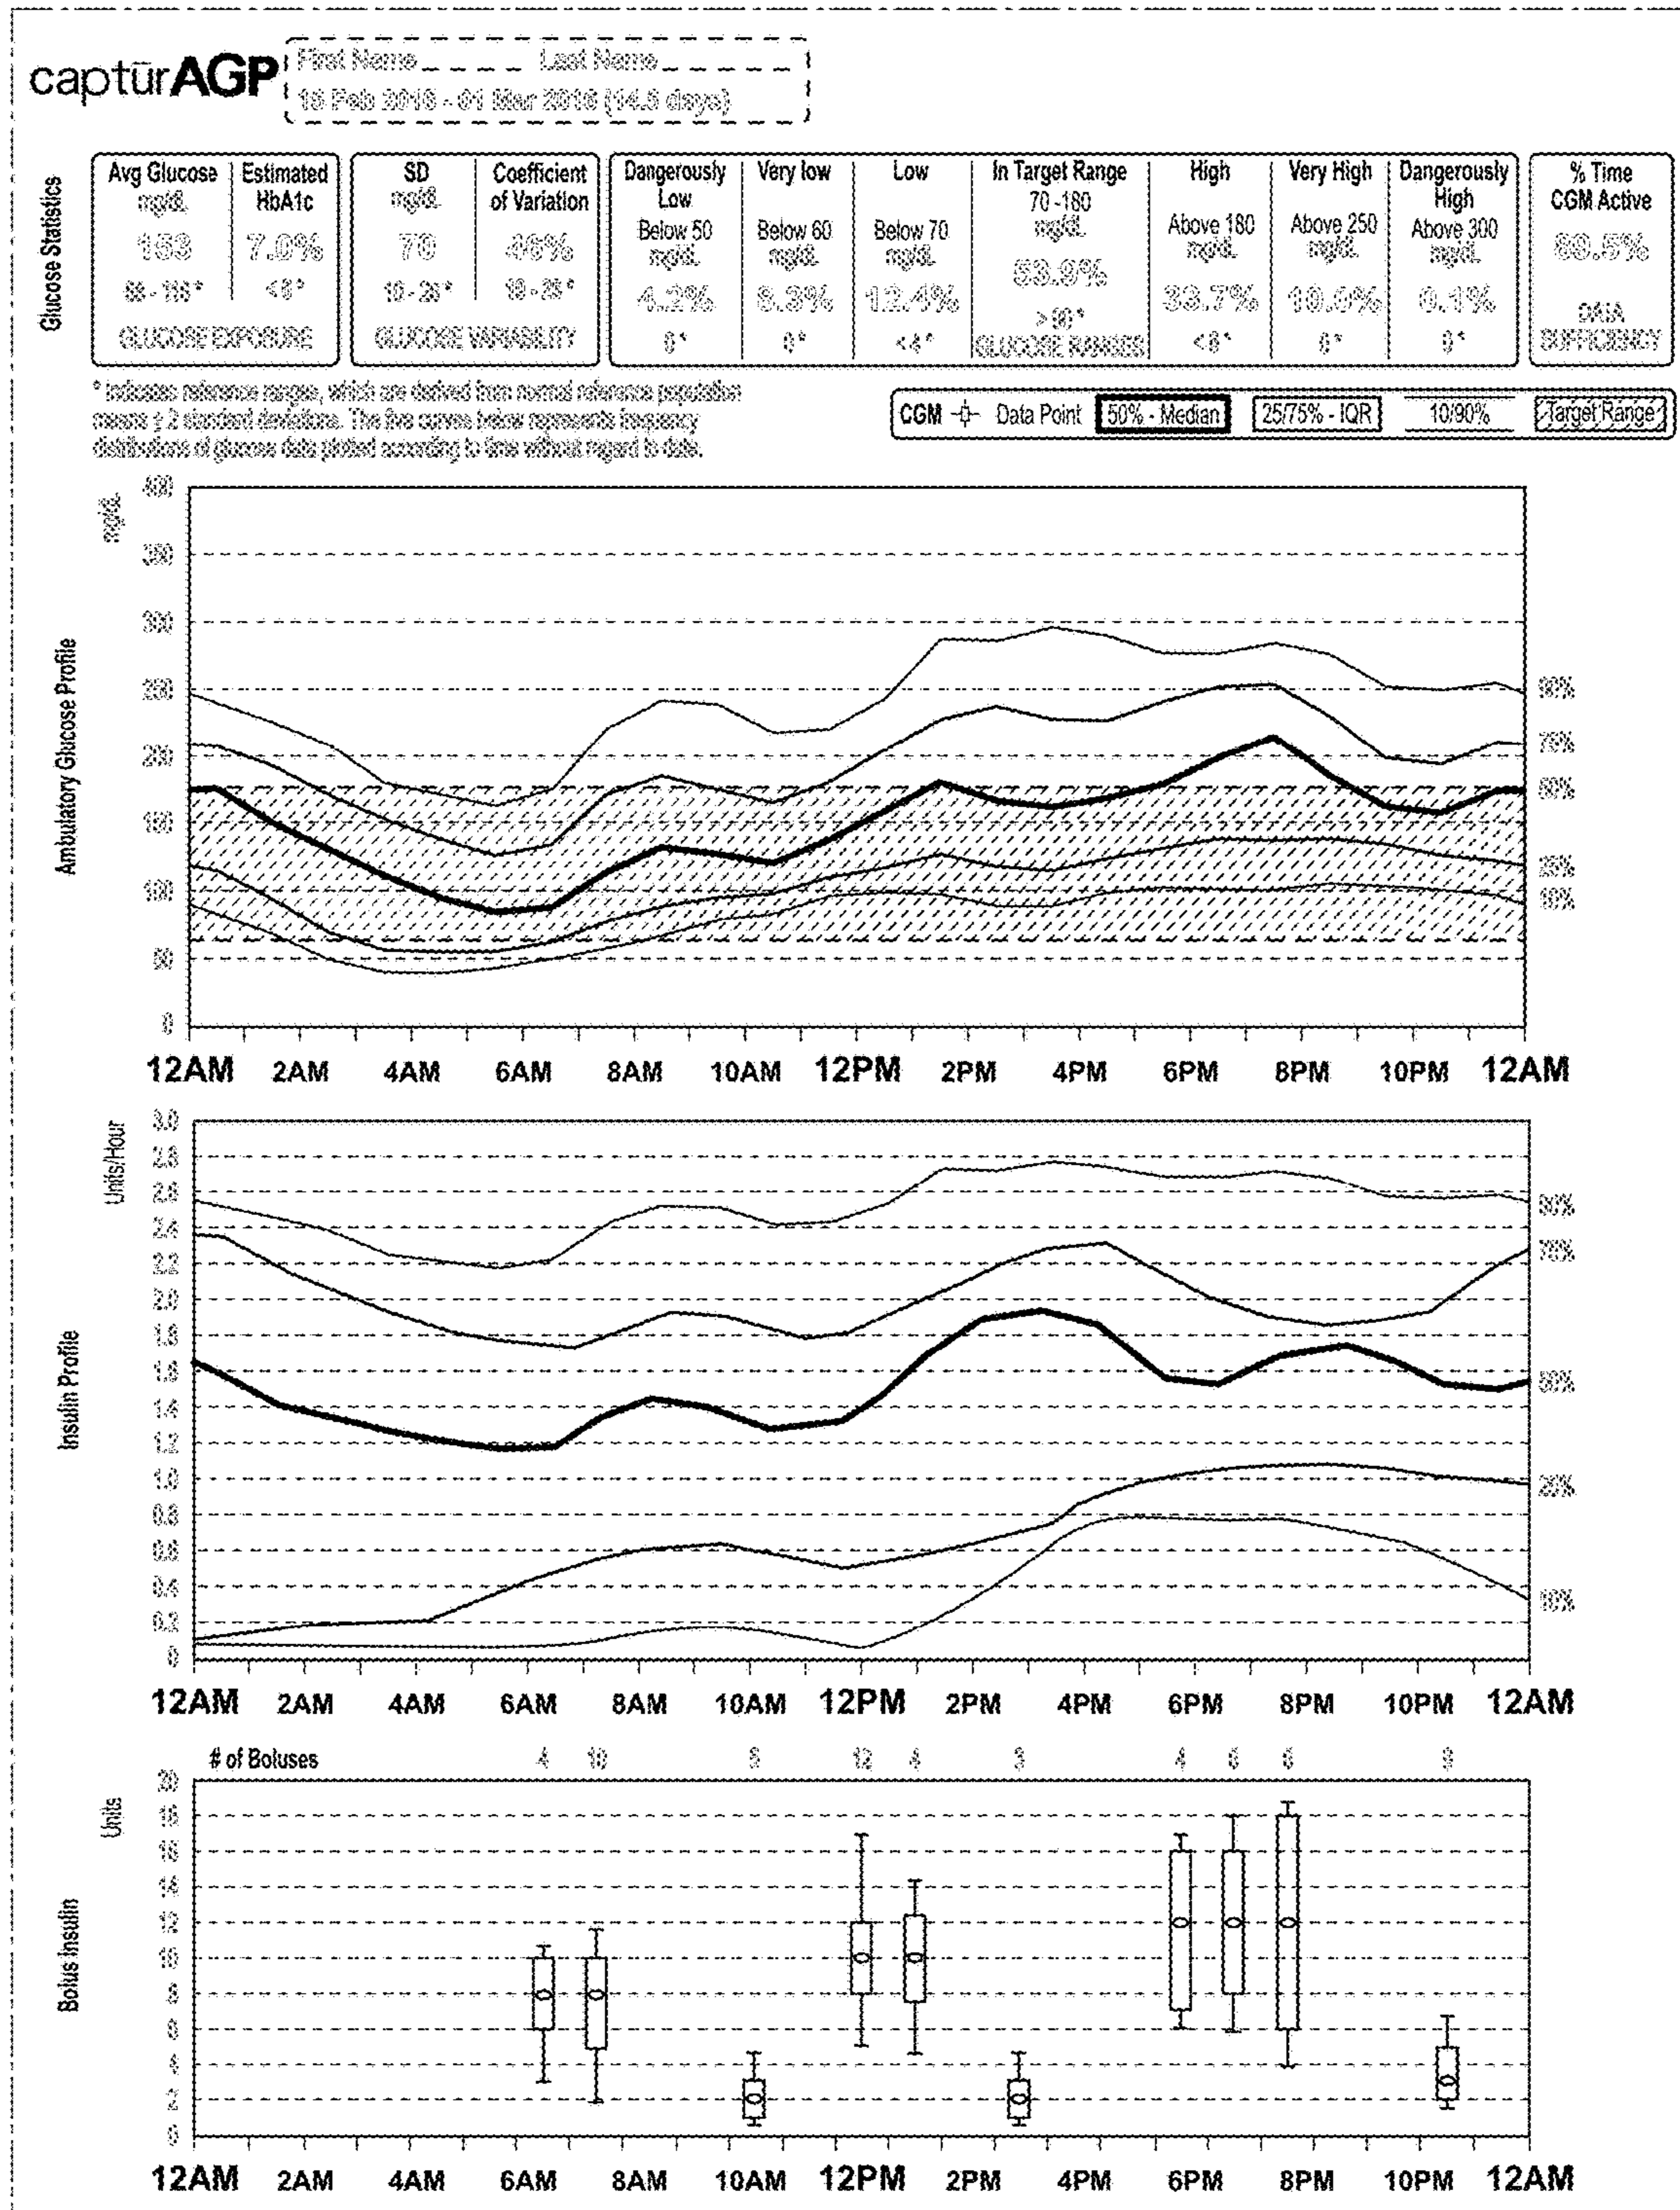


FIG. 2