



US00D805643S

(12) **United States Design Patent** (10) **Patent No.:** **US D805,643 S**
Wu (45) **Date of Patent:** **** Dec. 19, 2017**

(54) **INTELLIGENT HEART RATE MONITOR RING**
(71) Applicant: **Shenzhen DO Intelligent Technology Co., Ltd., Shenzhen (CN)**
(72) Inventor: **Da-Jun Wu, Shenzhen (CN)**
(73) Assignee: **SHENZHEN DO INTELLIGENT TECHNOLOGY CO., LTD., Shenzhen (CN)**
(**) Term: **15 Years**
(21) Appl. No.: **29/568,751**
(22) Filed: **Jun. 21, 2016**

(30) **Foreign Application Priority Data**
Dec. 22, 2015 (CN) 2015 3 0550938
(51) **LOC (10) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/167**
(58) **Field of Classification Search**
USPC D24/107, 164-168, 186; D10/1, 30-40, D10/70, 75, 78, 97, 98, 103; D11/3; D14/344, 511; 600/485, 490, 503
CPC A61B 5/0402; A61B 5/0404; A61B 5/021; A61B 5/024; A61B 5/02438; A61B 5/81; A61B 5/22; A61B 5/0225; A61B 5/681; A61B 5/0008; A61B 5/02141; A61B 5/742; A61B 2650/00
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
D611,150 S * 3/2010 Omaki D24/165
D616,099 S * 5/2010 Shibata D24/165
D637,094 S * 5/2011 Cobbett D10/32

D637,506 S * 5/2011 Toyoshima D10/70
D645,360 S * 9/2011 Kiser D10/32
D711,002 S * 8/2014 Ohnemus D24/186
D720,074 S * 12/2014 Suvilaakso D24/167
D721,292 S * 1/2015 Choi D10/70
D729,657 S * 5/2015 Behar D10/70
D729,658 S * 5/2015 Behar D10/70
D734,176 S * 7/2015 Isaacs D10/30
D738,759 S * 9/2015 Behar D10/39
D740,140 S * 10/2015 Behar D10/39
D740,702 S * 10/2015 Behar D10/39
D740,703 S * 10/2015 Behar D10/39
D742,529 S * 11/2015 Huffman D24/186
D744,356 S * 12/2015 Akana D10/70
D745,421 S * 12/2015 Akana D10/32
D746,477 S * 12/2015 Cha D24/186
D747,714 S * 1/2016 Erbeus D10/32
D749,002 S * 2/2016 Park D10/70
D751,069 S * 3/2016 Choi D10/32
D757,583 S * 5/2016 Roush D10/70


(Continued)

Primary Examiner — Wan Laymon
Assistant Examiner — Clint A Samuel
(74) *Attorney, Agent, or Firm* — WPAT, PC

(57) **CLAIM**
The ornamental design for an intelligent heart rate monitor ring, as shown and described.

DESCRIPTION
FIG. 1 is a perspective view of the intelligent heart rate monitor ring showing my new design.
FIG. 2 is a front view thereof;
FIG. 3 is a back view thereof;
FIG. 4 is a left view thereof;
FIG. 5 is a right view thereof;
FIG. 6 is a top view thereof;
FIG. 7 is a bottom view thereof; and
FIG. 8 is an another perspective view thereof; and,
FIG. 9 is a reference drawing when the ornamental design is in an unfolded status.

1 Claim, 9 Drawing Sheets

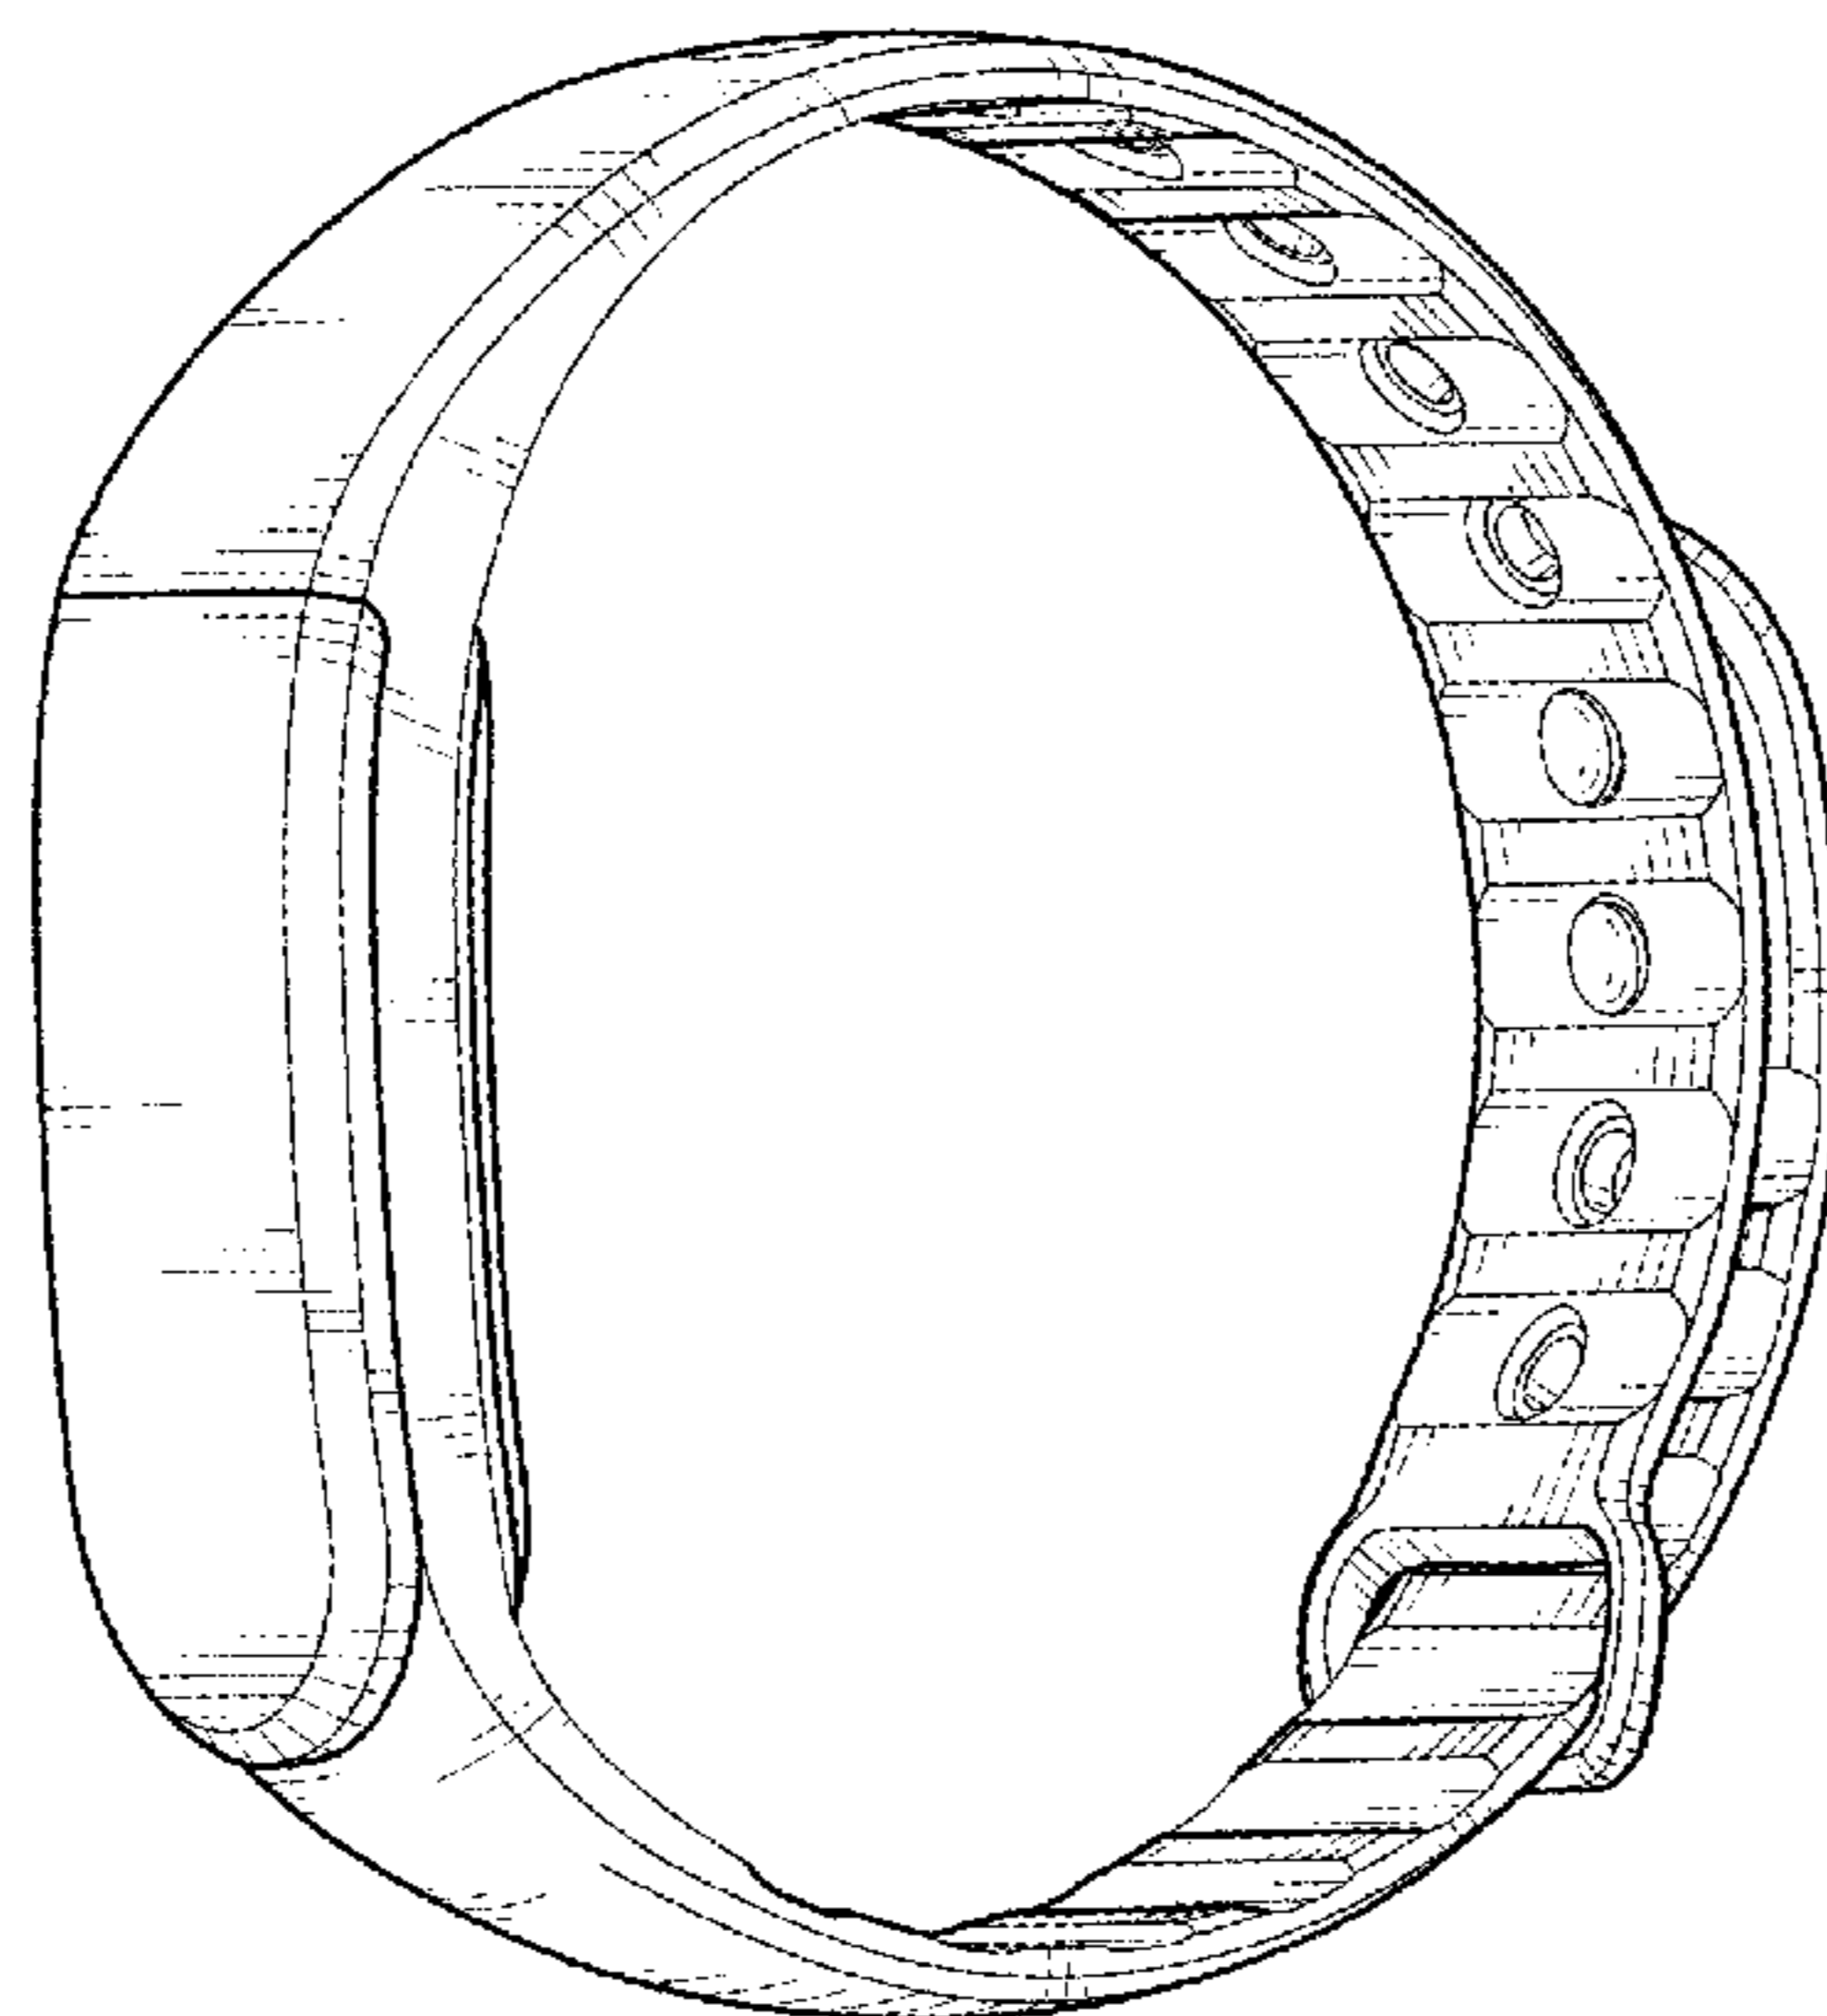

(56)

References Cited

U.S. PATENT DOCUMENTS

D760,391 S * 6/2016 Eshita D24/165
D766,758 S * 9/2016 Park D10/70
D767,769 S * 9/2016 Suvilaakso D24/186
D772,867 S * 11/2016 Park D10/39
D772,868 S * 11/2016 Park D10/39
D772,871 S * 11/2016 Park D14/138 R
D773,052 S * 11/2016 Wimmer, IV D10/103
D777,590 S * 1/2017 Nielsen D10/39
D779,989 S * 2/2017 Lee D10/70
D786,241 S * 5/2017 Chuang D14/344
D789,929 S * 6/2017 Tan D14/344

* cited by examiner

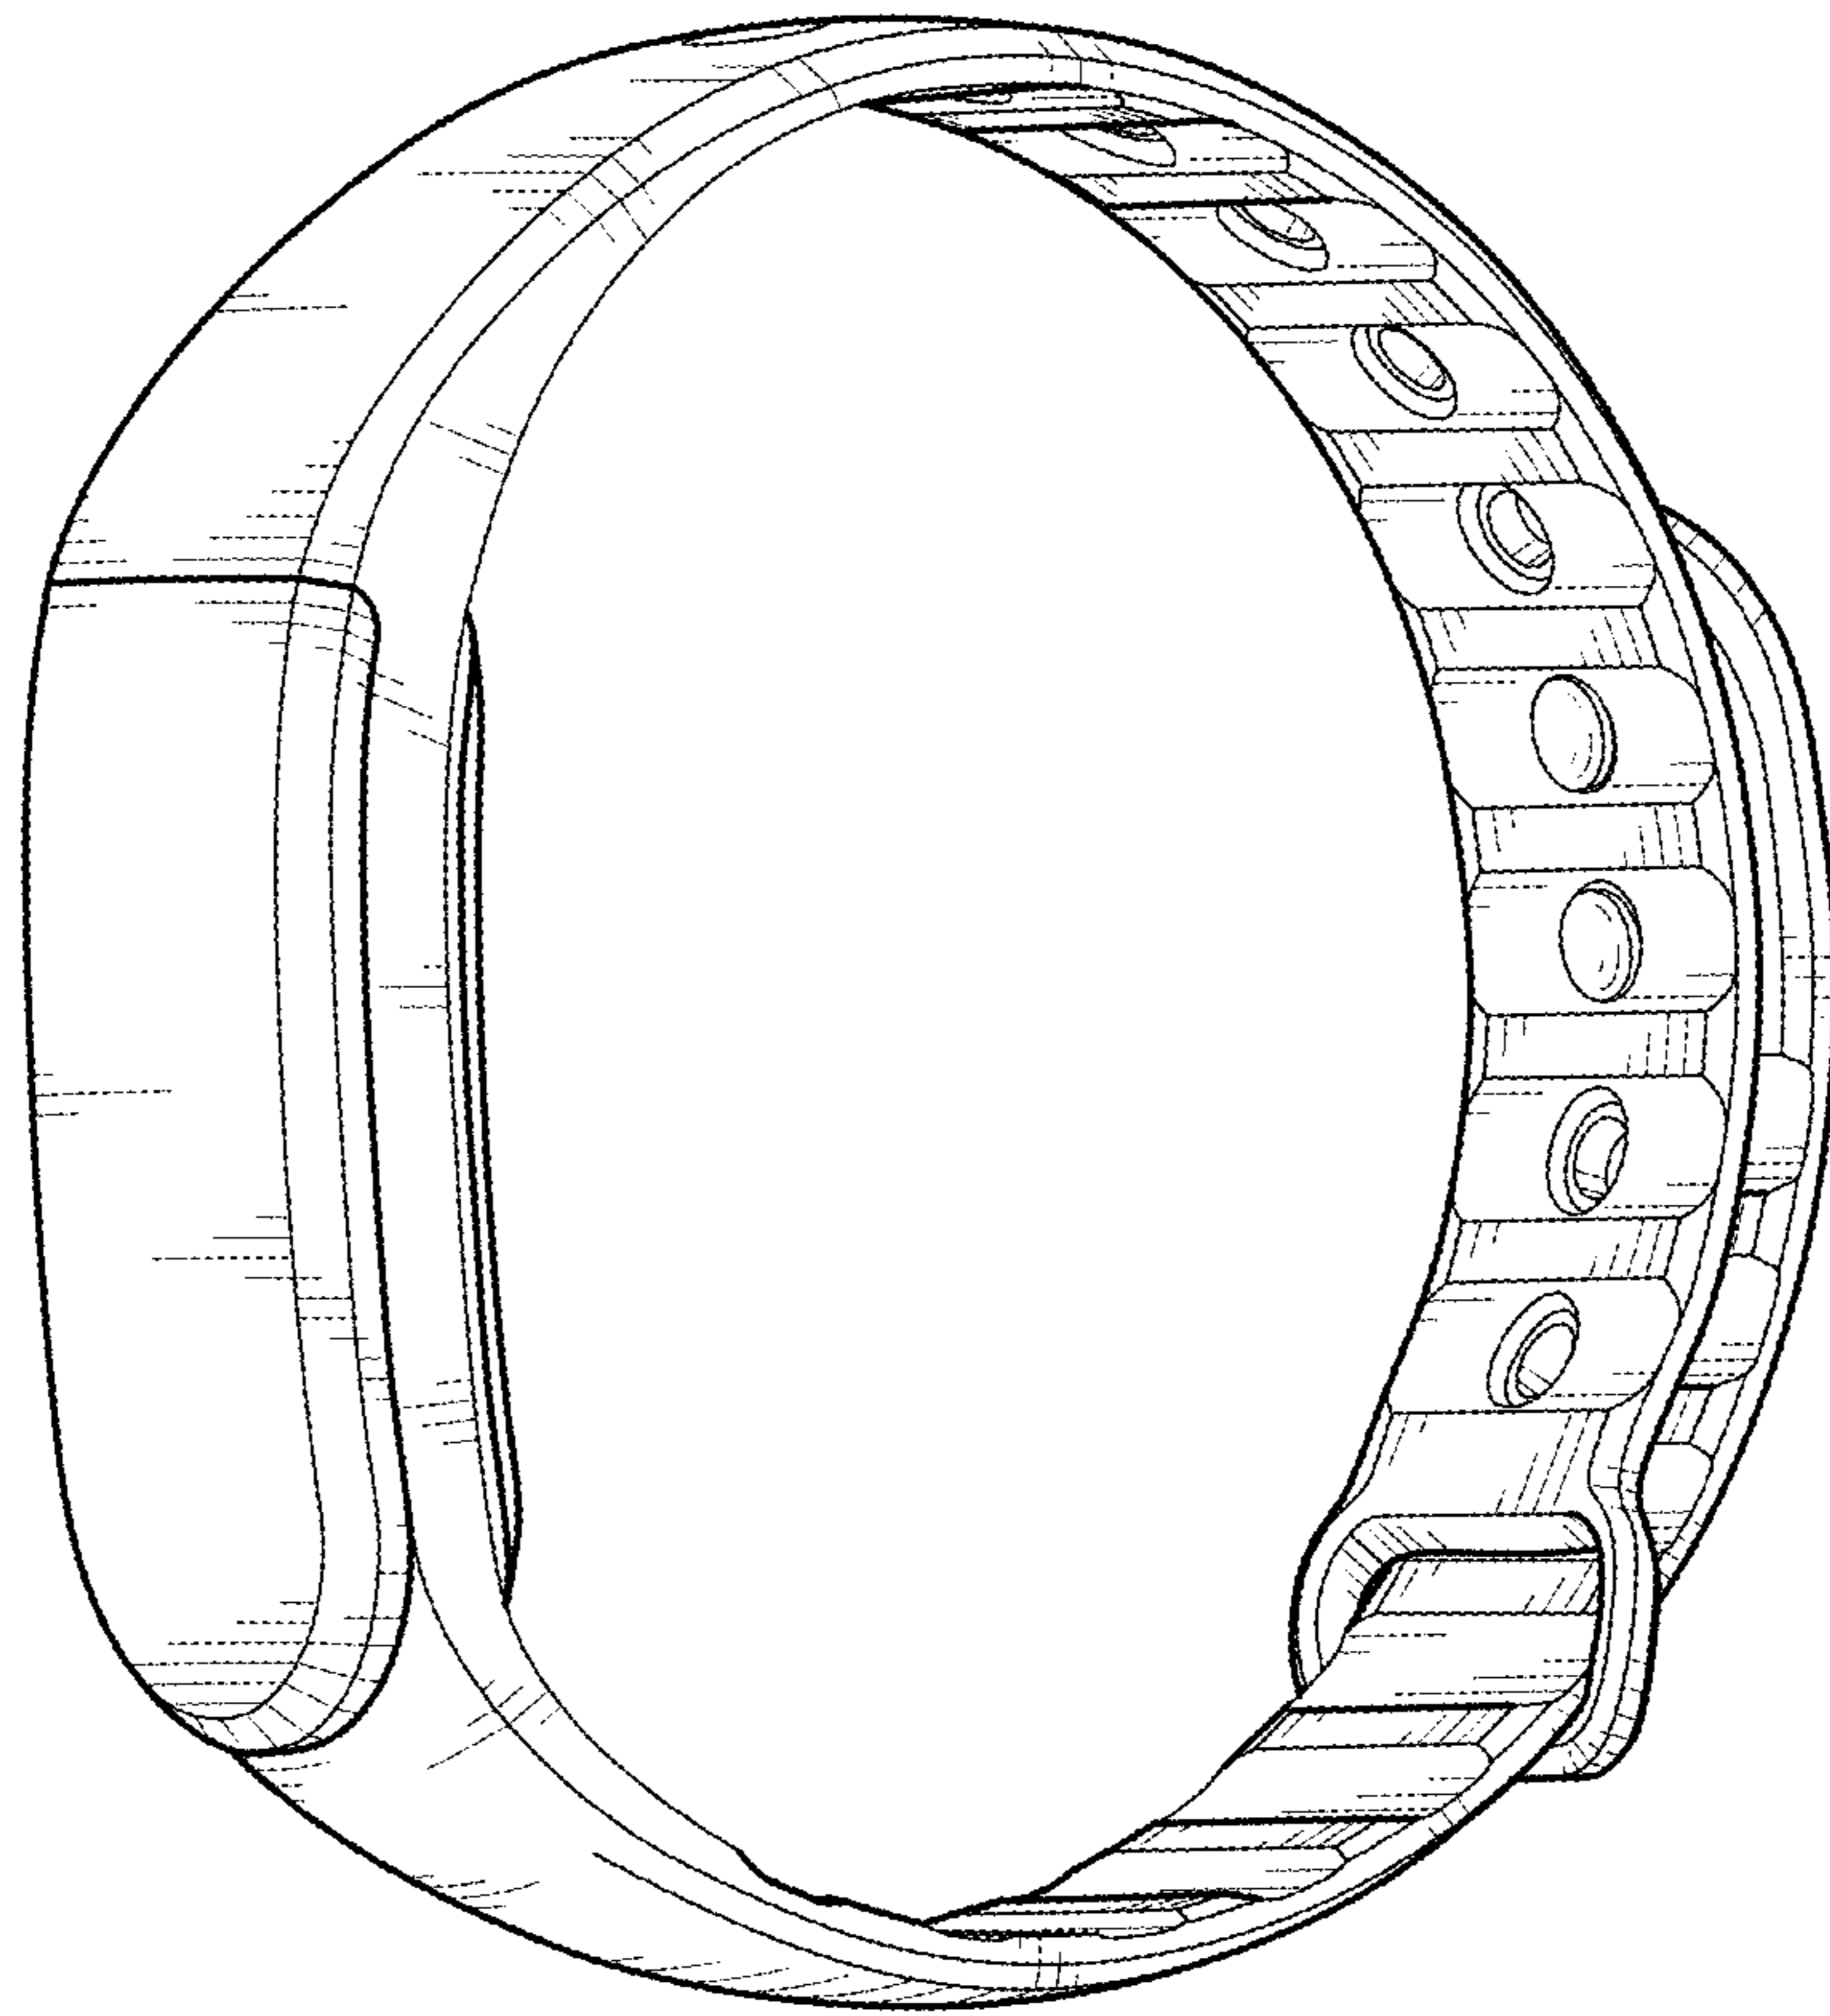


FIG. 1

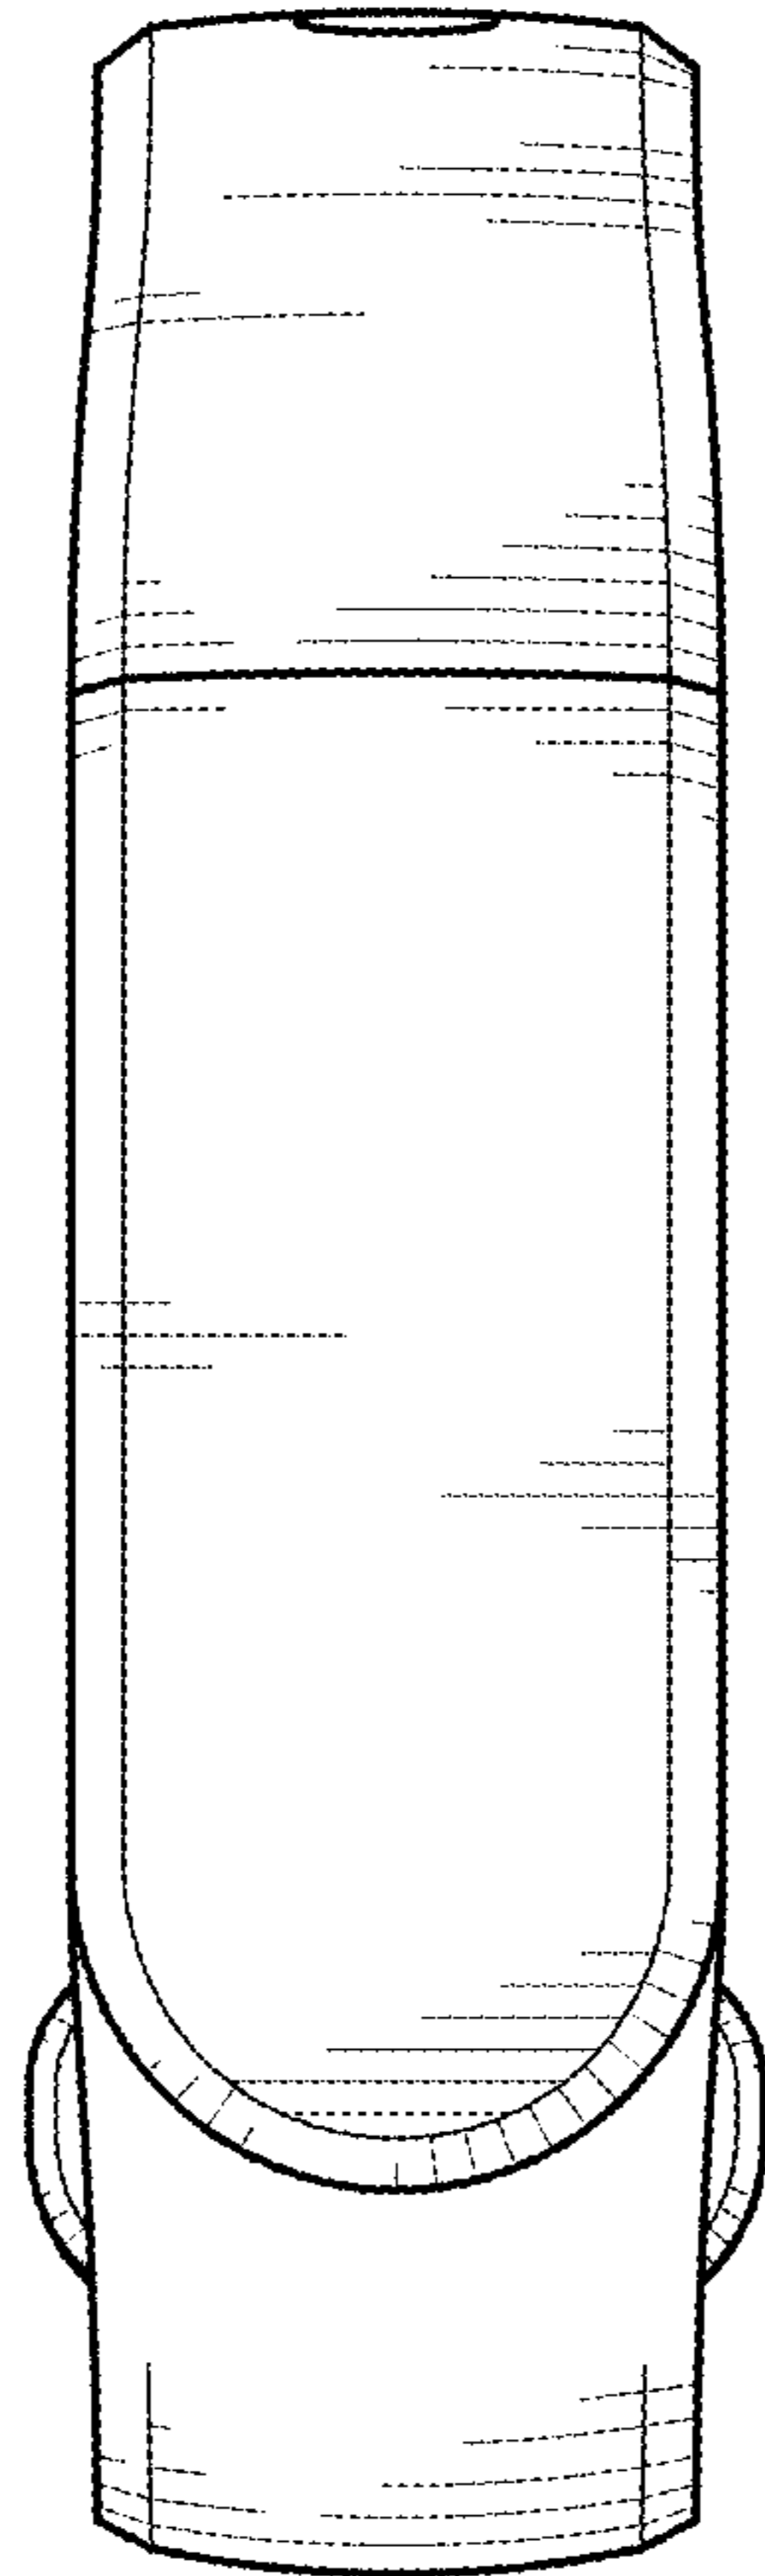


FIG. 2

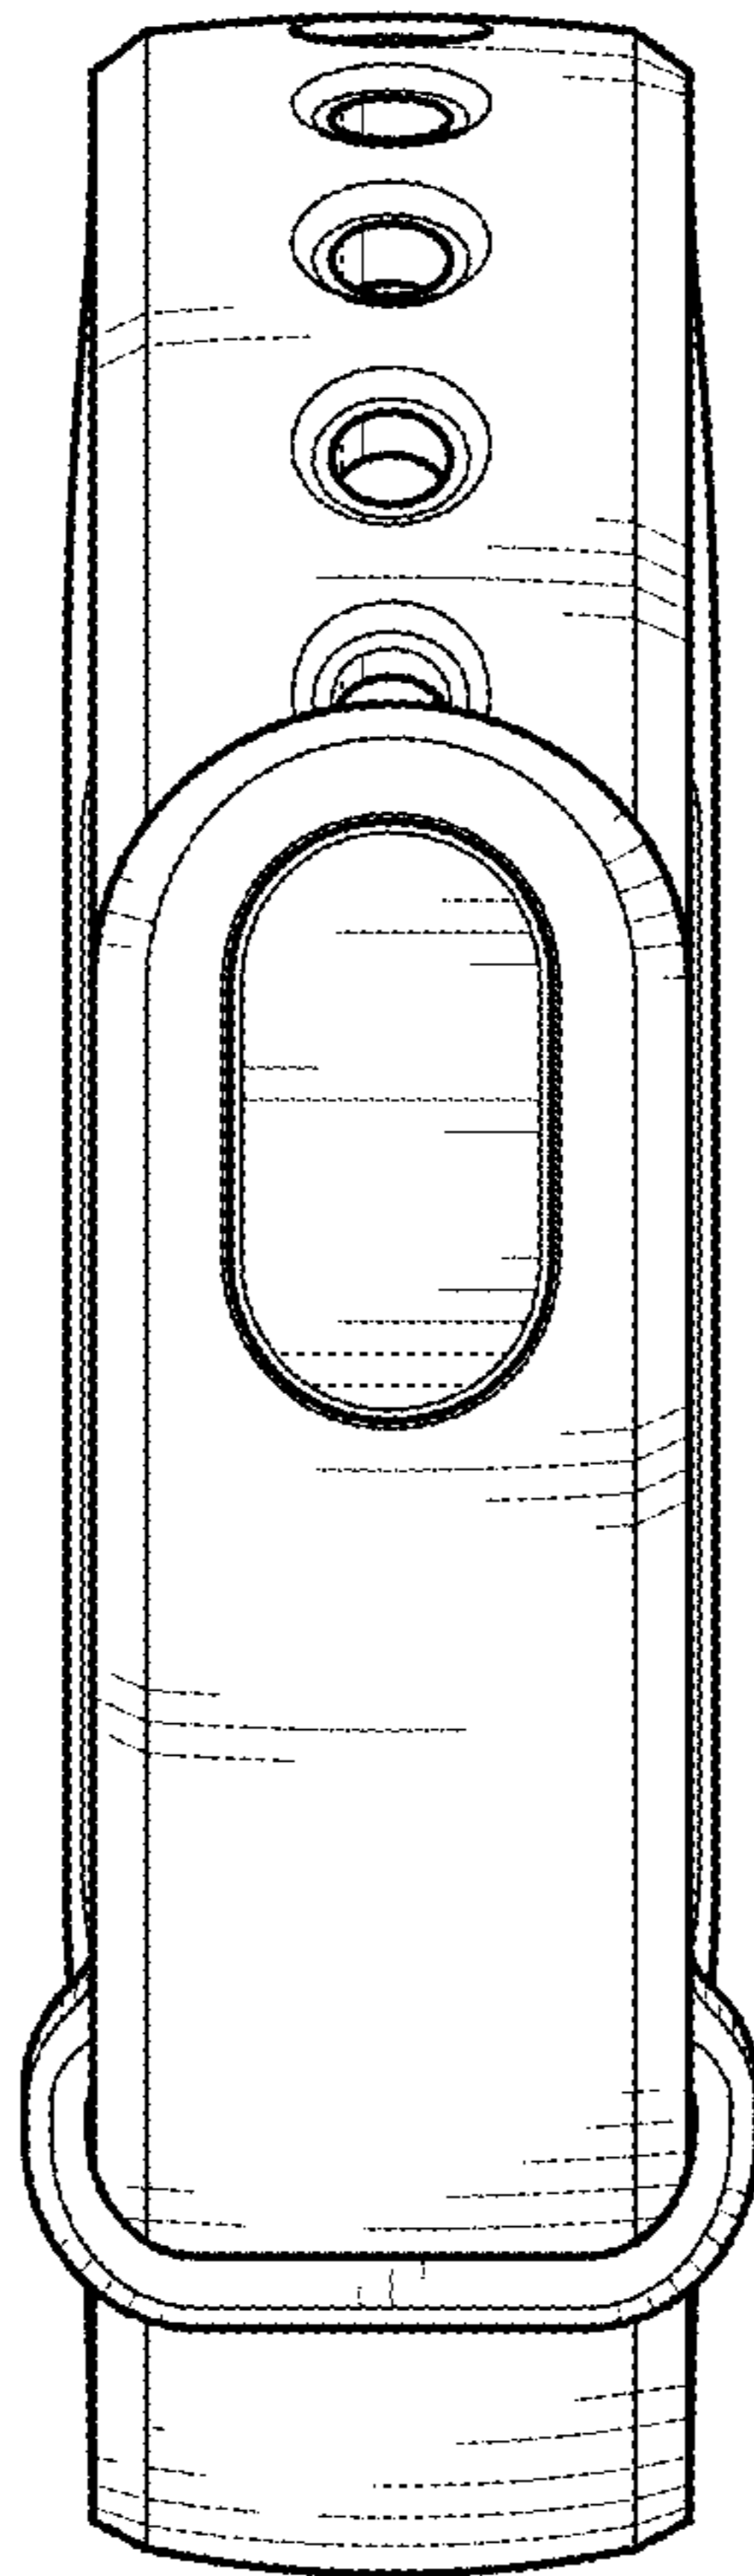


FIG. 3

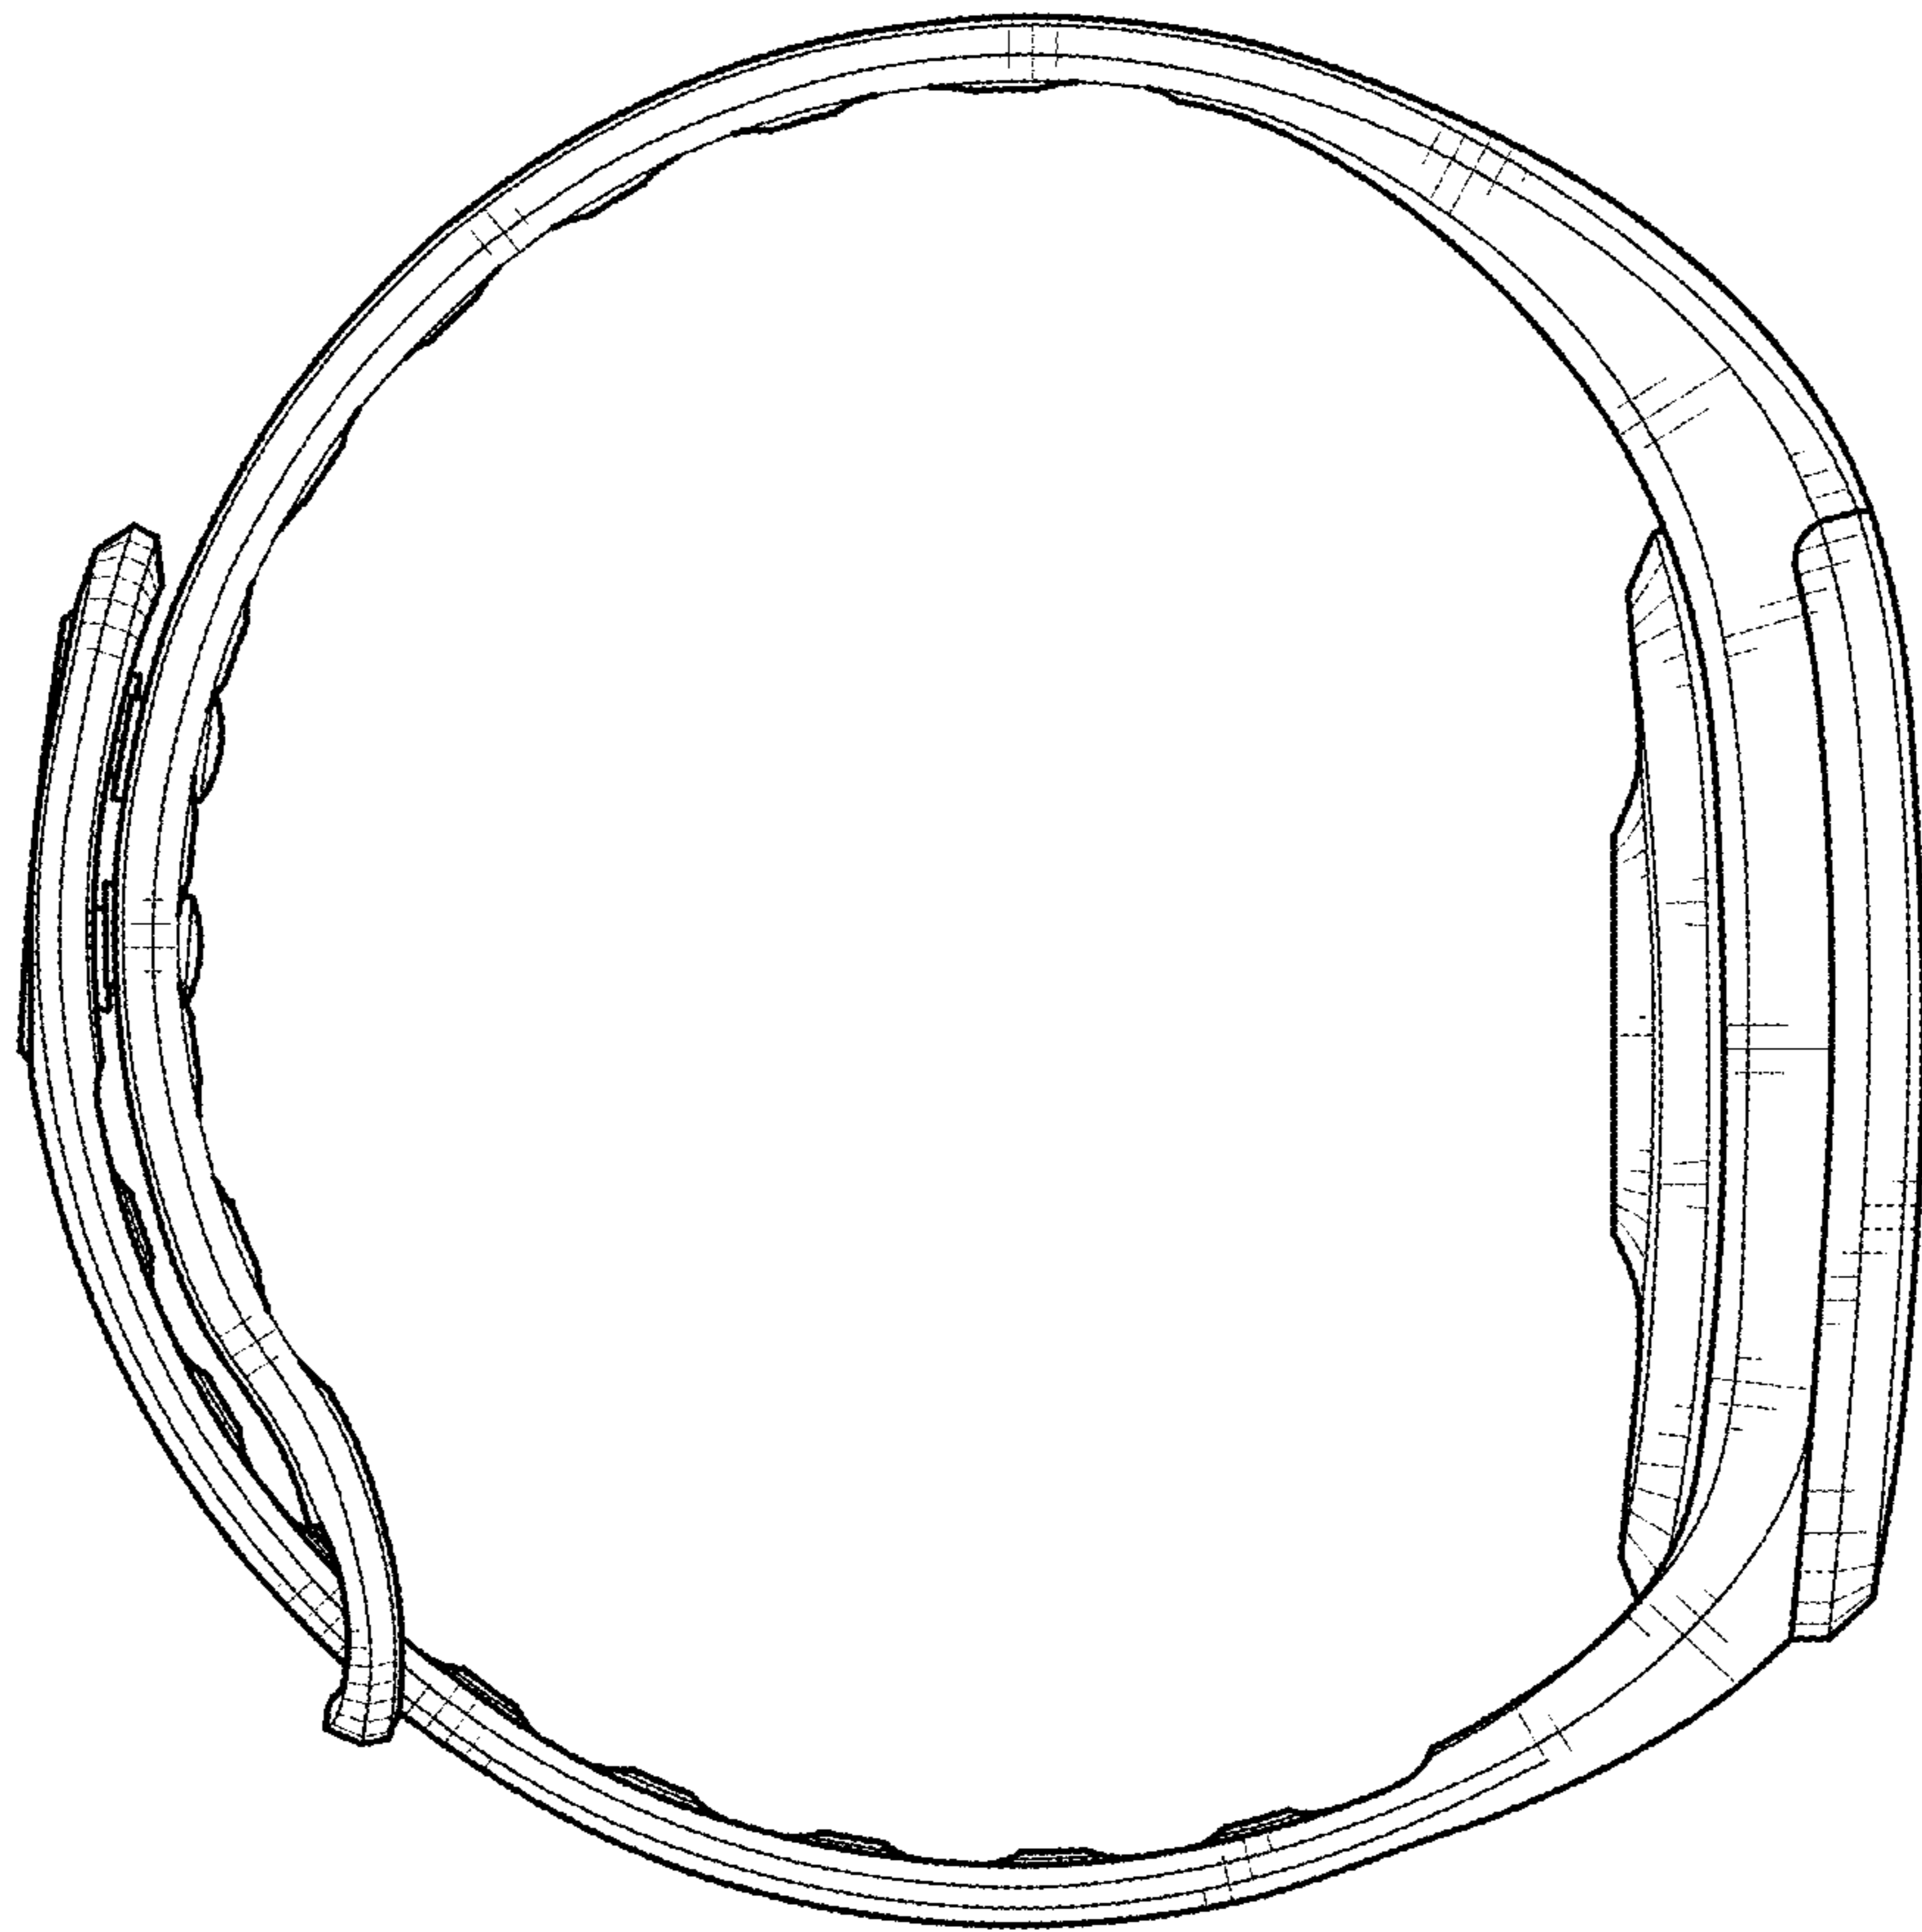


FIG. 4

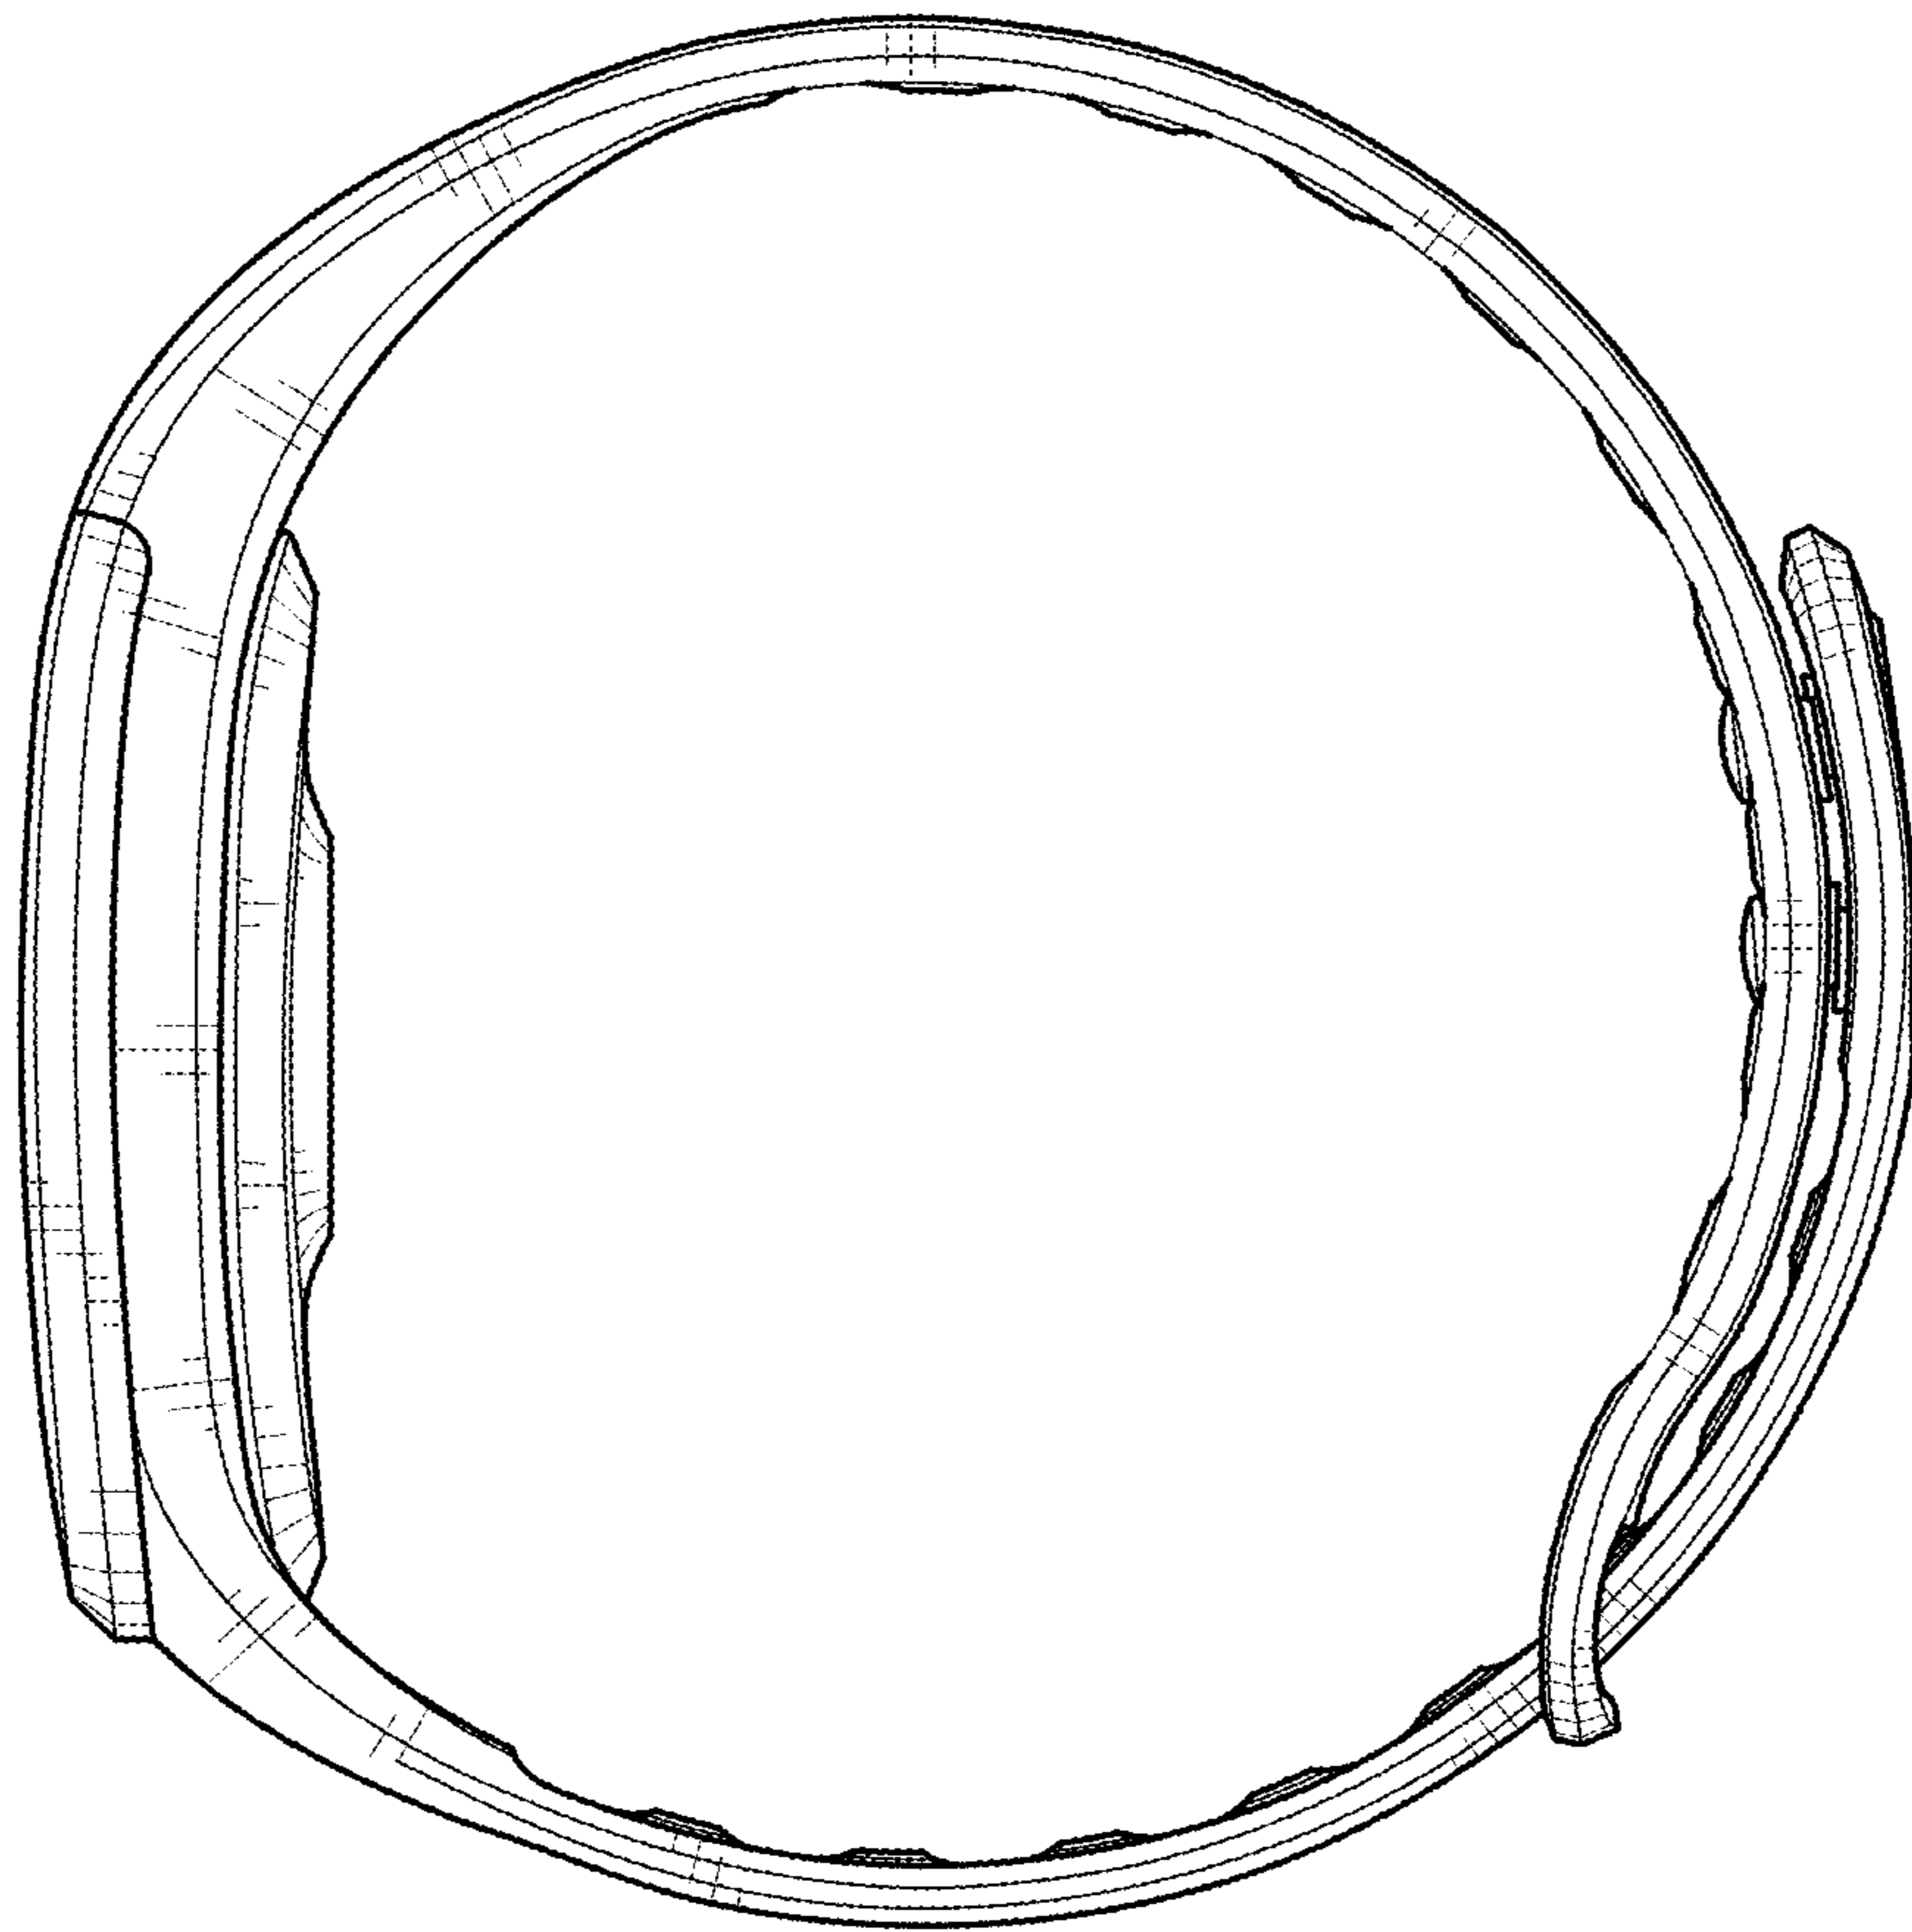


FIG. 5

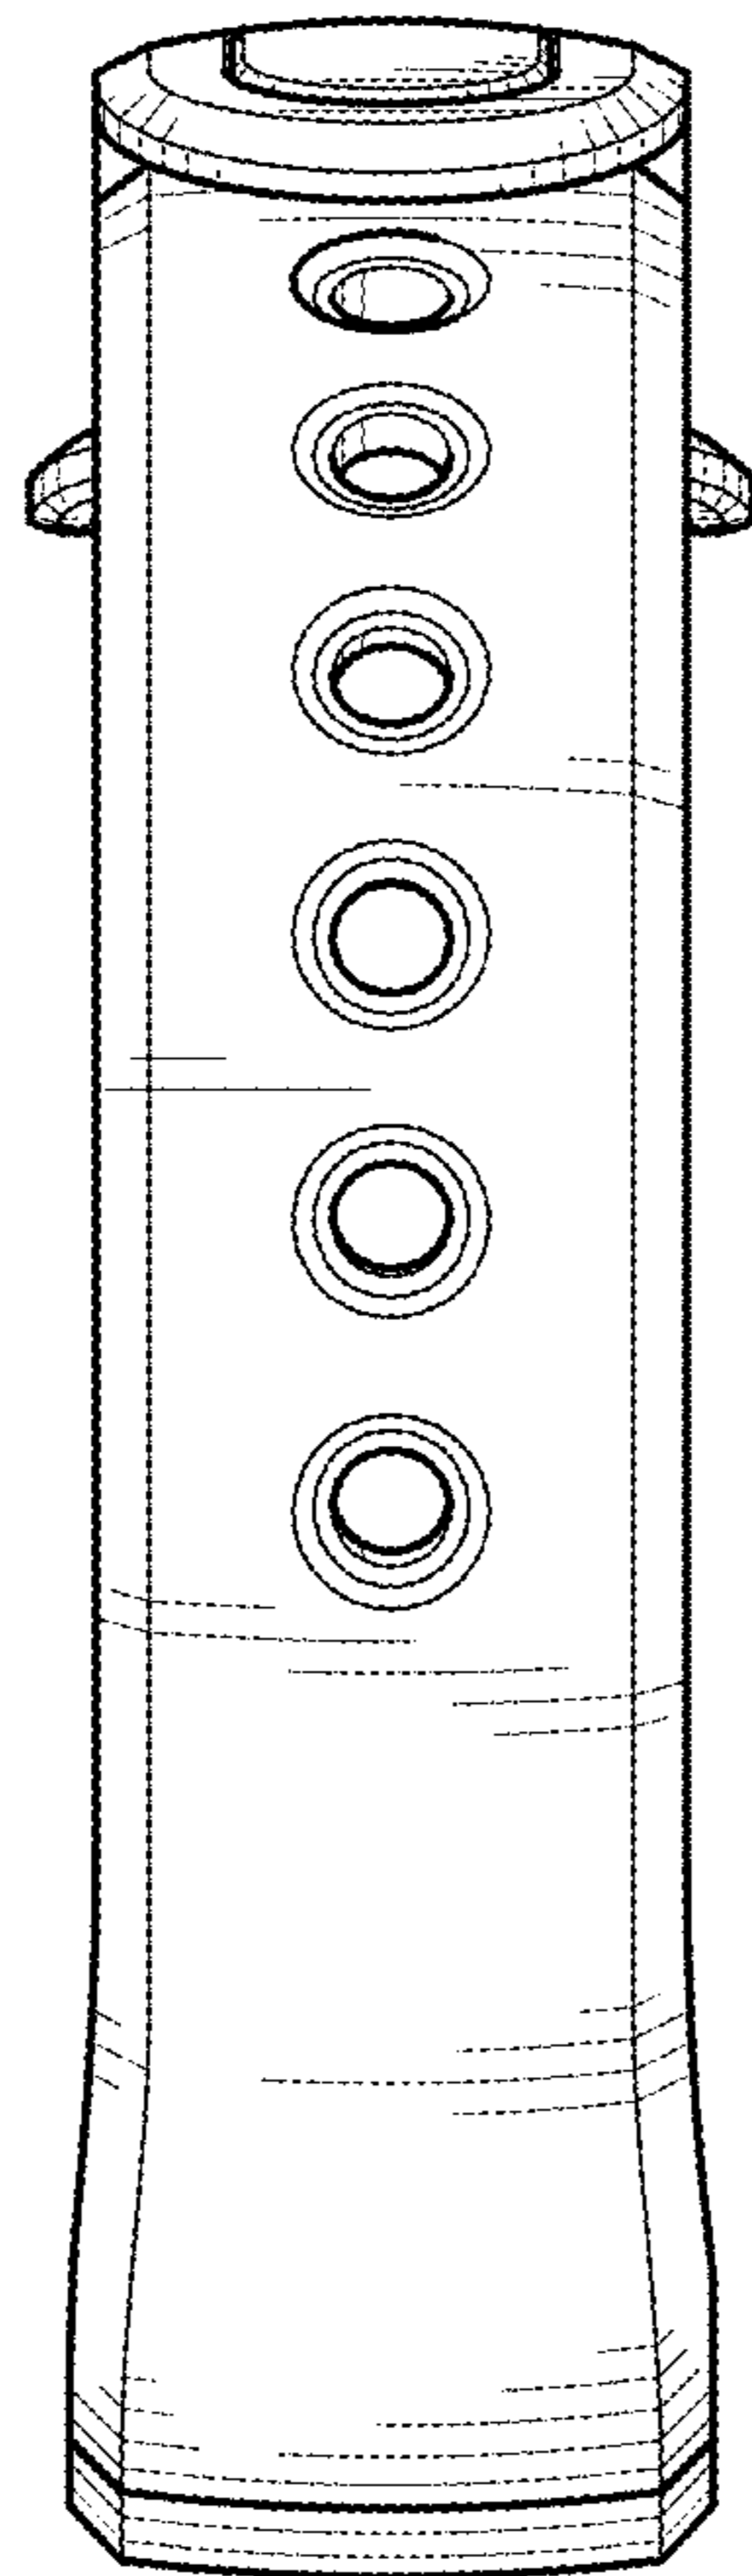


FIG. 6

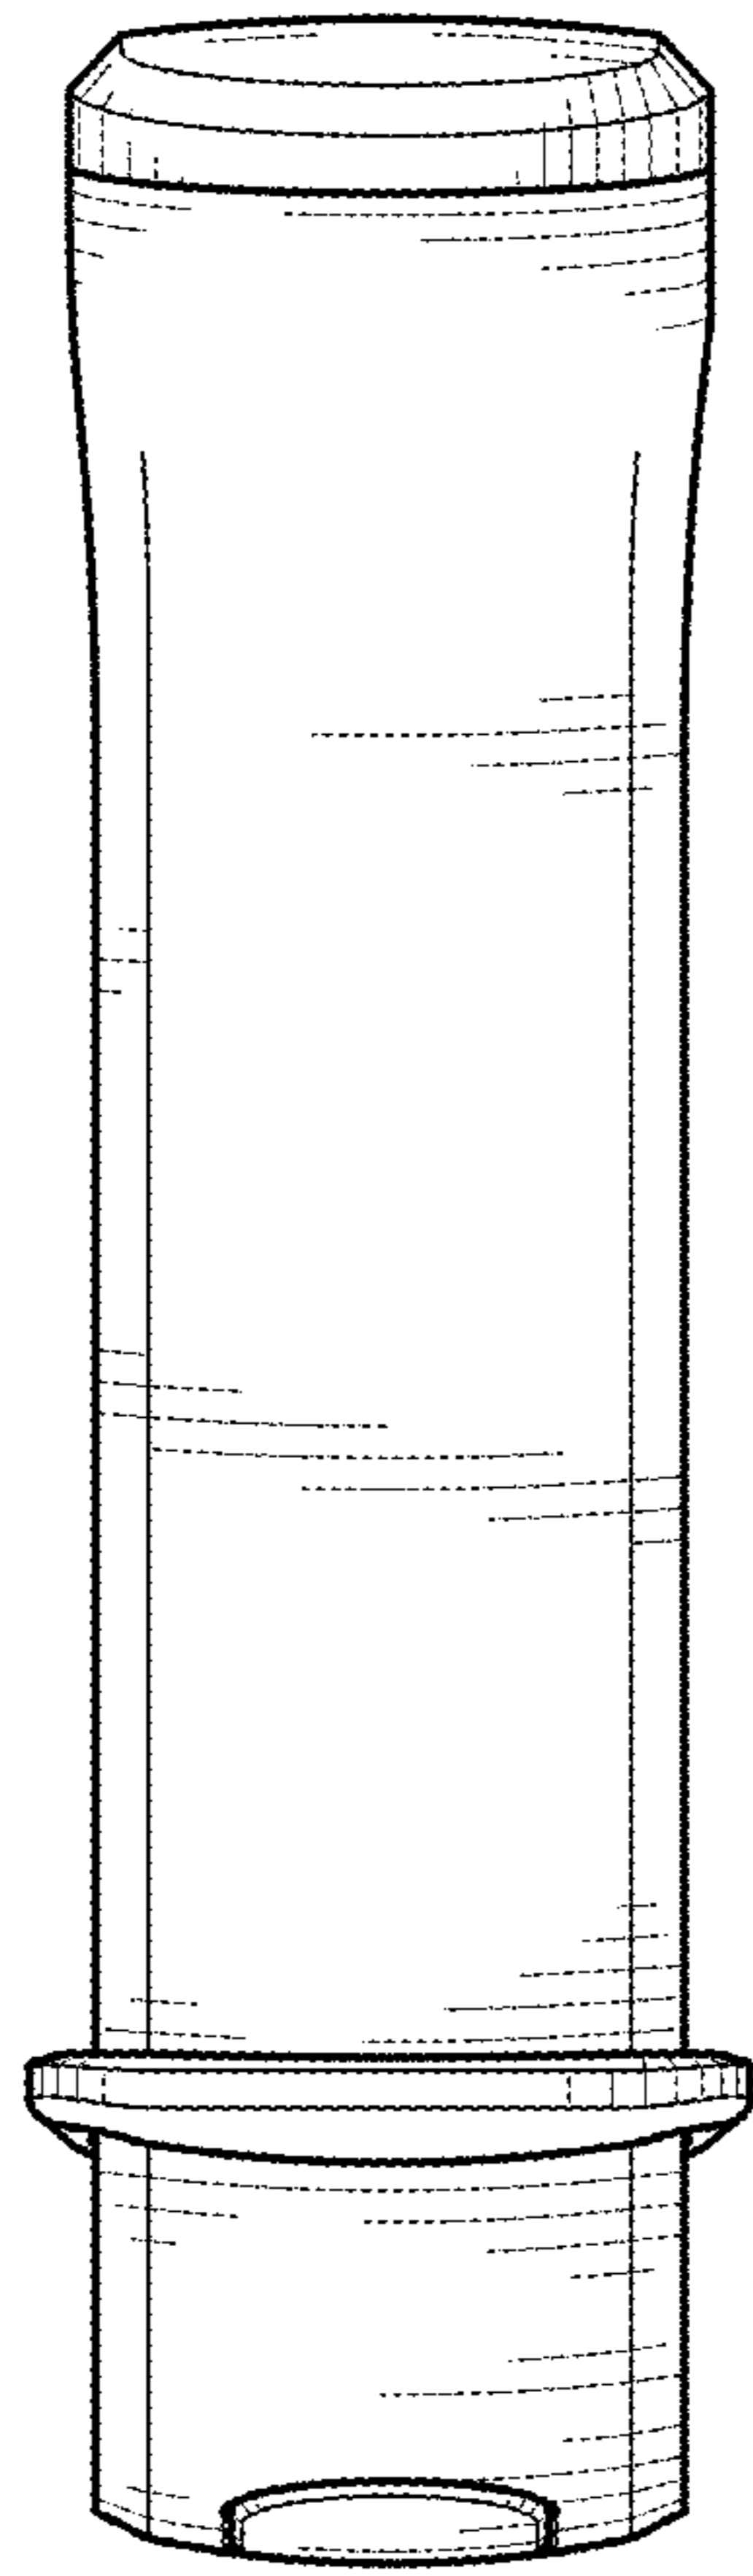


FIG. 7

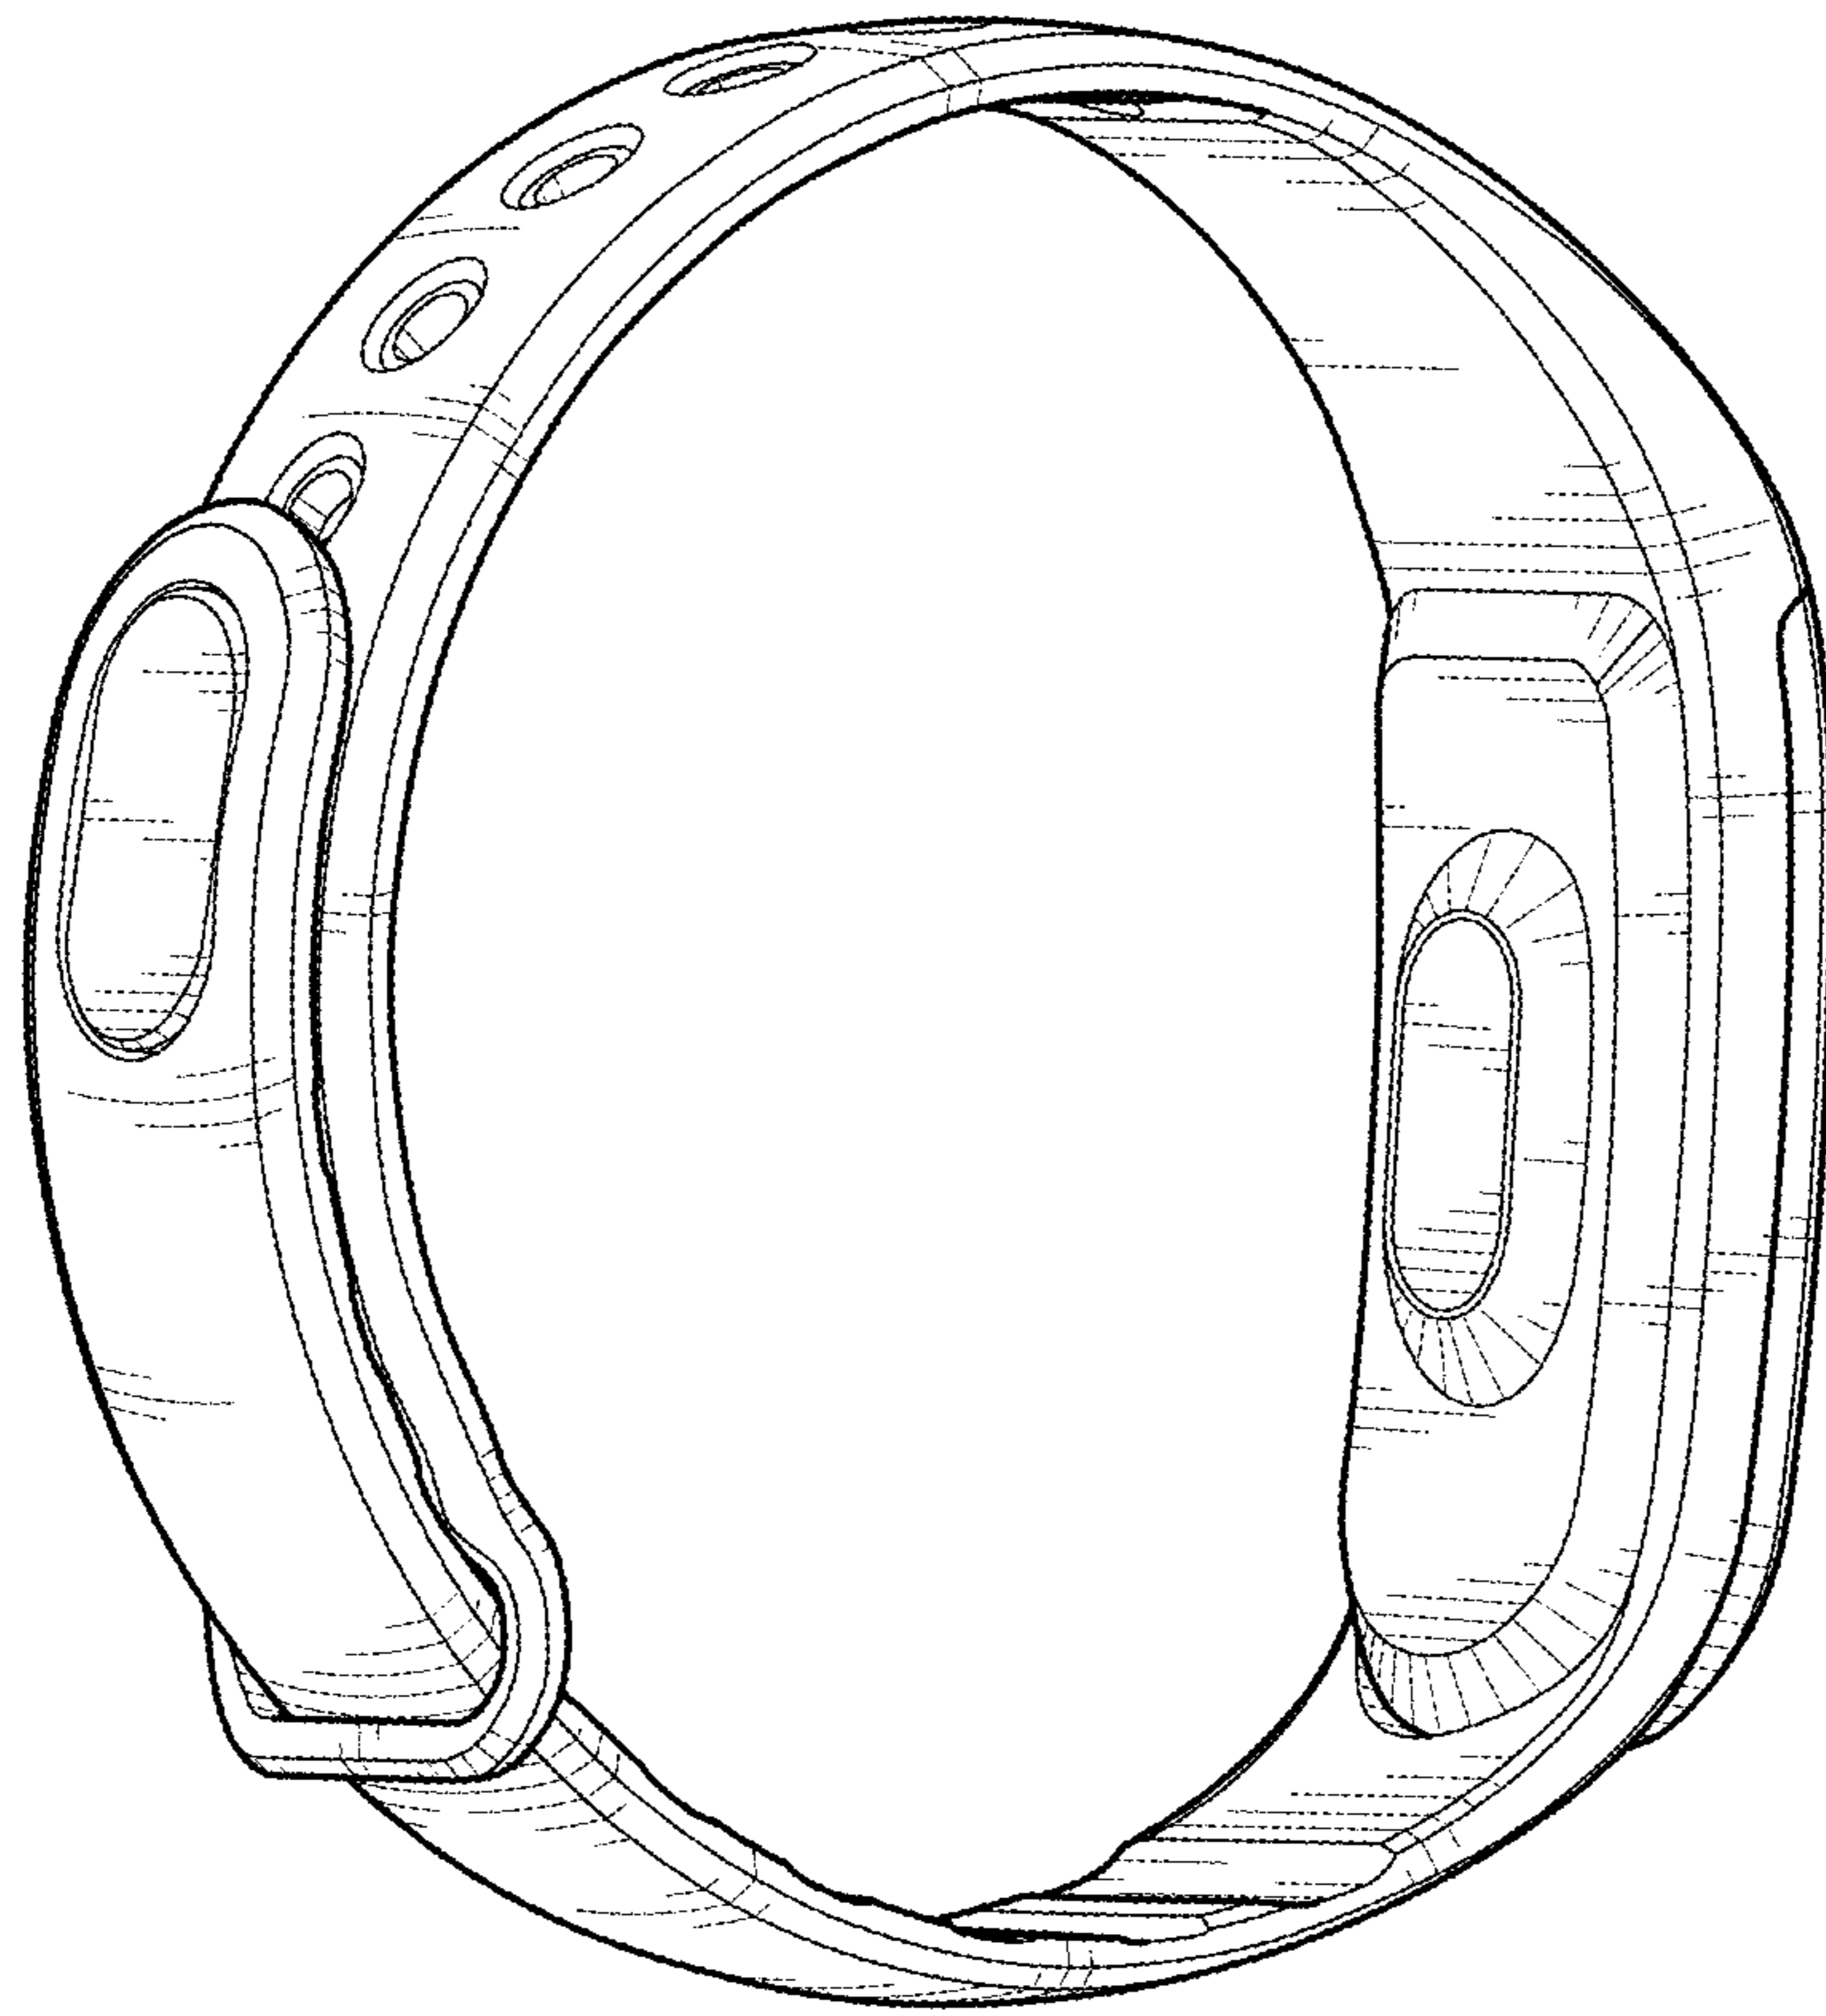


FIG. 8

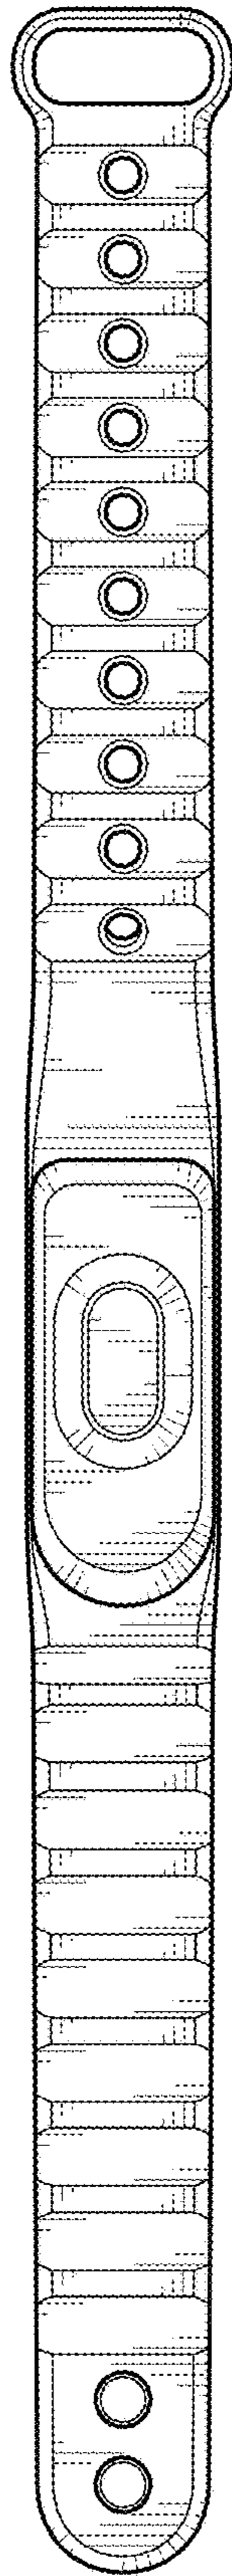


FIG. 9