

US00D806878S

(12) **United States Design Patent** (10) **Patent No.:** **US D806,878 S**
Chang et al. (45) **Date of Patent:** **** Jan. 2, 2018**

(54) **MAGNETIC RESONANCE TOMOGRAPHY
DIAGNOSIS APPARATUS**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Toshiba Medical Systems
Corporation**, Otawara-shi, Tochigi-ken
(JP)

CN 302144424 10/2012
CN 302632883 11/2013

(Continued)

(72) Inventors: **Shianwei Chang**, Kawasaki (JP); **Kana
Nishimura**, Tokyo (JP)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Banner & Witcoff, Ltd.

(73) Assignee: **Toshiba Medical Systems
Corporation**, Otawara-shi, Tochigi-ken
(JP)

(57) **CLAIM**

The ornamental design for a magnetic resonance tomogra-
phy diagnosis apparatus, as shown and described.

(**) Term: **15 Years**

(21) Appl. No.: **29/570,903**

DESCRIPTION

(22) Filed: **Jul. 13, 2016**

(30) **Foreign Application Priority Data**

Apr. 6, 2016 (JP) 2016-008977

(51) **LOC (11) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**

(58) **Field of Classification Search**
USPC D24/107, 158–161, 185, 186, 187, 231
CPC .. A61B 6/03; A61B 6/035; A61B 5/05; A61B
5/055

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS


D564,096 S * 3/2008 Banryu D24/158
D683,023 S 5/2013 Andersson et al.
D683,025 S * 5/2013 Banryu D24/158
D701,309 S * 3/2014 Ohmukai D24/158
D715,444 S * 10/2014 Zhi D24/159
D715,945 S 10/2014 Zhang
D738,505 S * 9/2015 Eberler D24/158
D753,828 S * 4/2016 Baba D24/158

(Continued)

FIG. 1 is a first perspective view of a magnetic resonance
tomography diagnosis apparatus showing our new design;
FIG. 2 is a second perspective view thereof;
FIG. 3 is a rear perspective view thereof,
FIG. 4 is a front elevational view thereof,
FIG. 5 is a rear elevational view thereof,
FIG. 6 is a top plan view thereof,
FIG. 7 is a bottom plan view thereof,
FIG. 8 is a left side elevational view thereof,
FIG. 9 is a right side elevational view thereof,
FIG. 10 is a cross-sectional view thereof; taken along line
10-10 in FIG. 4;
FIG. 11 is a cross-sectional view thereof; taken along line
11-11 in FIG. 4;
FIG. 12 is an enlarged view of the part partitioned by **12-12**
in FIG. 4;
FIG. 13 is an enlarged view of the part partitioned by **13-13**
in FIG. 10; and,
FIG. 14 is an enlarged view of the part partitioned by **14-14**
in FIG. 11.

The broken lines in the figures show portions of the mag-
netic resonance tomography diagnosis apparatus which form
no part of the claimed design.

1 Claim, 14 Drawing Sheets

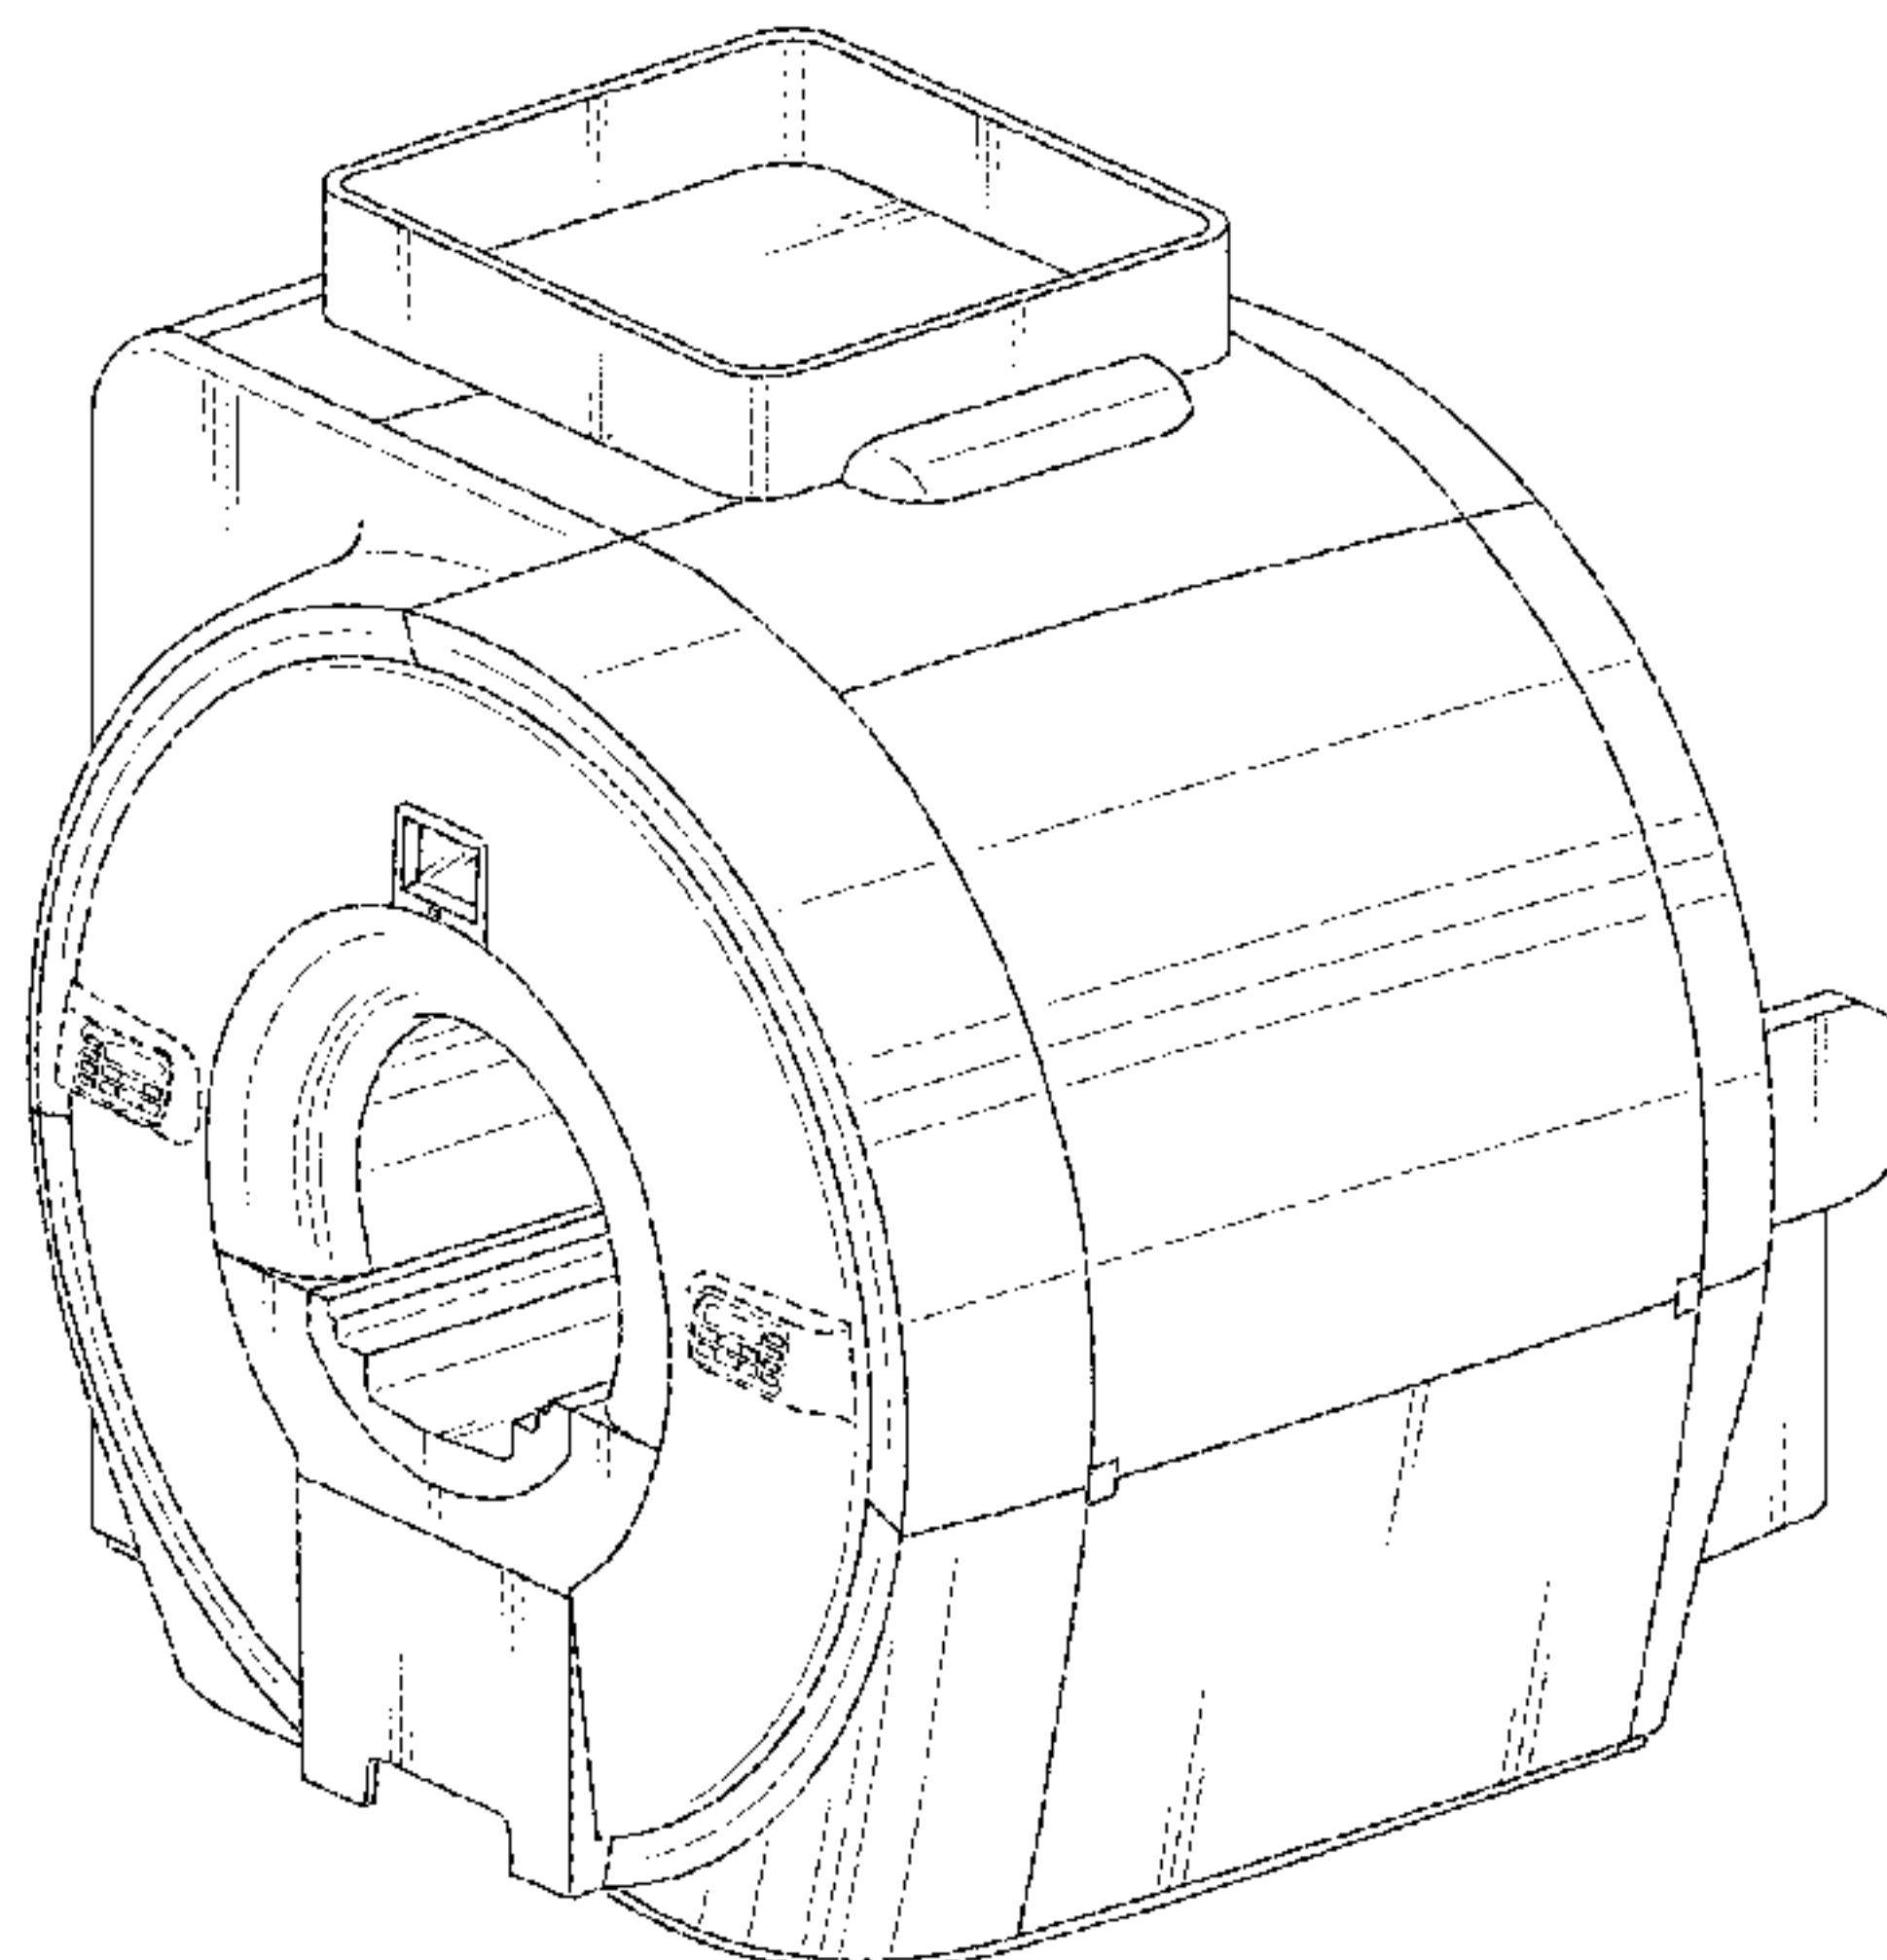

(56)

References Cited

U.S. PATENT DOCUMENTS

D785,181	S	*	4/2017	Grosshauser		D24/158
D794,799	S	*	8/2017	Achleitner		D24/158
2016/0235377	A1	*	8/2016	Yun		A61B 6/4488

FOREIGN PATENT DOCUMENTS

CN	303209087	5/2015
JP	1456980	12/2012
JP	1470199	5/2013

* cited by examiner

Fig. 1

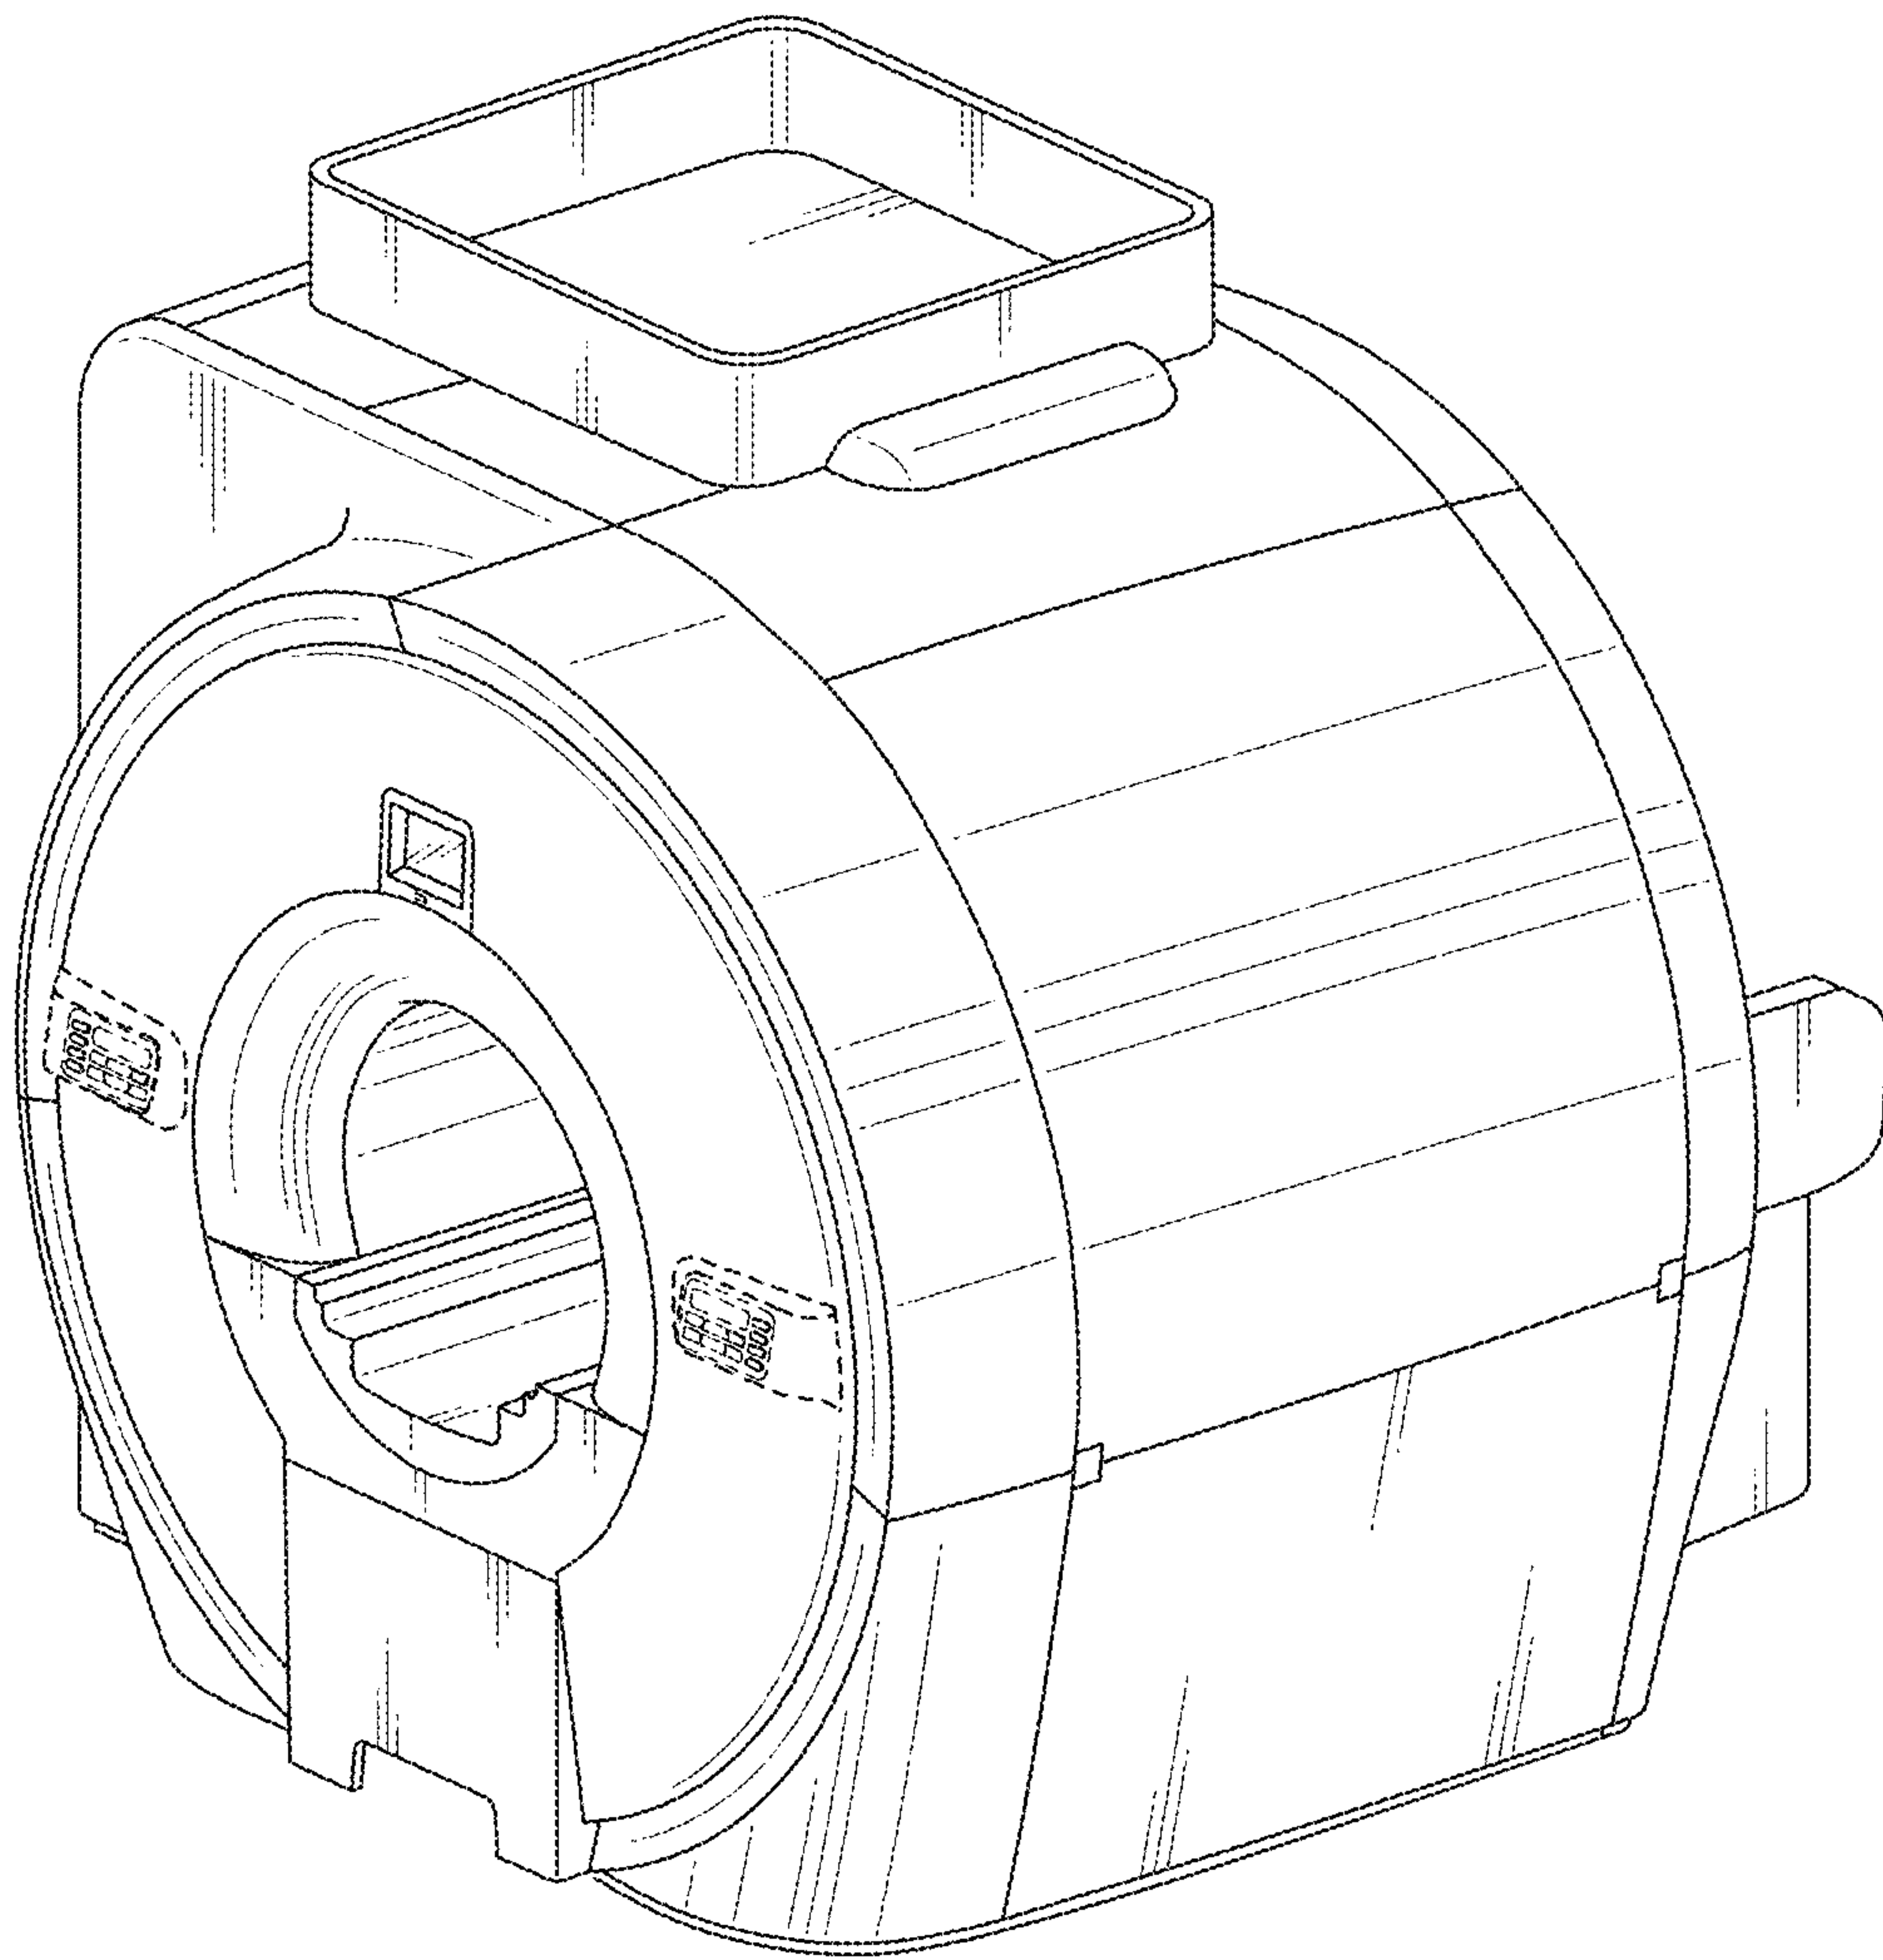


Fig. 2

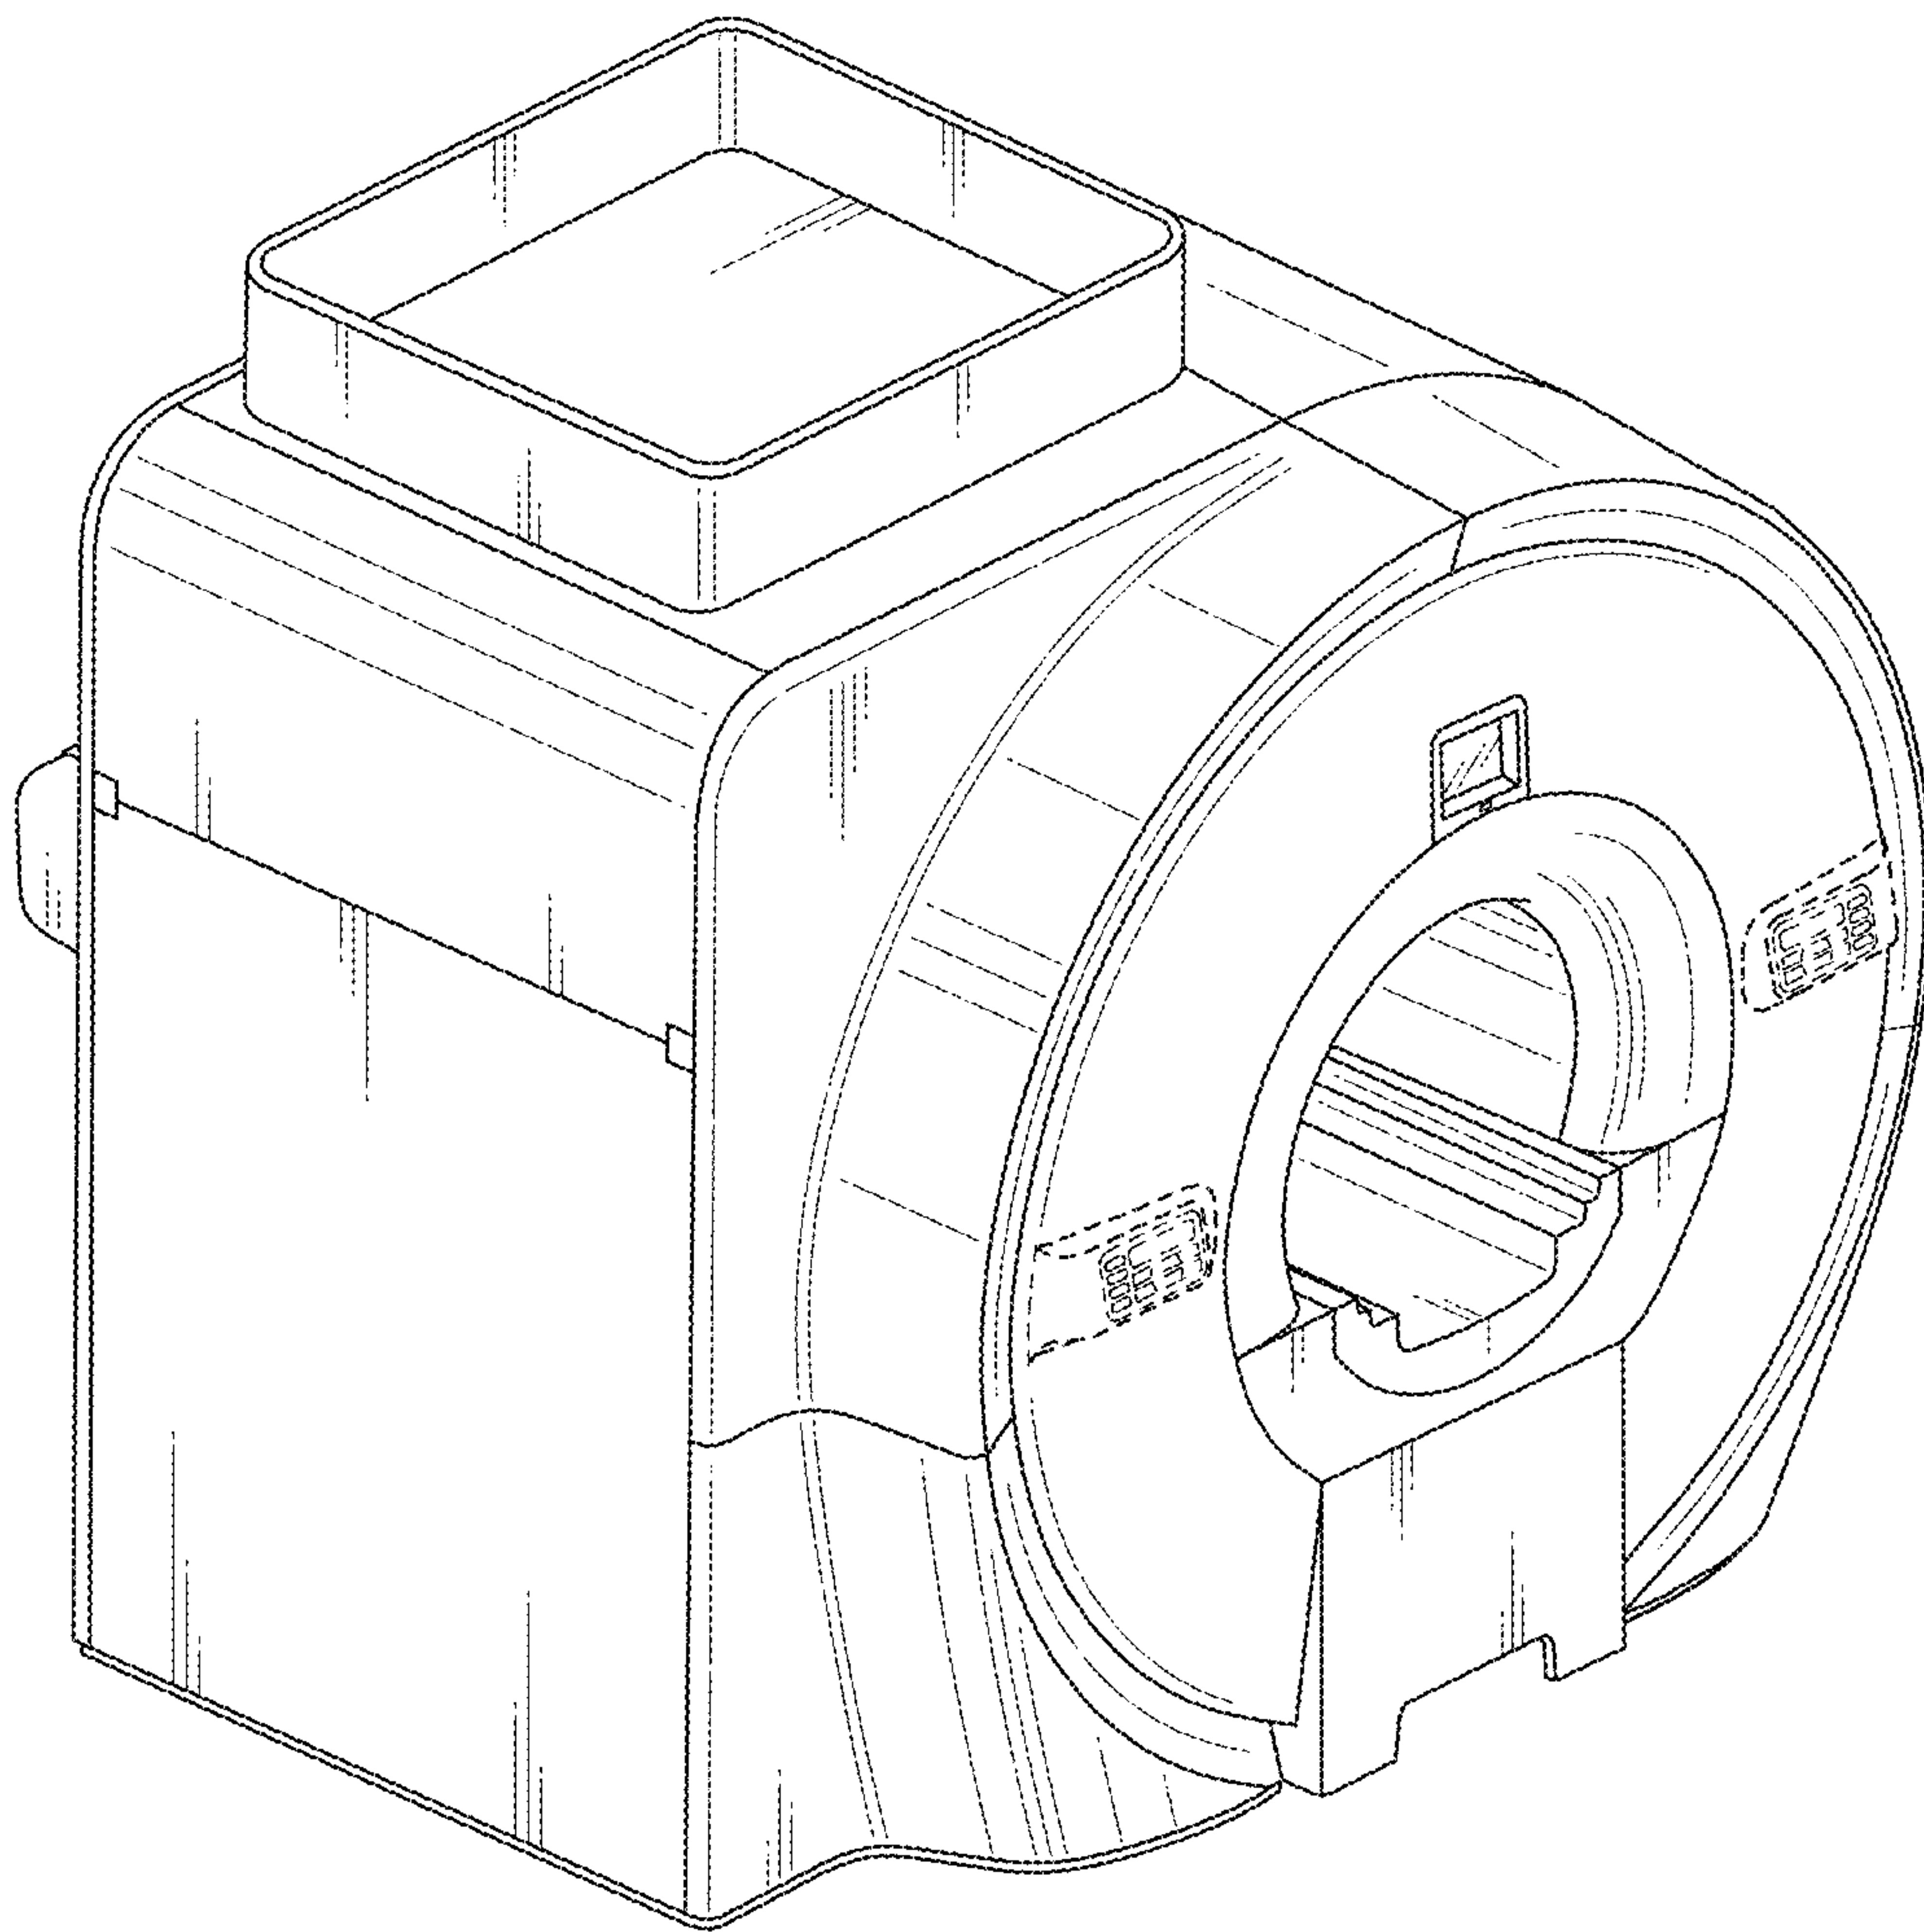


Fig. 3

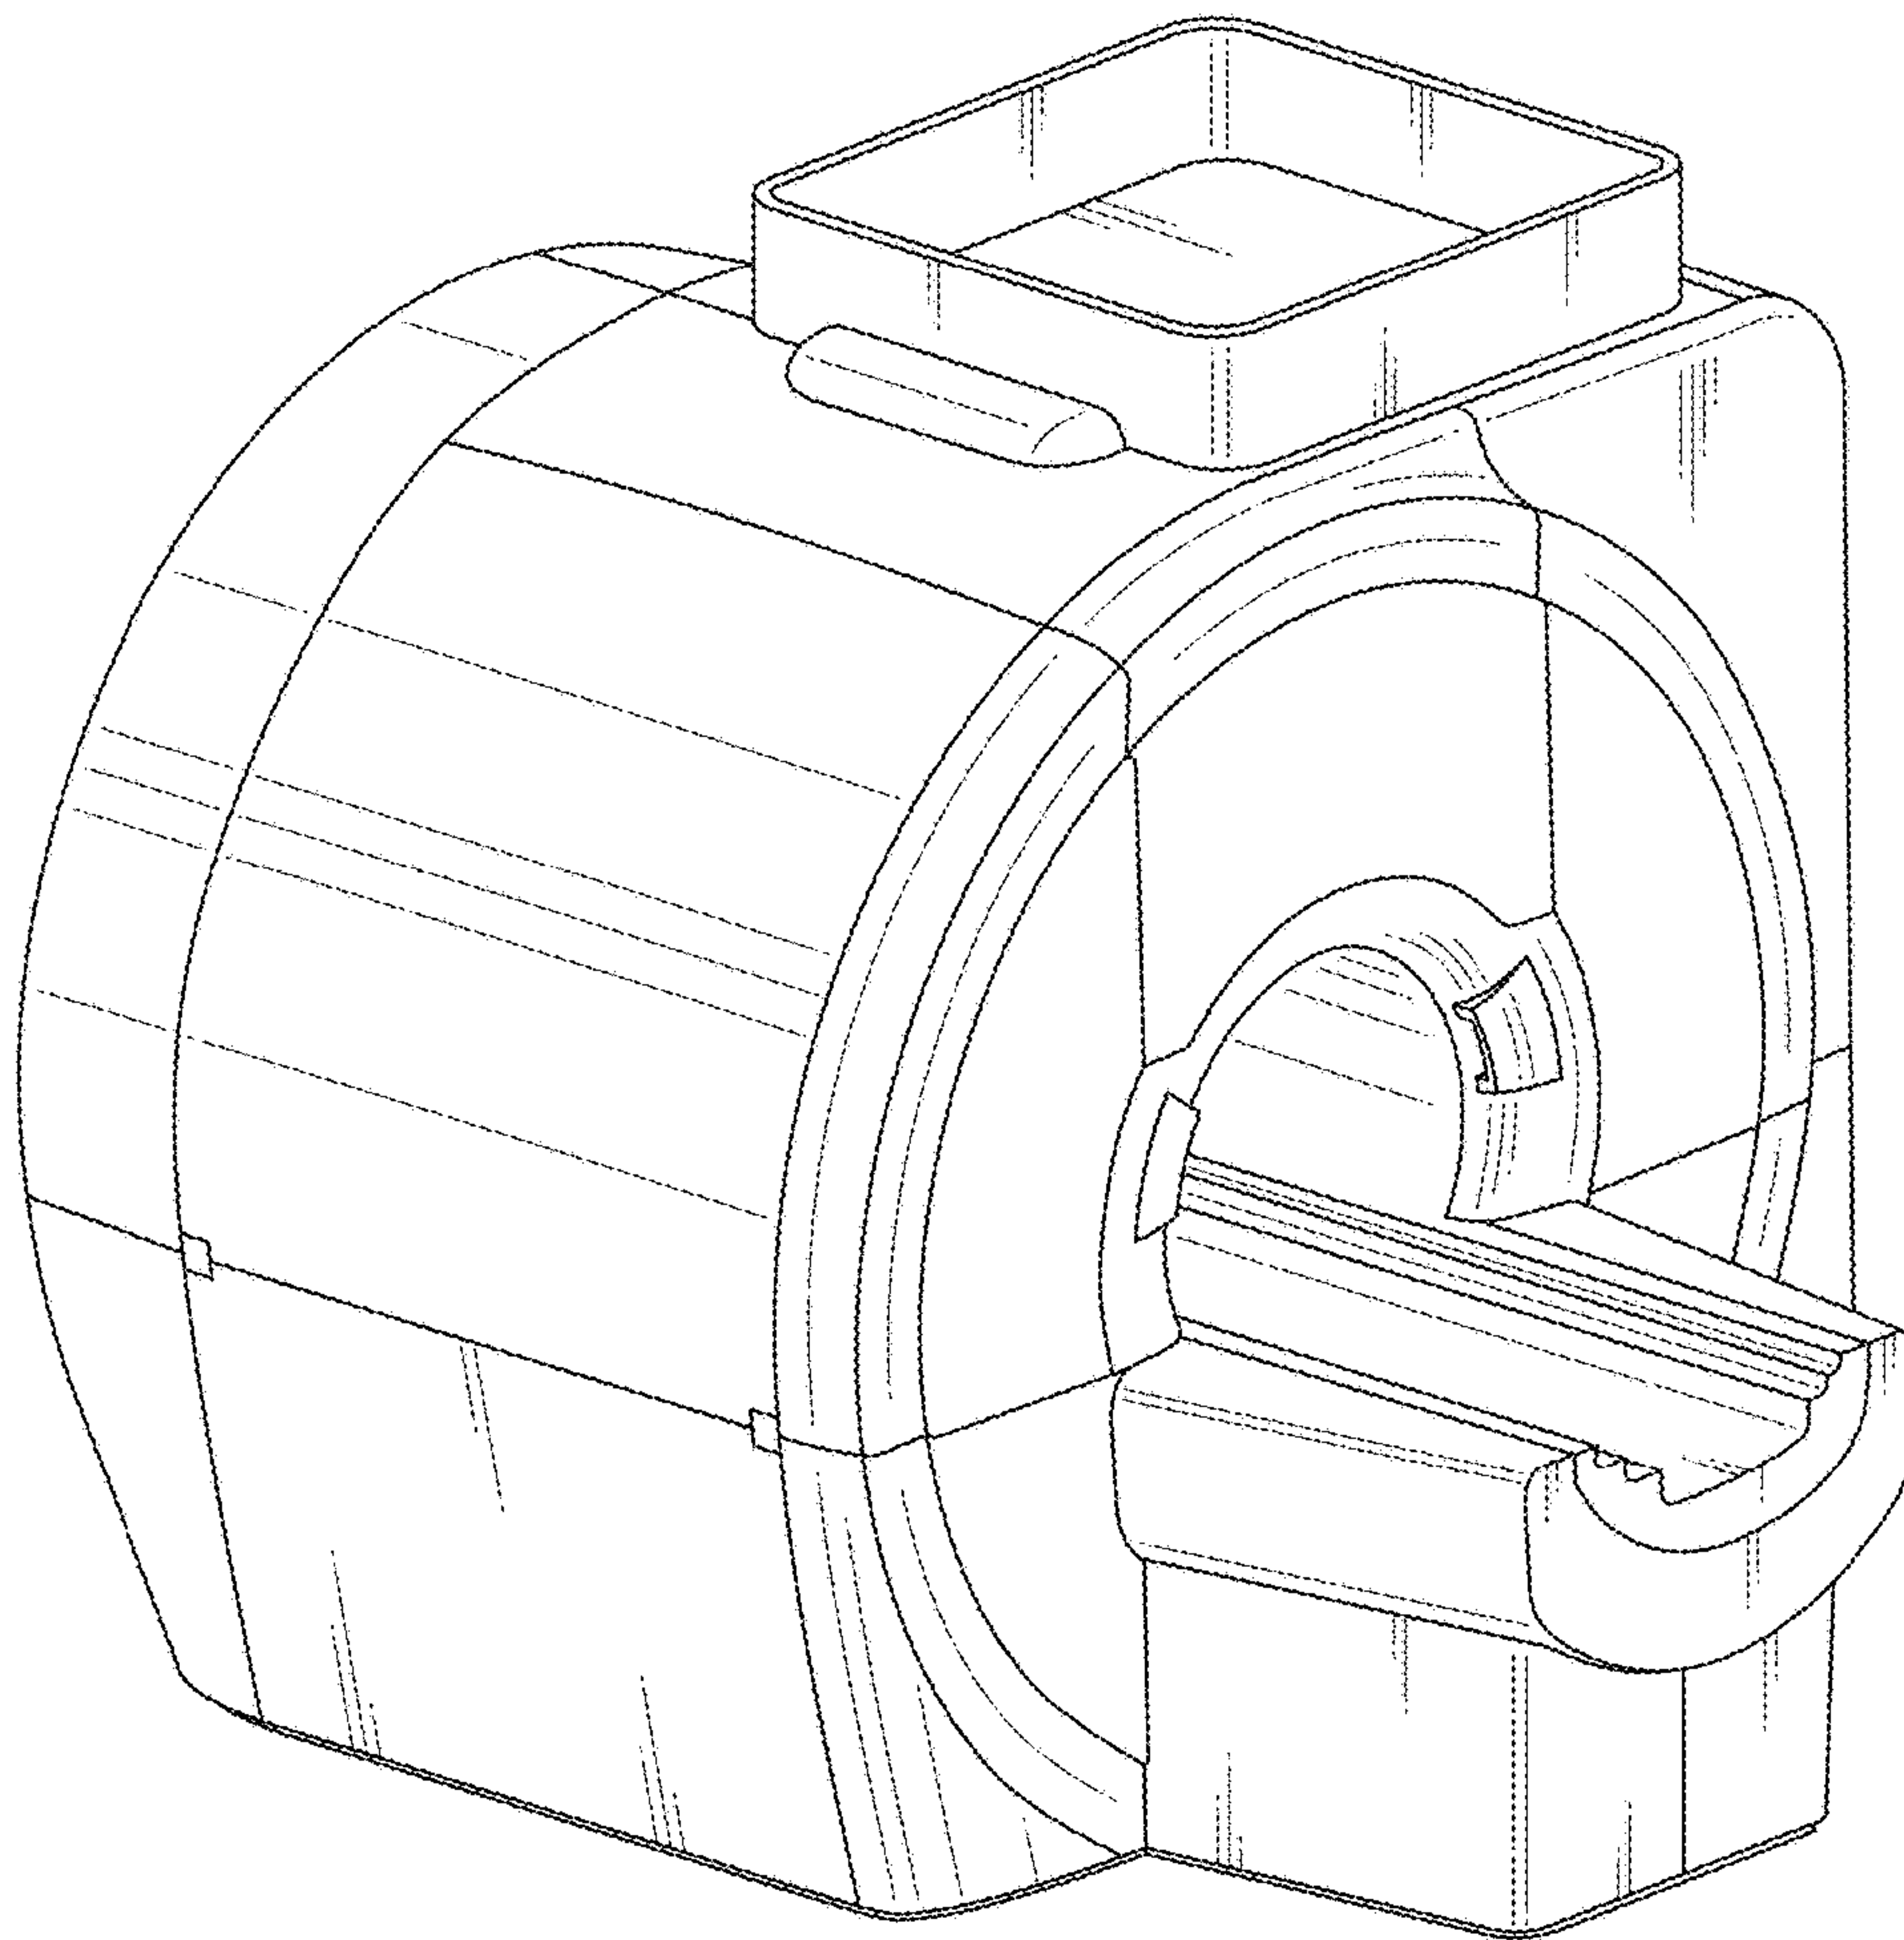


Fig. 4

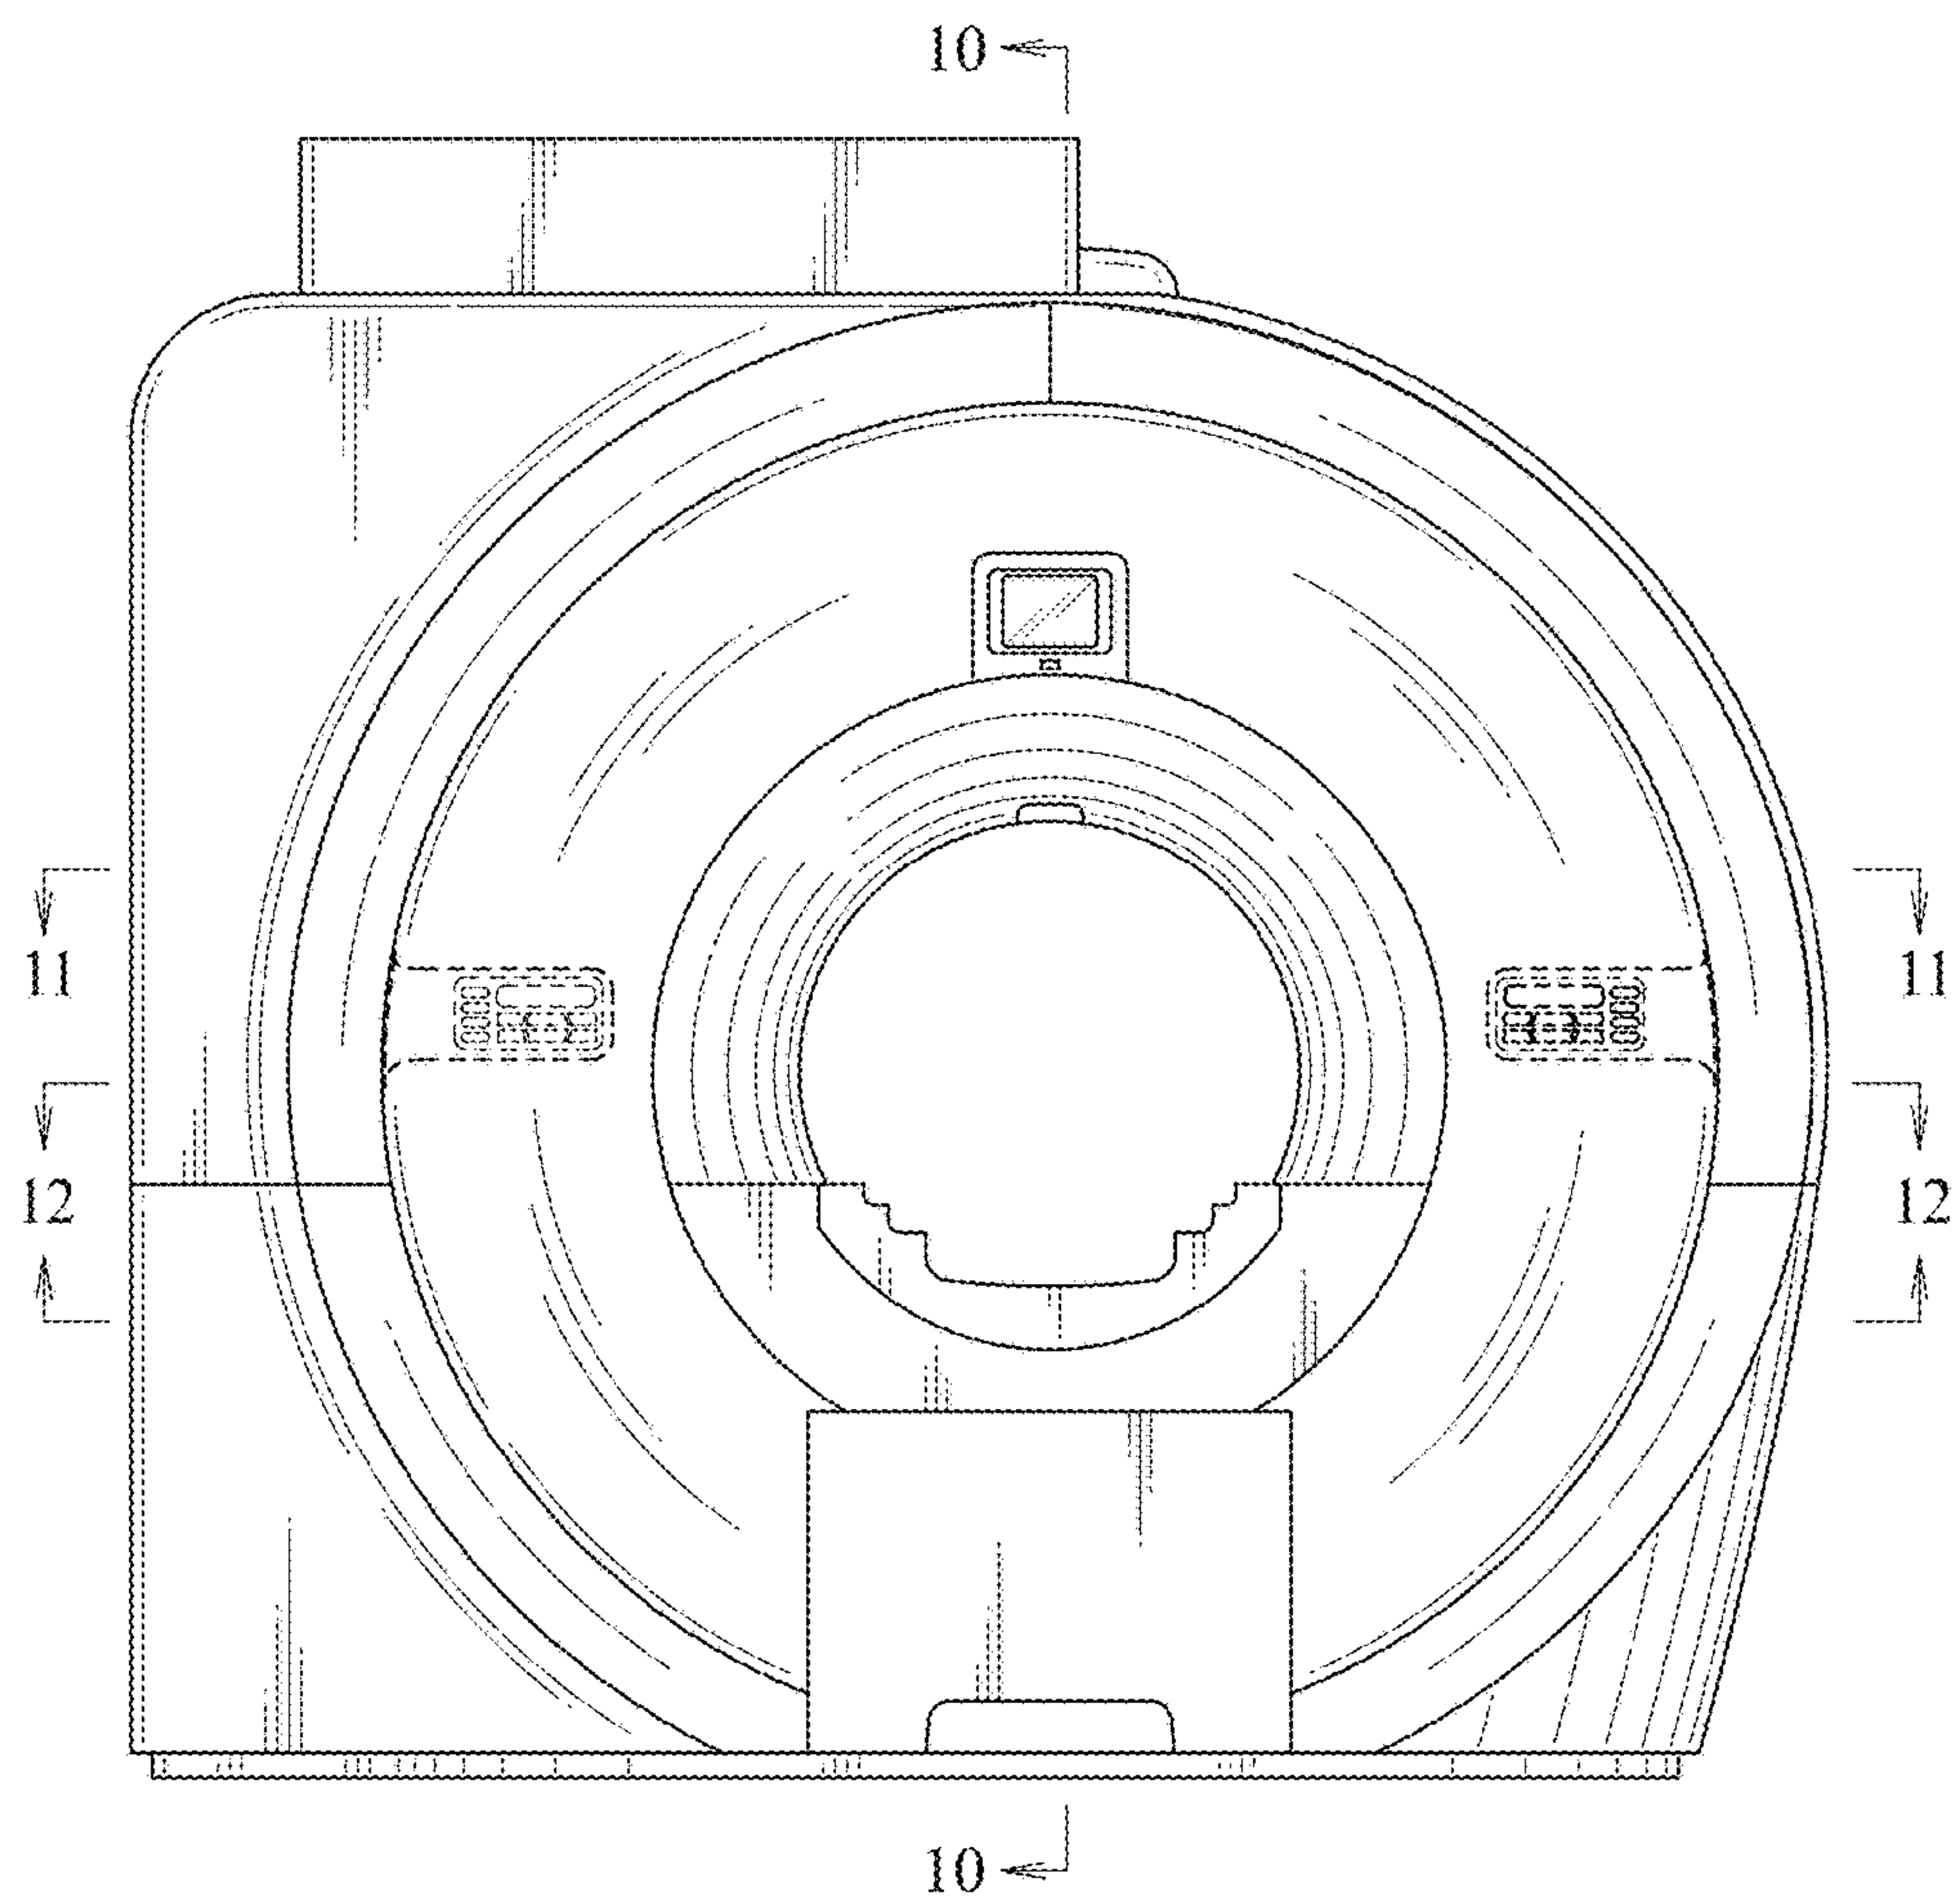


Fig. 5

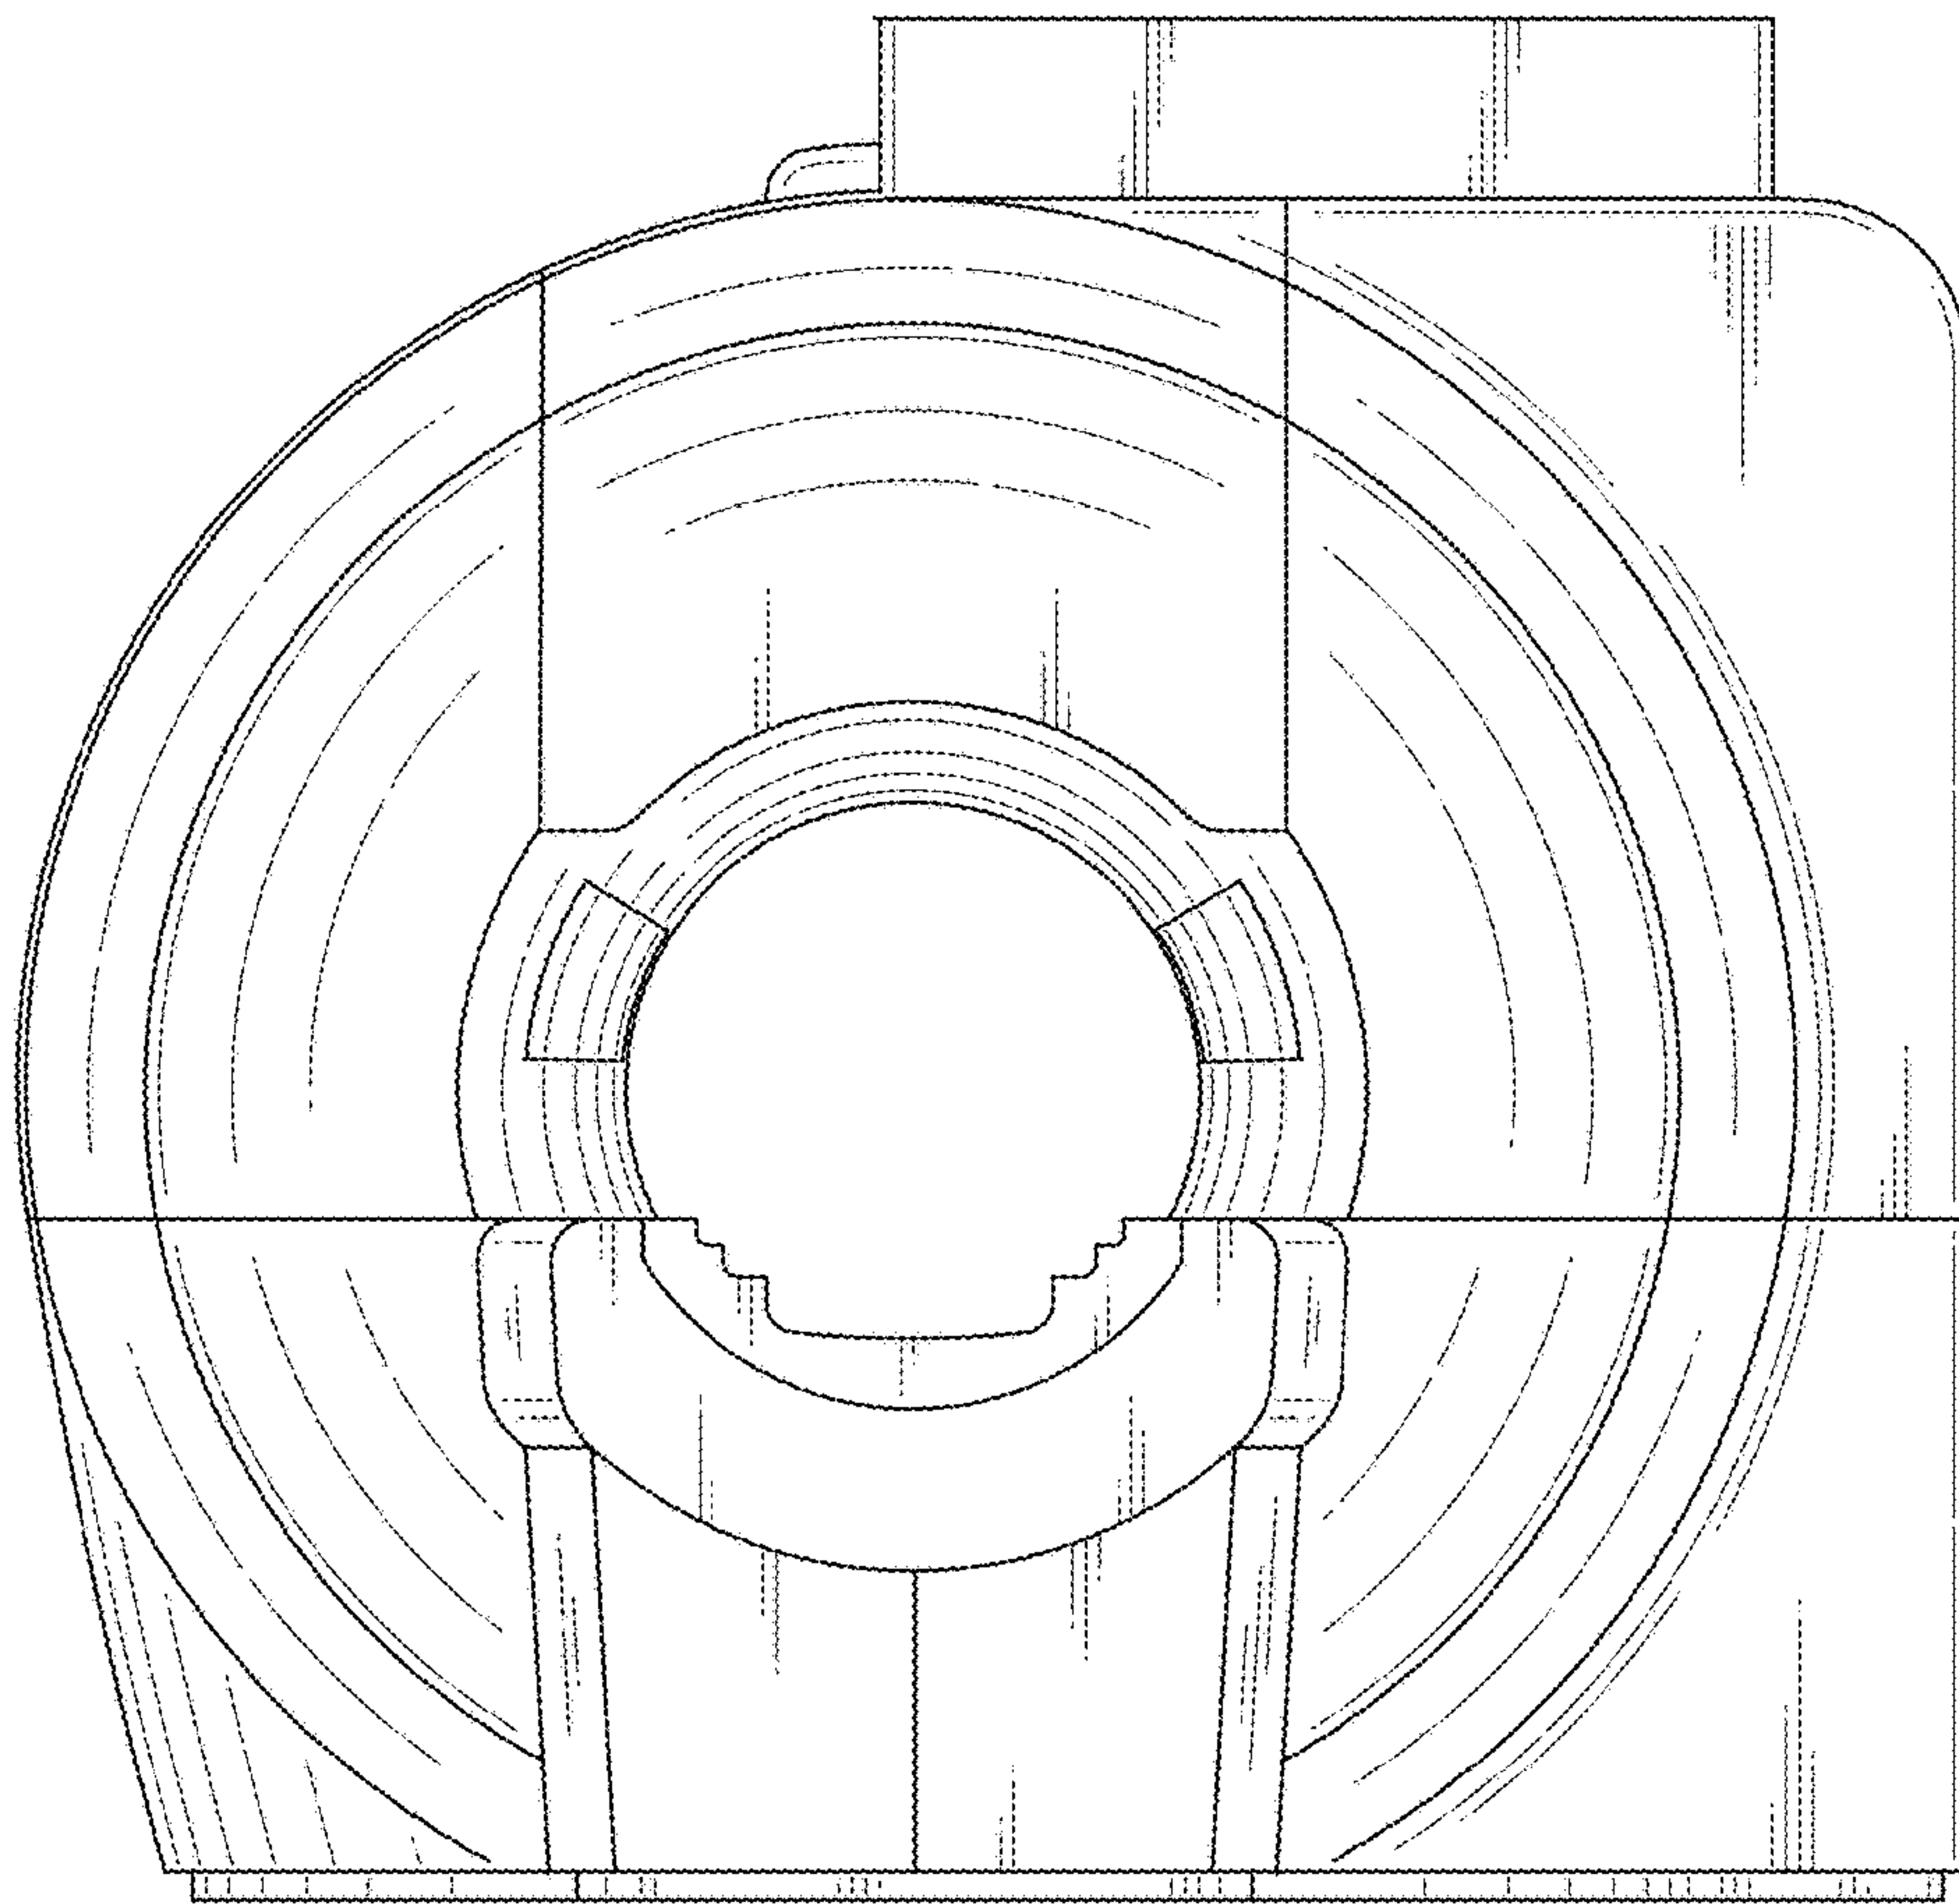


Fig. 6

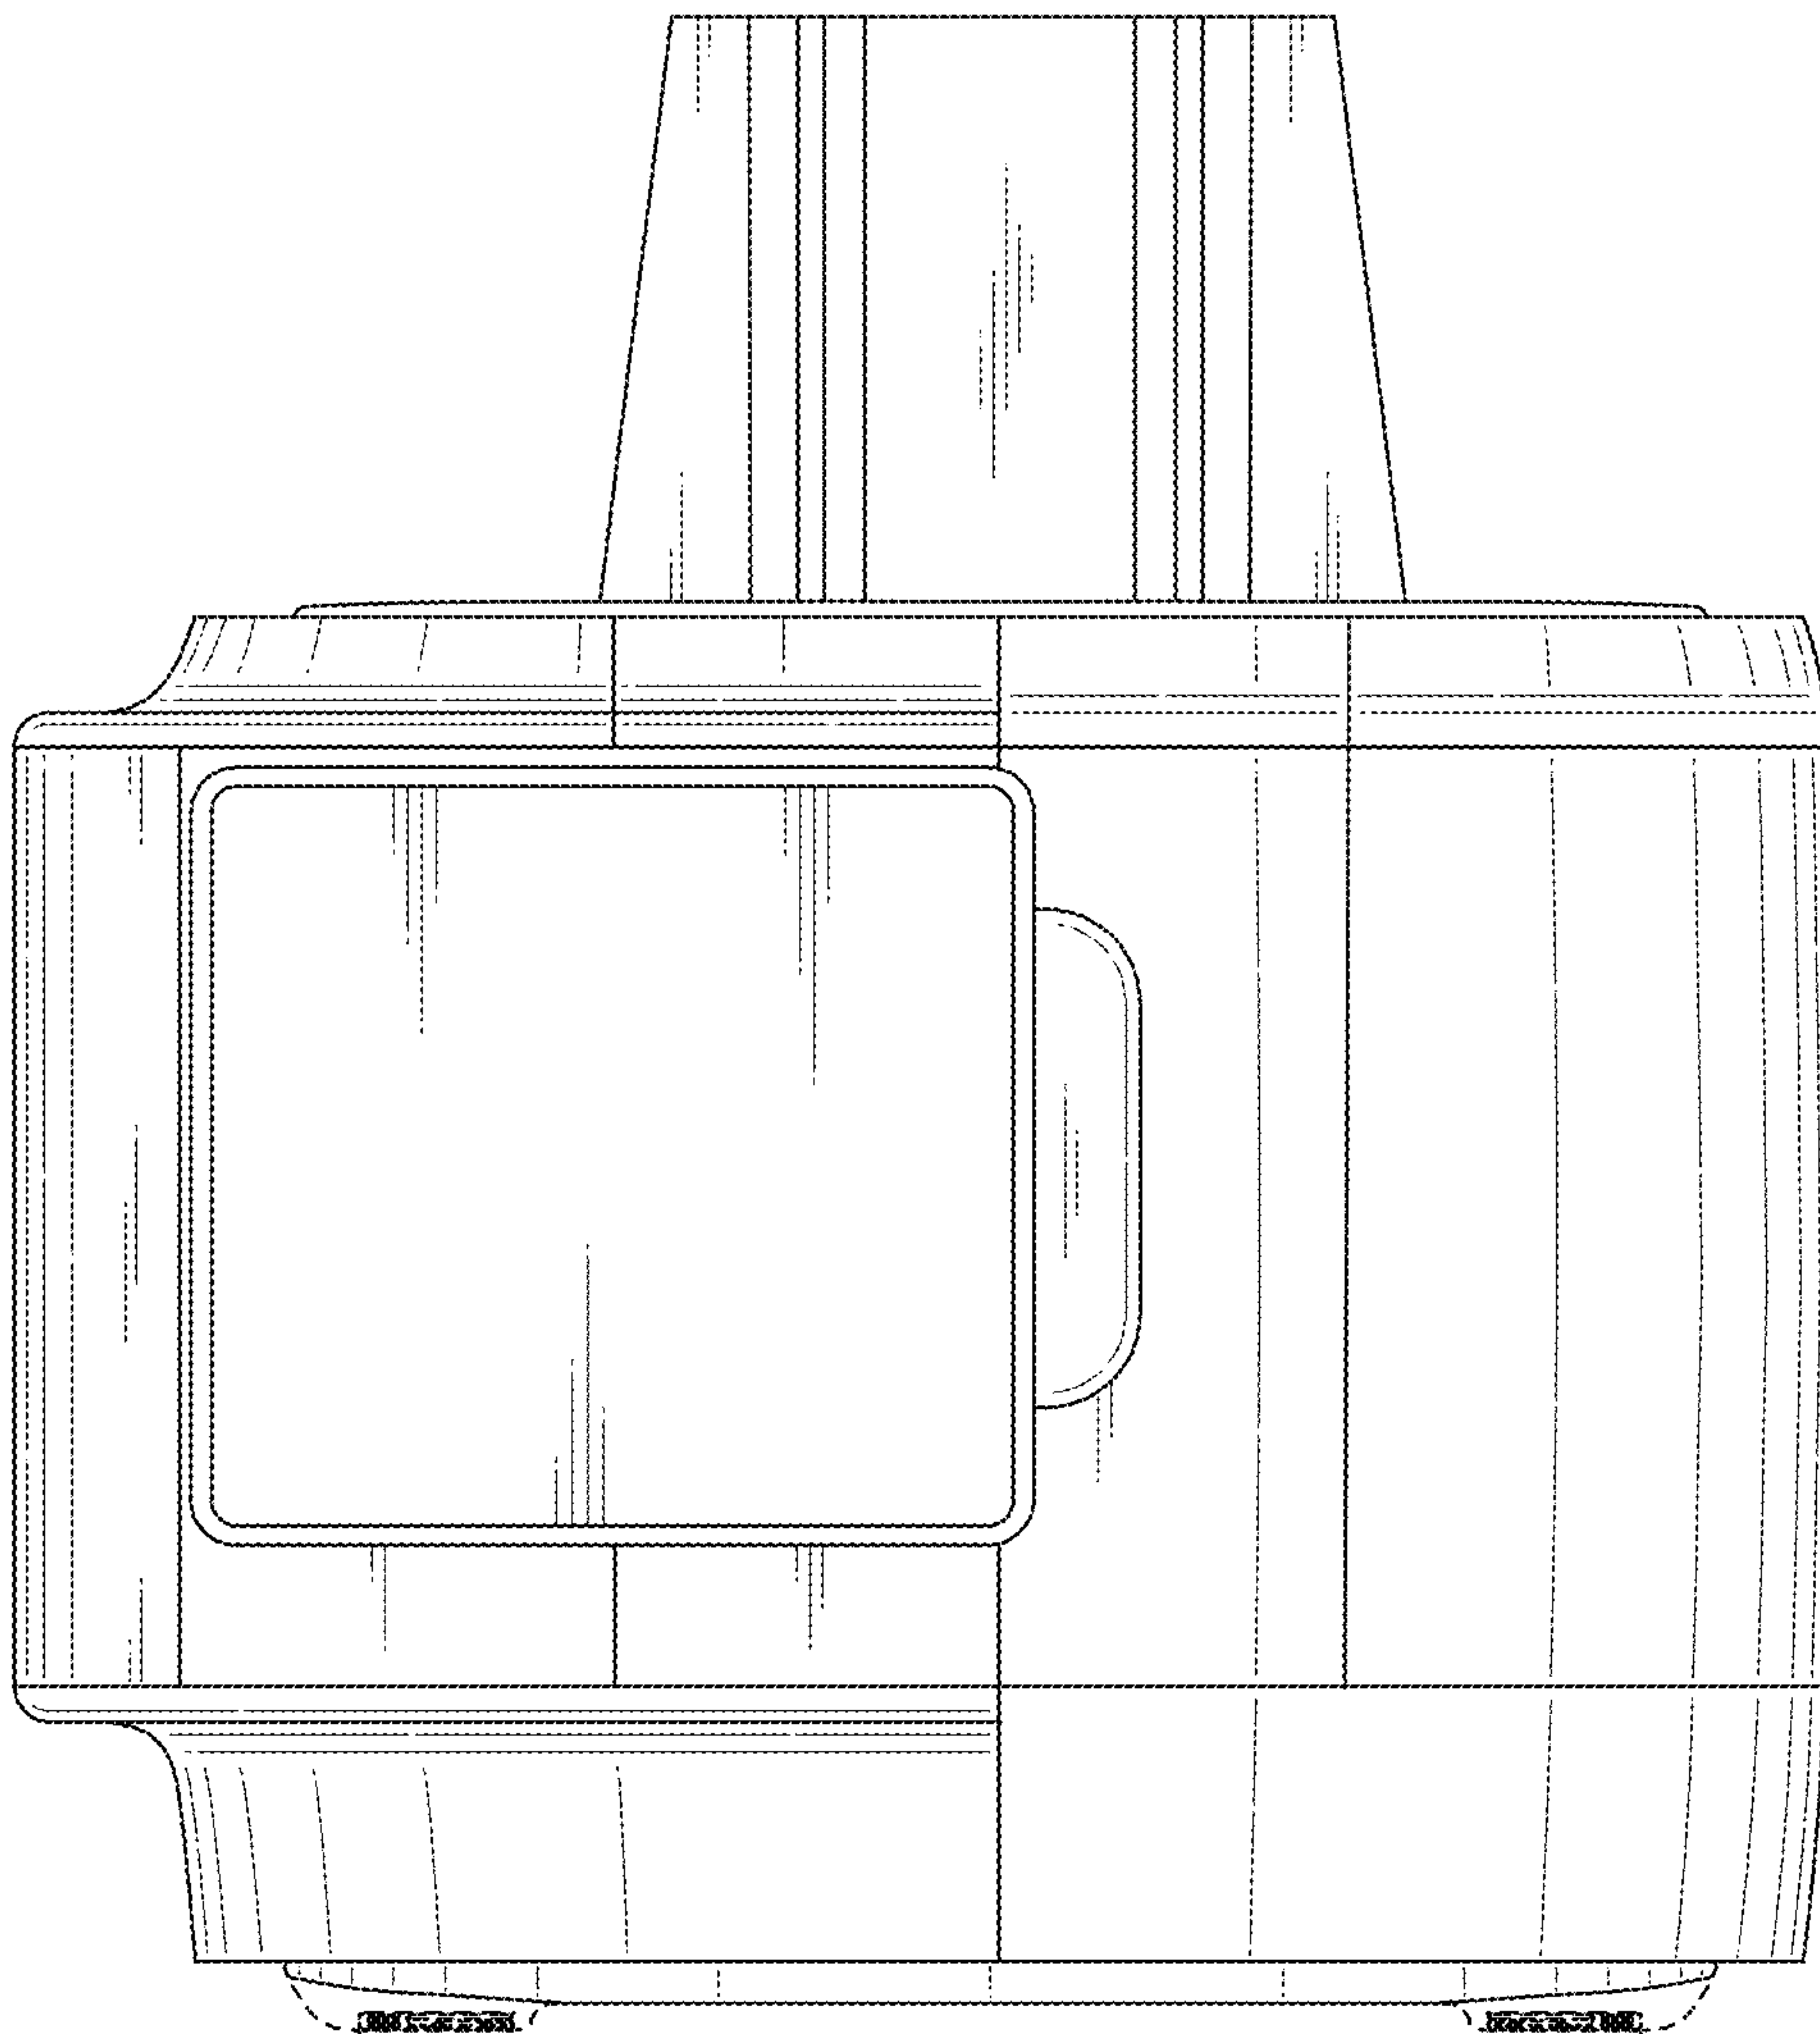


Fig. 7

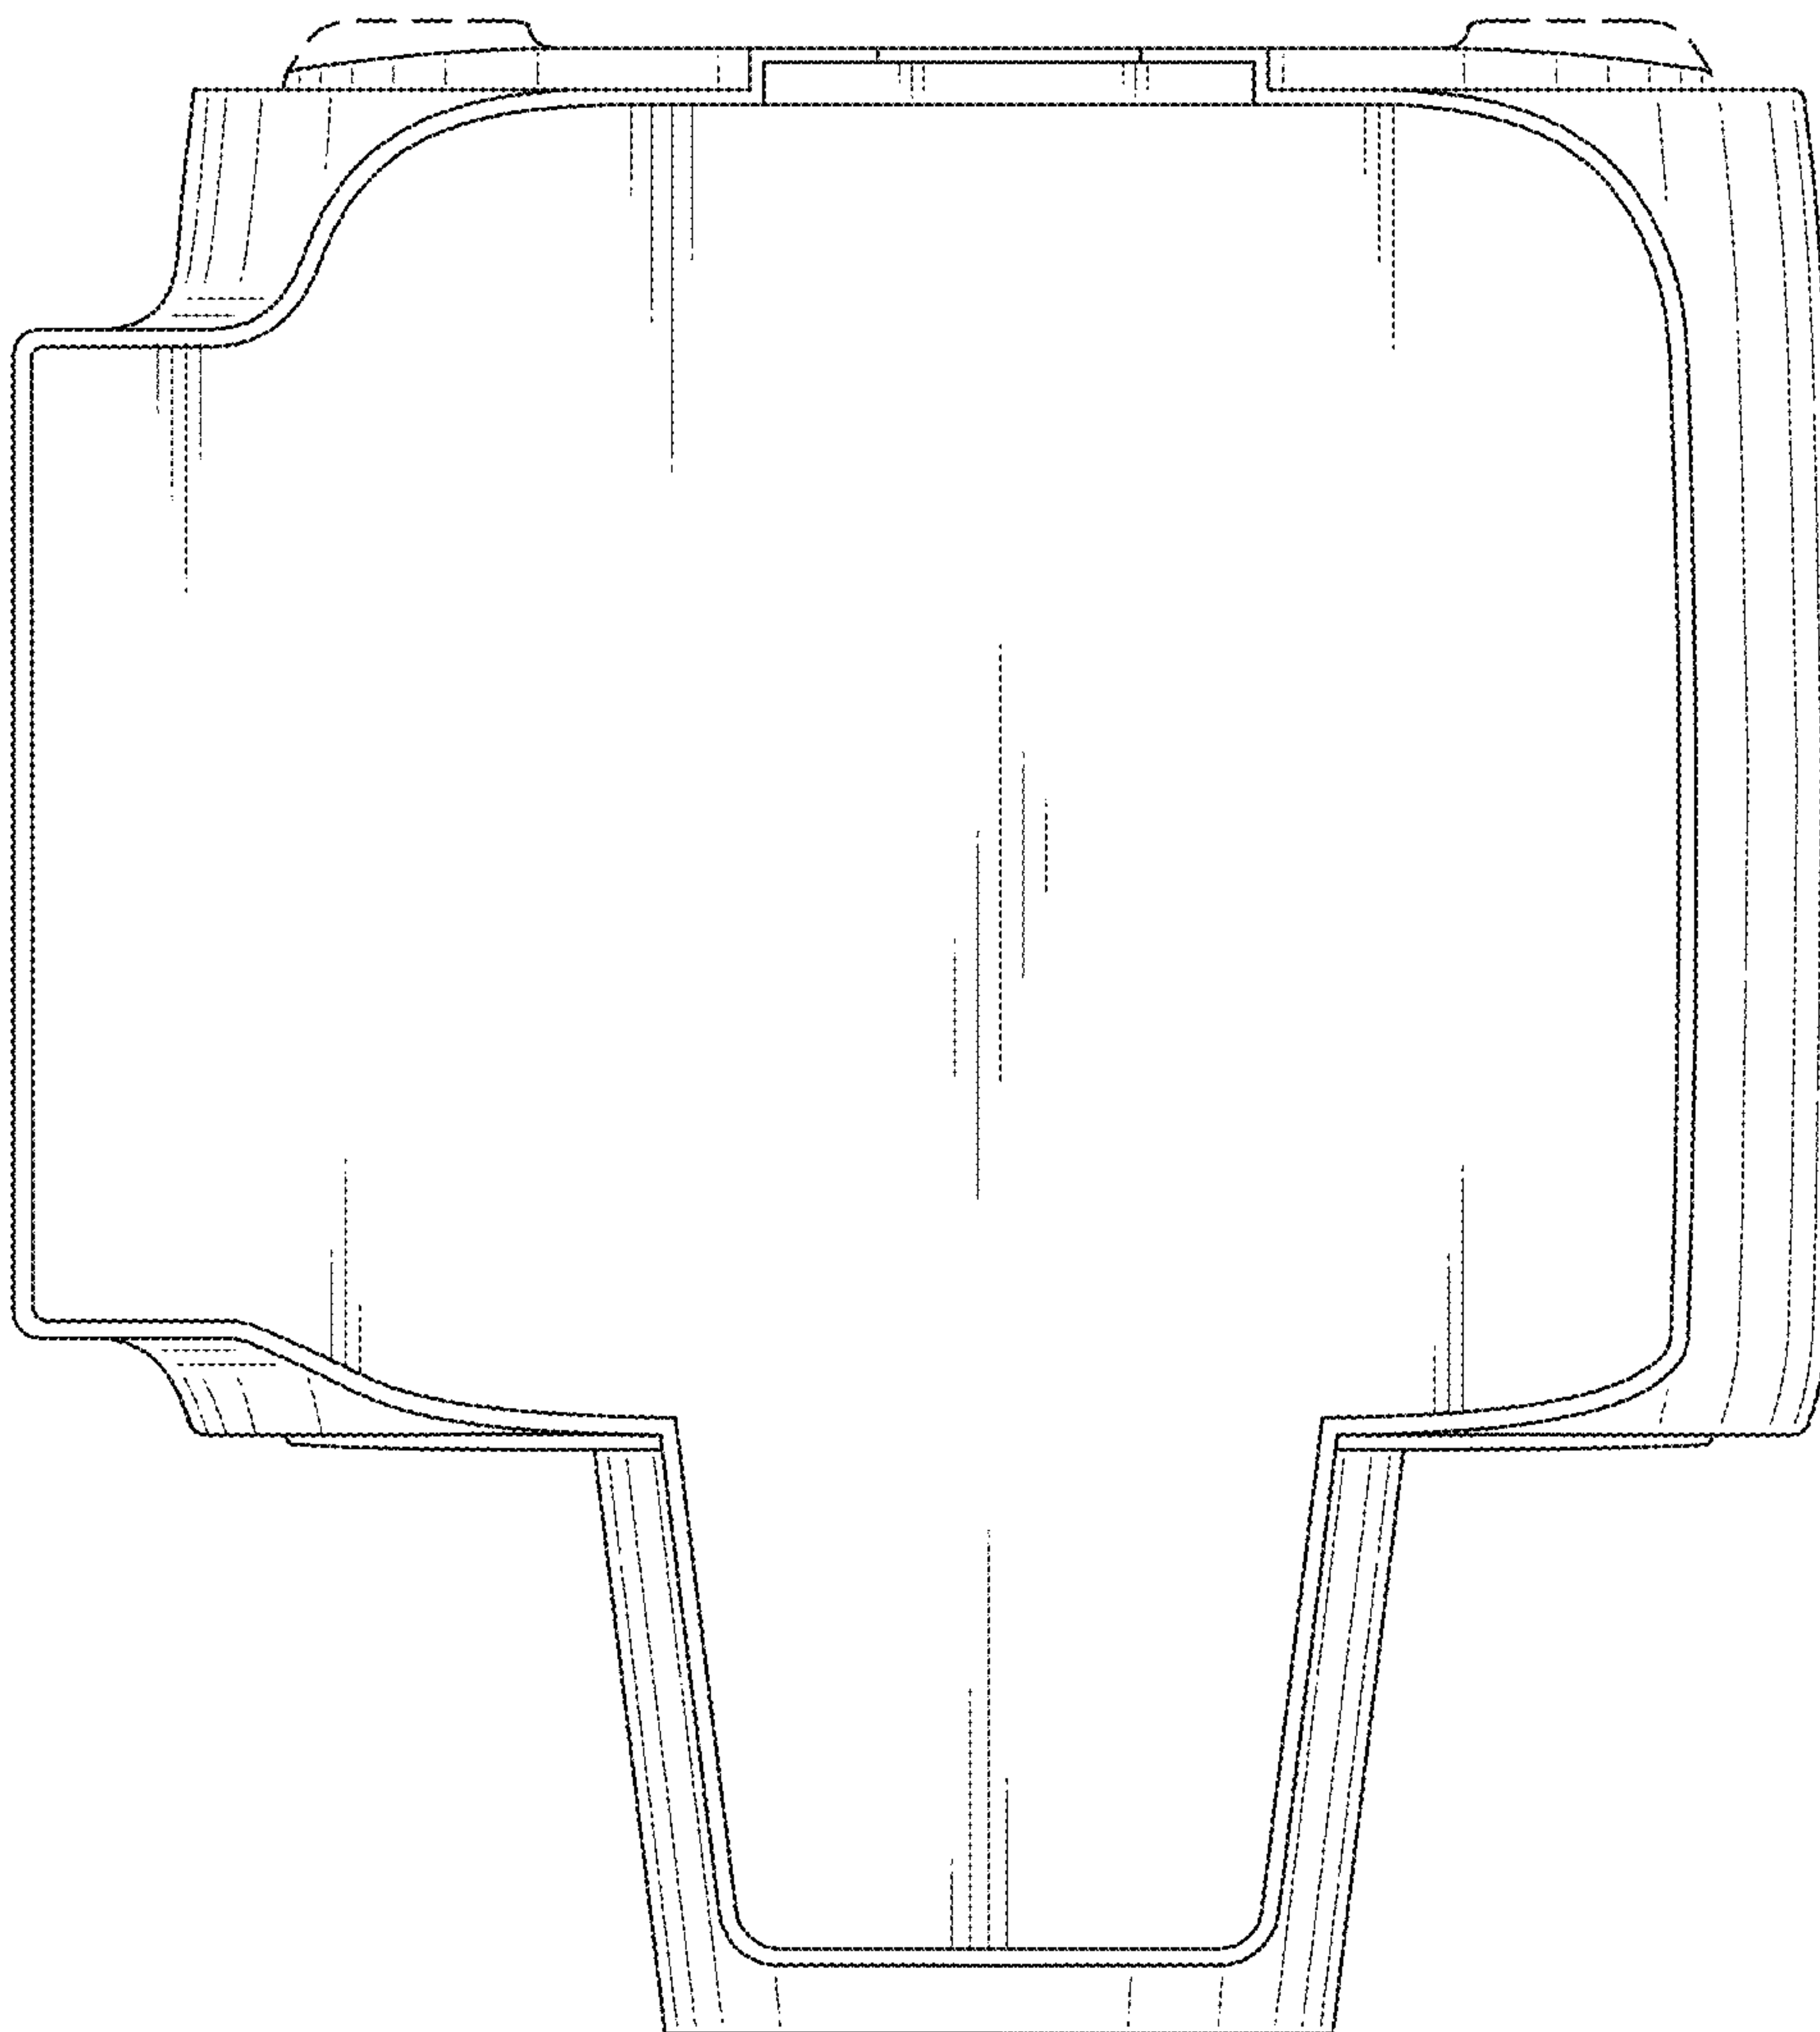


Fig. 8

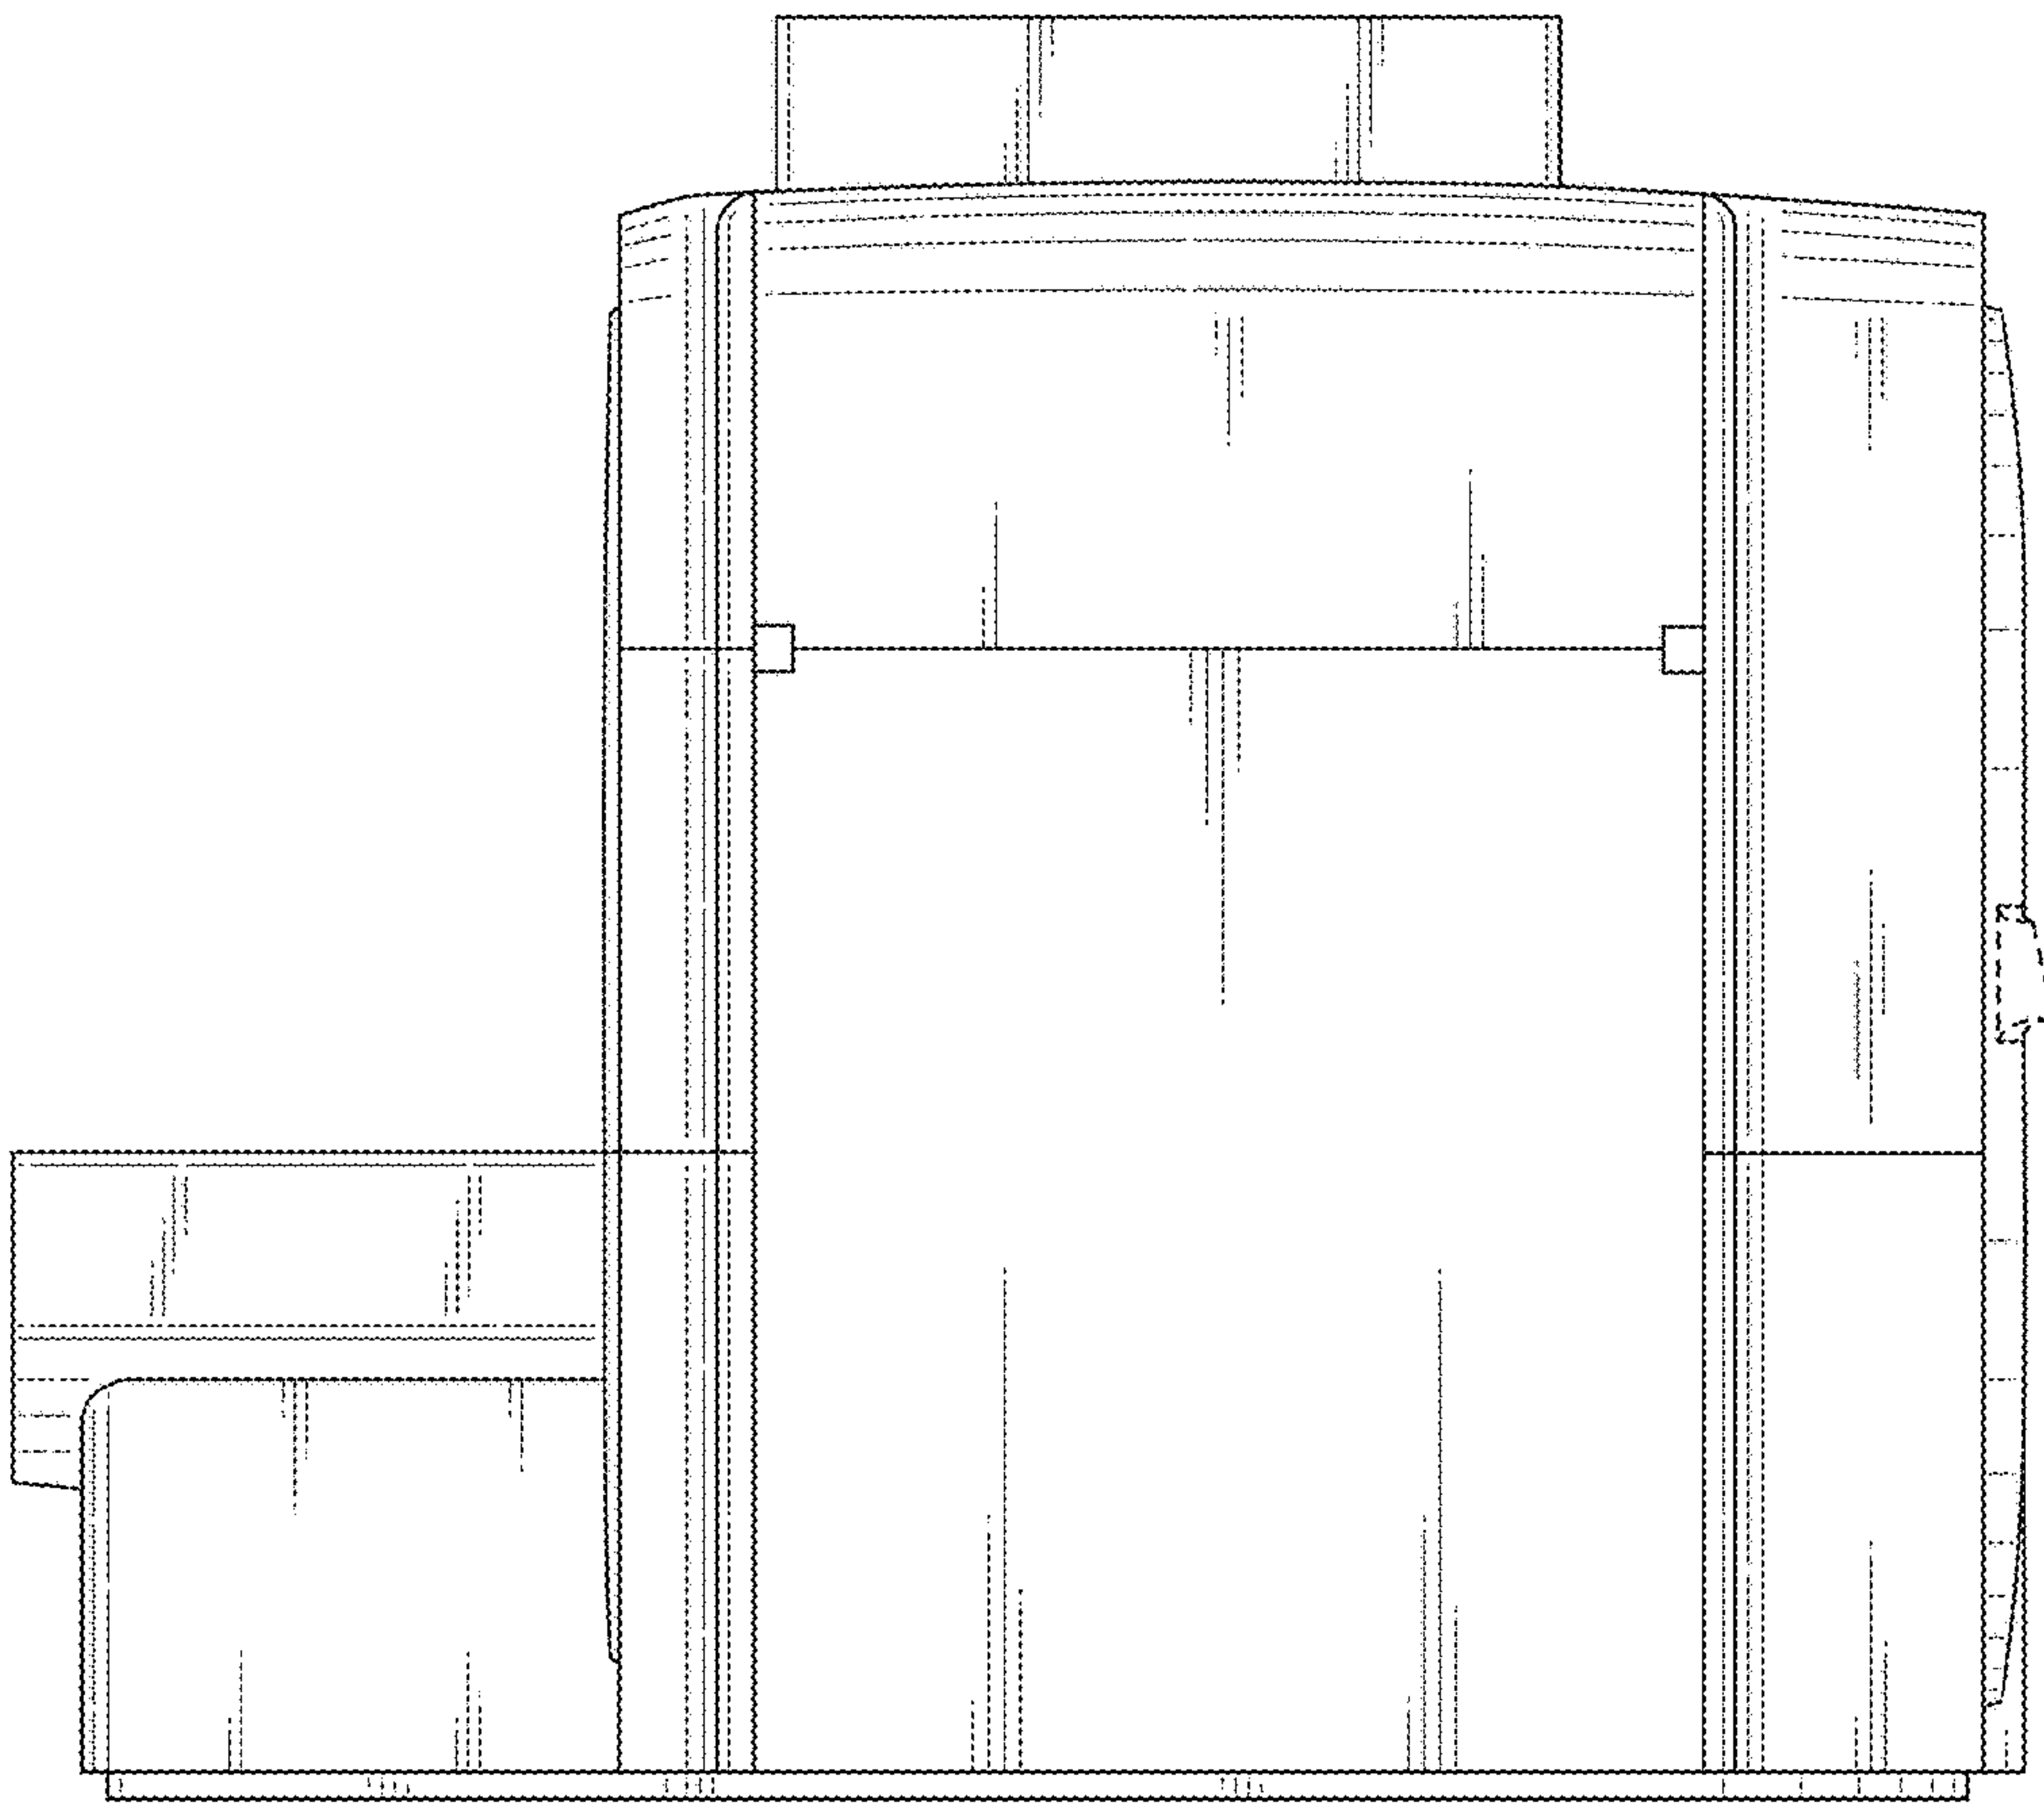


Fig. 9

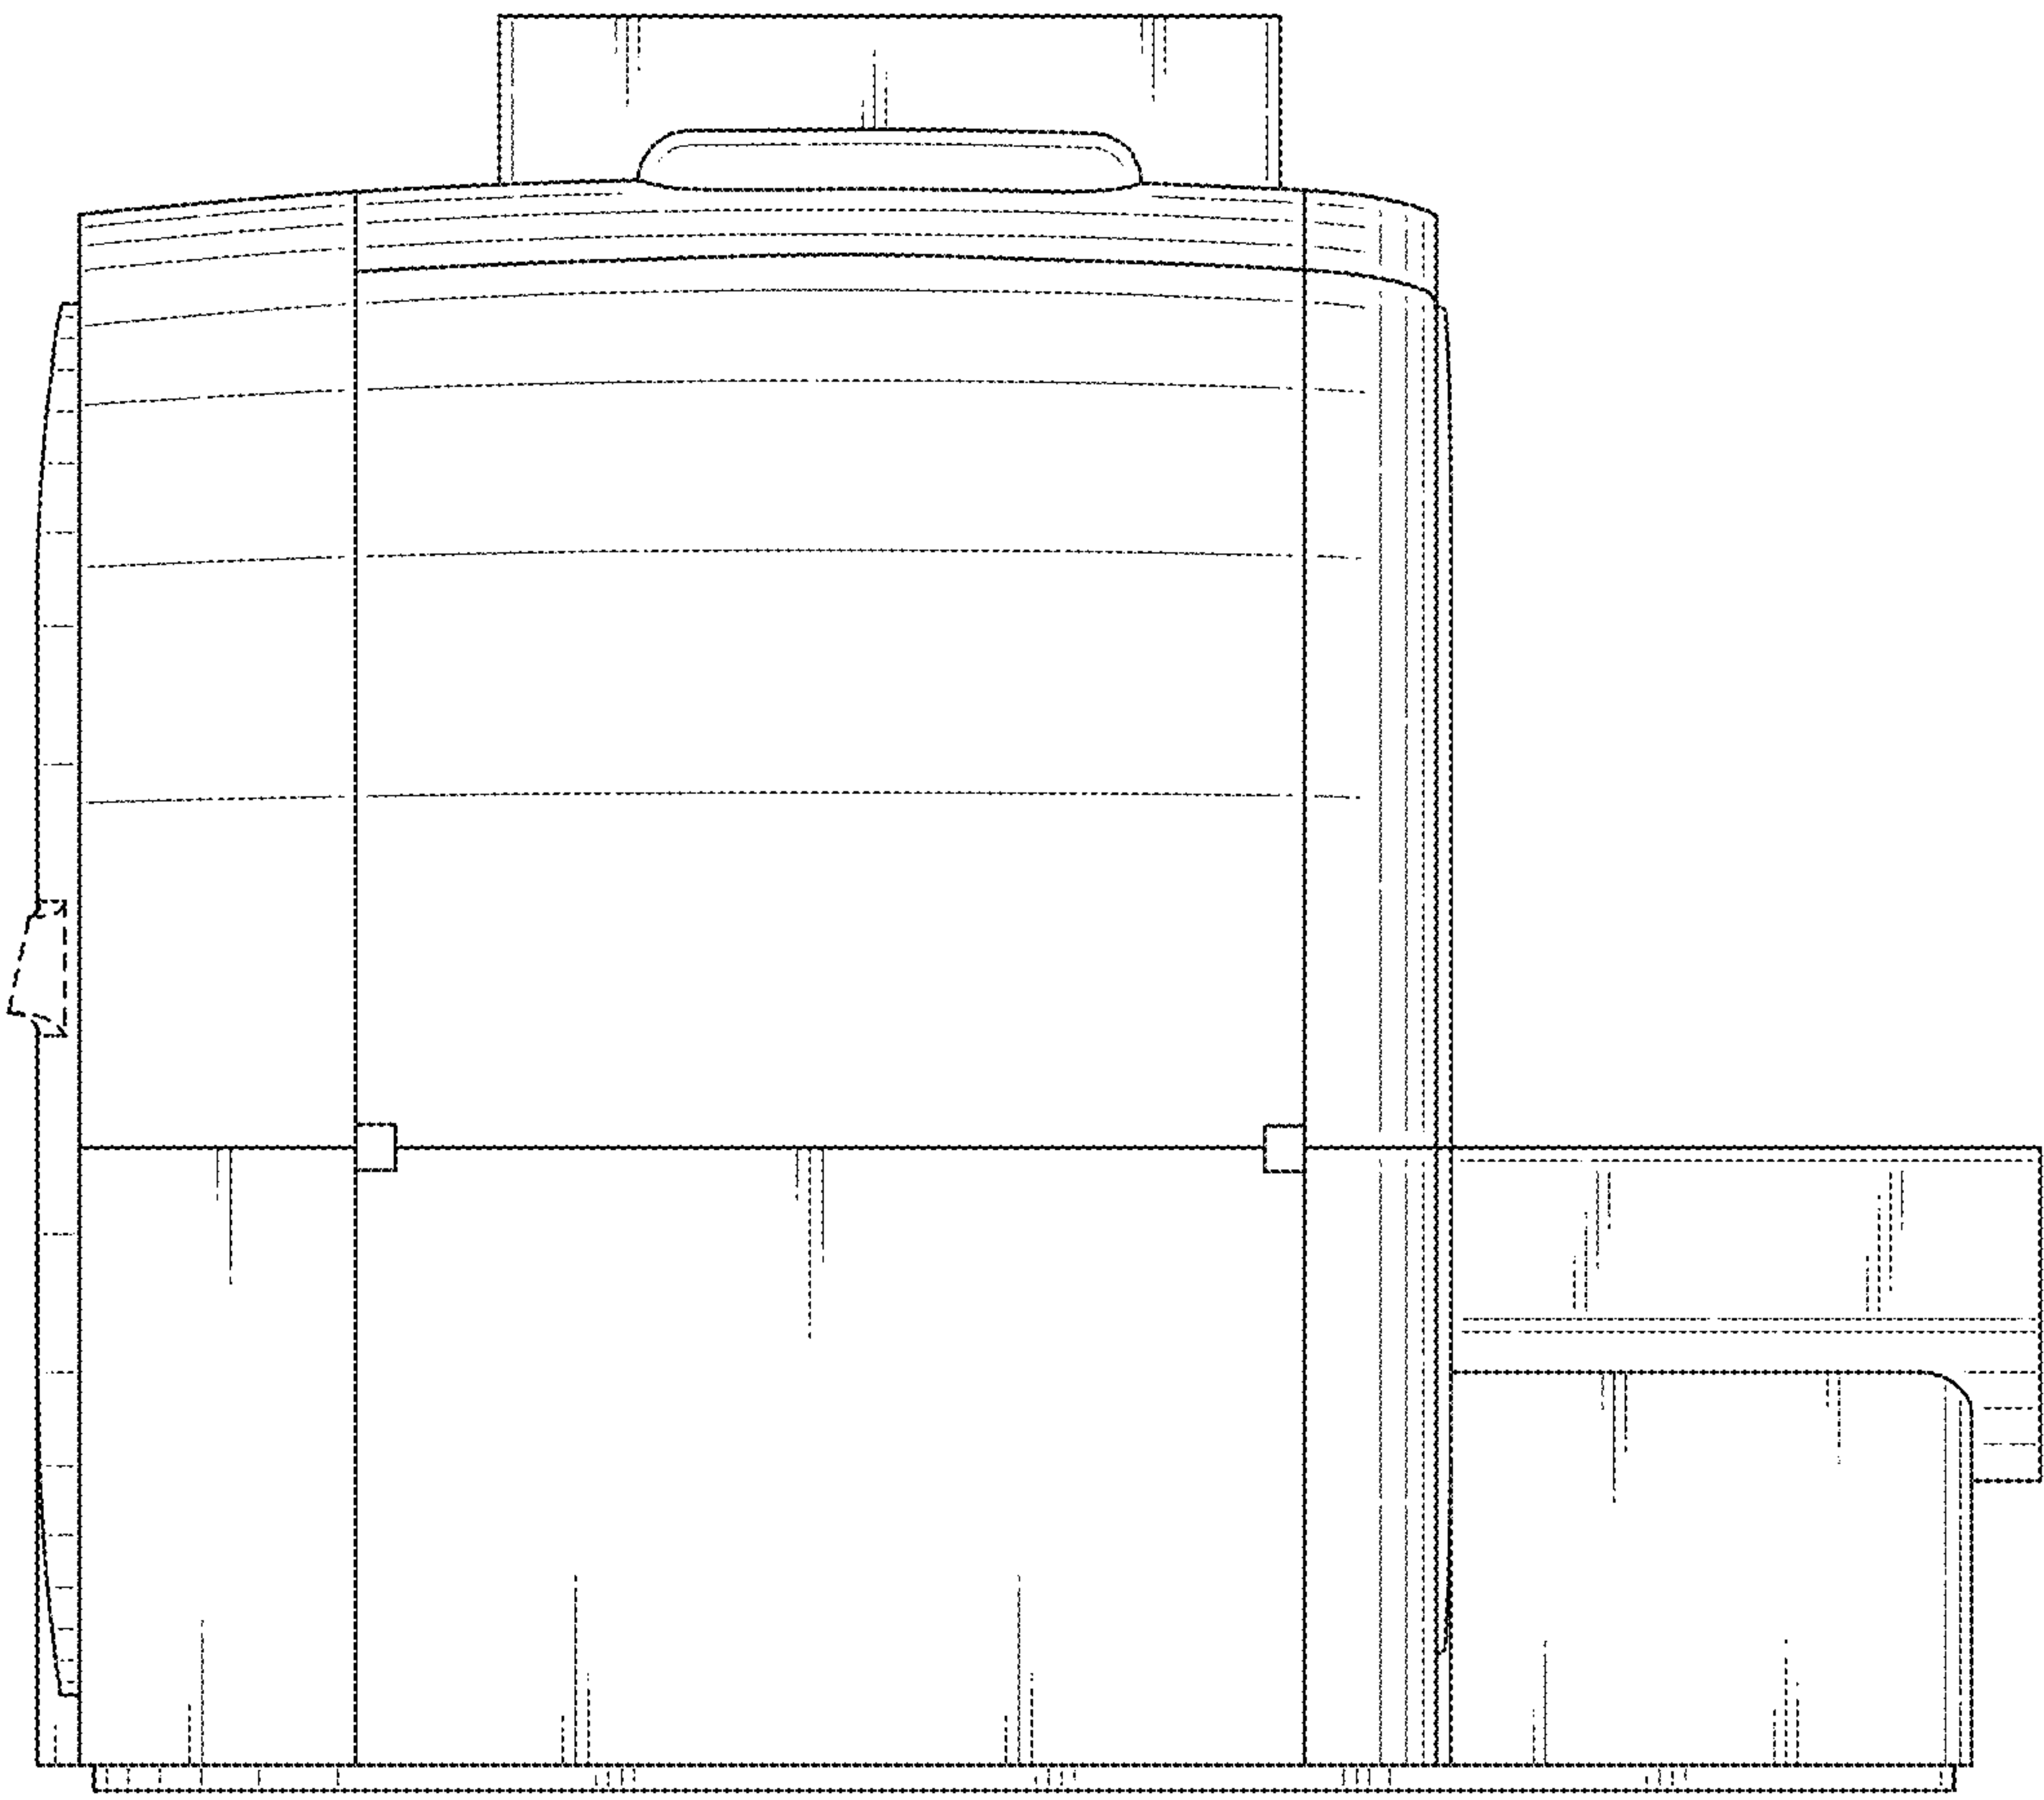


Fig. 10

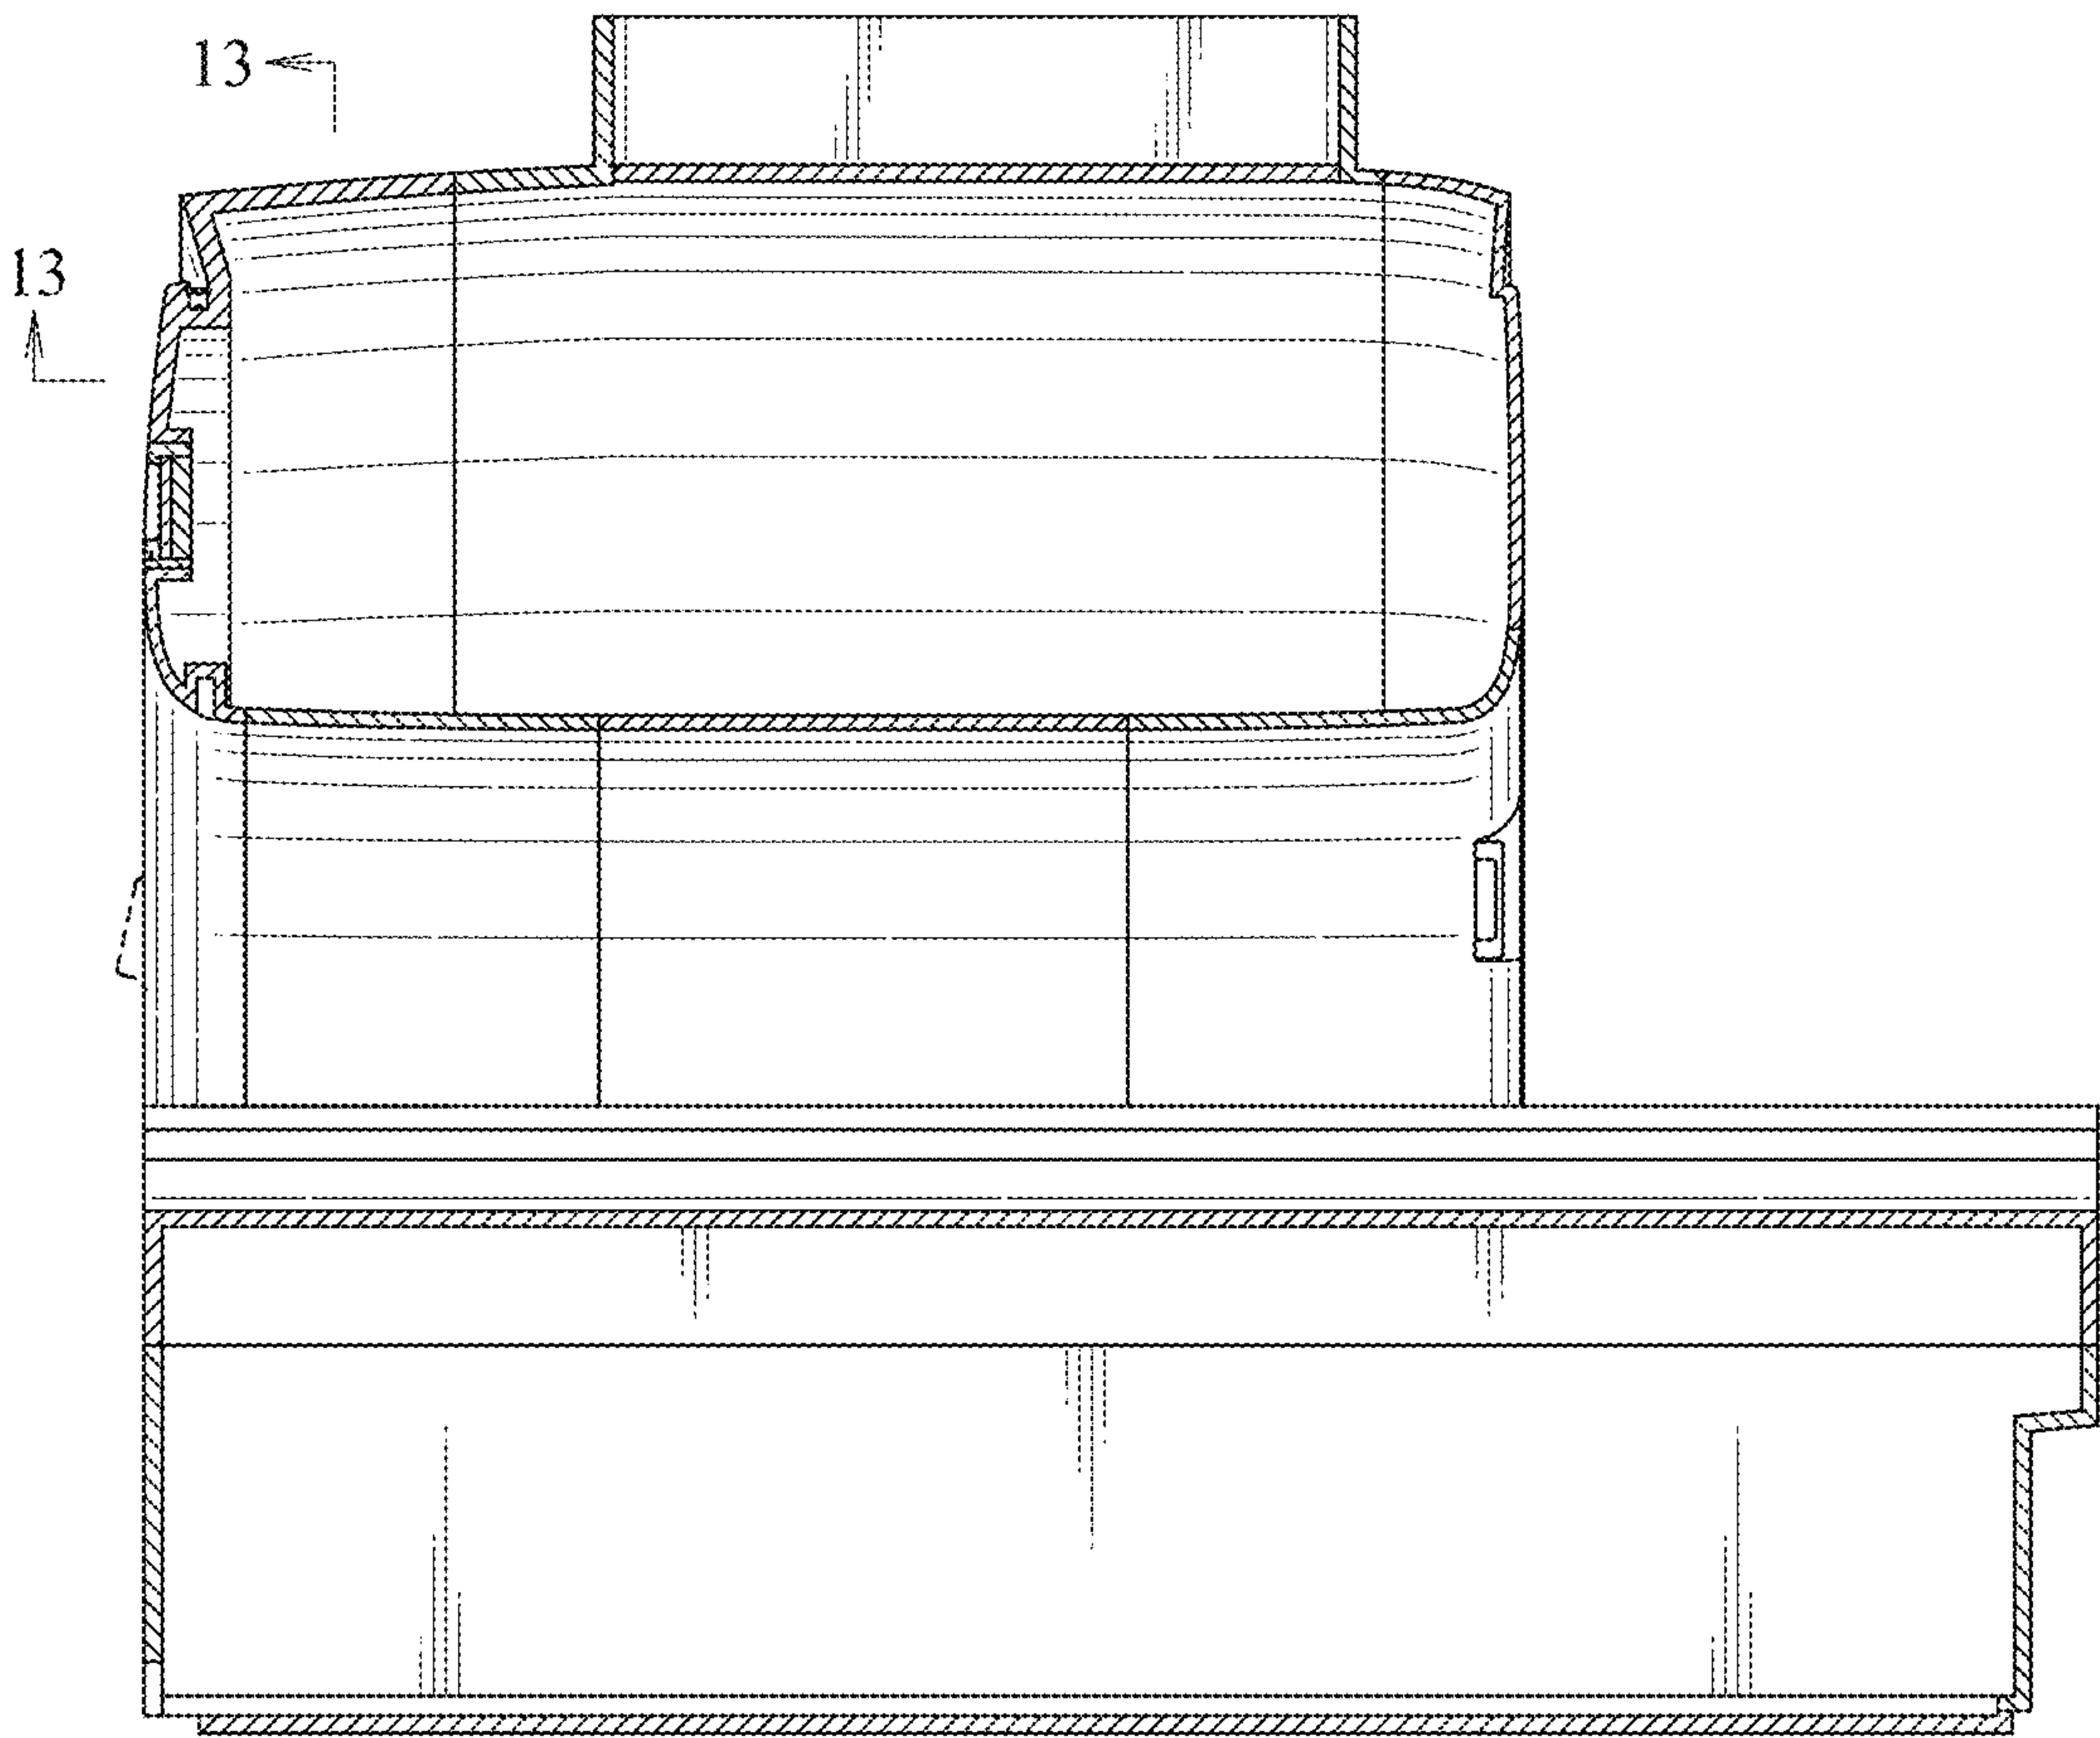


Fig. 11

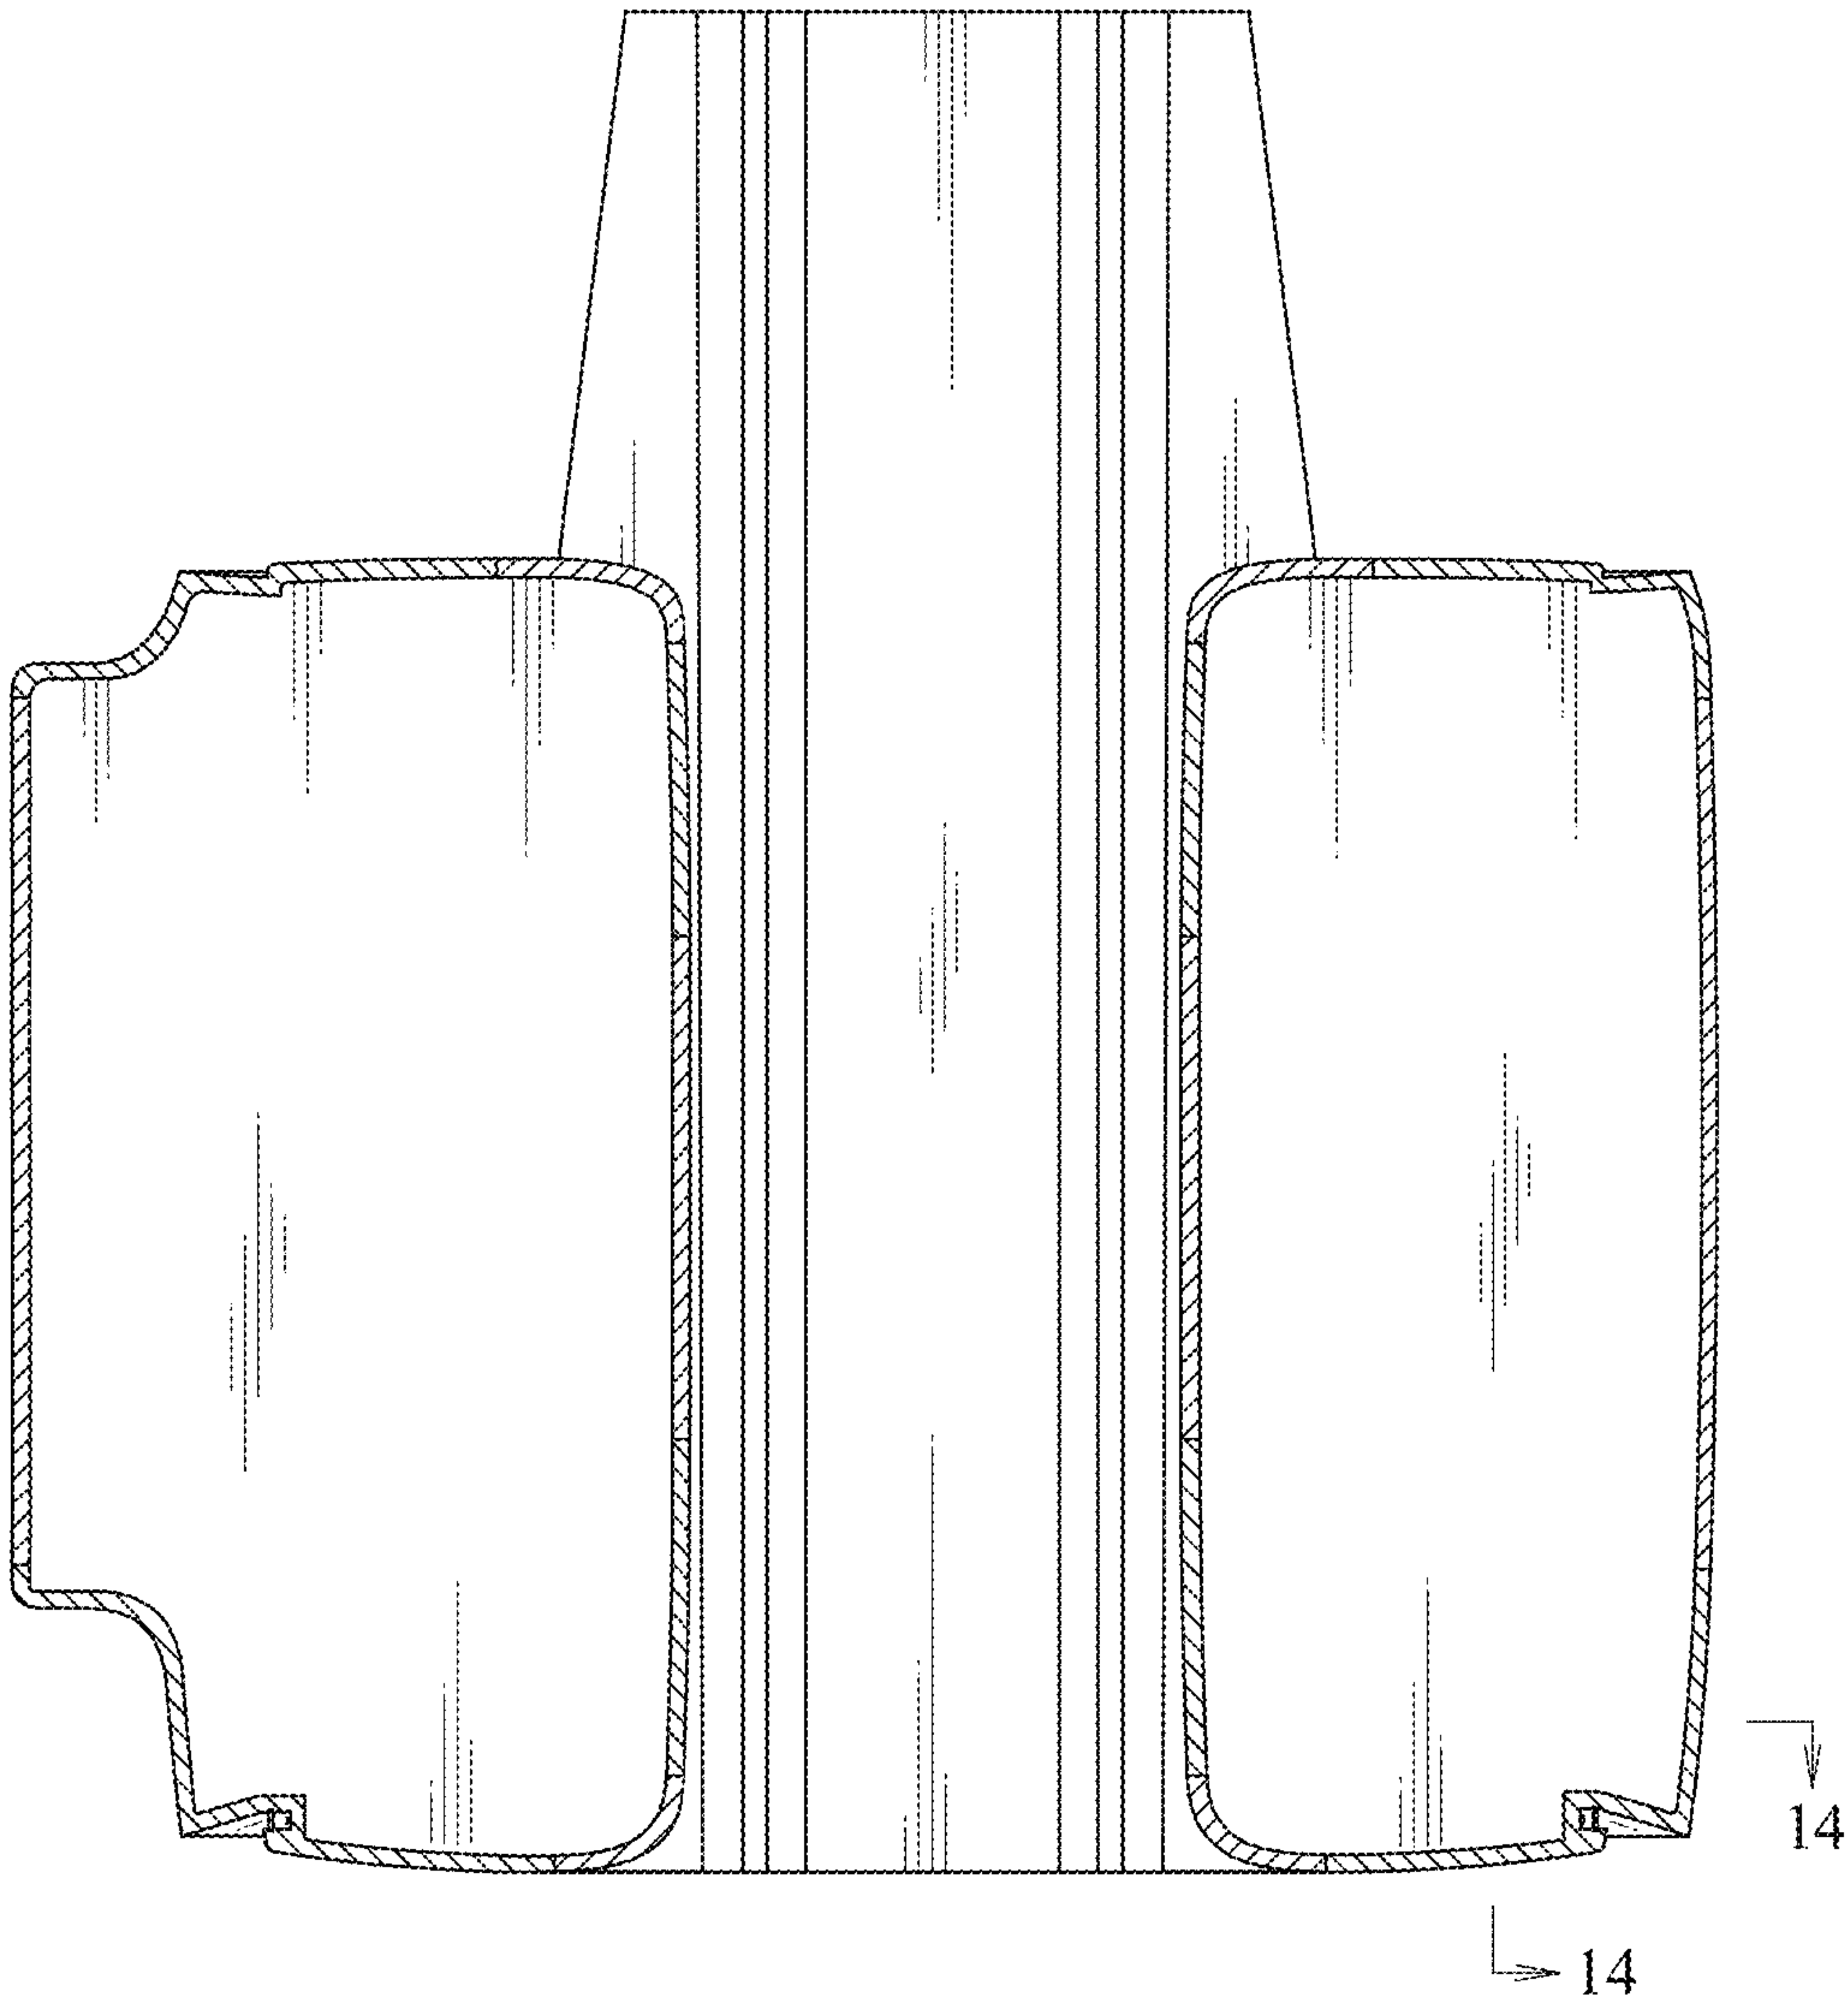


Fig. 12

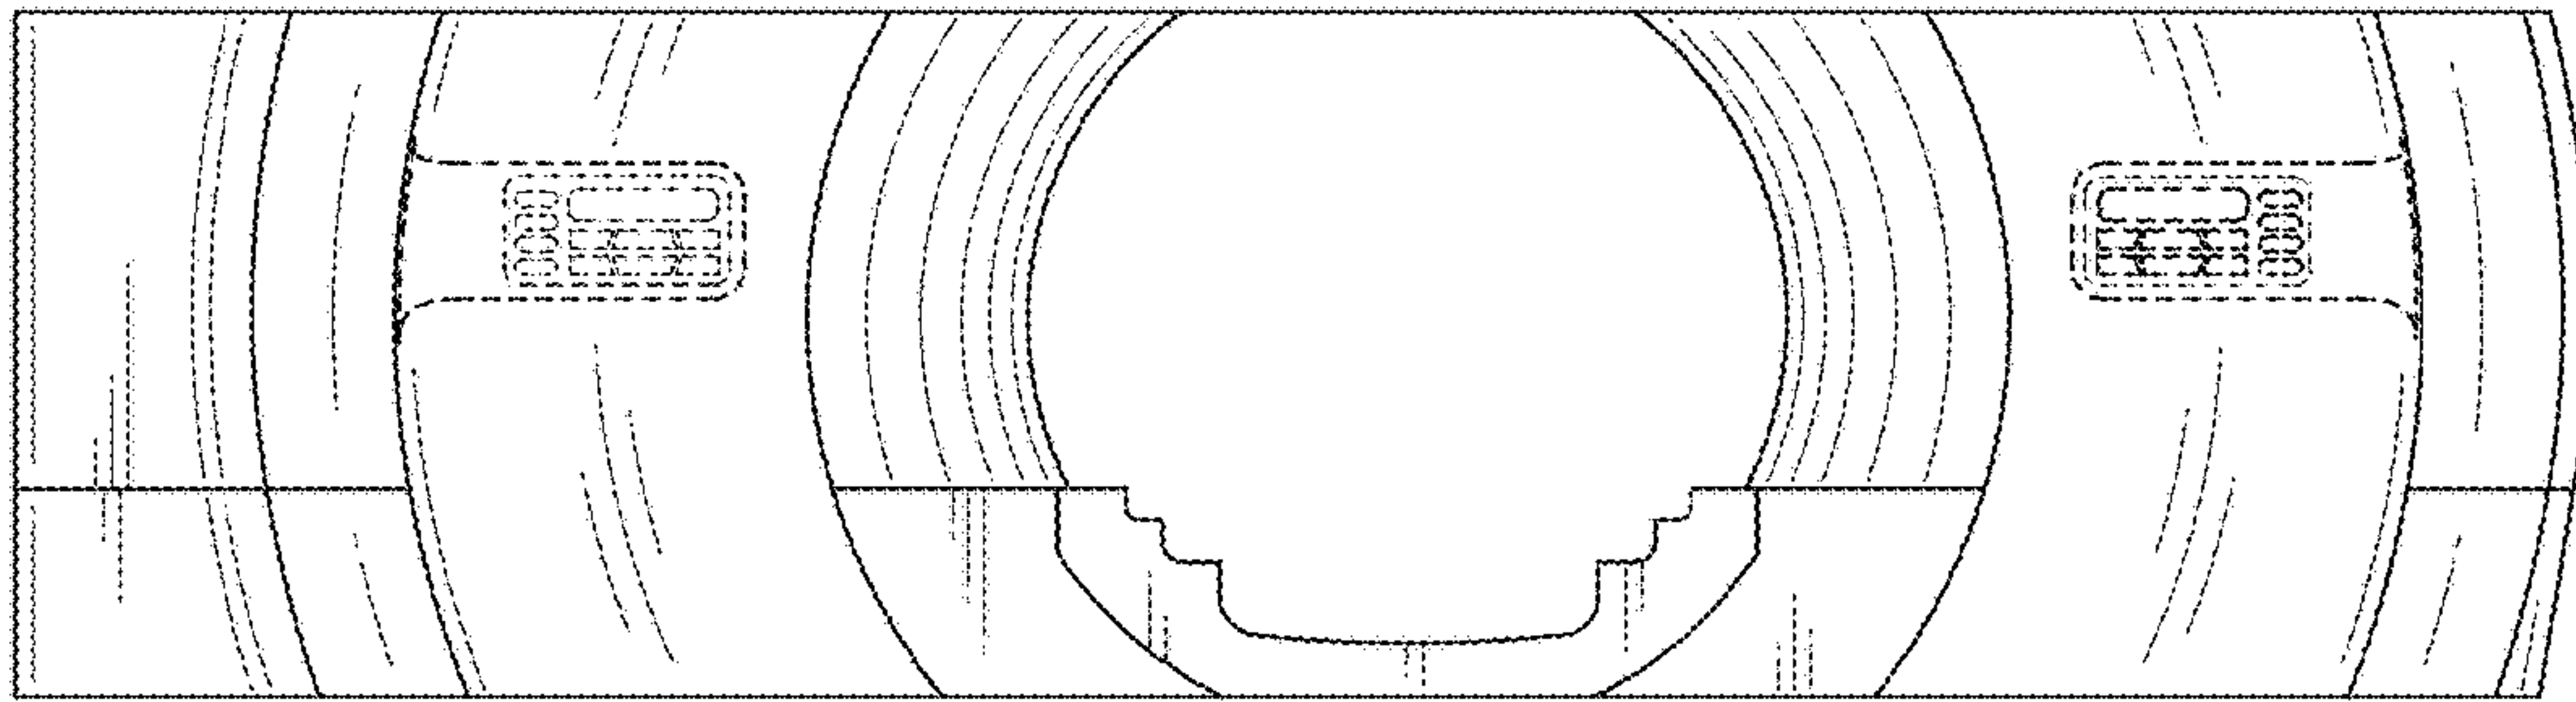


Fig. 13

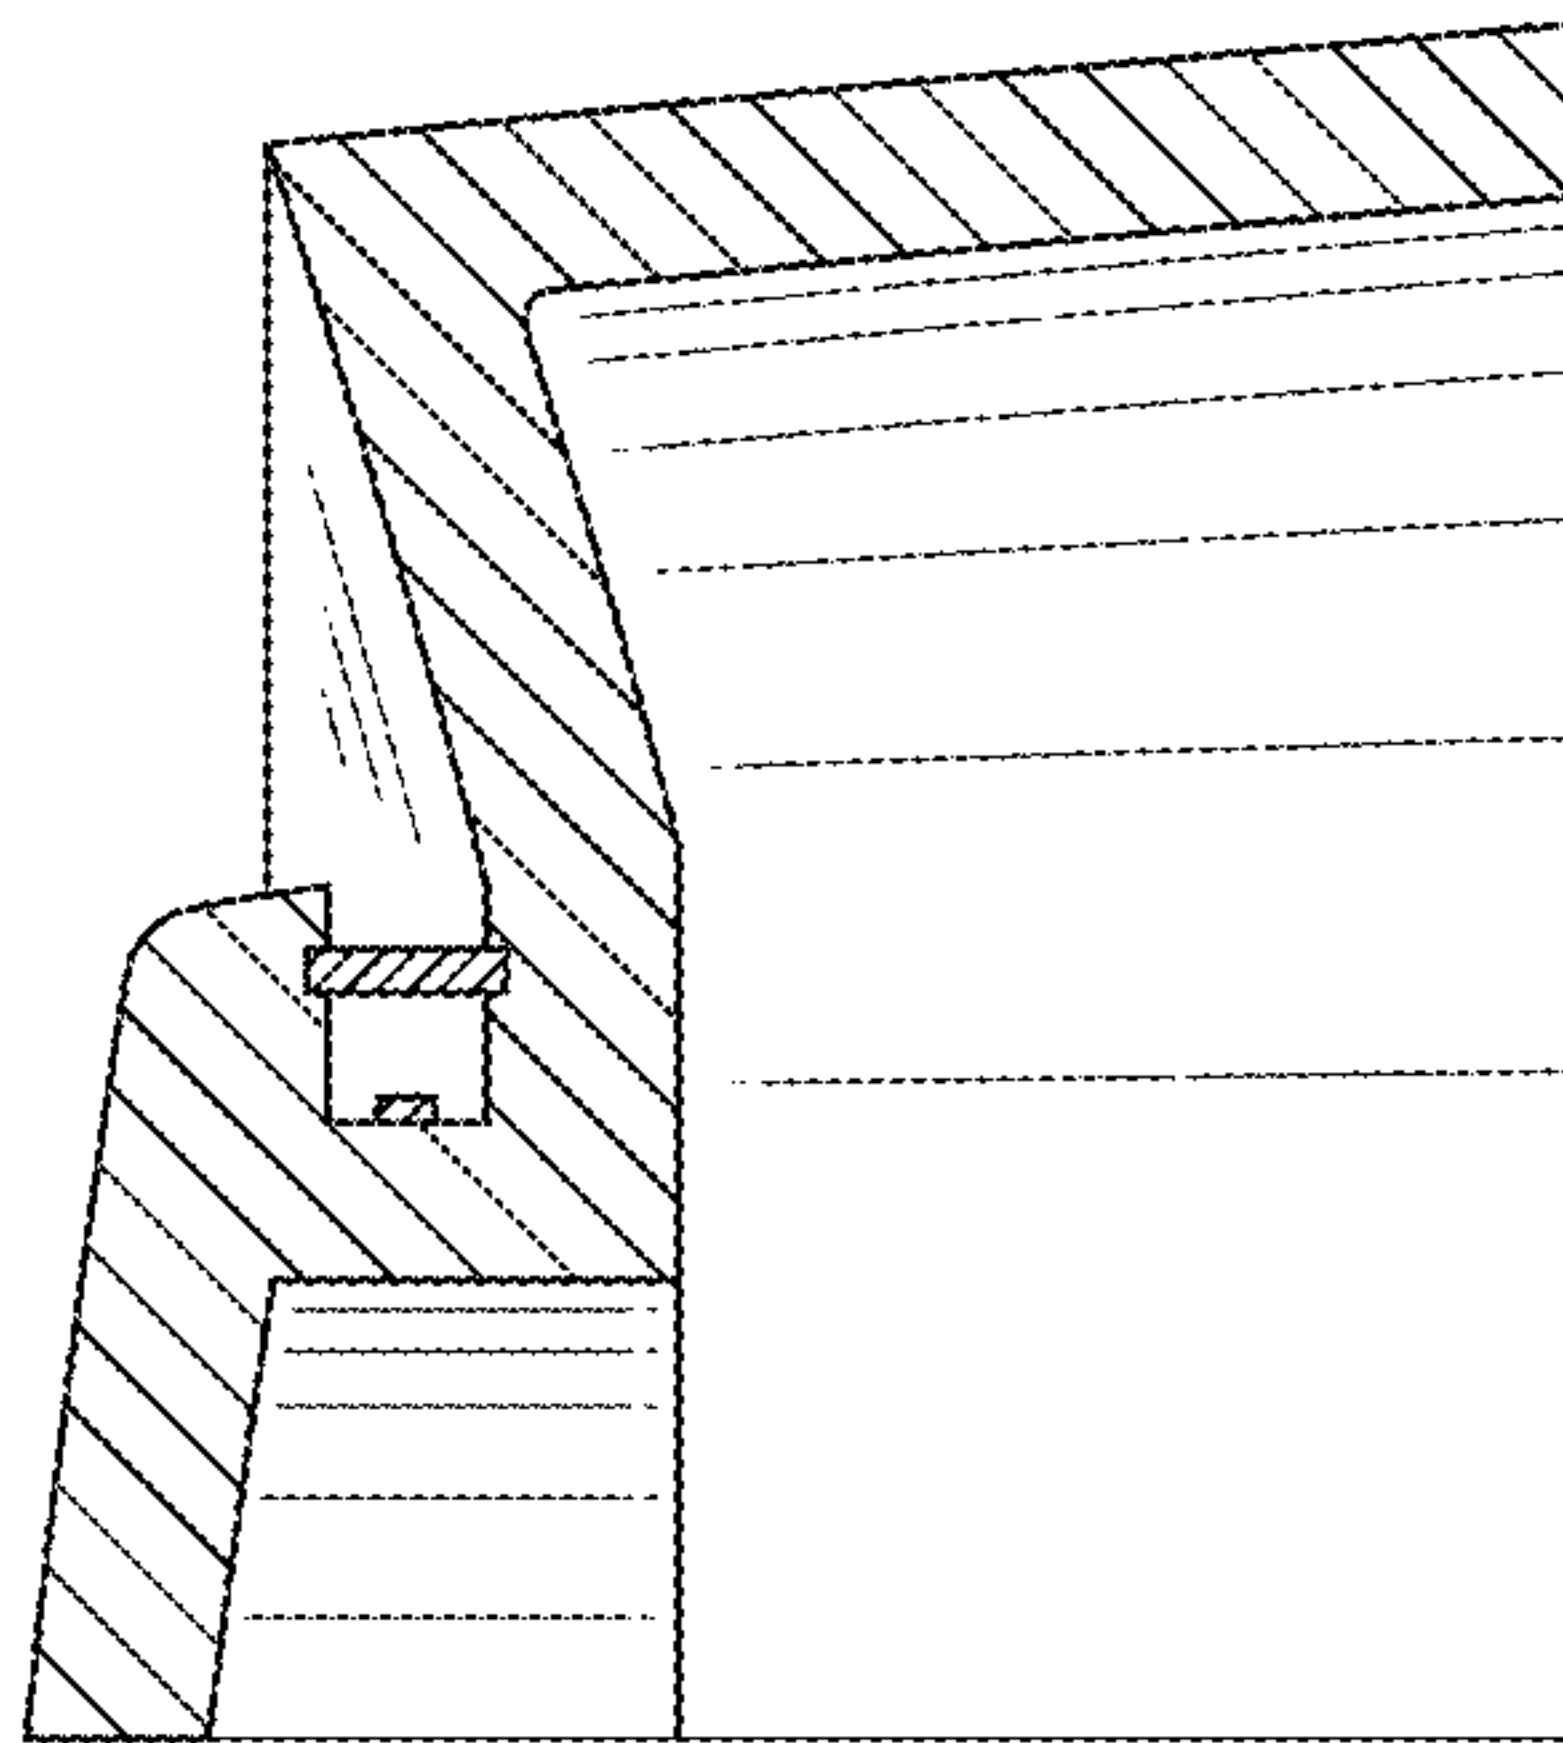


Fig. 14

