



US00D808017S

(12) **United States Design Patent**
Ito et al.

(10) **Patent No.:** **US D808,017 S**
(45) **Date of Patent:** **** Jan. 16, 2018**

(54) **OXYGEN CONCENTRATING APPARATUS**
(71) Applicant: **TEIJIN PHARMA LIMITED**, Tokyo (JP)
(72) Inventors: **Shinichi Ito**, Tokyo (JP); **Hideo Nawata**, Tokyo (JP)
(73) Assignee: **Teijin Pharma Limited**, Tokyo (JP)
(**) Term: **15 Years**

D734,446 S * 7/2015 Salmon D24/108
D734,856 S * 7/2015 Weichert D24/186
D744,658 S * 12/2015 Hilkey-Boyatt D11/86
D746,476 S * 12/2015 Noda D24/186
D748,803 S * 2/2016 Zhang D24/170
D749,541 S * 2/2016 Wong D14/170
D790,685 S * 6/2017 Silkaitis D24/110.5
2005/0161044 A1 * 7/2005 Yoshida A61M 16/101
128/205.27
2012/0291884 A1 * 11/2012 Yamaura A61M 16/10
137/455
2013/0233168 A1 * 9/2013 Richey, II B01D 53/0454
95/1

(21) Appl. No.: **29/575,068**

(22) Filed: **Aug. 22, 2016**

(30) **Foreign Application Priority Data**

Feb. 24, 2016 (JP) 2016-003974

(51) **LOC (11) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/164**

(58) **Field of Classification Search**
USPC D24/164, 170, 185, 186, 110, 110.1,
D24/110.4, 110.5, 110.6
CPC .. A61M 16/06; A61M 16/101; A61M 16/107;
A61M 2016/1025; A61M 16/10; A61M
2202/0208

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D249,063 S * 8/1978 James D13/162
D490,155 S * 5/2004 Nakamura D24/164
D513,074 S * 12/2005 Nakamura D24/164
D550,360 S * 9/2007 McCombs D24/164
D604,417 S 11/2009 Fujimoto et al.
D606,655 S * 12/2009 Wilkinson D24/164
D642,273 S * 7/2011 McCombs D24/164
D693,005 S 11/2013 Nawata et al.
D702,353 S 4/2014 Fujimoto et al.

(Continued)

FOREIGN PATENT DOCUMENTS

JP 1096642 S 1/2001
JP 1154513 S 9/2002

(Continued)

Primary Examiner — Holly H Baynham

Assistant Examiner — Calvin E Vansant

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC


(57) **CLAIM**

The ornamental design for an oxygen concentrating apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an oxygen concentrating apparatus showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a left elevational view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is a rear elevational view thereof; FIG. 6 is a top plan view thereof; FIG. 7 is a bottom plan view thereof; and, FIG. 8 is a rear perspective view thereof. The broken lines depict portions of the oxygen concentrating apparatus that form no part of the claim.

1 Claim, 6 Drawing Sheets

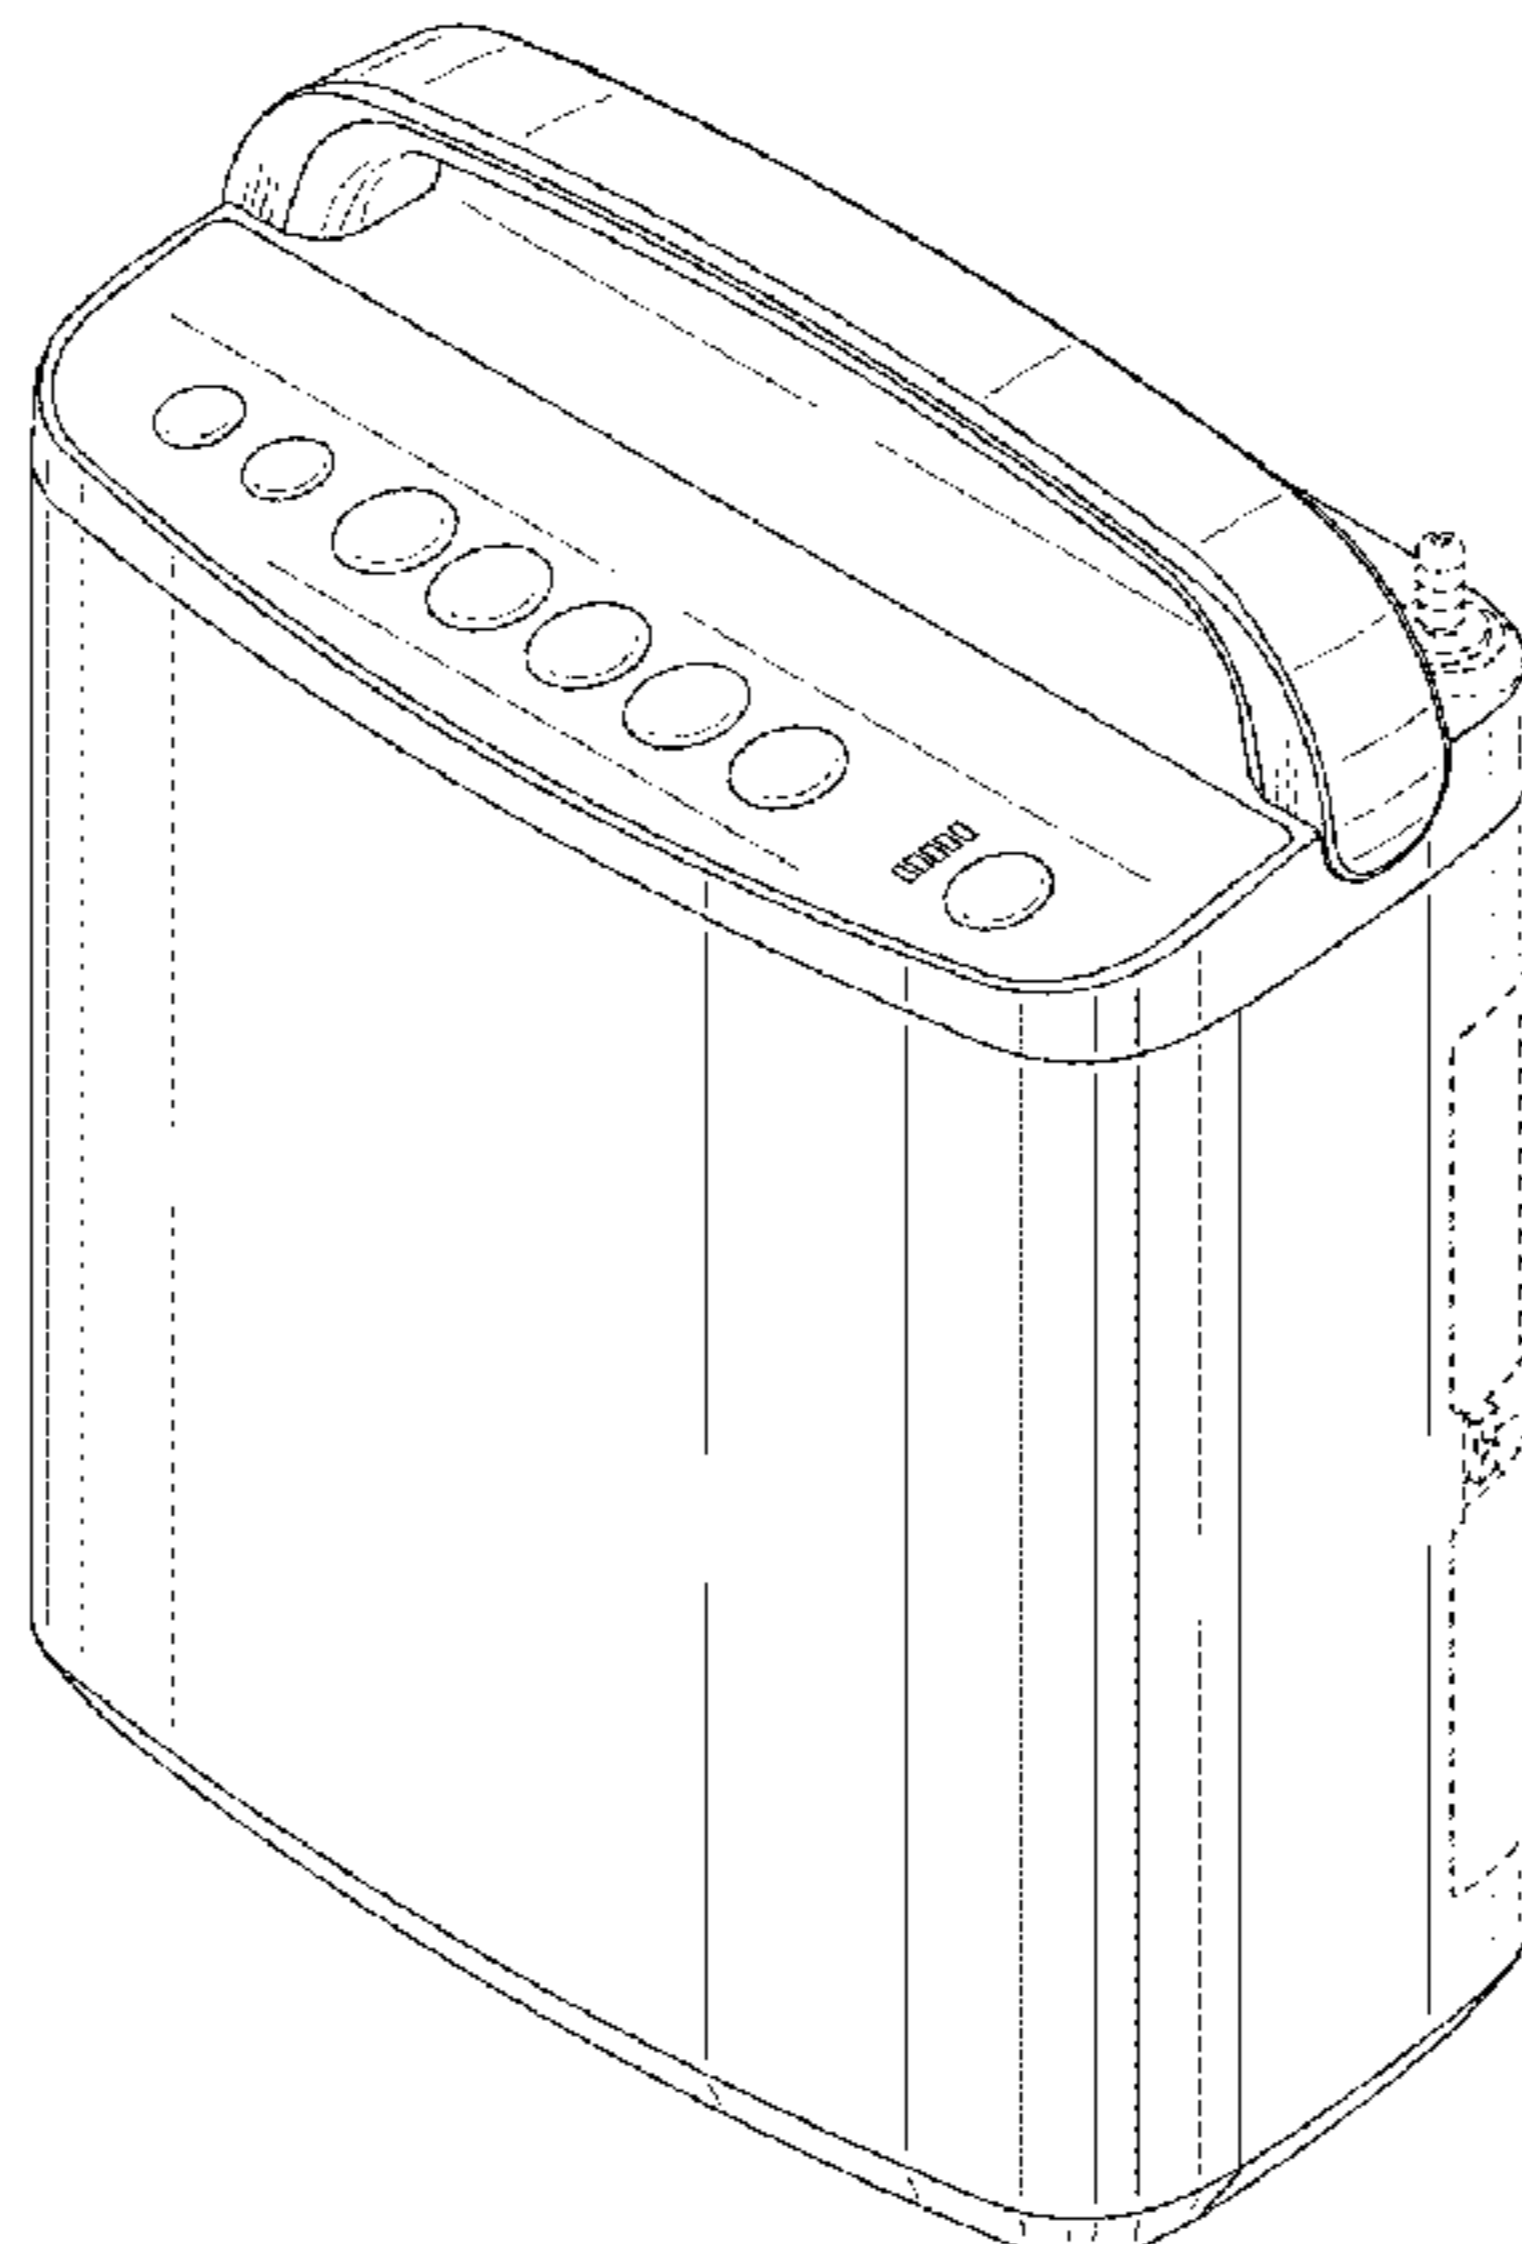

(56)

References Cited

U.S. PATENT DOCUMENTS

2015/0196727 A1* 7/2015 Ahmad A61M 16/101
128/202.26

FOREIGN PATENT DOCUMENTS

JP 1154786 S 9/2002
JP 1167851 S 3/2003
JP 1319419 S 1/2008
JP 1349622 S 1/2009
JP 2010119766 A * 6/2010
JP 1404303 S 12/2010
JP 1451754 S 9/2012
JP 1461487 S 2/2013
WO WO-2005028059 A2 * 3/2005 B01D 53/0407

* cited by examiner

FIG. 1

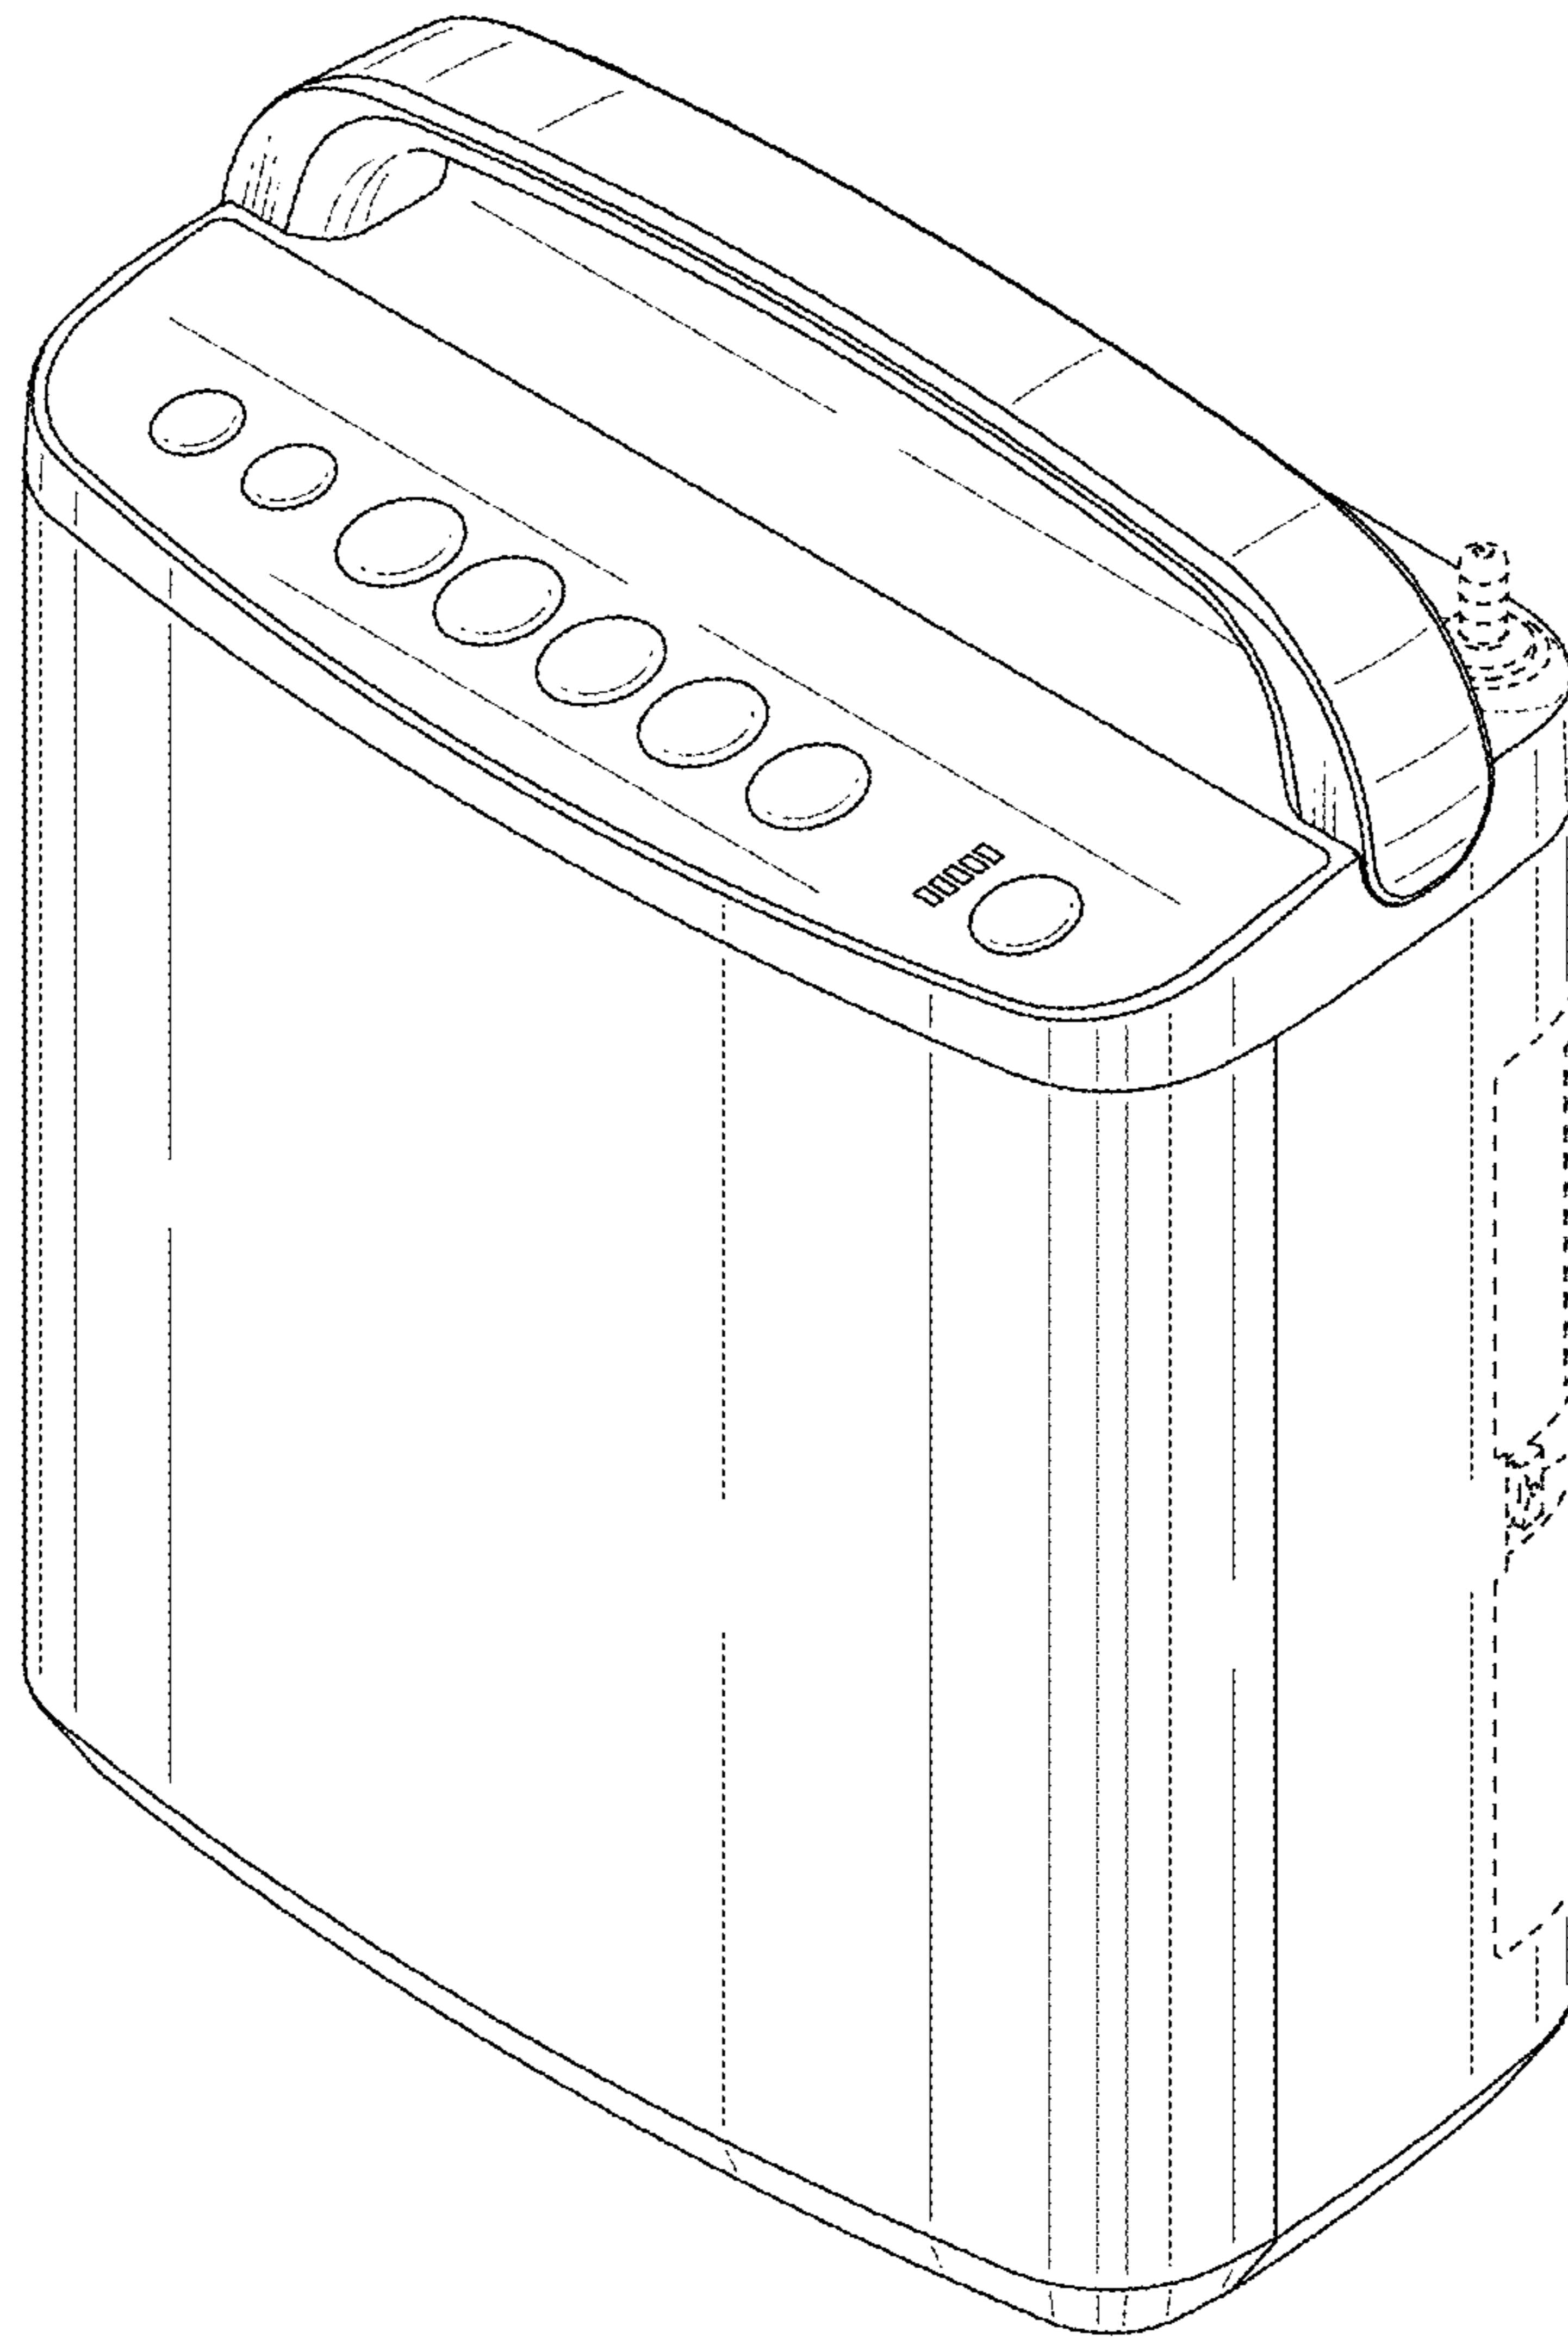


FIG. 2

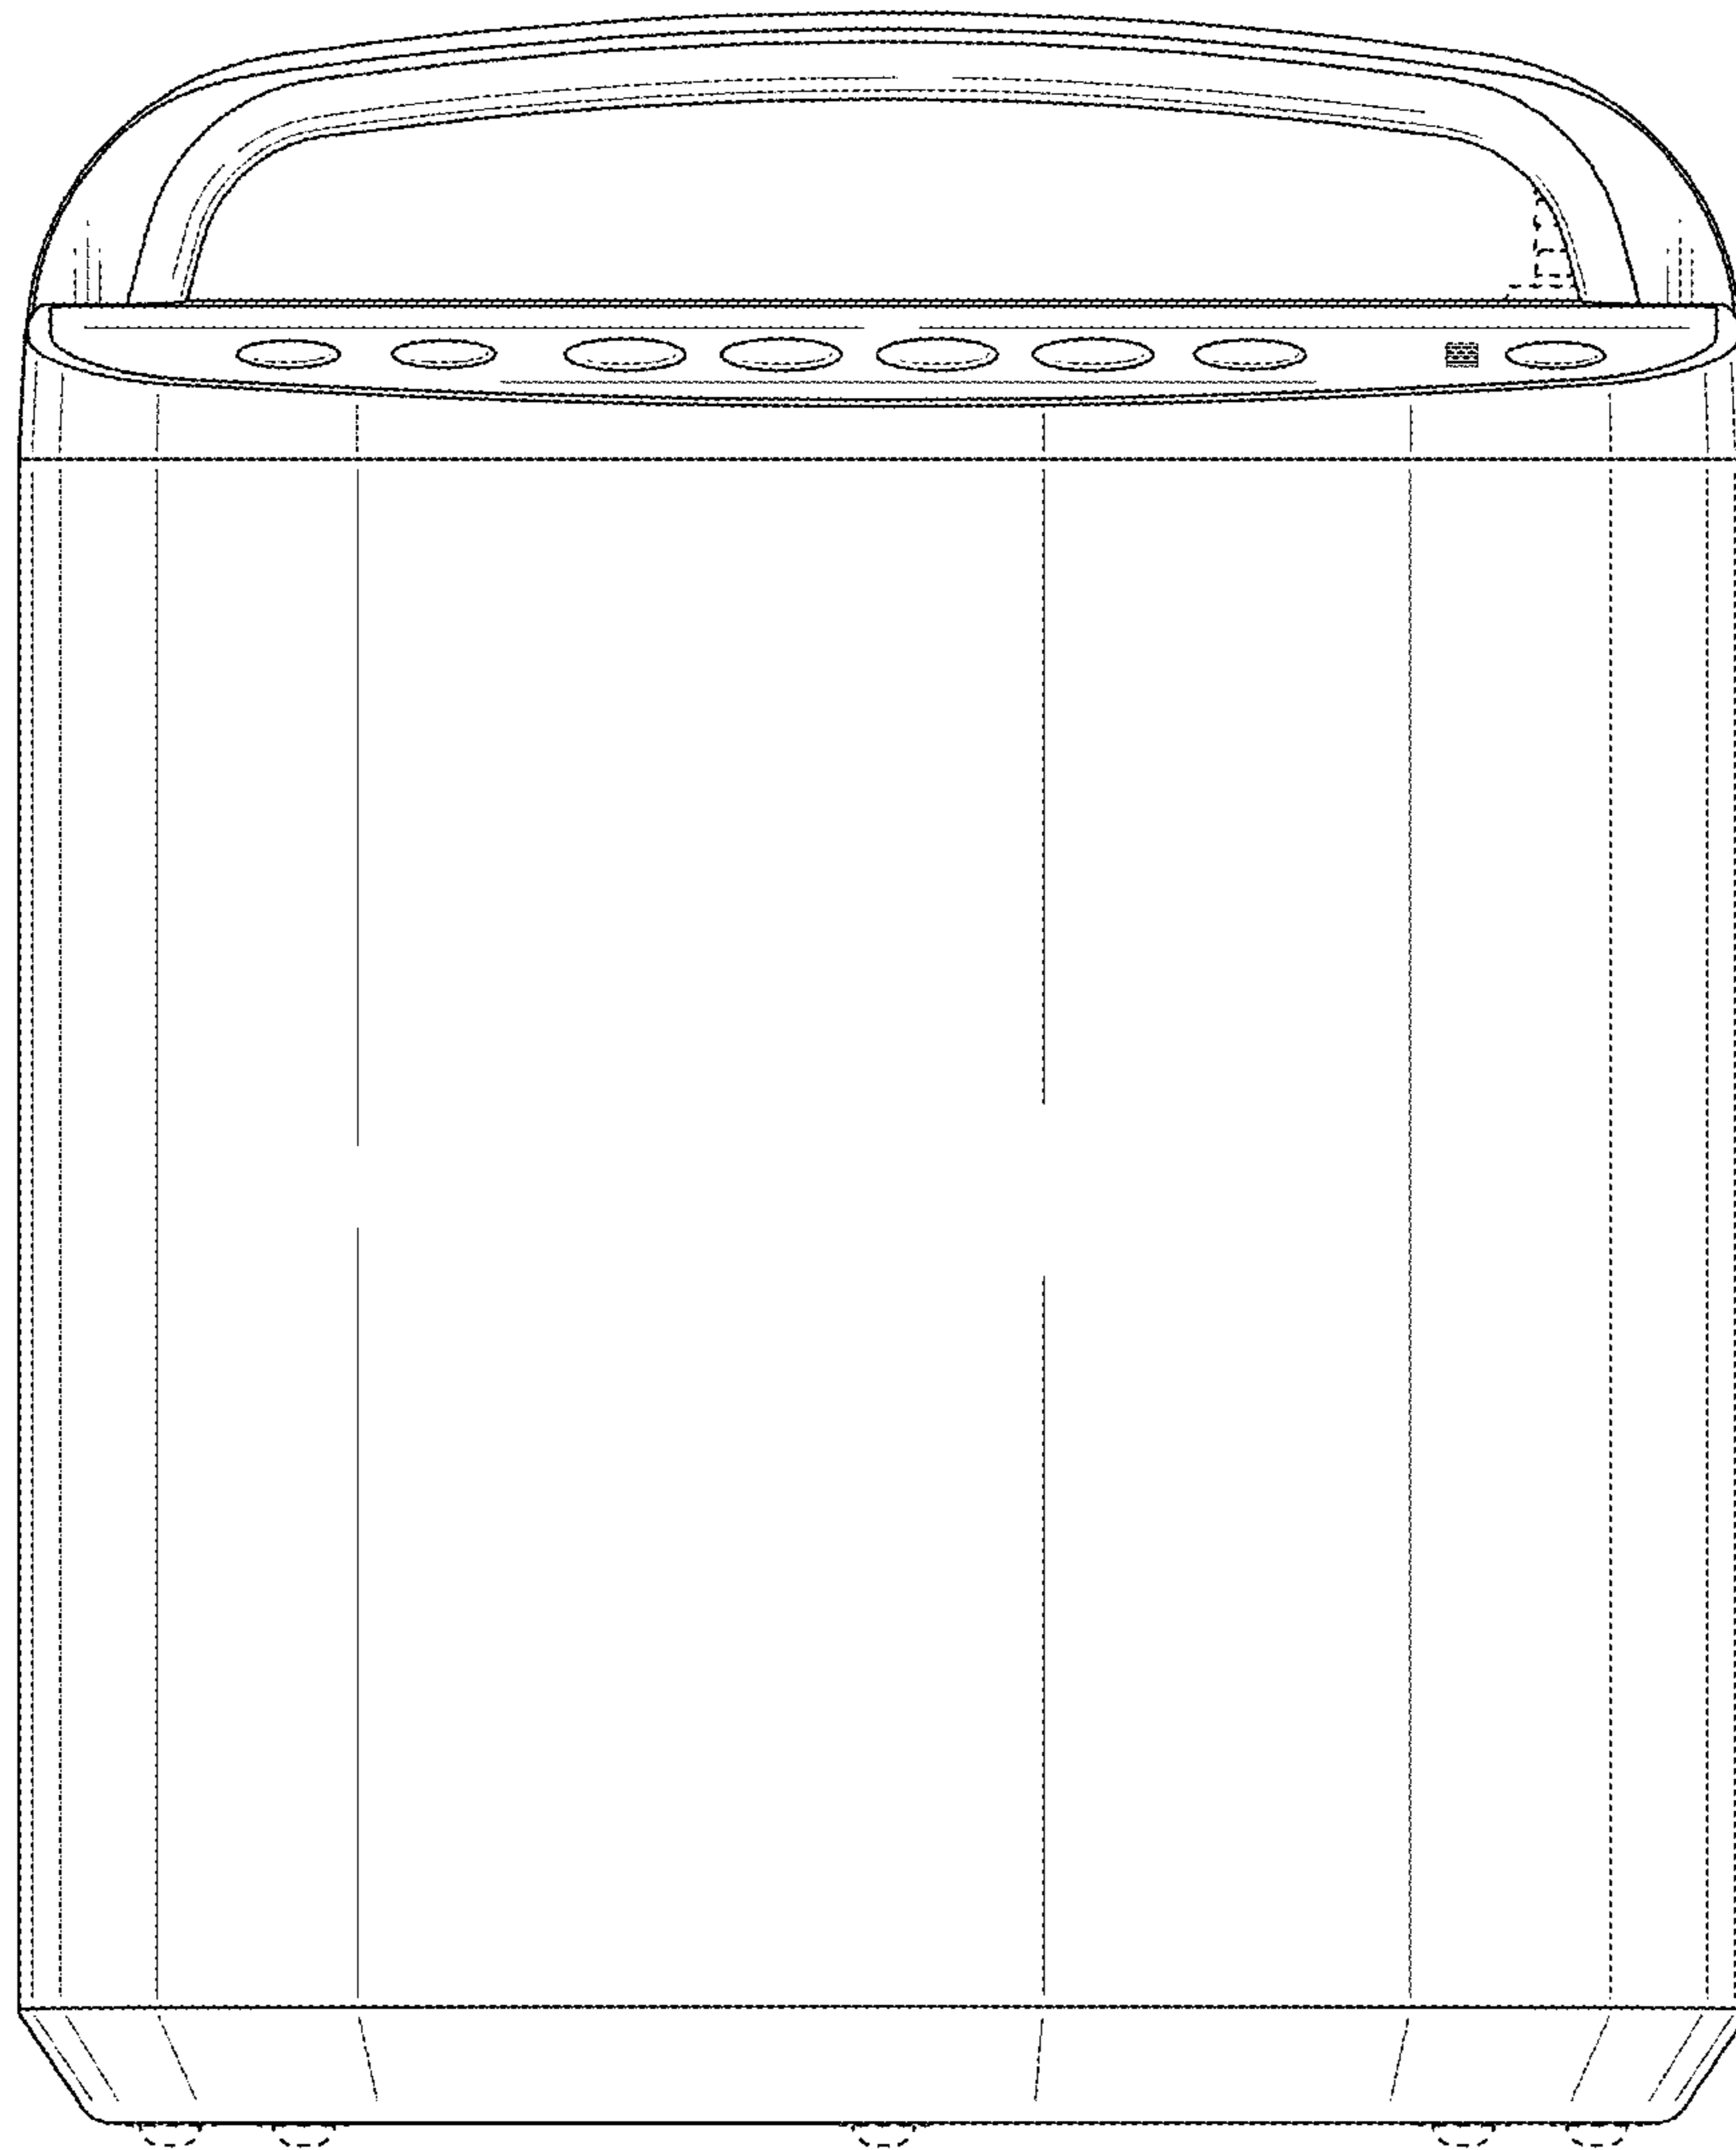


FIG. 3

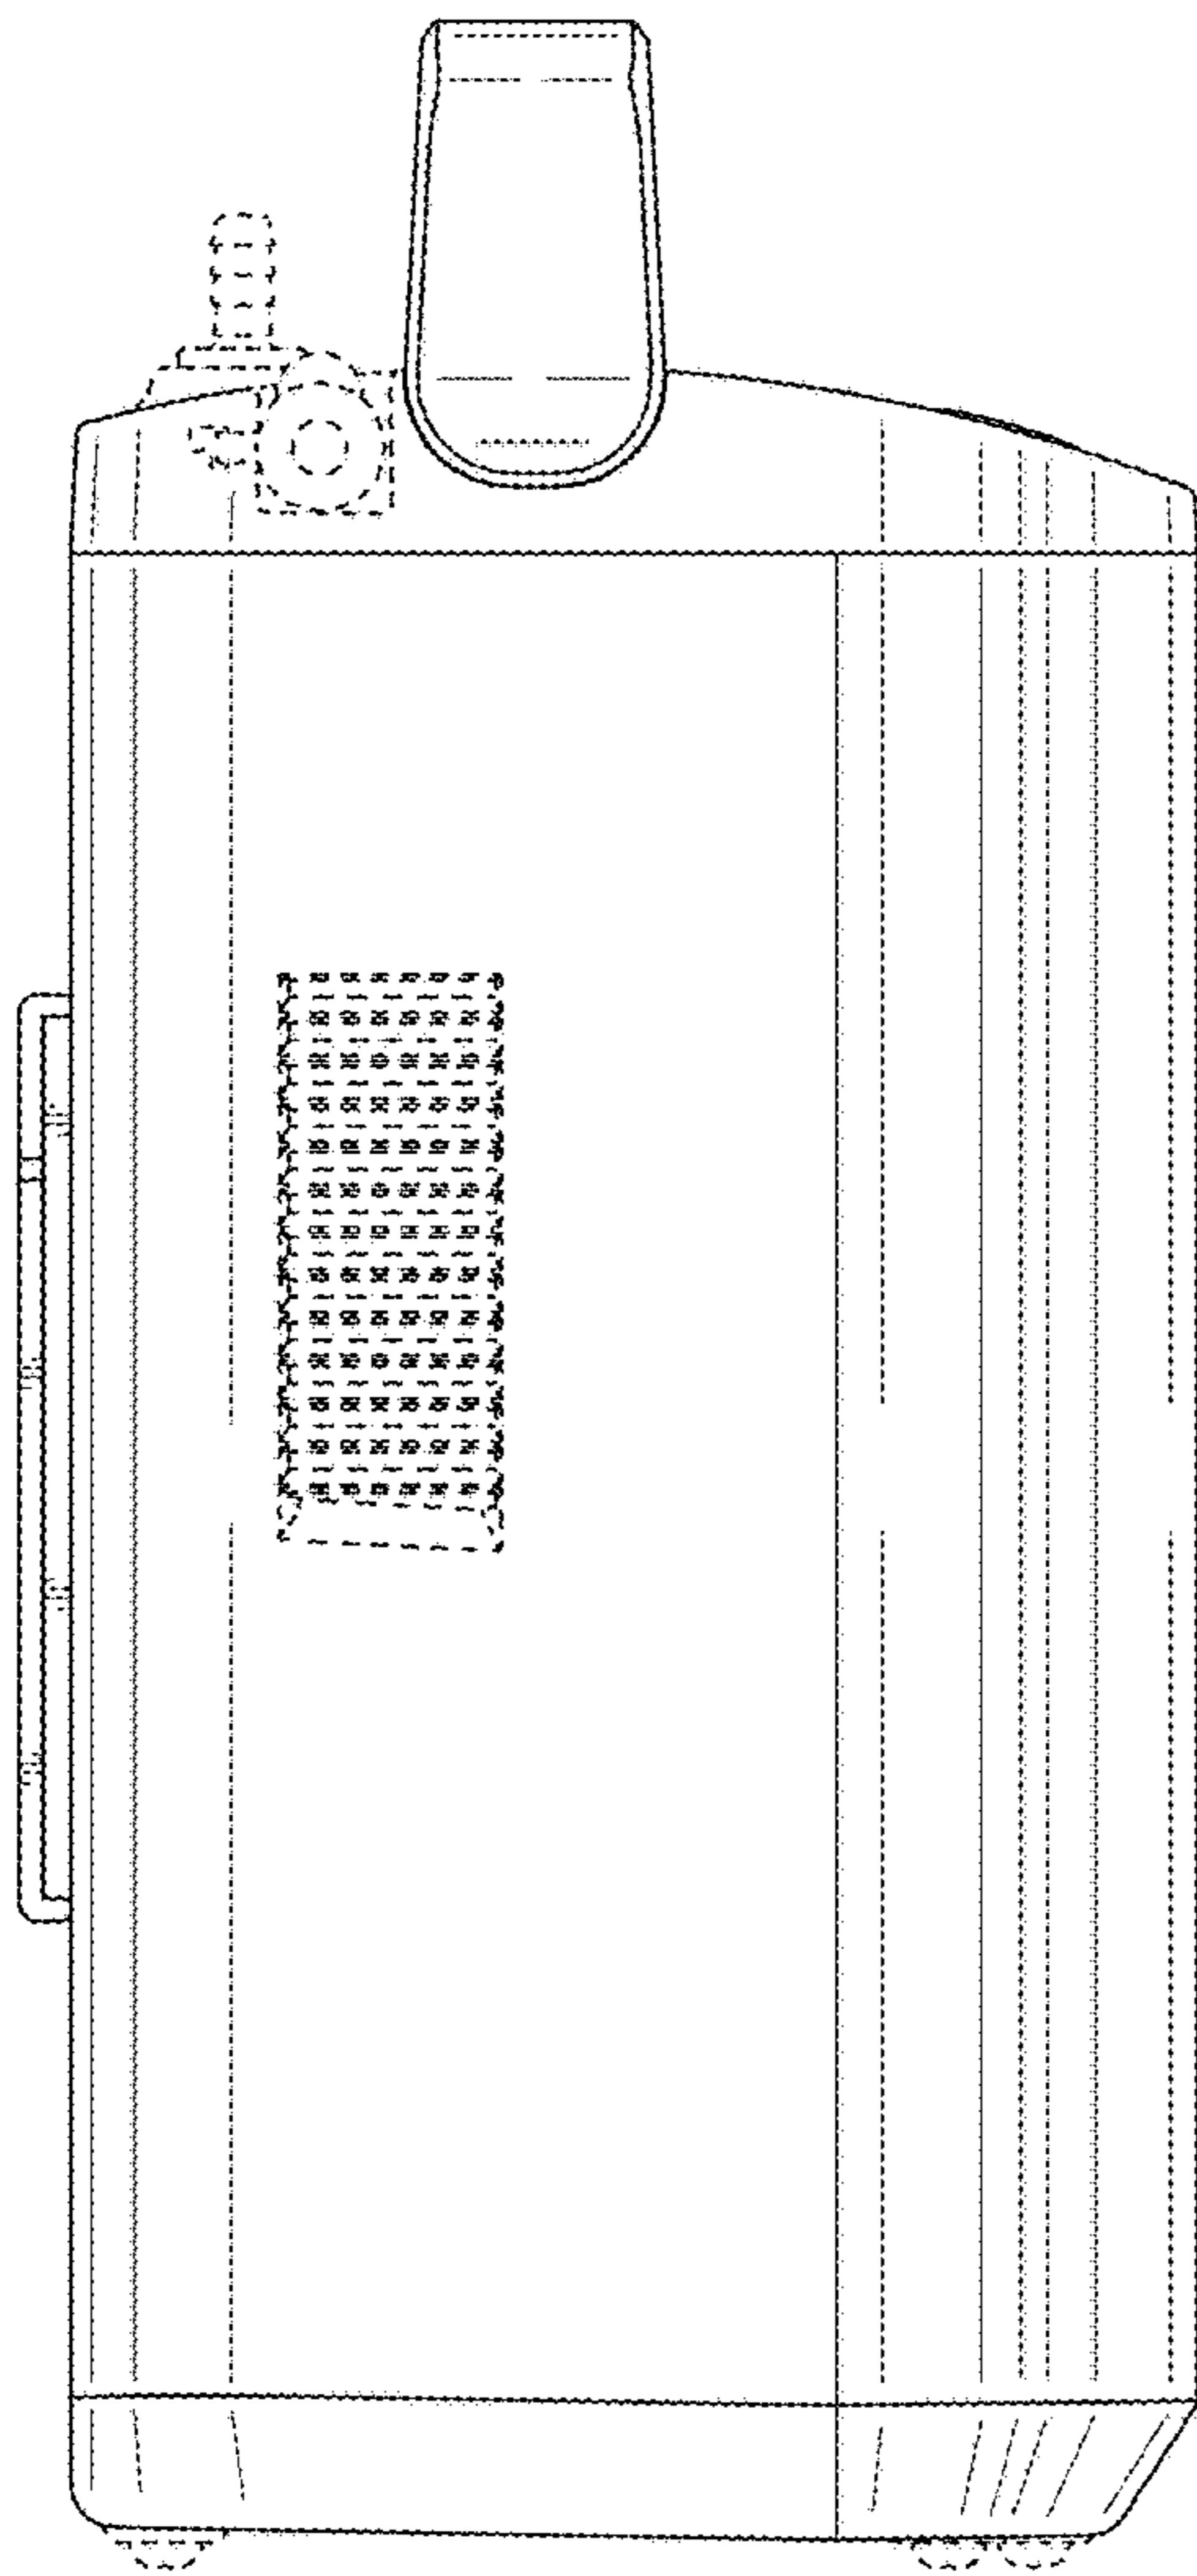


FIG. 4

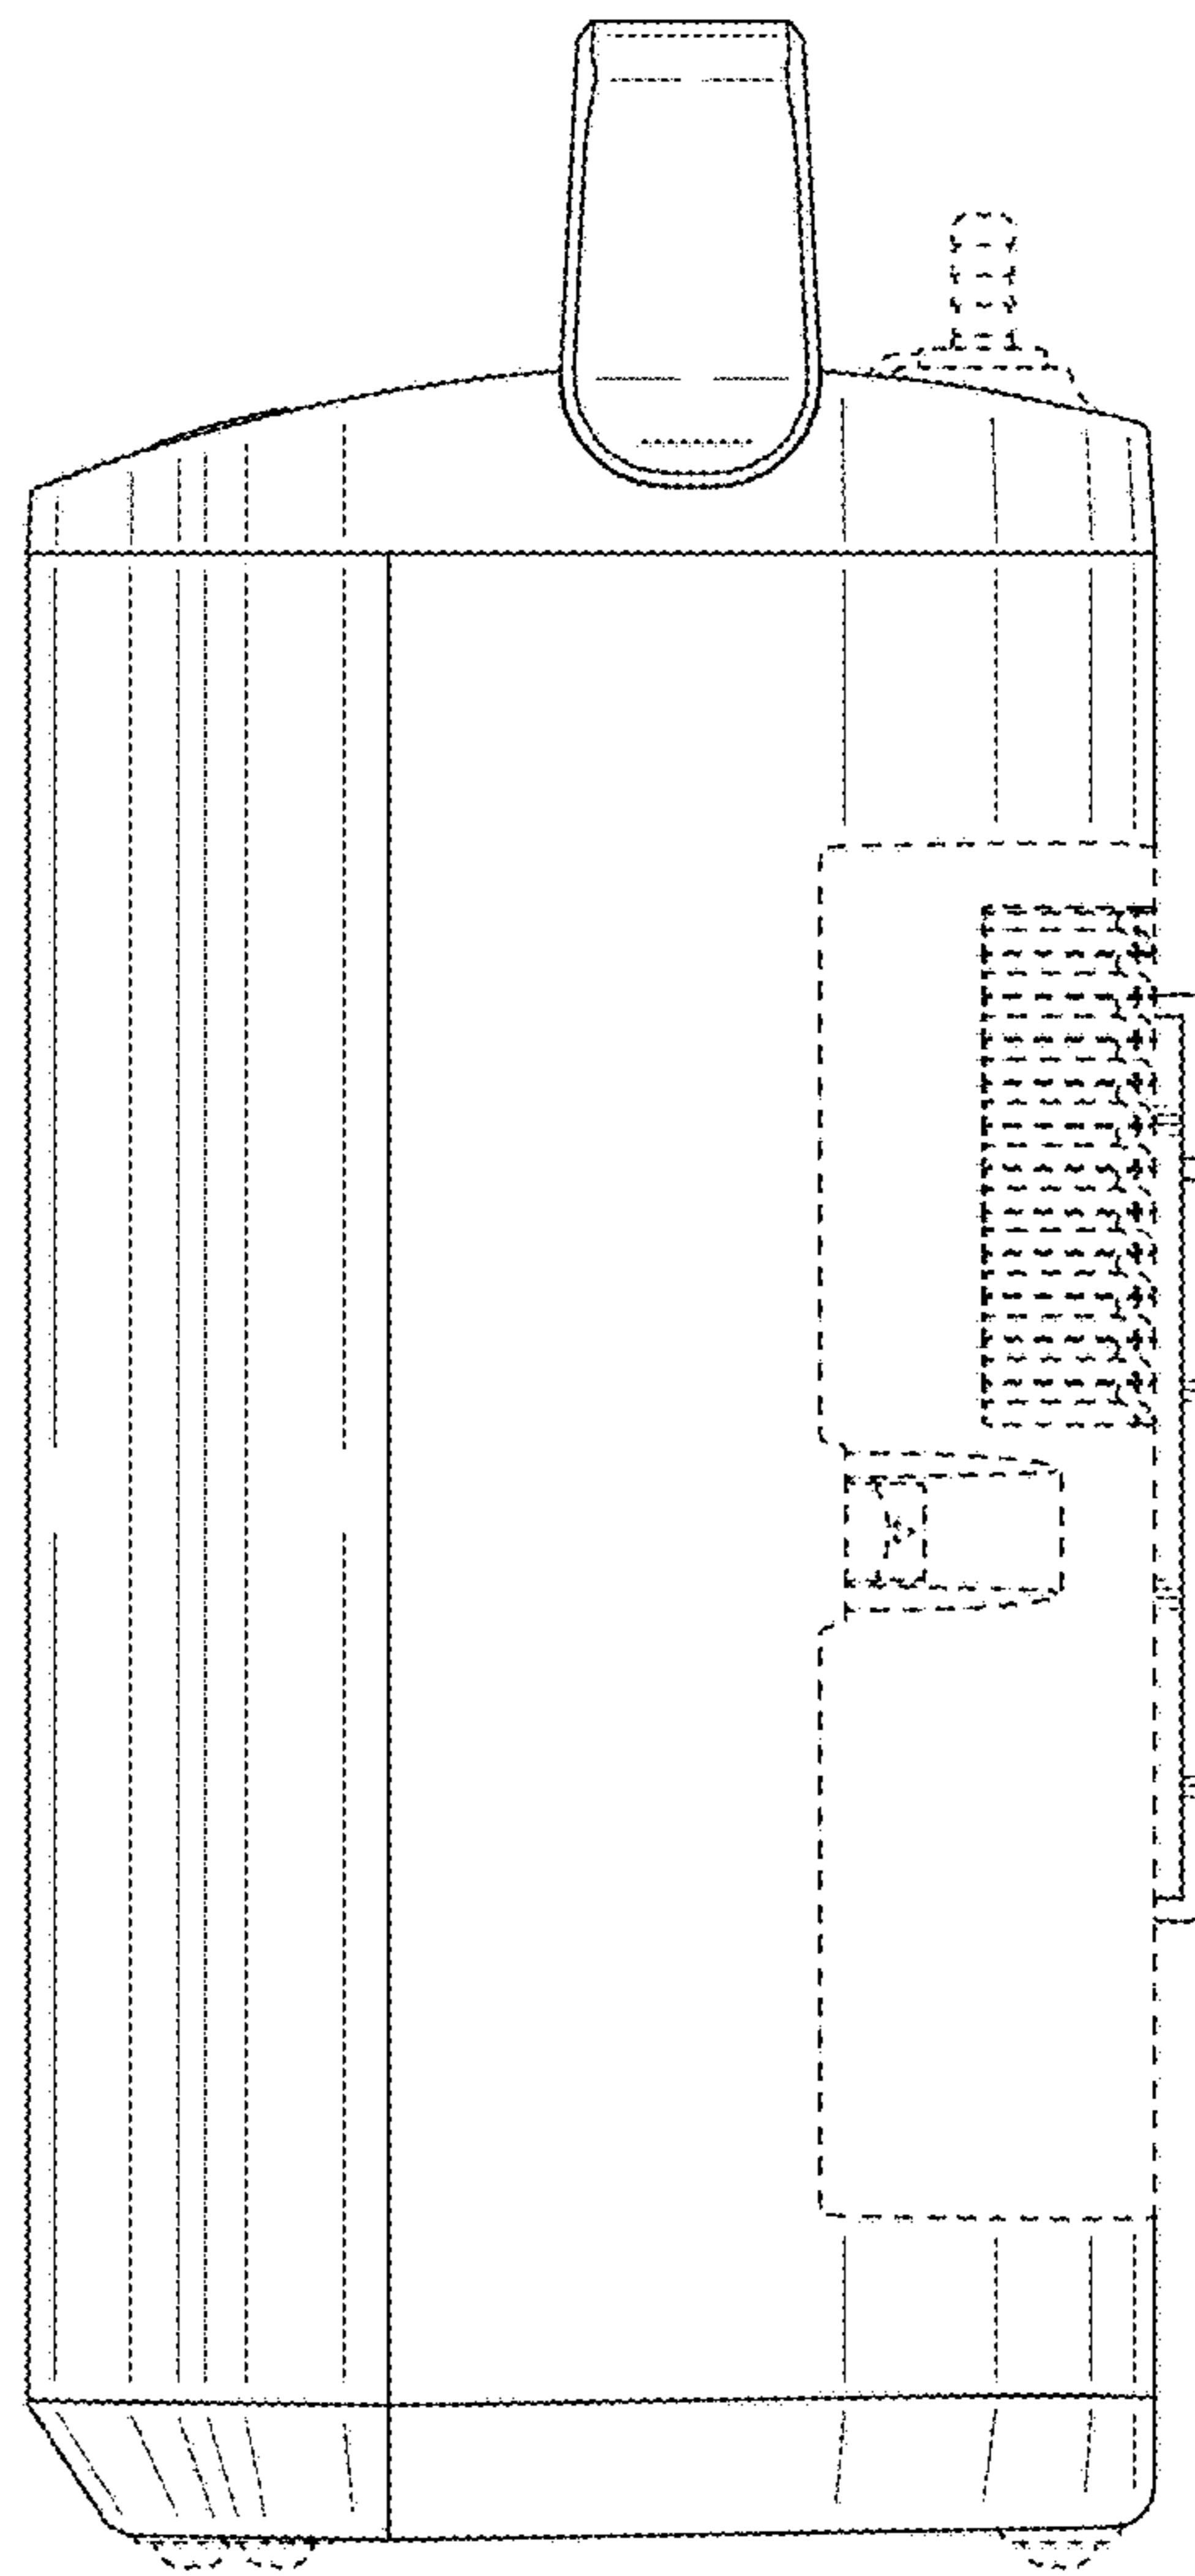


FIG. 5

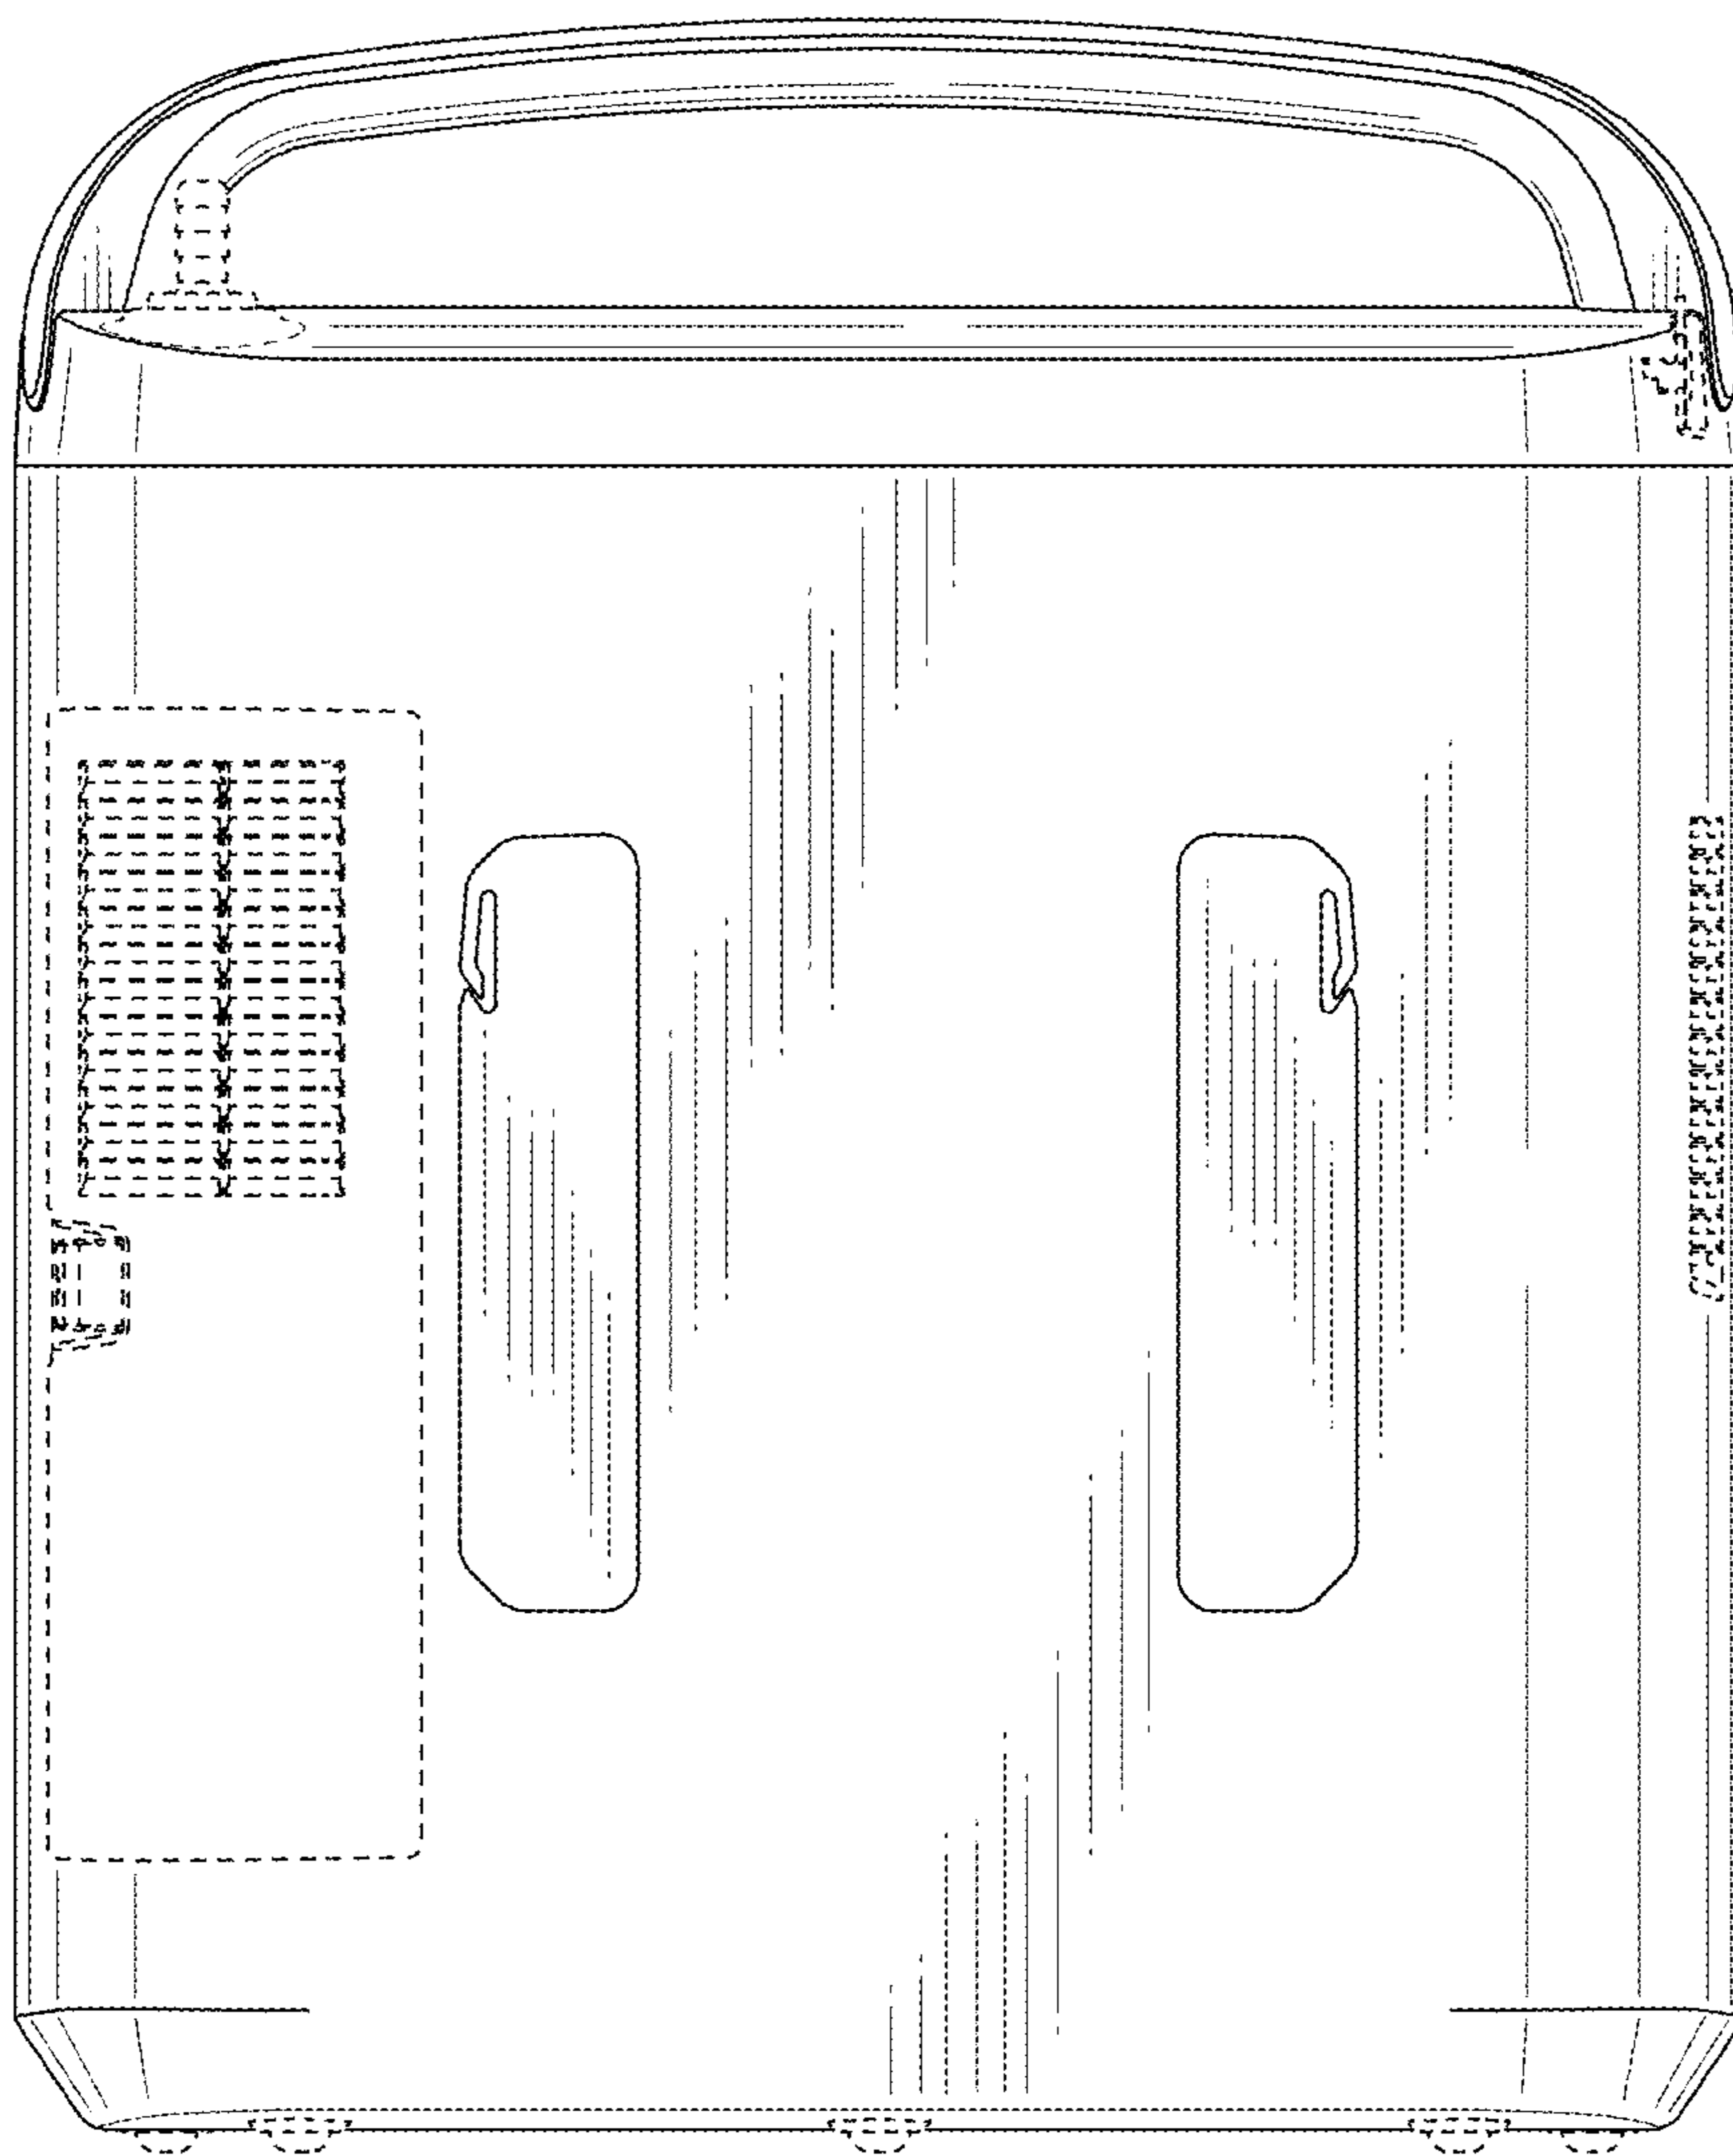


FIG. 6

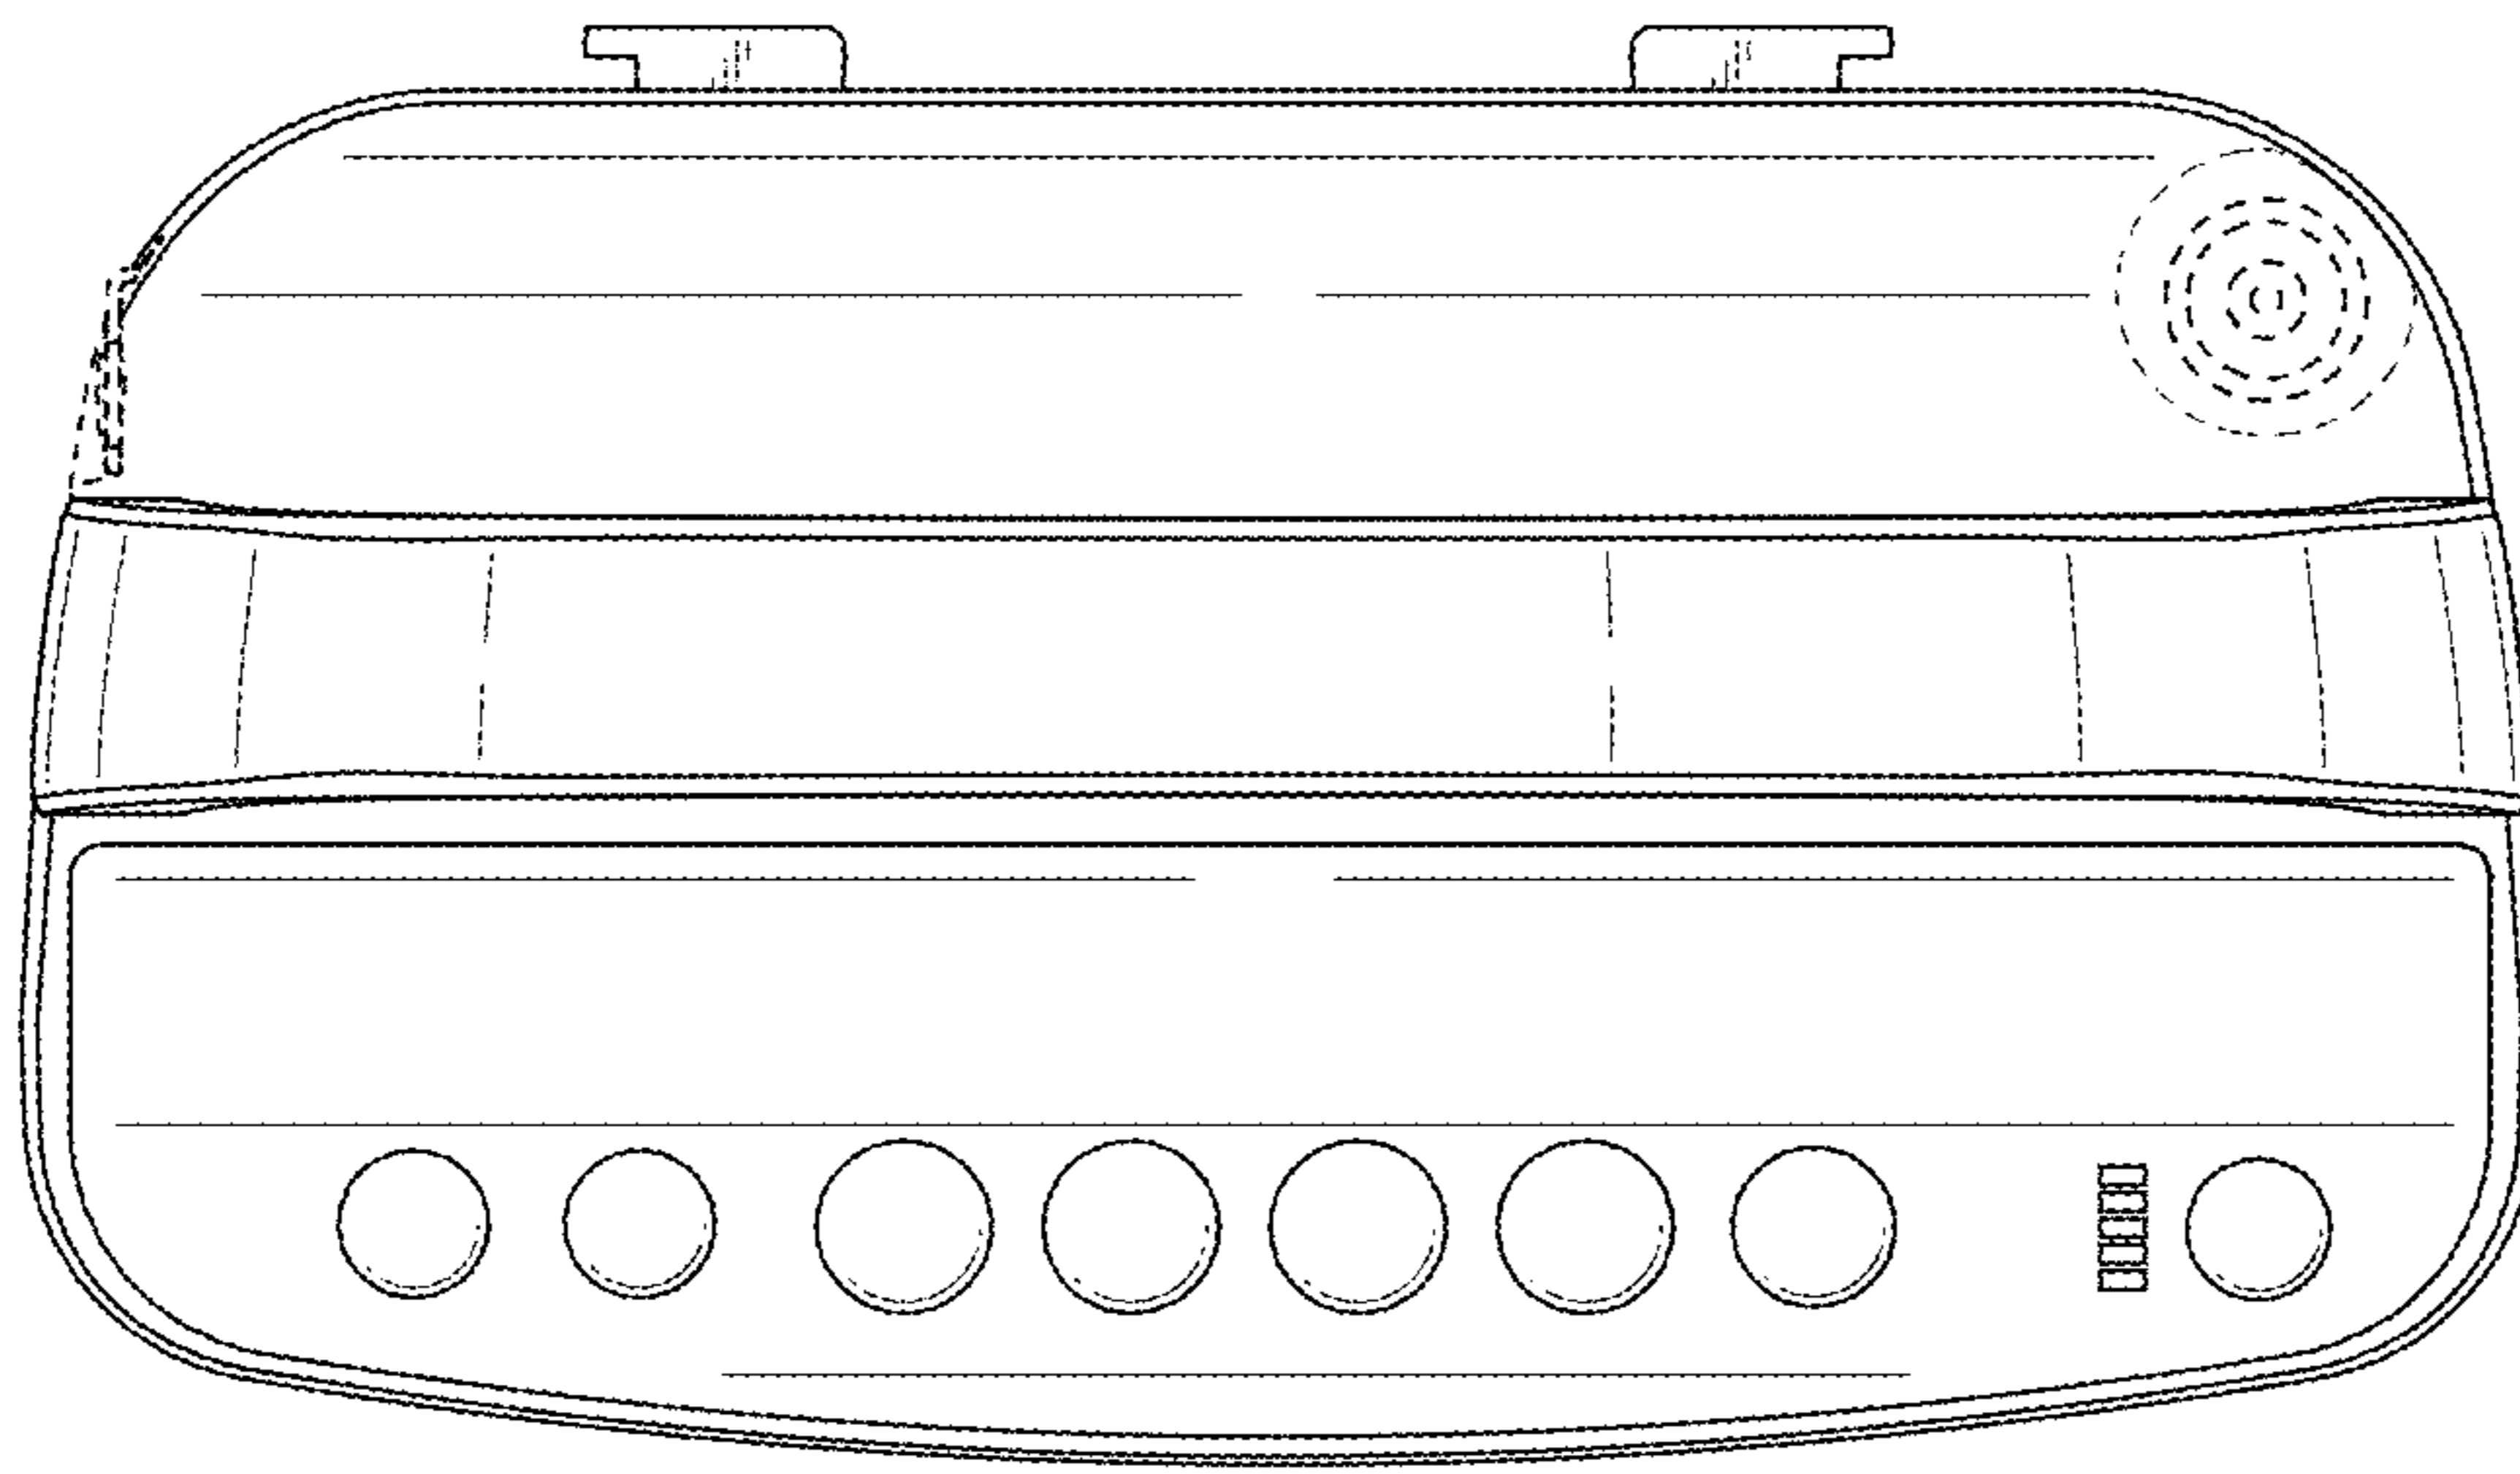


FIG. 7

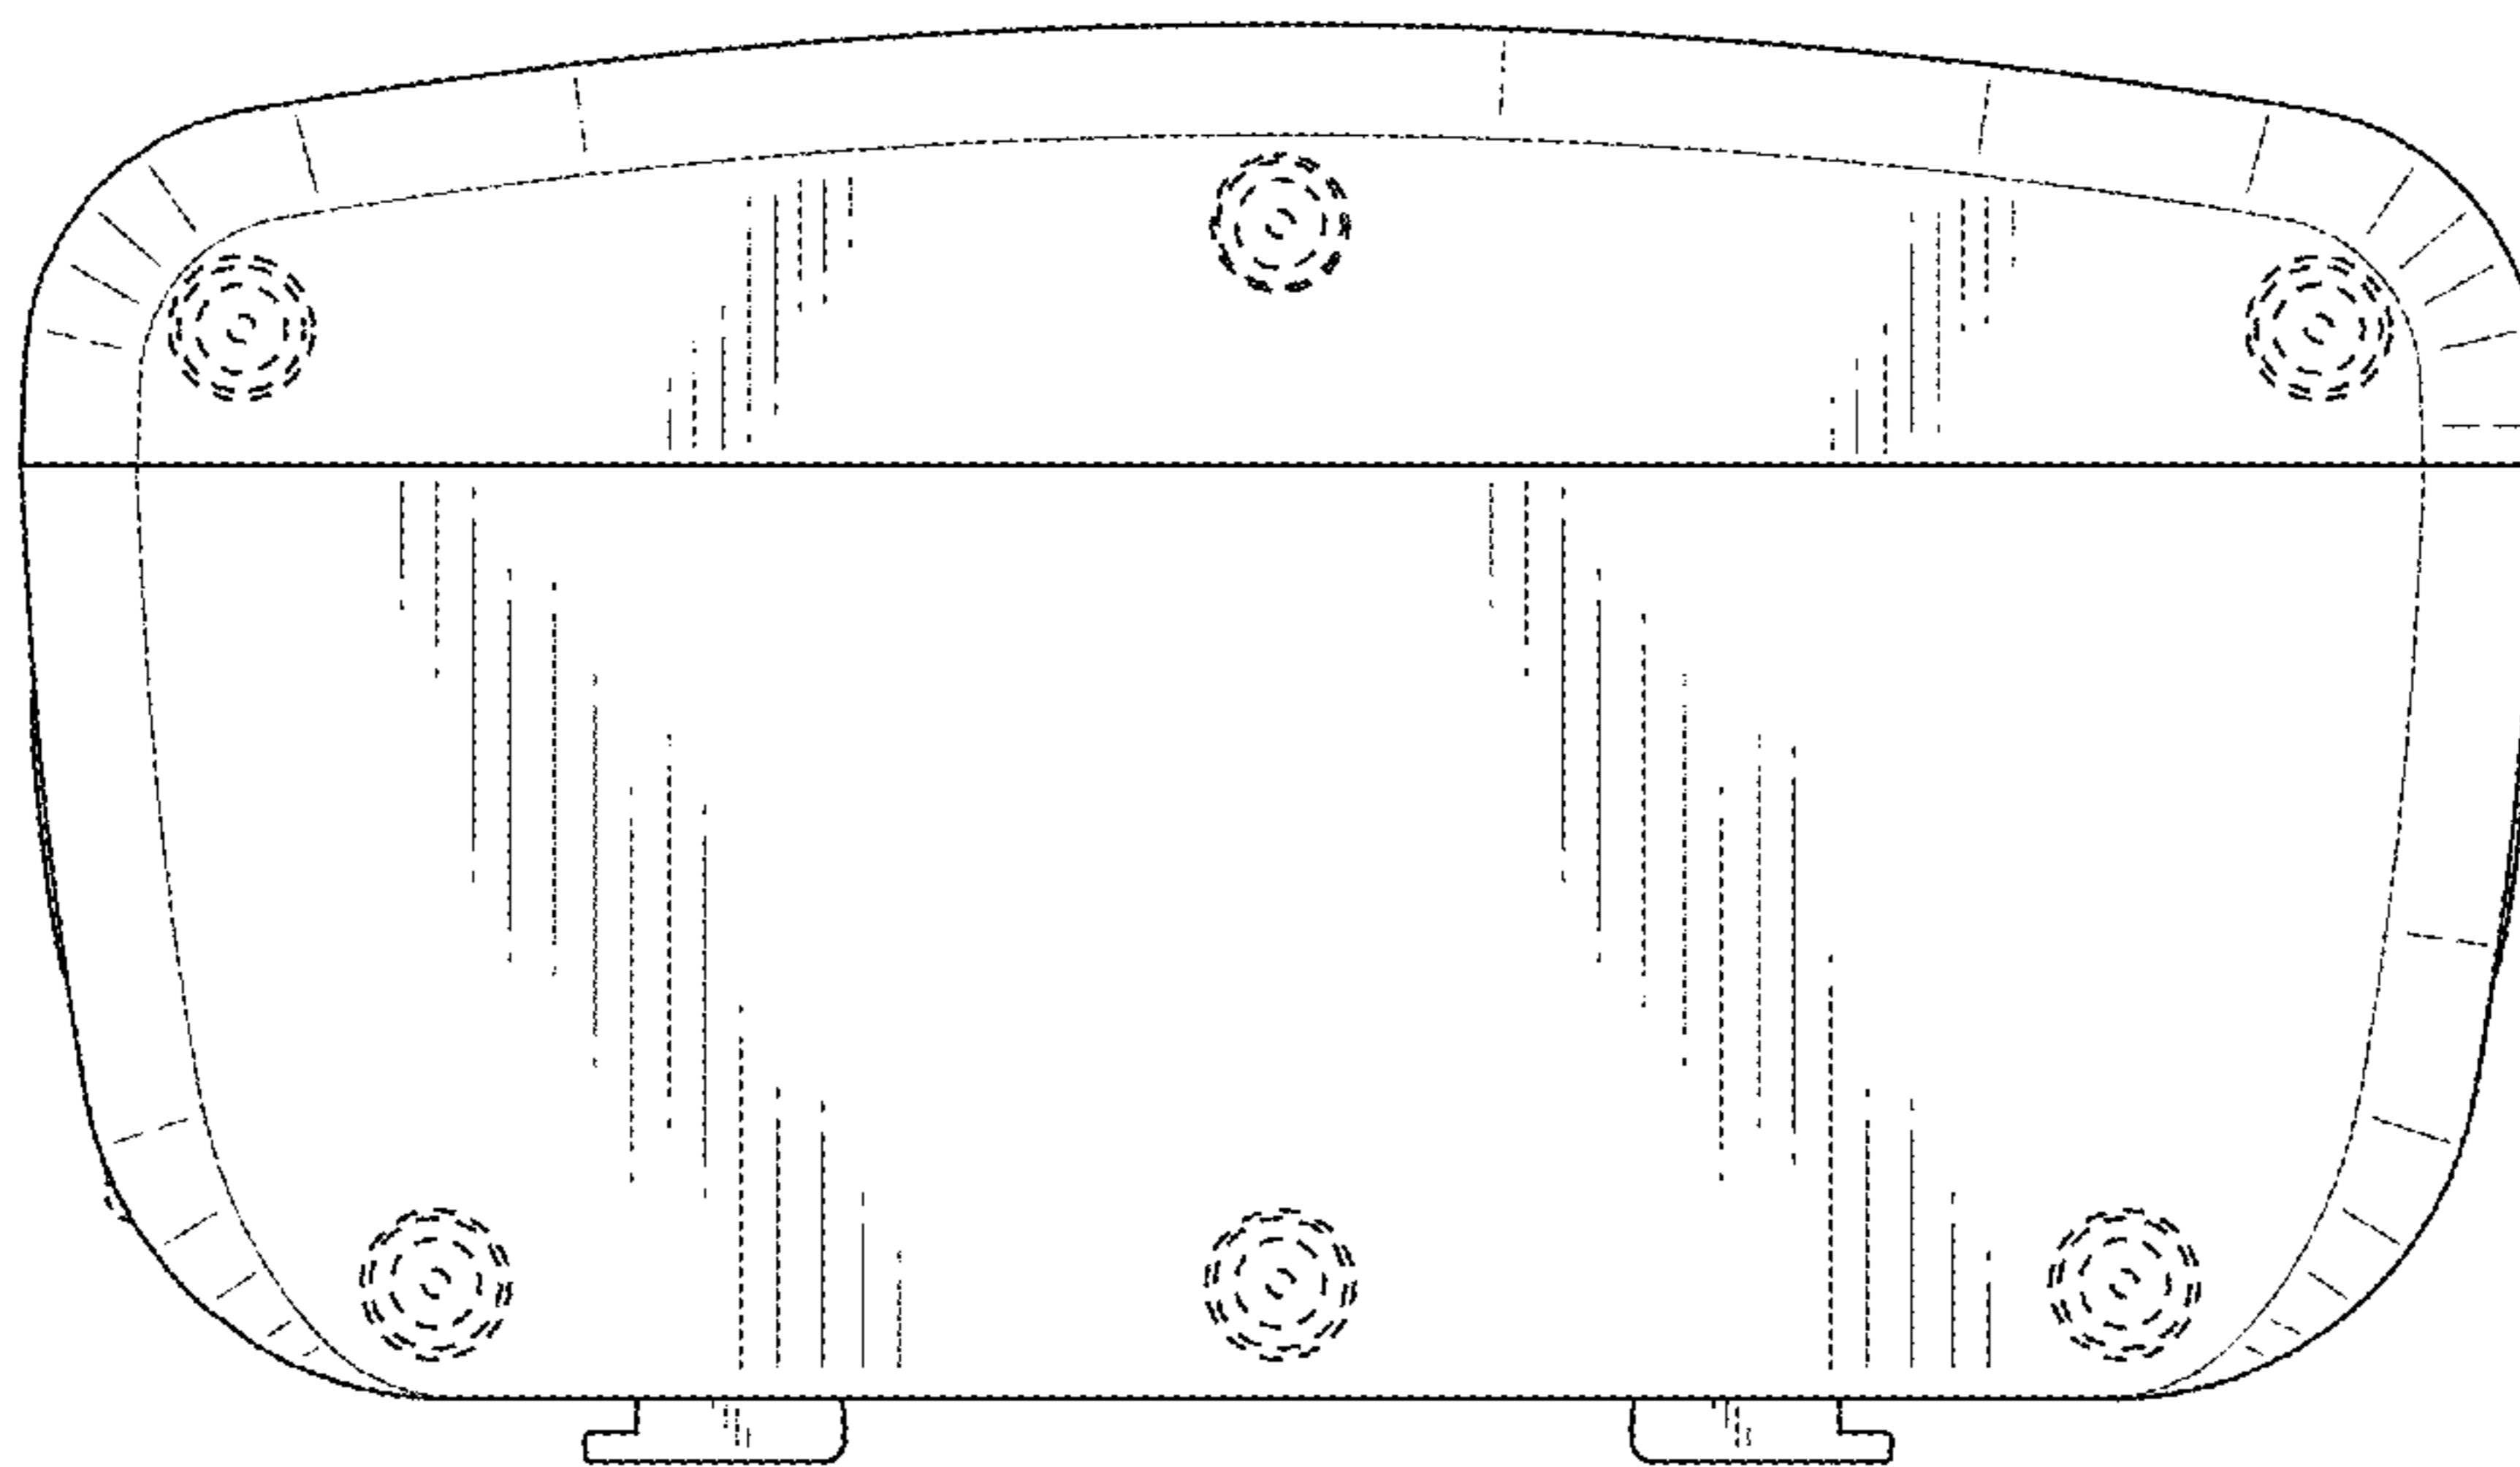


FIG. 8

