



US00D810284S

(12) **United States Design Patent** (10) **Patent No.:** **US D810,284 S**
Frostå (45) **Date of Patent:** **** *Feb. 13, 2018**

- (54) **ADHESIVE RING FOR STOMA**
- (71) Applicant: **Coloplast A/S**, Humlebaek (DK)
- (72) Inventor: **Isak Frostå**, Malmö (SE)
- (73) Assignee: **Coloplast A/S**, Humlebaek (DK)
- (*) Notice: This patent is subject to a terminal disclaimer.
- (**) Term: **15 Years**
- (21) Appl. No.: **29/554,362**
- (22) Filed: **Feb. 11, 2016**
- (51) **LOC (11) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/118**
- (58) **Field of Classification Search**
USPC D24/108, 118, 127, 128, 111; 604/317,
604/327, 408, 403, 108, 339, 92, 415,
604/410, 332, 333; D9/707, 709, 696
CPC A61F 13/00051; A61F 13/02; A61F
13/0226; A61F 13/0246; A61F 13/0259;
A61F 5/445
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS

3,299,442 A	1/1967	White et al.
4,397,641 A	8/1983	Jacobs
4,439,191 A	3/1984	Hogan
4,519,793 A	5/1985	Galindo
4,815,459 A	3/1989	Beran
D303,574 S	9/1989	Steer
4,890,608 A	1/1990	Steer
5,389,081 A	2/1995	Castro
D379,654 S	6/1997	Holtermann
D398,990 S	9/1998	Briggs et al.
D460,550 S	7/2002	Falconer
7,129,389 B1	10/2006	Watson
7,422,578 B2	9/2008	Shan et al.

D607,559 S	1/2010	Schena	
D639,002 S *	5/2011	Dunn	D32/37
D639,003 S *	5/2011	Dunn	D32/37
D639,004 S *	5/2011	Dunn	D32/37
8,197,844 B2	6/2012	Yanaki	

(Continued)

OTHER PUBLICATIONS

Coloplast Brava™ product images, Apr. 2013.

Primary Examiner — Garth Rademaker
Assistant Examiner — Samantha Q. Lawrence
(74) *Attorney, Agent, or Firm* — Coloplast Corp.,
Coloplast A/S; Nick Baumann


(57) **CLAIM**

The ornamental design for an adhesive ring for stoma, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an adhesive ring for stoma; FIG. 2 is a front view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 3 is a back view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 4 is a left side view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 5 is a right side view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 6 is a top plan of the adhesive ring for stoma illustrated in FIG. 1; and, FIG. 7 is a bottom plan view of the adhesive ring for stoma illustrated in FIG. 1. The broken lines shown in FIGS. 1-7 illustrate portions of the adhesive ring for stoma that form no part of the claimed design. The heavy broken lines shown in FIGS. 1-3 illustrate the boundaries of the claimed design and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

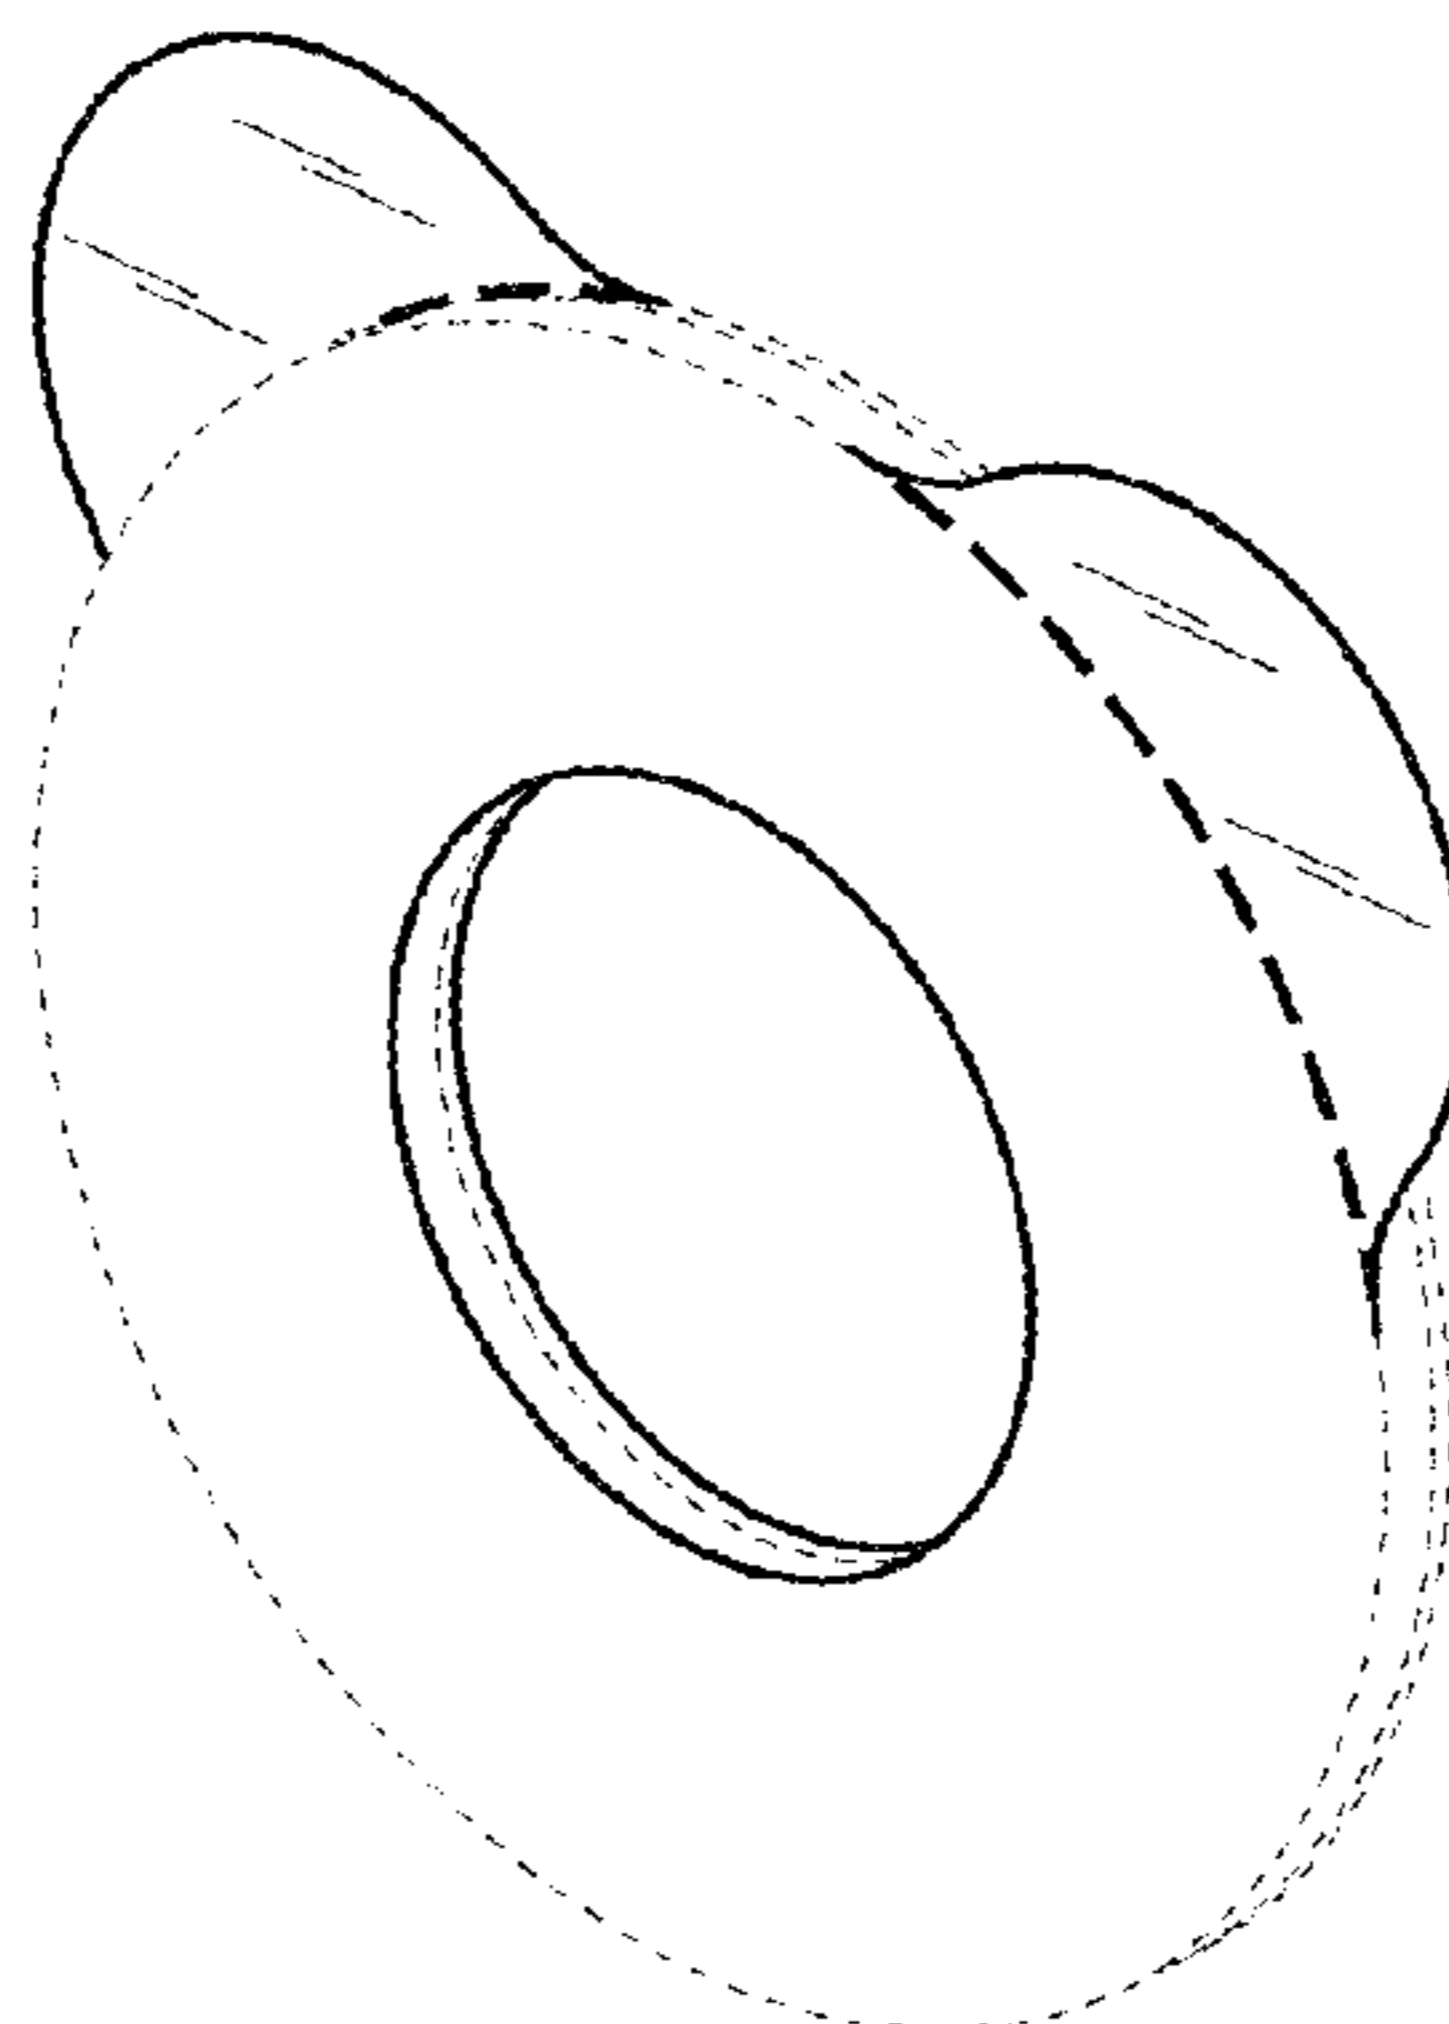

(56)

References Cited

U.S. PATENT DOCUMENTS

8,328,779 B2 * 12/2012 Fenton A61F 5/443
604/332
8,377,020 B1 2/2013 Berven
8,419,767 B2 4/2013 Al-Qbandi et al.
D750,770 S 3/2016 Green
D754,332 S 4/2016 Fahl
D754,848 S 4/2016 Masters et al.
D764,136 S * 8/2016 Stravitz D34/10
9,463,298 B2 * 10/2016 Persson A61M 16/047

* cited by examiner

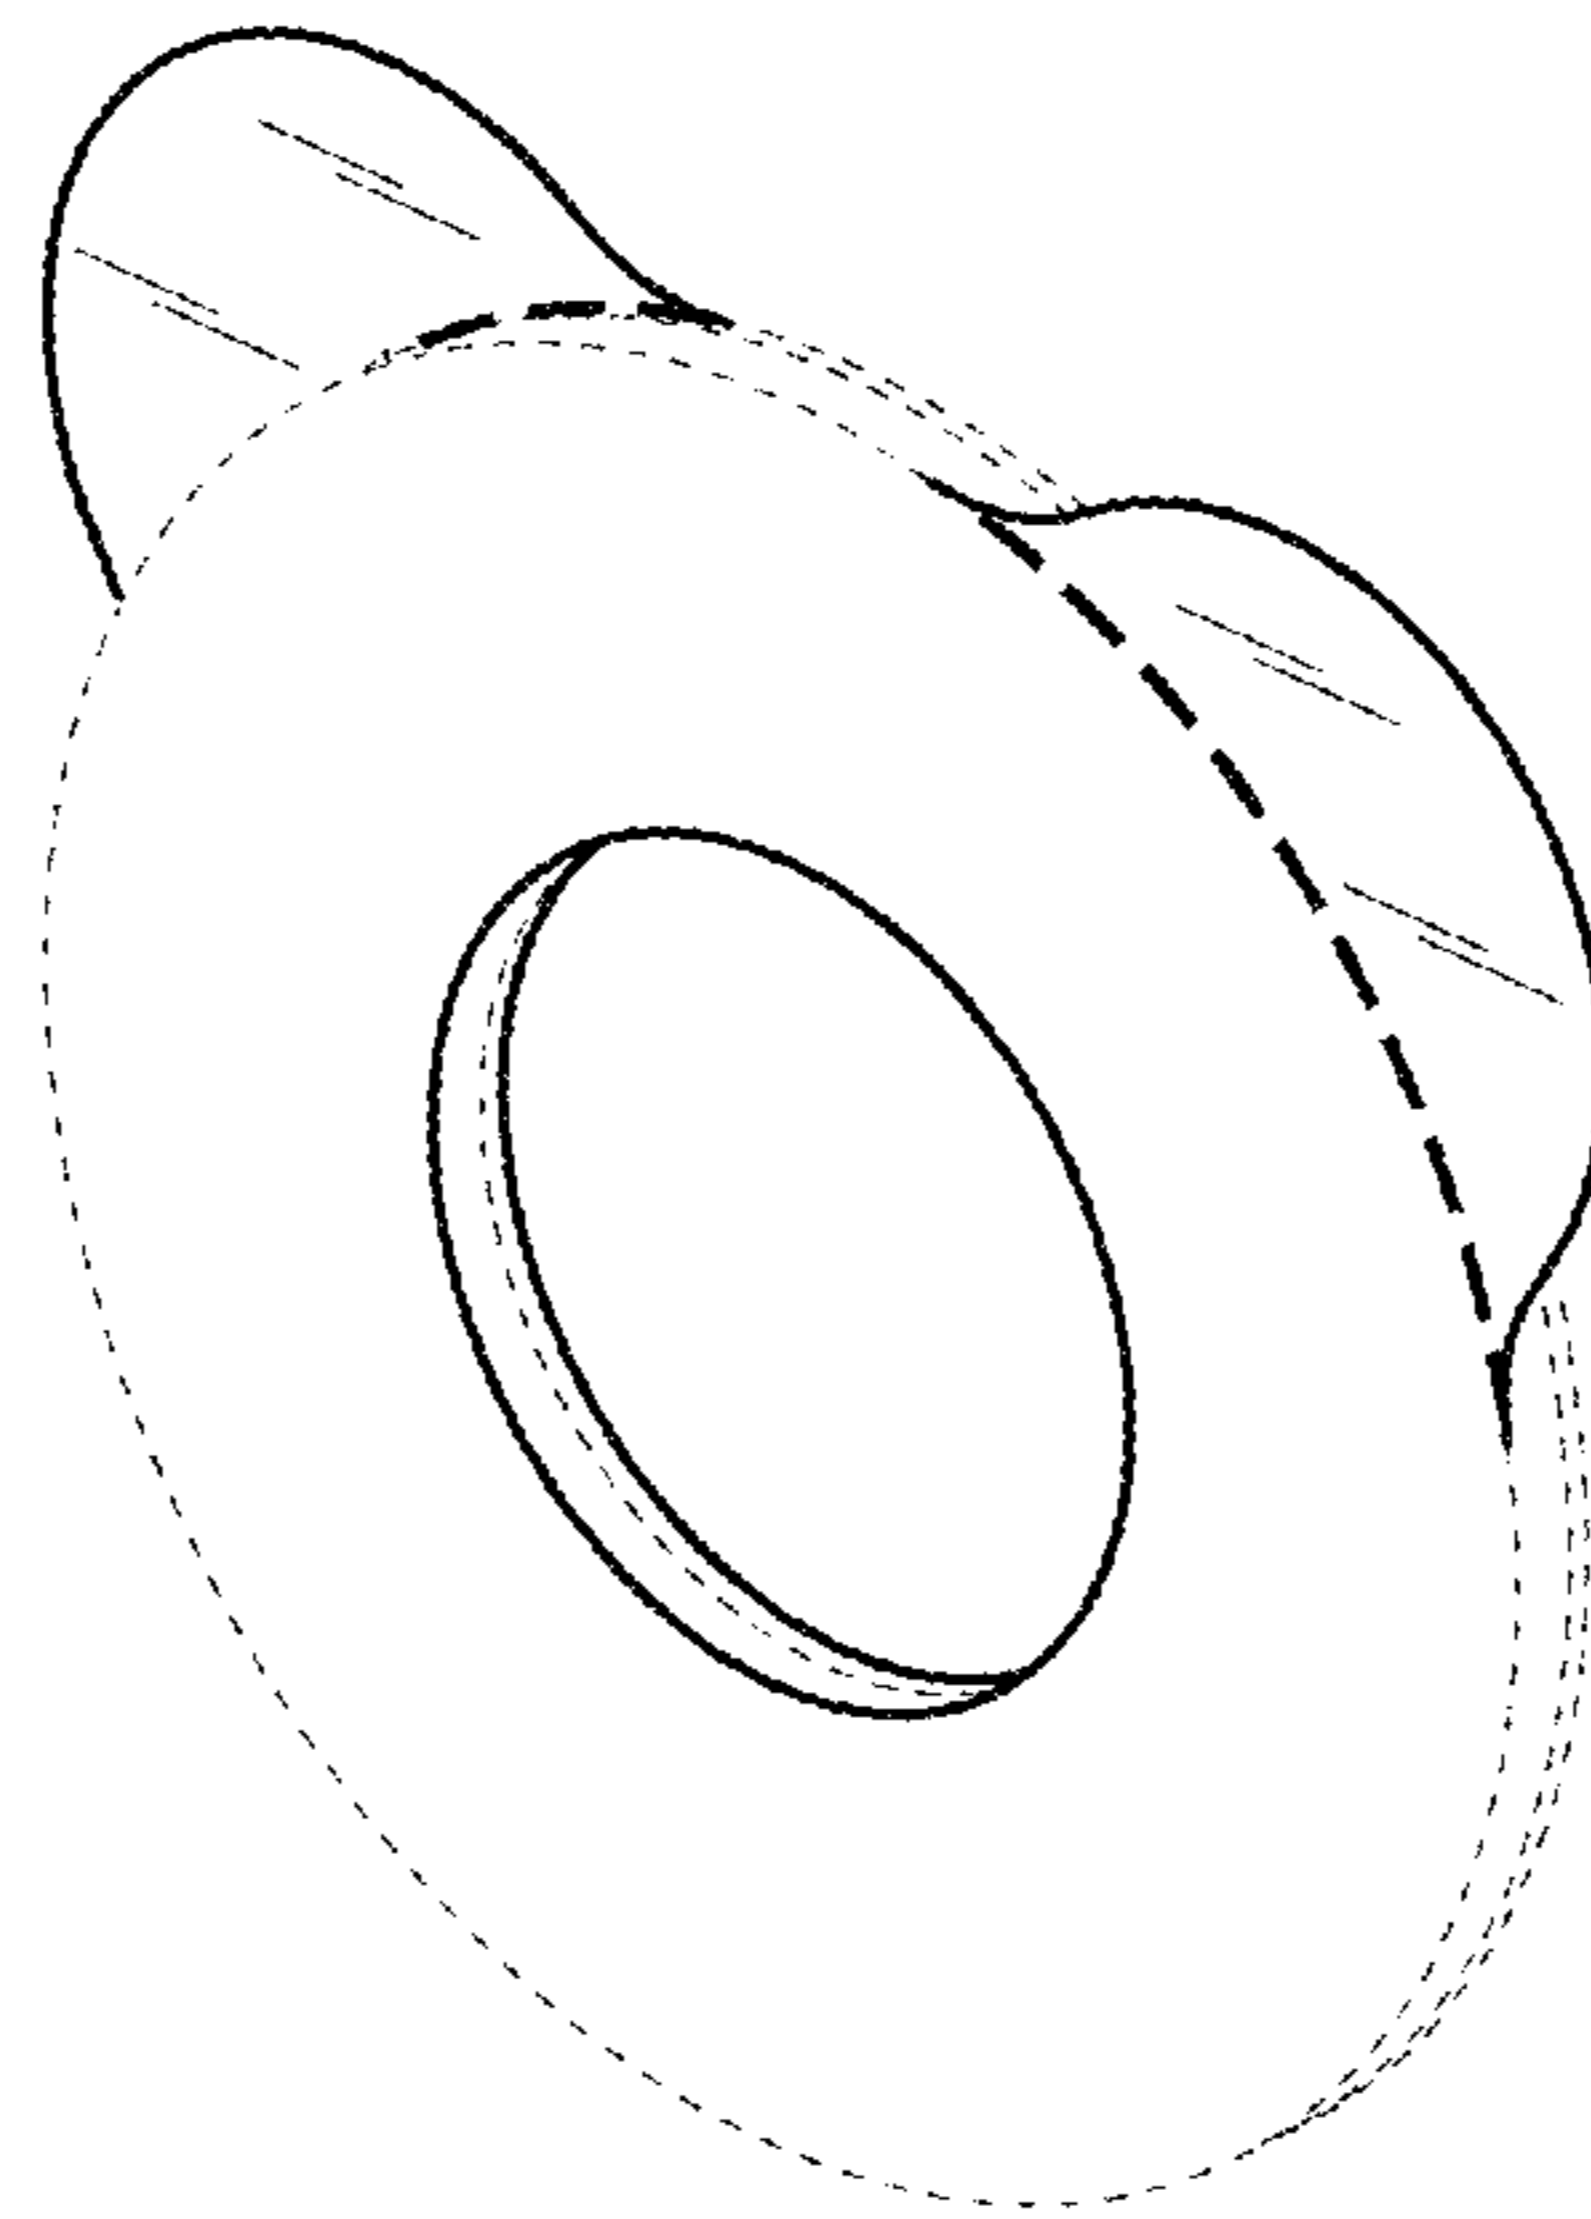


Fig. 1

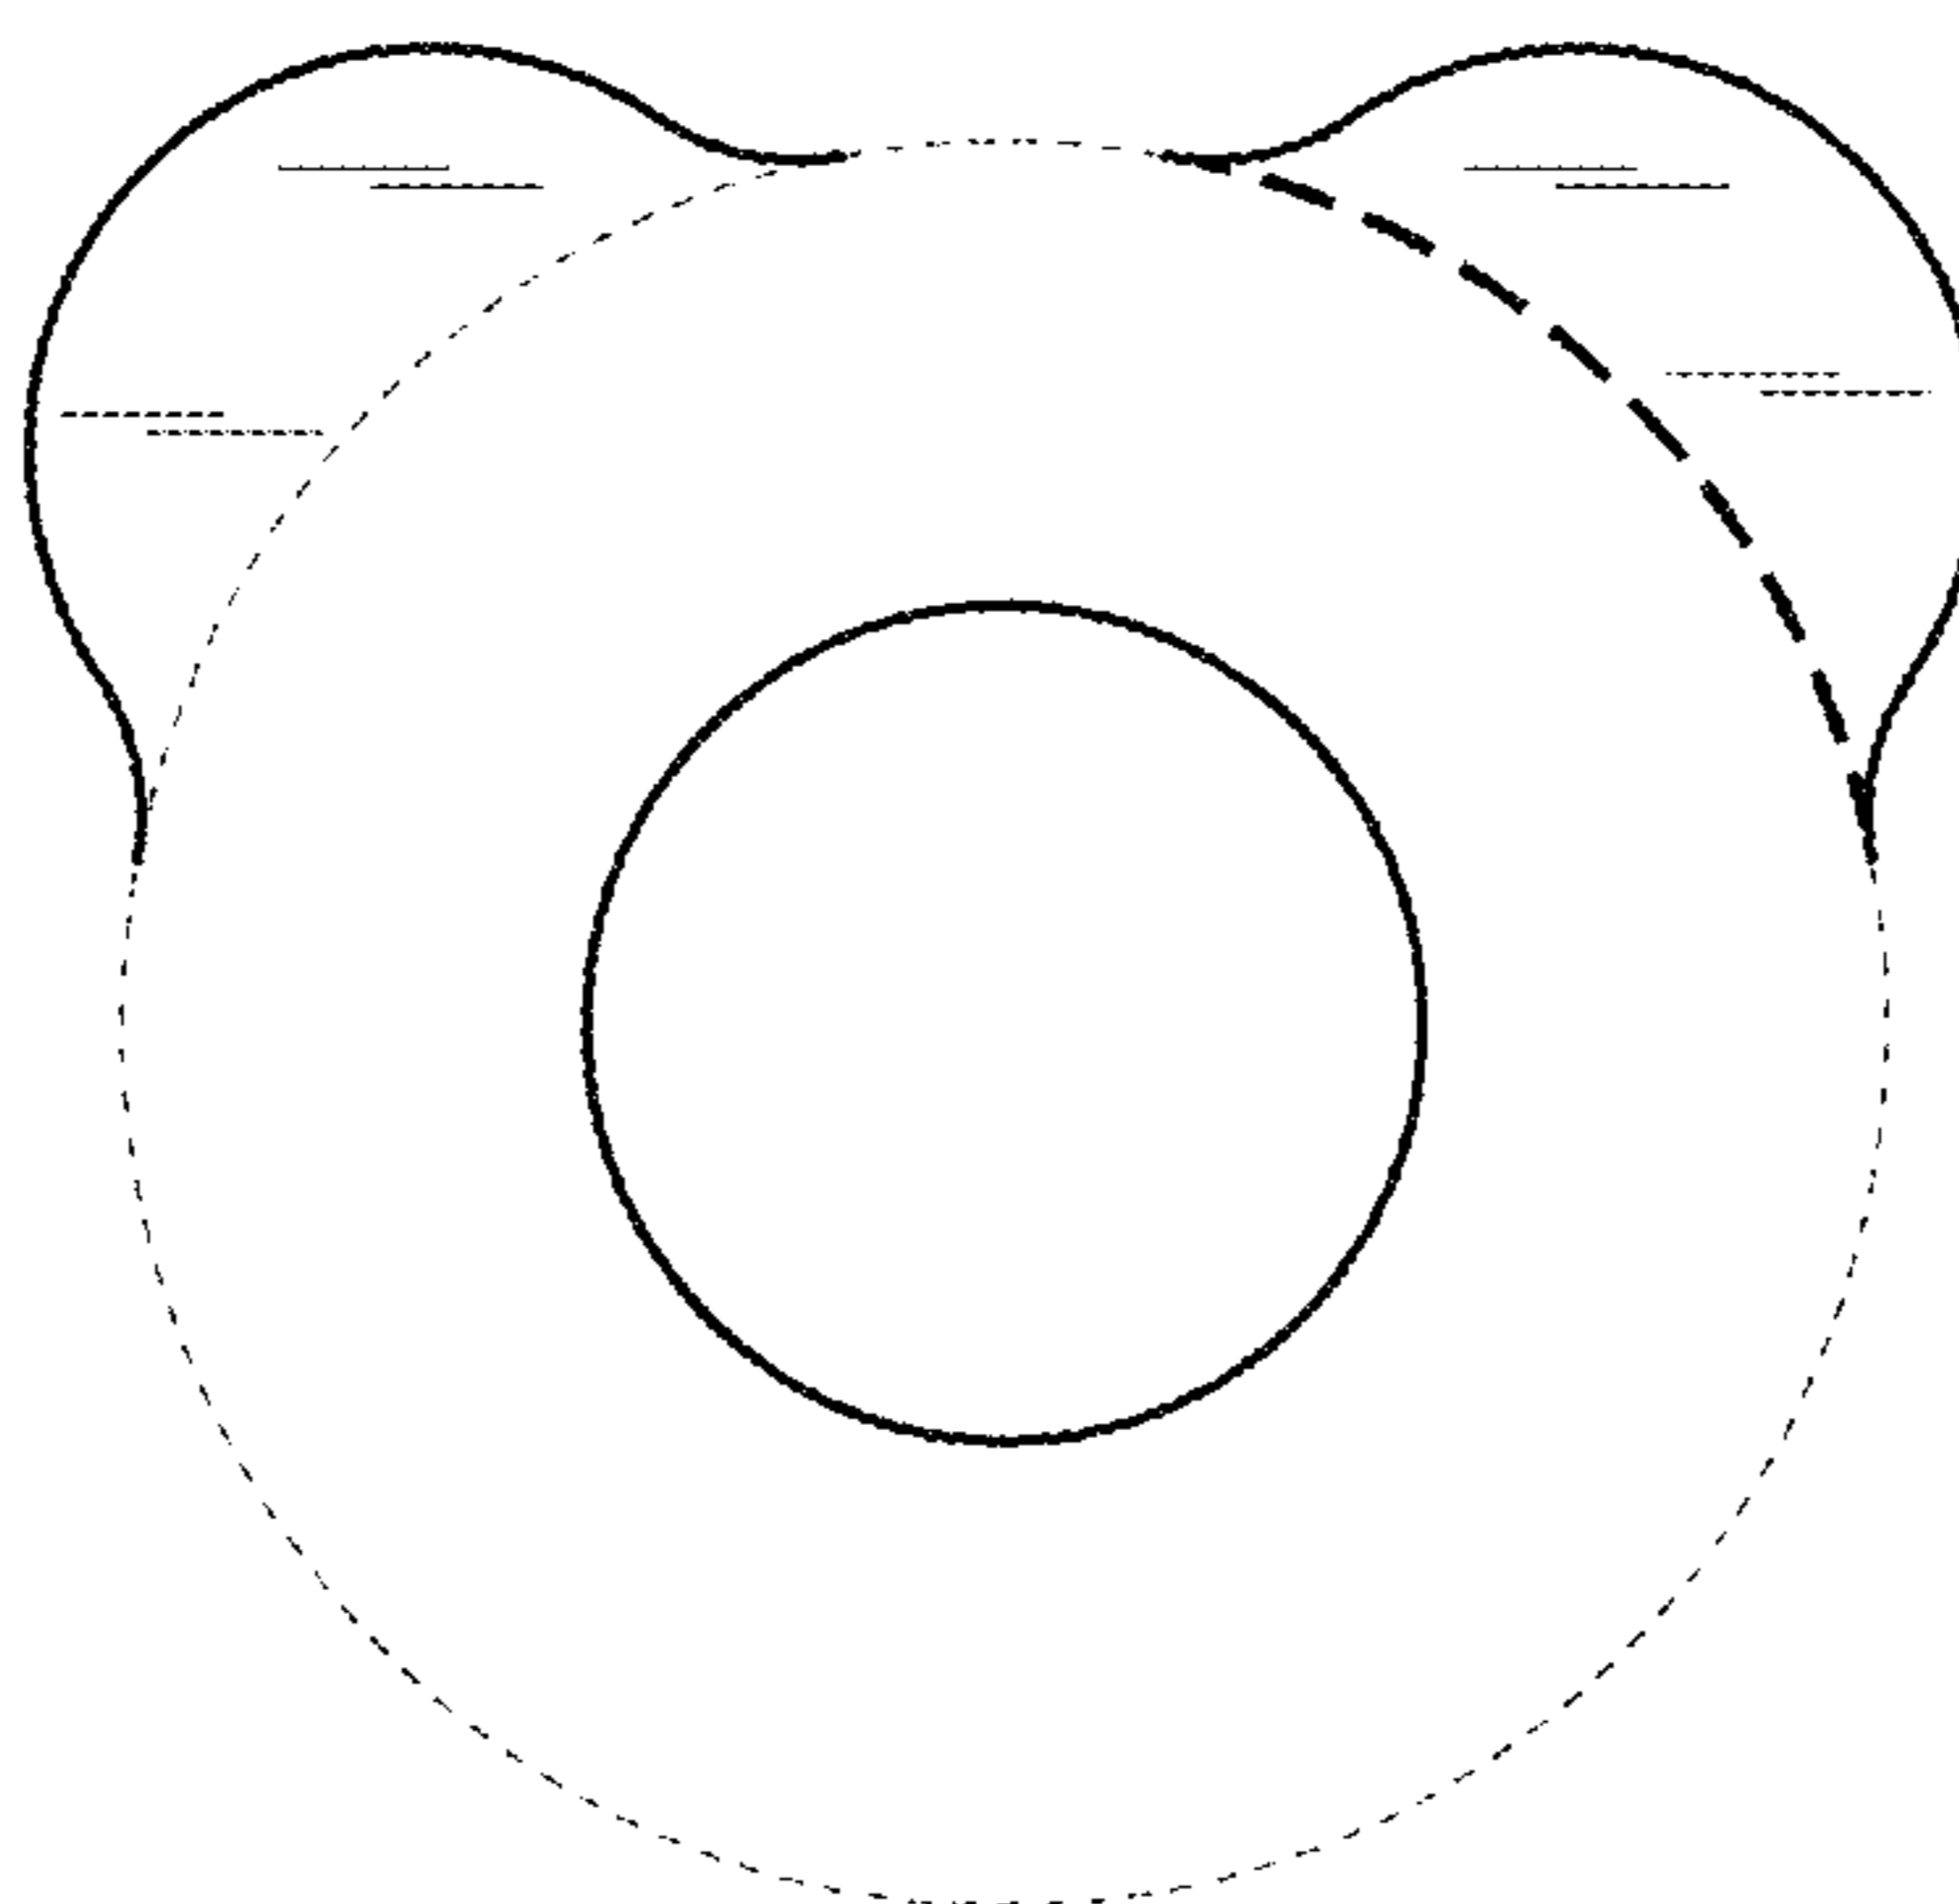


Fig. 2

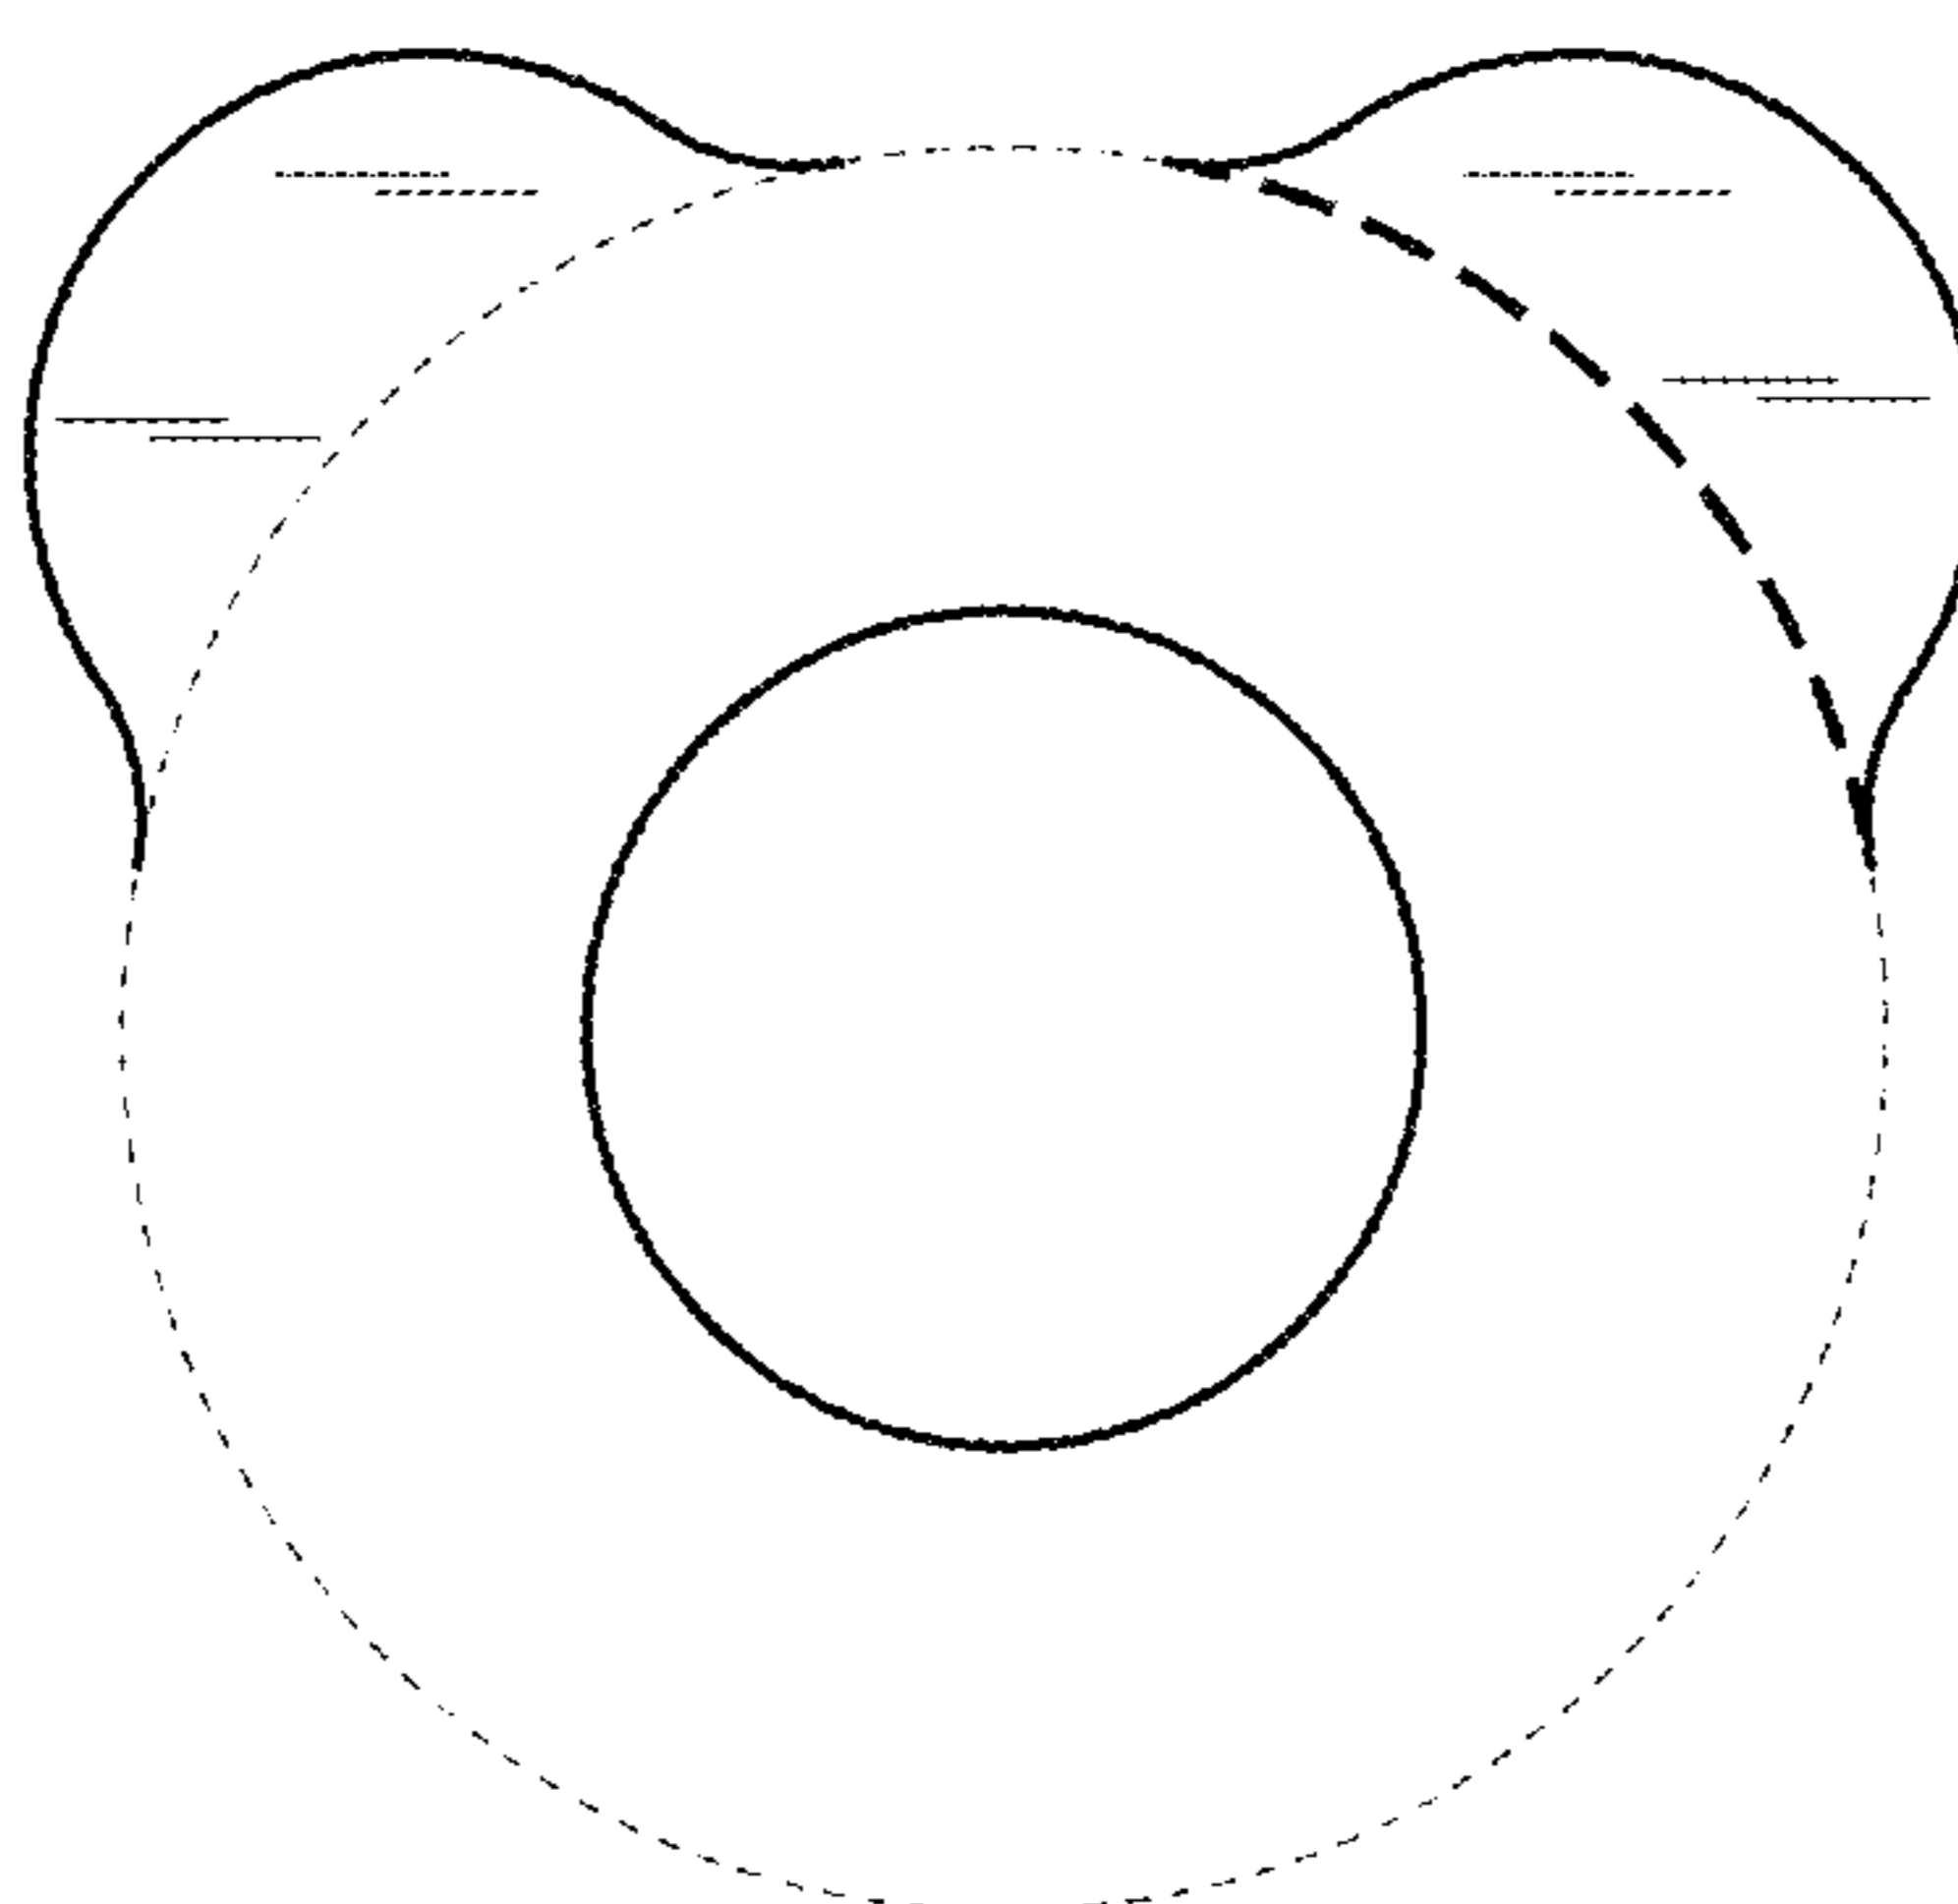


Fig. 3

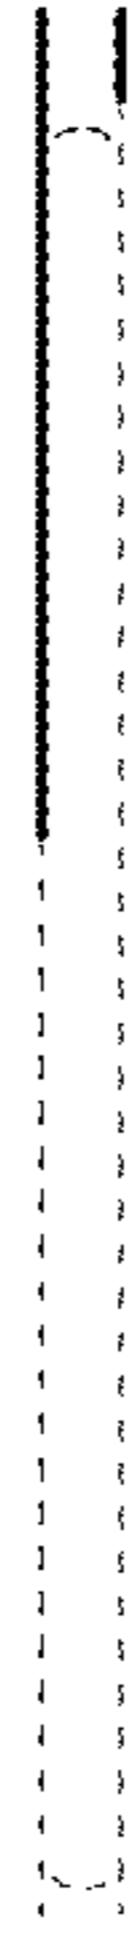


Fig. 4

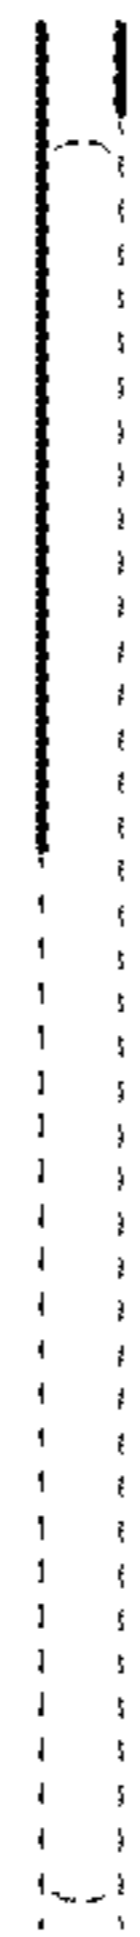


Fig. 5

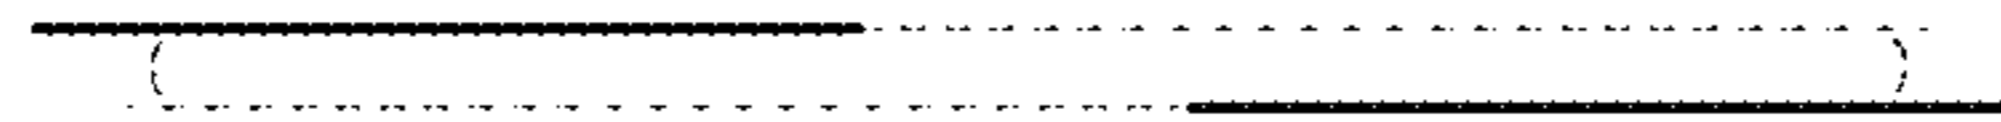


Fig. 6

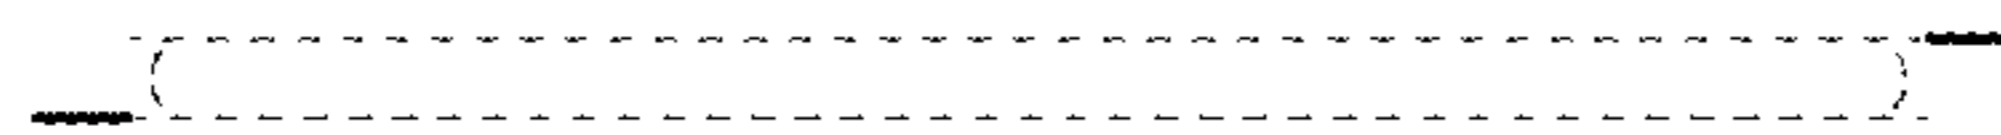


Fig. 7