



US00D810929S

(12) **United States Design Patent** (10) **Patent No.:** **US D810,929 S**
Frostå (45) **Date of Patent:** **** *Feb. 20, 2018**

(54) **ADHESIVE RING FOR STOMA**
(71) Applicant: **Coloplast A/S**, Humlebaek (DK)
(72) Inventor: **Isak Frostå**, Malmö (SE)
(73) Assignee: **Coloplast A/S**, Humlebaek (DK)
(*) Notice: This patent is subject to a terminal disclaimer.
(**) Term: **15 Years**
(21) Appl. No.: **29/554,364**
(22) Filed: **Feb. 11, 2016**
(51) **LOC (11) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/118**
(58) **Field of Classification Search**
USPC D24/108, 118, 127, 128, 111; 604/317,
604/327, 408, 403, 108, 339, 92, 415,
604/410, 332, 333; D9/707, 709, 696
CPC A61F 13/00051; A61F 13/02; A61F
13/0226; A61F 13/0246; A61F 13/0259;
A61F 5/445
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
3,299,442 A 1/1967 White et al.
4,397,641 A 8/1983 Jacobs
4,439,191 A 3/1984 Hogan
4,519,793 A 5/1985 Galindo
4,815,459 A 3/1989 Beran
D303,574 S 9/1989 Steer
4,890,608 A 1/1990 Steer
5,389,081 A 2/1995 Castro
D379,654 S 6/1997 Holtermann
D398,990 S 9/1998 Briggs et al.
D460,550 S 7/2002 Falconer
7,129,389 B1 10/2006 Watson
7,422,578 B2 9/2008 Shan et al.


D607,559 S 1/2010 Schena
D639,002 S * 5/2011 Dunn D32/37
D639,003 S * 5/2011 Dunn D32/37
D639,004 S * 5/2011 Dunn D32/37
8,197,844 B2 6/2012 Yanaki
(Continued)

OTHER PUBLICATIONS
Coloplast Brava™ product images, Apr. 2013.
Primary Examiner — Garth Rademaker
Assistant Examiner — Samantha Q. Lawrence
(74) *Attorney, Agent, or Firm* — Coloplast Corp.,
Coloplast A/S; Nick Baumann

(57) **CLAIM**
The ornamental design for an adhesive ring for stoma, as shown and described.

DESCRIPTION
FIG. 1 is a perspective view of an adhesive ring for stoma; FIG. 2 is a front view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 3 is a back view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 4 is a left side view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 5 is a right side view of the adhesive ring for stoma illustrated in FIG. 1; FIG. 6 is a top plan view of the adhesive ring for stoma illustrated in FIG. 1; and, FIG. 7 is a bottom plan view of the adhesive ring for stoma illustrated in FIG. 1.
The broken lines shown in FIGS. 1-7 illustrate portions of the adhesive ring for stoma that form no part of the claimed design. The heavy broken lines shown in FIGS. 1-3 illustrate boundaries of the claimed design and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

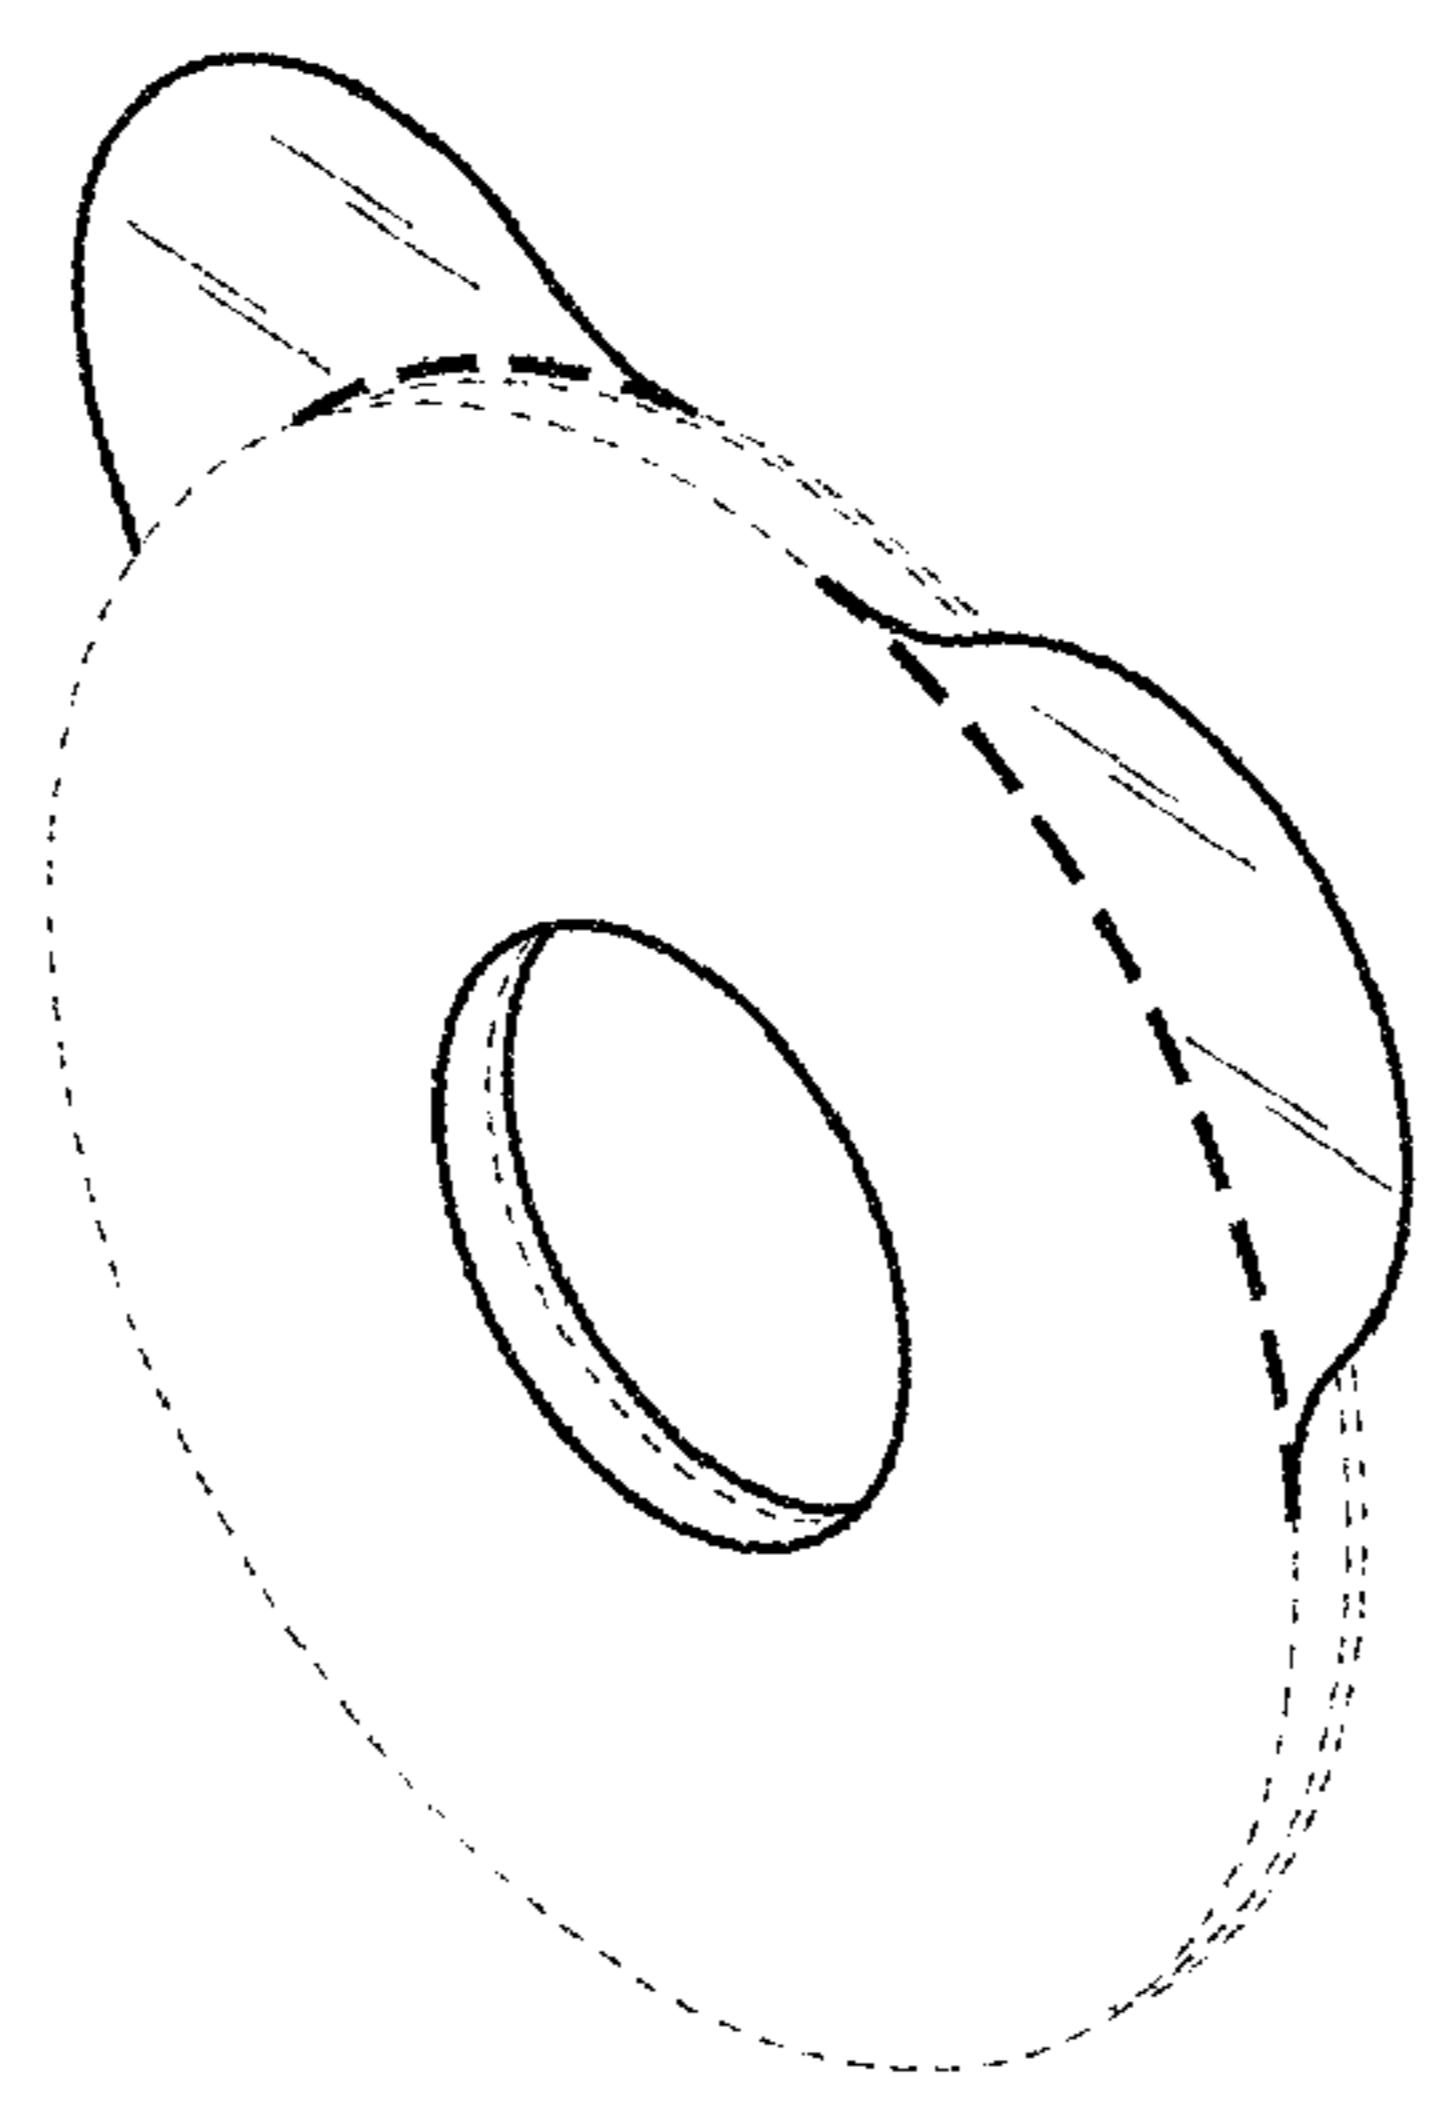

(56)

References Cited

U.S. PATENT DOCUMENTS

8,328,779 B2 * 12/2012 Fenton A61F 5/443
604/332
8,377,020 B1 2/2013 Berven
8,419,767 B2 4/2013 Al-Qbandi et al.
D750,770 S 3/2016 Green
D754,332 S 4/2016 Fahl
D754,848 S 4/2016 Masters et al.
D764,136 S * 8/2016 Stravitz D34/10
9,463,298 B2 * 10/2016 Persson A61M 16/047

* cited by examiner

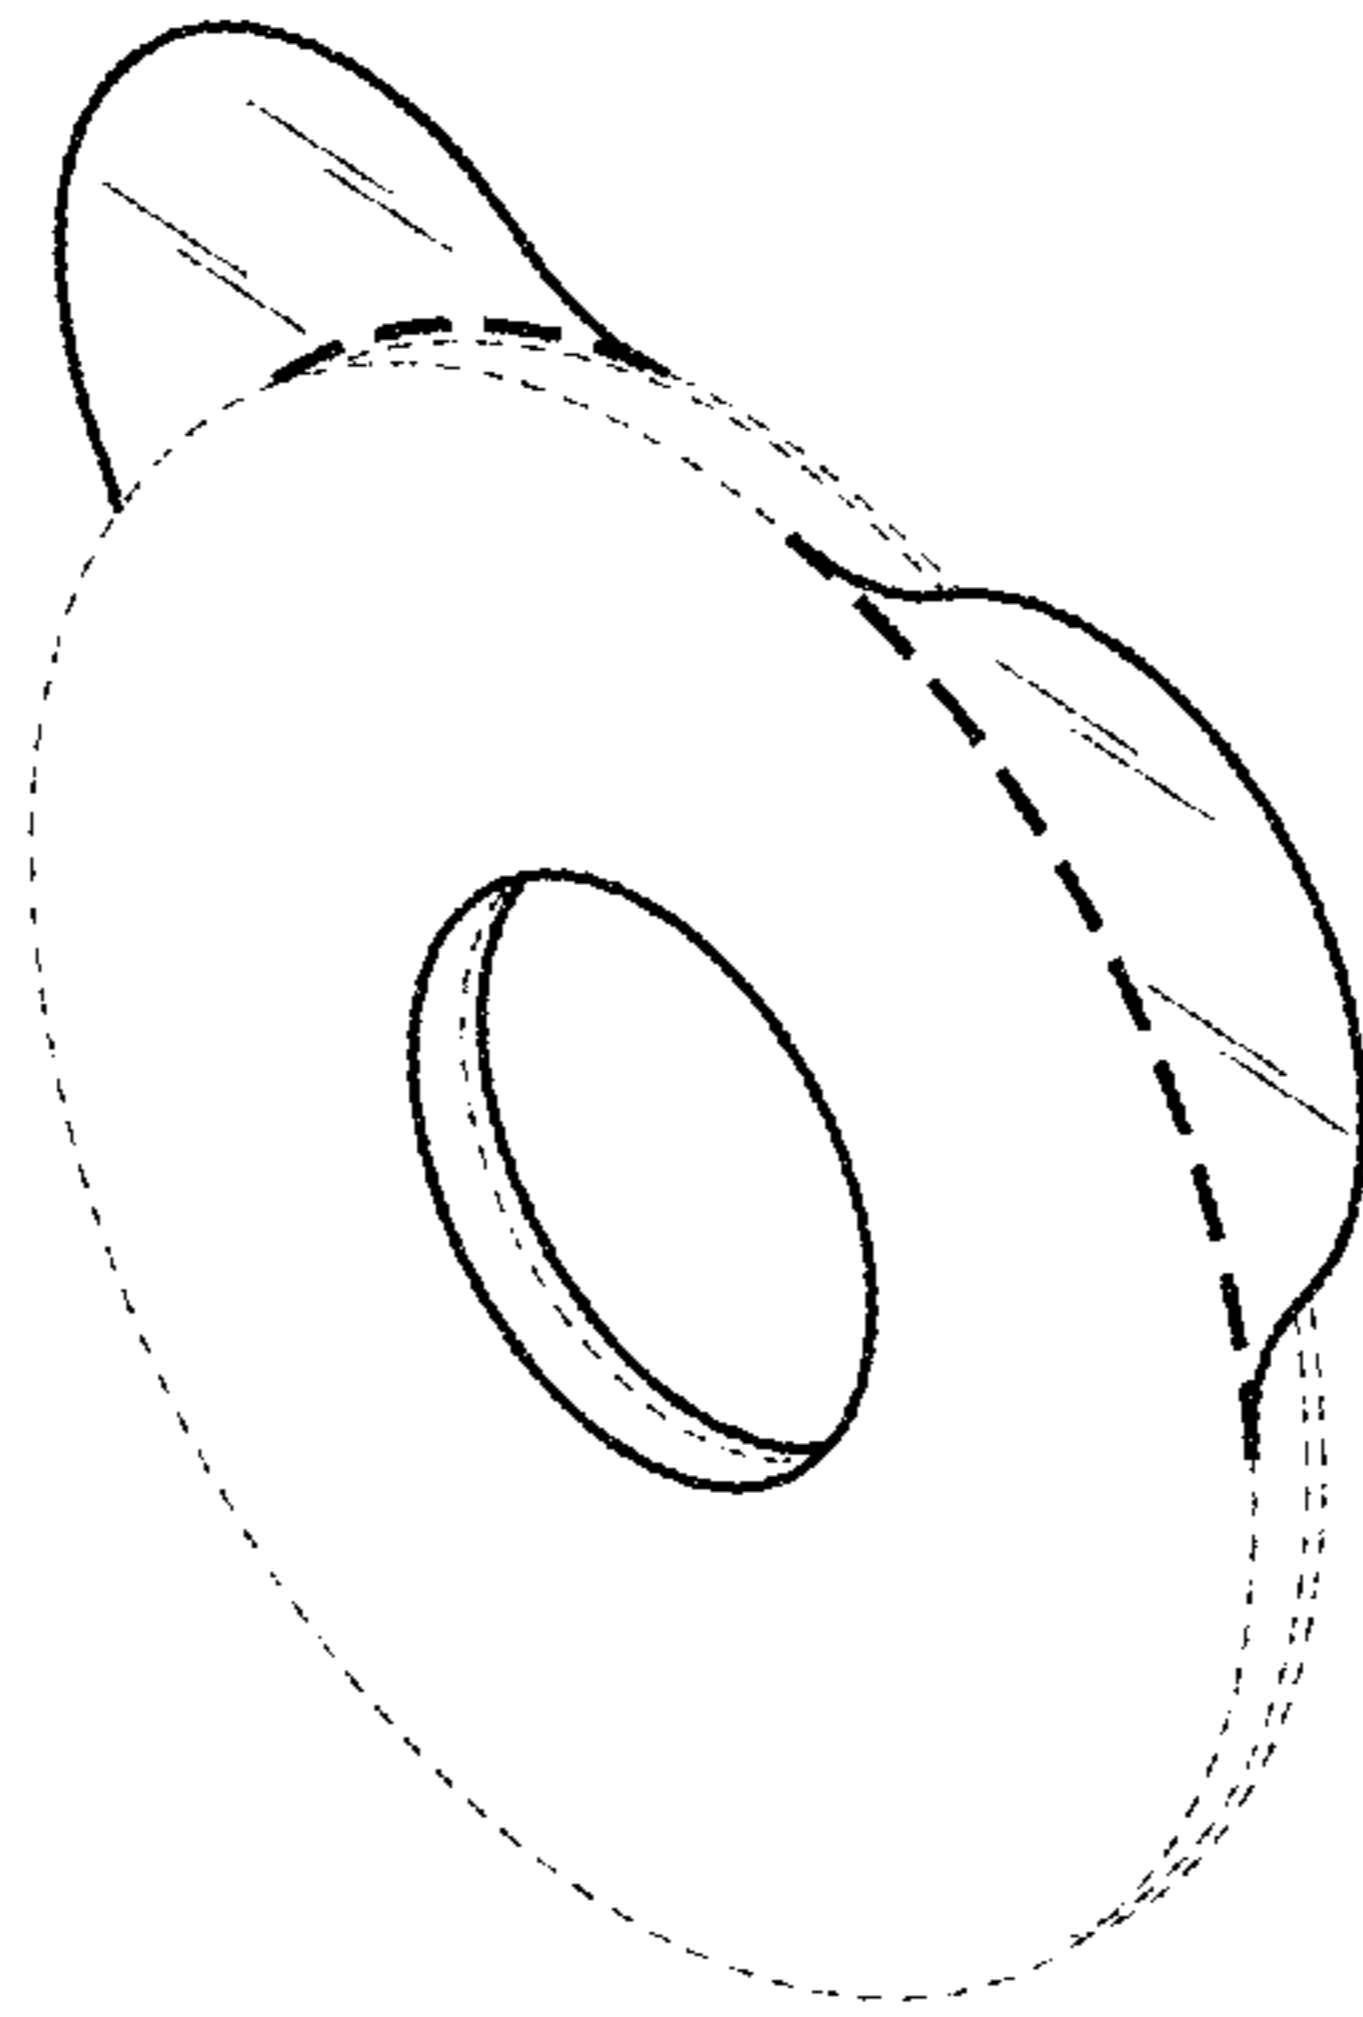


Fig. 1

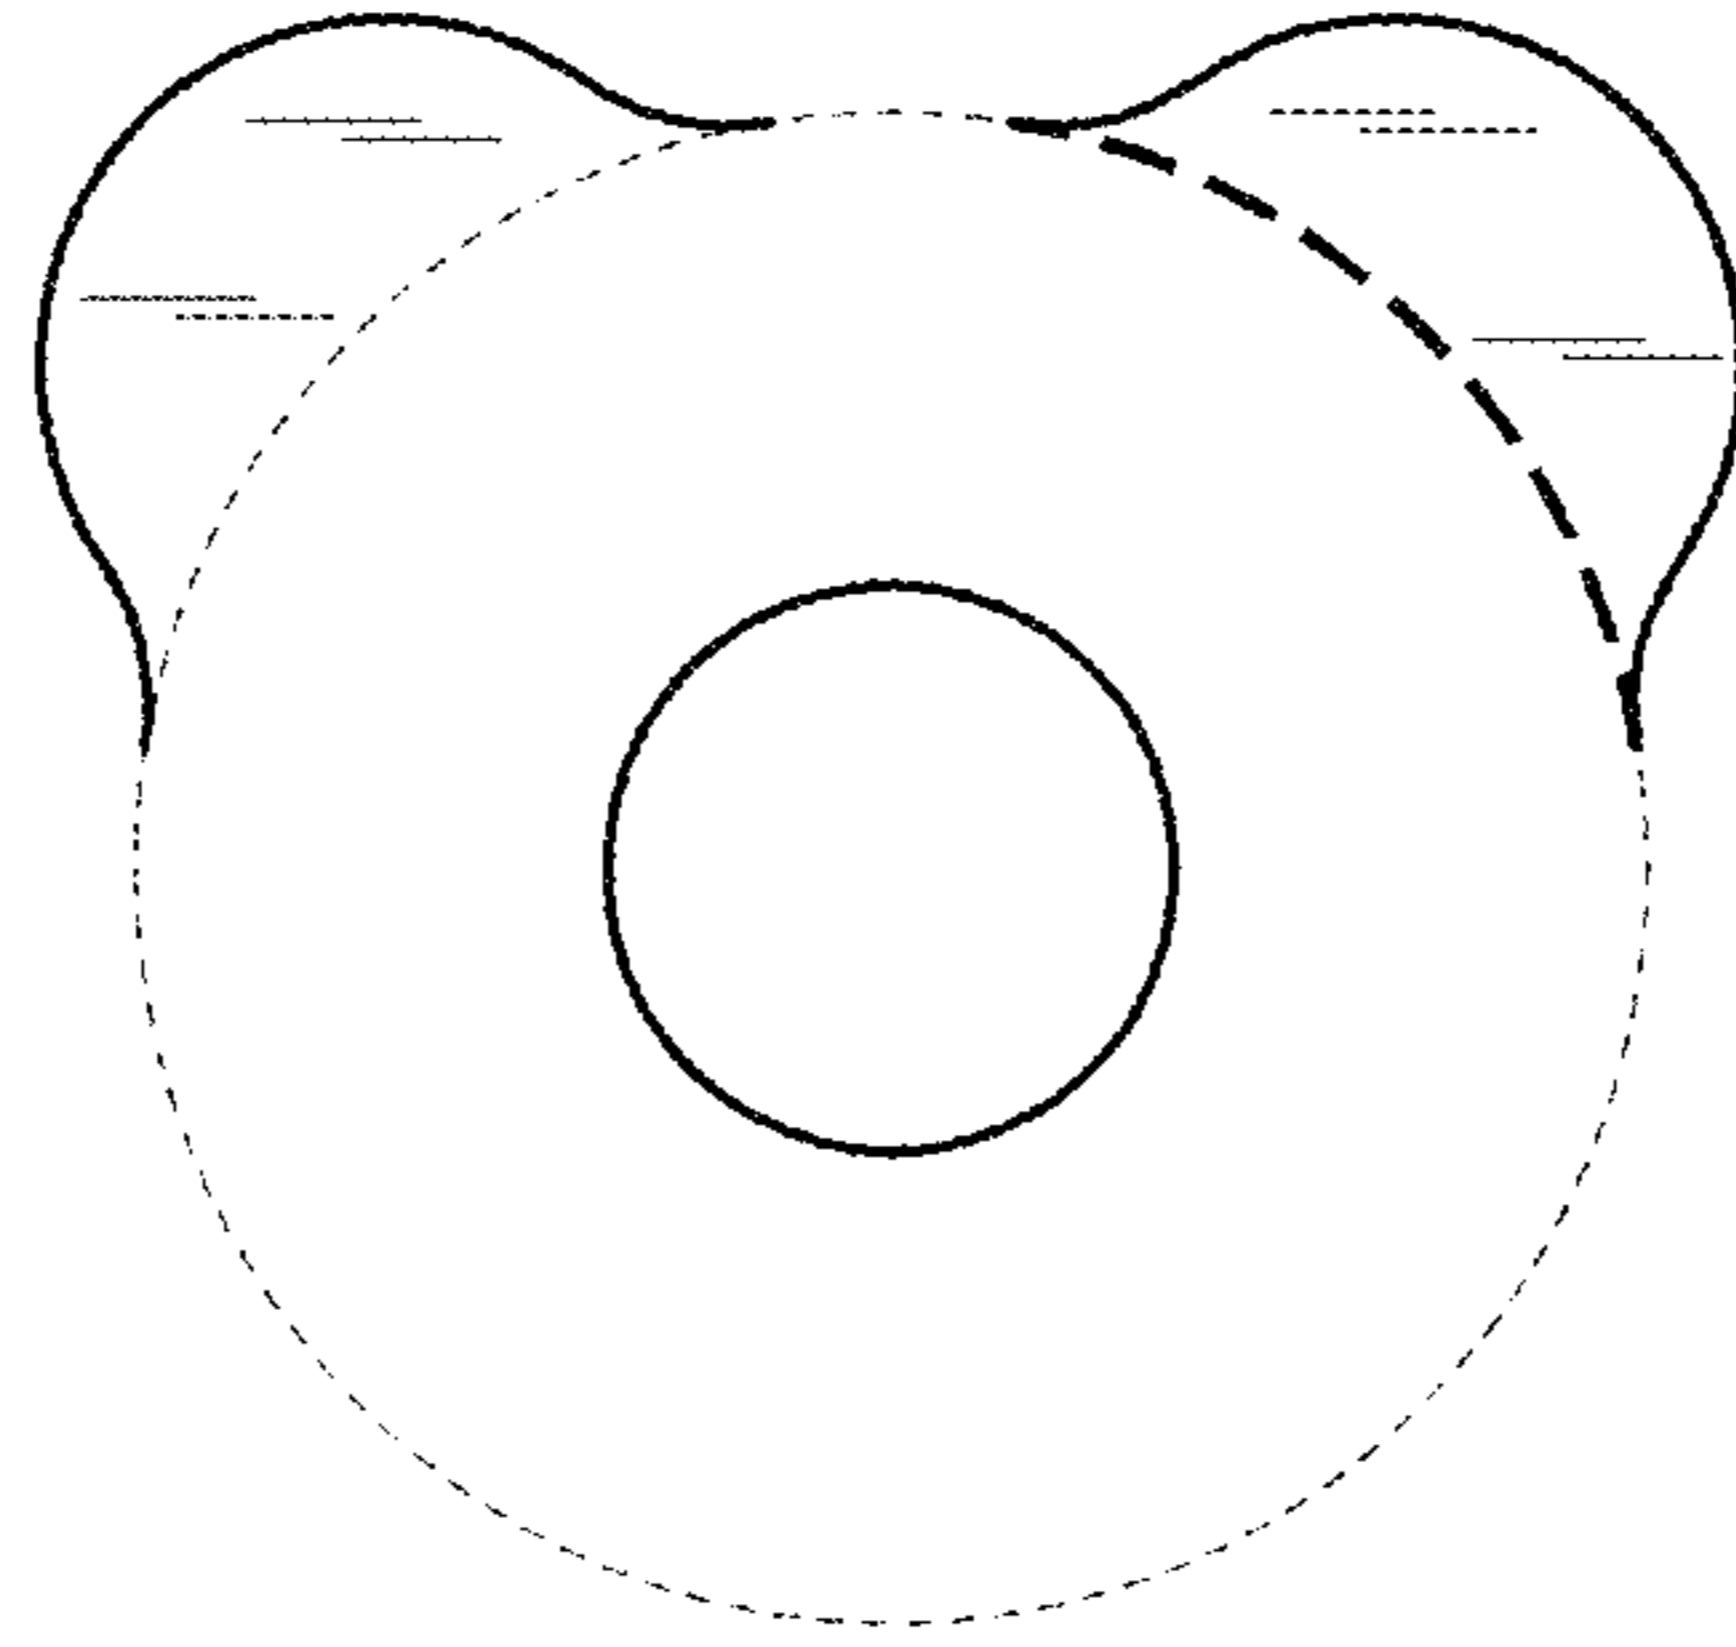


Fig. 2

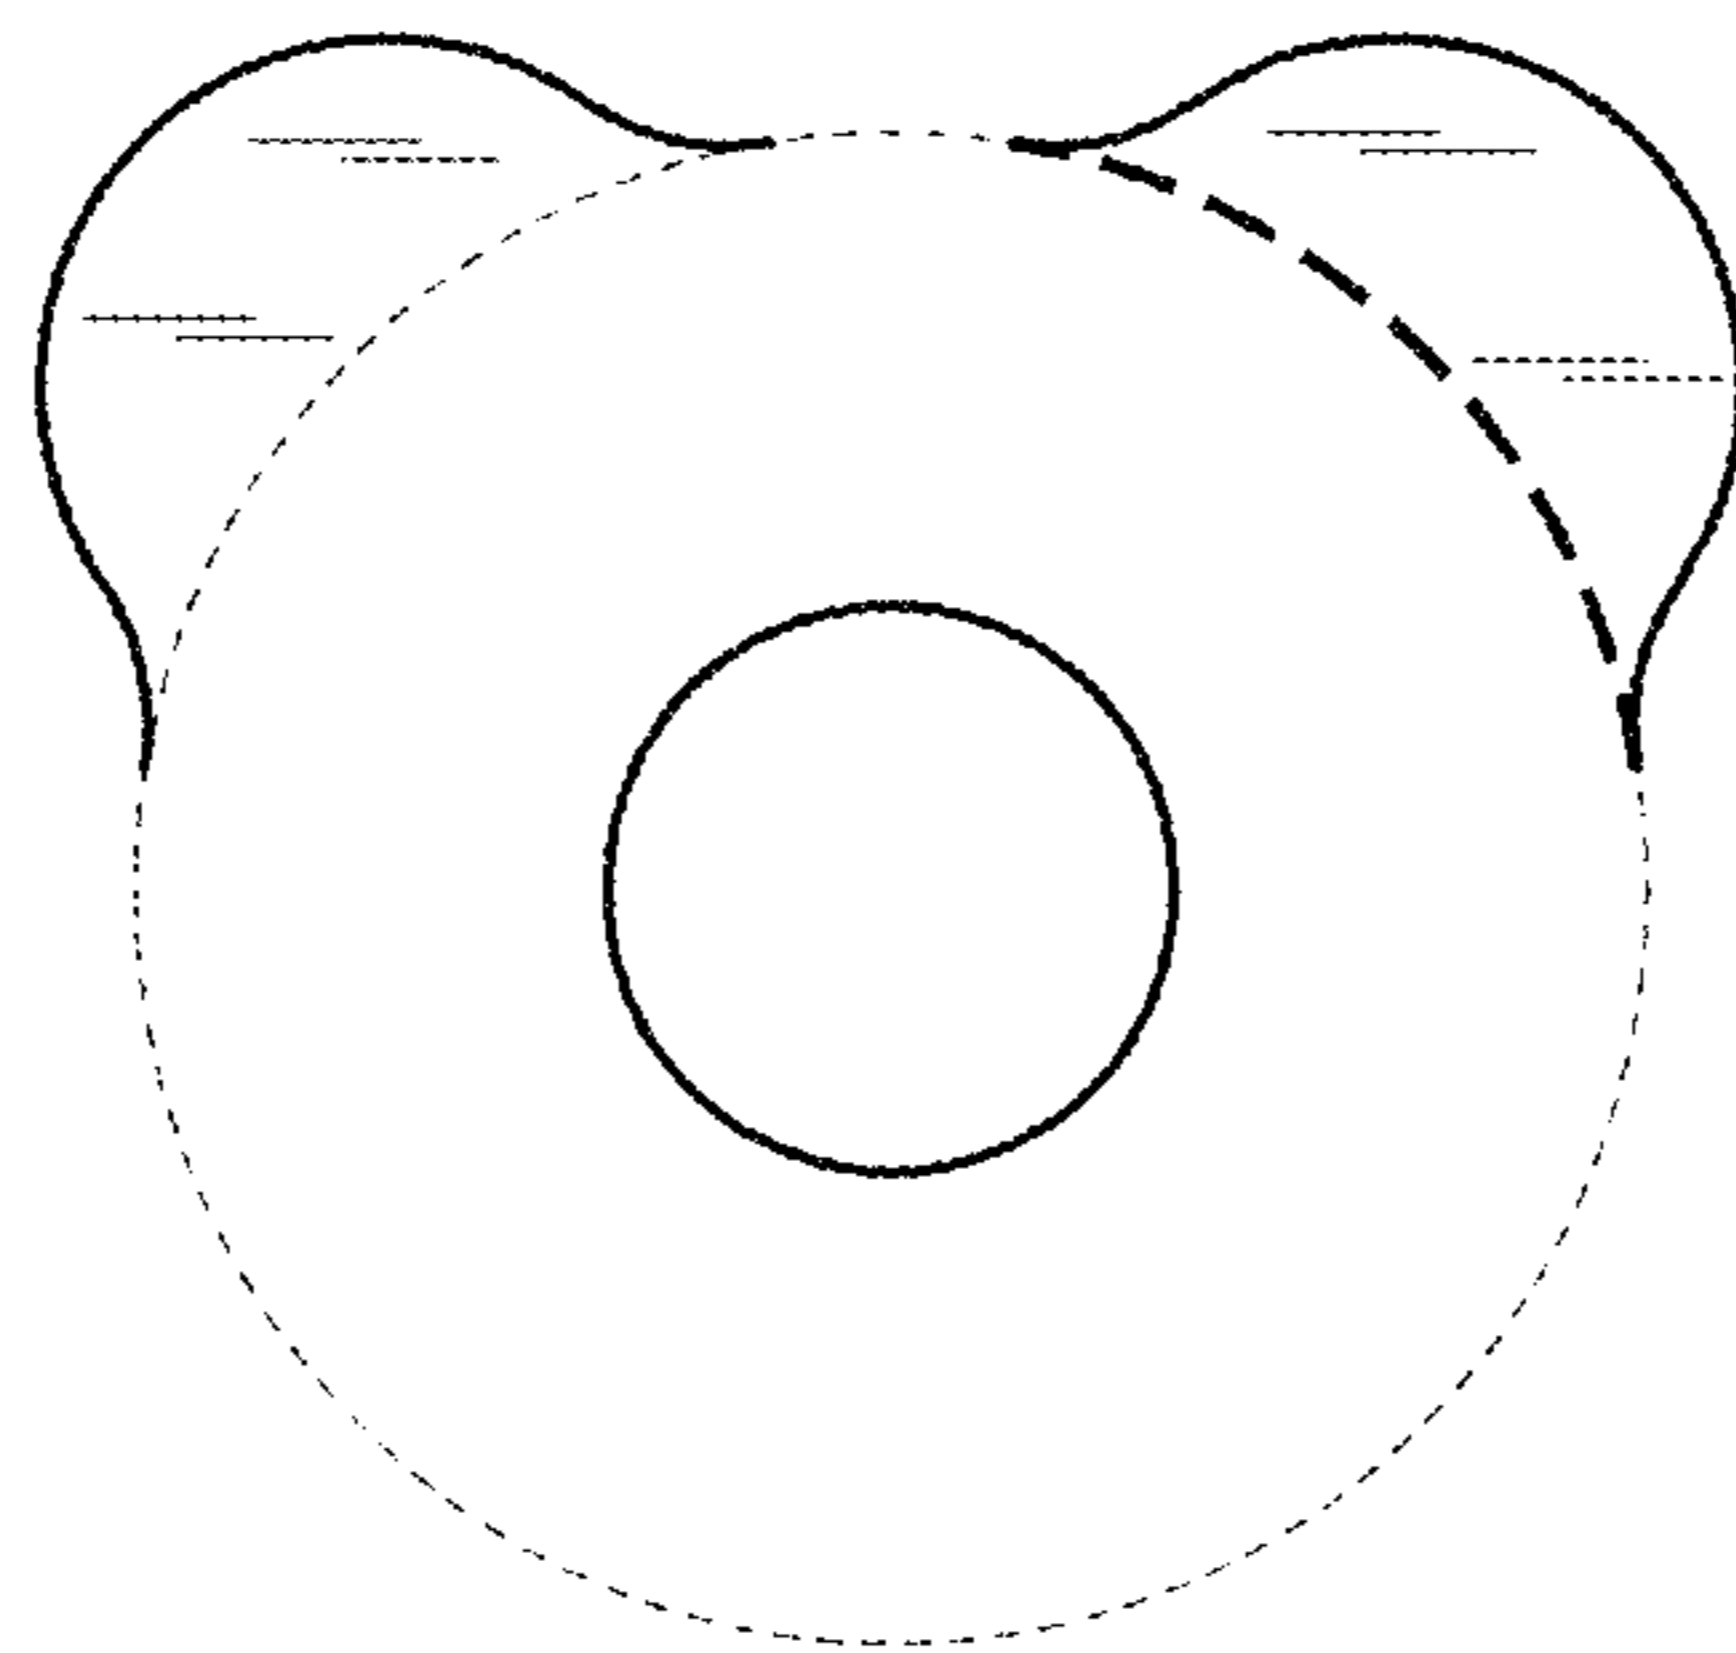


Fig. 3



Fig. 4

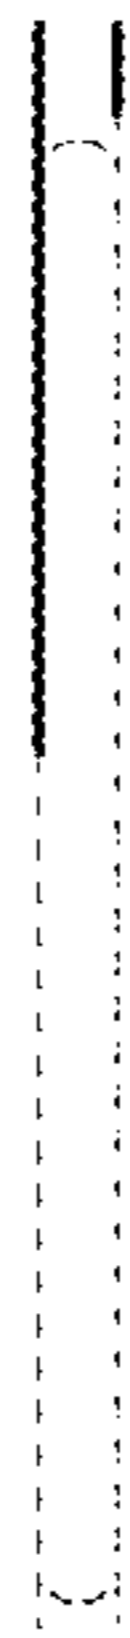


Fig. 5

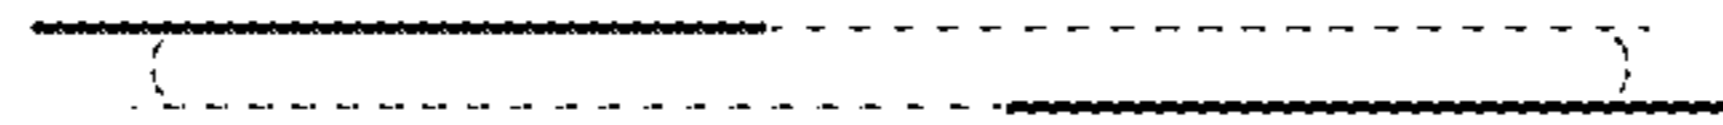


Fig. 6

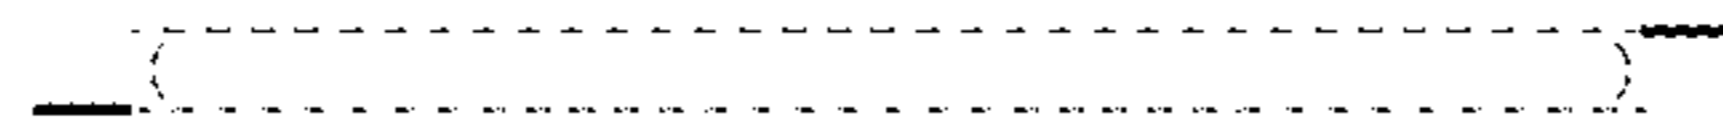


Fig. 7