



US00D811581S

(12) **United States Design Patent** (10) **Patent No.:** **US D811,581 S**
Danford (45) **Date of Patent:** **** Feb. 27, 2018**

(54) **RESISTANCE BREATHING DEVICE**

5,799,652 A 9/1998 Kotliar
5,848,589 A 12/1998 Welnetz
5,850,833 A 12/1998 Kotliar

(71) Applicant: **TrainingMask L.L.C.**, Cadillac, MI (US)

(Continued)

(72) Inventor: **Casey Danford**, Cadillac, MI (US)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **TrainingMask LLC**, Cadillac, MI (US)

CN 1311705 A 9/2001
CN 3416108 12/2004

(**) Term: **15 Years**

(Continued)

(21) Appl. No.: **29/556,825**

OTHER PUBLICATIONS

(22) Filed: **Mar. 3, 2016**

Printouts of Phantom Athletics website <http://www.phantom-trainingmask.com/en/> advertising a resistance breathing device, accessed Jan. 26, 2016 (8 pages).

(51) **LOC (11) Cl.** **29-02**

(Continued)

(52) **U.S. Cl.**

USPC **D24/110.1**; D29/108

(58) **Field of Classification Search**

USPC D24/110.1, 110.6, 127, 162, 164; D29/108

CPC A61B 18/02; A62B 18/025; A62B 23/025; A62B 7/10; A62B 9/02; A63B 23/18

See application file for complete search history.

Primary Examiner — Barbara Fox

Assistant Examiner — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Greenberg Traurig, LLP

(57) **CLAIM**

An ornamental design for a resistance breathing device, as shown and described.

(56) **References Cited**

DESCRIPTION

U.S. PATENT DOCUMENTS

| | | | |
|--------------|---------|--------------|---------------|
| 938,247 A | 10/1909 | Kuhn | |
| 3,097,642 A | 7/1963 | Russell | |
| 3,633,575 A | 1/1972 | Brumfield | |
| 3,850,171 A | 11/1974 | Ball et al. | |
| D246,012 S * | 10/1977 | Minette | D29/108 |
| 4,064,876 A | 12/1977 | Mulchi | |
| 4,221,381 A | 9/1980 | Ericson | |
| 4,549,543 A | 10/1985 | Moon | |
| 4,601,465 A | 7/1986 | Roy | |
| 4,739,987 A | 4/1988 | Nicholson | |
| 4,770,413 A | 9/1988 | Green | |
| 4,961,420 A | 10/1990 | Cappa et al. | |
| 4,973,047 A | 11/1990 | Norell | |
| 5,117,821 A | 6/1992 | White | |
| 5,167,819 A | 12/1992 | Iana et al. | |
| 5,697,105 A | 12/1997 | White | |

FIG. 1 is a top perspective view of a resistance breathing device showing my new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof;


FIG. 5 is right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines in the drawings illustrate stitching on the resistance breathing device that forms part of the claimed design. The dotted lines in the drawings depict portions of the resistance breathing device that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

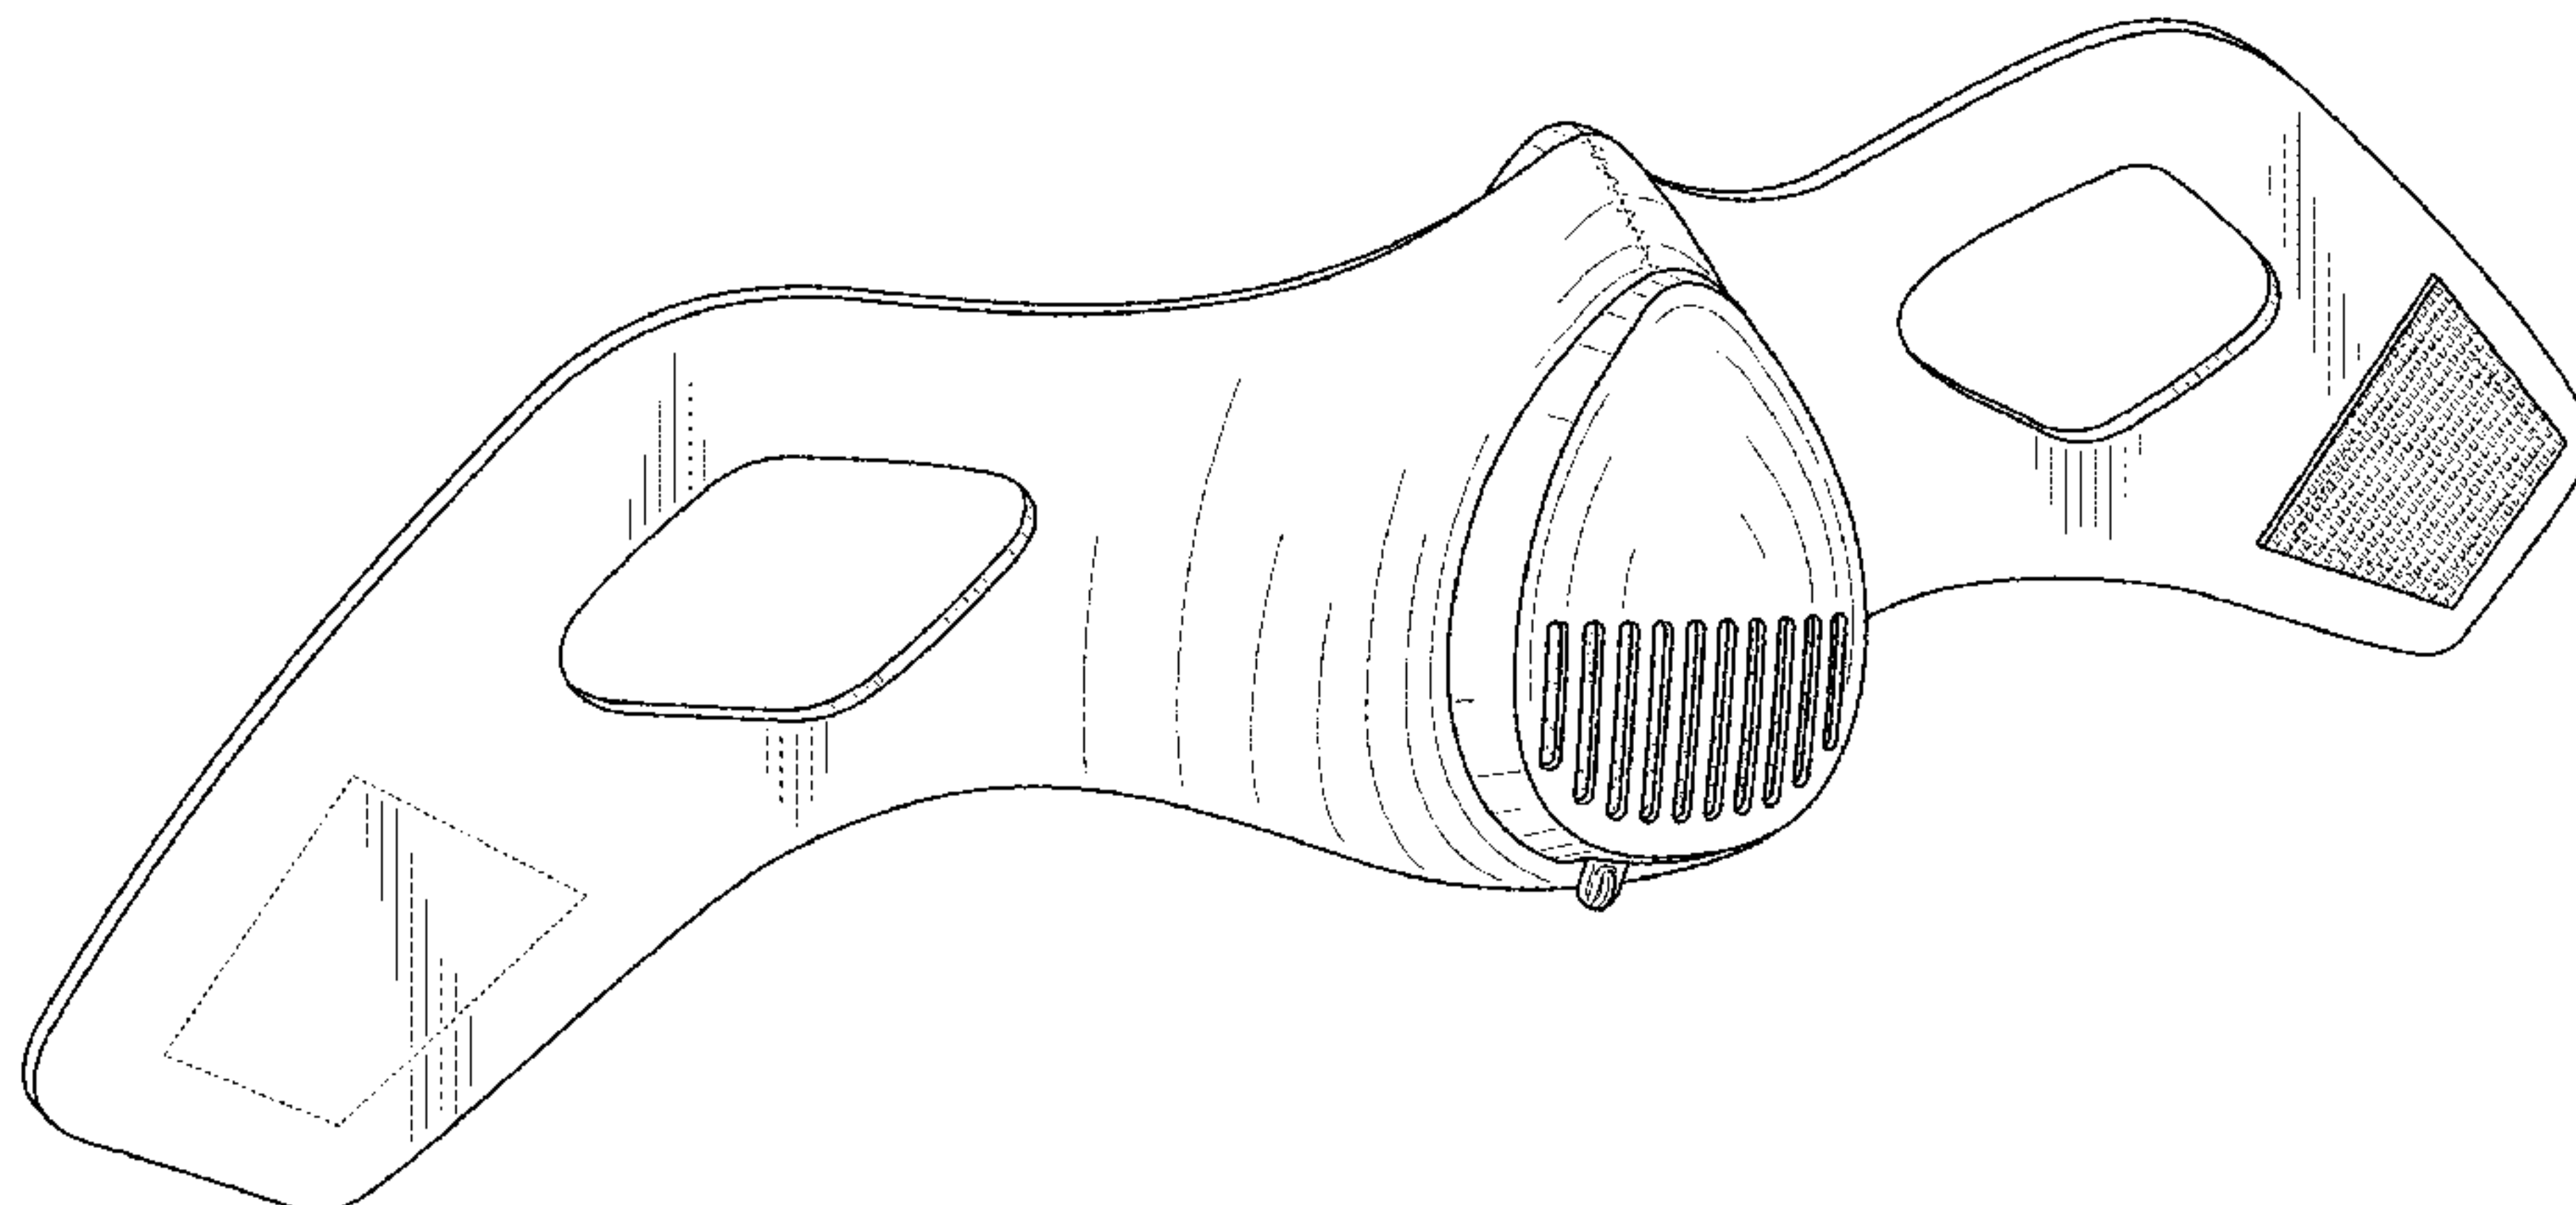

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | |
|--------------|------|---------|-------------------|--------------|
| 5,924,419 | A | 7/1999 | Kotliar | |
| 5,964,222 | A | 10/1999 | Kotliar | |
| 6,070,578 | A | 6/2000 | Baughman et al. | |
| D440,302 | S | 4/2001 | Wolfe | |
| 6,471,621 | B2 | 10/2002 | Hörstel et al. | |
| 6,508,850 | B1 | 1/2003 | Kotliar | |
| 6,554,746 | B1 | 4/2003 | McConnell et al. | |
| 6,606,751 | B1 | 8/2003 | Kalhok et al. | |
| 6,644,308 | B2 | 11/2003 | Kalhok et al. | |
| 7,523,755 | B2 | 4/2009 | Richardson et al. | |
| 7,931,733 | B2 | 4/2011 | Kotliar | |
| D645,956 | S | 9/2011 | Grimsley | |
| D665,903 | S * | 8/2012 | Sullivan | D24/110.1 |
| 8,365,734 | B1 | 2/2013 | Lehman | |
| D681,192 | S | 4/2013 | D'Souza et al. | |
| 8,590,533 | B2 | 11/2013 | Danford | |
| D694,875 | S | 12/2013 | D'Souza et al. | |
| 9,067,086 | B2 | 6/2015 | Danford | |
| 9,579,540 | B1 * | 2/2017 | Danford | A63B 21/0004 |
| 9,643,048 | B1 * | 5/2017 | Danford | A61M 16/20 |
| 2001/0007651 | A1 | 7/2001 | Fust | |
| 2001/0029750 | A1 | 10/2001 | Kotliar | |
| 2002/0023762 | A1 | 2/2002 | Kotliar | |
| 2002/0100893 | A1 | 8/2002 | Shultz | |
| 2002/0162556 | A1 | 11/2002 | Smith et al. | |
| 2003/0005934 | A1 | 1/2003 | Japuntich et al. | |
| 2004/0146842 | A1 | 7/2004 | Carlucci et al. | |
| 2004/0226563 | A1 | 11/2004 | Xu et al. | |
| 2008/0178884 | A1 | 7/2008 | Gerson et al. | |
| 2008/0202774 | A1 | 8/2008 | Kotliar | |
| 2008/0210240 | A1 | 9/2008 | Kotliar | |
| 2009/0320848 | A1 | 12/2009 | Steindorf et al. | |
| 2010/0101584 | A1 | 4/2010 | Bledstein et al. | |
| 2011/0212811 | A1 | 9/2011 | Rutten | |
| 2012/0103339 | A1 | 5/2012 | Koehler | |
| 2013/0319420 | A1 | 12/2013 | Danford | |
| 2016/0089553 | A1 | 3/2016 | Dickstein et al. | |
| 2016/0129286 | A1 | 5/2016 | Danford | |
| 2016/0129287 | A1 | 5/2016 | Danford | |
| 2017/0144000 | A1 * | 5/2017 | Danford | A62B 23/025 |

FOREIGN PATENT DOCUMENTS

| | | |
|----|--------------|---------|
| CN | 3525464 | 5/2006 |
| CN | 3611368D | 2/2007 |
| CN | 300733965 | 1/2008 |
| CN | 300798841D S | 7/2008 |
| CN | 300853751D S | 11/2008 |
| CN | 301345091 S | 9/2010 |
| CN | 301345092 S | 9/2010 |
| CN | 102421485 A | 4/2012 |
| CN | 302364261 S | 3/2013 |
| CN | 302560932 S | 9/2013 |
| CN | 302675148 S | 12/2013 |
| CN | 203523849 U | 4/2014 |
| CN | 302827495 S | 5/2014 |
| CN | 302857904 S | 6/2014 |
| CN | 302857912 S | 6/2014 |
| CN | 302857913 S | 6/2014 |
| CN | 302919473 S | 8/2014 |
| CN | 302945765 S | 9/2014 |
| CN | 303061361 S | 12/2014 |

| | | |
|----|-------------------|---------|
| CN | 303312122 S | 7/2015 |
| EP | 2 425 875 A1 | 3/2012 |
| JP | D2004-19667 | 4/2005 |
| JP | 2010-42087 A | 2/2010 |
| JP | D2010-021935 | 7/2011 |
| KR | 30-0514514 | 12/2008 |
| KR | 30-2008-0014298 | 4/2009 |
| KR | 20-2010-0004312 U | 4/2010 |
| KR | 30-0586700 | 1/2011 |
| KR | 30-0778665 | 1/2015 |
| WO | 00/04957 A1 | 2/2000 |
| WO | 2010/127161 A2 | 11/2010 |
| WO | WOD082862 | 2/2014 |

OTHER PUBLICATIONS

Photographs of a resistance breathing device, purchased Jun. 3, 2016, along with redacted invoice for such purchase (5 pages).

Utility U.S. Appl. No. 14/951,837, filed Nov. 25, 2015, entitled "Resistance and Filtration Breathing Device" (39 pages).

Utility U.S. Appl. No. 14/989,400, filed Jan. 6, 2016, entitled "Resistance Breathing Device" (43 pages).

Design U.S. Appl. No. 29/544,300, filed Nov. 2, 2015, entitled "Resistance and Filtration Breathing Device" (7 pages).

Design U.S. Appl. No. 29/544,580, filed Nov. 4, 2015, entitled "Resistance Breathing Device" (7 pages).

International Search Report and Written Opinion dated Dec. 7, 2015, issued in International (PCT) Patent Application No. PCT/US2015/051364, filed Sep. 22, 2015 (15 pages).

Design Patent Right Evaluation Report dated Mar. 21, 2016, issued by the State Intellectual Property Office of China in Patent No. ZL201530349470.4 and English-language translation thereof (31 pages).

Utility U.S. Appl. No. 15/077,567, filed Mar. 22, 2016, entitled "Resistance Breathing Device" (36 pages).

Office Action for Applicant's related Japan Design Application No. 2016-001555, dated Jul. 5, 2016 by the Japanese Patent Office, and English-language translation thereof (4 pages).

ReBNA product catalogue published by Patent Works, Inc., obtained by the Japan National Center for Industrial Property Information and Training on Mar. 21, 2008 (1 page).

Design Patent Right Evaluation Report completed Jul. 4, 2016, issued by the State Intellectual Property Office of China in Applicant's related China Design Patent No. ZL201530482604.X and English-language translation thereof (18 pages).

Design Patent Right Evaluation Report completed Jul. 4, 2016, issued by the State Intellectual Property Office of China in Applicant's related China Design Patent No. ZL201530482542.2 and English-language translation thereof (23 pages).

Patentability Assessment Report, completed Jul. 20, 2016, issued by the State Intellectual Property Office of China in Applicant's related China Utility Patent No. ZL2015208912778 and English-language translation thereof (15 pages).

International Search Report and the Written Opinion of the International Searching Authority, dated Aug. 8, 2016, issued by the European Patent Office in Applicant's related International Application No. PCT/US2015/064042 (11 pages).

* cited by examiner

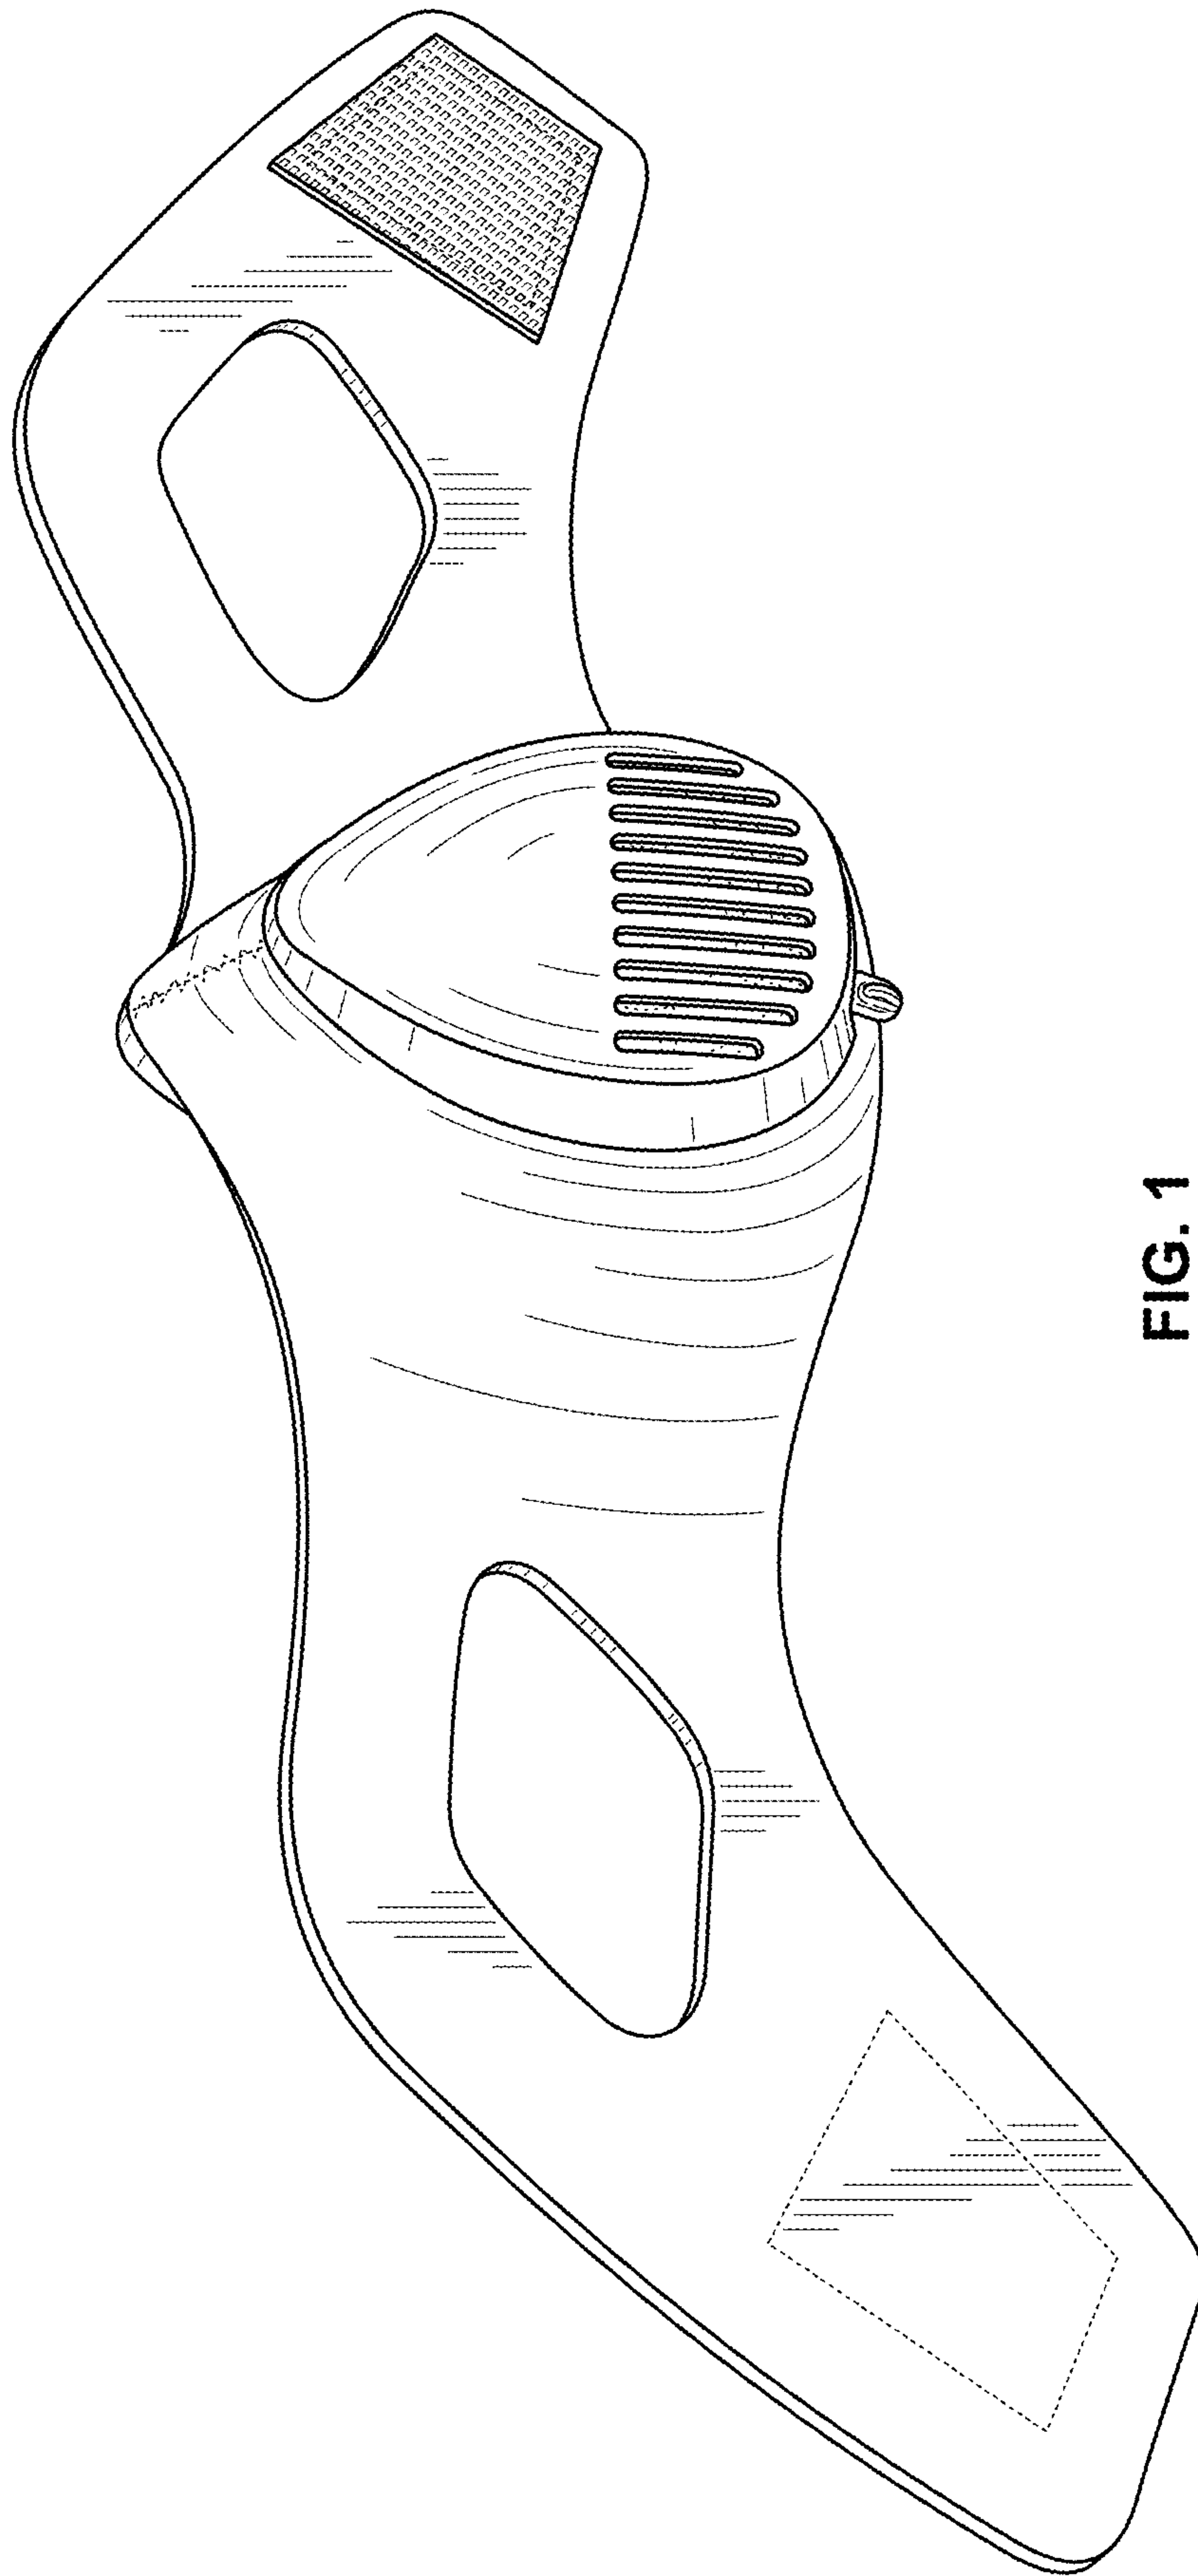


FIG. 1

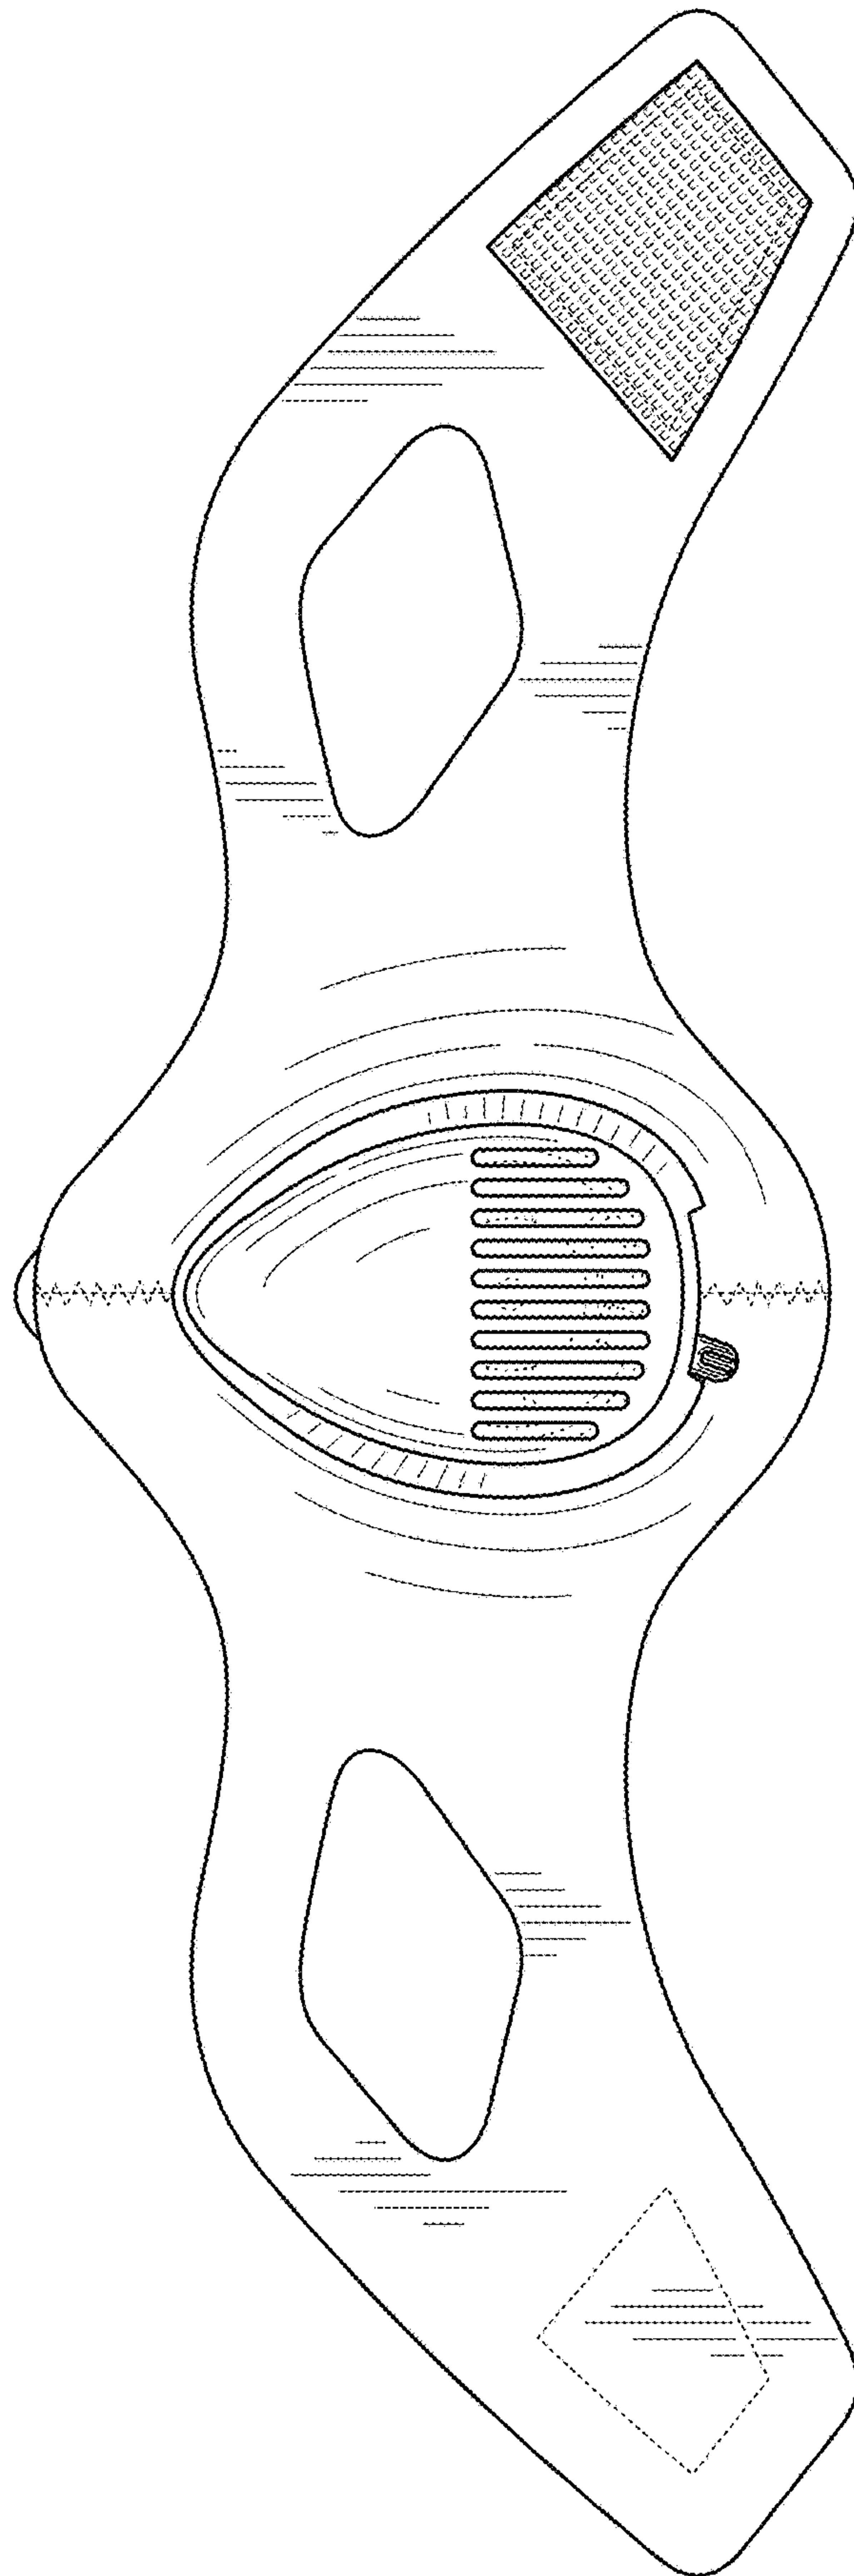


FIG. 2

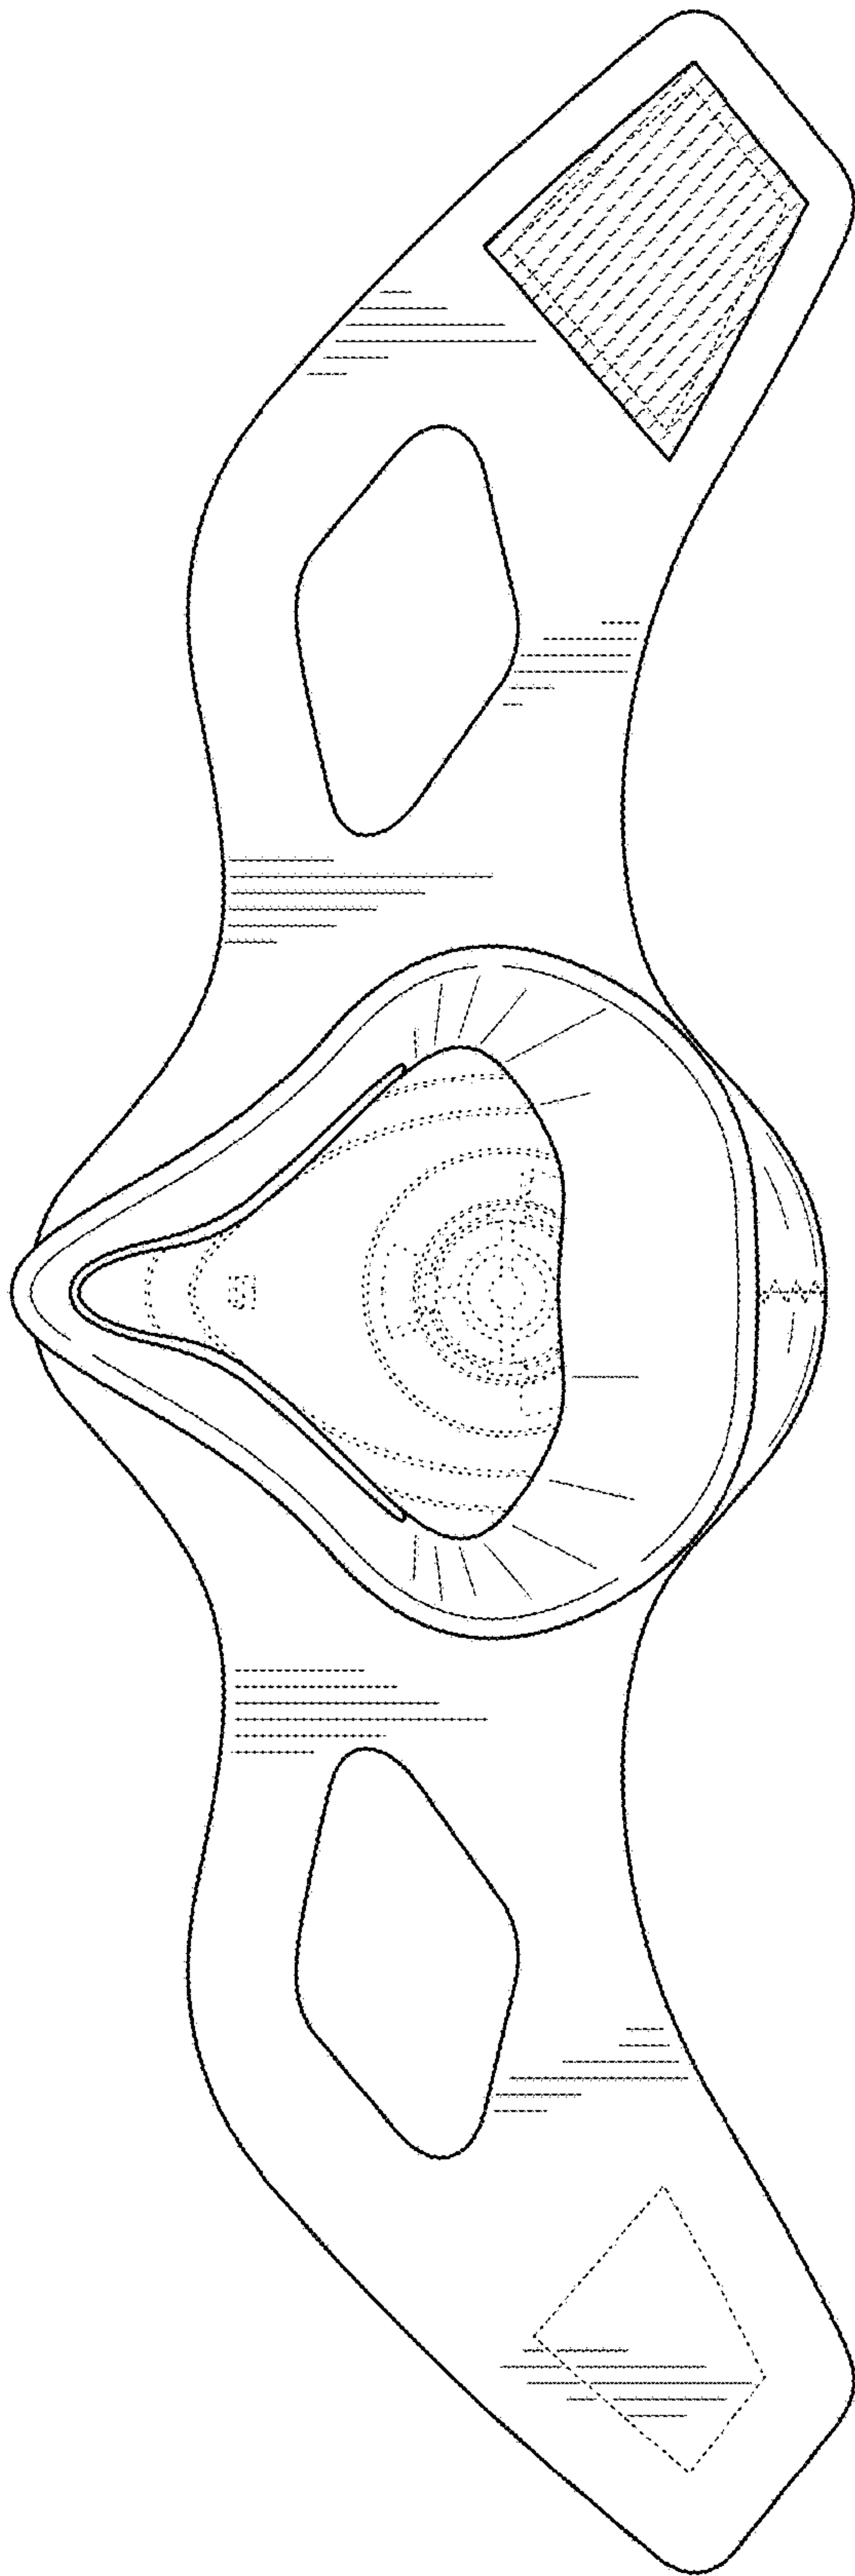


FIG. 3

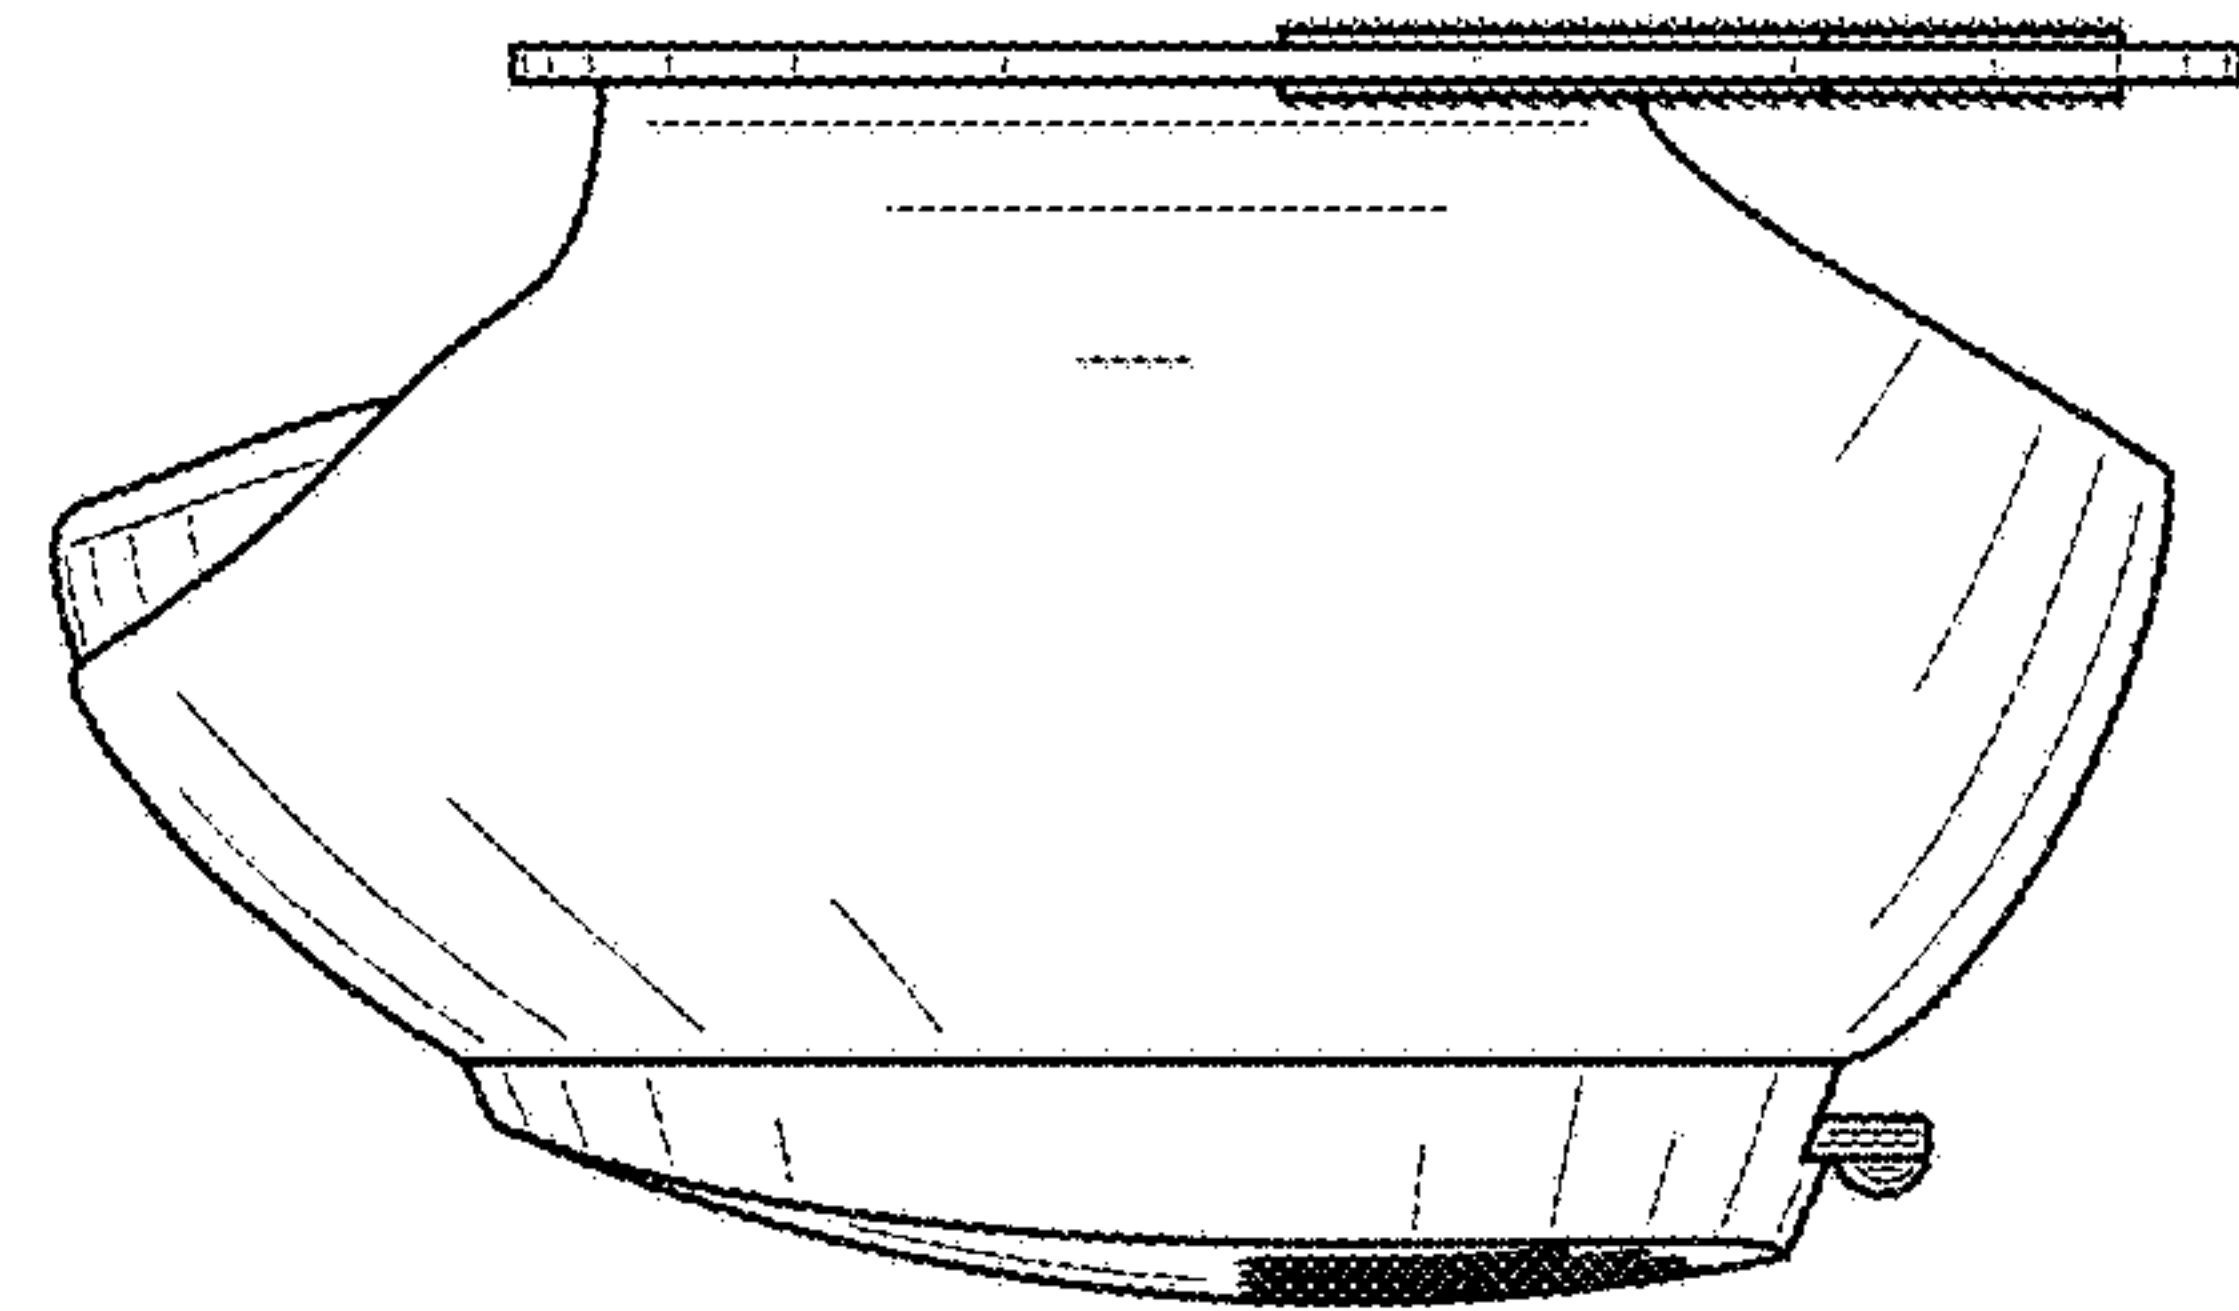


FIG. 4

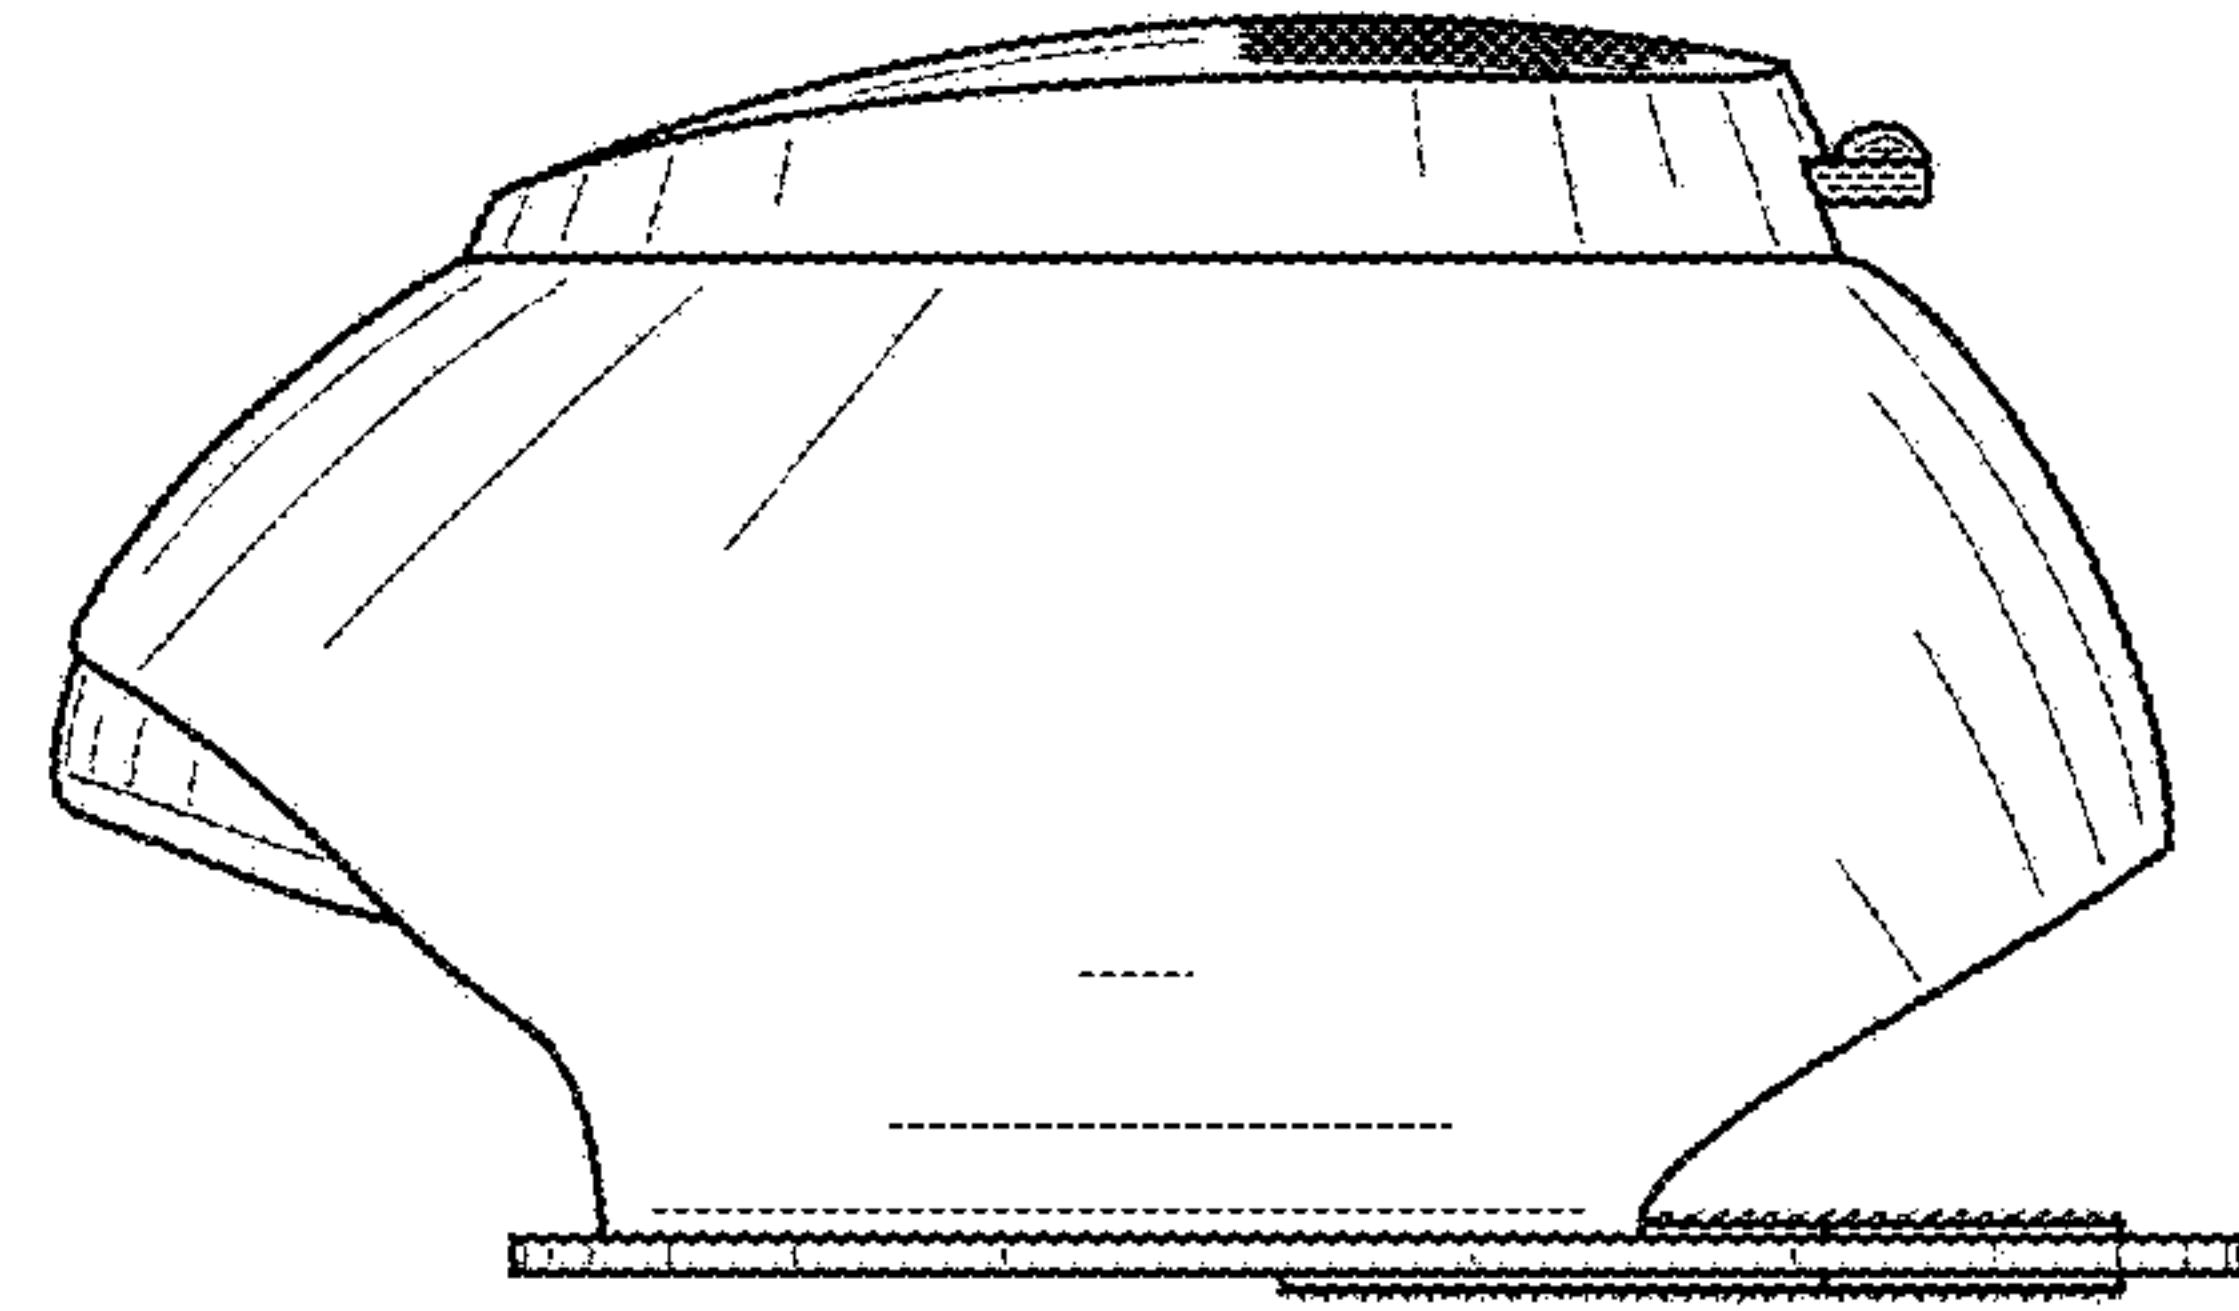


FIG. 5