



US00D816840S

(12) **United States Design Patent**  
**Shah et al.**

(10) **Patent No.:** **US D816,840 S**

(45) **Date of Patent:** **\*\* May 1, 2018**

(54) **PROXIMAL HUMERAL FRACTURE PLATE**

(71) Applicant: **Flower Orthopedics Corporation**,  
Horsham, PA (US)

(72) Inventors: **Anup A. Shah**, Sugar Land, TX (US);  
**Joshua T. Woody**, Houston, TX (US)

(73) Assignee: **Flower Orthopedics Corporation**,  
Horsham, PA (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/524,660**

(22) Filed: **Apr. 22, 2015**

(51) **LOC (11) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/155**

(58) **Field of Classification Search**  
USPC ..... D24/155-157

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,919,670	A	4/1990	Dale et al.
5,066,296	A	11/1991	Chapman et al.
5,112,333	A	5/1992	Fixel
5,489,309	A	2/1996	Lackey et al.
5,507,517	A	4/1996	Krawczak

(Continued)

**OTHER PUBLICATIONS**

Zimmer Periarticular Locking Plate System Brochure, undated.  
Produced by Zimmer Trauma, (18 pages).

(Continued)

*Primary Examiner* — Charles Hanson

(74) *Attorney, Agent, or Firm* — Riverside Law LLP

(57) **CLAIM**

The ornamental design for the proximal humeral fracture plate, as shown and described.

**DESCRIPTION**

FIG. 1 is an environmental perspective view of a proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 2 is an anterior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 3 is a lateral view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 4 is a medial view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 5 is a posterior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 6 is a superior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 7 is an inferior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus.

FIG. 8 is an environmental perspective view of a proximal humeral fracture plate for repairing a fracture of a patient's right humerus.

FIG. 9 is an anterior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus.

FIG. 10 is a lateral view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus.

FIG. 11 is a medial view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus.


FIG. 12 is a posterior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus.

FIG. 13 is a superior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus; and,

FIG. 14 is an inferior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus.

The broken line showing of bones in FIGS. 1 and 8 is included for the purpose of illustrating environment and forms no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

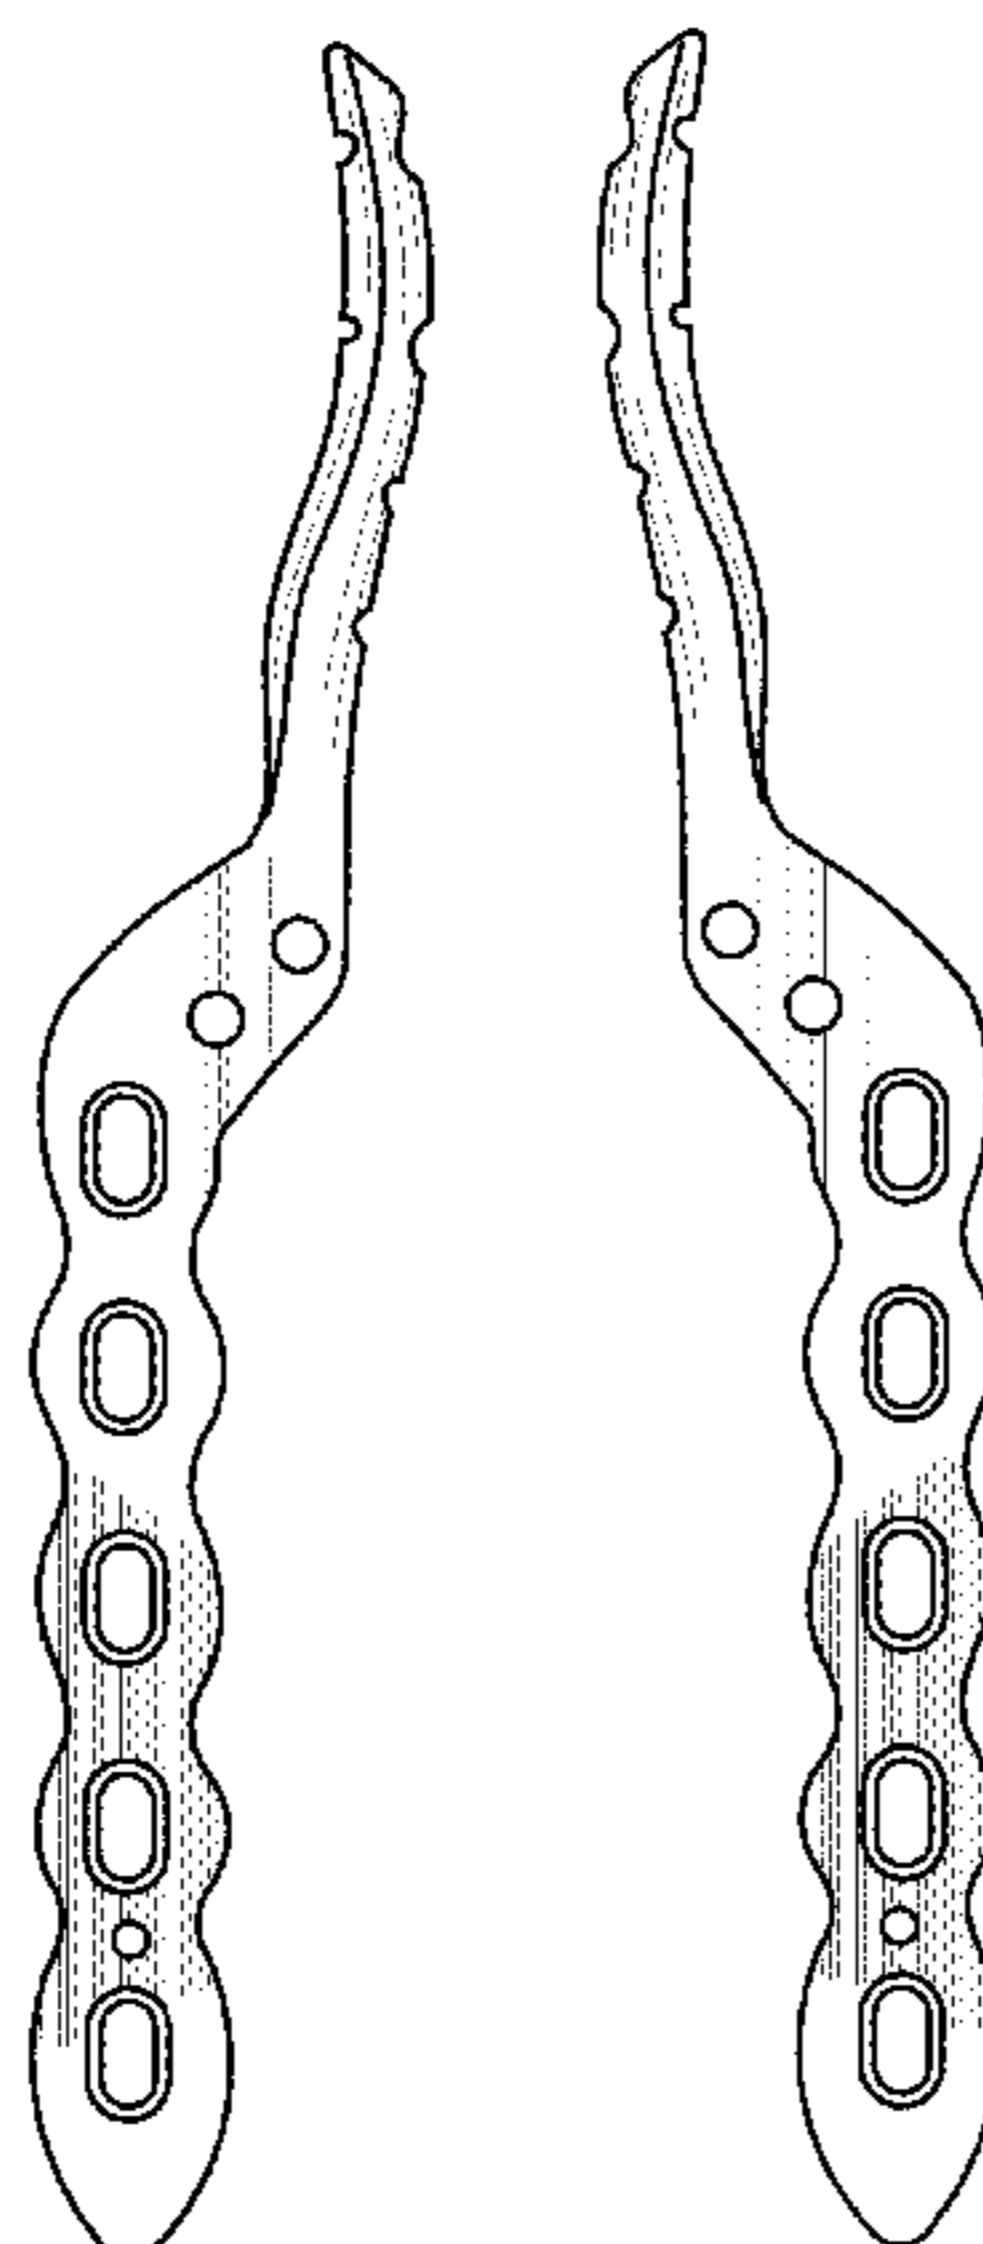

(58) **Field of Classification Search**

CPC ..... A61B 17/8061; A61B 17/7059; A61B 17/8052; A61B 17/8605; A61B 17/8085; A61B 17/809; A61B 17/8014; A61B 17/8033; A61B 17/8004; A61B 17/888; A61B 17/842; A61B 17/8023; A61B 17/8009; A61B 17/86; A61B 17/1739; A61B 17/8066; A61B 17/1671; A61B 17/1757; A61B 17/8071; A61B 17/176; A61B 2017/1782; A61B 2017/1775

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,096,040	A	8/2000	Esser	
D576,731	S *	9/2008	Strnad .....	D24/155
D589,148	S *	3/2009	Strnad .....	D24/155
D589,149	S *	3/2009	Strnad .....	D24/155
7,655,029	B2	2/2010	Niederberger et al.	
7,731,718	B2	6/2010	Schwamberger et al.	
D646,785	S *	10/2011	Milford .....	D24/155
RE43,482	E	6/2012	Mikol et al.	
D664,253	S *	7/2012	Pech .....	D24/155
D665,082	S *	8/2012	Milford .....	D24/155
8,287,538	B2	10/2012	Brenzel et al.	
8,337,534	B2	12/2012	Celli et al.	
D700,334	S *	2/2014	Borostyankoi .....	D24/155
8,906,070	B2	12/2014	Medoff	
2005/0085818	A1 *	4/2005	Huebner .....	A61B 17/1728 606/281
2005/0245931	A1 *	11/2005	Orbay .....	A61B 17/1728 606/291
2007/0088360	A1 *	4/2007	Orbay .....	A61B 17/8057 606/287
2008/0021477	A1 *	1/2008	Strnad .....	A61B 17/8033 606/287
2011/0224736	A1	9/2011	Humphery	
2011/0313422	A1	12/2011	Schwager et al.	
2012/0016366	A1	1/2012	Eglseder	
2012/0136396	A1	5/2012	Baker et al.	
2012/0179208	A1	7/2012	Geissler et al.	
2012/0226323	A1	9/2012	Gonzalez-Hernandez	
2013/0096629	A1	4/2013	Rollinghof et al.	

OTHER PUBLICATIONS

AxSOS Locking Plate System Brochure, copyrighted 2011. Produced by Stryker, (24 pages).

Fernandez, Dell'Oca, "Helical Implants," Injury, International Journal of the Care of the Injured, 33-SA-29-40, published by Elsevier Science, Inc. (2002), unknown city and/or country (12 pages).

Gardener, Michael et al., "Helical Plating of the Proximal Humerus," Injury, International Journal of the Care of the Injured, 36-1197-1200, published by Elsevier Science, Inc. (2005), unknown city and/or country (4 pages).

Hanchen, Marc et al., "Mono-versus polyaxial locking plates in distal femur fractures: a prospective randomized multicenter clinical trial," 38-857-863, International Orthopedics published online on Dec. 11, 2013, Springer-Verlag, Berlin Heidelberg (7 pages).

Apivatthakakul, T. et al., "Danger zone for locking screw placement in minimally invasive plate osteosynthesis," Injury, International Journal of the Care of the Injured, 41-169-172, published by Elsevier Science, Inc. (2010), unknown city and/or country (4 pages).

Yang, Kyu Hyun, "Helical plate fixation for treatment of comminuted fractures of the proximal and middle one-third of the humerus," Injury, International Journal of the Care of the Injured, 36-75-80, published by Elsevier Science, Inc. (2005), unknown city and/or country (6 pages).

Tan, James Chung Hai et al., "Minimally Invasive Helical Plating for Shaft of Humerus Fractures: Technique and Outcome," The Open Orthopedics Journal, 2012, vol. 6, 184-188, published by Bentham Open 2012, unknown city and/or country (5 pages).

Apivatthakakul, T. et al., Minimally invasive plate osteosynthesis (MIPO) of the humeral shaft fracture Is it possible? A cadaveric study and preliminary report, International Journal of the Care of the Injured, 36-530-538, published by Elsevier Science, Inc. (2005), unknown city and/or country (9 pages).

Fernandez, Dell'Oca, "The principle of helical implants Unusual ideas worth considering," Injury, International Journal of the Care of the Injured, 33-SA-1-27, published by Elsevier Science, Inc. (2002), unknown city and/or country (27 pages).

Valdez, Victor, "Minimally Invasive Plate Osteosynthesis Using a Helical Plate for Metadiaphyseal Complex Fractures of the Proximal Humerus," Ortopedia Pediatrica y Cirugia Articular, published online at www.helio.com and dated Mar. 27, 2014, unknown city and/or country (9 pages).

Smith & Nephew, Peri-Loc Locked Plating System—Proximal Humerus Fracture with Shaft Extension Case Study, Produced by Smith & Nephew, Inc. copyright 2010, (4 pages).

Smith & Nephew, Peri-Loc Locked Plating System, Produced by Smith & Nephew, Inc. copyright 2014, (68 pages).

\* cited by examiner

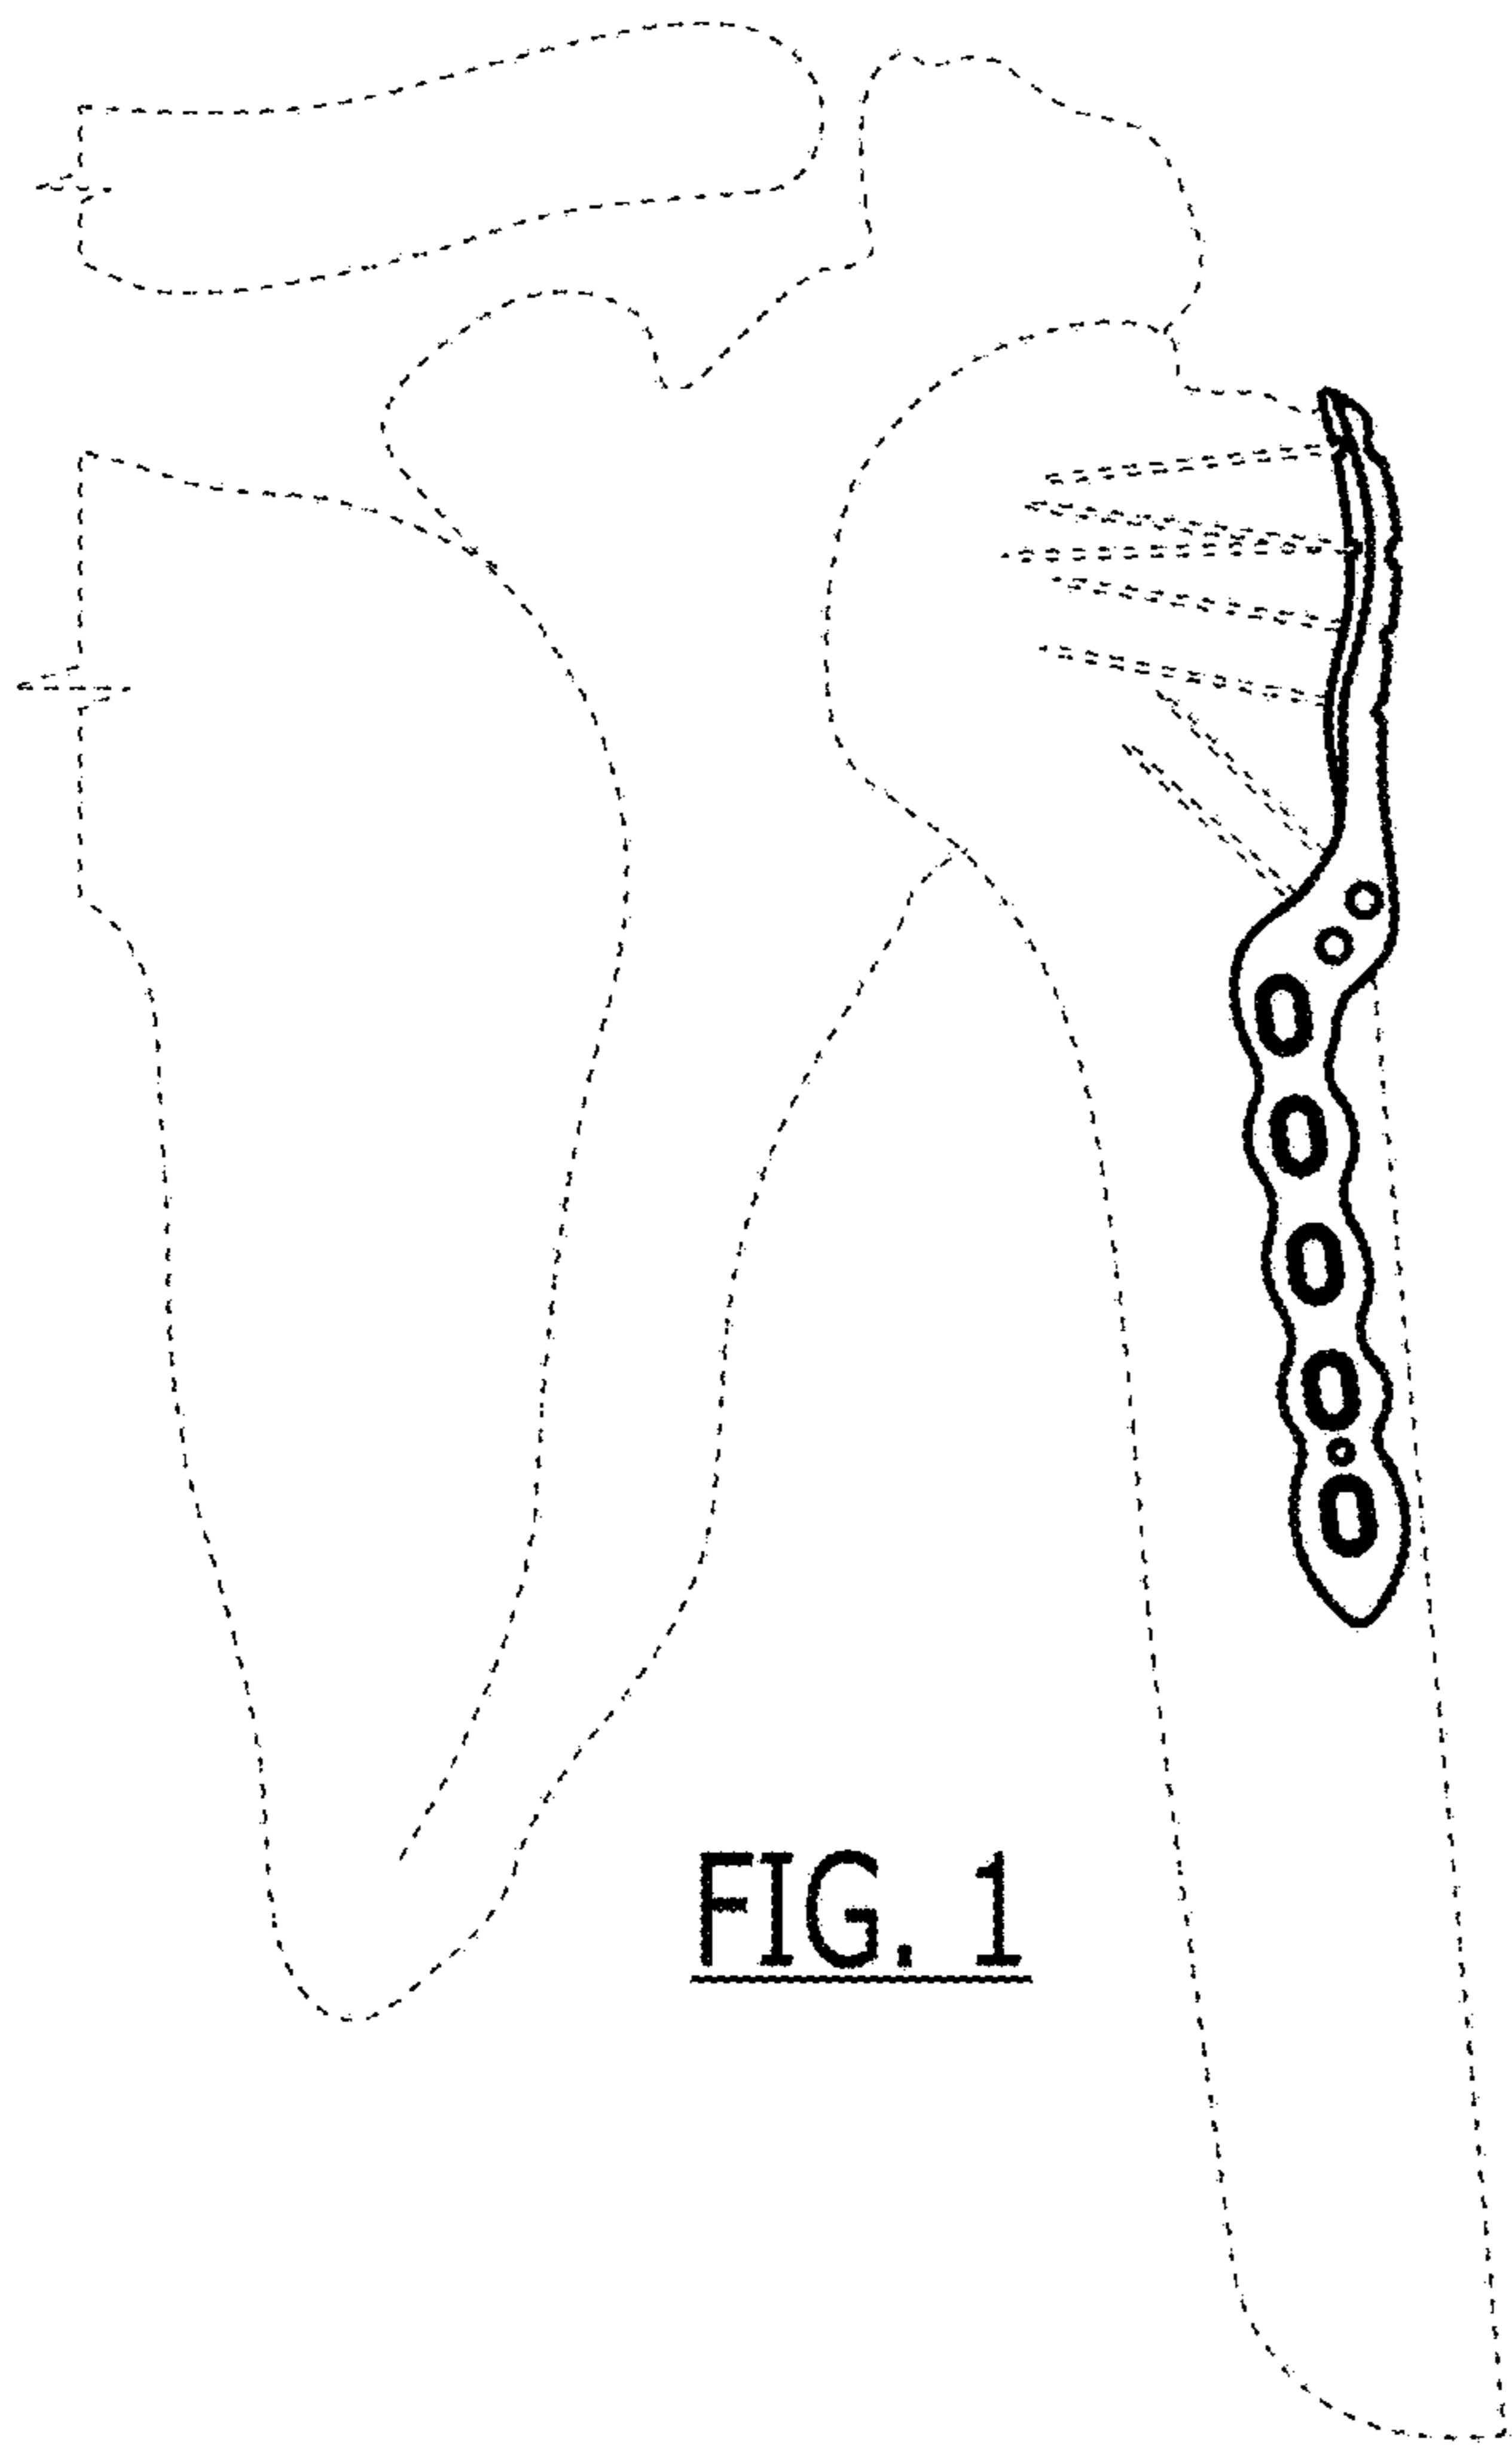


FIG. 1

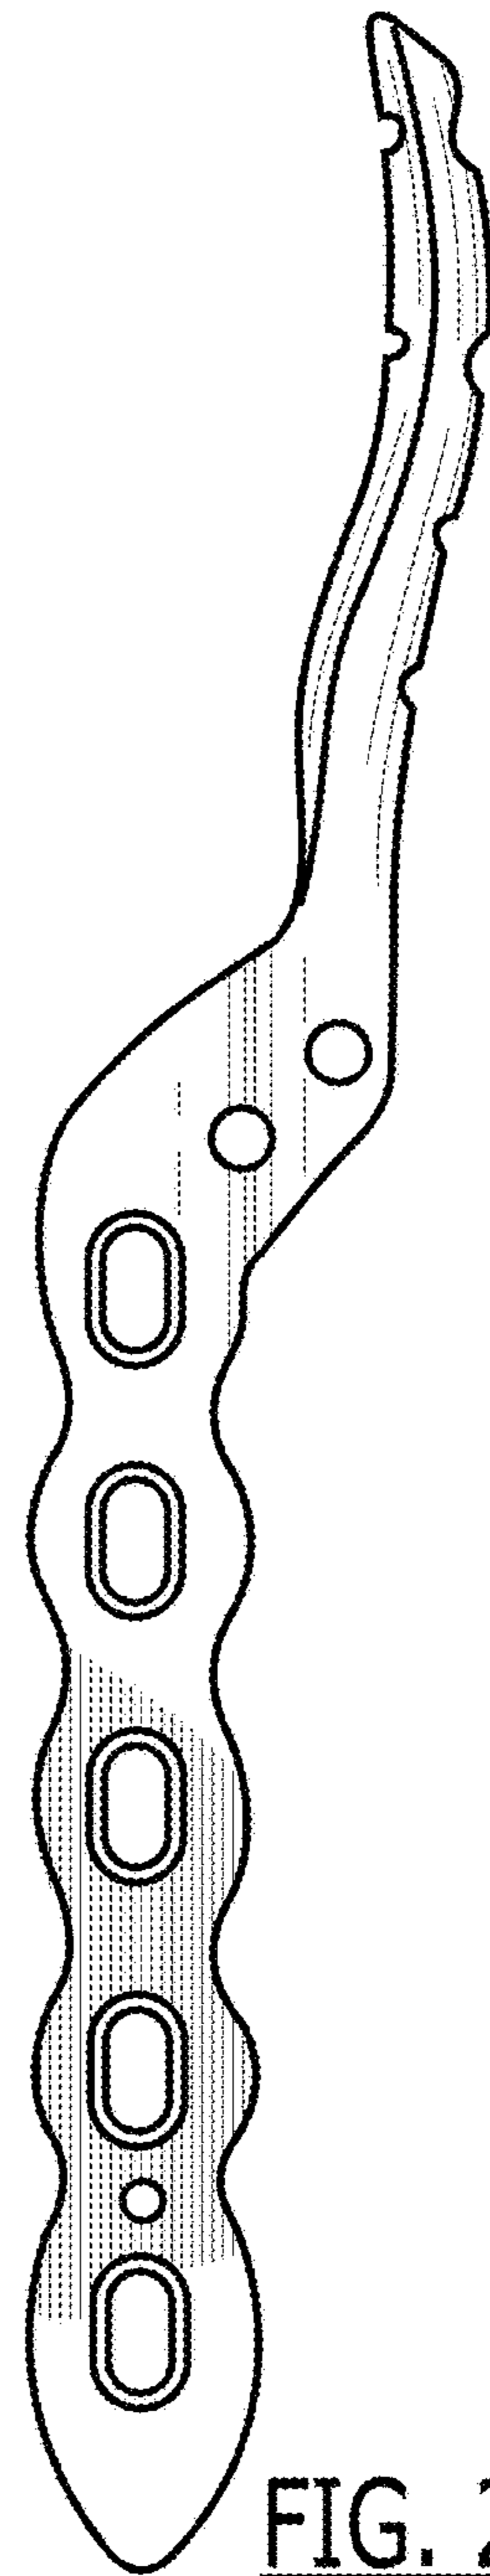


FIG. 2

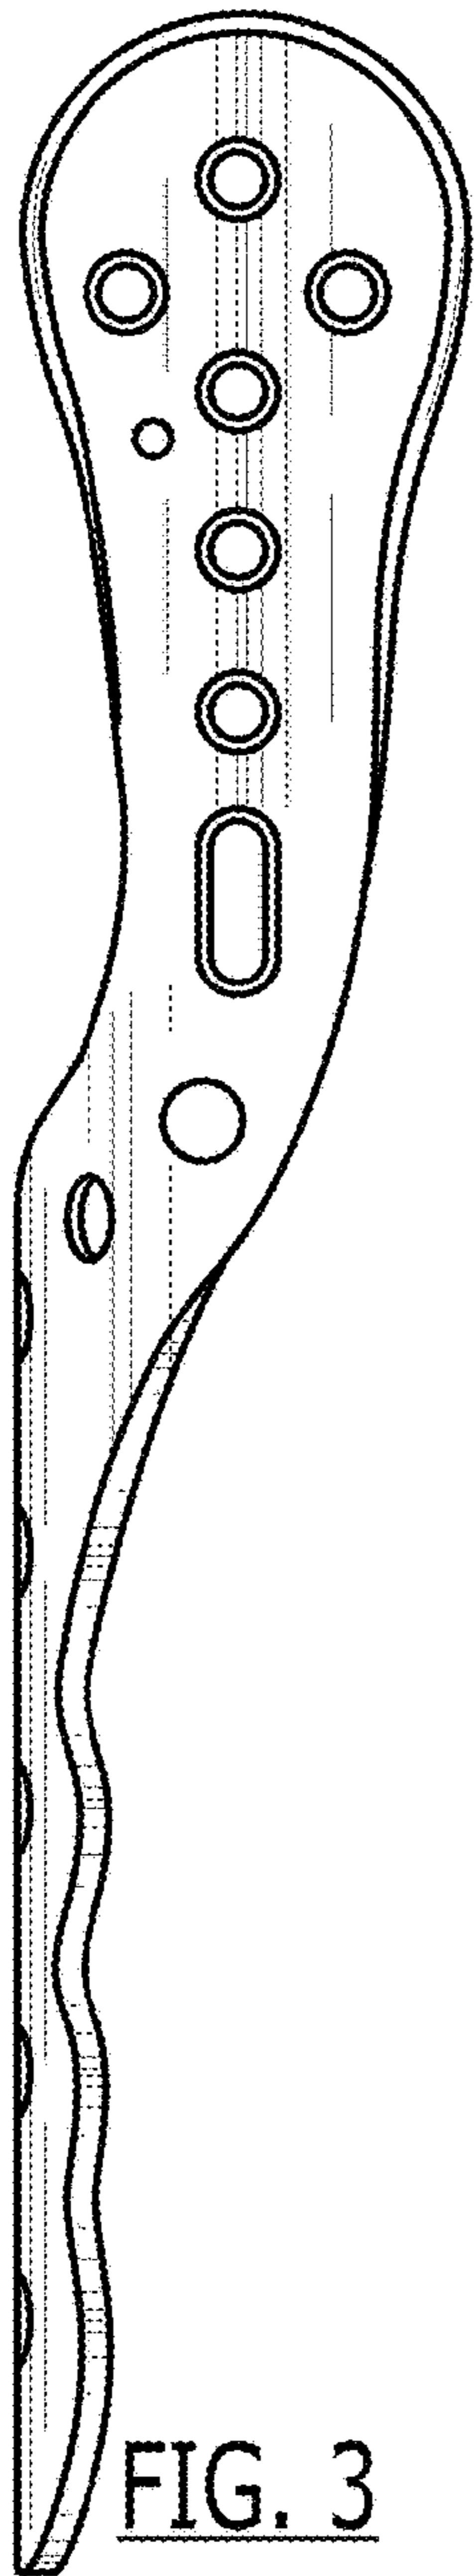


FIG. 3

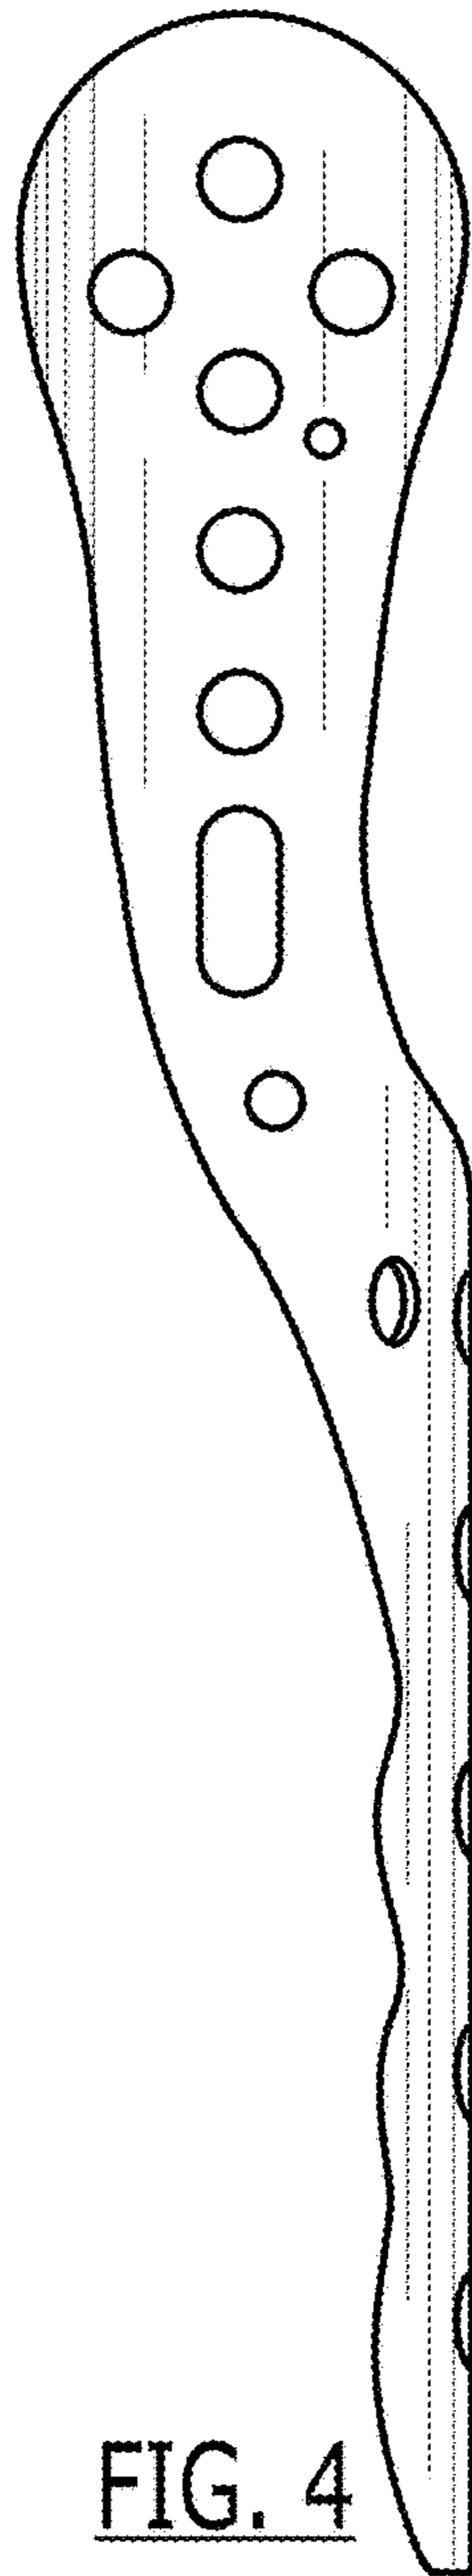


FIG. 4

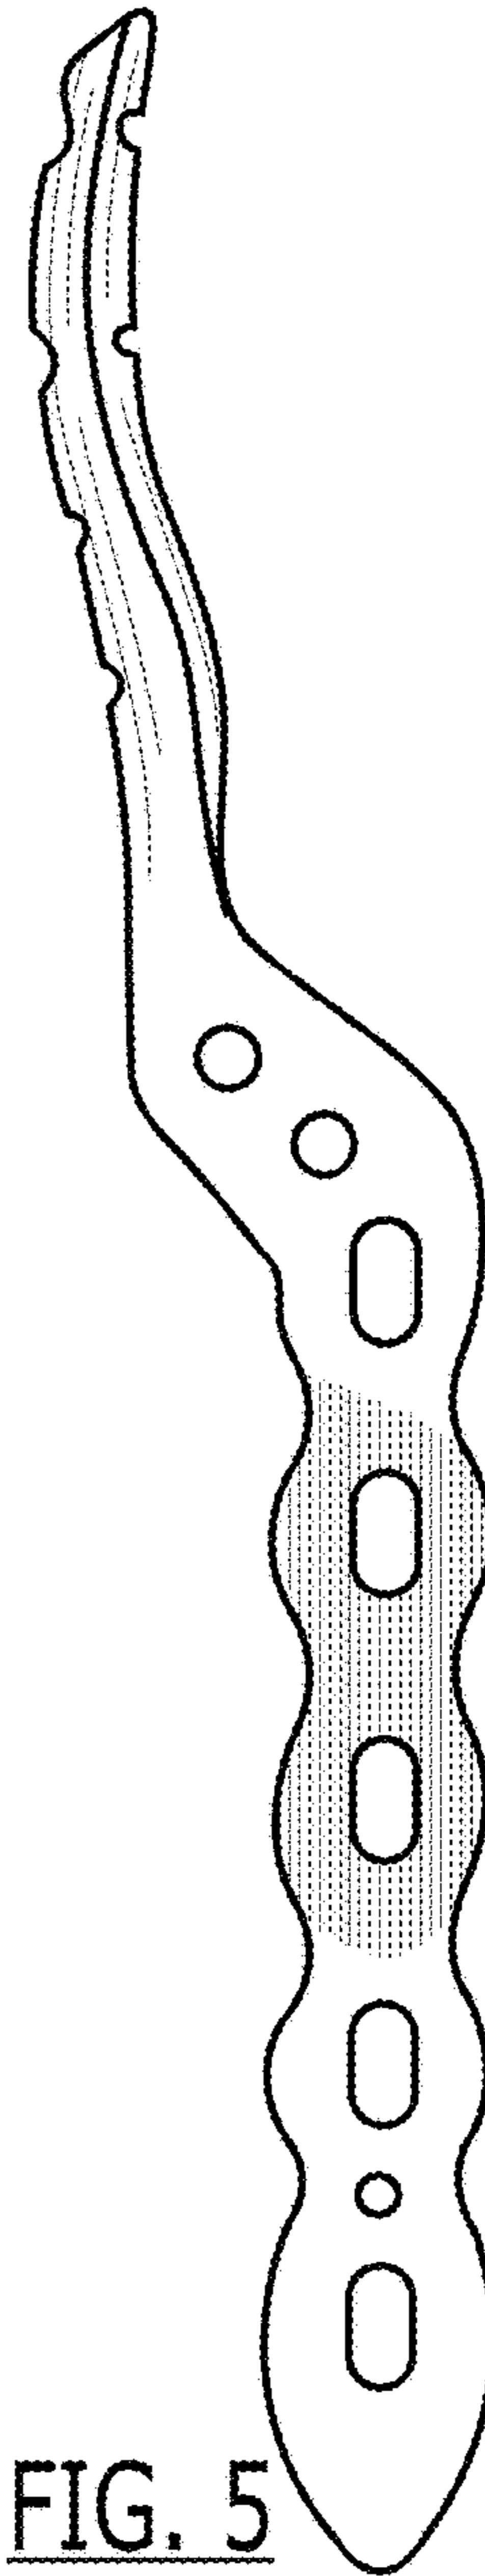


FIG. 5

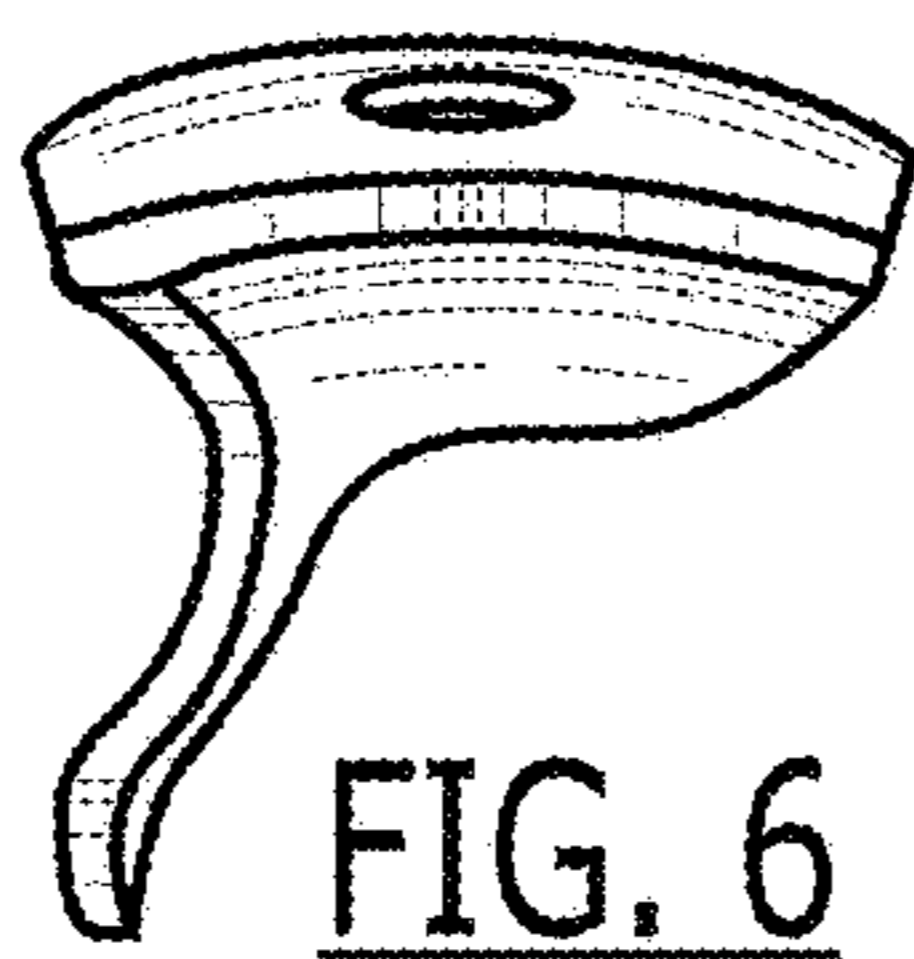


FIG. 6

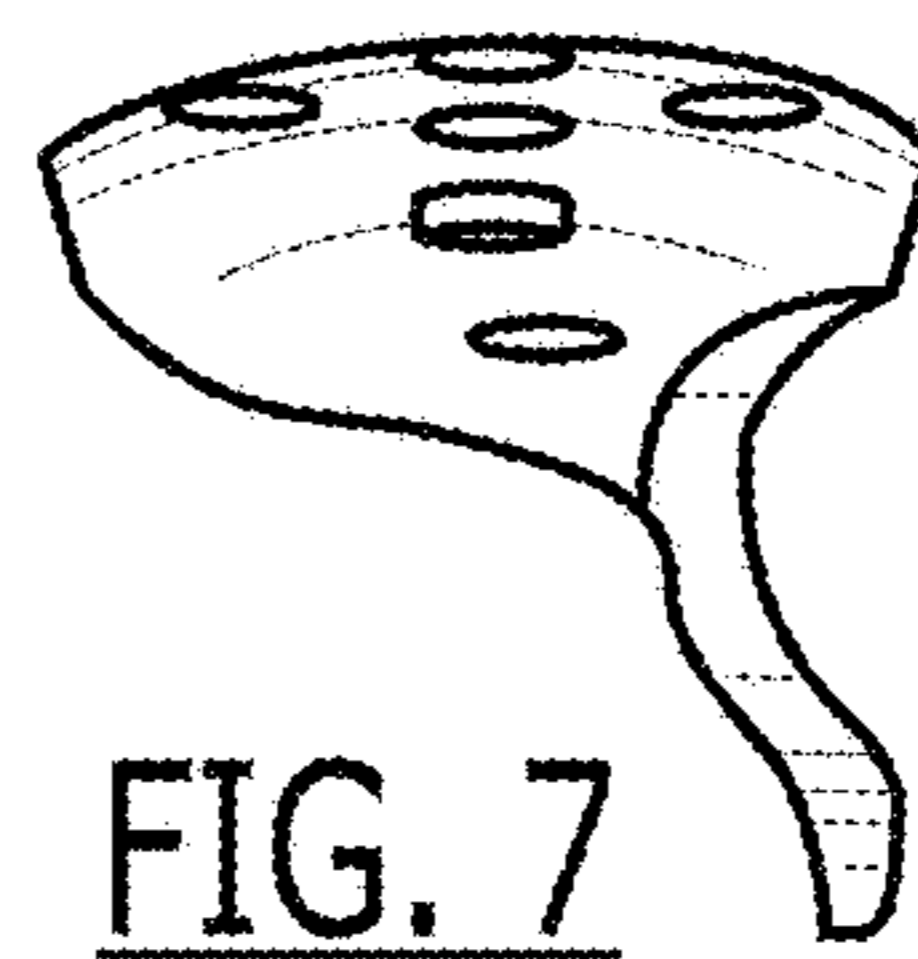


FIG. 7

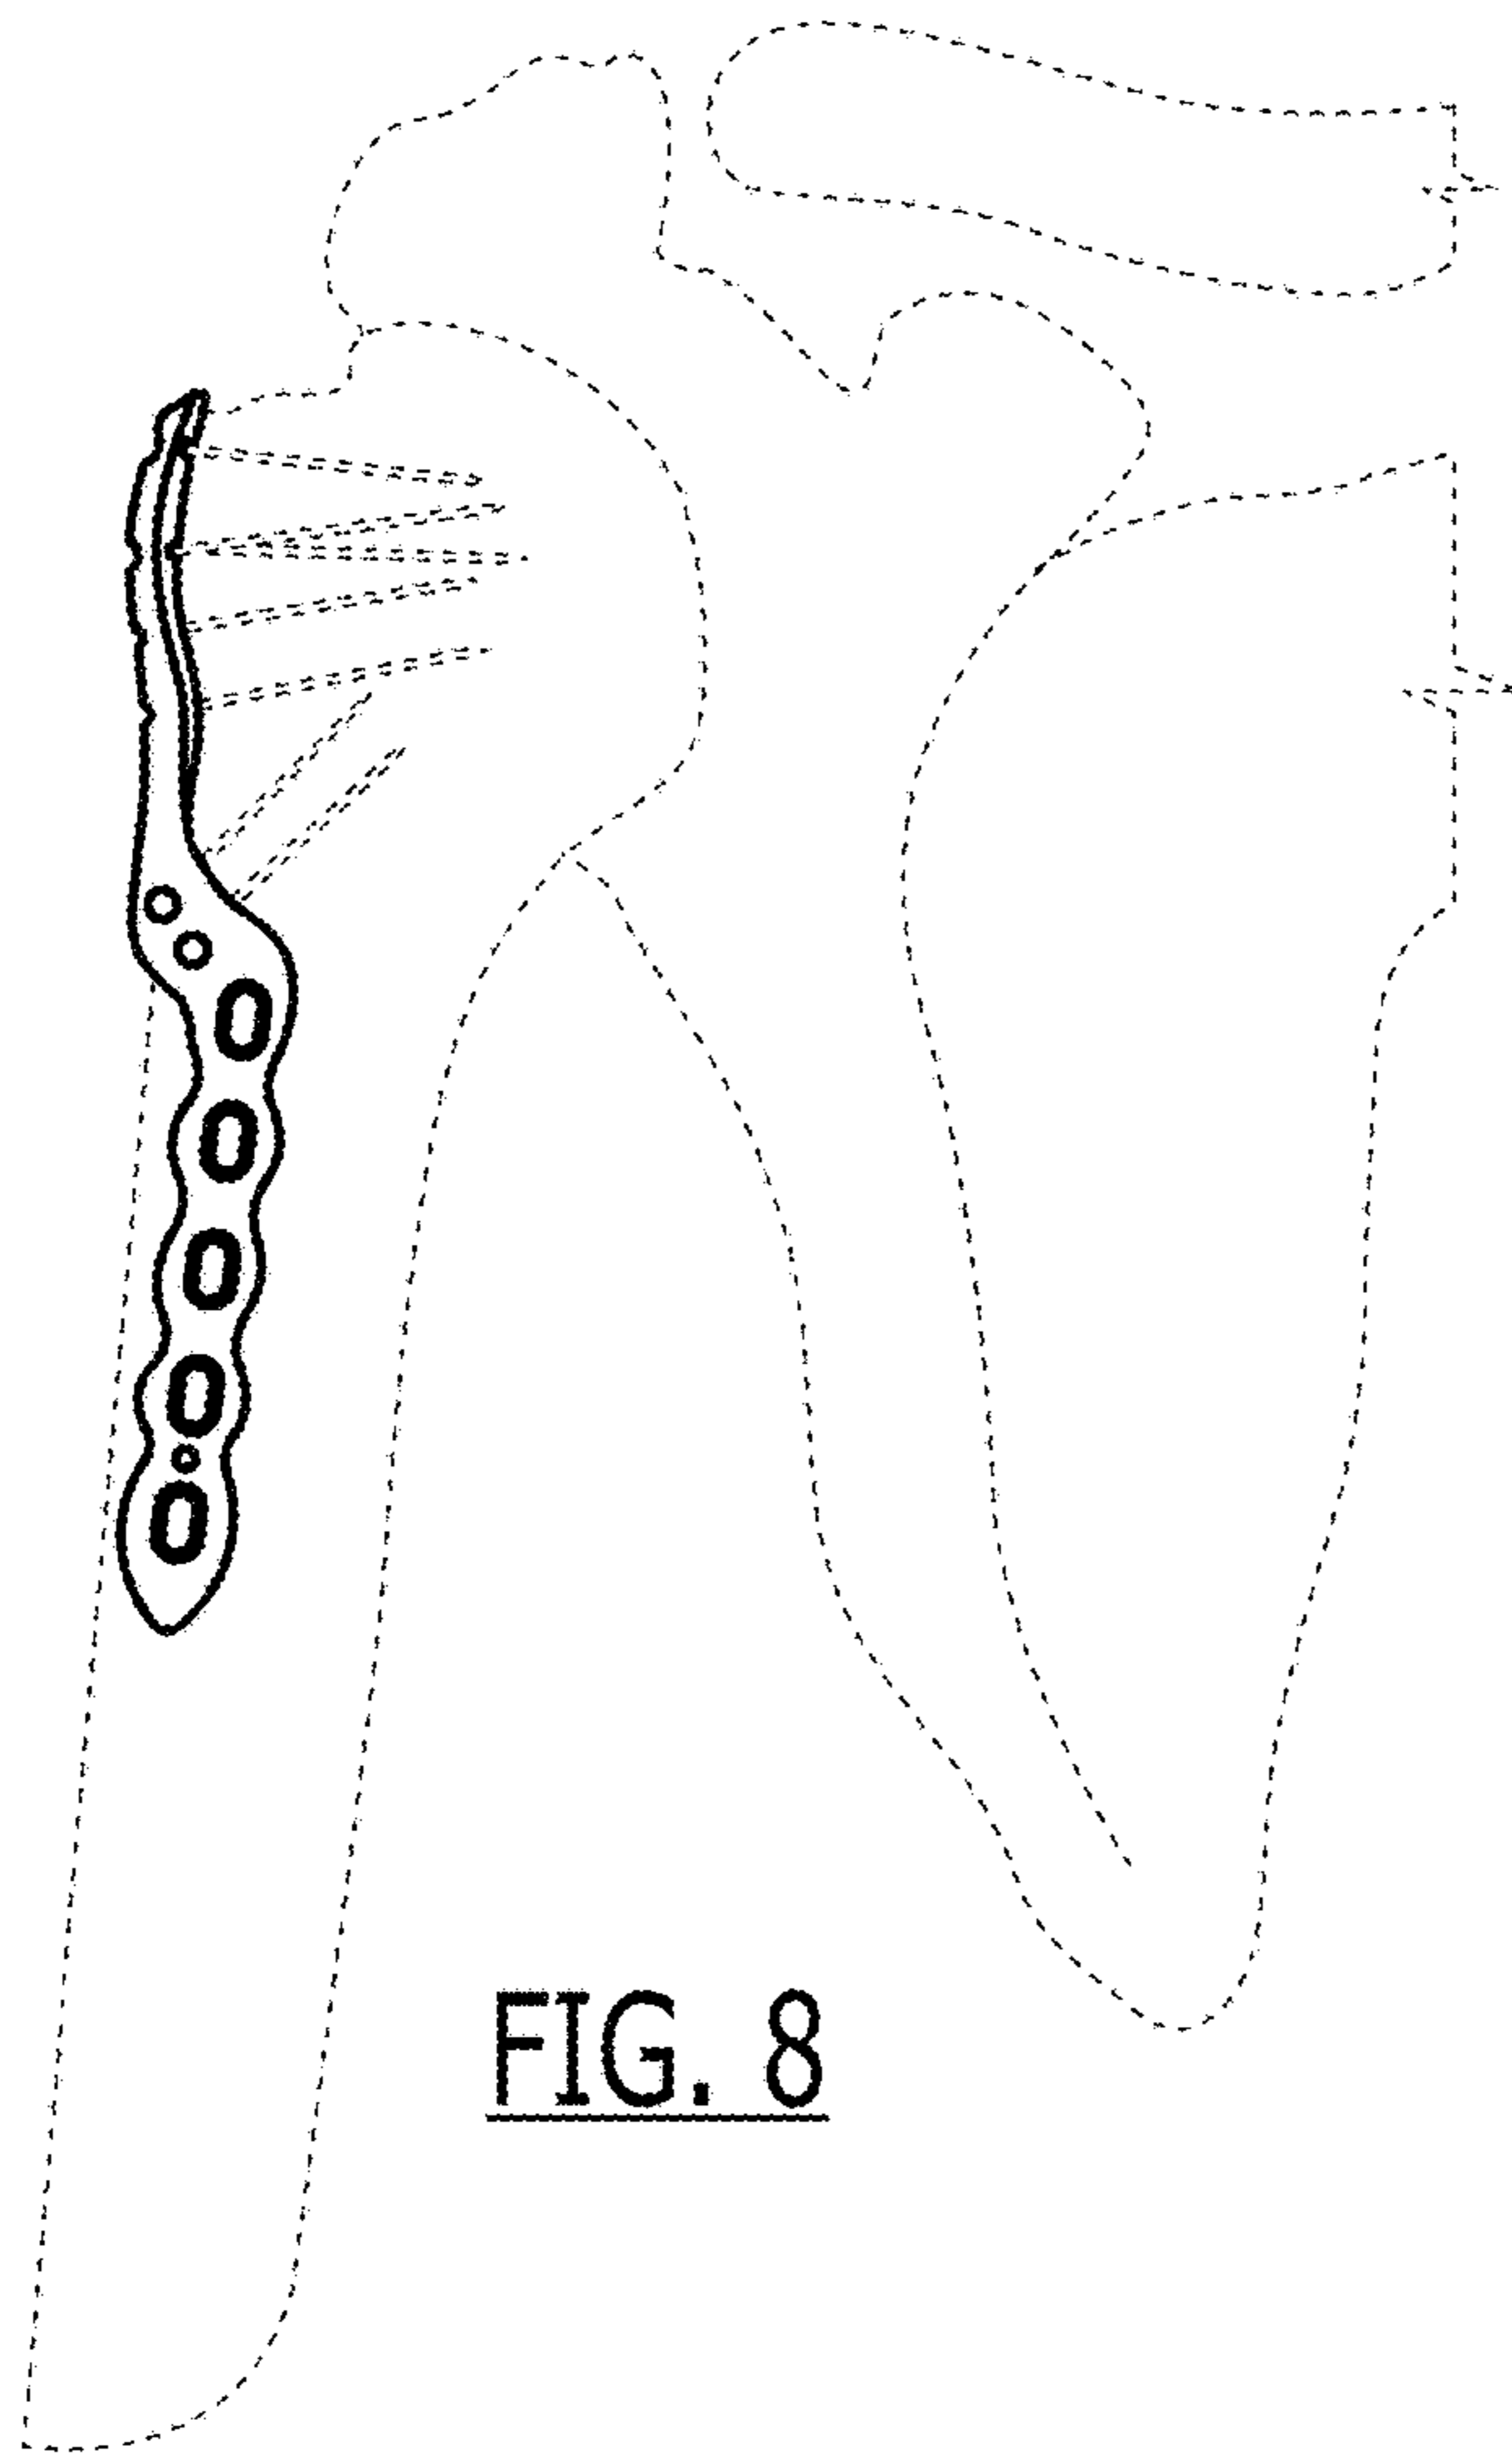


FIG. 8

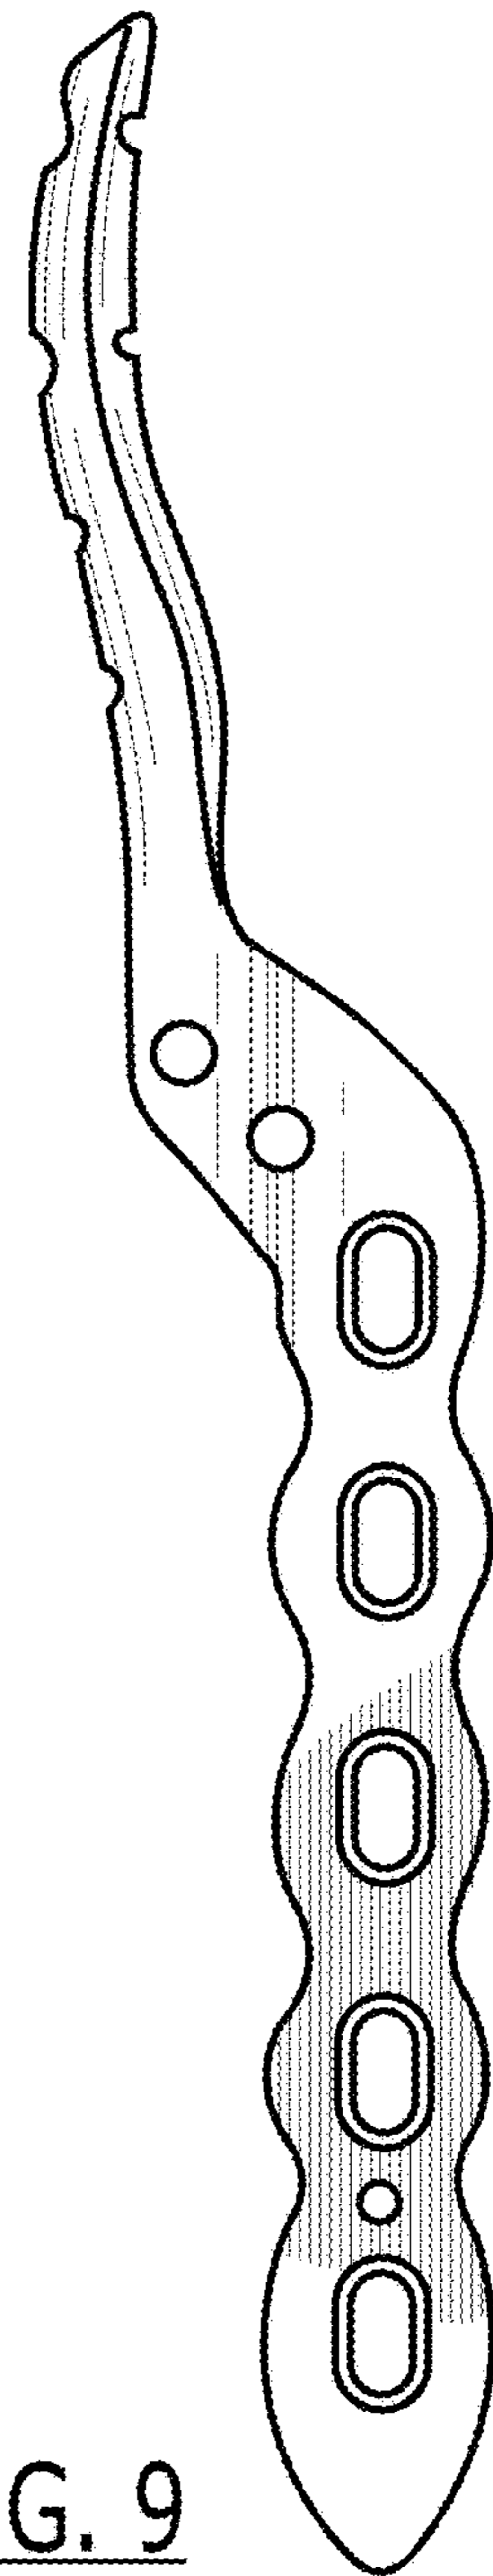


FIG. 9

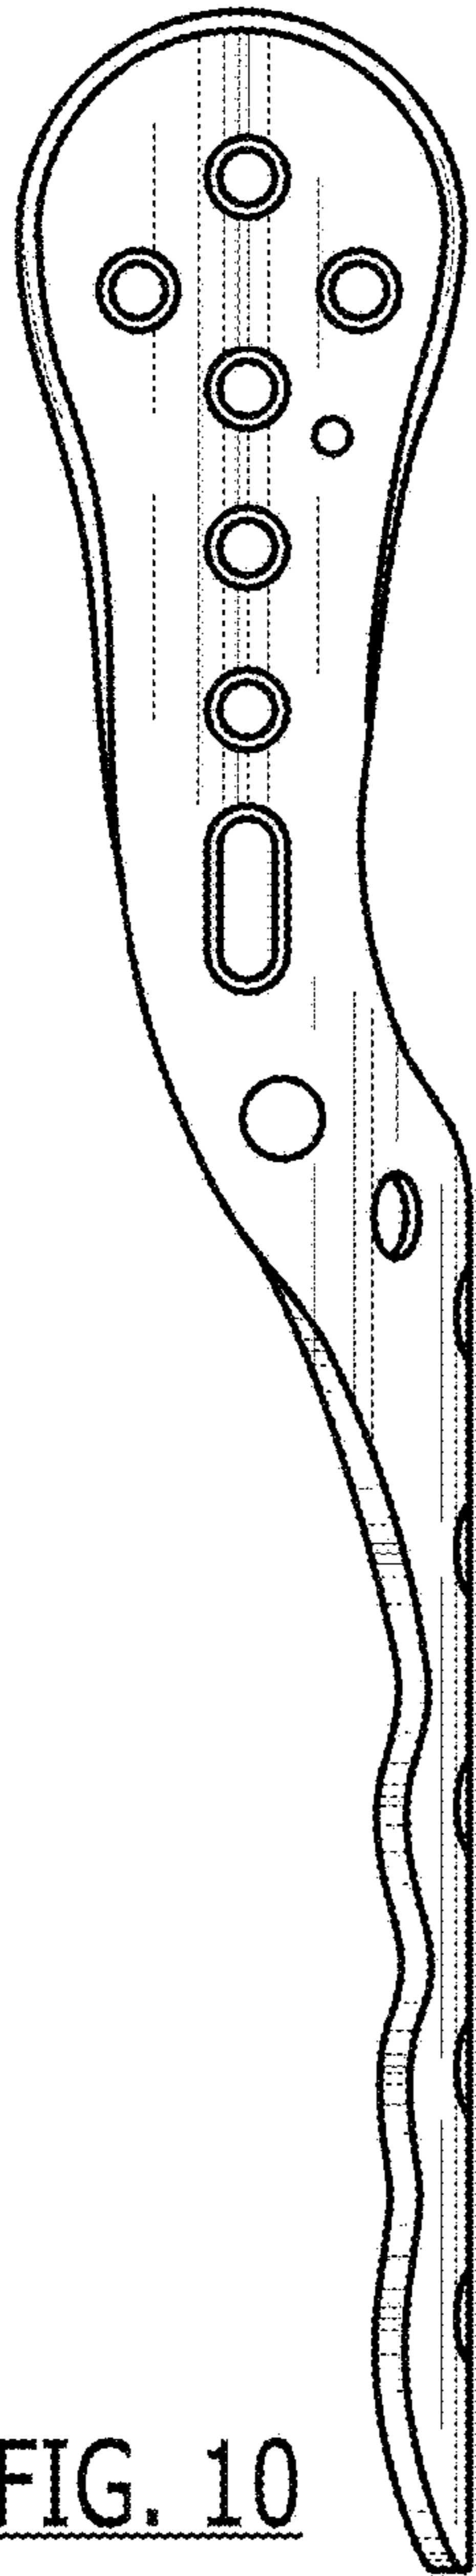


FIG. 10

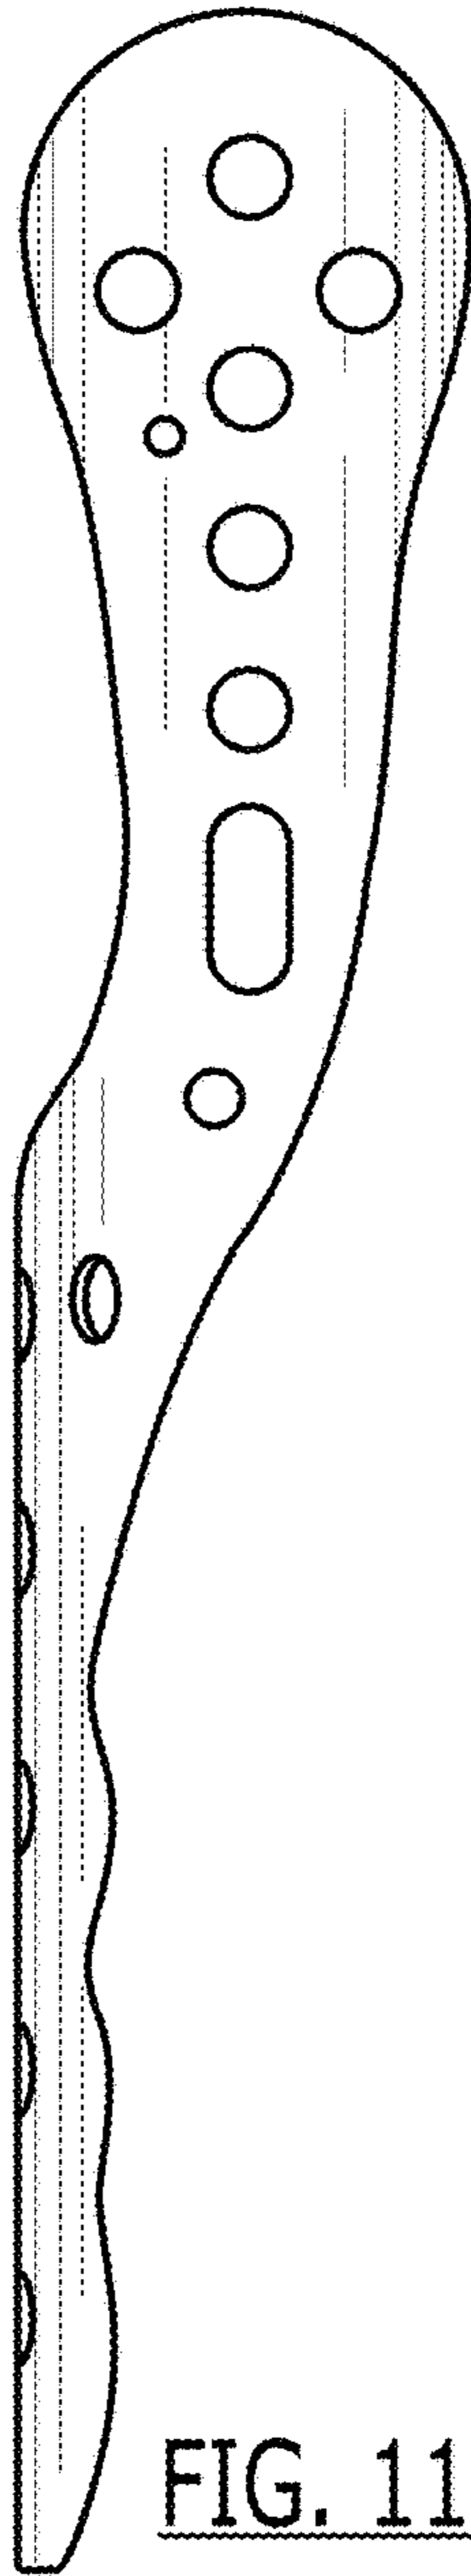


FIG. 11

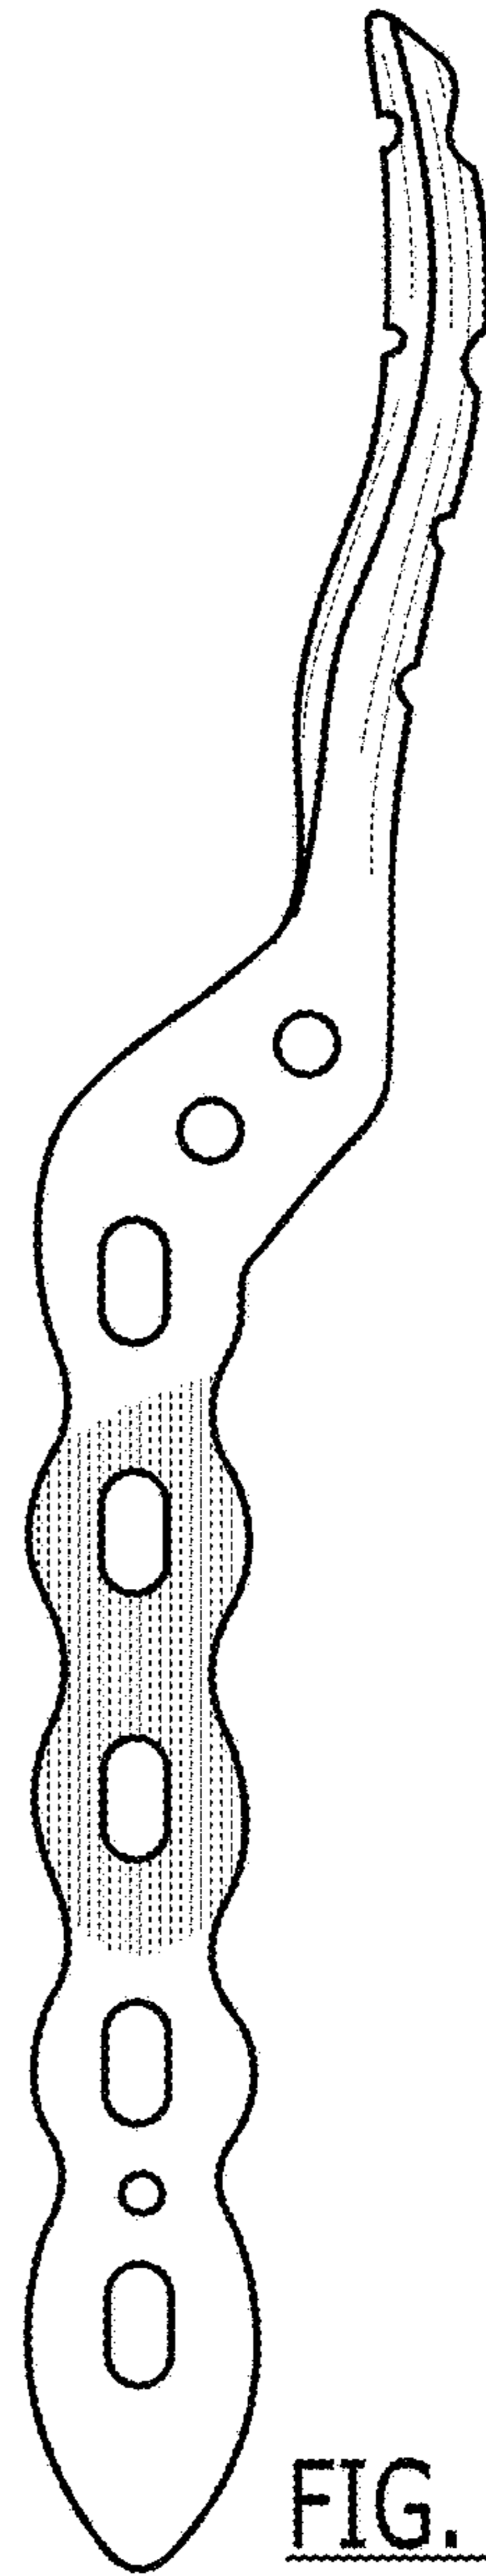


FIG. 12

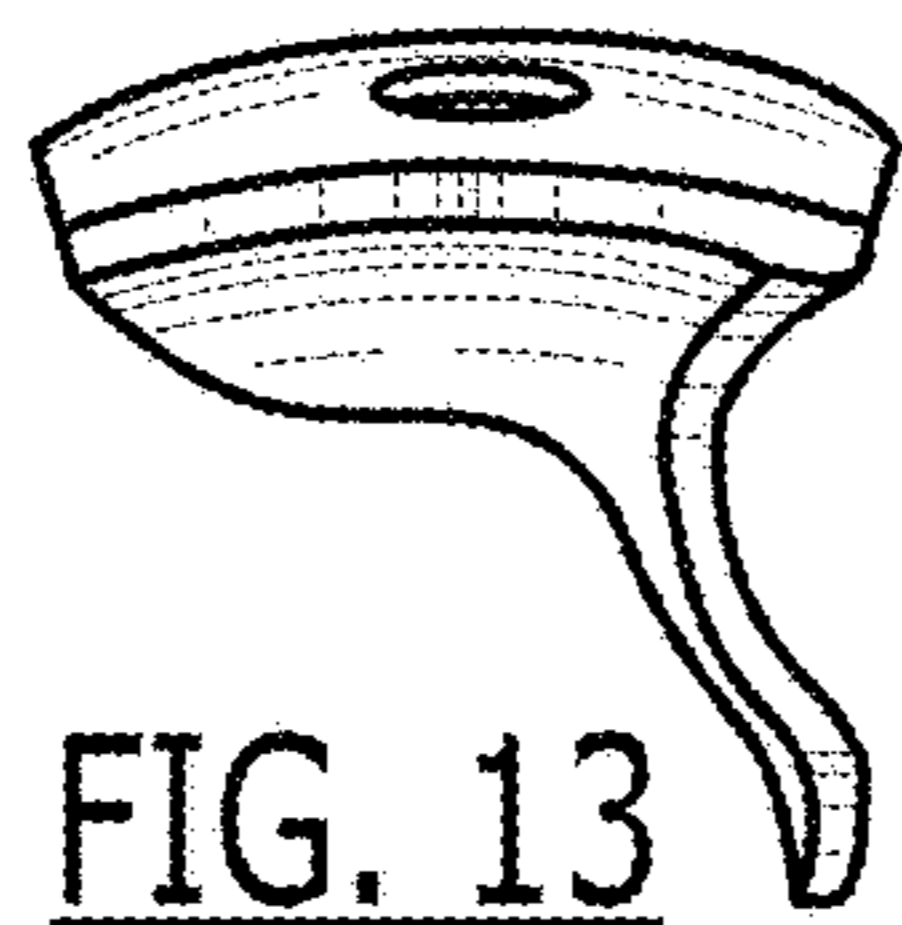


FIG. 13

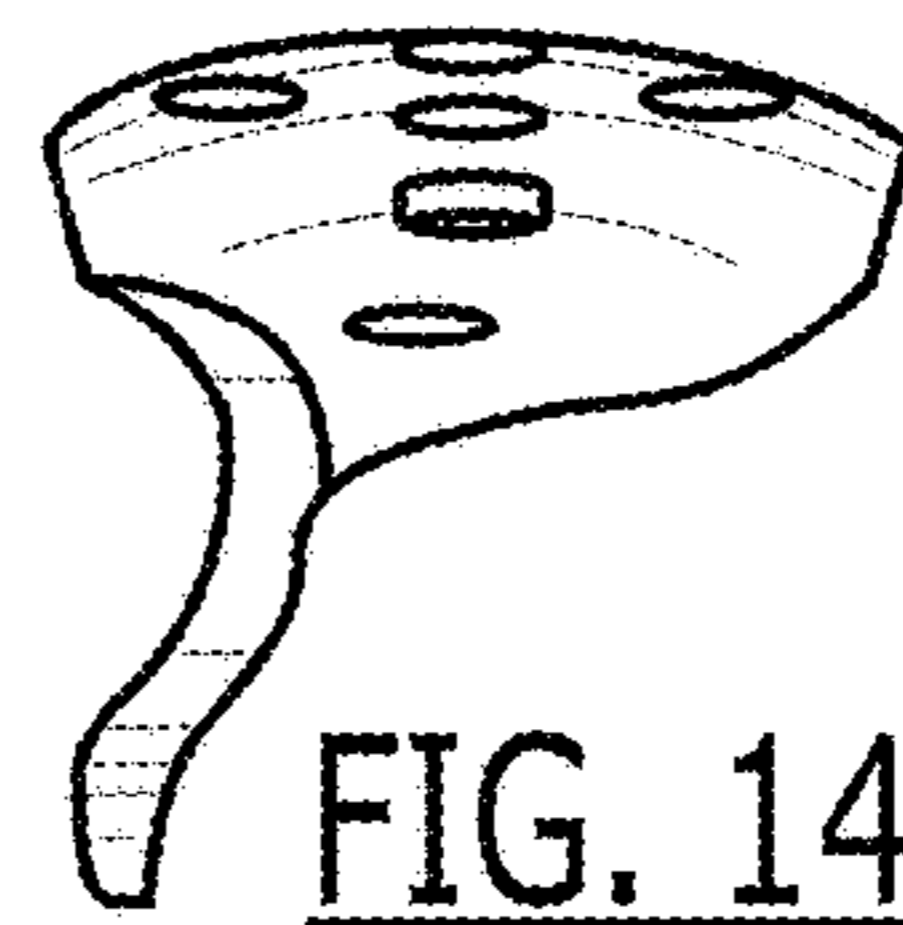


FIG. 14