



US00D817406S

(12) **United States Design Patent** (10) **Patent No.:** **US D817,406 S**
Rowe et al. (45) **Date of Patent:** **** May 8, 2018**

(54) **CLINICAL SIGNAGE FRAME** 1,483,874 A * 2/1924 Dey G09F 1/12 40/618
(71) Applicant: **Michael Graves & Associates,** 1,577,427 A * 3/1926 Smith G09F 15/0075 40/564
Princeton, NJ (US)
2,162,025 A 6/1939 McClaughry et al.
(72) Inventors: **Thomas Rowe,** Princeton, NJ (US); 2,812,605 A 11/1957 Whaley et al.
James Wisniewski, Buckingham, PA 4,379,341 A 4/1983 Toyooka et al.
(US) 4,679,341 A 7/1987 Goldman
(Continued)

(73) Assignee: **Michael Graves Design Group, Inc.,**
Princeton, NJ (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/544,159**

(22) Filed: **Oct. 30, 2015**

Related U.S. Application Data

(63) Continuation of application No. 14/664,156, filed on
Mar. 20, 2015, now abandoned.

(51) **LOC (11) Cl.** **20-03**

(52) **U.S. Cl.**
USPC **D20/43**

(58) **Field of Classification Search**
USPC D20/10, 19, 42, 43, 99; D6/300, 301
CPC G09F 1/00; G09F 1/03; G09F 1/12; G09F
3/00; G09F 3/18; G09F 3/185; G09F
3/20; G09F 3/201; G09F 7/00; G09F
7/02; G09F 7/08; G09F 7/10; G09F
2001/106; G09F 2007/1843; G09F
2007/1856; G09F 11/00; G07F 3/18
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

252,408 A * 1/1882 Wilbur G09F 1/12 232/33
316,527 A * 4/1885 Cushman G09F 3/18 40/653

OTHER PUBLICATIONS

Non Final Office Action, U.S. Appl. No. 14/664,156, dated Nov. 3,
2016, 9 pages.

Primary Examiner — Mary Ann Calabrese

(74) *Attorney, Agent, or Firm* — Kilpatrick Townsend &
Stockton LLP

(57) **CLAIM**

The ornamental design for a clinical signage frame, as
shown and described.

DESCRIPTION

FIG. 1 is a right perspective view of the clinical signage
frame.

FIG. 2 is a left perspective view of the clinical signage frame
of FIG. 1.

FIG. 3 is a front view of the clinical signage frame of FIG.
1.


FIG. 4 is rear view of the clinical signage frame of FIG. 1.
FIG. 5 is a right side view of the clinical signage frame of
FIG. 1.

FIG. 6 is a left side view of the clinical signage frame of
FIG. 1.

FIG. 7 is a bottom view of the clinical signage frame of FIG.
1; and,

FIG. 8 is a top view of the clinical signage frame of FIG. 1.
The broken lines form no part of the claimed design.

1 Claim, 6 Drawing Sheets

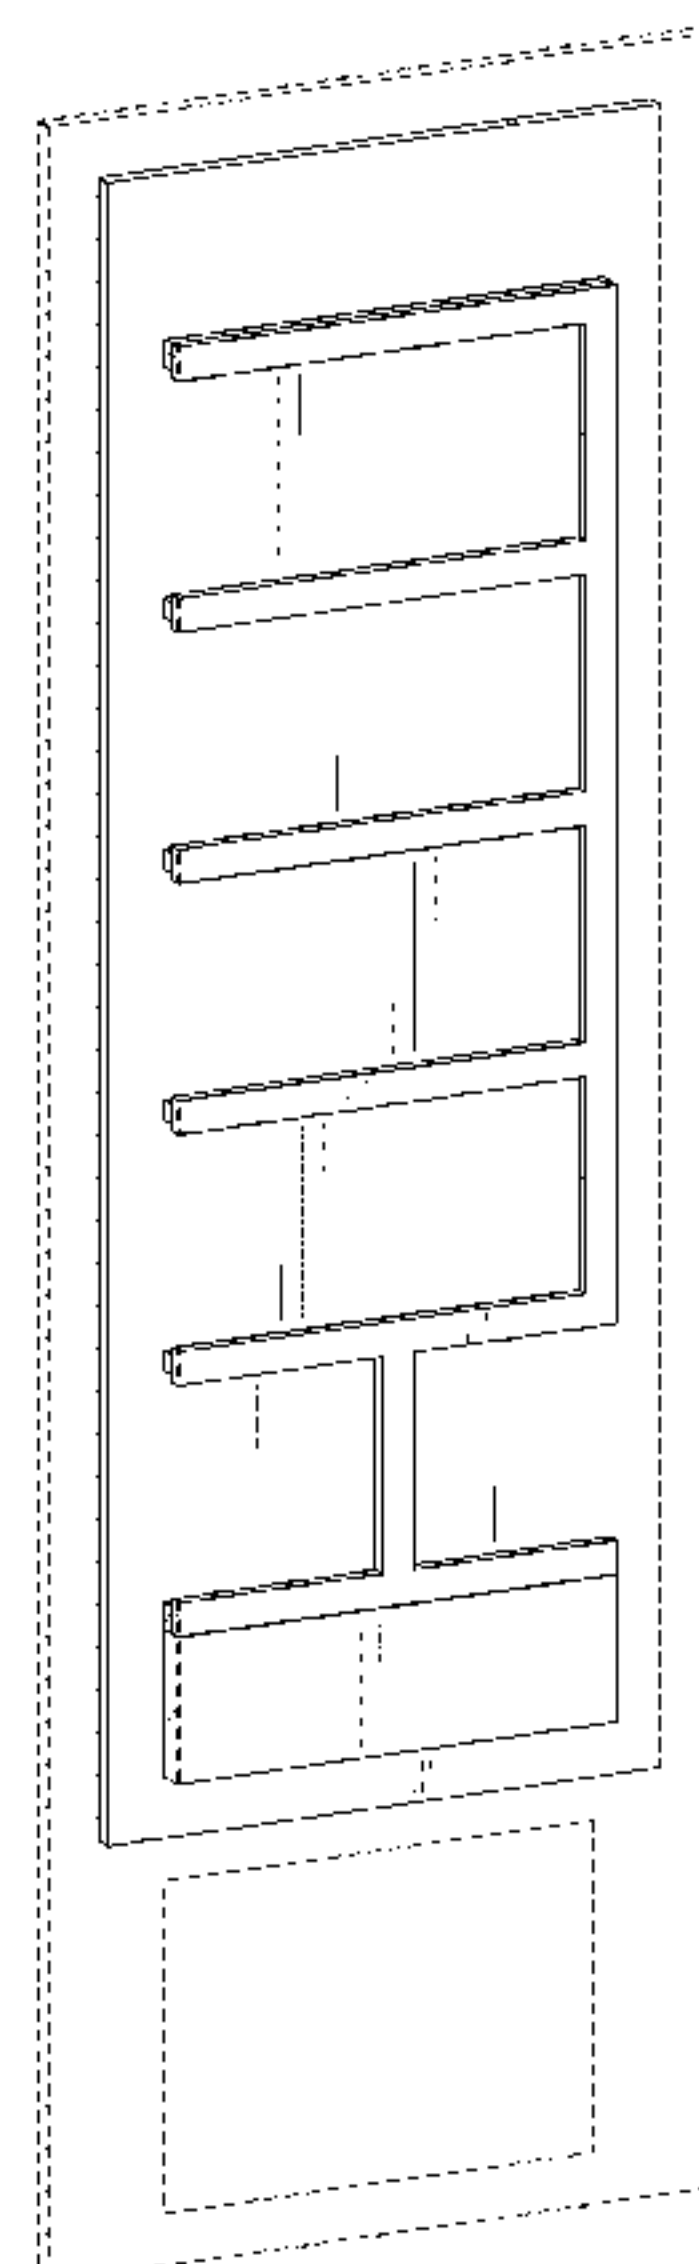

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,257,472	A *	11/1993	Harnois		G09F 3/202
					40/607.14
7,981,381	B2	7/2011	Lurvey et al.		
2010/0199532	A1	8/2010	Blue et al.		
2012/0272553	A1	11/2012	Bell et al.		
2015/0269873	A1	9/2015	Rowe et al.		

* cited by examiner

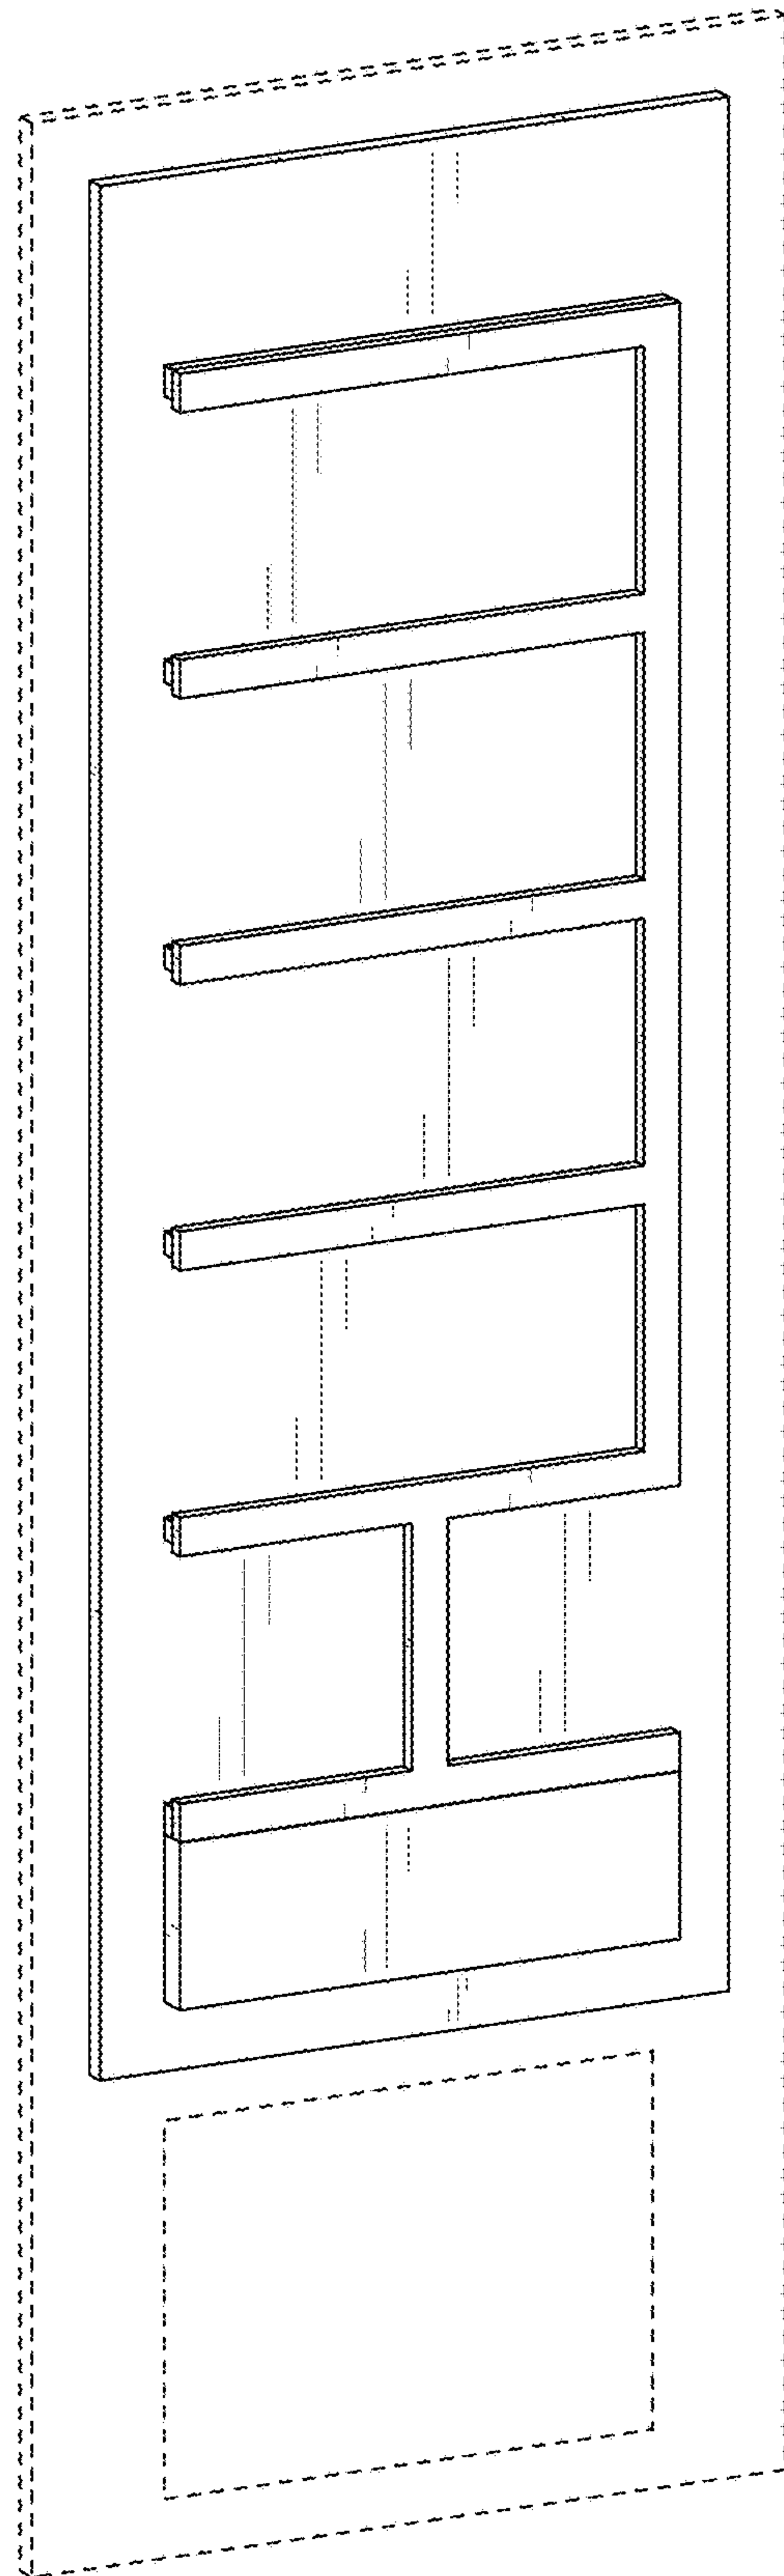


FIG. 1

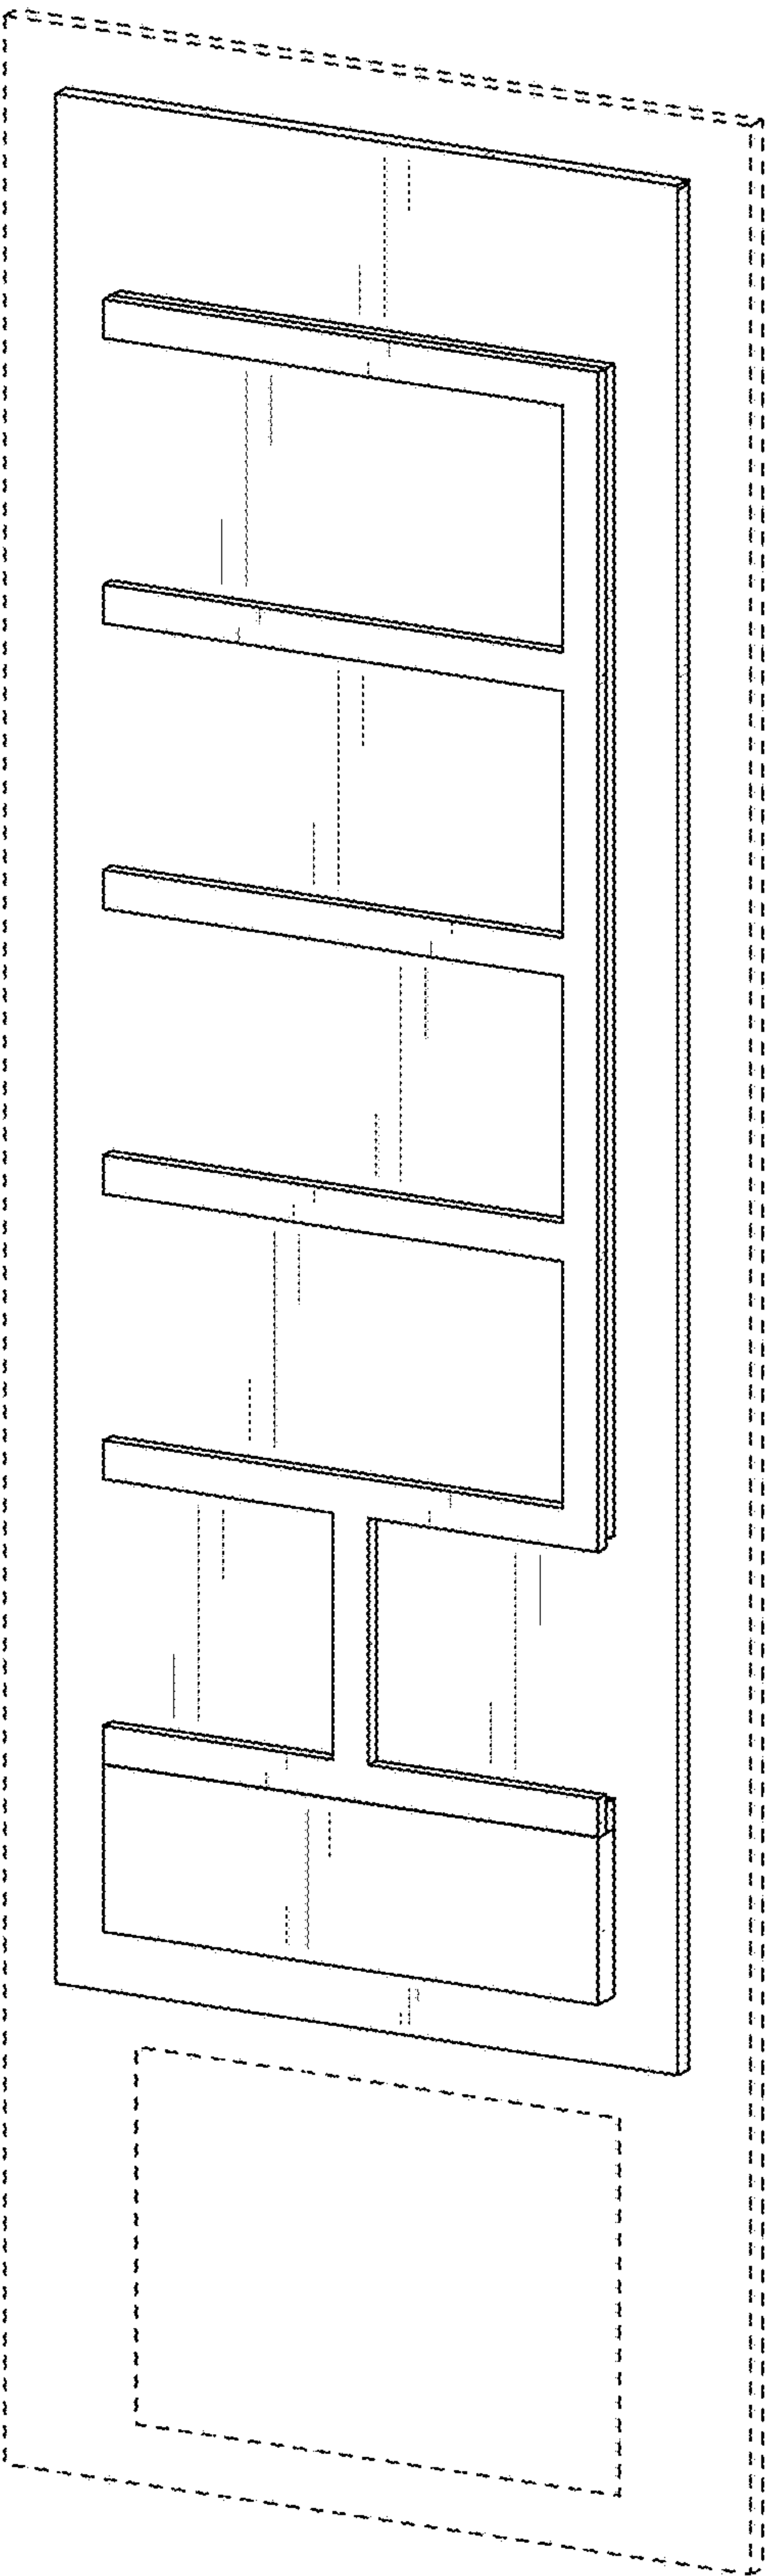


FIG. 2

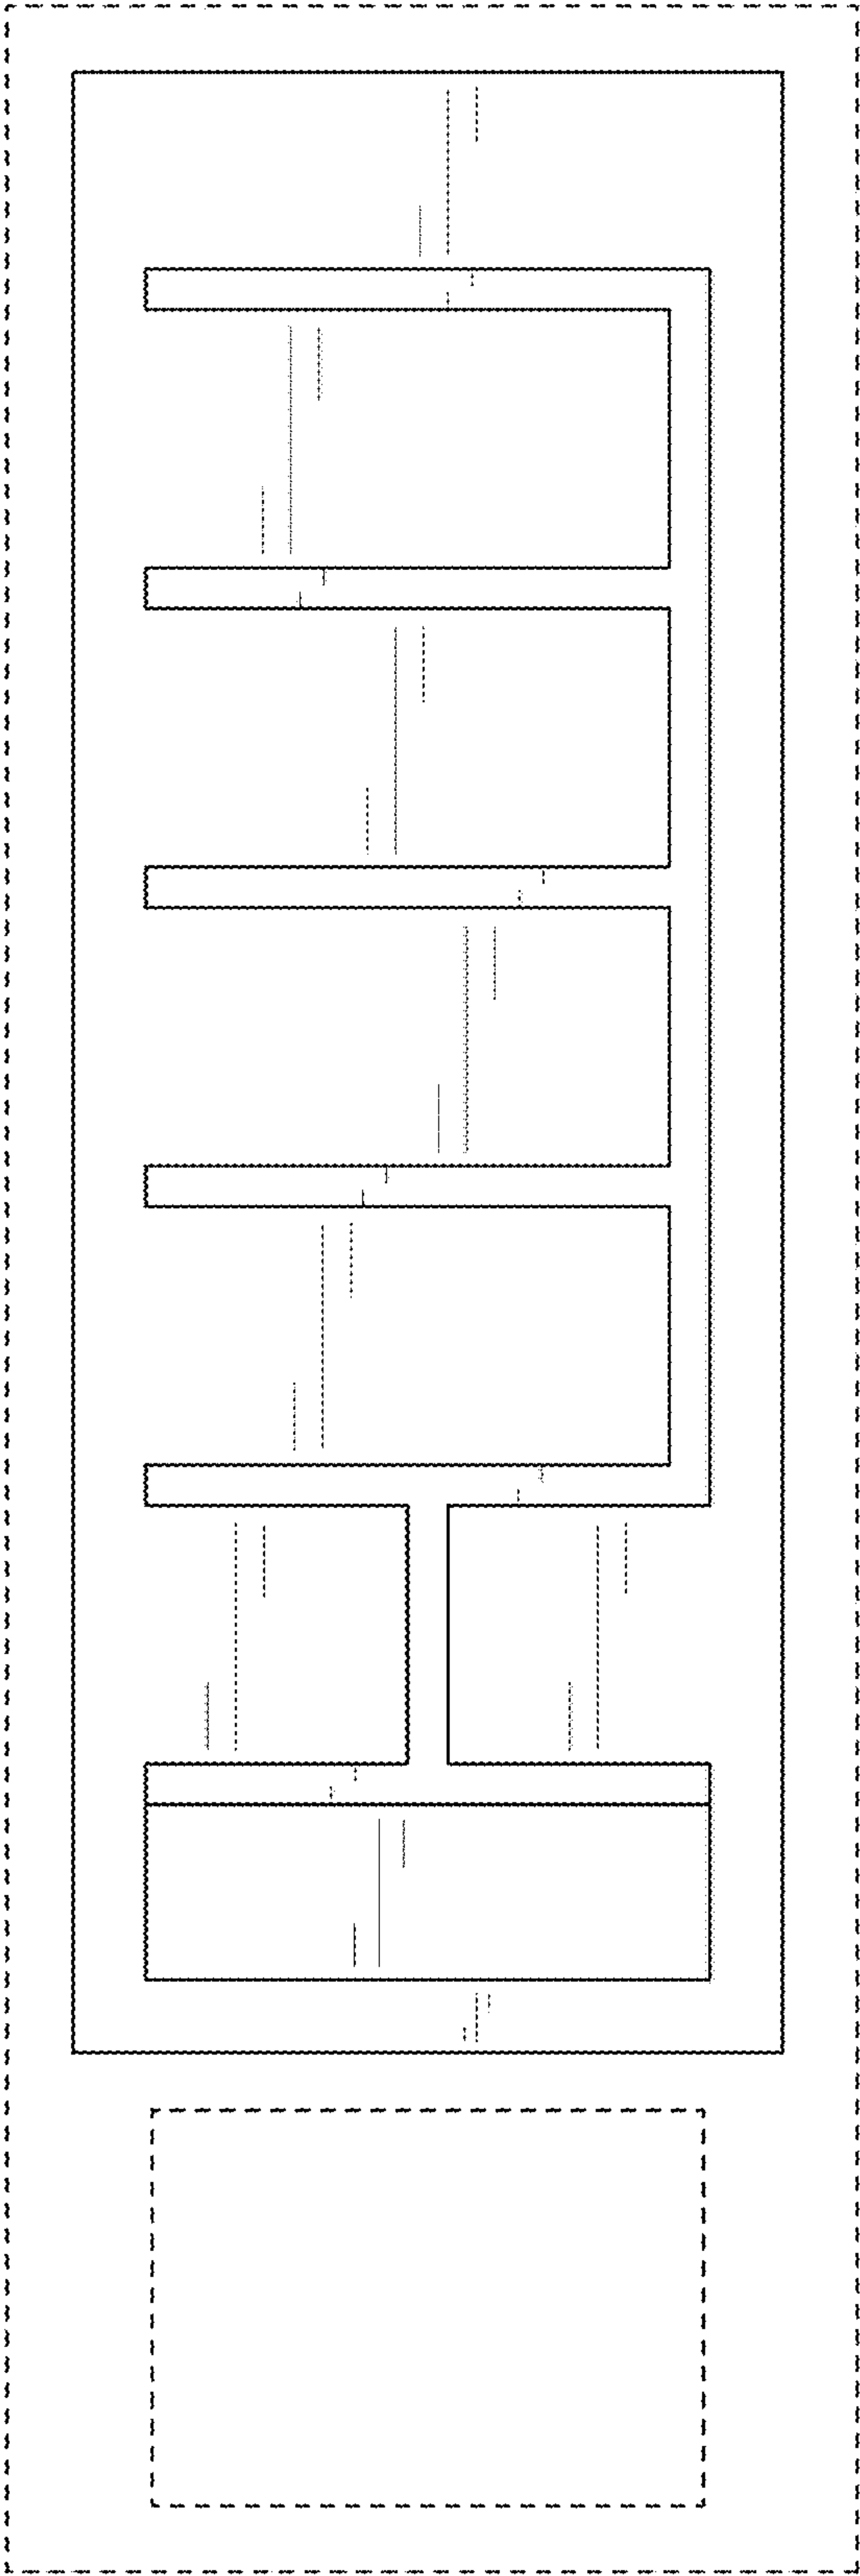


FIG. 3

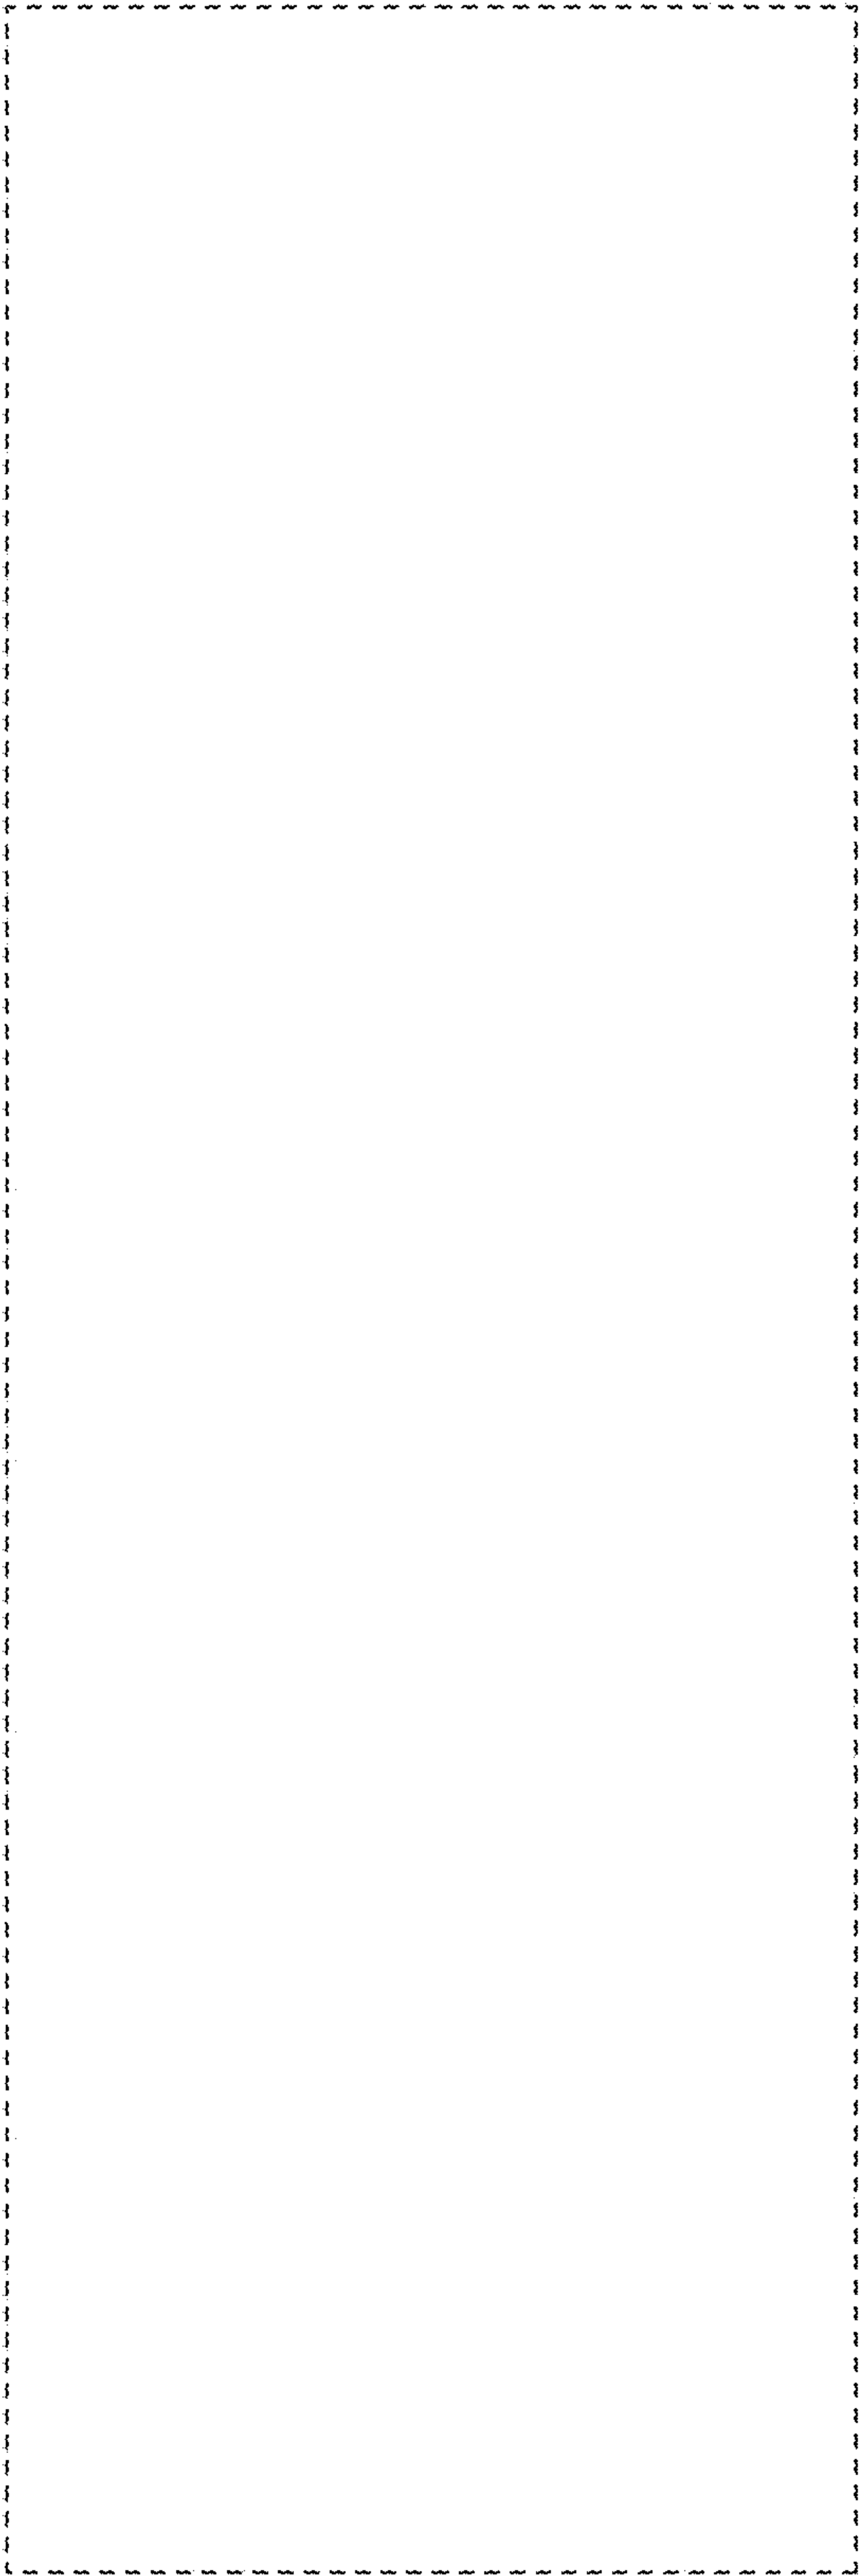


FIG. 4



FIG. 5



FIG. 6

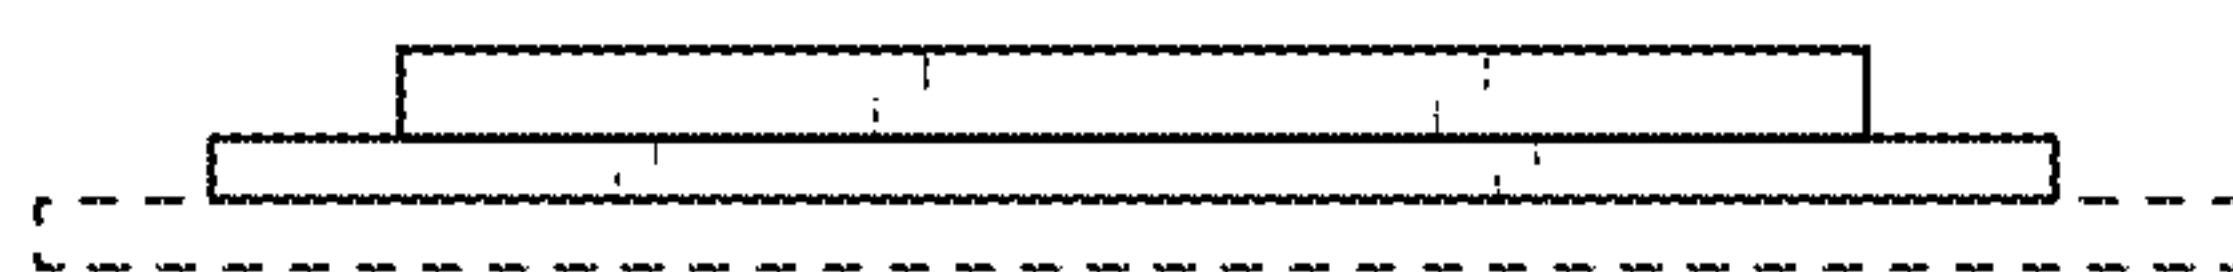


FIG. 7

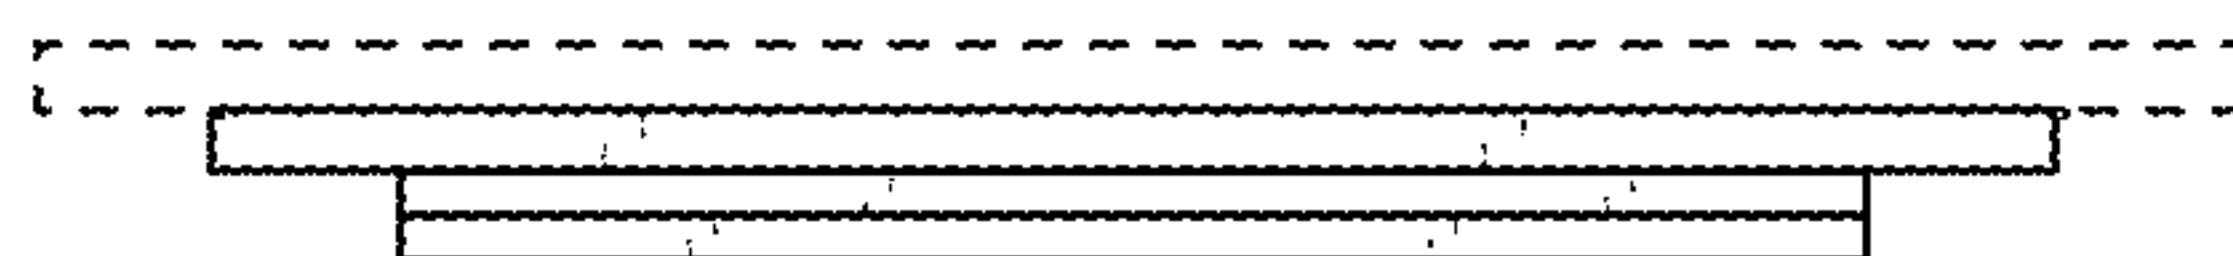


FIG. 8