



US00D818594S

(12) **United States Design Patent** (10) **Patent No.:** **US D818,594 S**
Asai et al. (45) **Date of Patent:** **** May 22, 2018**

(54) **MEDICAL PROBE**
(71) Applicant: **KONICA MINOLTA, INC.**,
Chiyoda-ku, Tokyo (JP)
(72) Inventors: **Tomonari Asai**, Hachioji (JP);
Kenichiro Uchihara, Nagareyama (JP)
(73) Assignee: **KONICA MINOLTA, INC.**,
Chiyoda-ku, Tokyo (JP)

D687,153 S * 7/2013 Torzilli D24/187
D701,606 S * 3/2014 Ohmukai D24/187
D703,331 S * 4/2014 Kitayama D24/187
(Continued)

FOREIGN PATENT DOCUMENTS

JP 1095570 S 1/2001
JP 1133882 H 2/2002
(Continued)

OTHER PUBLICATIONS

Linear “hockey stick” ultrasound transducer, posted at medicalexpo.com, available Nov. 20, 2015, © 2017, [online], visited Sep. 11, 2017, URL:<http://www.medicalexpo.com/prod/zonare-medical-systems/product-70629-532063.html>.
(Continued)

(**) Term: **15 Years**
(21) Appl. No.: **29/571,831**
(22) Filed: **Jul. 22, 2016**
(30) **Foreign Application Priority Data**

Feb. 1, 2016 (JP) 2016-002017

(51) **LOC (11) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164,
D24/165, 167, 170, 186–187; D10/57,
D10/60, 78, 80; 600/407, 439, 446, 459,
600/461; 378/98.7, 98.8, 189
CPC A61B 8/445; A61B 8/4455; A61B 8/4461;
A61B 5/0095; A61B 8/4483; A61B 8/46
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,381,795 A * 1/1995 Nordgren A61B 8/06
600/459
5,482,047 A * 1/1996 Nordgren A61B 8/06
174/263
D369,307 S * 4/1996 Imling D10/78
D616,992 S * 6/2010 Kitayama D24/186
D638,946 S * 5/2011 Egorov D24/187

Primary Examiner — Anhdao Doan
Assistant Examiner — Mary Malley
(74) *Attorney, Agent, or Firm* — Buchanan Ingersoll & Rooney PC


(57) **CLAIM**

The ornamental design for a medical probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical probe;
FIG. 2 is a front view thereof, the opposite side being a mirror image of the side shown herein;
FIG. 3 is a left side view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a top view thereof;
FIG. 6 is a bottom view thereof; and,
FIG. 7 is an enlarged cross-sectional view taken along line 7-7 in FIG. 2 in which the internal mechanism is omitted thereof.
The broken lines show portions of the medical probe that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

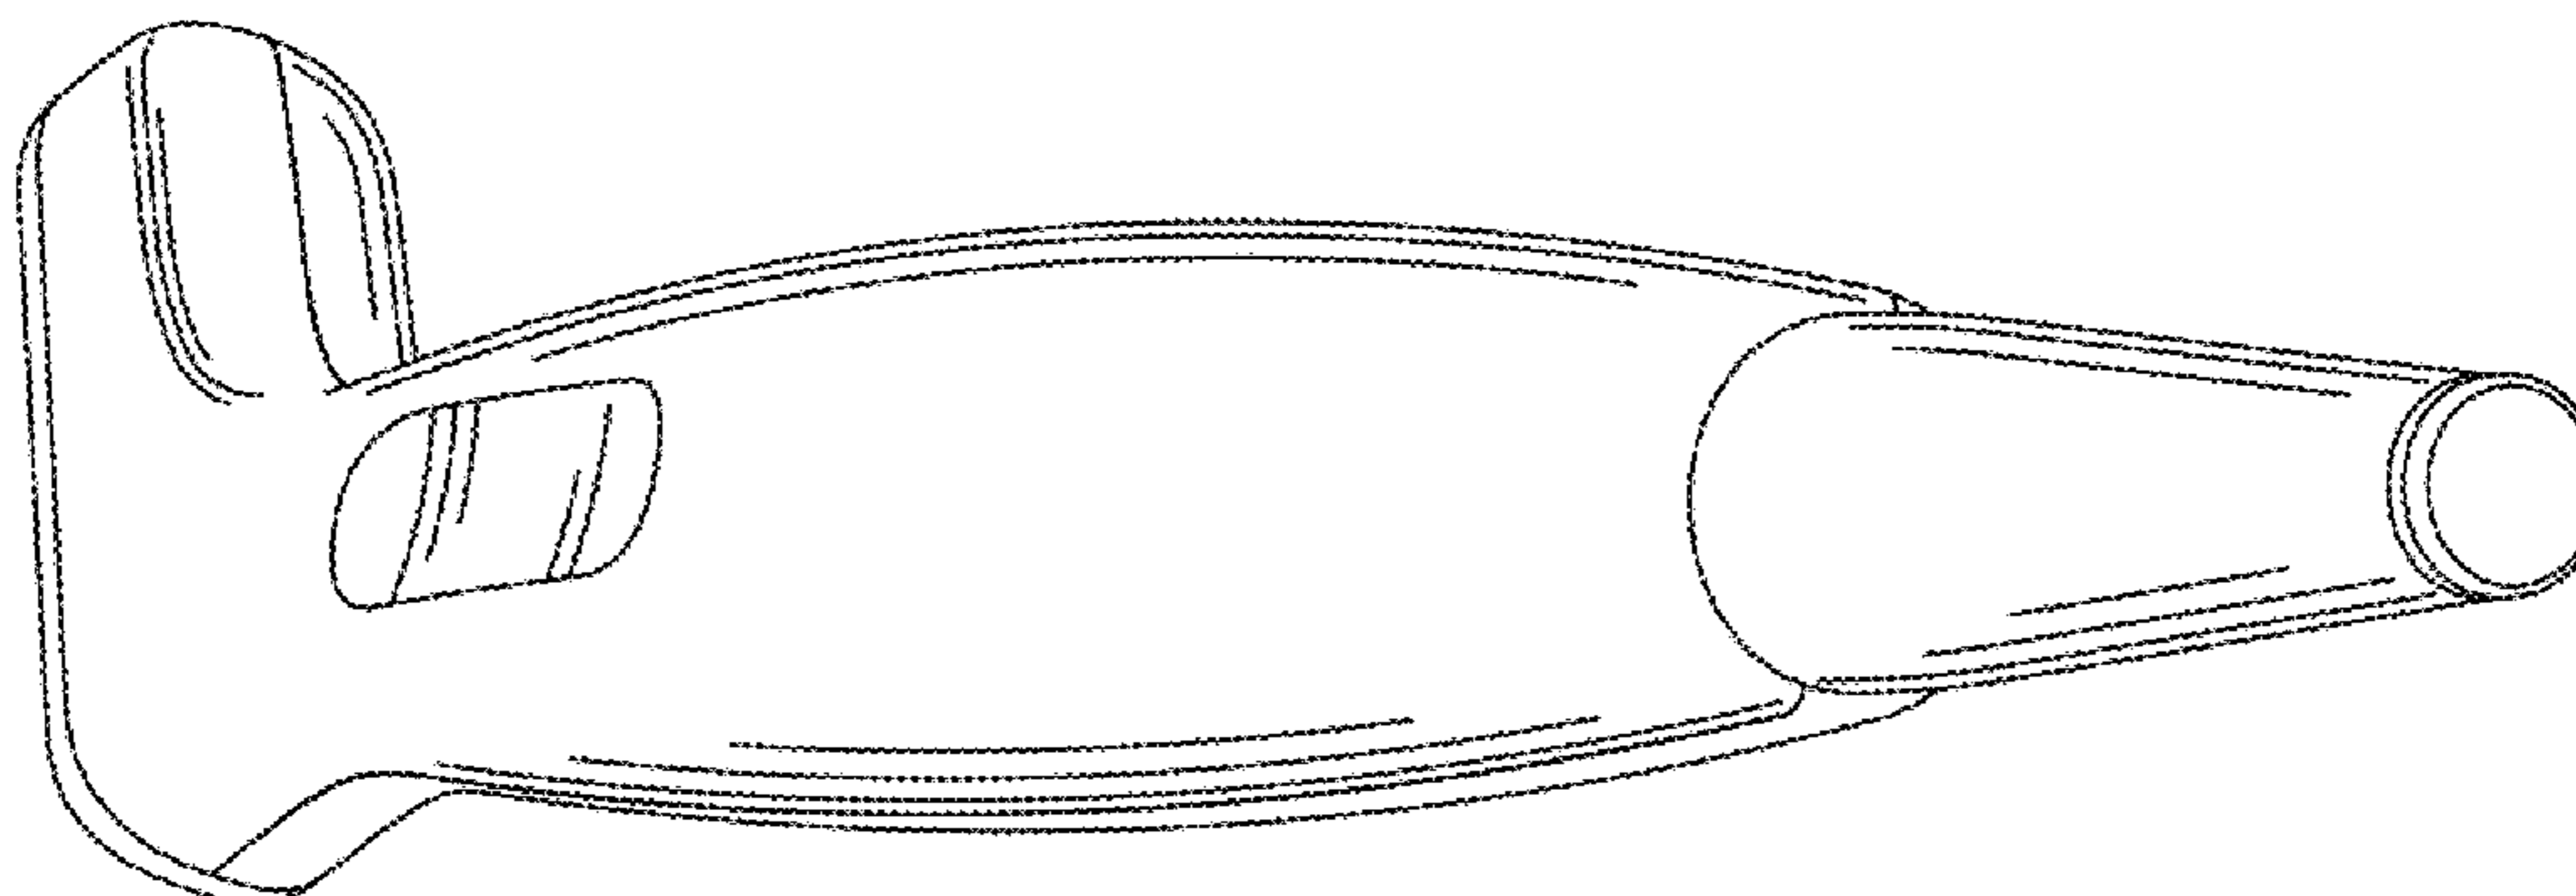

(56)

References Cited

U.S. PATENT DOCUMENTS

D703,333 S	*	4/2014	Saeki	D24/187
D728,802 S	*	5/2015	Matsumura	D24/187
D729,166 S	*	5/2015	Baba	D13/133
D748,808 S	*	2/2016	Matsumura	D24/187
D782,684 S	*	3/2017	Pippel	D24/186

FOREIGN PATENT DOCUMENTS

JP	1386815 J	5/2010
JP	1515349 J	1/2015

OTHER PUBLICATIONS

An introduction to small animal veterinary probes, posted at bcftechnology.co.uk, posted Aug. 24, 2016, © BCF Technology, [online], visited Sep. 11, 2017, URL:<https://www.bcftechnology.co.uk/8931>.*

Imaging of the Hand, posted at radiologykey.com, posted on Jan. 17, 2016, [online], visited Sep. 11, 2017, URL:<https://radiologykey.com/imaging-of-the-hand/>.*

Acuson S1000 14L5 sp Transducer, posted at umiultrasound.com, posting date not available, © 2015 [online], visited Sep. 11, 2017, URL:<http://www.umiultrasound.com/ultrasound-transducers/acuson/acuson-s1000/1205-1415-sp-transducer>.*

L8-18i-D Probe, posted at services.gehealthcare.com, no posting date available, © 2017 General Electric Company, [online], visited Sep. 12, 2017, URL:<https://services.gehealthcare.com/gehcstorefront/p/5410798>.*

Office Action (Notification of Reason(s) for Refusal) dated Sep. 20, 2016, by the Japanese Patent Office in Japanese Patent Application No. D2016-002017, and an English Translation of the Office Action. (4 pages).

* cited by examiner

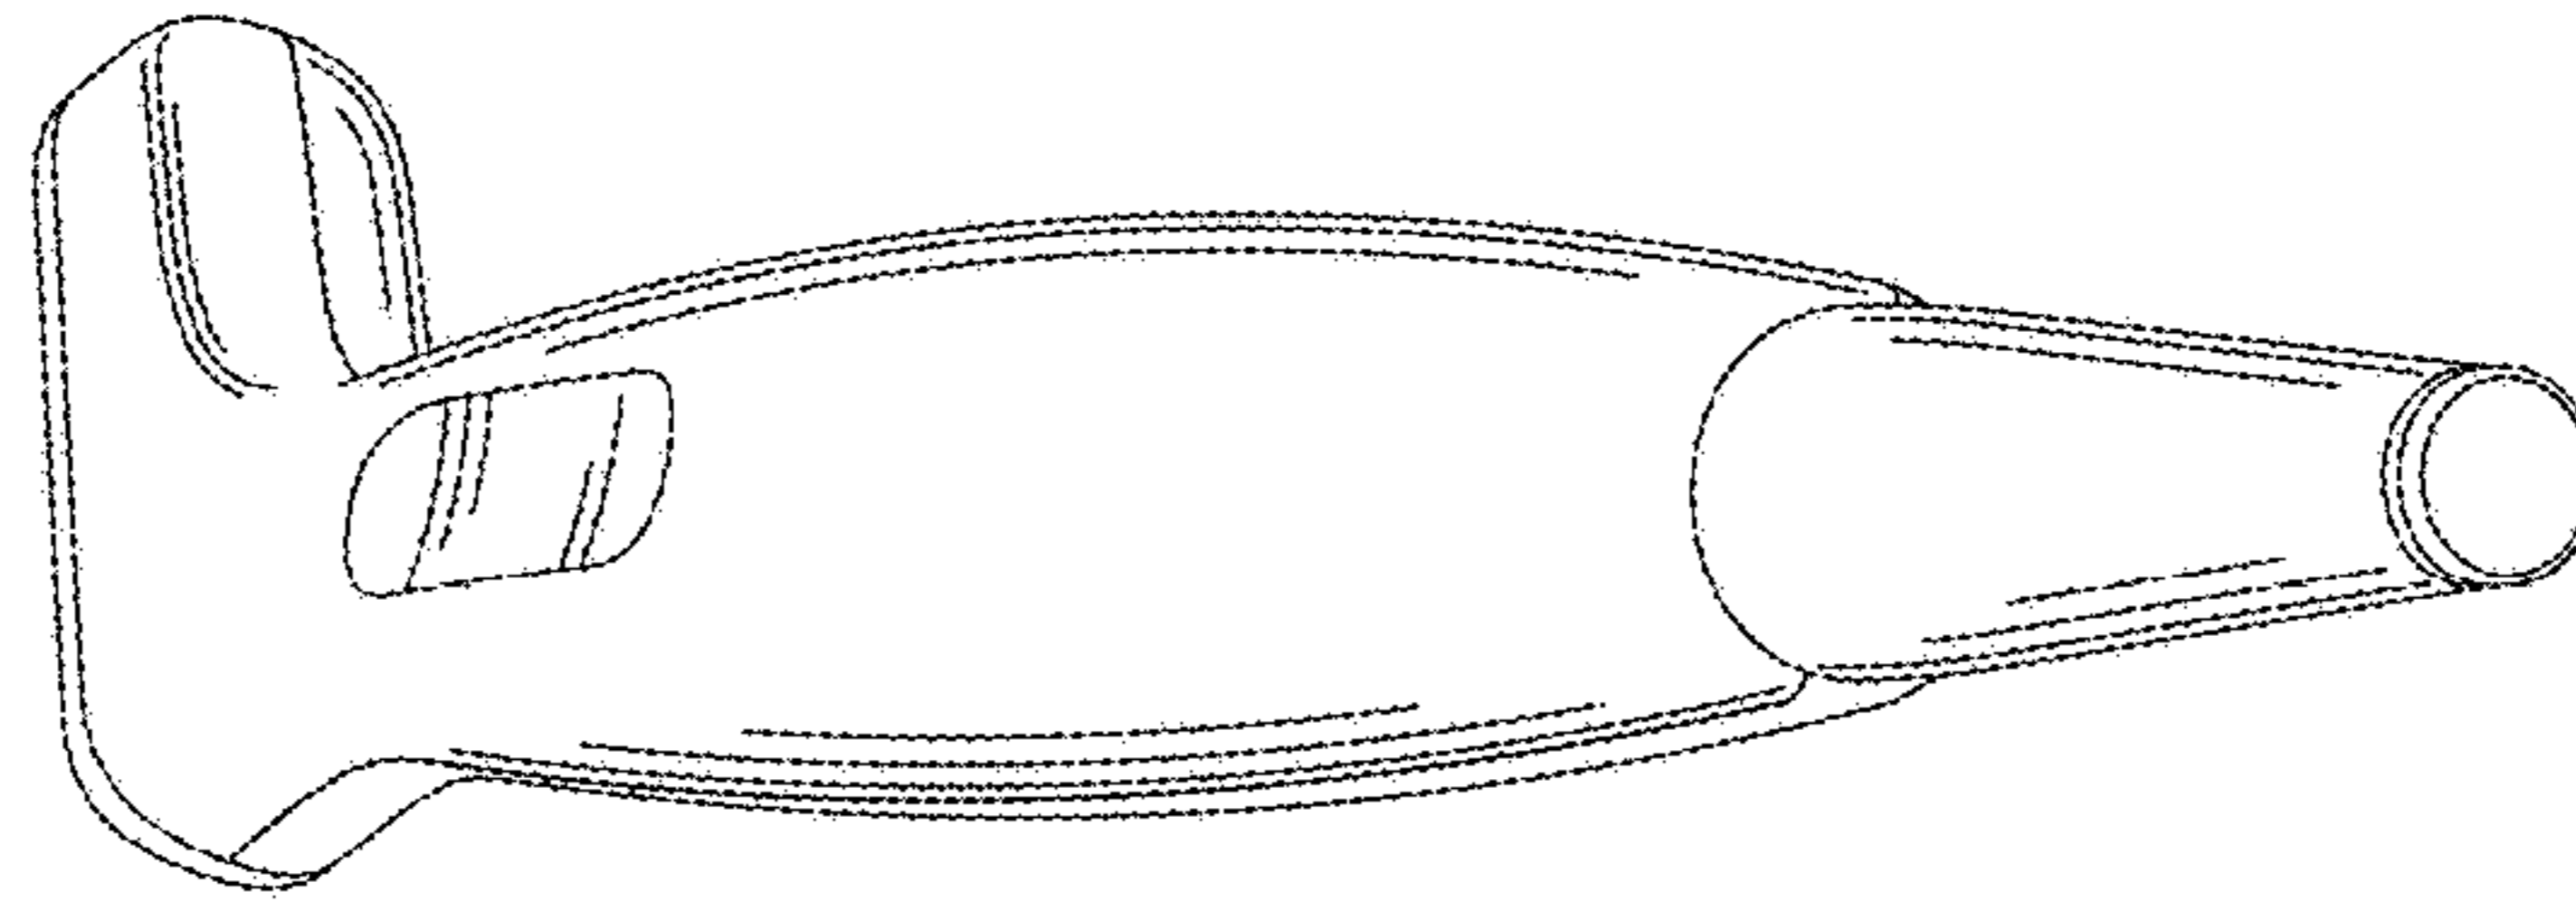


FIG. 1

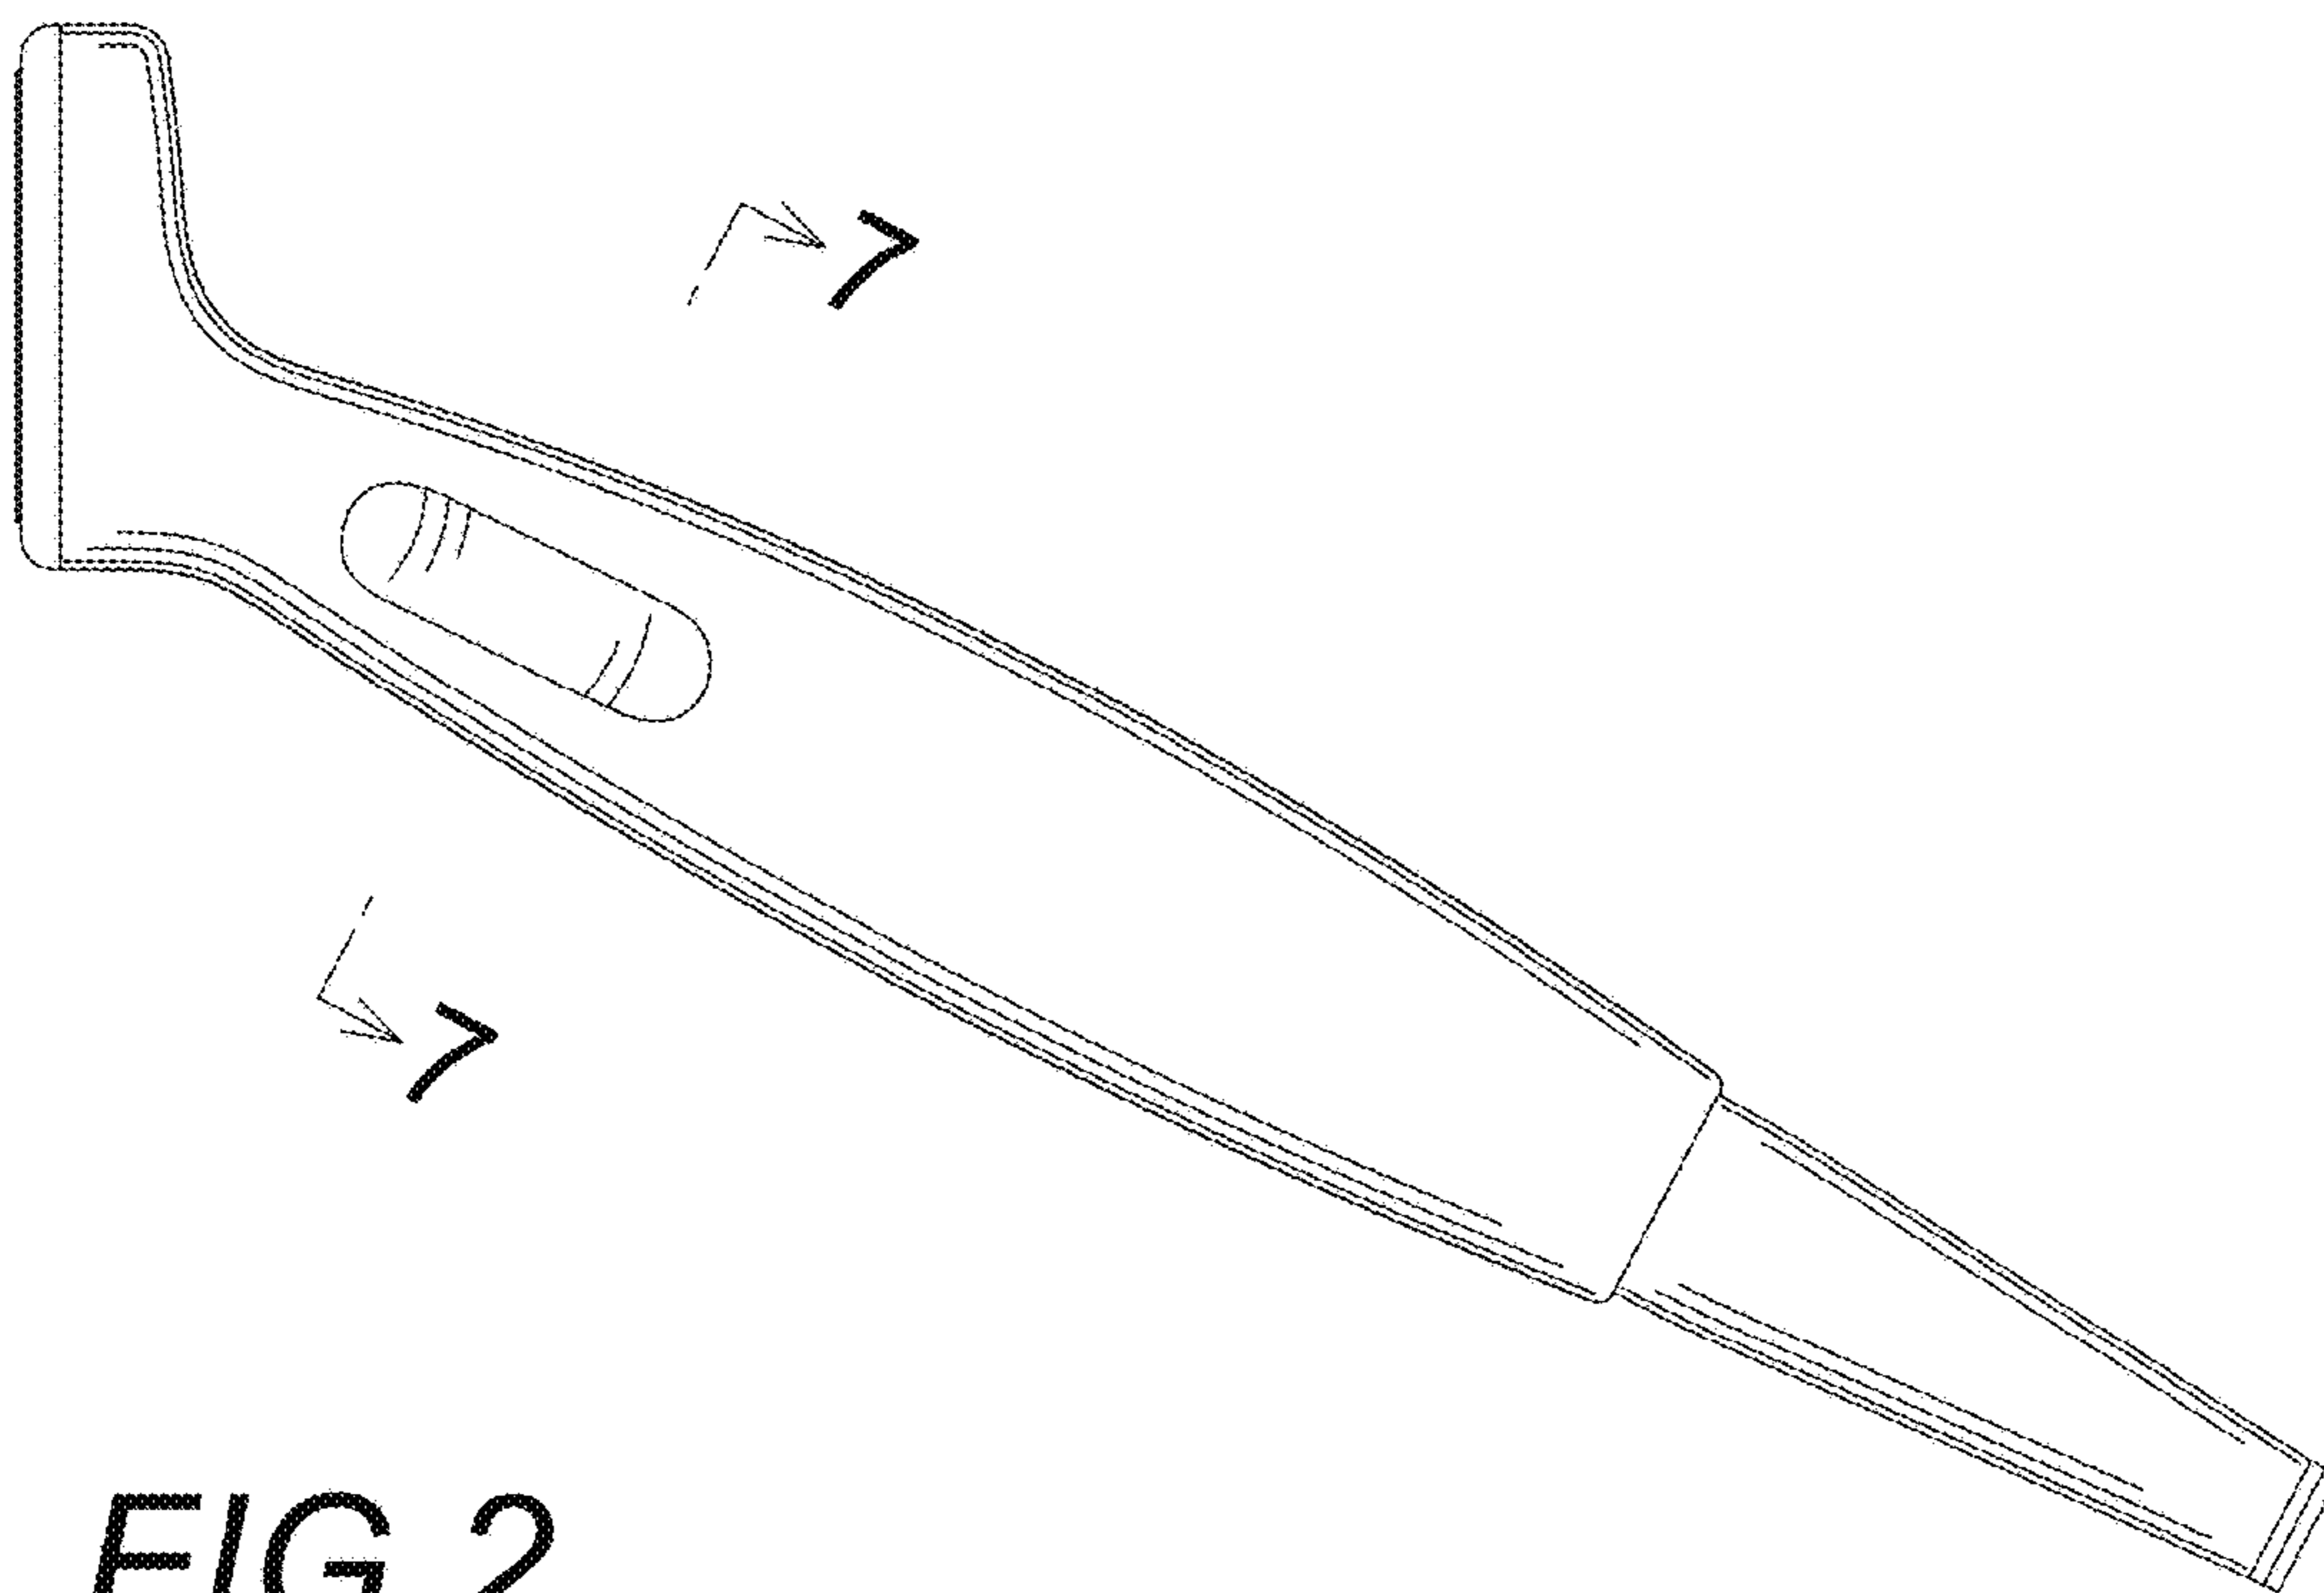


FIG. 2

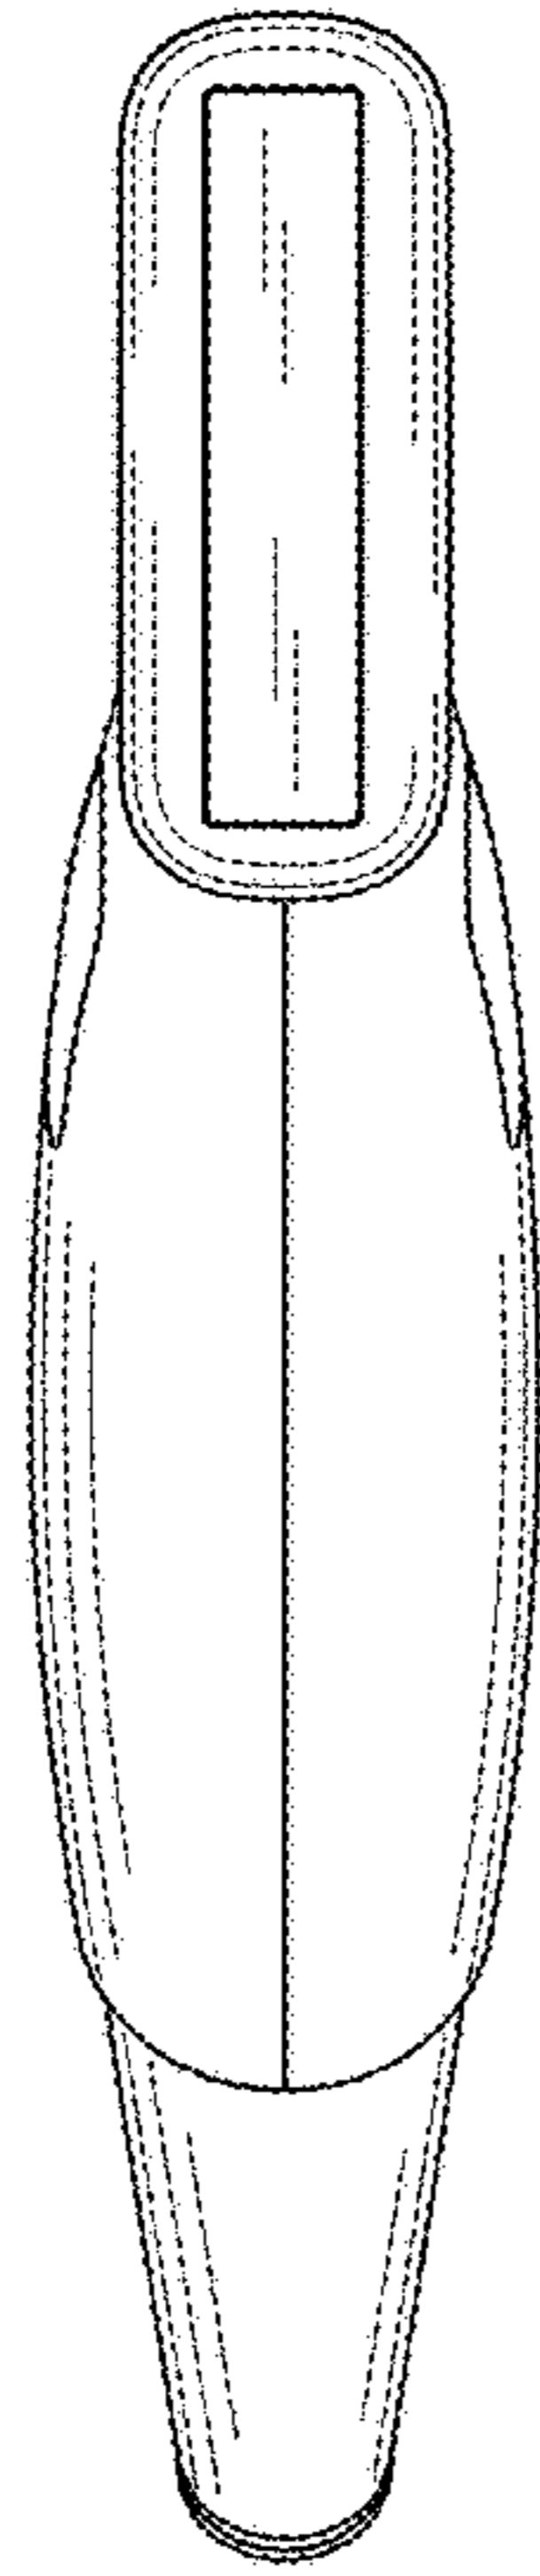


FIG. 3

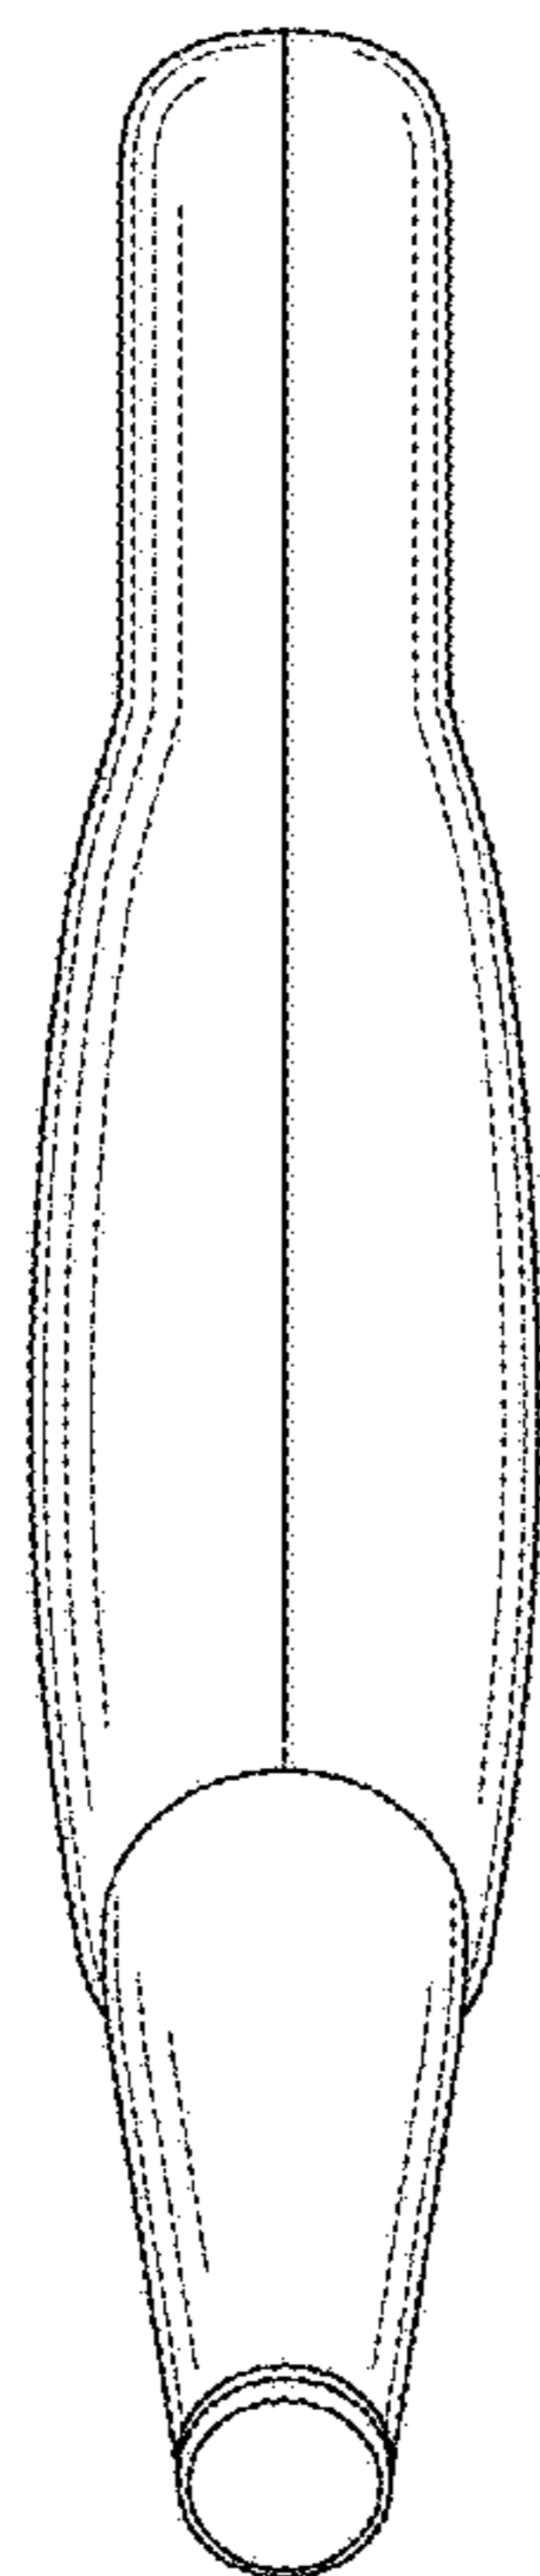


FIG. 4

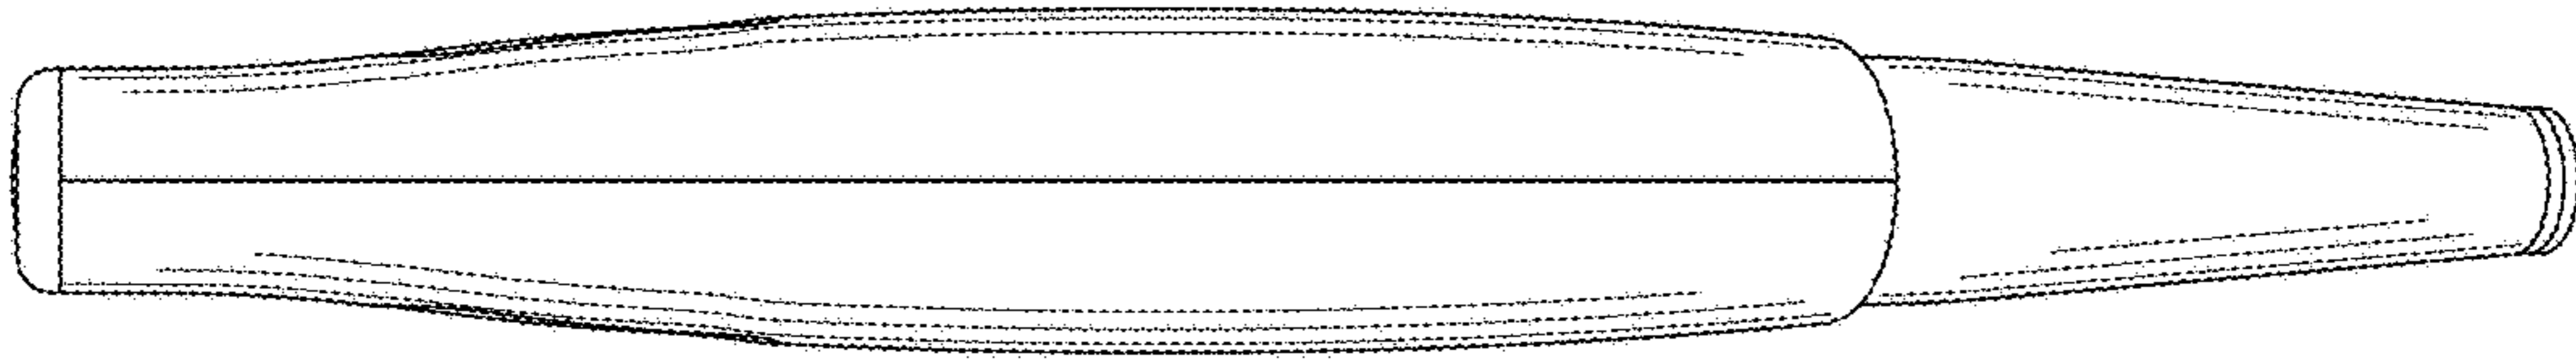


FIG. 5

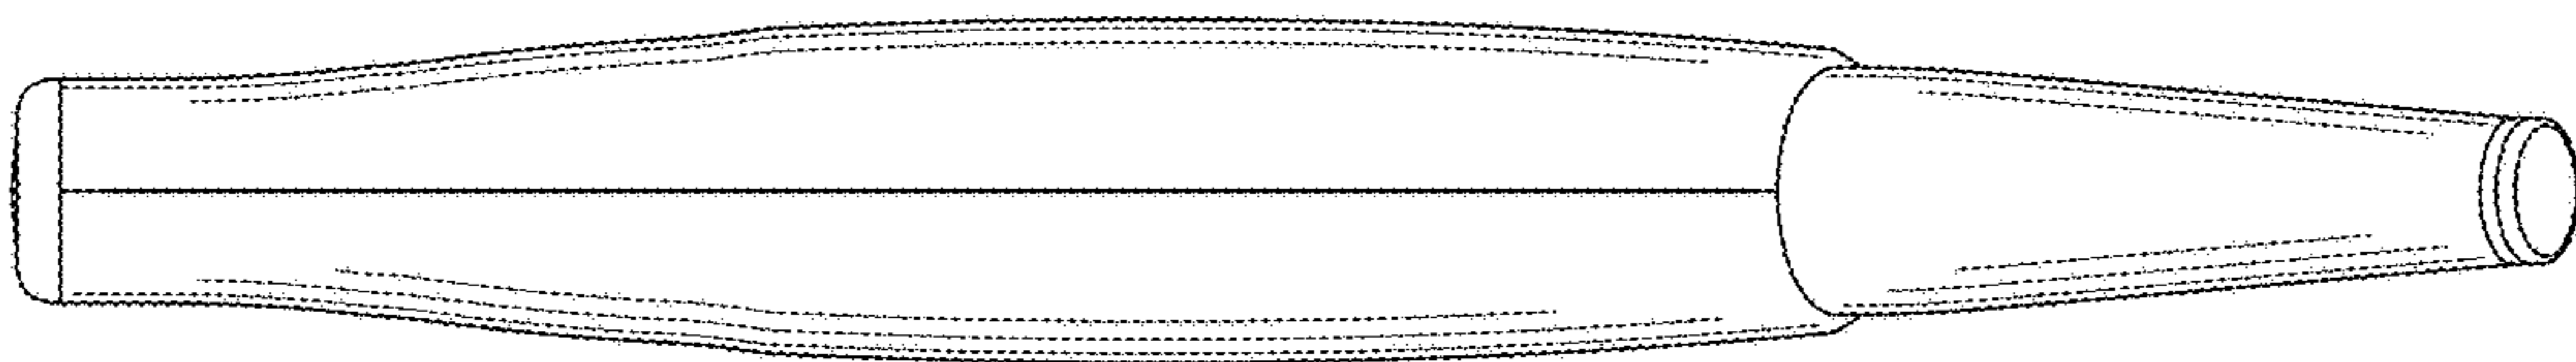


FIG. 6

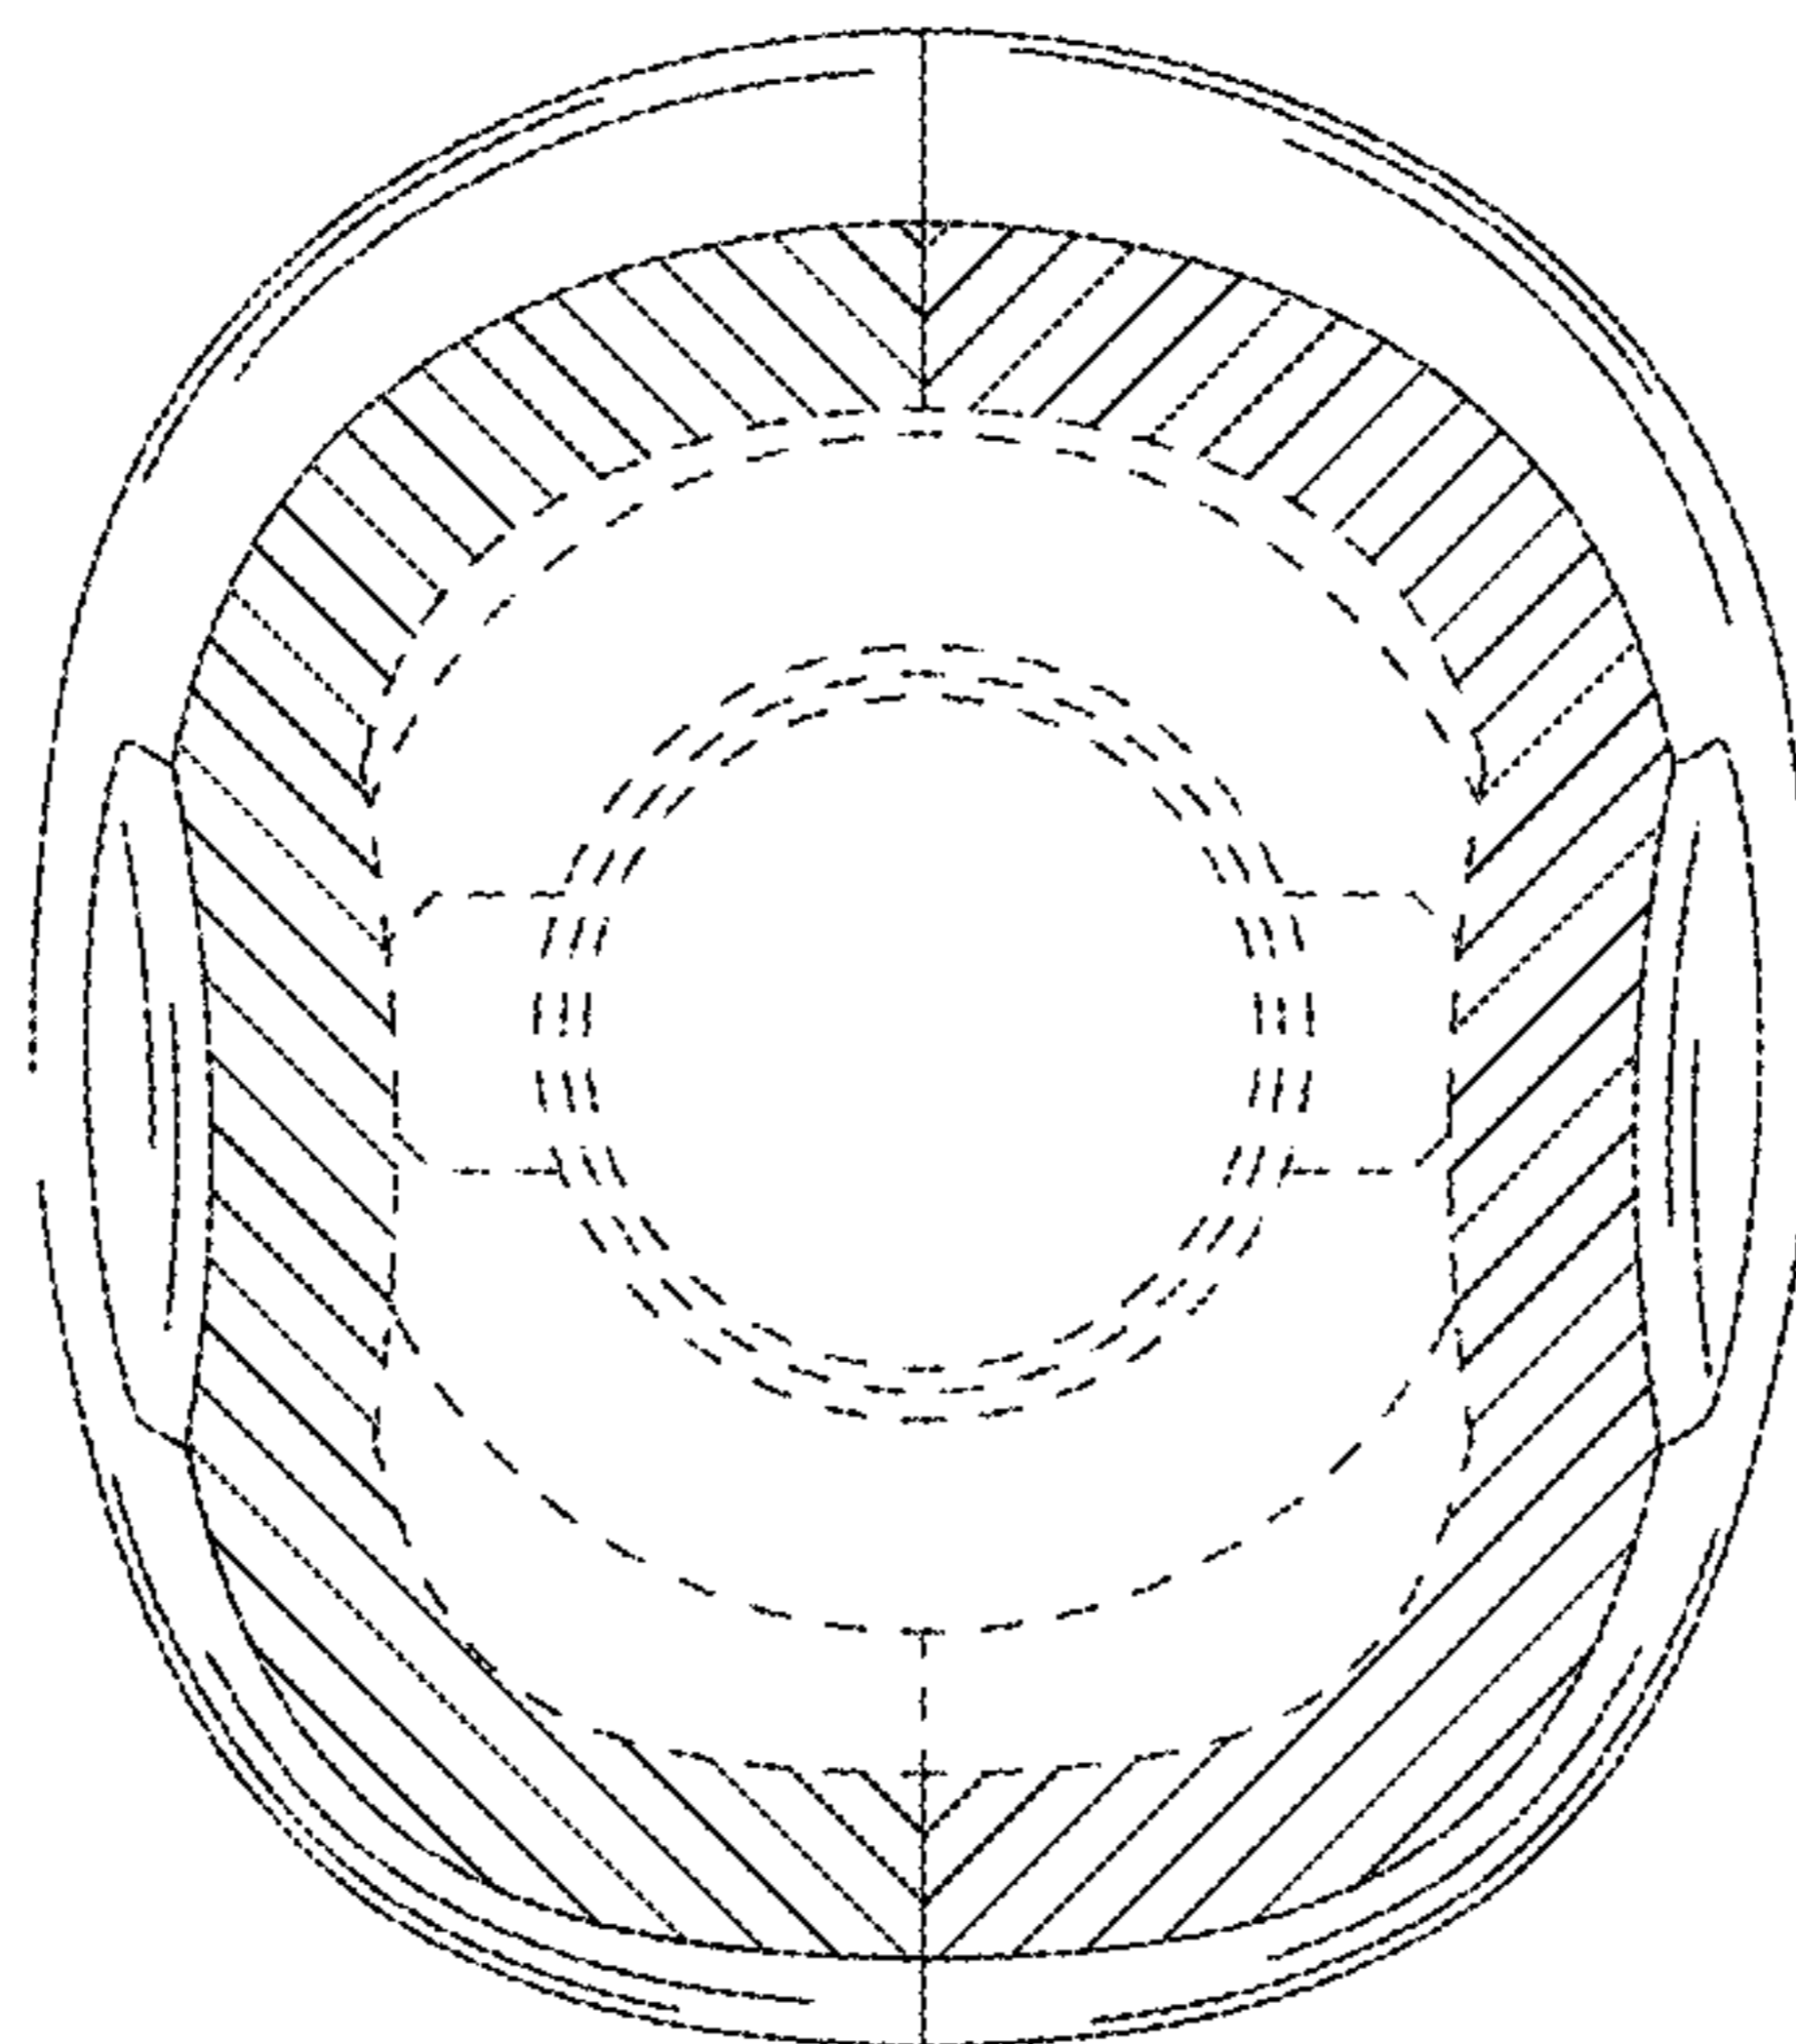


FIG. 7