



US00D819042S

(12) **United States Design Patent** (10) **Patent No.:** **US D819,042 S**
Ebler et al. (45) **Date of Patent:** **** May 29, 2018**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE FOR A MEDICAL DEVICE**

(71) Applicant: **MAQUET Cardiopulmonary GmbH, Rastatt (DE)**

(72) Inventors: **Ralph J. Ebler, Warwick, NY (US); Daniel Medart, Hillsdale, NJ (US)**

(73) Assignee: **MAQUET CARDIOPULMONARY GmbH, Rastatt (DE)**

(**) Term: **15 Years**

(21) Appl. No.: **29/541,759**

(22) Filed: **Oct. 7, 2015**

(51) **LOC (11) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485-488, 490, 494, 489, 491-493, D14/495

CPC . G06F 3/0482; G06F 3/04842; G06F 3/04817
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D479,720 S	9/2003	Ohashi et al.	
D510,582 S	10/2005	Hoang et al.	
D548,238 S	8/2007	Fletcher	
D548,732 S	8/2007	Fletcher	
D565,627 S *	4/2008	Kase	D14/486
D570,363 S	6/2008	Ulm et al.	
D574,010 S	7/2008	Borovsky et al.	
D575,792 S	8/2008	Benson	
D593,117 S	5/2009	Lettau	
D594,018 S	6/2009	Ball et al.	
D626,140 S *	10/2010	McLaughlin	D14/486

D629,005 S *	12/2010	Jewitt	D14/485
D632,698 S	2/2011	Judy et al.	
D632,699 S	2/2011	Judy et al.	
D633,919 S	3/2011	Chen	
D640,264 S	6/2011	Fujii et al.	
D653,672 S	2/2012	Friedlander	
D655,301 S *	3/2012	Ray	D14/486
D655,710 S *	3/2012	Inada	D14/485
D656,946 S *	4/2012	Judy	D14/486
D657,369 S	4/2012	Hecht et al.	
D658,196 S	4/2012	Wood et al.	
D660,864 S	5/2012	Anzures et al.	
D662,507 S *	6/2012	Mori	D14/486
D664,152 S *	7/2012	Ray	D14/486
D665,414 S *	8/2012	Lee	D14/488
D667,419 S *	9/2012	Rai	D14/486
D675,224 S *	1/2013	Lee	D14/488
D678,895 S	3/2013	Ebler et al.	

(Continued)

OTHER PUBLICATIONS

Sorin | S5 Brochure, Sorin Group USA, Inc., 2010.

(Continued)

Primary Examiner — Sheryl Lane

Assistant Examiner — Nicole Shiflet

(74) *Attorney, Agent, or Firm* — Wesley Scott Ashton


(57) **CLAIM**

The ornamental design for a display screen or portion thereof with graphical user interface for a medical device, as shown and described.

DESCRIPTION

The FIGURE is a front view of a display screen or portion thereof with graphical user interface for a medical device. The broken lines showing portions of the graphical user interface and the display screen form no part of the claimed design.

1 Claim, 1 Drawing Sheet

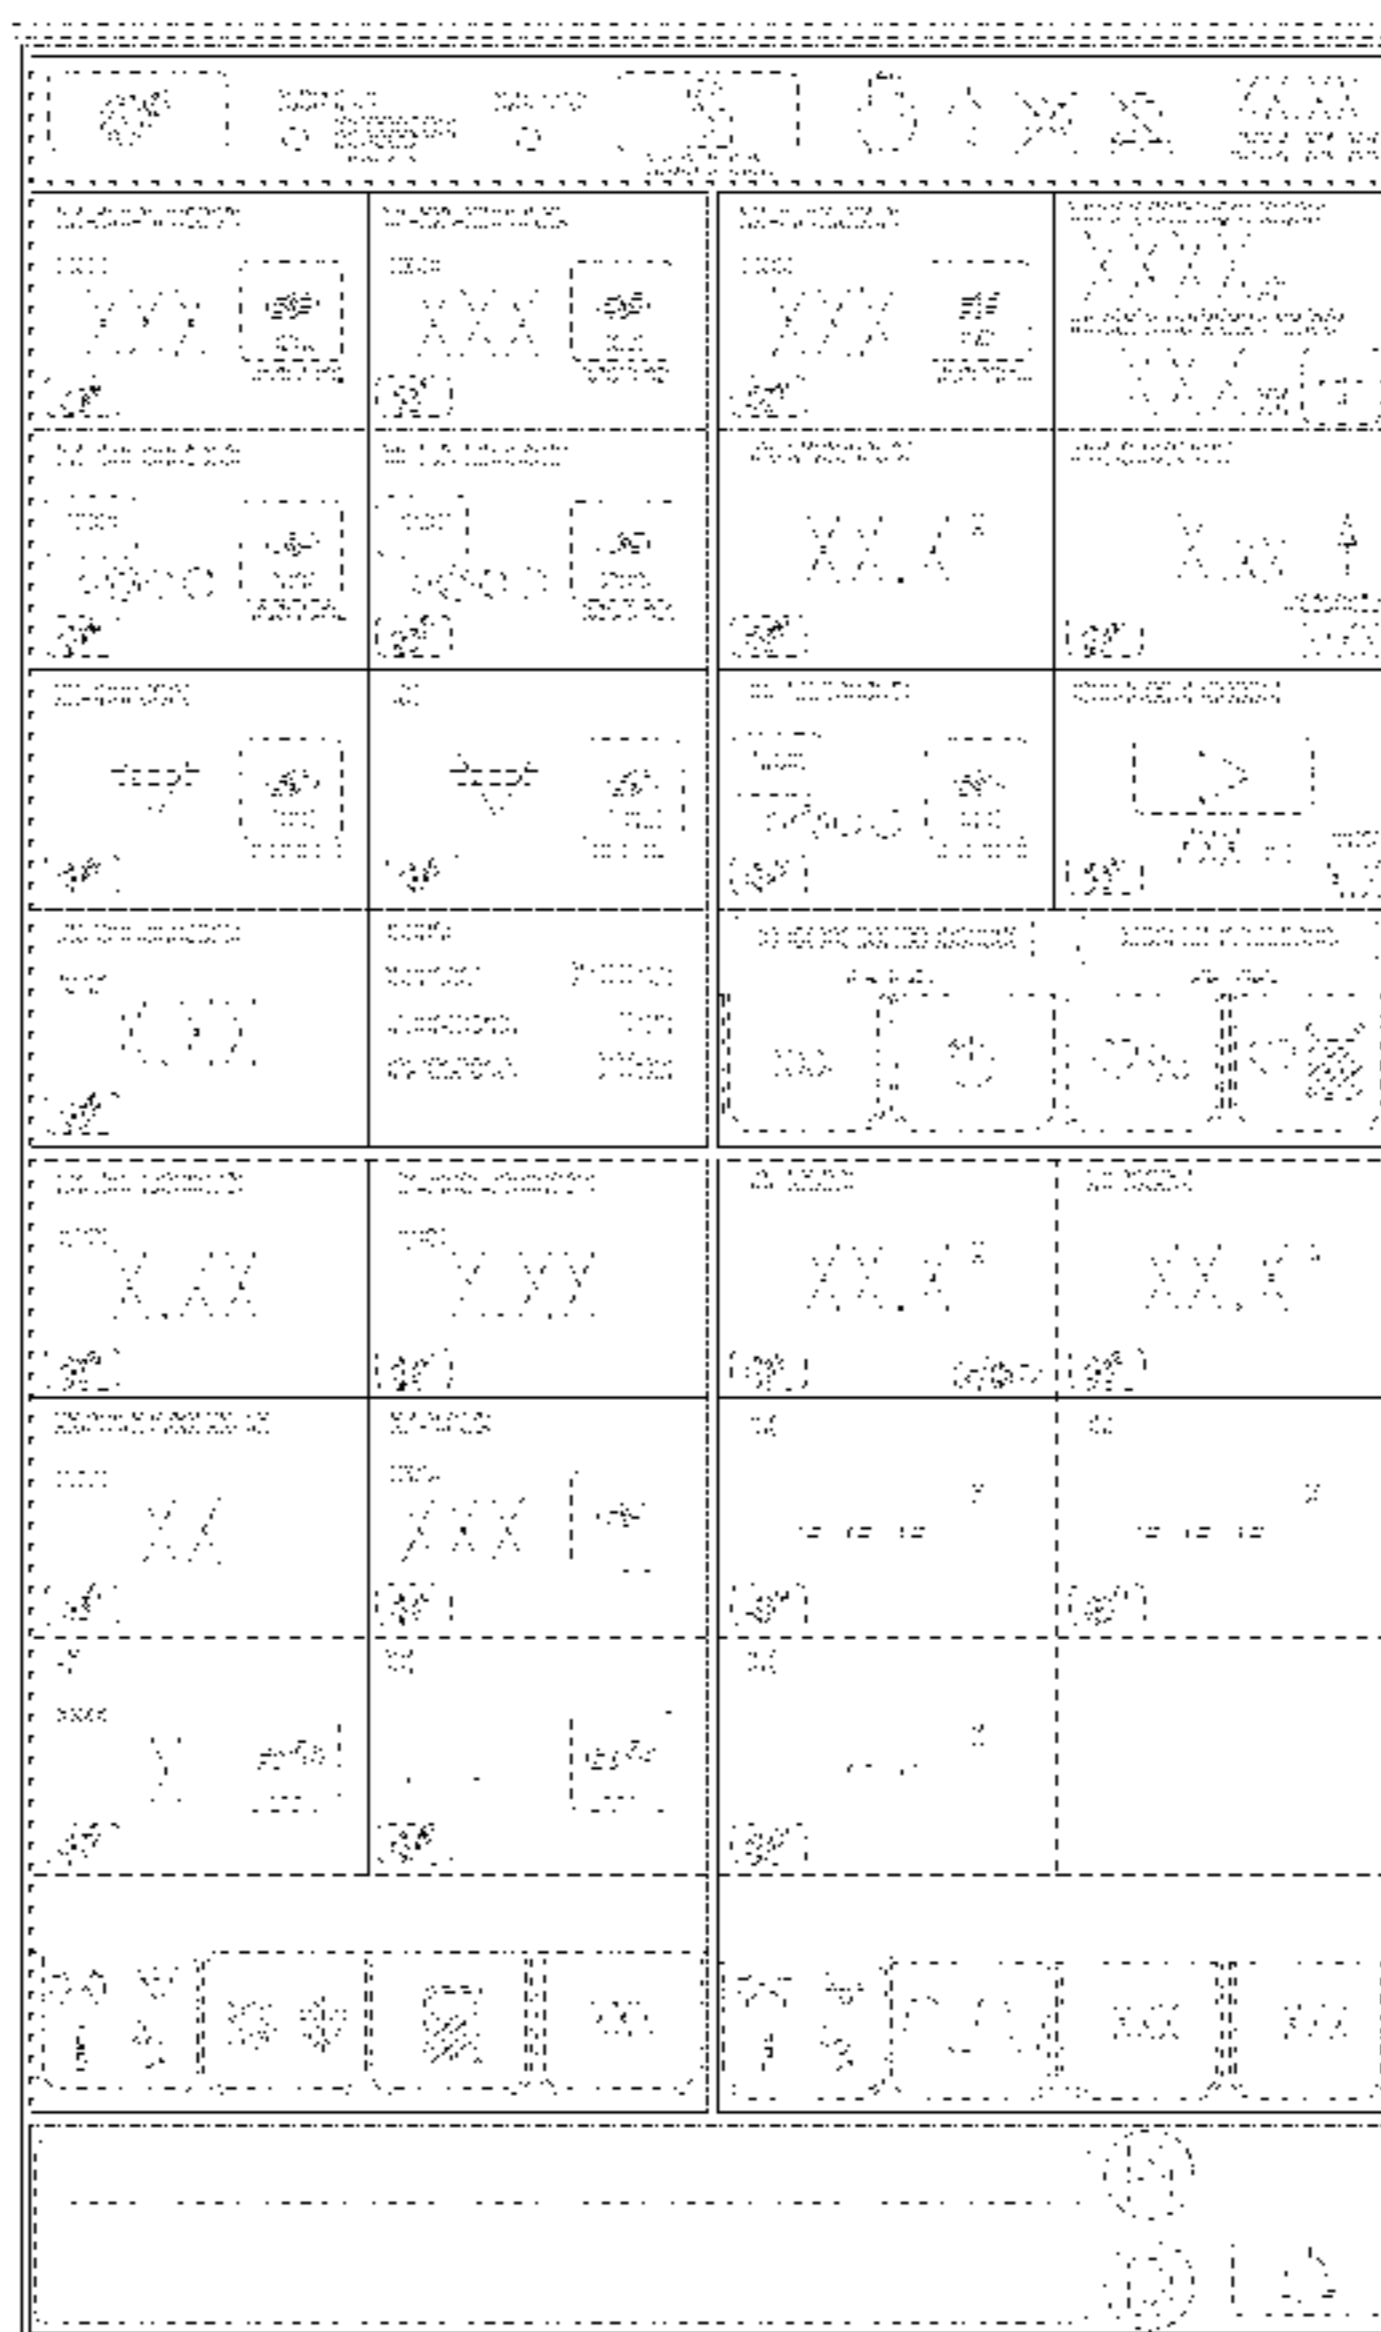

(56)

References Cited

U.S. PATENT DOCUMENTS

D682,288 S * 5/2013 Donahue D14/486
 D689,085 S * 9/2013 Pasceri et al.
 D701,236 S * 3/2014 Hatta D14/486
 D702,247 S * 4/2014 d'Amore D14/485
 D703,681 S * 4/2014 d'Amore D14/485
 D709,901 S * 7/2014 Landis D14/486
 D710,377 S * 8/2014 Rydenhag
 D712,908 S * 9/2014 Rodenhouse D14/485
 D722,318 S * 2/2015 Moore D14/486
 D722,319 S * 2/2015 Moore D14/486
 D722,322 S * 2/2015 Strayle D14/486
 D722,611 S * 2/2015 Moore D14/486
 D728,586 S * 5/2015 Konno D14/485
 D728,601 S * 5/2015 Angelides D14/486
 D729,267 S * 5/2015 Yoo et al.
 D731,507 S * 6/2015 Kyakuno D14/485
 D732,549 S * 6/2015 Kim D14/485
 D733,172 S * 6/2015 Angelides D14/486
 D735,743 S * 8/2015 Kanenari D14/486
 D737,304 S * 8/2015 Urdan D14/486
 D742,892 S * 11/2015 Mitchell D14/485
 D746,310 S * 12/2015 Ta D14/485
 D750,099 S * 2/2016 Seo D14/485
 D751,088 S * 3/2016 Seo D14/485
 D752,076 S * 3/2016 Guesnon
 D753,169 S * 4/2016 Kim D14/486
 D754,143 S * 4/2016 Sugimoto D14/485
 D754,161 S * 4/2016 Wilder D14/486
 D754,163 S * 4/2016 Park D14/486
 D754,172 S * 4/2016 Ferreira D14/486
 D754,680 S * 4/2016 Lee D14/485
 D754,701 S * 4/2016 Seo D14/486
 D754,703 S * 4/2016 Moon et al.
 D755,821 S * 5/2016 Lee D14/486
 D757,059 S * 5/2016 Gray D14/486
 D759,100 S * 6/2016 Pal et al.
 D763,274 S * 8/2016 Edwards D14/485
 D764,488 S * 8/2016 Bae D14/485
 D765,698 S * 9/2016 Kwon
 D768,174 S * 10/2016 Kim D14/486
 D769,290 S * 10/2016 Choi D14/486
 D769,291 S * 10/2016 Kim D14/486
 D772,887 S * 11/2016 Frew D14/485
 D776,701 S * 1/2017 Huang D14/486
 D780,189 S * 2/2017 Yang D14/485
 D781,308 S * 3/2017 Austin D14/485
 D782,496 S * 3/2017 Contreras et al.
 D783,039 S * 4/2017 Park D14/486
 D786,910 S * 5/2017 Higuchi D14/486
 D787,543 S * 5/2017 Qiu D14/486
 D791,810 S * 7/2017 Hatzikostas D14/486
 2003/0135087 A1 * 7/2003 Hickie et al.
 2007/0011702 A1 * 1/2007 Vaysman H04N 21/84
 725/45
 2007/0288868 A1 * 12/2007 Rhee G06F 3/04817
 715/840

2013/0187780 A1 * 7/2013 Angelides A61B 5/0002
 340/573.1
 2014/0127063 A1 * 5/2014 Petersen et al.
 2017/0102846 A1 * 4/2017 Ebler et al.

OTHER PUBLICATIONS

MetaVision Perfusion™, A point-of-care clinical information system for perfusionists, Maquet Getinge Group 2015 (<http://www.maquet.com/int/products/metavision-perfusion/>).
 Heart-Lung Machine HL20 Brochure, Maquet Cardiopulmonary AG 2012.
 “Heart Lung Machine Fundraising.” Aug. 18, 2015. Web. Nov. 6, 2015. <<http://www.heartcentreforchildren.com.au/heart-lung-machine-fundraising.html>>.
 Heart-lung machines. surgeryencyclopedia.com. Advameg, Inc. 2015. Web. Nov. 5, 2015. <<http://www.surgeryencyclopedia.com/Fi-La/Heart-Lung-Machines.html>>.
 Machine coeur-poumon HL30. Feb. 21, 2013. Web. Nov. 18, 2015. <<file:///C:/Users/u2002449/Downloads/rnes-130225-MachineCoeurPoumonHL30-Maquet.pdf>>.
 Terumo Advanced Perfusion System 1. Terumo Cardiovascular Group. Nov. 2014. Web. Nov. 18, 2015. <http://www.terumo-cvs.com/doc/848594_Terumo-System1_Brochure%20Nov2013_LowRes_Pgs.pdf>.
 Product Catalog Jostra HL 20. Maquet Cardiopulmonary AG. Web. Nov. 18, 2015. <http://glavm.ru/upload/information_system_18/2/8/7/item_287/information_items_property_343.pdf>.
 Sorin | S5 System Operating Instructions, Sorin Group Deutschland GmbH, 2006, 2007.
 Hessel, Eugene A., “Circuitry and Cannulation Techniques”, Chapter 5, Cardiopulmonary Bypass: Principles and Practices, edited by Glenn P. Gravlee, 3rd edition, 2008, pp. 63-65.
 Product Brochure—CS300 IABP—Product Features—2009 Publication—Maquet Cardiovascular LLC. U.S.A.
 Product Brochure—CS100 IABP—Intelligent Counterpulsation—2010 Publication—Maquet Cardiovascular LLC. U.S.A.
 Operators Guide—The CS100/CS100i Abbreviated Operator’s Guide—2009 Publication—Maquet Cardiovascular LLC. U.S.A.
 Operators Guide—Datascope Abbreviated Operator’s Guide for the System 97 Intra-Aortic Balloon Pump—Published prior to 2009—Datascope Corp. U.S.A.
 Brochure—Sensation and CS300 IABP System Smaller Meets Faster—Published in 2009—Maquet Cardiovascular LLC. U.S.A.
 Brochure—CS300 IABP Product Features—Published in 2009—Maquet Cardiovascular LLC. U.S.A.
 Sorin article, <http://www.sorin.com/products/cardiac-surgery/perfusion/hlm/s5>, printed on Jun. 13, 2015, 11 pages.
 Official Action—dated Dec. 6, 2017—for Japanese Patent Application No. 2017-12102, which corresponds to this pending application.
 Image—Runner Advance C7270/C7260 (image cited in Official Action for Japanese Patent Application No. 2017-12102).
 Image—1 Urbano L 02—<http://www.kyocera.co.jp/prdct/telecom/consumer/102/function1/index.html> (image and website cited in Official Action for Japanese Patent Application No. 2017-12102).

* cited by examiner

