



US00D819224S

(12) **United States Design Patent**  
**Anderson**

(10) **Patent No.:** **US D819,224 S**  
(45) **Date of Patent:** **\*\* May 29, 2018**

(54) **URINE TEST DEVICE**  
(71) Applicant: **Global Icle Test Ltd.**, Hartlepool (GB)  
(72) Inventor: **John Robert Anderson**, Wingate (GB)  
(73) Assignee: **Global Icle Test Ltd.**, Hartlepool (GB)  
(\*\*) Term: **15 Years**

5,060,317 A \* 10/1991 Bertelsen ..... A61B 10/007  
4/144.2  
5,111,539 A \* 5/1992 Hiruta ..... A61B 5/02241  
4/301  
5,409,473 A \* 4/1995 Rosenshein ..... A61B 10/007  
600/574  
D379,663 S \* 6/1997 Pearson ..... D10/81  
D383,549 S \* 9/1997 Arnett ..... D10/81  
D387,848 S \* 12/1997 Thompson ..... D23/208  
6,146,590 A \* 11/2000 Mazurek ..... G01N 33/54386  
422/401

(21) Appl. No.: **29/605,349**

(Continued)

(22) Filed: **May 25, 2017**

FOREIGN PATENT DOCUMENTS

(51) **LOC (11) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/223**

JP 2009229214 A 10/2009  
WO 2004036343 A2 4/2004

(58) **Field of Classification Search**  
USPC ..... D24/216, 122, 127, 128, 223, 224;  
D10/81, 103; D23/208  
CPC . A61B 10/007; A61B 5/0002; A61B 5/02241;  
A61B 5/14507; A61B 5/20; A61B 5/201;  
A61B 5/7435; B01L 3/5023; B65D  
50/046; E03D 11/00; E03D 11/02; E03D  
9/00; E03D 9/032; G01N 21/78; G01N  
33/48; G01N 33/493; G01N 33/52; G01N  
33/523; G01N 33/525; G01N 33/528;  
G01N 33/54366; G01N 33/54386; G01N  
33/54388; G01N 33/558; G01N 33/62;  
G01N 33/721

*Primary Examiner* — Ian Simmons  
*Assistant Examiner* — Mark Cavanna  
(74) *Attorney, Agent, or Firm* — James Creighton Wray

See application file for complete search history.

(57) **CLAIM**

The ornamental design for a urine test device, as shown and described.

(56) **References Cited**


**DESCRIPTION**

U.S. PATENT DOCUMENTS

4,203,169 A \* 5/1980 Dale ..... A61B 10/007  
4/144.1  
D266,694 S \* 10/1982 Boger ..... D24/223  
4,901,736 A \* 2/1990 Huang ..... E03D 11/02  
600/573  
D307,934 S \* 5/1990 Verebelyi ..... D23/208  
5,047,206 A \* 9/1991 Dombrowski ..... G01N 33/525  
156/73.1

FIG. 1 is a front, right and top perspective view of a urine test device.  
FIG. 2 is a rear elevation of the urine test device shown in FIG. 1.  
FIG. 3 is a left side elevation of the urine test device shown in FIGS. 1 and 2.  
FIG. 4 is a front elevation of the urine test device shown in FIGS. 1-3.  
FIG. 5 is a right side elevation of the urine test device shown in FIGS. 1-4.  
FIG. 6 is a plan view of the urine test device shown in FIGS. 1-5; and,  
FIG. 7 is a bottom view of the urine test device shown in FIGS. 1-6.

**1 Claim, 7 Drawing Sheets**

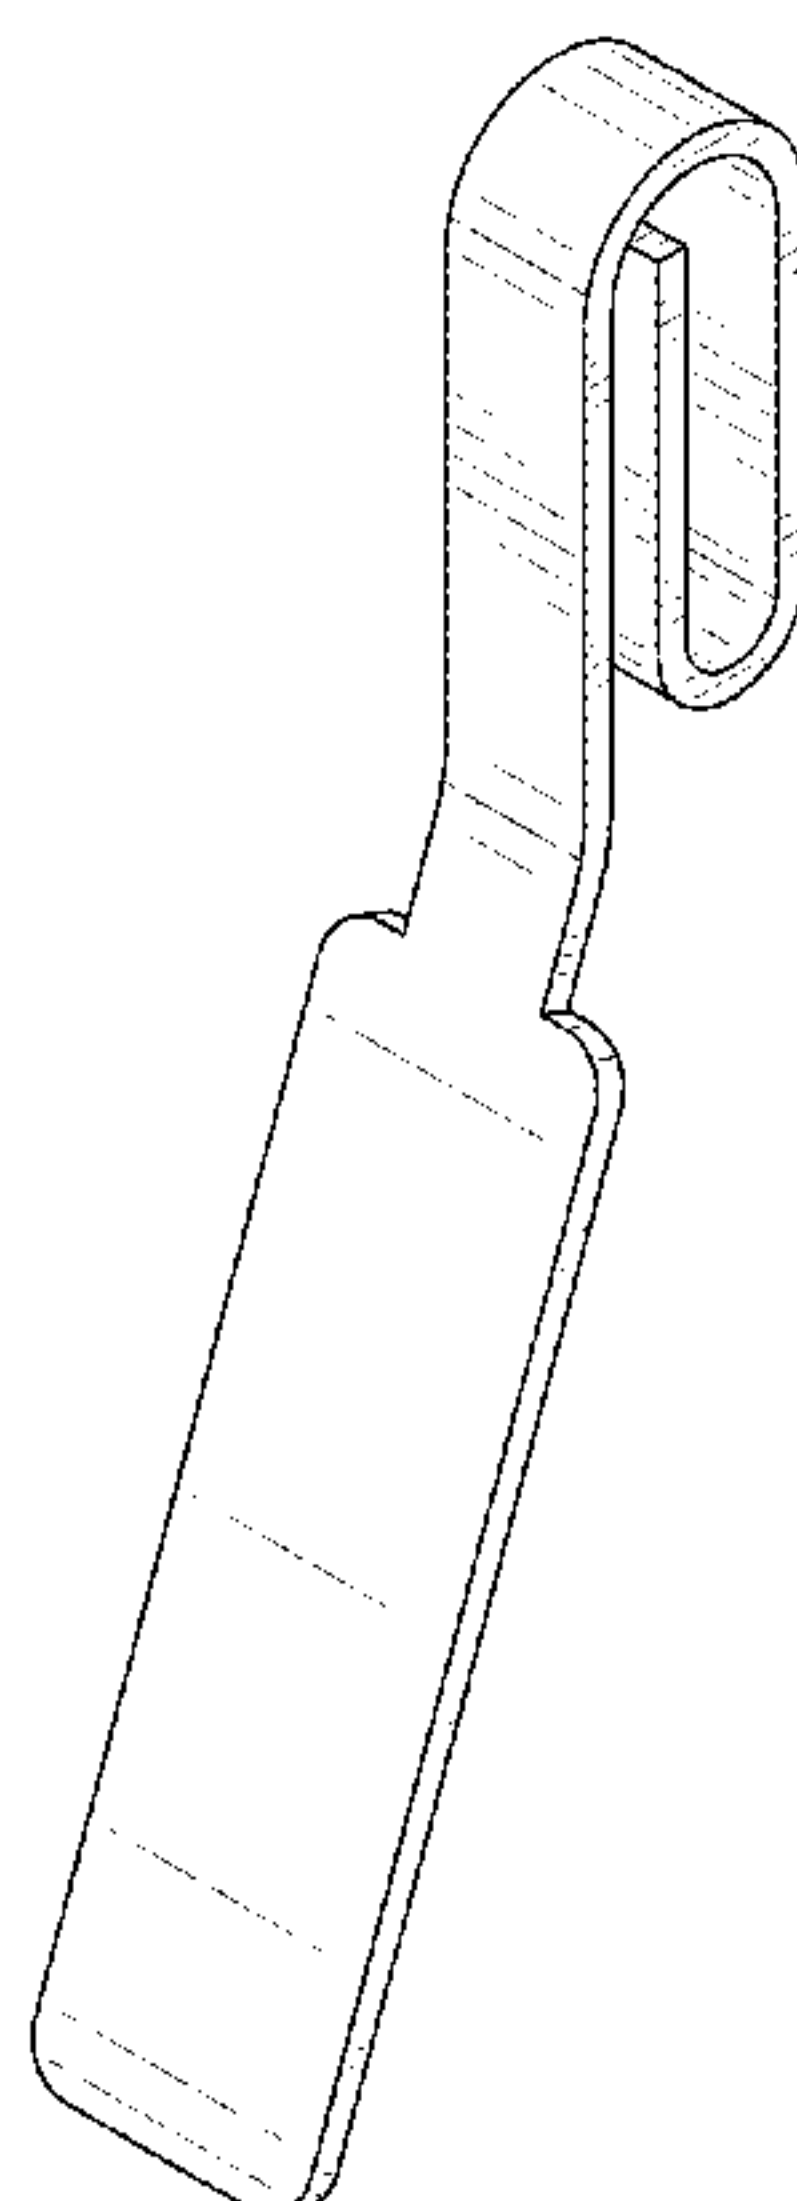


(56)

References Cited


U.S. PATENT DOCUMENTS

6,311,340 B1 \* 11/2001 Thompson ..... B65D 50/046  
4/231  
6,319,676 B1 \* 11/2001 Nazareth ..... G01N 33/558  
422/408  
6,372,516 B1 \* 4/2002 Sun ..... B01L 3/5023  
422/408  
D476,056 S \* 6/2003 Woolley ..... D23/208  
6,572,564 B2 \* 6/2003 Ito ..... A61B 5/0002  
4/314  
6,740,293 B1 \* 5/2004 Deng ..... A61B 10/007  
422/412  
D499,812 S \* 12/2004 Wu ..... D24/223  
6,998,273 B1 \* 2/2006 Fleming ..... G01N 33/558  
422/412  
7,011,634 B2 \* 3/2006 Paasch ..... A61B 10/007  
4/144.1  
D547,418 S \* 7/2007 King ..... D23/208  
D548,359 S \* 8/2007 Illein ..... D24/223  
D558,856 S \* 1/2008 King ..... D23/208  
D634,023 S \* 3/2011 Wei ..... D24/223  
D676,569 S \* 2/2013 Laverack ..... D24/223  
D676,570 S \* 2/2013 Chance ..... D24/223  
D720,864 S \* 1/2015 Behar ..... D24/223  
9,151,754 B2 \* 10/2015 Snowden ..... G01N 33/558  
2002/0001852 A1 \* 1/2002 Mendel-Hartvig .. G01N 33/558  
436/514  
2013/0323828 A1 \* 12/2013 Matumura ..... G01N 33/52  
435/287.9  
2015/0359522 A1 \* 12/2015 Recht ..... G01N 33/62  
600/573  
2017/0067872 A1 \* 3/2017 Anderson ..... A61B 10/007


\* cited by examiner

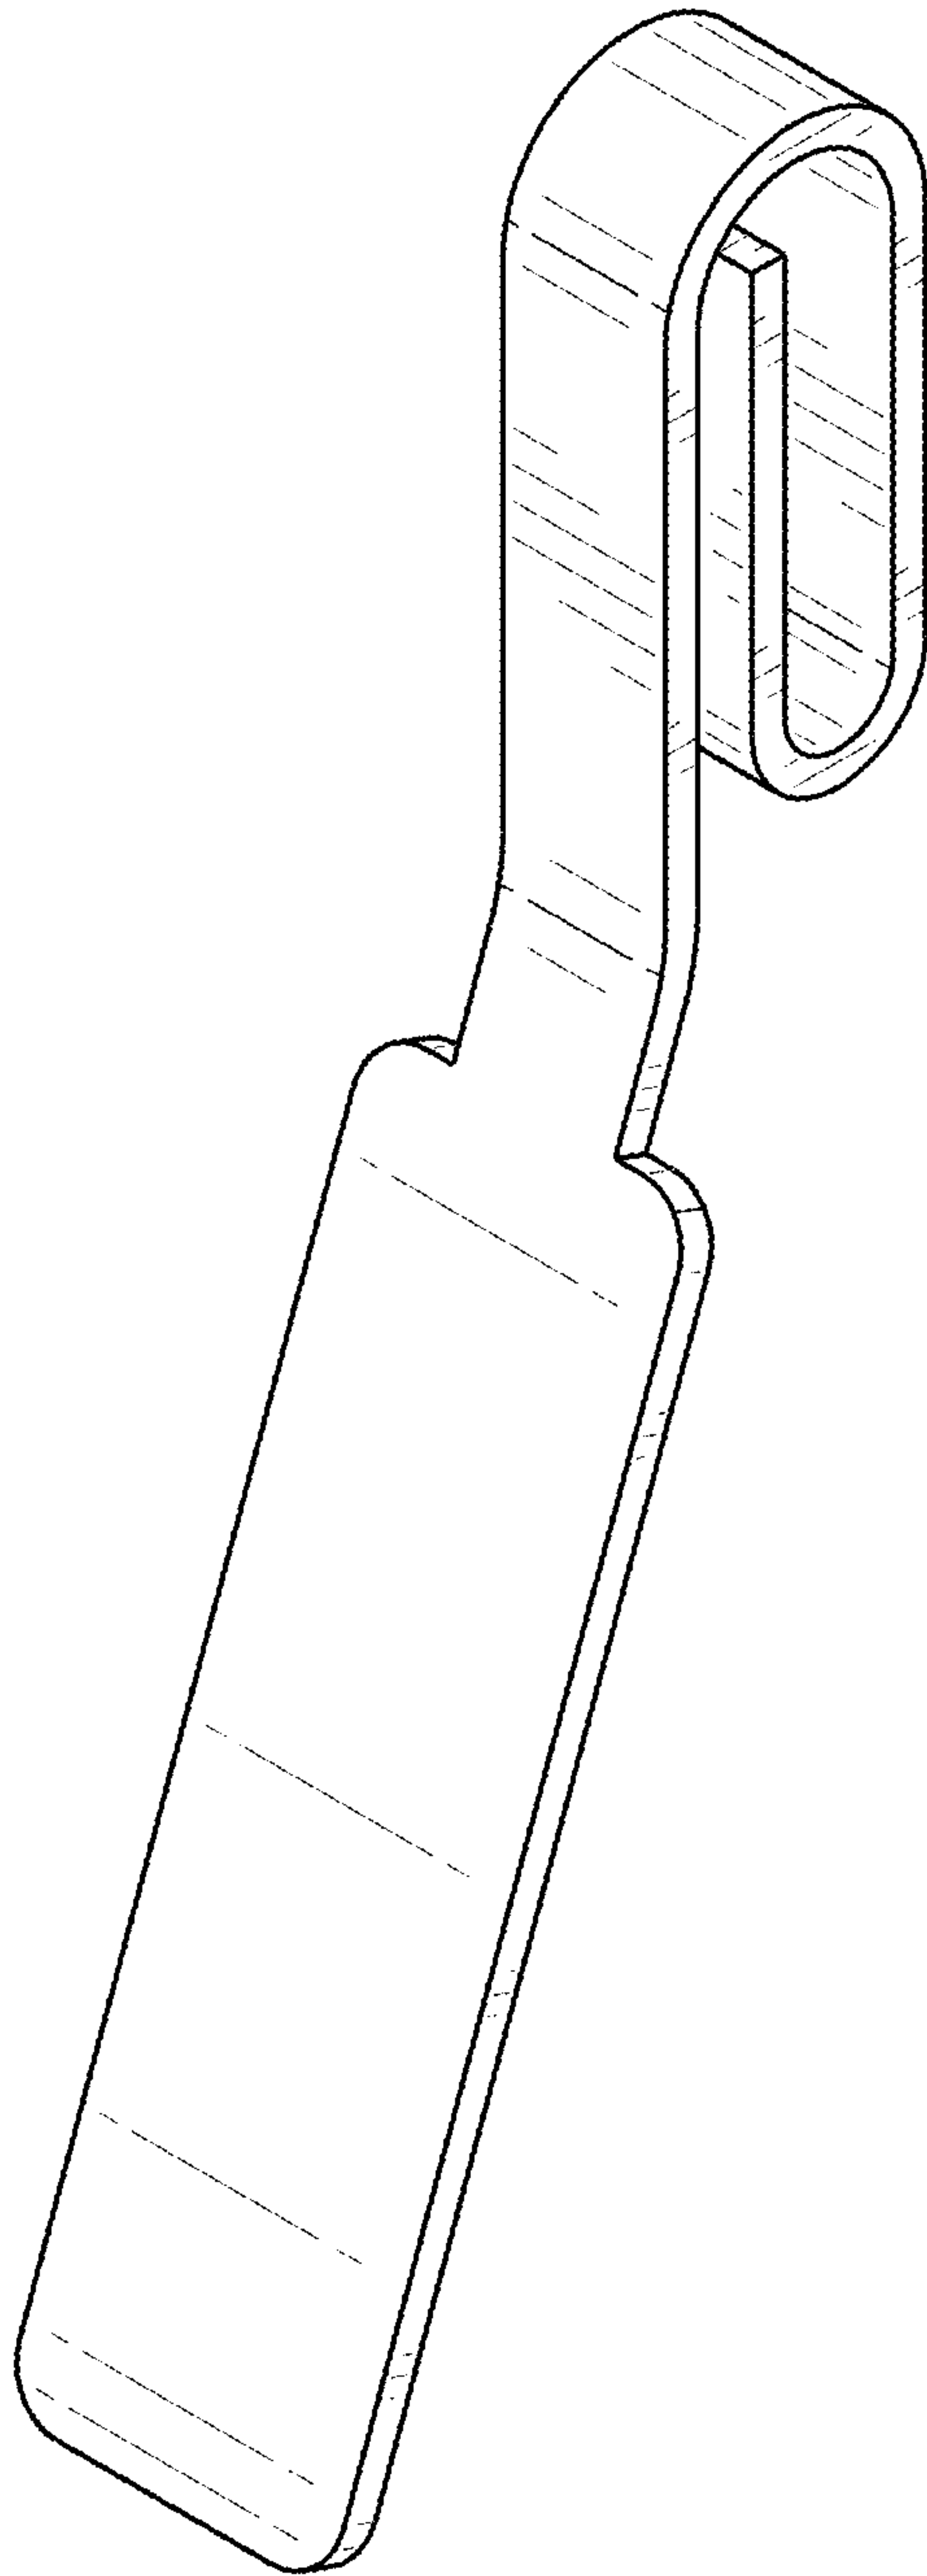


**FIG. 1**

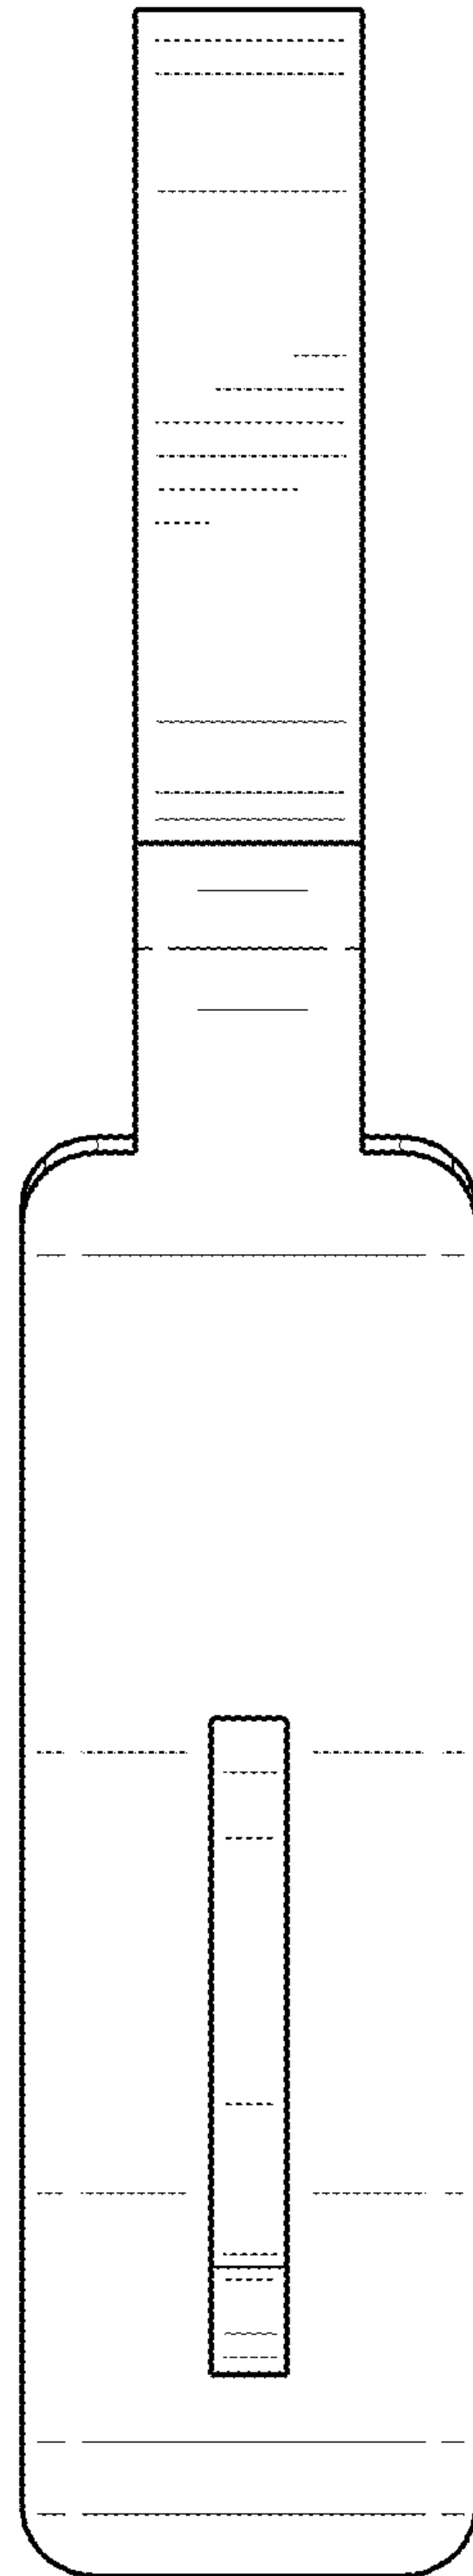


**FIG. 2**

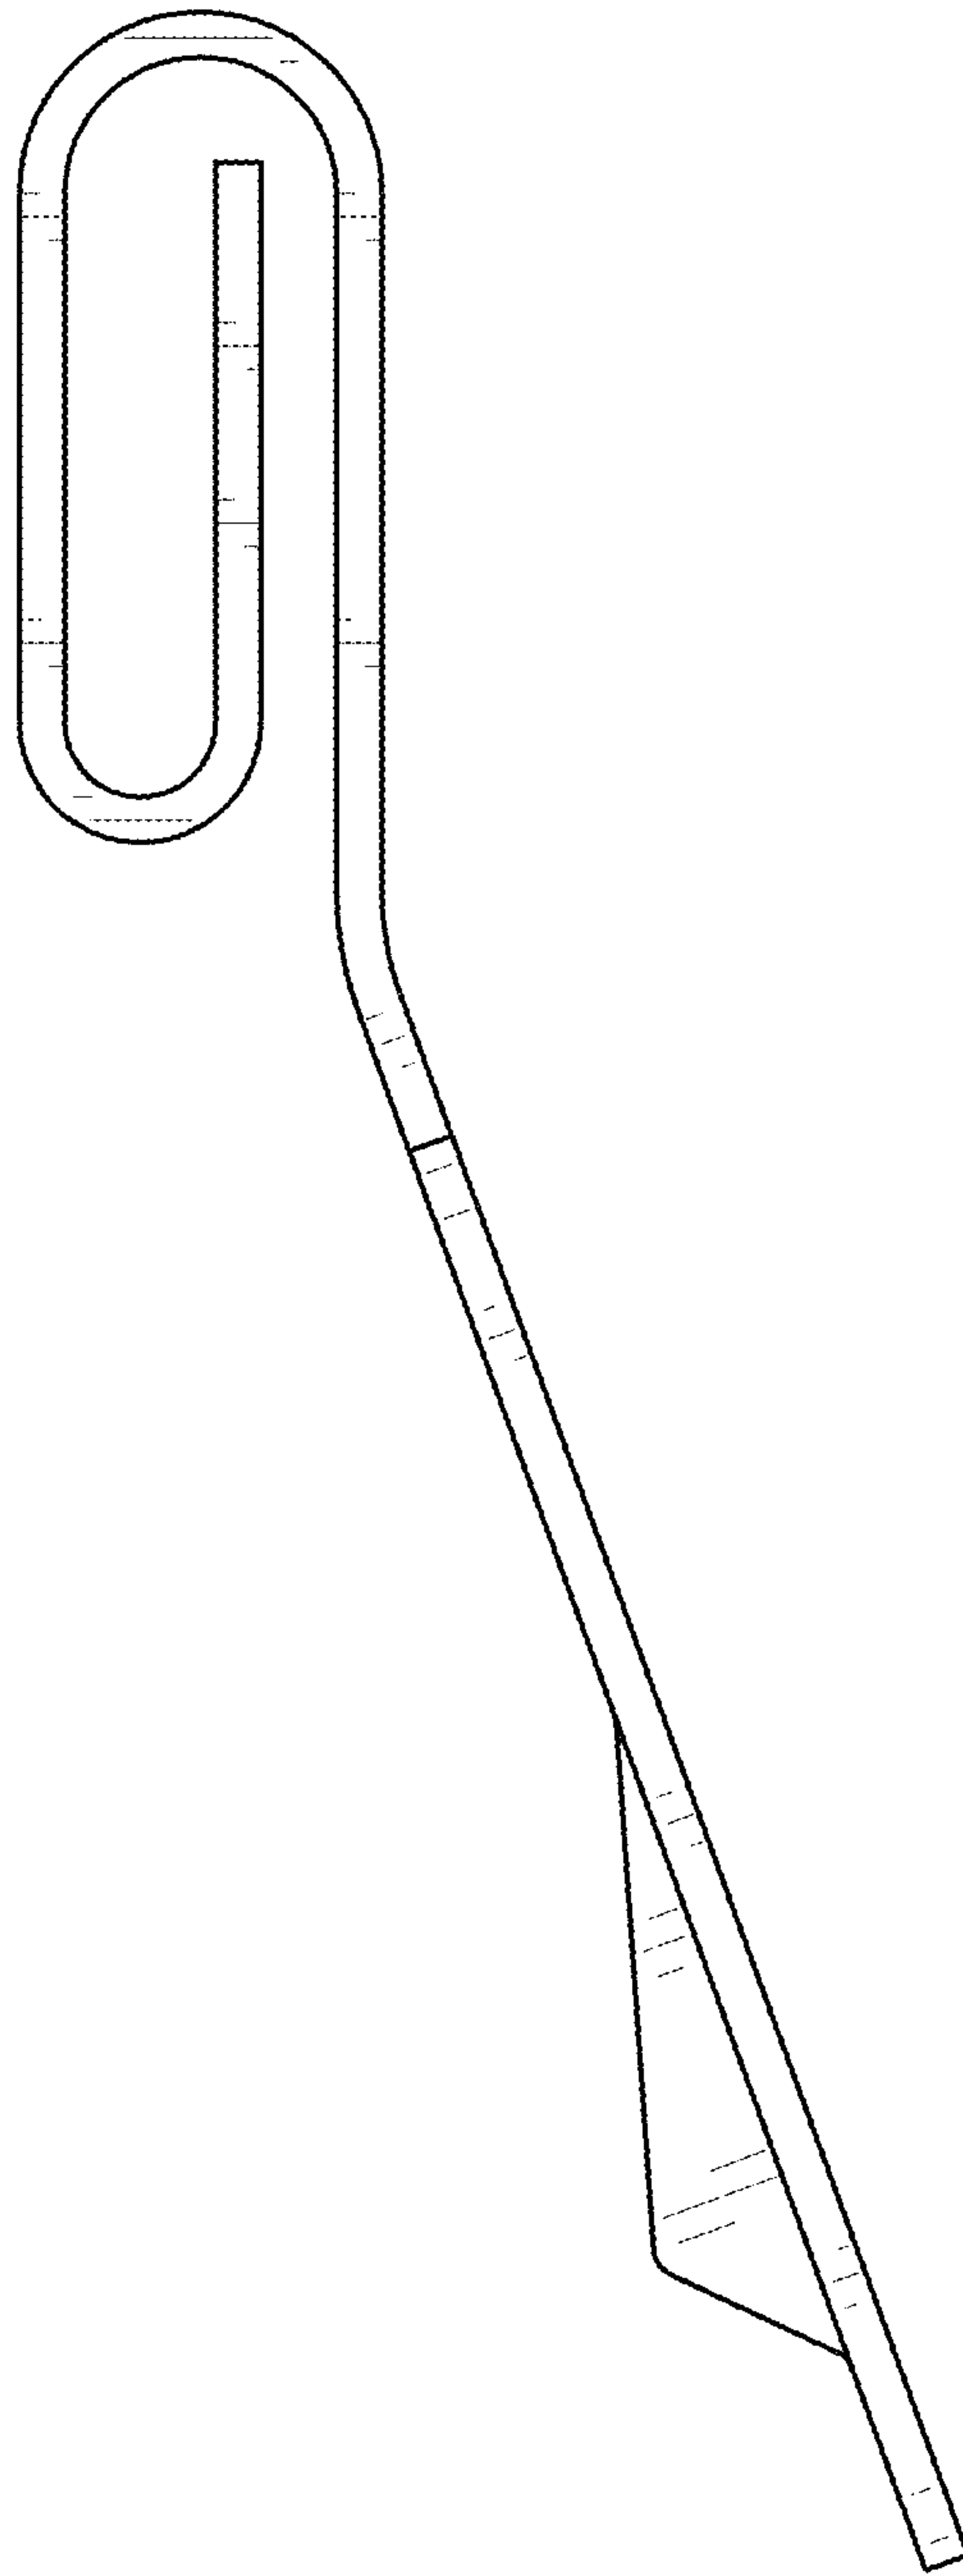


**FIG. 3**

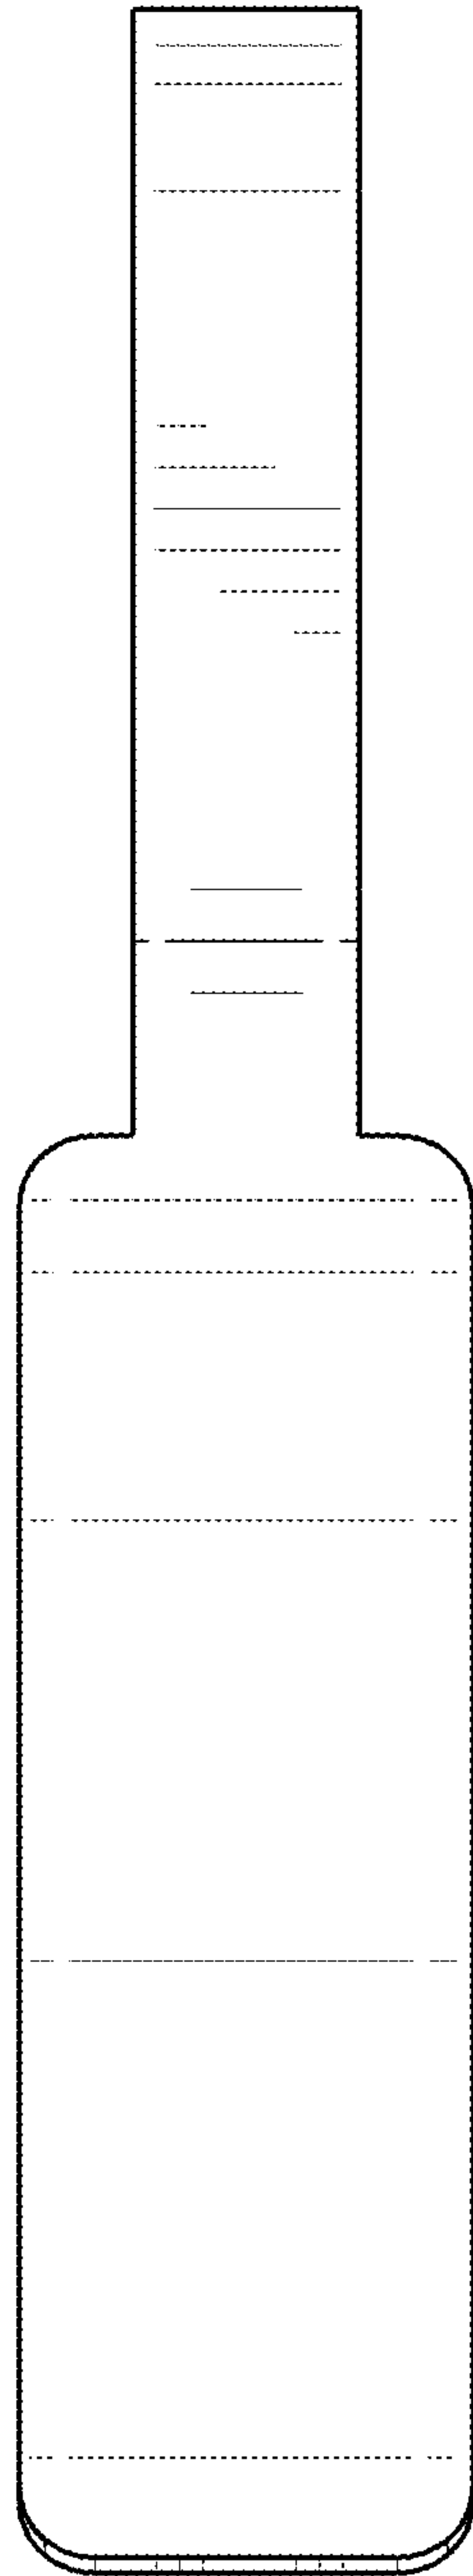

**FIG. 4**

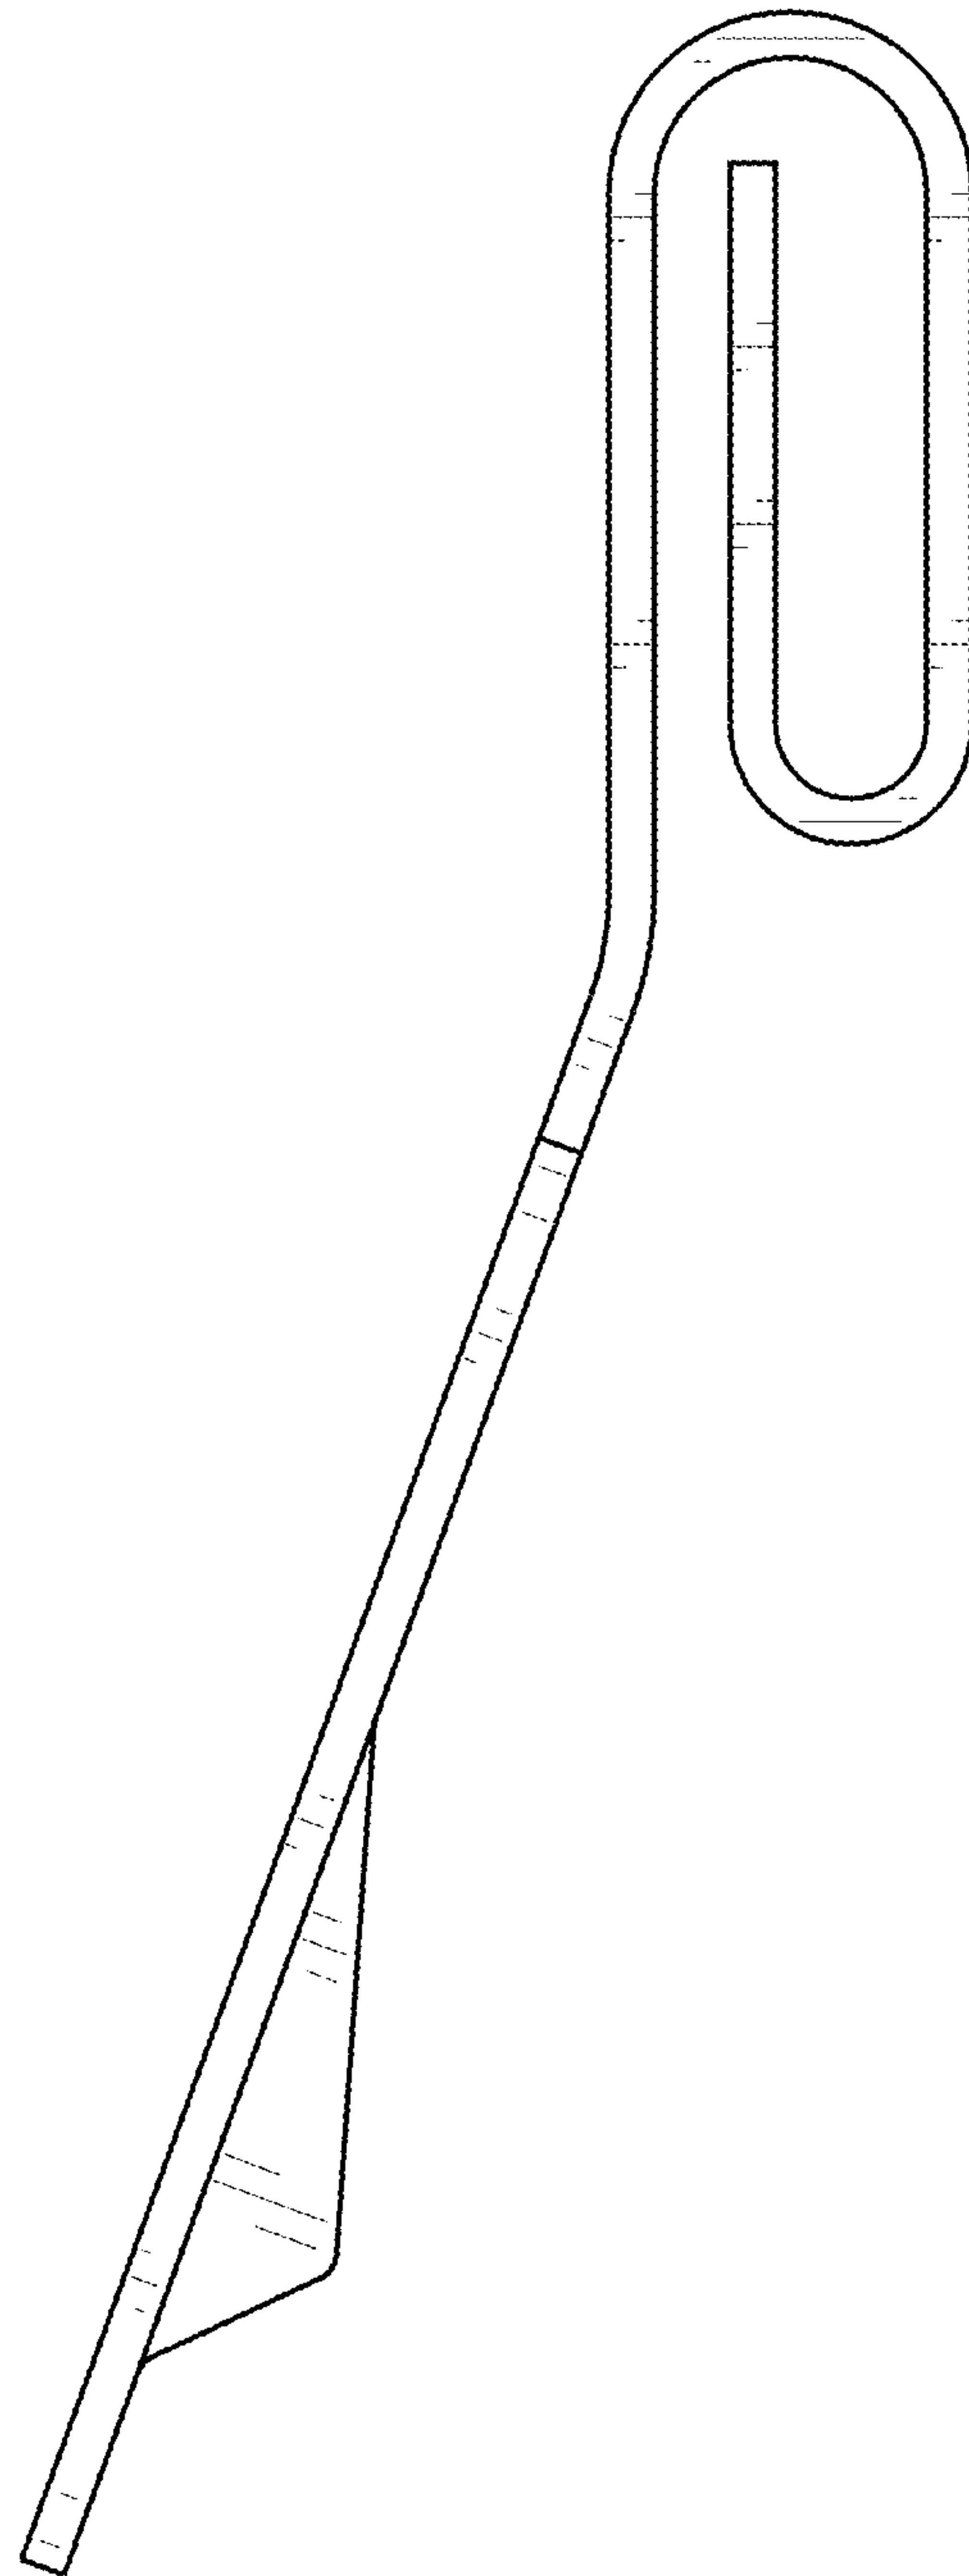


**FIG. 5**

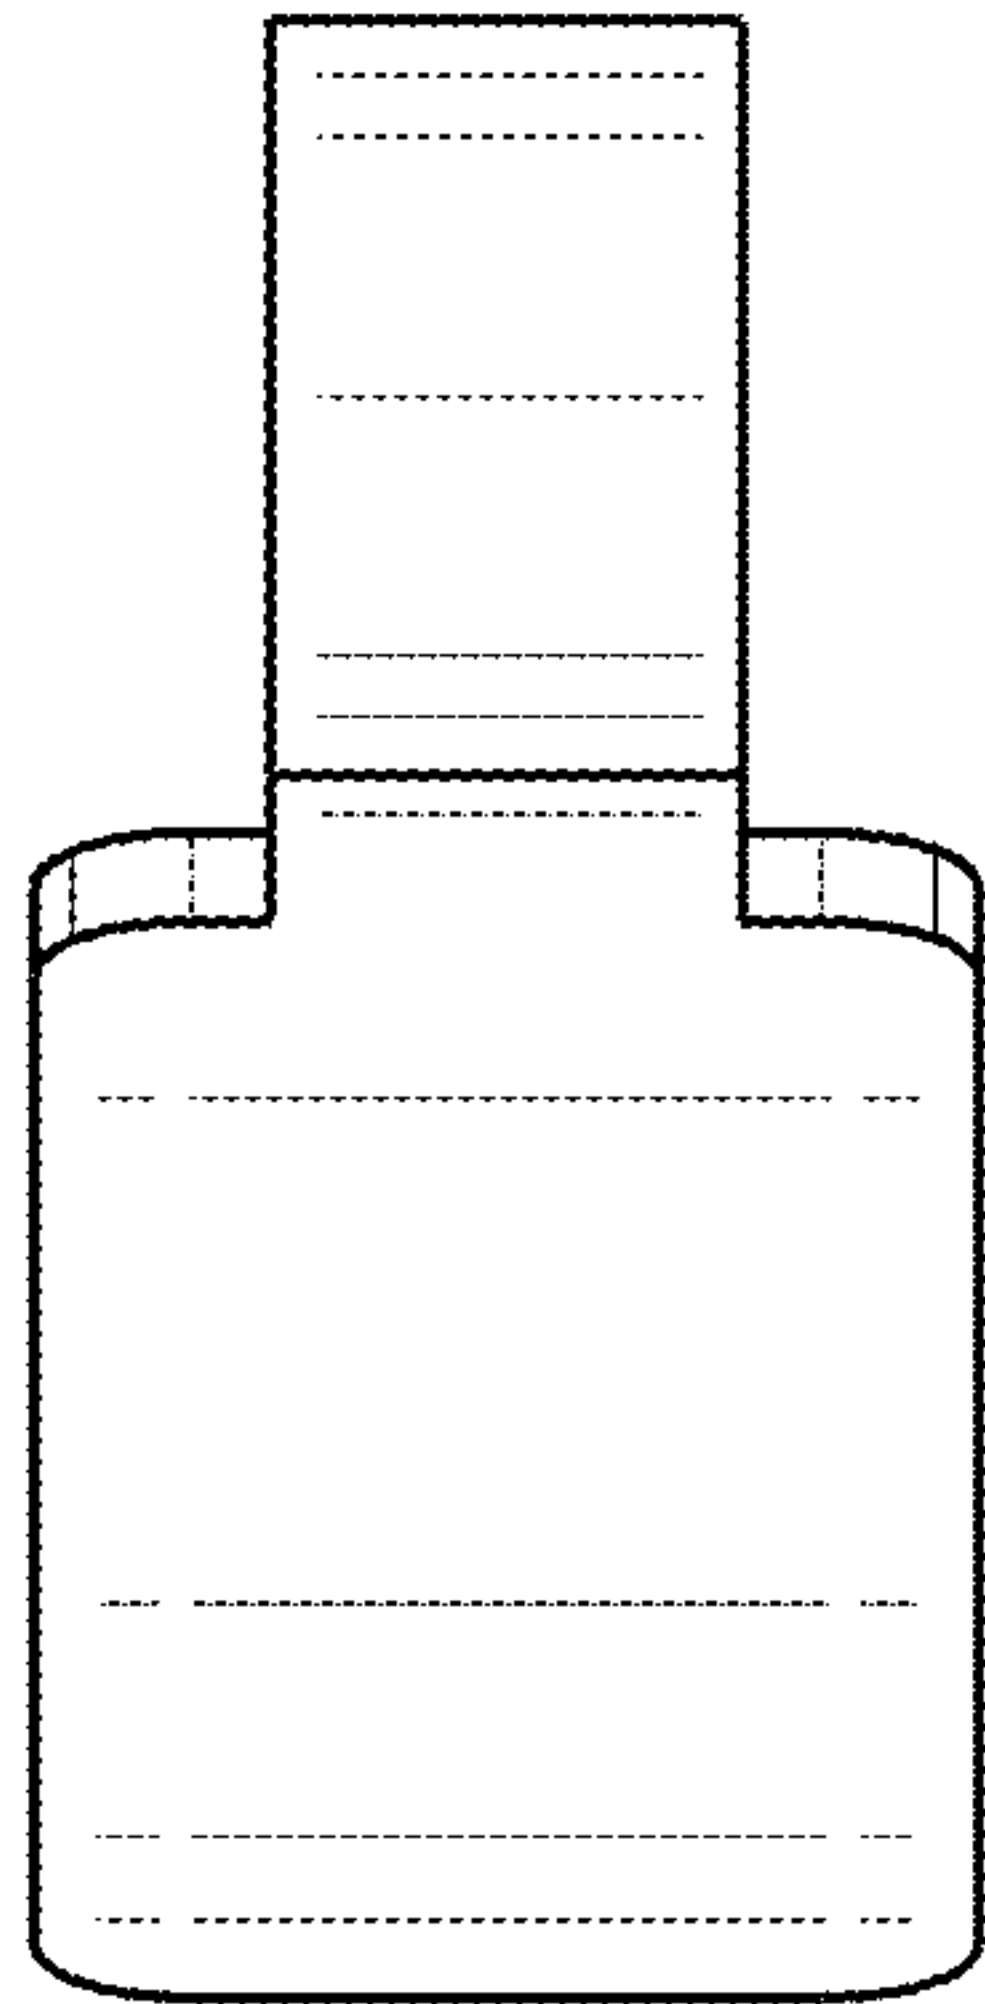

**FIG. 6**



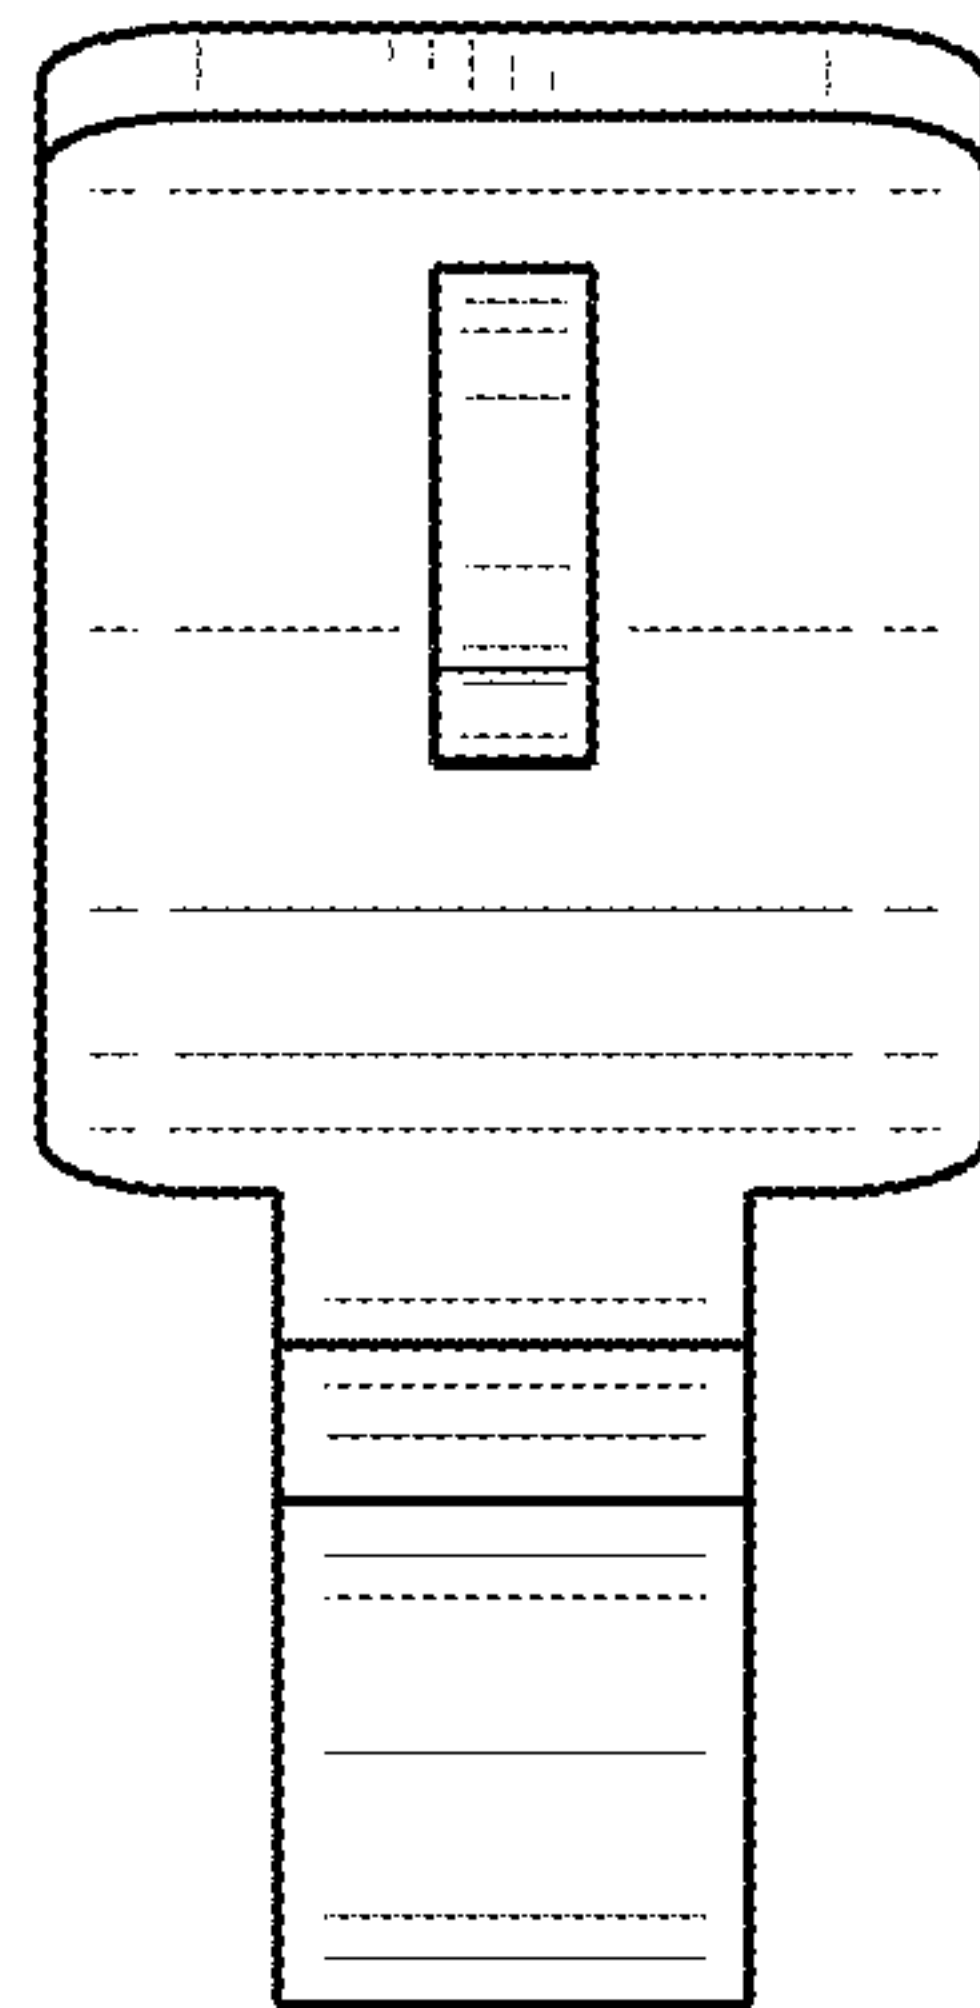

**FIG. 7**